

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
 Data File : PP059672.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 19:12
 Operator : YP\AJ
 Sample : 04246-08 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC247799LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/01/2023
 Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:37:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.410	3.638	2180044	3466386	1.844m	1.794
2) SA Decachlor...	10.194	8.661	1982967	3496493	2.536	2.533

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
Data File : PP059672.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 19:12
Operator : YP\AJ
Sample : 04246-08 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC247799LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/01/2023
Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:37:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

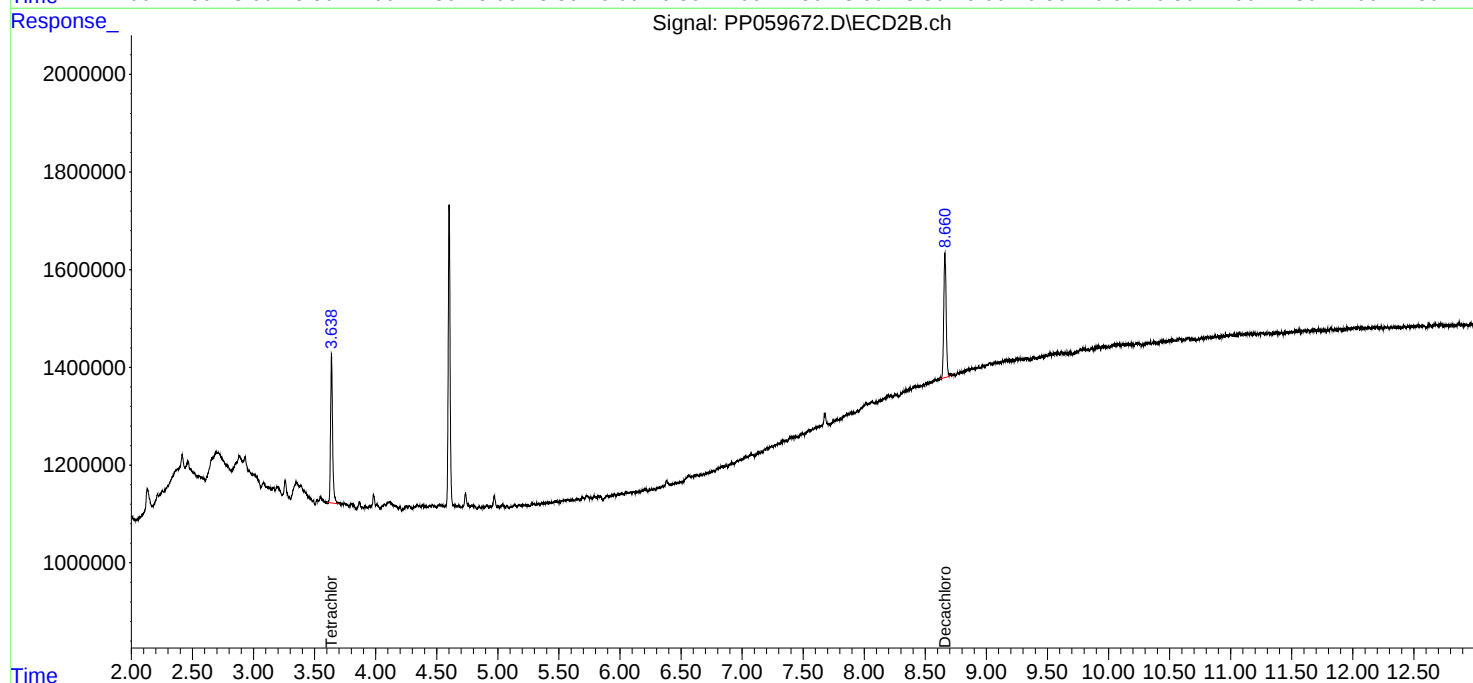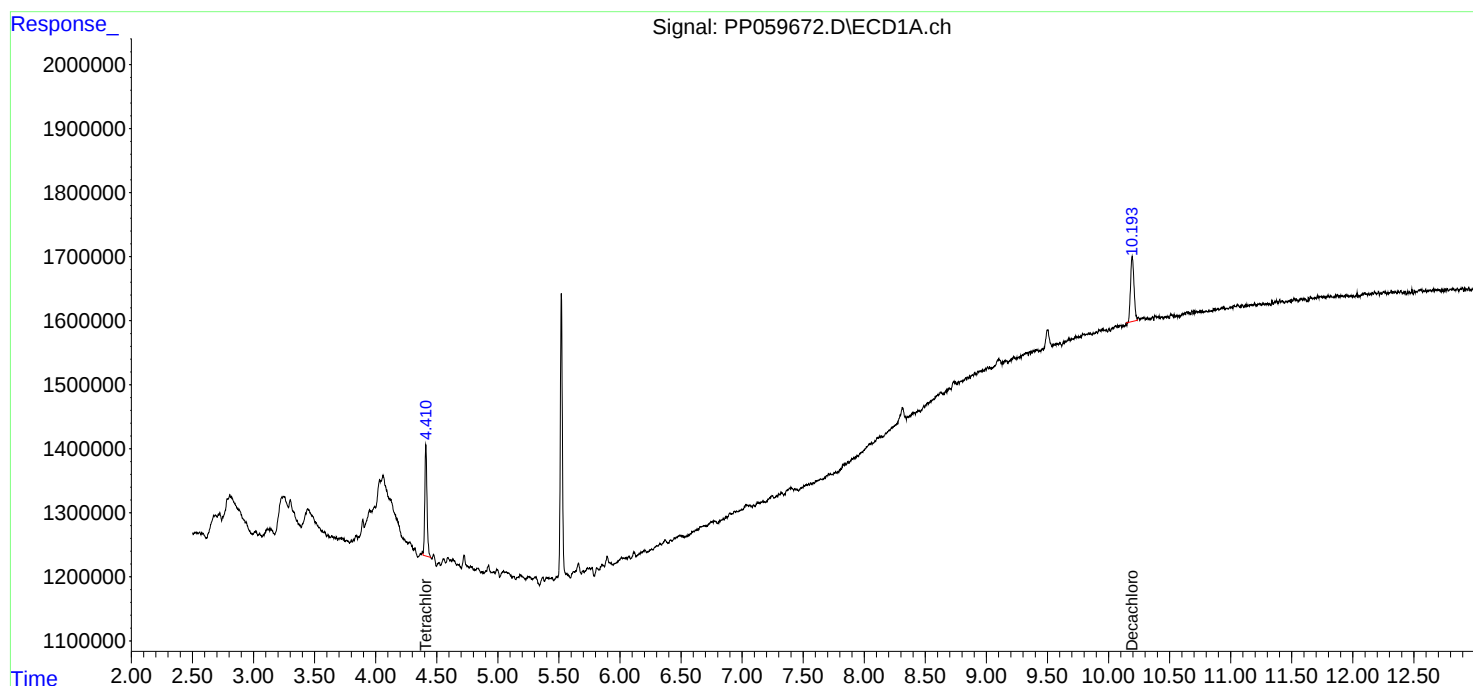

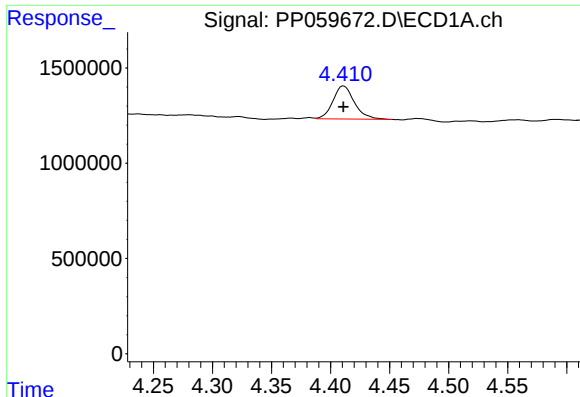


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 2180044
Conc: 1.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC247799LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/01/2023
Supervised By :Ankita Jodhani 09/05/2023

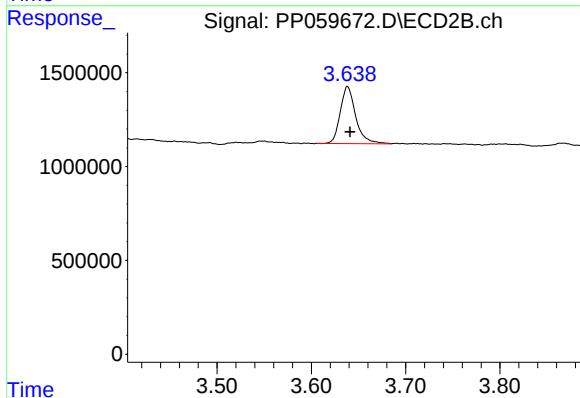


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 3466386
Conc: 1.79 ng/ml

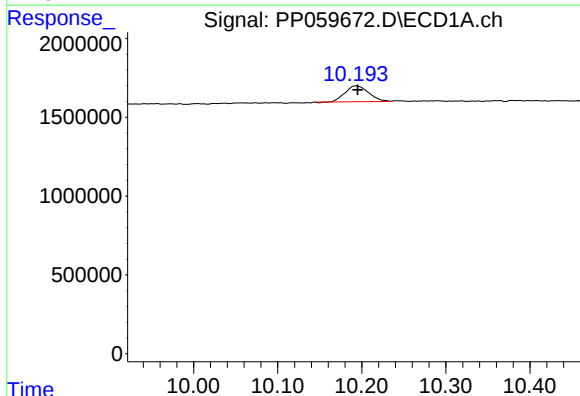

#2 Decachlorobiphenyl

R.T.: 10.194 min
Delta R.T.: -0.002 min
Response: 1982967
Conc: 2.54 ng/ml

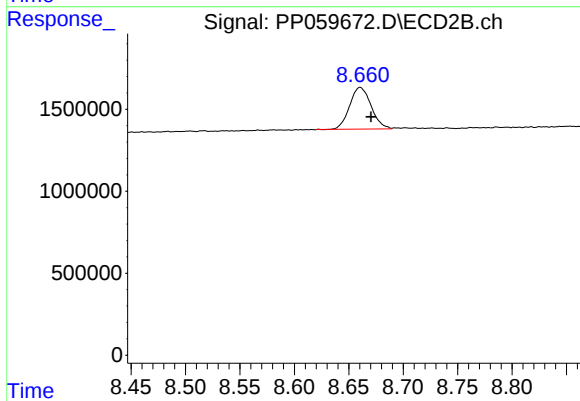

#2 Decachlorobiphenyl

R.T.: 8.661 min
Delta R.T.: -0.010 min
Response: 3496493
Conc: 2.53 ng/ml