

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
 Data File : PP059678.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 31 Aug 2023 20:50
 Operator : YP\AJ
 Sample : 04246-14 10X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC704970LOK-END-1-2

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/05/2023
 Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 02:44:31 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 24 01:16:04 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.410	3.638	1712963	2245602	1.449	1.162
2) SA Decachlor...	10.193	8.659	1720339	2174846	2.200	1.576 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP083123\
Data File : PP059678.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 31 Aug 2023 20:50
Operator : YP\AJ
Sample : 04246-14 10X
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC704970LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 02:44:31 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082323.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 24 01:16:04 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

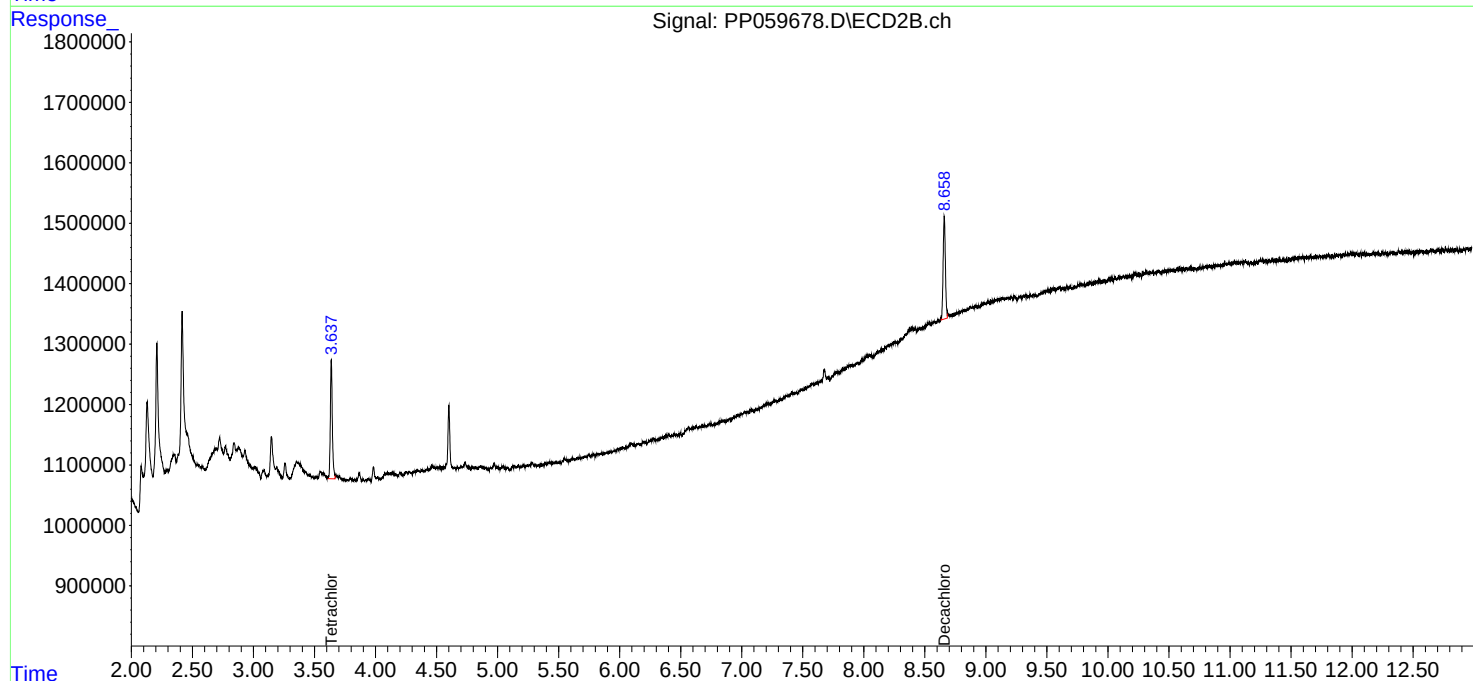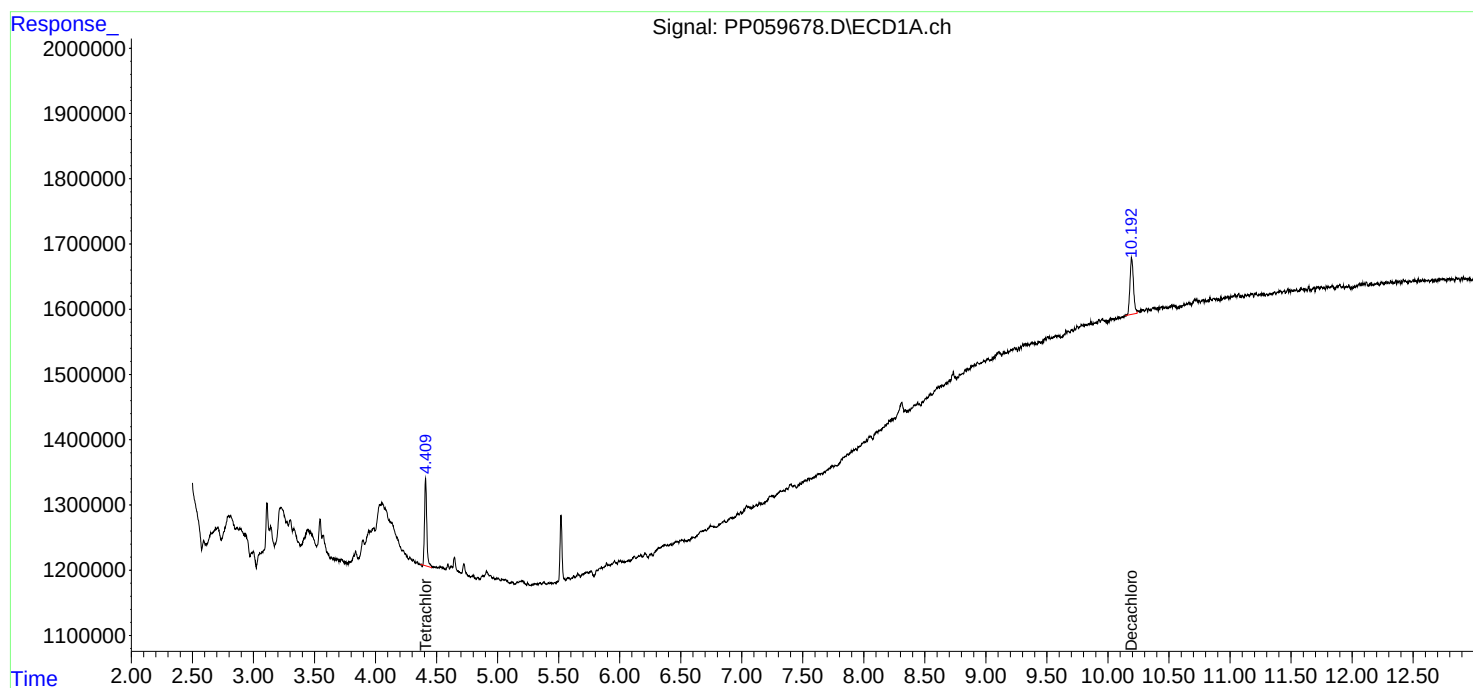

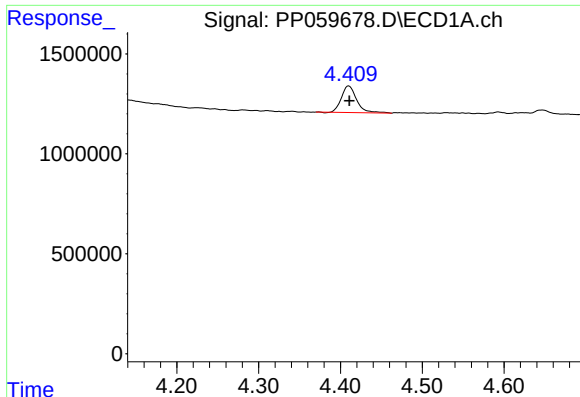


#1 Tetrachloro-m-xylene

R.T.: 4.410 min
Delta R.T.: 0.000 min
Response: 1712963
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC704970LOK-END-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/05/2023
Supervised By :Ankita Jodhani 09/05/2023

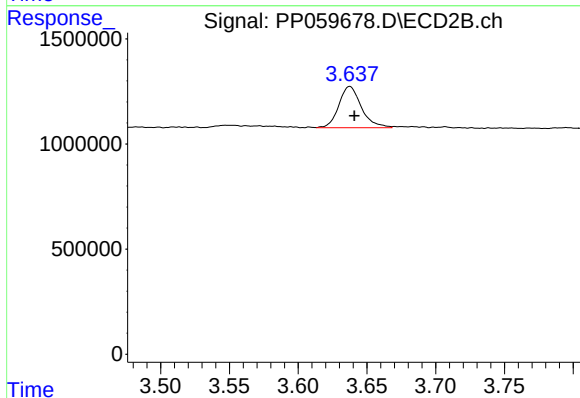


#1 Tetrachloro-m-xylene

R.T.: 3.638 min
Delta R.T.: -0.003 min
Response: 2245602
Conc: 1.16 ng/ml

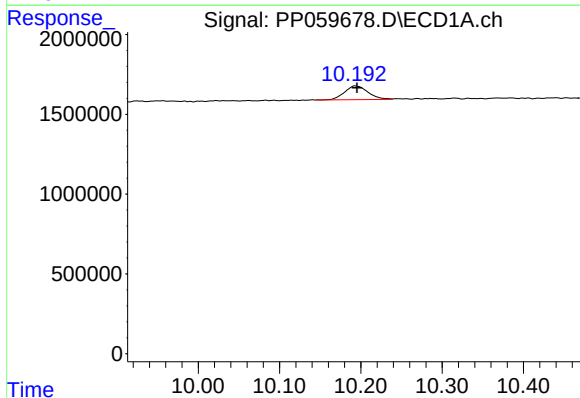

#2 Decachlorobiphenyl

R.T.: 10.193 min
Delta R.T.: -0.002 min
Response: 1720339
Conc: 2.20 ng/ml

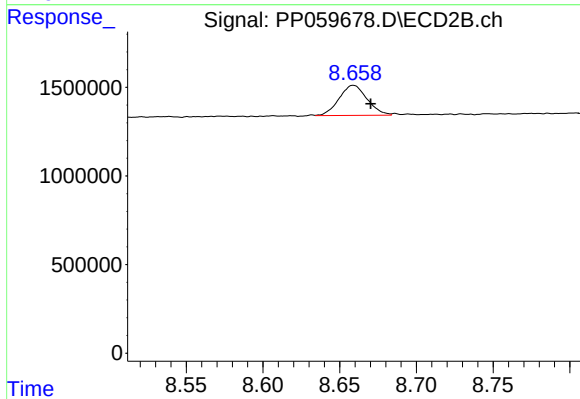

#2 Decachlorobiphenyl

R.T.: 8.659 min
Delta R.T.: -0.012 min
Response: 2174846
Conc: 1.58 ng/ml