

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090121\
 Data File : PP039121.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Sep 2021 17:41
 Operator : AJ\MA
 Sample : M3610-01RE
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 YORK-ST-MH-1RE

Manual Integrations
 APPROVED

mohammad
 9/2/2021 2:47:01 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 12:16:23 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.873	3.858	564919	463131	14.799	19.217m#
2) SA Decachlor...	10.854	9.114	256408	238316	10.649	10.540

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090121\
Data File : PP039121.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Sep 2021 17:41
Operator : AJ\MA
Sample : M3610-01RE
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
YORK-ST-MH-1RE


Manual Integrations
APPROVED

mohammad
9/2/2021 2:47:01 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 12:16:23 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

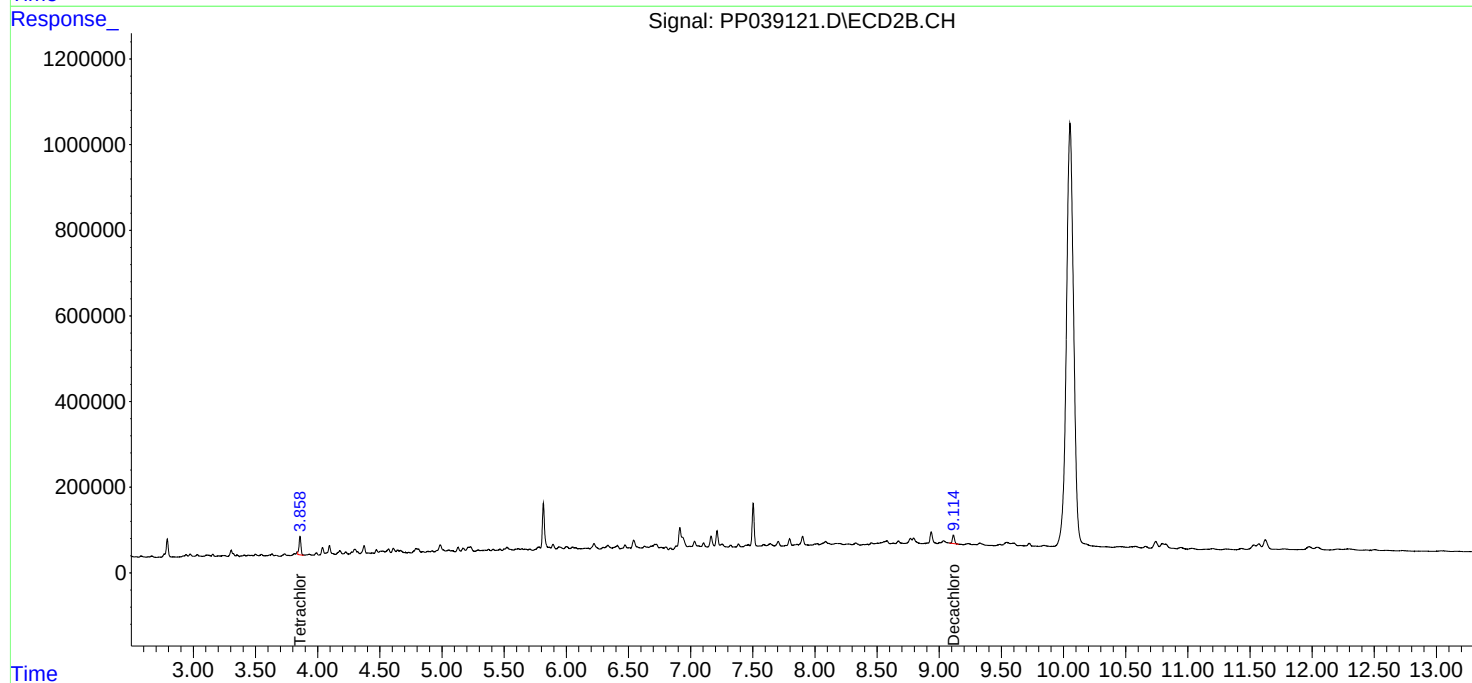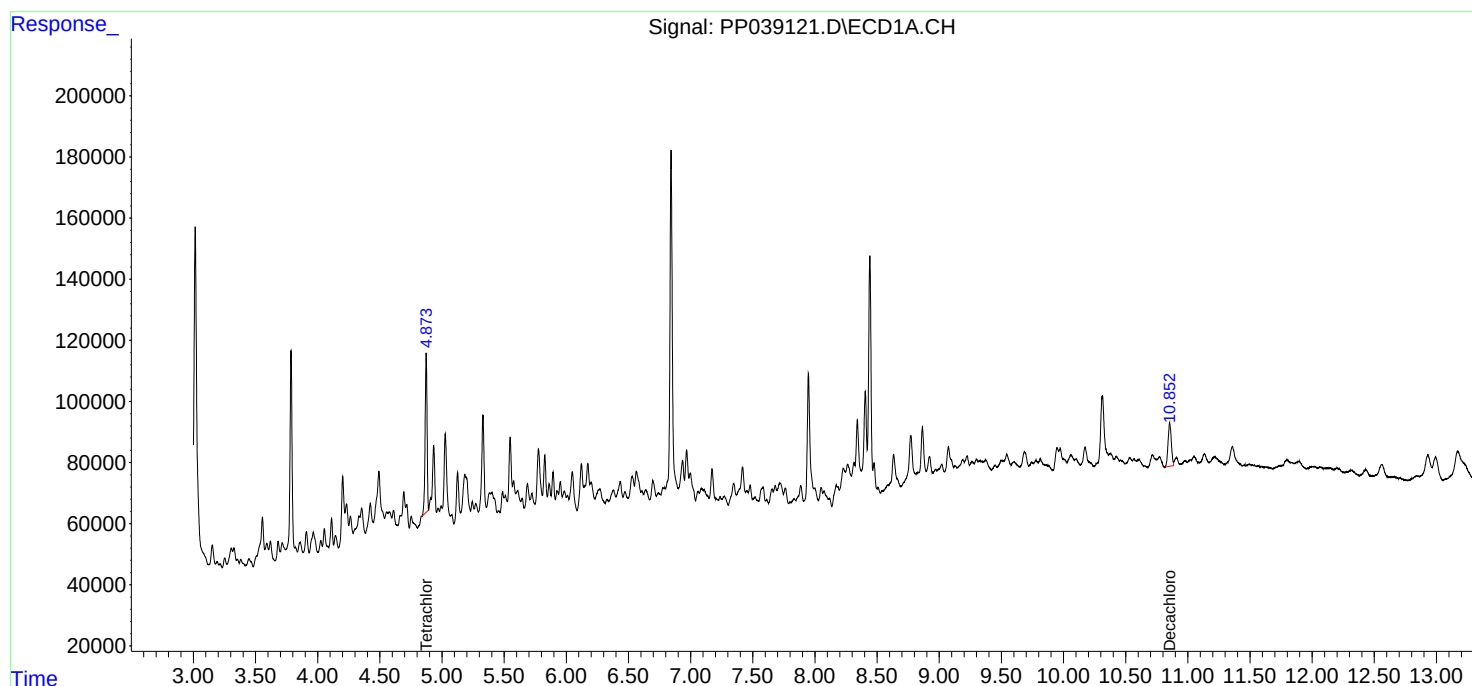

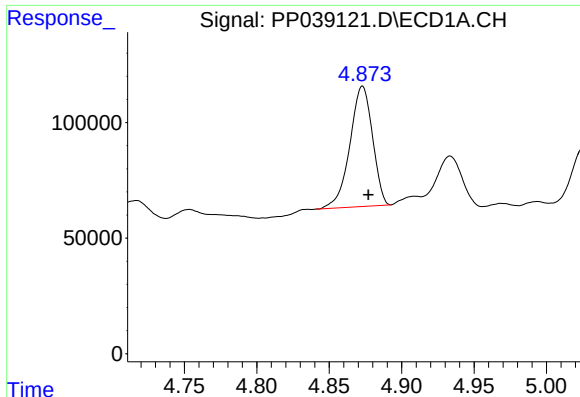


#1 Tetrachloro-m-xylene

R.T.: 4.873 min
Delta R.T.: -0.004 min
Response: 564919
Conc: 14.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
YORK-ST-MH-1RE


Manual Integrations
APPROVED

mohammad
9/2/2021 2:47:01 PM

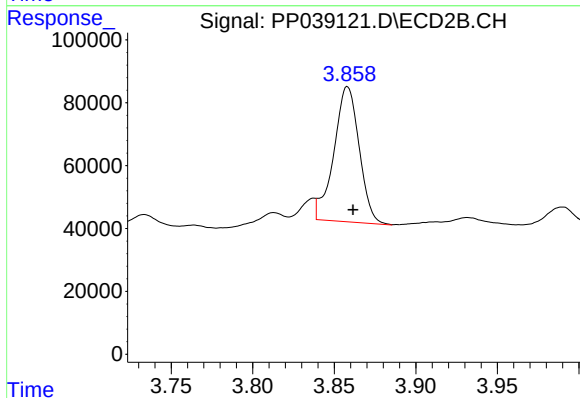


#1 Tetrachloro-m-xylene

R.T.: 3.858 min
Delta R.T.: -0.004 min
Response: 463131
Conc: 19.22 ng/ml m

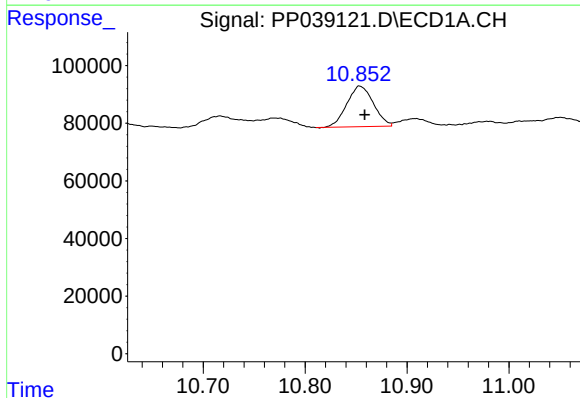

#2 Decachlorobiphenyl

R.T.: 10.854 min
Delta R.T.: -0.005 min
Response: 256408
Conc: 10.65 ng/ml

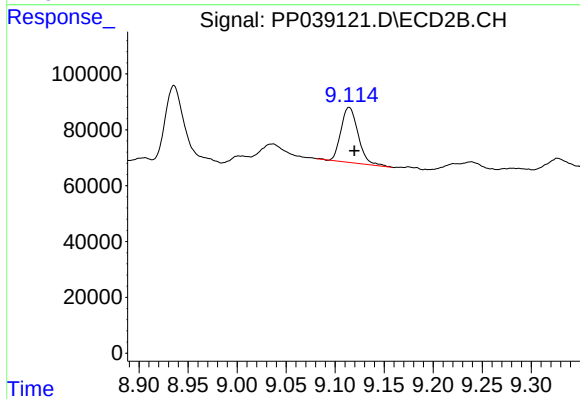

#2 Decachlorobiphenyl

R.T.: 9.114 min
Delta R.T.: -0.005 min
Response: 238316
Conc: 10.54 ng/ml