

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090121\
 Data File : PP039123.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 01 Sep 2021 18:15
 Operator : AJ\MA
 Sample : M3610-02RE
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 YORK-ST-MH-2RE

Manual Integrations
 APPROVED

mohammad
 9/2/2021 2:47:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 12:16:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Aug 26 09:31:39 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.875	3.860	771471	601392	20.211	24.954m
2) SA Decachlor...	10.857	9.116	451138	407828	18.737	18.036m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090121\
Data File : PP039123.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 01 Sep 2021 18:15
Operator : AJ\MA
Sample : M3610-02RE
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
YORK-ST-MH-2RE


Manual Integrations
APPROVED

mohammad
9/2/2021 2:47:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 12:16:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082521.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Aug 26 09:31:39 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

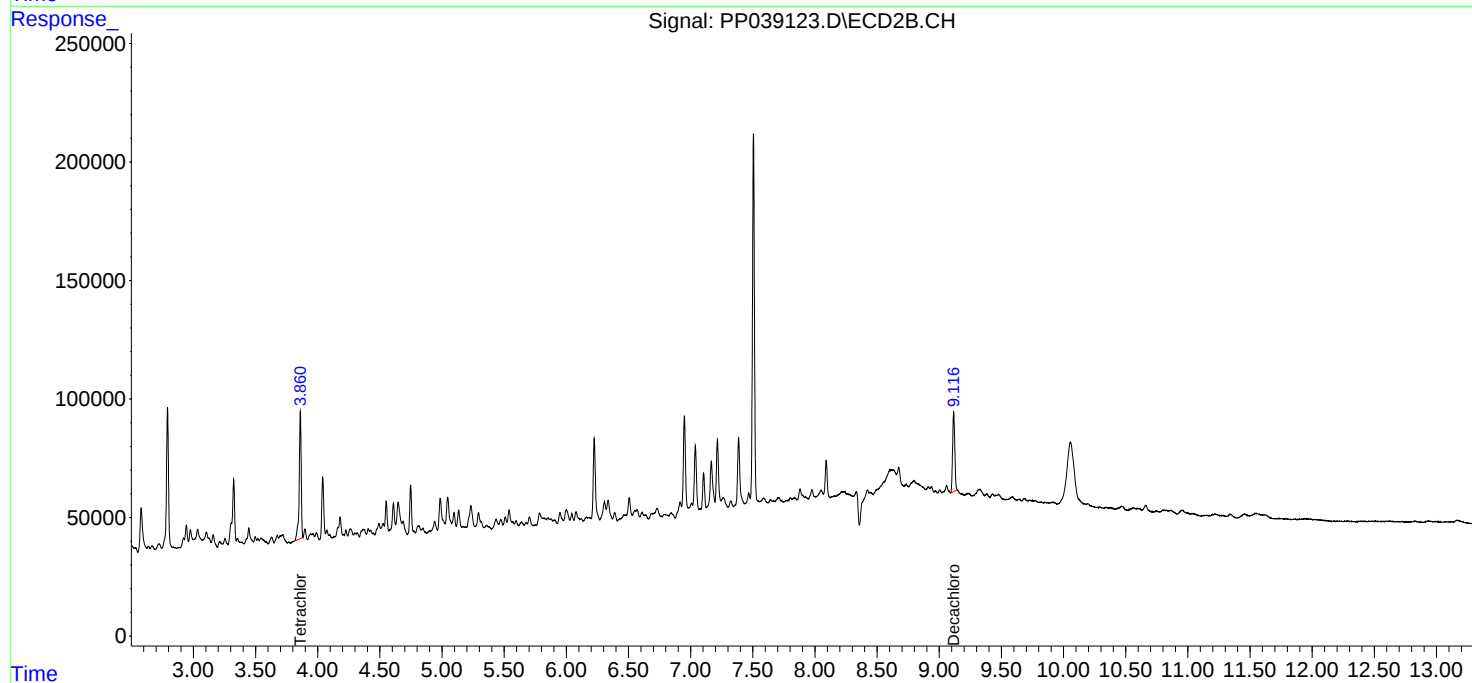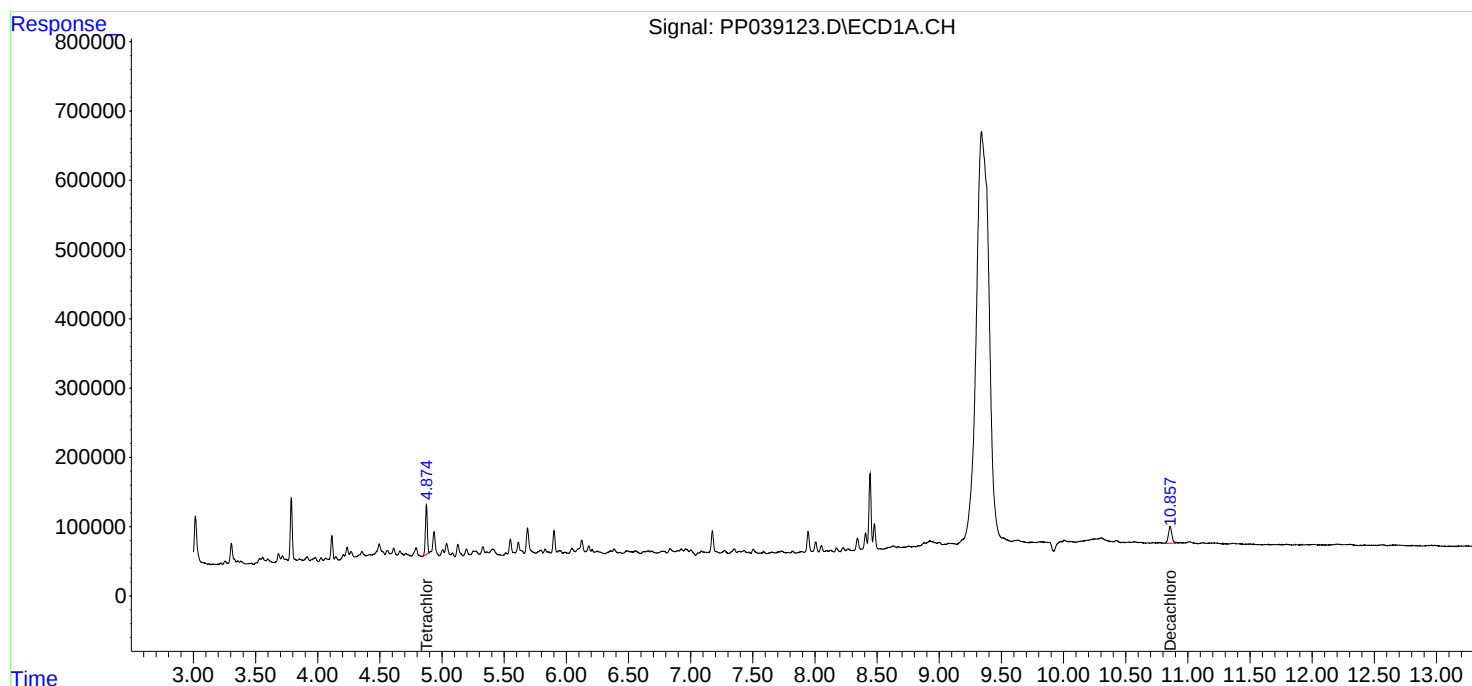

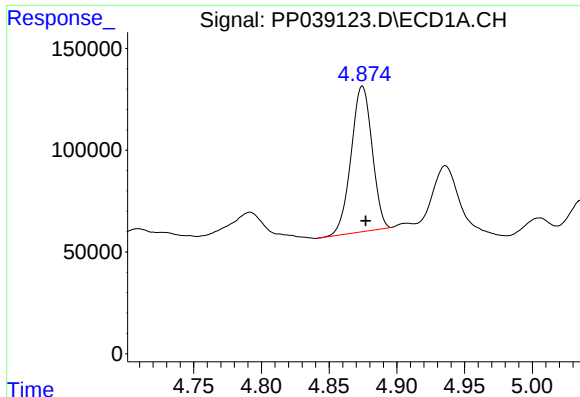


#1 Tetrachloro-m-xylene

R.T.: 4.875 min
Delta R.T.: -0.002 min
Response: 771471
Conc: 20.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
YORK-ST-MH-2RE


Manual Integrations
APPROVED

mohammad
9/2/2021 2:47:15 PM

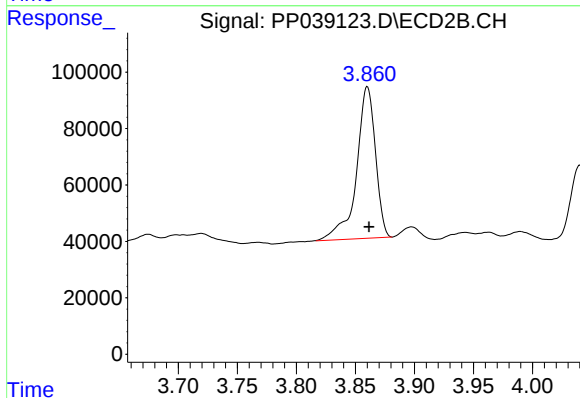


#1 Tetrachloro-m-xylene

R.T.: 3.860 min
Delta R.T.: -0.002 min
Response: 601392
Conc: 24.95 ng/ml m

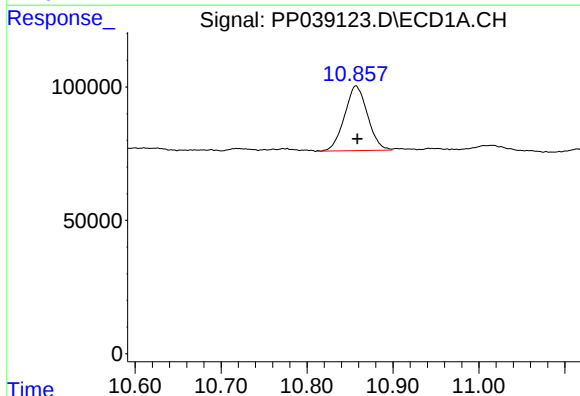

#2 Decachlorobiphenyl

R.T.: 10.857 min
Delta R.T.: -0.002 min
Response: 451138
Conc: 18.74 ng/ml

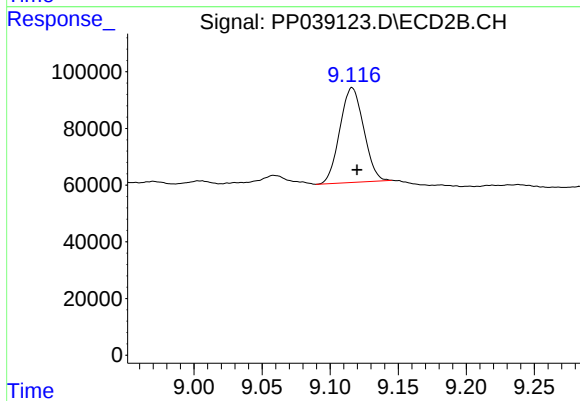

#2 Decachlorobiphenyl

R.T.: 9.116 min
Delta R.T.: -0.004 min
Response: 407828
Conc: 18.04 ng/ml m