

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090122\
 Data File : PP051155.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 18:06
 Operator : YP\AJ
 Sample : N4466-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SASP2-T-5-(17-23)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 01 18:58:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 26 17:33:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.462	3.718	33772616	38340117	18.123	21.758
2) SA Decachlor...	10.262	8.798	38991053	23448293	21.614	21.949

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090122\
Data File : PP051155.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 18:06
Operator : YP\AJ
Sample : N4466-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SASP2-T-5-(17-23)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 01 18:58:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082622.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 26 17:33:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

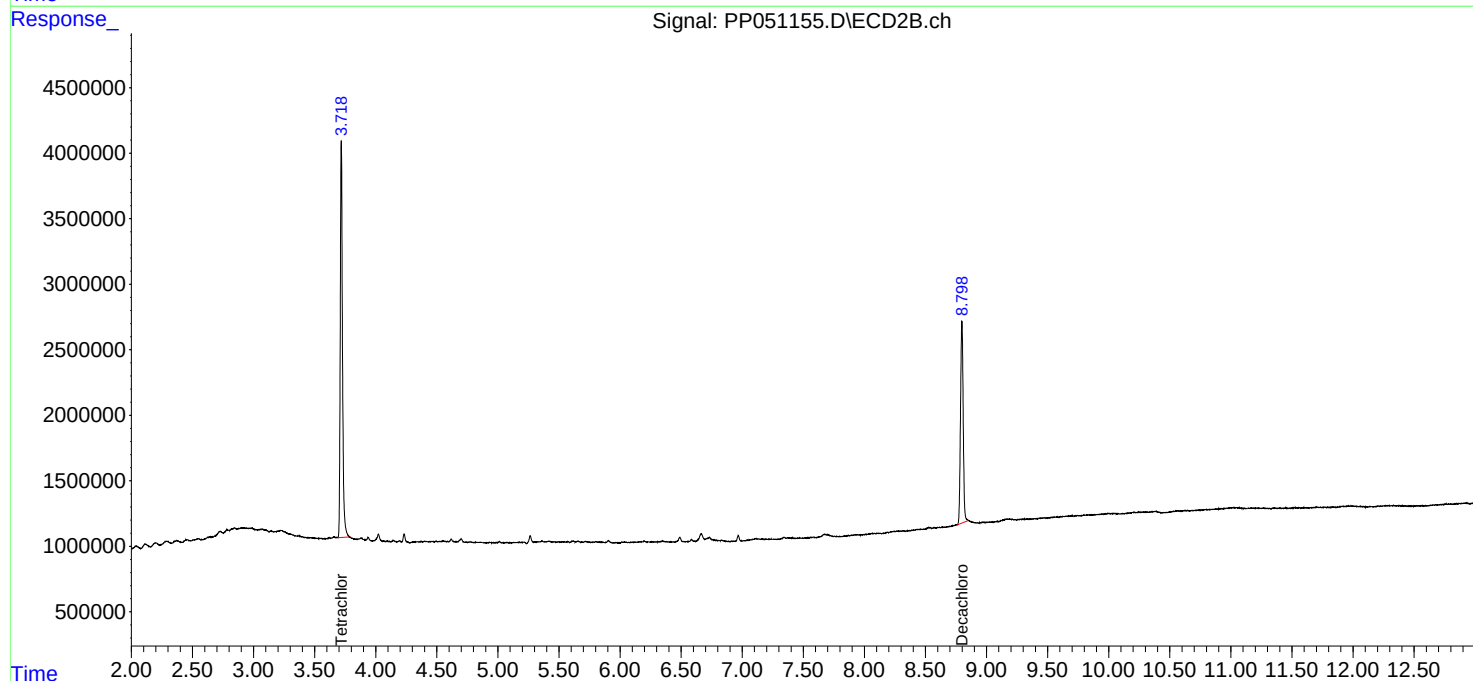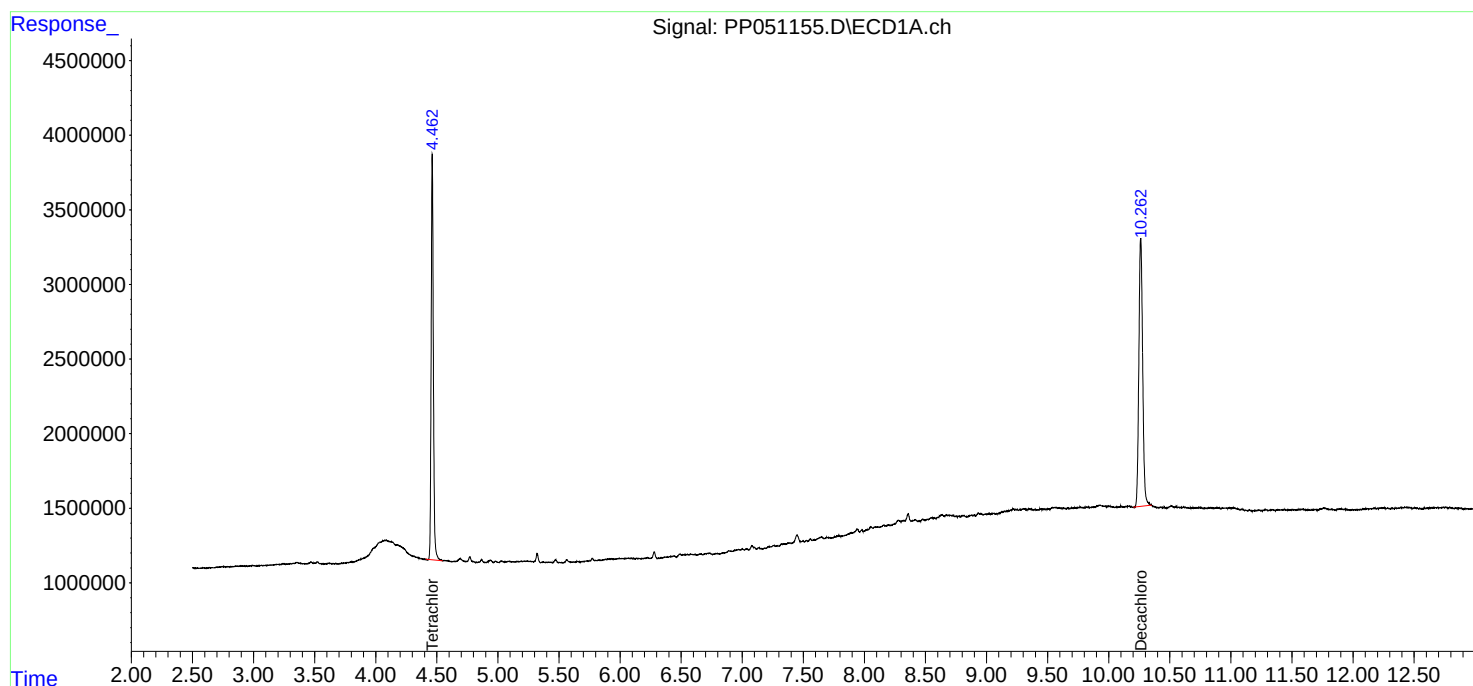


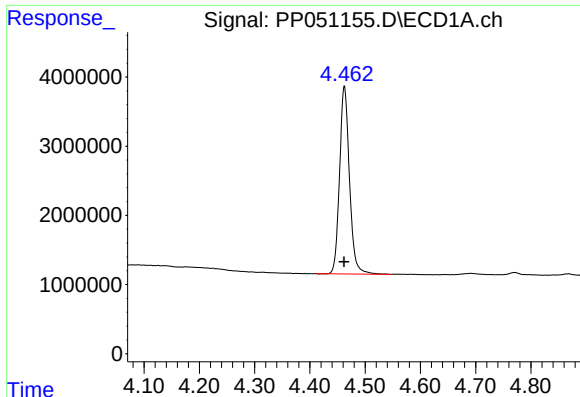

#1 Tetrachloro-m-xylene


R.T.: 4.462 min
Delta R.T.: 0.000 min
Response: 33772616
Conc: 18.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
SASP2-T-5-(17-23)

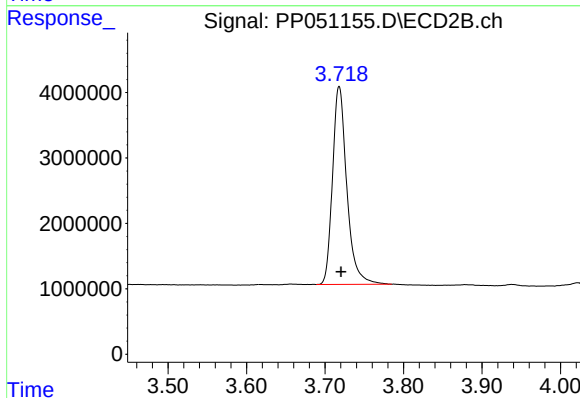


#1 Tetrachloro-m-xylene

R.T.: 3.718 min
Delta R.T.: -0.003 min
Response: 38340117
Conc: 21.76 ng/ml

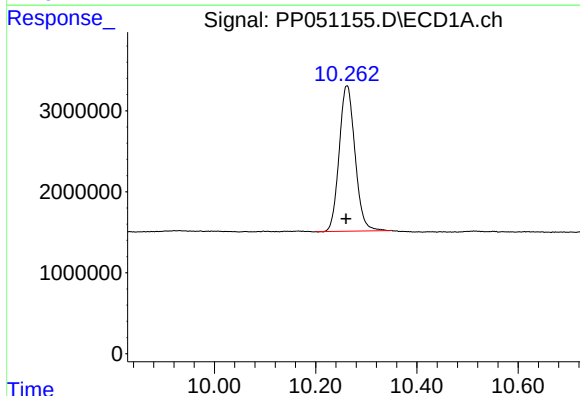

#2 Decachlorobiphenyl

R.T.: 10.262 min
Delta R.T.: 0.002 min
Response: 38991053
Conc: 21.61 ng/ml

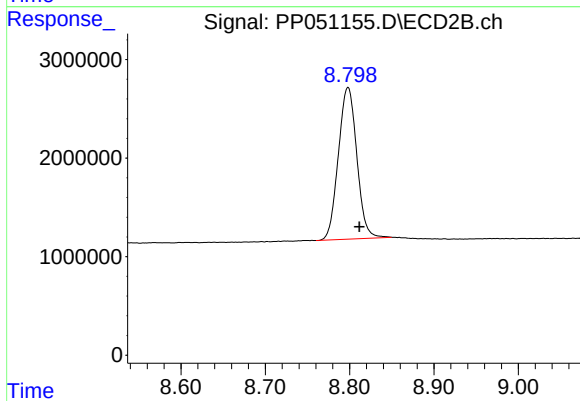

#2 Decachlorobiphenyl

R.T.: 8.798 min
Delta R.T.: -0.013 min
Response: 23448293
Conc: 21.95 ng/ml