

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090122\
 Data File : PP051170.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 01 Sep 2022 22:44
 Operator : YP\AJ
 Sample : N4437-02RE
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BASMENT-STAND-PIPERE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 02 01:11:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082622.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Aug 26 17:33:33 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.460	3.716	27242497	27252451	14.619	15.466
2) SA Decachlor...	10.259	8.794	31098280	18997487	17.239	17.783

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090122\
Data File : PP051170.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 01 Sep 2022 22:44
Operator : YP\AJ
Sample : N4437-02RE
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BASMENT-STAND-PIPERE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 02 01:11:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP082622.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Aug 26 17:33:33 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

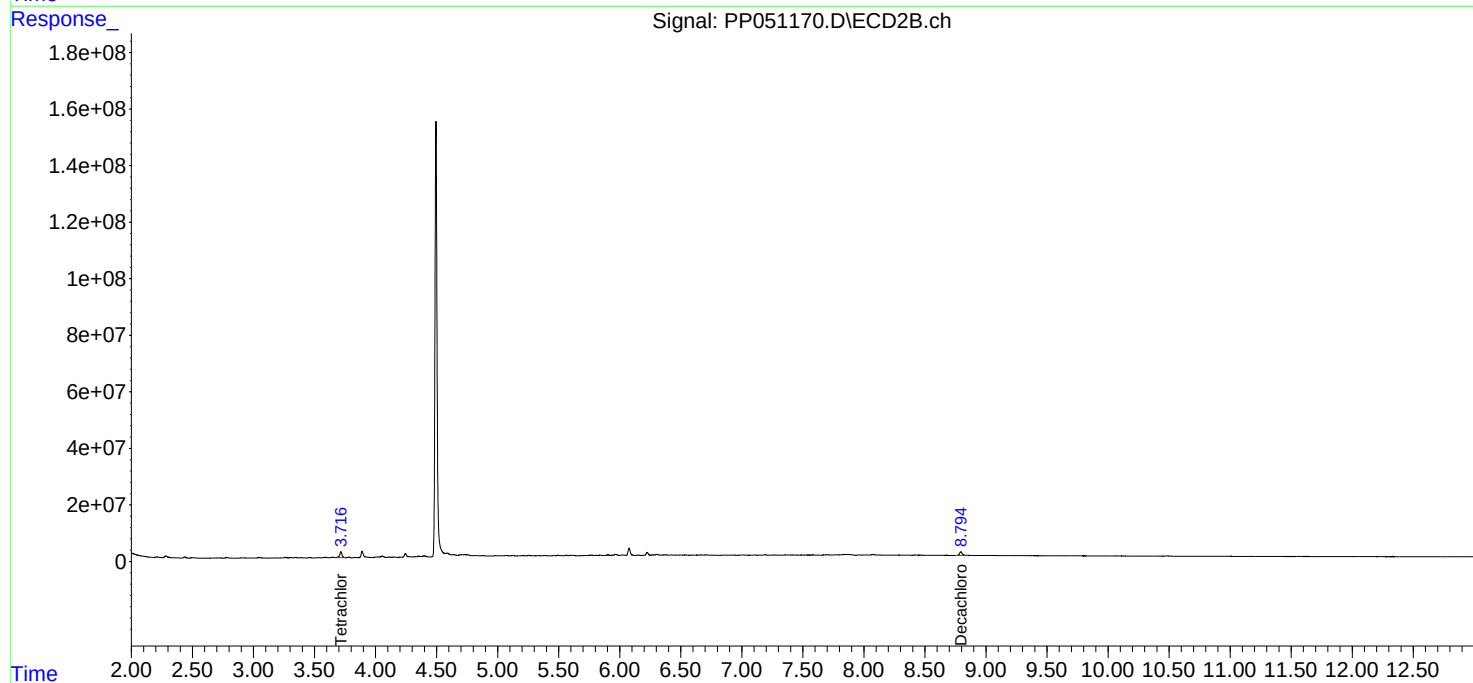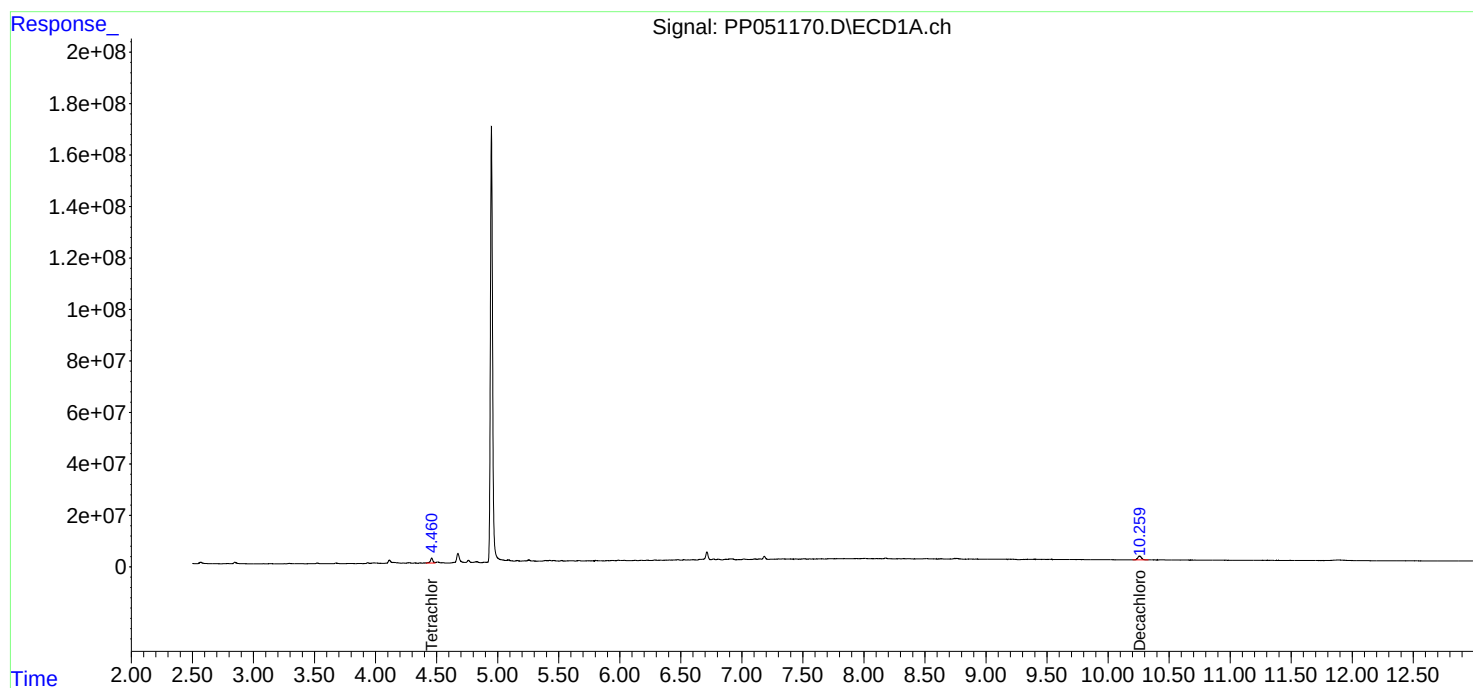


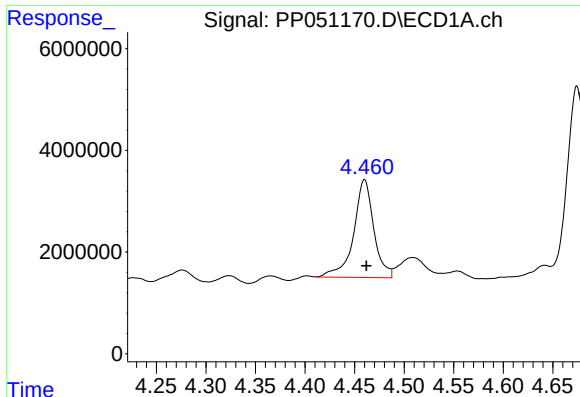

#1 Tetrachloro-m-xylene


R.T.: 4.460 min
Delta R.T.: -0.002 min
Response: 27242497
Conc: 14.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
BASMENT-STAND-PIPERE

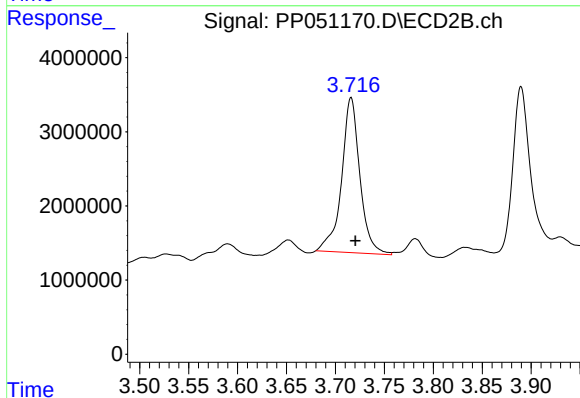


#1 Tetrachloro-m-xylene

R.T.: 3.716 min
Delta R.T.: -0.005 min
Response: 27252451
Conc: 15.47 ng/ml

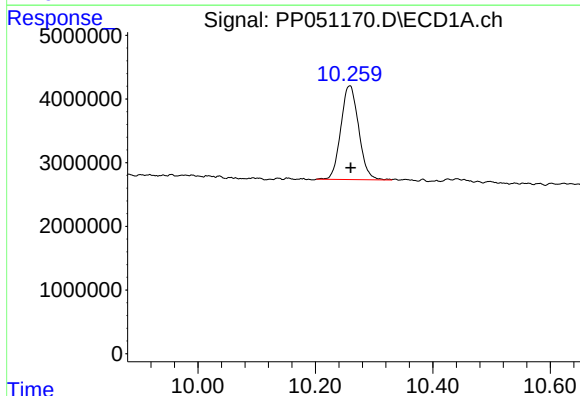

#2 Decachlorobiphenyl

R.T.: 10.259 min
Delta R.T.: -0.001 min
Response: 31098280
Conc: 17.24 ng/ml

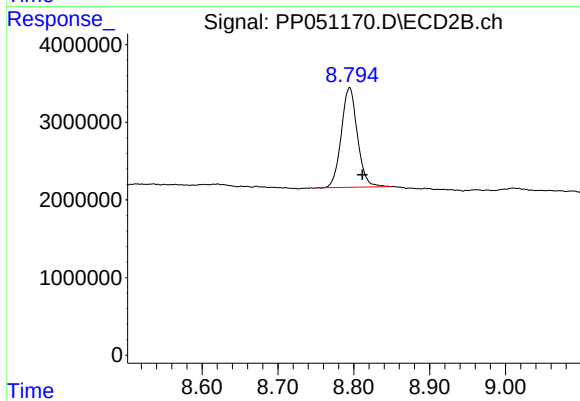

#2 Decachlorobiphenyl

R.T.: 8.794 min
Delta R.T.: -0.017 min
Response: 18997487
Conc: 17.78 ng/ml