

Data Path : P:\HPCHEM1\ECD_P\Data\PP090315\
Data File : PP011560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2015 19:35
Operator : IZ/UA
Sample : G3526-13
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SB-16(0-0.16)

Manual Integrations
APPROVED

ugo
9/9/2015 10:25:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 03:33:59 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 03 15:00:38 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	5.170	4.190	831809	1073779	19.023	18.697
2) SA Decachlor...	11.500	9.289	380766	568066	9.955m	10.002

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : P:\HPCHEM1\ECD_P\Data\PP090315\
Data File : PP011560.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 03 Sep 2015 19:35
Operator : IZ/UA
Sample : G3526-13
Misc :
ALS Vial : 34 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampled :
SB-16(0-0.16)


Manual Integrations
APPROVED

ugo
9/9/2015 10:25:37 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 04 03:33:59 2015
Quant Method : P:\HPCHEM1\ECD_P\methods\PP090315.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Sep 03 15:00:38 2015
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

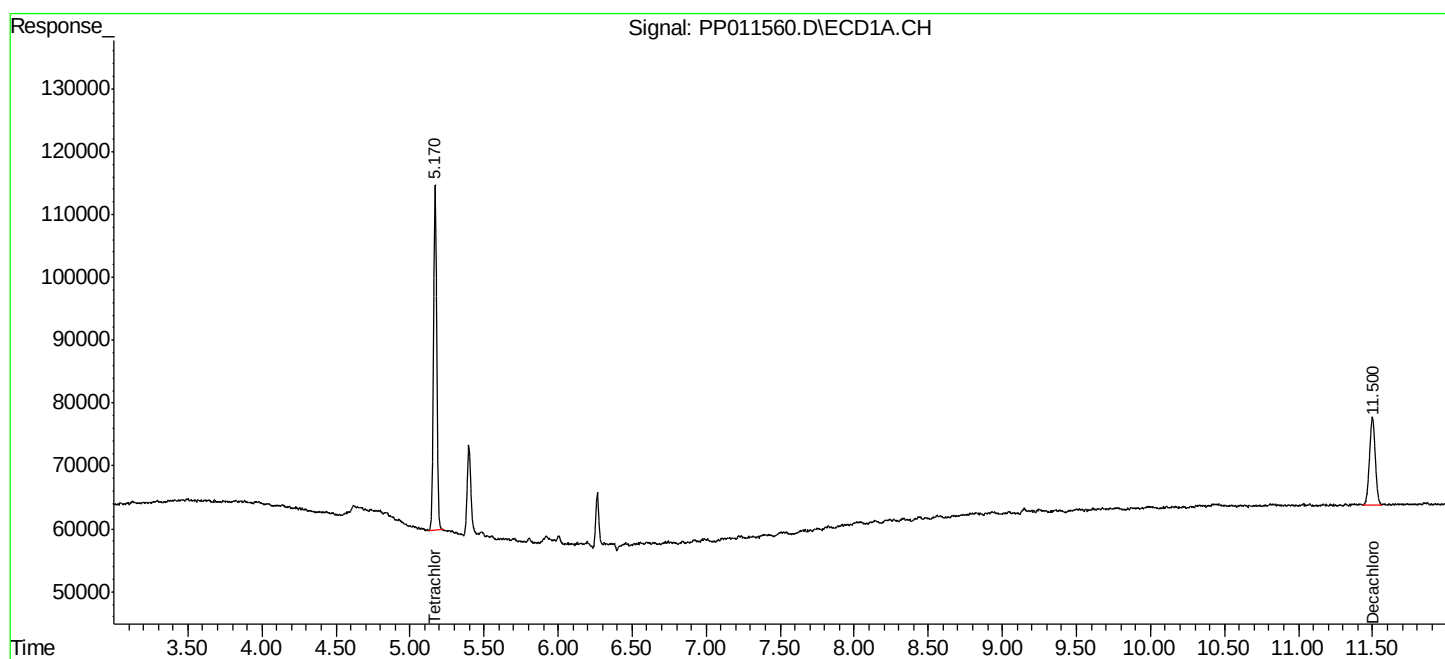

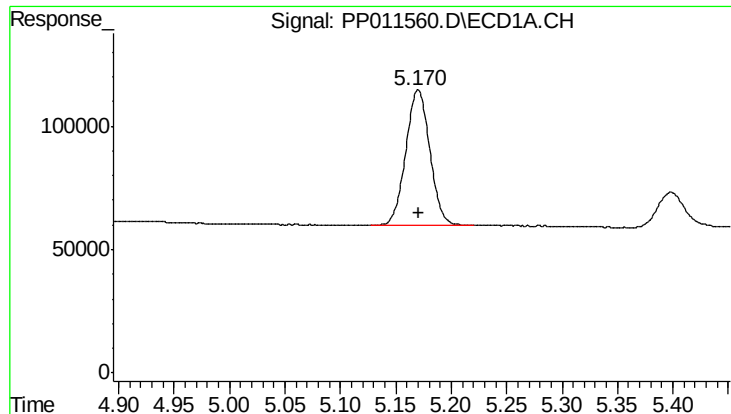


#1 Tetrachloro-m-xylene

R.T.: 5.170 min
Delta R.T.: 0.000 min
Response: 831809
Conc: 19.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
SB-16(0-0.16)


Manual Integrations
APPROVED

ugo
9/9/2015 10:25:37 AM

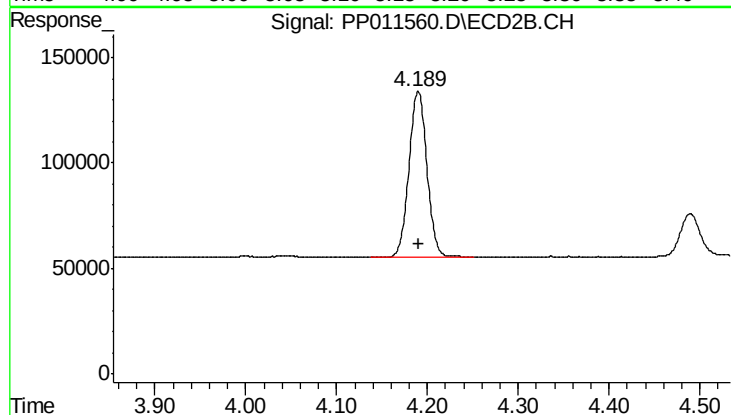


#1 Tetrachloro-m-xylene

R.T.: 4.190 min
Delta R.T.: 0.000 min
Response: 1073779
Conc: 18.70 ng/ml

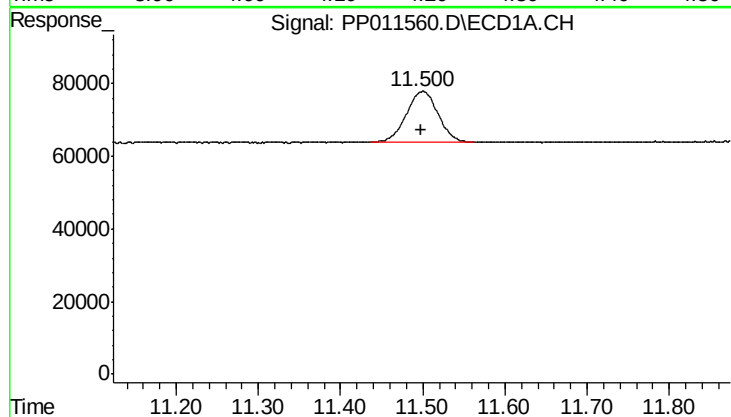

#2 Decachlorobiphenyl

R.T.: 11.500 min
Delta R.T.: 0.001 min
Response: 380766
Conc: 9.95 ng/ml m

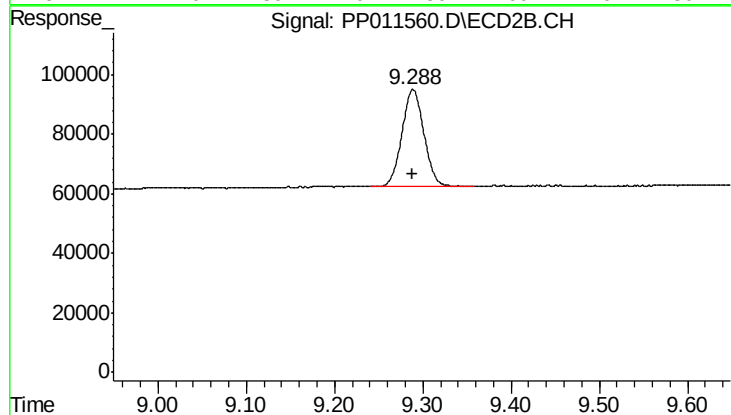

#2 Decachlorobiphenyl

R.T.: 9.289 min
Delta R.T.: 0.000 min
Response: 568066
Conc: 10.00 ng/ml