

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074853.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 12:57
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1660 WATER LOD 25PPB
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:58:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.658	3.799	25225414	93462531	20.614	19.329
2)	SA Decachlor...	10.442	8.812	19687032	116.3E6	19.936	15.504
Target Compounds							
3)	L1 AR-1016-1	5.809	4.895	1320710	12054106	29.956	23.665
4)	L1 AR-1016-2	5.831	4.953	1949991	5356559	31.030	22.505 #
5)	L1 AR-1016-3	5.894	5.073	1521914	3283383	33.885	23.809 #
6)	L1 AR-1016-4	5.991	5.117	1063070	4578764	30.216	32.751
7)	L1 AR-1016-5	6.284	5.329	957127	3283147	28.841	19.768 #
8)	L2 AR-1221-1	4.857	4.000	521475	315069	29.641	5.093 #
9)	L2 AR-1221-2	4.958	4.091	560542	1710392	41.966	37.830
10)	L2 AR-1221-3	5.018	4.173	652601	2494434	17.213	15.183
11)	L3 AR-1232-1	5.018	4.173	652601	2494434	21.486	19.473
12)	L3 AR-1232-2	5.545	4.895	936673	12054106	59.440	52.004
13)	L3 AR-1232-3	5.831	5.073	1949991	3283383	63.843	54.669
14)	L3 AR-1232-4	5.991	5.156	1063070	3276099	61.558	44.447 #
15)	L3 AR-1232-5	6.086	5.329	1367243	3283147	105.327	52.883 #
16)	L4 AR-1242-1	5.809	4.895	1320710	12054106	34.506	28.581
17)	L4 AR-1242-2	5.831	4.953	1949991	5356559	34.524	26.745
18)	L4 AR-1242-3	5.894	5.073	1521914	3283383	37.483	27.755 #
19)	L4 AR-1242-4	5.991	5.156	1063070	3276099	33.491	19.141 #
20)	L4 AR-1242-5	6.724	5.679	1019261	4969197	28.257	26.837
21)	L5 AR-1248-1	5.809	4.895	1320710	12054106	43.697	43.652
22)	L5 AR-1248-2	6.086	5.117	1367243	4578764	31.725	25.905
23)	L5 AR-1248-3	6.284	5.156	957127	3276099	20.494	14.419 #
24)	L5 AR-1248-4	6.658	5.329	1978156	3283147	35.966	15.059 #
25)	L5 AR-1248-5	6.724	5.757f	1019261	16137456	18.375	43.933 #
26)	L6 AR-1254-1	6.658	5.679	1978156	4969197	33.948	10.424 #
27)	L6 AR-1254-2	6.875	5.829	1028933	5309582	12.607	15.078
28)	L6 AR-1254-3	7.231	6.241	2184330	7770334	24.486	12.537 #
29)	L6 AR-1254-4	7.521	6.460	541353	1333328	8.213	2.845 #
30)	L6 AR-1254-5	7.934	6.871	3166851	9238878	38.116	18.836 #
31)	L7 AR-1260-1	7.401	6.360	1698798	8706209	29.386	23.203
32)	L7 AR-1260-2	7.655	6.545	2307942	15227953	33.488	28.796
33)	L7 AR-1260-3	8.013	6.700	1897617	8070305	36.573	18.638 #
34)	L7 AR-1260-4	8.241	7.171	2111191	7596288	33.095	19.913 #
35)	L7 AR-1260-5	8.567	7.409	3514976	17101758	30.993	17.025 #
36)	L8 AR-1262-1	8.241	6.910	2111191	10430243	27.412	14.747 #
37)	L8 AR-1262-2	8.567	7.171	3514976	7596288	26.552	14.588 #
38)	L8 AR-1262-3	8.899	7.696	2166011	5794439	22.281	12.427 #
39)	L8 AR-1262-4	8.965	7.754	1274483	15267548	16.919	18.577
40)	L8 AR-1262-5	9.653	8.252	996072	3509529	16.341	9.795 #
41)	L9 AR-1268-1	8.899	7.696	2166011	5794439	13.367	4.108 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 12:57
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1660 WATER LOD 25PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:58:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.965	7.754	1274483	15267548	8.685	11.198 #
43)	L9 AR-1268-3	9.228	7.963	151829	894114	1.229	0.857 #
44)	L9 AR-1268-4	9.653	8.252	996072	3509529	14.809	9.161 #
45)	L9 AR-1268-5	10.087	8.554	321934	1967036	0.870	0.627 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074853.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 12:57
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1660 WATER LOD 25PPB
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:58:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

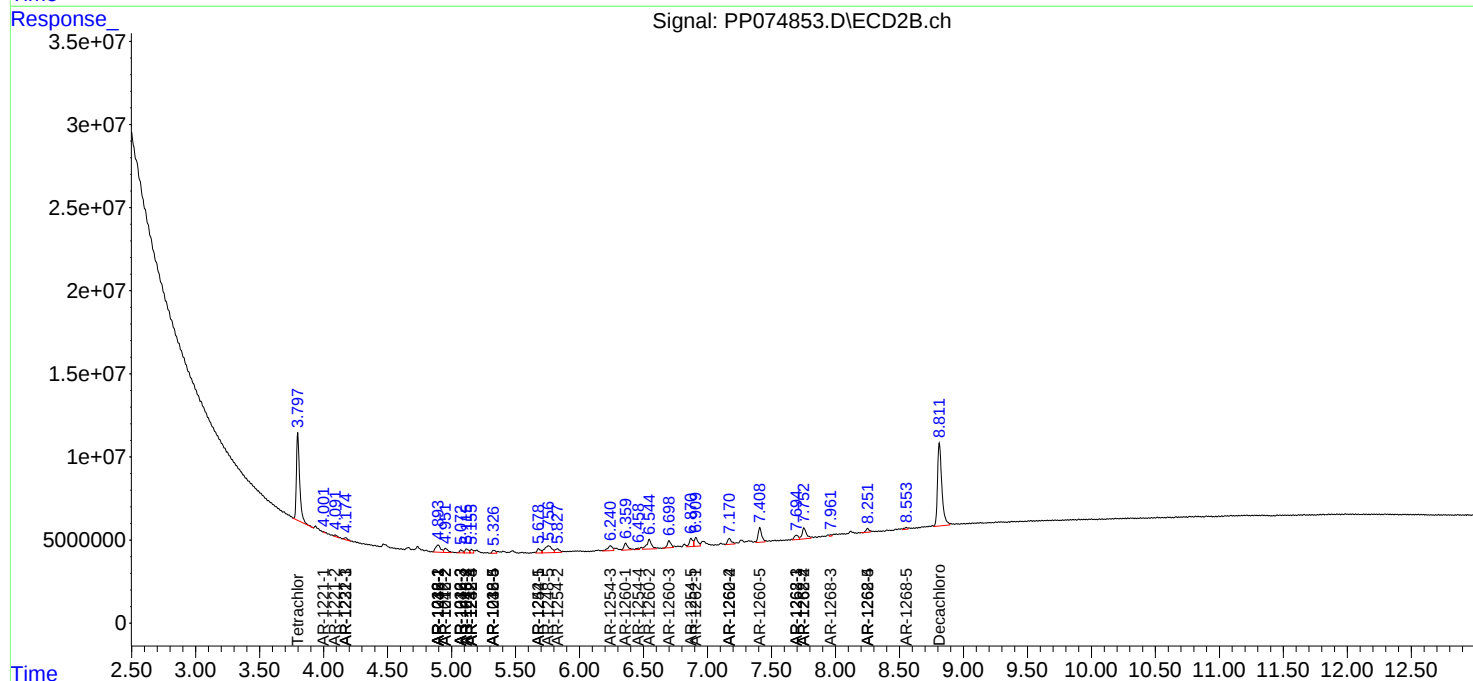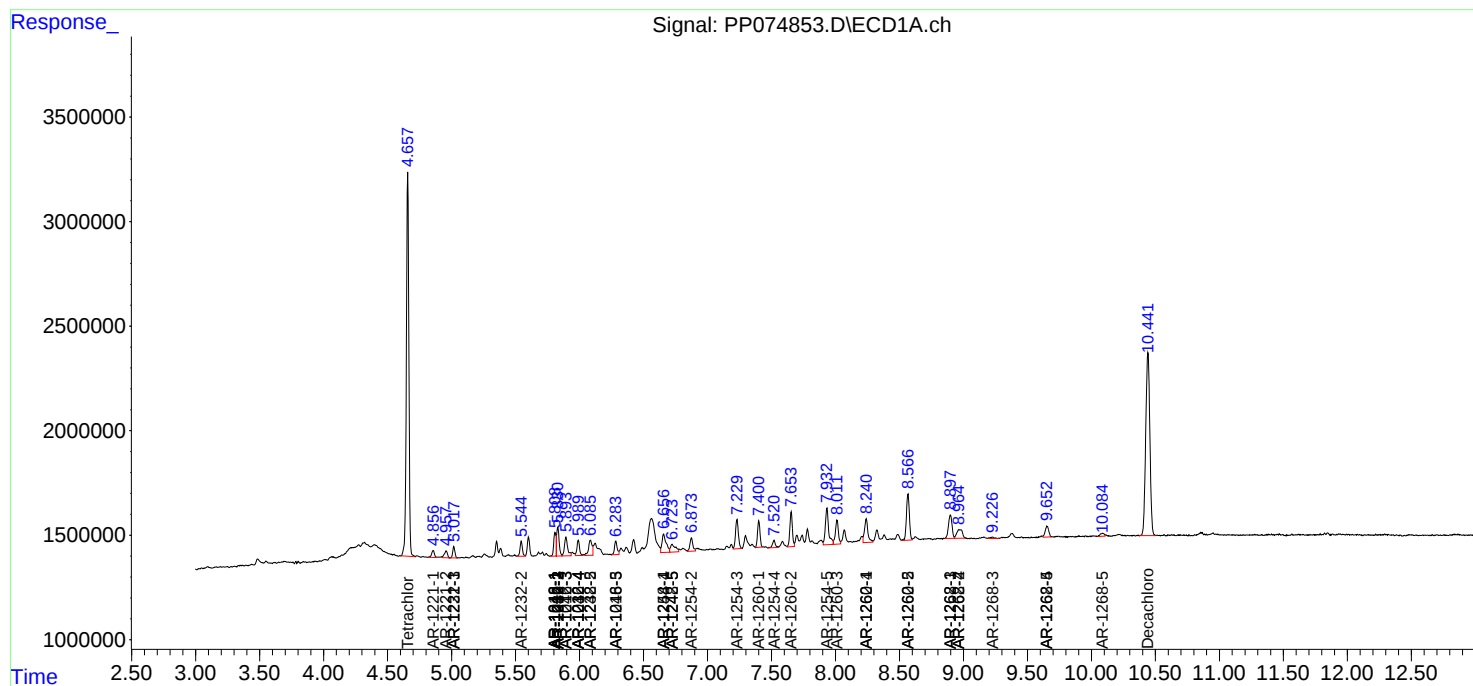


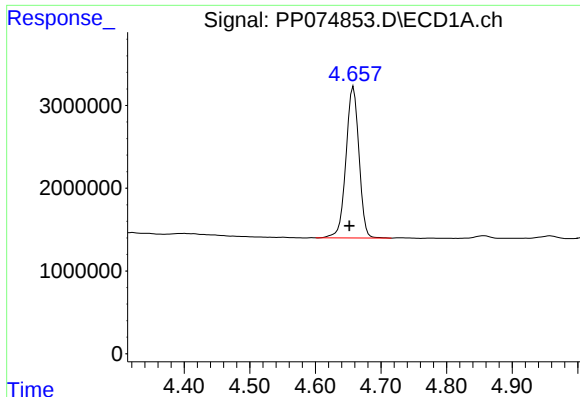

#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: 0.006 min
Response: 25225414
Conc: 20.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

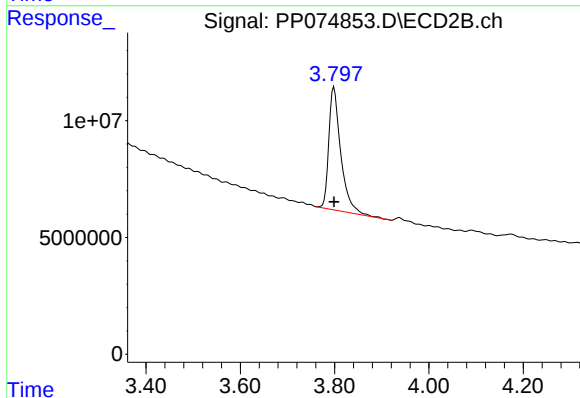


#1 Tetrachloro-m-xylene

R.T.: 3.799 min
Delta R.T.: 0.000 min
Response: 93462531
Conc: 19.33 ng/ml

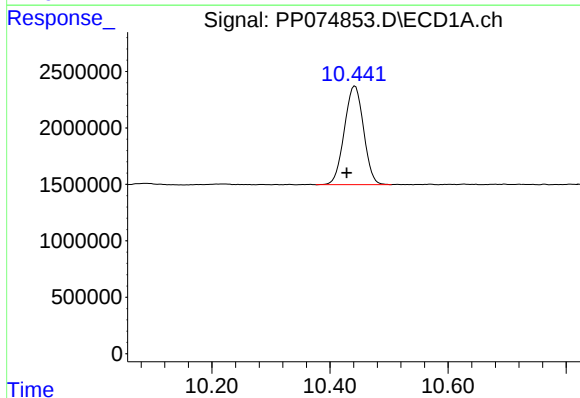


#2 Decachlorobiphenyl

R.T.: 10.442 min
Delta R.T.: 0.014 min
Response: 19687032
Conc: 19.94 ng/ml

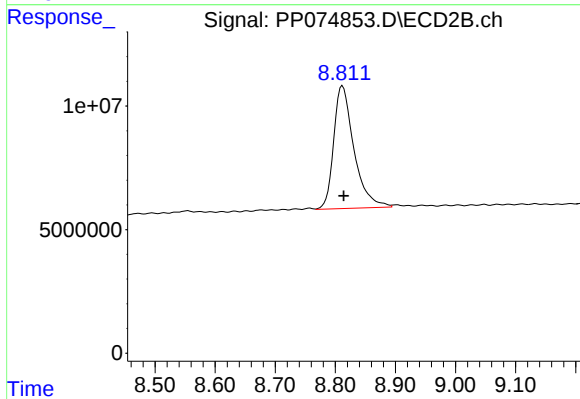

#2 Decachlorobiphenyl


R.T.: 8.812 min
Delta R.T.: -0.002 min
Response: 116264318
Conc: 15.50 ng/ml

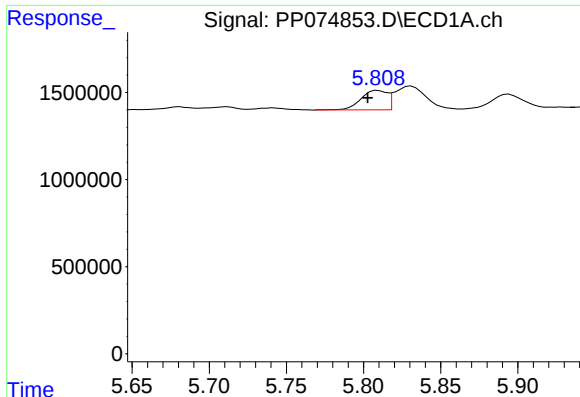

#3 AR-1016-1


R.T.: 5.809 min
Delta R.T.: 0.007 min
Response: 1320710
Conc: 29.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

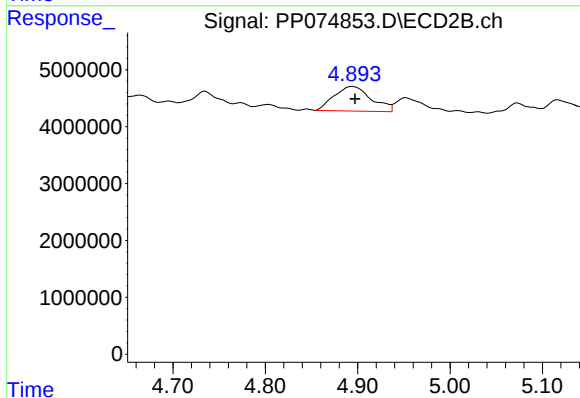


#3 AR-1016-1

R.T.: 4.895 min
Delta R.T.: -0.003 min
Response: 12054106
Conc: 23.67 ng/ml

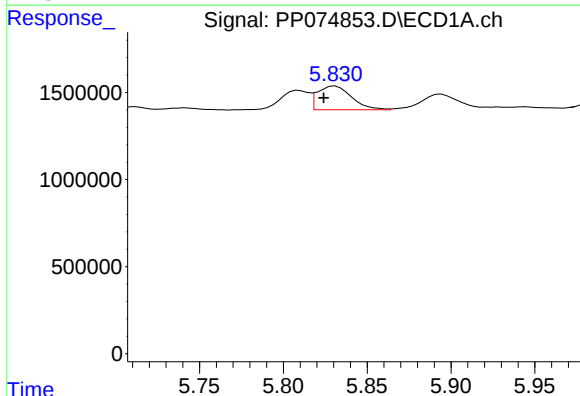


#4 AR-1016-2

R.T.: 5.831 min
Delta R.T.: 0.007 min
Response: 1949991
Conc: 31.03 ng/ml

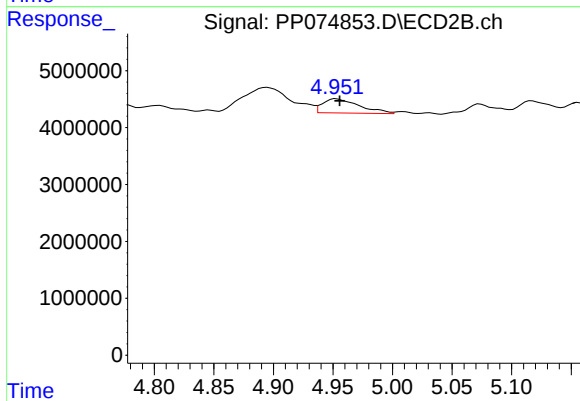

#4 AR-1016-2


R.T.: 4.953 min
Delta R.T.: -0.003 min
Response: 5356559
Conc: 22.51 ng/ml

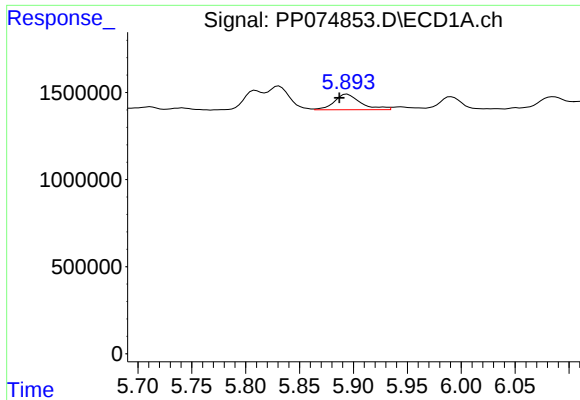

#5 AR-1016-3


R.T.: 5.894 min
Delta R.T.: 0.007 min
Response: 1521914
Conc: 33.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

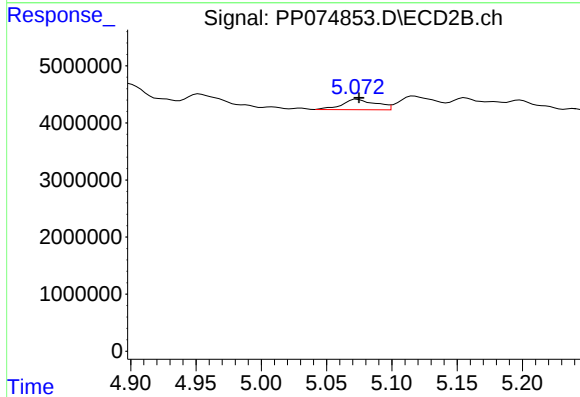


#5 AR-1016-3

R.T.: 5.073 min
Delta R.T.: -0.002 min
Response: 3283383
Conc: 23.81 ng/ml

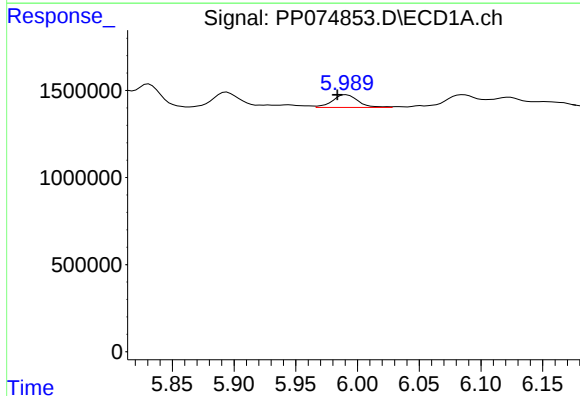


#6 AR-1016-4

R.T.: 5.991 min
Delta R.T.: 0.007 min
Response: 1063070
Conc: 30.22 ng/ml

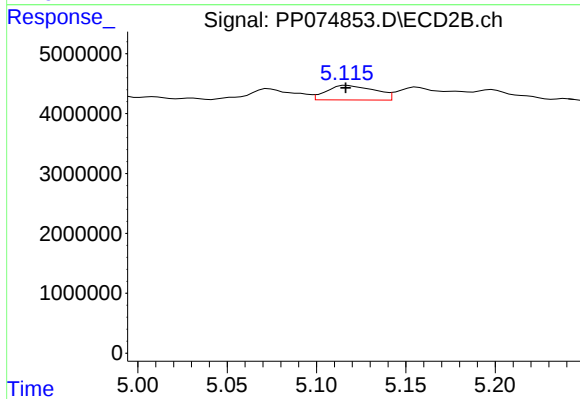

#6 AR-1016-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 4578764
Conc: 32.75 ng/ml

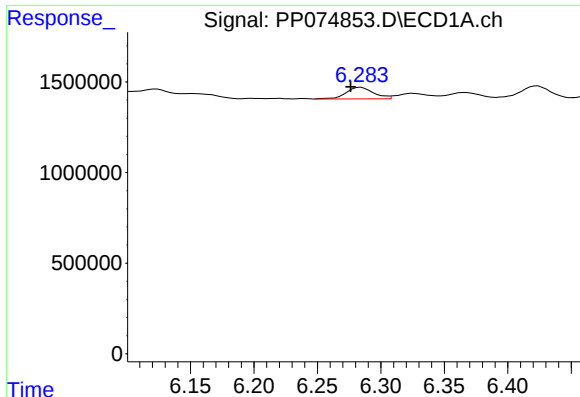

#7 AR-1016-5


R.T.: 6.284 min
Delta R.T.: 0.008 min
Response: 957127
Conc: 28.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

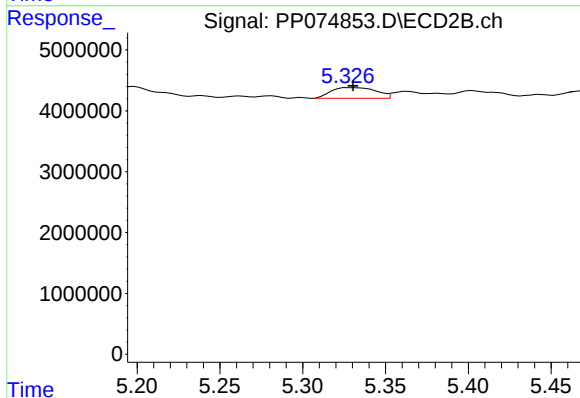


#7 AR-1016-5

R.T.: 5.329 min
Delta R.T.: 0.000 min
Response: 3283147
Conc: 19.77 ng/ml

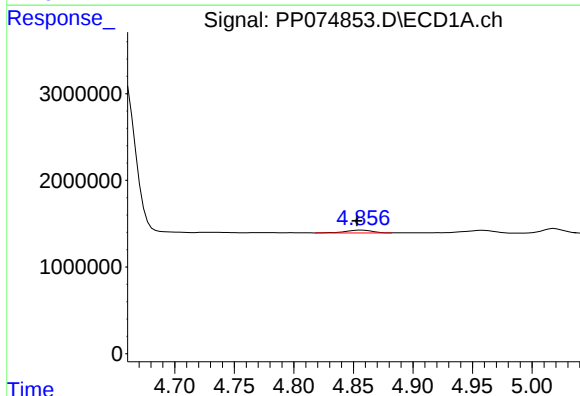


#8 AR-1221-1

R.T.: 4.857 min
Delta R.T.: 0.004 min
Response: 521475
Conc: 29.64 ng/ml

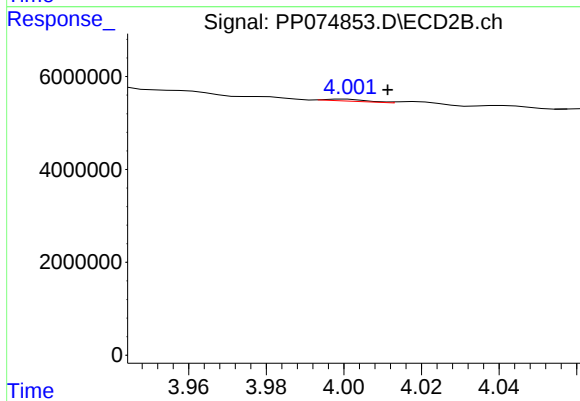

#8 AR-1221-1


R.T.: 4.000 min
Delta R.T.: -0.011 min
Response: 315069
Conc: 5.09 ng/ml

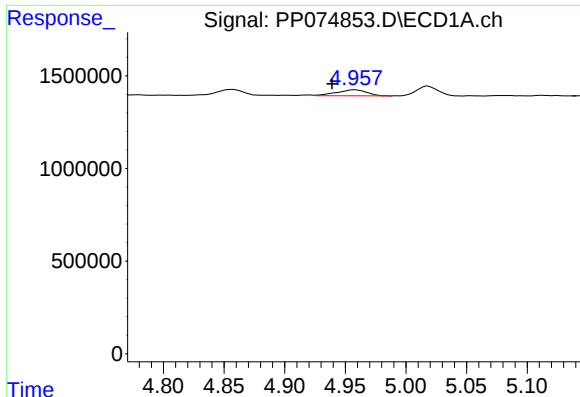

#9 AR-1221-2


R.T.: 4.958 min
Delta R.T.: 0.019 min
Response: 560542
Conc: 41.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

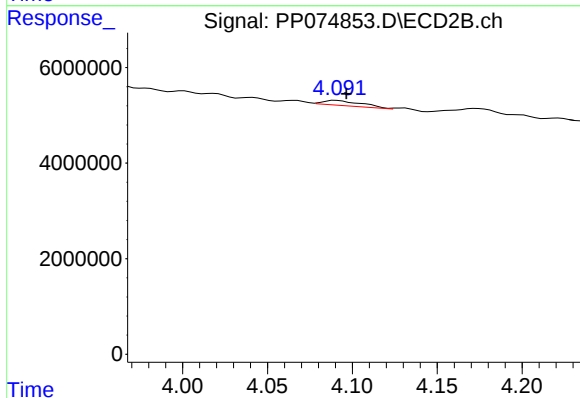


#9 AR-1221-2

R.T.: 4.091 min
Delta R.T.: -0.006 min
Response: 1710392
Conc: 37.83 ng/ml

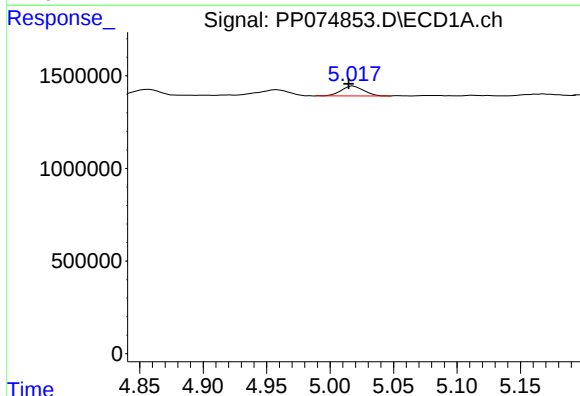


#10 AR-1221-3

R.T.: 5.018 min
Delta R.T.: 0.004 min
Response: 652601
Conc: 17.21 ng/ml

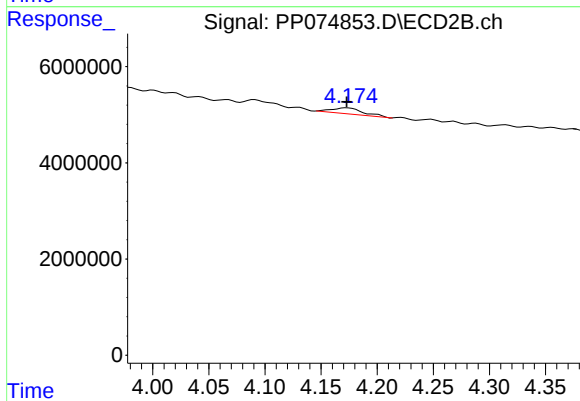

#10 AR-1221-3


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 2494434
Conc: 15.18 ng/ml

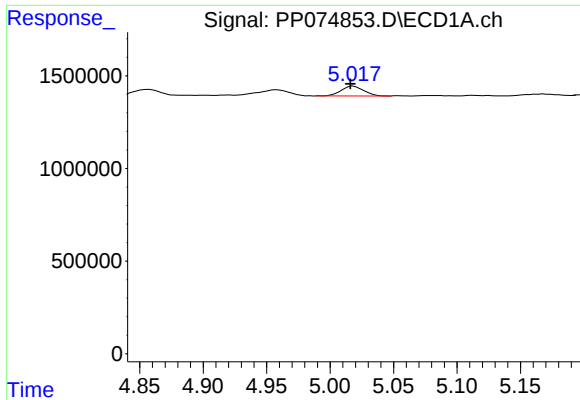

#11 AR-1232-1


R.T.: 5.018 min
Delta R.T.: 0.002 min
Response: 652601
Conc: 21.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

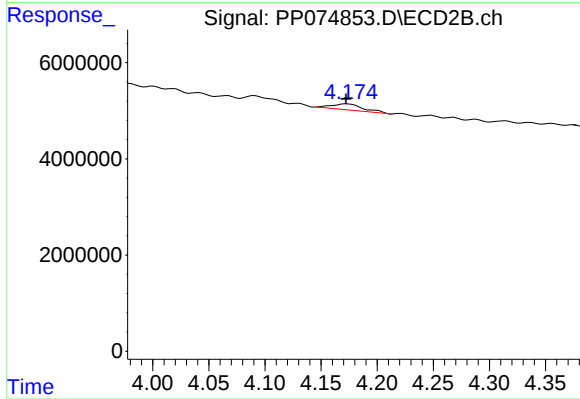


#11 AR-1232-1

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 2494434
Conc: 19.47 ng/ml

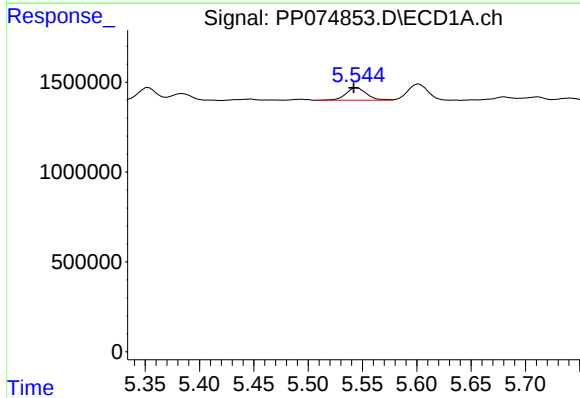


#12 AR-1232-2

R.T.: 5.545 min
Delta R.T.: 0.003 min
Response: 936673
Conc: 59.44 ng/ml

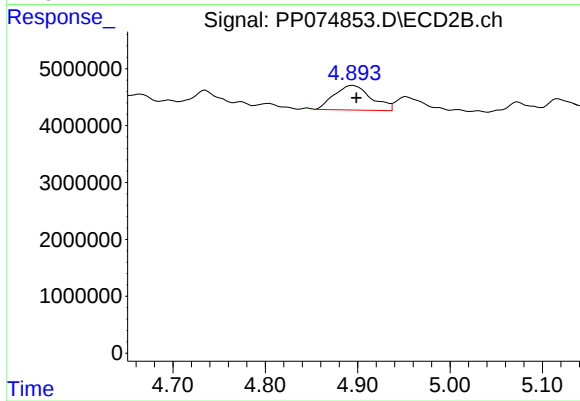

#12 AR-1232-2


R.T.: 4.895 min
Delta R.T.: -0.004 min
Response: 12054106
Conc: 52.00 ng/ml

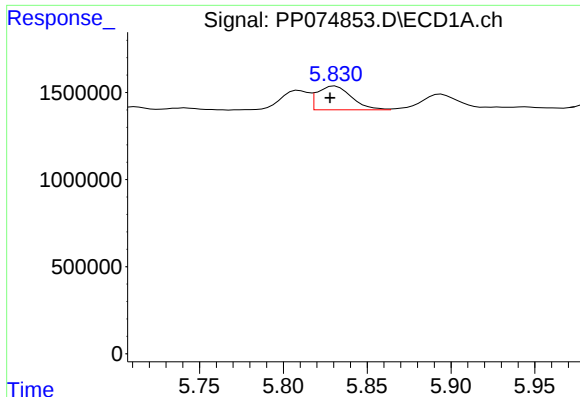

#13 AR-1232-3


R.T.: 5.831 min
Delta R.T.: 0.003 min
Response: 1949991
Conc: 63.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

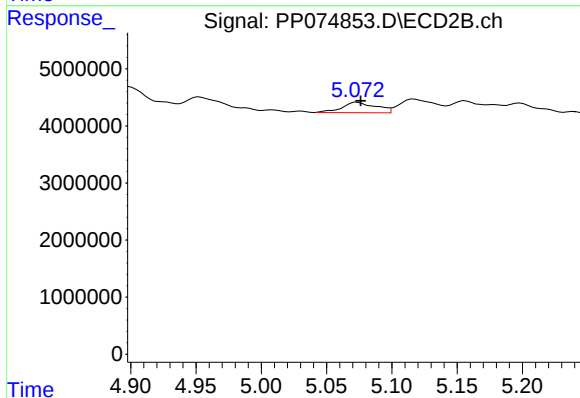


#13 AR-1232-3

R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 3283383
Conc: 54.67 ng/ml

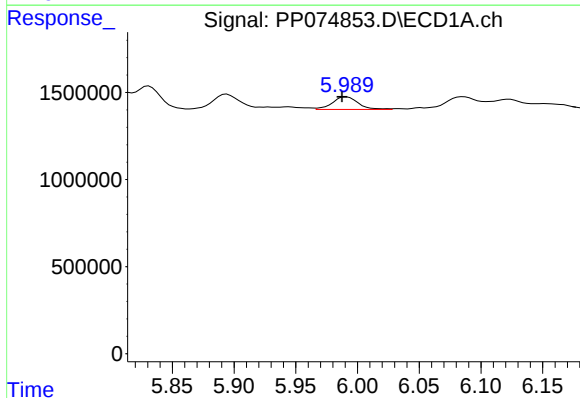


#14 AR-1232-4

R.T.: 5.991 min
Delta R.T.: 0.003 min
Response: 1063070
Conc: 61.56 ng/ml

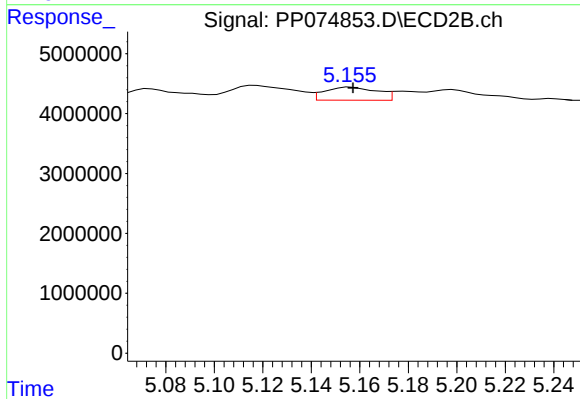

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: -0.001 min
Response: 3276099
Conc: 44.45 ng/ml

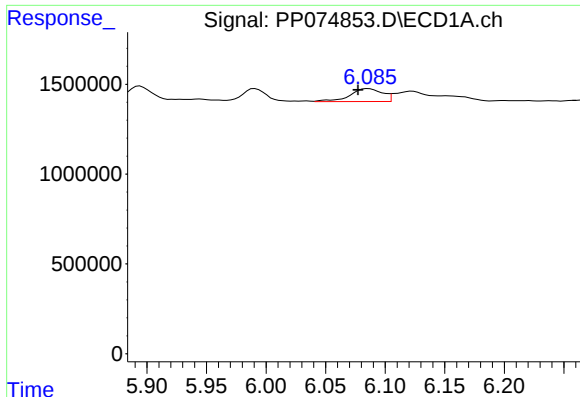

#15 AR-1232-5


R.T.: 6.086 min
Delta R.T.: 0.009 min
Response: 1367243
Conc: 105.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

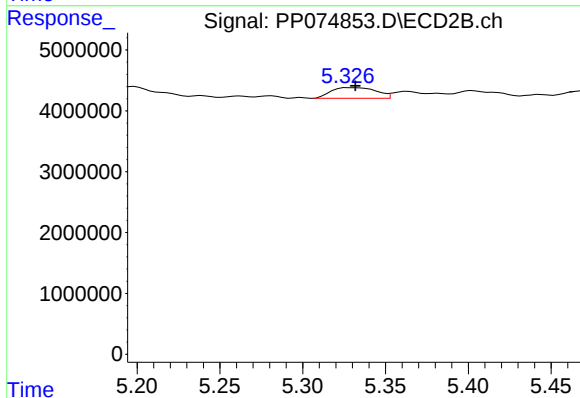


#15 AR-1232-5

R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 3283147
Conc: 52.88 ng/ml

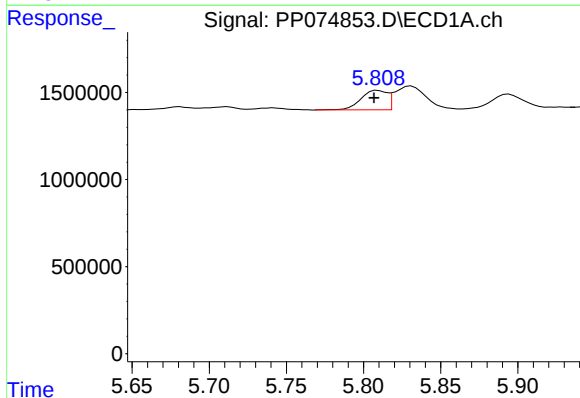


#16 AR-1242-1

R.T.: 5.809 min
Delta R.T.: 0.002 min
Response: 1320710
Conc: 34.51 ng/ml

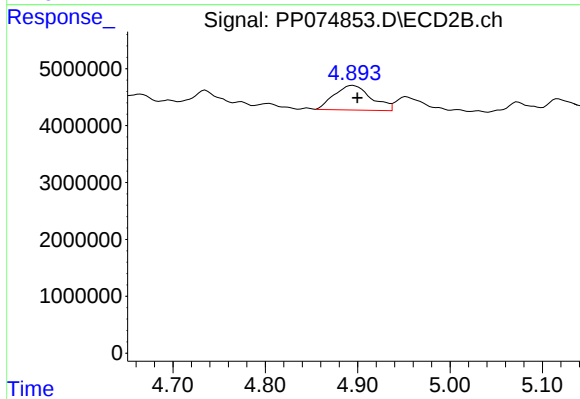

#16 AR-1242-1


R.T.: 4.895 min
Delta R.T.: -0.005 min
Response: 12054106
Conc: 28.58 ng/ml

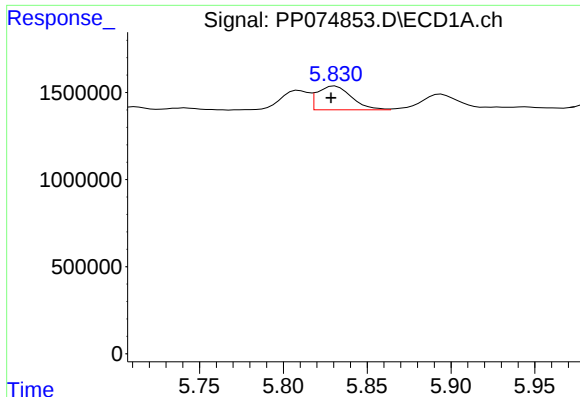

#17 AR-1242-2


R.T.: 5.831 min
Delta R.T.: 0.003 min
Response: 1949991
Conc: 34.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

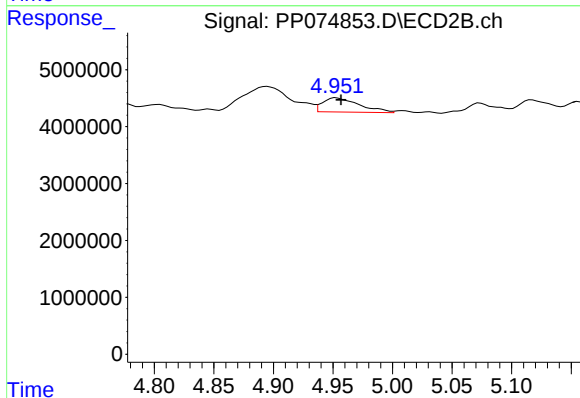


#17 AR-1242-2

R.T.: 4.953 min
Delta R.T.: -0.004 min
Response: 5356559
Conc: 26.75 ng/ml

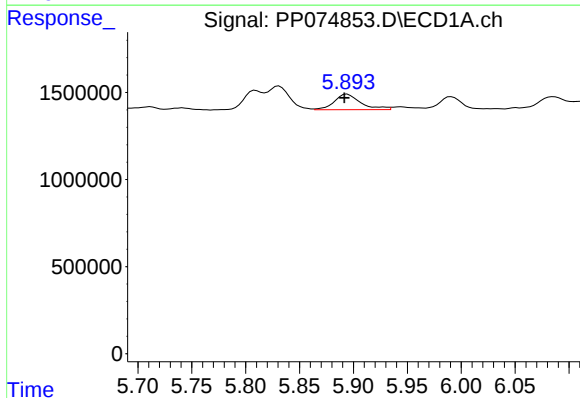


#18 AR-1242-3

R.T.: 5.894 min
Delta R.T.: 0.003 min
Response: 1521914
Conc: 37.48 ng/ml

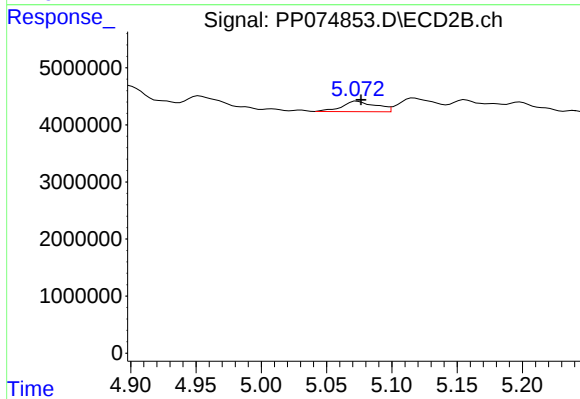

#18 AR-1242-3


R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 3283383
Conc: 27.76 ng/ml

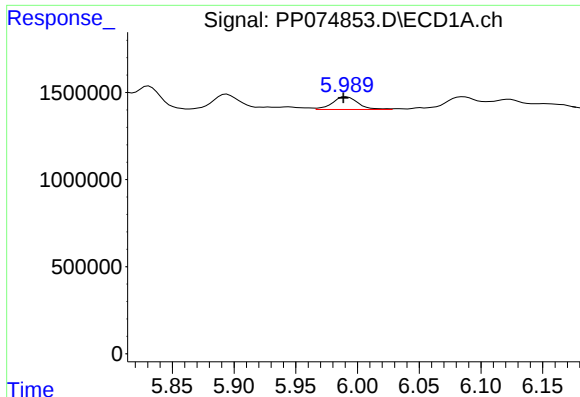

#19 AR-1242-4


R.T.: 5.991 min
Delta R.T.: 0.002 min
Response: 1063070
Conc: 33.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

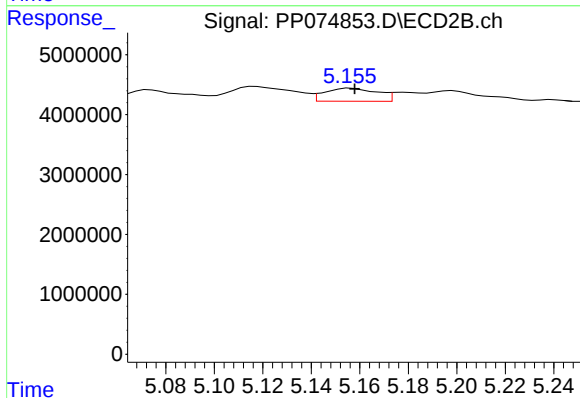


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 3276099
Conc: 19.14 ng/ml

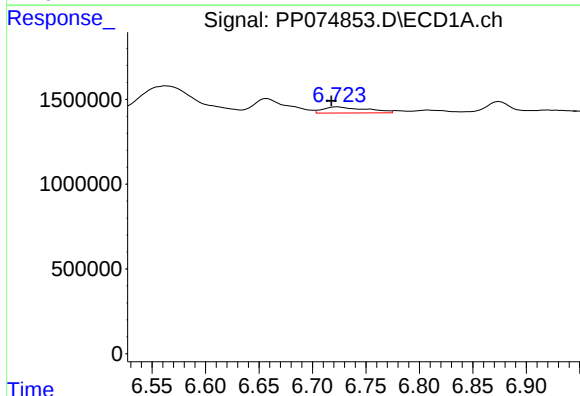


#20 AR-1242-5

R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 1019261
Conc: 28.26 ng/ml

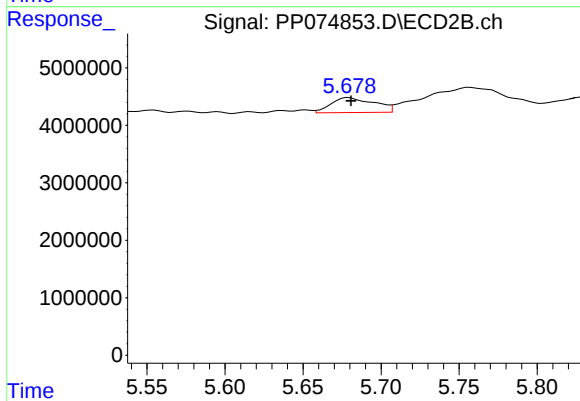

#20 AR-1242-5


R.T.: 5.679 min
Delta R.T.: -0.001 min
Response: 4969197
Conc: 26.84 ng/ml

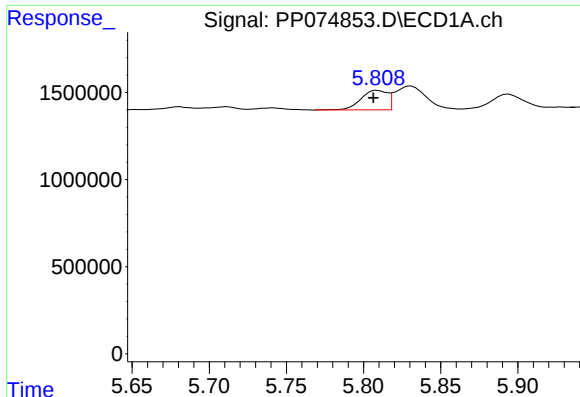

#21 AR-1248-1


R.T.: 5.809 min
Delta R.T.: 0.003 min
Response: 1320710
Conc: 43.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

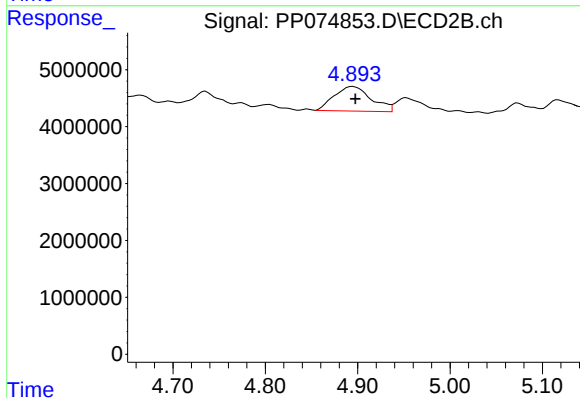


#21 AR-1248-1

R.T.: 4.895 min
Delta R.T.: -0.003 min
Response: 12054106
Conc: 43.65 ng/ml

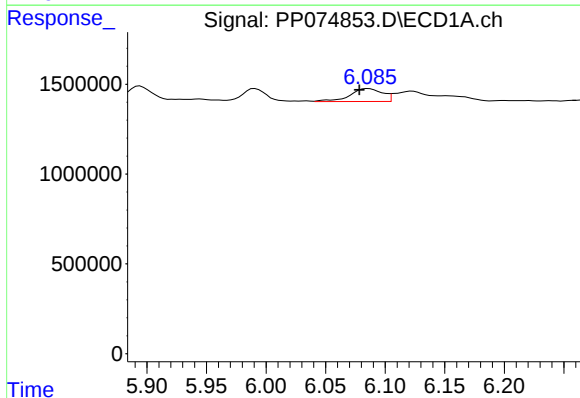


#22 AR-1248-2

R.T.: 6.086 min
Delta R.T.: 0.008 min
Response: 1367243
Conc: 31.73 ng/ml

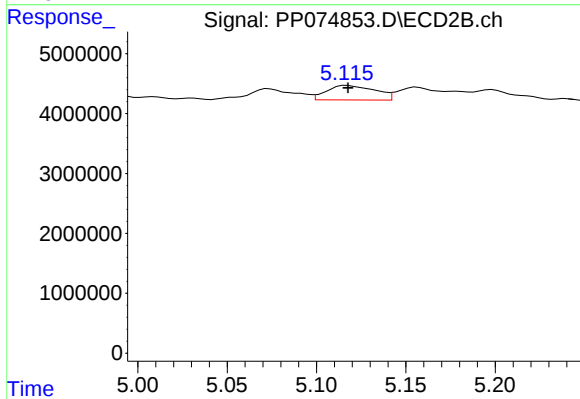

#22 AR-1248-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 4578764
Conc: 25.90 ng/ml

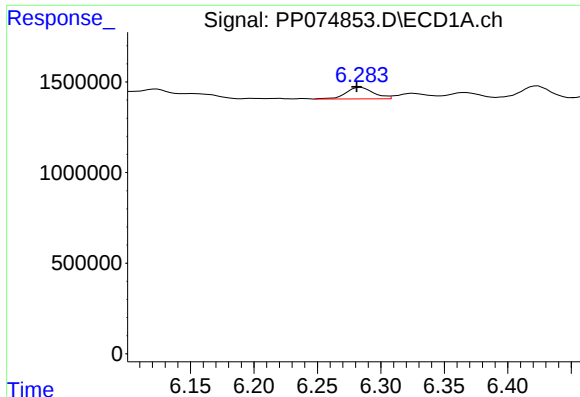

#23 AR-1248-3


R.T.: 6.284 min
Delta R.T.: 0.003 min
Response: 957127
Conc: 20.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

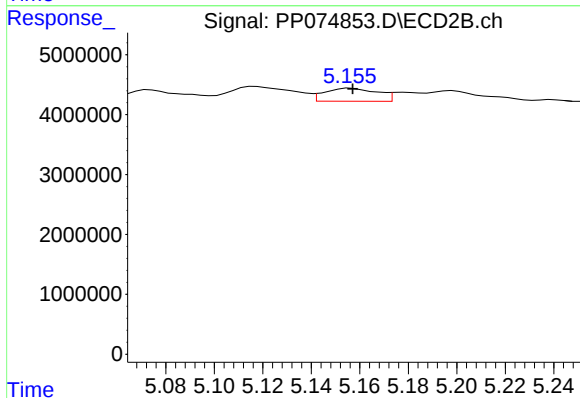


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: 0.000 min
Response: 3276099
Conc: 14.42 ng/ml

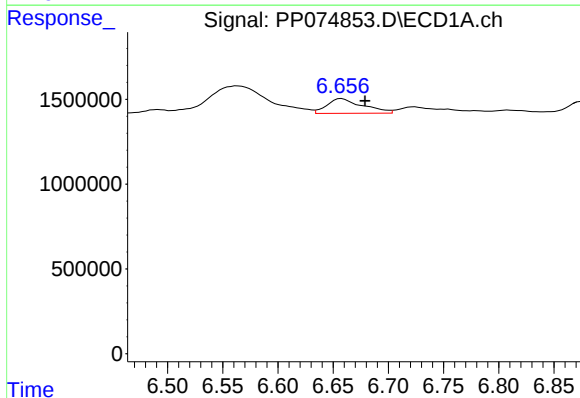


#24 AR-1248-4

R.T.: 6.658 min
Delta R.T.: -0.021 min
Response: 1978156
Conc: 35.97 ng/ml

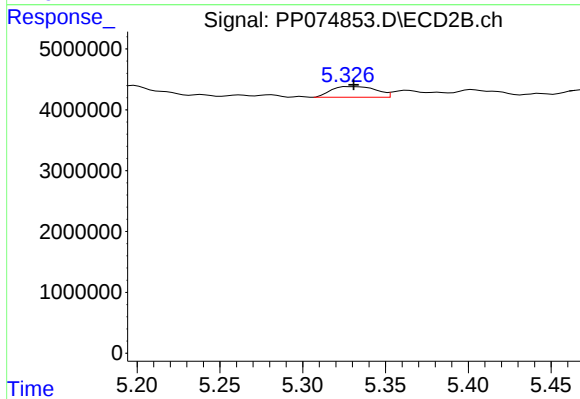

#24 AR-1248-4


R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 3283147
Conc: 15.06 ng/ml

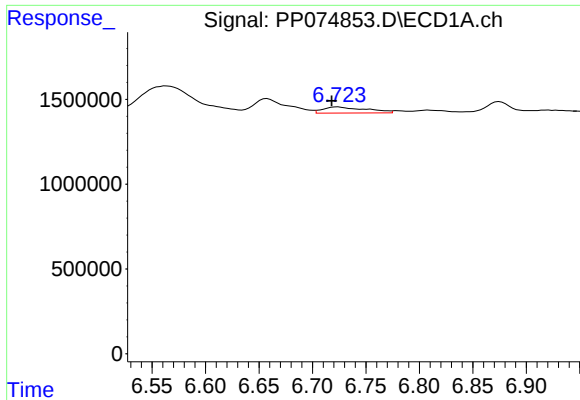

#25 AR-1248-5


R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 1019261
Conc: 18.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

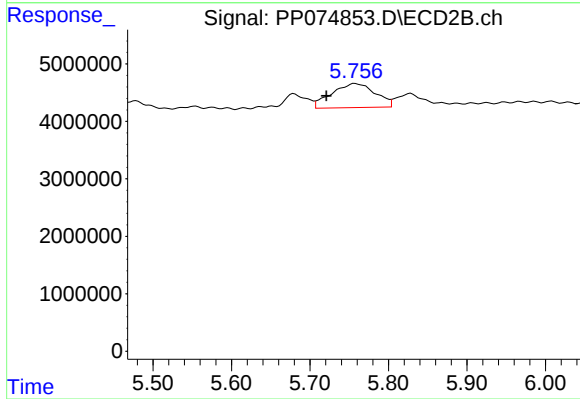


#25 AR-1248-5

R.T.: 5.757 min
Delta R.T.: 0.036 min
Response: 16137456
Conc: 43.93 ng/ml

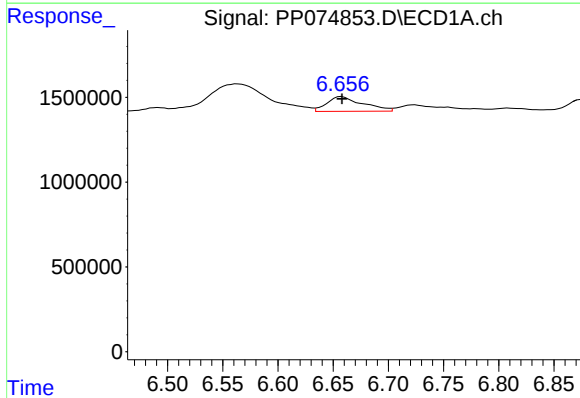


#26 AR-1254-1

R.T.: 6.658 min
Delta R.T.: 0.000 min
Response: 1978156
Conc: 33.95 ng/ml

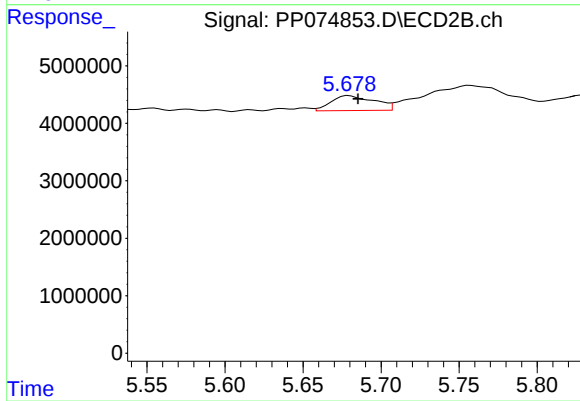

#26 AR-1254-1


R.T.: 5.679 min
Delta R.T.: -0.006 min
Response: 4969197
Conc: 10.42 ng/ml

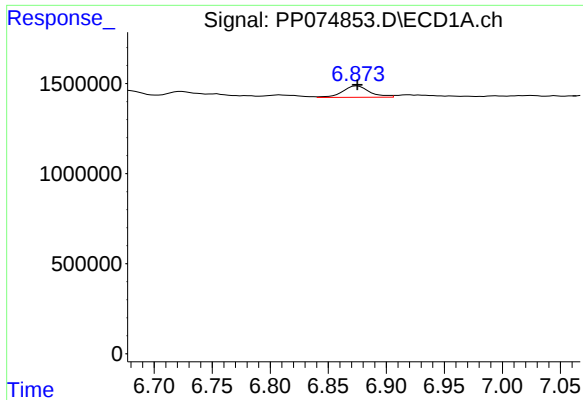

#27 AR-1254-2


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 1028933
Conc: 12.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

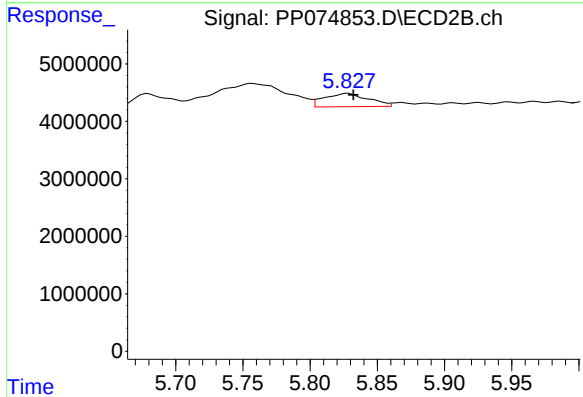


#27 AR-1254-2

R.T.: 5.829 min
Delta R.T.: -0.004 min
Response: 5309582
Conc: 15.08 ng/ml

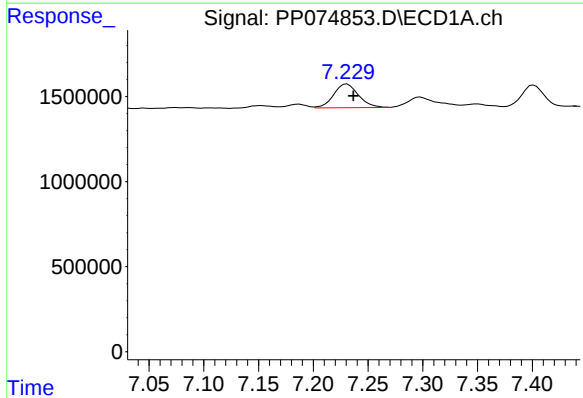


#28 AR-1254-3

R.T.: 7.231 min
Delta R.T.: -0.006 min
Response: 2184330
Conc: 24.49 ng/ml

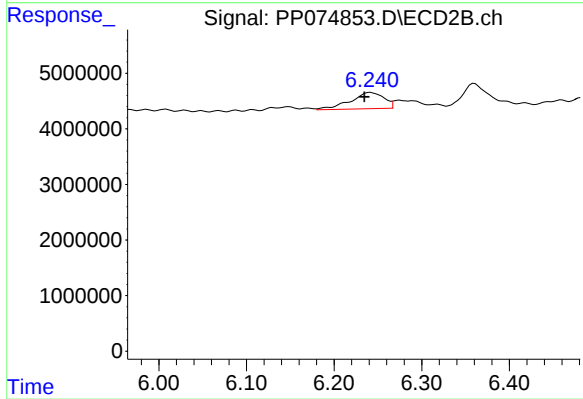

#28 AR-1254-3


R.T.: 6.241 min
Delta R.T.: 0.007 min
Response: 7770334
Conc: 12.54 ng/ml

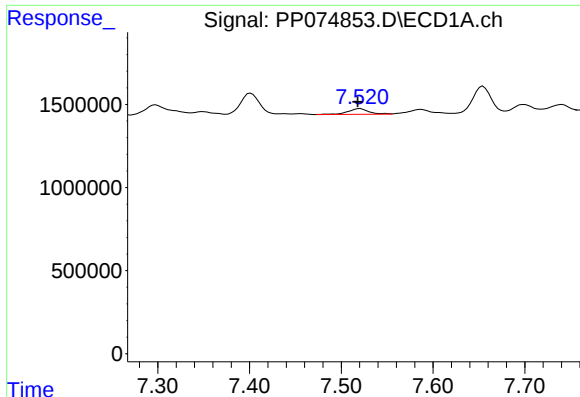

#29 AR-1254-4


R.T.: 7.521 min
Delta R.T.: 0.003 min
Response: 541353
Conc: 8.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

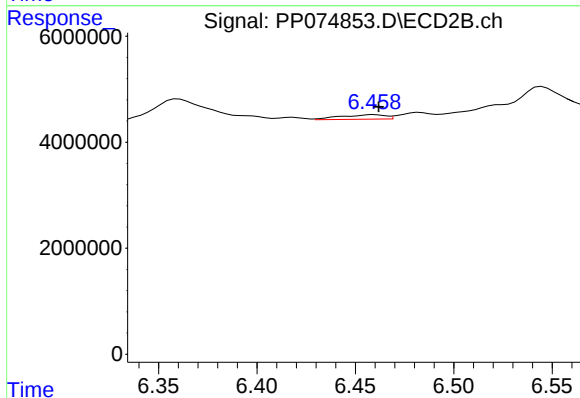


#29 AR-1254-4

R.T.: 6.460 min
Delta R.T.: -0.002 min
Response: 1333328
Conc: 2.85 ng/ml

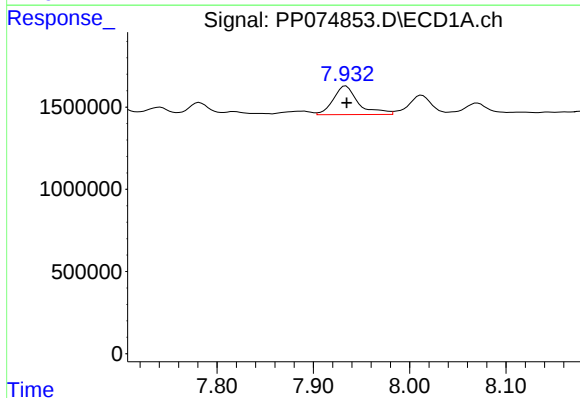


#30 AR-1254-5

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 3166851
Conc: 38.12 ng/ml

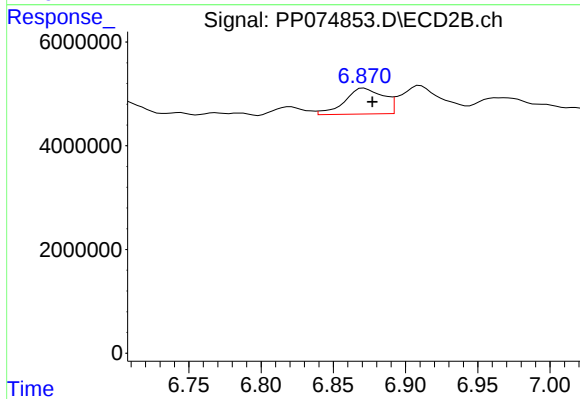

#30 AR-1254-5


R.T.: 6.871 min
Delta R.T.: -0.006 min
Response: 9238878
Conc: 18.84 ng/ml

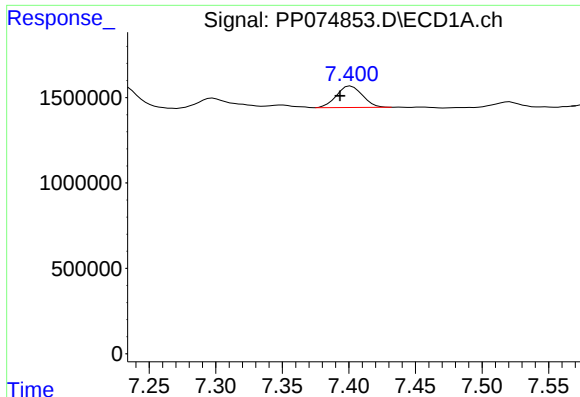

#31 AR-1260-1


R.T.: 7.401 min
Delta R.T.: 0.008 min
Response: 1698798
Conc: 29.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

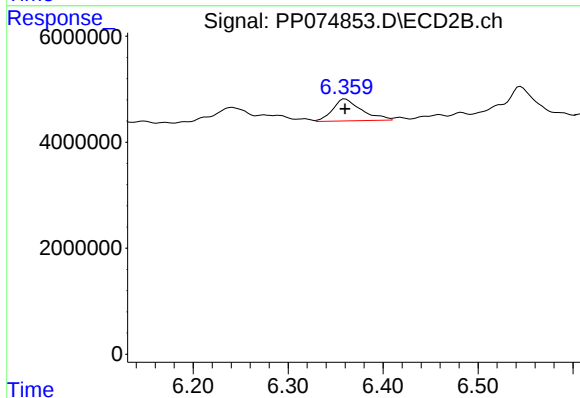


#31 AR-1260-1

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 8706209
Conc: 23.20 ng/ml

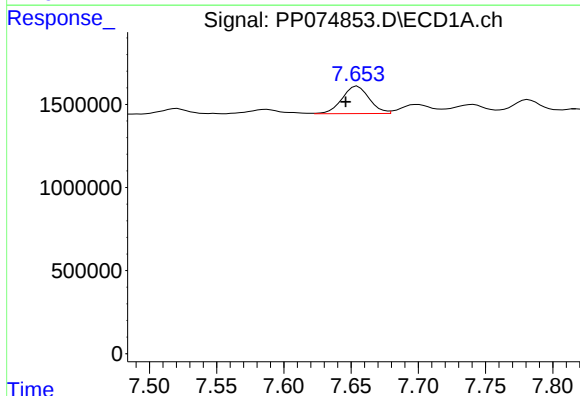


#32 AR-1260-2

R.T.: 7.655 min
Delta R.T.: 0.009 min
Response: 2307942
Conc: 33.49 ng/ml

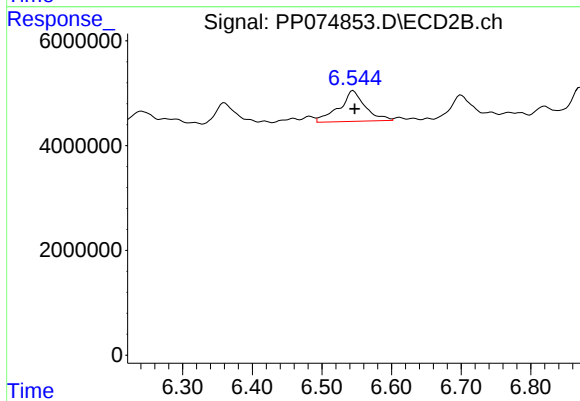

#32 AR-1260-2


R.T.: 6.545 min
Delta R.T.: -0.002 min
Response: 15227953
Conc: 28.80 ng/ml

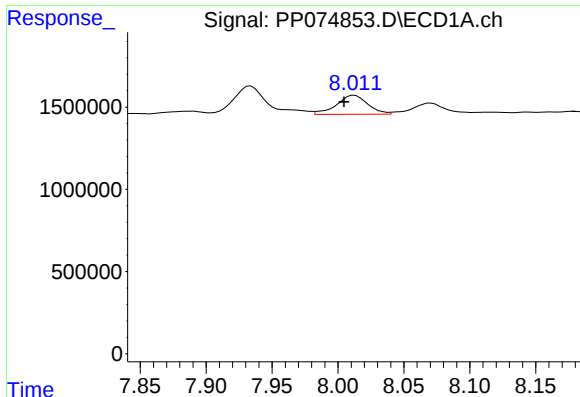

#33 AR-1260-3


R.T.: 8.013 min
Delta R.T.: 0.008 min
Response: 1897617
Conc: 36.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

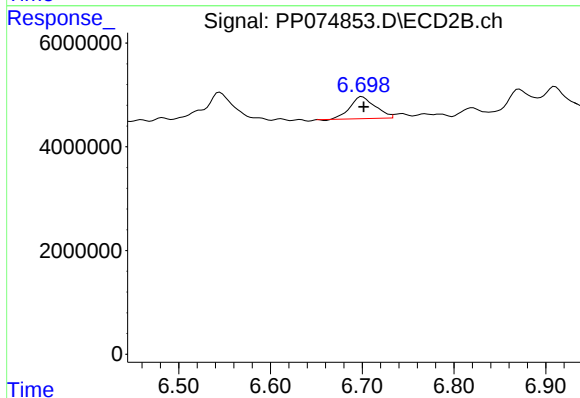


#33 AR-1260-3

R.T.: 6.700 min
Delta R.T.: -0.002 min
Response: 8070305
Conc: 18.64 ng/ml

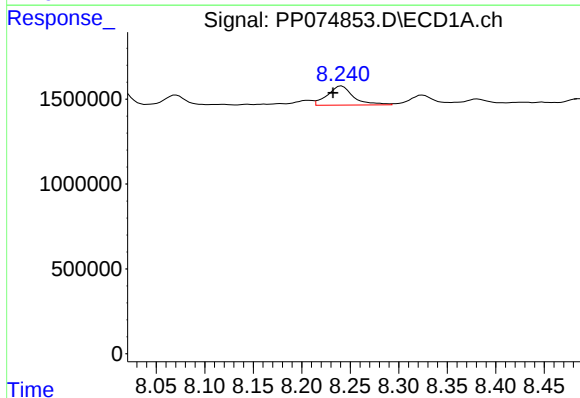


#34 AR-1260-4

R.T.: 8.241 min
Delta R.T.: 0.009 min
Response: 2111191
Conc: 33.09 ng/ml

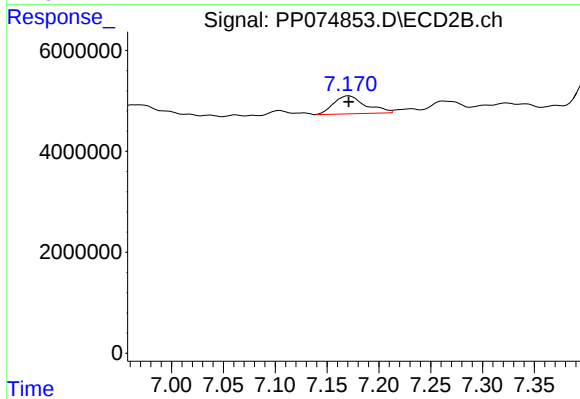

#34 AR-1260-4


R.T.: 7.171 min
Delta R.T.: 0.000 min
Response: 7596288
Conc: 19.91 ng/ml

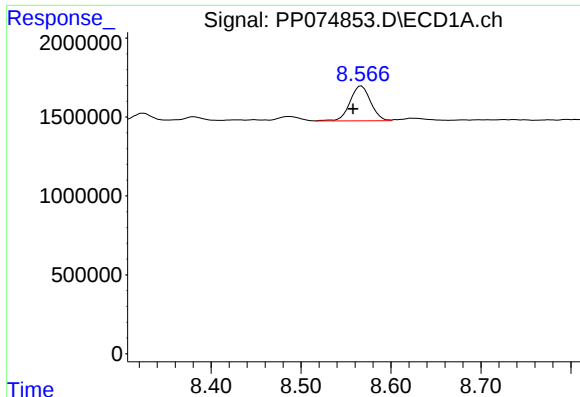

#35 AR-1260-5


R.T.: 8.567 min
Delta R.T.: 0.009 min
Response: 3514976
Conc: 30.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

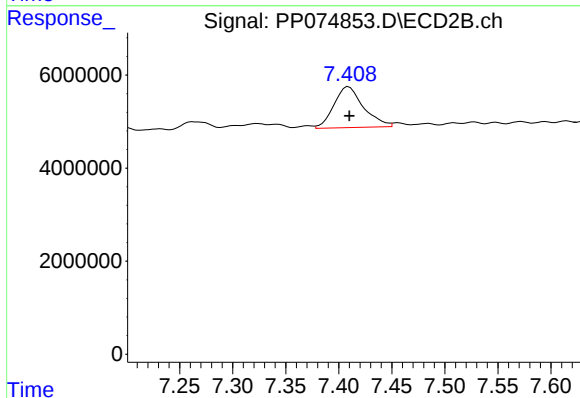


#35 AR-1260-5

R.T.: 7.409 min
Delta R.T.: 0.000 min
Response: 17101758
Conc: 17.03 ng/ml

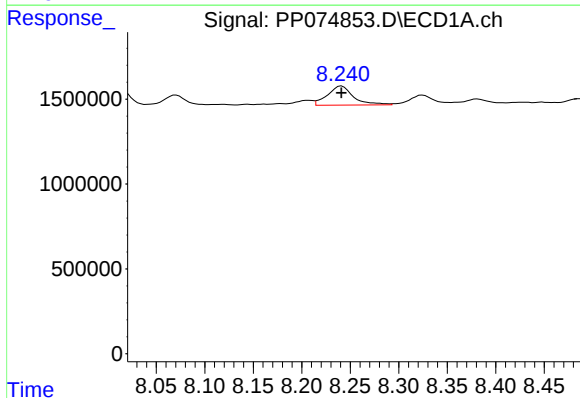


#36 AR-1262-1

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 2111191
Conc: 27.41 ng/ml

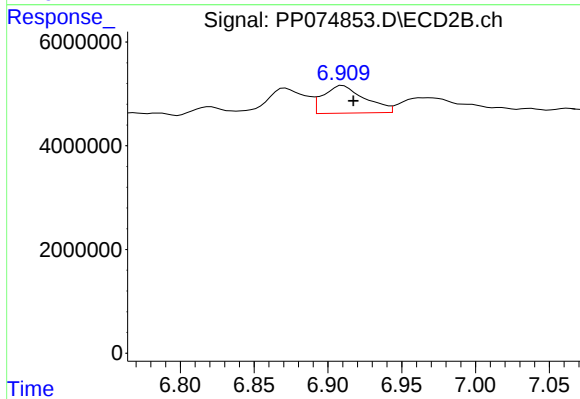

#36 AR-1262-1


R.T.: 6.910 min
Delta R.T.: -0.007 min
Response: 10430243
Conc: 14.75 ng/ml

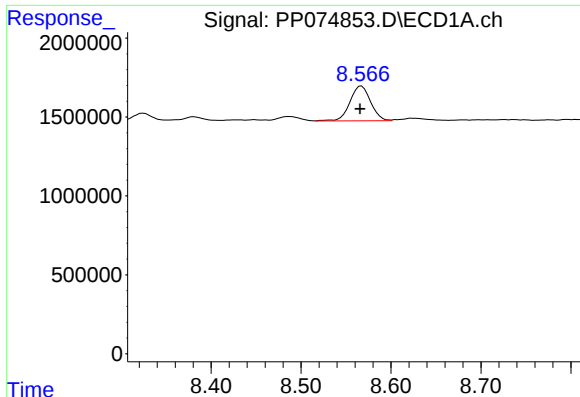

#37 AR-1262-2


R.T.: 8.567 min
Delta R.T.: 0.002 min
Response: 3514976
Conc: 26.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

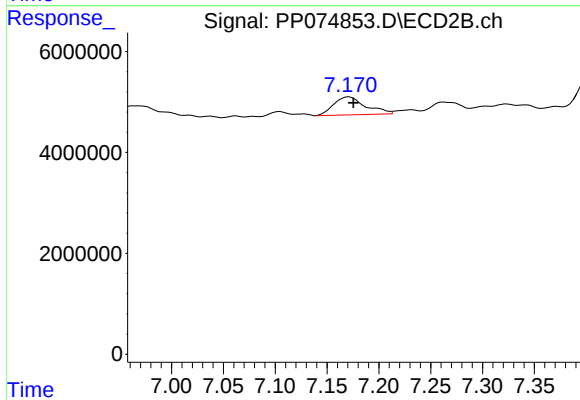


#37 AR-1262-2

R.T.: 7.171 min
Delta R.T.: -0.004 min
Response: 7596288
Conc: 14.59 ng/ml

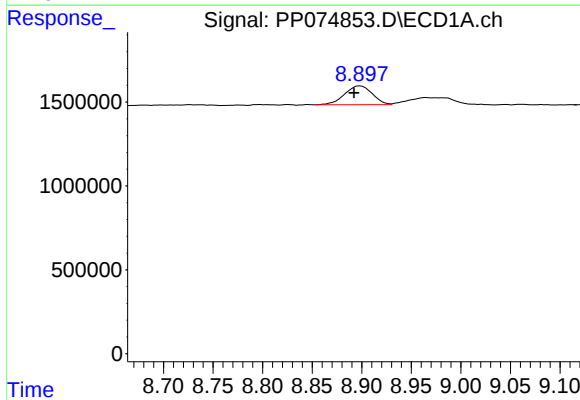


#38 AR-1262-3

R.T.: 8.899 min
Delta R.T.: 0.006 min
Response: 2166011
Conc: 22.28 ng/ml

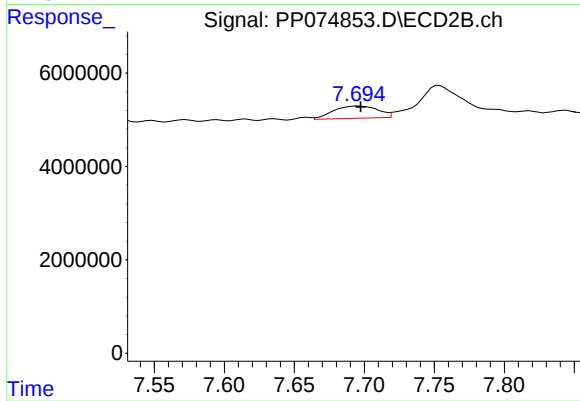

#38 AR-1262-3


R.T.: 7.696 min
Delta R.T.: -0.002 min
Response: 5794439
Conc: 12.43 ng/ml

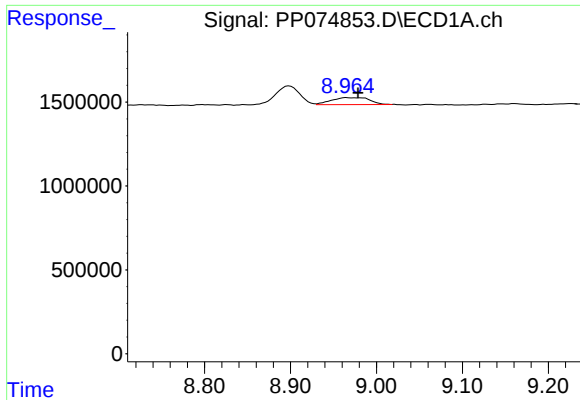

#39 AR-1262-4


R.T.: 8.965 min
Delta R.T.: -0.014 min
Response: 1274483
Conc: 16.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

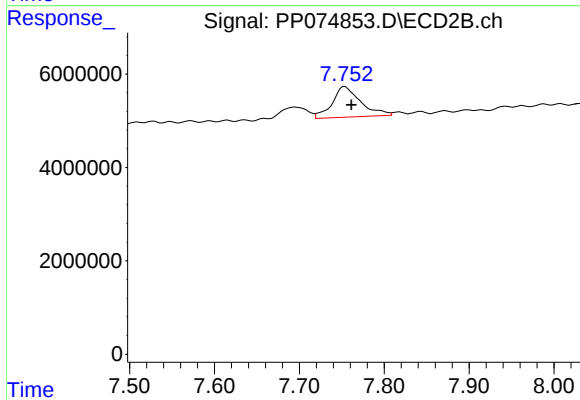


#39 AR-1262-4

R.T.: 7.754 min
Delta R.T.: -0.008 min
Response: 15267548
Conc: 18.58 ng/ml

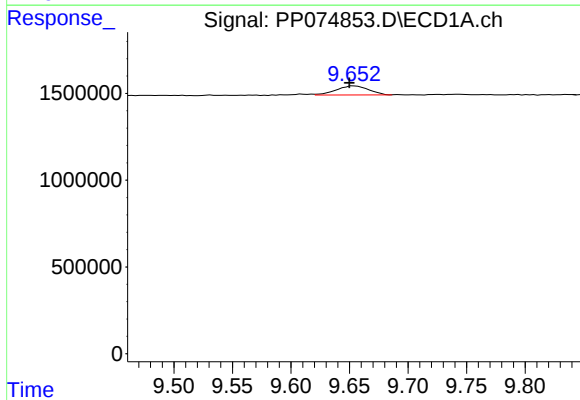


#40 AR-1262-5

R.T.: 9.653 min
Delta R.T.: 0.003 min
Response: 996072
Conc: 16.34 ng/ml

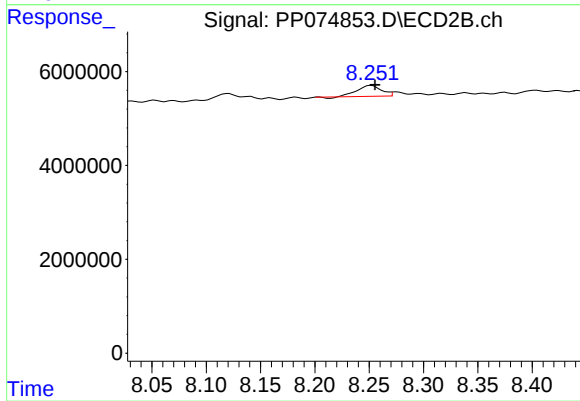

#40 AR-1262-5


R.T.: 8.252 min
Delta R.T.: -0.003 min
Response: 3509529
Conc: 9.79 ng/ml

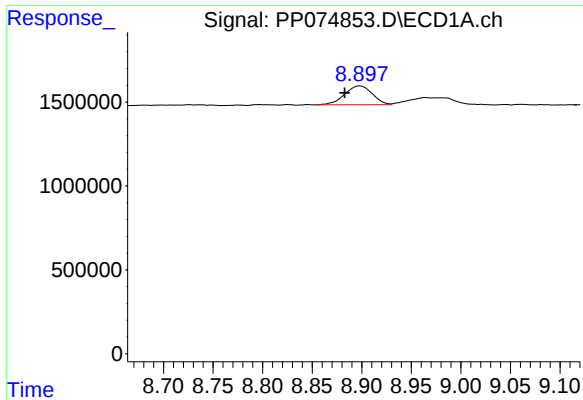

#41 AR-1268-1


R.T.: 8.899 min
Delta R.T.: 0.016 min
Response: 2166011
Conc: 13.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

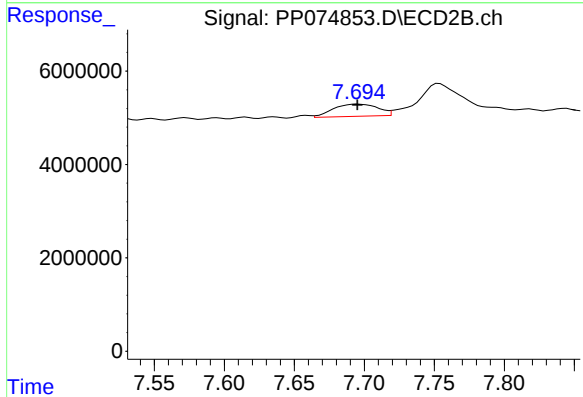


#41 AR-1268-1

R.T.: 7.696 min
Delta R.T.: 0.000 min
Response: 5794439
Conc: 4.11 ng/ml

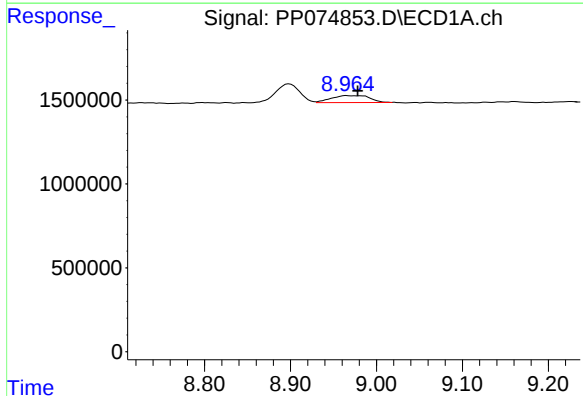


#42 AR-1268-2

R.T.: 8.965 min
Delta R.T.: -0.013 min
Response: 1274483
Conc: 8.69 ng/ml

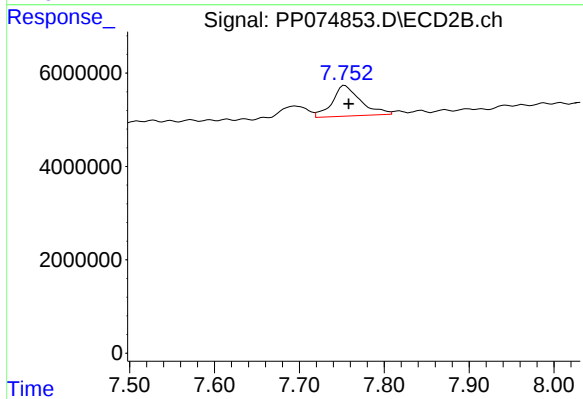

#42 AR-1268-2


R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 15267548
Conc: 11.20 ng/ml

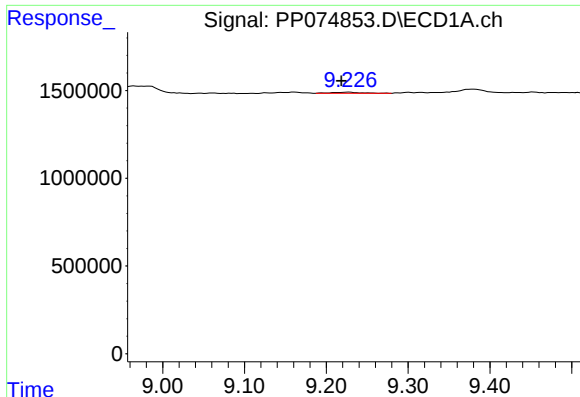

#43 AR-1268-3


R.T.: 9.228 min
Delta R.T.: 0.009 min
Response: 151829
Conc: 1.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

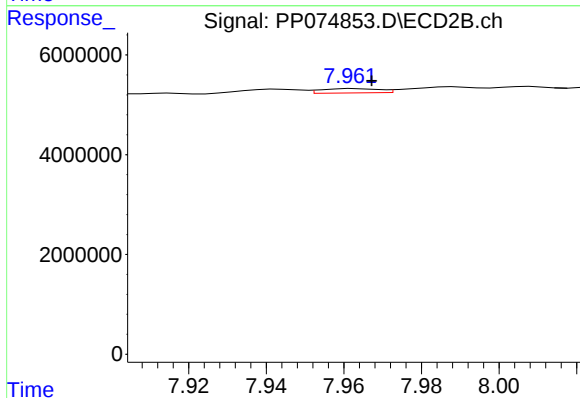


#43 AR-1268-3

R.T.: 7.963 min
Delta R.T.: -0.005 min
Response: 894114
Conc: 0.86 ng/ml

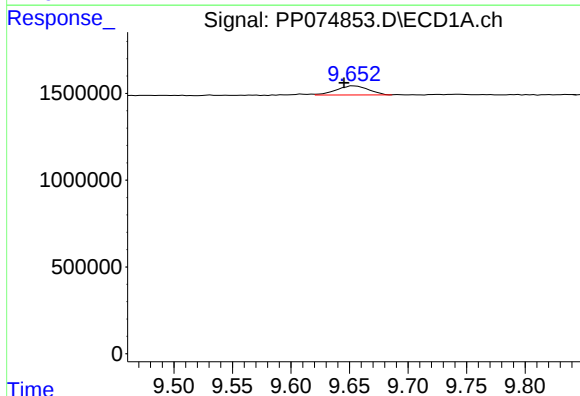


#44 AR-1268-4

R.T.: 9.653 min
Delta R.T.: 0.008 min
Response: 996072
Conc: 14.81 ng/ml

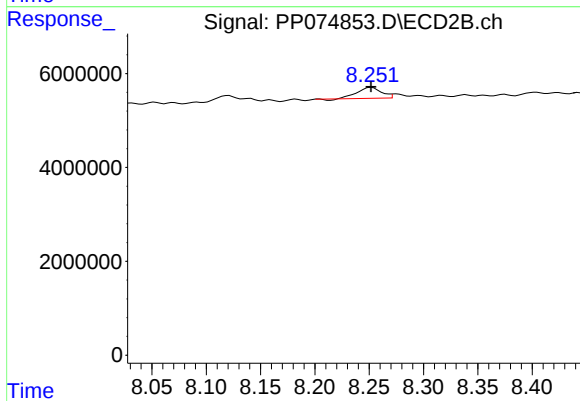

#44 AR-1268-4


R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 3509529
Conc: 9.16 ng/ml

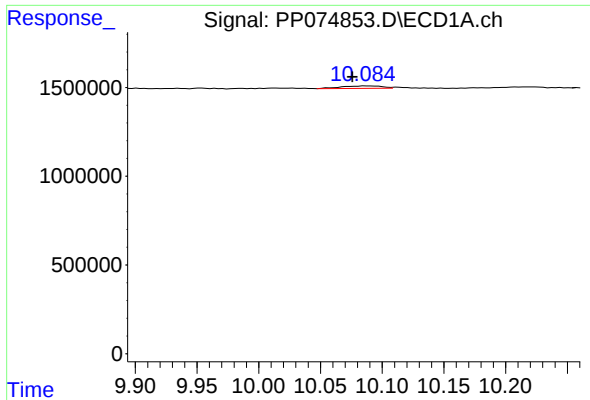

#45 AR-1268-5

R.T.: 10.087 min
Delta R.T.: 0.011 min
Response: 321934
Conc: 0.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

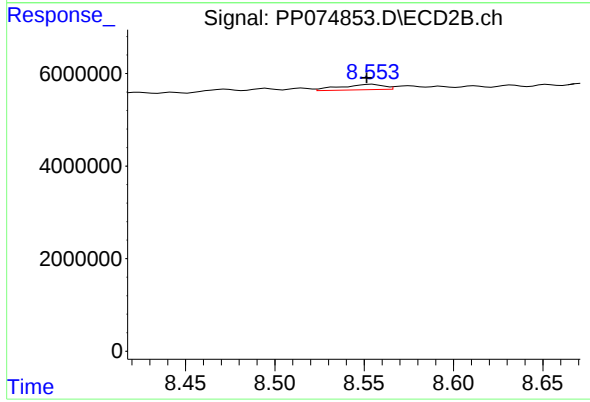

#45 AR-1268-5

R.T.: 8.554 min
Delta R.T.: 0.003 min
Response: 1967036
Conc: 0.63 ng/ml