

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 13:13
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1221 WATER LOD 25PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:59:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.661	3.802	25574579	91213305	20.900	18.864
2)	SA Decachlor...	10.446	8.816	19969451	117.0E6	20.222	15.604
Target Compounds							
3)	L1 AR-1016-1	5.810	4.898	134178	443468	3.043	0.871 #
4)	L1 AR-1016-2	5.837	4.958	169150	605942	2.692	2.546
5)	L1 AR-1016-3	5.895	5.065	259061	217394	5.768	1.576 #
6)	L1 AR-1016-4	5.944f	5.125	378702	1010619	10.764	7.229 #
7)	L1 AR-1016-5	6.304	5.325	144853	317173	4.365	1.910 #
8)	L2 AR-1221-1	4.863	4.013	479605	1136410	27.261	18.368 #
9)	L2 AR-1221-2	4.963	4.094	673933	1843881	50.455	40.783
10)	L2 AR-1221-3	5.022	4.172	874804	3458391	23.074	21.050
11)	L3 AR-1232-1	5.022	4.172	874804	3458391	28.801	26.999
12)	L3 AR-1232-2	5.495f	4.898	146925	443468	9.324	1.913 #
13)	L3 AR-1232-3	5.837	5.085	169150	205211	5.538	3.417 #
14)	L3 AR-1232-4	5.944f	5.165	378702	589792	21.929	8.002 #
15)	L3 AR-1232-5	6.115f	5.325	637114	317173	49.081	5.109 #
16)	L4 AR-1242-1	5.810	4.898	134178	443468	3.506	1.051 #
17)	L4 AR-1242-2	5.837	4.958	169150	605942	2.995	3.025
18)	L4 AR-1242-3	5.895	5.085	259061	205211	6.380	1.735 #
19)	L4 AR-1242-4	5.944f	5.165	378702	589792	11.931	3.446 #
20)	L4 AR-1242-5	6.705	5.682	103651	634549	2.874	3.427
21)	L5 AR-1248-1	5.810	4.898	134178	443468	4.439	1.606 #
22)	L5 AR-1248-2	6.115f	5.125	637114	1010619	14.784	5.718 #
23)	L5 AR-1248-3	6.304	5.165	144853	589792	3.102	2.596
24)	L5 AR-1248-4	6.660	5.325	806481	317173	14.663	1.455 #
25)	L5 AR-1248-5	6.705	5.703	103651	905163	1.869	2.464 #
26)	L6 AR-1254-1	6.660	5.682	806481	634549	13.841	1.331 #
27)	L6 AR-1254-2	6.880	5.823	282094	1139430	3.456	3.236
28)	L6 AR-1254-3	7.233	6.237	2406108	1073327	26.972	1.732 #
29)	L6 AR-1254-4	7.523	6.459	293950	543240	4.460	1.159 #
30)	L6 AR-1254-5	7.935	6.881	377564	733007	4.544	1.494 #
31)	L7 AR-1260-1	7.398	6.358	15014	532202	0.260	1.418 #
32)	L7 AR-1260-2	7.659	6.563	226488	461030	3.286	0.872 #
33)	L7 AR-1260-3	8.004	6.705	149908	576366	2.889	1.331 #
34)	L7 AR-1260-4	8.226	7.178	62572	144124	0.981	0.378 #
35)	L7 AR-1260-5	0.000	7.403	0	411252	N.D.	0.409 #
36)	L8 AR-1262-1	8.226	6.922	62572	373408	0.812	0.528 #
37)	L8 AR-1262-2	0.000	7.178	0	144124	N.D.	0.277 #
38)	L8 AR-1262-3	0.000	7.697	0	957468	N.D.	2.053 #
39)	L8 AR-1262-4	0.000	7.763	0	1005208	N.D.	1.223 #
40)	L8 AR-1262-5	9.660	8.263	13452	407280	0.221	1.137 #
41)	L9 AR-1268-1	0.000	7.697	0	957468	N.D.	0.679 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074854.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 13:13
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1221 WATER LOD 25PPB
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:59:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.763	0	1005208	N.D.	0.737 #
43) L9	AR-1268-3	9.157f	7.979	148574	1195732	1.202	1.146
44) L9	AR-1268-4	9.660	8.263	13452	407280	0.200	1.063 #
45) L9	AR-1268-5	10.096	8.559	178083	615270	0.481	0.196 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074854.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 13:13
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1221 WATER LOD 25PPB
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:59:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

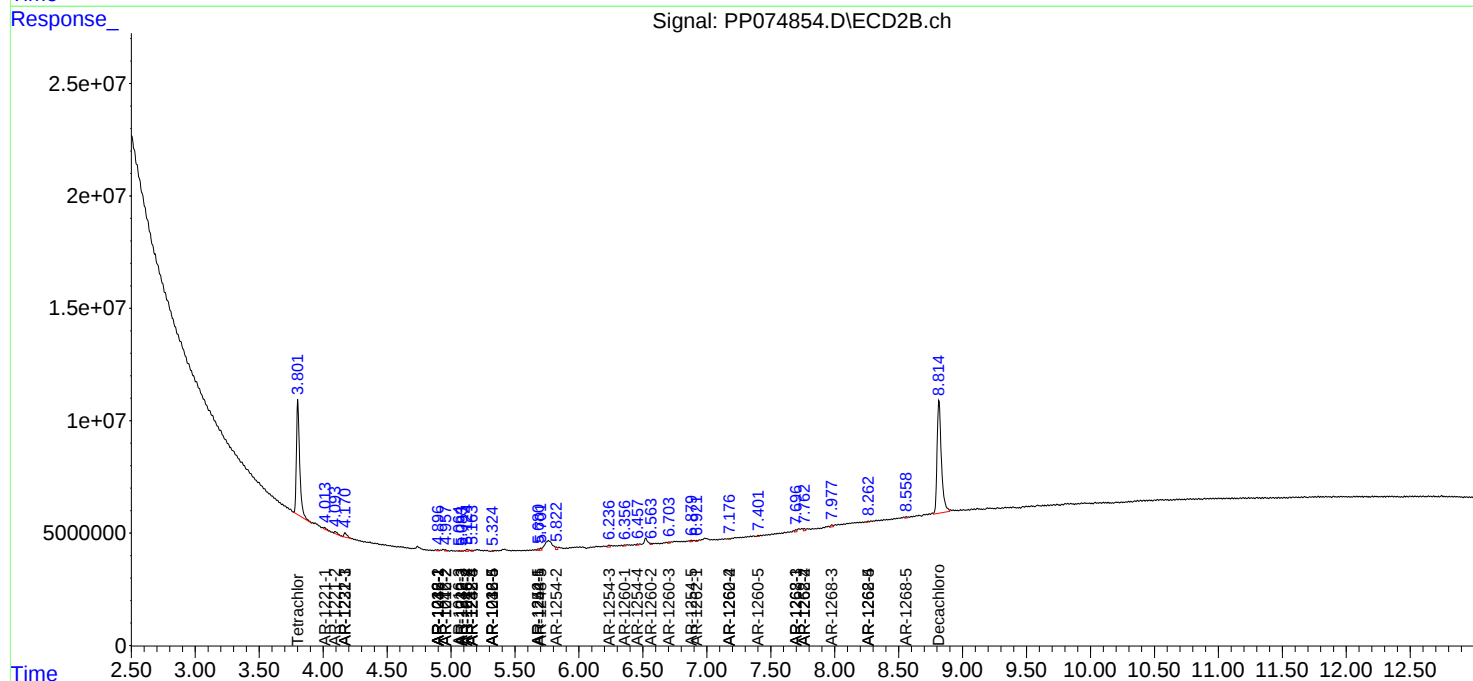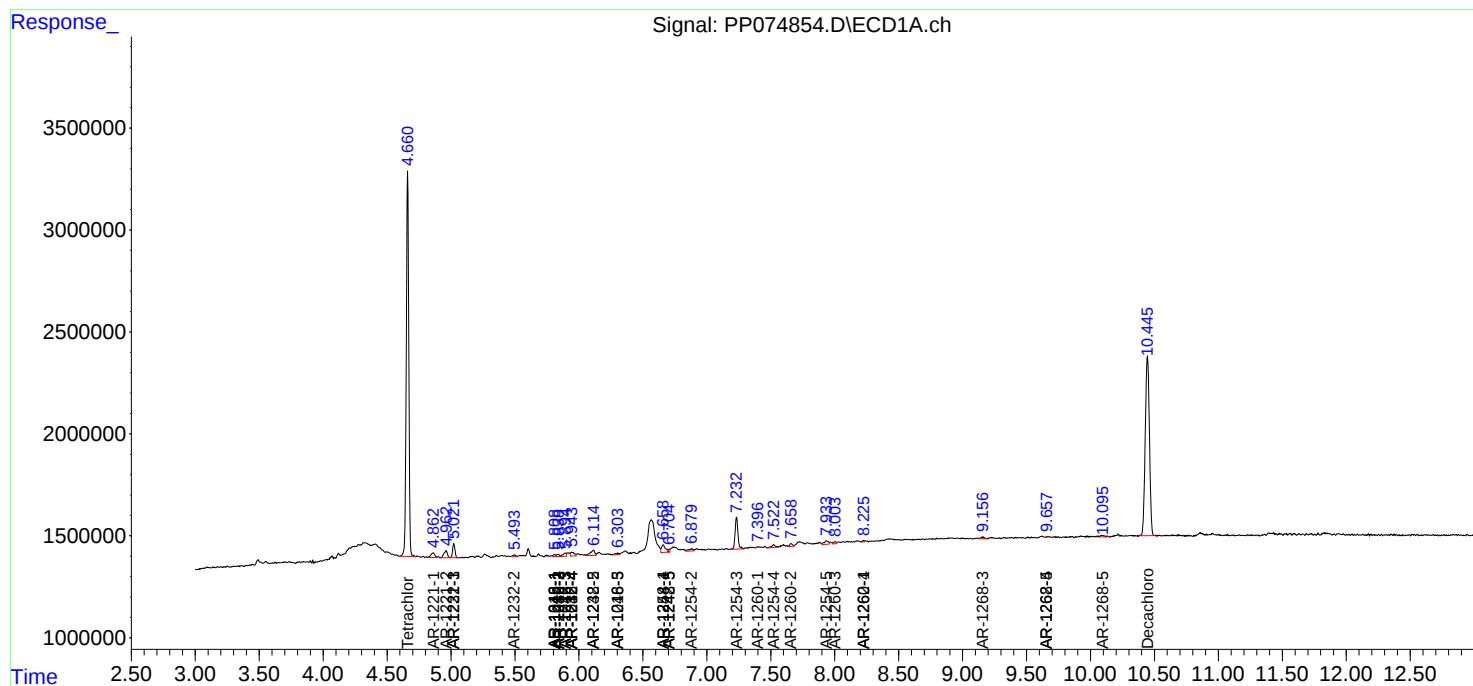


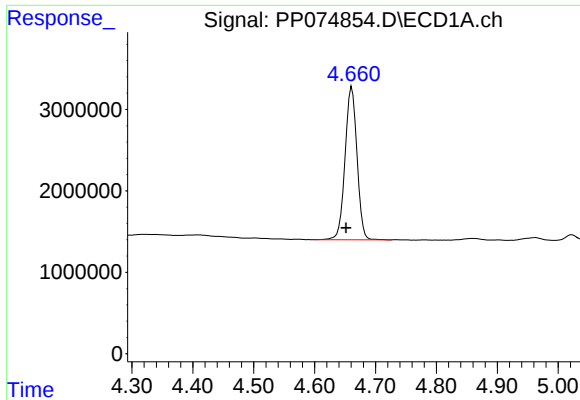

#1 Tetrachloro-m-xylene


R.T.: 4.661 min
Delta R.T.: 0.009 min
Response: 25574579
Conc: 20.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

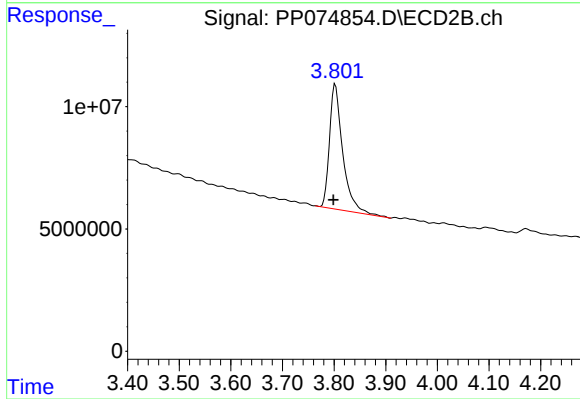


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: 0.004 min
Response: 91213305
Conc: 18.86 ng/ml

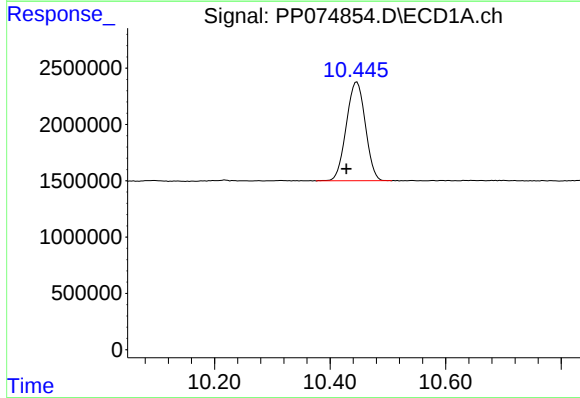


#2 Decachlorobiphenyl

R.T.: 10.446 min
Delta R.T.: 0.018 min
Response: 19969451
Conc: 20.22 ng/ml

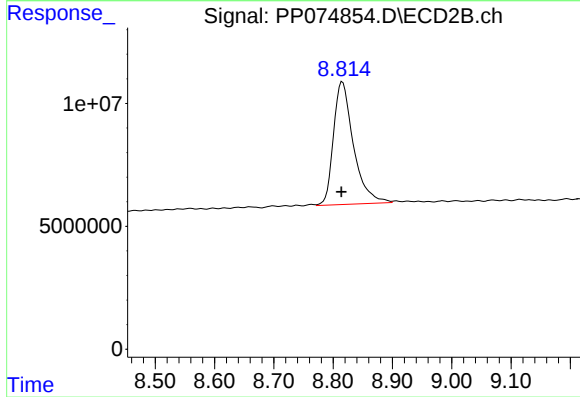

#2 Decachlorobiphenyl


R.T.: 8.816 min
Delta R.T.: 0.002 min
Response: 117015164
Conc: 15.60 ng/ml

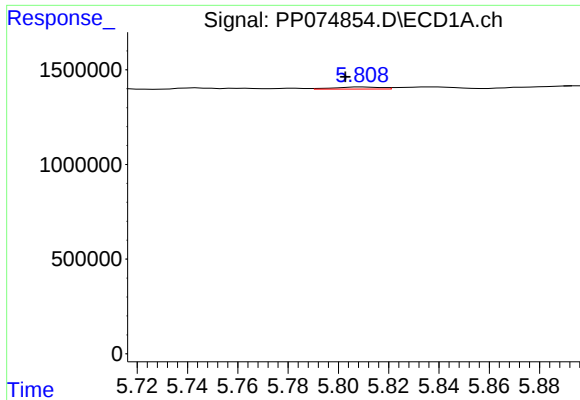

#3 AR-1016-1


R.T.: 5.810 min
Delta R.T.: 0.007 min
Response: 134178
Conc: 3.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

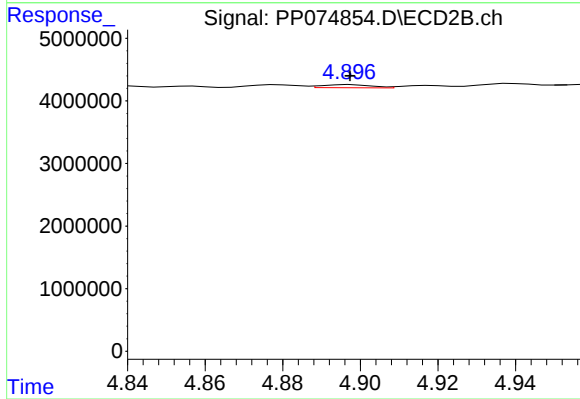


#3 AR-1016-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 443468
Conc: 0.87 ng/ml

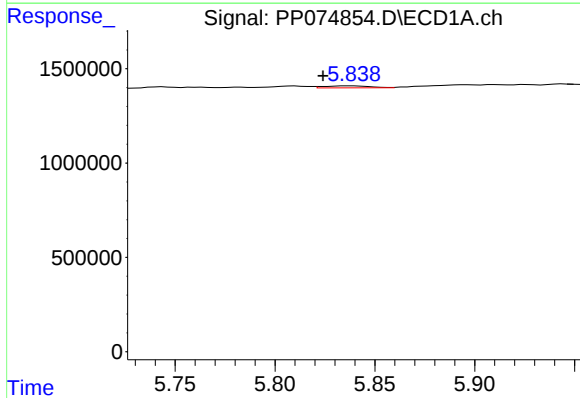


#4 AR-1016-2

R.T.: 5.837 min
Delta R.T.: 0.013 min
Response: 169150
Conc: 2.69 ng/ml

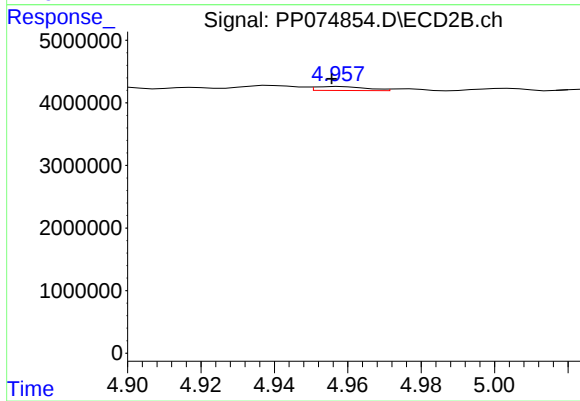

#4 AR-1016-2


R.T.: 4.958 min
Delta R.T.: 0.002 min
Response: 605942
Conc: 2.55 ng/ml

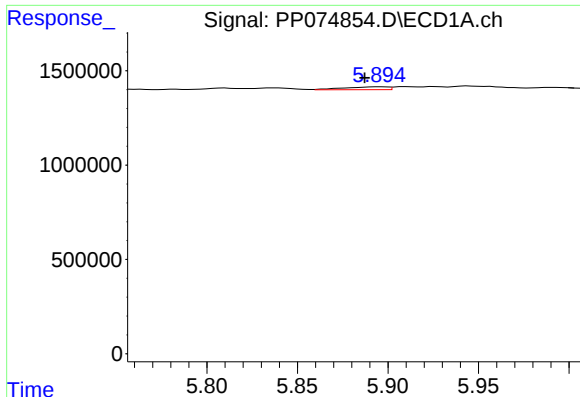

#5 AR-1016-3


R.T.: 5.895 min
Delta R.T.: 0.008 min
Response: 259061
Conc: 5.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

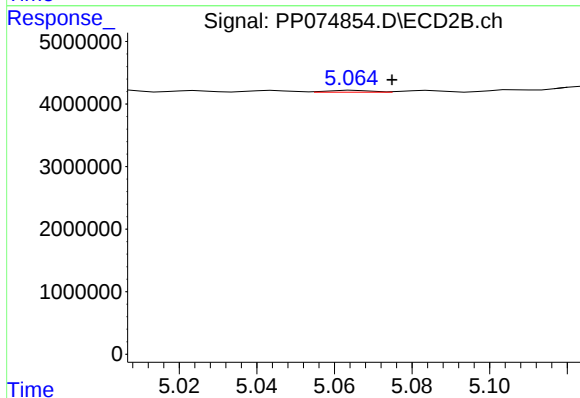


#5 AR-1016-3

R.T.: 5.065 min
Delta R.T.: -0.010 min
Response: 217394
Conc: 1.58 ng/ml

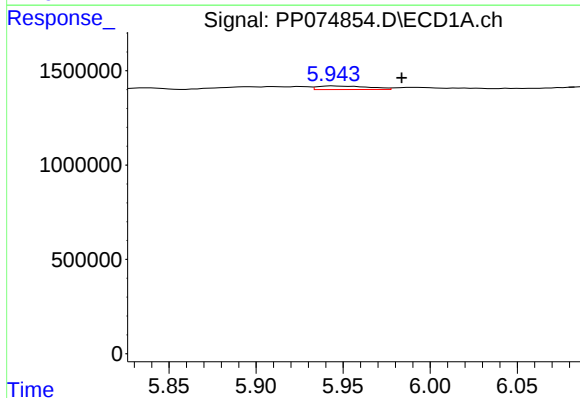


#6 AR-1016-4

R.T.: 5.944 min
Delta R.T.: -0.039 min
Response: 378702
Conc: 10.76 ng/ml

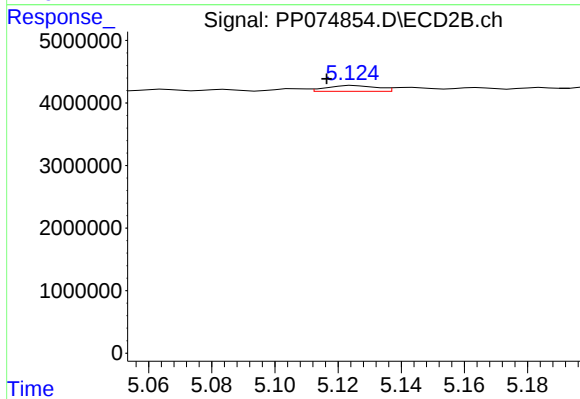

#6 AR-1016-4


R.T.: 5.125 min
Delta R.T.: 0.009 min
Response: 1010619
Conc: 7.23 ng/ml

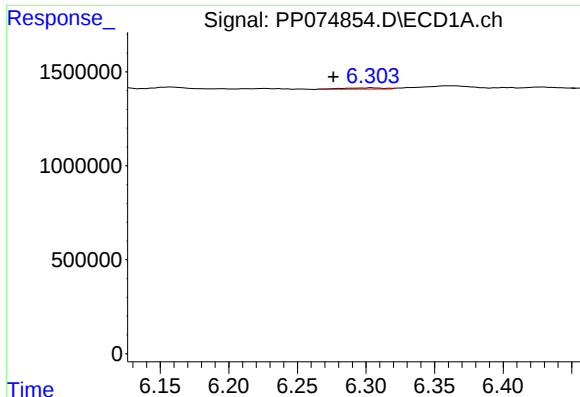

#7 AR-1016-5


R.T.: 6.304 min
Delta R.T.: 0.028 min
Response: 144853
Conc: 4.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

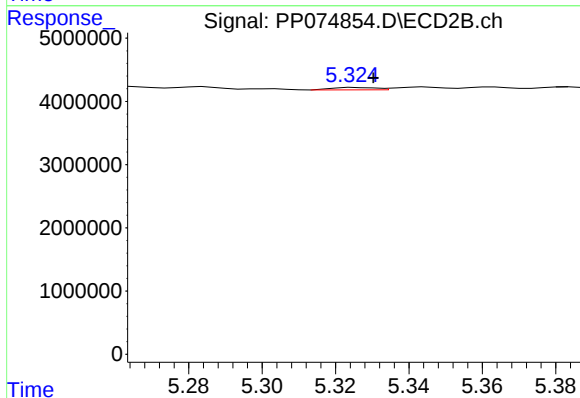


#7 AR-1016-5

R.T.: 5.325 min
Delta R.T.: -0.005 min
Response: 317173
Conc: 1.91 ng/ml

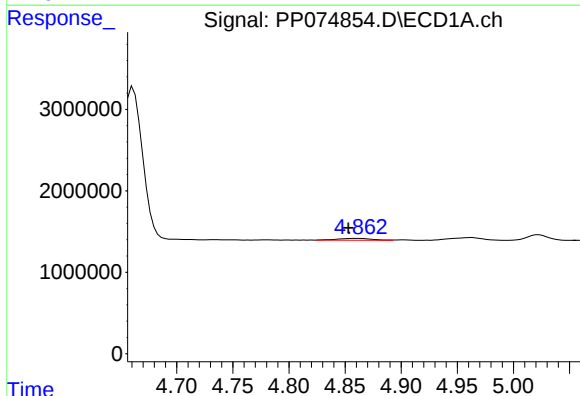


#8 AR-1221-1

R.T.: 4.863 min
Delta R.T.: 0.010 min
Response: 479605
Conc: 27.26 ng/ml

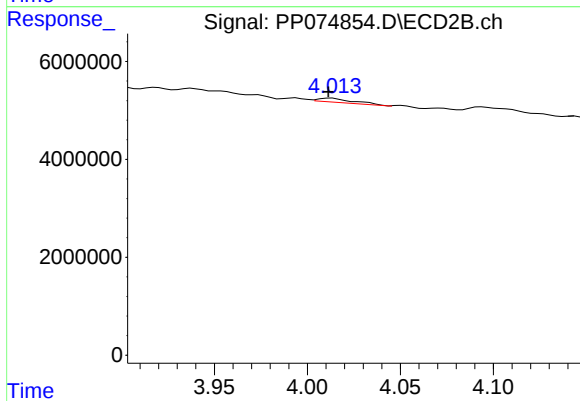

#8 AR-1221-1


R.T.: 4.013 min
Delta R.T.: 0.002 min
Response: 1136410
Conc: 18.37 ng/ml

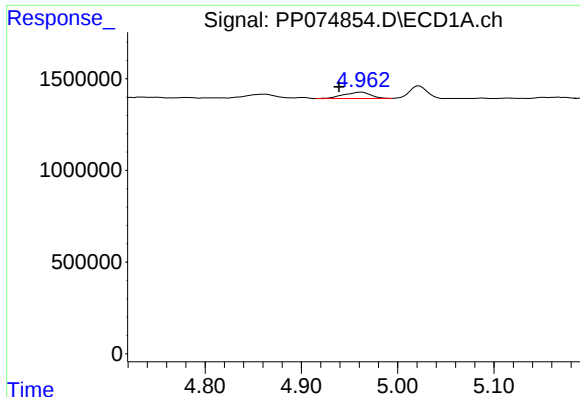

#9 AR-1221-2


R.T.: 4.963 min
Delta R.T.: 0.023 min
Response: 673933
Conc: 50.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

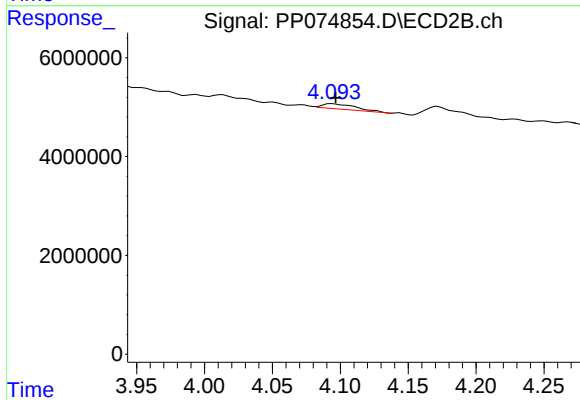


#9 AR-1221-2

R.T.: 4.094 min
Delta R.T.: -0.003 min
Response: 1843881
Conc: 40.78 ng/ml

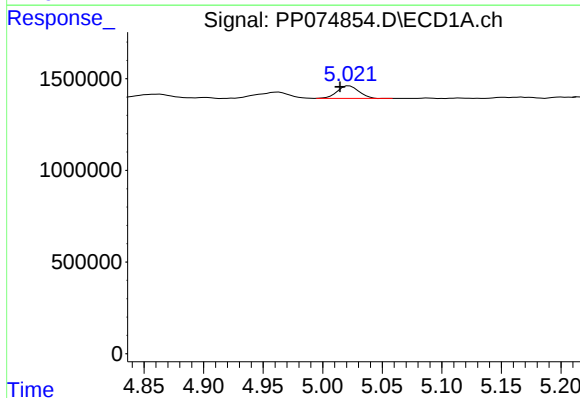


#10 AR-1221-3

R.T.: 5.022 min
Delta R.T.: 0.008 min
Response: 874804
Conc: 23.07 ng/ml

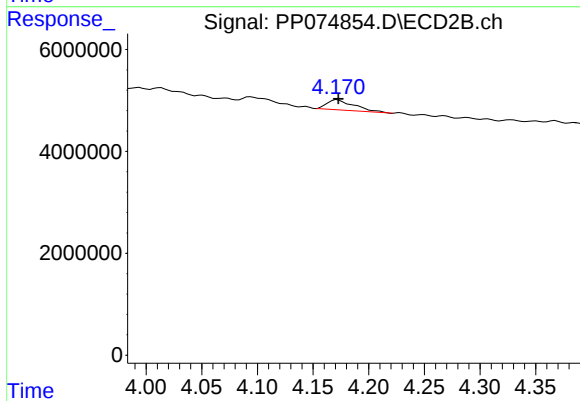

#10 AR-1221-3


R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 3458391
Conc: 21.05 ng/ml

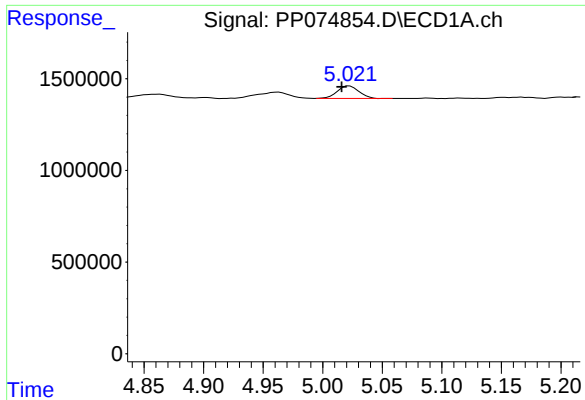

#11 AR-1232-1


R.T.: 5.022 min
Delta R.T.: 0.006 min
Response: 874804
Conc: 28.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

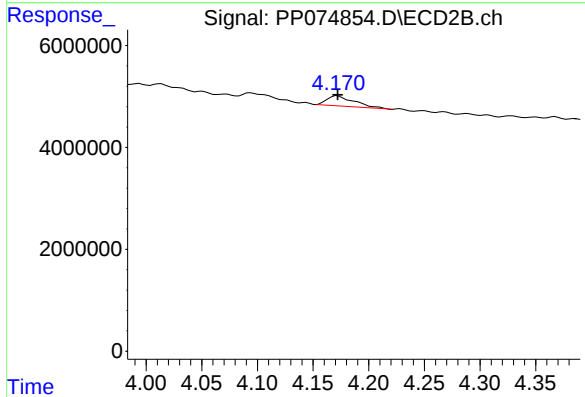


#11 AR-1232-1

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 3458391
Conc: 27.00 ng/ml

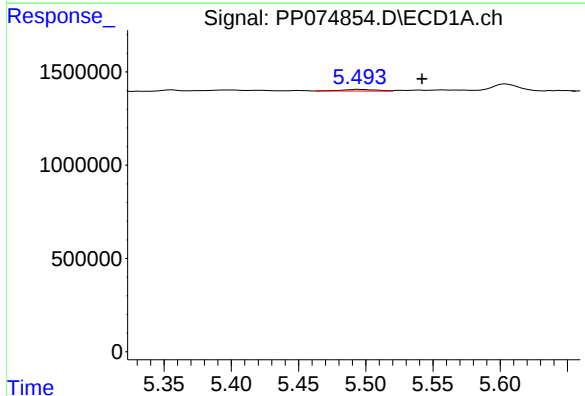


#12 AR-1232-2

R.T.: 5.495 min
Delta R.T.: -0.047 min
Response: 146925
Conc: 9.32 ng/ml

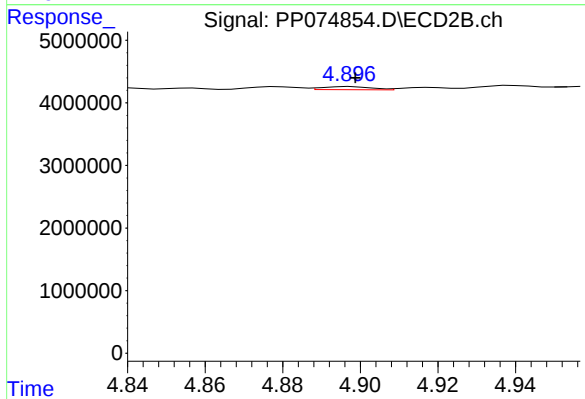

#12 AR-1232-2


R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 443468
Conc: 1.91 ng/ml

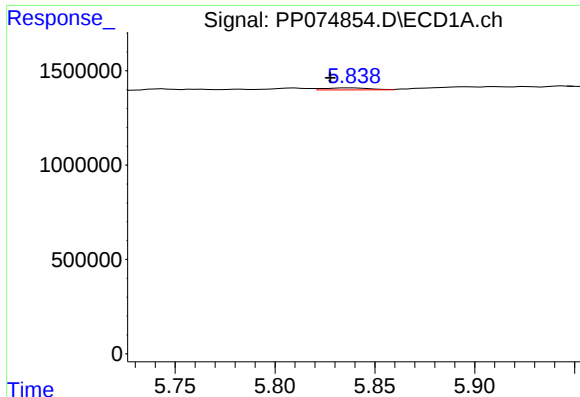

#13 AR-1232-3


R.T.: 5.837 min
Delta R.T.: 0.009 min
Response: 169150
Conc: 5.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

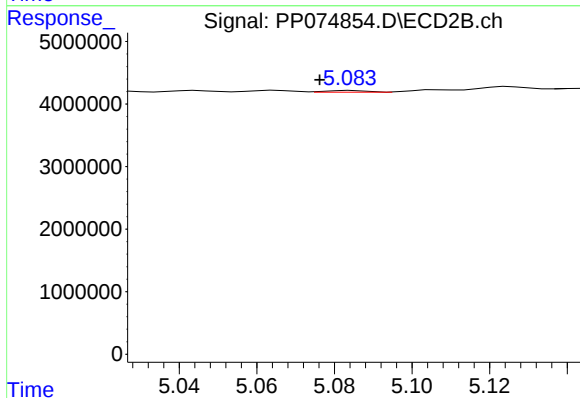


#13 AR-1232-3

R.T.: 5.085 min
Delta R.T.: 0.009 min
Response: 205211
Conc: 3.42 ng/ml

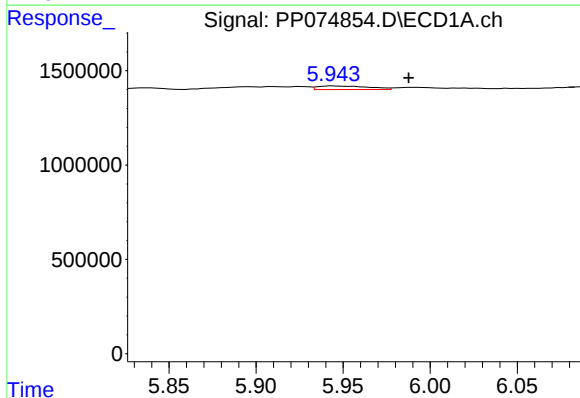


#14 AR-1232-4

R.T.: 5.944 min
Delta R.T.: -0.043 min
Response: 378702
Conc: 21.93 ng/ml

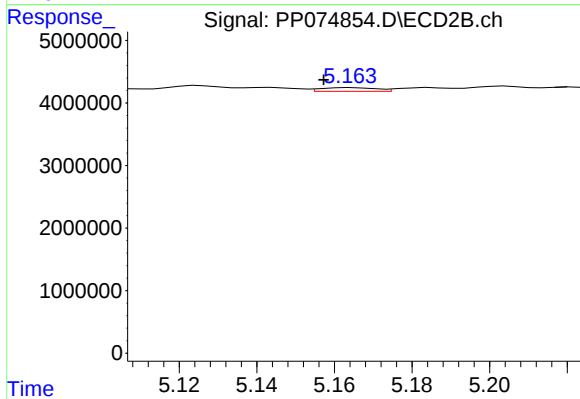

#14 AR-1232-4


R.T.: 5.165 min
Delta R.T.: 0.007 min
Response: 589792
Conc: 8.00 ng/ml

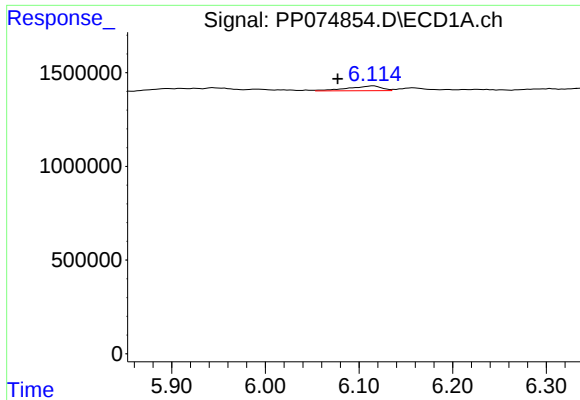

#15 AR-1232-5


R.T.: 6.115 min
Delta R.T.: 0.038 min
Response: 637114
Conc: 49.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

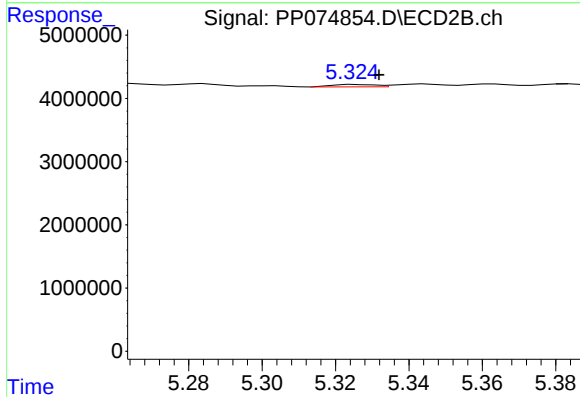


#15 AR-1232-5

R.T.: 5.325 min
Delta R.T.: -0.006 min
Response: 317173
Conc: 5.11 ng/ml

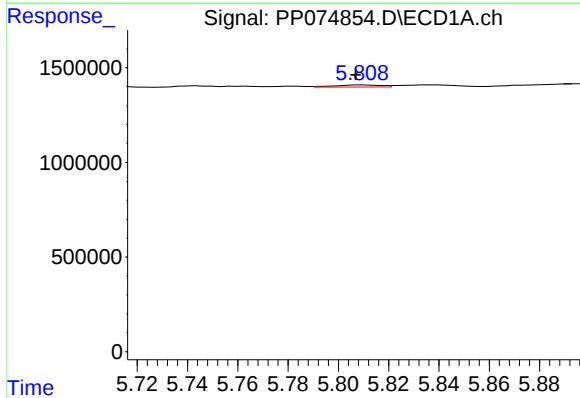


#16 AR-1242-1

R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 134178
Conc: 3.51 ng/ml

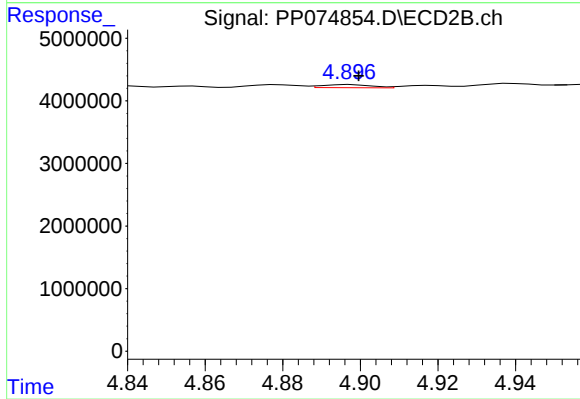

#16 AR-1242-1


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 443468
Conc: 1.05 ng/ml

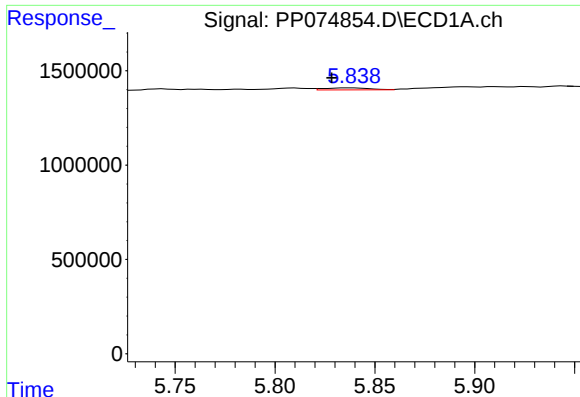

#17 AR-1242-2


R.T.: 5.837 min
Delta R.T.: 0.009 min
Response: 169150
Conc: 2.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

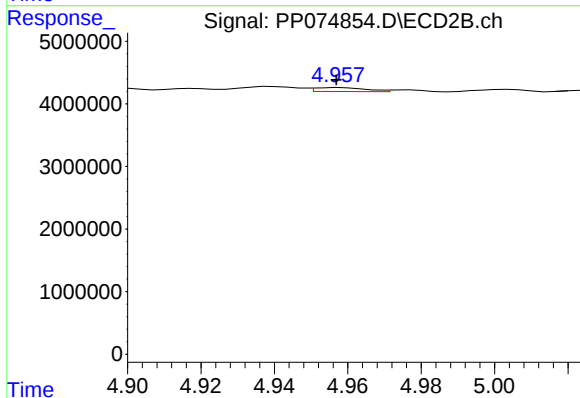


#17 AR-1242-2

R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 605942
Conc: 3.03 ng/ml

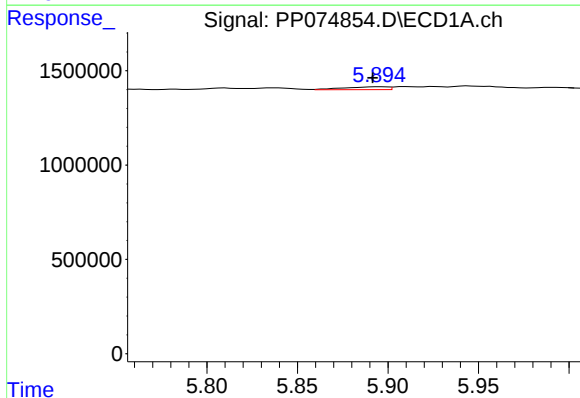


#18 AR-1242-3

R.T.: 5.895 min
Delta R.T.: 0.003 min
Response: 259061
Conc: 6.38 ng/ml

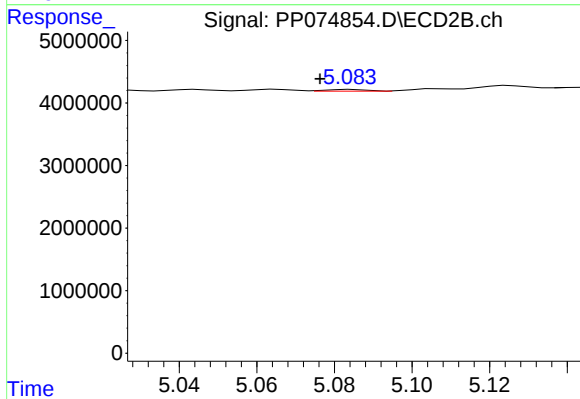

#18 AR-1242-3


R.T.: 5.085 min
Delta R.T.: 0.009 min
Response: 205211
Conc: 1.73 ng/ml

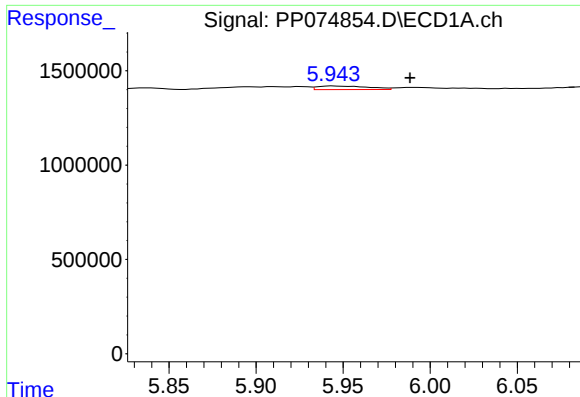

#19 AR-1242-4


R.T.: 5.944 min
Delta R.T.: -0.044 min
Response: 378702
Conc: 11.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

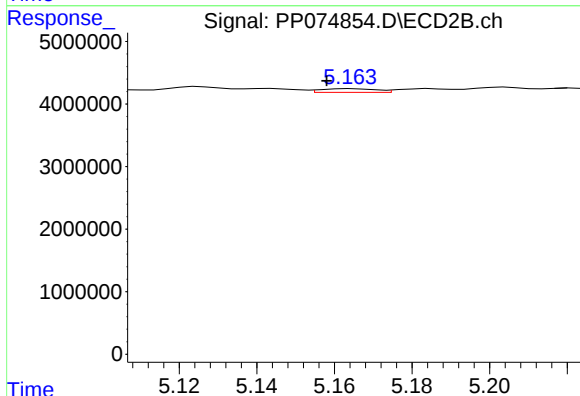


#19 AR-1242-4

R.T.: 5.165 min
Delta R.T.: 0.007 min
Response: 589792
Conc: 3.45 ng/ml

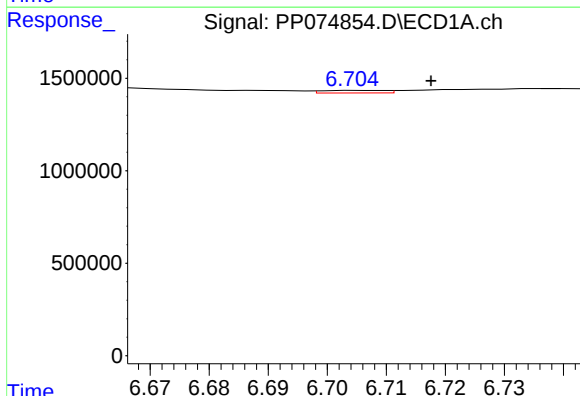


#20 AR-1242-5

R.T.: 6.705 min
Delta R.T.: -0.012 min
Response: 103651
Conc: 2.87 ng/ml

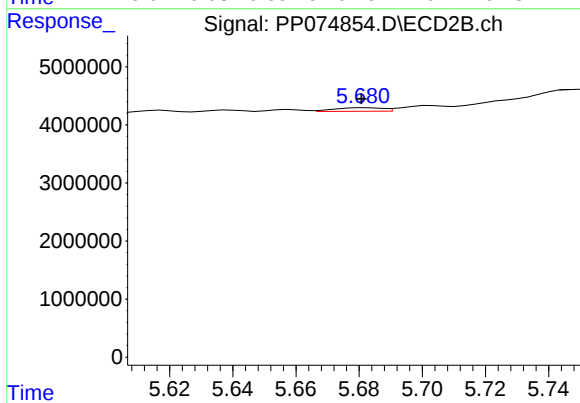

#20 AR-1242-5


R.T.: 5.682 min
Delta R.T.: 0.001 min
Response: 634549
Conc: 3.43 ng/ml

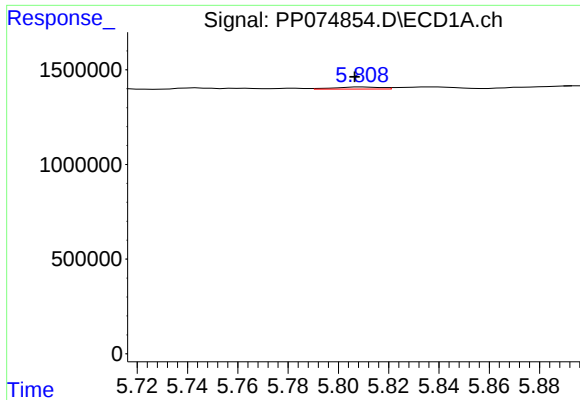

#21 AR-1248-1


R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 134178
Conc: 4.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

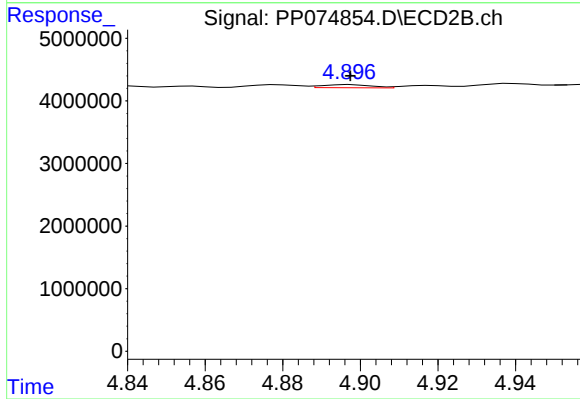


#21 AR-1248-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 443468
Conc: 1.61 ng/ml

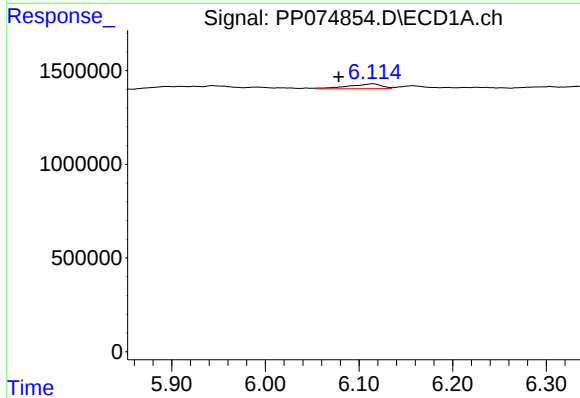


#22 AR-1248-2

R.T.: 6.115 min
Delta R.T.: 0.037 min
Response: 637114
Conc: 14.78 ng/ml

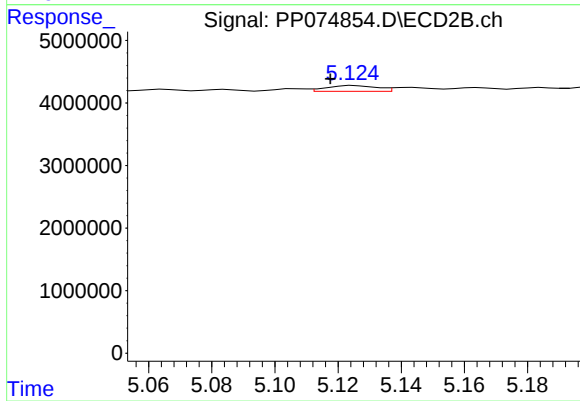

#22 AR-1248-2


R.T.: 5.125 min
Delta R.T.: 0.008 min
Response: 1010619
Conc: 5.72 ng/ml

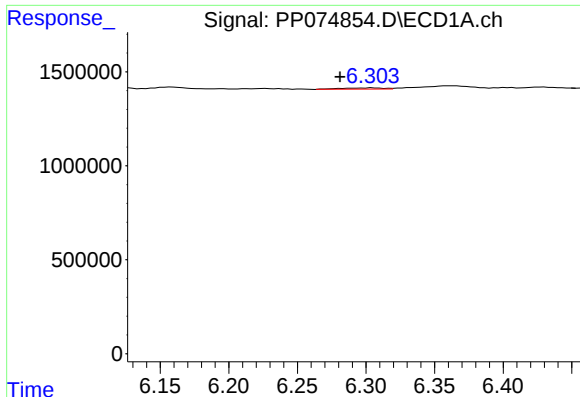

#23 AR-1248-3


R.T.: 6.304 min
Delta R.T.: 0.023 min
Response: 144853
Conc: 3.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

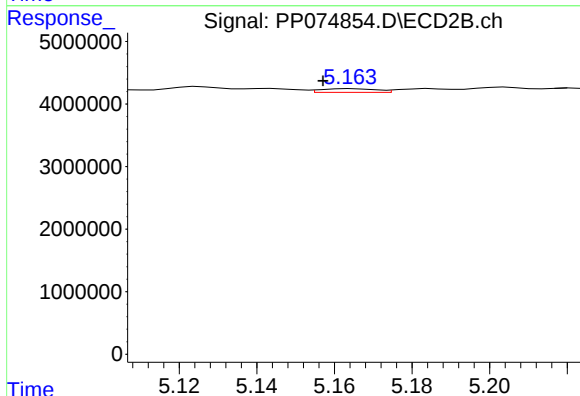


#23 AR-1248-3

R.T.: 5.165 min
Delta R.T.: 0.007 min
Response: 589792
Conc: 2.60 ng/ml

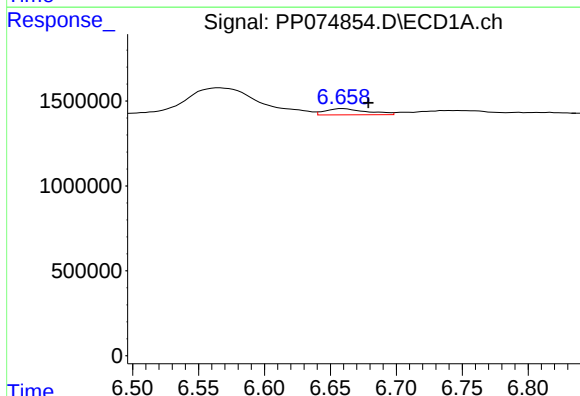


#24 AR-1248-4

R.T.: 6.660 min
Delta R.T.: -0.019 min
Response: 806481
Conc: 14.66 ng/ml

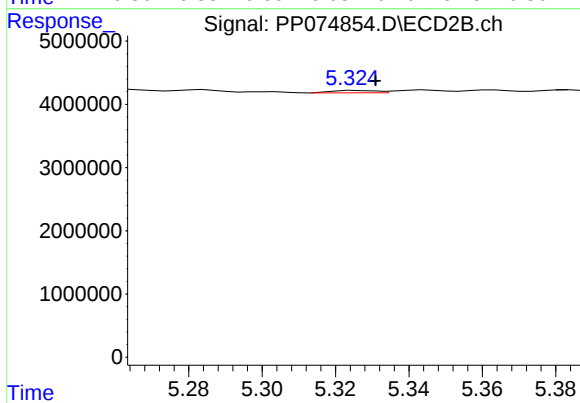

#24 AR-1248-4


R.T.: 5.325 min
Delta R.T.: -0.005 min
Response: 317173
Conc: 1.45 ng/ml

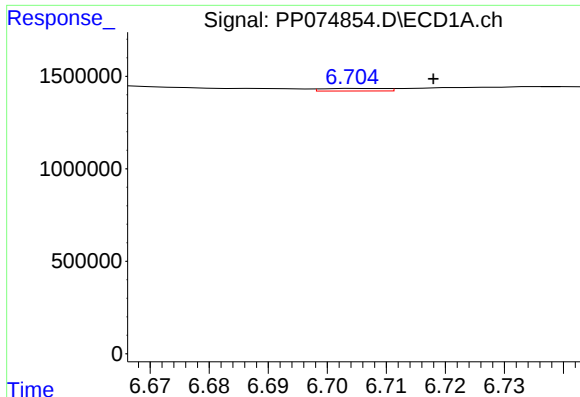

#25 AR-1248-5


R.T.: 6.705 min
Delta R.T.: -0.013 min
Response: 103651
Conc: 1.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

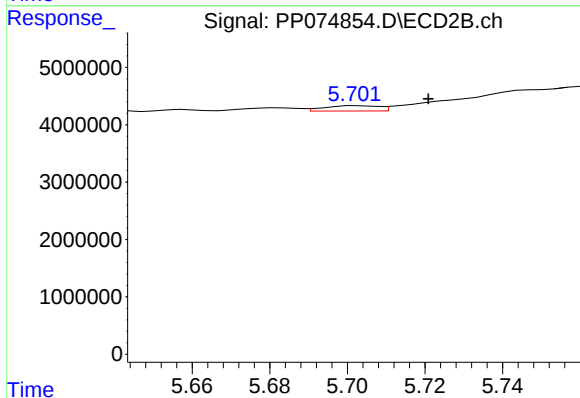


#25 AR-1248-5

R.T.: 5.703 min
Delta R.T.: -0.018 min
Response: 905163
Conc: 2.46 ng/ml

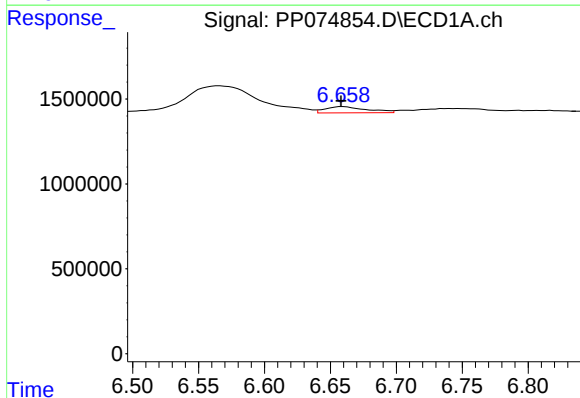


#26 AR-1254-1

R.T.: 6.660 min
Delta R.T.: 0.002 min
Response: 806481
Conc: 13.84 ng/ml

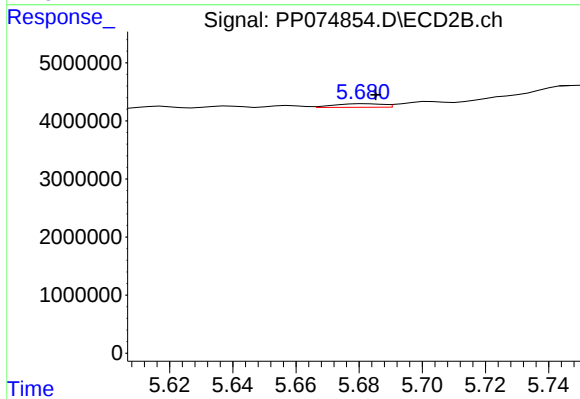

#26 AR-1254-1


R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 634549
Conc: 1.33 ng/ml

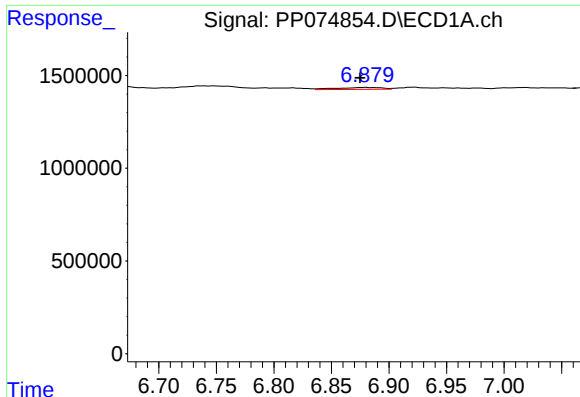

#27 AR-1254-2


R.T.: 6.880 min
Delta R.T.: 0.005 min
Response: 282094
Conc: 3.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

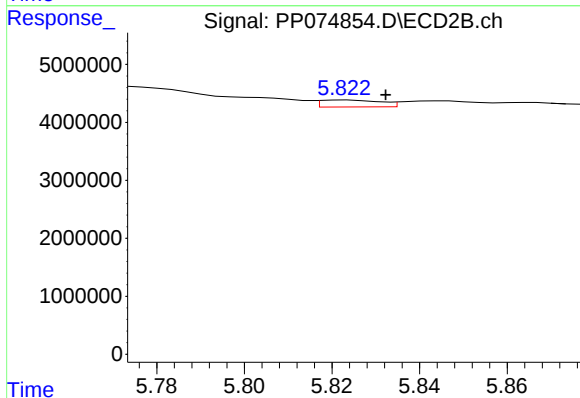


#27 AR-1254-2

R.T.: 5.823 min
Delta R.T.: -0.009 min
Response: 1139430
Conc: 3.24 ng/ml

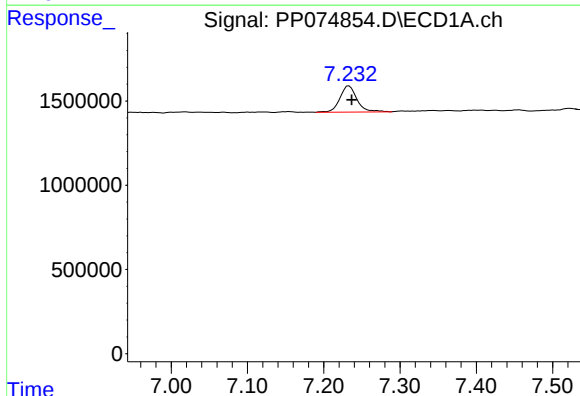


#28 AR-1254-3

R.T.: 7.233 min
Delta R.T.: -0.004 min
Response: 2406108
Conc: 26.97 ng/ml

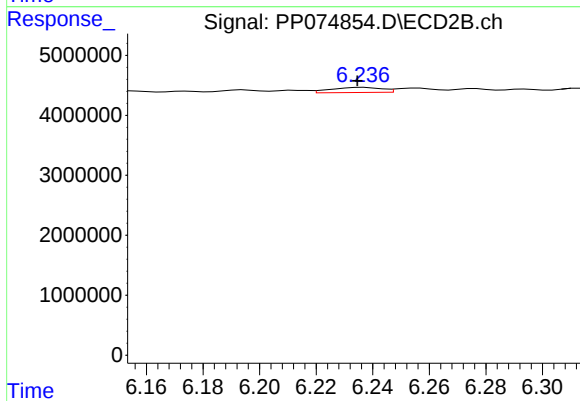

#28 AR-1254-3


R.T.: 6.237 min
Delta R.T.: 0.002 min
Response: 1073327
Conc: 1.73 ng/ml

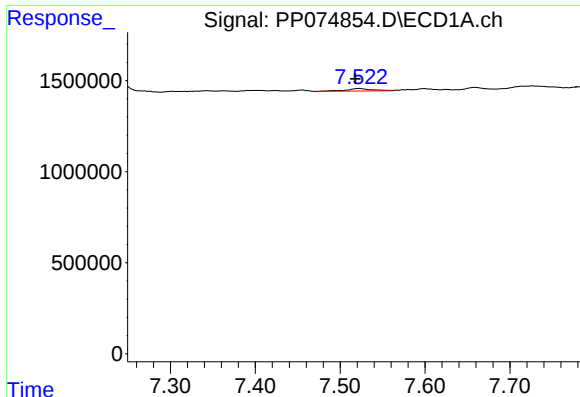

#29 AR-1254-4


R.T.: 7.523 min
Delta R.T.: 0.005 min
Response: 293950
Conc: 4.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

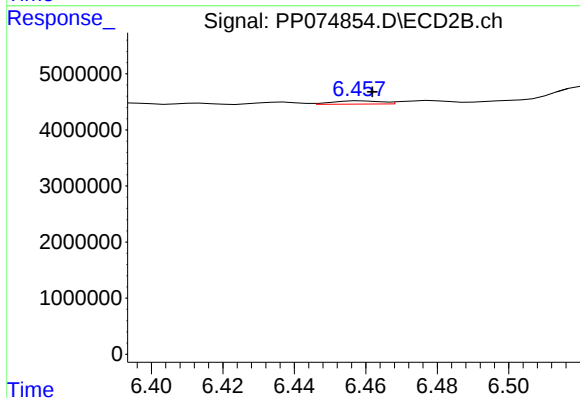


#29 AR-1254-4

R.T.: 6.459 min
Delta R.T.: -0.003 min
Response: 543240
Conc: 1.16 ng/ml

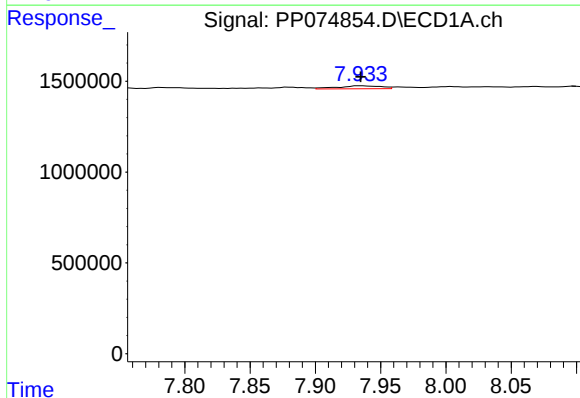


#30 AR-1254-5

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 377564
Conc: 4.54 ng/ml

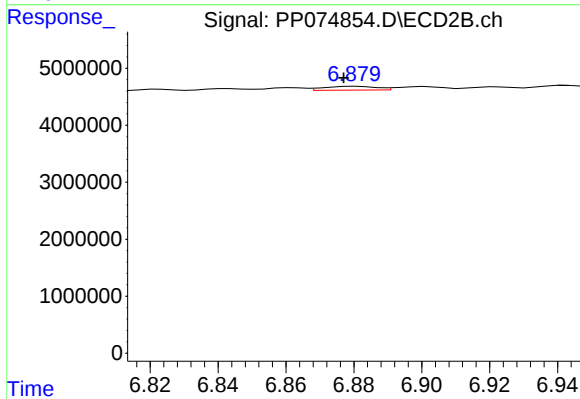

#30 AR-1254-5


R.T.: 6.881 min
Delta R.T.: 0.004 min
Response: 733007
Conc: 1.49 ng/ml

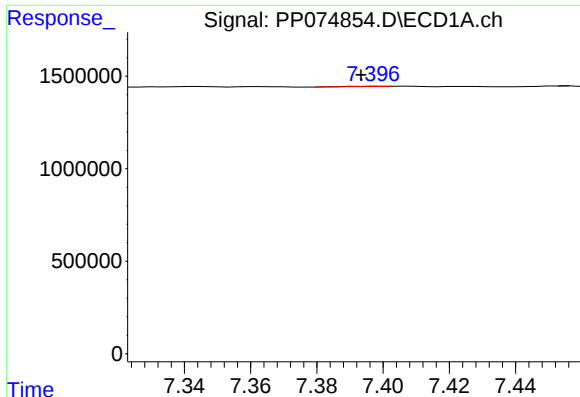

#31 AR-1260-1


R.T.: 7.398 min
Delta R.T.: 0.004 min
Response: 15014
Conc: 0.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

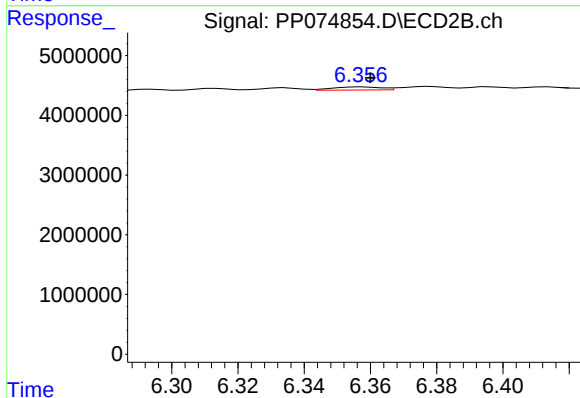


#31 AR-1260-1

R.T.: 6.358 min
Delta R.T.: -0.002 min
Response: 532202
Conc: 1.42 ng/ml

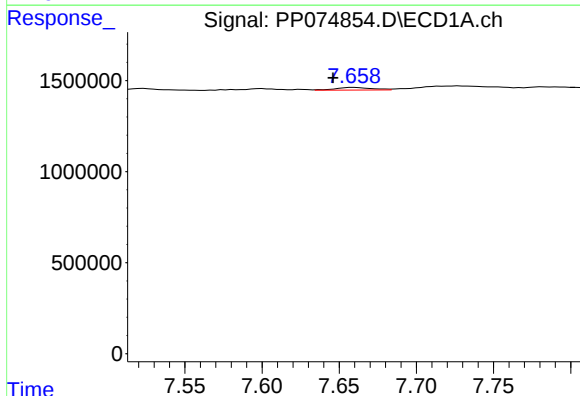


#32 AR-1260-2

R.T.: 7.659 min
Delta R.T.: 0.013 min
Response: 226488
Conc: 3.29 ng/ml

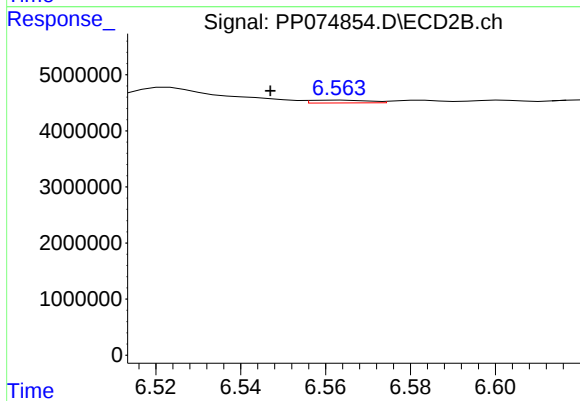

#32 AR-1260-2


R.T.: 6.563 min
Delta R.T.: 0.016 min
Response: 461030
Conc: 0.87 ng/ml

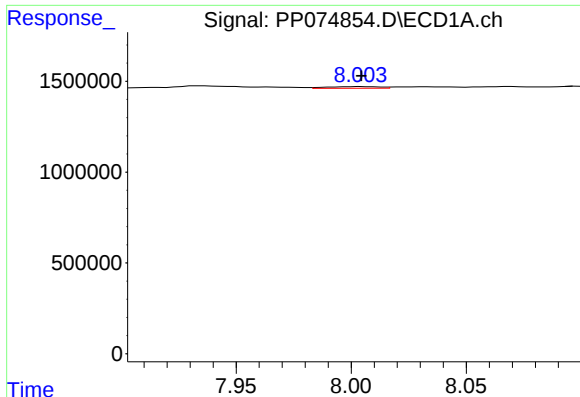

#33 AR-1260-3


R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 149908
Conc: 2.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

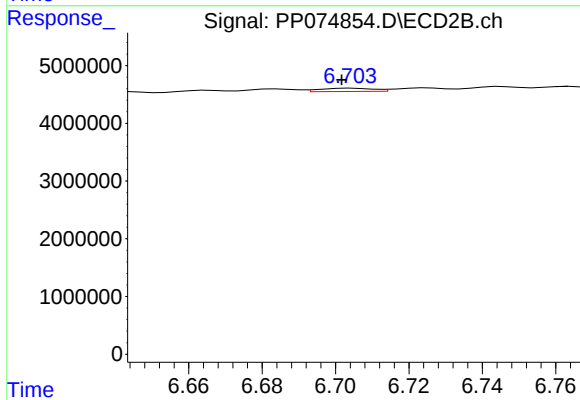


#33 AR-1260-3

R.T.: 6.705 min
Delta R.T.: 0.003 min
Response: 576366
Conc: 1.33 ng/ml

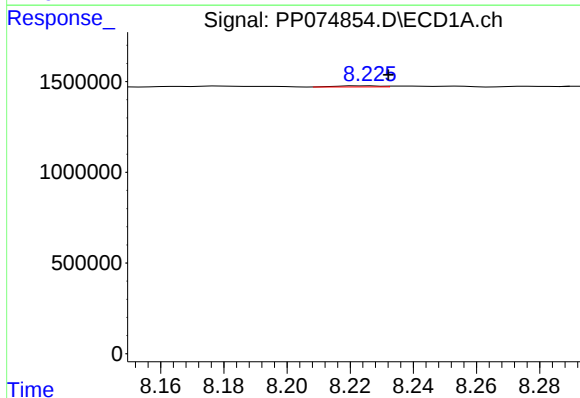


#34 AR-1260-4

R.T.: 8.226 min
Delta R.T.: -0.006 min
Response: 62572
Conc: 0.98 ng/ml

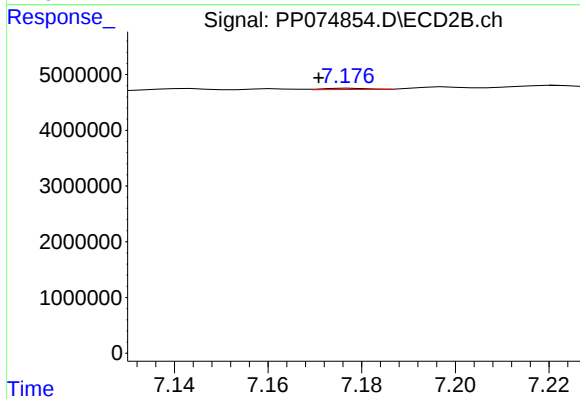

#34 AR-1260-4

R.T.: 7.178 min
Delta R.T.: 0.007 min
Response: 144124
Conc: 0.38 ng/ml

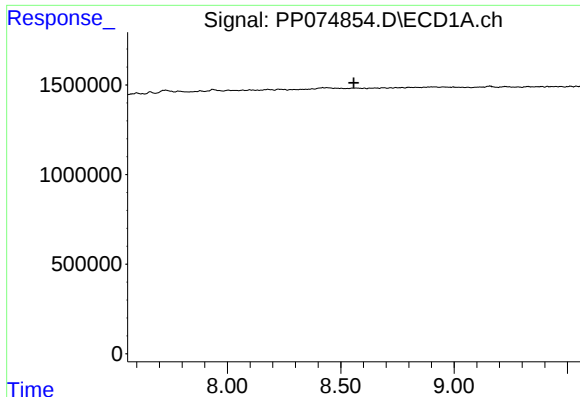

#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.558 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

#35 AR-1260-5


R.T.: 7.403 min
Delta R.T.: -0.007 min
Response: 411252
Conc: 0.41 ng/ml

#36 AR-1262-1

R.T.: 8.226 min
Delta R.T.: -0.015 min
Response: 62572
Conc: 0.81 ng/ml

#36 AR-1262-1


R.T.: 6.922 min
Delta R.T.: 0.005 min
Response: 373408
Conc: 0.53 ng/ml

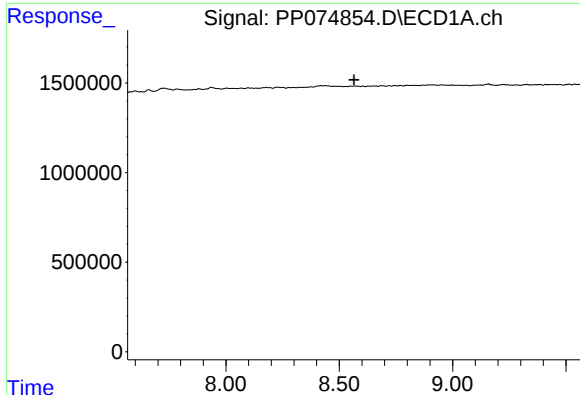

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

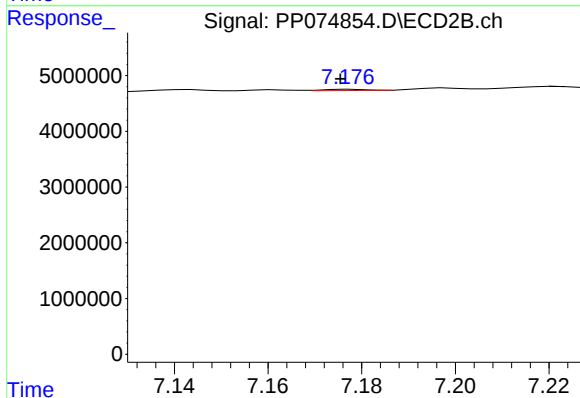


#37 AR-1262-2

R.T.: 7.178 min
Delta R.T.: 0.003 min
Response: 144124
Conc: 0.28 ng/ml

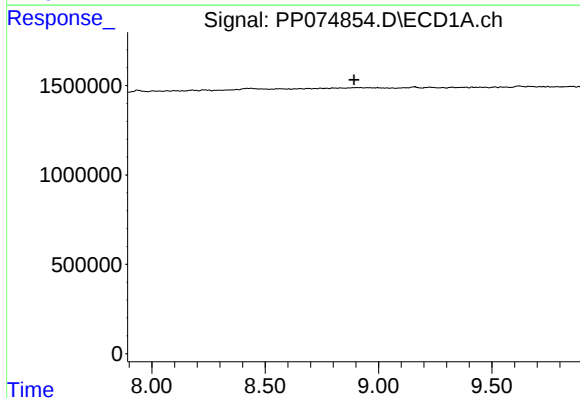


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.892 min
Response: 0
Conc: N.D.

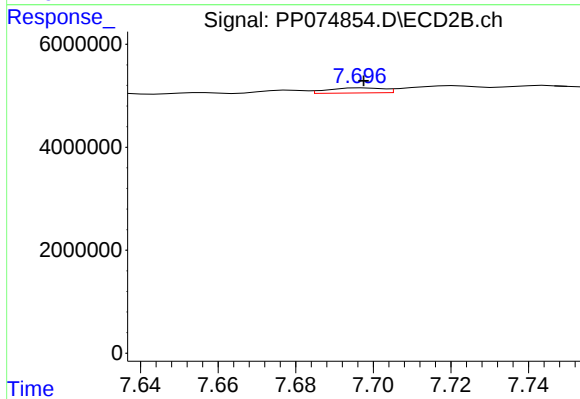

#38 AR-1262-3


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 957468
Conc: 2.05 ng/ml

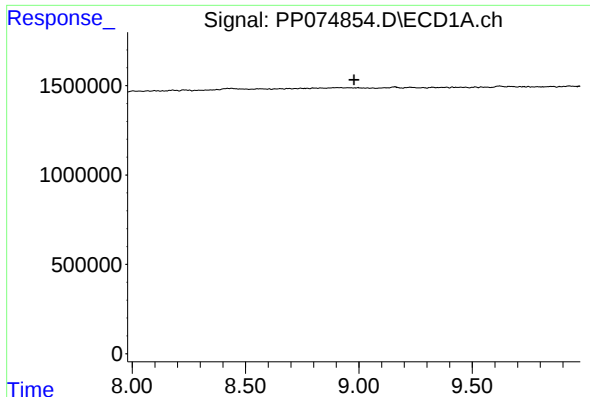

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

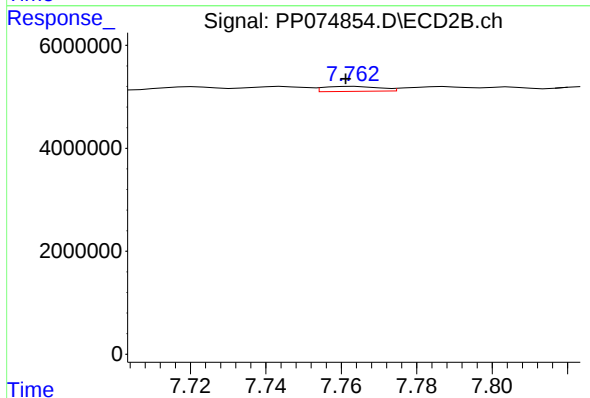


#39 AR-1262-4

R.T.: 7.763 min
Delta R.T.: 0.002 min
Response: 1005208
Conc: 1.22 ng/ml

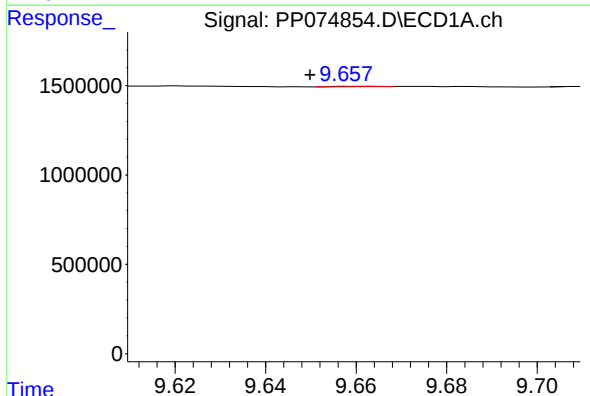


#40 AR-1262-5

R.T.: 9.660 min
Delta R.T.: 0.010 min
Response: 13452
Conc: 0.22 ng/ml

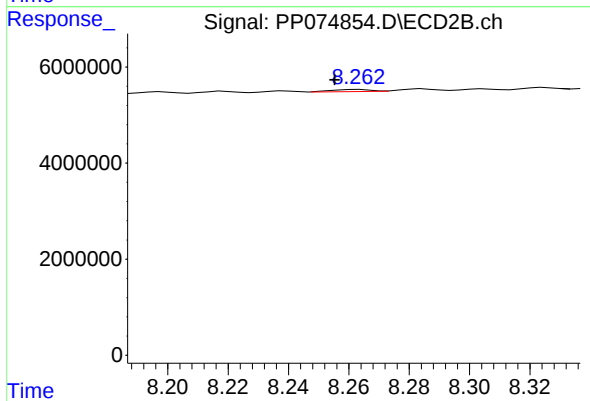

#40 AR-1262-5


R.T.: 8.263 min
Delta R.T.: 0.008 min
Response: 407280
Conc: 1.14 ng/ml

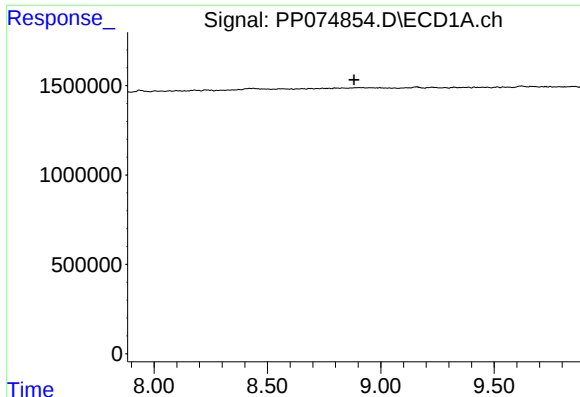

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

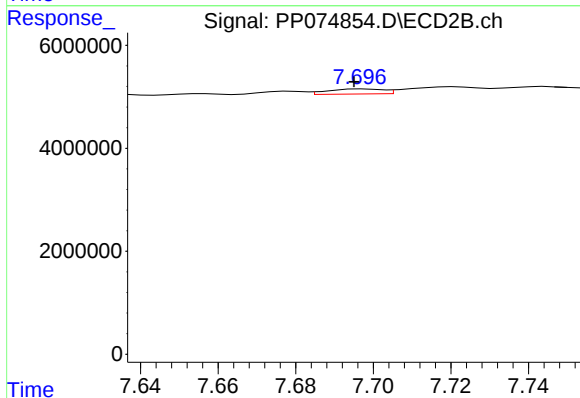


#41 AR-1268-1

R.T.: 7.697 min
Delta R.T.: 0.002 min
Response: 957468
Conc: 0.68 ng/ml

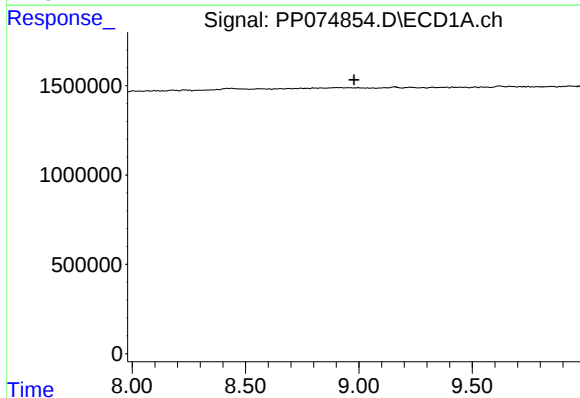


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

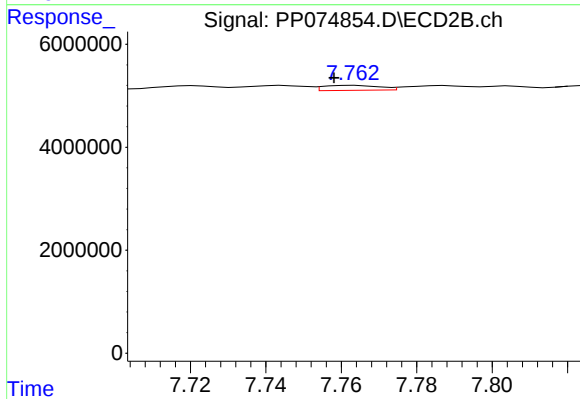

#42 AR-1268-2


R.T.: 7.763 min
Delta R.T.: 0.005 min
Response: 1005208
Conc: 0.74 ng/ml

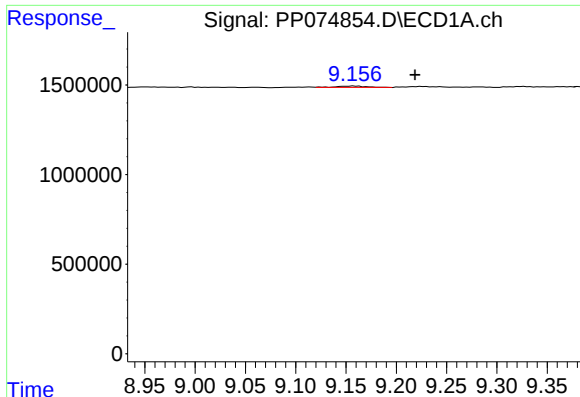

#43 AR-1268-3


R.T.: 9.157 min
Delta R.T.: -0.061 min
Response: 148574
Conc: 1.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

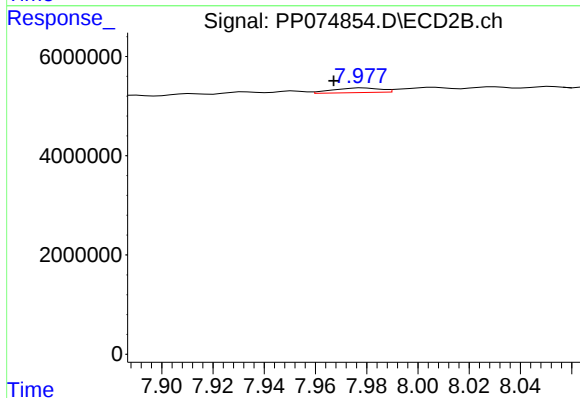


#43 AR-1268-3

R.T.: 7.979 min
Delta R.T.: 0.011 min
Response: 1195732
Conc: 1.15 ng/ml

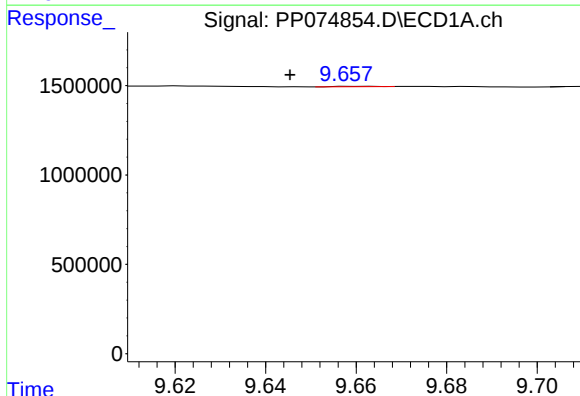


#44 AR-1268-4

R.T.: 9.660 min
Delta R.T.: 0.015 min
Response: 13452
Conc: 0.20 ng/ml

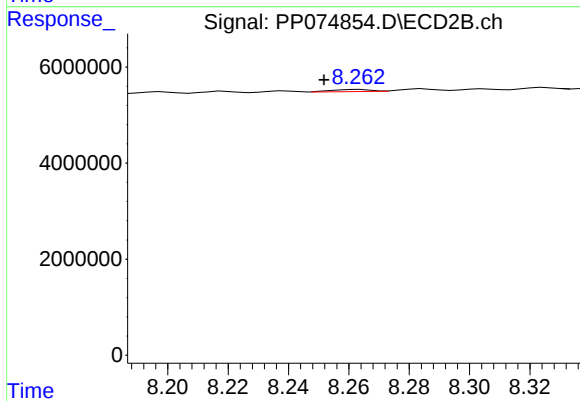

#44 AR-1268-4


R.T.: 8.263 min
Delta R.T.: 0.012 min
Response: 407280
Conc: 1.06 ng/ml

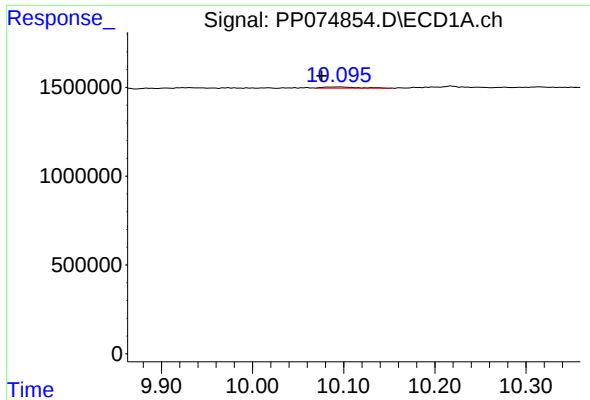

#45 AR-1268-5

R.T.: 10.096 min
Delta R.T.: 0.020 min
Response: 178083
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

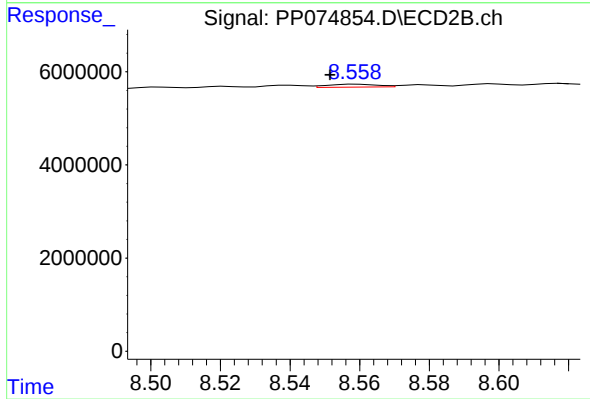

#45 AR-1268-5

R.T.: 8.559 min
Delta R.T.: 0.008 min
Response: 615270
Conc: 0.20 ng/ml