

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074855.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 13:29
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1232 WATER LOD 25PPB
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 01:59:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.662	3.802	24889454	88158529	20.340	18.232
2) SA Decachlor...	10.445	8.815	19632366	115.3E6	19.881	15.376
Target Compounds						
3) L1 AR-1016-1	5.814	4.898	452296	4444290	10.259	8.725
4) L1 AR-1016-2	5.814	4.955	452296	2548250	7.197	10.706 #
5) L1 AR-1016-3	5.900	5.074	900689	717966	20.054	5.206 #
6) L1 AR-1016-4	5.996	5.117	492059	900967	13.986	6.445 #
7) L1 AR-1016-5	6.289	5.338	380114	1483849	11.454	8.934
8) L2 AR-1221-1	4.859	4.005	453447	1023564	25.775	16.544 #
9) L2 AR-1221-2	4.962	4.096	682364	1608730	51.086	35.582 #
10) L2 AR-1221-3	5.024	4.171	788183	2329580	20.789	14.179 #
11) L3 AR-1232-1	5.024	4.171	788183	2329580	25.949	18.186 #
12) L3 AR-1232-2	5.549	4.898	372901	4444290	23.664	19.173
13) L3 AR-1232-3	5.836	5.074	742470	717966	24.308	11.954 #
14) L3 AR-1232-4	5.996	5.155	492059	1183488	28.493	16.057 #
15) L3 AR-1232-5	6.089	5.338	730856	1483849	56.302	23.901 #
16) L4 AR-1242-1	5.814	4.898	452296	4444290	11.817	10.538
17) L4 AR-1242-2	5.836	4.955	742470	2548250	13.145	12.723
18) L4 AR-1242-3	5.900	5.074	900689	717966	22.183	6.069 #
19) L4 AR-1242-4	5.996	5.155	492059	1183488	15.502	6.915 #
20) L4 AR-1242-5	6.727	5.688	1287431	2631637	35.692	14.212 #
21) L5 AR-1248-1	5.814	4.898	452296	4444290	14.965	16.094
22) L5 AR-1248-2	6.089	5.117	730856	900967	16.959	5.097 #
23) L5 AR-1248-3	6.289	5.155	380114	1183488	8.139	5.209 #
24) L5 AR-1248-4	6.686	5.338	669075	1483849	12.165	6.806 #
25) L5 AR-1248-5	6.727	5.688	1287431	2631637	23.209	7.164 #
26) L6 AR-1254-1	6.660	5.688	805785	2631637	13.829	5.520 #
27) L6 AR-1254-2	6.881	5.823	634715	1473935	7.777	4.186 #
28) L6 AR-1254-3	7.234	6.227	2244433	791950	25.160	1.278 #
29) L6 AR-1254-4	7.523	6.456	433598	761451	6.578	1.625 #
30) L6 AR-1254-5	7.939	6.880	589567	777893	7.096	1.586 #
31) L7 AR-1260-1	7.407	6.357	68929	549662	1.192	1.465
32) L7 AR-1260-2	7.662	6.557	1374938	449186	19.950	0.849 #
33) L7 AR-1260-3	8.006	6.680	209847	6072012	4.044	14.023 #
34) L7 AR-1260-4	8.230	7.164	428136	139302	6.711	0.365 #
35) L7 AR-1260-5	8.571	7.405	279003	373053	2.460	0.371 #
36) L8 AR-1262-1	8.230	6.921	428136	580285	5.559	0.820 #
37) L8 AR-1262-2	8.571	7.164	279003	139302	2.108	0.268 #
38) L8 AR-1262-3	0.000	7.703	0	575798	N.D.	1.235 #
39) L8 AR-1262-4	0.000	7.760	0	481830	N.D.	0.586 #
40) L8 AR-1262-5	9.615f	8.255	128805	223427	2.113	0.624 #
41) L9 AR-1268-1	0.000	7.703	0	575798	N.D.	0.408 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 13:29
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1232 WATER LOD 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:59:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.760	0	481830	N.D.	0.353 #
43)	L9 AR-1268-3	9.156f	7.977	164587	727754	1.332	0.698 #
44)	L9 AR-1268-4	9.615	8.255	128805	223427	1.915	0.583 #
45)	L9 AR-1268-5	0.000	8.558	0	500289	N.D.	0.160 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074855.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 13:29
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1232 WATER LOD 25PPB
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 01:59:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

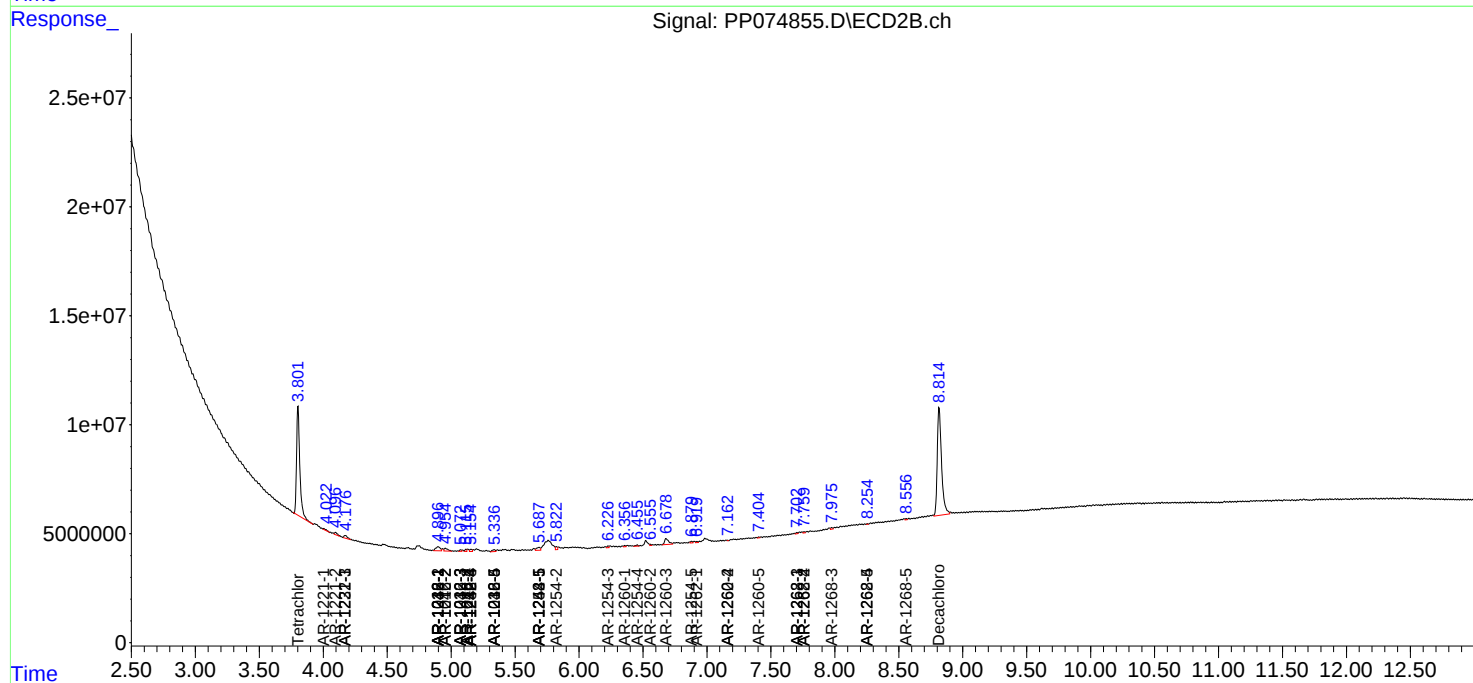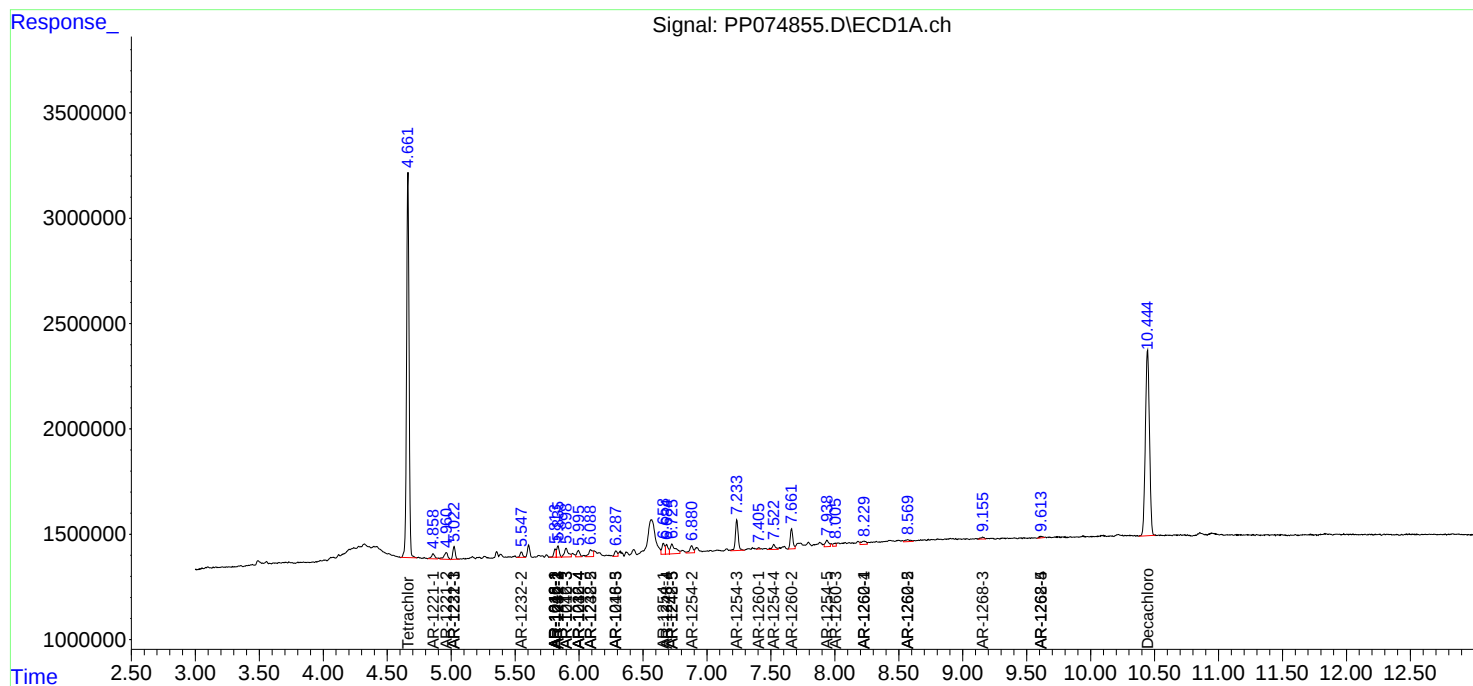


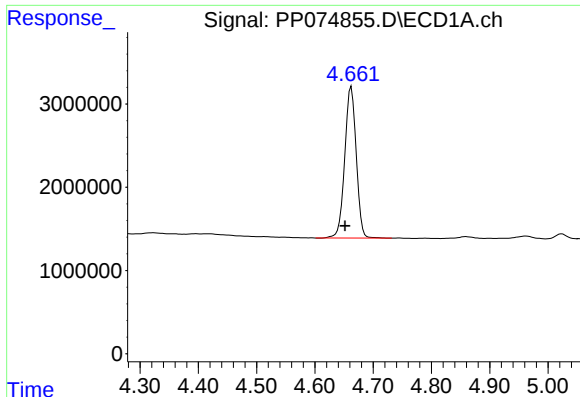

#1 Tetrachloro-m-xylene


R.T.: 4.662 min
Delta R.T.: 0.010 min
Response: 24889454
Conc: 20.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

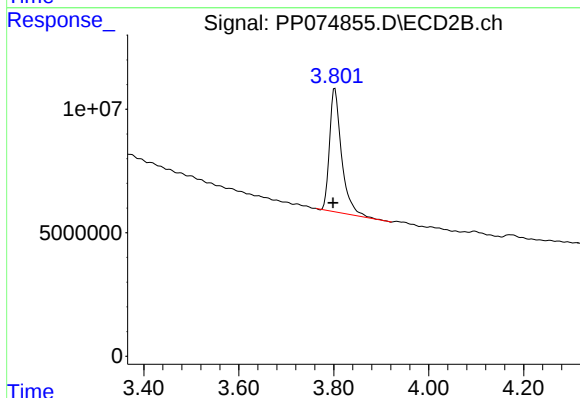


#1 Tetrachloro-m-xylene

R.T.: 3.802 min
Delta R.T.: 0.004 min
Response: 88158529
Conc: 18.23 ng/ml

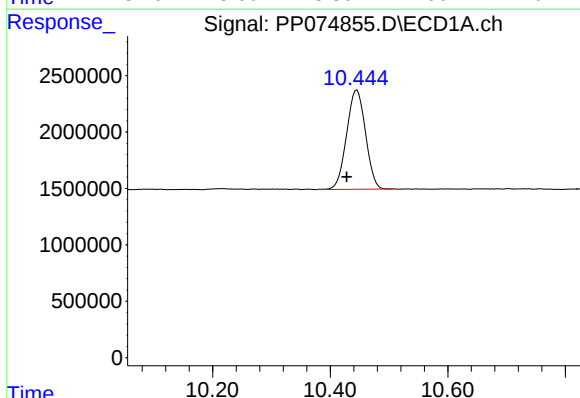


#2 Decachlorobiphenyl

R.T.: 10.445 min
Delta R.T.: 0.017 min
Response: 19632366
Conc: 19.88 ng/ml

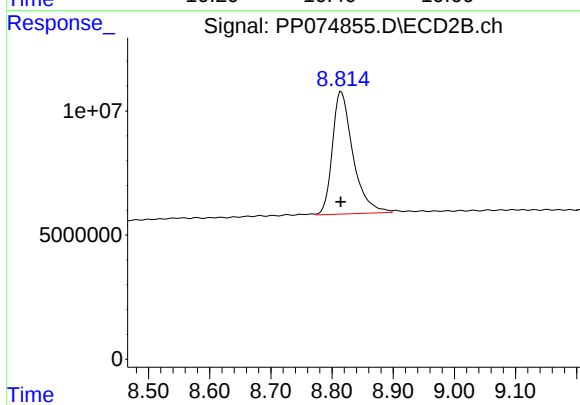

#2 Decachlorobiphenyl


R.T.: 8.815 min
Delta R.T.: 0.001 min
Response: 115305532
Conc: 15.38 ng/ml

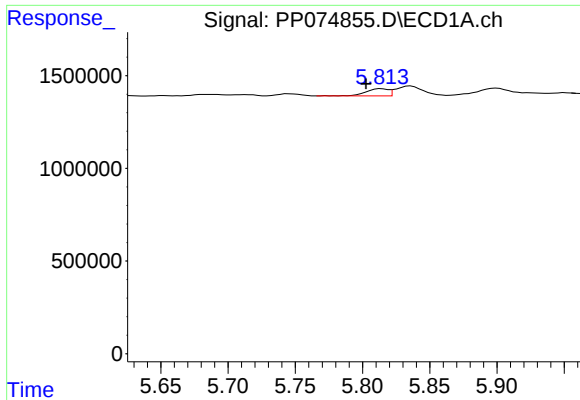

#3 AR-1016-1


R.T.: 5.814 min
Delta R.T.: 0.011 min
Response: 452296
Conc: 10.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

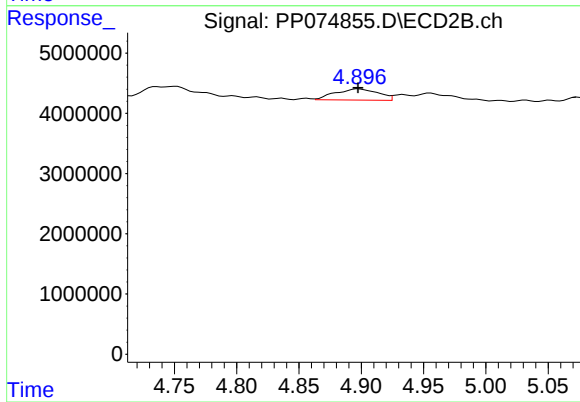


#3 AR-1016-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 4444290
Conc: 8.73 ng/ml

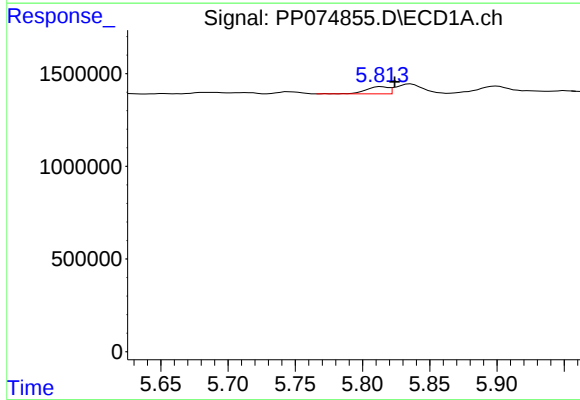


#4 AR-1016-2

R.T.: 5.814 min
Delta R.T.: -0.010 min
Response: 452296
Conc: 7.20 ng/ml

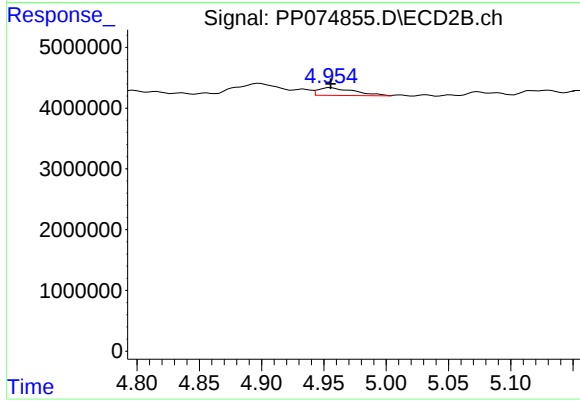

#4 AR-1016-2


R.T.: 4.955 min
Delta R.T.: 0.000 min
Response: 2548250
Conc: 10.71 ng/ml

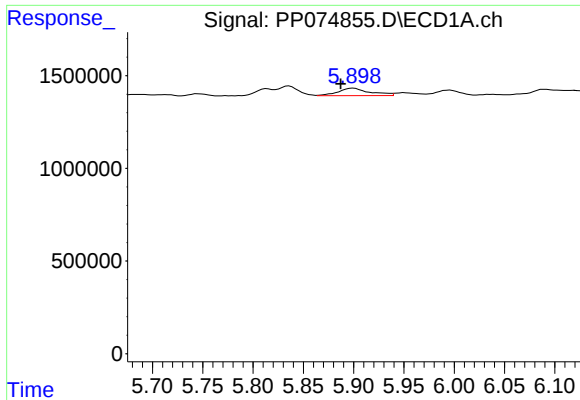

#5 AR-1016-3


R.T.: 5.900 min
Delta R.T.: 0.013 min
Response: 900689
Conc: 20.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

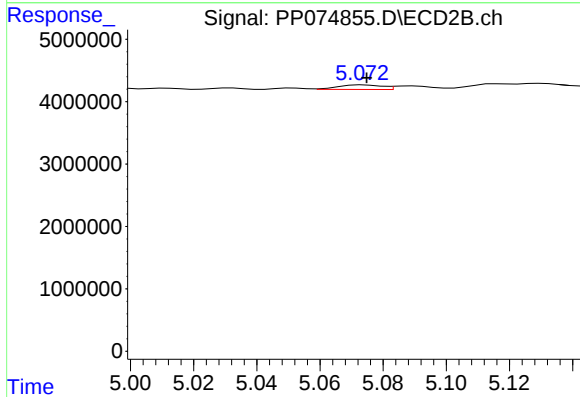


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 717966
Conc: 5.21 ng/ml

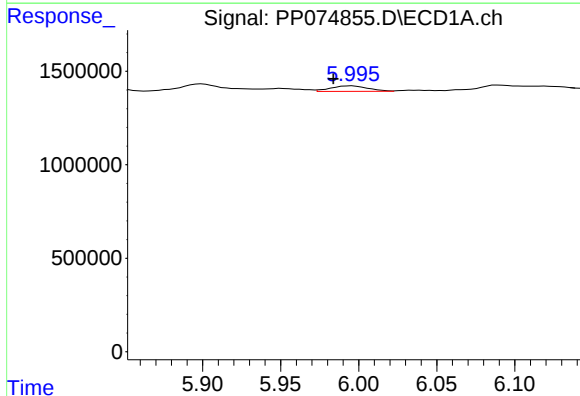


#6 AR-1016-4

R.T.: 5.996 min
Delta R.T.: 0.012 min
Response: 492059
Conc: 13.99 ng/ml

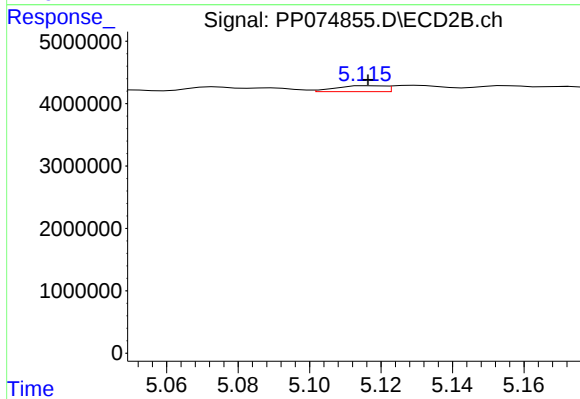

#6 AR-1016-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 900967
Conc: 6.44 ng/ml

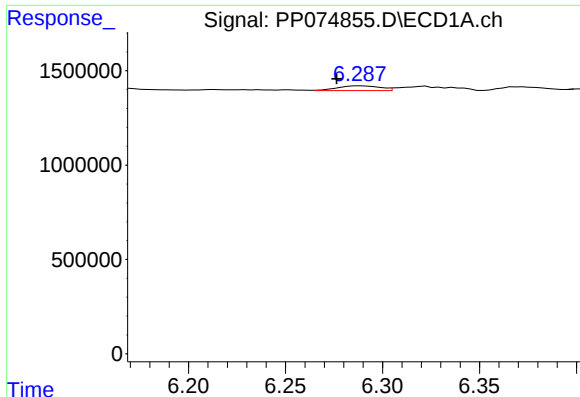

#7 AR-1016-5


R.T.: 6.289 min
Delta R.T.: 0.012 min
Response: 380114
Conc: 11.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

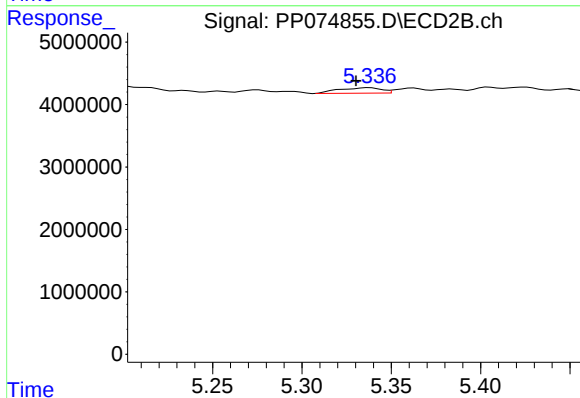


#7 AR-1016-5

R.T.: 5.338 min
Delta R.T.: 0.007 min
Response: 1483849
Conc: 8.93 ng/ml

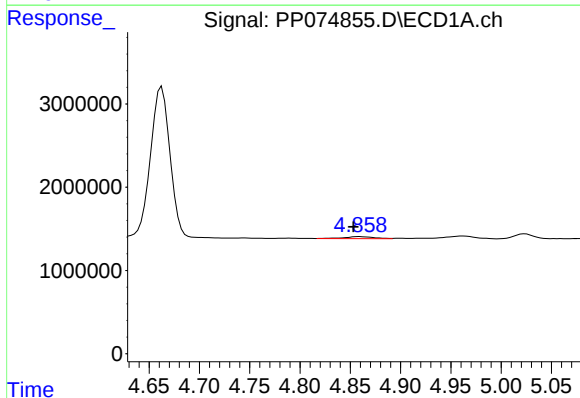


#8 AR-1221-1

R.T.: 4.859 min
Delta R.T.: 0.006 min
Response: 453447
Conc: 25.77 ng/ml

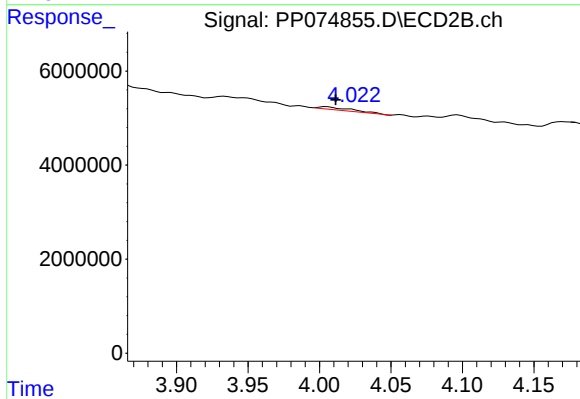

#8 AR-1221-1


R.T.: 4.005 min
Delta R.T.: -0.006 min
Response: 1023564
Conc: 16.54 ng/ml

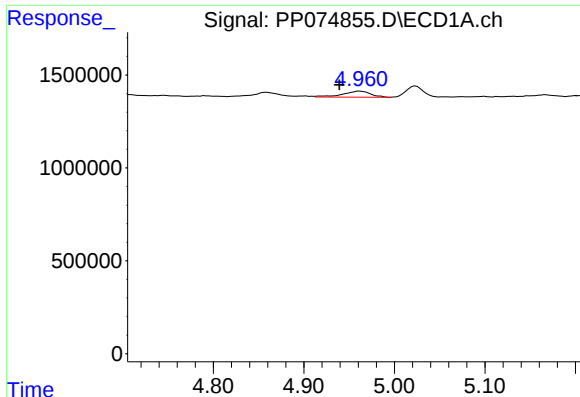

#9 AR-1221-2


R.T.: 4.962 min
Delta R.T.: 0.023 min
Response: 682364
Conc: 51.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

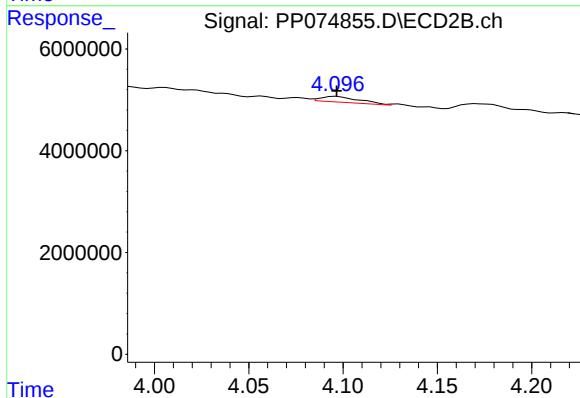


#9 AR-1221-2

R.T.: 4.096 min
Delta R.T.: 0.000 min
Response: 1608730
Conc: 35.58 ng/ml

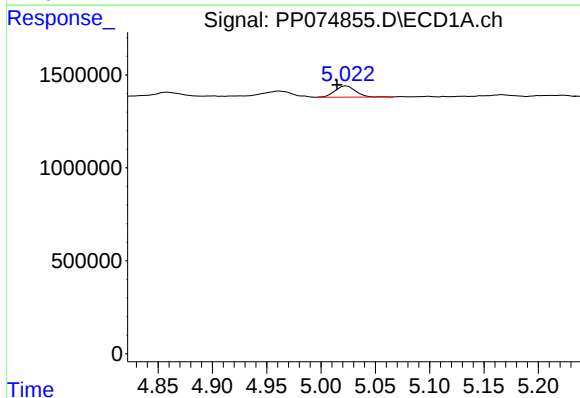


#10 AR-1221-3

R.T.: 5.024 min
Delta R.T.: 0.009 min
Response: 788183
Conc: 20.79 ng/ml

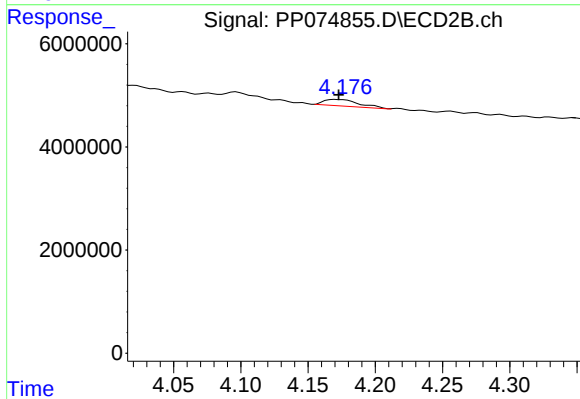

#10 AR-1221-3


R.T.: 4.171 min
Delta R.T.: -0.002 min
Response: 2329580
Conc: 14.18 ng/ml

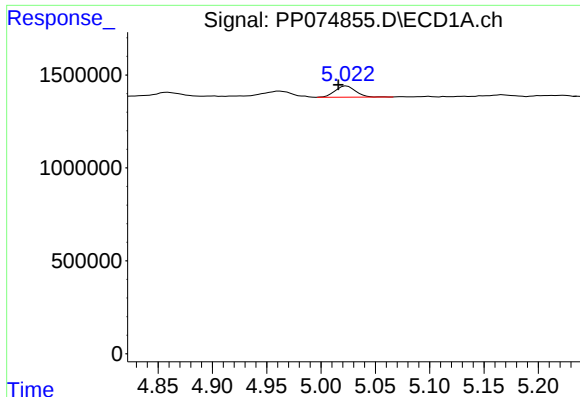

#11 AR-1232-1


R.T.: 5.024 min
Delta R.T.: 0.008 min
Response: 788183
Conc: 25.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

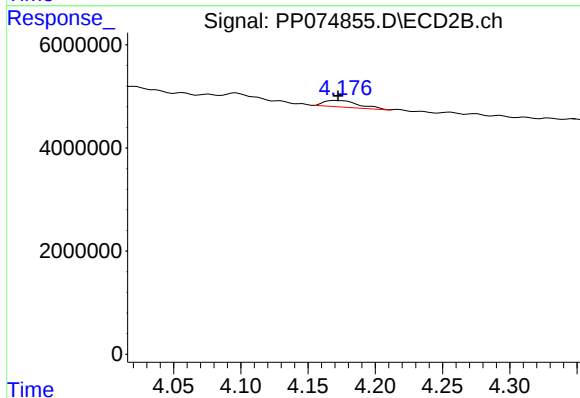


#11 AR-1232-1

R.T.: 4.171 min
Delta R.T.: -0.002 min
Response: 2329580
Conc: 18.19 ng/ml

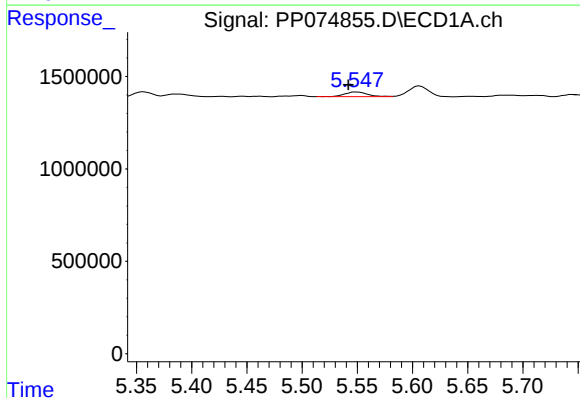


#12 AR-1232-2

R.T.: 5.549 min
Delta R.T.: 0.008 min
Response: 372901
Conc: 23.66 ng/ml

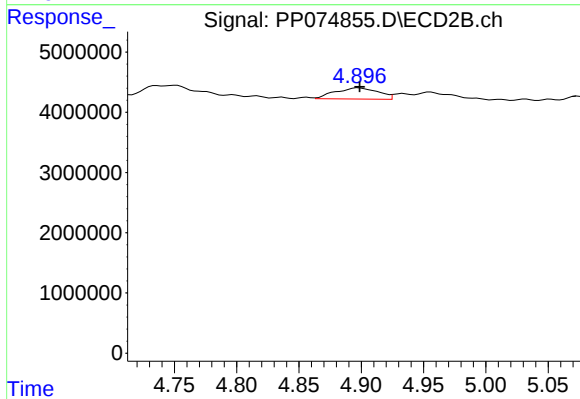

#12 AR-1232-2


R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 4444290
Conc: 19.17 ng/ml

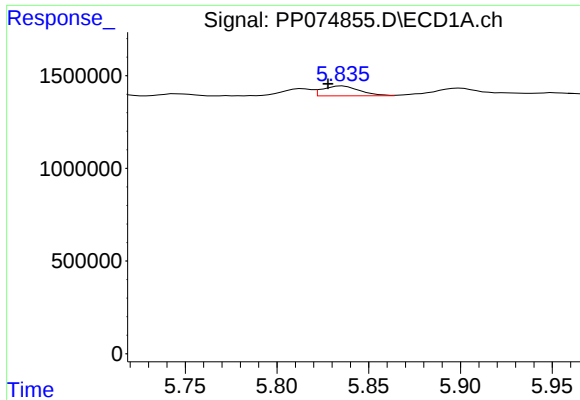

#13 AR-1232-3


R.T.: 5.836 min
Delta R.T.: 0.008 min
Response: 742470
Conc: 24.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

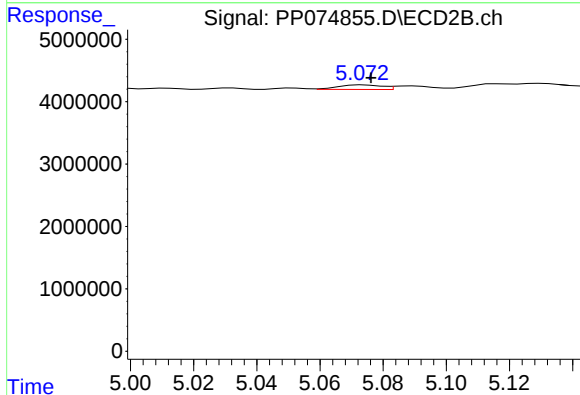


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 717966
Conc: 11.95 ng/ml

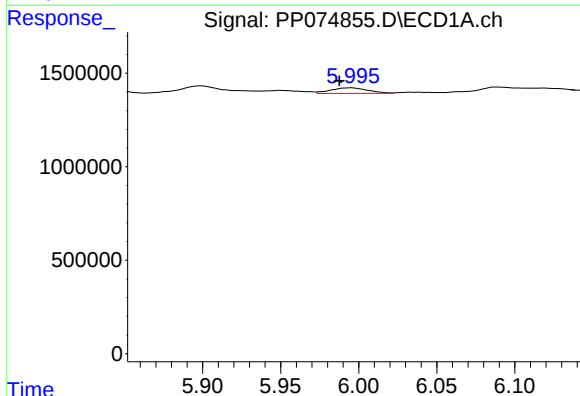


#14 AR-1232-4

R.T.: 5.996 min
Delta R.T.: 0.008 min
Response: 492059
Conc: 28.49 ng/ml

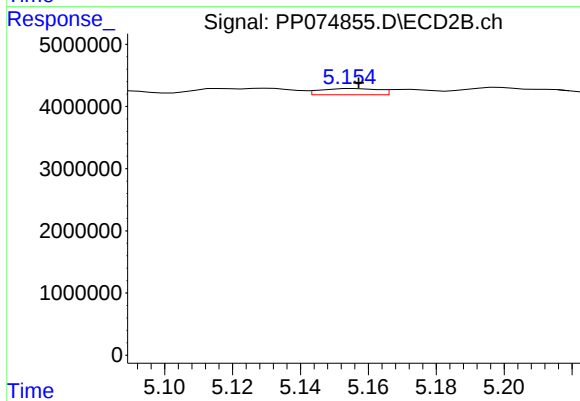

#14 AR-1232-4


R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 1183488
Conc: 16.06 ng/ml

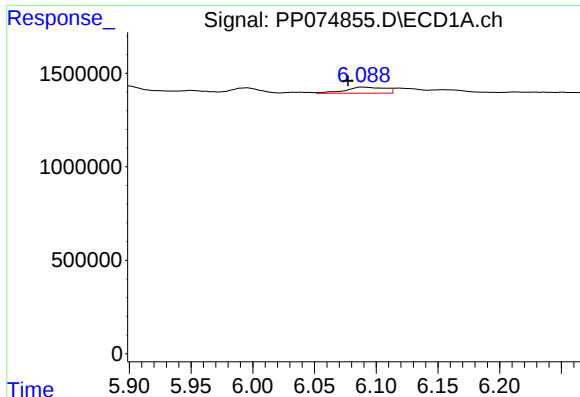

#15 AR-1232-5


R.T.: 6.089 min
Delta R.T.: 0.012 min
Response: 730856
Conc: 56.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

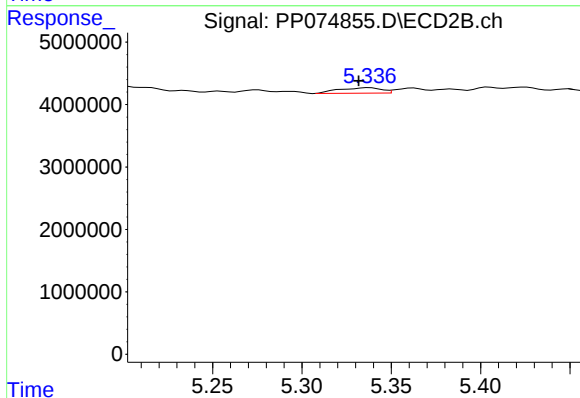


#15 AR-1232-5

R.T.: 5.338 min
Delta R.T.: 0.006 min
Response: 1483849
Conc: 23.90 ng/ml

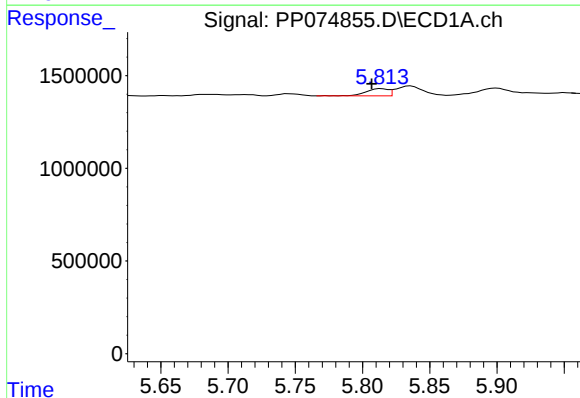


#16 AR-1242-1

R.T.: 5.814 min
Delta R.T.: 0.007 min
Response: 452296
Conc: 11.82 ng/ml

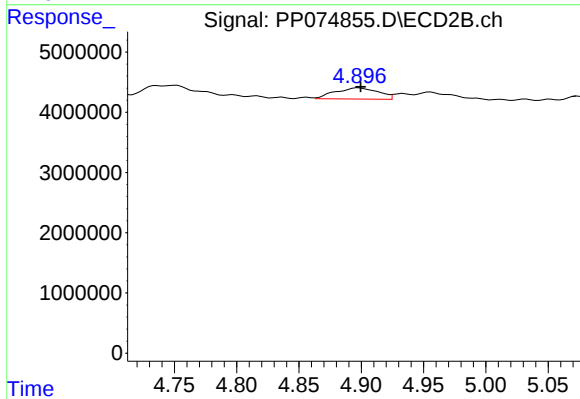

#16 AR-1242-1


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 4444290
Conc: 10.54 ng/ml

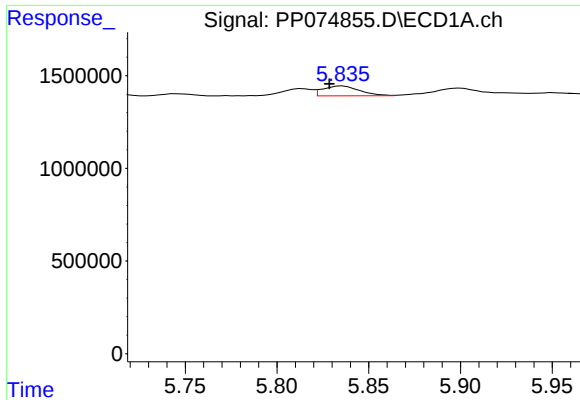

#17 AR-1242-2


R.T.: 5.836 min
Delta R.T.: 0.007 min
Response: 742470
Conc: 13.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

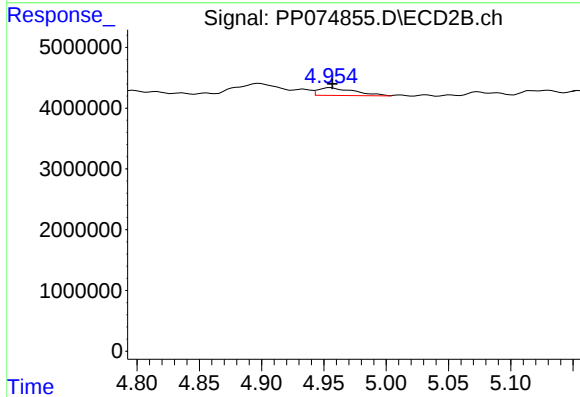


#17 AR-1242-2

R.T.: 4.955 min
Delta R.T.: -0.002 min
Response: 2548250
Conc: 12.72 ng/ml

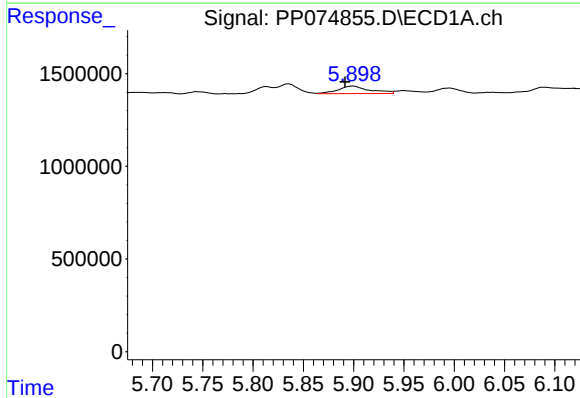


#18 AR-1242-3

R.T.: 5.900 min
Delta R.T.: 0.008 min
Response: 900689
Conc: 22.18 ng/ml

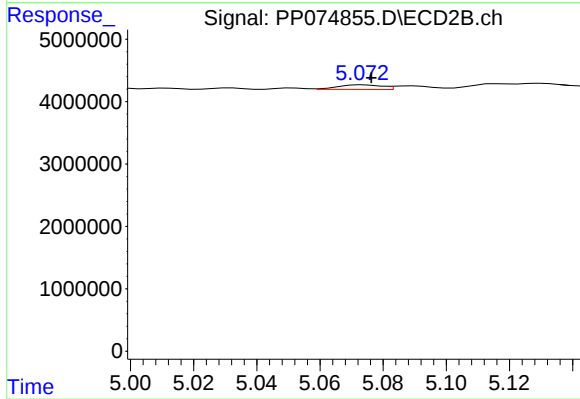

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 717966
Conc: 6.07 ng/ml

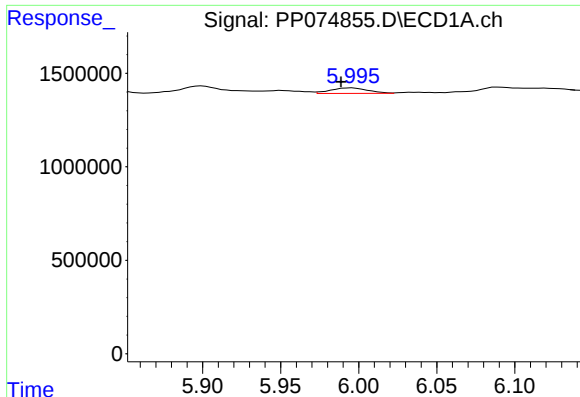

#19 AR-1242-4


R.T.: 5.996 min
Delta R.T.: 0.007 min
Response: 492059
Conc: 15.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

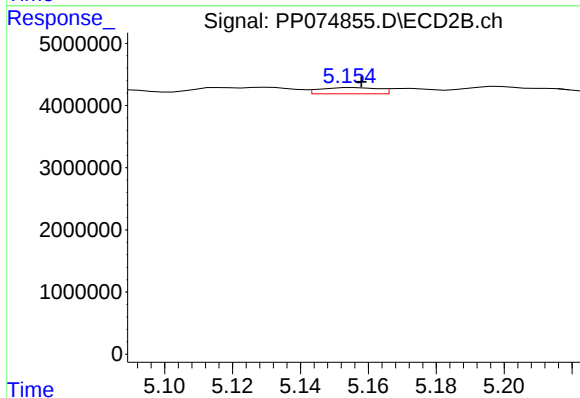


#19 AR-1242-4

R.T.: 5.155 min
Delta R.T.: -0.003 min
Response: 1183488
Conc: 6.91 ng/ml

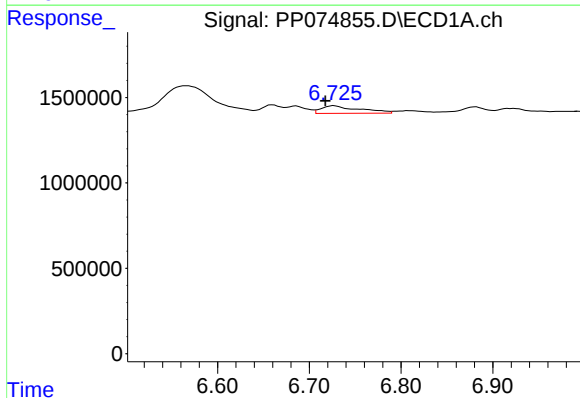


#20 AR-1242-5

R.T.: 6.727 min
Delta R.T.: 0.009 min
Response: 1287431
Conc: 35.69 ng/ml

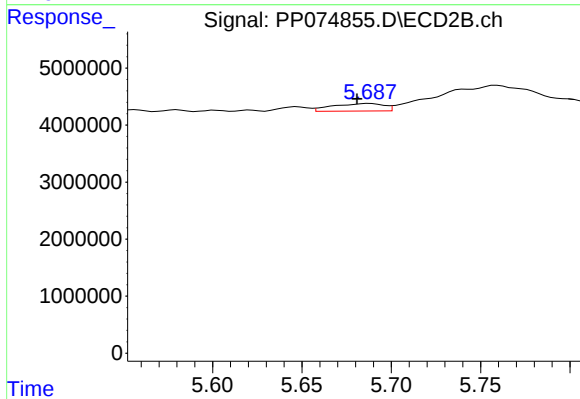

#20 AR-1242-5


R.T.: 5.688 min
Delta R.T.: 0.007 min
Response: 2631637
Conc: 14.21 ng/ml

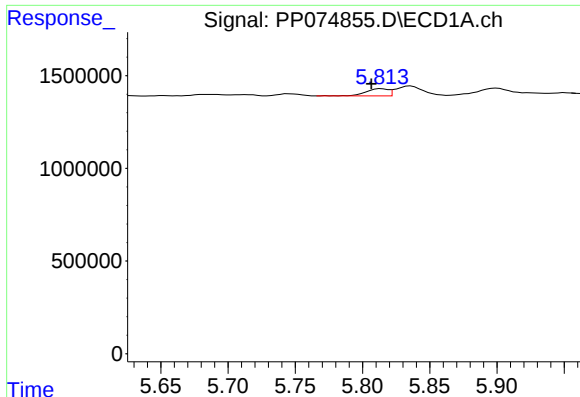

#21 AR-1248-1


R.T.: 5.814 min
Delta R.T.: 0.008 min
Response: 452296
Conc: 14.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

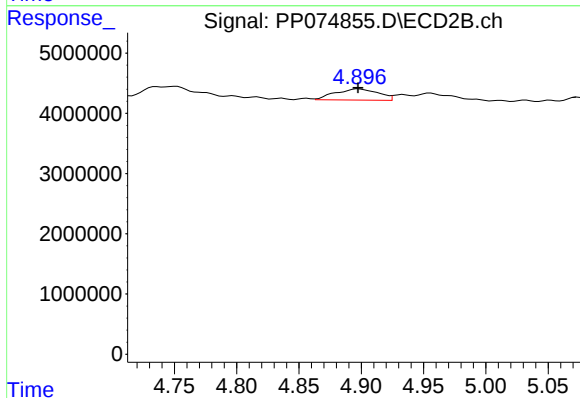


#21 AR-1248-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 4444290
Conc: 16.09 ng/ml

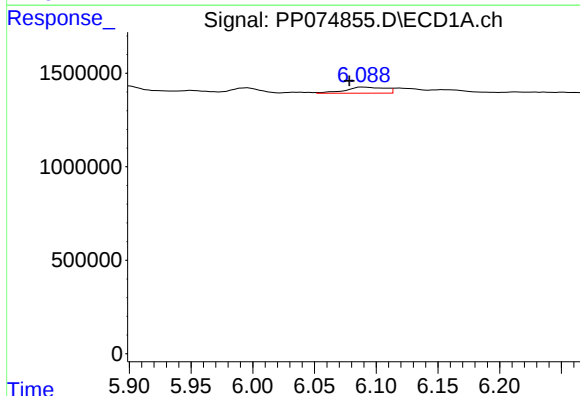


#22 AR-1248-2

R.T.: 6.089 min
Delta R.T.: 0.011 min
Response: 730856
Conc: 16.96 ng/ml

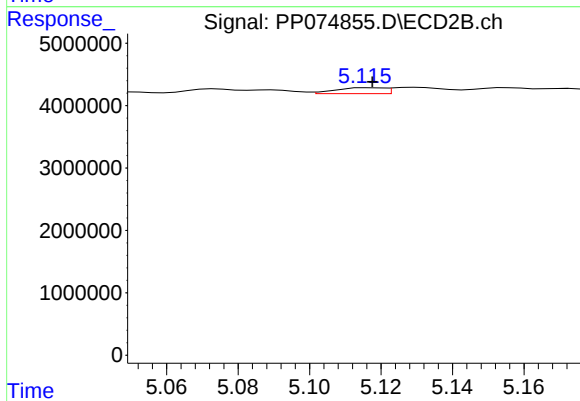

#22 AR-1248-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 900967
Conc: 5.10 ng/ml

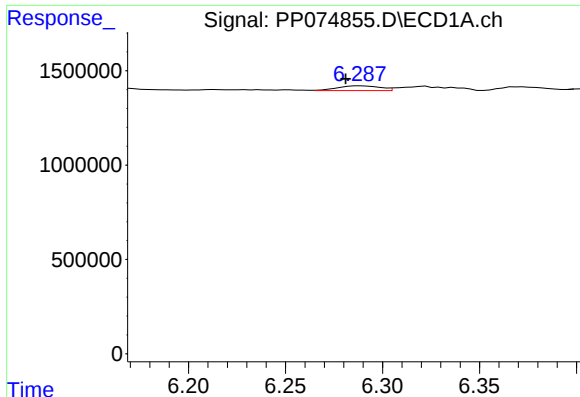

#23 AR-1248-3


R.T.: 6.289 min
Delta R.T.: 0.008 min
Response: 380114
Conc: 8.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

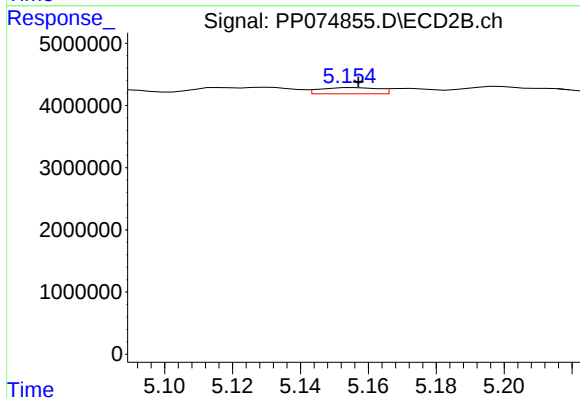


#23 AR-1248-3

R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 1183488
Conc: 5.21 ng/ml

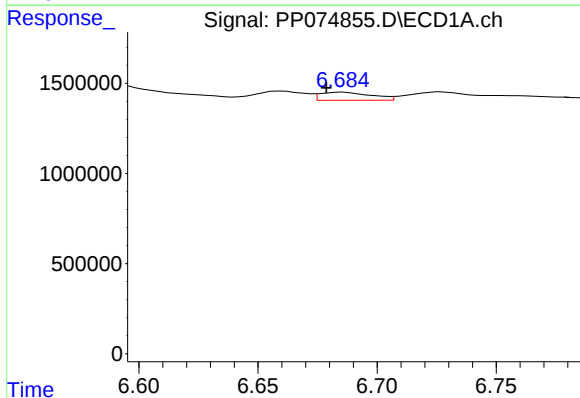


#24 AR-1248-4

R.T.: 6.686 min
Delta R.T.: 0.007 min
Response: 669075
Conc: 12.16 ng/ml

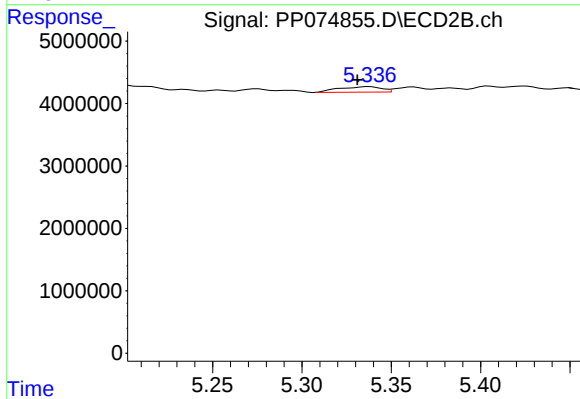

#24 AR-1248-4


R.T.: 5.338 min
Delta R.T.: 0.007 min
Response: 1483849
Conc: 6.81 ng/ml

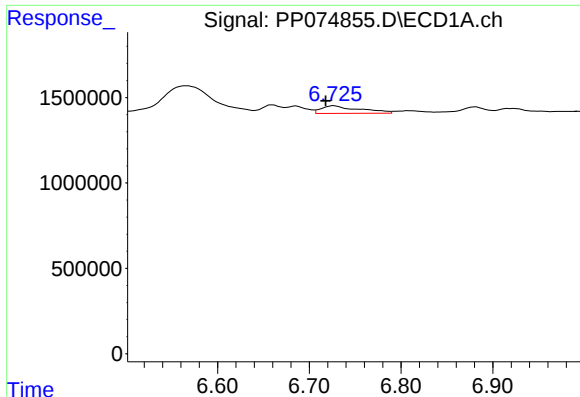

#25 AR-1248-5


R.T.: 6.727 min
Delta R.T.: 0.009 min
Response: 1287431
Conc: 23.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

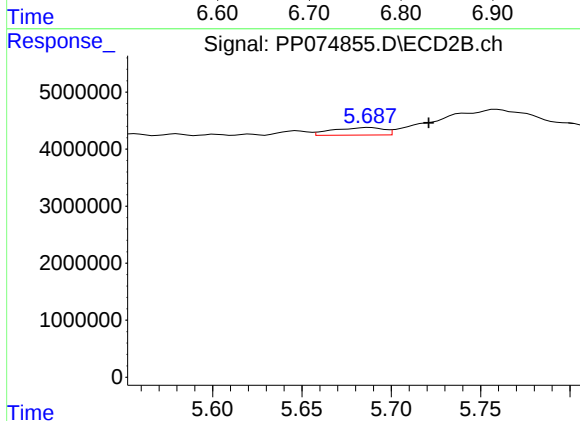


#25 AR-1248-5

R.T.: 5.688 min
Delta R.T.: -0.033 min
Response: 2631637
Conc: 7.16 ng/ml

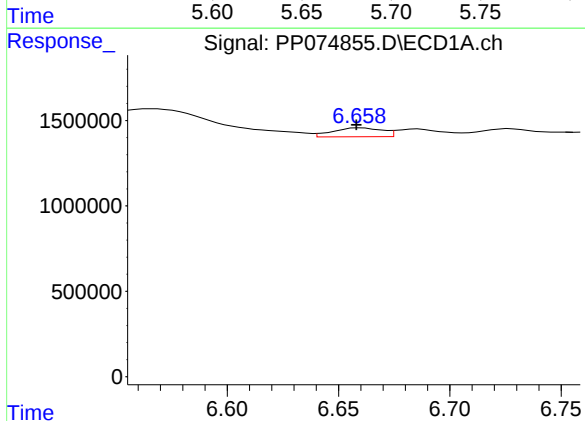


#26 AR-1254-1

R.T.: 6.660 min
Delta R.T.: 0.002 min
Response: 805785
Conc: 13.83 ng/ml

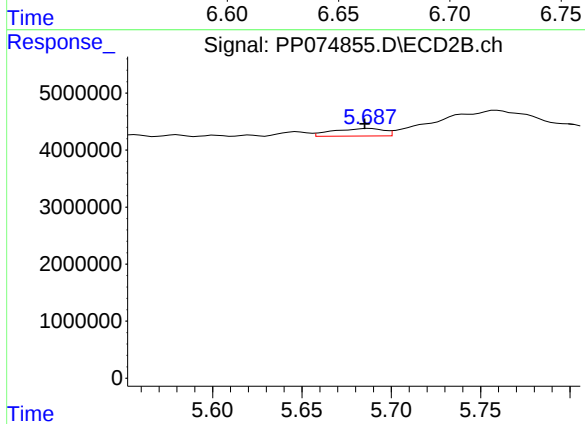

#26 AR-1254-1


R.T.: 5.688 min
Delta R.T.: 0.003 min
Response: 2631637
Conc: 5.52 ng/ml

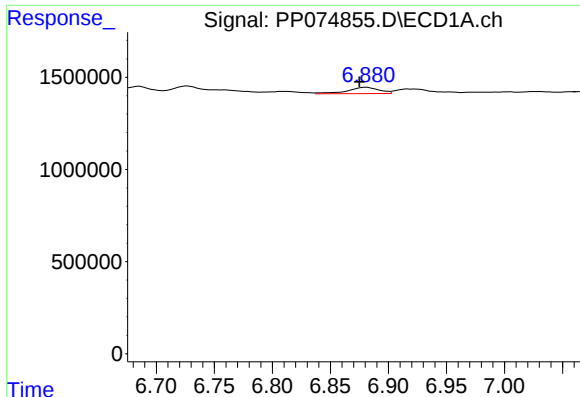

#27 AR-1254-2


R.T.: 6.881 min
Delta R.T.: 0.006 min
Response: 634715
Conc: 7.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

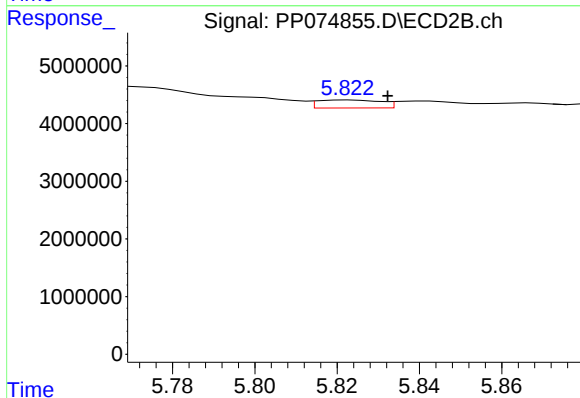


#27 AR-1254-2

R.T.: 5.823 min
Delta R.T.: -0.009 min
Response: 1473935
Conc: 4.19 ng/ml

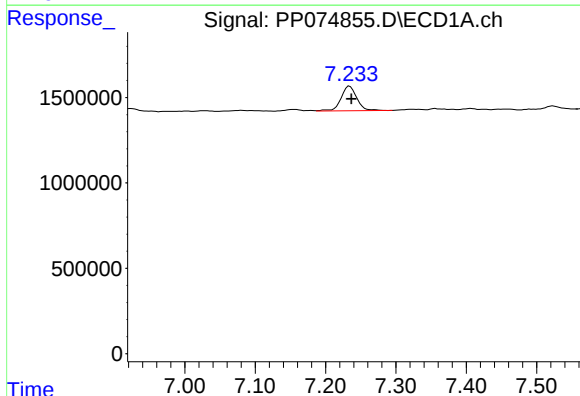


#28 AR-1254-3

R.T.: 7.234 min
Delta R.T.: -0.003 min
Response: 2244433
Conc: 25.16 ng/ml

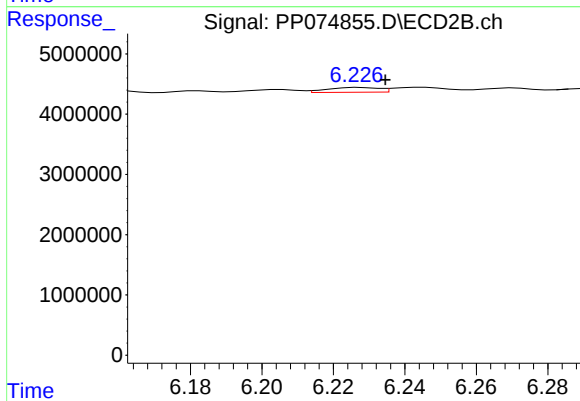

#28 AR-1254-3


R.T.: 6.227 min
Delta R.T.: -0.007 min
Response: 791950
Conc: 1.28 ng/ml

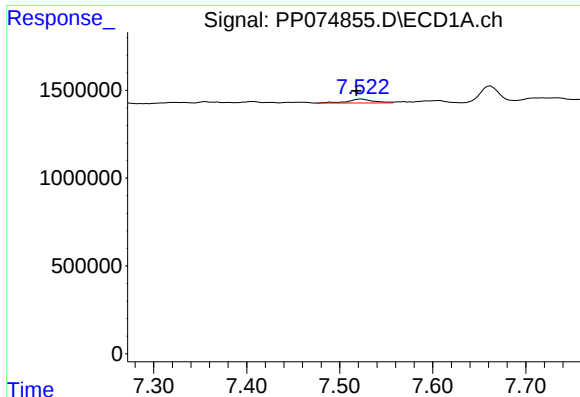

#29 AR-1254-4


R.T.: 7.523 min
Delta R.T.: 0.005 min
Response: 433598
Conc: 6.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

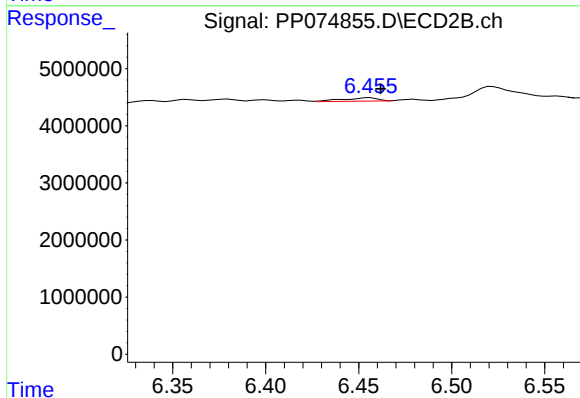


#29 AR-1254-4

R.T.: 6.456 min
Delta R.T.: -0.006 min
Response: 761451
Conc: 1.62 ng/ml

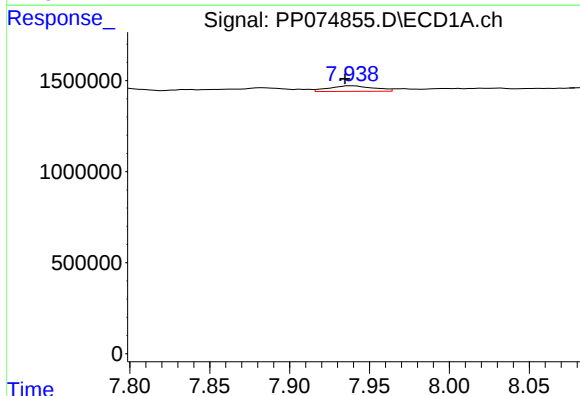


#30 AR-1254-5

R.T.: 7.939 min
Delta R.T.: 0.005 min
Response: 589567
Conc: 7.10 ng/ml

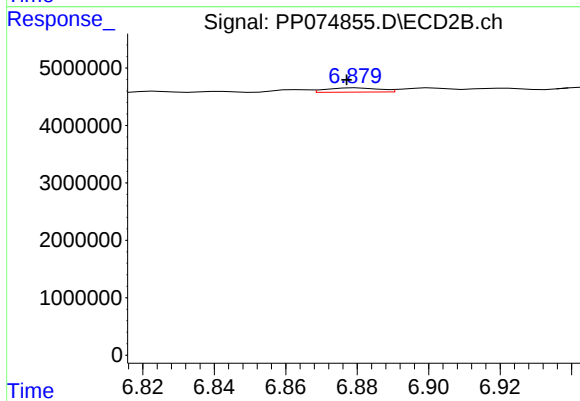

#30 AR-1254-5


R.T.: 6.880 min
Delta R.T.: 0.003 min
Response: 777893
Conc: 1.59 ng/ml

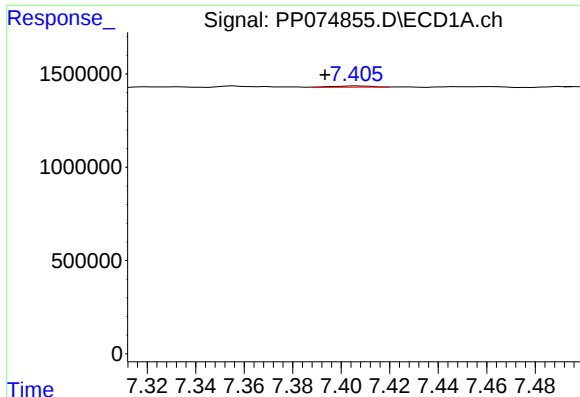

#31 AR-1260-1


R.T.: 7.407 min
Delta R.T.: 0.013 min
Response: 68929
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

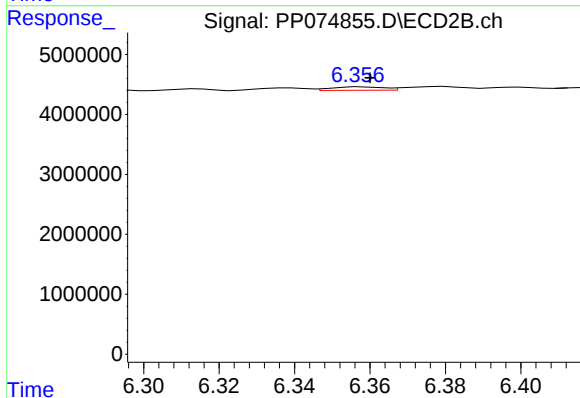


#31 AR-1260-1

R.T.: 6.357 min
Delta R.T.: -0.003 min
Response: 549662
Conc: 1.46 ng/ml

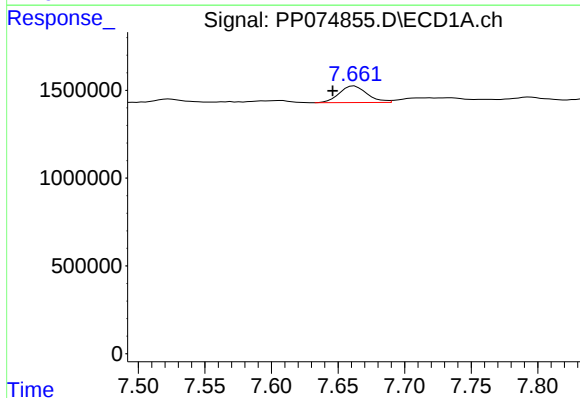


#32 AR-1260-2

R.T.: 7.662 min
Delta R.T.: 0.016 min
Response: 1374938
Conc: 19.95 ng/ml

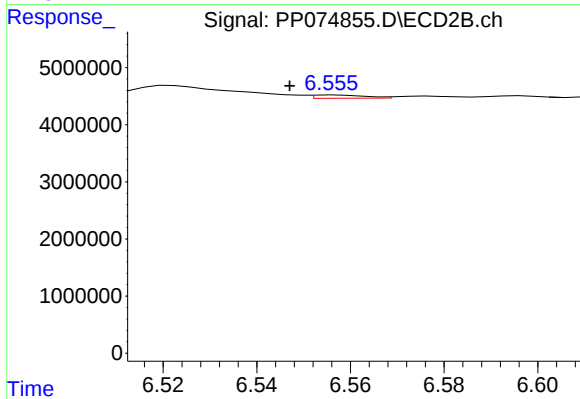

#32 AR-1260-2


R.T.: 6.557 min
Delta R.T.: 0.010 min
Response: 449186
Conc: 0.85 ng/ml

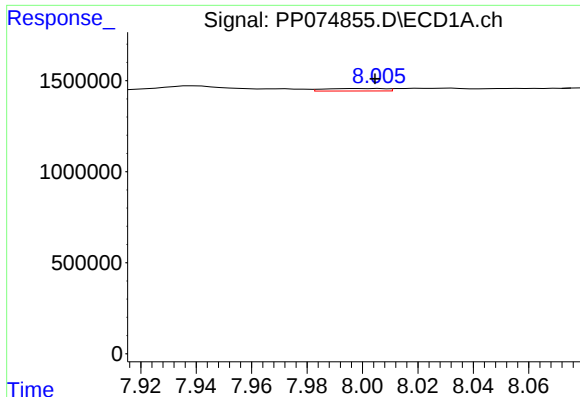

#33 AR-1260-3


R.T.: 8.006 min
Delta R.T.: 0.001 min
Response: 209847
Conc: 4.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

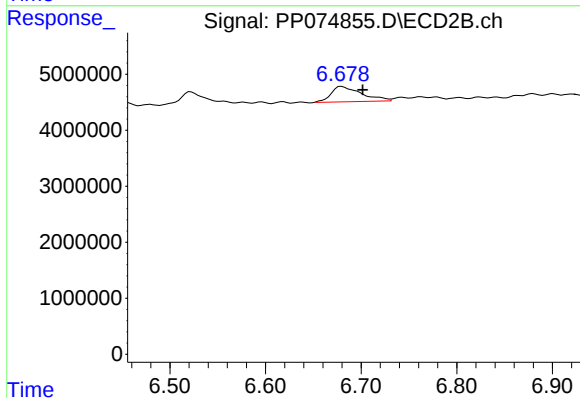


#33 AR-1260-3

R.T.: 6.680 min
Delta R.T.: -0.022 min
Response: 6072012
Conc: 14.02 ng/ml

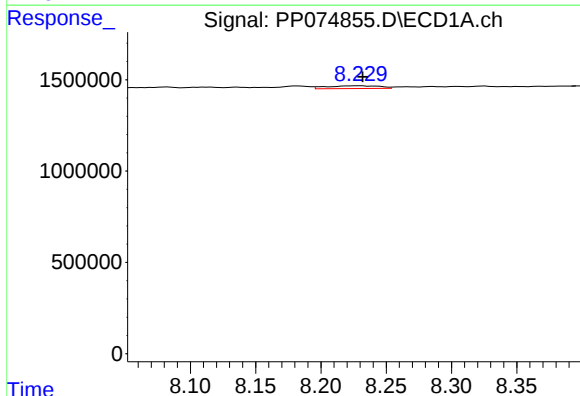


#34 AR-1260-4

R.T.: 8.230 min
Delta R.T.: -0.002 min
Response: 428136
Conc: 6.71 ng/ml

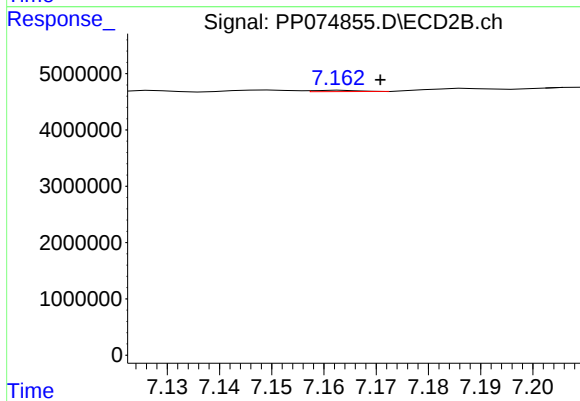

#34 AR-1260-4


R.T.: 7.164 min
Delta R.T.: -0.007 min
Response: 139302
Conc: 0.37 ng/ml

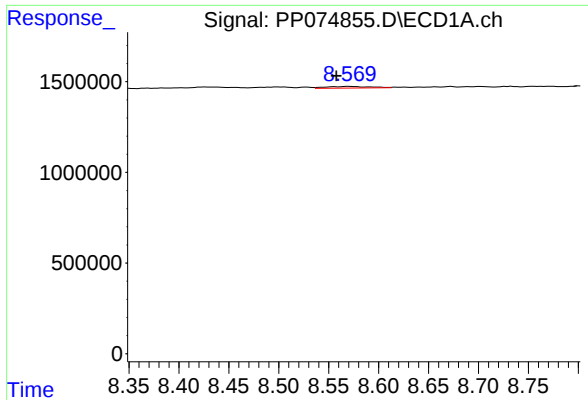

#35 AR-1260-5


R.T.: 8.571 min
Delta R.T.: 0.013 min
Response: 279003
Conc: 2.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

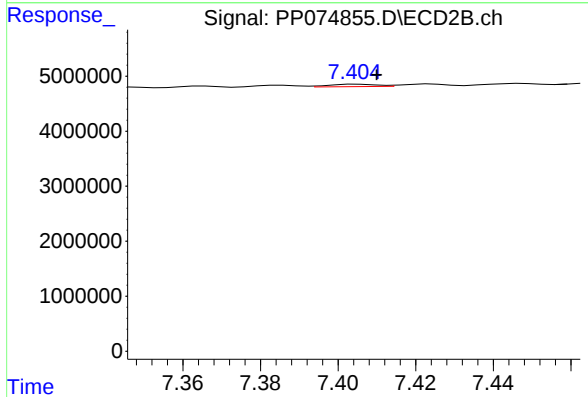


#35 AR-1260-5

R.T.: 7.405 min
Delta R.T.: -0.005 min
Response: 373053
Conc: 0.37 ng/ml

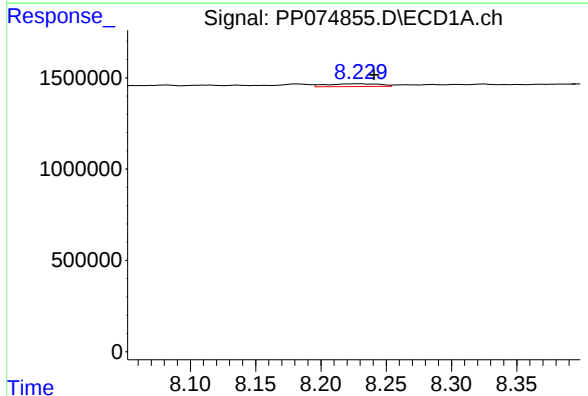


#36 AR-1262-1

R.T.: 8.230 min
Delta R.T.: -0.011 min
Response: 428136
Conc: 5.56 ng/ml

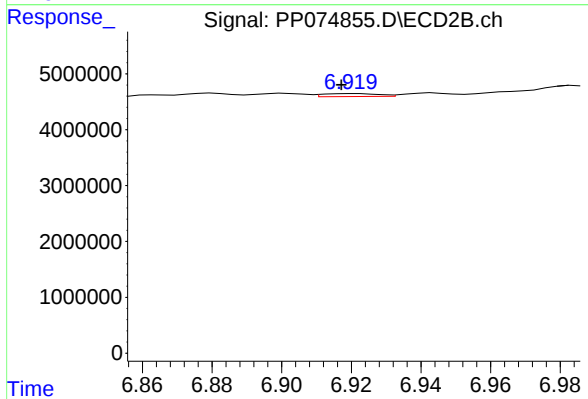

#36 AR-1262-1


R.T.: 6.921 min
Delta R.T.: 0.004 min
Response: 580285
Conc: 0.82 ng/ml

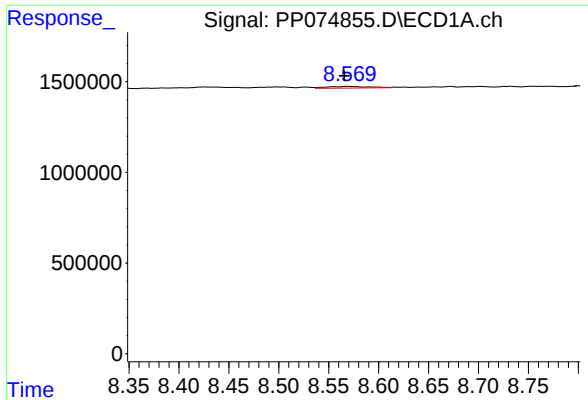

#37 AR-1262-2


R.T.: 8.571 min
Delta R.T.: 0.005 min
Response: 279003
Conc: 2.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

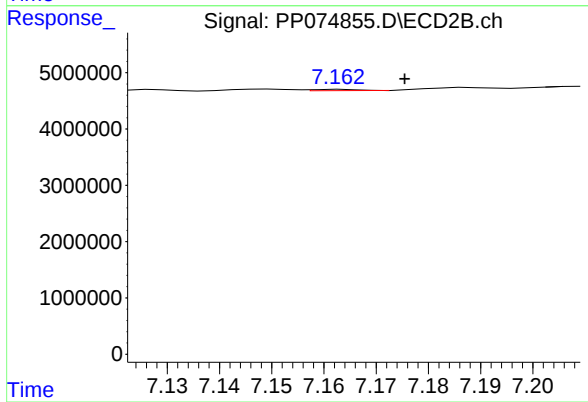


#37 AR-1262-2

R.T.: 7.164 min
Delta R.T.: -0.012 min
Response: 139302
Conc: 0.27 ng/ml

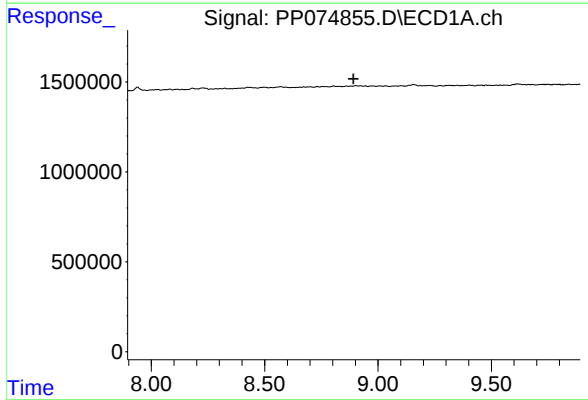


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

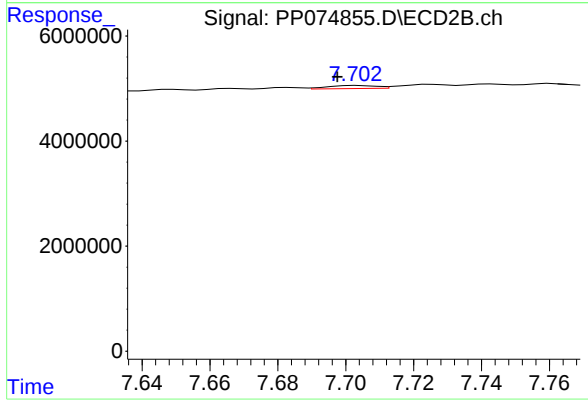

#38 AR-1262-3


R.T.: 7.703 min
Delta R.T.: 0.006 min
Response: 575798
Conc: 1.23 ng/ml

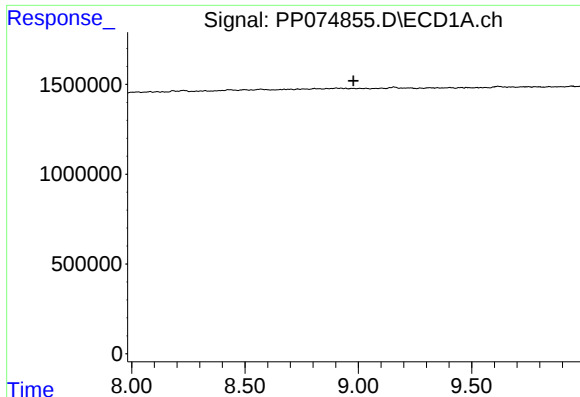

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

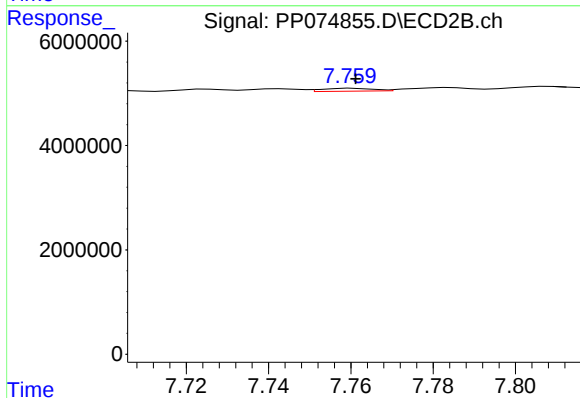


#39 AR-1262-4

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 481830
Conc: 0.59 ng/ml

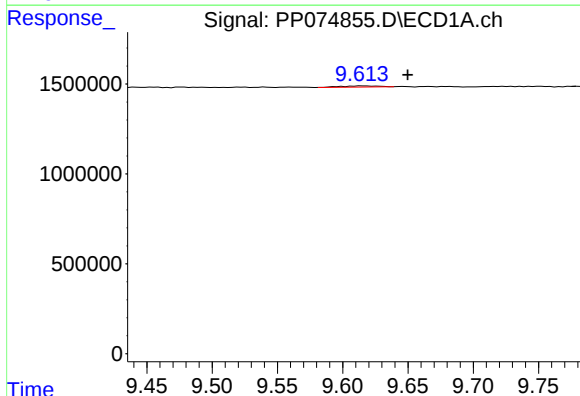


#40 AR-1262-5

R.T.: 9.615 min
Delta R.T.: -0.035 min
Response: 128805
Conc: 2.11 ng/ml

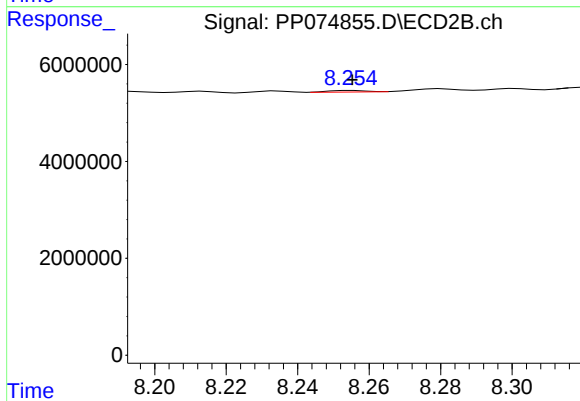

#40 AR-1262-5


R.T.: 8.255 min
Delta R.T.: 0.000 min
Response: 223427
Conc: 0.62 ng/ml

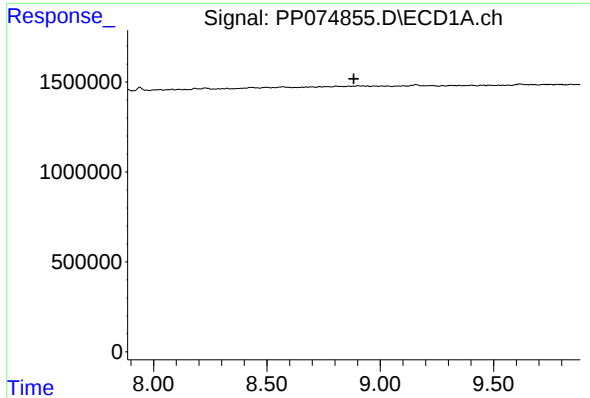

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

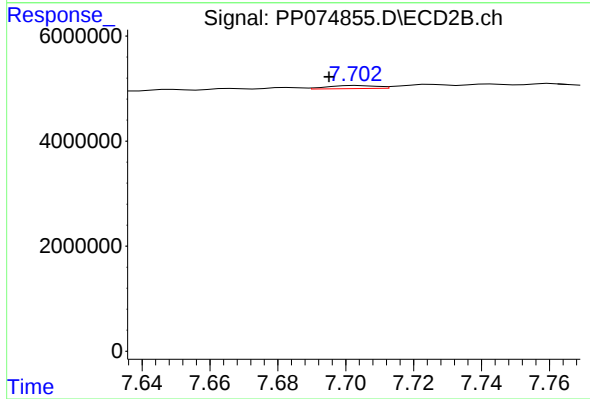


#41 AR-1268-1

R.T.: 7.703 min
Delta R.T.: 0.008 min
Response: 575798
Conc: 0.41 ng/ml

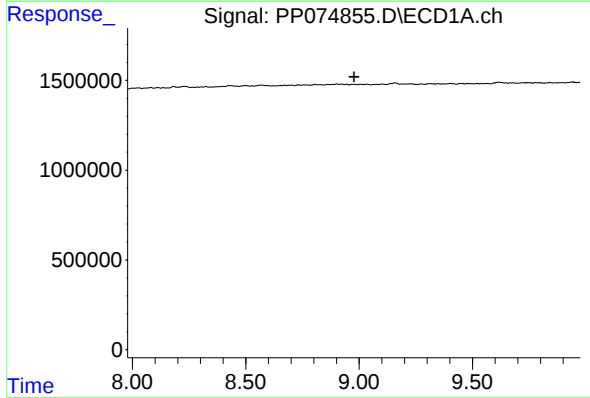


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

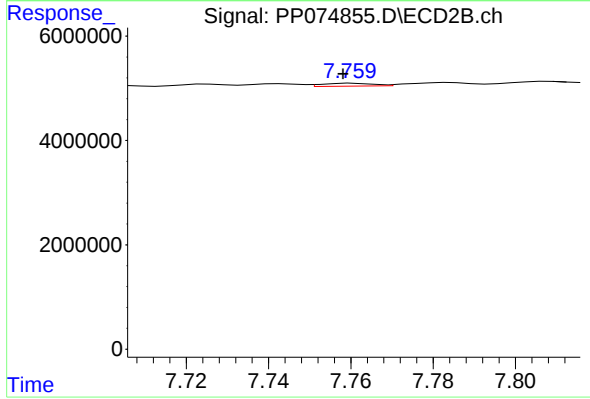

#42 AR-1268-2


R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 481830
Conc: 0.35 ng/ml

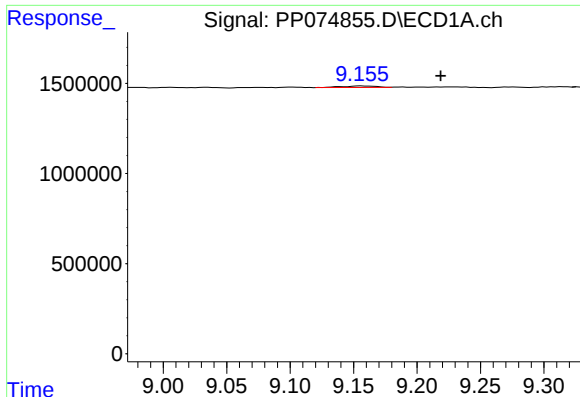

#43 AR-1268-3


R.T.: 9.156 min
Delta R.T.: -0.063 min
Response: 164587
Conc: 1.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

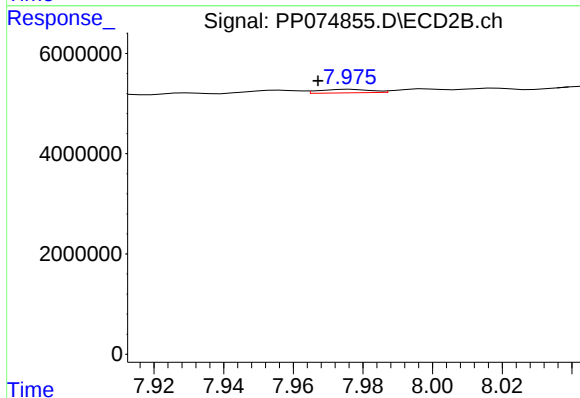


#43 AR-1268-3

R.T.: 7.977 min
Delta R.T.: 0.010 min
Response: 727754
Conc: 0.70 ng/ml

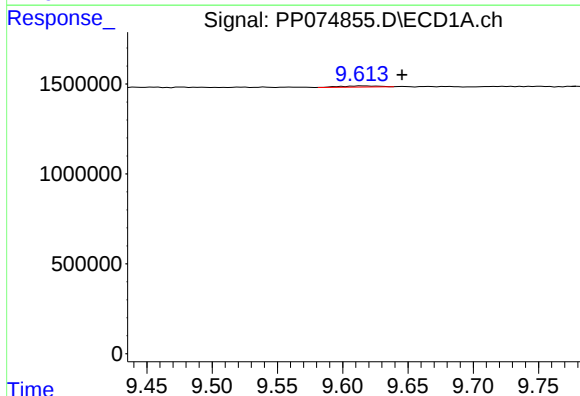


#44 AR-1268-4

R.T.: 9.615 min
Delta R.T.: -0.031 min
Response: 128805
Conc: 1.91 ng/ml

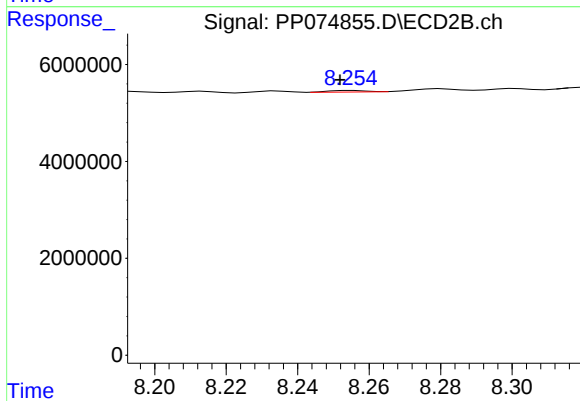

#44 AR-1268-4


R.T.: 8.255 min
Delta R.T.: 0.004 min
Response: 223427
Conc: 0.58 ng/ml

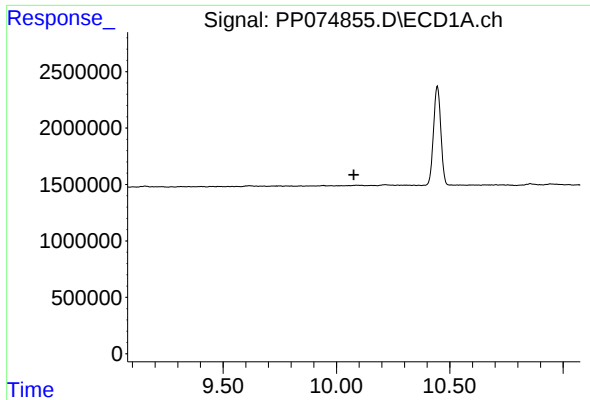

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

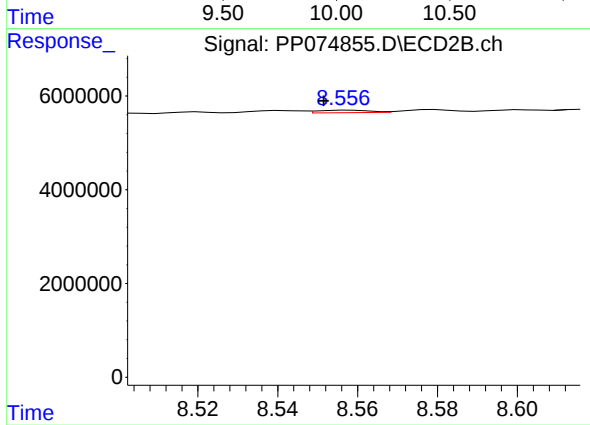

#45 AR-1268-5

R.T.: 8.558 min
Delta R.T.: 0.007 min
Response: 500289
Conc: 0.16 ng/ml