

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074856.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 13:45
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1242 WATER LOD 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:00:02 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.661	3.800	25507595	91738008	20.845	18.972
2)	SA Decachlor...	10.444	8.814	20102170	118.3E6	20.356	15.772
Target Compounds							
3)	L1 AR-1016-1	5.812	4.897	965743	8118735	21.904	15.939 #
4)	L1 AR-1016-2	5.834	4.957	1454045	4535959	23.138	19.057
5)	L1 AR-1016-3	5.897	5.072	1176484	2317691	26.194	16.807 #
6)	L1 AR-1016-4	5.993	5.123	831997	3222783	23.649	23.052
7)	L1 AR-1016-5	6.287	5.329	715355	2968845	21.556	17.876
8)	L2 AR-1221-1	4.858	4.015	650550	435333	36.978	7.037 #
9)	L2 AR-1221-2	4.963	4.100	556010	1569057	41.626	34.704
10)	L2 AR-1221-3	5.022	4.166	517144	1468443	13.640	8.938 #
11)	L3 AR-1232-1	5.022	4.166	517144	1468443	17.026	11.464 #
12)	L3 AR-1232-2	5.547	4.897	740670	8118735	47.002	35.026 #
13)	L3 AR-1232-3	5.834	5.072	1454045	2317691	47.605	38.590
14)	L3 AR-1232-4	5.993	5.164	831997	3511272	48.178	47.638
15)	L3 AR-1232-5	6.083	5.329	744260	2968845	57.335	47.820
16)	L4 AR-1242-1	5.812	4.897	965743	8118735	25.232	19.250
17)	L4 AR-1242-2	5.834	4.957	1454045	4535959	25.744	22.648
18)	L4 AR-1242-3	5.897	5.072	1176484	2317691	28.975	19.592 #
19)	L4 AR-1242-4	5.993	5.164	831997	3511272	26.211	20.515
20)	L4 AR-1242-5	6.724	5.682	1458131	4490170	40.424	24.250 #
21)	L5 AR-1248-1	5.812	4.897	965743	8118735	31.953	29.400
22)	L5 AR-1248-2	6.083	5.123	744260	3222783	17.270	18.233
23)	L5 AR-1248-3	6.287	5.164	715355	3511272	15.317	15.454
24)	L5 AR-1248-4	6.684	5.329	926188	2968845	16.840	13.617
25)	L5 AR-1248-5	6.724	5.753	1458131	11802011	26.287	32.130
26)	L6 AR-1254-1	6.659	5.682	978440	4490170	16.792	9.419 #
27)	L6 AR-1254-2	6.880	5.833	772031	2536476	9.459	7.203
28)	L6 AR-1254-3	7.233	6.228	2571665	1590052	28.828	2.565 #
29)	L6 AR-1254-4	7.520	6.458	595357	1085081	9.032	2.315 #
30)	L6 AR-1254-5	7.938	6.875	560002	1516786	6.740	3.092 #
31)	L7 AR-1260-1	7.405	6.365	74690	679454	1.292	1.811 #
32)	L7 AR-1260-2	7.657	6.558	465351	441035	6.752	0.834 #
33)	L7 AR-1260-3	8.004	6.704	335772	908087	6.471	2.097 #
34)	L7 AR-1260-4	8.226	7.179	175274	190338	2.748	0.499 #
35)	L7 AR-1260-5	8.560	7.414	39158	384750	0.345	0.383
36)	L8 AR-1262-1	8.226	6.915	175274	559772	2.276	0.791 #
37)	L8 AR-1262-2	8.560	7.179	39158	190338	0.296	0.366
38)	L8 AR-1262-3	0.000	7.696	0	842383	N.D.	1.807 #
39)	L8 AR-1262-4	0.000	7.761	0	1174769	N.D.	1.429 #
40)	L8 AR-1262-5	9.622	8.257	99847	326352	1.638	0.911 #
41)	L9 AR-1268-1	0.000	7.696	0	842383	N.D.	0.597 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 13:45
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1242 WATER LOD 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:00:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.761	0	1174769	N.D.	0.862 #
43) L9	AR-1268-3	9.164f	7.961	94372	574519	0.764	0.551 #
44) L9	AR-1268-4	9.622	8.257	99847	326352	1.484	0.852 #
45) L9	AR-1268-5	10.094	8.557	86274	432525	0.233	0.138 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP074856\
Data File : PP074856.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 13:45
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1242 WATER LOD 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:00:02 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

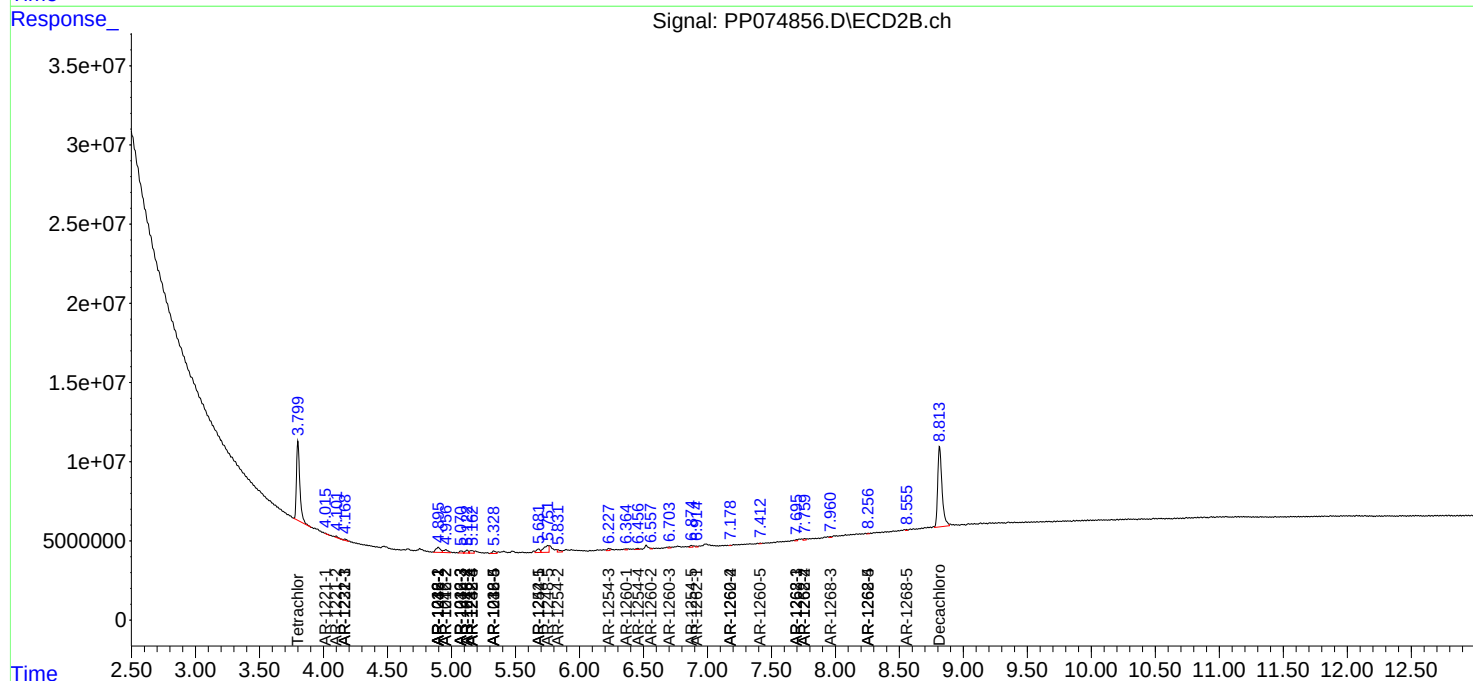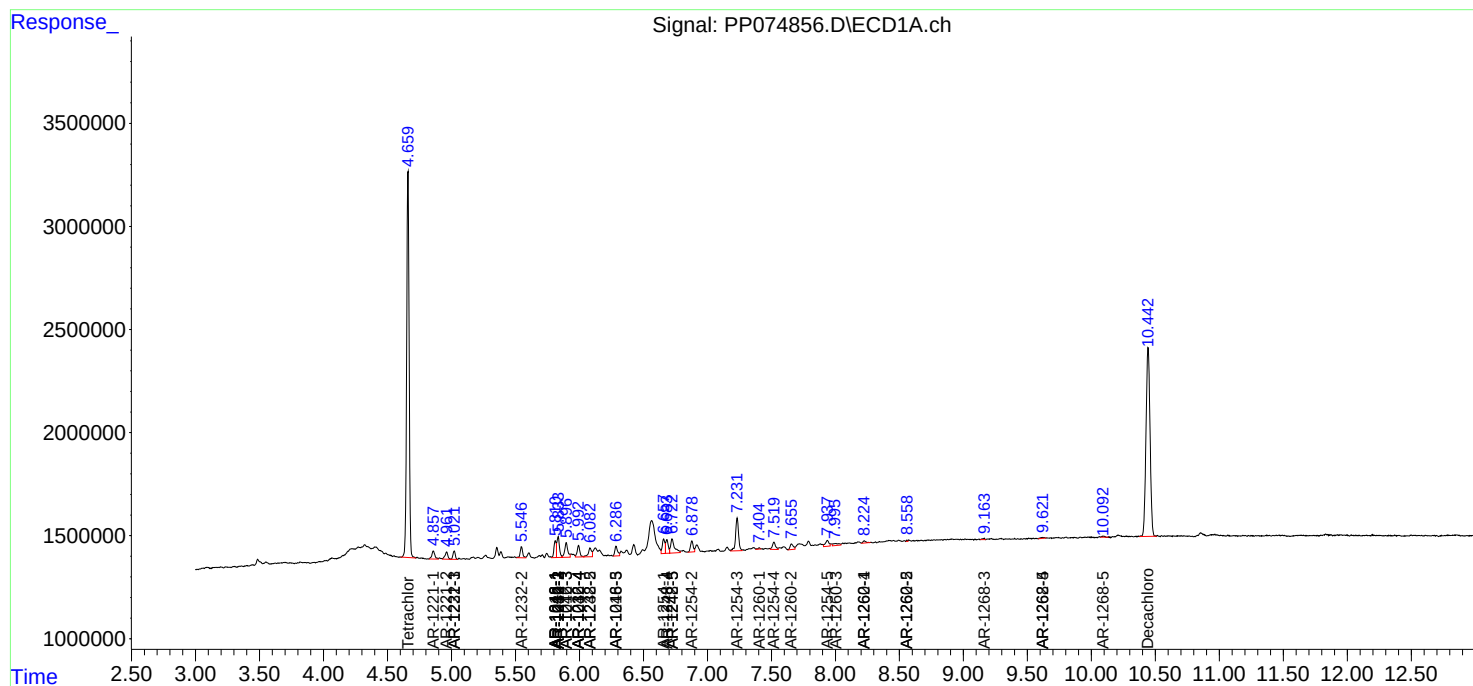


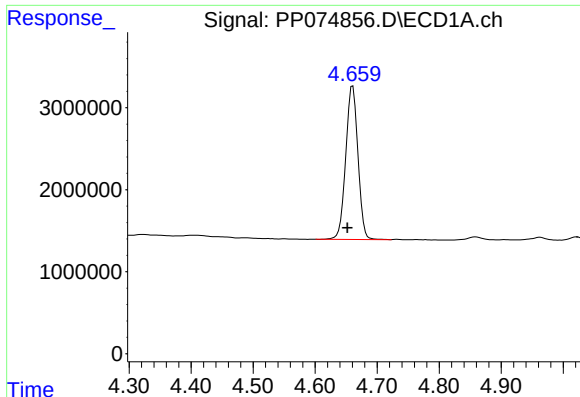

#1 Tetrachloro-m-xylene


R.T.: 4.661 min
Delta R.T.: 0.009 min
Response: 25507595
Conc: 20.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

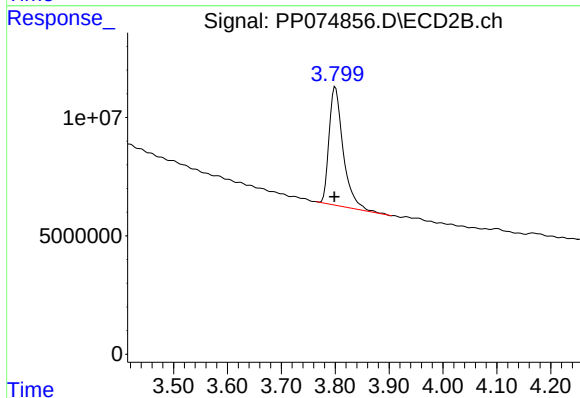


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.002 min
Response: 91738008
Conc: 18.97 ng/ml

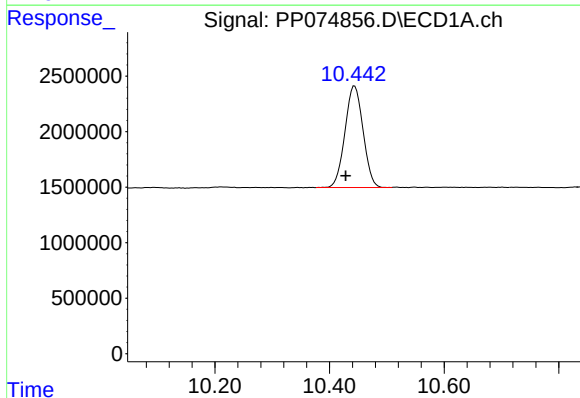


#2 Decachlorobiphenyl

R.T.: 10.444 min
Delta R.T.: 0.015 min
Response: 20102170
Conc: 20.36 ng/ml

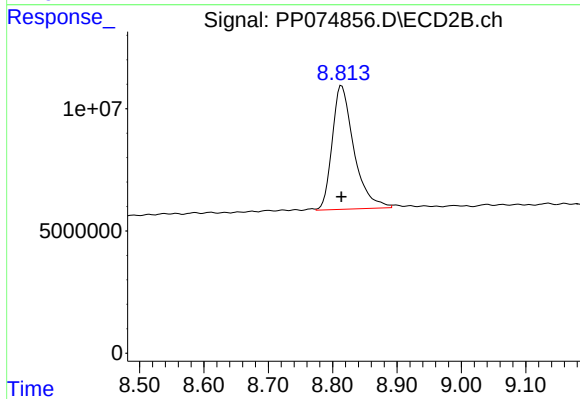

#2 Decachlorobiphenyl


R.T.: 8.814 min
Delta R.T.: 0.000 min
Response: 118279193
Conc: 15.77 ng/ml

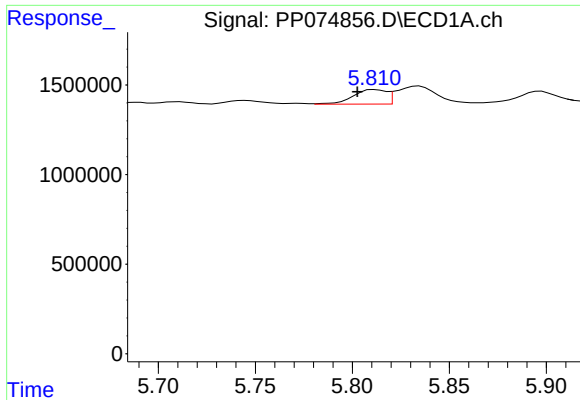

#3 AR-1016-1


R.T.: 5.812 min
Delta R.T.: 0.009 min
Response: 965743
Conc: 21.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

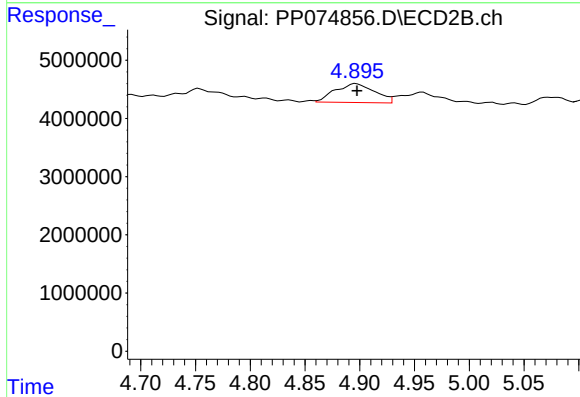


#3 AR-1016-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 8118735
Conc: 15.94 ng/ml

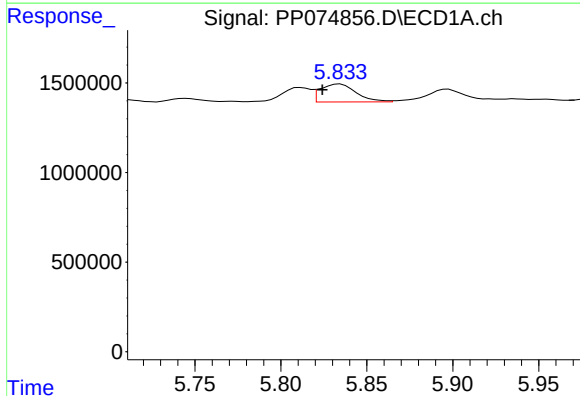


#4 AR-1016-2

R.T.: 5.834 min
Delta R.T.: 0.010 min
Response: 1454045
Conc: 23.14 ng/ml

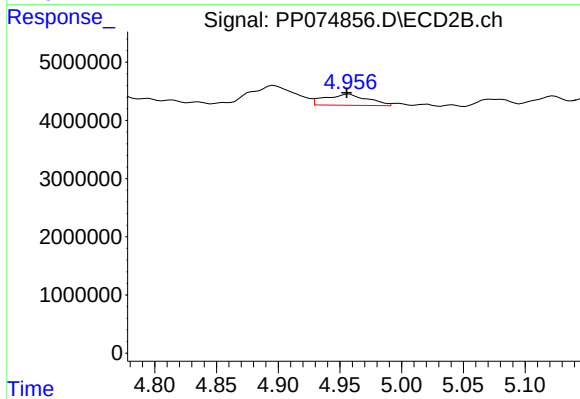

#4 AR-1016-2


R.T.: 4.957 min
Delta R.T.: 0.002 min
Response: 4535959
Conc: 19.06 ng/ml

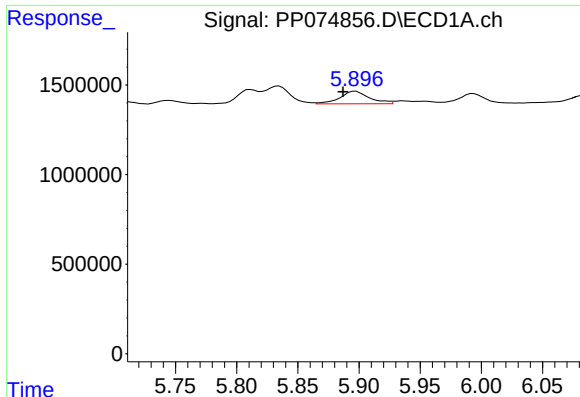

#5 AR-1016-3


R.T.: 5.897 min
Delta R.T.: 0.010 min
Response: 1176484
Conc: 26.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

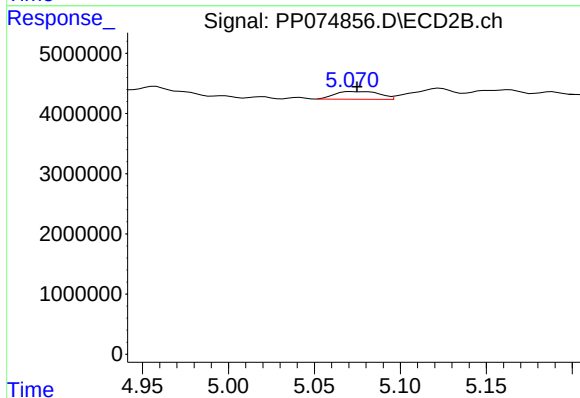


#5 AR-1016-3

R.T.: 5.072 min
Delta R.T.: -0.003 min
Response: 2317691
Conc: 16.81 ng/ml

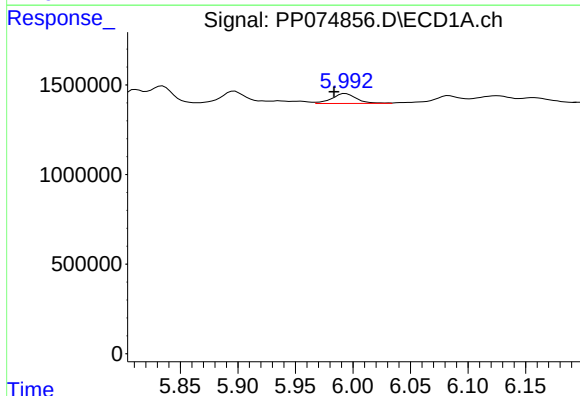


#6 AR-1016-4

R.T.: 5.993 min
Delta R.T.: 0.010 min
Response: 831997
Conc: 23.65 ng/ml

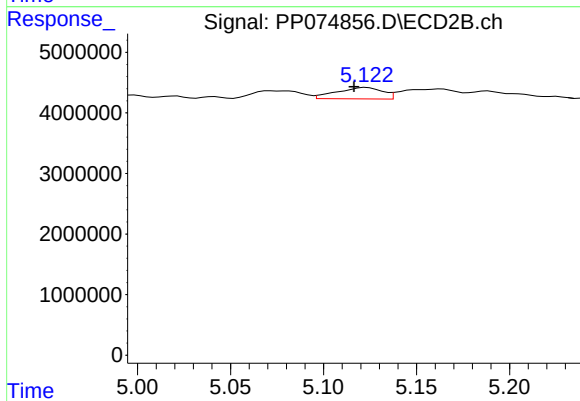

#6 AR-1016-4


R.T.: 5.123 min
Delta R.T.: 0.007 min
Response: 3222783
Conc: 23.05 ng/ml

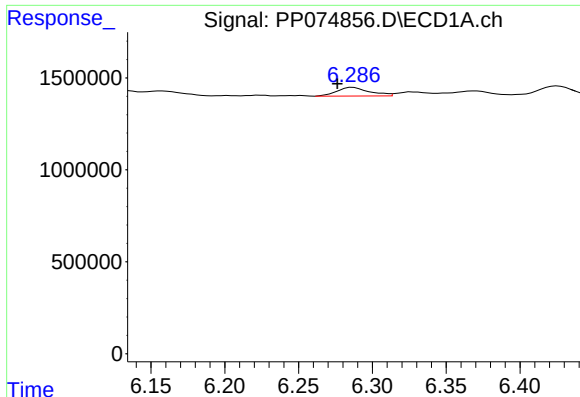

#7 AR-1016-5


R.T.: 6.287 min
Delta R.T.: 0.011 min
Response: 715355
Conc: 21.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

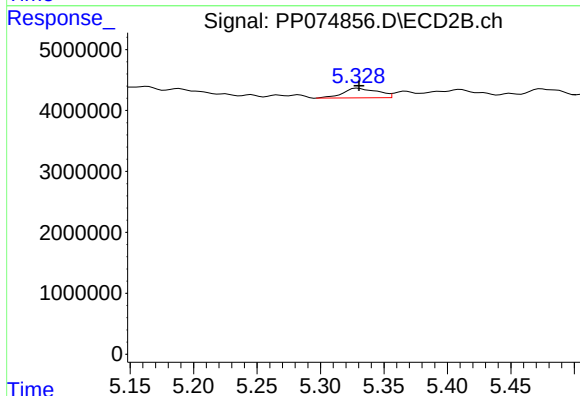


#7 AR-1016-5

R.T.: 5.329 min
Delta R.T.: -0.001 min
Response: 2968845
Conc: 17.88 ng/ml

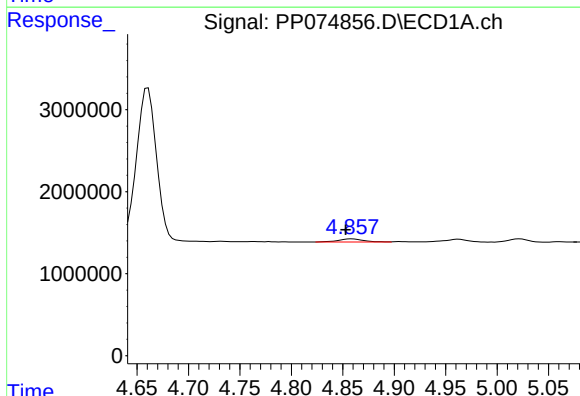


#8 AR-1221-1

R.T.: 4.858 min
Delta R.T.: 0.005 min
Response: 650550
Conc: 36.98 ng/ml

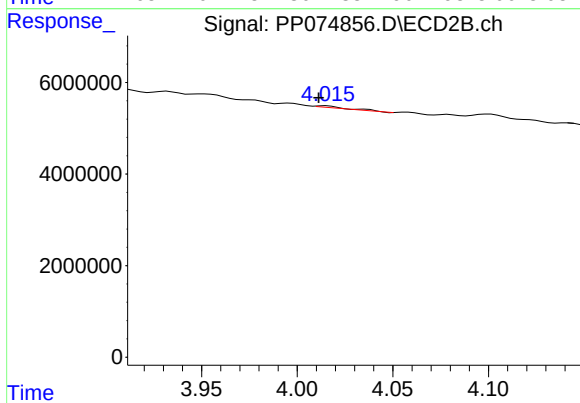

#8 AR-1221-1


R.T.: 4.015 min
Delta R.T.: 0.004 min
Response: 435333
Conc: 7.04 ng/ml

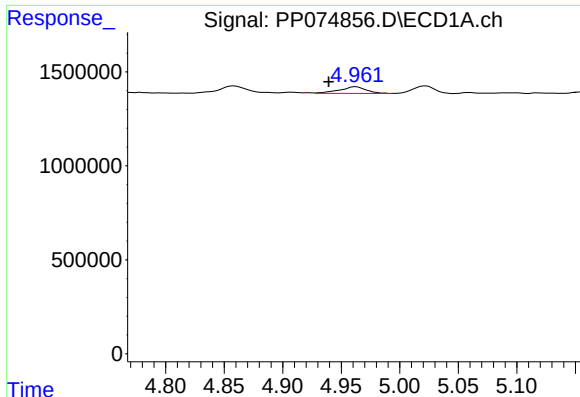

#9 AR-1221-2


R.T.: 4.963 min
Delta R.T.: 0.024 min
Response: 556010
Conc: 41.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

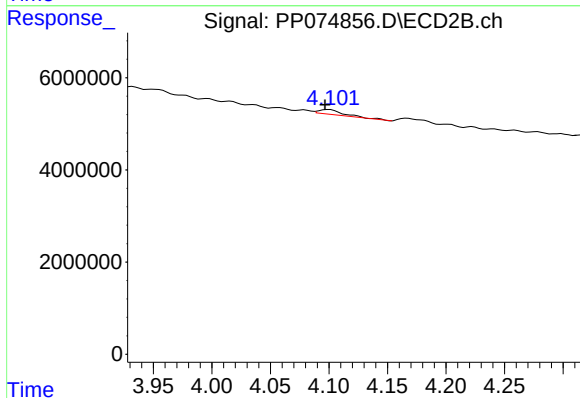


#9 AR-1221-2

R.T.: 4.100 min
Delta R.T.: 0.004 min
Response: 1569057
Conc: 34.70 ng/ml

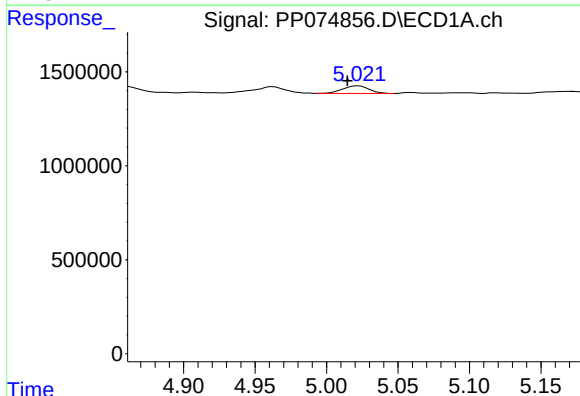


#10 AR-1221-3

R.T.: 5.022 min
Delta R.T.: 0.008 min
Response: 517144
Conc: 13.64 ng/ml

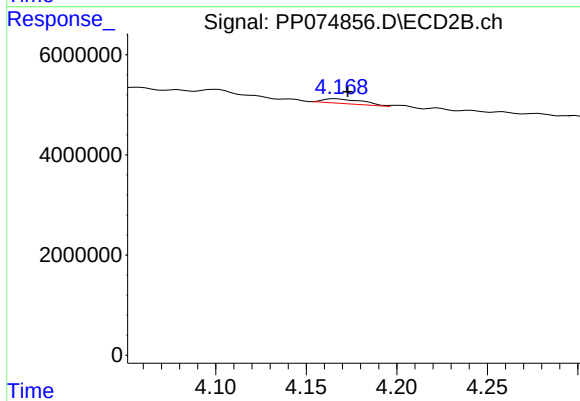

#10 AR-1221-3


R.T.: 4.166 min
Delta R.T.: -0.006 min
Response: 1468443
Conc: 8.94 ng/ml

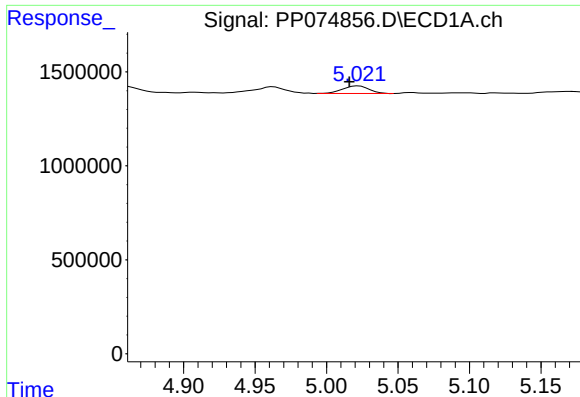

#11 AR-1232-1


R.T.: 5.022 min
Delta R.T.: 0.006 min
Response: 517144
Conc: 17.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

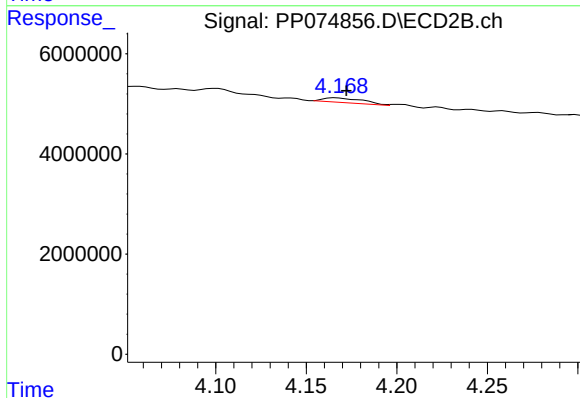


#11 AR-1232-1

R.T.: 4.166 min
Delta R.T.: -0.006 min
Response: 1468443
Conc: 11.46 ng/ml

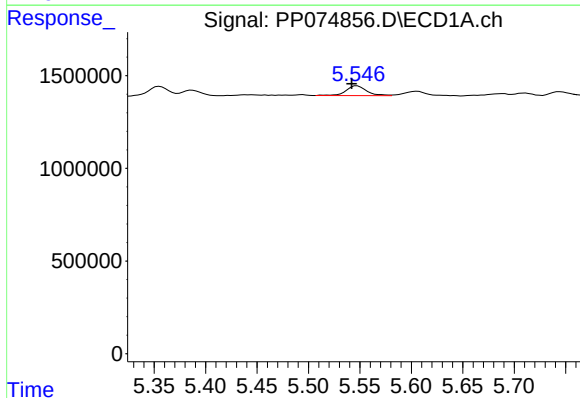


#12 AR-1232-2

R.T.: 5.547 min
Delta R.T.: 0.005 min
Response: 740670
Conc: 47.00 ng/ml

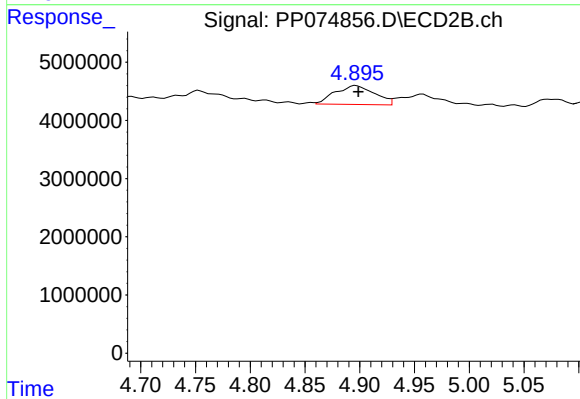

#12 AR-1232-2


R.T.: 4.897 min
Delta R.T.: -0.002 min
Response: 8118735
Conc: 35.03 ng/ml

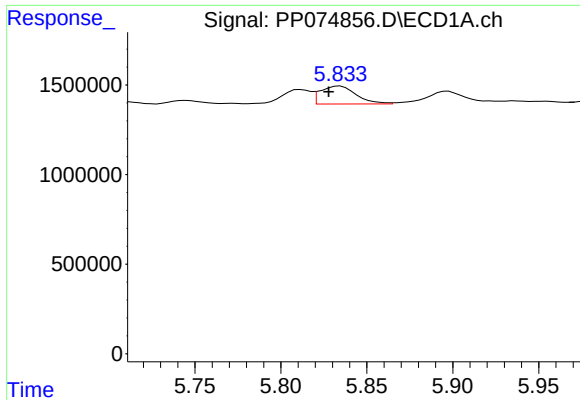

#13 AR-1232-3


R.T.: 5.834 min
Delta R.T.: 0.007 min
Response: 1454045
Conc: 47.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

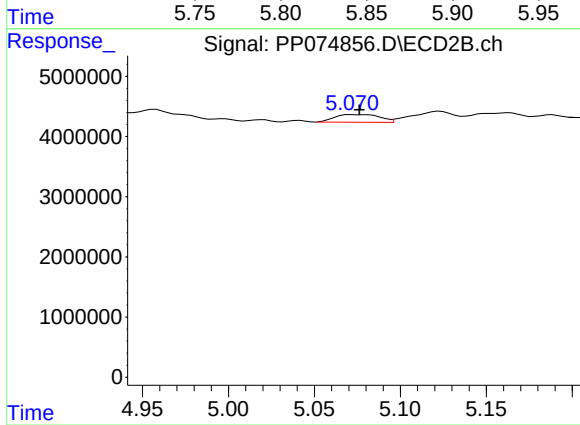


#13 AR-1232-3

R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 2317691
Conc: 38.59 ng/ml

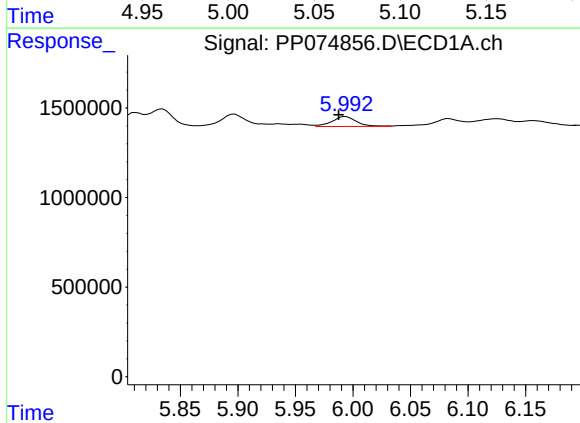


#14 AR-1232-4

R.T.: 5.993 min
Delta R.T.: 0.006 min
Response: 831997
Conc: 48.18 ng/ml

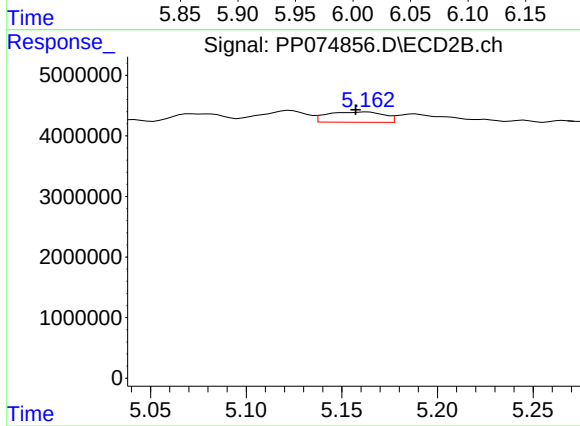

#14 AR-1232-4


R.T.: 5.164 min
Delta R.T.: 0.006 min
Response: 3511272
Conc: 47.64 ng/ml

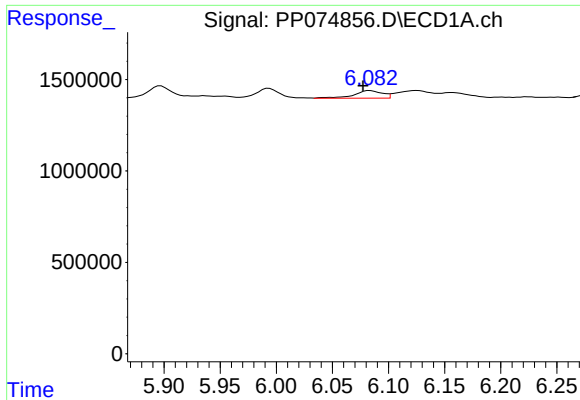

#15 AR-1232-5


R.T.: 6.083 min
Delta R.T.: 0.006 min
Response: 744260
Conc: 57.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

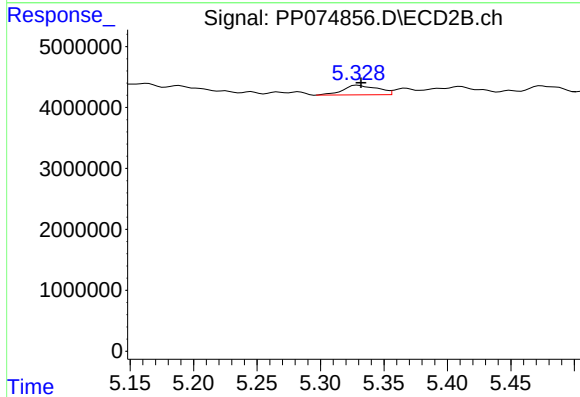


#15 AR-1232-5

R.T.: 5.329 min
Delta R.T.: -0.003 min
Response: 2968845
Conc: 47.82 ng/ml

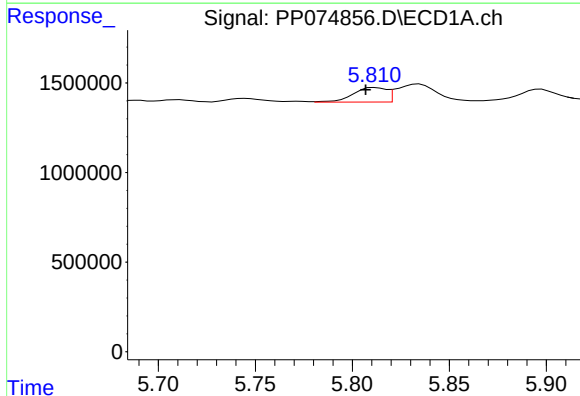


#16 AR-1242-1

R.T.: 5.812 min
Delta R.T.: 0.005 min
Response: 965743
Conc: 25.23 ng/ml

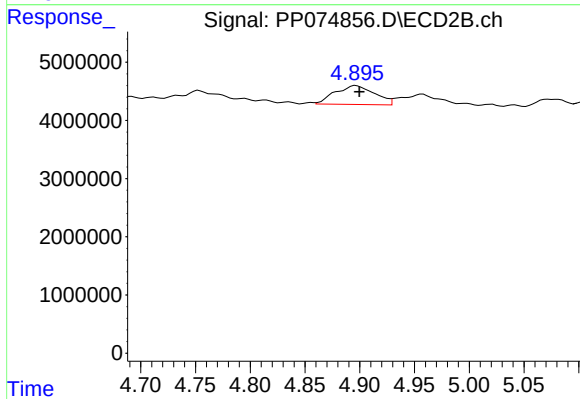

#16 AR-1242-1


R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 8118735
Conc: 19.25 ng/ml

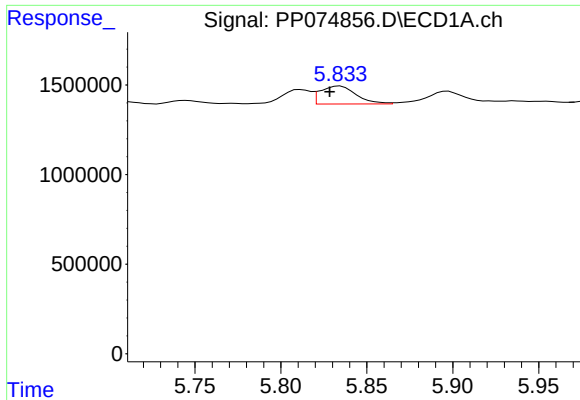

#17 AR-1242-2


R.T.: 5.834 min
Delta R.T.: 0.006 min
Response: 1454045
Conc: 25.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

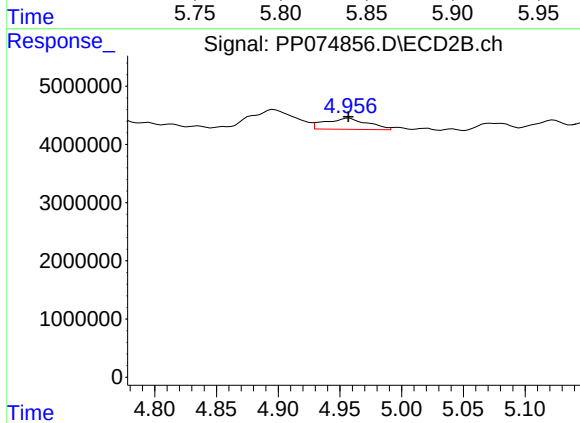


#17 AR-1242-2

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 4535959
Conc: 22.65 ng/ml

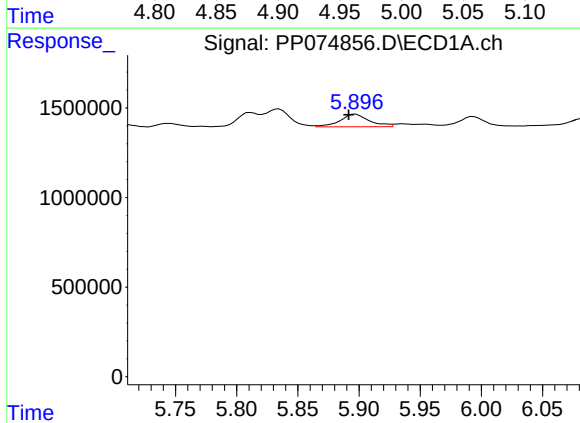


#18 AR-1242-3

R.T.: 5.897 min
Delta R.T.: 0.006 min
Response: 1176484
Conc: 28.98 ng/ml

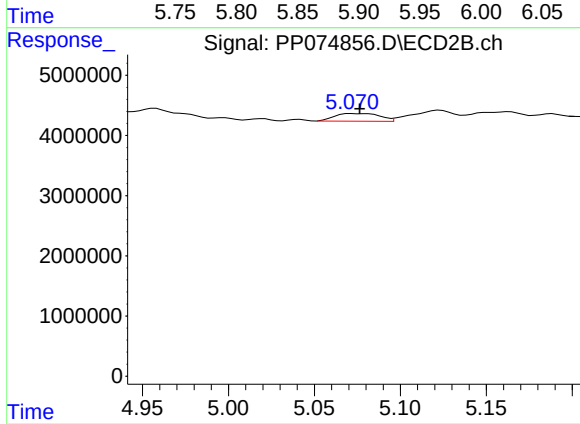

#18 AR-1242-3


R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 2317691
Conc: 19.59 ng/ml

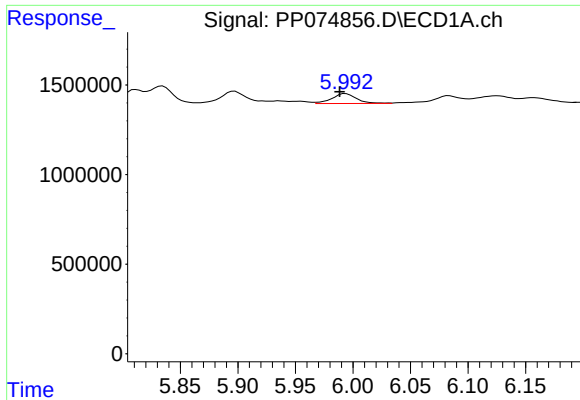

#19 AR-1242-4


R.T.: 5.993 min
Delta R.T.: 0.005 min
Response: 831997
Conc: 26.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

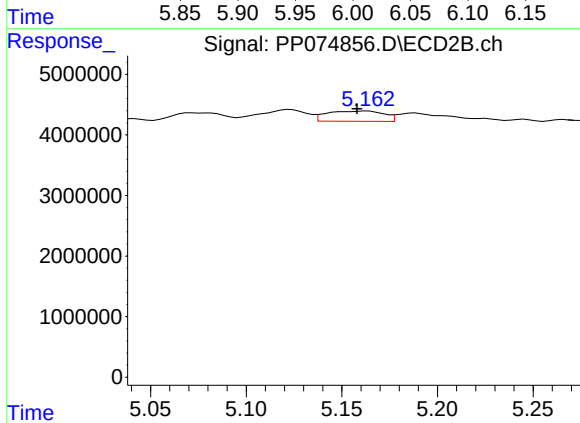


#19 AR-1242-4

R.T.: 5.164 min
Delta R.T.: 0.006 min
Response: 3511272
Conc: 20.51 ng/ml

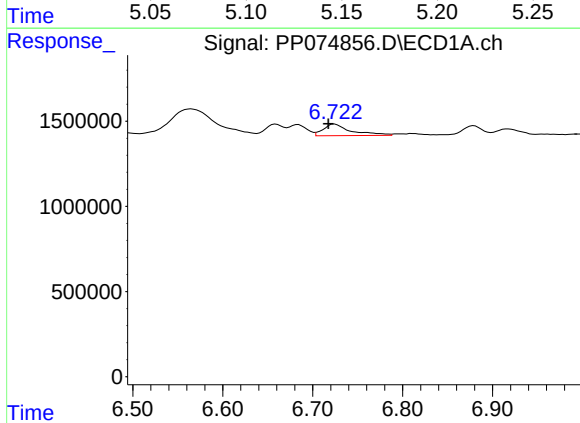


#20 AR-1242-5

R.T.: 6.724 min
Delta R.T.: 0.007 min
Response: 1458131
Conc: 40.42 ng/ml

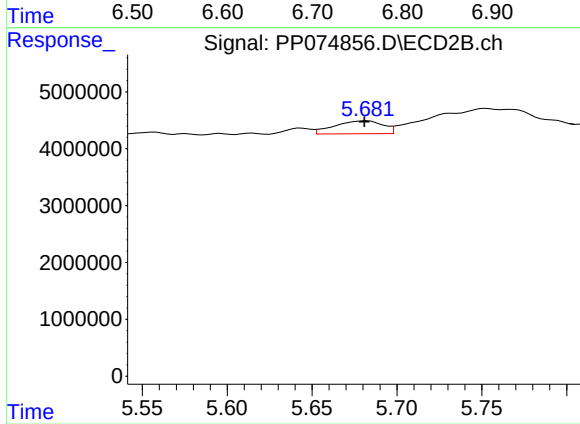

#20 AR-1242-5


R.T.: 5.682 min
Delta R.T.: 0.002 min
Response: 4490170
Conc: 24.25 ng/ml

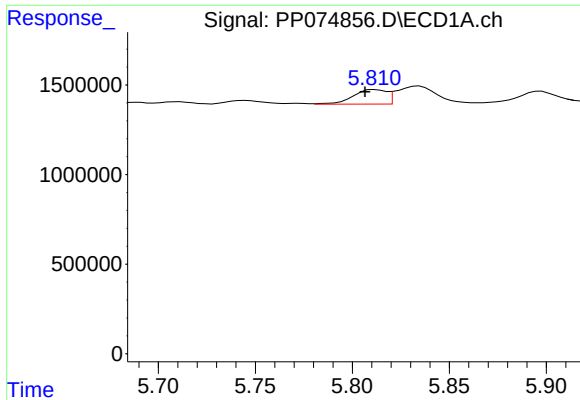

#21 AR-1248-1


R.T.: 5.812 min
Delta R.T.: 0.005 min
Response: 965743
Conc: 31.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

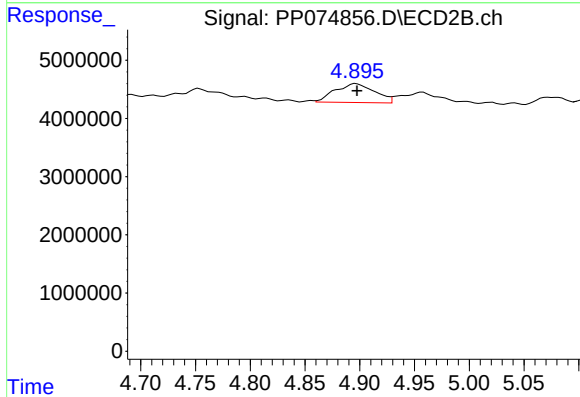


#21 AR-1248-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 8118735
Conc: 29.40 ng/ml

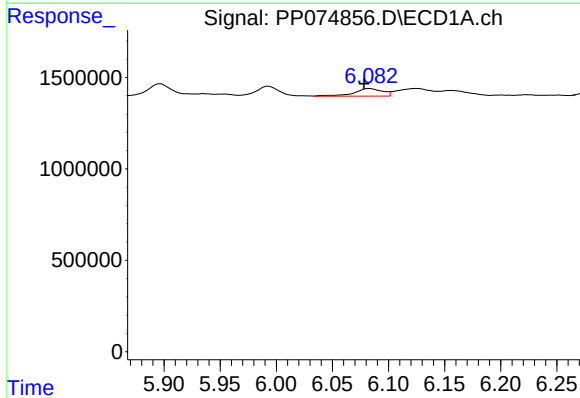


#22 AR-1248-2

R.T.: 6.083 min
Delta R.T.: 0.005 min
Response: 744260
Conc: 17.27 ng/ml

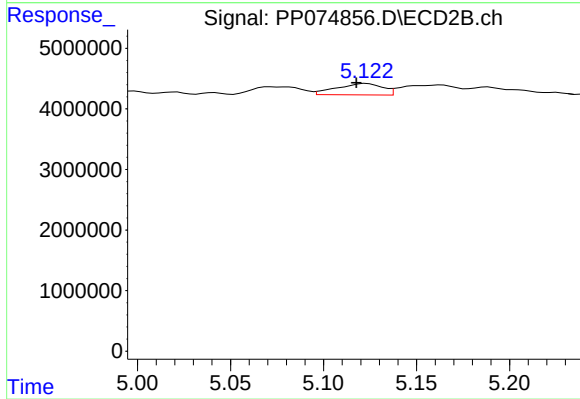

#22 AR-1248-2


R.T.: 5.123 min
Delta R.T.: 0.006 min
Response: 3222783
Conc: 18.23 ng/ml

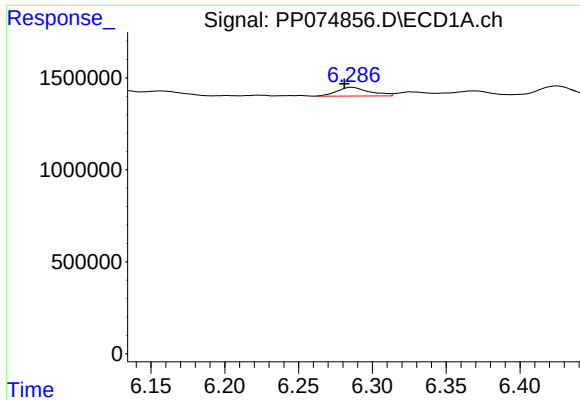

#23 AR-1248-3


R.T.: 6.287 min
Delta R.T.: 0.006 min
Response: 715355
Conc: 15.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

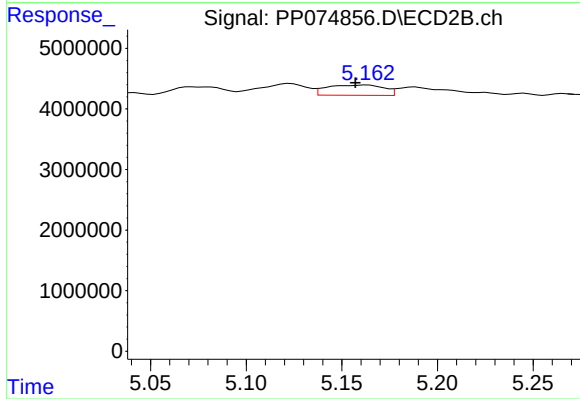


#23 AR-1248-3

R.T.: 5.164 min
Delta R.T.: 0.006 min
Response: 3511272
Conc: 15.45 ng/ml

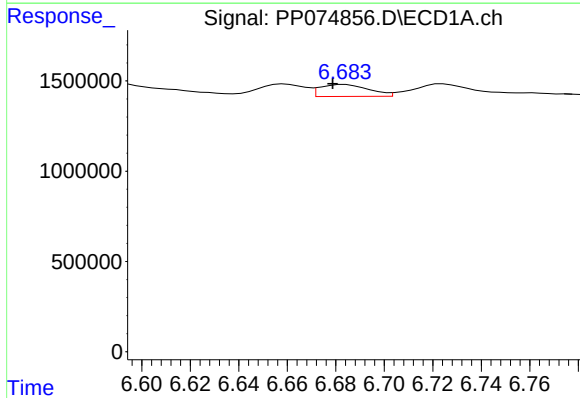


#24 AR-1248-4

R.T.: 6.684 min
Delta R.T.: 0.005 min
Response: 926188
Conc: 16.84 ng/ml

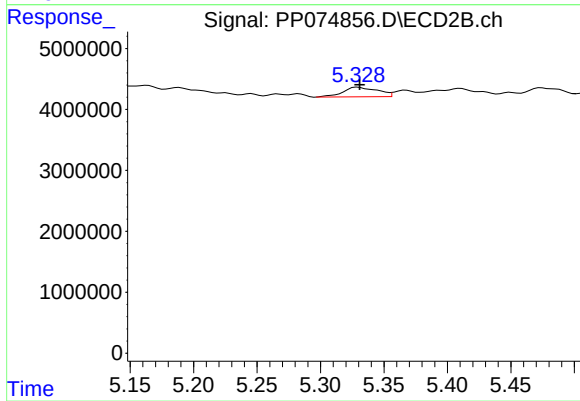

#24 AR-1248-4


R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 2968845
Conc: 13.62 ng/ml

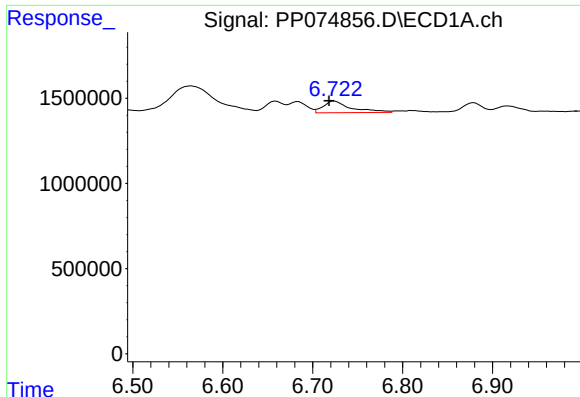

#25 AR-1248-5


R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 1458131
Conc: 26.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

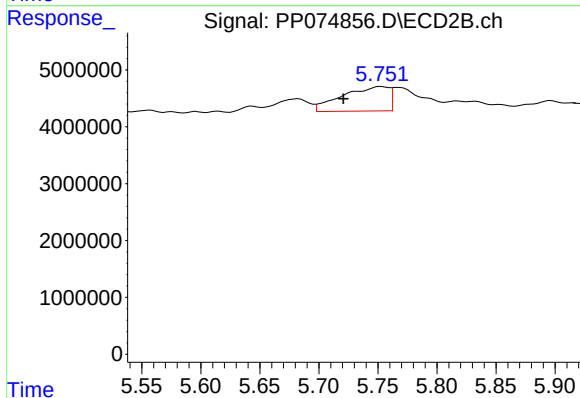


#25 AR-1248-5

R.T.: 5.753 min
Delta R.T.: 0.032 min
Response: 11802011
Conc: 32.13 ng/ml

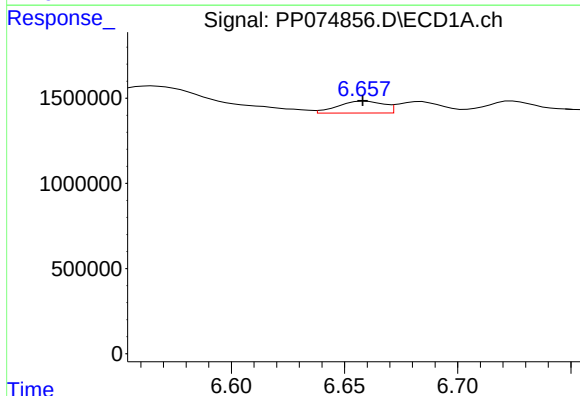


#26 AR-1254-1

R.T.: 6.659 min
Delta R.T.: 0.000 min
Response: 978440
Conc: 16.79 ng/ml

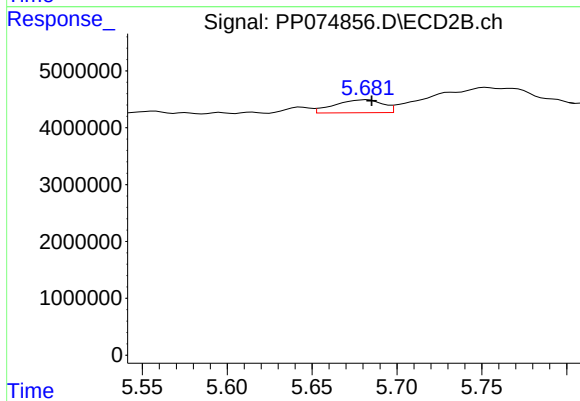

#26 AR-1254-1


R.T.: 5.682 min
Delta R.T.: -0.003 min
Response: 4490170
Conc: 9.42 ng/ml

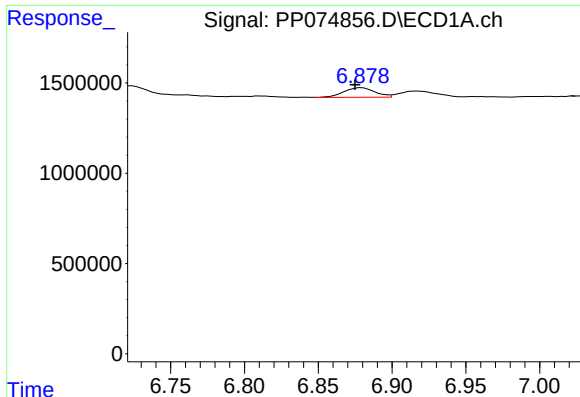

#27 AR-1254-2


R.T.: 6.880 min
Delta R.T.: 0.005 min
Response: 772031
Conc: 9.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

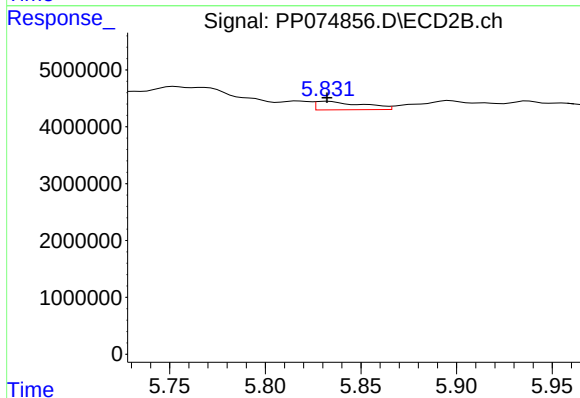


#27 AR-1254-2

R.T.: 5.833 min
Delta R.T.: 0.000 min
Response: 2536476
Conc: 7.20 ng/ml

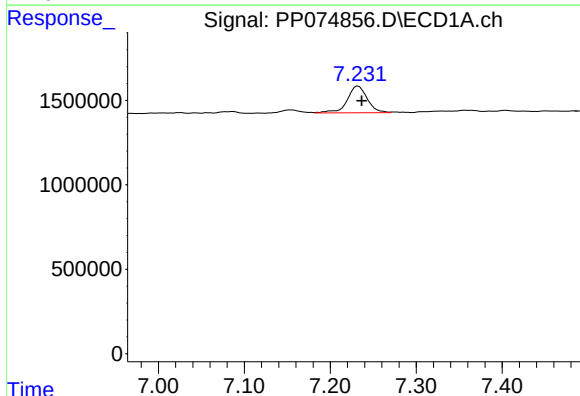


#28 AR-1254-3

R.T.: 7.233 min
Delta R.T.: -0.004 min
Response: 2571665
Conc: 28.83 ng/ml

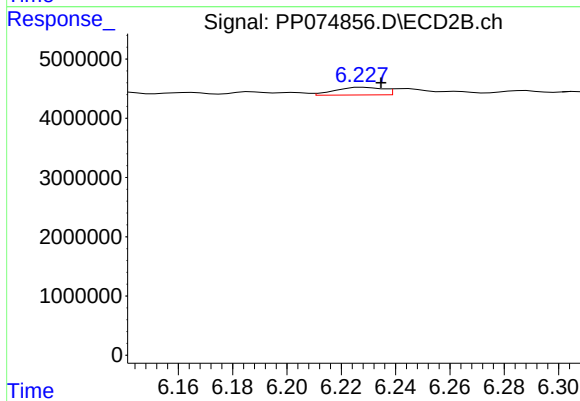

#28 AR-1254-3


R.T.: 6.228 min
Delta R.T.: -0.006 min
Response: 1590052
Conc: 2.57 ng/ml

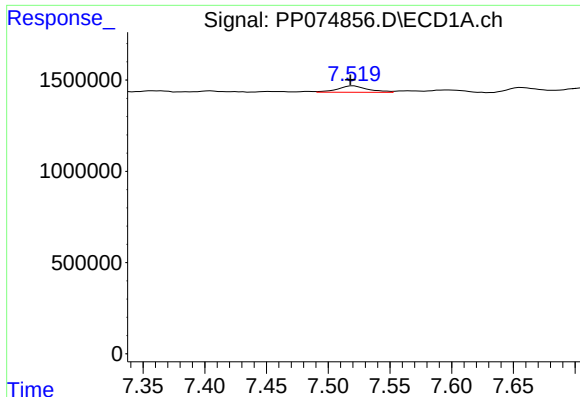

#29 AR-1254-4


R.T.: 7.520 min
Delta R.T.: 0.002 min
Response: 595357
Conc: 9.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

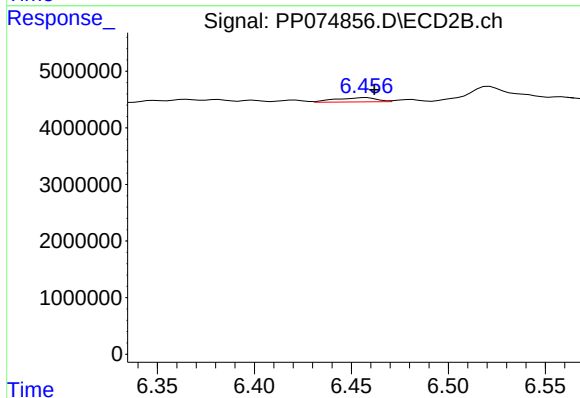


#29 AR-1254-4

R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 1085081
Conc: 2.32 ng/ml

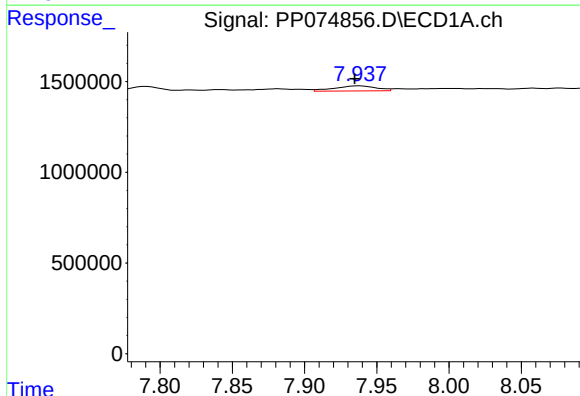


#30 AR-1254-5

R.T.: 7.938 min
Delta R.T.: 0.003 min
Response: 560002
Conc: 6.74 ng/ml

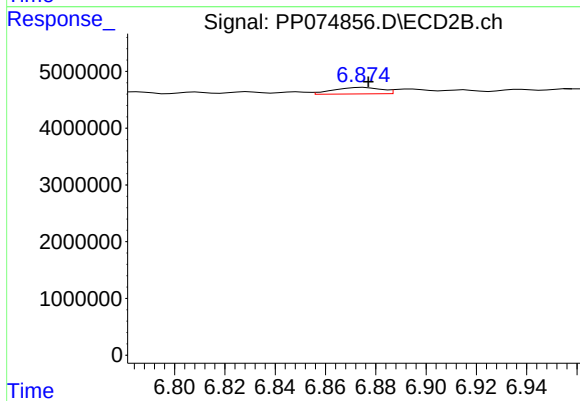

#30 AR-1254-5


R.T.: 6.875 min
Delta R.T.: -0.002 min
Response: 1516786
Conc: 3.09 ng/ml

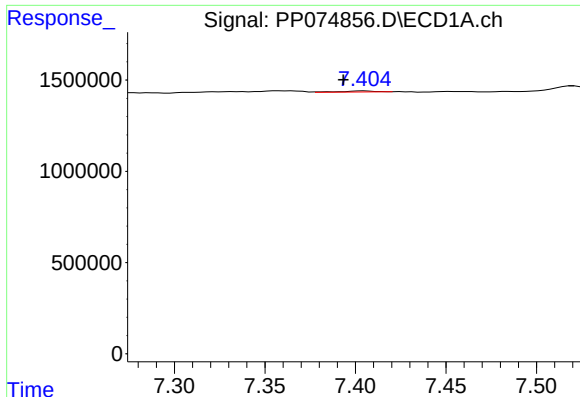

#31 AR-1260-1


R.T.: 7.405 min
Delta R.T.: 0.012 min
Response: 74690
Conc: 1.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

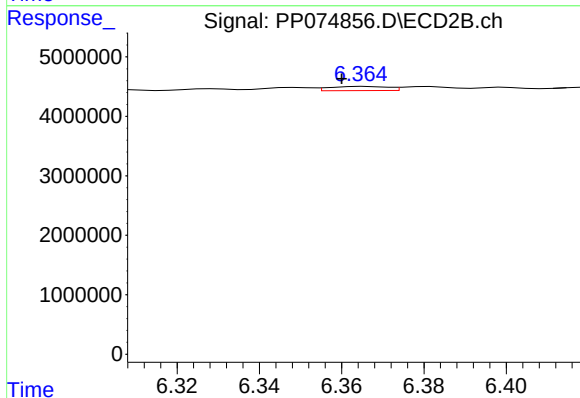


#31 AR-1260-1

R.T.: 6.365 min
Delta R.T.: 0.005 min
Response: 679454
Conc: 1.81 ng/ml

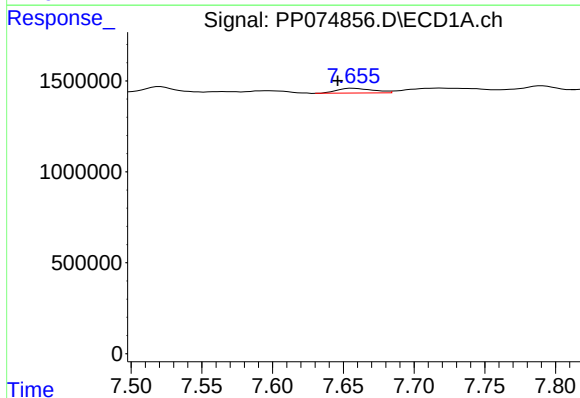


#32 AR-1260-2

R.T.: 7.657 min
Delta R.T.: 0.011 min
Response: 465351
Conc: 6.75 ng/ml

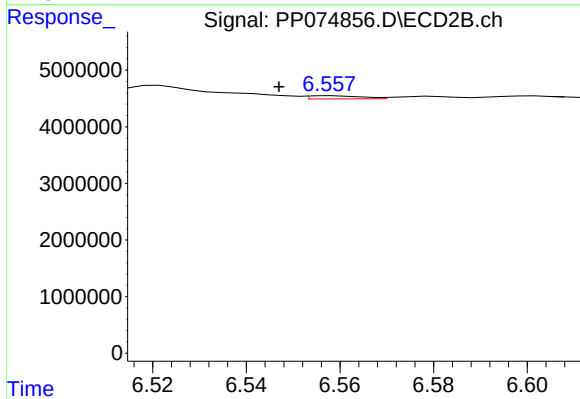

#32 AR-1260-2


R.T.: 6.558 min
Delta R.T.: 0.011 min
Response: 441035
Conc: 0.83 ng/ml

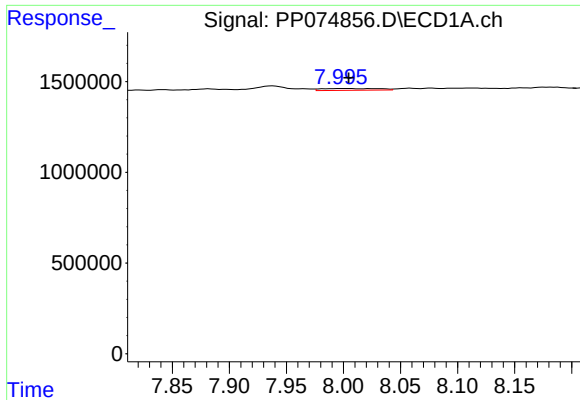

#33 AR-1260-3


R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 335772
Conc: 6.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

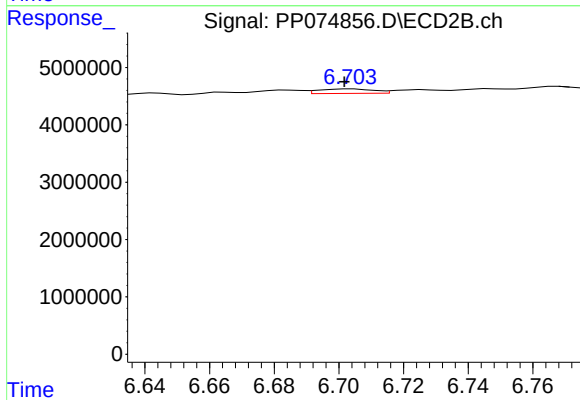


#33 AR-1260-3

R.T.: 6.704 min
Delta R.T.: 0.002 min
Response: 908087
Conc: 2.10 ng/ml

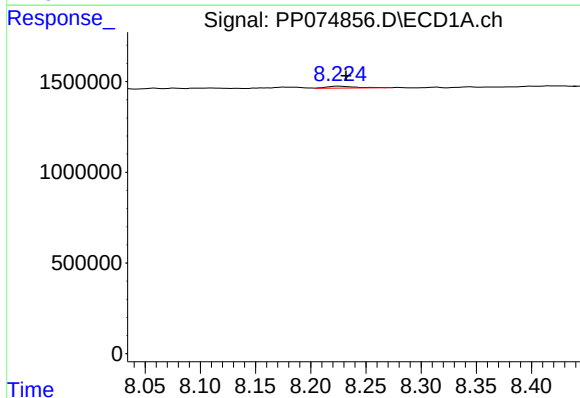


#34 AR-1260-4

R.T.: 8.226 min
Delta R.T.: -0.006 min
Response: 175274
Conc: 2.75 ng/ml

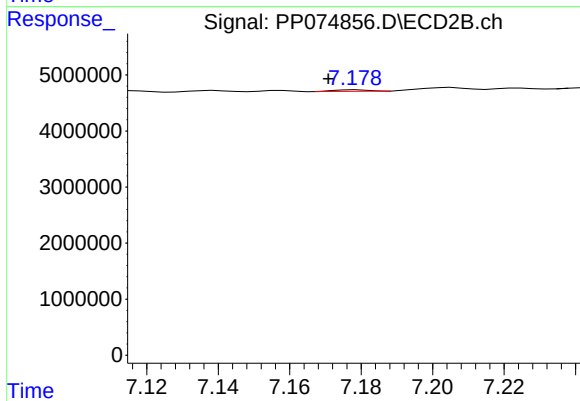

#34 AR-1260-4


R.T.: 7.179 min
Delta R.T.: 0.008 min
Response: 190338
Conc: 0.50 ng/ml

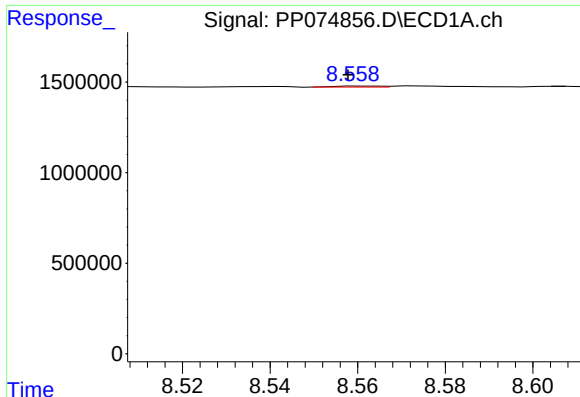

#35 AR-1260-5


R.T.: 8.560 min
Delta R.T.: 0.002 min
Response: 39158
Conc: 0.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

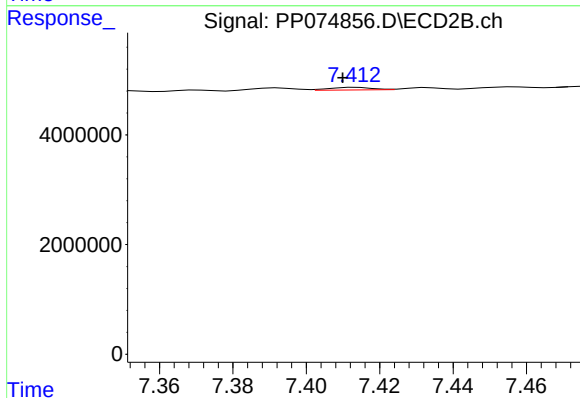


#35 AR-1260-5

R.T.: 7.414 min
Delta R.T.: 0.004 min
Response: 384750
Conc: 0.38 ng/ml

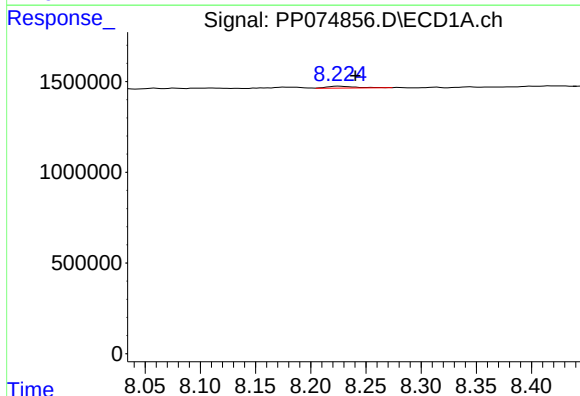


#36 AR-1262-1

R.T.: 8.226 min
Delta R.T.: -0.015 min
Response: 175274
Conc: 2.28 ng/ml

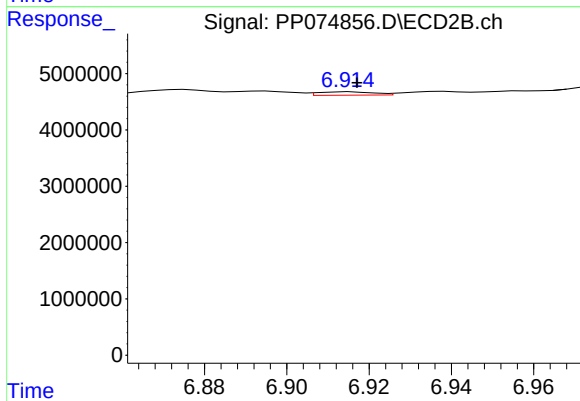

#36 AR-1262-1


R.T.: 6.915 min
Delta R.T.: -0.002 min
Response: 559772
Conc: 0.79 ng/ml

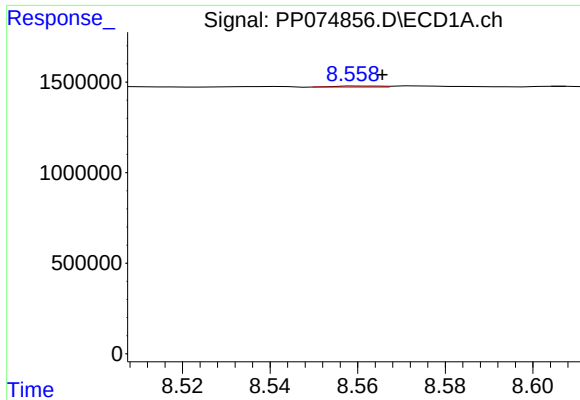

#37 AR-1262-2


R.T.: 8.560 min
Delta R.T.: -0.006 min
Response: 39158
Conc: 0.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

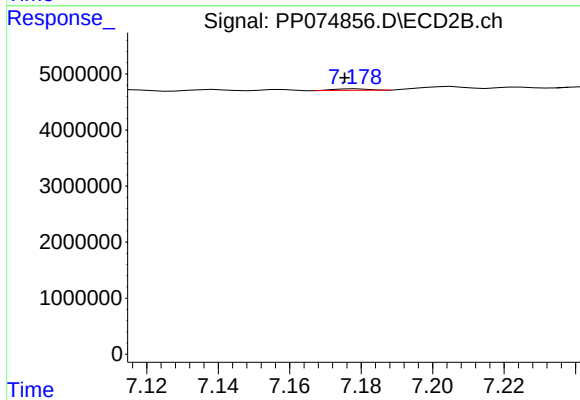


#37 AR-1262-2

R.T.: 7.179 min
Delta R.T.: 0.003 min
Response: 190338
Conc: 0.37 ng/ml

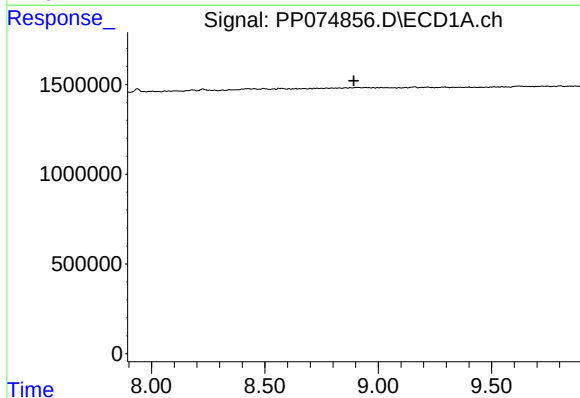


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

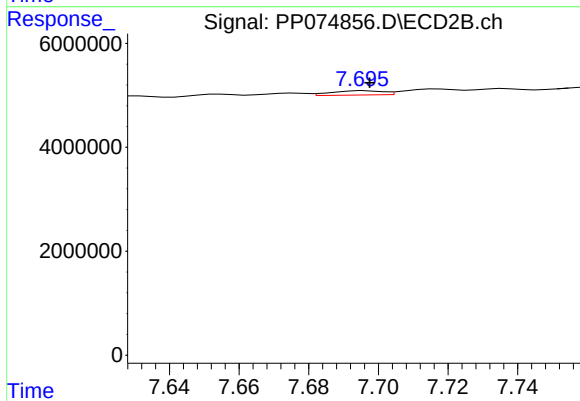

#38 AR-1262-3


R.T.: 7.696 min
Delta R.T.: -0.002 min
Response: 842383
Conc: 1.81 ng/ml

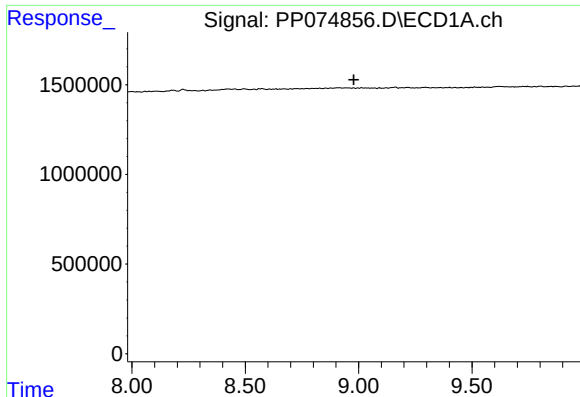

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

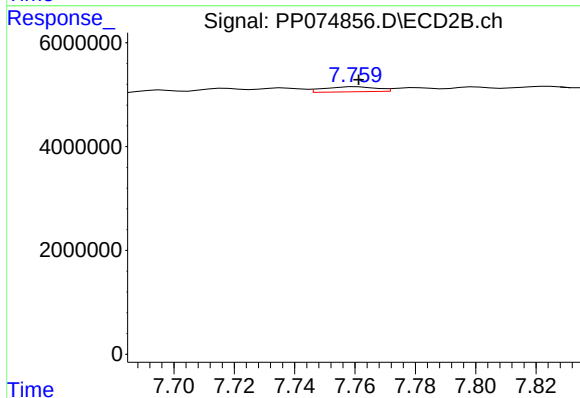


#39 AR-1262-4

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 1174769
Conc: 1.43 ng/ml

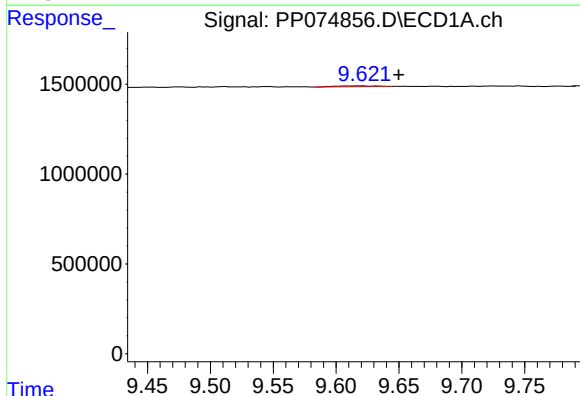


#40 AR-1262-5

R.T.: 9.622 min
Delta R.T.: -0.028 min
Response: 99847
Conc: 1.64 ng/ml

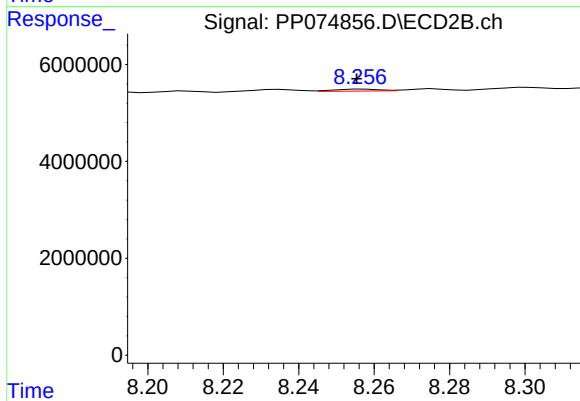

#40 AR-1262-5


R.T.: 8.257 min
Delta R.T.: 0.002 min
Response: 326352
Conc: 0.91 ng/ml

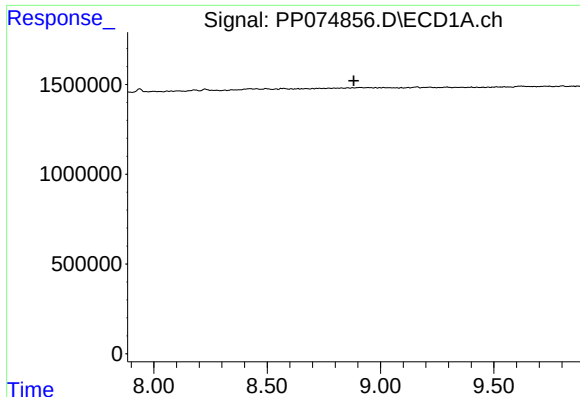

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

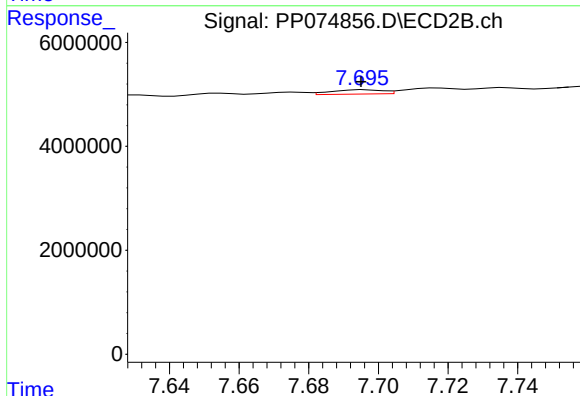


#41 AR-1268-1

R.T.: 7.696 min
Delta R.T.: 0.000 min
Response: 842383
Conc: 0.60 ng/ml

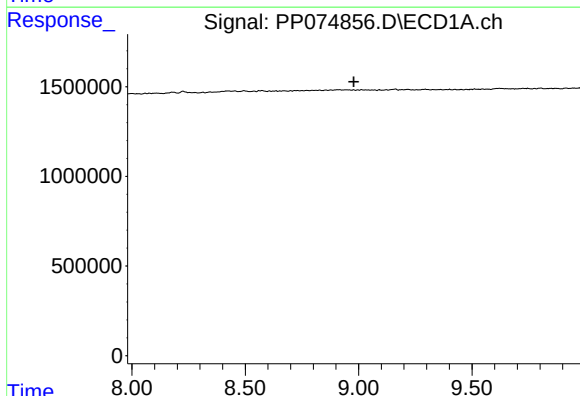


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

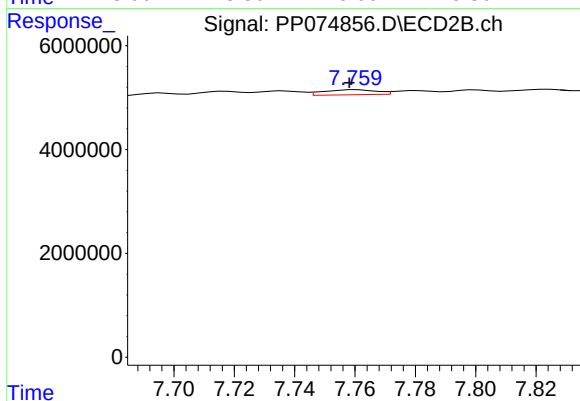

#42 AR-1268-2


R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 1174769
Conc: 0.86 ng/ml

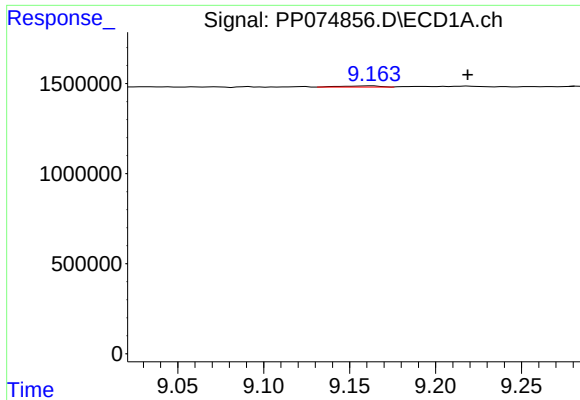

#43 AR-1268-3


R.T.: 9.164 min
Delta R.T.: -0.055 min
Response: 94372
Conc: 0.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

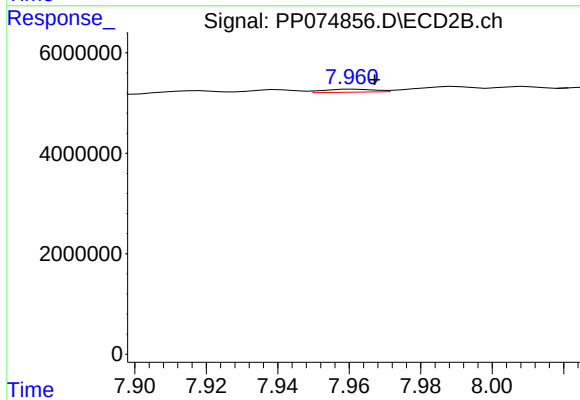


#43 AR-1268-3

R.T.: 7.961 min
Delta R.T.: -0.006 min
Response: 574519
Conc: 0.55 ng/ml

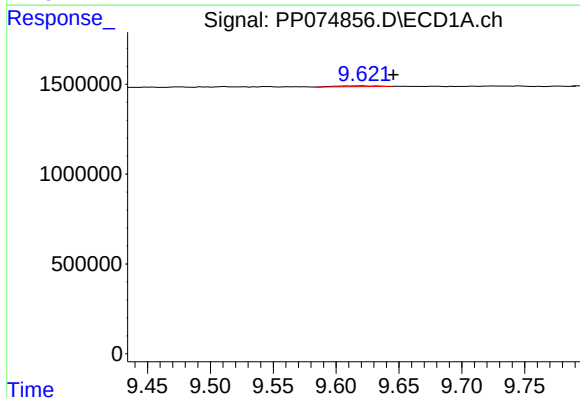


#44 AR-1268-4

R.T.: 9.622 min
Delta R.T.: -0.024 min
Response: 99847
Conc: 1.48 ng/ml

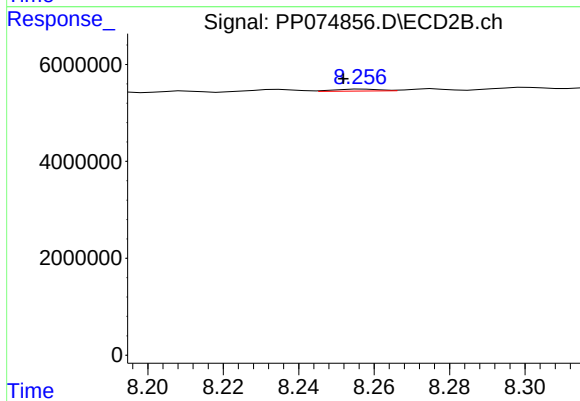

#44 AR-1268-4


R.T.: 8.257 min
Delta R.T.: 0.005 min
Response: 326352
Conc: 0.85 ng/ml

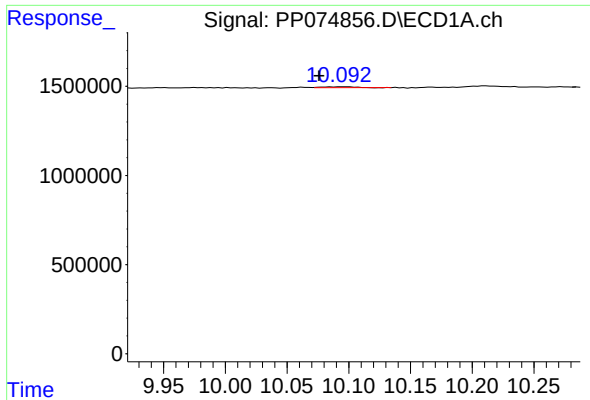

#45 AR-1268-5

R.T.: 10.094 min
Delta R.T.: 0.018 min
Response: 86274
Conc: 0.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

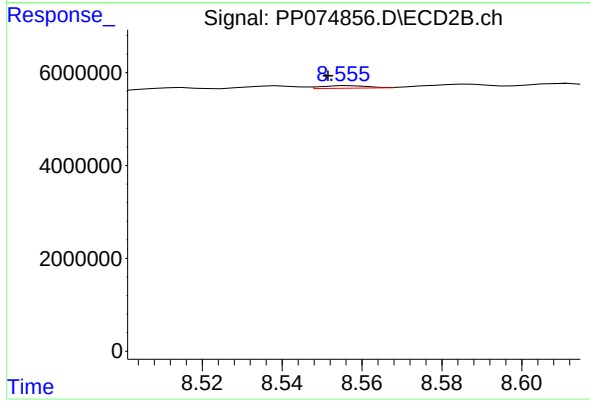

#45 AR-1268-5

R.T.: 8.557 min
Delta R.T.: 0.005 min
Response: 432525
Conc: 0.14 ng/ml