

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074875.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 19:59
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1660 WATER LOD 40PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:07:55 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.660	3.797	27098474	100.6E6	22.145	20.805
2)	SA Decachlor...	10.439	8.808	20921120	133.7E6	21.186	17.831
Target Compounds							
3)	L1 AR-1016-1	5.811	4.895	2258980	19489904	51.237	38.264 #
4)	L1 AR-1016-2	5.833	4.955	3215246	8767763	51.164	36.837 #
5)	L1 AR-1016-3	5.896	5.075	2255642	4766960	50.221	34.567 #
6)	L1 AR-1016-4	5.993	5.115	1733235	4906557	49.265	35.096 #
7)	L1 AR-1016-5	6.285	5.330	1576307	6295851	47.499	37.908
8)	L2 AR-1221-1	4.858	4.004	904569	652375	51.417	10.545 #
9)	L2 AR-1221-2	4.960	4.087	743408	1692001	55.656	37.424 #
10)	L2 AR-1221-3	5.021	4.167	1159338	3587013	30.579	21.833 #
11)	L3 AR-1232-1	5.021	4.167	1159338	3587013	38.169	28.003 #
12)	L3 AR-1232-2	5.547	4.895	1586578	19489904	100.683	84.083
13)	L3 AR-1232-3	5.833	5.075	3215246	4766960	105.267	79.370
14)	L3 AR-1232-4	5.993	5.157	1733235	10352253	100.365	140.451 #
15)	L3 AR-1232-5	6.082	5.330	1462636	6295851	112.676	101.409
16)	L4 AR-1242-1	5.811	4.895	2258980	19489904	59.019	46.212
17)	L4 AR-1242-2	5.833	4.955	3215246	8767763	56.925	43.777
18)	L4 AR-1242-3	5.896	5.075	2255642	4766960	55.554	40.296 #
19)	L4 AR-1242-4	5.993	5.157	1733235	10352253	54.604	60.483
20)	L4 AR-1242-5	6.724	5.679	1016776	7060906	28.188	38.133 #
21)	L5 AR-1248-1	5.811	4.895	2258980	19489904	74.741	70.579
22)	L5 AR-1248-2	6.082	5.115	1462636	4906557	33.939	27.759
23)	L5 AR-1248-3	6.285	5.157	1576307	10352253	33.751	45.564 #
24)	L5 AR-1248-4	6.659	5.330	2828441	6295851	51.425	28.877 #
25)	L5 AR-1248-5	6.724	5.754	1016776	19471345	18.330	53.009 #
26)	L6 AR-1254-1	6.659	5.679	2828441	7060906	48.541	14.812 #
27)	L6 AR-1254-2	6.875	5.827	1445362	8080450	17.709	22.947 #
28)	L6 AR-1254-3	7.233	6.241	2129630	11319502	23.873	18.263
29)	L6 AR-1254-4	7.519	6.454	227760	1125848	3.455	2.402 #
30)	L6 AR-1254-5	7.934	6.871	4729609	14859883	56.925	30.295 #
31)	L7 AR-1260-1	7.403	6.358	2586499	13436869	44.742	35.810
32)	L7 AR-1260-2	7.656	6.544	3324414	21131475	48.238	39.960
33)	L7 AR-1260-3	8.013	6.699	2823167	16059205	54.412	37.088 #
34)	L7 AR-1260-4	8.241	7.168	3938108	13071533	61.733	34.266 #
35)	L7 AR-1260-5	8.567	7.406	5468537	28973873	48.218	28.845 #
36)	L8 AR-1262-1	8.241	6.908	3938108	18970966	51.134	26.823 #
37)	L8 AR-1262-2	8.567	7.168	5468537	13071533	41.309	25.103 #
38)	L8 AR-1262-3	8.898	7.692	3582579	9230242	36.853	19.795 #
39)	L8 AR-1262-4	8.967	7.752	2189478	22495730	29.065	27.372
40)	L8 AR-1262-5	9.651	8.249	1700128	7438845	27.891	20.761 #
41)	L9 AR-1268-1	8.898	7.692	3582579	9230242	22.109	6.544 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 19:59
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1660 WATER LOD 40PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:07:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.967	7.752	2189478	22495730	14.921	16.499
43)	L9 AR-1268-3	9.222	7.954	550172	974787	4.452	0.934 #
44)	L9 AR-1268-4	9.651	8.249	1700128	7438845	25.276	19.418
45)	L9 AR-1268-5	10.083	8.545	523979	2740598	1.416	0.874 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074875.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 19:59
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1660 WATER LOD 40PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:07:55 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

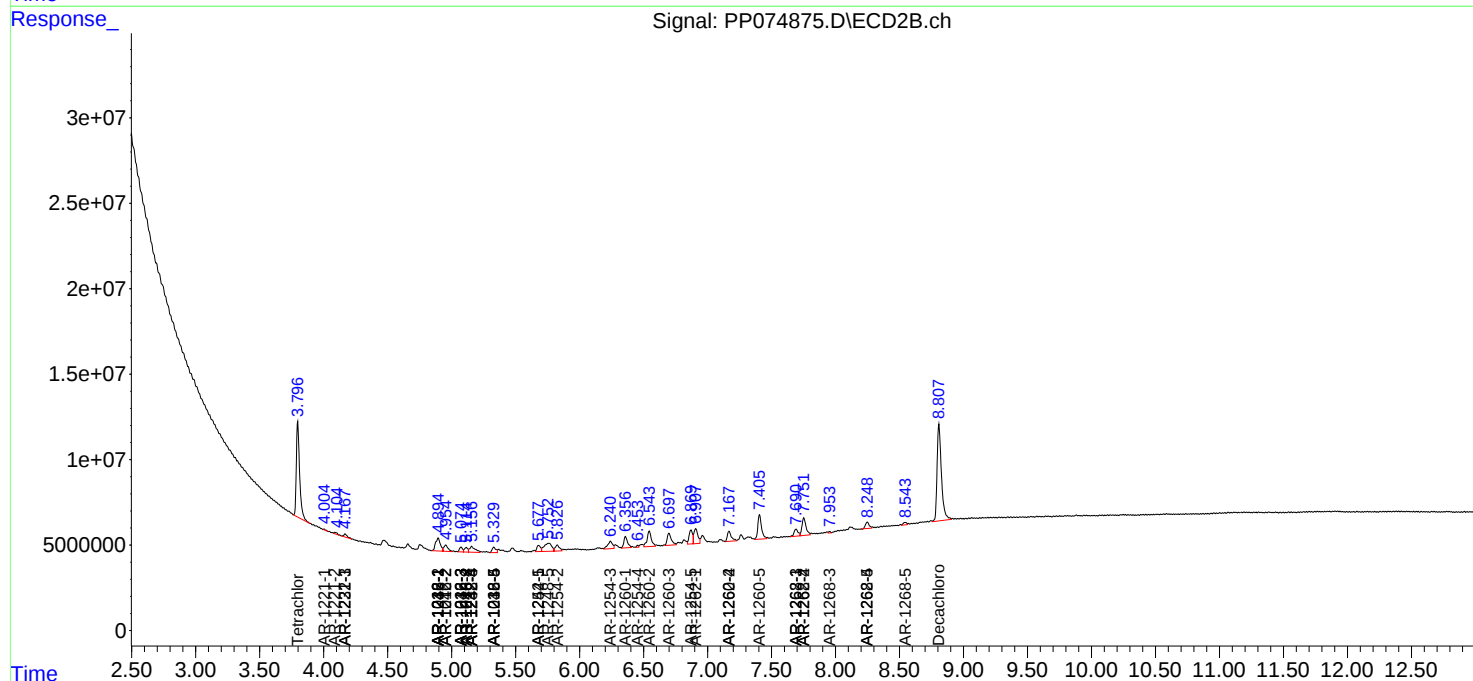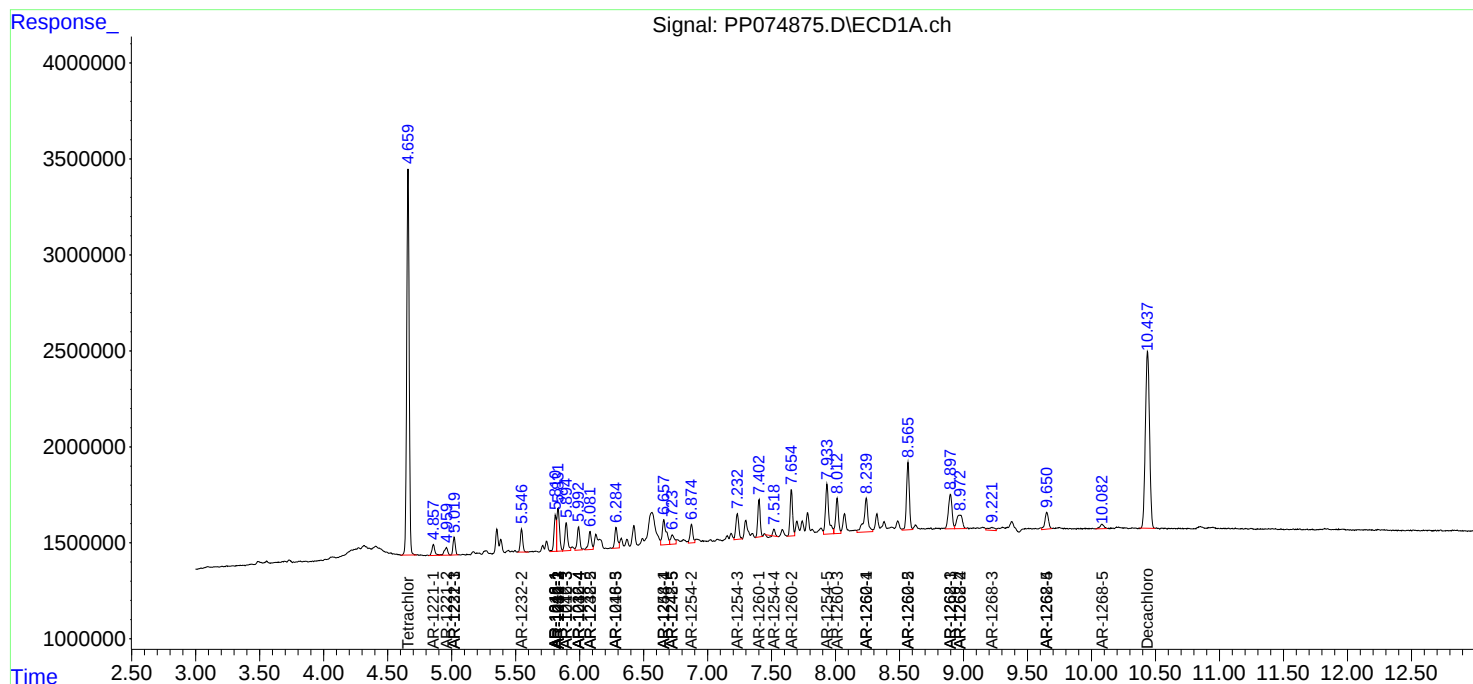


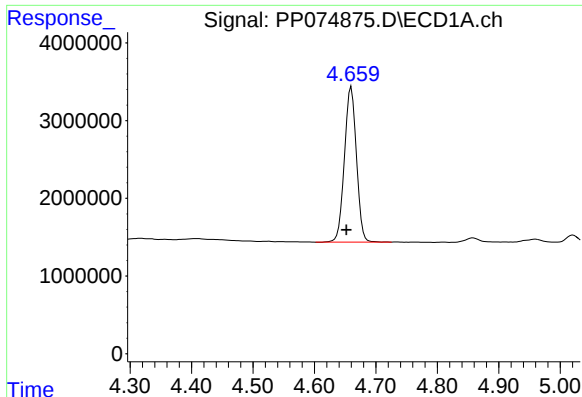

#1 Tetrachloro-m-xylene


R.T.: 4.660 min
Delta R.T.: 0.008 min
Response: 27098474
Conc: 22.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

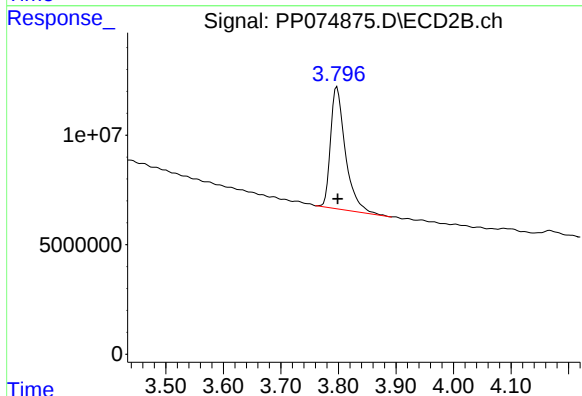


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: -0.001 min
Response: 100598961
Conc: 20.80 ng/ml

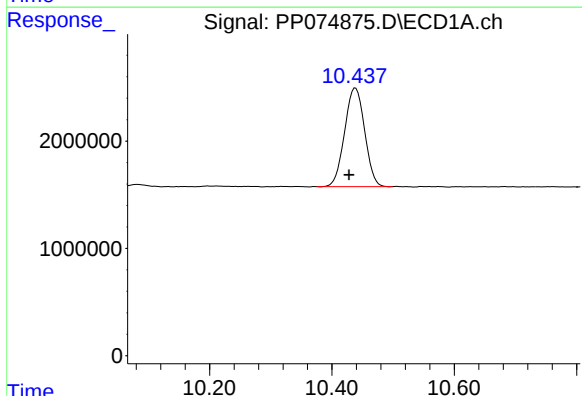


#2 Decachlorobiphenyl

R.T.: 10.439 min
Delta R.T.: 0.010 min
Response: 20921120
Conc: 21.19 ng/ml

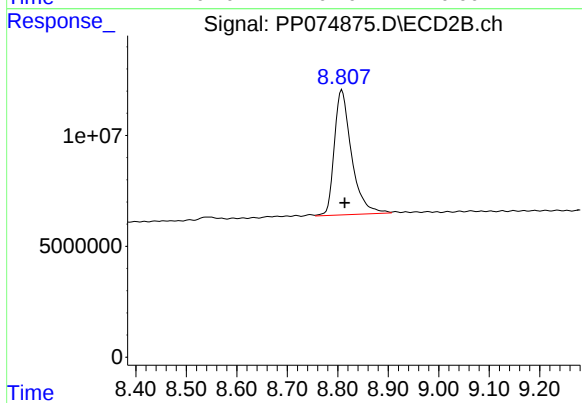

#2 Decachlorobiphenyl


R.T.: 8.808 min
Delta R.T.: -0.006 min
Response: 133715676
Conc: 17.83 ng/ml

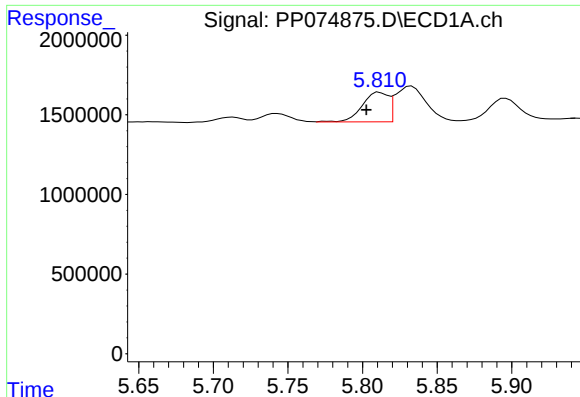

#3 AR-1016-1


R.T.: 5.811 min
Delta R.T.: 0.008 min
Response: 2258980
Conc: 51.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

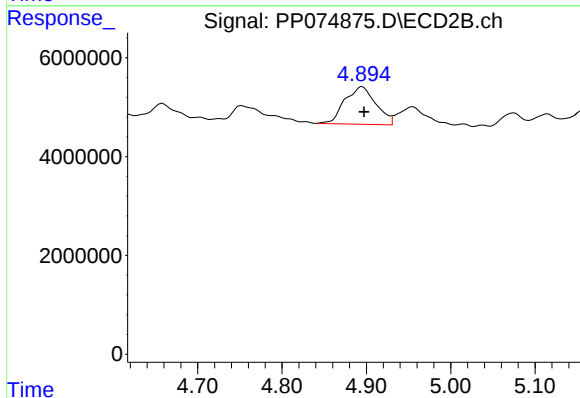


#3 AR-1016-1

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 19489904
Conc: 38.26 ng/ml

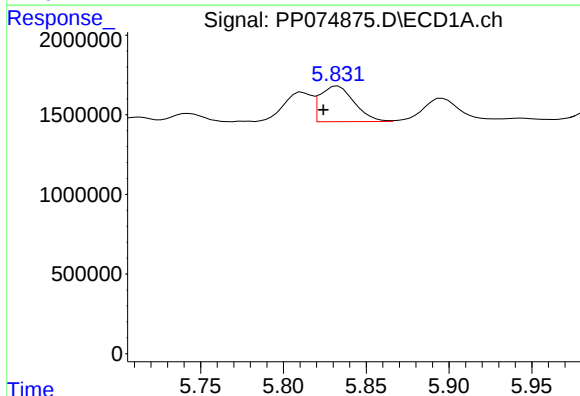


#4 AR-1016-2

R.T.: 5.833 min
Delta R.T.: 0.009 min
Response: 3215246
Conc: 51.16 ng/ml

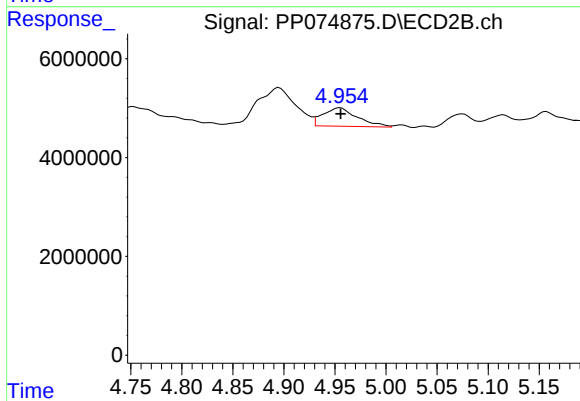

#4 AR-1016-2


R.T.: 4.955 min
Delta R.T.: 0.000 min
Response: 8767763
Conc: 36.84 ng/ml

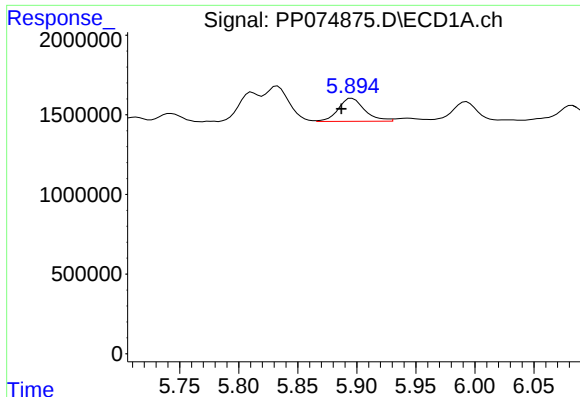

#5 AR-1016-3


R.T.: 5.896 min
Delta R.T.: 0.009 min
Response: 2255642
Conc: 50.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

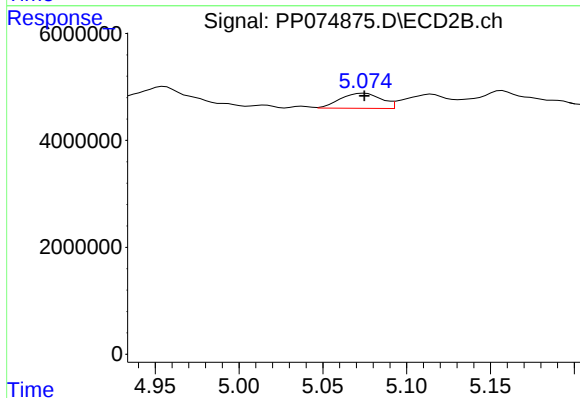


#5 AR-1016-3

R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 4766960
Conc: 34.57 ng/ml

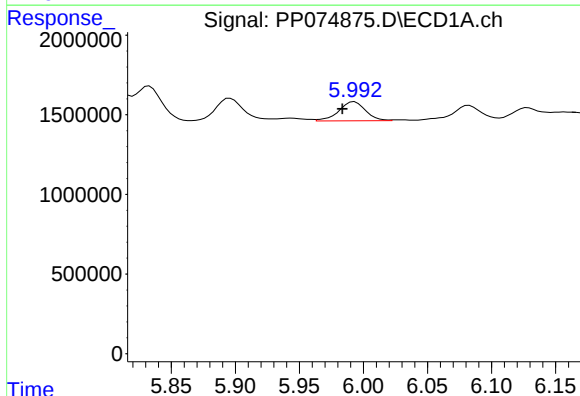


#6 AR-1016-4

R.T.: 5.993 min
Delta R.T.: 0.009 min
Response: 1733235
Conc: 49.27 ng/ml

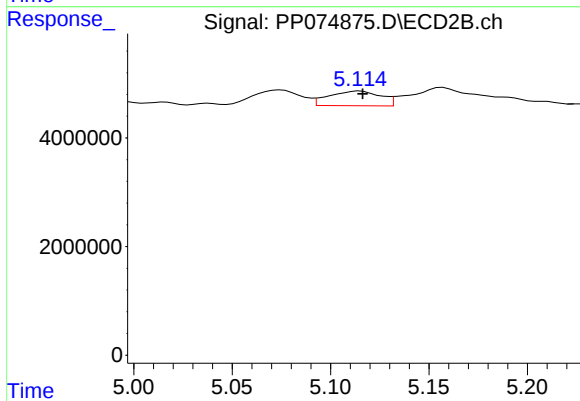

#6 AR-1016-4


R.T.: 5.115 min
Delta R.T.: -0.001 min
Response: 4906557
Conc: 35.10 ng/ml

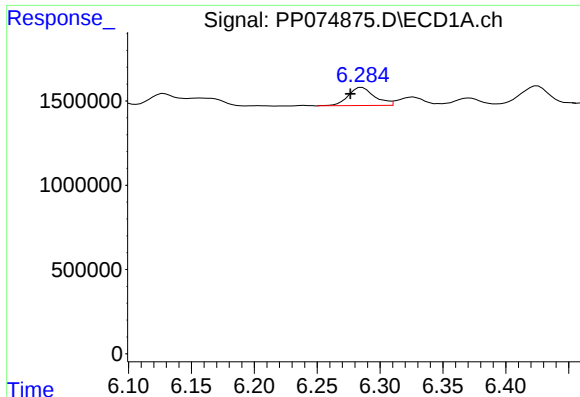

#7 AR-1016-5


R.T.: 6.285 min
Delta R.T.: 0.009 min
Response: 1576307
Conc: 47.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

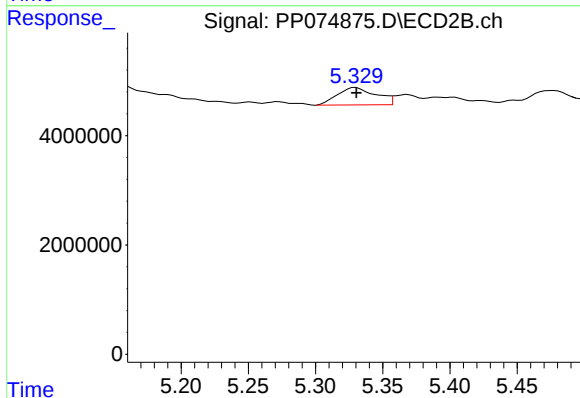


#7 AR-1016-5

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 6295851
Conc: 37.91 ng/ml

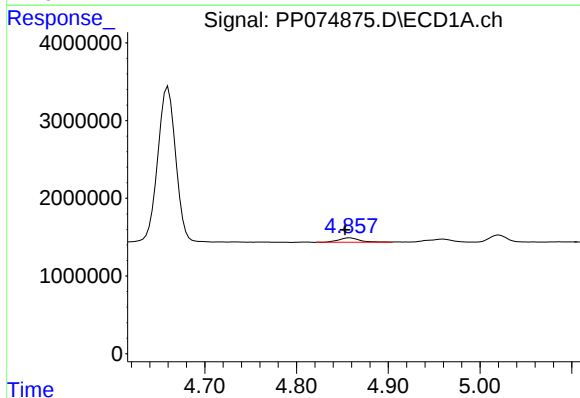


#8 AR-1221-1

R.T.: 4.858 min
Delta R.T.: 0.005 min
Response: 904569
Conc: 51.42 ng/ml

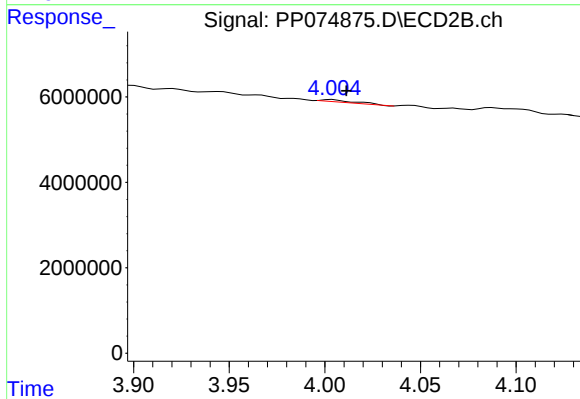

#8 AR-1221-1


R.T.: 4.004 min
Delta R.T.: -0.007 min
Response: 652375
Conc: 10.54 ng/ml

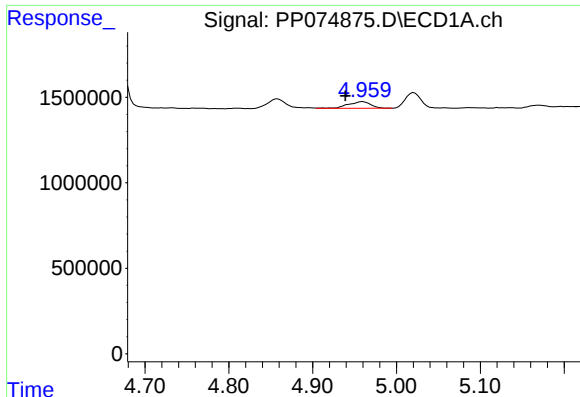

#9 AR-1221-2


R.T.: 4.960 min
Delta R.T.: 0.021 min
Response: 743408
Conc: 55.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

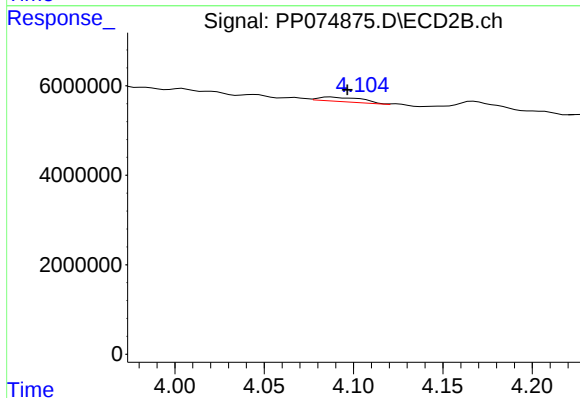


#9 AR-1221-2

R.T.: 4.087 min
Delta R.T.: -0.009 min
Response: 1692001
Conc: 37.42 ng/ml

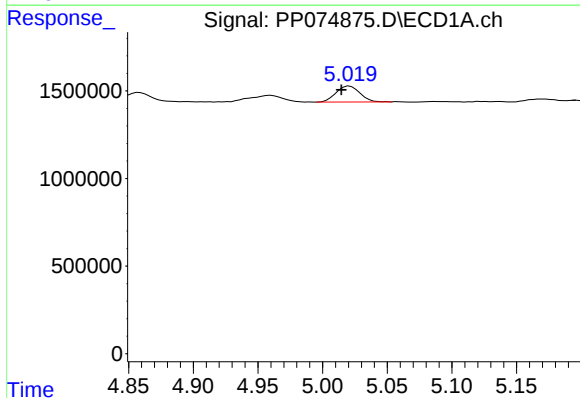


#10 AR-1221-3

R.T.: 5.021 min
Delta R.T.: 0.006 min
Response: 1159338
Conc: 30.58 ng/ml

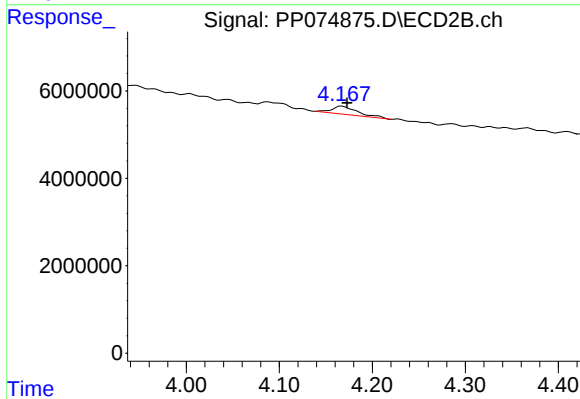

#10 AR-1221-3


R.T.: 4.167 min
Delta R.T.: -0.006 min
Response: 3587013
Conc: 21.83 ng/ml

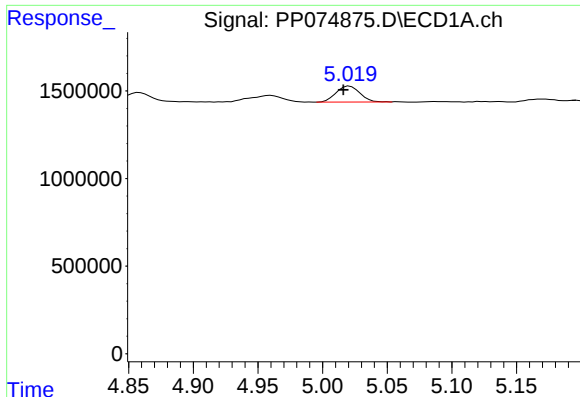

#11 AR-1232-1


R.T.: 5.021 min
Delta R.T.: 0.005 min
Response: 1159338
Conc: 38.17 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

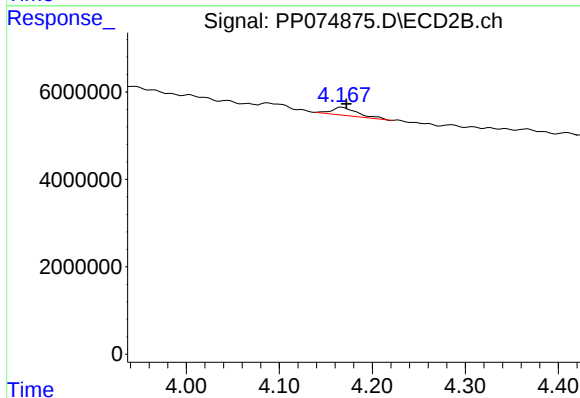


#11 AR-1232-1

R.T.: 4.167 min
Delta R.T.: -0.005 min
Response: 3587013
Conc: 28.00 ng/ml

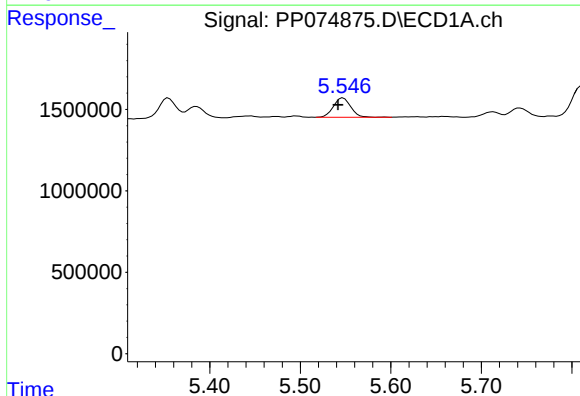


#12 AR-1232-2

R.T.: 5.547 min
Delta R.T.: 0.005 min
Response: 1586578
Conc: 100.68 ng/ml

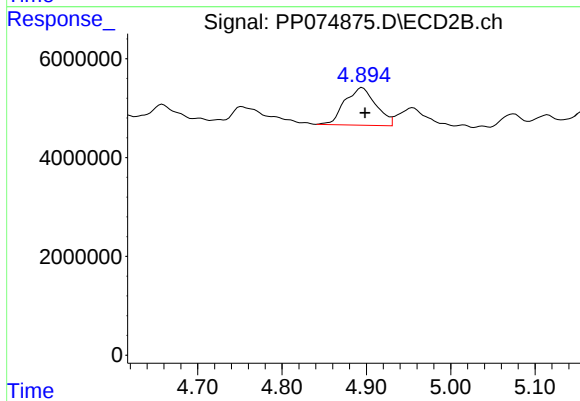

#12 AR-1232-2


R.T.: 4.895 min
Delta R.T.: -0.003 min
Response: 19489904
Conc: 84.08 ng/ml

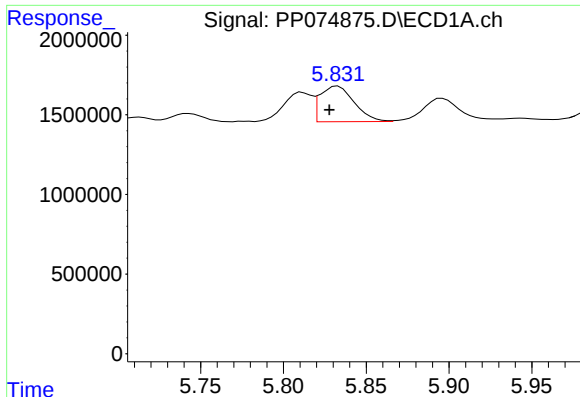

#13 AR-1232-3


R.T.: 5.833 min
Delta R.T.: 0.005 min
Response: 3215246
Conc: 105.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

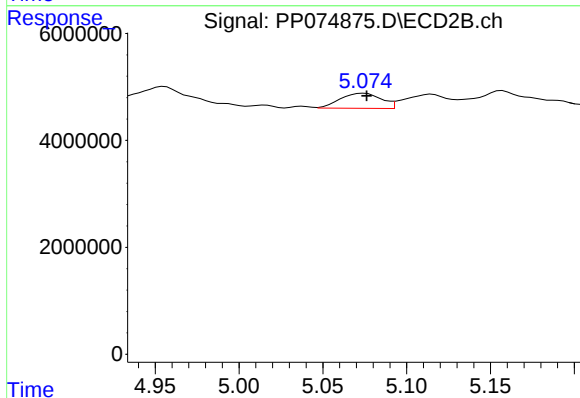


#13 AR-1232-3

R.T.: 5.075 min
Delta R.T.: -0.001 min
Response: 4766960
Conc: 79.37 ng/ml

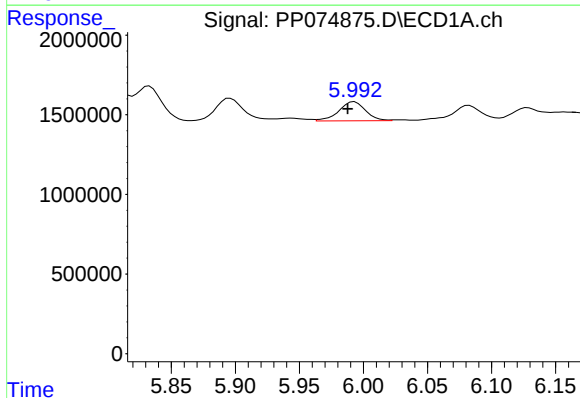


#14 AR-1232-4

R.T.: 5.993 min
Delta R.T.: 0.005 min
Response: 1733235
Conc: 100.37 ng/ml

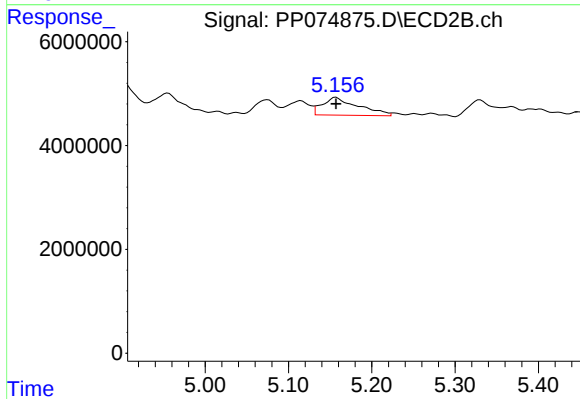

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 10352253
Conc: 140.45 ng/ml

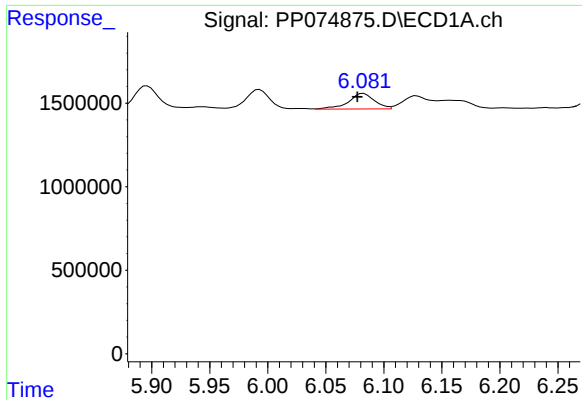

#15 AR-1232-5


R.T.: 6.082 min
Delta R.T.: 0.005 min
Response: 1462636
Conc: 112.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

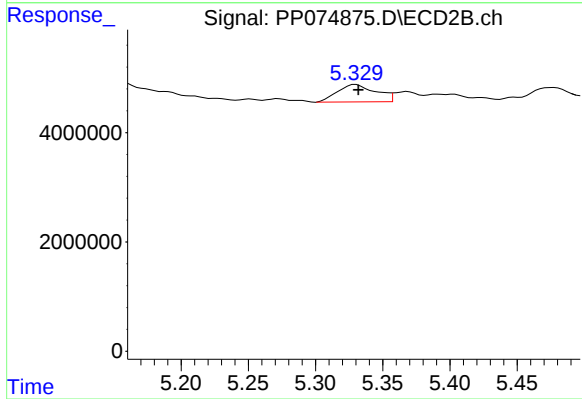


#15 AR-1232-5

R.T.: 5.330 min
Delta R.T.: -0.002 min
Response: 6295851
Conc: 101.41 ng/ml

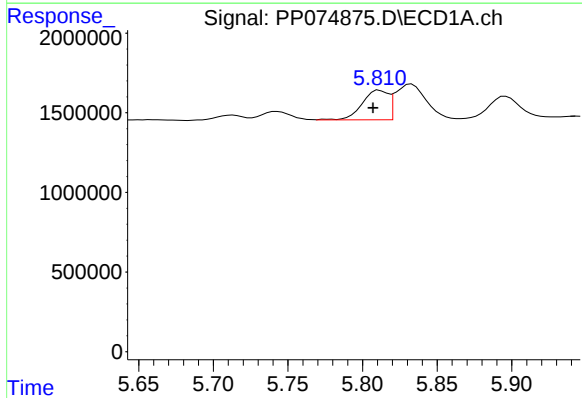


#16 AR-1242-1

R.T.: 5.811 min
Delta R.T.: 0.004 min
Response: 2258980
Conc: 59.02 ng/ml

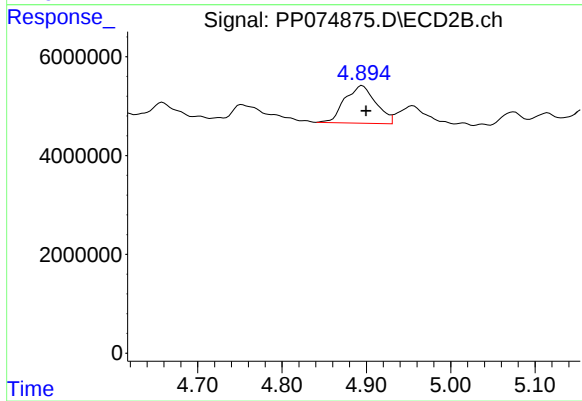

#16 AR-1242-1


R.T.: 4.895 min
Delta R.T.: -0.004 min
Response: 19489904
Conc: 46.21 ng/ml

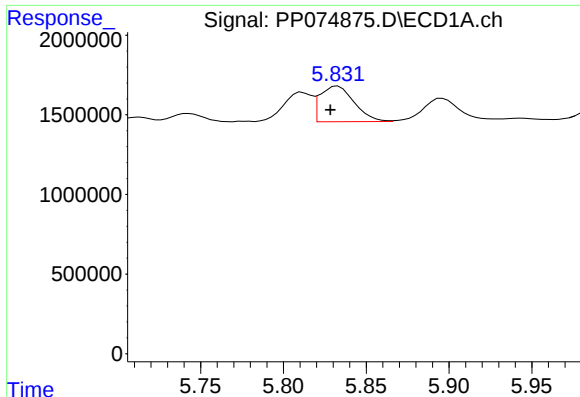

#17 AR-1242-2


R.T.: 5.833 min
Delta R.T.: 0.004 min
Response: 3215246
Conc: 56.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

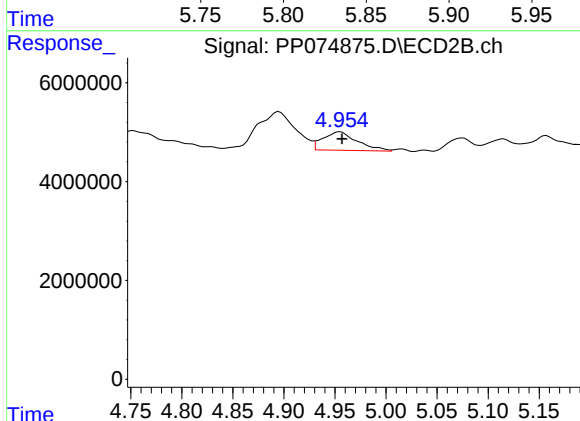


#17 AR-1242-2

R.T.: 4.955 min
Delta R.T.: -0.001 min
Response: 8767763
Conc: 43.78 ng/ml

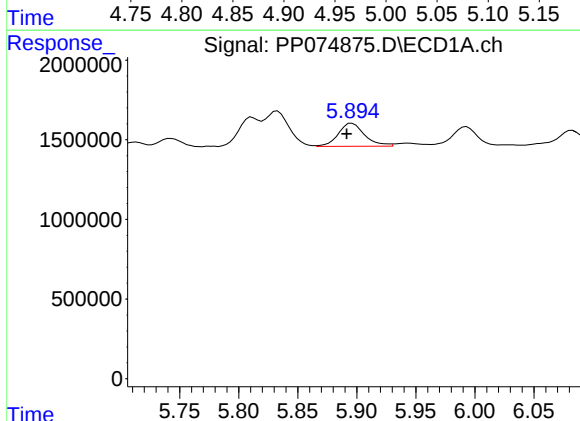


#18 AR-1242-3

R.T.: 5.896 min
Delta R.T.: 0.004 min
Response: 2255642
Conc: 55.55 ng/ml

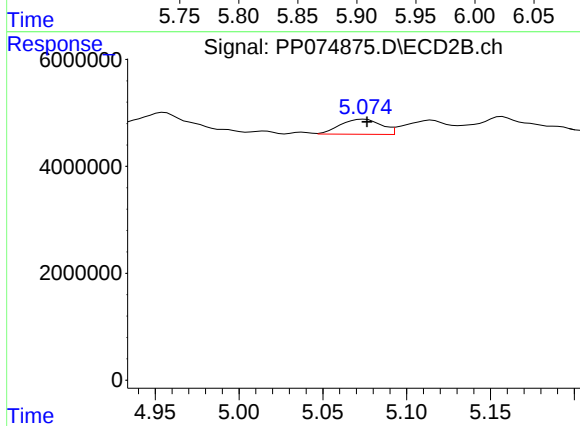

#18 AR-1242-3


R.T.: 5.075 min
Delta R.T.: -0.001 min
Response: 4766960
Conc: 40.30 ng/ml

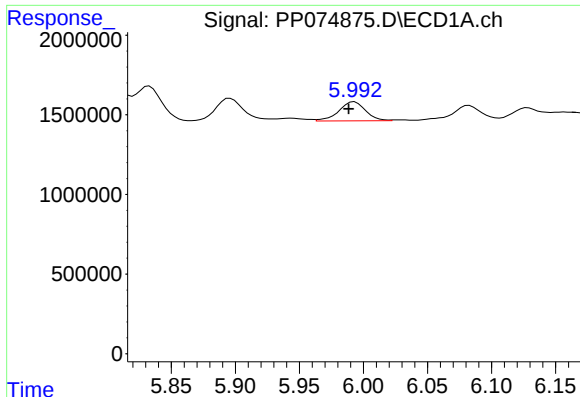

#19 AR-1242-4


R.T.: 5.993 min
Delta R.T.: 0.004 min
Response: 1733235
Conc: 54.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

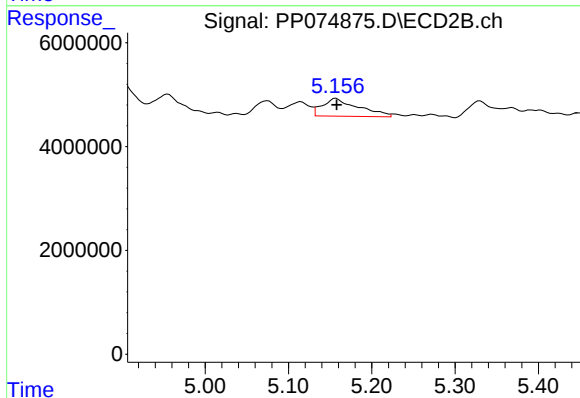


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 10352253
Conc: 60.48 ng/ml

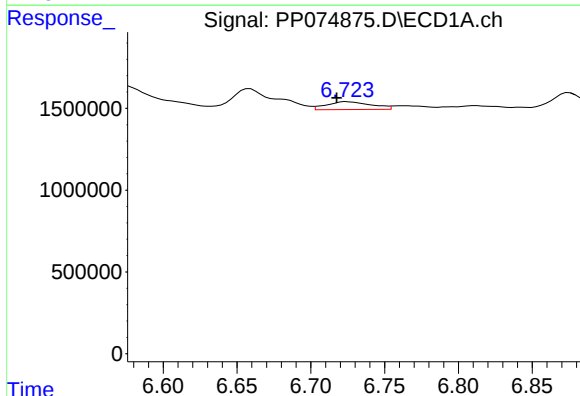


#20 AR-1242-5

R.T.: 6.724 min
Delta R.T.: 0.007 min
Response: 1016776
Conc: 28.19 ng/ml

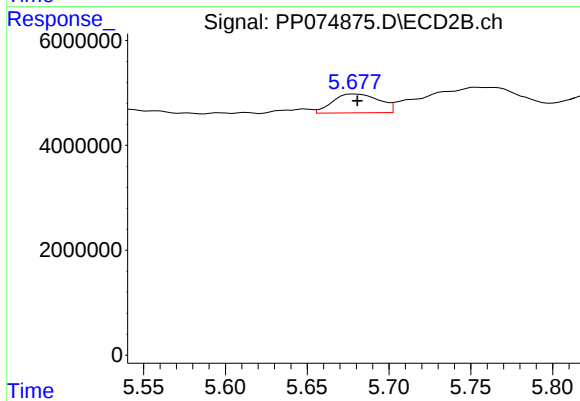

#20 AR-1242-5


R.T.: 5.679 min
Delta R.T.: -0.002 min
Response: 7060906
Conc: 38.13 ng/ml

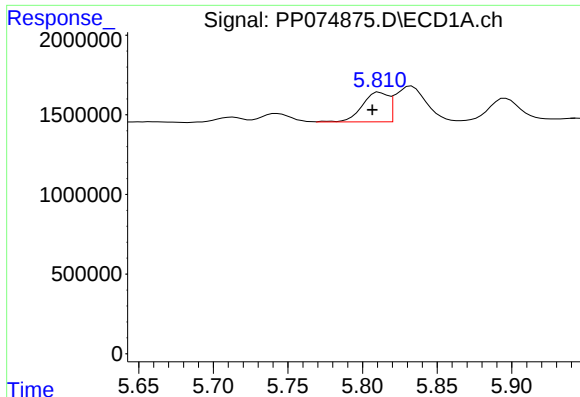

#21 AR-1248-1


R.T.: 5.811 min
Delta R.T.: 0.005 min
Response: 2258980
Conc: 74.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

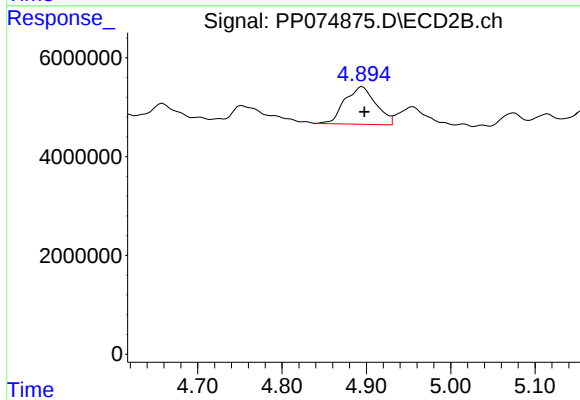


#21 AR-1248-1

R.T.: 4.895 min
Delta R.T.: -0.002 min
Response: 19489904
Conc: 70.58 ng/ml

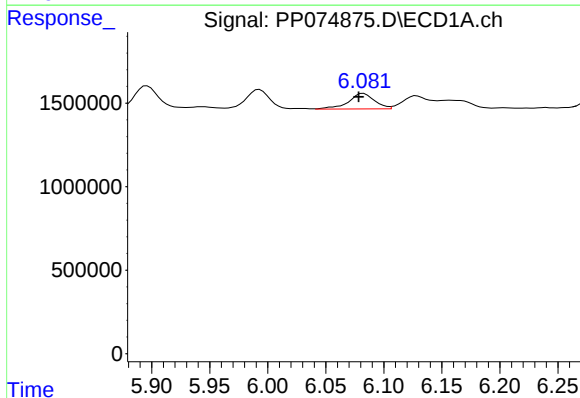


#22 AR-1248-2

R.T.: 6.082 min
Delta R.T.: 0.004 min
Response: 1462636
Conc: 33.94 ng/ml

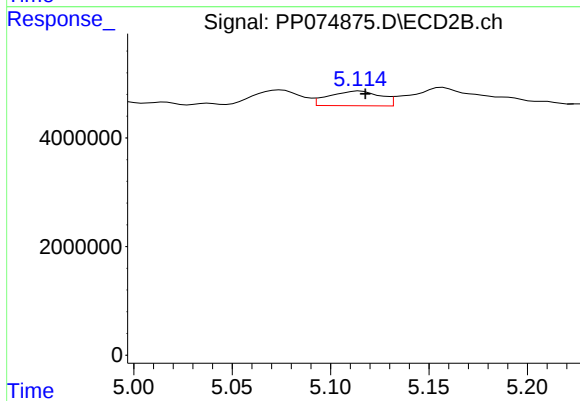

#22 AR-1248-2


R.T.: 5.115 min
Delta R.T.: -0.002 min
Response: 4906557
Conc: 27.76 ng/ml

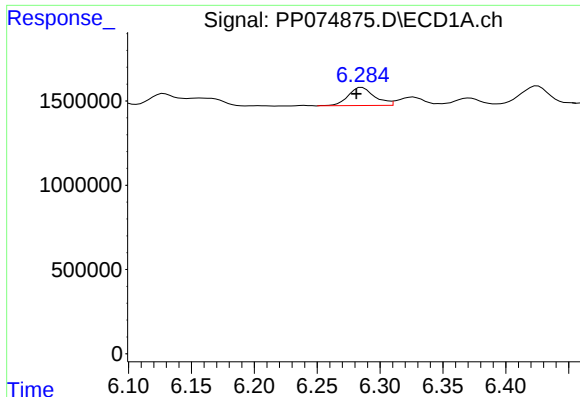

#23 AR-1248-3


R.T.: 6.285 min
Delta R.T.: 0.004 min
Response: 1576307
Conc: 33.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

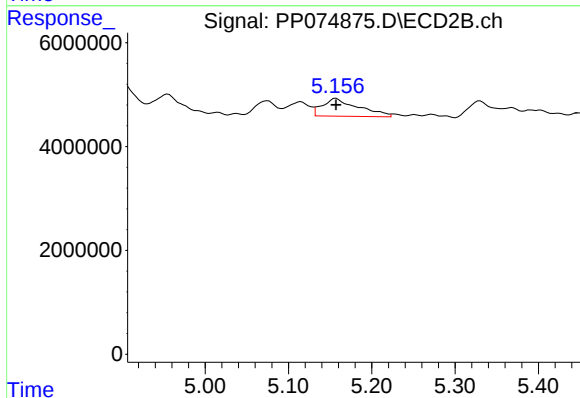


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 10352253
Conc: 45.56 ng/ml

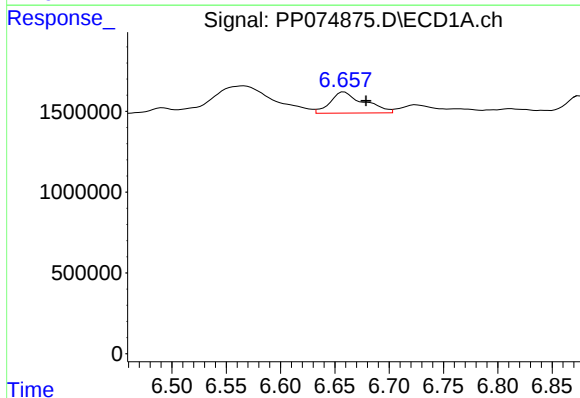


#24 AR-1248-4

R.T.: 6.659 min
Delta R.T.: -0.020 min
Response: 2828441
Conc: 51.43 ng/ml

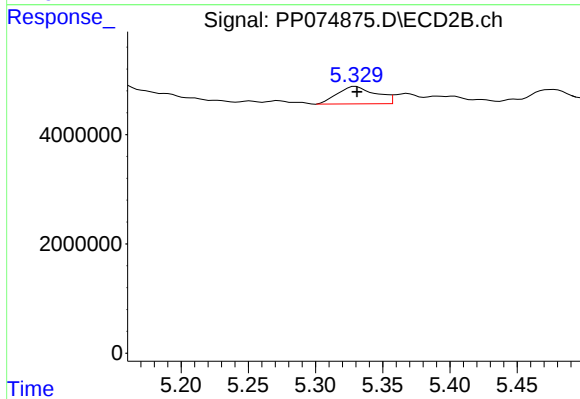

#24 AR-1248-4


R.T.: 5.330 min
Delta R.T.: -0.001 min
Response: 6295851
Conc: 28.88 ng/ml

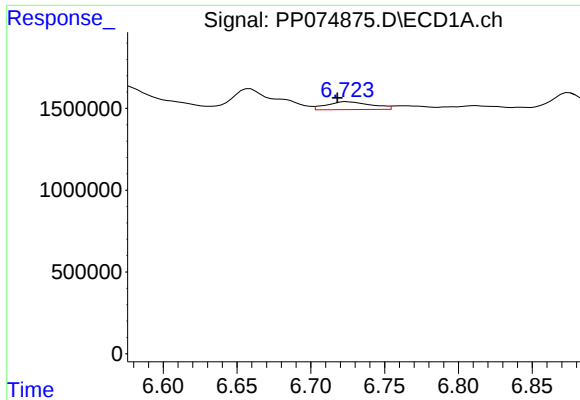

#25 AR-1248-5


R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 1016776
Conc: 18.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

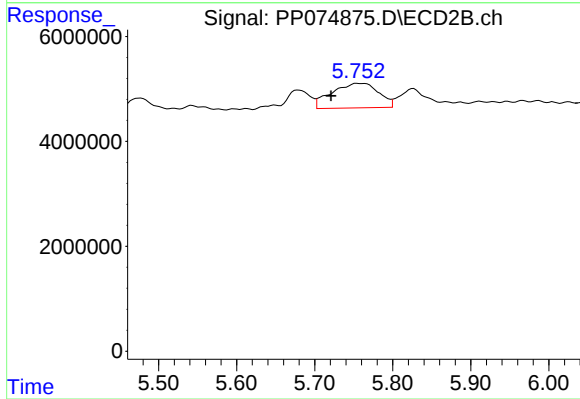


#25 AR-1248-5

R.T.: 5.754 min
Delta R.T.: 0.033 min
Response: 19471345
Conc: 53.01 ng/ml

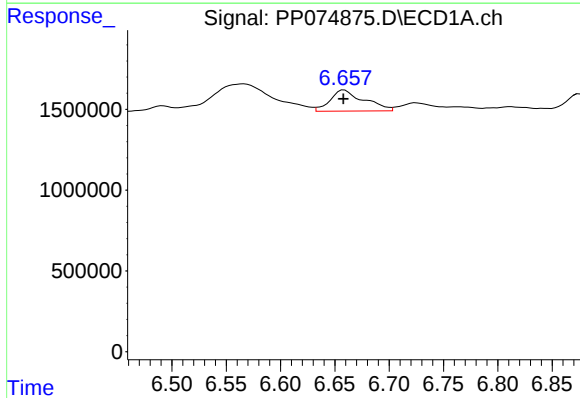


#26 AR-1254-1

R.T.: 6.659 min
Delta R.T.: 0.000 min
Response: 2828441
Conc: 48.54 ng/ml

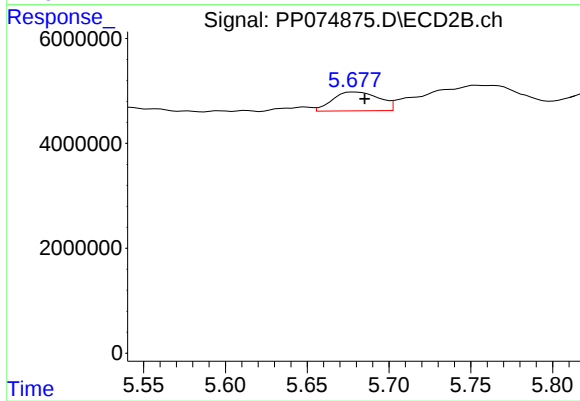

#26 AR-1254-1


R.T.: 5.679 min
Delta R.T.: -0.006 min
Response: 7060906
Conc: 14.81 ng/ml

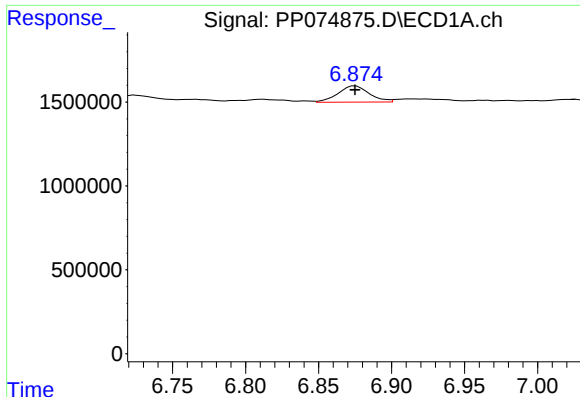

#27 AR-1254-2


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 1445362
Conc: 17.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

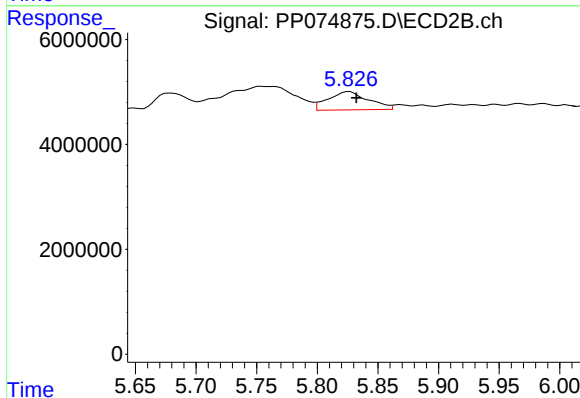


#27 AR-1254-2

R.T.: 5.827 min
Delta R.T.: -0.005 min
Response: 8080450
Conc: 22.95 ng/ml

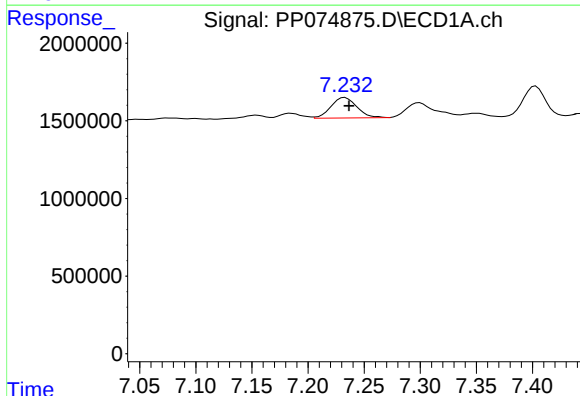


#28 AR-1254-3

R.T.: 7.233 min
Delta R.T.: -0.004 min
Response: 2129630
Conc: 23.87 ng/ml

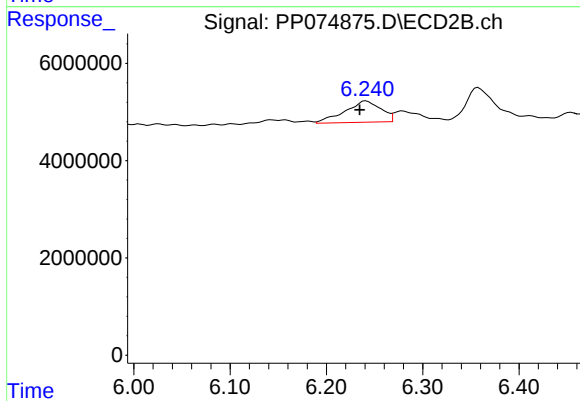

#28 AR-1254-3


R.T.: 6.241 min
Delta R.T.: 0.006 min
Response: 11319502
Conc: 18.26 ng/ml

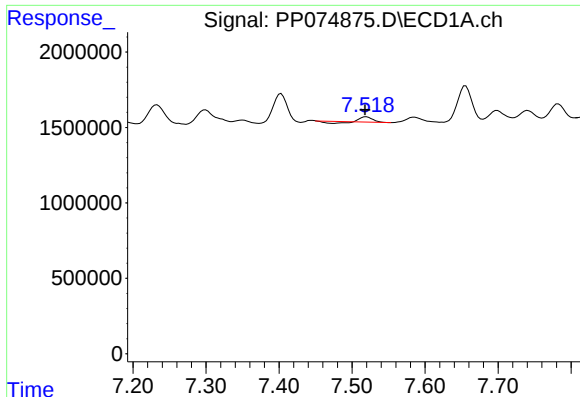

#29 AR-1254-4


R.T.: 7.519 min
Delta R.T.: 0.002 min
Response: 227760
Conc: 3.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

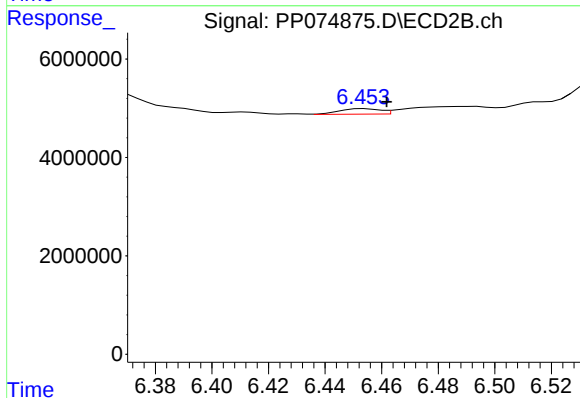


#29 AR-1254-4

R.T.: 6.454 min
Delta R.T.: -0.008 min
Response: 1125848
Conc: 2.40 ng/ml

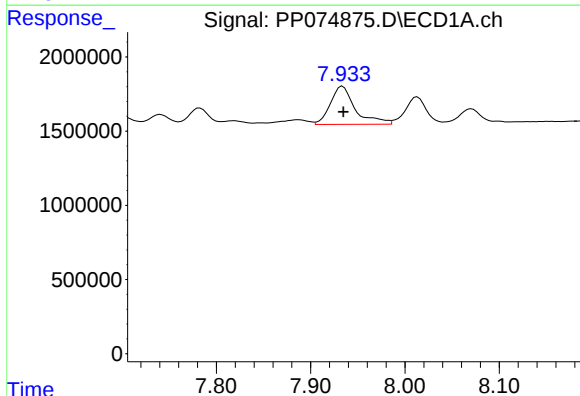


#30 AR-1254-5

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 4729609
Conc: 56.92 ng/ml

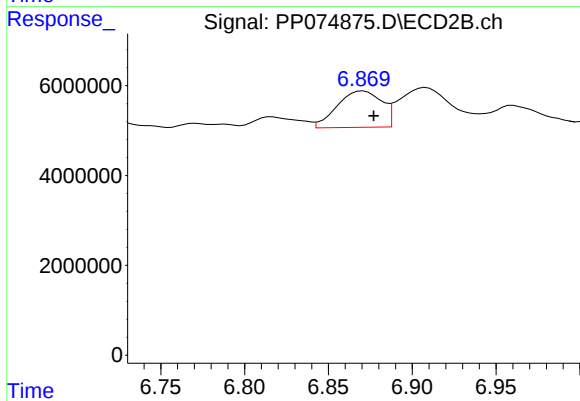

#30 AR-1254-5


R.T.: 6.871 min
Delta R.T.: -0.006 min
Response: 14859883
Conc: 30.30 ng/ml

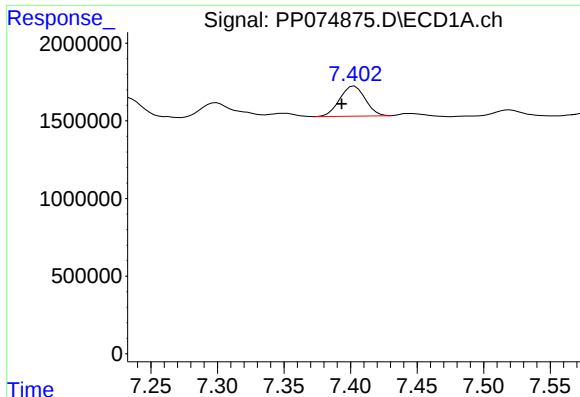

#31 AR-1260-1


R.T.: 7.403 min
Delta R.T.: 0.010 min
Response: 2586499
Conc: 44.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

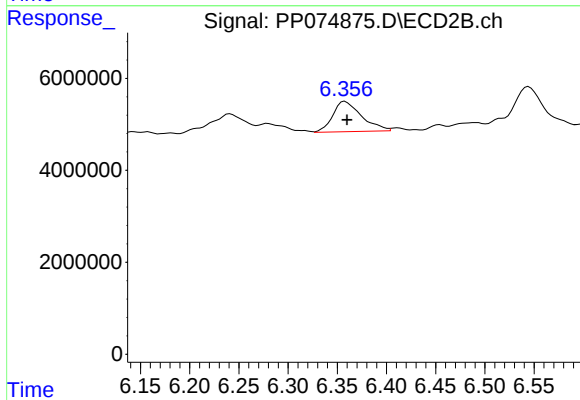


#31 AR-1260-1

R.T.: 6.358 min
Delta R.T.: -0.002 min
Response: 13436869
Conc: 35.81 ng/ml

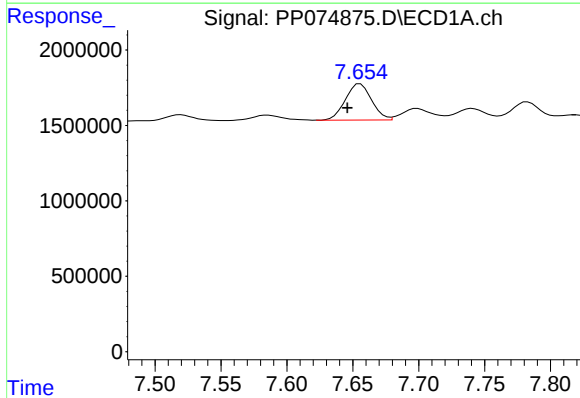


#32 AR-1260-2

R.T.: 7.656 min
Delta R.T.: 0.010 min
Response: 3324414
Conc: 48.24 ng/ml

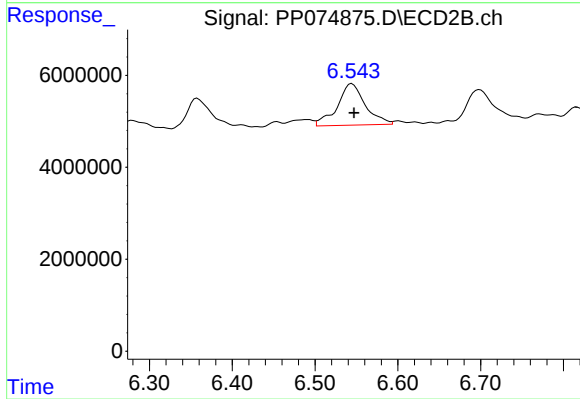

#32 AR-1260-2


R.T.: 6.544 min
Delta R.T.: -0.003 min
Response: 21131475
Conc: 39.96 ng/ml

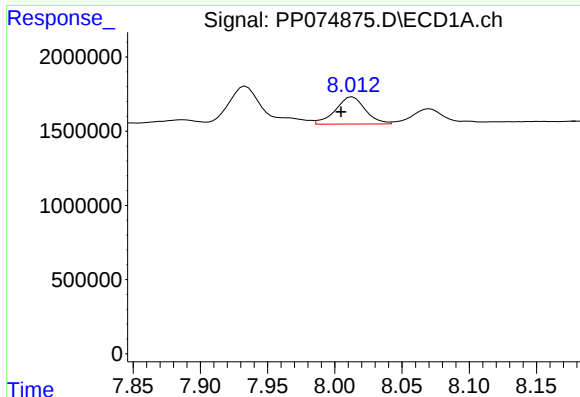

#33 AR-1260-3


R.T.: 8.013 min
Delta R.T.: 0.009 min
Response: 2823167
Conc: 54.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

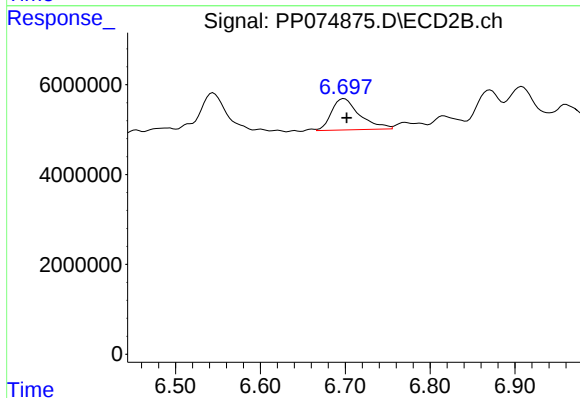


#33 AR-1260-3

R.T.: 6.699 min
Delta R.T.: -0.003 min
Response: 16059205
Conc: 37.09 ng/ml

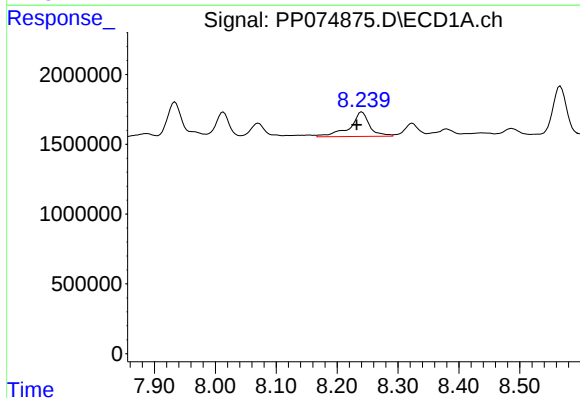


#34 AR-1260-4

R.T.: 8.241 min
Delta R.T.: 0.009 min
Response: 3938108
Conc: 61.73 ng/ml

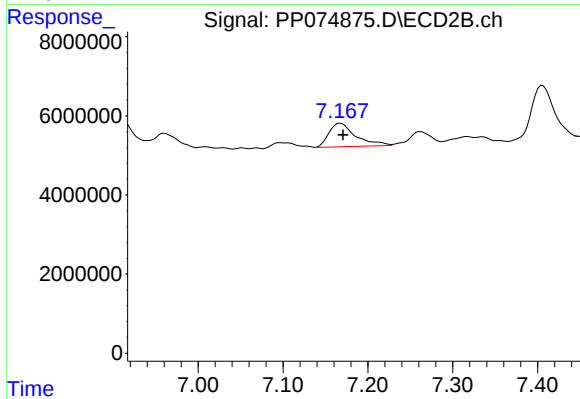

#34 AR-1260-4


R.T.: 7.168 min
Delta R.T.: -0.003 min
Response: 13071533
Conc: 34.27 ng/ml

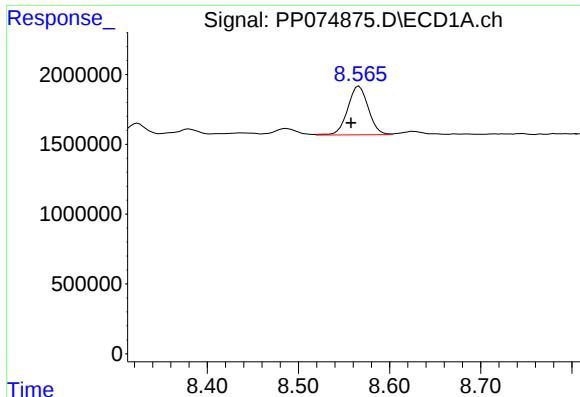

#35 AR-1260-5


R.T.: 8.567 min
Delta R.T.: 0.009 min
Response: 5468537
Conc: 48.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

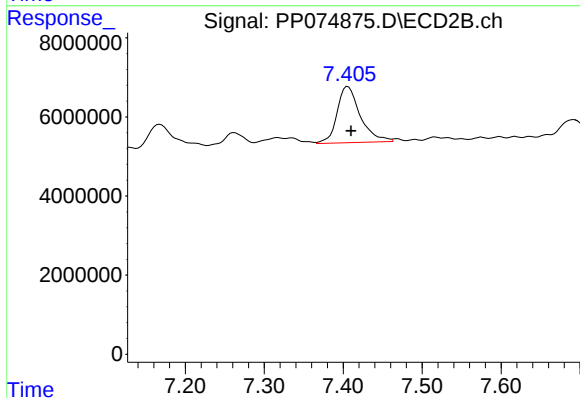


#35 AR-1260-5

R.T.: 7.406 min
Delta R.T.: -0.004 min
Response: 28973873
Conc: 28.84 ng/ml

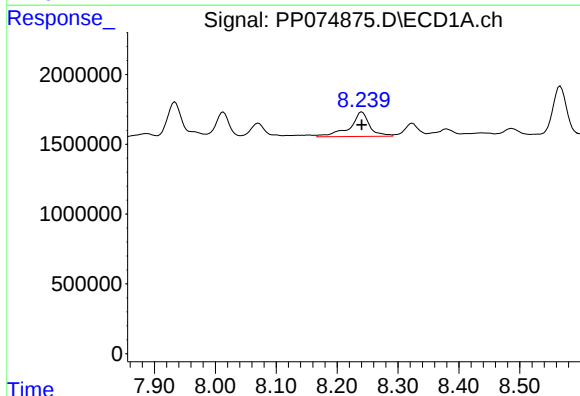


#36 AR-1262-1

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 3938108
Conc: 51.13 ng/ml

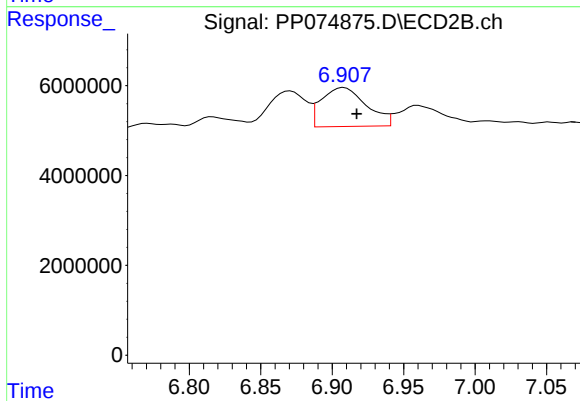

#36 AR-1262-1


R.T.: 6.908 min
Delta R.T.: -0.009 min
Response: 18970966
Conc: 26.82 ng/ml

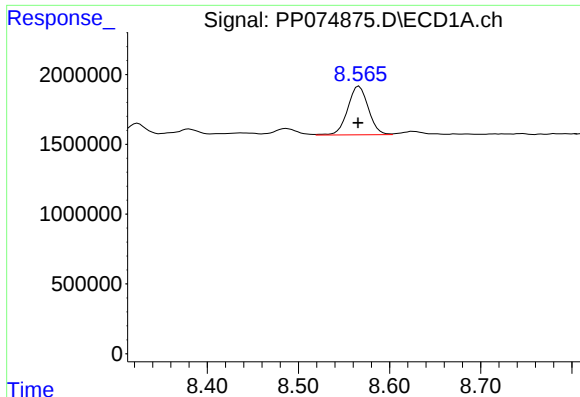

#37 AR-1262-2


R.T.: 8.567 min
Delta R.T.: 0.000 min
Response: 5468537
Conc: 41.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

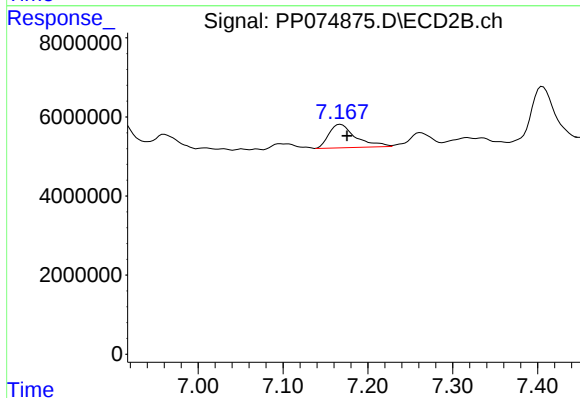


#37 AR-1262-2

R.T.: 7.168 min
Delta R.T.: -0.008 min
Response: 13071533
Conc: 25.10 ng/ml

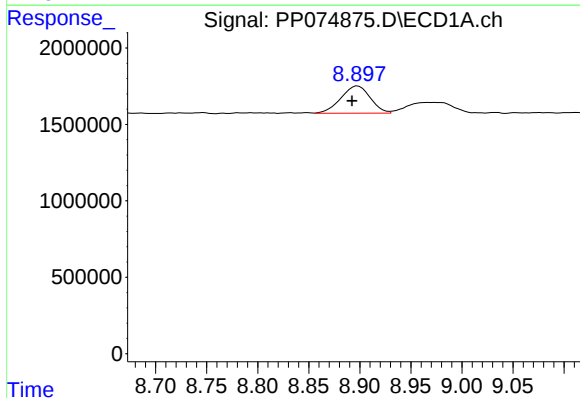


#38 AR-1262-3

R.T.: 8.898 min
Delta R.T.: 0.006 min
Response: 3582579
Conc: 36.85 ng/ml

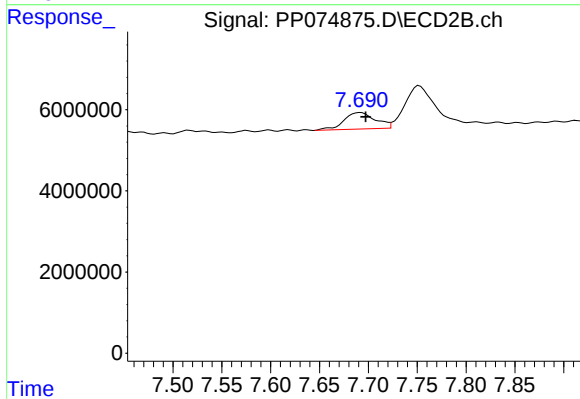

#38 AR-1262-3


R.T.: 7.692 min
Delta R.T.: -0.005 min
Response: 9230242
Conc: 19.79 ng/ml

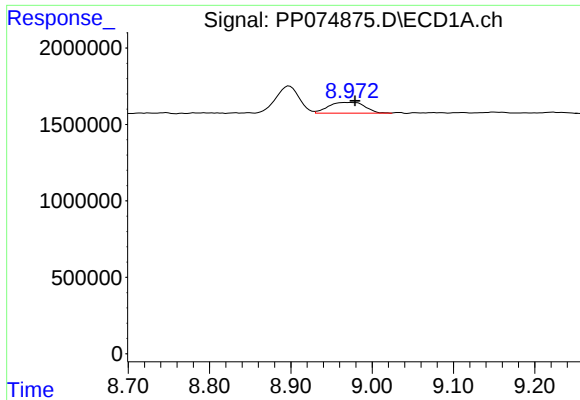

#39 AR-1262-4


R.T.: 8.967 min
Delta R.T.: -0.011 min
Response: 2189478
Conc: 29.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

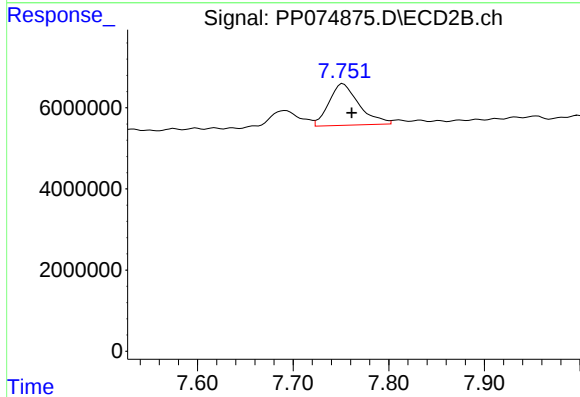


#39 AR-1262-4

R.T.: 7.752 min
Delta R.T.: -0.009 min
Response: 22495730
Conc: 27.37 ng/ml

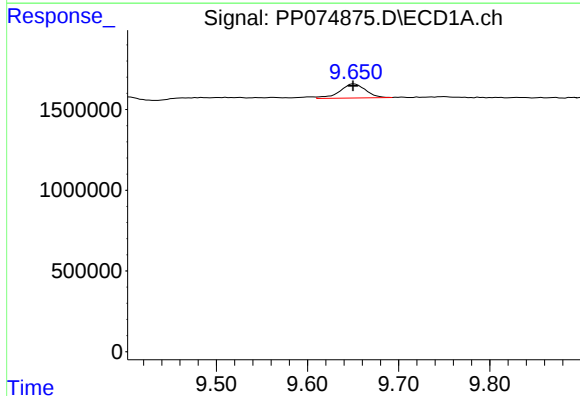


#40 AR-1262-5

R.T.: 9.651 min
Delta R.T.: 0.001 min
Response: 1700128
Conc: 27.89 ng/ml

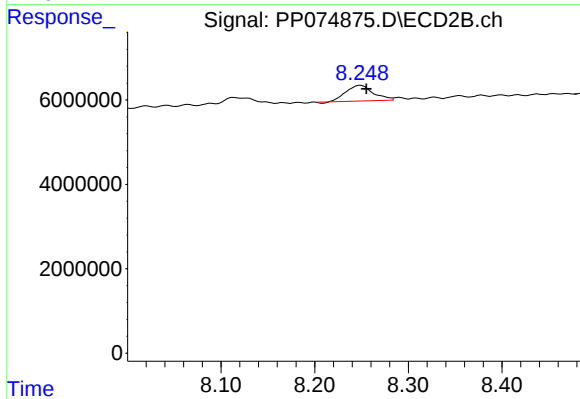

#40 AR-1262-5


R.T.: 8.249 min
Delta R.T.: -0.006 min
Response: 7438845
Conc: 20.76 ng/ml

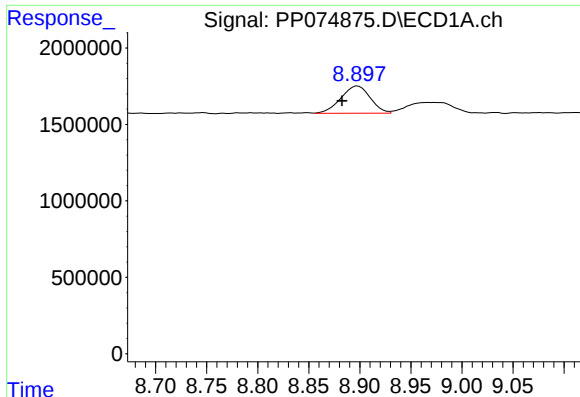

#41 AR-1268-1


R.T.: 8.898 min
Delta R.T.: 0.015 min
Response: 3582579
Conc: 22.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

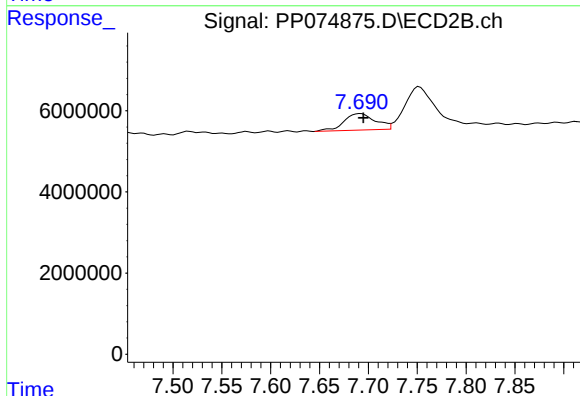


#41 AR-1268-1

R.T.: 7.692 min
Delta R.T.: -0.003 min
Response: 9230242
Conc: 6.54 ng/ml

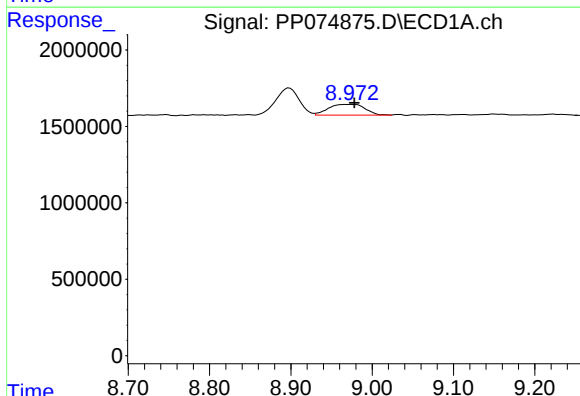


#42 AR-1268-2

R.T.: 8.967 min
Delta R.T.: -0.011 min
Response: 2189478
Conc: 14.92 ng/ml

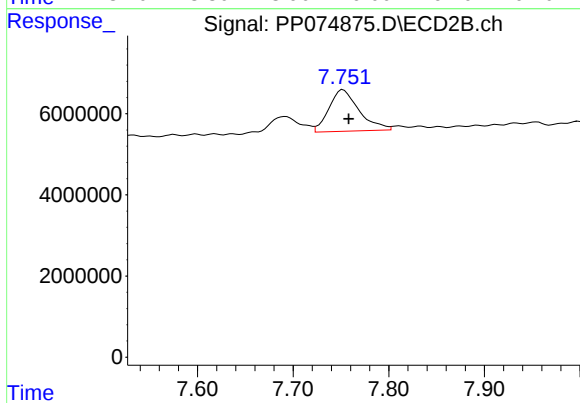

#42 AR-1268-2


R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 22495730
Conc: 16.50 ng/ml

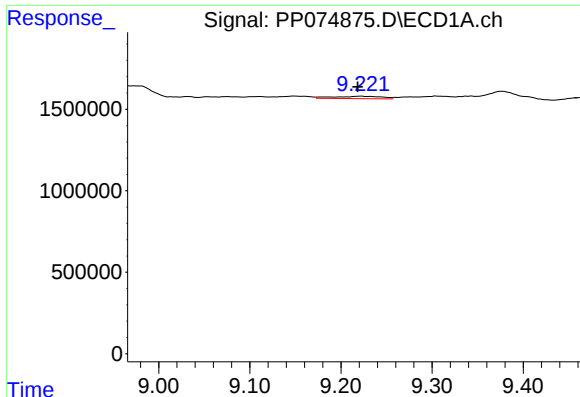

#43 AR-1268-3


R.T.: 9.222 min
Delta R.T.: 0.004 min
Response: 550172
Conc: 4.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

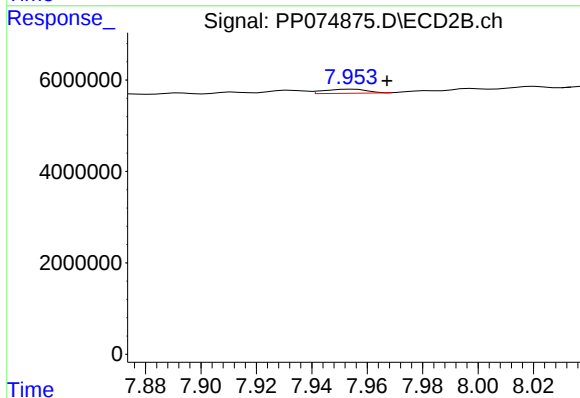


#43 AR-1268-3

R.T.: 7.954 min
Delta R.T.: -0.013 min
Response: 974787
Conc: 0.93 ng/ml

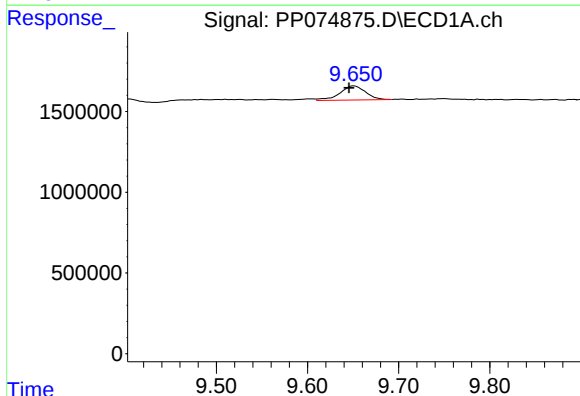


#44 AR-1268-4

R.T.: 9.651 min
Delta R.T.: 0.006 min
Response: 1700128
Conc: 25.28 ng/ml

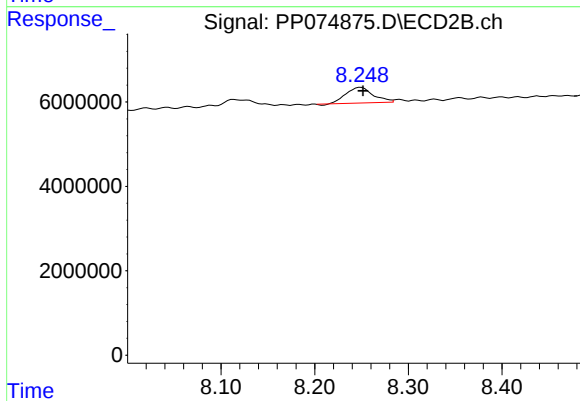

#44 AR-1268-4


R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 7438845
Conc: 19.42 ng/ml

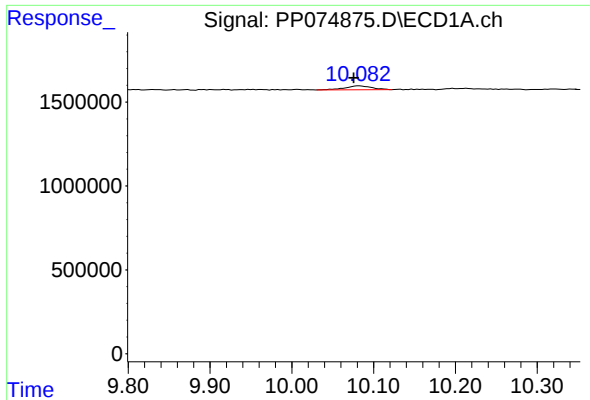

#45 AR-1268-5

R.T.: 10.083 min
Delta R.T.: 0.007 min
Response: 523979
Conc: 1.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

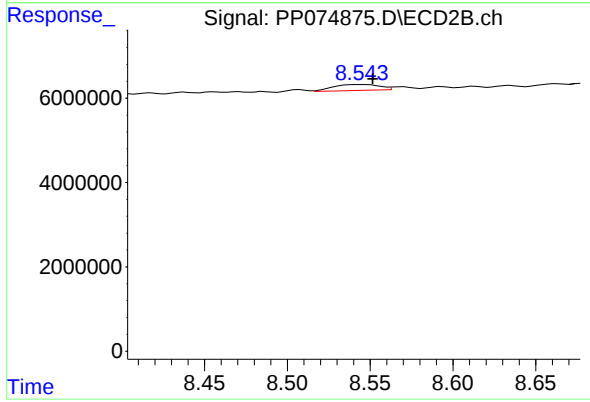

#45 AR-1268-5

R.T.: 8.545 min
Delta R.T.: -0.007 min
Response: 2740598
Conc: 0.87 ng/ml