

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074876.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 20:16
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1221 WATER LOD 40PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:08:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.659	3.800	26997688	98876939	22.063	20.448
2)	SA Decachlor...	10.437	8.810	20960348	132.5E6	21.225	17.675
Target Compounds							
3)	L1 AR-1016-1	5.830	4.897	420410	688890	9.536	1.352 #
4)	L1 AR-1016-2	5.830	4.961	420410	977981	6.690	4.109 #
5)	L1 AR-1016-3	5.897	5.072	447535	514333	9.964	3.730 #
6)	L1 AR-1016-4	5.985	5.109	145532	365813	4.137	2.617 #
7)	L1 AR-1016-5	0.000	5.326	0	552294	N.D.	3.325 #
8)	L2 AR-1221-1	4.857	4.010	747905	1526119	42.512	24.668 #
9)	L2 AR-1221-2	4.950	4.095	858180	2116053	64.249	46.803 #
10)	L2 AR-1221-3	5.020	4.171	1577290	5509802	41.603	33.536
11)	L3 AR-1232-1	5.020	4.171	1577290	5509802	51.929	43.013
12)	L3 AR-1232-2	5.543	4.897	148113	688890	9.399	2.972 #
13)	L3 AR-1232-3	5.830	5.072	420410	514333	13.764	8.564 #
14)	L3 AR-1232-4	5.985	5.152	145532	767420	8.427	10.412
15)	L3 AR-1232-5	6.086	5.326	103831	552294	7.999	8.896
16)	L4 AR-1242-1	5.830	4.897	420410	688890	10.984	1.633 #
17)	L4 AR-1242-2	5.830	4.961	420410	977981	7.443	4.883 #
18)	L4 AR-1242-3	5.897	5.072	447535	514333	11.022	4.348 #
19)	L4 AR-1242-4	5.985	5.152	145532	767420	4.585	4.484
20)	L4 AR-1242-5	6.721	5.662	385318	581277	10.682	3.139 #
21)	L5 AR-1248-1	5.830	4.897	420410	688890	13.910	2.495 #
22)	L5 AR-1248-2	6.086	5.109	103831	365813	2.409	2.070
23)	L5 AR-1248-3	0.000	5.152	0	767420	N.D.	3.378 #
24)	L5 AR-1248-4	6.655	5.326	1282857	552294	23.324	2.533 #
25)	L5 AR-1248-5	6.721	5.755	385318	23992133	6.946	65.316 #
26)	L6 AR-1254-1	6.655	5.662	1282857	581277	22.016	1.219 #
27)	L6 AR-1254-2	6.871	5.834	552988	1670366	6.775	4.744 #
28)	L6 AR-1254-3	7.228	6.241	3850748	558352	43.167	0.901 #
29)	L6 AR-1254-4	7.516	6.463	27688	348837	0.420	0.744 #
30)	L6 AR-1254-5	7.935	6.886	34612	746729	0.417	1.522 #
31)	L7 AR-1260-1	7.397	6.353	33894	666330	0.586	1.776 #
32)	L7 AR-1260-2	7.664	6.559	185243	456010	2.688	0.862 #
33)	L7 AR-1260-3	8.000	6.701	49158	450156	0.947	1.040
34)	L7 AR-1260-4	0.000	7.163	0	574405	N.D.	1.506 #
35)	L7 AR-1260-5	8.553	7.402	30830	632243	0.272	0.629 #
36)	L8 AR-1262-1	0.000	6.926	0	405630	N.D.	0.574 #
37)	L8 AR-1262-2	8.553	7.187	30830	757281	0.233	1.454 #
38)	L8 AR-1262-3	0.000	7.701	0	4832702	N.D.	10.364 #
39)	L8 AR-1262-4	0.000	7.760	0	1708404	N.D.	2.079 #
40)	L8 AR-1262-5	9.634	8.253	88386	163138	1.450	0.455 #
41)	L9 AR-1268-1	0.000	7.701	0	4832702	N.D.	3.426 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 20:16
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1221 WATER LOD 40PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:08:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	0.000	7.760	0	1708404	N.D.	1.253 #
43)	L9 AR-1268-3	9.152f	7.957	316888	772692	2.564	0.741 #
44)	L9 AR-1268-4	9.634	8.253	88386	163138	1.314	0.426 #
45)	L9 AR-1268-5	10.071	8.545	50958	489735	0.138	0.156


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074876.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 20:16
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1221 WATER LOD 40PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:08:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

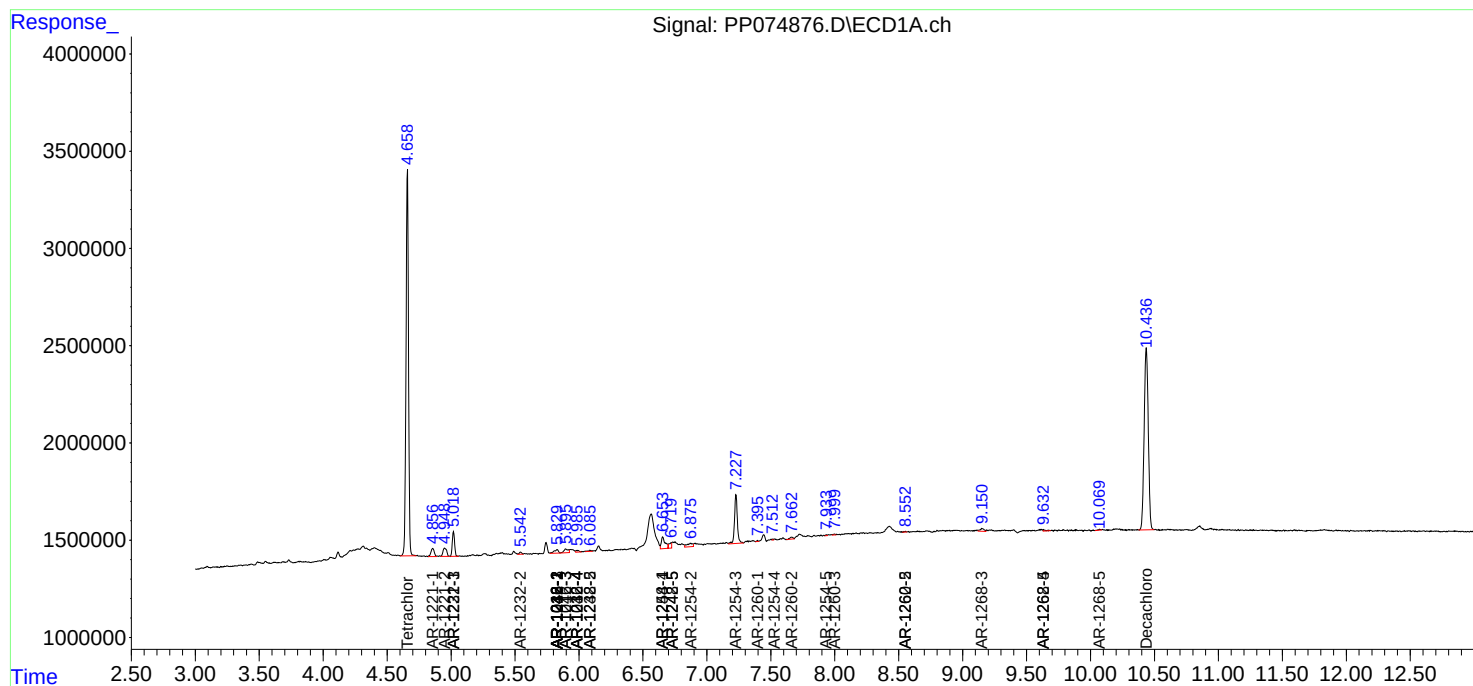


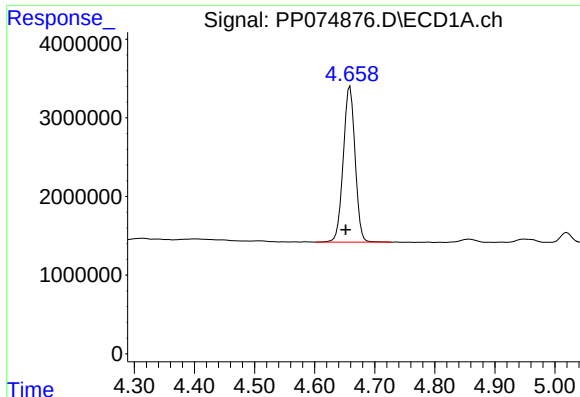

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.007 min
Response: 26997688
Conc: 22.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

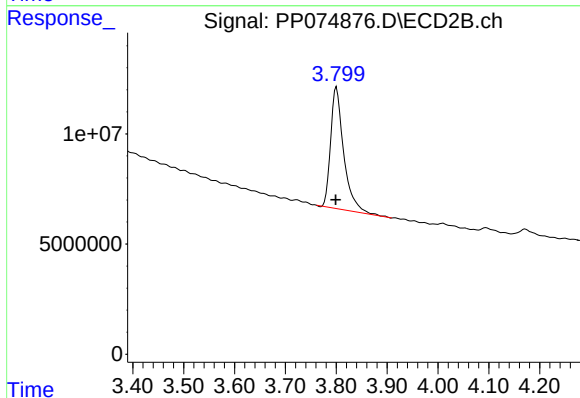


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.002 min
Response: 98876939
Conc: 20.45 ng/ml

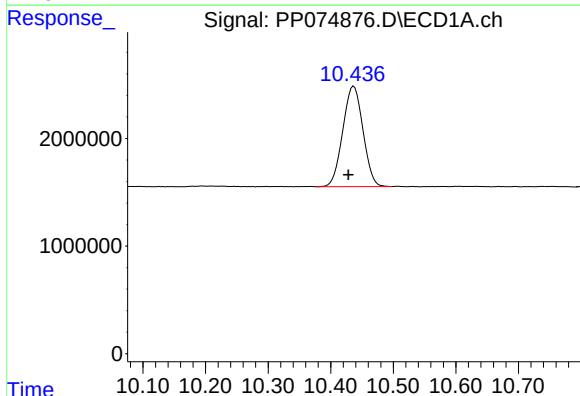


#2 Decachlorobiphenyl

R.T.: 10.437 min
Delta R.T.: 0.009 min
Response: 20960348
Conc: 21.23 ng/ml

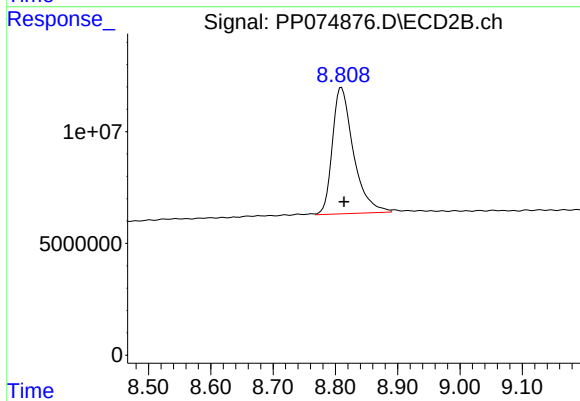

#2 Decachlorobiphenyl


R.T.: 8.810 min
Delta R.T.: -0.004 min
Response: 132547842
Conc: 17.67 ng/ml

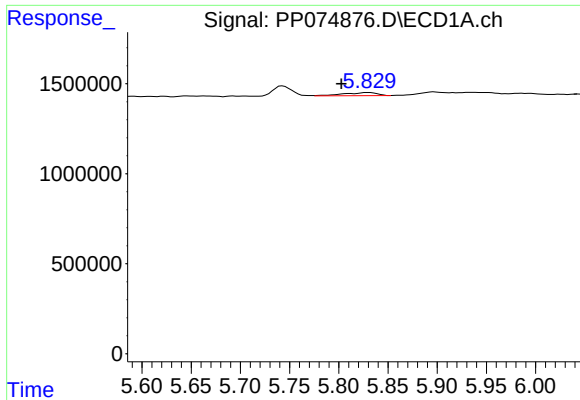

#3 AR-1016-1


R.T.: 5.830 min
Delta R.T.: 0.028 min
Response: 420410
Conc: 9.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

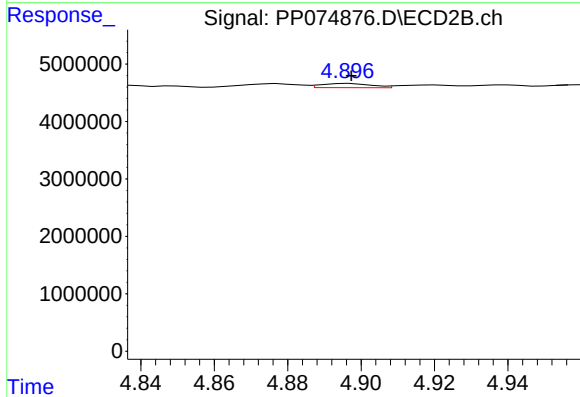


#3 AR-1016-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 688890
Conc: 1.35 ng/ml

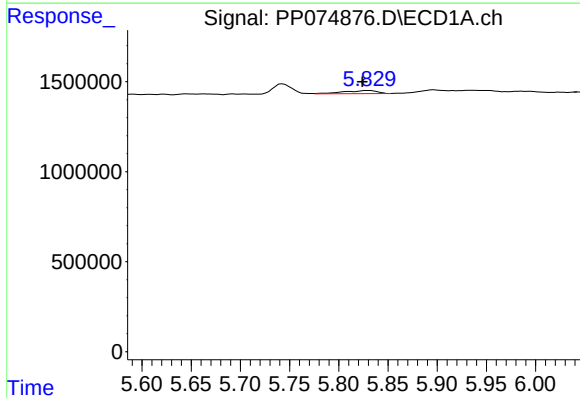


#4 AR-1016-2

R.T.: 5.830 min
Delta R.T.: 0.006 min
Response: 420410
Conc: 6.69 ng/ml

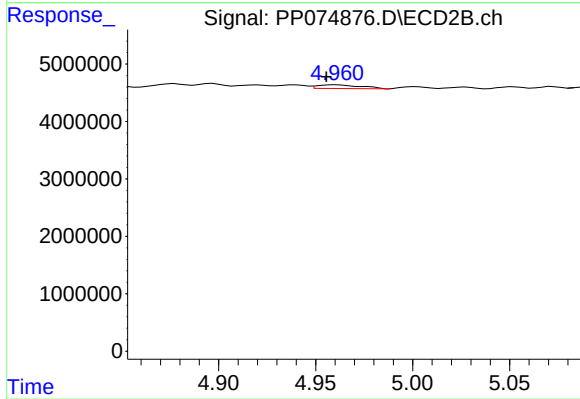

#4 AR-1016-2


R.T.: 4.961 min
Delta R.T.: 0.005 min
Response: 977981
Conc: 4.11 ng/ml

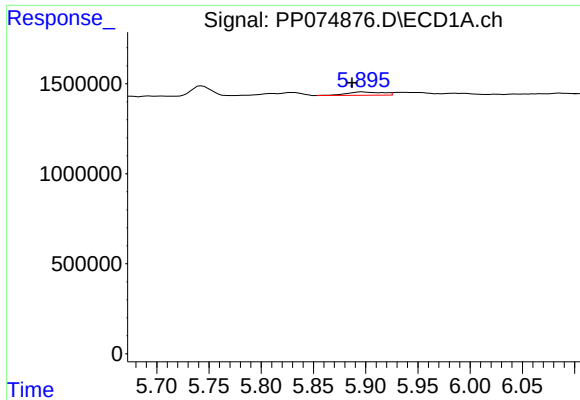

#5 AR-1016-3


R.T.: 5.897 min
Delta R.T.: 0.010 min
Response: 447535
Conc: 9.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

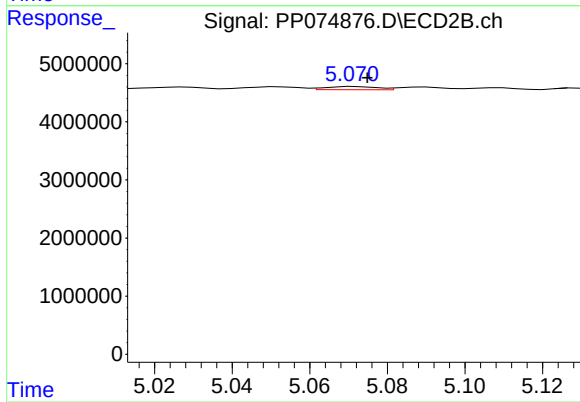


#5 AR-1016-3

R.T.: 5.072 min
Delta R.T.: -0.003 min
Response: 514333
Conc: 3.73 ng/ml

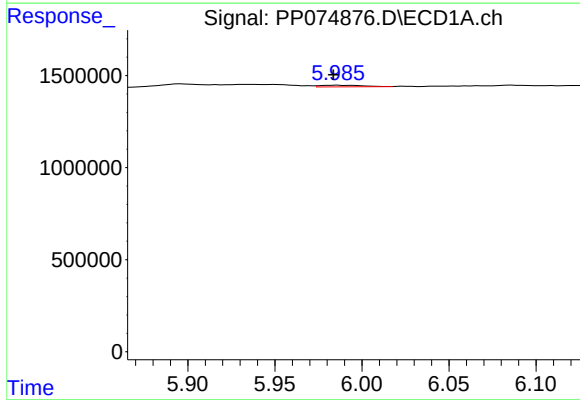


#6 AR-1016-4

R.T.: 5.985 min
Delta R.T.: 0.002 min
Response: 145532
Conc: 4.14 ng/ml

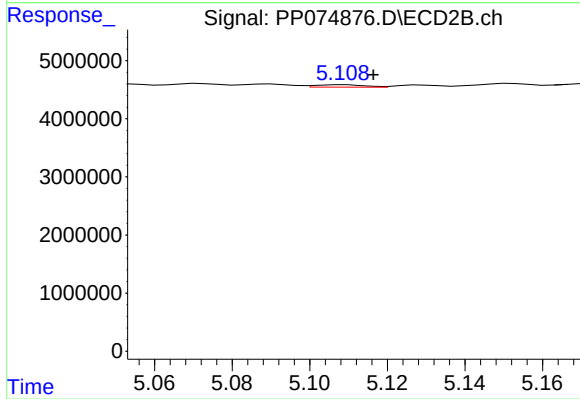

#6 AR-1016-4


R.T.: 5.109 min
Delta R.T.: -0.007 min
Response: 365813
Conc: 2.62 ng/ml

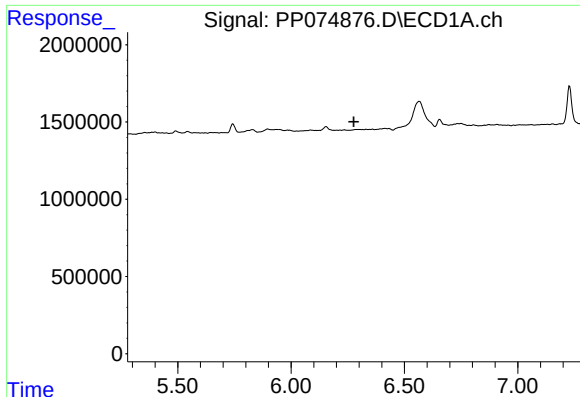

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

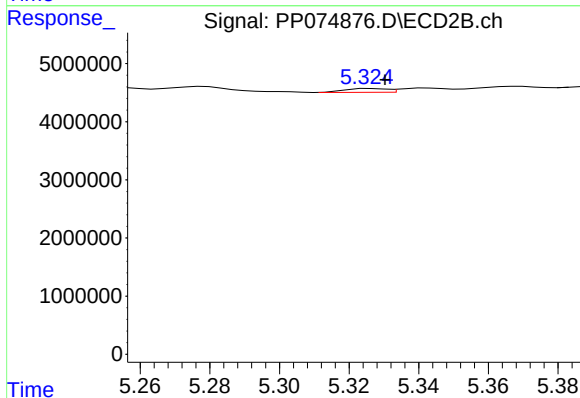


#7 AR-1016-5

R.T.: 5.326 min
Delta R.T.: -0.004 min
Response: 552294
Conc: 3.33 ng/ml

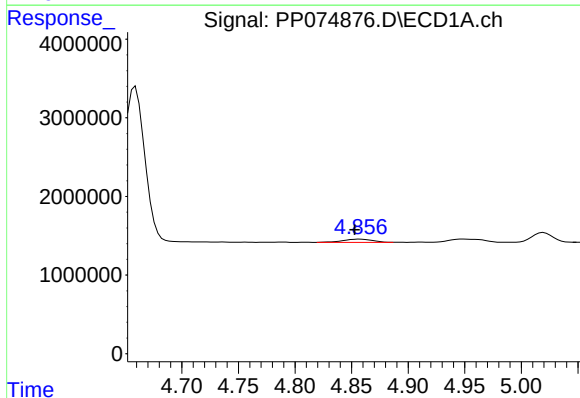


#8 AR-1221-1

R.T.: 4.857 min
Delta R.T.: 0.004 min
Response: 747905
Conc: 42.51 ng/ml

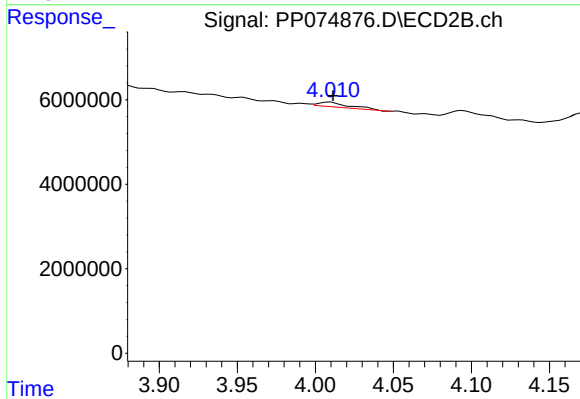

#8 AR-1221-1


R.T.: 4.010 min
Delta R.T.: -0.001 min
Response: 1526119
Conc: 24.67 ng/ml

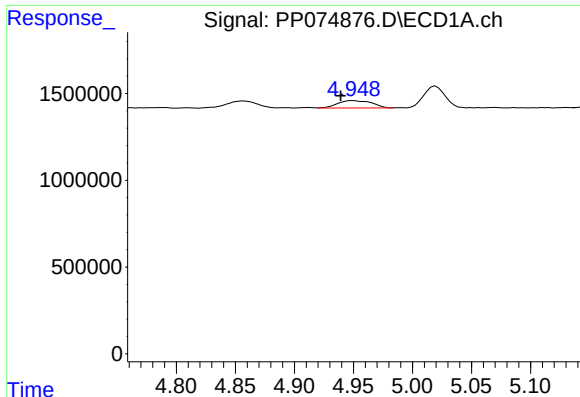

#9 AR-1221-2


R.T.: 4.950 min
Delta R.T.: 0.010 min
Response: 858180
Conc: 64.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

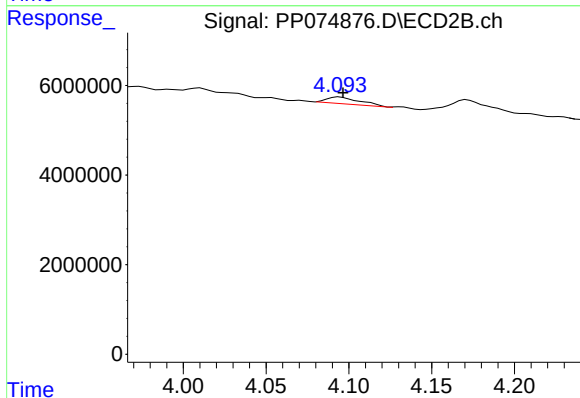


#9 AR-1221-2

R.T.: 4.095 min
Delta R.T.: -0.002 min
Response: 2116053
Conc: 46.80 ng/ml

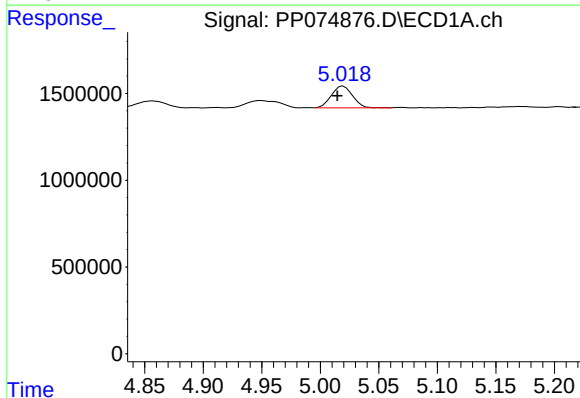


#10 AR-1221-3

R.T.: 5.020 min
Delta R.T.: 0.005 min
Response: 1577290
Conc: 41.60 ng/ml

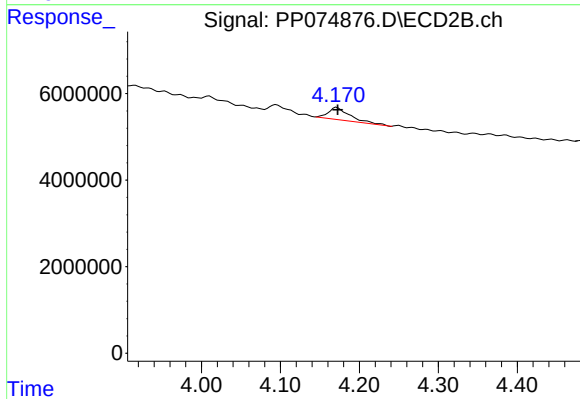

#10 AR-1221-3


R.T.: 4.171 min
Delta R.T.: -0.001 min
Response: 5509802
Conc: 33.54 ng/ml

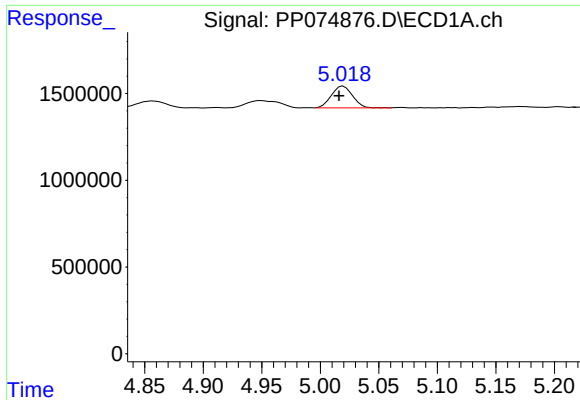

#11 AR-1232-1


R.T.: 5.020 min
Delta R.T.: 0.004 min
Response: 1577290
Conc: 51.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

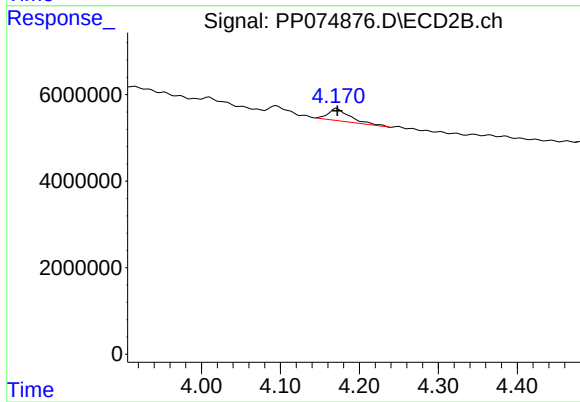


#11 AR-1232-1

R.T.: 4.171 min
Delta R.T.: 0.000 min
Response: 5509802
Conc: 43.01 ng/ml

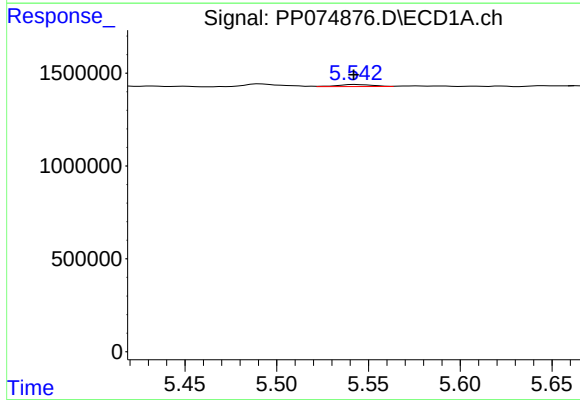


#12 AR-1232-2

R.T.: 5.543 min
Delta R.T.: 0.001 min
Response: 148113
Conc: 9.40 ng/ml

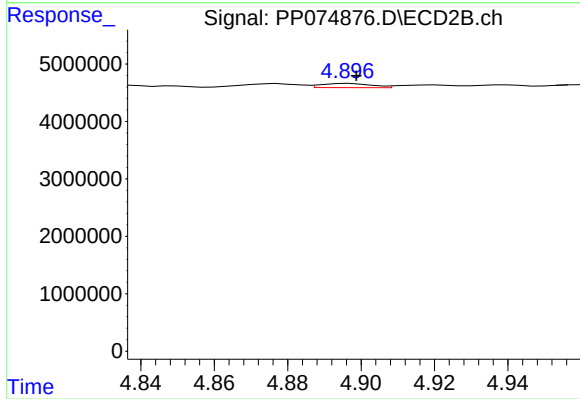

#12 AR-1232-2


R.T.: 4.897 min
Delta R.T.: -0.002 min
Response: 688890
Conc: 2.97 ng/ml

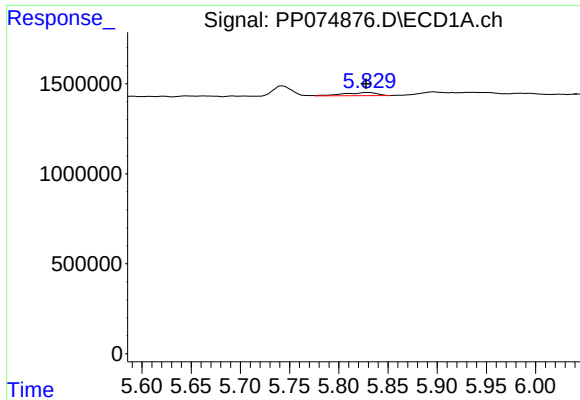

#13 AR-1232-3


R.T.: 5.830 min
Delta R.T.: 0.003 min
Response: 420410
Conc: 13.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

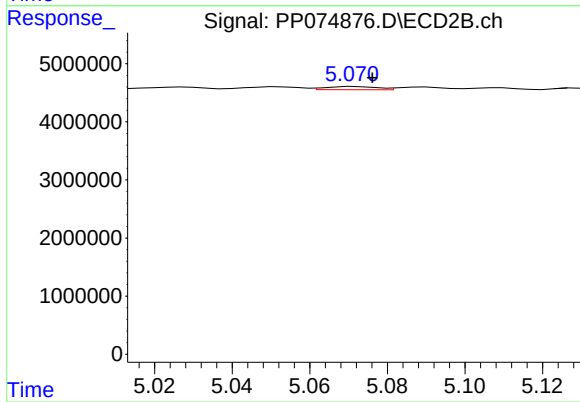


#13 AR-1232-3

R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 514333
Conc: 8.56 ng/ml

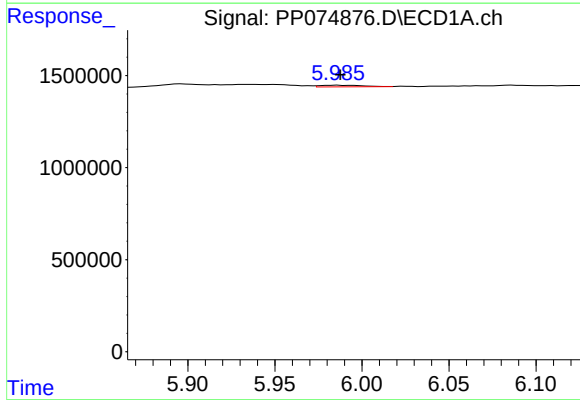


#14 AR-1232-4

R.T.: 5.985 min
Delta R.T.: -0.002 min
Response: 145532
Conc: 8.43 ng/ml

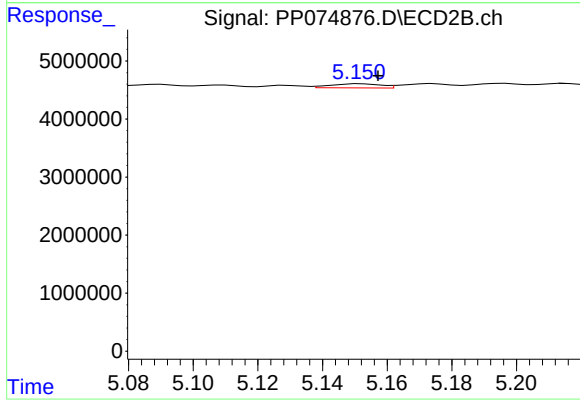

#14 AR-1232-4


R.T.: 5.152 min
Delta R.T.: -0.005 min
Response: 767420
Conc: 10.41 ng/ml

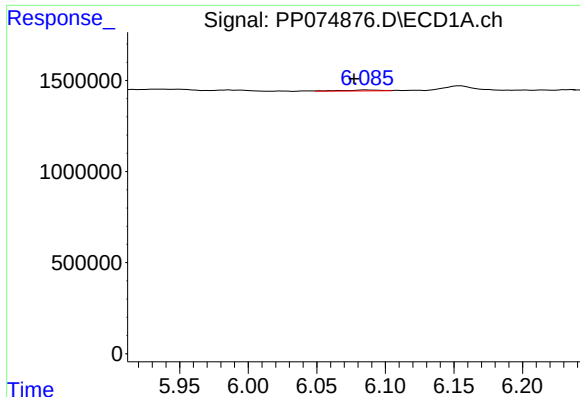

#15 AR-1232-5


R.T.: 6.086 min
Delta R.T.: 0.009 min
Response: 103831
Conc: 8.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

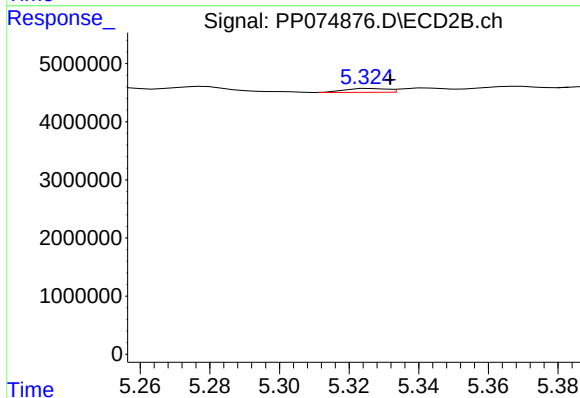


#15 AR-1232-5

R.T.: 5.326 min
Delta R.T.: -0.006 min
Response: 552294
Conc: 8.90 ng/ml

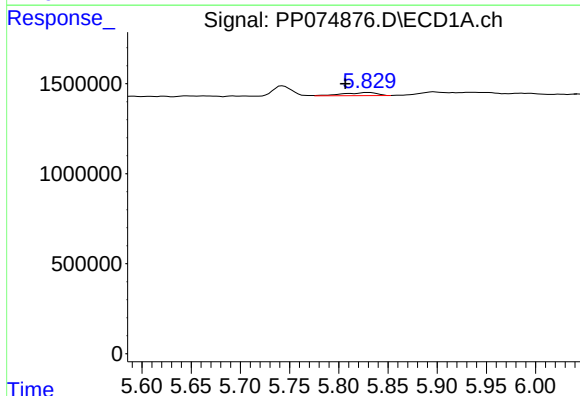


#16 AR-1242-1

R.T.: 5.830 min
Delta R.T.: 0.023 min
Response: 420410
Conc: 10.98 ng/ml

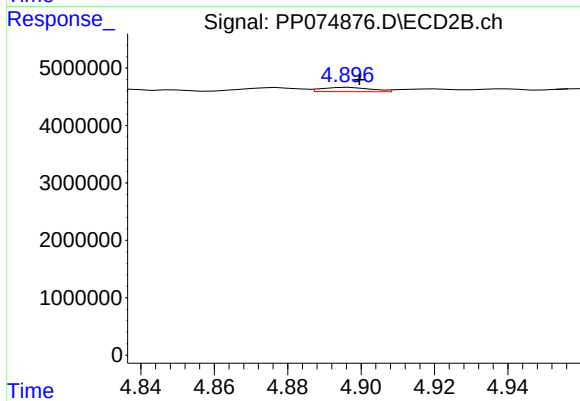

#16 AR-1242-1


R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 688890
Conc: 1.63 ng/ml

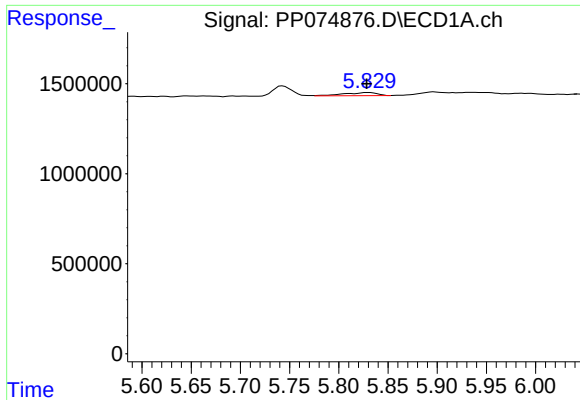

#17 AR-1242-2


R.T.: 5.830 min
Delta R.T.: 0.002 min
Response: 420410
Conc: 7.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

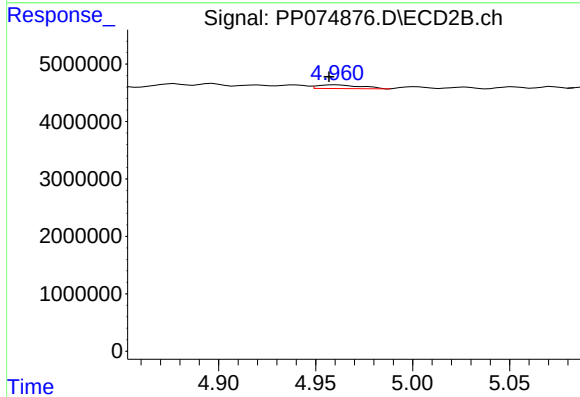


#17 AR-1242-2

R.T.: 4.961 min
Delta R.T.: 0.004 min
Response: 977981
Conc: 4.88 ng/ml

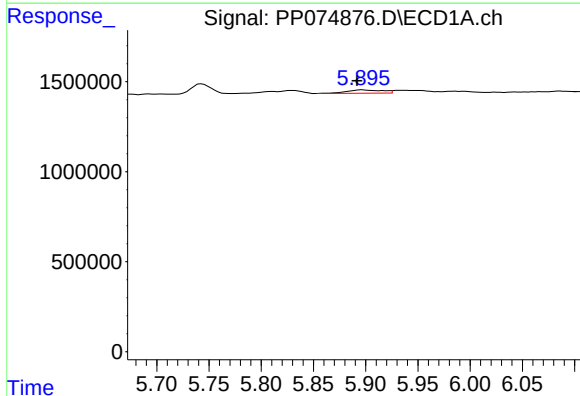


#18 AR-1242-3

R.T.: 5.897 min
Delta R.T.: 0.005 min
Response: 447535
Conc: 11.02 ng/ml

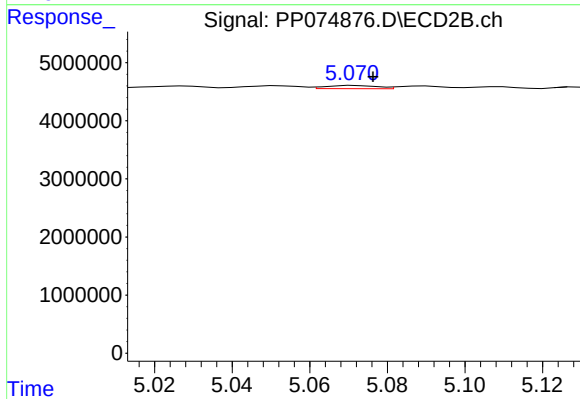

#18 AR-1242-3


R.T.: 5.072 min
Delta R.T.: -0.005 min
Response: 514333
Conc: 4.35 ng/ml

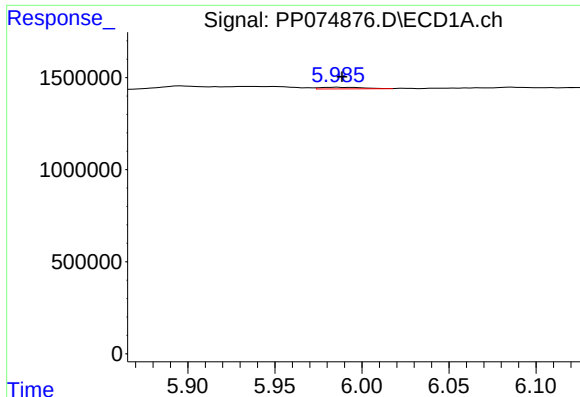

#19 AR-1242-4


R.T.: 5.985 min
Delta R.T.: -0.003 min
Response: 145532
Conc: 4.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

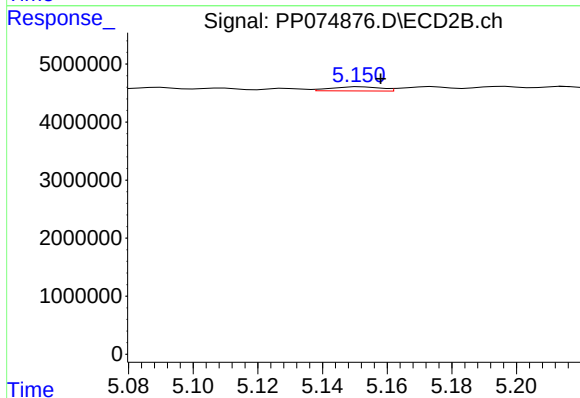


#19 AR-1242-4

R.T.: 5.152 min
Delta R.T.: -0.006 min
Response: 767420
Conc: 4.48 ng/ml

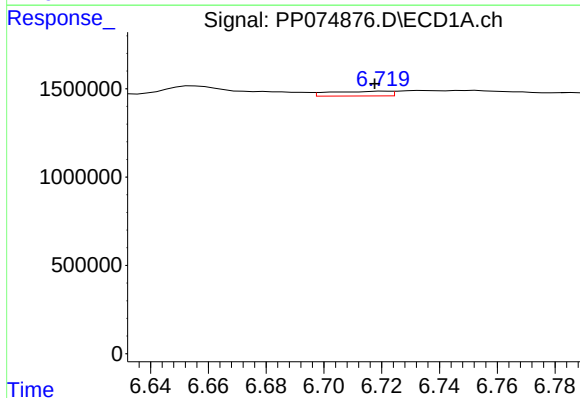


#20 AR-1242-5

R.T.: 6.721 min
Delta R.T.: 0.003 min
Response: 385318
Conc: 10.68 ng/ml

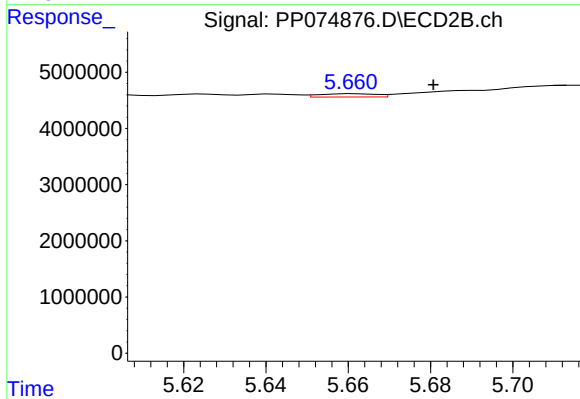

#20 AR-1242-5


R.T.: 5.662 min
Delta R.T.: -0.019 min
Response: 581277
Conc: 3.14 ng/ml

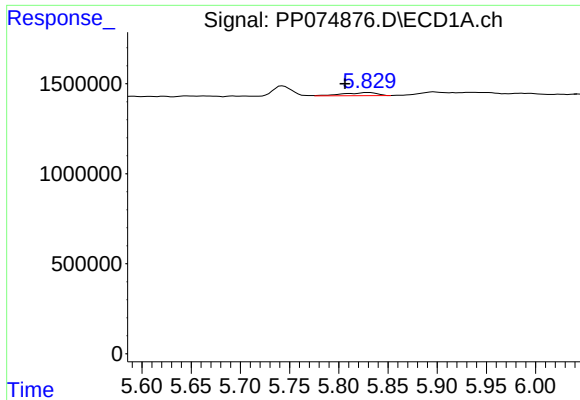

#21 AR-1248-1


R.T.: 5.830 min
Delta R.T.: 0.024 min
Response: 420410
Conc: 13.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

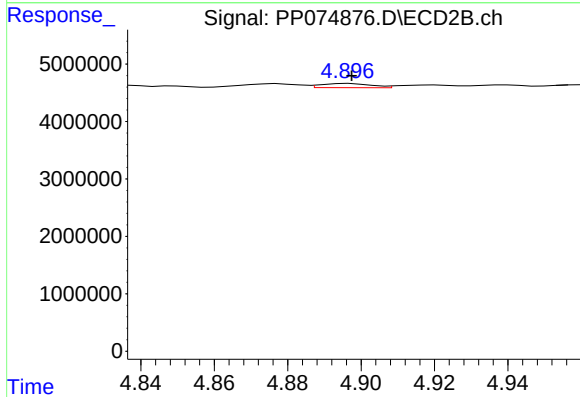


#21 AR-1248-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 688890
Conc: 2.49 ng/ml

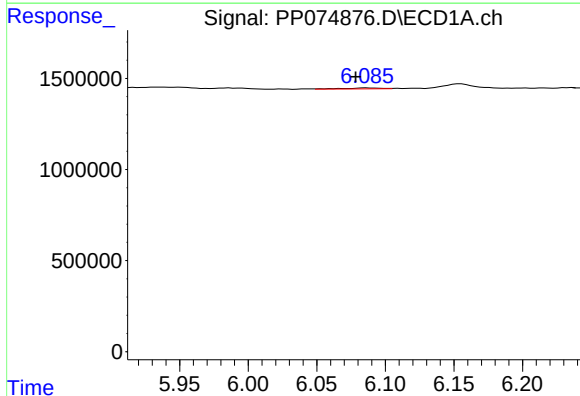


#22 AR-1248-2

R.T.: 6.086 min
Delta R.T.: 0.008 min
Response: 103831
Conc: 2.41 ng/ml

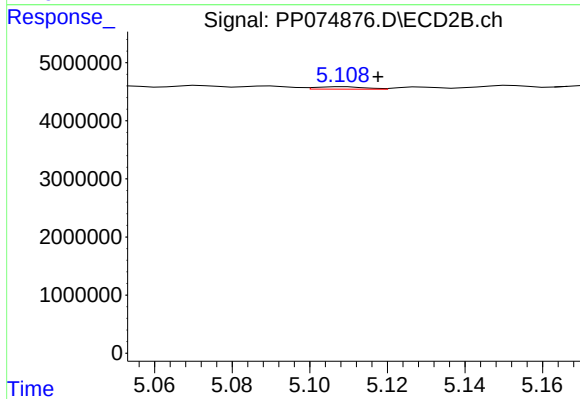

#22 AR-1248-2


R.T.: 5.109 min
Delta R.T.: -0.009 min
Response: 365813
Conc: 2.07 ng/ml

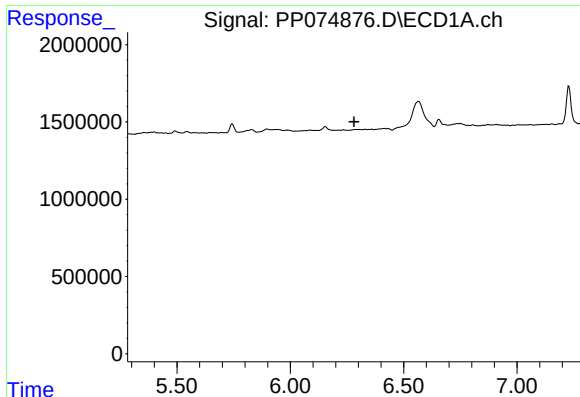

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

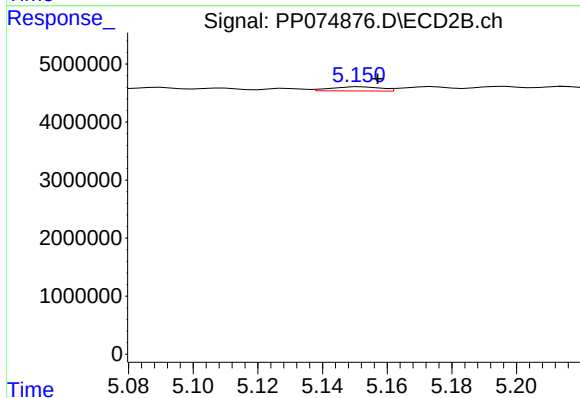


#23 AR-1248-3

R.T.: 5.152 min
Delta R.T.: -0.005 min
Response: 767420
Conc: 3.38 ng/ml

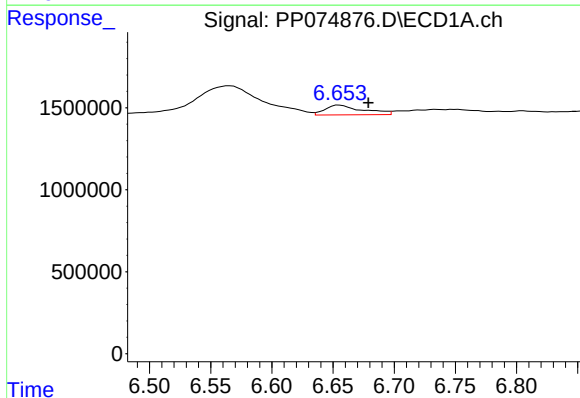


#24 AR-1248-4

R.T.: 6.655 min
Delta R.T.: -0.024 min
Response: 1282857
Conc: 23.32 ng/ml

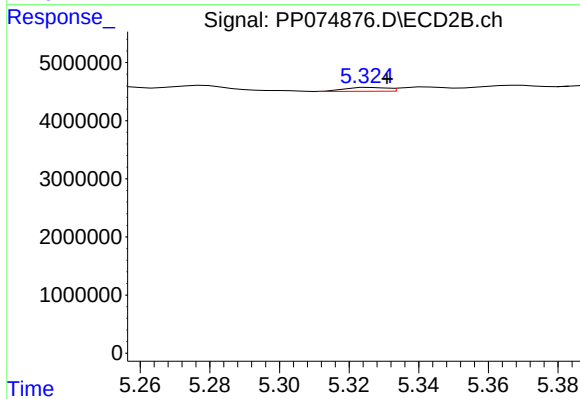

#24 AR-1248-4


R.T.: 5.326 min
Delta R.T.: -0.005 min
Response: 552294
Conc: 2.53 ng/ml

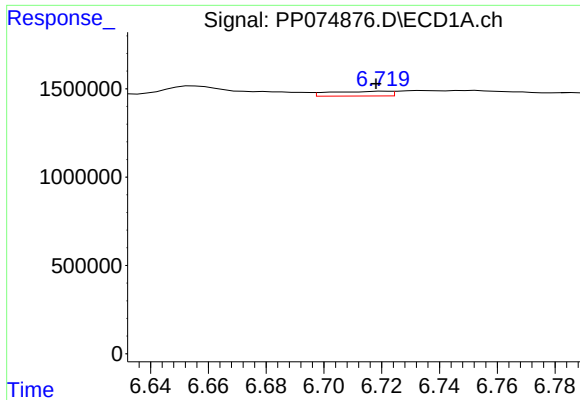

#25 AR-1248-5


R.T.: 6.721 min
Delta R.T.: 0.003 min
Response: 385318
Conc: 6.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

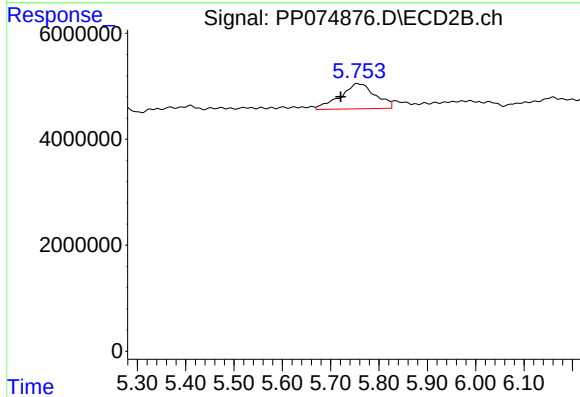


#25 AR-1248-5

R.T.: 5.755 min
Delta R.T.: 0.034 min
Response: 23992133
Conc: 65.32 ng/ml

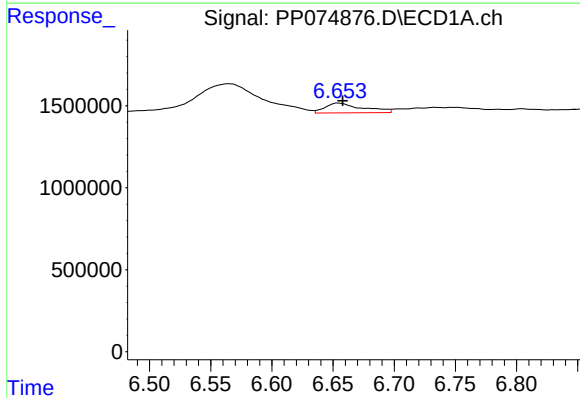


#26 AR-1254-1

R.T.: 6.655 min
Delta R.T.: -0.003 min
Response: 1282857
Conc: 22.02 ng/ml

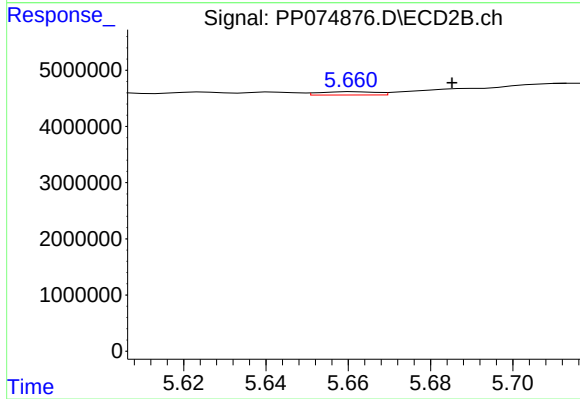

#26 AR-1254-1


R.T.: 5.662 min
Delta R.T.: -0.024 min
Response: 581277
Conc: 1.22 ng/ml

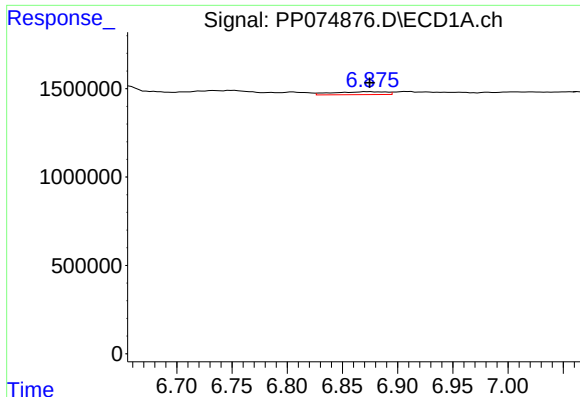

#27 AR-1254-2


R.T.: 6.871 min
Delta R.T.: -0.004 min
Response: 552988
Conc: 6.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

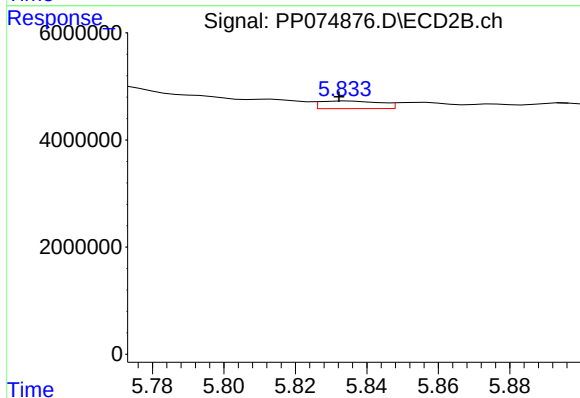


#27 AR-1254-2

R.T.: 5.834 min
Delta R.T.: 0.002 min
Response: 1670366
Conc: 4.74 ng/ml

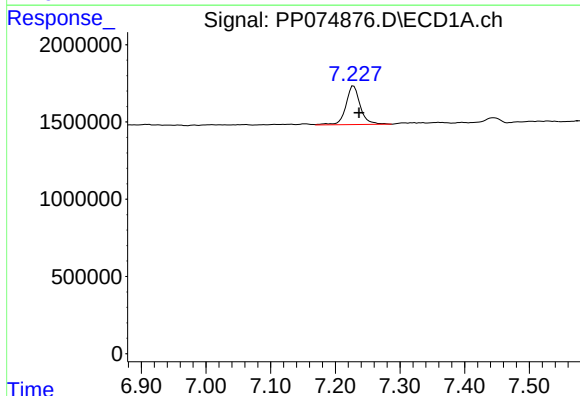


#28 AR-1254-3

R.T.: 7.228 min
Delta R.T.: -0.008 min
Response: 3850748
Conc: 43.17 ng/ml

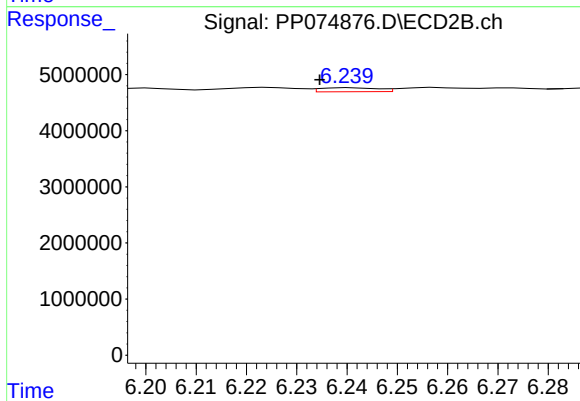

#28 AR-1254-3


R.T.: 6.241 min
Delta R.T.: 0.006 min
Response: 558352
Conc: 0.90 ng/ml

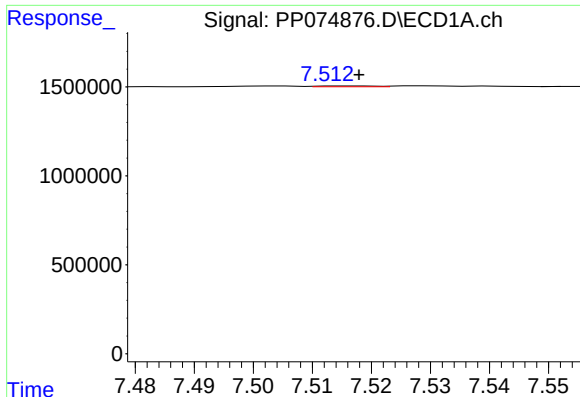

#29 AR-1254-4


R.T.: 7.516 min
Delta R.T.: -0.002 min
Response: 27688
Conc: 0.42 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

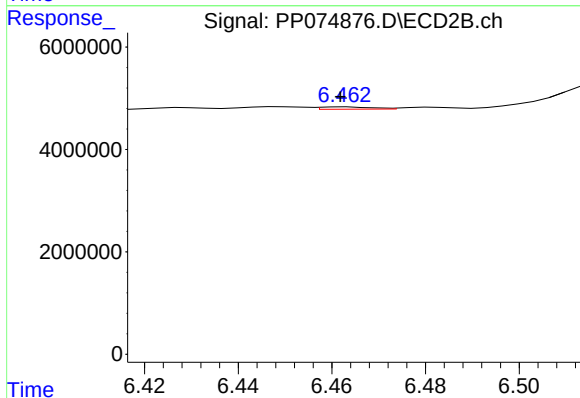


#29 AR-1254-4

R.T.: 6.463 min
Delta R.T.: 0.001 min
Response: 348837
Conc: 0.74 ng/ml

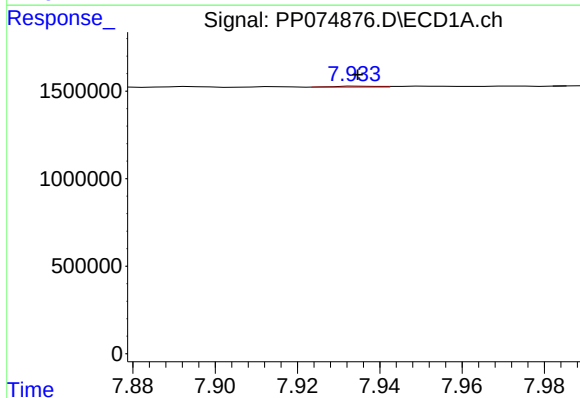


#30 AR-1254-5

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 34612
Conc: 0.42 ng/ml

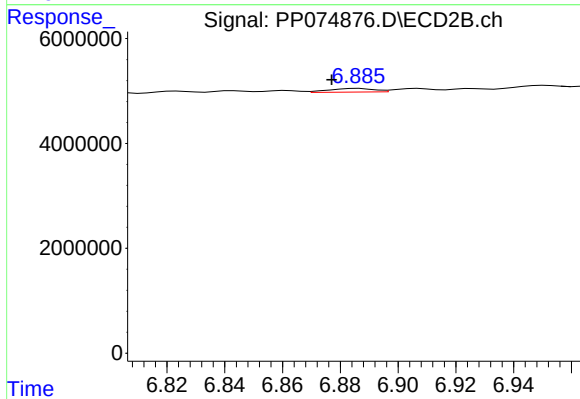

#30 AR-1254-5


R.T.: 6.886 min
Delta R.T.: 0.009 min
Response: 746729
Conc: 1.52 ng/ml

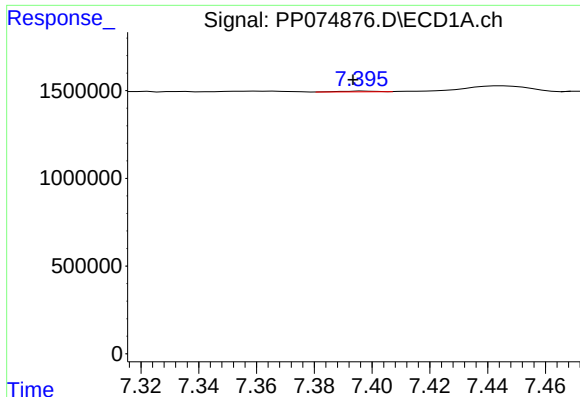

#31 AR-1260-1


R.T.: 7.397 min
Delta R.T.: 0.003 min
Response: 33894
Conc: 0.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

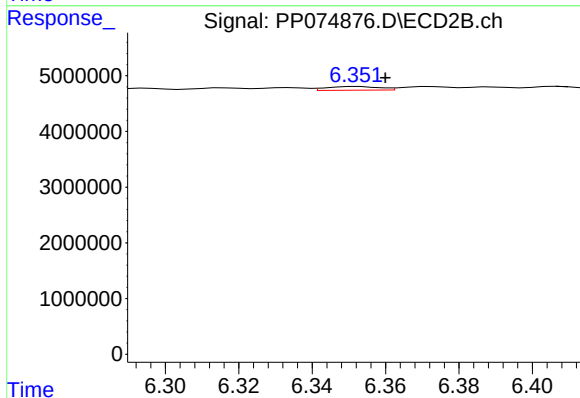


#31 AR-1260-1

R.T.: 6.353 min
Delta R.T.: -0.008 min
Response: 666330
Conc: 1.78 ng/ml

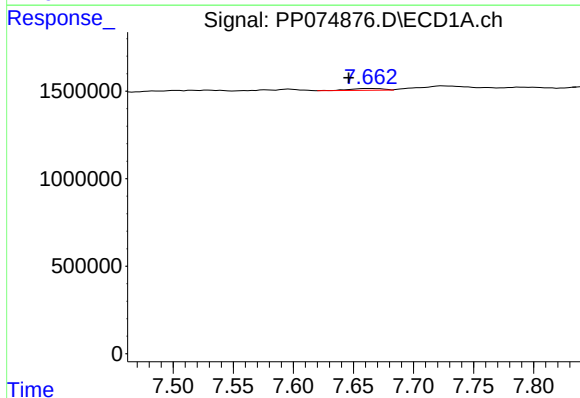


#32 AR-1260-2

R.T.: 7.664 min
Delta R.T.: 0.018 min
Response: 185243
Conc: 2.69 ng/ml

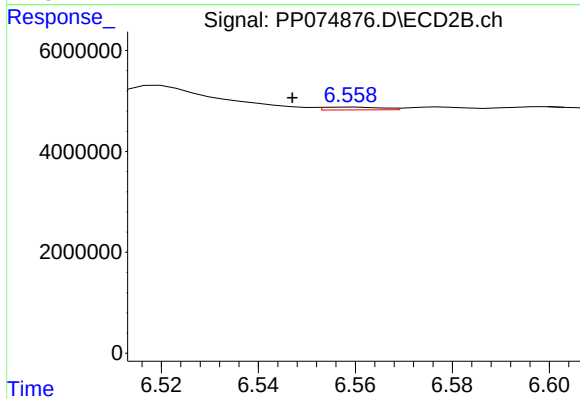

#32 AR-1260-2


R.T.: 6.559 min
Delta R.T.: 0.012 min
Response: 456010
Conc: 0.86 ng/ml

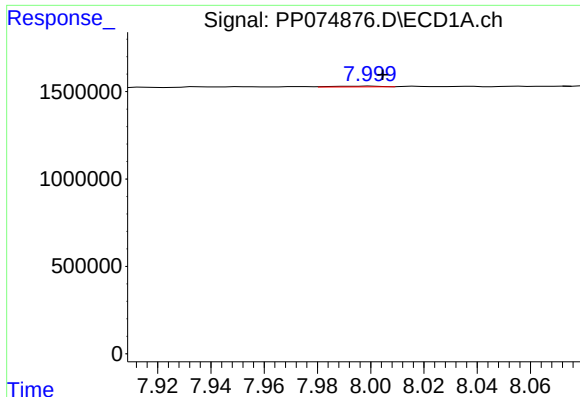

#33 AR-1260-3


R.T.: 8.000 min
Delta R.T.: -0.004 min
Response: 49158
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

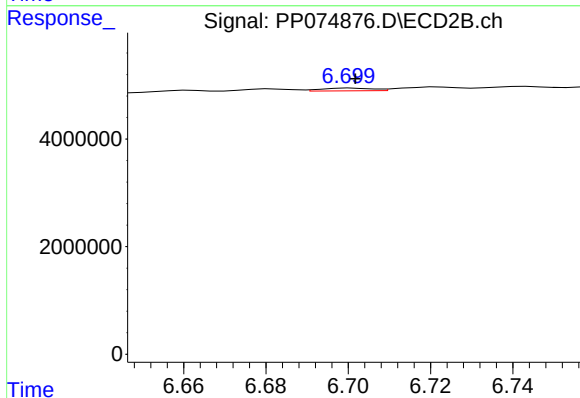


#33 AR-1260-3

R.T.: 6.701 min
Delta R.T.: -0.001 min
Response: 450156
Conc: 1.04 ng/ml

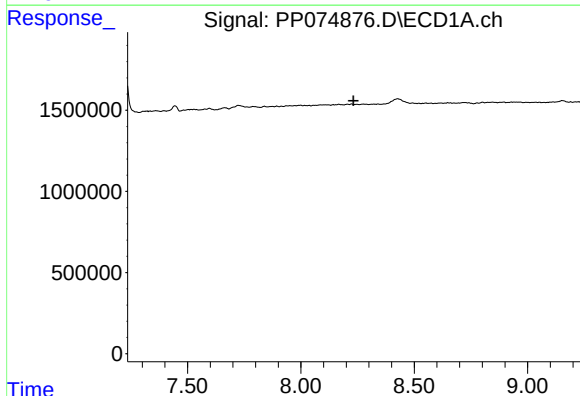


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.232 min
Response: 0
Conc: N.D.

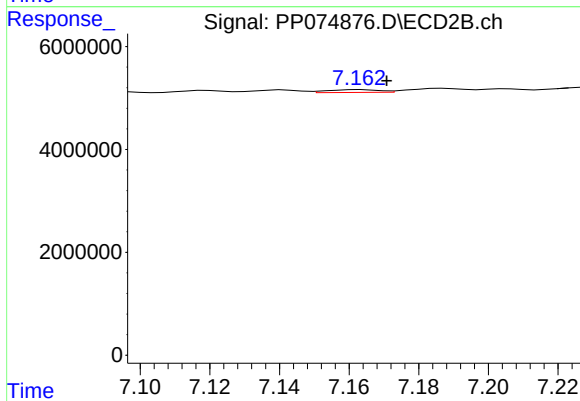

#34 AR-1260-4


R.T.: 7.163 min
Delta R.T.: -0.007 min
Response: 574405
Conc: 1.51 ng/ml

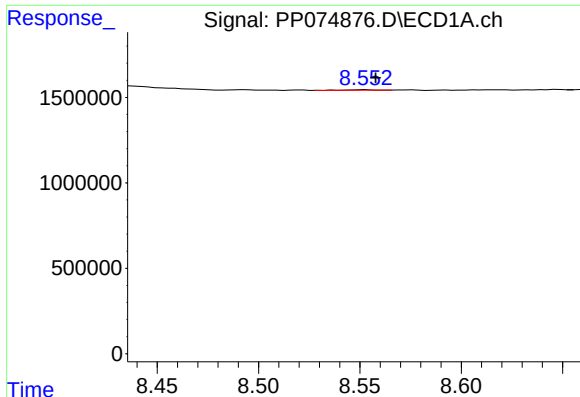

#35 AR-1260-5


R.T.: 8.553 min
Delta R.T.: -0.005 min
Response: 30830
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

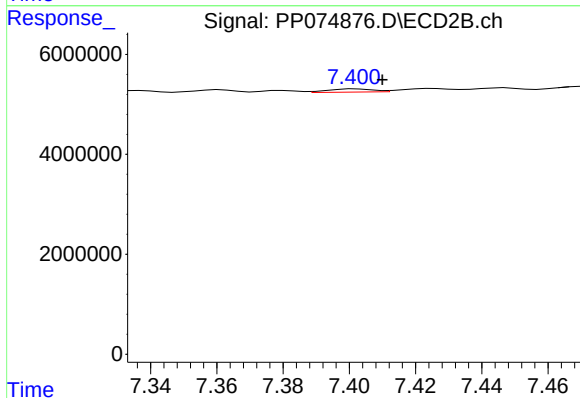


#35 AR-1260-5

R.T.: 7.402 min
Delta R.T.: -0.008 min
Response: 632243
Conc: 0.63 ng/ml

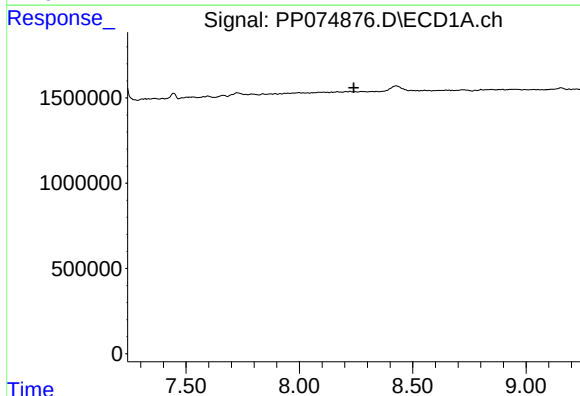


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.241 min
Response: 0
Conc: N.D.

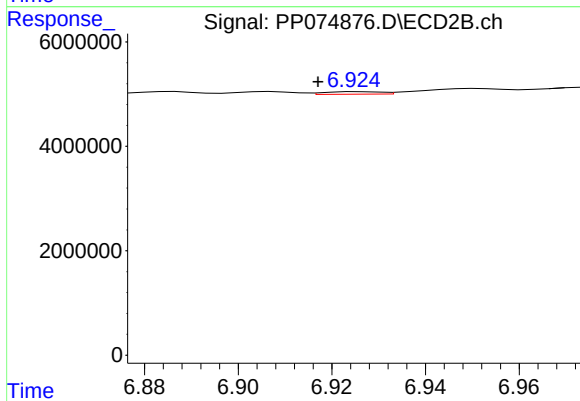

#36 AR-1262-1


R.T.: 6.926 min
Delta R.T.: 0.009 min
Response: 405630
Conc: 0.57 ng/ml

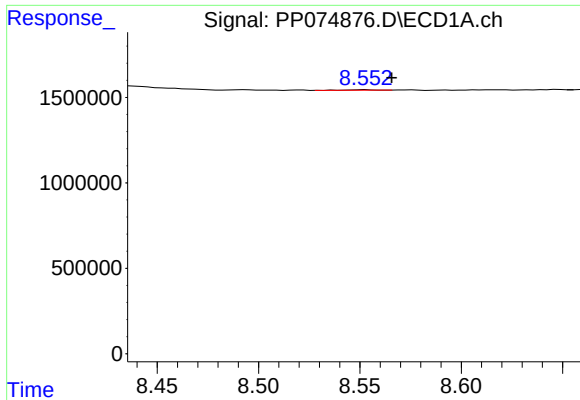

#37 AR-1262-2


R.T.: 8.553 min
Delta R.T.: -0.013 min
Response: 30830
Conc: 0.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

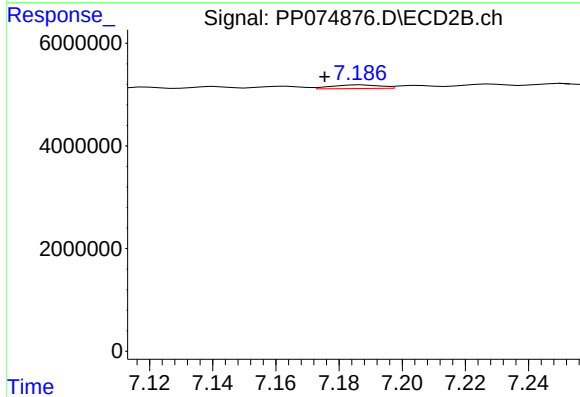


#37 AR-1262-2

R.T.: 7.187 min
Delta R.T.: 0.012 min
Response: 757281
Conc: 1.45 ng/ml

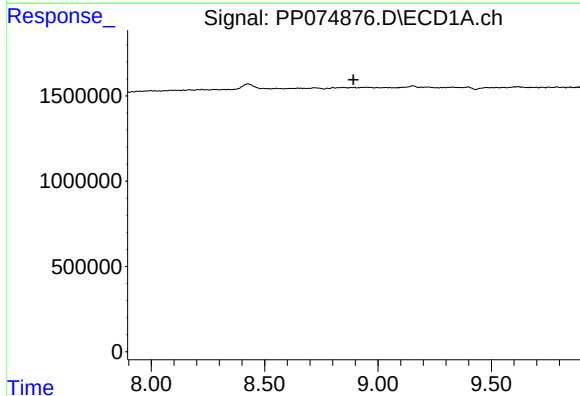


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

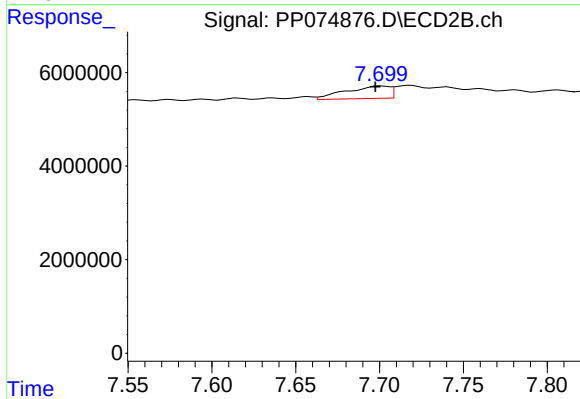

#38 AR-1262-3


R.T.: 7.701 min
Delta R.T.: 0.003 min
Response: 4832702
Conc: 10.36 ng/ml

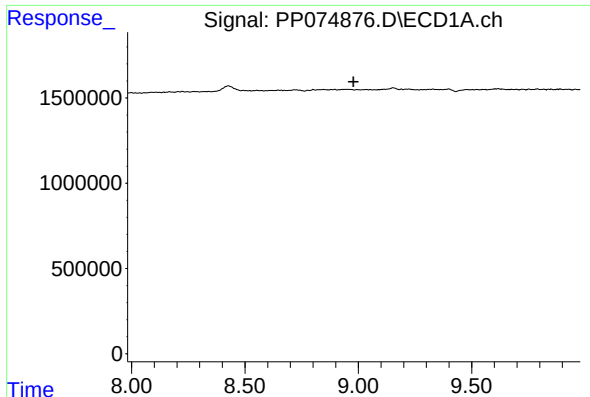

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

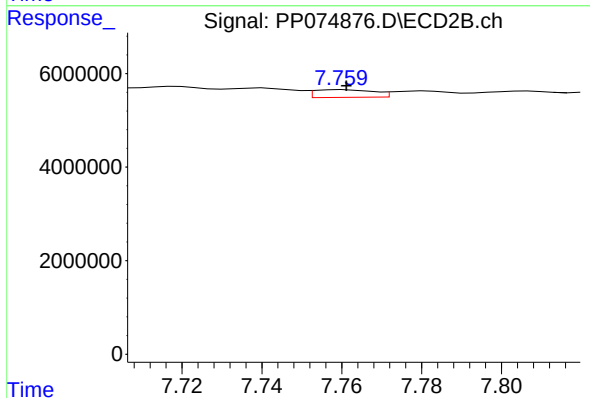


#39 AR-1262-4

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 1708404
Conc: 2.08 ng/ml

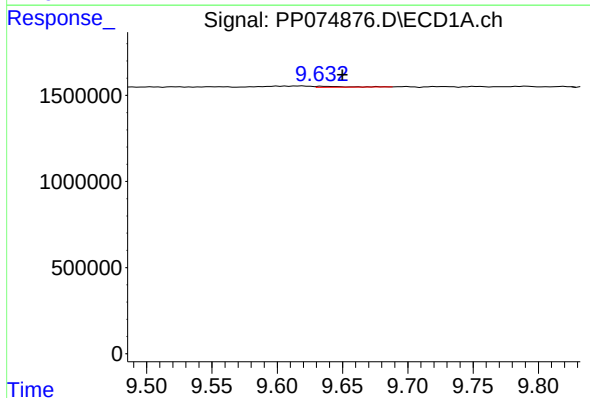


#40 AR-1262-5

R.T.: 9.634 min
Delta R.T.: -0.015 min
Response: 88386
Conc: 1.45 ng/ml

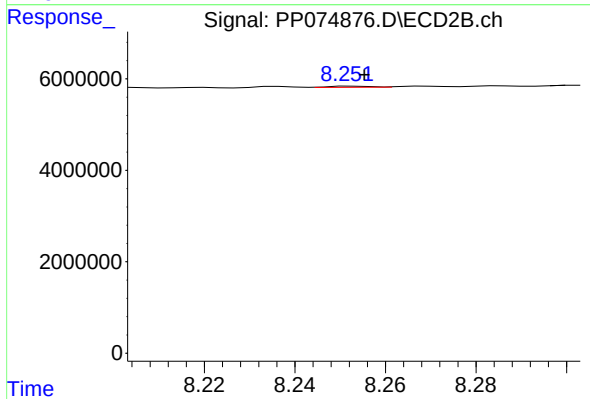

#40 AR-1262-5


R.T.: 8.253 min
Delta R.T.: -0.002 min
Response: 163138
Conc: 0.46 ng/ml

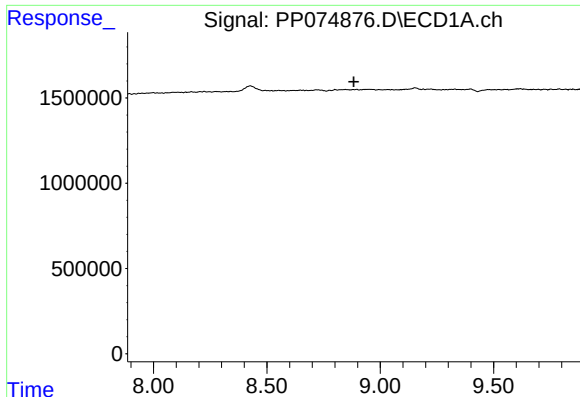

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

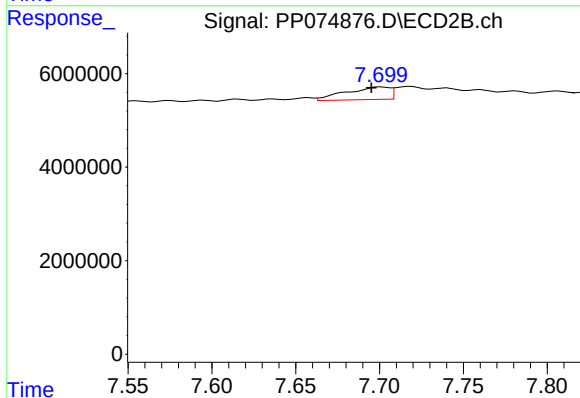


#41 AR-1268-1

R.T.: 7.701 min
Delta R.T.: 0.006 min
Response: 4832702
Conc: 3.43 ng/ml

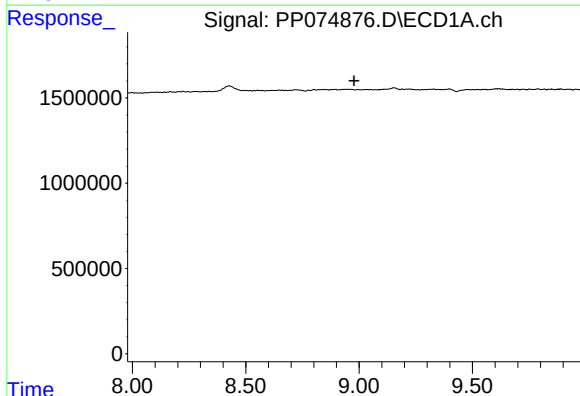


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

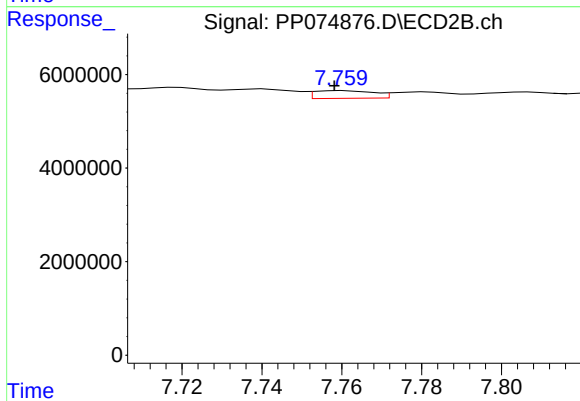

#42 AR-1268-2


R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 1708404
Conc: 1.25 ng/ml

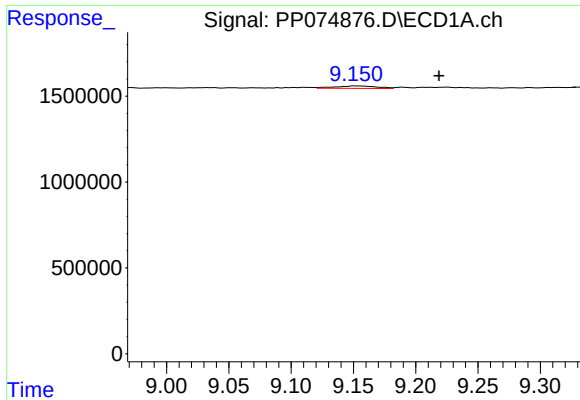

#43 AR-1268-3


R.T.: 9.152 min
Delta R.T.: -0.067 min
Response: 316888
Conc: 2.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

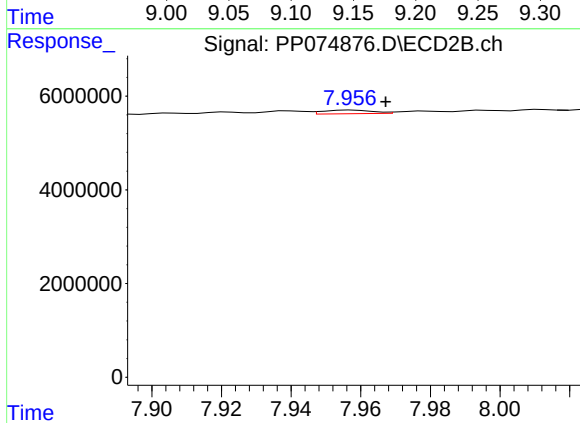


#43 AR-1268-3

R.T.: 7.957 min
Delta R.T.: -0.010 min
Response: 772692
Conc: 0.74 ng/ml

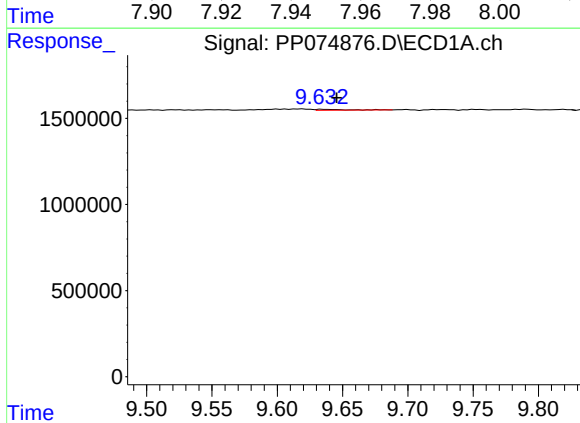


#44 AR-1268-4

R.T.: 9.634 min
Delta R.T.: -0.011 min
Response: 88386
Conc: 1.31 ng/ml

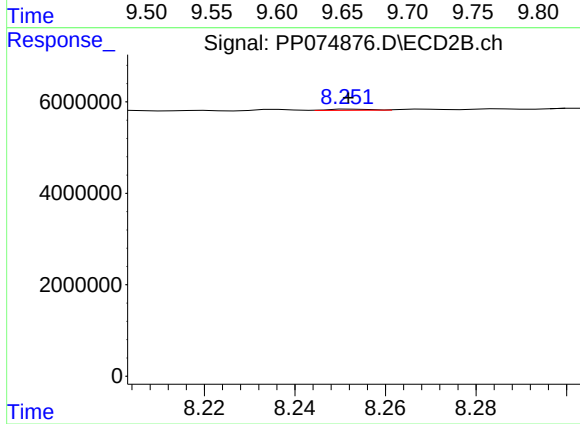

#44 AR-1268-4


R.T.: 8.253 min
Delta R.T.: 0.001 min
Response: 163138
Conc: 0.43 ng/ml

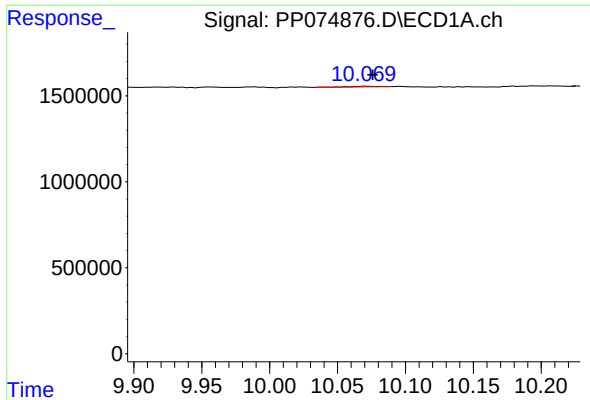

#45 AR-1268-5

R.T.: 10.071 min
Delta R.T.: -0.005 min
Response: 50958
Conc: 0.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

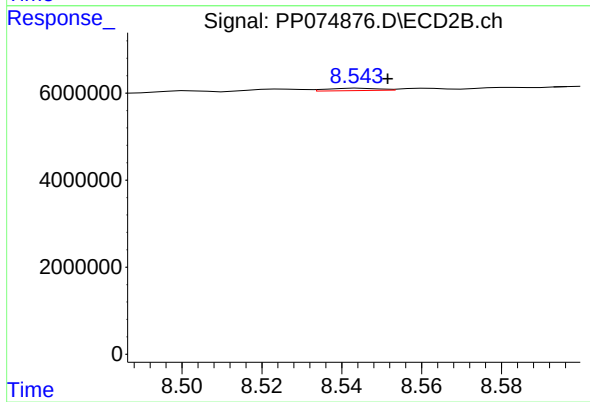

#45 AR-1268-5

R.T.: 8.545 min
Delta R.T.: -0.007 min
Response: 489735
Conc: 0.16 ng/ml