

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 20:32
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1232 WATER LOD 40PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:08:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.659	3.801	26618235	95226893	21.752	19.694
2)	SA Decachlor...	10.438	8.810	20421885	130.2E6	20.680	17.362
Target Compounds							
3)	L1 AR-1016-1	5.811	4.897	1107680	8379866	25.124	16.452 #
4)	L1 AR-1016-2	5.832	4.960	1601908	5155273	25.491	21.659
5)	L1 AR-1016-3	5.896	5.073	1465343	4960558	32.626	35.971
6)	L1 AR-1016-4	5.992	5.111	1186078	1663118	33.713	11.896 #
7)	L1 AR-1016-5	6.285	5.350	2150749	6695128	64.809	40.312 #
8)	L2 AR-1221-1	4.859	4.005	697266	1601698	39.634	25.889 #
9)	L2 AR-1221-2	4.961	4.090	979021	2894292	73.295	64.016
10)	L2 AR-1221-3	5.020	4.170	1303355	3678414	34.378	22.389 #
11)	L3 AR-1232-1	5.020	4.170	1303355	3678414	42.910	28.716 #
12)	L3 AR-1232-2	5.547	4.897	727538	8379866	46.169	36.152
13)	L3 AR-1232-3	5.832	5.073	1601908	4960558	52.446	82.594 #
14)	L3 AR-1232-4	5.992	5.156	1186078	3439602	68.681	46.666 #
15)	L3 AR-1232-5	6.083	5.350	984084	6695128	75.810	107.840 #
16)	L4 AR-1242-1	5.811	4.897	1107680	8379866	28.940	19.869 #
17)	L4 AR-1242-2	5.832	4.960	1601908	5155273	28.361	25.740
18)	L4 AR-1242-3	5.896	5.073	1465343	4960558	36.090	41.933
19)	L4 AR-1242-4	5.992	5.156	1186078	3439602	37.366	20.096 #
20)	L4 AR-1242-5	6.721	5.708	2159131	15987924	59.858	86.345 #
21)	L5 AR-1248-1	5.811	4.897	1107680	8379866	36.649	30.346
22)	L5 AR-1248-2	6.083	5.111	984084	1663118	22.835	9.409 #
23)	L5 AR-1248-3	6.285	5.156	2150749	3439602	46.051	15.139 #
24)	L5 AR-1248-4	6.680	5.350	1199727	6695128	21.813	30.709 #
25)	L5 AR-1248-5	6.721	5.708	2159131	15987924	38.924	43.526
26)	L6 AR-1254-1	6.657	5.708	2637962	15987924	45.272	33.538 #
27)	L6 AR-1254-2	6.878	5.825	1916404	4107446	23.481	11.664 #
28)	L6 AR-1254-3	7.229	6.234	11947338	2721568	133.929	4.391 #
29)	L6 AR-1254-4	7.519	6.467	197425	2158838	2.995	4.607 #
30)	L6 AR-1254-5	7.938	6.868	413500	1161321	4.977	2.368 #
31)	L7 AR-1260-1	7.397	6.369	100944	1965632	1.746	5.239 #
32)	L7 AR-1260-2	7.653	6.521	198231	30640825	2.876	57.942 #
33)	L7 AR-1260-3	8.010	6.704	304428	1435290	5.867	3.315 #
34)	L7 AR-1260-4	0.000	7.164	0	830323	N.D.	2.177 #
35)	L7 AR-1260-5	0.000	7.416	0	365762	N.D.	0.364 #
36)	L8 AR-1262-1	0.000	6.909	0	1061006	N.D.	1.500 #
37)	L8 AR-1262-2	0.000	7.184	0	685513	N.D.	1.316 #
38)	L8 AR-1262-3	0.000	7.709	0	67456738	N.D.	144.665 #
39)	L8 AR-1262-4	0.000	7.709f	0	67456738	N.D.	82.078 #
40)	L8 AR-1262-5	9.622	8.246	108045	184648	1.773	0.515 #
41)	L9 AR-1268-1	0.000	7.709	0	67456738	N.D.	47.825 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074877.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 20:32
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1232 WATER LOD 40PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:08:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.709f	0	67456738	N.D.	49.476 #
43) L9	AR-1268-3	9.153f	7.962	835531	503375	6.761	0.483 #
44) L9	AR-1268-4	9.622	8.246	108045	184648	1.606	0.482 #
45) L9	AR-1268-5	10.081	8.546	60698	561113	0.164	0.179



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074877.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 20:32
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1232 WATER LOD 40PPB
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:08:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

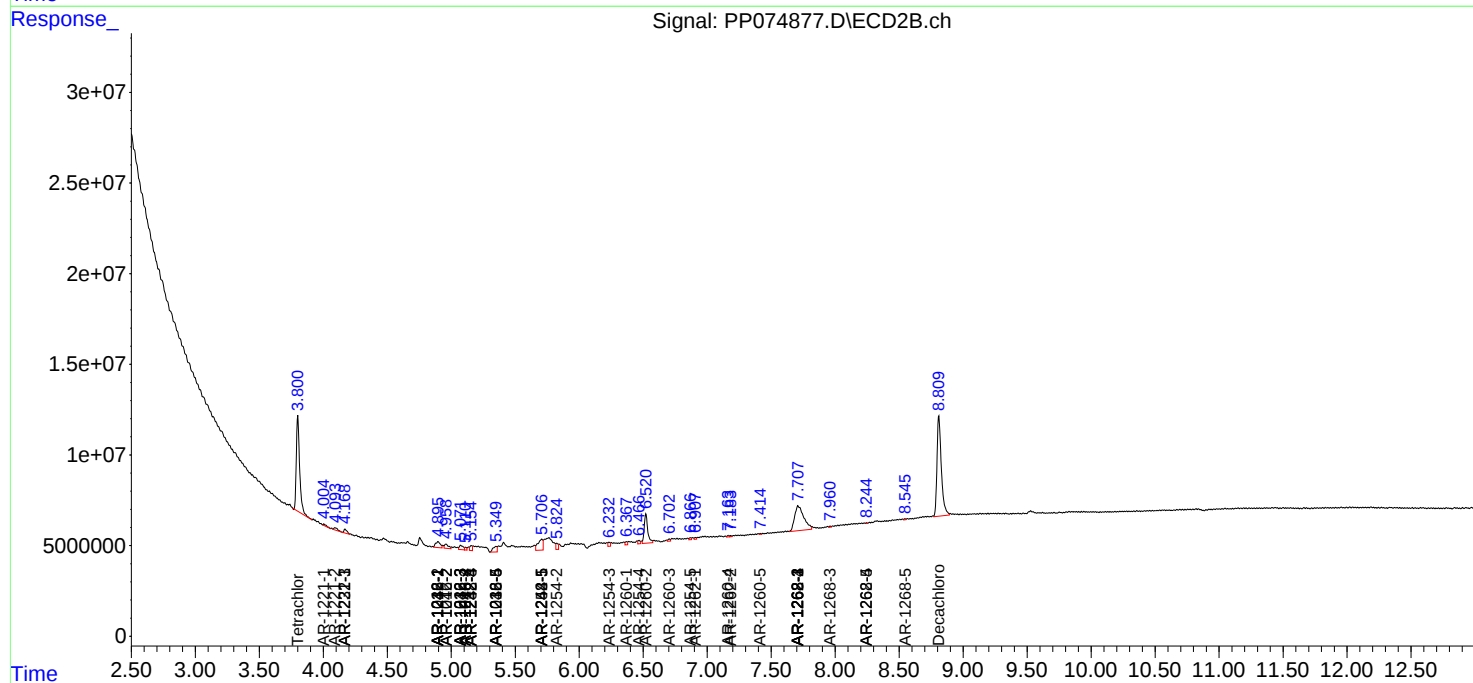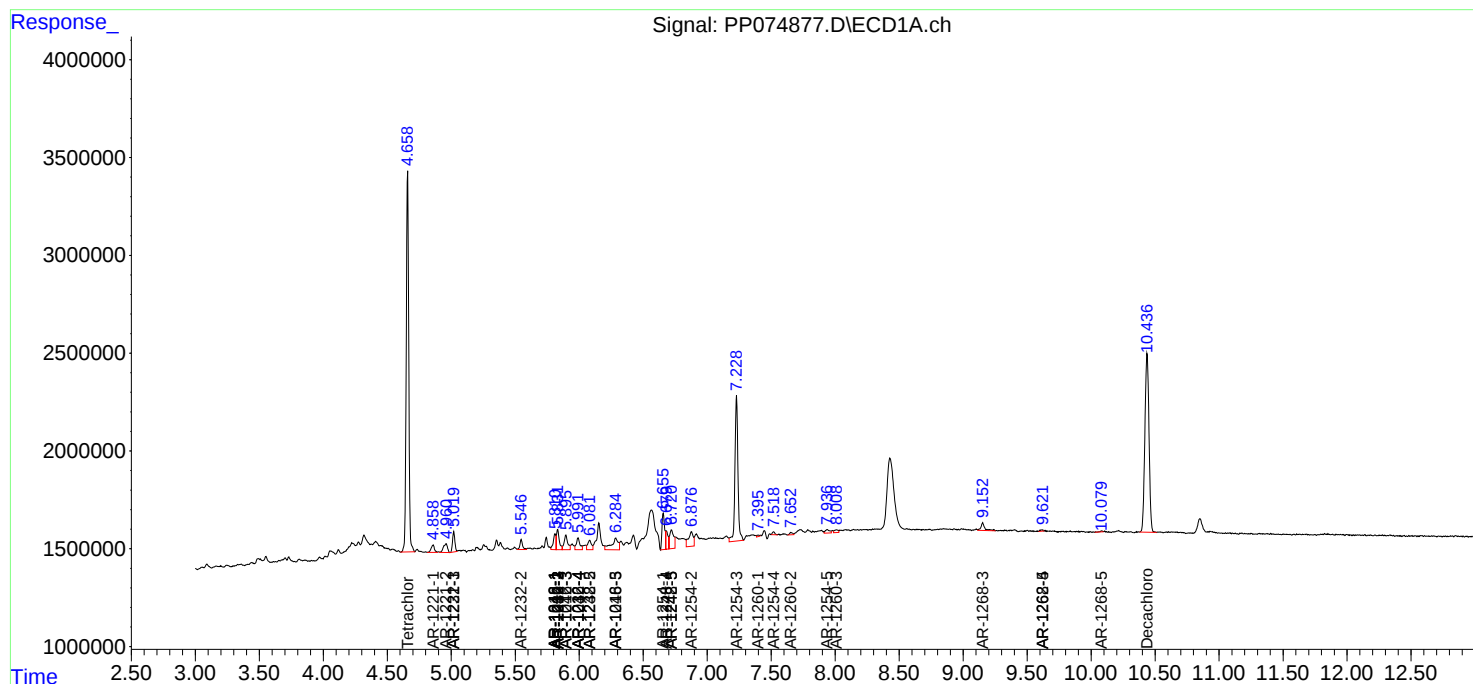


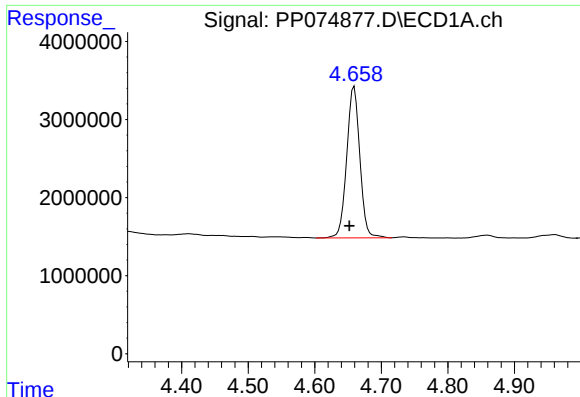

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.007 min
Response: 26618235
Conc: 21.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

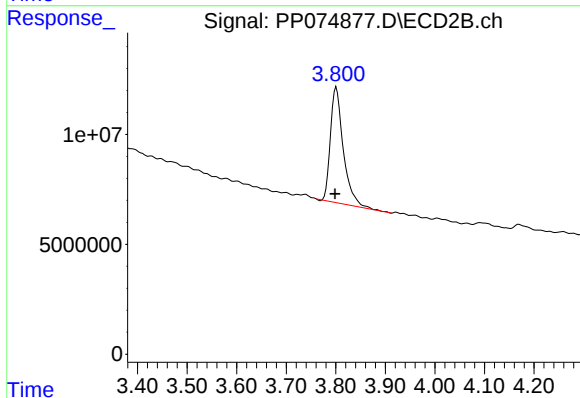


#1 Tetrachloro-m-xylene

R.T.: 3.801 min
Delta R.T.: 0.002 min
Response: 95226893
Conc: 19.69 ng/ml

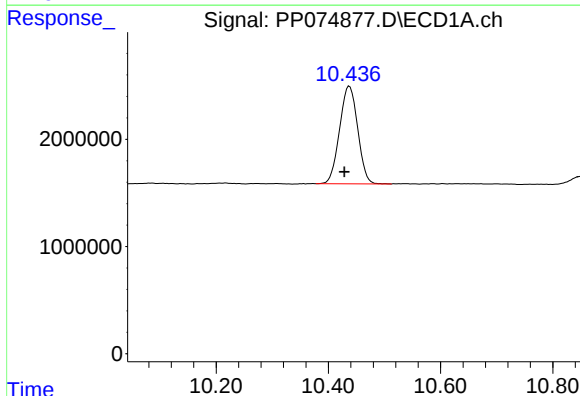


#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.009 min
Response: 20421885
Conc: 20.68 ng/ml

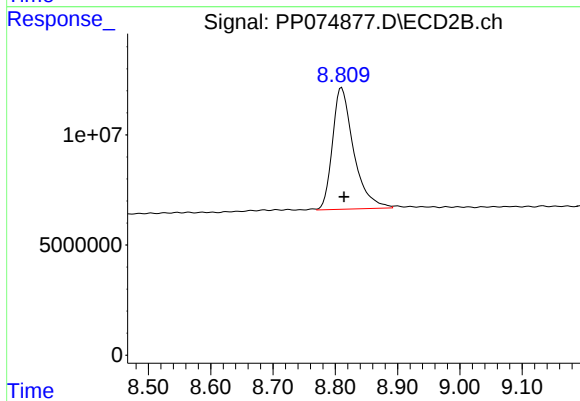

#2 Decachlorobiphenyl


R.T.: 8.810 min
Delta R.T.: -0.004 min
Response: 130203947
Conc: 17.36 ng/ml

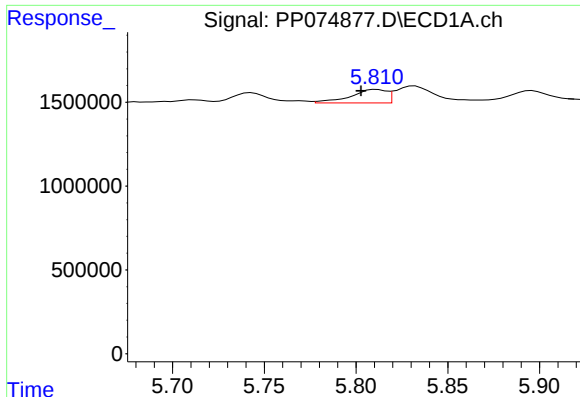

#3 AR-1016-1


R.T.: 5.811 min
Delta R.T.: 0.009 min
Response: 1107680
Conc: 25.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

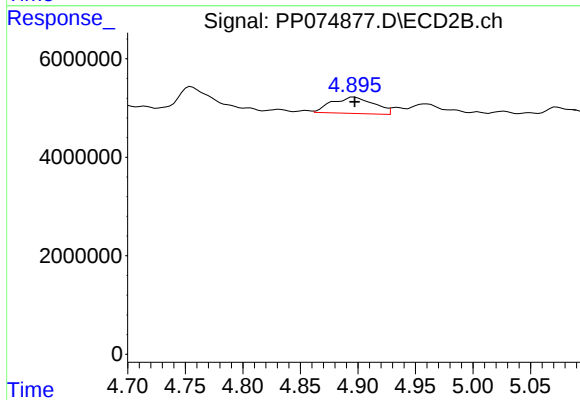


#3 AR-1016-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 8379866
Conc: 16.45 ng/ml

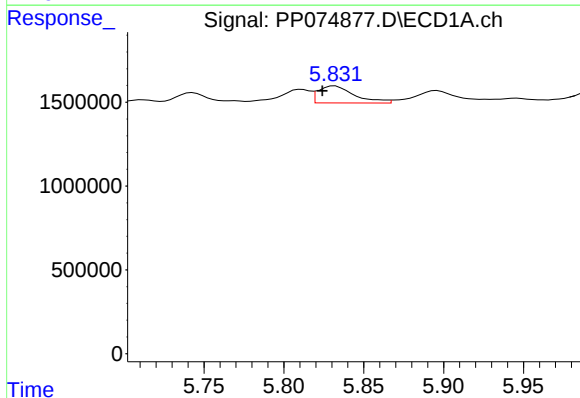


#4 AR-1016-2

R.T.: 5.832 min
Delta R.T.: 0.008 min
Response: 1601908
Conc: 25.49 ng/ml

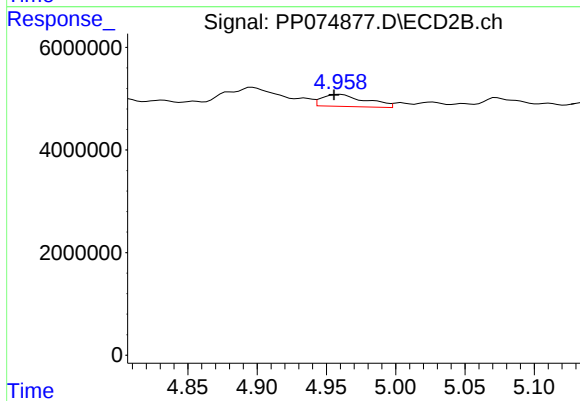

#4 AR-1016-2


R.T.: 4.960 min
Delta R.T.: 0.004 min
Response: 5155273
Conc: 21.66 ng/ml

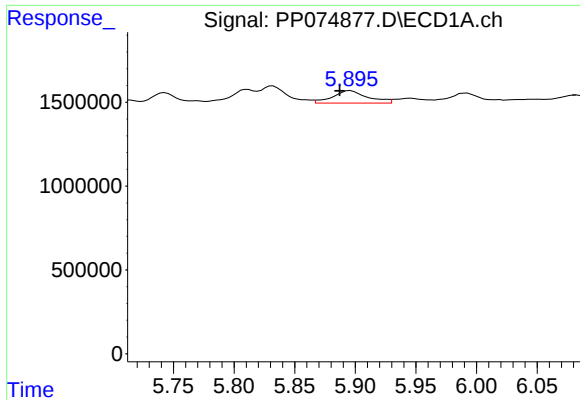

#5 AR-1016-3


R.T.: 5.896 min
Delta R.T.: 0.009 min
Response: 1465343
Conc: 32.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

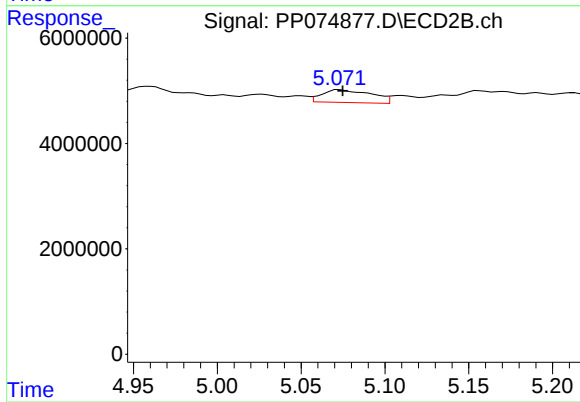


#5 AR-1016-3

R.T.: 5.073 min
Delta R.T.: -0.002 min
Response: 4960558
Conc: 35.97 ng/ml

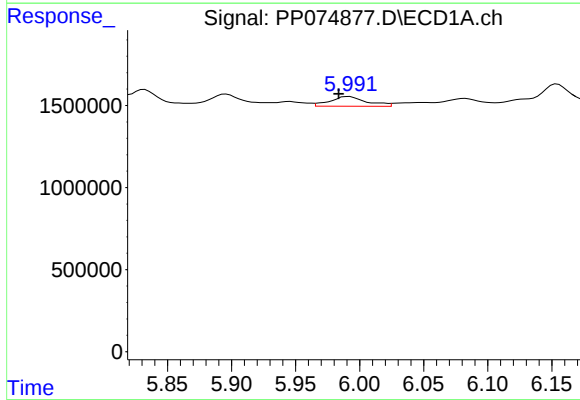


#6 AR-1016-4

R.T.: 5.992 min
Delta R.T.: 0.008 min
Response: 1186078
Conc: 33.71 ng/ml

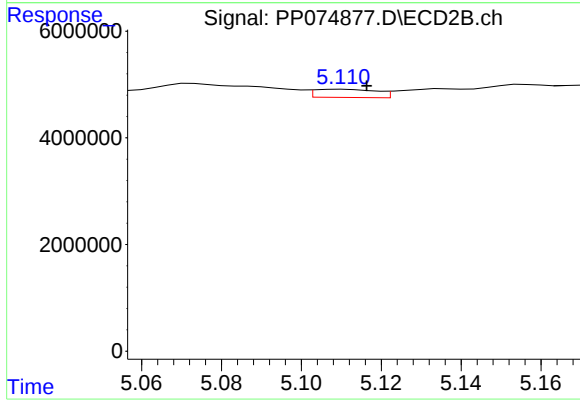

#6 AR-1016-4


R.T.: 5.111 min
Delta R.T.: -0.006 min
Response: 1663118
Conc: 11.90 ng/ml

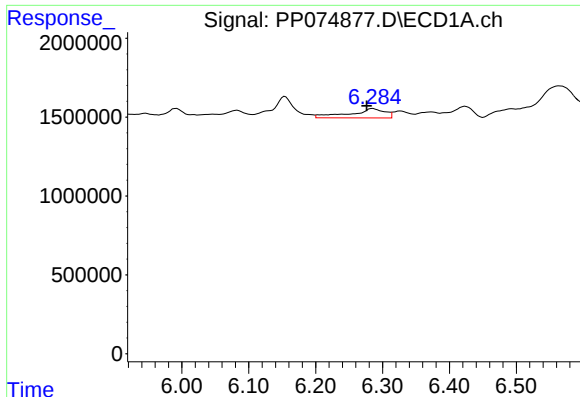

#7 AR-1016-5


R.T.: 6.285 min
Delta R.T.: 0.009 min
Response: 2150749
Conc: 64.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

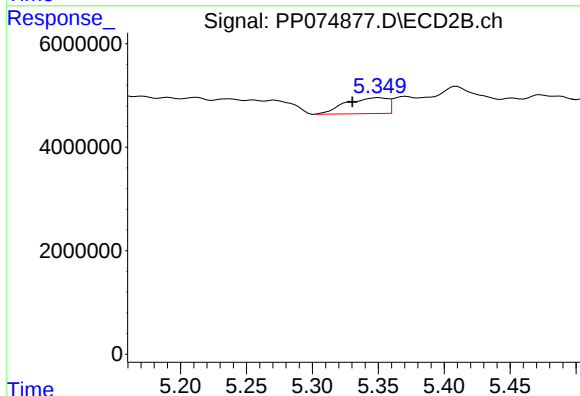


#7 AR-1016-5

R.T.: 5.350 min
Delta R.T.: 0.020 min
Response: 6695128
Conc: 40.31 ng/ml

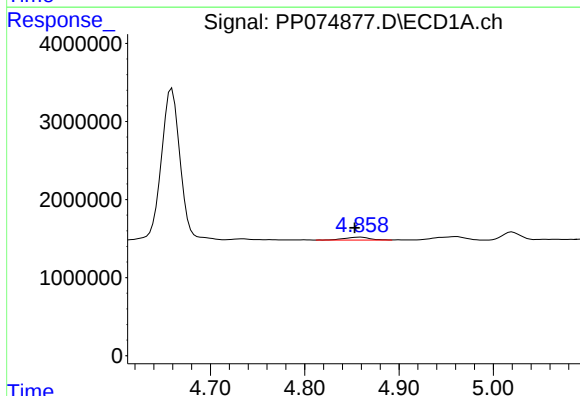


#8 AR-1221-1

R.T.: 4.859 min
Delta R.T.: 0.007 min
Response: 697266
Conc: 39.63 ng/ml

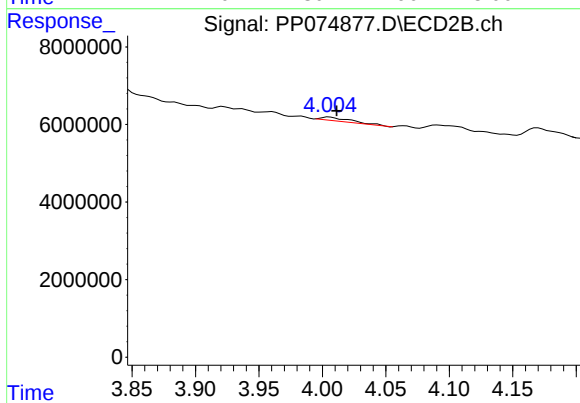

#8 AR-1221-1


R.T.: 4.005 min
Delta R.T.: -0.006 min
Response: 1601698
Conc: 25.89 ng/ml

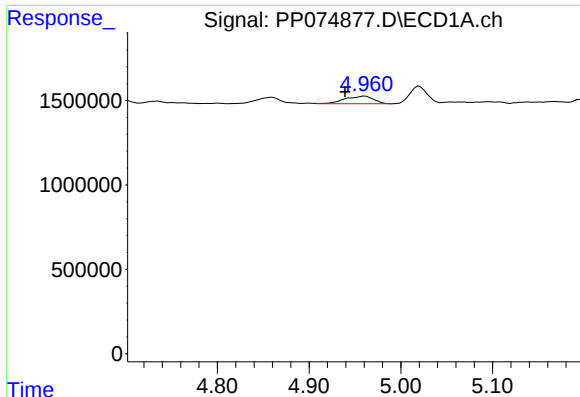

#9 AR-1221-2


R.T.: 4.961 min
Delta R.T.: 0.022 min
Response: 979021
Conc: 73.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

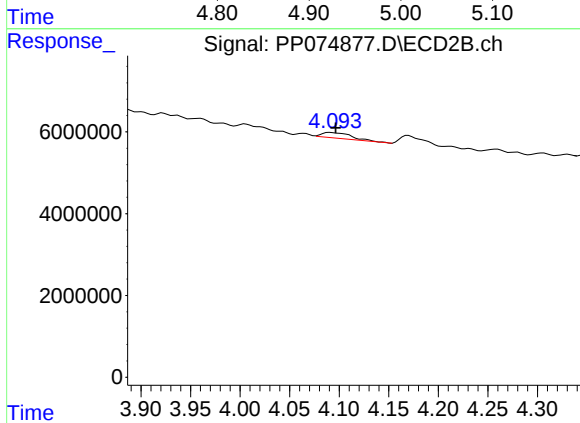


#9 AR-1221-2

R.T.: 4.090 min
Delta R.T.: -0.006 min
Response: 2894292
Conc: 64.02 ng/ml

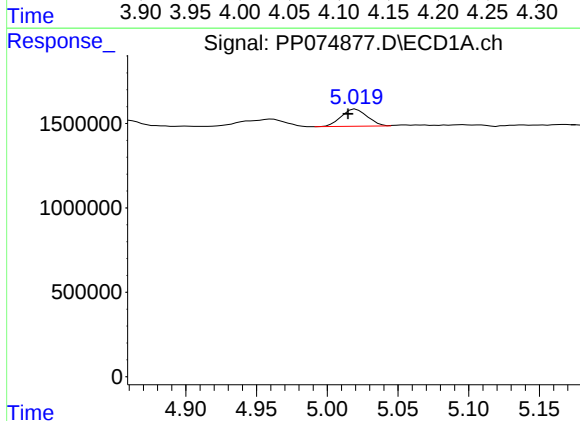


#10 AR-1221-3

R.T.: 5.020 min
Delta R.T.: 0.005 min
Response: 1303355
Conc: 34.38 ng/ml

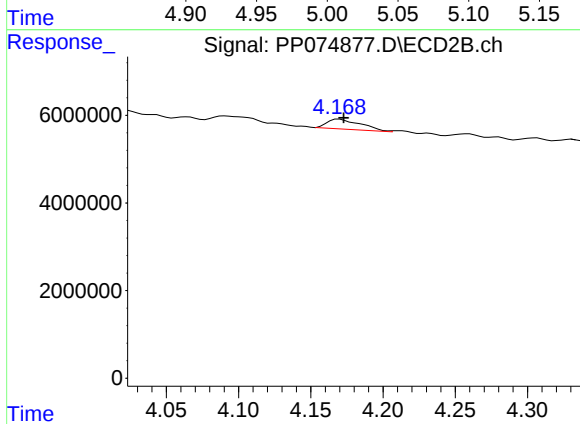

#10 AR-1221-3


R.T.: 4.170 min
Delta R.T.: -0.003 min
Response: 3678414
Conc: 22.39 ng/ml

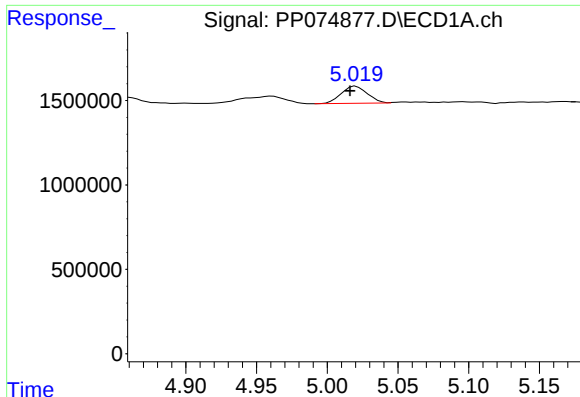

#11 AR-1232-1


R.T.: 5.020 min
Delta R.T.: 0.004 min
Response: 1303355
Conc: 42.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

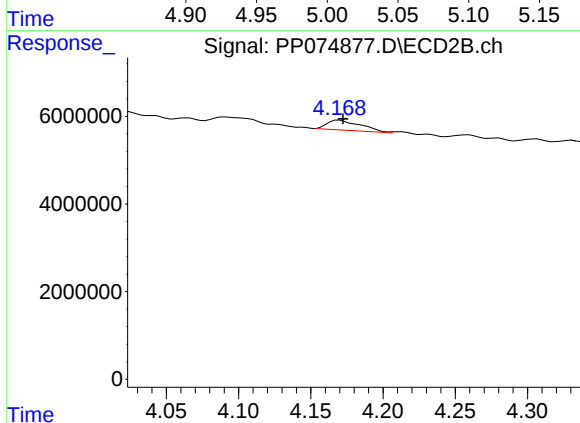


#11 AR-1232-1

R.T.: 4.170 min
Delta R.T.: -0.003 min
Response: 3678414
Conc: 28.72 ng/ml

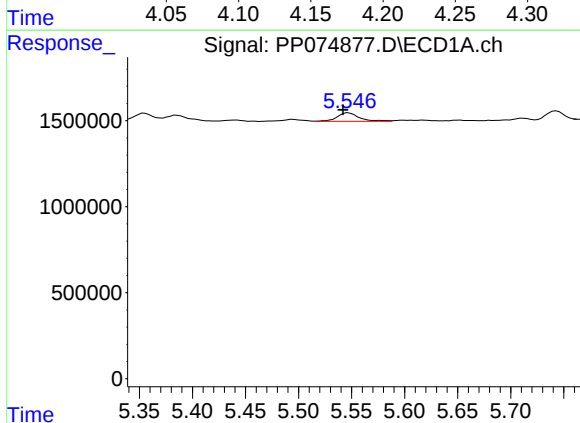


#12 AR-1232-2

R.T.: 5.547 min
Delta R.T.: 0.005 min
Response: 727538
Conc: 46.17 ng/ml

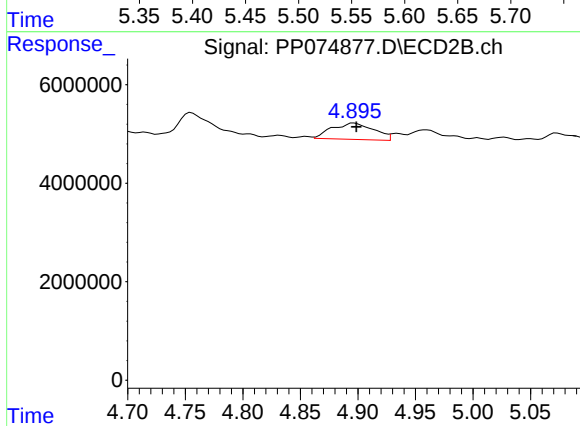

#12 AR-1232-2


R.T.: 4.897 min
Delta R.T.: -0.002 min
Response: 8379866
Conc: 36.15 ng/ml

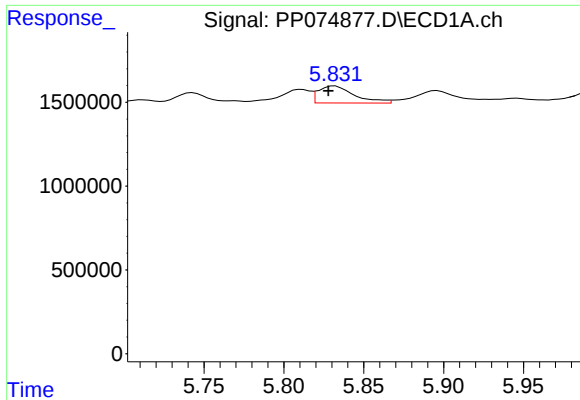

#13 AR-1232-3


R.T.: 5.832 min
Delta R.T.: 0.004 min
Response: 1601908
Conc: 52.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

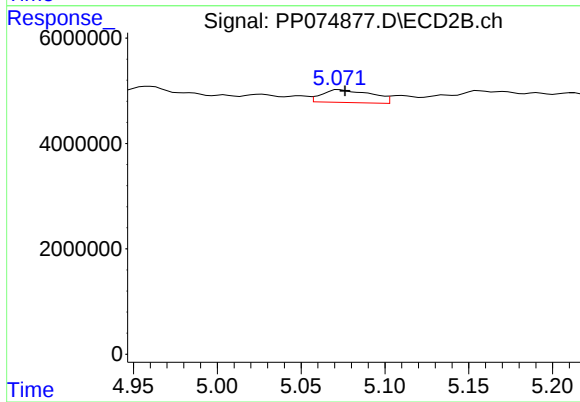


#13 AR-1232-3

R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 4960558
Conc: 82.59 ng/ml

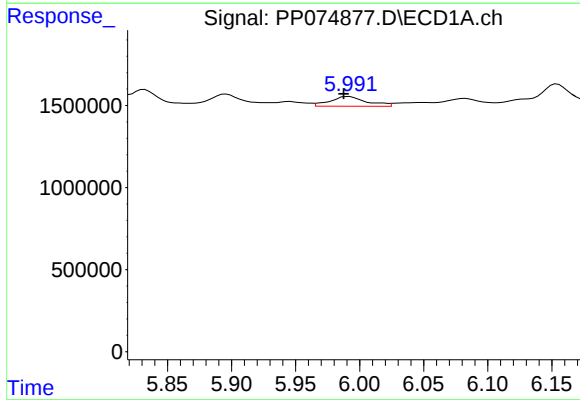


#14 AR-1232-4

R.T.: 5.992 min
Delta R.T.: 0.004 min
Response: 1186078
Conc: 68.68 ng/ml

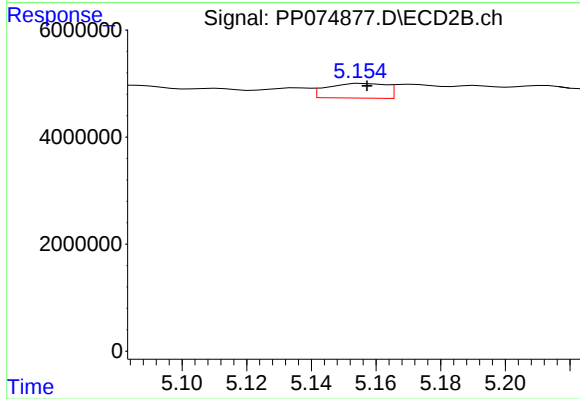

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: -0.001 min
Response: 3439602
Conc: 46.67 ng/ml

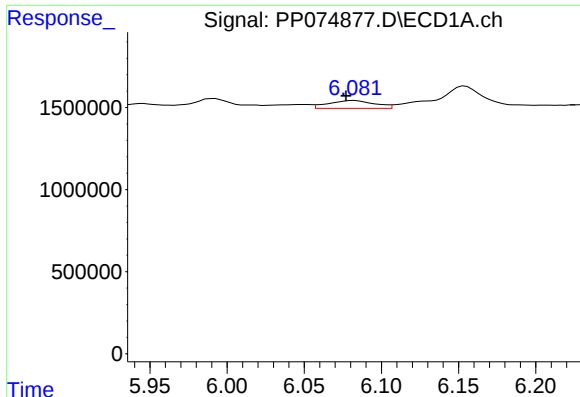

#15 AR-1232-5


R.T.: 6.083 min
Delta R.T.: 0.005 min
Response: 984084
Conc: 75.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

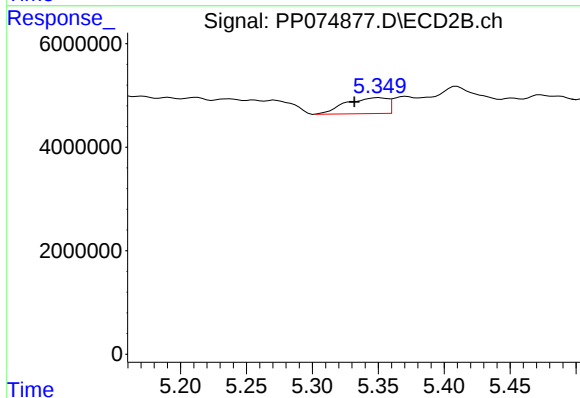


#15 AR-1232-5

R.T.: 5.350 min
Delta R.T.: 0.018 min
Response: 6695128
Conc: 107.84 ng/ml

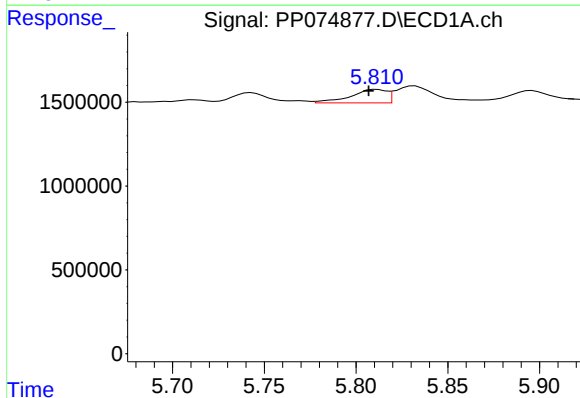


#16 AR-1242-1

R.T.: 5.811 min
Delta R.T.: 0.004 min
Response: 1107680
Conc: 28.94 ng/ml

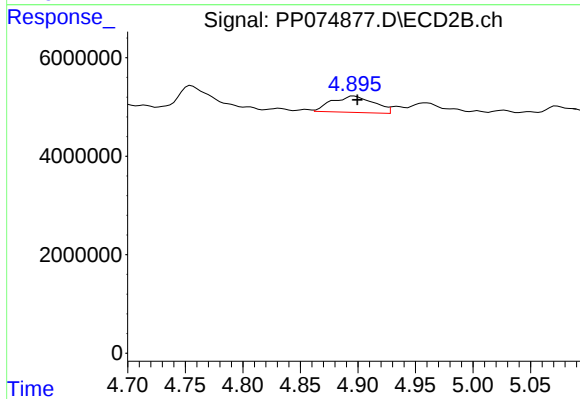

#16 AR-1242-1


R.T.: 4.897 min
Delta R.T.: -0.003 min
Response: 8379866
Conc: 19.87 ng/ml

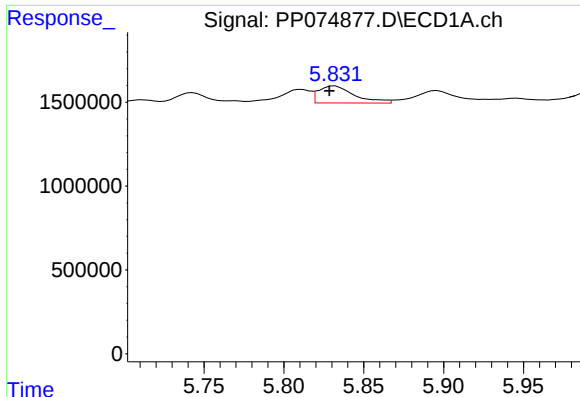

#17 AR-1242-2


R.T.: 5.832 min
Delta R.T.: 0.004 min
Response: 1601908
Conc: 28.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

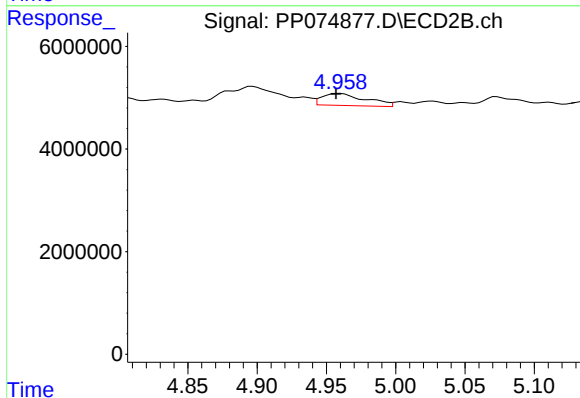


#17 AR-1242-2

R.T.: 4.960 min
Delta R.T.: 0.003 min
Response: 5155273
Conc: 25.74 ng/ml

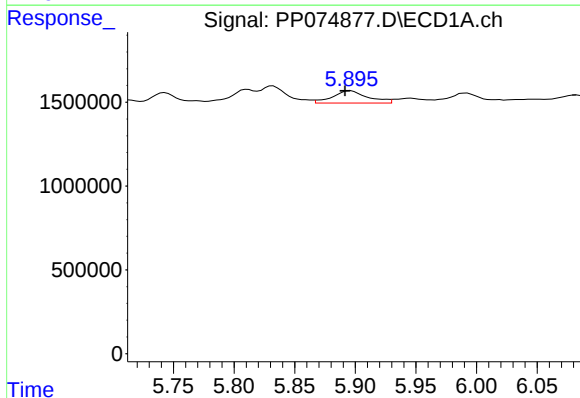


#18 AR-1242-3

R.T.: 5.896 min
Delta R.T.: 0.004 min
Response: 1465343
Conc: 36.09 ng/ml

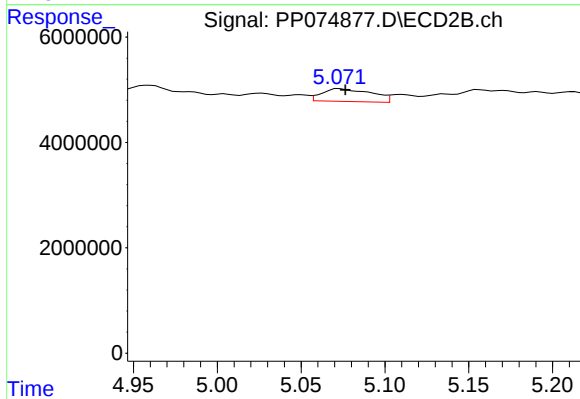

#18 AR-1242-3


R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 4960558
Conc: 41.93 ng/ml

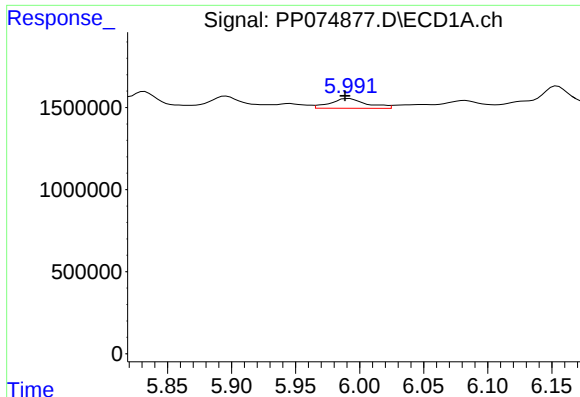

#19 AR-1242-4


R.T.: 5.992 min
Delta R.T.: 0.003 min
Response: 1186078
Conc: 37.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

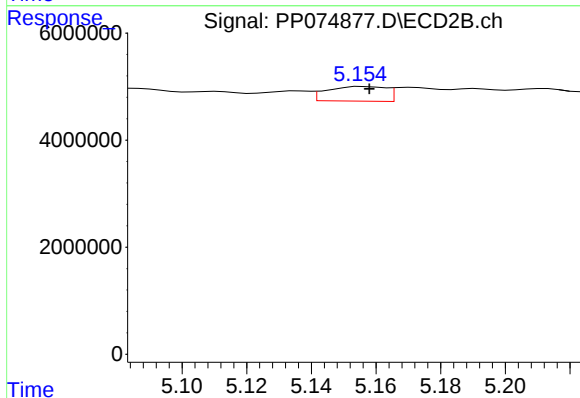


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 3439602
Conc: 20.10 ng/ml

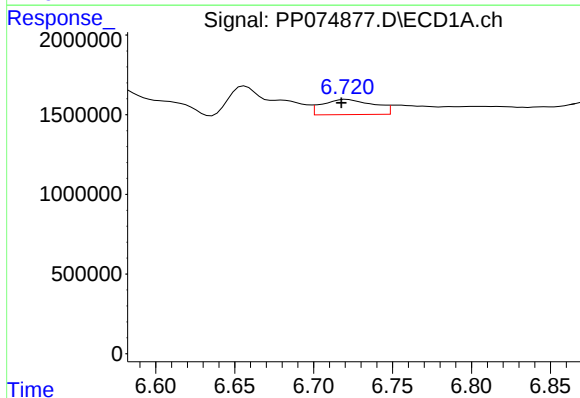


#20 AR-1242-5

R.T.: 6.721 min
Delta R.T.: 0.003 min
Response: 2159131
Conc: 59.86 ng/ml

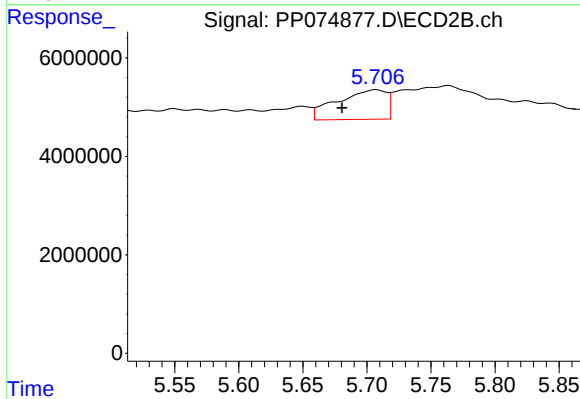

#20 AR-1242-5


R.T.: 5.708 min
Delta R.T.: 0.027 min
Response: 15987924
Conc: 86.34 ng/ml

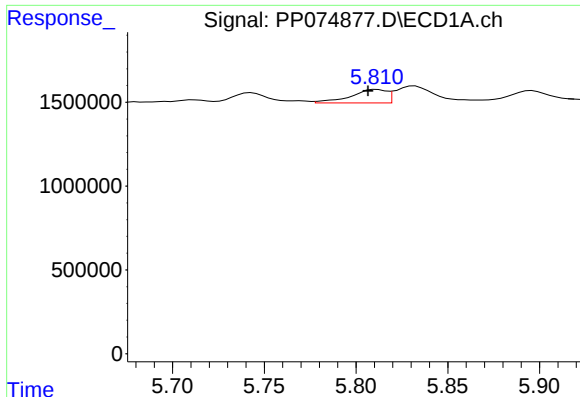

#21 AR-1248-1


R.T.: 5.811 min
Delta R.T.: 0.005 min
Response: 1107680
Conc: 36.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

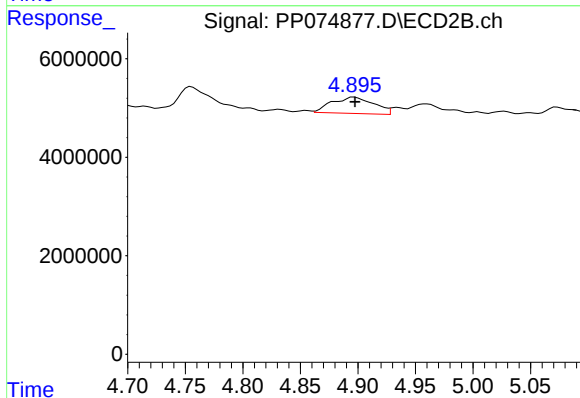


#21 AR-1248-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 8379866
Conc: 30.35 ng/ml

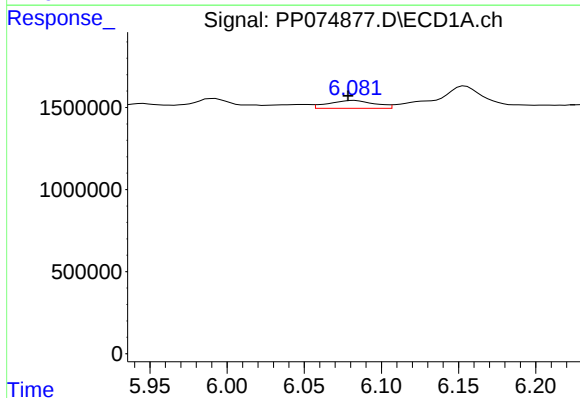


#22 AR-1248-2

R.T.: 6.083 min
Delta R.T.: 0.004 min
Response: 984084
Conc: 22.83 ng/ml

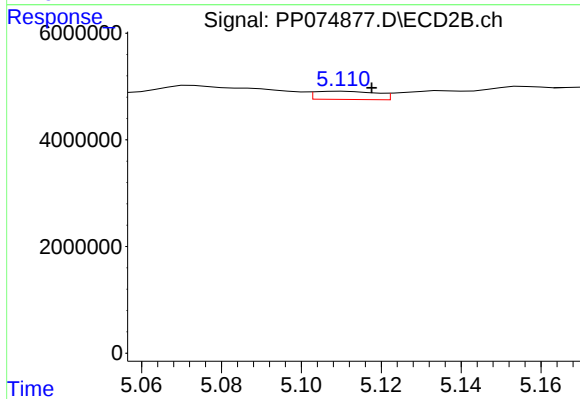

#22 AR-1248-2


R.T.: 5.111 min
Delta R.T.: -0.007 min
Response: 1663118
Conc: 9.41 ng/ml

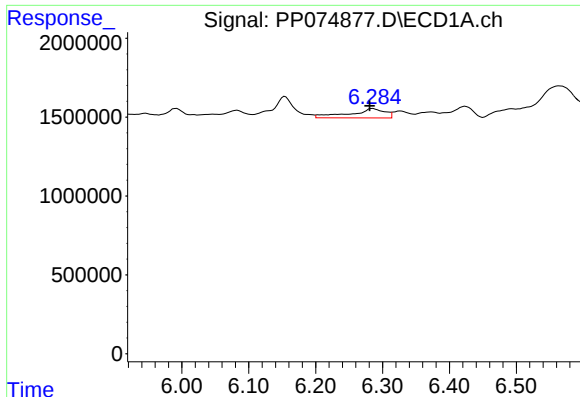

#23 AR-1248-3


R.T.: 6.285 min
Delta R.T.: 0.004 min
Response: 2150749
Conc: 46.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

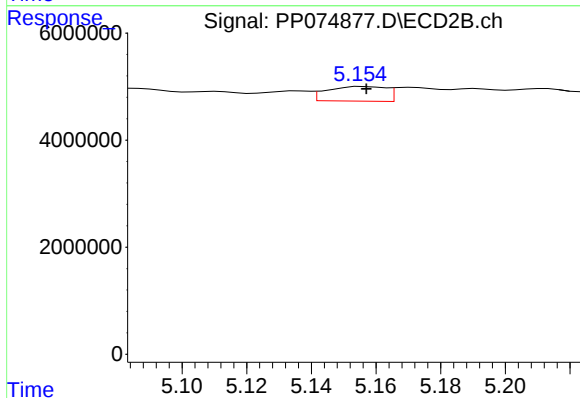


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: -0.001 min
Response: 3439602
Conc: 15.14 ng/ml

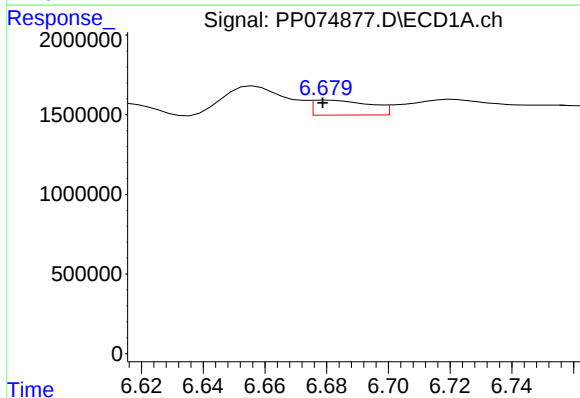


#24 AR-1248-4

R.T.: 6.680 min
Delta R.T.: 0.002 min
Response: 1199727
Conc: 21.81 ng/ml

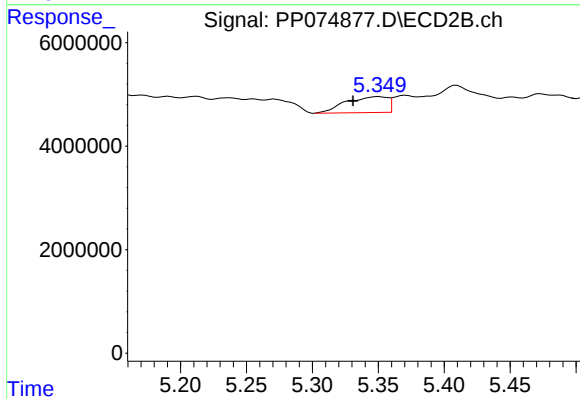

#24 AR-1248-4


R.T.: 5.350 min
Delta R.T.: 0.019 min
Response: 6695128
Conc: 30.71 ng/ml

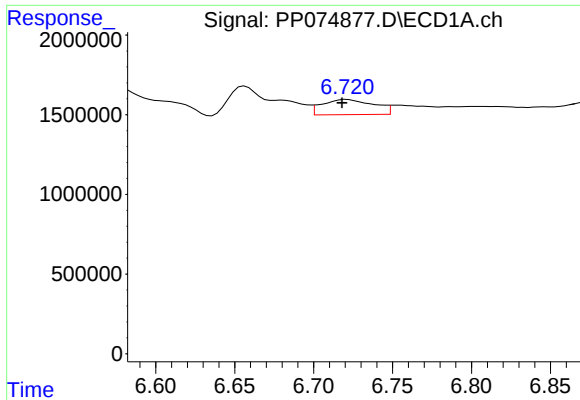

#25 AR-1248-5


R.T.: 6.721 min
Delta R.T.: 0.003 min
Response: 2159131
Conc: 38.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

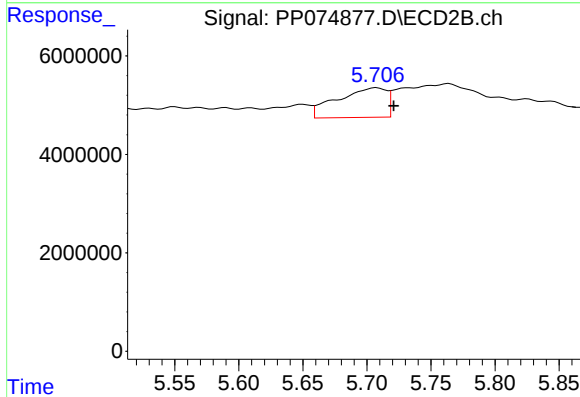


#25 AR-1248-5

R.T.: 5.708 min
Delta R.T.: -0.013 min
Response: 15987924
Conc: 43.53 ng/ml

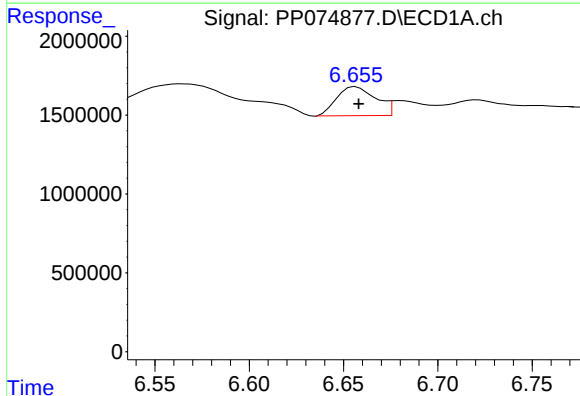


#26 AR-1254-1

R.T.: 6.657 min
Delta R.T.: -0.001 min
Response: 2637962
Conc: 45.27 ng/ml

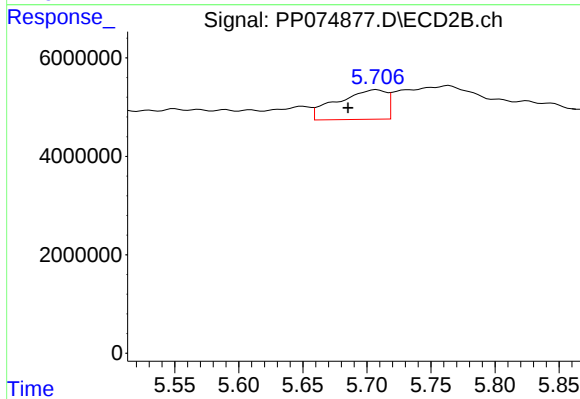

#26 AR-1254-1


R.T.: 5.708 min
Delta R.T.: 0.023 min
Response: 15987924
Conc: 33.54 ng/ml

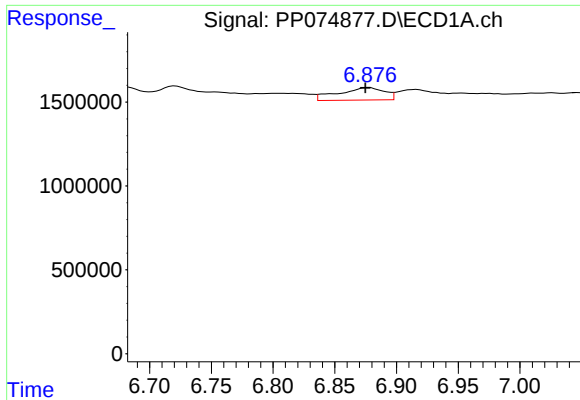

#27 AR-1254-2


R.T.: 6.878 min
Delta R.T.: 0.003 min
Response: 1916404
Conc: 23.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

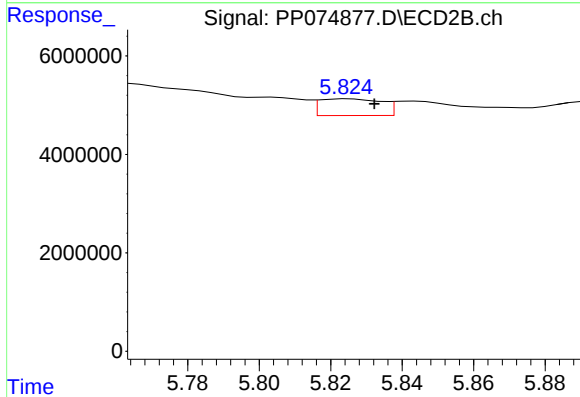


#27 AR-1254-2

R.T.: 5.825 min
Delta R.T.: -0.007 min
Response: 4107446
Conc: 11.66 ng/ml

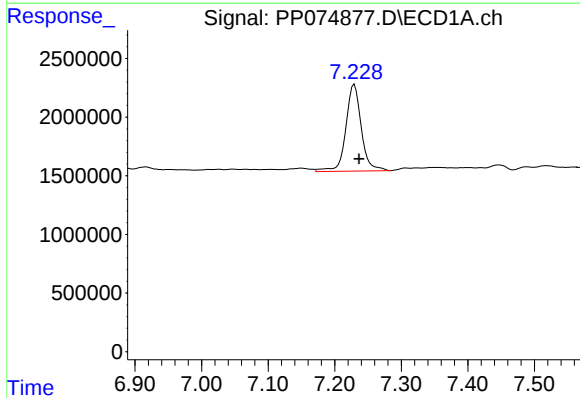


#28 AR-1254-3

R.T.: 7.229 min
Delta R.T.: -0.007 min
Response: 11947338
Conc: 133.93 ng/ml

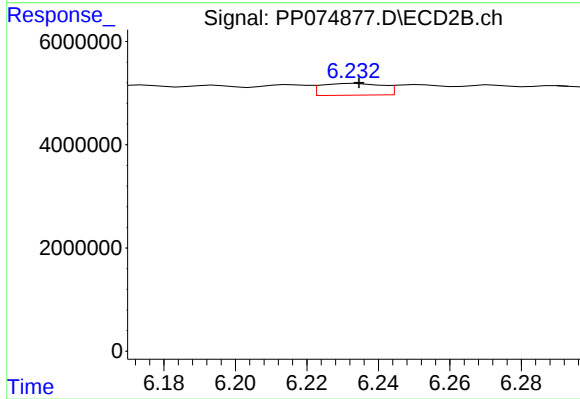

#28 AR-1254-3


R.T.: 6.234 min
Delta R.T.: 0.000 min
Response: 2721568
Conc: 4.39 ng/ml

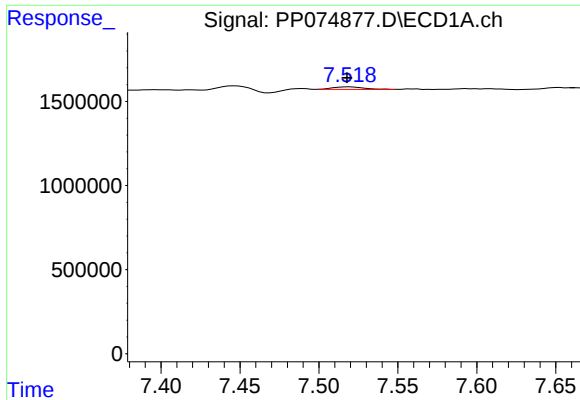

#29 AR-1254-4


R.T.: 7.519 min
Delta R.T.: 0.001 min
Response: 197425
Conc: 3.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

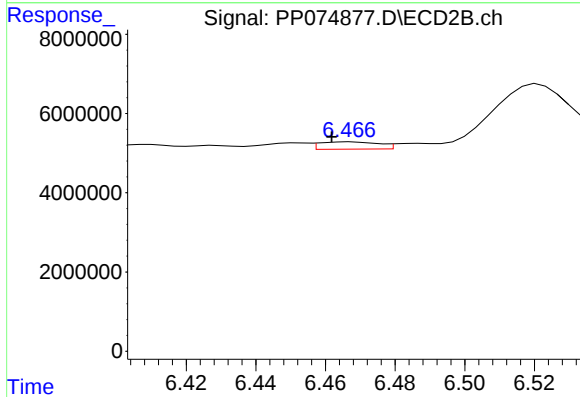


#29 AR-1254-4

R.T.: 6.467 min
Delta R.T.: 0.006 min
Response: 2158838
Conc: 4.61 ng/ml

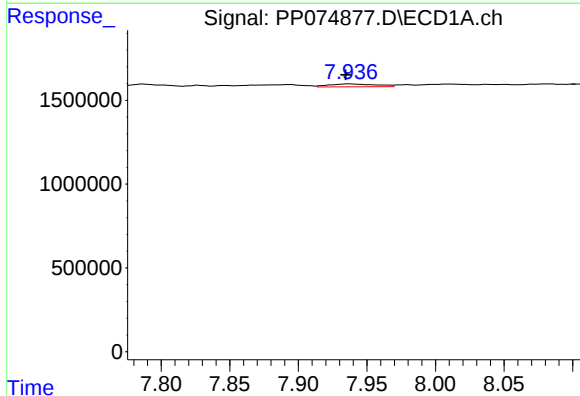


#30 AR-1254-5

R.T.: 7.938 min
Delta R.T.: 0.003 min
Response: 413500
Conc: 4.98 ng/ml

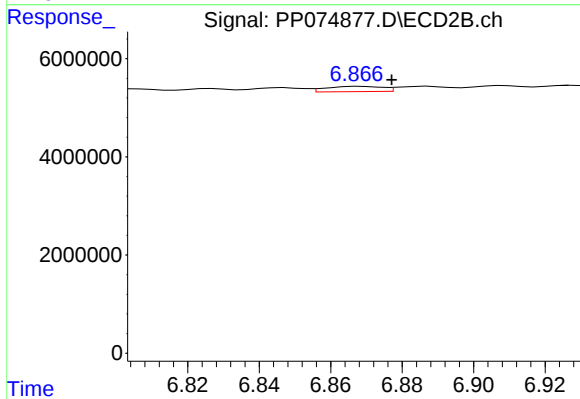

#30 AR-1254-5


R.T.: 6.868 min
Delta R.T.: -0.009 min
Response: 1161321
Conc: 2.37 ng/ml

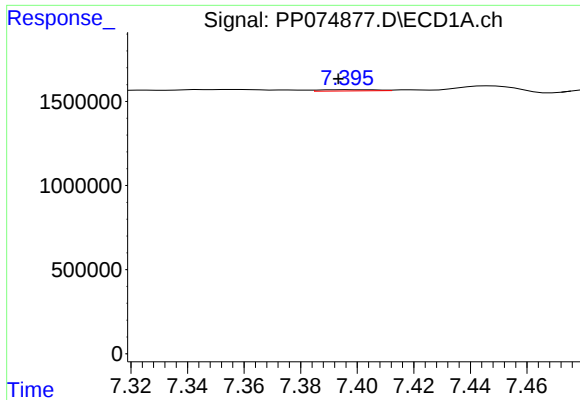

#31 AR-1260-1


R.T.: 7.397 min
Delta R.T.: 0.004 min
Response: 100944
Conc: 1.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

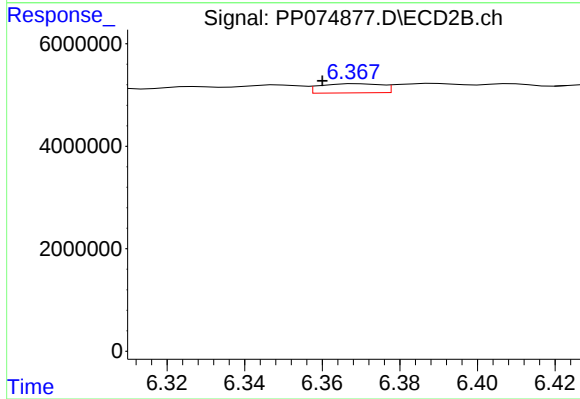


#31 AR-1260-1

R.T.: 6.369 min
Delta R.T.: 0.009 min
Response: 1965632
Conc: 5.24 ng/ml

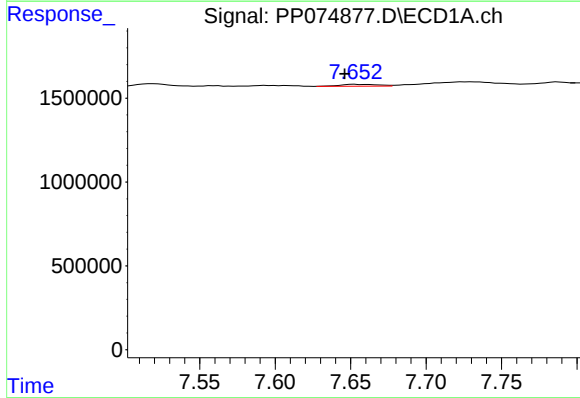


#32 AR-1260-2

R.T.: 7.653 min
Delta R.T.: 0.007 min
Response: 198231
Conc: 2.88 ng/ml

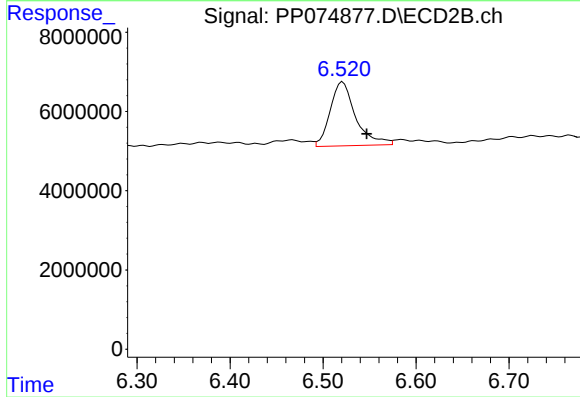

#32 AR-1260-2


R.T.: 6.521 min
Delta R.T.: -0.026 min
Response: 30640825
Conc: 57.94 ng/ml

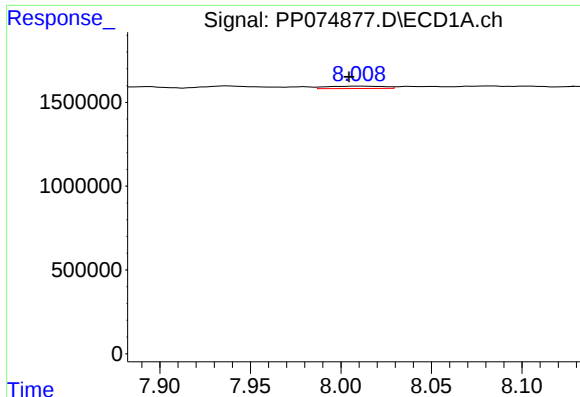

#33 AR-1260-3


R.T.: 8.010 min
Delta R.T.: 0.005 min
Response: 304428
Conc: 5.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

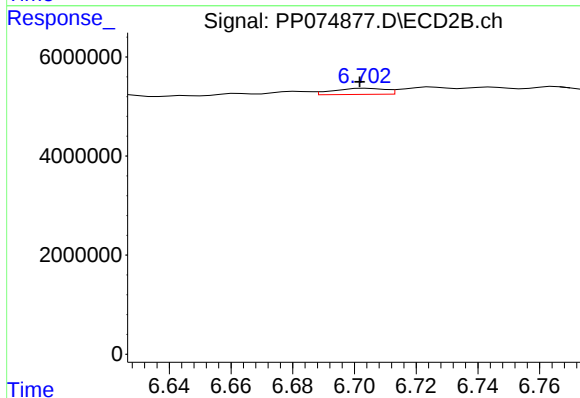


#33 AR-1260-3

R.T.: 6.704 min
Delta R.T.: 0.002 min
Response: 1435290
Conc: 3.31 ng/ml

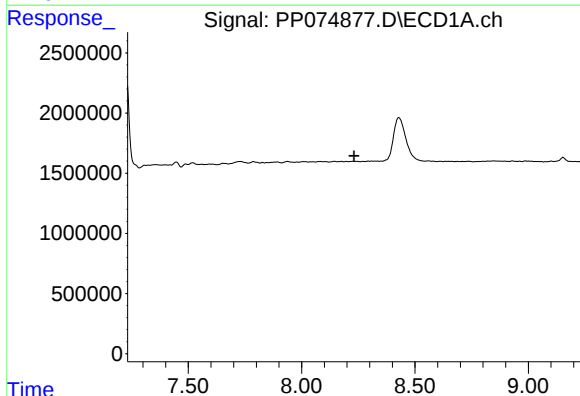


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 8.232 min
Response: 0
Conc: N.D.

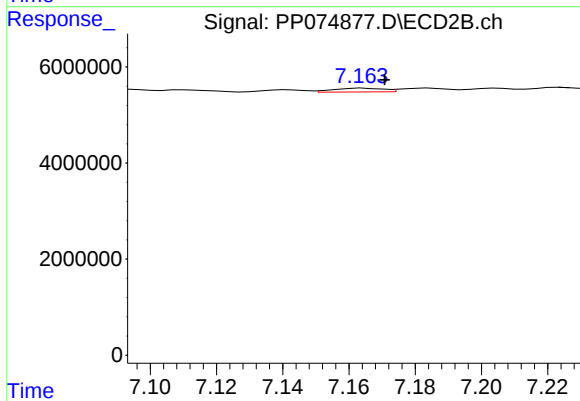

#34 AR-1260-4


R.T.: 7.164 min
Delta R.T.: -0.006 min
Response: 830323
Conc: 2.18 ng/ml

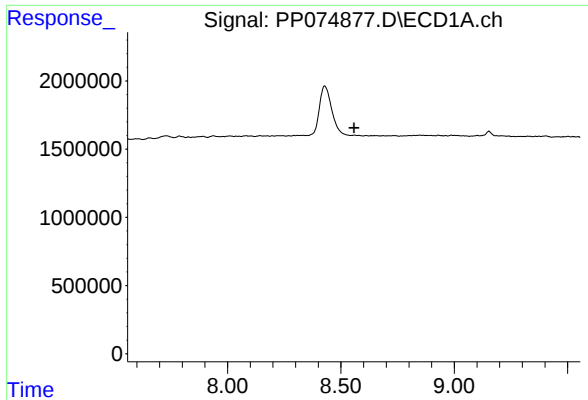

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.558 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

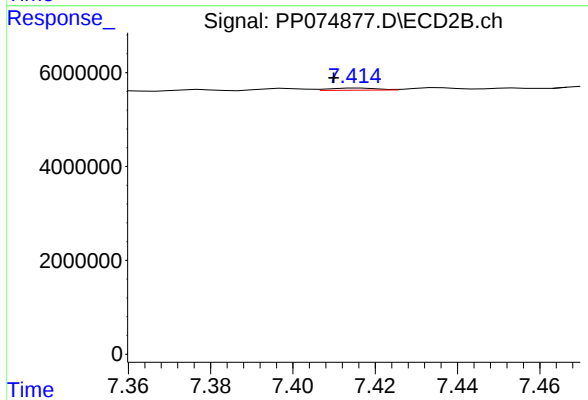


#35 AR-1260-5

R.T.: 7.416 min
Delta R.T.: 0.006 min
Response: 365762
Conc: 0.36 ng/ml

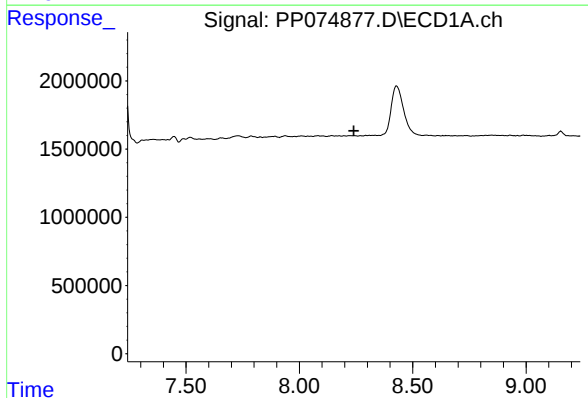


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T.: 8.241 min
Response: 0
Conc: N.D.

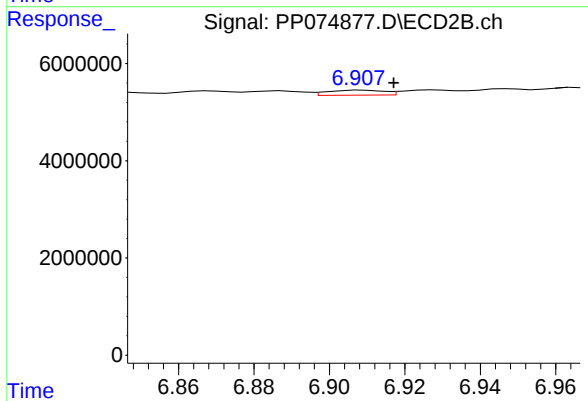

#36 AR-1262-1


R.T.: 6.909 min
Delta R.T.: -0.008 min
Response: 1061006
Conc: 1.50 ng/ml

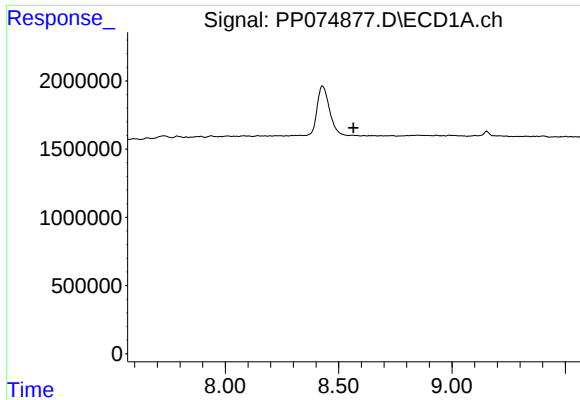

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

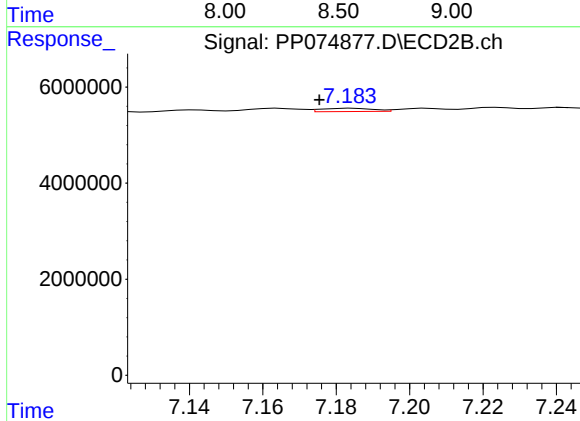


#37 AR-1262-2

R.T.: 7.184 min
Delta R.T.: 0.009 min
Response: 685513
Conc: 1.32 ng/ml

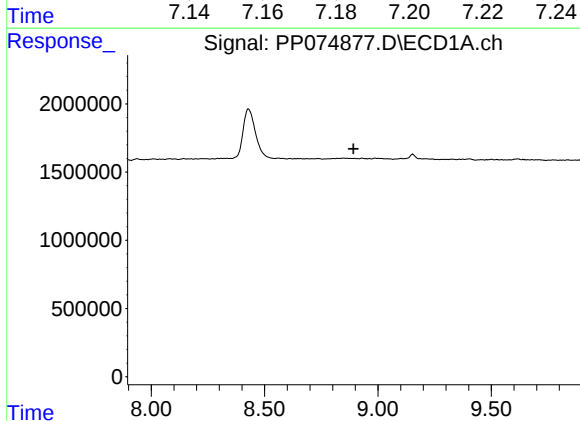


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.892 min
Response: 0
Conc: N.D.

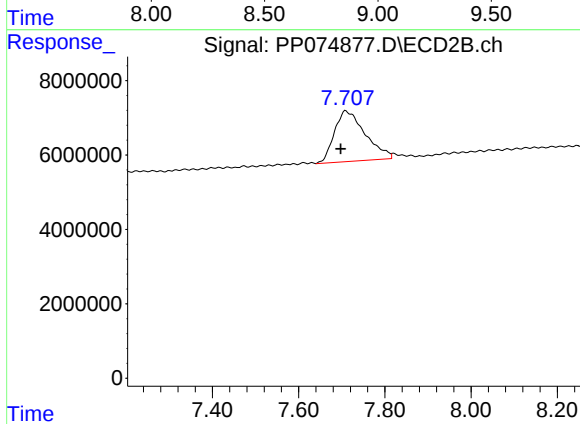

#38 AR-1262-3


R.T.: 7.709 min
Delta R.T.: 0.011 min
Response: 67456738
Conc: 144.66 ng/ml

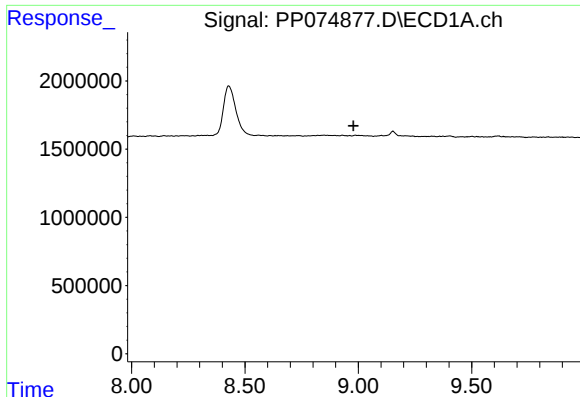

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

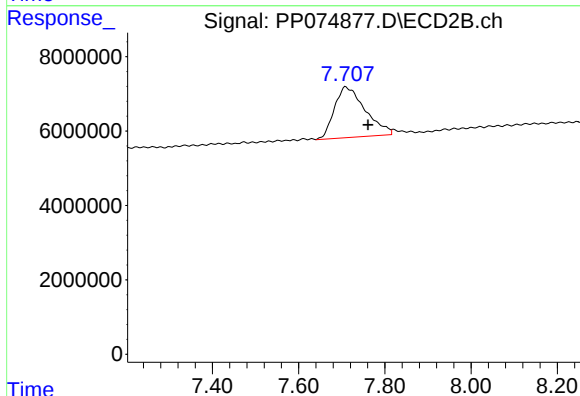


#39 AR-1262-4

R.T.: 7.709 min
Delta R.T.: -0.053 min
Response: 67456738
Conc: 82.08 ng/ml

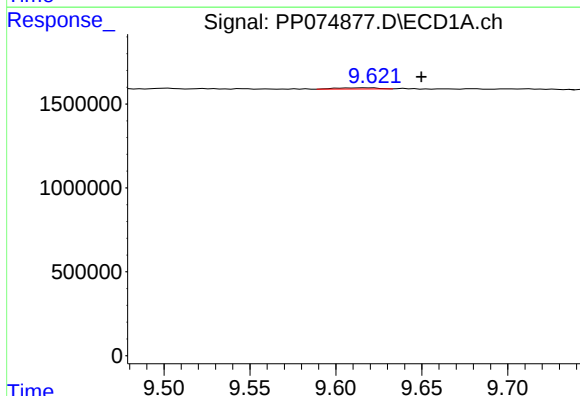


#40 AR-1262-5

R.T.: 9.622 min
Delta R.T.: -0.028 min
Response: 108045
Conc: 1.77 ng/ml

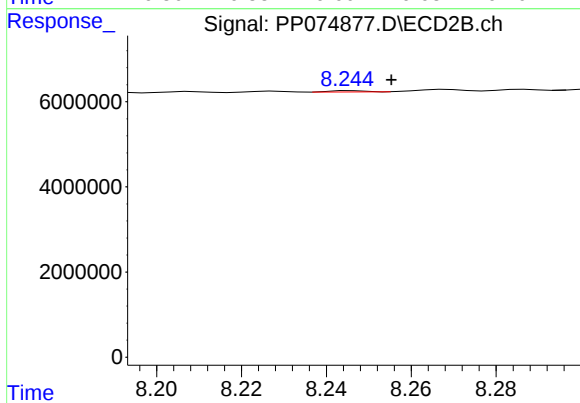

#40 AR-1262-5


R.T.: 8.246 min
Delta R.T.: -0.010 min
Response: 184648
Conc: 0.52 ng/ml

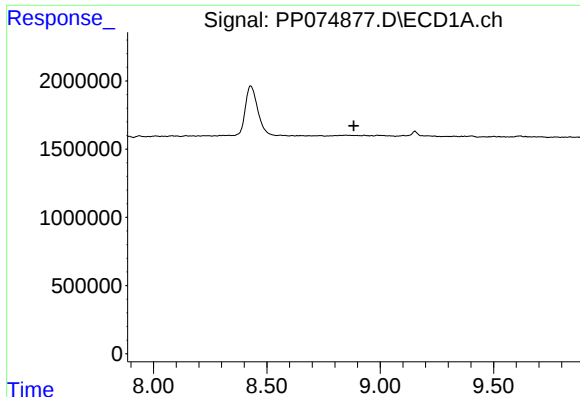

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

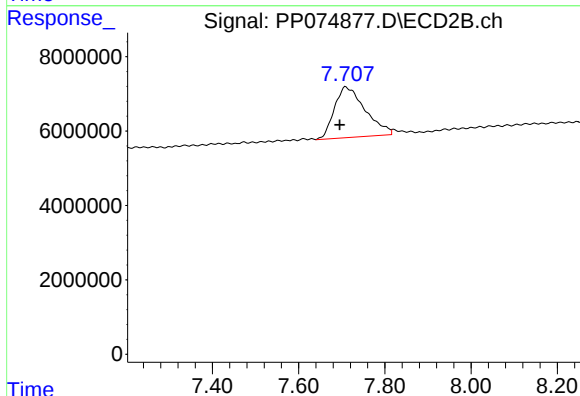


#41 AR-1268-1

R.T.: 7.709 min
Delta R.T.: 0.014 min
Response: 67456738
Conc: 47.82 ng/ml

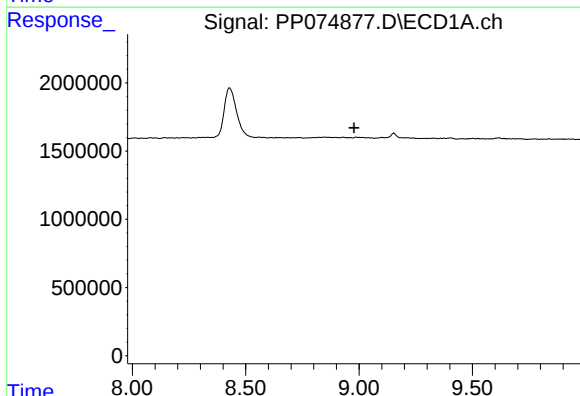


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

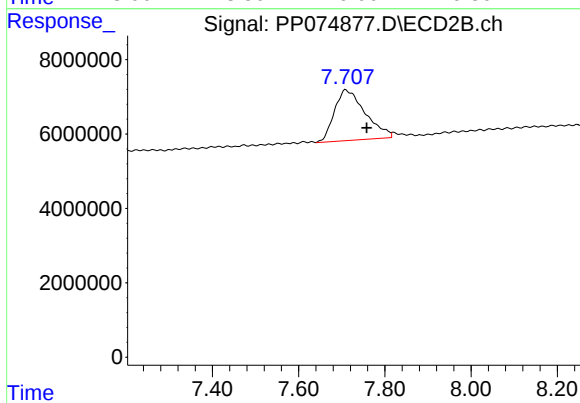

#42 AR-1268-2


R.T.: 7.709 min
Delta R.T.: -0.049 min
Response: 67456738
Conc: 49.48 ng/ml

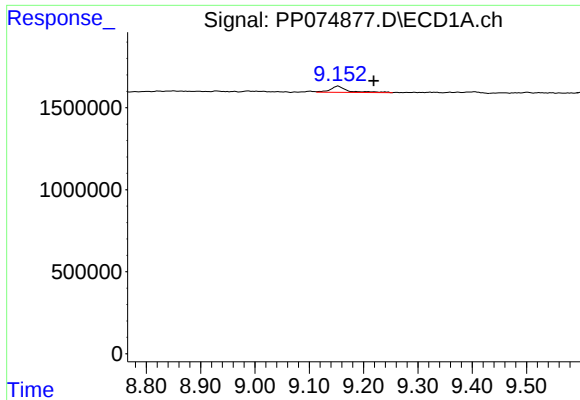

#43 AR-1268-3


R.T.: 9.153 min
Delta R.T.: -0.066 min
Response: 835531
Conc: 6.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

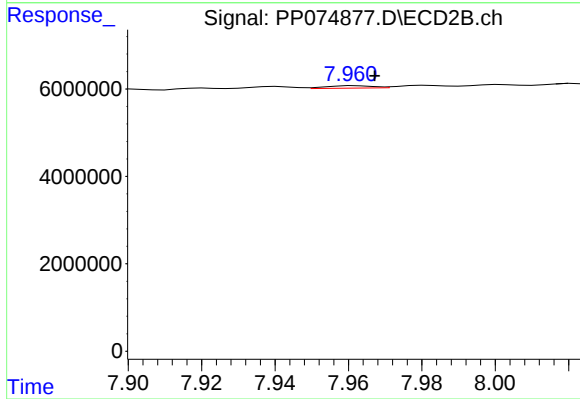


#43 AR-1268-3

R.T.: 7.962 min
Delta R.T.: -0.006 min
Response: 503375
Conc: 0.48 ng/ml

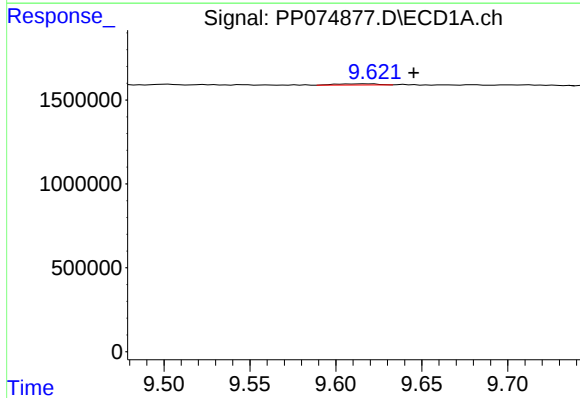


#44 AR-1268-4

R.T.: 9.622 min
Delta R.T.: -0.023 min
Response: 108045
Conc: 1.61 ng/ml

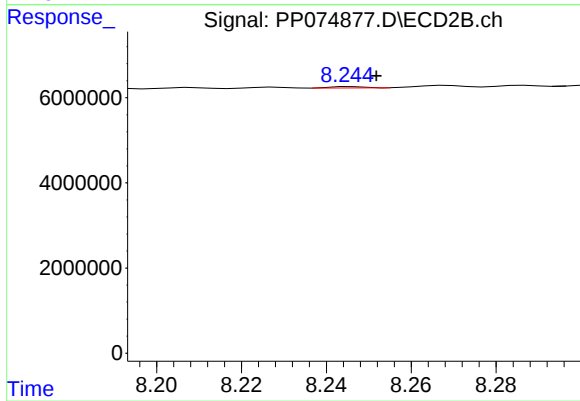

#44 AR-1268-4


R.T.: 8.246 min
Delta R.T.: -0.006 min
Response: 184648
Conc: 0.48 ng/ml

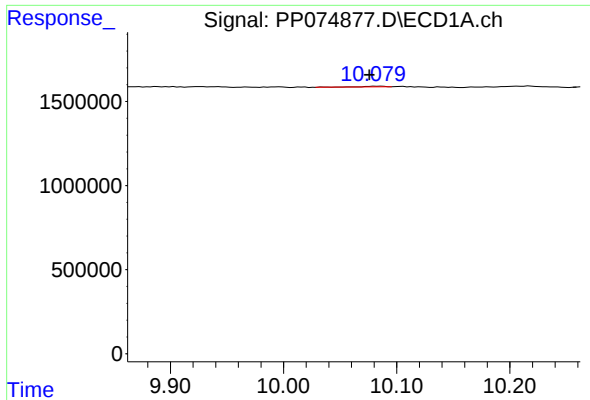

#45 AR-1268-5

R.T.: 10.081 min
Delta R.T.: 0.005 min
Response: 60698
Conc: 0.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

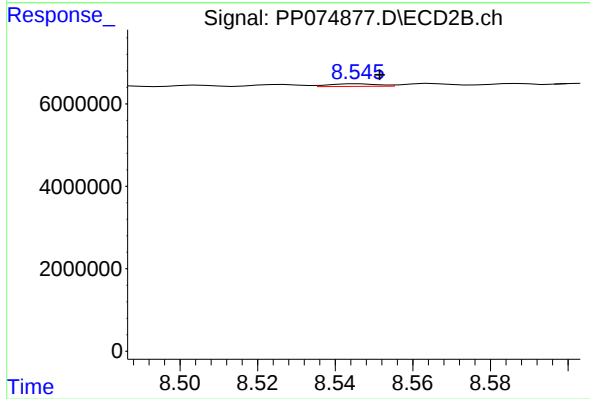

#45 AR-1268-5

R.T.: 8.546 min
Delta R.T.: -0.005 min
Response: 561113
Conc: 0.18 ng/ml