

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
 Data File : PP074881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Sep 2025 21:37
 Operator : YP\AJ
 Sample : Q2893-07
 Misc : AR1262 WATER LOD 40PPB
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 02:10:19 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.658	3.803	26492170	96139279	21.649	19.882
2)	SA Decachlor...	10.438	8.813	20899000	130.8E6	21.163	17.442
Target Compounds							
3)	L1 AR-1016-1	5.808	4.904	87804	331086	1.992	0.650 #
4)	L1 AR-1016-2	5.836	4.964	88123	342668	1.402	1.440
5)	L1 AR-1016-3	5.905	5.081	295733	265137	6.584	1.923 #
6)	L1 AR-1016-4	5.941f	5.117	326183	191099	9.271	1.367 #
7)	L1 AR-1016-5	0.000	5.334	0	571420	N.D.	3.441 #
8)	L2 AR-1221-1	0.000	4.005	0	140628	N.D.	2.273 #
9)	L2 AR-1221-2	4.960	4.095	436093	1114579	32.649	24.652
10)	L2 AR-1221-3	4.960f	4.179	436093	103961	11.503	0.633 #
11)	L3 AR-1232-1	4.960f	4.179	436093	103961	14.357	0.812 #
12)	L3 AR-1232-2	0.000	4.904	0	331086	N.D.	1.428 #
13)	L3 AR-1232-3	5.836	5.081	88123	265137	2.885	4.415 #
14)	L3 AR-1232-4	5.941f	5.157	326183	570452	18.888	7.739 #
15)	L3 AR-1232-5	6.083	5.334	162217	571420	12.497	9.204 #
16)	L4 AR-1242-1	5.808	4.904	87804	331086	2.294	0.785 #
17)	L4 AR-1242-2	5.836	4.964	88123	342668	1.560	1.711
18)	L4 AR-1242-3	5.905	5.081	295733	265137	7.284	2.241 #
19)	L4 AR-1242-4	5.941f	5.157	326183	570452	10.276	3.333 #
20)	L4 AR-1242-5	6.735	5.696	988789	2096536	27.413	11.323 #
21)	L5 AR-1248-1	5.808	4.904	87804	331086	2.905	1.199 #
22)	L5 AR-1248-2	6.083	5.117	162217	191099	3.764	1.081 #
23)	L5 AR-1248-3	0.000	5.157	0	570452	N.D.	2.511 #
24)	L5 AR-1248-4	6.657	5.334	1244660	571420	22.630	2.621 #
25)	L5 AR-1248-5	6.735	5.711	988789	1129944	17.826	3.076 #
26)	L6 AR-1254-1	6.657	5.696	1244660	2096536	21.360	4.398 #
27)	L6 AR-1254-2	6.874	5.832	545897	3384269	6.689	9.611 #
28)	L6 AR-1254-3	7.229	6.247	3170375	7589615	35.540	12.245 #
29)	L6 AR-1254-4	7.519	6.458	219883	915800	3.336	1.954 #
30)	L6 AR-1254-5	7.931	6.877	2479478	6641778	29.843	13.541 #
31)	L7 AR-1260-1	7.402	6.362	1962759	10550855	33.952	28.119
32)	L7 AR-1260-2	7.654	6.549	2484755	20097018	36.054	38.004
33)	L7 AR-1260-3	8.012	6.708	3585722	10340935	69.109	23.882 #
34)	L7 AR-1260-4	8.241	7.174	3323803	13692123	52.103	35.893 #
35)	L7 AR-1260-5	8.566	7.412	5530242	27011977	48.762	26.891 #
36)	L8 AR-1262-1	8.241	6.914	3323803	20048793	43.157	28.347 #
37)	L8 AR-1262-2	8.566	7.174	5530242	13692123	41.775	26.295 #
38)	L8 AR-1262-3	8.893	7.697	3821810	17745727	39.314	38.057
39)	L8 AR-1262-4	8.977	7.759	2838877	24968569	37.686	30.381
40)	L8 AR-1262-5	9.652	8.253	2270087	8975399	37.241	25.049 #
41)	L9 AR-1268-1	8.893	7.697	3821810	17745727	23.586	12.581 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 21:37
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1262 WATER LOD 40PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:10:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.977	7.759	2838877	24968569	19.347	18.313
43)	L9 AR-1268-3	9.220	7.967	277872	914153	2.248	0.876 #
44)	L9 AR-1268-4	9.652	8.253	2270087	8975399	33.749	23.429 #
45)	L9 AR-1268-5	10.082	8.553	794349	3476677	2.146	1.109 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090425\
Data File : PP074881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Sep 2025 21:37
Operator : YP\AJ
Sample : Q2893-07
Misc : AR1262 WATER LOD 40PPB
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 02:10:19 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

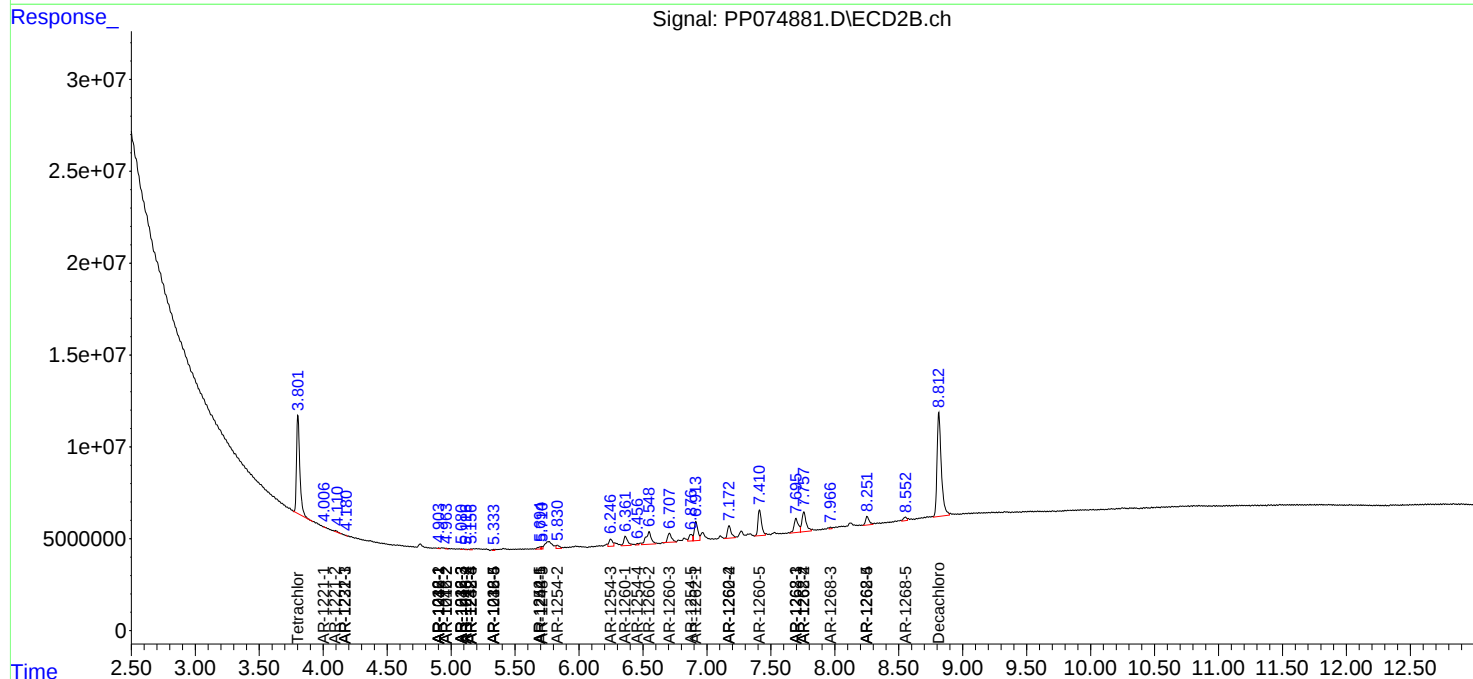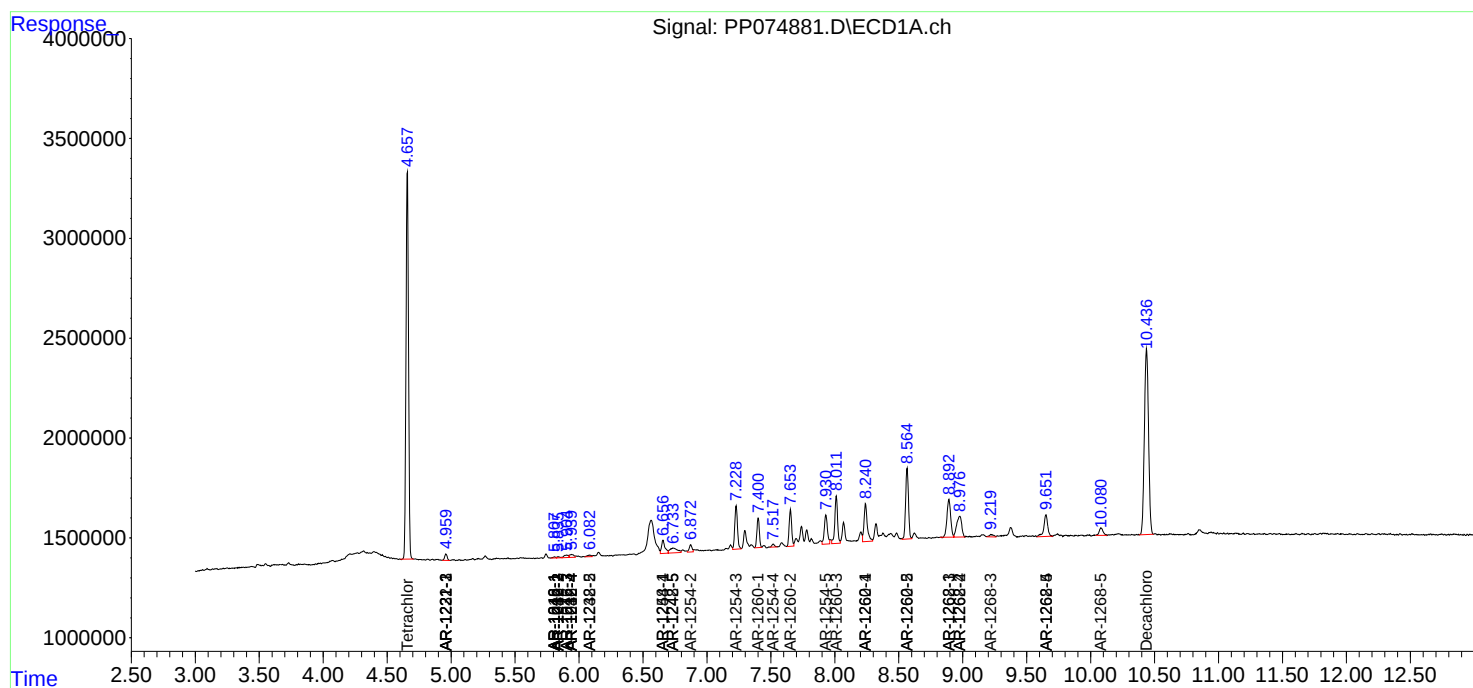


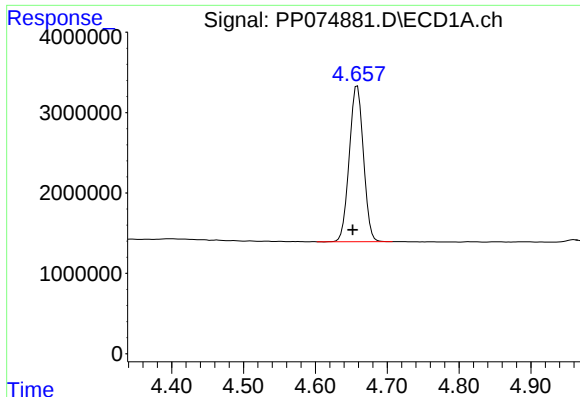

#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: 0.006 min
Response: 26492170
Conc: 21.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

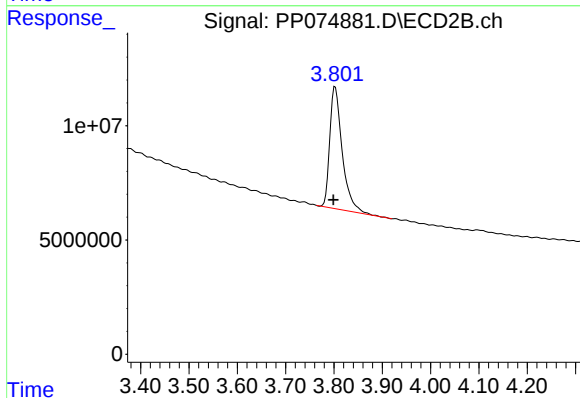


#1 Tetrachloro-m-xylene

R.T.: 3.803 min
Delta R.T.: 0.004 min
Response: 96139279
Conc: 19.88 ng/ml

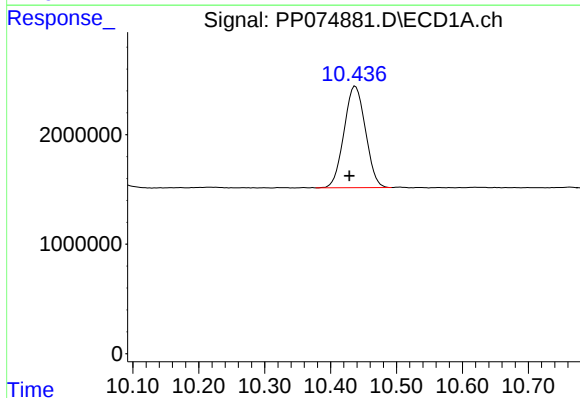


#2 Decachlorobiphenyl

R.T.: 10.438 min
Delta R.T.: 0.009 min
Response: 20899000
Conc: 21.16 ng/ml

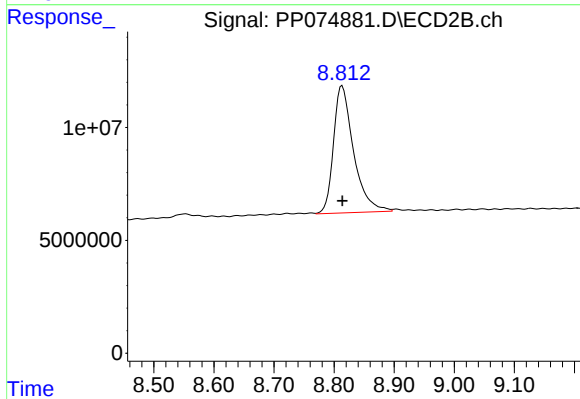

#2 Decachlorobiphenyl


R.T.: 8.813 min
Delta R.T.: 0.000 min
Response: 130802293
Conc: 17.44 ng/ml

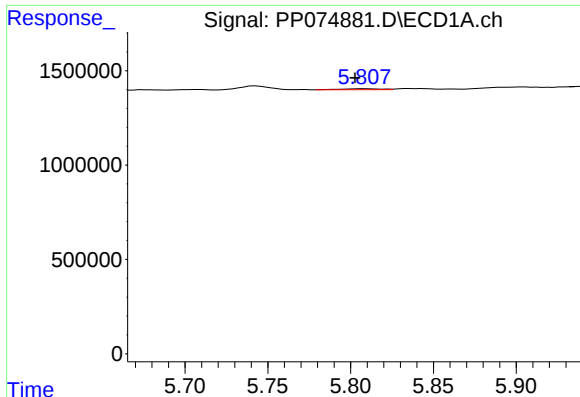

#3 AR-1016-1


R.T.: 5.808 min
Delta R.T.: 0.005 min
Response: 87804
Conc: 1.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

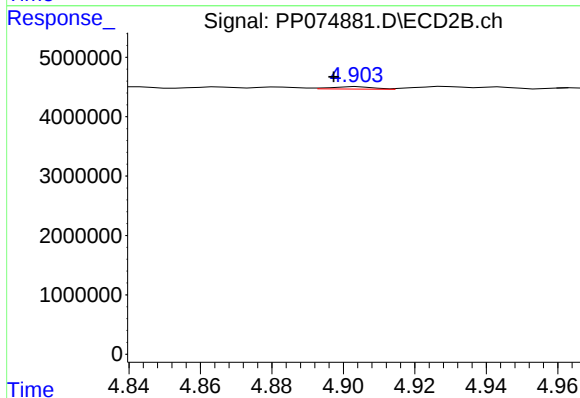


#3 AR-1016-1

R.T.: 4.904 min
Delta R.T.: 0.007 min
Response: 331086
Conc: 0.65 ng/ml

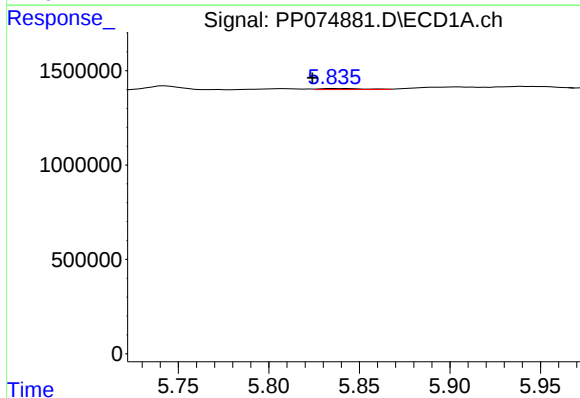


#4 AR-1016-2

R.T.: 5.836 min
Delta R.T.: 0.012 min
Response: 88123
Conc: 1.40 ng/ml

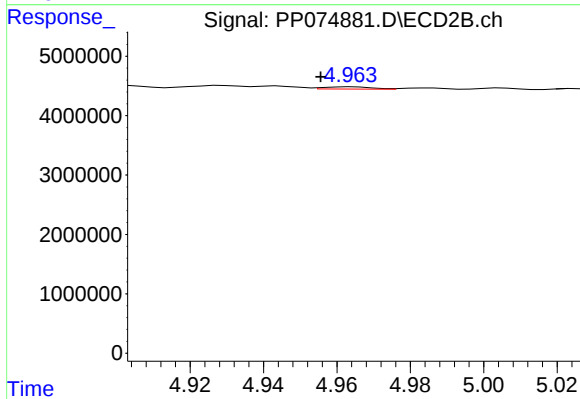

#4 AR-1016-2


R.T.: 4.964 min
Delta R.T.: 0.009 min
Response: 342668
Conc: 1.44 ng/ml

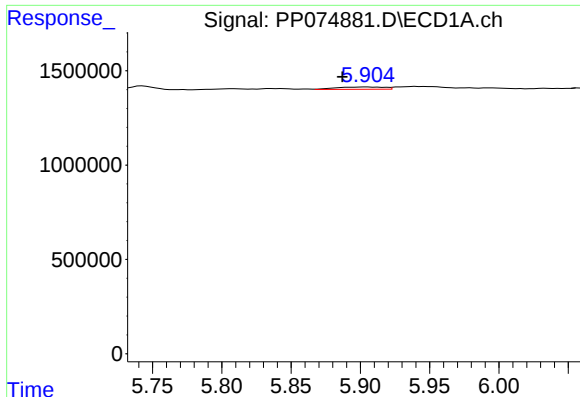

#5 AR-1016-3


R.T.: 5.905 min
Delta R.T.: 0.018 min
Response: 295733
Conc: 6.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

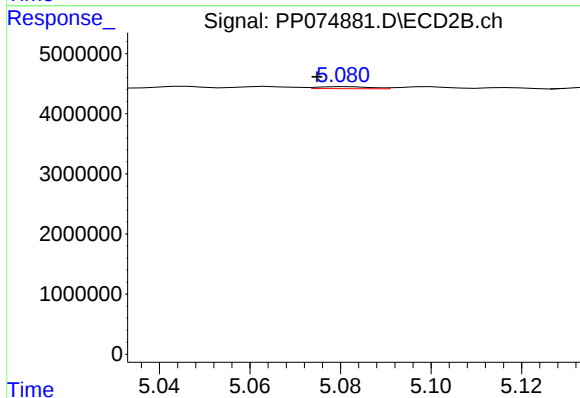


#5 AR-1016-3

R.T.: 5.081 min
Delta R.T.: 0.007 min
Response: 265137
Conc: 1.92 ng/ml

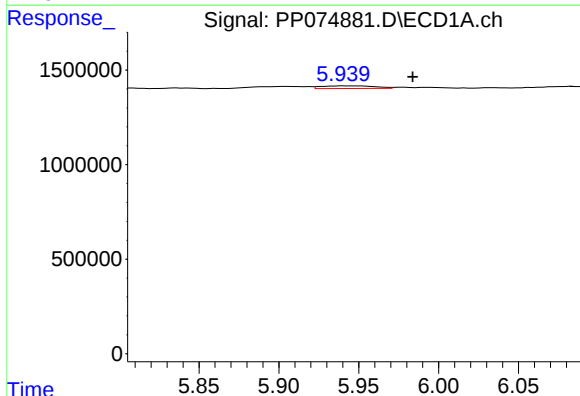


#6 AR-1016-4

R.T.: 5.941 min
Delta R.T.: -0.043 min
Response: 326183
Conc: 9.27 ng/ml

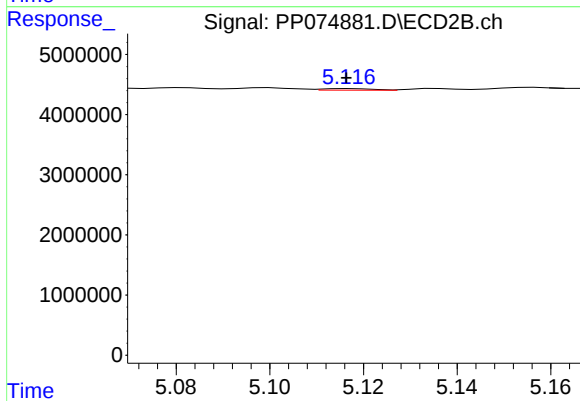

#6 AR-1016-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 191099
Conc: 1.37 ng/ml

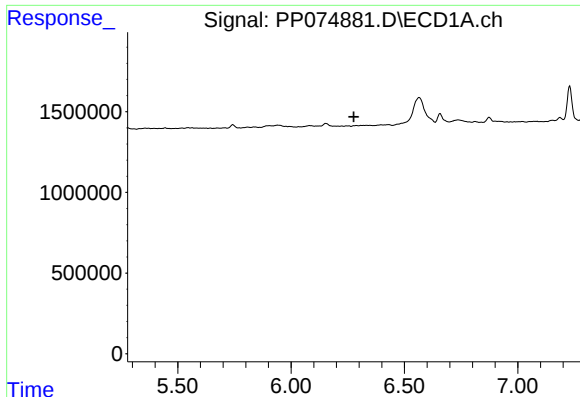

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.276 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

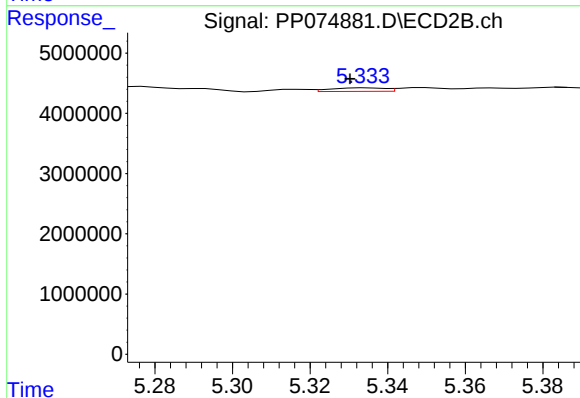


#7 AR-1016-5

R.T.: 5.334 min
Delta R.T.: 0.004 min
Response: 571420
Conc: 3.44 ng/ml

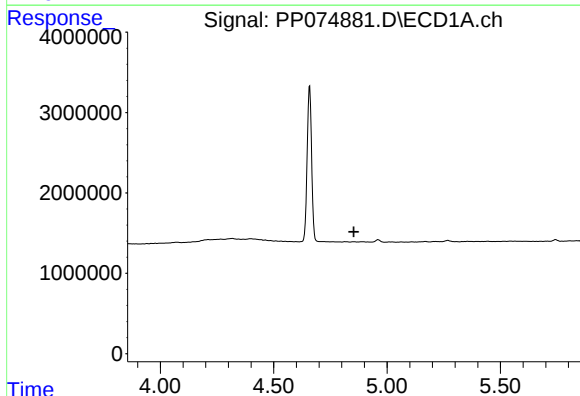


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T.: 4.853 min
Response: 0
Conc: N.D.

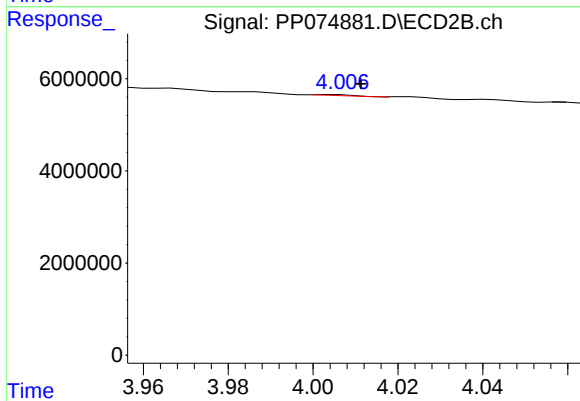

#8 AR-1221-1


R.T.: 4.005 min
Delta R.T.: -0.007 min
Response: 140628
Conc: 2.27 ng/ml

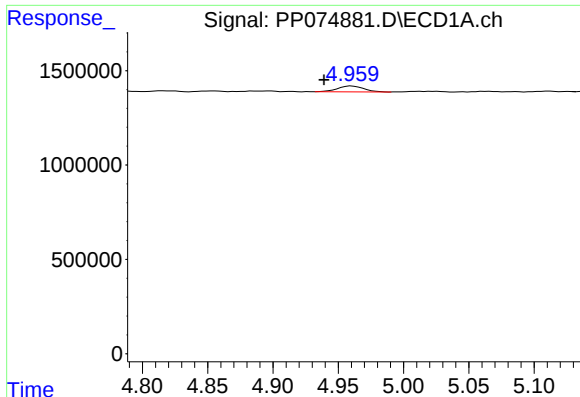

#9 AR-1221-2


R.T.: 4.960 min
Delta R.T.: 0.021 min
Response: 436093
Conc: 32.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

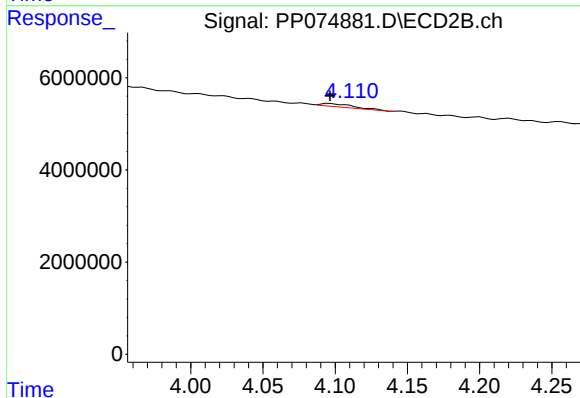


#9 AR-1221-2

R.T.: 4.095 min
Delta R.T.: -0.001 min
Response: 1114579
Conc: 24.65 ng/ml

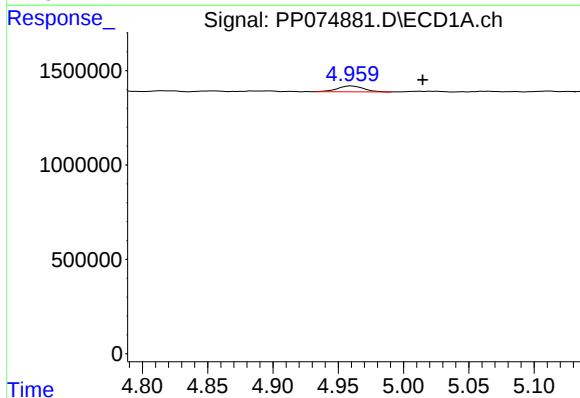


#10 AR-1221-3

R.T.: 4.960 min
Delta R.T.: -0.054 min
Response: 436093
Conc: 11.50 ng/ml

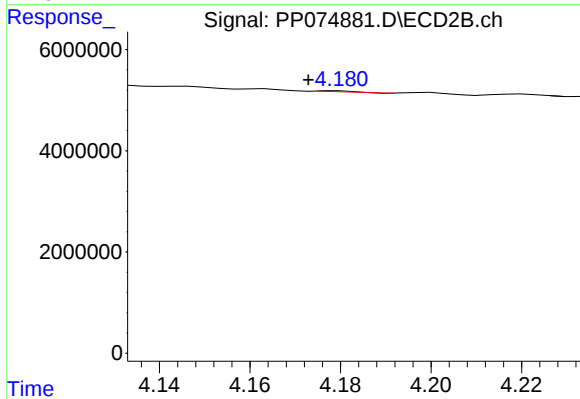

#10 AR-1221-3


R.T.: 4.179 min
Delta R.T.: 0.007 min
Response: 103961
Conc: 0.63 ng/ml

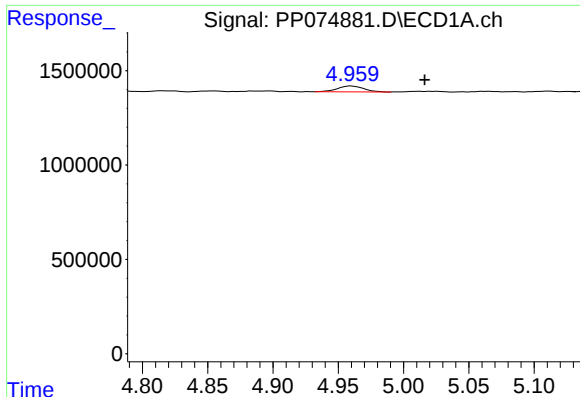

#11 AR-1232-1


R.T.: 4.960 min
Delta R.T.: -0.056 min
Response: 436093
Conc: 14.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

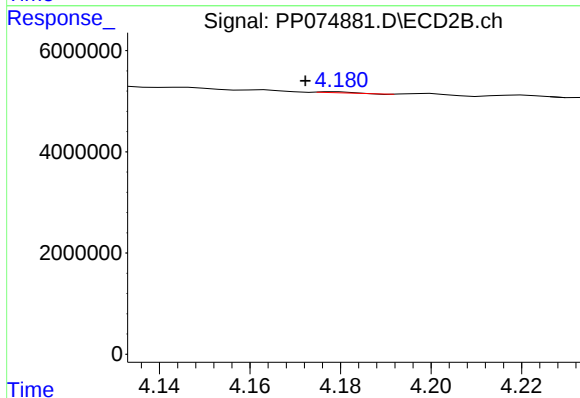


#11 AR-1232-1

R.T.: 4.179 min
Delta R.T.: 0.007 min
Response: 103961
Conc: 0.81 ng/ml

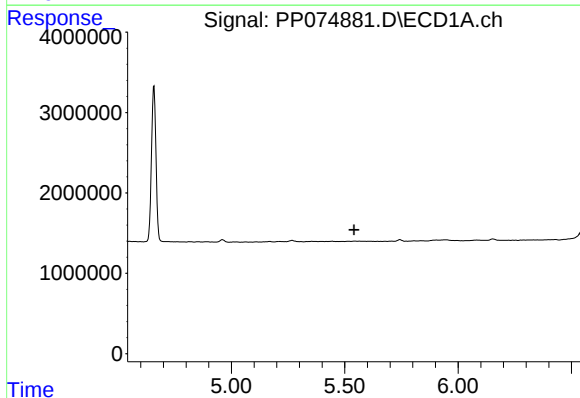


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.542 min
Response: 0
Conc: N.D.

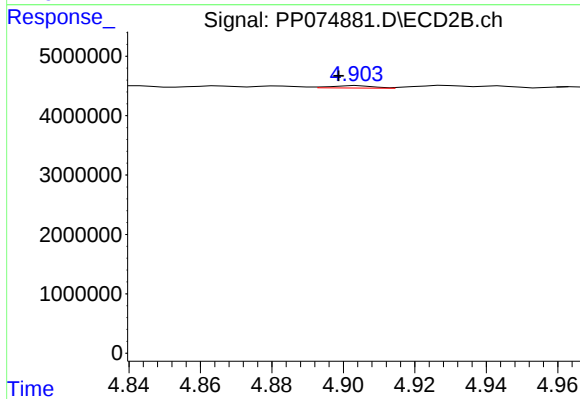

#12 AR-1232-2


R.T.: 4.904 min
Delta R.T.: 0.005 min
Response: 331086
Conc: 1.43 ng/ml

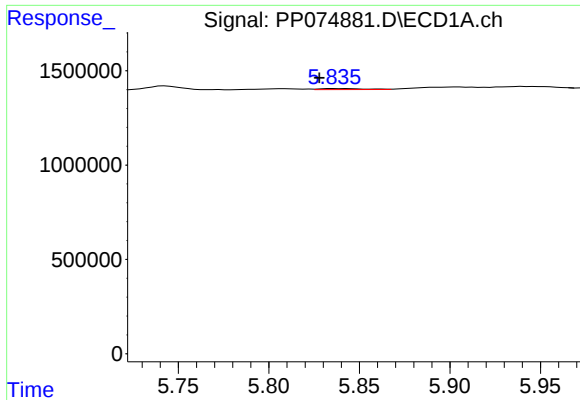

#13 AR-1232-3


R.T.: 5.836 min
Delta R.T.: 0.008 min
Response: 88123
Conc: 2.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

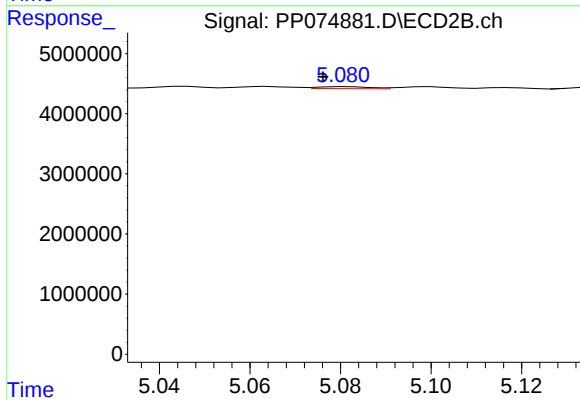


#13 AR-1232-3

R.T.: 5.081 min
Delta R.T.: 0.005 min
Response: 265137
Conc: 4.41 ng/ml

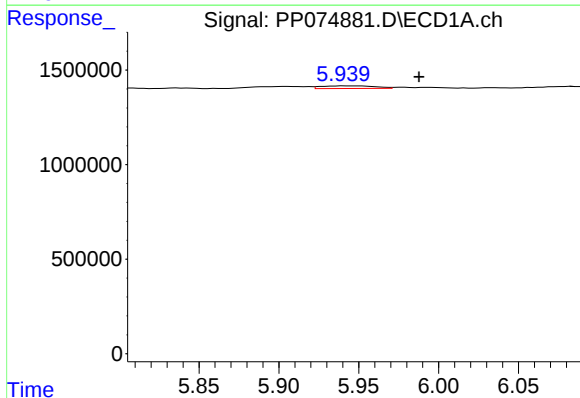


#14 AR-1232-4

R.T.: 5.941 min
Delta R.T.: -0.047 min
Response: 326183
Conc: 18.89 ng/ml

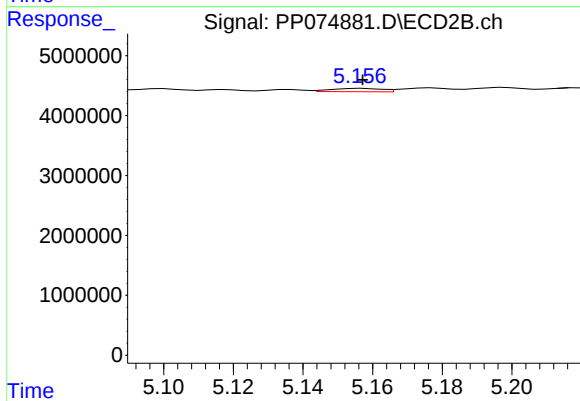

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 570452
Conc: 7.74 ng/ml

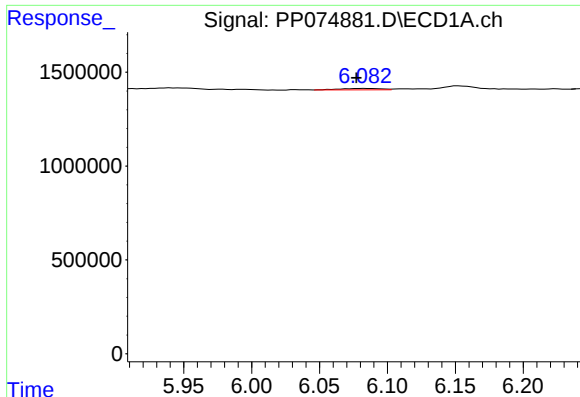

#15 AR-1232-5


R.T.: 6.083 min
Delta R.T.: 0.005 min
Response: 162217
Conc: 12.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

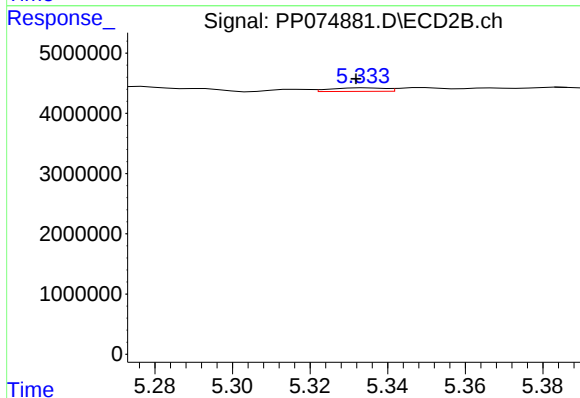


#15 AR-1232-5

R.T.: 5.334 min
Delta R.T.: 0.002 min
Response: 571420
Conc: 9.20 ng/ml

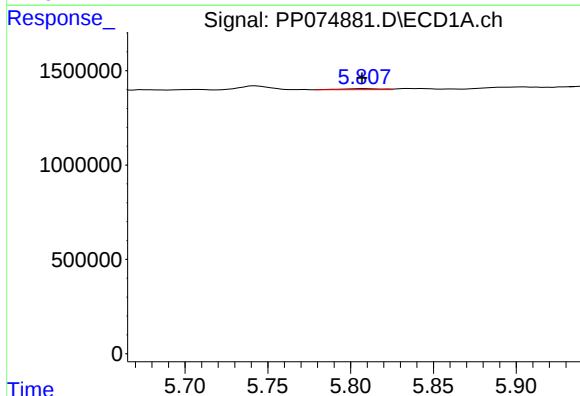


#16 AR-1242-1

R.T.: 5.808 min
Delta R.T.: 0.001 min
Response: 87804
Conc: 2.29 ng/ml

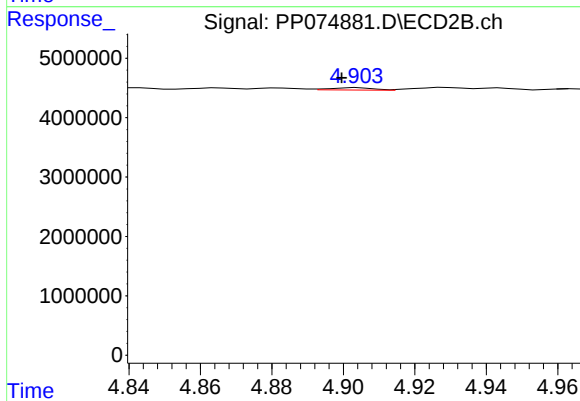

#16 AR-1242-1


R.T.: 4.904 min
Delta R.T.: 0.005 min
Response: 331086
Conc: 0.79 ng/ml

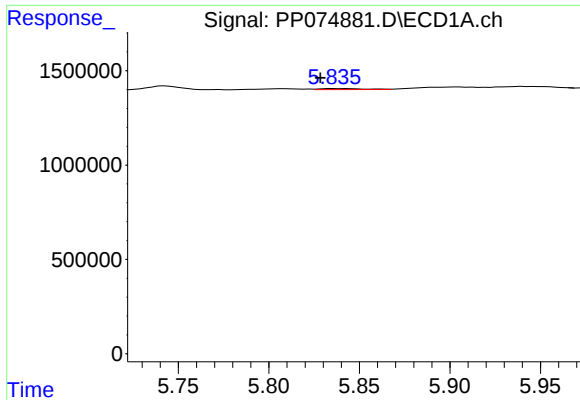

#17 AR-1242-2


R.T.: 5.836 min
Delta R.T.: 0.008 min
Response: 88123
Conc: 1.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

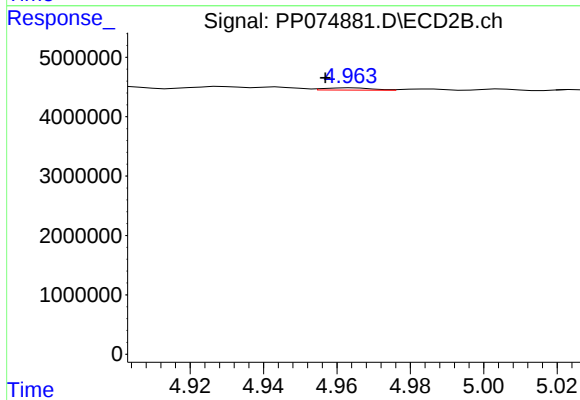


#17 AR-1242-2

R.T.: 4.964 min
Delta R.T.: 0.007 min
Response: 342668
Conc: 1.71 ng/ml

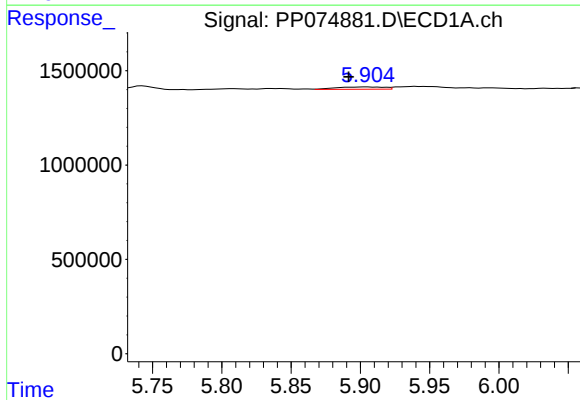


#18 AR-1242-3

R.T.: 5.905 min
Delta R.T.: 0.013 min
Response: 295733
Conc: 7.28 ng/ml

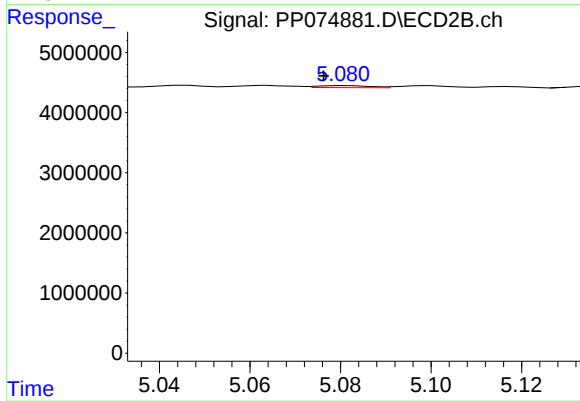

#18 AR-1242-3


R.T.: 5.081 min
Delta R.T.: 0.005 min
Response: 265137
Conc: 2.24 ng/ml

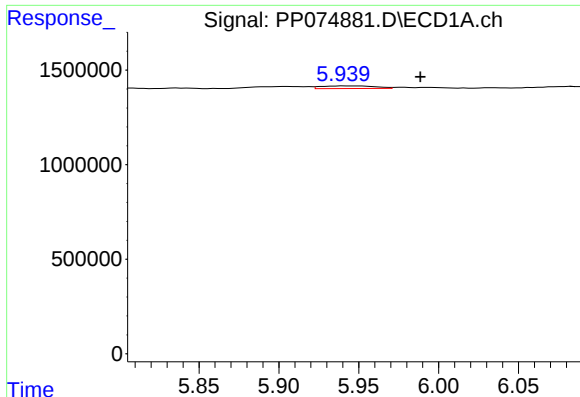

#19 AR-1242-4


R.T.: 5.941 min
Delta R.T.: -0.048 min
Response: 326183
Conc: 10.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

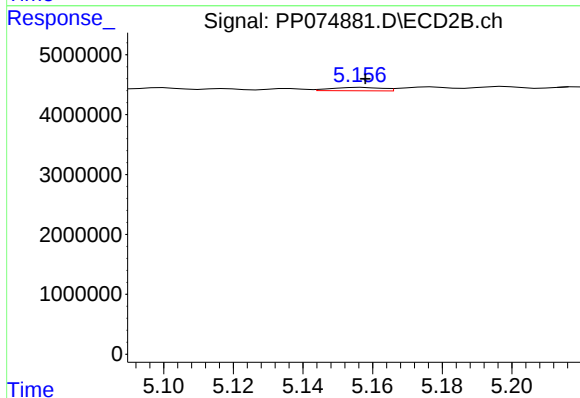


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: -0.001 min
Response: 570452
Conc: 3.33 ng/ml

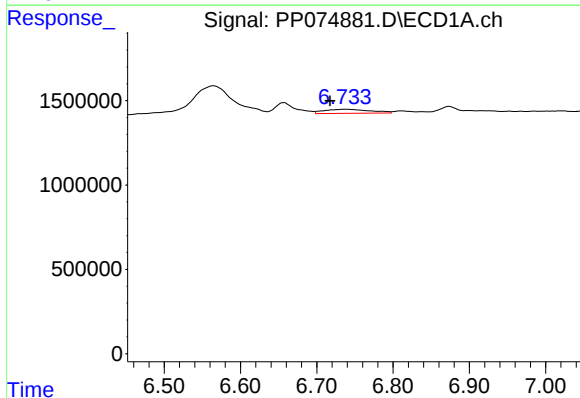


#20 AR-1242-5

R.T.: 6.735 min
Delta R.T.: 0.018 min
Response: 988789
Conc: 27.41 ng/ml

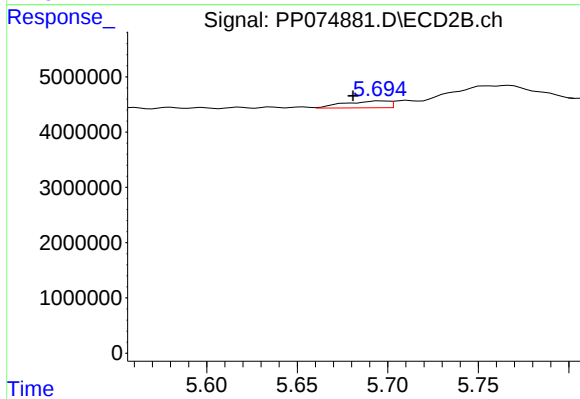

#20 AR-1242-5


R.T.: 5.696 min
Delta R.T.: 0.015 min
Response: 2096536
Conc: 11.32 ng/ml

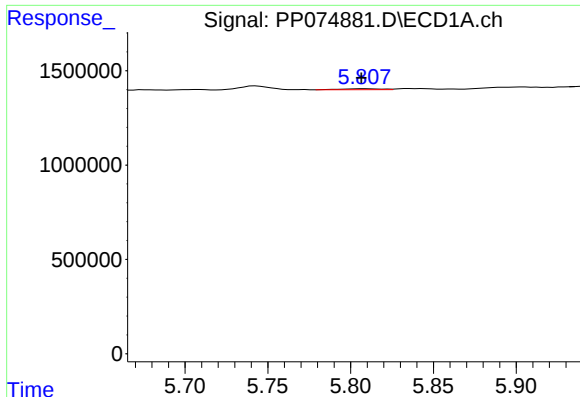

#21 AR-1248-1


R.T.: 5.808 min
Delta R.T.: 0.002 min
Response: 87804
Conc: 2.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

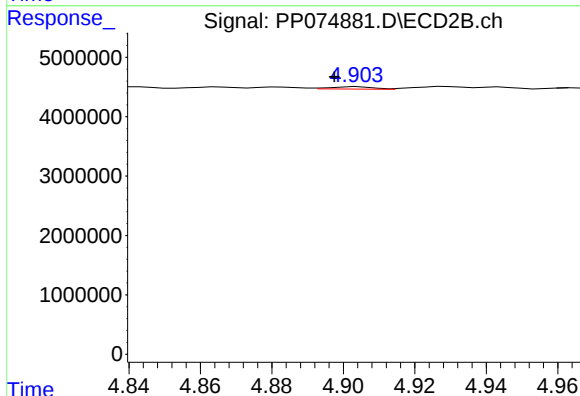


#21 AR-1248-1

R.T.: 4.904 min
Delta R.T.: 0.007 min
Response: 331086
Conc: 1.20 ng/ml

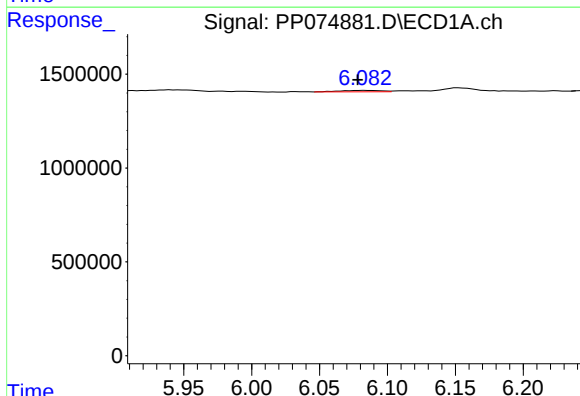


#22 AR-1248-2

R.T.: 6.083 min
Delta R.T.: 0.004 min
Response: 162217
Conc: 3.76 ng/ml

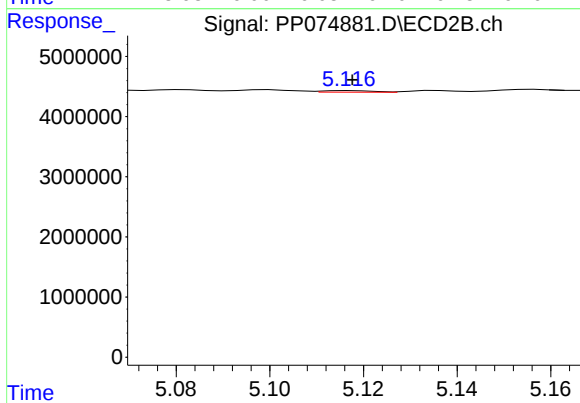

#22 AR-1248-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 191099
Conc: 1.08 ng/ml

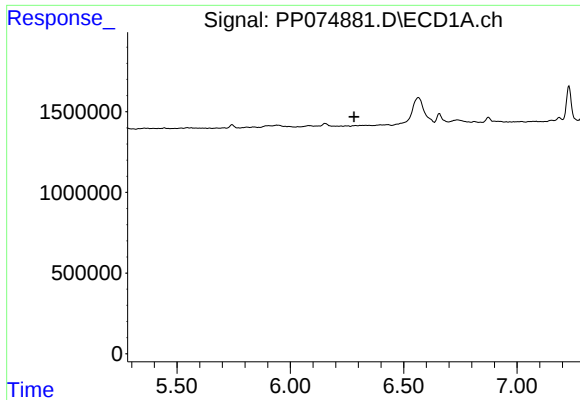

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 6.281 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

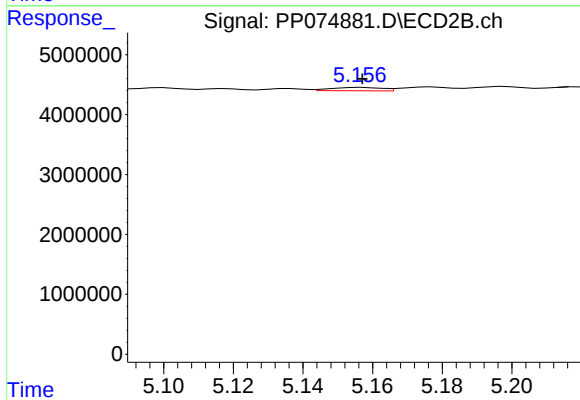


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 570452
Conc: 2.51 ng/ml

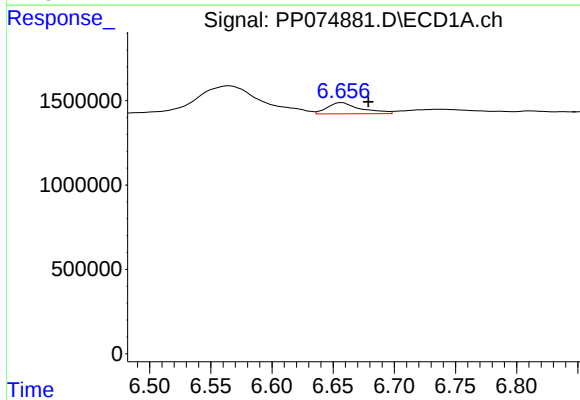


#24 AR-1248-4

R.T.: 6.657 min
Delta R.T.: -0.021 min
Response: 1244660
Conc: 22.63 ng/ml

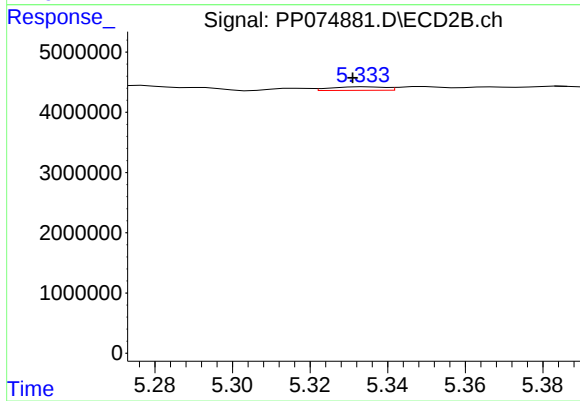

#24 AR-1248-4


R.T.: 5.334 min
Delta R.T.: 0.003 min
Response: 571420
Conc: 2.62 ng/ml

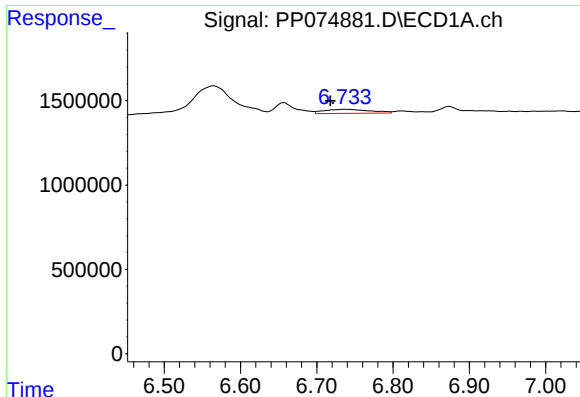

#25 AR-1248-5


R.T.: 6.735 min
Delta R.T.: 0.017 min
Response: 988789
Conc: 17.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

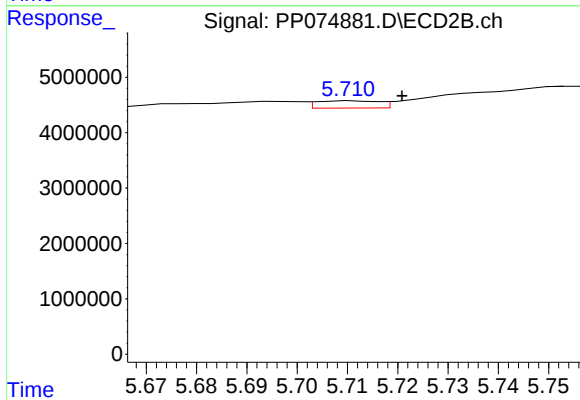


#25 AR-1248-5

R.T.: 5.711 min
Delta R.T.: -0.010 min
Response: 1129944
Conc: 3.08 ng/ml

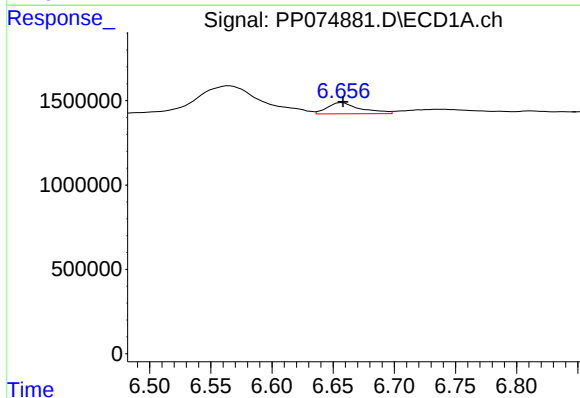


#26 AR-1254-1

R.T.: 6.657 min
Delta R.T.: 0.000 min
Response: 1244660
Conc: 21.36 ng/ml

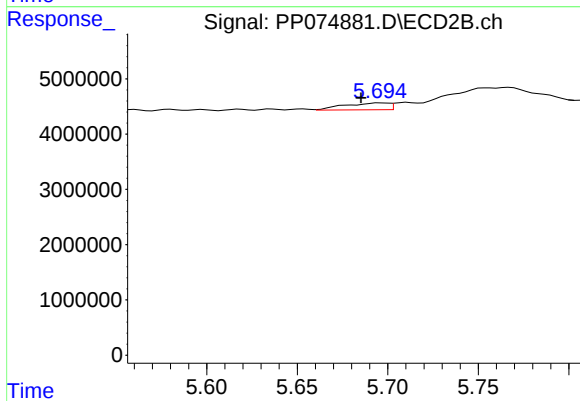

#26 AR-1254-1


R.T.: 5.696 min
Delta R.T.: 0.011 min
Response: 2096536
Conc: 4.40 ng/ml

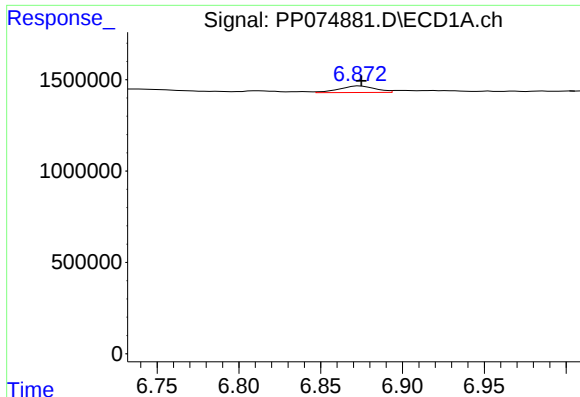

#27 AR-1254-2


R.T.: 6.874 min
Delta R.T.: -0.001 min
Response: 545897
Conc: 6.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

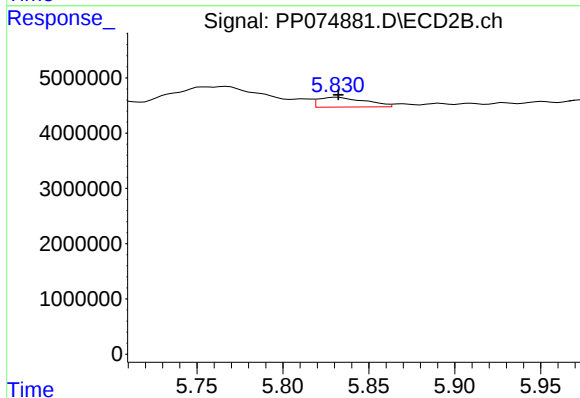


#27 AR-1254-2

R.T.: 5.832 min
Delta R.T.: 0.000 min
Response: 3384269
Conc: 9.61 ng/ml

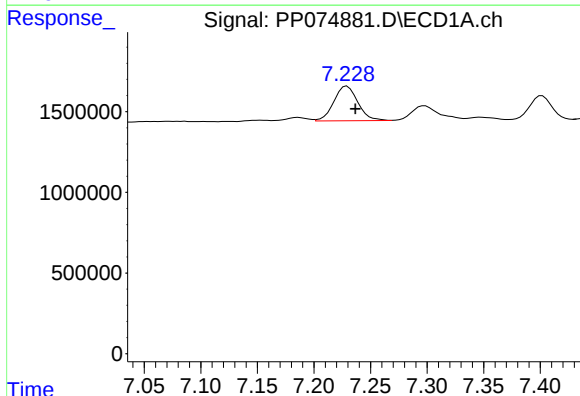


#28 AR-1254-3

R.T.: 7.229 min
Delta R.T.: -0.008 min
Response: 3170375
Conc: 35.54 ng/ml

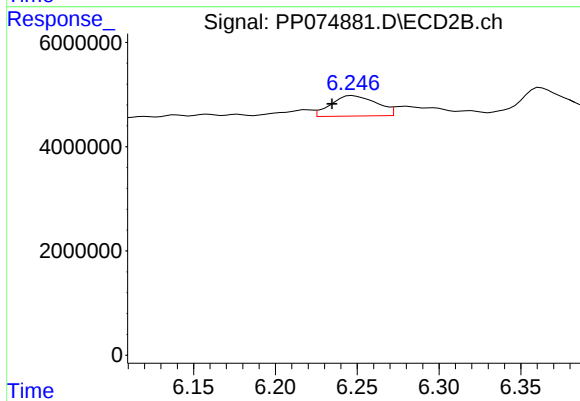

#28 AR-1254-3


R.T.: 6.247 min
Delta R.T.: 0.013 min
Response: 7589615
Conc: 12.25 ng/ml

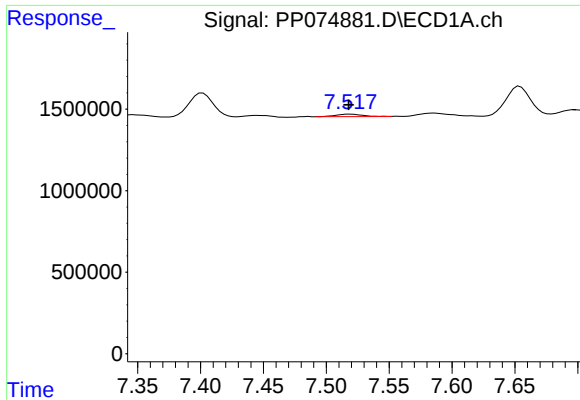

#29 AR-1254-4


R.T.: 7.519 min
Delta R.T.: 0.001 min
Response: 219883
Conc: 3.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

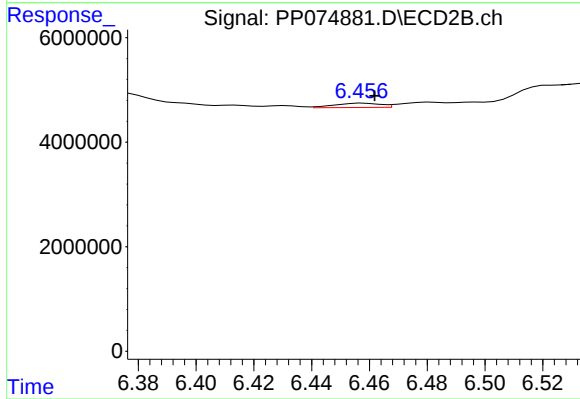


#29 AR-1254-4

R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 915800
Conc: 1.95 ng/ml

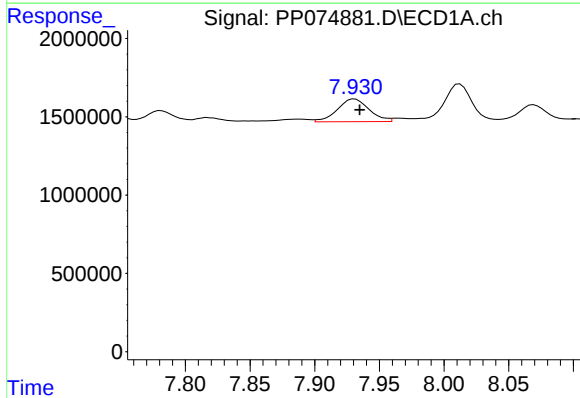


#30 AR-1254-5

R.T.: 7.931 min
Delta R.T.: -0.004 min
Response: 2479478
Conc: 29.84 ng/ml

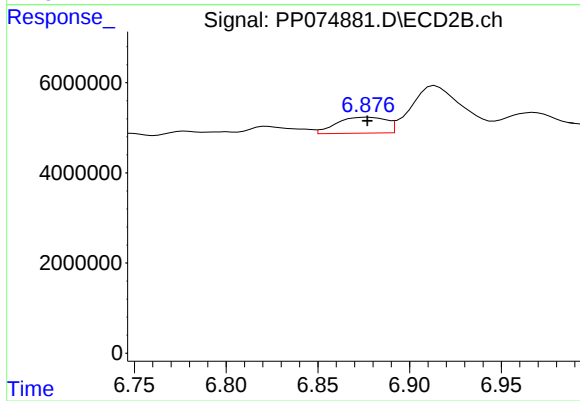

#30 AR-1254-5


R.T.: 6.877 min
Delta R.T.: 0.000 min
Response: 6641778
Conc: 13.54 ng/ml

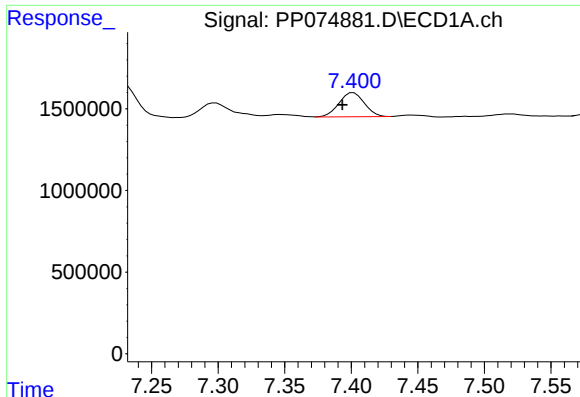

#31 AR-1260-1


R.T.: 7.402 min
Delta R.T.: 0.008 min
Response: 1962759
Conc: 33.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

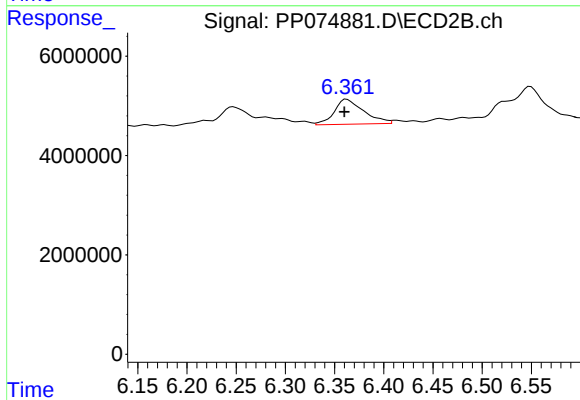


#31 AR-1260-1

R.T.: 6.362 min
Delta R.T.: 0.002 min
Response: 10550855
Conc: 28.12 ng/ml

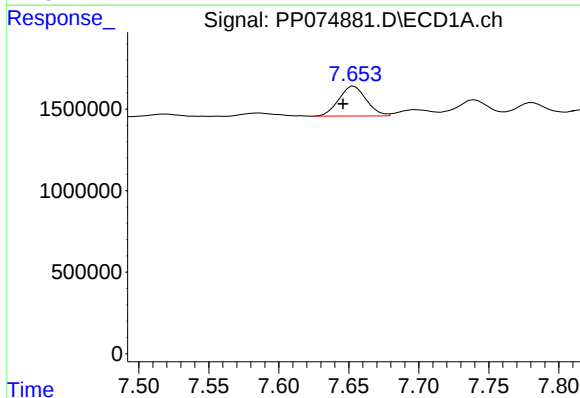


#32 AR-1260-2

R.T.: 7.654 min
Delta R.T.: 0.008 min
Response: 2484755
Conc: 36.05 ng/ml

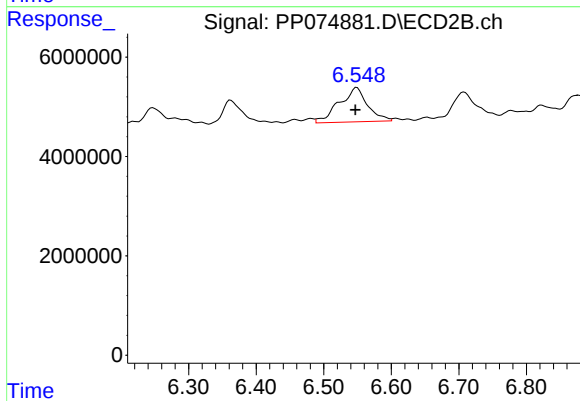

#32 AR-1260-2


R.T.: 6.549 min
Delta R.T.: 0.002 min
Response: 20097018
Conc: 38.00 ng/ml

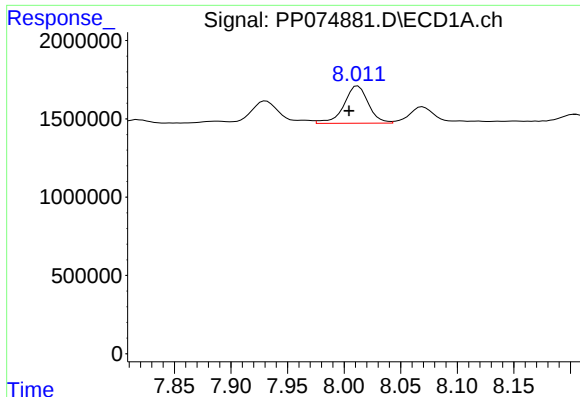

#33 AR-1260-3


R.T.: 8.012 min
Delta R.T.: 0.008 min
Response: 3585722
Conc: 69.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

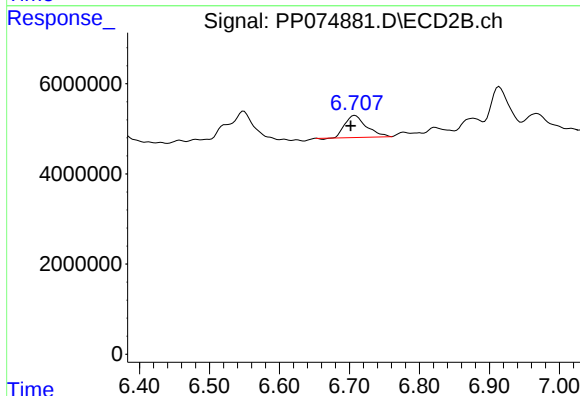


#33 AR-1260-3

R.T.: 6.708 min
Delta R.T.: 0.006 min
Response: 10340935
Conc: 23.88 ng/ml

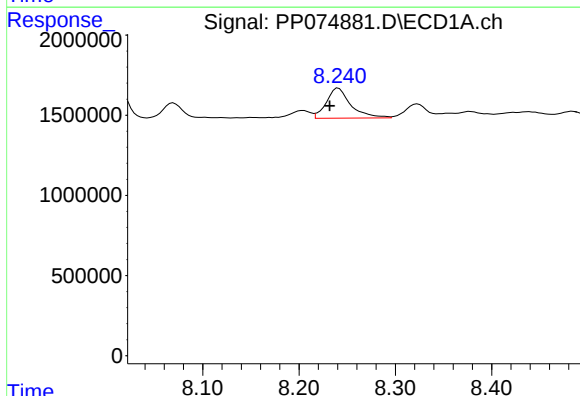


#34 AR-1260-4

R.T.: 8.241 min
Delta R.T.: 0.009 min
Response: 3323803
Conc: 52.10 ng/ml

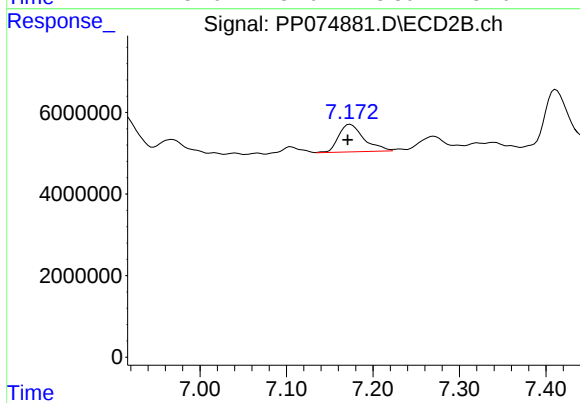

#34 AR-1260-4


R.T.: 7.174 min
Delta R.T.: 0.003 min
Response: 13692123
Conc: 35.89 ng/ml

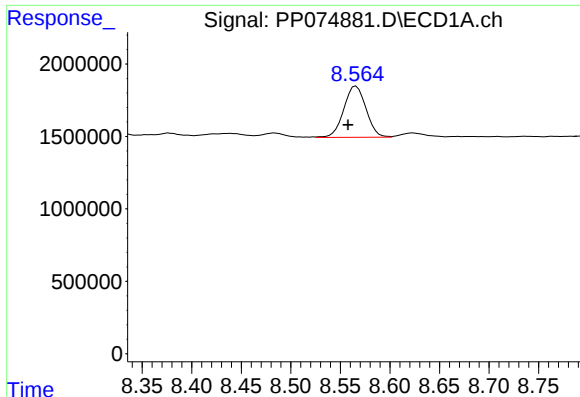

#35 AR-1260-5


R.T.: 8.566 min
Delta R.T.: 0.008 min
Response: 5530242
Conc: 48.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

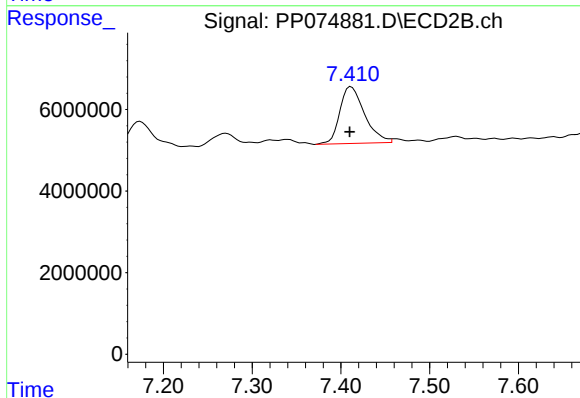


#35 AR-1260-5

R.T.: 7.412 min
Delta R.T.: 0.002 min
Response: 27011977
Conc: 26.89 ng/ml

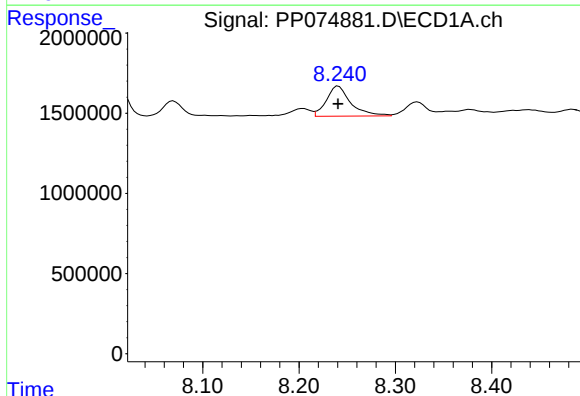


#36 AR-1262-1

R.T.: 8.241 min
Delta R.T.: 0.000 min
Response: 3323803
Conc: 43.16 ng/ml

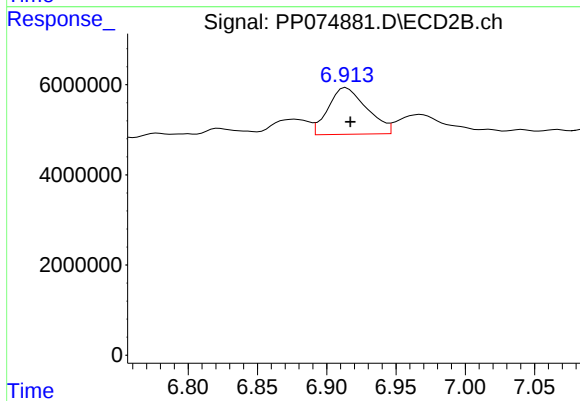

#36 AR-1262-1


R.T.: 6.914 min
Delta R.T.: -0.003 min
Response: 20048793
Conc: 28.35 ng/ml

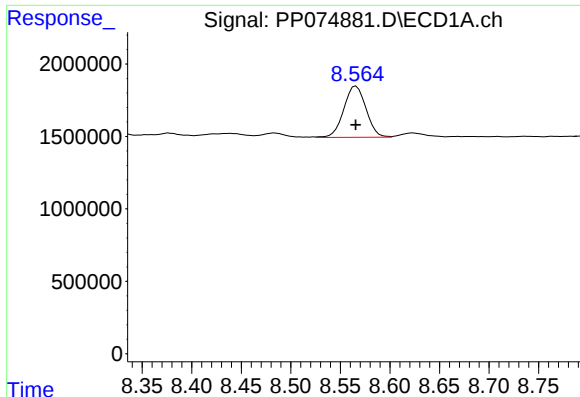

#37 AR-1262-2


R.T.: 8.566 min
Delta R.T.: 0.000 min
Response: 5530242
Conc: 41.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

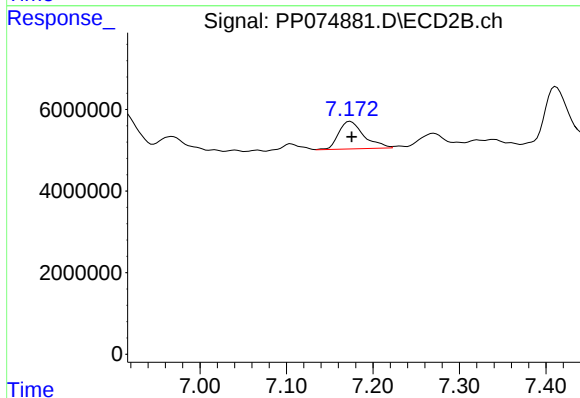


#37 AR-1262-2

R.T.: 7.174 min
Delta R.T.: -0.002 min
Response: 13692123
Conc: 26.29 ng/ml

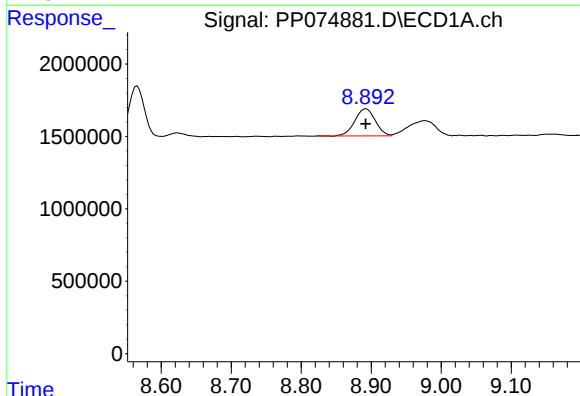


#38 AR-1262-3

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 3821810
Conc: 39.31 ng/ml

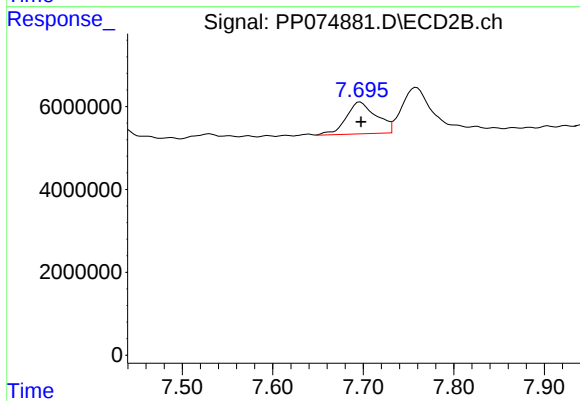

#38 AR-1262-3


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 17745727
Conc: 38.06 ng/ml

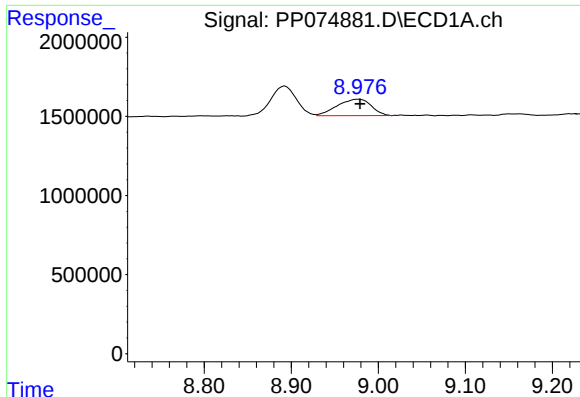

#39 AR-1262-4


R.T.: 8.977 min
Delta R.T.: -0.002 min
Response: 2838877
Conc: 37.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

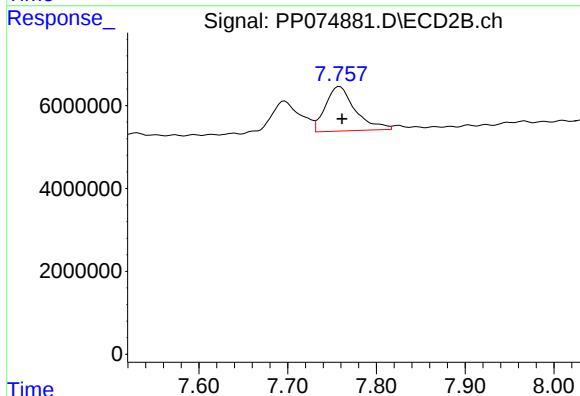


#39 AR-1262-4

R.T.: 7.759 min
Delta R.T.: -0.003 min
Response: 24968569
Conc: 30.38 ng/ml

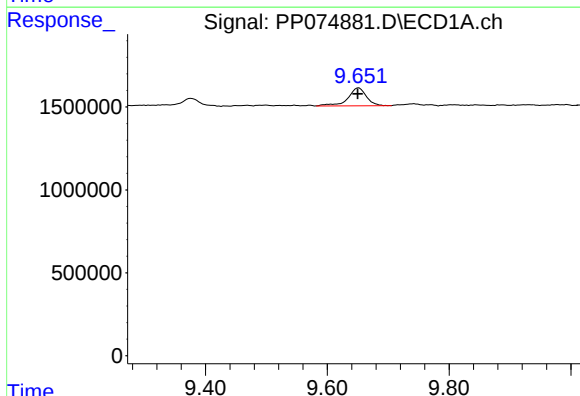


#40 AR-1262-5

R.T.: 9.652 min
Delta R.T.: 0.002 min
Response: 2270087
Conc: 37.24 ng/ml

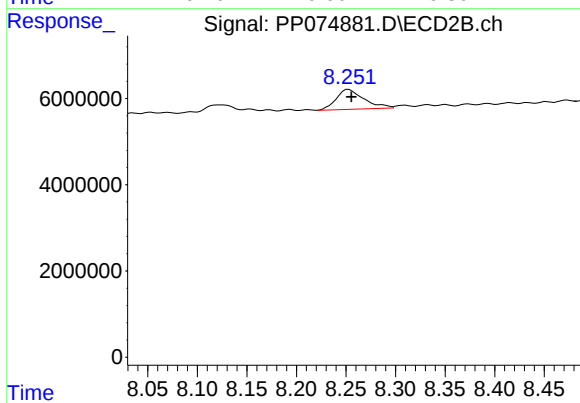

#40 AR-1262-5


R.T.: 8.253 min
Delta R.T.: -0.003 min
Response: 8975399
Conc: 25.05 ng/ml

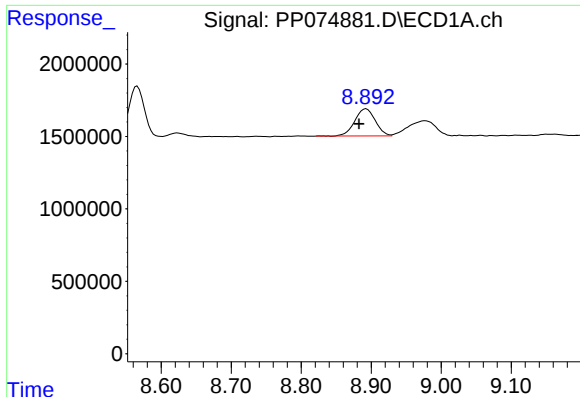

#41 AR-1268-1


R.T.: 8.893 min
Delta R.T.: 0.010 min
Response: 3821810
Conc: 23.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

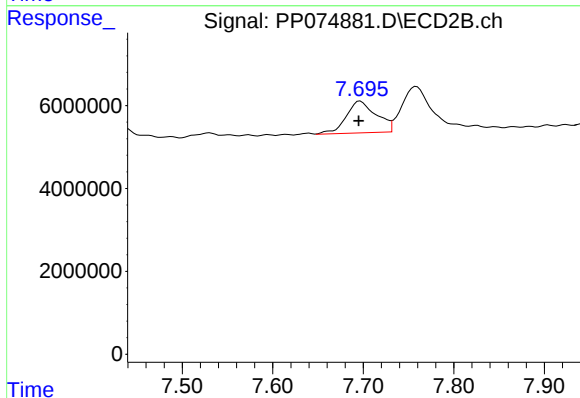


#41 AR-1268-1

R.T.: 7.697 min
Delta R.T.: 0.002 min
Response: 17745727
Conc: 12.58 ng/ml

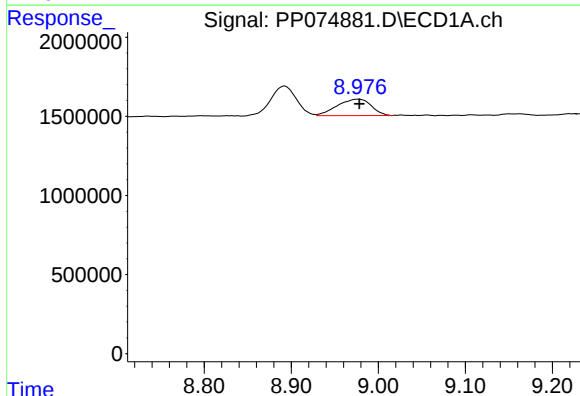


#42 AR-1268-2

R.T.: 8.977 min
Delta R.T.: 0.000 min
Response: 2838877
Conc: 19.35 ng/ml

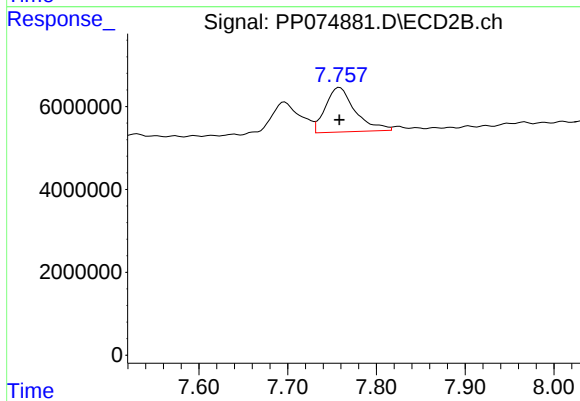

#42 AR-1268-2


R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 24968569
Conc: 18.31 ng/ml

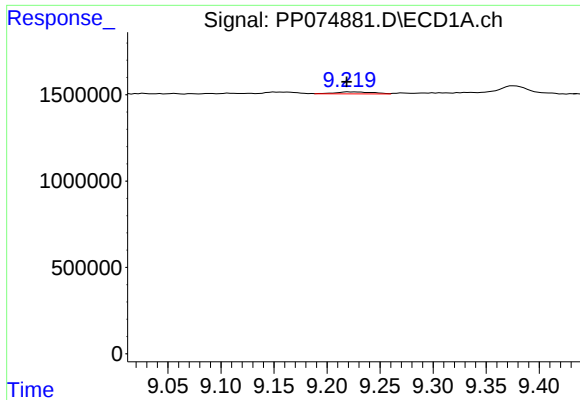

#43 AR-1268-3


R.T.: 9.220 min
Delta R.T.: 0.001 min
Response: 277872
Conc: 2.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

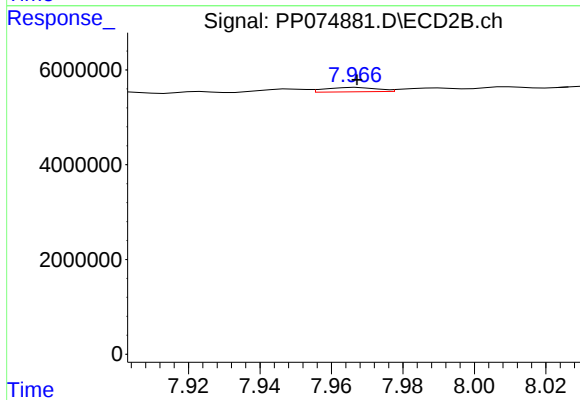


#43 AR-1268-3

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 914153
Conc: 0.88 ng/ml

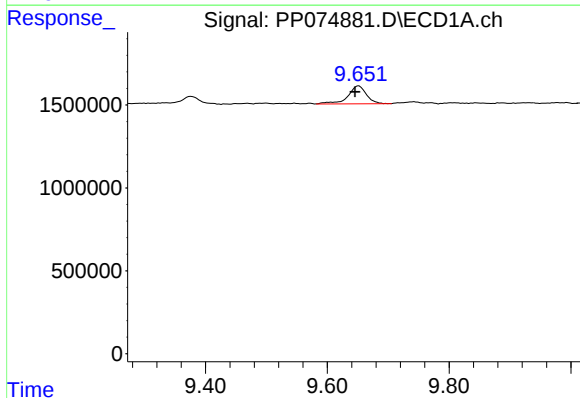


#44 AR-1268-4

R.T.: 9.652 min
Delta R.T.: 0.006 min
Response: 2270087
Conc: 33.75 ng/ml

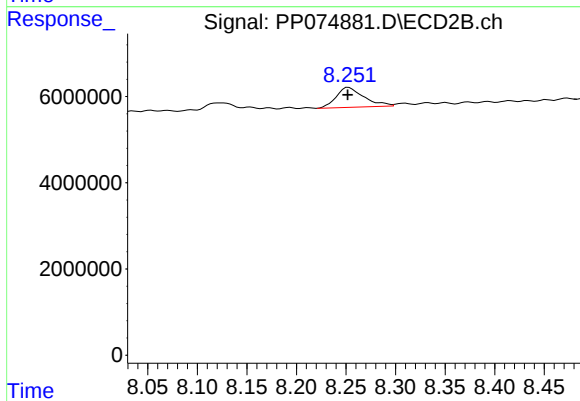

#44 AR-1268-4


R.T.: 8.253 min
Delta R.T.: 0.000 min
Response: 8975399
Conc: 23.43 ng/ml

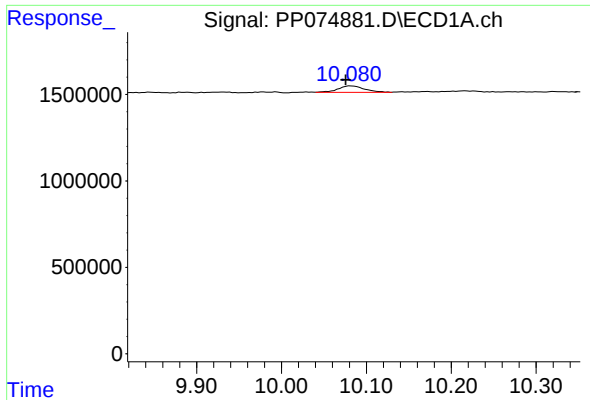

#45 AR-1268-5

R.T.: 10.082 min
Delta R.T.: 0.006 min
Response: 794349
Conc: 2.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
LOD-MDL-WATER-01-QT3-2025

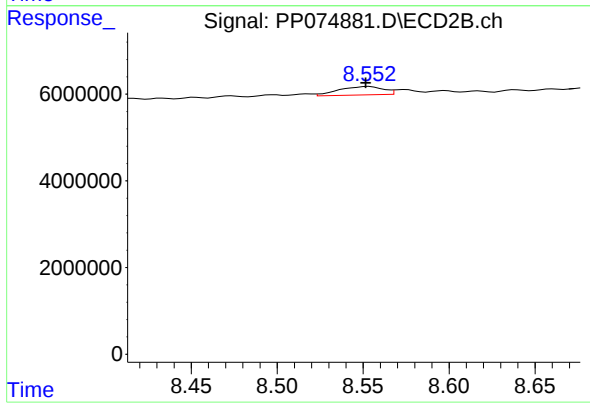

#45 AR-1268-5

R.T.: 8.553 min
Delta R.T.: 0.002 min
Response: 3476677
Conc: 1.11 ng/ml