

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 20:12
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1660 WATER MDL 25PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:43:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.659	3.800	27114459	99154844	22.158	20.506
2)	SA Decachlor...	10.436	8.809	21783286	136.6E6	22.059	18.220
Target Compounds							
3)	L1 AR-1016-1	5.809	4.896	1421656	11832725	32.245	23.231 #
4)	L1 AR-1016-2	5.832	4.953	2136054	5118574	33.991	21.505 #
5)	L1 AR-1016-3	5.895	5.079	1573148	3055586	35.026	22.157 #
6)	L1 AR-1016-4	5.991	5.117	1195022	3588289	33.967	25.667
7)	L1 AR-1016-5	6.284	5.332	1119817	4995210	33.744	30.077
8)	L2 AR-1221-1	4.856	4.021	657986	446891	37.401	7.223 #
9)	L2 AR-1221-2	4.959	4.090	727351	1248855	54.454	27.622 #
10)	L2 AR-1221-3	5.019	4.168	758742	2137715	20.013	13.012 #
11)	L3 AR-1232-1	5.019	4.168	758742	2137715	24.980	16.688 #
12)	L3 AR-1232-2	5.546	4.896	1015660	11832725	64.453	51.049
13)	L3 AR-1232-3	5.832	5.079	2136054	3055586	69.934	50.876 #
14)	L3 AR-1232-4	5.991	5.157	1195022	3964867	69.199	53.792
15)	L3 AR-1232-5	6.082	5.332	1109690	4995210	85.486	80.459
16)	L4 AR-1242-1	5.809	4.896	1421656	11832725	37.143	28.056
17)	L4 AR-1242-2	5.832	4.953	2136054	5118574	37.818	25.557 #
18)	L4 AR-1242-3	5.895	5.079	1573148	3055586	38.745	25.830 #
19)	L4 AR-1242-4	5.991	5.157	1195022	3964867	37.648	23.165 #
20)	L4 AR-1242-5	6.725	5.684	1204952	6216768	33.405	33.574
21)	L5 AR-1248-1	5.809	4.896	1421656	11832725	47.037	42.850
22)	L5 AR-1248-2	6.082	5.117	1109690	3588289	25.749	20.301
23)	L5 AR-1248-3	6.284	5.157	1119817	3964867	23.977	17.451 #
24)	L5 AR-1248-4	6.679	5.332	640754	4995210	11.650	22.912 #
25)	L5 AR-1248-5	6.725	5.751	1204952	8594250	21.722	23.397
26)	L6 AR-1254-1	6.656	5.684	1651768	6216768	28.347	13.041 #
27)	L6 AR-1254-2	6.873	5.826	1103693	6026067	13.523	17.113 #
28)	L6 AR-1254-3	7.230	6.244	2143380	7544567	24.027	12.172 #
29)	L6 AR-1254-4	7.518	6.463	432360	1504879	6.559	3.211 #
30)	L6 AR-1254-5	7.932	6.871	3095101	9584099	37.252	19.539 #
31)	L7 AR-1260-1	7.401	6.361	1683876	8257672	29.128	22.007
32)	L7 AR-1260-2	7.653	6.545	2404031	15531513	34.883	29.370
33)	L7 AR-1260-3	8.011	6.701	1908473	10807969	36.783	24.961 #
34)	L7 AR-1260-4	8.239	7.169	2621517	8179320	41.094	21.441 #
35)	L7 AR-1260-5	8.564	7.408	3814942	18696683	33.638	18.613 #
36)	L8 AR-1262-1	8.239	6.909	2621517	11187004	34.039	15.817 #
37)	L8 AR-1262-2	8.564	7.169	3814942	8179320	28.818	15.708 #
38)	L8 AR-1262-3	8.896	7.693	2423516	11027269	24.930	23.649
39)	L8 AR-1262-4	8.969	7.754	1471169	18419865	19.530	22.412
40)	L8 AR-1262-5	9.649	8.247	1177831	4203962	19.323	11.733 #
41)	L9 AR-1268-1	8.896	7.693	2423516	11027269	14.956	7.818 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074919.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 20:12
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1660 WATER MDL 25PPB
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:43:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.969	7.754	1471169	18419865	10.026	13.510 #
43) L9	AR-1268-3	9.155f	7.974	146663	934563	1.187	0.896
44) L9	AR-1268-4	9.649	8.247	1177831	4203962	17.511	10.974 #
45) L9	AR-1268-5	10.081	8.554	422491	860236	1.141	0.274 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
Data File : PP074919.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 20:12
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1660 WATER MDL 25PPB
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:43:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

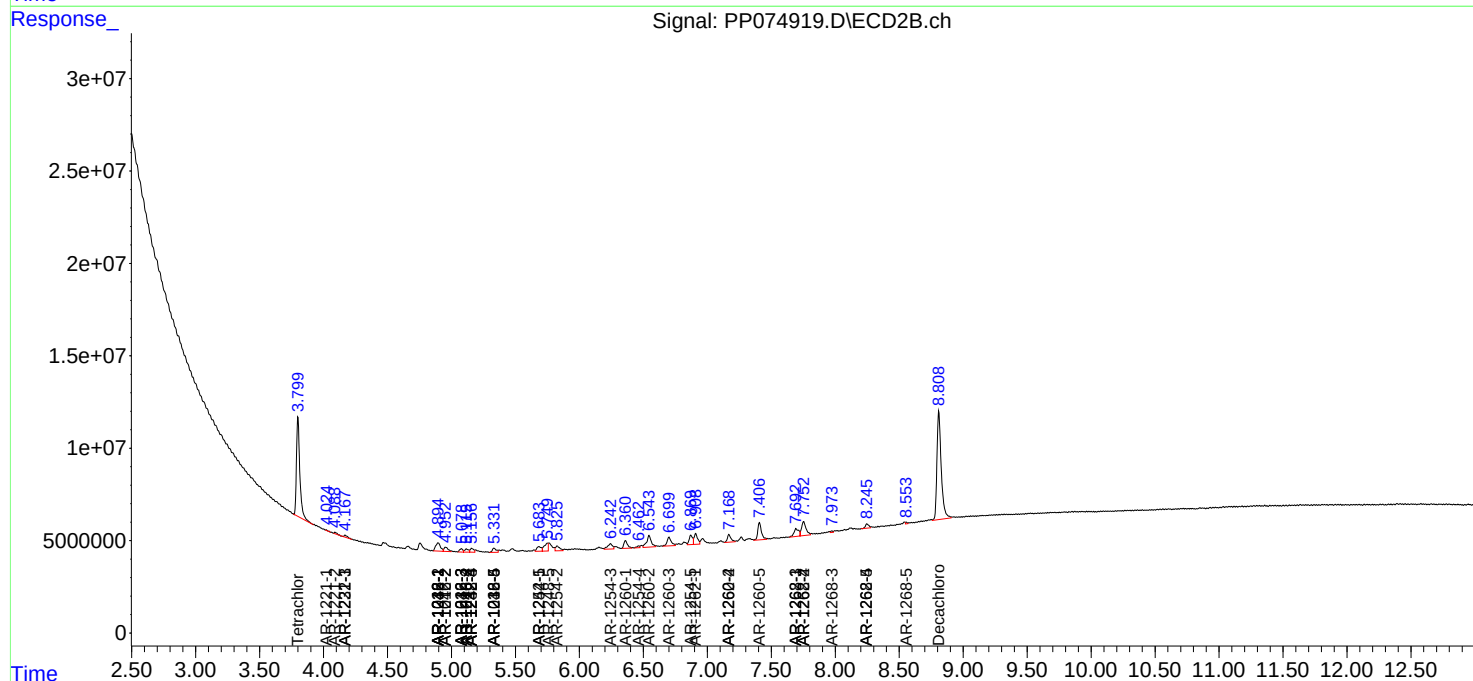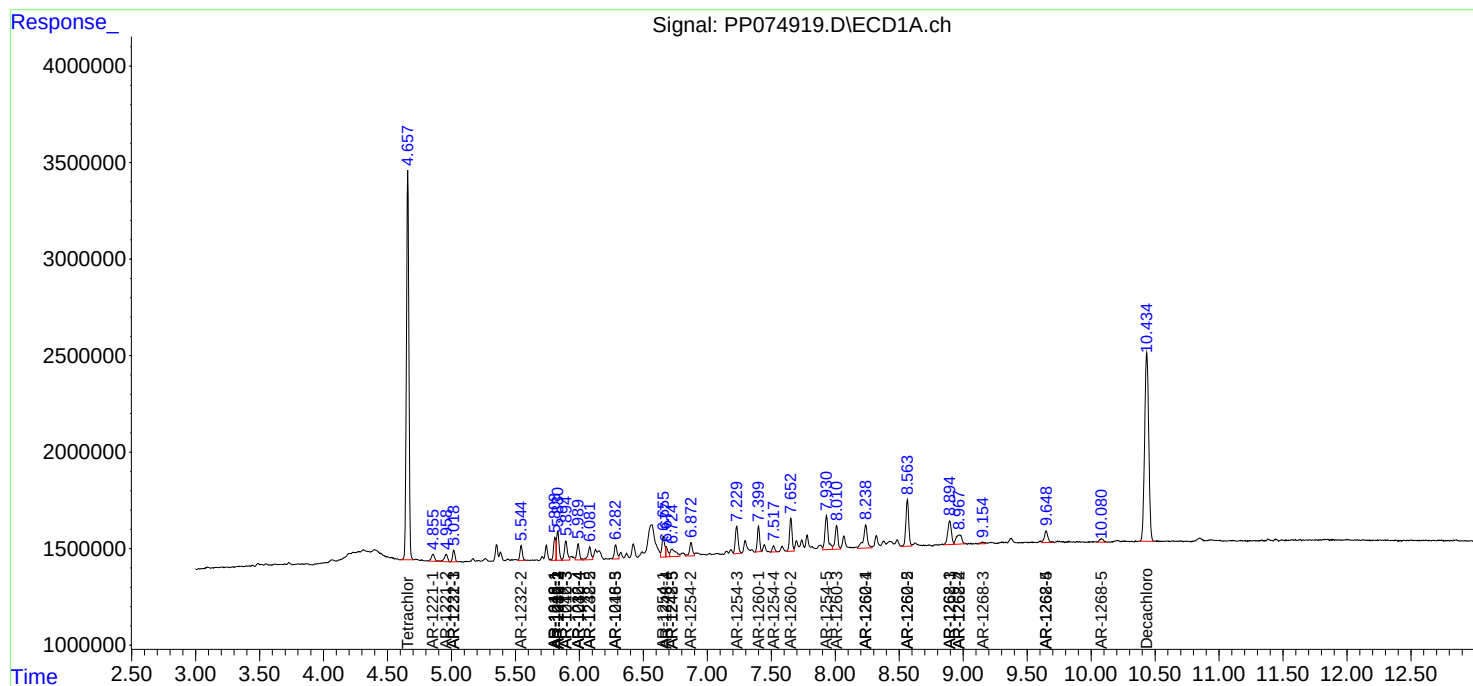


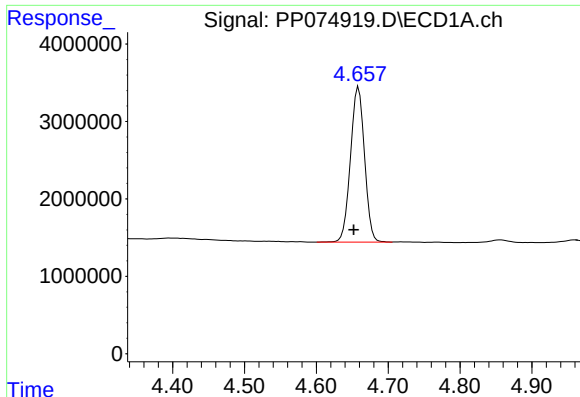

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.007 min
Response: 27114459
Conc: 22.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

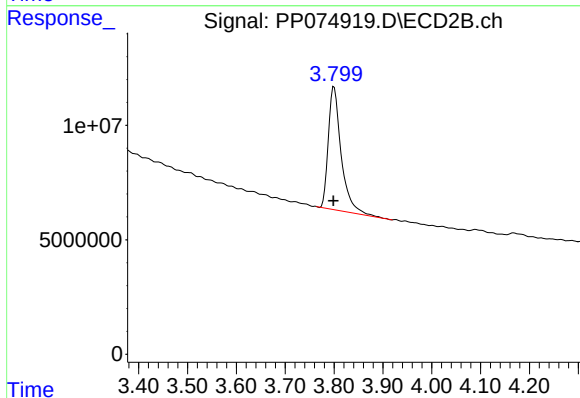


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.001 min
Response: 99154844
Conc: 20.51 ng/ml

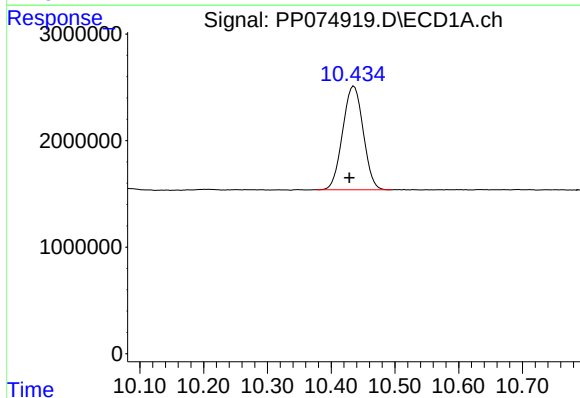


#2 Decachlorobiphenyl

R.T.: 10.436 min
Delta R.T.: 0.007 min
Response: 21783286
Conc: 22.06 ng/ml

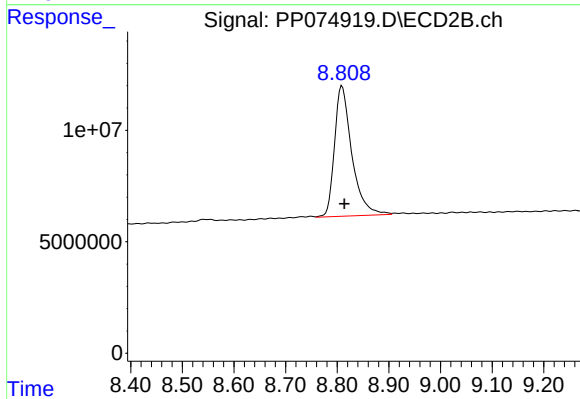

#2 Decachlorobiphenyl


R.T.: 8.809 min
Delta R.T.: -0.005 min
Response: 136632103
Conc: 18.22 ng/ml

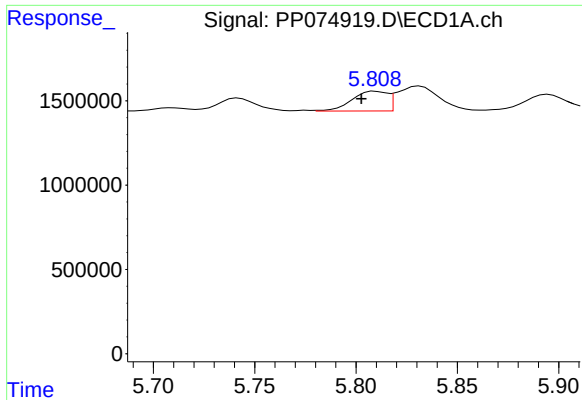

#3 AR-1016-1


R.T.: 5.809 min
Delta R.T.: 0.007 min
Response: 1421656
Conc: 32.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

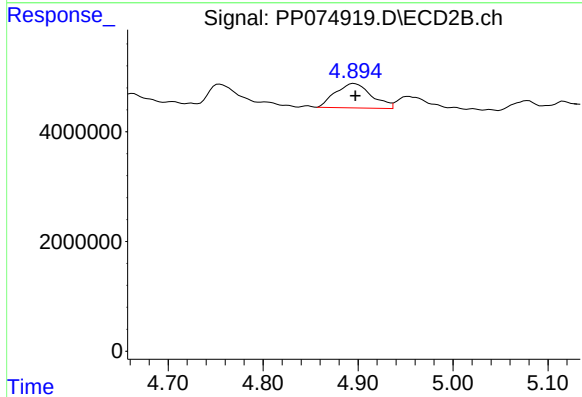


#3 AR-1016-1

R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 11832725
Conc: 23.23 ng/ml

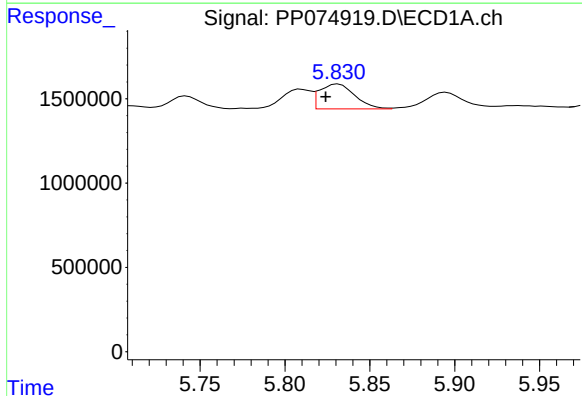


#4 AR-1016-2

R.T.: 5.832 min
Delta R.T.: 0.007 min
Response: 2136054
Conc: 33.99 ng/ml

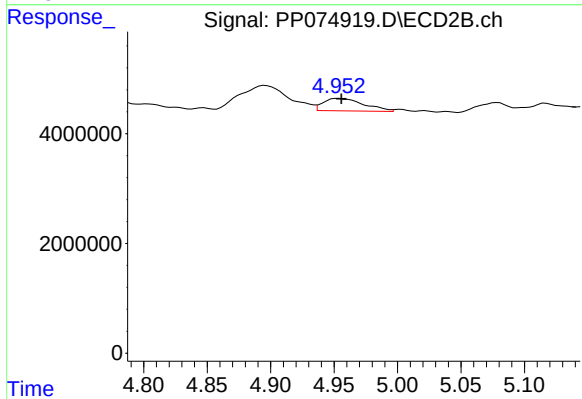

#4 AR-1016-2


R.T.: 4.953 min
Delta R.T.: -0.003 min
Response: 5118574
Conc: 21.51 ng/ml

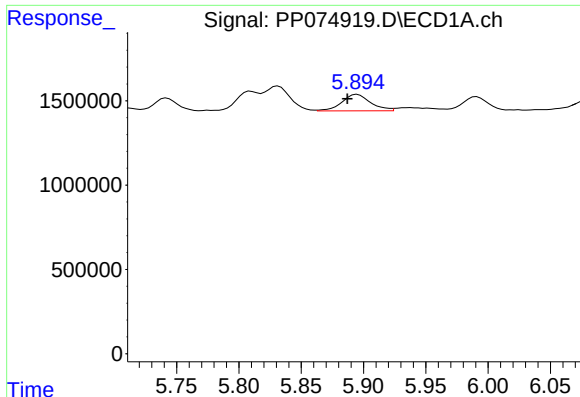

#5 AR-1016-3


R.T.: 5.895 min
Delta R.T.: 0.008 min
Response: 1573148
Conc: 35.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

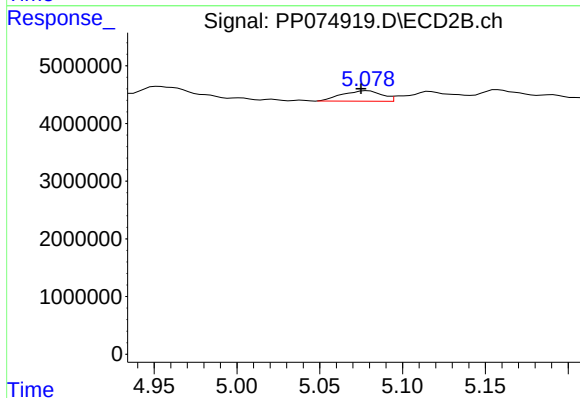


#5 AR-1016-3

R.T.: 5.079 min
Delta R.T.: 0.004 min
Response: 3055586
Conc: 22.16 ng/ml

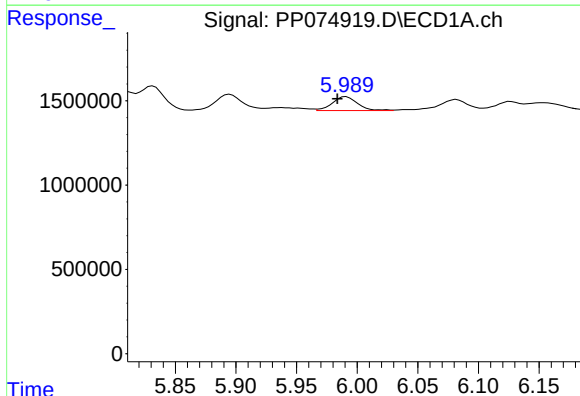


#6 AR-1016-4

R.T.: 5.991 min
Delta R.T.: 0.007 min
Response: 1195022
Conc: 33.97 ng/ml

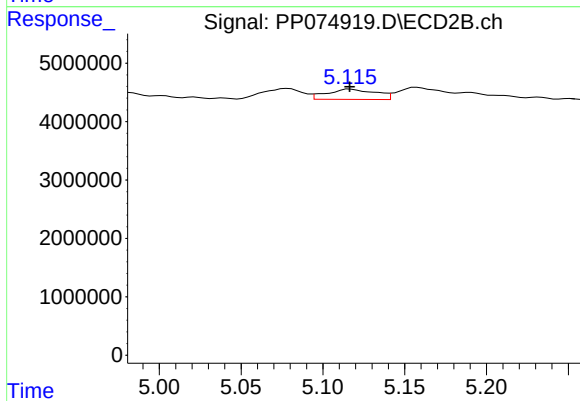

#6 AR-1016-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 3588289
Conc: 25.67 ng/ml

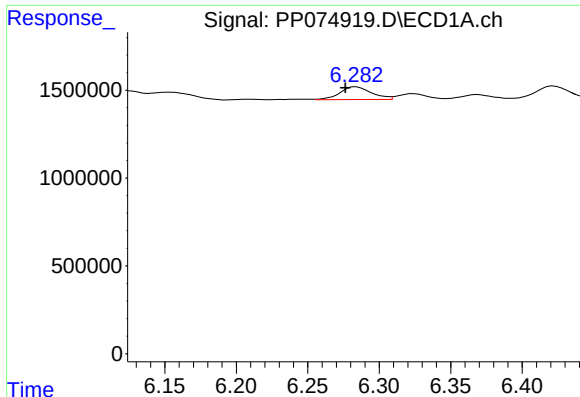

#7 AR-1016-5


R.T.: 6.284 min
Delta R.T.: 0.007 min
Response: 1119817
Conc: 33.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

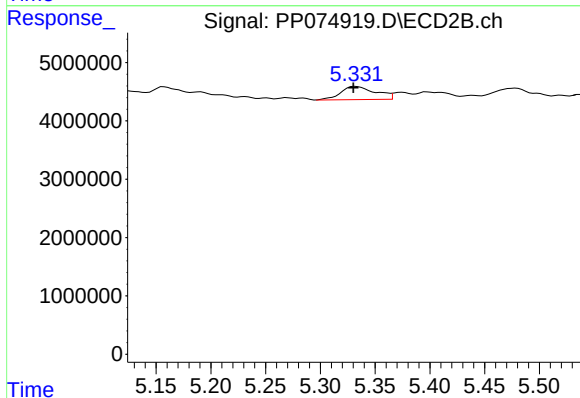


#7 AR-1016-5

R.T.: 5.332 min
Delta R.T.: 0.002 min
Response: 4995210
Conc: 30.08 ng/ml

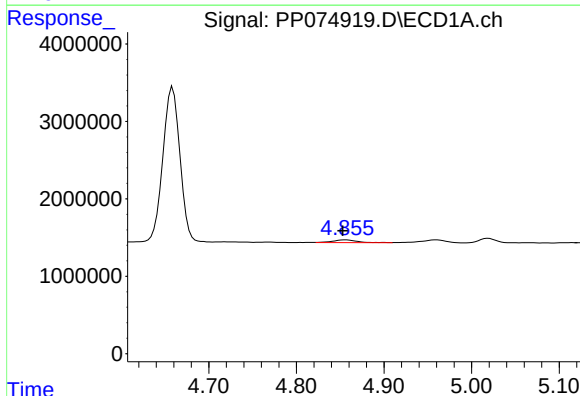


#8 AR-1221-1

R.T.: 4.856 min
Delta R.T.: 0.003 min
Response: 657986
Conc: 37.40 ng/ml

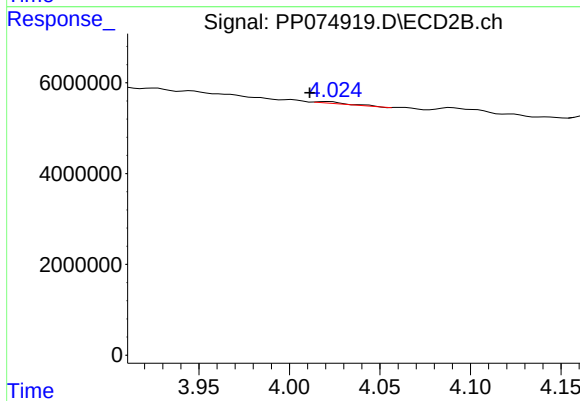

#8 AR-1221-1


R.T.: 4.021 min
Delta R.T.: 0.010 min
Response: 446891
Conc: 7.22 ng/ml

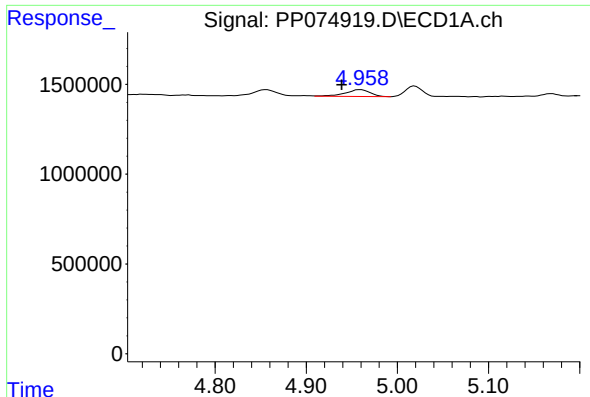

#9 AR-1221-2


R.T.: 4.959 min
Delta R.T.: 0.020 min
Response: 727351
Conc: 54.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

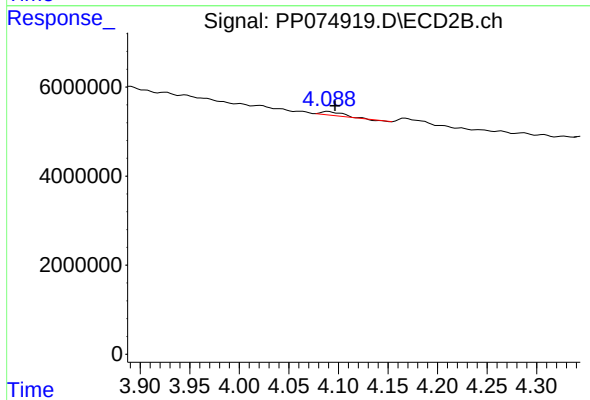


#9 AR-1221-2

R.T.: 4.090 min
Delta R.T.: -0.007 min
Response: 1248855
Conc: 27.62 ng/ml

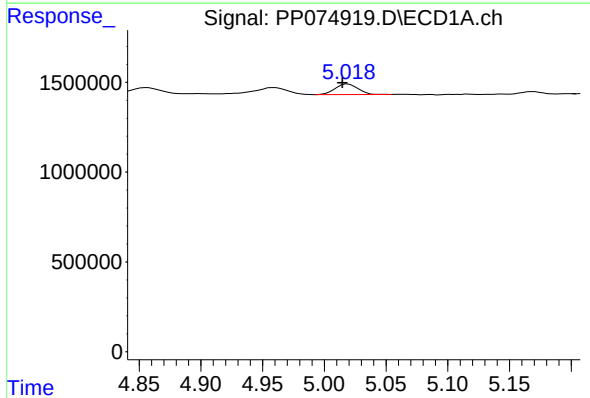


#10 AR-1221-3

R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 758742
Conc: 20.01 ng/ml

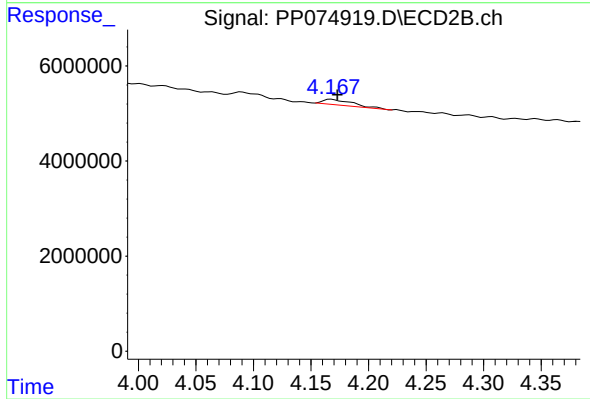

#10 AR-1221-3


R.T.: 4.168 min
Delta R.T.: -0.005 min
Response: 2137715
Conc: 13.01 ng/ml

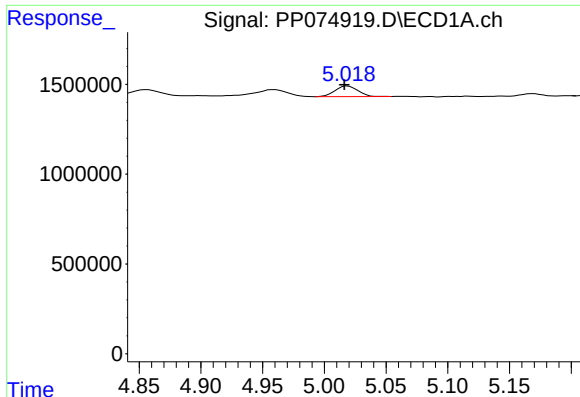

#11 AR-1232-1


R.T.: 5.019 min
Delta R.T.: 0.003 min
Response: 758742
Conc: 24.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

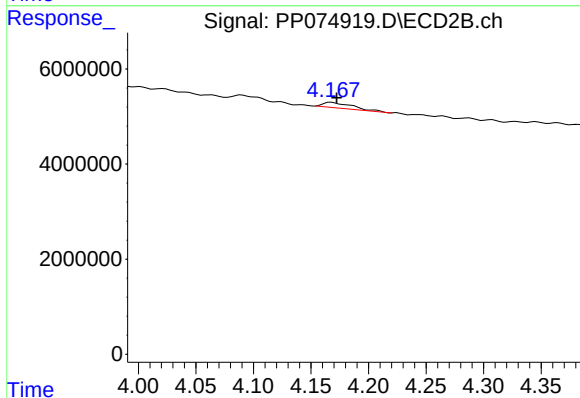


#11 AR-1232-1

R.T.: 4.168 min
Delta R.T.: -0.005 min
Response: 2137715
Conc: 16.69 ng/ml

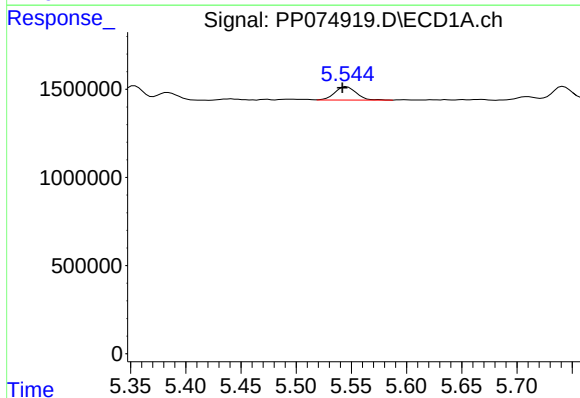


#12 AR-1232-2

R.T.: 5.546 min
Delta R.T.: 0.004 min
Response: 1015660
Conc: 64.45 ng/ml

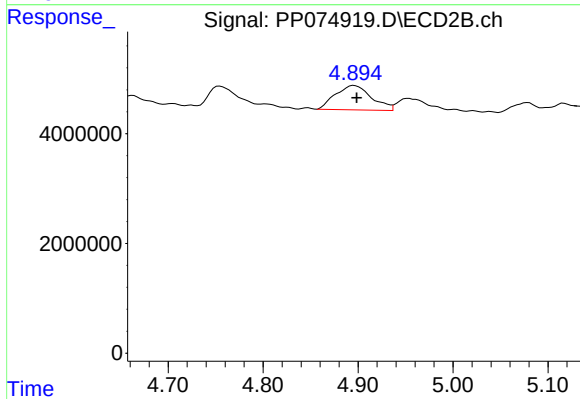

#12 AR-1232-2


R.T.: 4.896 min
Delta R.T.: -0.003 min
Response: 11832725
Conc: 51.05 ng/ml

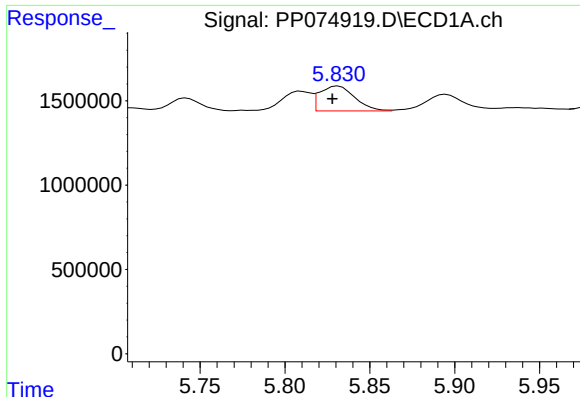

#13 AR-1232-3


R.T.: 5.832 min
Delta R.T.: 0.004 min
Response: 2136054
Conc: 69.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

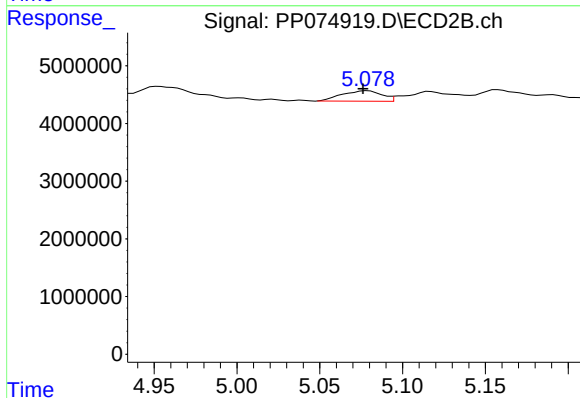


#13 AR-1232-3

R.T.: 5.079 min
Delta R.T.: 0.003 min
Response: 3055586
Conc: 50.88 ng/ml

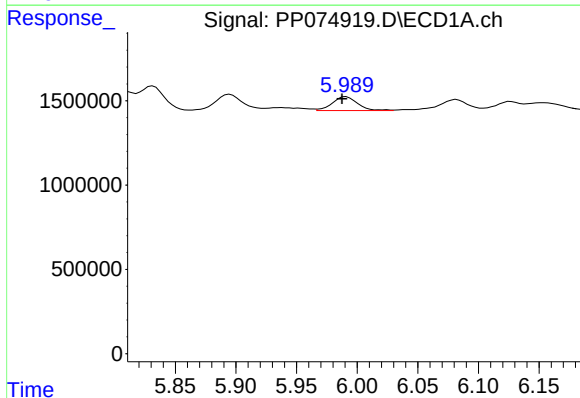


#14 AR-1232-4

R.T.: 5.991 min
Delta R.T.: 0.003 min
Response: 1195022
Conc: 69.20 ng/ml

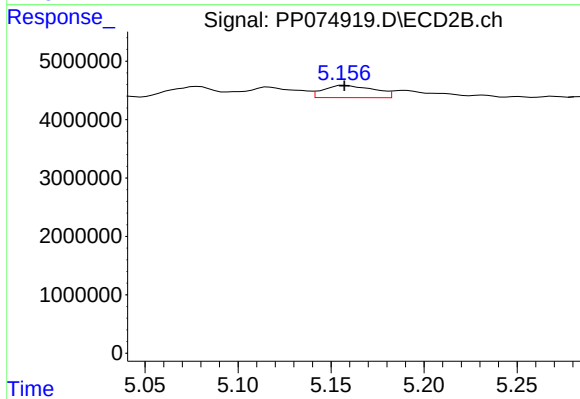

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 3964867
Conc: 53.79 ng/ml

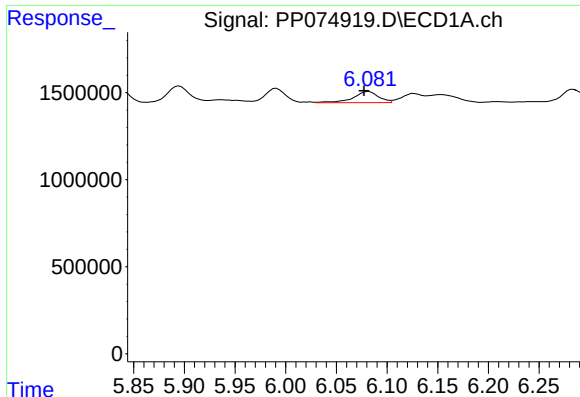

#15 AR-1232-5


R.T.: 6.082 min
Delta R.T.: 0.005 min
Response: 1109690
Conc: 85.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

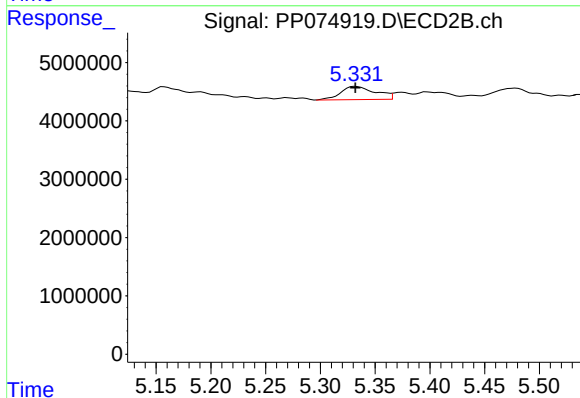


#15 AR-1232-5

R.T.: 5.332 min
Delta R.T.: 0.000 min
Response: 4995210
Conc: 80.46 ng/ml

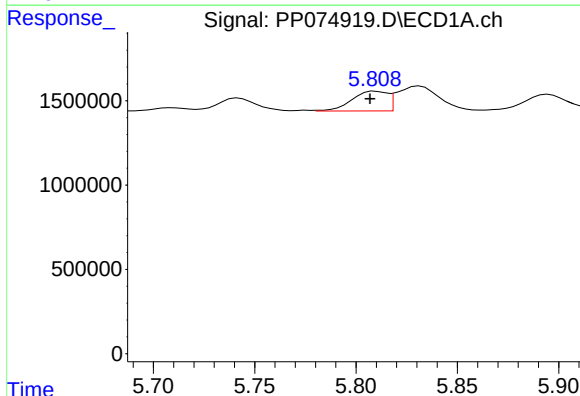


#16 AR-1242-1

R.T.: 5.809 min
Delta R.T.: 0.002 min
Response: 1421656
Conc: 37.14 ng/ml

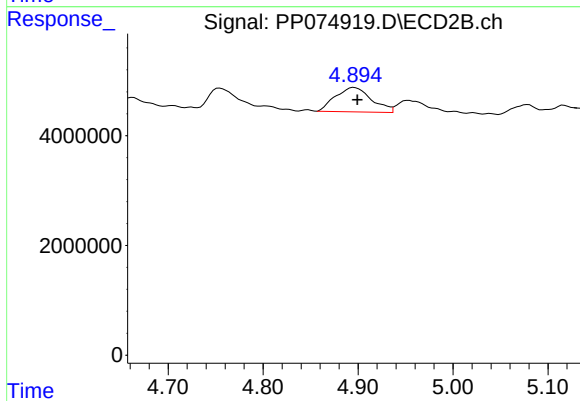

#16 AR-1242-1


R.T.: 4.896 min
Delta R.T.: -0.004 min
Response: 11832725
Conc: 28.06 ng/ml

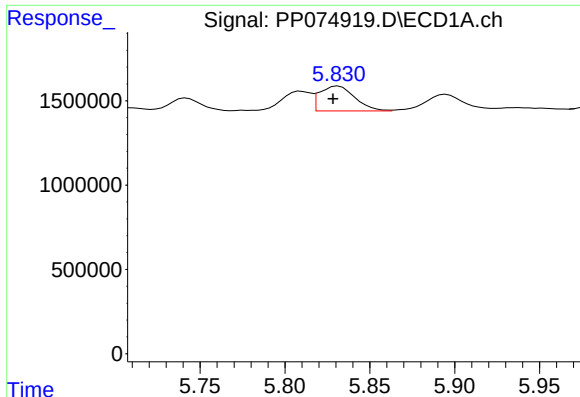

#17 AR-1242-2


R.T.: 5.832 min
Delta R.T.: 0.003 min
Response: 2136054
Conc: 37.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

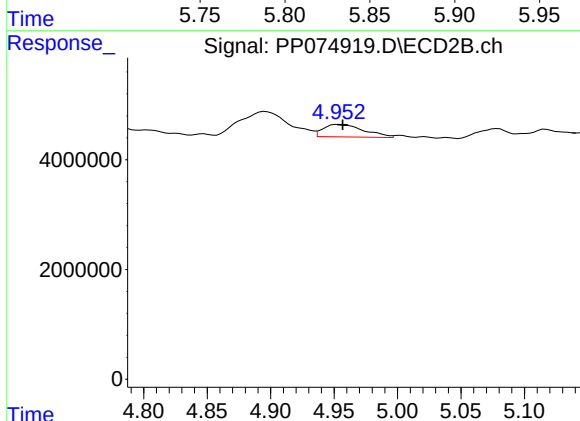


#17 AR-1242-2

R.T.: 4.953 min
Delta R.T.: -0.004 min
Response: 5118574
Conc: 25.56 ng/ml

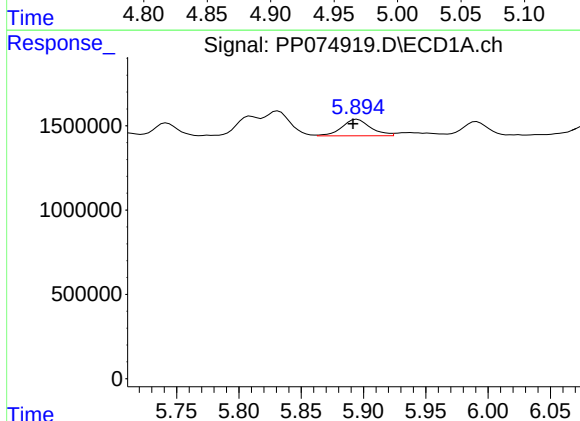


#18 AR-1242-3

R.T.: 5.895 min
Delta R.T.: 0.003 min
Response: 1573148
Conc: 38.74 ng/ml

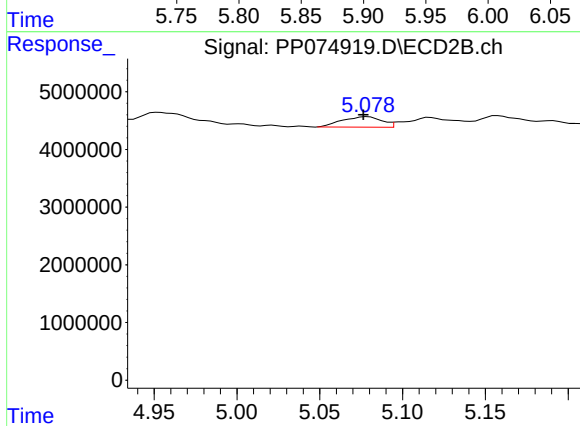

#18 AR-1242-3


R.T.: 5.079 min
Delta R.T.: 0.003 min
Response: 3055586
Conc: 25.83 ng/ml

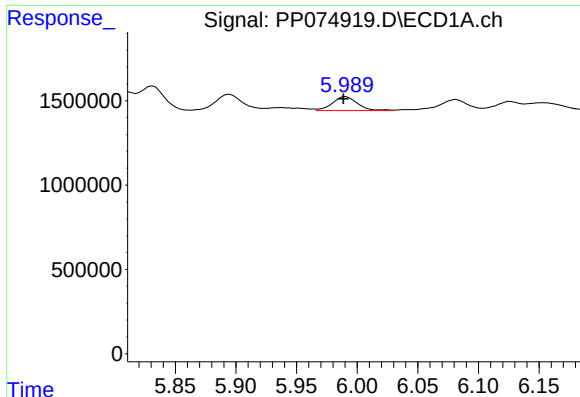

#19 AR-1242-4


R.T.: 5.991 min
Delta R.T.: 0.002 min
Response: 1195022
Conc: 37.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

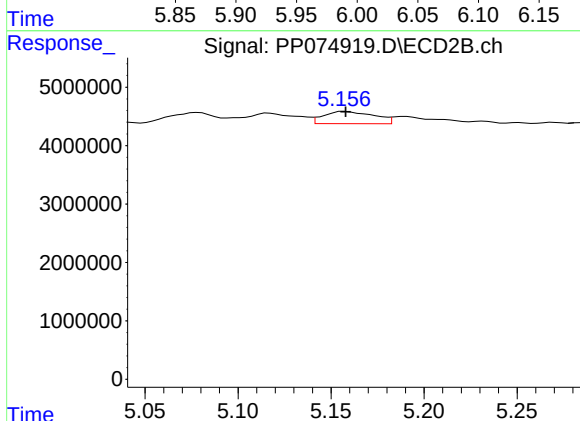


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 3964867
Conc: 23.16 ng/ml

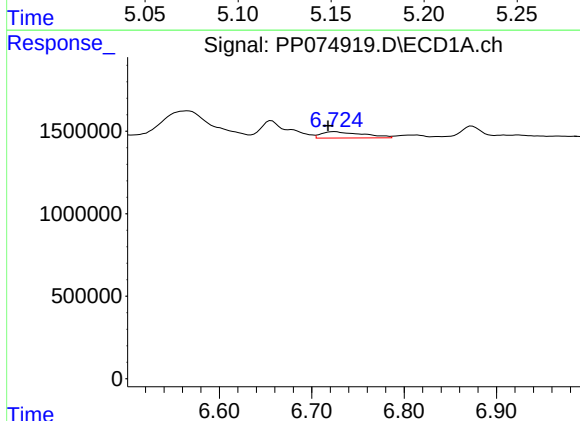


#20 AR-1242-5

R.T.: 6.725 min
Delta R.T.: 0.007 min
Response: 1204952
Conc: 33.41 ng/ml

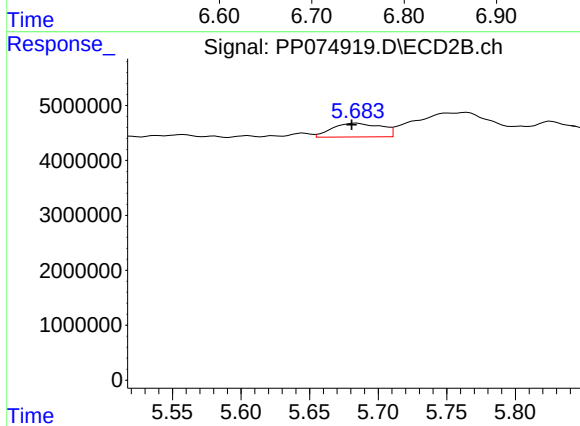

#20 AR-1242-5


R.T.: 5.684 min
Delta R.T.: 0.003 min
Response: 6216768
Conc: 33.57 ng/ml

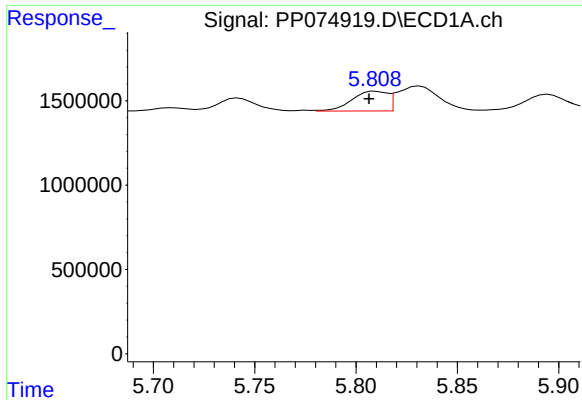

#21 AR-1248-1


R.T.: 5.809 min
Delta R.T.: 0.003 min
Response: 1421656
Conc: 47.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

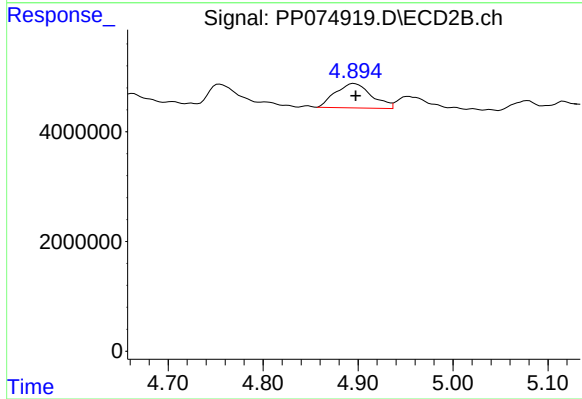


#21 AR-1248-1

R.T.: 4.896 min
Delta R.T.: -0.002 min
Response: 11832725
Conc: 42.85 ng/ml

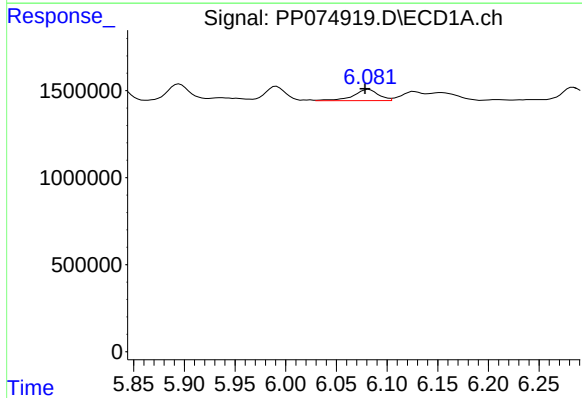


#22 AR-1248-2

R.T.: 6.082 min
Delta R.T.: 0.004 min
Response: 1109690
Conc: 25.75 ng/ml

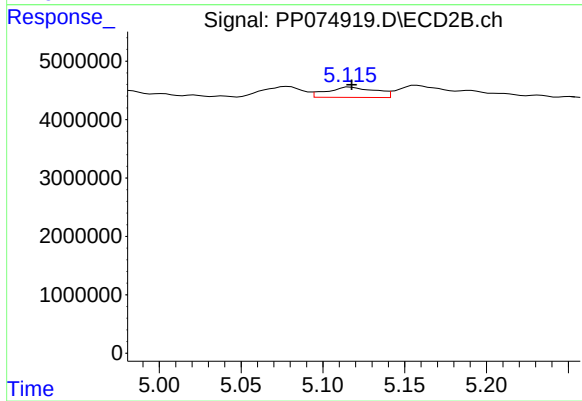

#22 AR-1248-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 3588289
Conc: 20.30 ng/ml

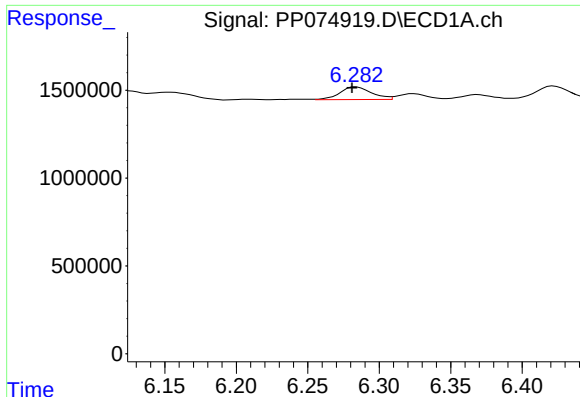

#23 AR-1248-3


R.T.: 6.284 min
Delta R.T.: 0.003 min
Response: 1119817
Conc: 23.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

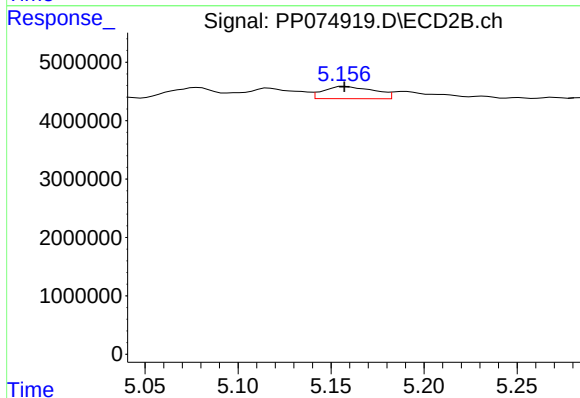


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 3964867
Conc: 17.45 ng/ml

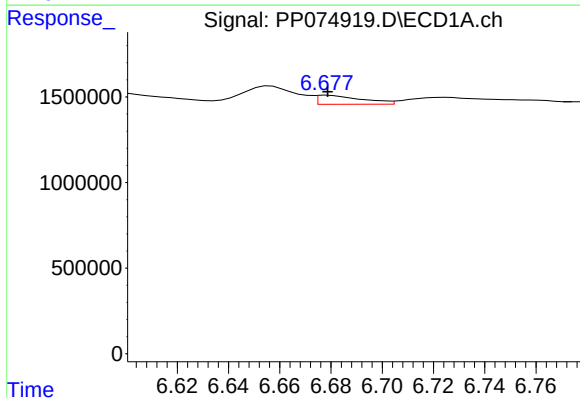


#24 AR-1248-4

R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 640754
Conc: 11.65 ng/ml

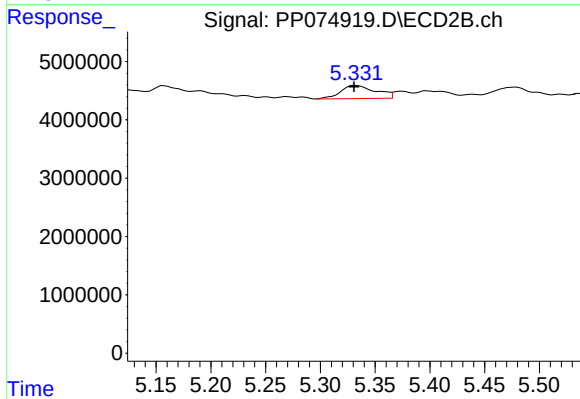

#24 AR-1248-4


R.T.: 5.332 min
Delta R.T.: 0.001 min
Response: 4995210
Conc: 22.91 ng/ml

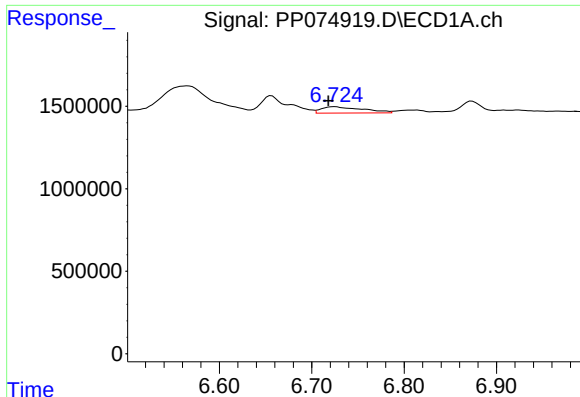

#25 AR-1248-5


R.T.: 6.725 min
Delta R.T.: 0.007 min
Response: 1204952
Conc: 21.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

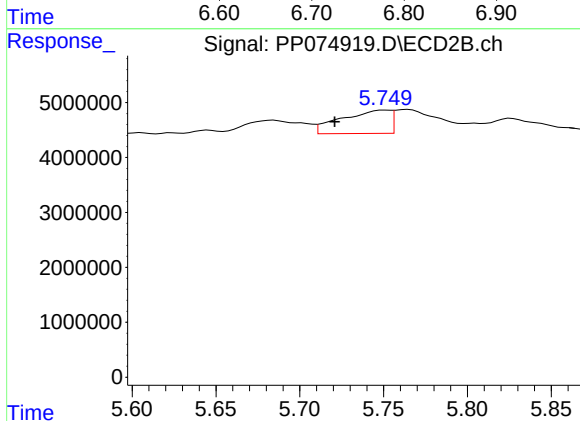


#25 AR-1248-5

R.T.: 5.751 min
Delta R.T.: 0.030 min
Response: 8594250
Conc: 23.40 ng/ml

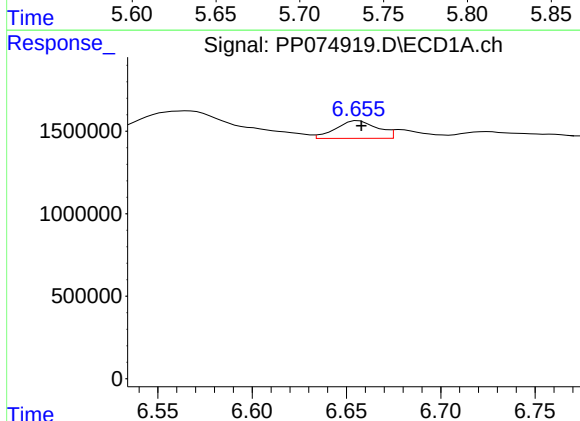


#26 AR-1254-1

R.T.: 6.656 min
Delta R.T.: -0.002 min
Response: 1651768
Conc: 28.35 ng/ml

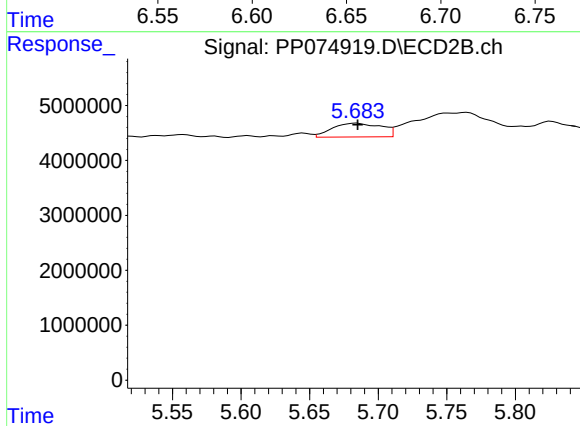

#26 AR-1254-1


R.T.: 5.684 min
Delta R.T.: 0.000 min
Response: 6216768
Conc: 13.04 ng/ml

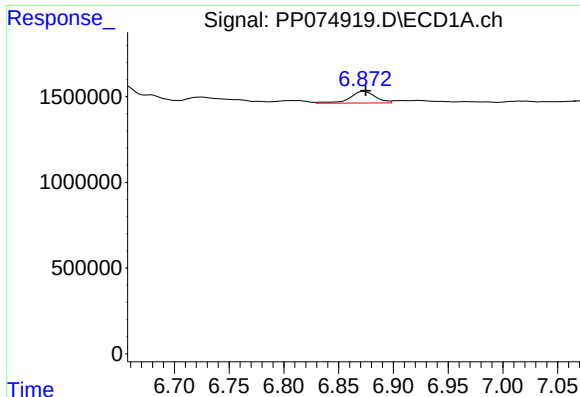

#27 AR-1254-2


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 1103693
Conc: 13.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

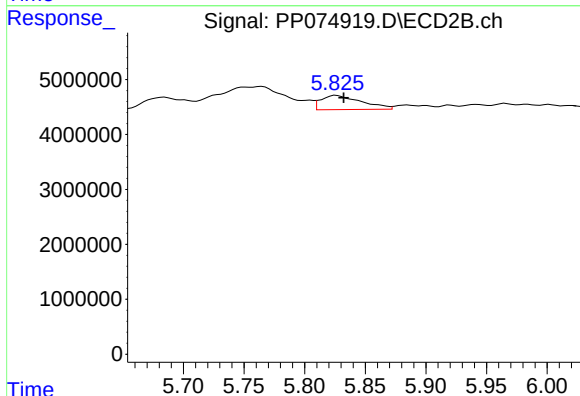


#27 AR-1254-2

R.T.: 5.826 min
Delta R.T.: -0.006 min
Response: 6026067
Conc: 17.11 ng/ml

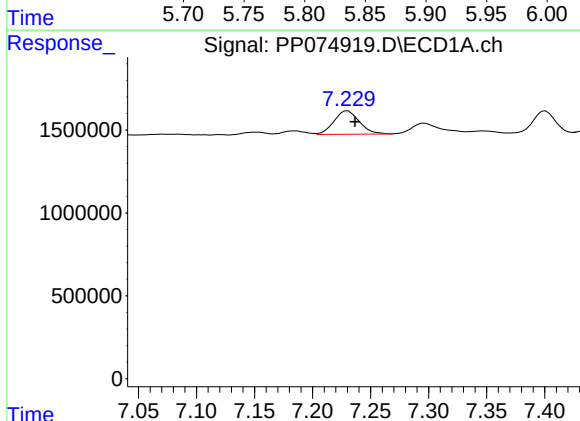


#28 AR-1254-3

R.T.: 7.230 min
Delta R.T.: -0.007 min
Response: 2143380
Conc: 24.03 ng/ml

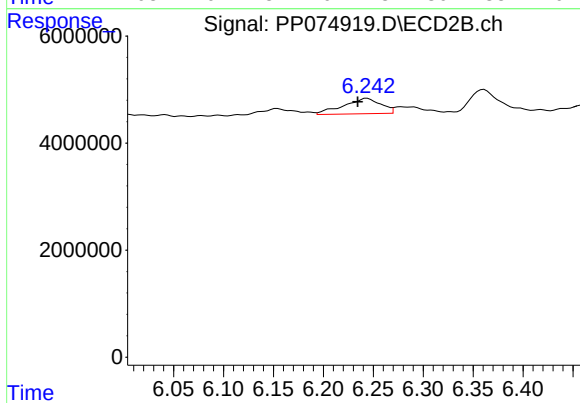

#28 AR-1254-3


R.T.: 6.244 min
Delta R.T.: 0.009 min
Response: 7544567
Conc: 12.17 ng/ml

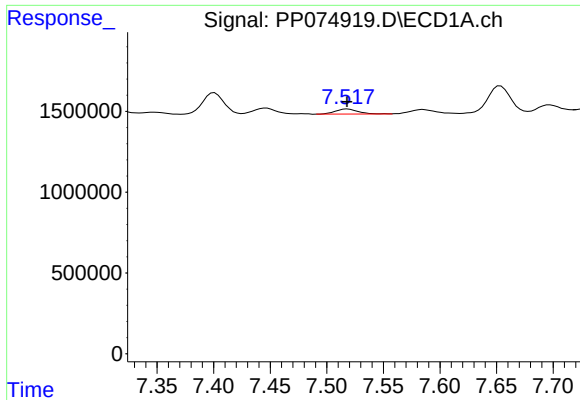

#29 AR-1254-4


R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 432360
Conc: 6.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

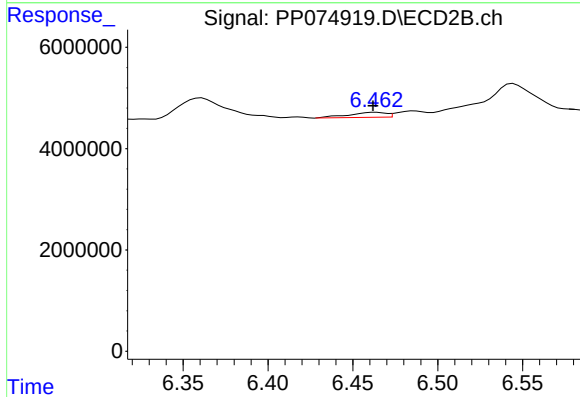


#29 AR-1254-4

R.T.: 6.463 min
Delta R.T.: 0.002 min
Response: 1504879
Conc: 3.21 ng/ml

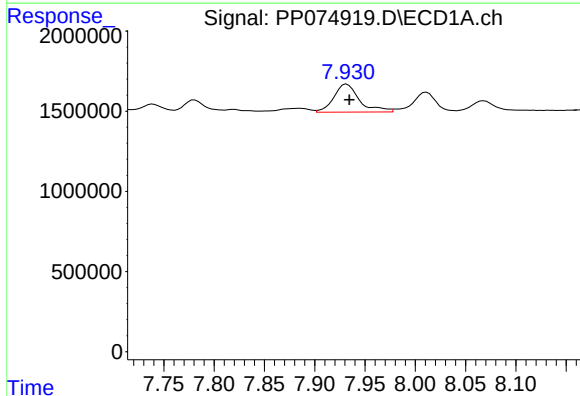


#30 AR-1254-5

R.T.: 7.932 min
Delta R.T.: -0.003 min
Response: 3095101
Conc: 37.25 ng/ml

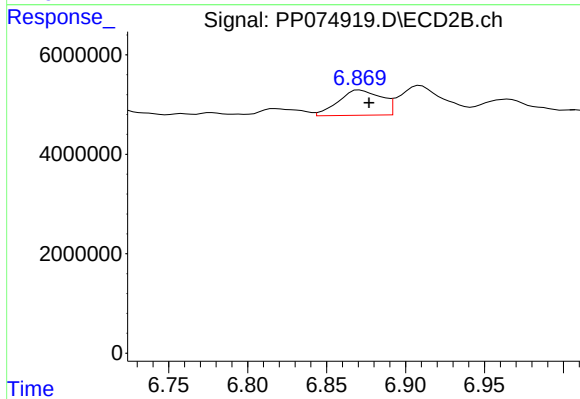

#30 AR-1254-5


R.T.: 6.871 min
Delta R.T.: -0.006 min
Response: 9584099
Conc: 19.54 ng/ml

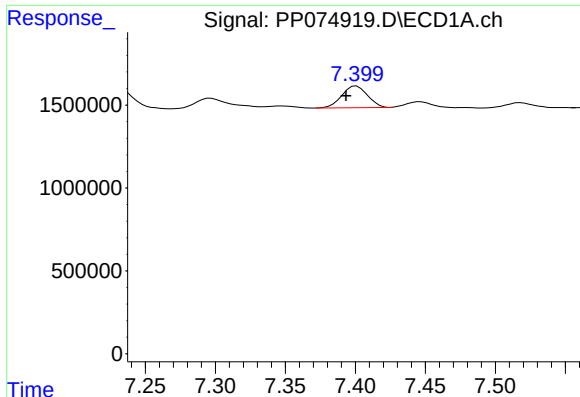

#31 AR-1260-1


R.T.: 7.401 min
Delta R.T.: 0.007 min
Response: 1683876
Conc: 29.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

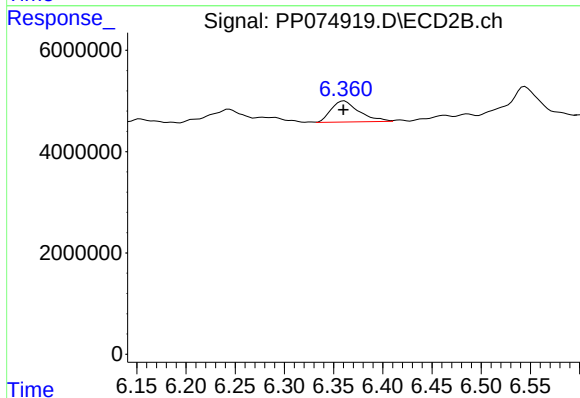


#31 AR-1260-1

R.T.: 6.361 min
Delta R.T.: 0.000 min
Response: 8257672
Conc: 22.01 ng/ml

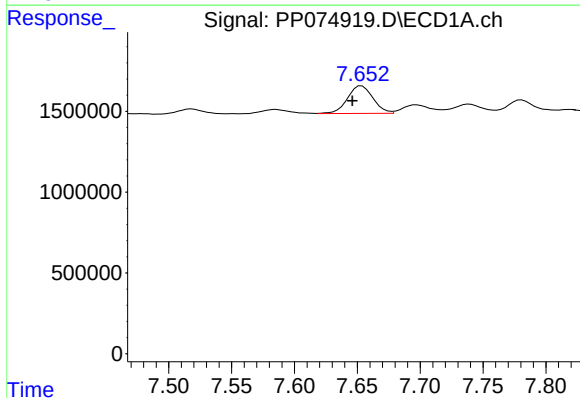


#32 AR-1260-2

R.T.: 7.653 min
Delta R.T.: 0.007 min
Response: 2404031
Conc: 34.88 ng/ml

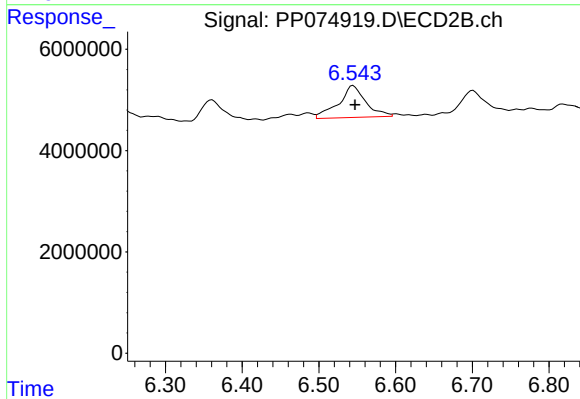

#32 AR-1260-2


R.T.: 6.545 min
Delta R.T.: -0.002 min
Response: 15531513
Conc: 29.37 ng/ml

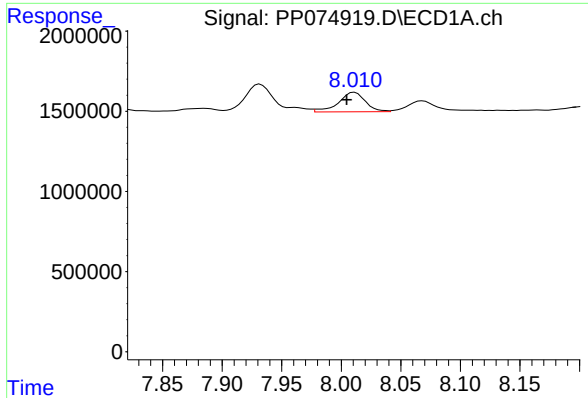

#33 AR-1260-3


R.T.: 8.011 min
Delta R.T.: 0.007 min
Response: 1908473
Conc: 36.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

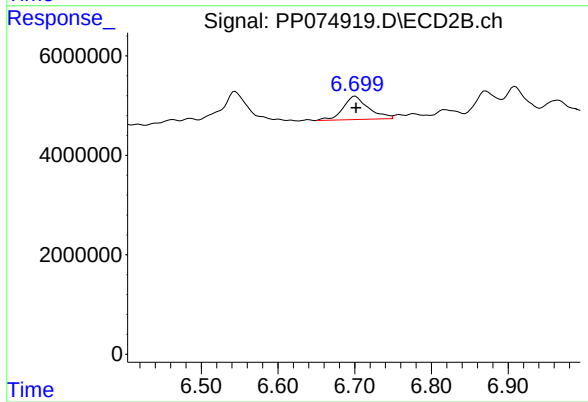


#33 AR-1260-3

R.T.: 6.701 min
Delta R.T.: 0.000 min
Response: 10807969
Conc: 24.96 ng/ml

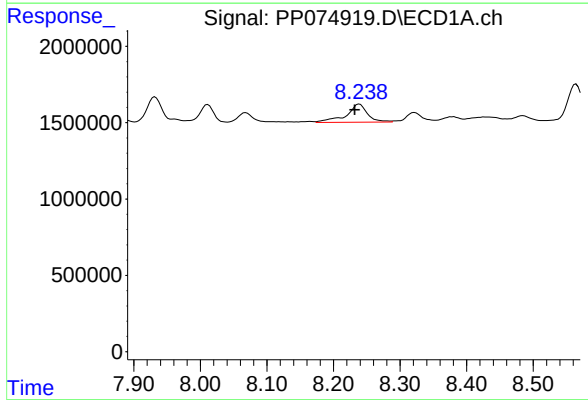


#34 AR-1260-4

R.T.: 8.239 min
Delta R.T.: 0.007 min
Response: 2621517
Conc: 41.09 ng/ml

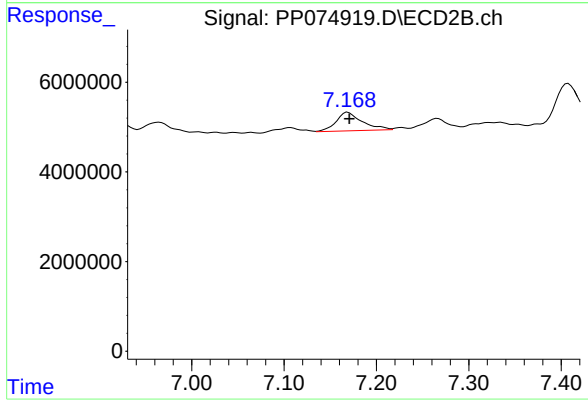

#34 AR-1260-4


R.T.: 7.169 min
Delta R.T.: -0.002 min
Response: 8179320
Conc: 21.44 ng/ml

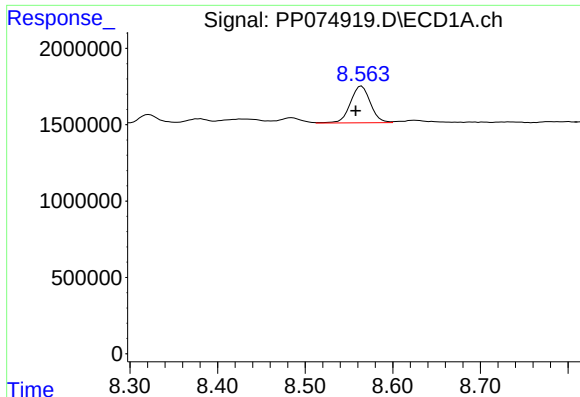

#35 AR-1260-5


R.T.: 8.564 min
Delta R.T.: 0.007 min
Response: 3814942
Conc: 33.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

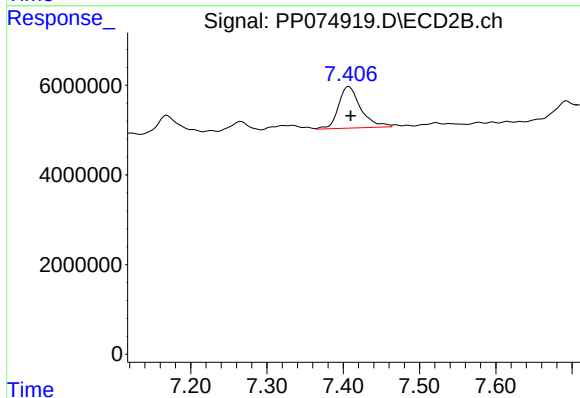


#35 AR-1260-5

R.T.: 7.408 min
Delta R.T.: -0.002 min
Response: 18696683
Conc: 18.61 ng/ml

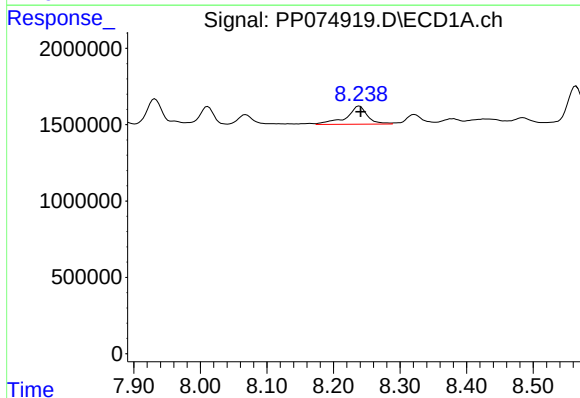


#36 AR-1262-1

R.T.: 8.239 min
Delta R.T.: -0.002 min
Response: 2621517
Conc: 34.04 ng/ml

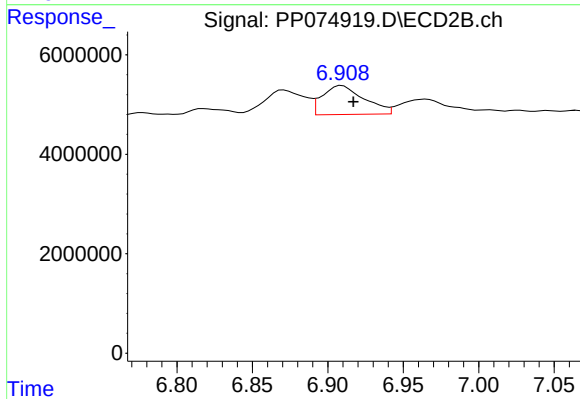

#36 AR-1262-1


R.T.: 6.909 min
Delta R.T.: -0.008 min
Response: 11187004
Conc: 15.82 ng/ml

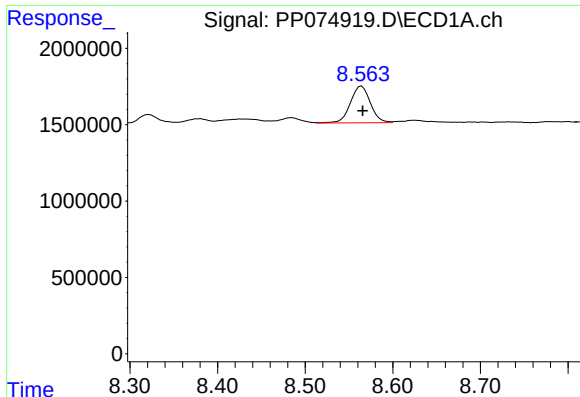

#37 AR-1262-2


R.T.: 8.564 min
Delta R.T.: -0.001 min
Response: 3814942
Conc: 28.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

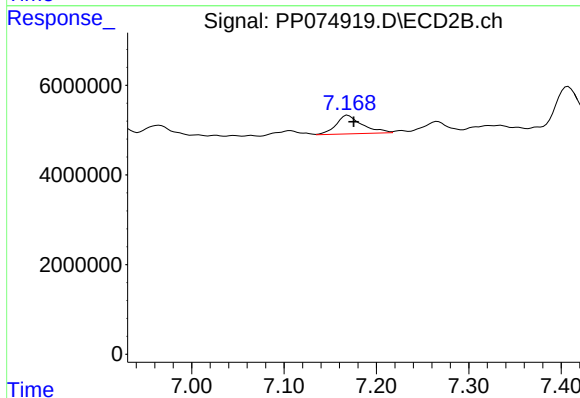


#37 AR-1262-2

R.T.: 7.169 min
Delta R.T.: -0.006 min
Response: 8179320
Conc: 15.71 ng/ml

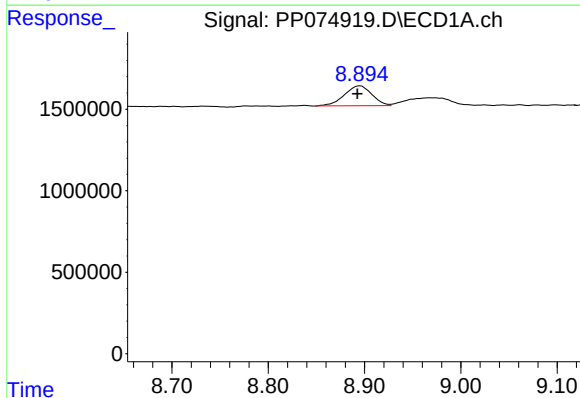


#38 AR-1262-3

R.T.: 8.896 min
Delta R.T.: 0.003 min
Response: 2423516
Conc: 24.93 ng/ml

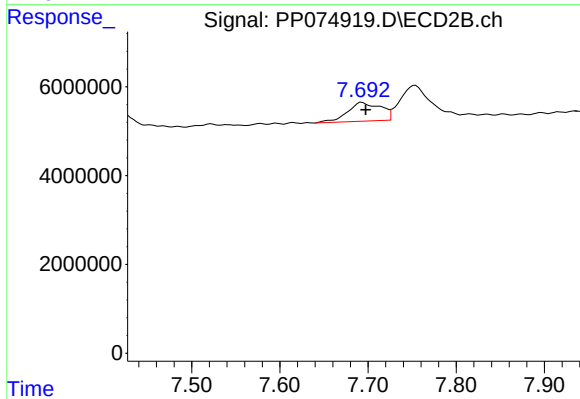

#38 AR-1262-3


R.T.: 7.693 min
Delta R.T.: -0.004 min
Response: 11027269
Conc: 23.65 ng/ml

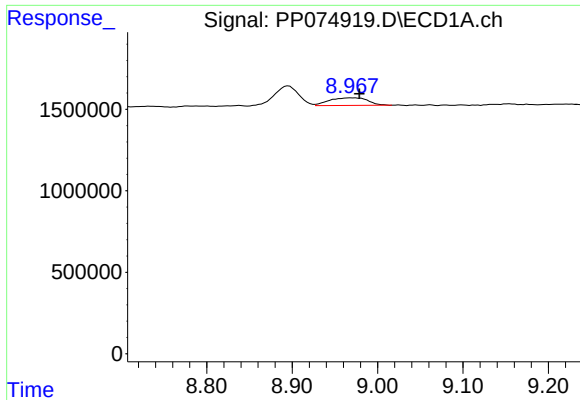

#39 AR-1262-4


R.T.: 8.969 min
Delta R.T.: -0.010 min
Response: 1471169
Conc: 19.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

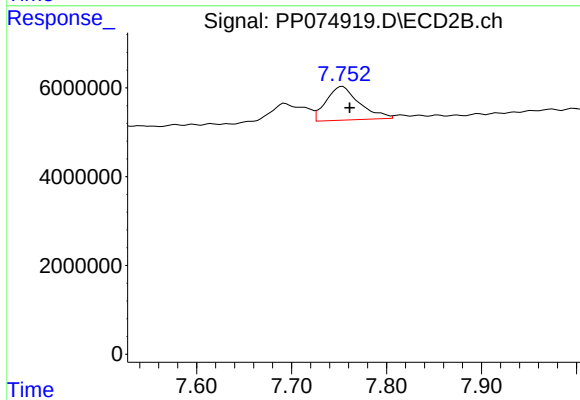


#39 AR-1262-4

R.T.: 7.754 min
Delta R.T.: -0.007 min
Response: 18419865
Conc: 22.41 ng/ml

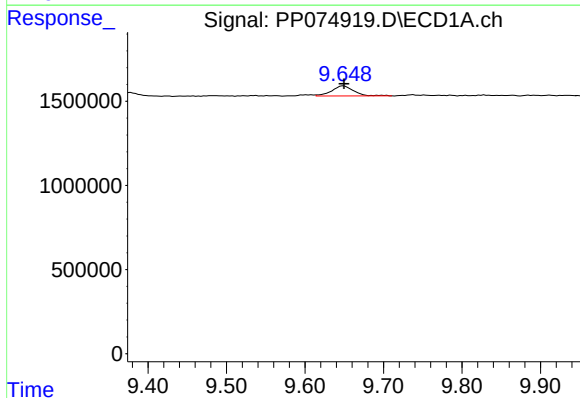


#40 AR-1262-5

R.T.: 9.649 min
Delta R.T.: 0.000 min
Response: 1177831
Conc: 19.32 ng/ml

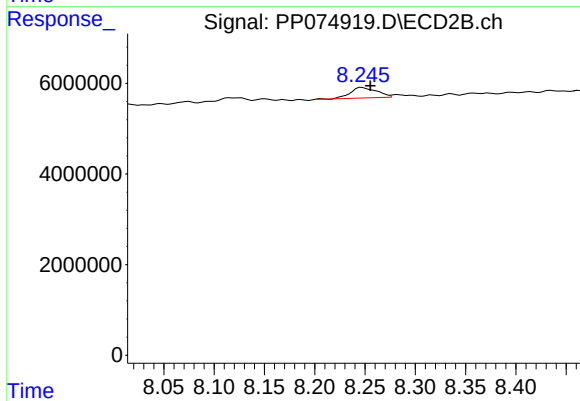

#40 AR-1262-5


R.T.: 8.247 min
Delta R.T.: -0.008 min
Response: 4203962
Conc: 11.73 ng/ml

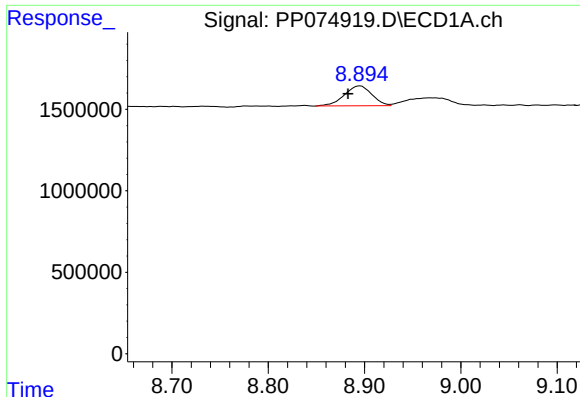

#41 AR-1268-1


R.T.: 8.896 min
Delta R.T.: 0.013 min
Response: 2423516
Conc: 14.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

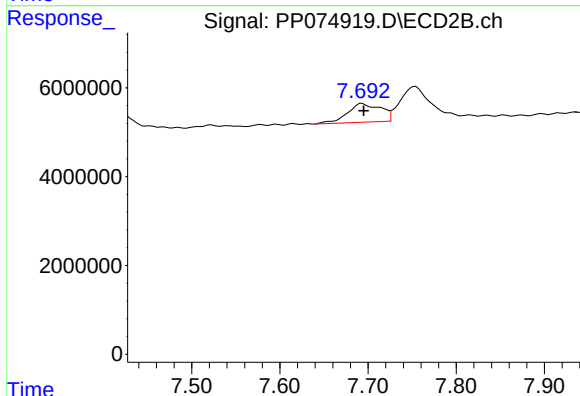


#41 AR-1268-1

R.T.: 7.693 min
Delta R.T.: -0.002 min
Response: 11027269
Conc: 7.82 ng/ml

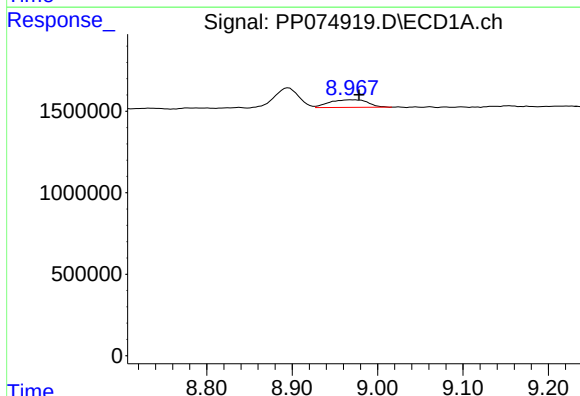


#42 AR-1268-2

R.T.: 8.969 min
Delta R.T.: -0.010 min
Response: 1471169
Conc: 10.03 ng/ml

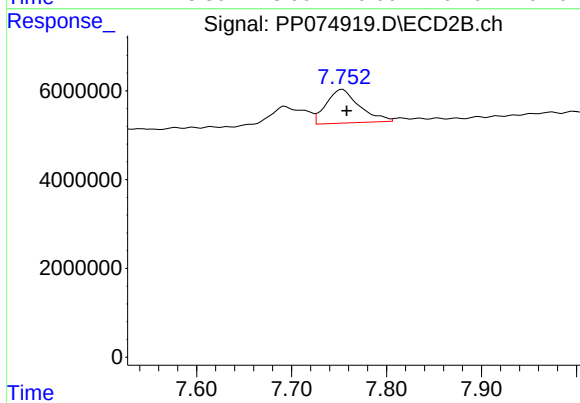

#42 AR-1268-2


R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 18419865
Conc: 13.51 ng/ml

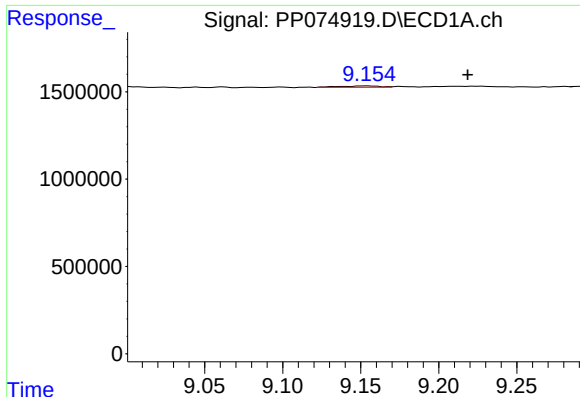

#43 AR-1268-3


R.T.: 9.155 min
Delta R.T.: -0.064 min
Response: 146663
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

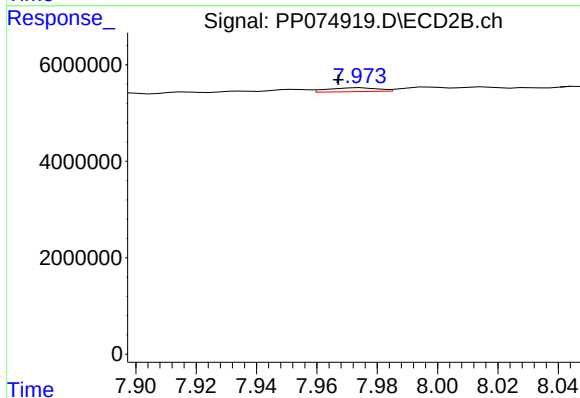


#43 AR-1268-3

R.T.: 7.974 min
Delta R.T.: 0.007 min
Response: 934563
Conc: 0.90 ng/ml

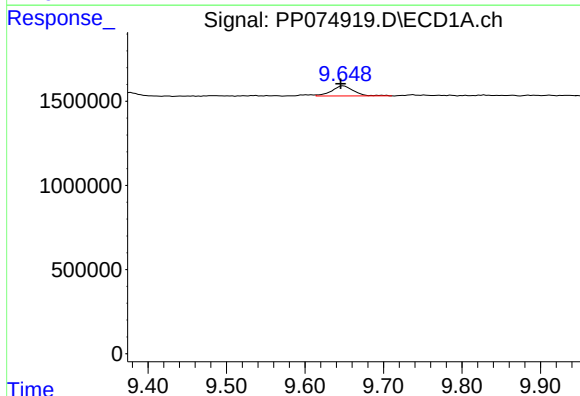


#44 AR-1268-4

R.T.: 9.649 min
Delta R.T.: 0.004 min
Response: 1177831
Conc: 17.51 ng/ml

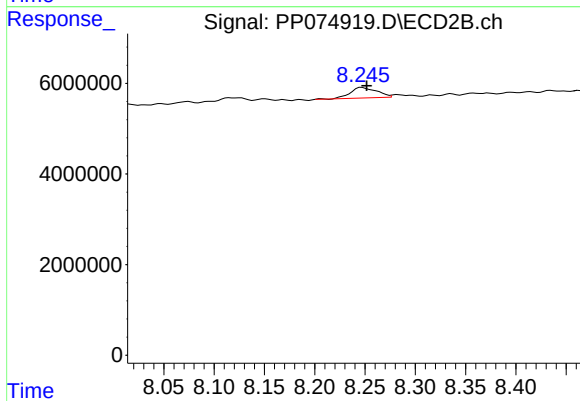

#44 AR-1268-4


R.T.: 8.247 min
Delta R.T.: -0.005 min
Response: 4203962
Conc: 10.97 ng/ml

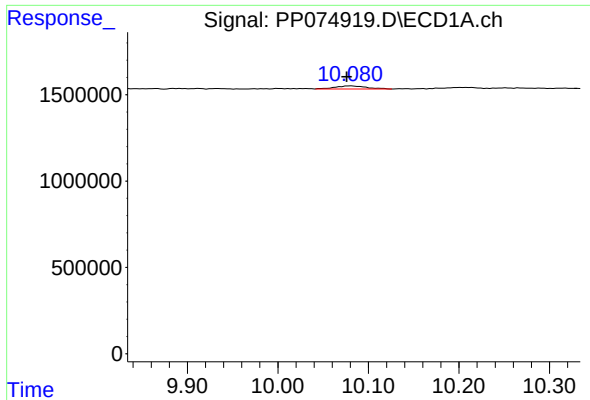

#45 AR-1268-5

R.T.: 10.081 min
Delta R.T.: 0.005 min
Response: 422491
Conc: 1.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

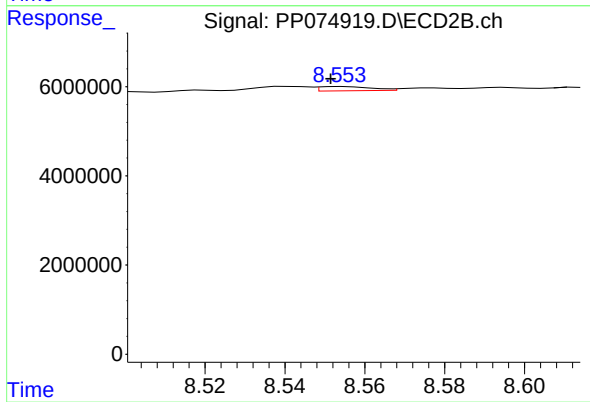

#45 AR-1268-5

R.T.: 8.554 min
Delta R.T.: 0.003 min
Response: 860236
Conc: 0.27 ng/ml