

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 20:28
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1221 WATER MDL 25PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:44:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.659	3.799	26335310	98922147	21.521	20.458
2)	SA Decachlor...	10.435	8.809	21211032	136.2E6	21.479	18.158
Target Compounds							
3)	L1 AR-1016-1	5.831	4.892	433347	529923	9.829	1.040 #
4)	L1 AR-1016-2	5.831	4.948	433347	746195	6.896	3.135 #
5)	L1 AR-1016-3	5.900	5.080	297917	659120	6.633	4.780 #
6)	L1 AR-1016-4	5.940f	5.114	359287	292743	10.212	2.094 #
7)	L1 AR-1016-5	6.304	5.333	106180	666385	3.200	4.012 #
8)	L2 AR-1221-1	4.857	4.012	460908	1140436	26.199	18.434 #
9)	L2 AR-1221-2	4.959	4.093	932092	1722757	69.782	38.104 #
10)	L2 AR-1221-3	5.019	4.170	931154	2733488	24.560	16.638 #
11)	L3 AR-1232-1	5.019	4.170	931154	2733488	30.656	21.339 #
12)	L3 AR-1232-2	5.548	4.892	177685	529923	11.276	2.286 #
13)	L3 AR-1232-3	5.831	5.080	433347	659120	14.188	10.974
14)	L3 AR-1232-4	5.940f	5.157	359287	624805	20.805	8.477 #
15)	L3 AR-1232-5	6.057	5.333	129237	666385	9.956	10.734
16)	L4 AR-1242-1	5.831	4.907	433347	269753	11.322	0.640 #
17)	L4 AR-1242-2	5.831	4.948	433347	746195	7.672	3.726 #
18)	L4 AR-1242-3	5.900	5.080	297917	659120	7.337	5.572
19)	L4 AR-1242-4	5.940f	5.157	359287	624805	11.319	3.650 #
20)	L4 AR-1242-5	6.725	5.663	444306	187477	12.318	1.012 #
21)	L5 AR-1248-1	5.831	4.892	433347	529923	14.338	1.919 #
22)	L5 AR-1248-2	6.057	5.114	129237	292743	2.999	1.656 #
23)	L5 AR-1248-3	6.304	5.157	106180	624805	2.273	2.750
24)	L5 AR-1248-4	6.697	5.333	120034	666385	2.182	3.057 #
25)	L5 AR-1248-5	6.725	5.761f	444306	19729481	8.010	53.712 #
26)	L6 AR-1254-1	6.655	5.663	899766	187477	15.441	0.393 #
27)	L6 AR-1254-2	6.873	5.841	215711	1087040	2.643	3.087
28)	L6 AR-1254-3	7.229	6.242	2292906	1029457	25.703	1.661 #
29)	L6 AR-1254-4	7.518	6.465	195613	857632	2.968	1.830 #
30)	L6 AR-1254-5	7.935	6.879	170321	641212	2.050	1.307 #
31)	L7 AR-1260-1	7.398	6.367	26669	794970	0.461	2.119 #
32)	L7 AR-1260-2	7.655	6.561	208401	689421	3.024	1.304 #
33)	L7 AR-1260-3	7.964f	6.699	30192	776780	0.582	1.794 #
34)	L7 AR-1260-4	8.226	7.164	134645	334758	2.111	0.878 #
35)	L7 AR-1260-5	0.000	7.413	0	472828	N.D.	0.471 #
36)	L8 AR-1262-1	8.226	6.918	134645	310086	1.748	0.438 #
37)	L8 AR-1262-2	0.000	7.183	0	429748	N.D.	0.825 #
38)	L8 AR-1262-3	0.000	7.698	0	4069954	N.D.	8.728 #
39)	L8 AR-1262-4	0.000	7.755	0	2381794	N.D.	2.898 #
40)	L8 AR-1262-5	9.607f	8.250	208617	316875	3.422	0.884 #
41)	L9 AR-1268-1	0.000	7.698	0	4069954	N.D.	2.885 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074920.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 20:28
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1221 WATER MDL 25PPB
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:44:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.755	0	2381794	N.D.	1.747 #
43) L9	AR-1268-3	9.149f	7.974	206991	512751	1.675	0.492 #
44) L9	AR-1268-4	9.607f	8.250	208617	316875	3.102	0.827 #
45) L9	AR-1268-5	10.082	8.547	138584	577436	0.374	0.184 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
Data File : PP074920.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 20:28
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1221 WATER MDL 25PPB
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:44:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

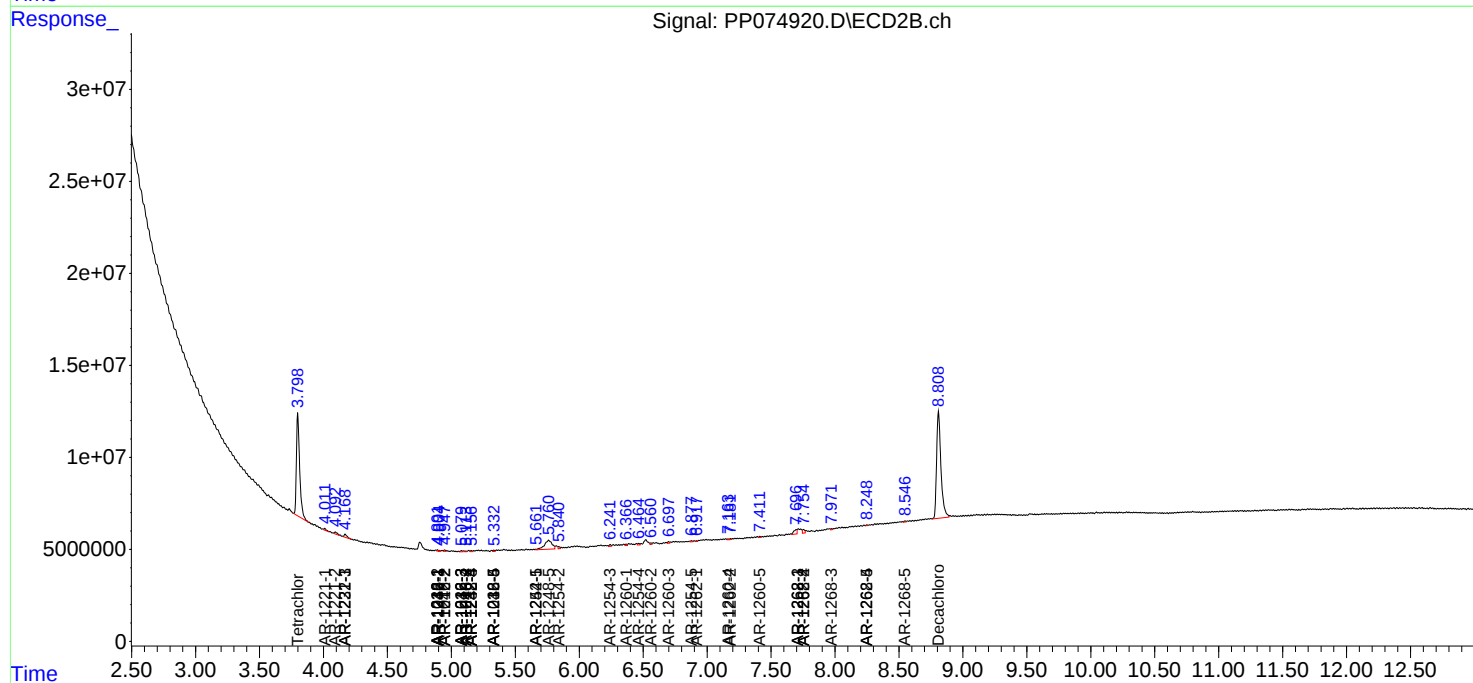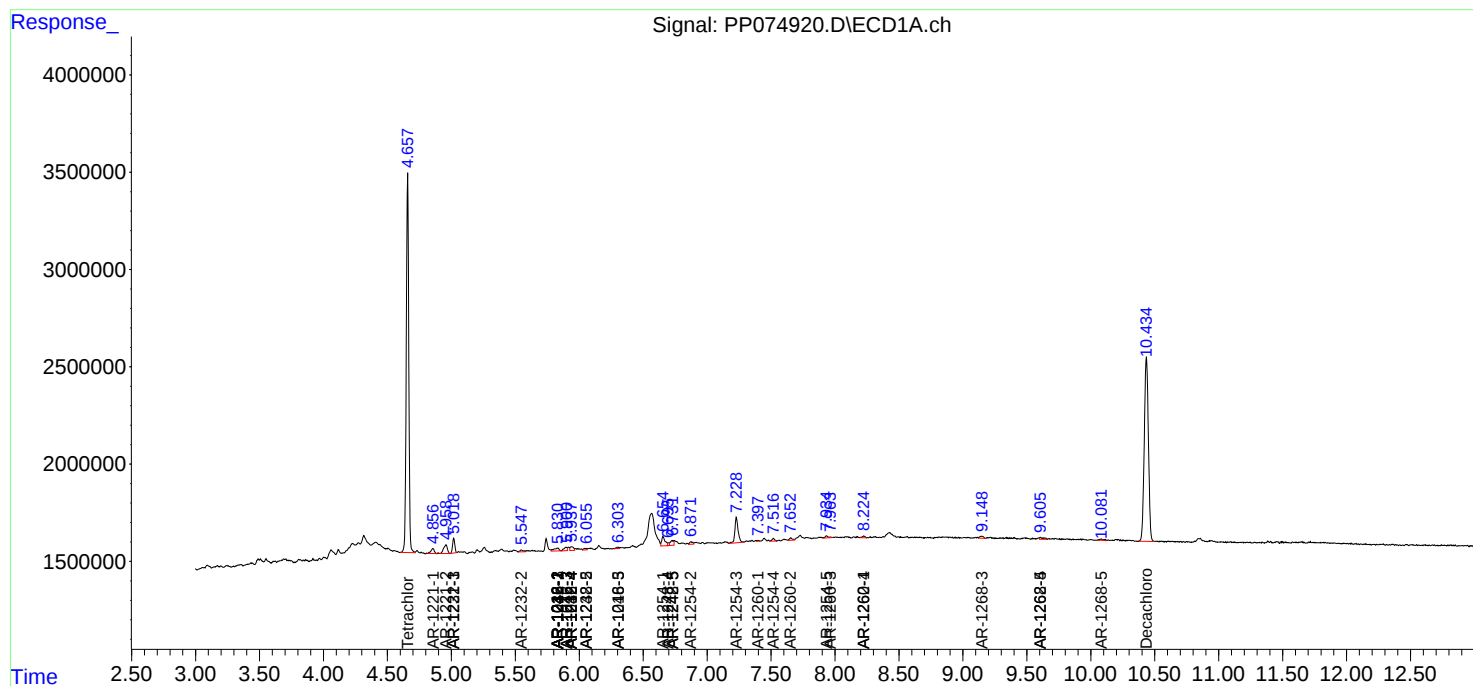


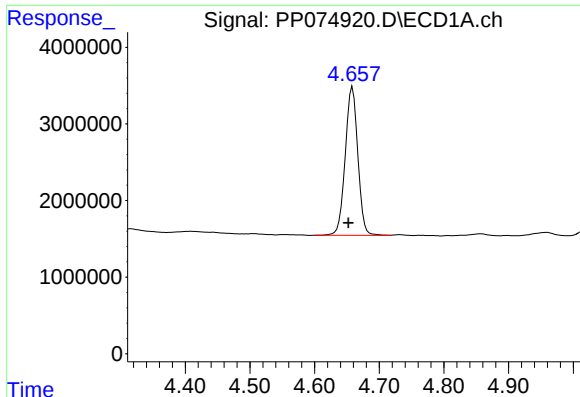

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.007 min
Response: 26335310
Conc: 21.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

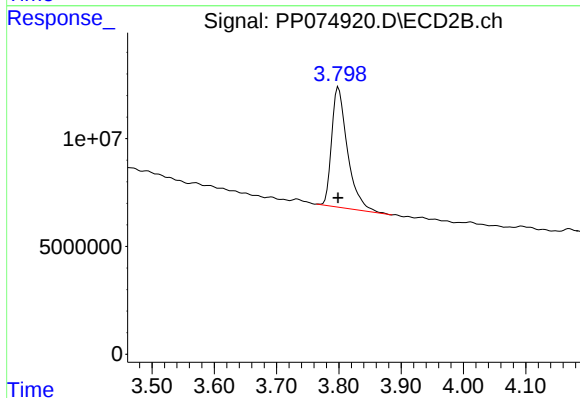


#1 Tetrachloro-m-xylene

R.T.: 3.799 min
Delta R.T.: 0.000 min
Response: 98922147
Conc: 20.46 ng/ml

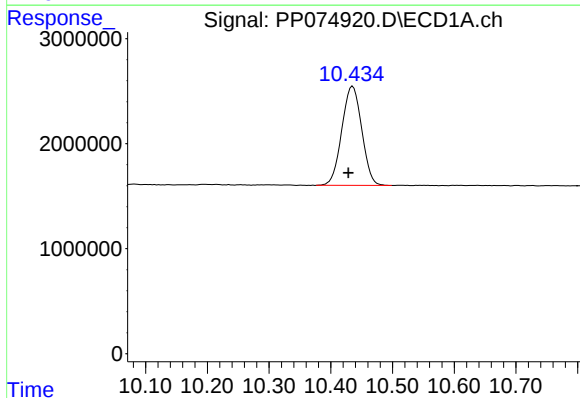


#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.007 min
Response: 21211032
Conc: 21.48 ng/ml

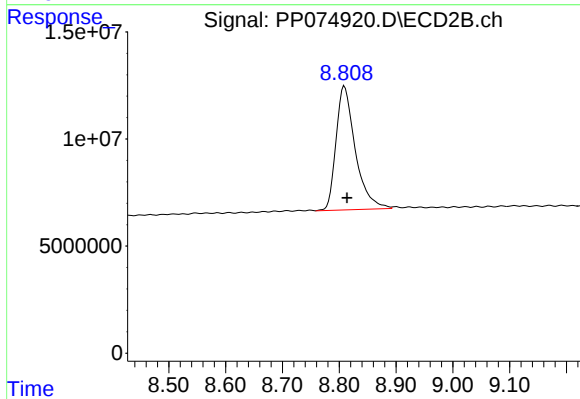

#2 Decachlorobiphenyl


R.T.: 8.809 min
Delta R.T.: -0.005 min
Response: 136170304
Conc: 18.16 ng/ml

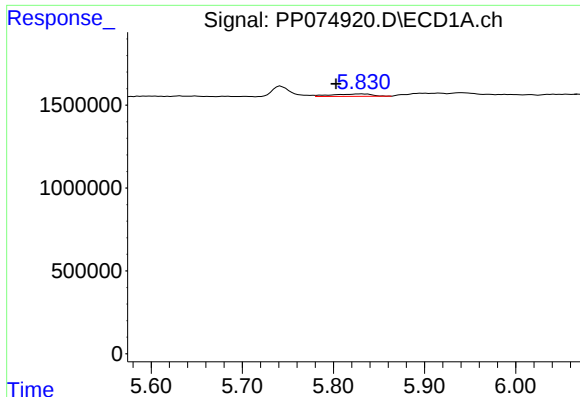

#3 AR-1016-1


R.T.: 5.831 min
Delta R.T.: 0.028 min
Response: 433347
Conc: 9.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

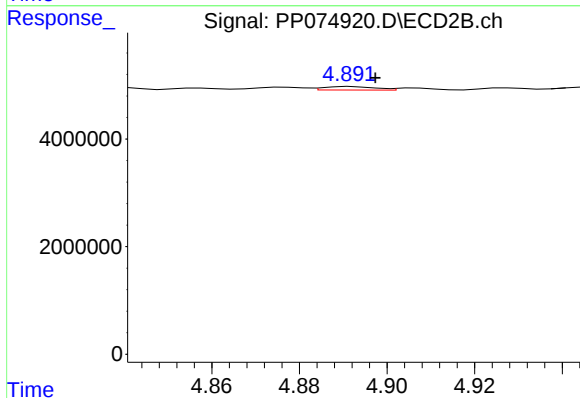


#3 AR-1016-1

R.T.: 4.892 min
Delta R.T.: -0.005 min
Response: 529923
Conc: 1.04 ng/ml

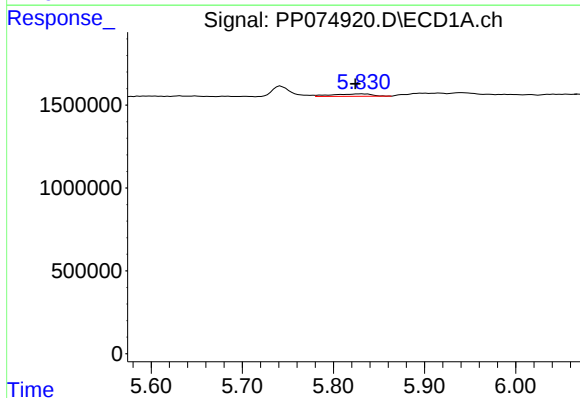


#4 AR-1016-2

R.T.: 5.831 min
Delta R.T.: 0.007 min
Response: 433347
Conc: 6.90 ng/ml

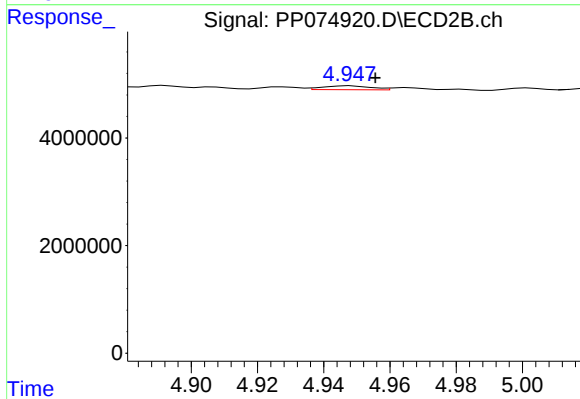

#4 AR-1016-2


R.T.: 4.948 min
Delta R.T.: -0.007 min
Response: 746195
Conc: 3.14 ng/ml

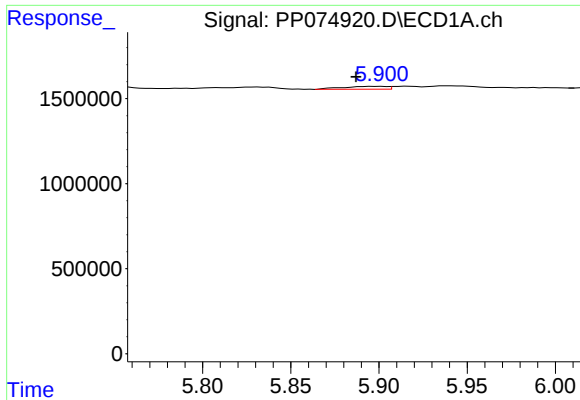

#5 AR-1016-3


R.T.: 5.900 min
Delta R.T.: 0.013 min
Response: 297917
Conc: 6.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

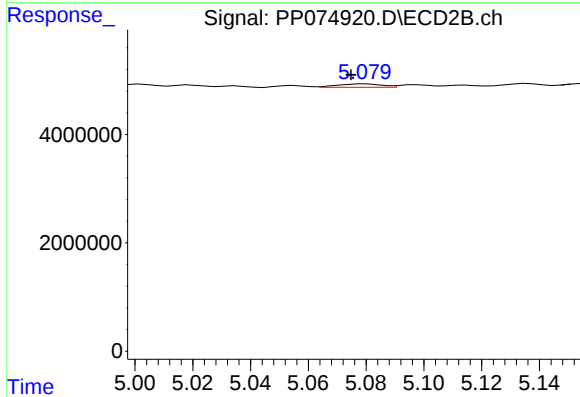


#5 AR-1016-3

R.T.: 5.080 min
Delta R.T.: 0.005 min
Response: 659120
Conc: 4.78 ng/ml

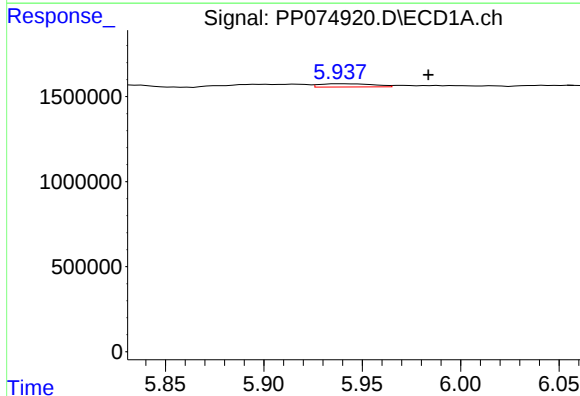


#6 AR-1016-4

R.T.: 5.940 min
Delta R.T.: -0.044 min
Response: 359287
Conc: 10.21 ng/ml

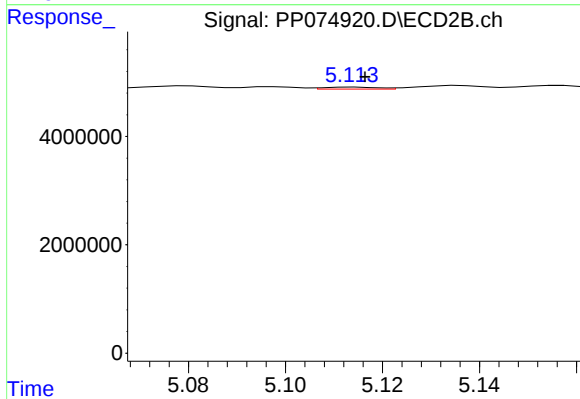

#6 AR-1016-4


R.T.: 5.114 min
Delta R.T.: -0.002 min
Response: 292743
Conc: 2.09 ng/ml

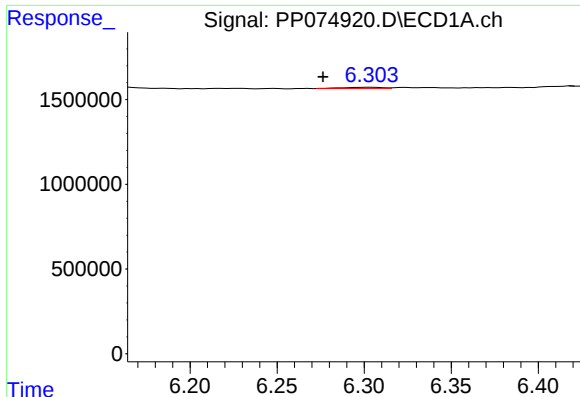

#7 AR-1016-5


R.T.: 6.304 min
Delta R.T.: 0.027 min
Response: 106180
Conc: 3.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

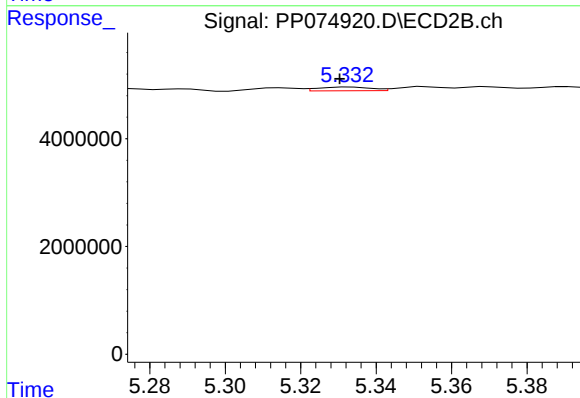


#7 AR-1016-5

R.T.: 5.333 min
Delta R.T.: 0.003 min
Response: 666385
Conc: 4.01 ng/ml

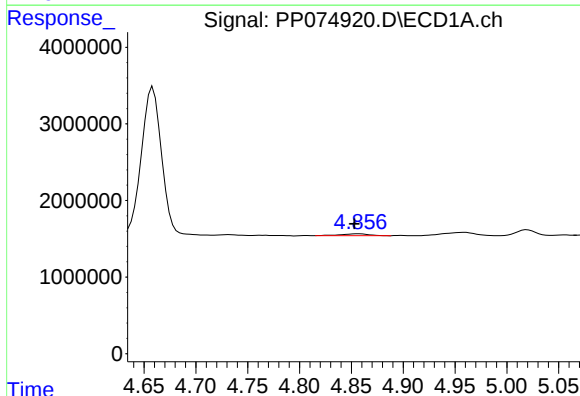


#8 AR-1221-1

R.T.: 4.857 min
Delta R.T.: 0.004 min
Response: 460908
Conc: 26.20 ng/ml

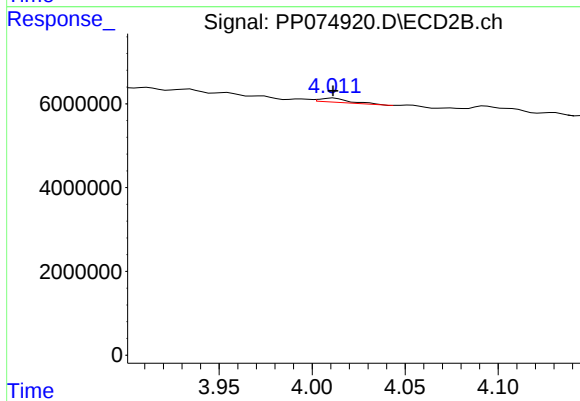

#8 AR-1221-1


R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 1140436
Conc: 18.43 ng/ml

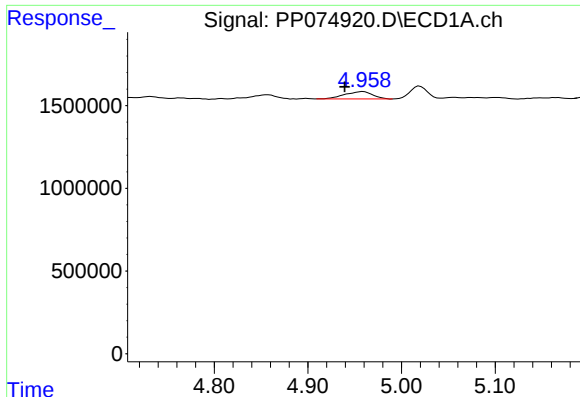

#9 AR-1221-2


R.T.: 4.959 min
Delta R.T.: 0.020 min
Response: 932092
Conc: 69.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

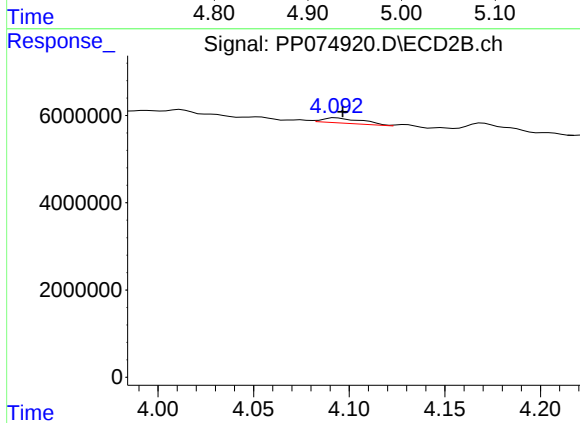


#9 AR-1221-2

R.T.: 4.093 min
Delta R.T.: -0.003 min
Response: 1722757
Conc: 38.10 ng/ml

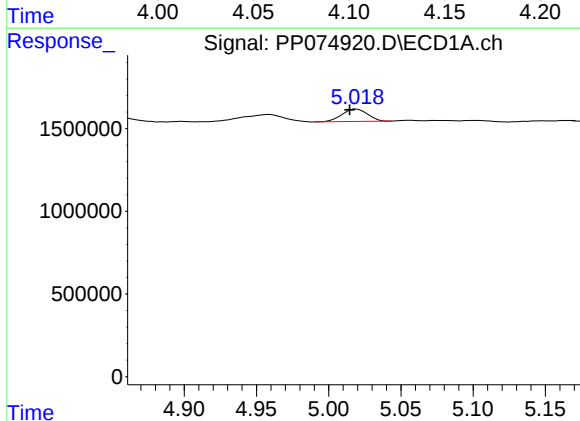


#10 AR-1221-3

R.T.: 5.019 min
Delta R.T.: 0.005 min
Response: 931154
Conc: 24.56 ng/ml

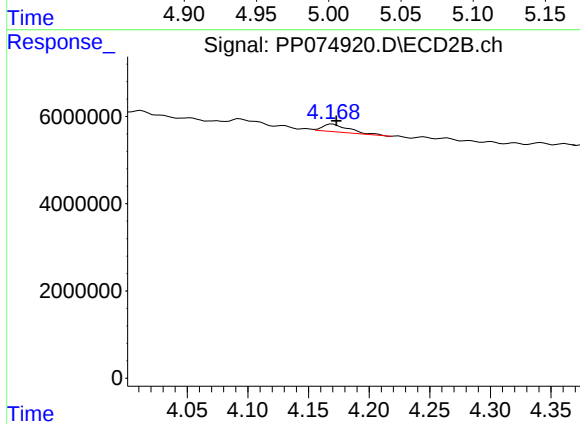

#10 AR-1221-3


R.T.: 4.170 min
Delta R.T.: -0.003 min
Response: 2733488
Conc: 16.64 ng/ml

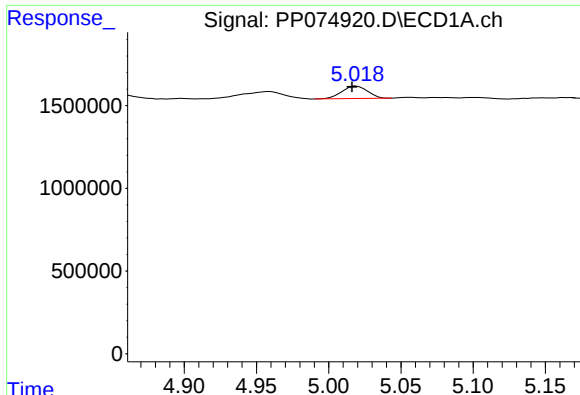

#11 AR-1232-1


R.T.: 5.019 min
Delta R.T.: 0.003 min
Response: 931154
Conc: 30.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

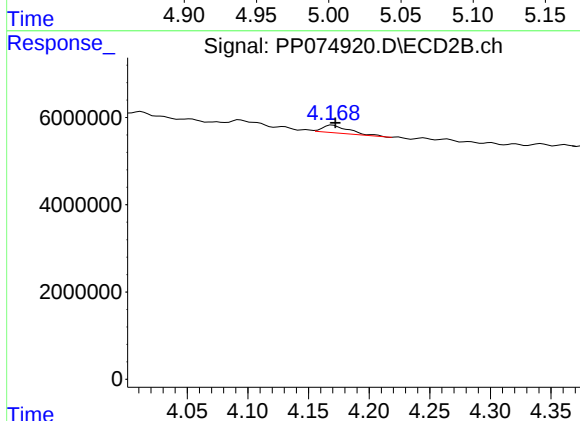


#11 AR-1232-1

R.T.: 4.170 min
Delta R.T.: -0.002 min
Response: 2733488
Conc: 21.34 ng/ml

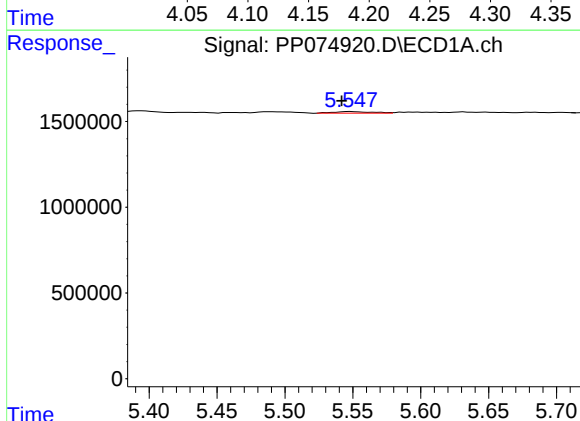


#12 AR-1232-2

R.T.: 5.548 min
Delta R.T.: 0.006 min
Response: 177685
Conc: 11.28 ng/ml

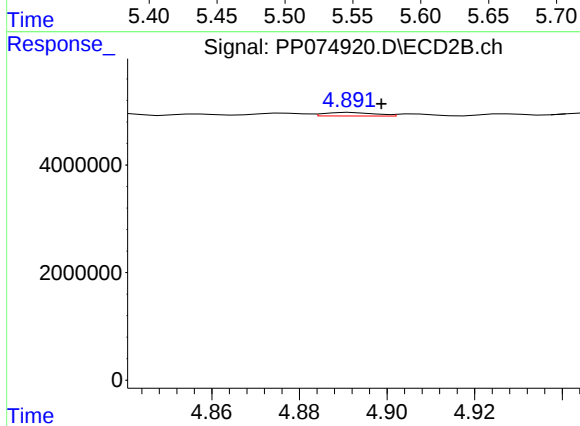

#12 AR-1232-2


R.T.: 4.892 min
Delta R.T.: -0.007 min
Response: 529923
Conc: 2.29 ng/ml

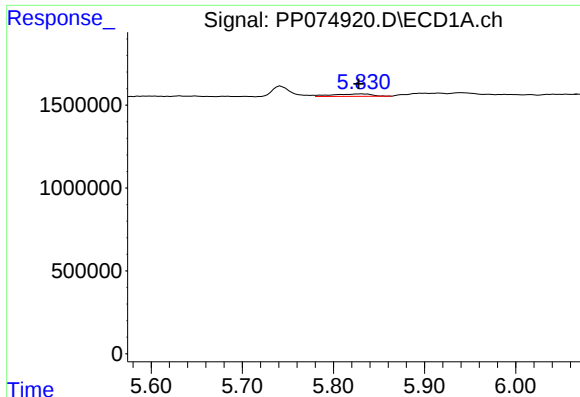

#13 AR-1232-3


R.T.: 5.831 min
Delta R.T.: 0.003 min
Response: 433347
Conc: 14.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

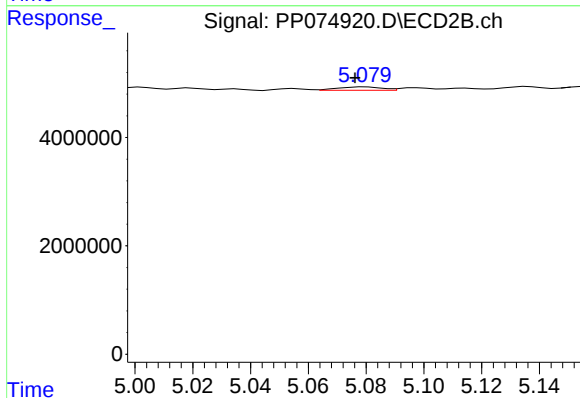


#13 AR-1232-3

R.T.: 5.080 min
Delta R.T.: 0.004 min
Response: 659120
Conc: 10.97 ng/ml

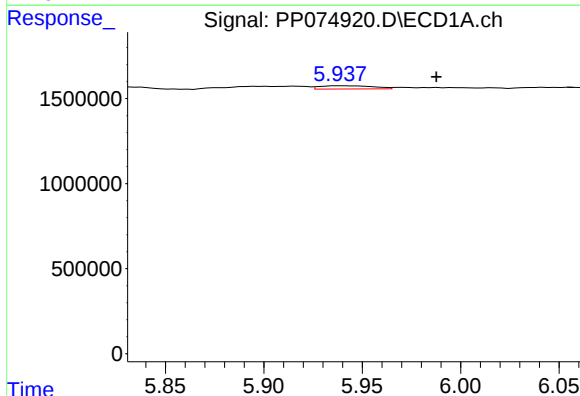


#14 AR-1232-4

R.T.: 5.940 min
Delta R.T.: -0.048 min
Response: 359287
Conc: 20.80 ng/ml

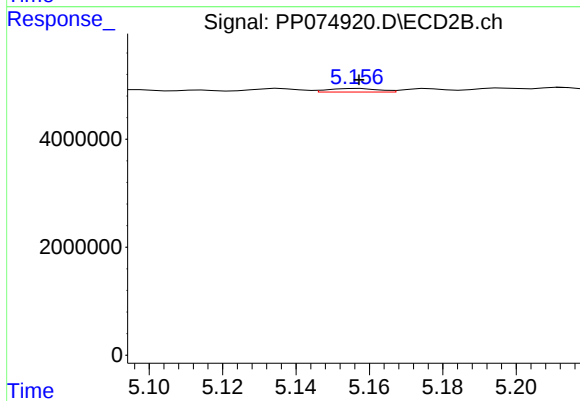

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 624805
Conc: 8.48 ng/ml

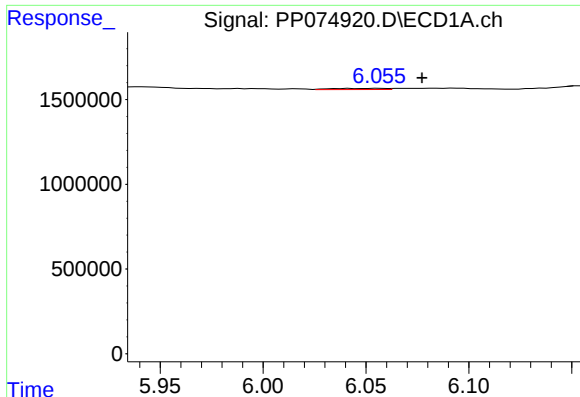

#15 AR-1232-5


R.T.: 6.057 min
Delta R.T.: -0.021 min
Response: 129237
Conc: 9.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

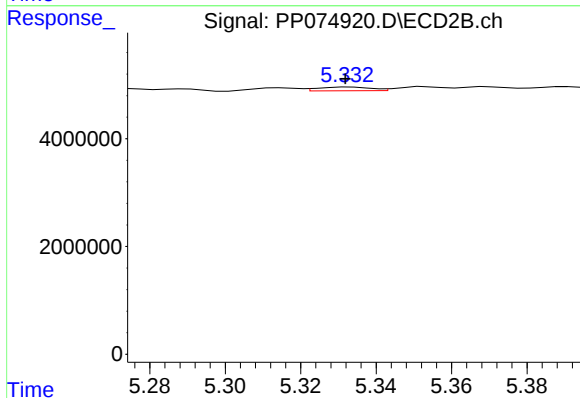


#15 AR-1232-5

R.T.: 5.333 min
Delta R.T.: 0.001 min
Response: 666385
Conc: 10.73 ng/ml

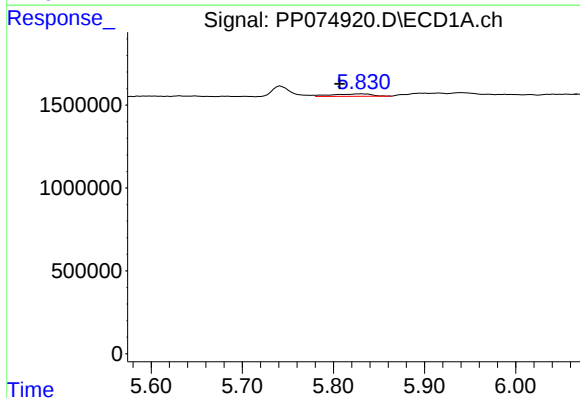


#16 AR-1242-1

R.T.: 5.831 min
Delta R.T.: 0.024 min
Response: 433347
Conc: 11.32 ng/ml

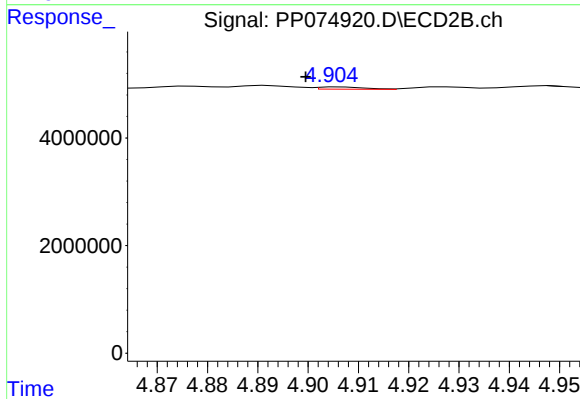

#16 AR-1242-1


R.T.: 4.907 min
Delta R.T.: 0.007 min
Response: 269753
Conc: 0.64 ng/ml

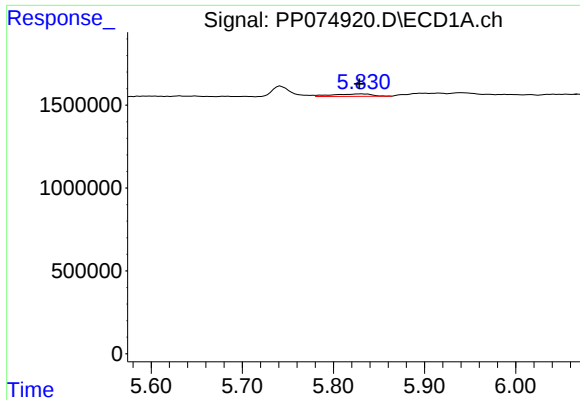

#17 AR-1242-2


R.T.: 5.831 min
Delta R.T.: 0.002 min
Response: 433347
Conc: 7.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

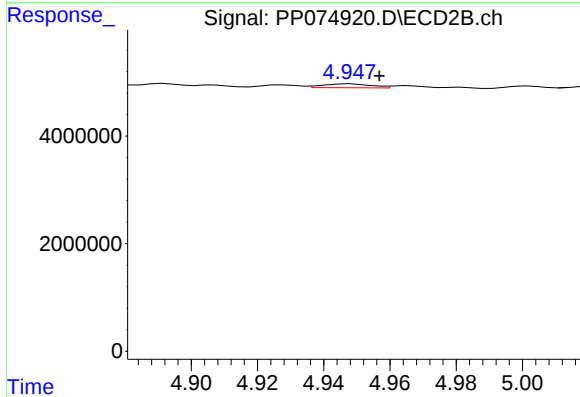


#17 AR-1242-2

R.T.: 4.948 min
Delta R.T.: -0.008 min
Response: 746195
Conc: 3.73 ng/ml

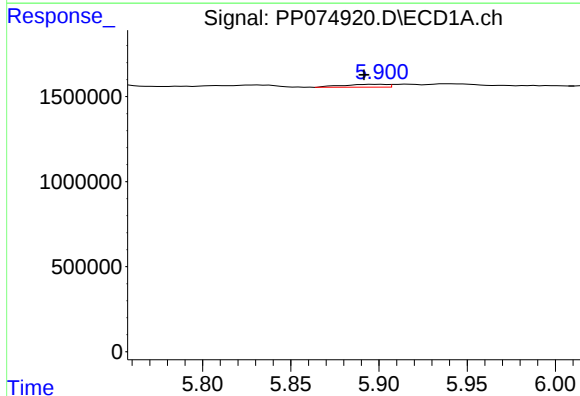


#18 AR-1242-3

R.T.: 5.900 min
Delta R.T.: 0.008 min
Response: 297917
Conc: 7.34 ng/ml

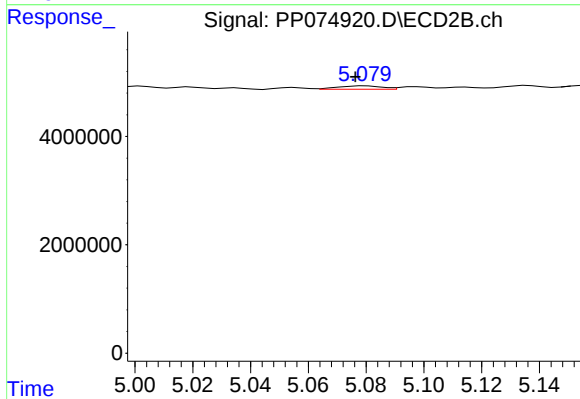

#18 AR-1242-3


R.T.: 5.080 min
Delta R.T.: 0.004 min
Response: 659120
Conc: 5.57 ng/ml

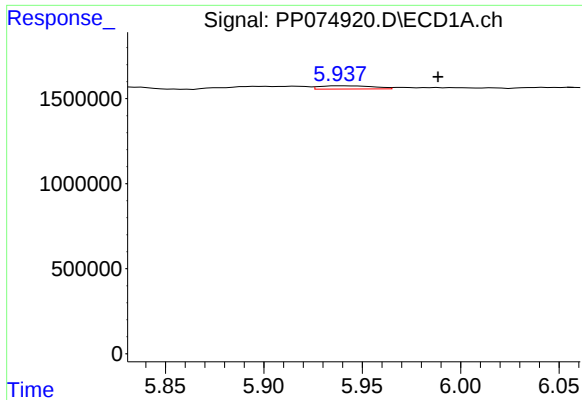

#19 AR-1242-4


R.T.: 5.940 min
Delta R.T.: -0.049 min
Response: 359287
Conc: 11.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

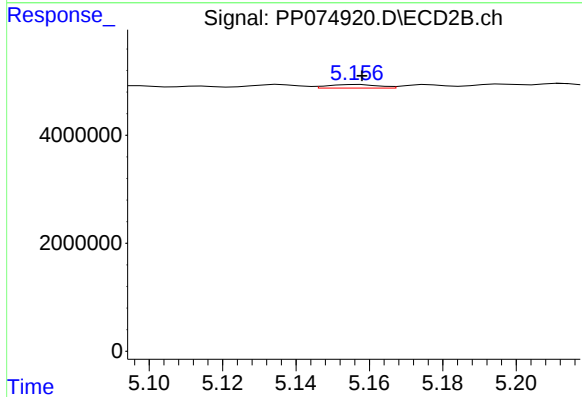


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 624805
Conc: 3.65 ng/ml

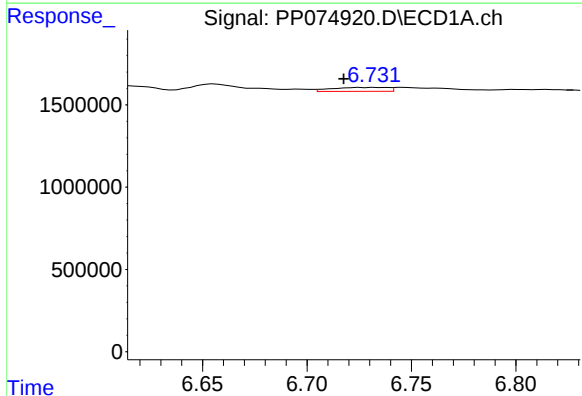


#20 AR-1242-5

R.T.: 6.725 min
Delta R.T.: 0.008 min
Response: 444306
Conc: 12.32 ng/ml

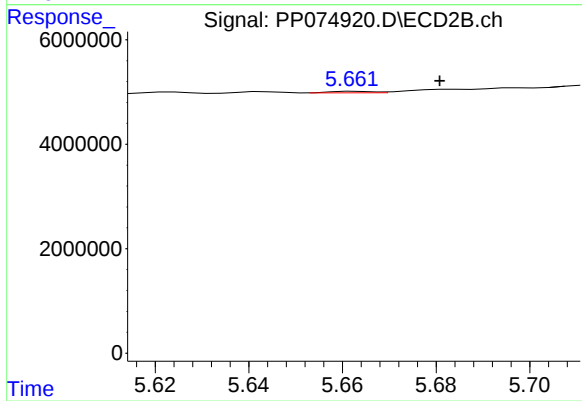

#20 AR-1242-5


R.T.: 5.663 min
Delta R.T.: -0.018 min
Response: 187477
Conc: 1.01 ng/ml

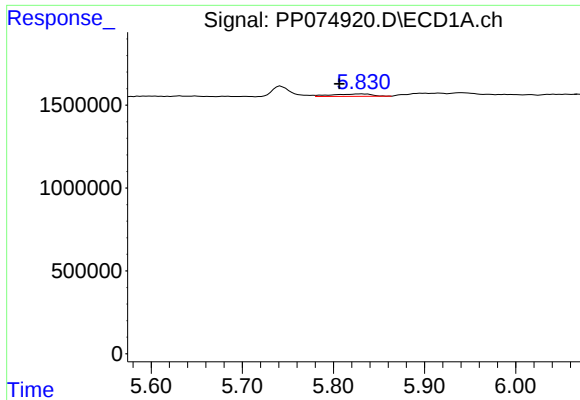

#21 AR-1248-1


R.T.: 5.831 min
Delta R.T.: 0.024 min
Response: 433347
Conc: 14.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

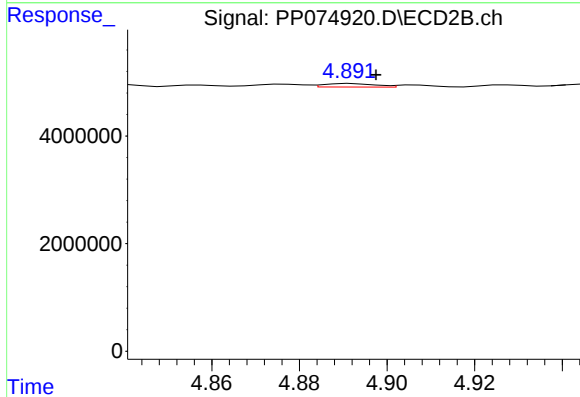


#21 AR-1248-1

R.T.: 4.892 min
Delta R.T.: -0.006 min
Response: 529923
Conc: 1.92 ng/ml

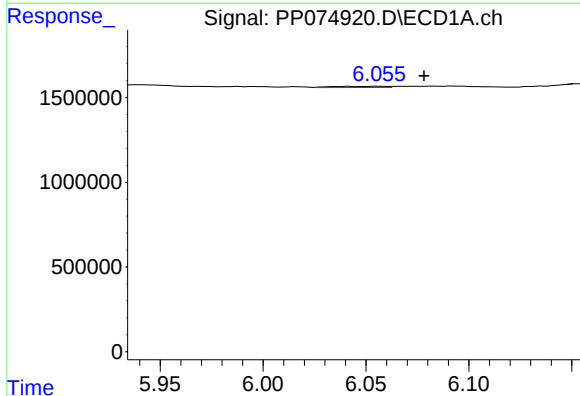


#22 AR-1248-2

R.T.: 6.057 min
Delta R.T.: -0.022 min
Response: 129237
Conc: 3.00 ng/ml

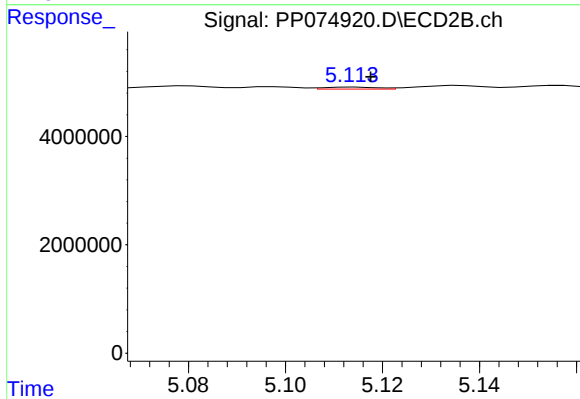

#22 AR-1248-2


R.T.: 5.114 min
Delta R.T.: -0.003 min
Response: 292743
Conc: 1.66 ng/ml

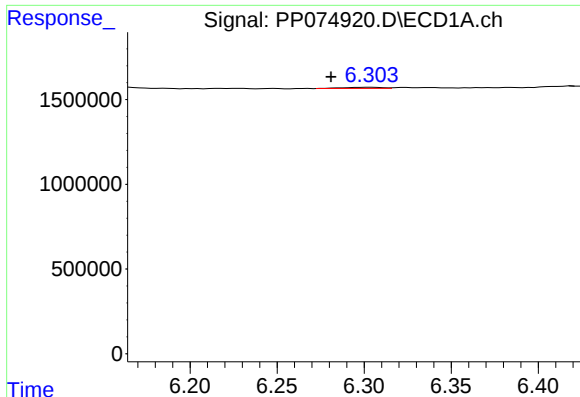

#23 AR-1248-3


R.T.: 6.304 min
Delta R.T.: 0.023 min
Response: 106180
Conc: 2.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

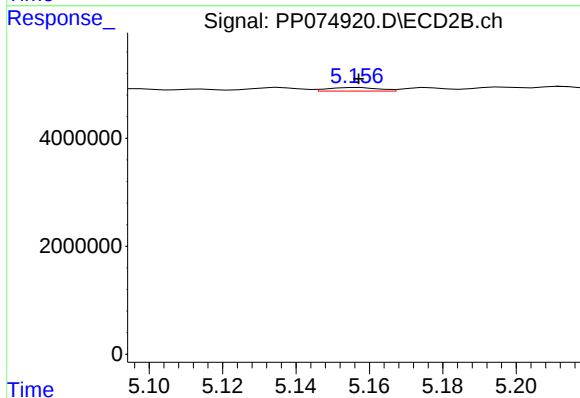


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 624805
Conc: 2.75 ng/ml

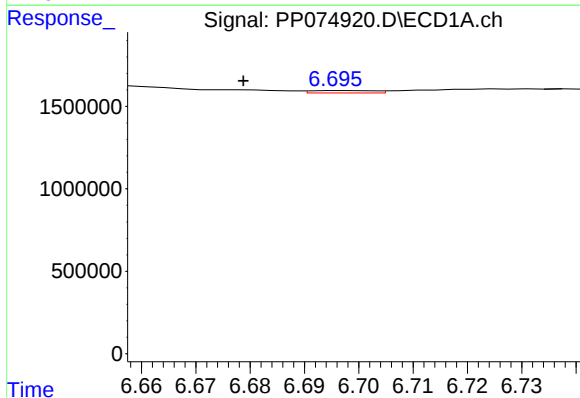


#24 AR-1248-4

R.T.: 6.697 min
Delta R.T.: 0.018 min
Response: 120034
Conc: 2.18 ng/ml

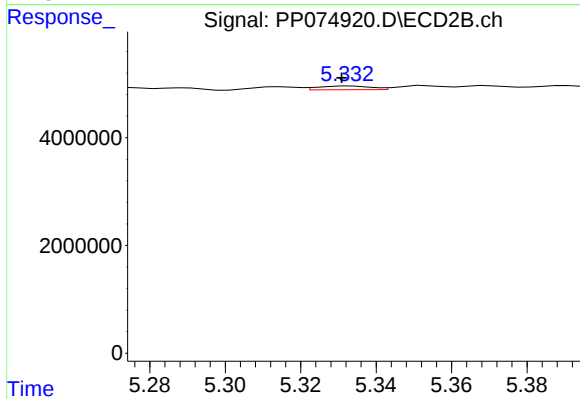

#24 AR-1248-4


R.T.: 5.333 min
Delta R.T.: 0.002 min
Response: 666385
Conc: 3.06 ng/ml

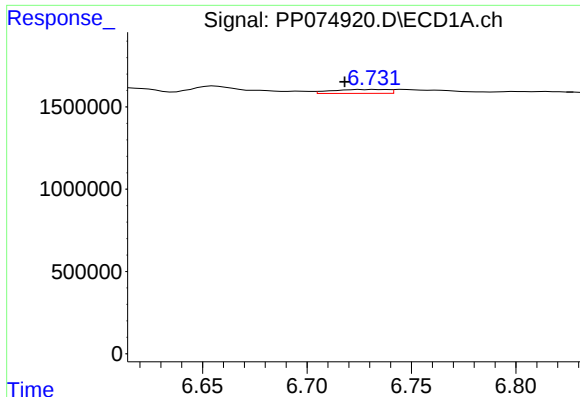

#25 AR-1248-5


R.T.: 6.725 min
Delta R.T.: 0.007 min
Response: 444306
Conc: 8.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

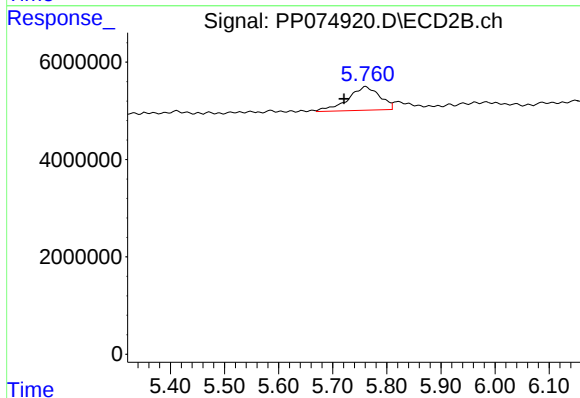


#25 AR-1248-5

R.T.: 5.761 min
Delta R.T.: 0.040 min
Response: 19729481
Conc: 53.71 ng/ml

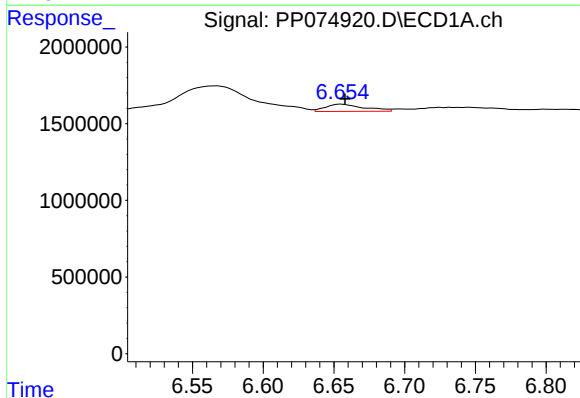


#26 AR-1254-1

R.T.: 6.655 min
Delta R.T.: -0.003 min
Response: 899766
Conc: 15.44 ng/ml

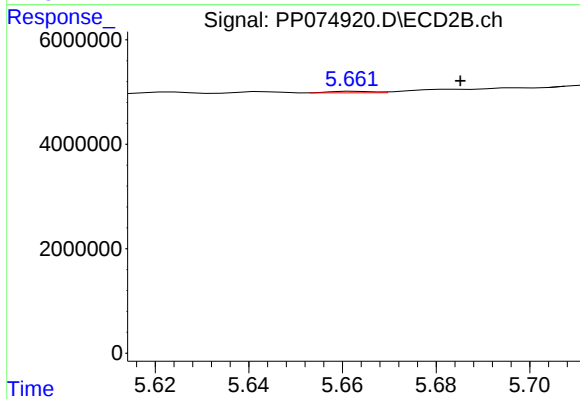

#26 AR-1254-1


R.T.: 5.663 min
Delta R.T.: -0.022 min
Response: 187477
Conc: 0.39 ng/ml

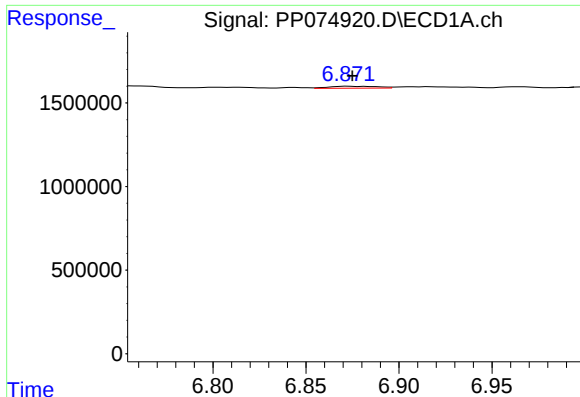

#27 AR-1254-2


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 215711
Conc: 2.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

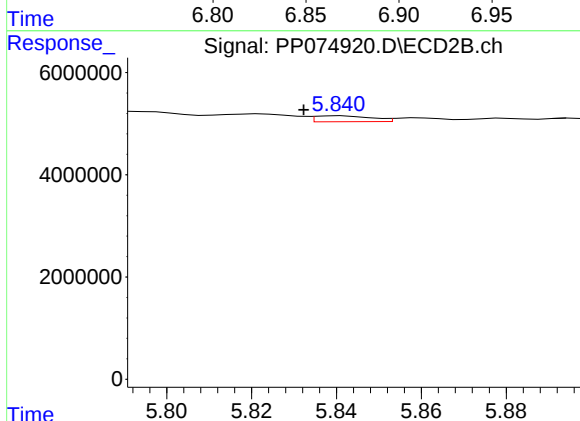


#27 AR-1254-2

R.T.: 5.841 min
Delta R.T.: 0.009 min
Response: 1087040
Conc: 3.09 ng/ml

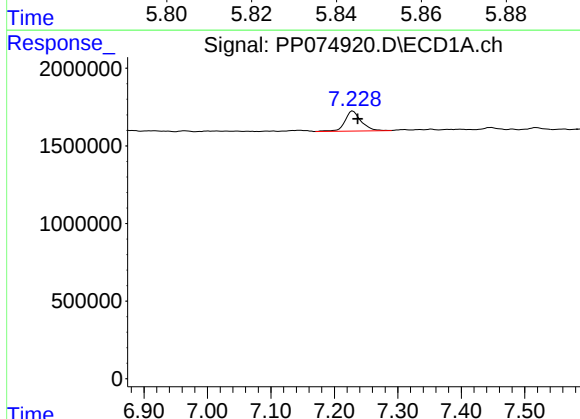


#28 AR-1254-3

R.T.: 7.229 min
Delta R.T.: -0.008 min
Response: 2292906
Conc: 25.70 ng/ml

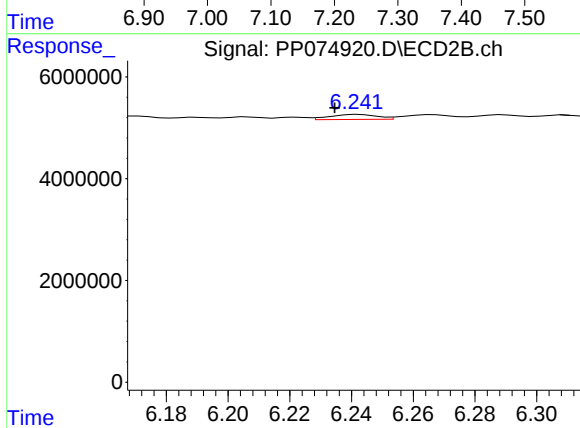

#28 AR-1254-3


R.T.: 6.242 min
Delta R.T.: 0.008 min
Response: 1029457
Conc: 1.66 ng/ml

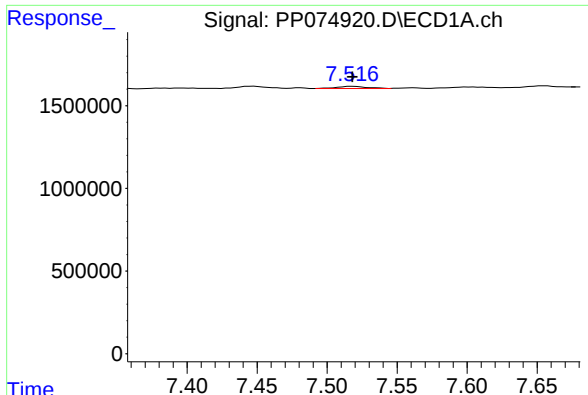

#29 AR-1254-4


R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 195613
Conc: 2.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

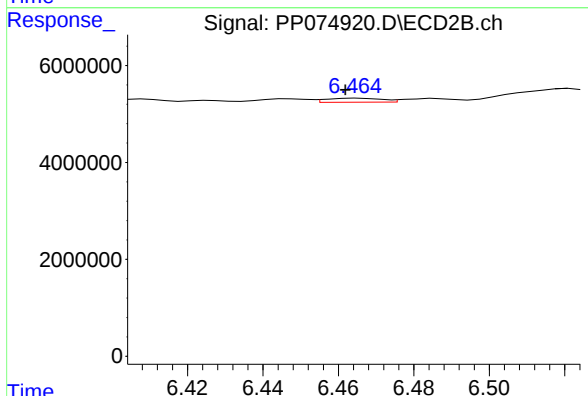


#29 AR-1254-4

R.T.: 6.465 min
Delta R.T.: 0.003 min
Response: 857632
Conc: 1.83 ng/ml

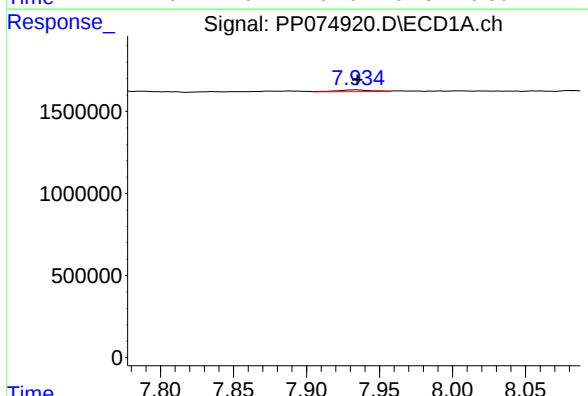


#30 AR-1254-5

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 170321
Conc: 2.05 ng/ml

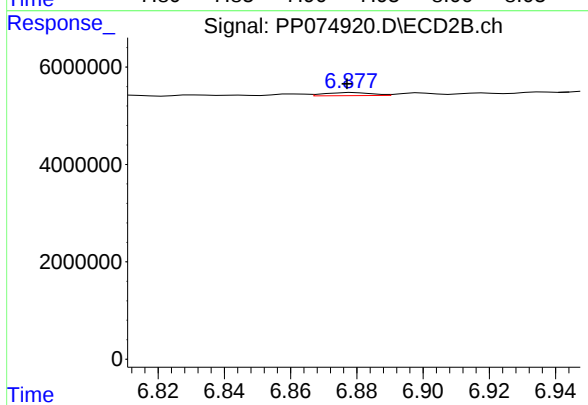

#30 AR-1254-5


R.T.: 6.879 min
Delta R.T.: 0.002 min
Response: 641212
Conc: 1.31 ng/ml

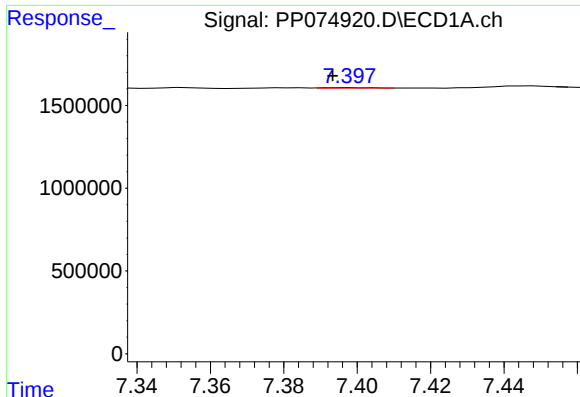

#31 AR-1260-1


R.T.: 7.398 min
Delta R.T.: 0.005 min
Response: 26669
Conc: 0.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

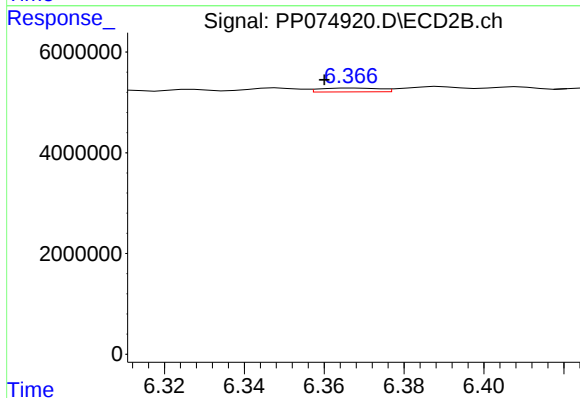


#31 AR-1260-1

R.T.: 6.367 min
Delta R.T.: 0.007 min
Response: 794970
Conc: 2.12 ng/ml

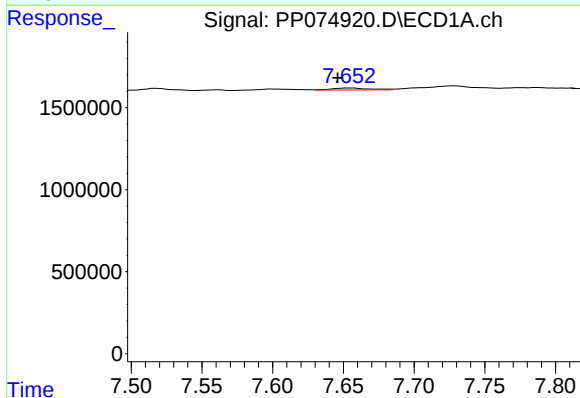


#32 AR-1260-2

R.T.: 7.655 min
Delta R.T.: 0.009 min
Response: 208401
Conc: 3.02 ng/ml

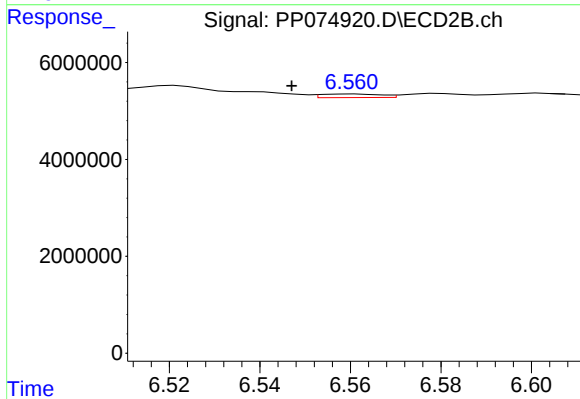

#32 AR-1260-2


R.T.: 6.561 min
Delta R.T.: 0.014 min
Response: 689421
Conc: 1.30 ng/ml

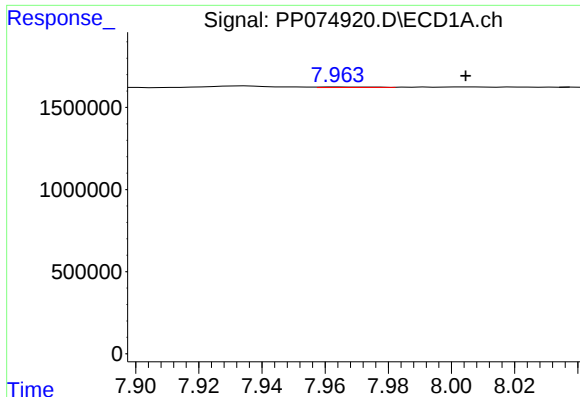

#33 AR-1260-3


R.T.: 7.964 min
Delta R.T.: -0.040 min
Response: 30192
Conc: 0.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

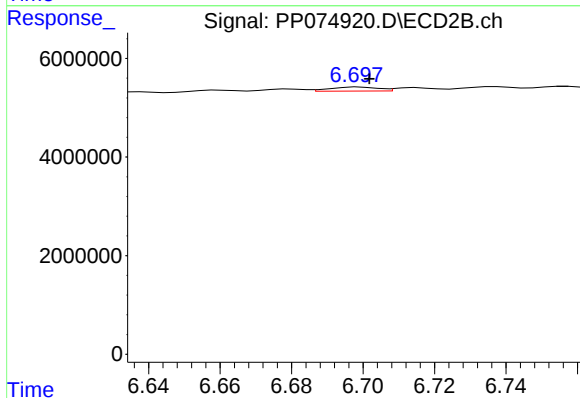


#33 AR-1260-3

R.T.: 6.699 min
Delta R.T.: -0.003 min
Response: 776780
Conc: 1.79 ng/ml

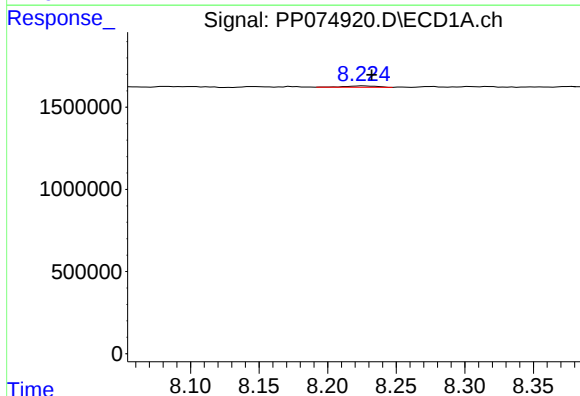


#34 AR-1260-4

R.T.: 8.226 min
Delta R.T.: -0.006 min
Response: 134645
Conc: 2.11 ng/ml

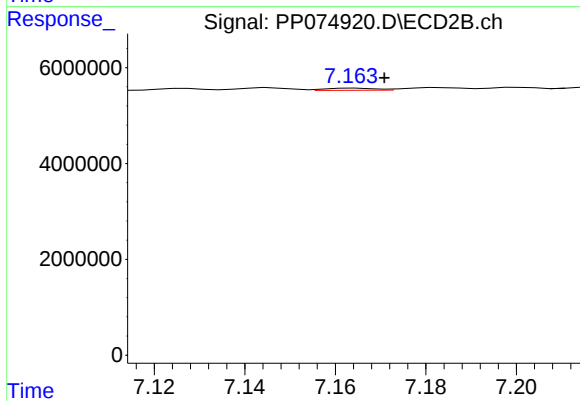

#34 AR-1260-4


R.T.: 7.164 min
Delta R.T.: -0.007 min
Response: 334758
Conc: 0.88 ng/ml

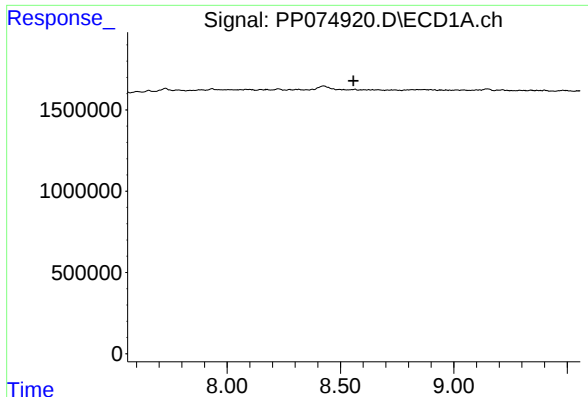

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.558 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

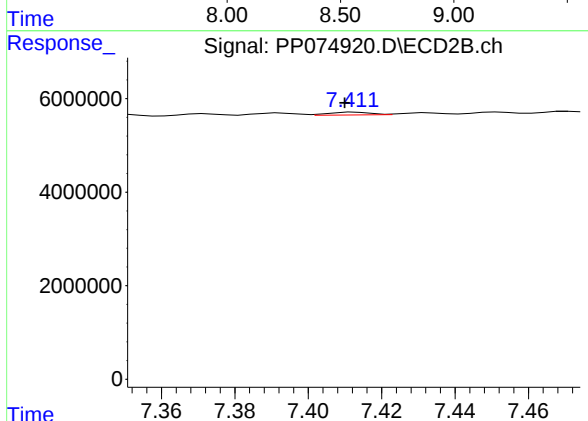


#35 AR-1260-5

R.T.: 7.413 min
Delta R.T.: 0.003 min
Response: 472828
Conc: 0.47 ng/ml

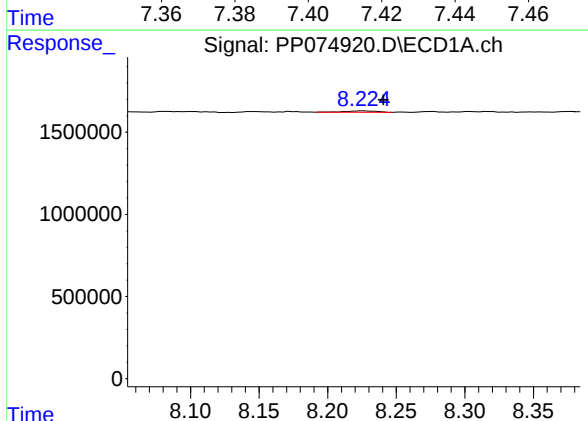


#36 AR-1262-1

R.T.: 8.226 min
Delta R.T.: -0.015 min
Response: 134645
Conc: 1.75 ng/ml

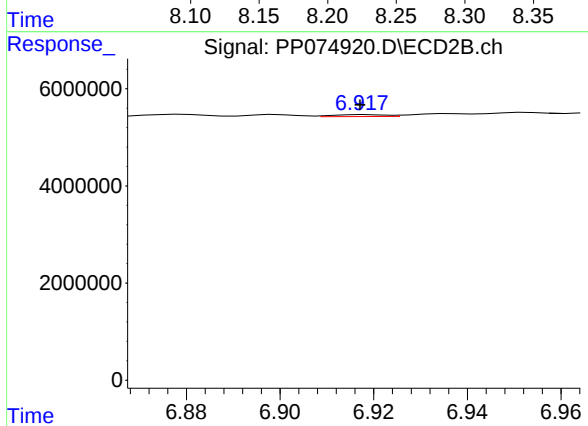

#36 AR-1262-1


R.T.: 6.918 min
Delta R.T.: 0.001 min
Response: 310086
Conc: 0.44 ng/ml

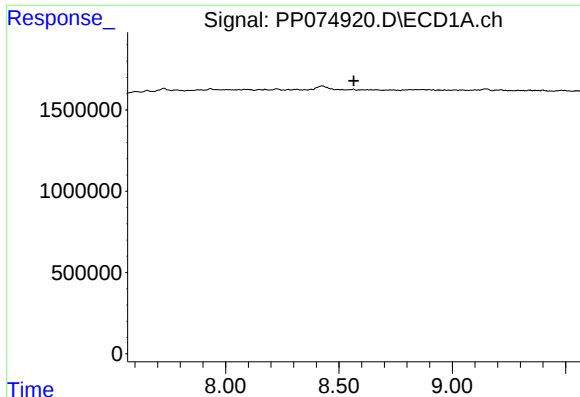

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.566 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

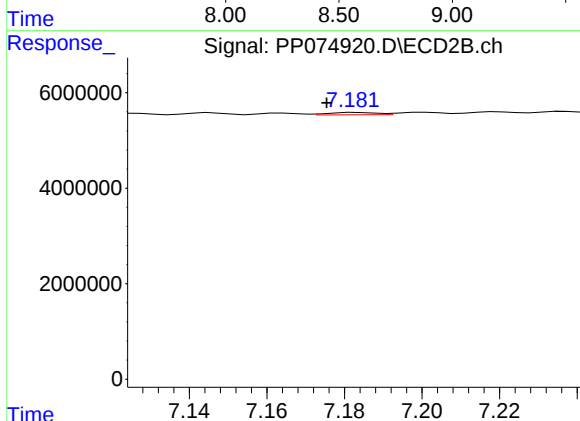


#37 AR-1262-2

R.T.: 7.183 min
Delta R.T.: 0.007 min
Response: 429748
Conc: 0.83 ng/ml

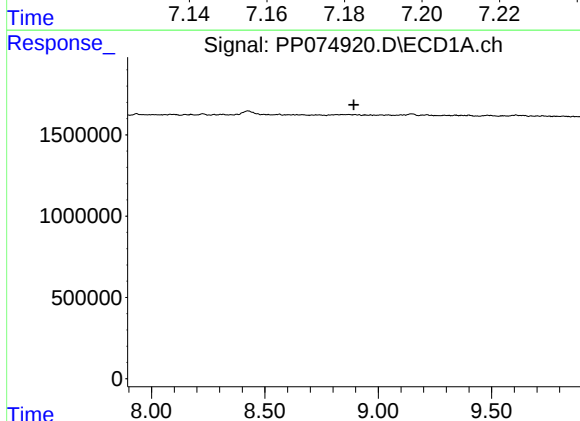


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 8.892 min
Response: 0
Conc: N.D.

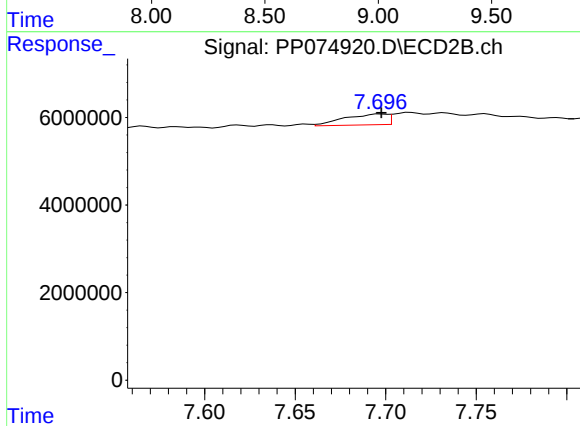

#38 AR-1262-3


R.T.: 7.698 min
Delta R.T.: 0.000 min
Response: 4069954
Conc: 8.73 ng/ml

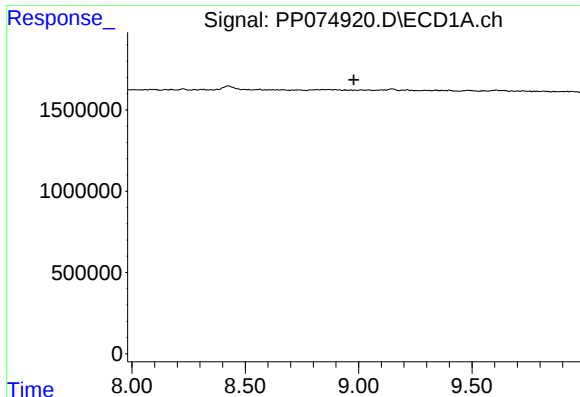

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

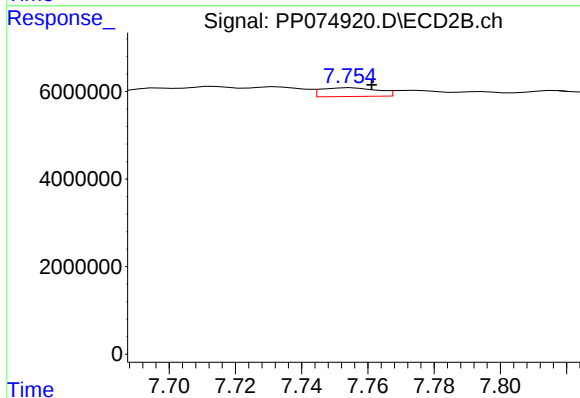


#39 AR-1262-4

R.T.: 7.755 min
Delta R.T.: -0.006 min
Response: 2381794
Conc: 2.90 ng/ml

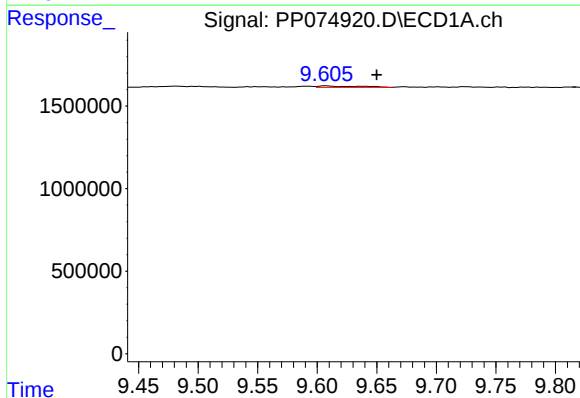


#40 AR-1262-5

R.T.: 9.607 min
Delta R.T.: -0.043 min
Response: 208617
Conc: 3.42 ng/ml

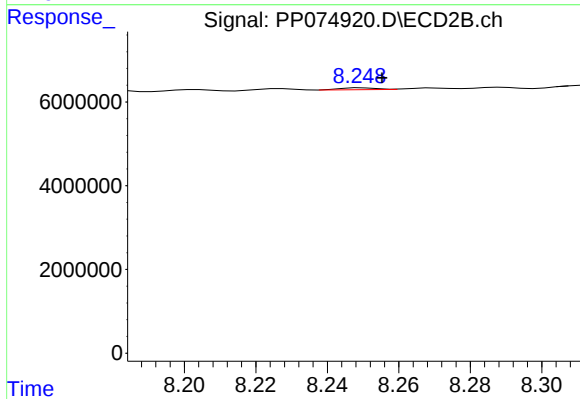

#40 AR-1262-5


R.T.: 8.250 min
Delta R.T.: -0.005 min
Response: 316875
Conc: 0.88 ng/ml

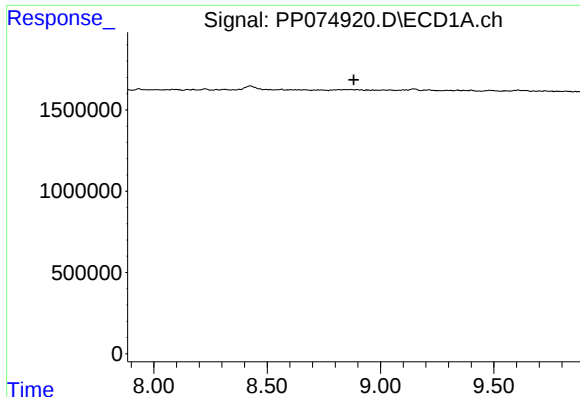

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

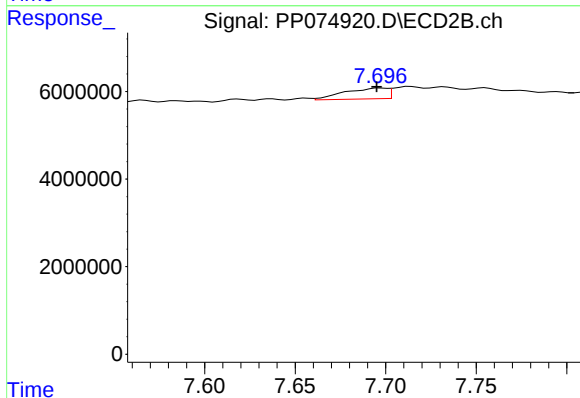


#41 AR-1268-1

R.T.: 7.698 min
Delta R.T.: 0.002 min
Response: 4069954
Conc: 2.89 ng/ml

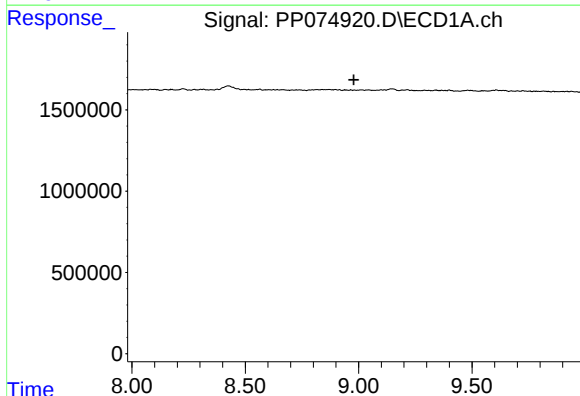


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

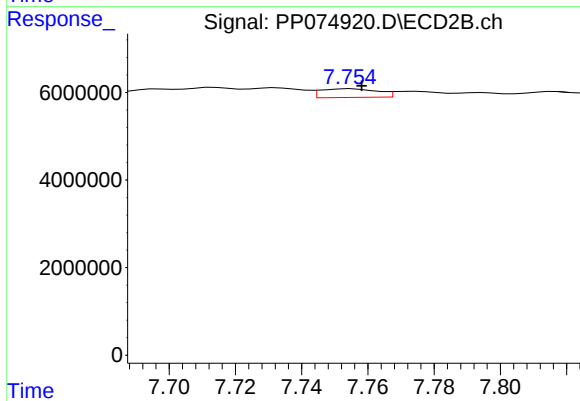

#42 AR-1268-2


R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 2381794
Conc: 1.75 ng/ml

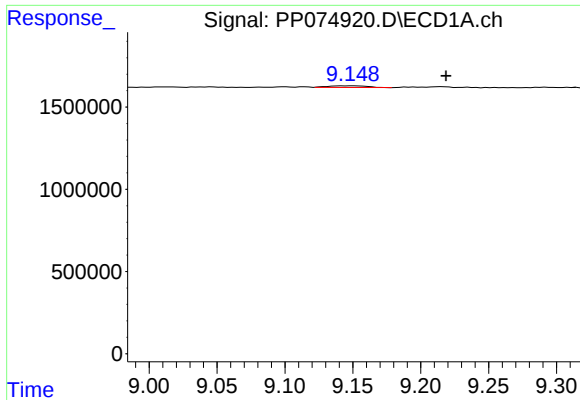

#43 AR-1268-3


R.T.: 9.149 min
Delta R.T.: -0.069 min
Response: 206991
Conc: 1.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

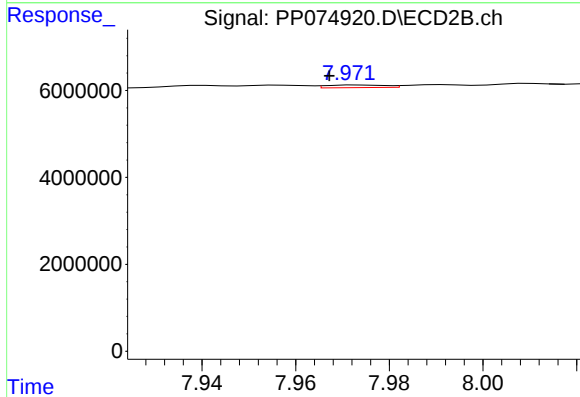


#43 AR-1268-3

R.T.: 7.974 min
Delta R.T.: 0.006 min
Response: 512751
Conc: 0.49 ng/ml

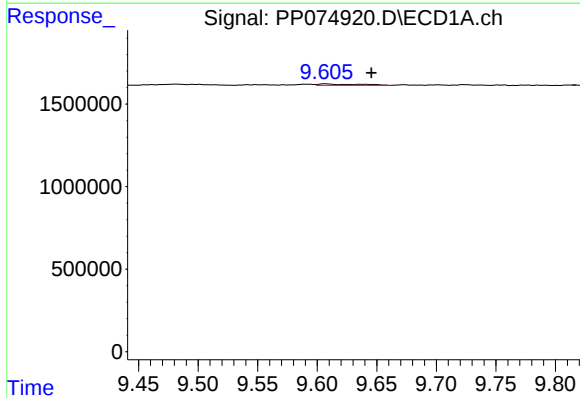


#44 AR-1268-4

R.T.: 9.607 min
Delta R.T.: -0.038 min
Response: 208617
Conc: 3.10 ng/ml

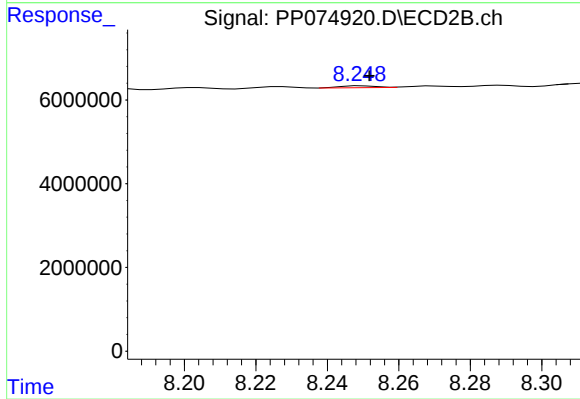

#44 AR-1268-4


R.T.: 8.250 min
Delta R.T.: -0.002 min
Response: 316875
Conc: 0.83 ng/ml

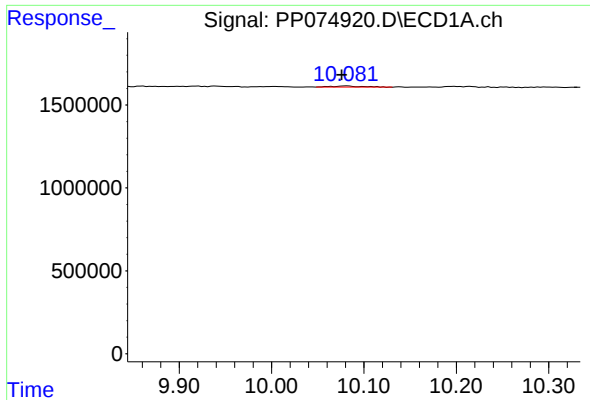

#45 AR-1268-5

R.T.: 10.082 min
Delta R.T.: 0.006 min
Response: 138584
Conc: 0.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

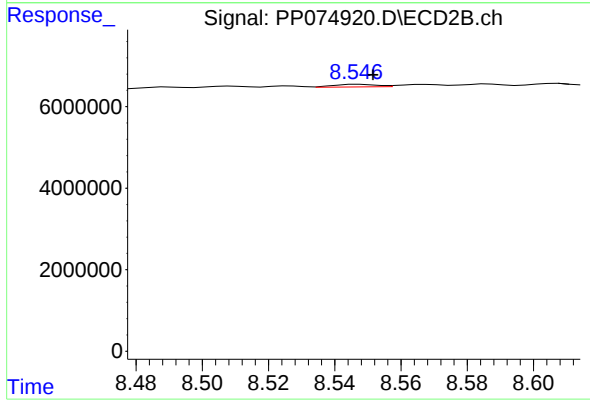

#45 AR-1268-5

R.T.: 8.547 min
Delta R.T.: -0.004 min
Response: 577436
Conc: 0.18 ng/ml