

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 20:44
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1232 WATER MDL 25PPB
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:44:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.658	3.800	27876039	103.1E6	22.780	21.313
2)	SA Decachlor...	10.435	8.808	22424853	141.3E6	22.708	18.847
Target Compounds							
3)	L1 AR-1016-1	5.810	4.898	655693	5310400	14.872	10.426 #
4)	L1 AR-1016-2	5.832	4.958	932301	2791028	14.836	11.726
5)	L1 AR-1016-3	5.894	5.073	865822	1669547	19.277	12.107 #
6)	L1 AR-1016-4	5.990	5.109	586031	692069	16.657	4.950 #
7)	L1 AR-1016-5	6.284	5.329	439298	2042955	13.237	12.301
8)	L2 AR-1221-1	4.856	4.018	525025	913427	29.843	14.764 #
9)	L2 AR-1221-2	4.959	4.095	846655	2166771	63.386	47.925
10)	L2 AR-1221-3	5.019	4.173	885689	2600596	23.361	15.829 #
11)	L3 AR-1232-1	5.019	4.173	885689	2600596	29.160	20.302 #
12)	L3 AR-1232-2	5.545	4.898	513616	5310400	32.594	22.910 #
13)	L3 AR-1232-3	5.832	5.073	932301	1669547	30.524	27.798
14)	L3 AR-1232-4	5.990	5.164	586031	2416896	33.935	32.790
15)	L3 AR-1232-5	6.081	5.329	483461	2042955	37.244	32.906
16)	L4 AR-1242-1	5.810	4.898	655693	5310400	17.131	12.591 #
17)	L4 AR-1242-2	5.832	4.958	932301	2791028	16.506	13.935
18)	L4 AR-1242-3	5.894	5.073	865822	1669547	21.324	14.113 #
19)	L4 AR-1242-4	5.990	5.164	586031	2416896	18.462	14.121
20)	L4 AR-1242-5	6.720	5.681	1393119	2391989	38.622	12.918 #
21)	L5 AR-1248-1	5.810	4.898	655693	5310400	21.694	19.231
22)	L5 AR-1248-2	6.081	5.125	483461	681455	11.218	3.855 #
23)	L5 AR-1248-3	6.284	5.164	439298	2416896	9.406	10.638
24)	L5 AR-1248-4	6.681	5.329	598892	2042955	10.889	9.370
25)	L5 AR-1248-5	6.720	5.758f	1393119	18228371	25.115	49.625 #
26)	L6 AR-1254-1	6.655	5.681	977659	2391989	16.778	5.018 #
27)	L6 AR-1254-2	6.877	5.821	630703	2270857	7.728	6.449
28)	L6 AR-1254-3	7.228	6.227	2295478	1217347	25.732	1.964 #
29)	L6 AR-1254-4	7.518	6.460	227530	1186431	3.452	2.532 #
30)	L6 AR-1254-5	7.935	6.875	528031	1381147	6.355	2.816 #
31)	L7 AR-1260-1	7.397	6.364	64511	499167	1.116	1.330
32)	L7 AR-1260-2	7.651	6.560	207232	497368	3.007	0.941 #
33)	L7 AR-1260-3	8.004	6.700	189184	646341	3.646	1.493 #
34)	L7 AR-1260-4	8.220	7.173	305311	493617	4.786	1.294 #
35)	L7 AR-1260-5	8.561	7.421	162011	493468	1.429	0.491 #
36)	L8 AR-1262-1	8.220	6.918	305311	536017	3.964	0.758 #
37)	L8 AR-1262-2	8.561	7.173	162011	493617	1.224	0.948
38)	L8 AR-1262-3	0.000	7.707	0	4698330	N.D.	10.076 #
39)	L8 AR-1262-4	0.000	7.758	0	1065996	N.D.	1.297 #
40)	L8 AR-1262-5	9.606f	8.248	128730	212505	2.112	0.593 #
41)	L9 AR-1268-1	0.000	7.707	0	4698330	N.D.	3.331 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074921.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 20:44
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1232 WATER MDL 25PPB
 ALS Vial : 16 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:44:35 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.758	0	1065996	N.D.	0.782 #
43) L9	AR-1268-3	9.152f	7.971	133506	570921	1.080	0.547 #
44) L9	AR-1268-4	9.606f	8.248	128730	212505	1.914	0.555 #
45) L9	AR-1268-5	10.084	8.556	78951	475639	0.213	0.152 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

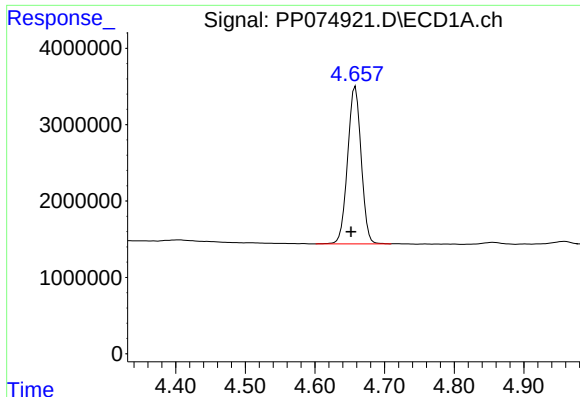

#1 Tetrachloro-m-xylene


R.T.: 4.658 min
Delta R.T.: 0.006 min
Response: 27876039
Conc: 22.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

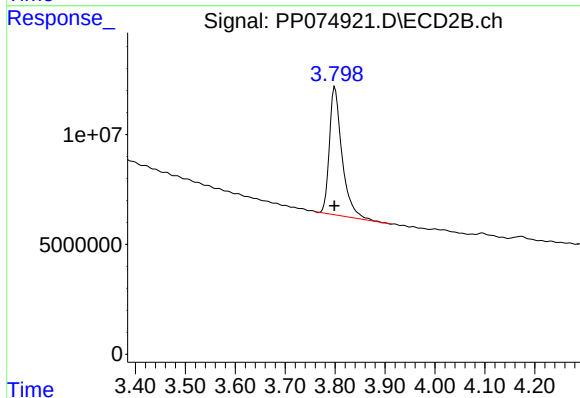


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 103056627
Conc: 21.31 ng/ml

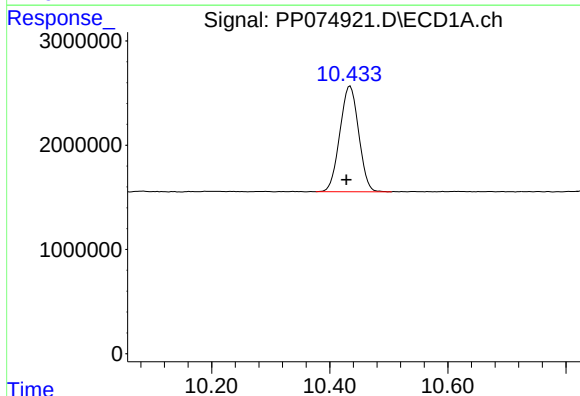


#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.006 min
Response: 22424853
Conc: 22.71 ng/ml

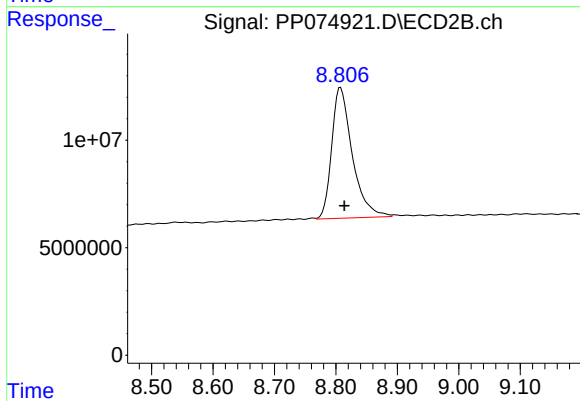

#2 Decachlorobiphenyl


R.T.: 8.808 min
Delta R.T.: -0.006 min
Response: 141336463
Conc: 18.85 ng/ml

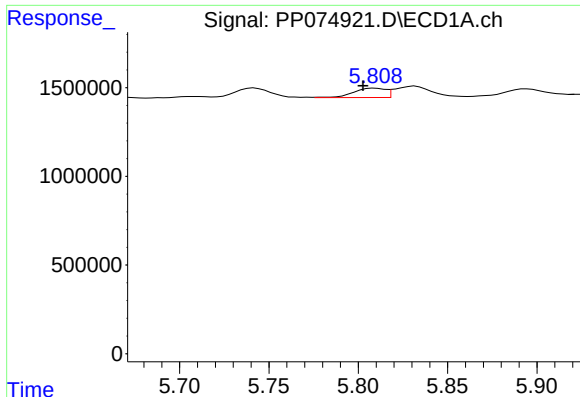

#3 AR-1016-1


R.T.: 5.810 min
Delta R.T.: 0.007 min
Response: 655693
Conc: 14.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

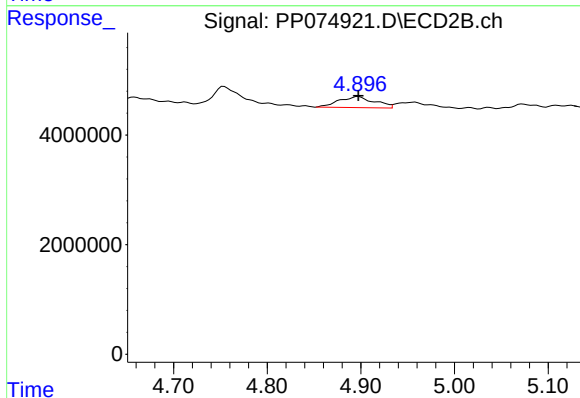


#3 AR-1016-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 5310400
Conc: 10.43 ng/ml

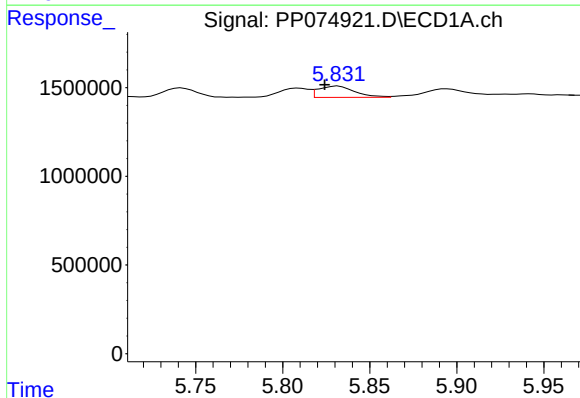


#4 AR-1016-2

R.T.: 5.832 min
Delta R.T.: 0.008 min
Response: 932301
Conc: 14.84 ng/ml

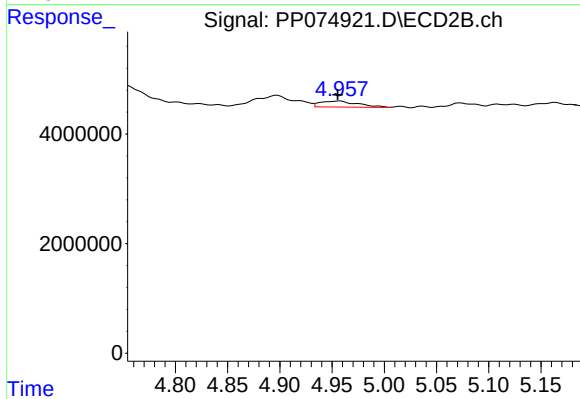

#4 AR-1016-2


R.T.: 4.958 min
Delta R.T.: 0.002 min
Response: 2791028
Conc: 11.73 ng/ml

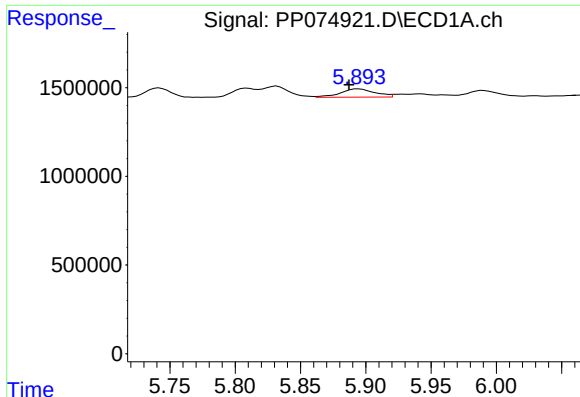

#5 AR-1016-3


R.T.: 5.894 min
Delta R.T.: 0.007 min
Response: 865822
Conc: 19.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

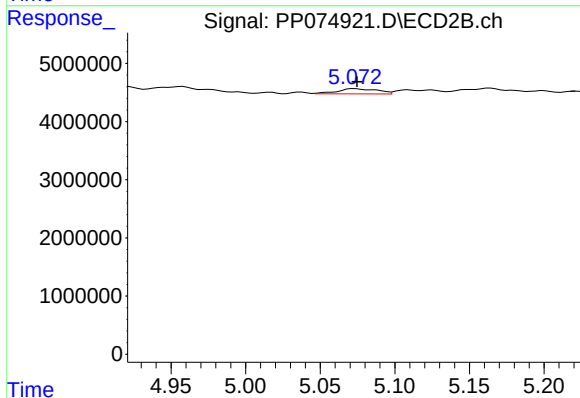


#5 AR-1016-3

R.T.: 5.073 min
Delta R.T.: -0.002 min
Response: 1669547
Conc: 12.11 ng/ml

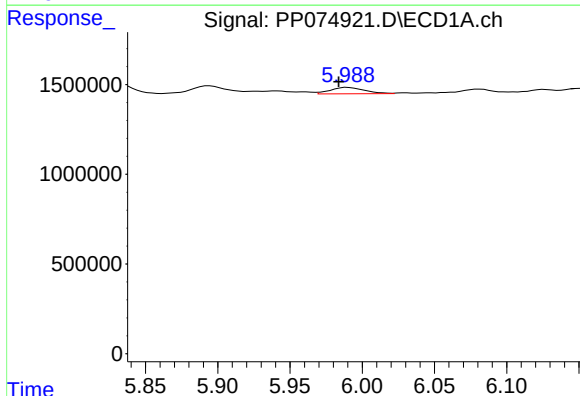


#6 AR-1016-4

R.T.: 5.990 min
Delta R.T.: 0.006 min
Response: 586031
Conc: 16.66 ng/ml

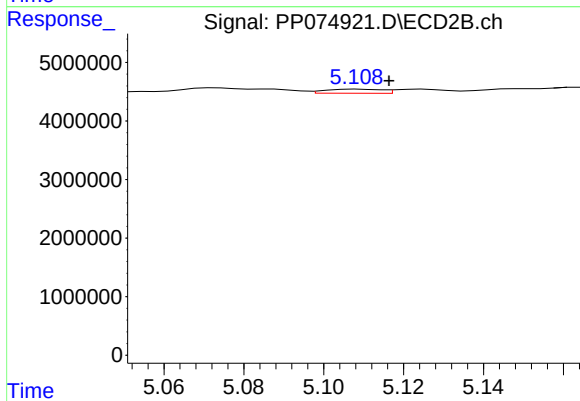

#6 AR-1016-4


R.T.: 5.109 min
Delta R.T.: -0.008 min
Response: 692069
Conc: 4.95 ng/ml

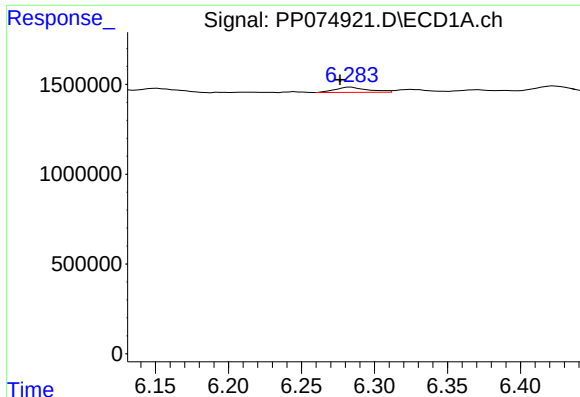

#7 AR-1016-5


R.T.: 6.284 min
Delta R.T.: 0.008 min
Response: 439298
Conc: 13.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

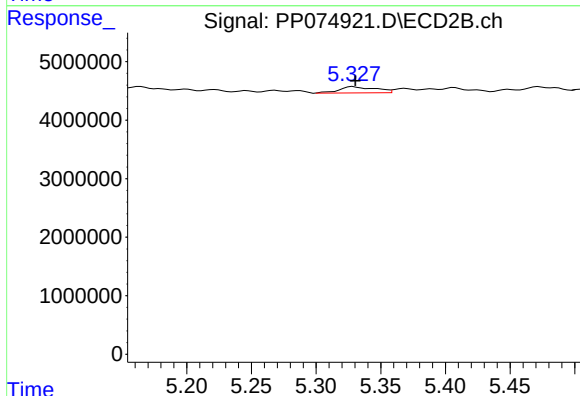


#7 AR-1016-5

R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 2042955
Conc: 12.30 ng/ml

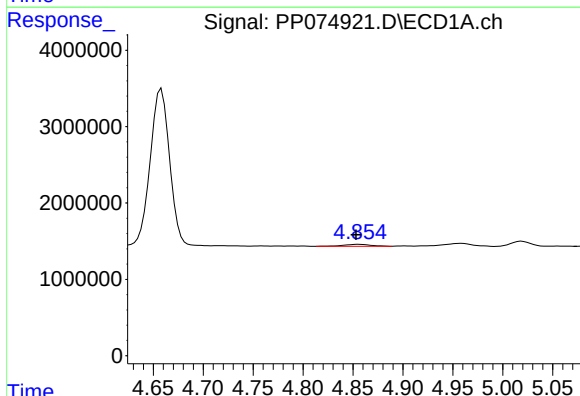


#8 AR-1221-1

R.T.: 4.856 min
Delta R.T.: 0.003 min
Response: 525025
Conc: 29.84 ng/ml

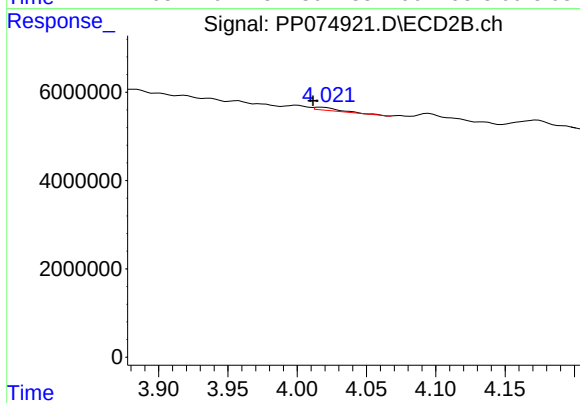

#8 AR-1221-1


R.T.: 4.018 min
Delta R.T.: 0.006 min
Response: 913427
Conc: 14.76 ng/ml

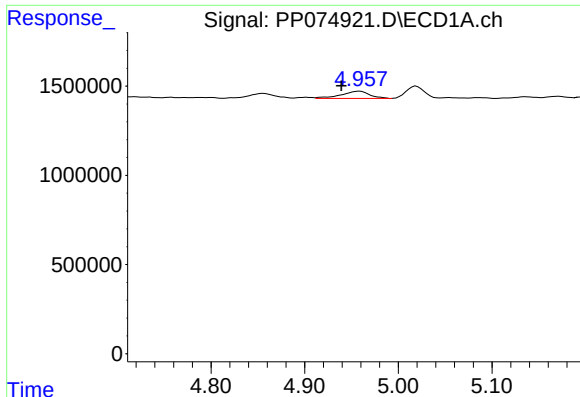

#9 AR-1221-2


R.T.: 4.959 min
Delta R.T.: 0.020 min
Response: 846655
Conc: 63.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

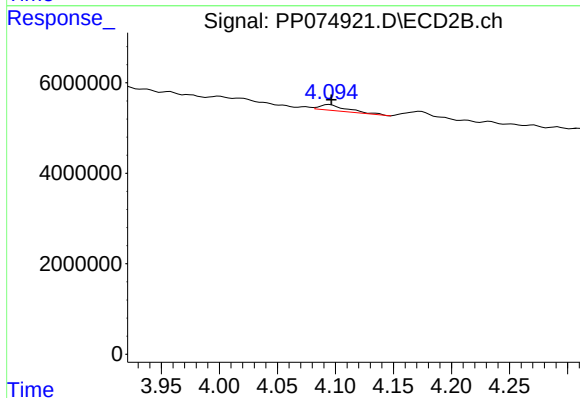


#9 AR-1221-2

R.T.: 4.095 min
Delta R.T.: -0.002 min
Response: 2166771
Conc: 47.92 ng/ml

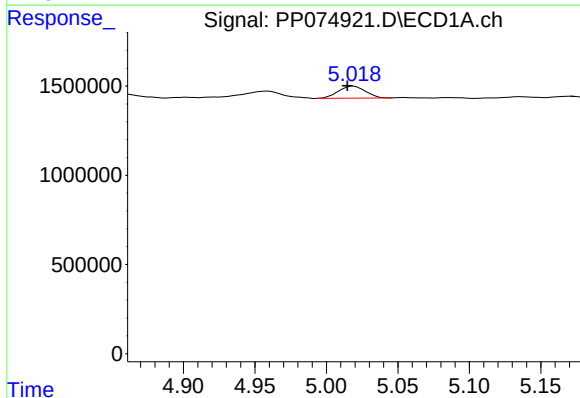


#10 AR-1221-3

R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 885689
Conc: 23.36 ng/ml

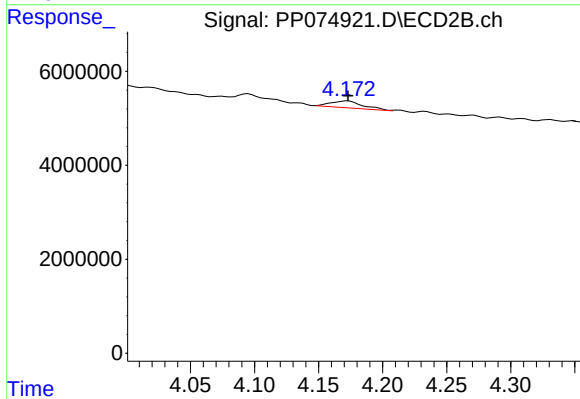

#10 AR-1221-3


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 2600596
Conc: 15.83 ng/ml

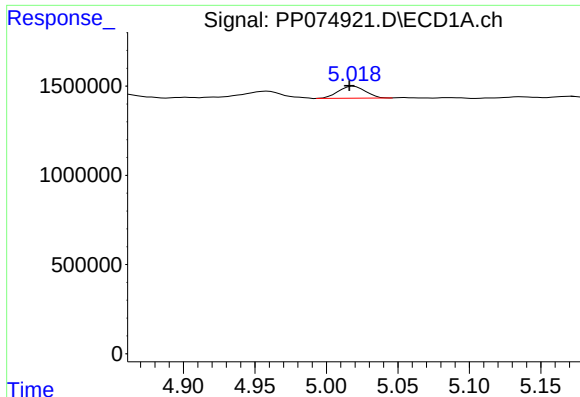

#11 AR-1232-1


R.T.: 5.019 min
Delta R.T.: 0.003 min
Response: 885689
Conc: 29.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

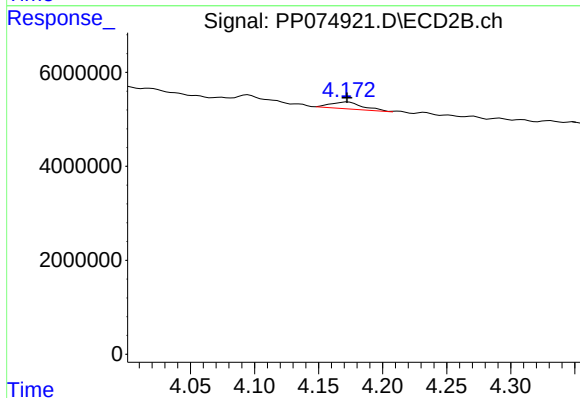


#11 AR-1232-1

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 2600596
Conc: 20.30 ng/ml

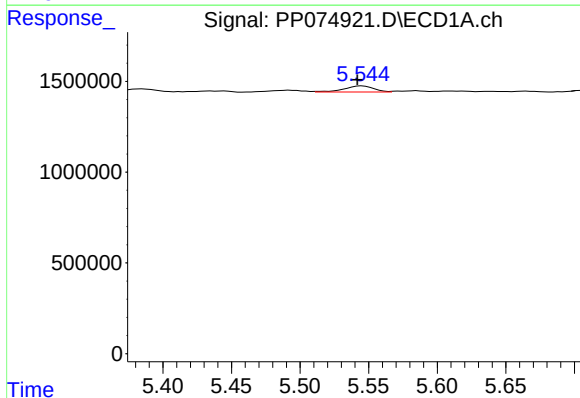


#12 AR-1232-2

R.T.: 5.545 min
Delta R.T.: 0.003 min
Response: 513616
Conc: 32.59 ng/ml

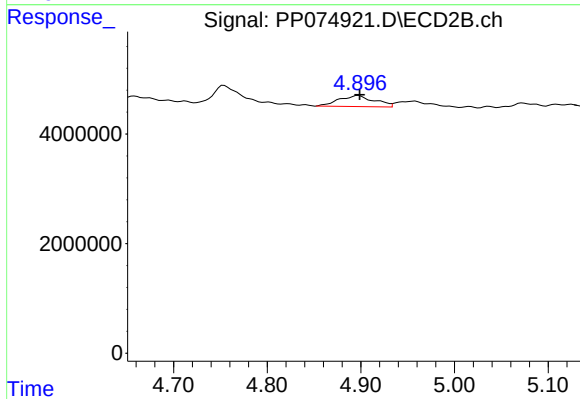

#12 AR-1232-2


R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 5310400
Conc: 22.91 ng/ml

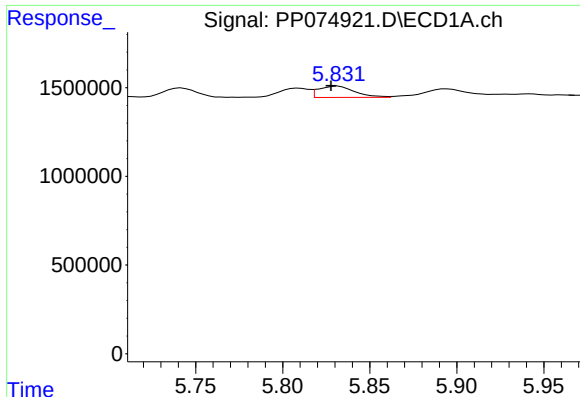

#13 AR-1232-3


R.T.: 5.832 min
Delta R.T.: 0.004 min
Response: 932301
Conc: 30.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

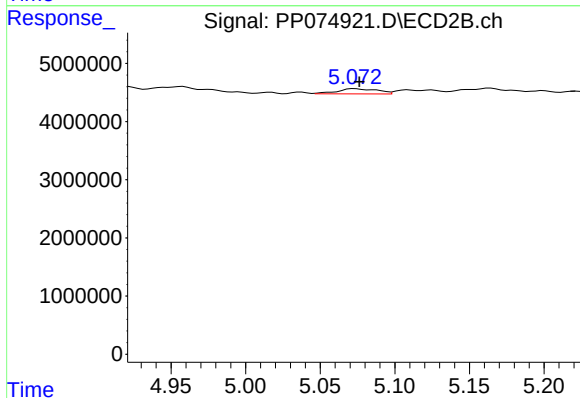


#13 AR-1232-3

R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 1669547
Conc: 27.80 ng/ml

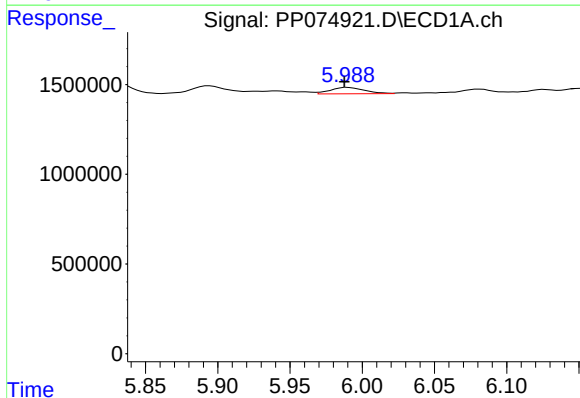


#14 AR-1232-4

R.T.: 5.990 min
Delta R.T.: 0.002 min
Response: 586031
Conc: 33.93 ng/ml

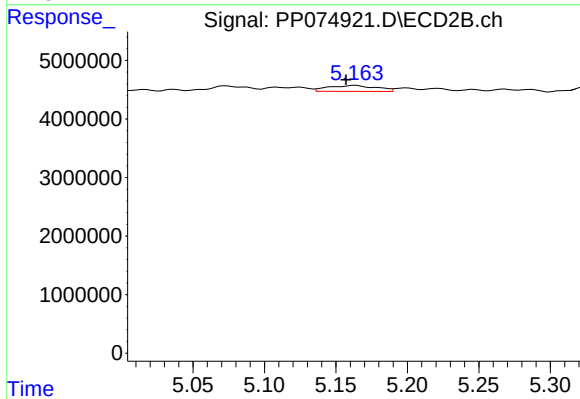

#14 AR-1232-4


R.T.: 5.164 min
Delta R.T.: 0.007 min
Response: 2416896
Conc: 32.79 ng/ml

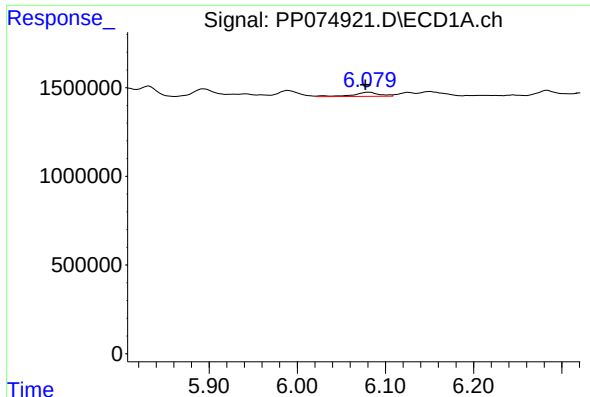

#15 AR-1232-5


R.T.: 6.081 min
Delta R.T.: 0.004 min
Response: 483461
Conc: 37.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

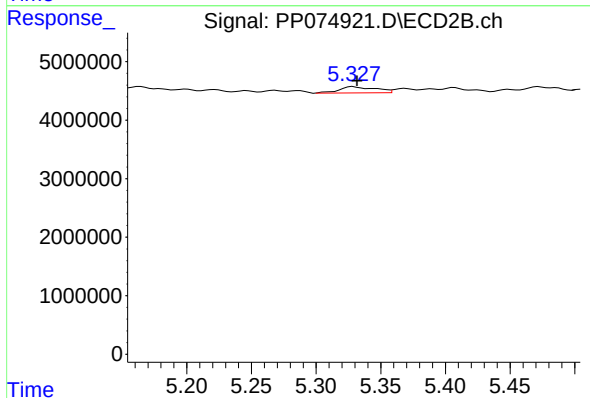


#15 AR-1232-5

R.T.: 5.329 min
Delta R.T.: -0.003 min
Response: 2042955
Conc: 32.91 ng/ml

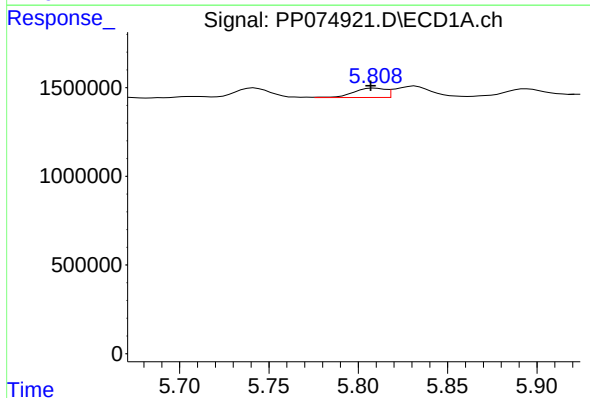


#16 AR-1242-1

R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 655693
Conc: 17.13 ng/ml

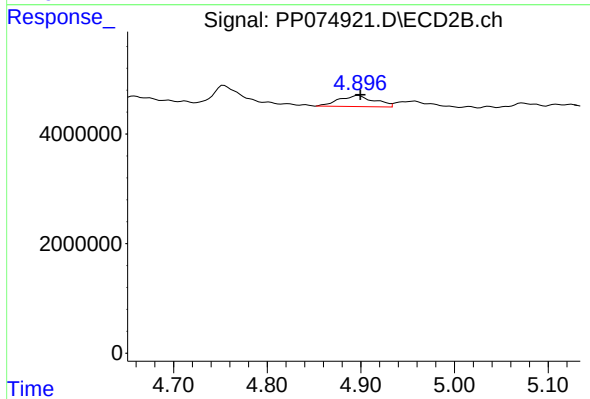

#16 AR-1242-1


R.T.: 4.898 min
Delta R.T.: -0.002 min
Response: 5310400
Conc: 12.59 ng/ml

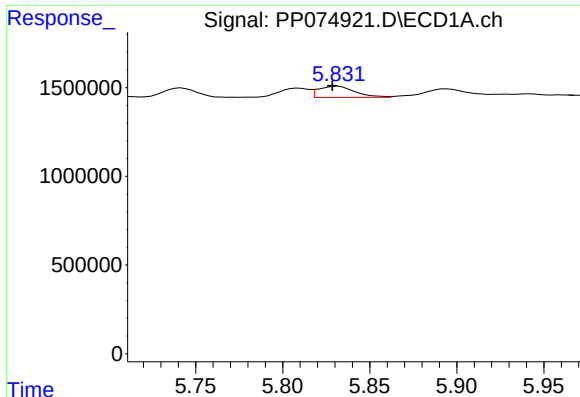

#17 AR-1242-2


R.T.: 5.832 min
Delta R.T.: 0.003 min
Response: 932301
Conc: 16.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

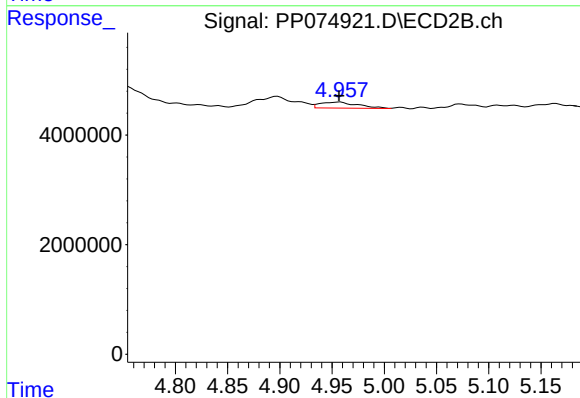


#17 AR-1242-2

R.T.: 4.958 min
Delta R.T.: 0.000 min
Response: 2791028
Conc: 13.94 ng/ml

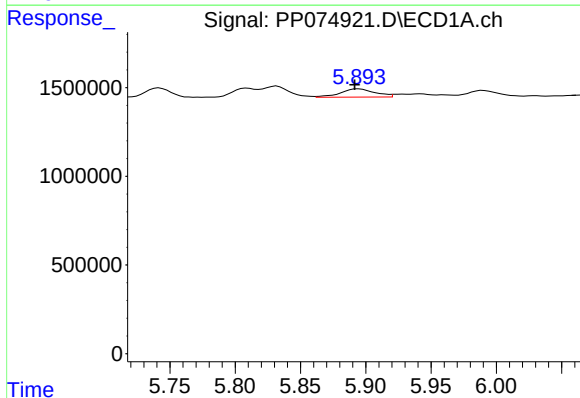


#18 AR-1242-3

R.T.: 5.894 min
Delta R.T.: 0.003 min
Response: 865822
Conc: 21.32 ng/ml

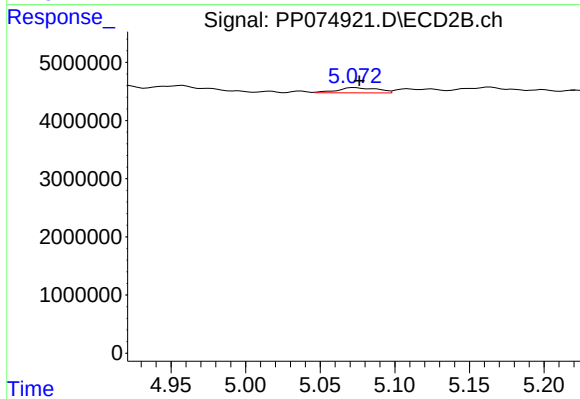

#18 AR-1242-3


R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 1669547
Conc: 14.11 ng/ml

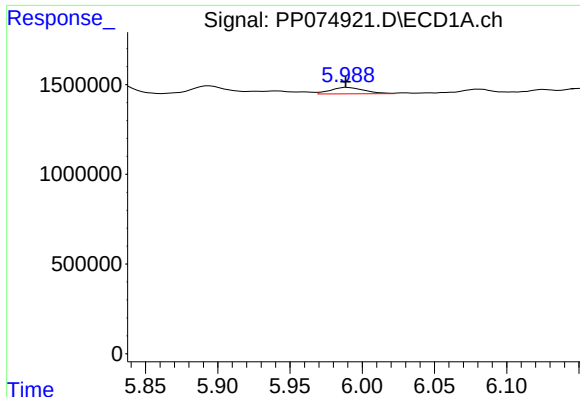

#19 AR-1242-4


R.T.: 5.990 min
Delta R.T.: 0.001 min
Response: 586031
Conc: 18.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

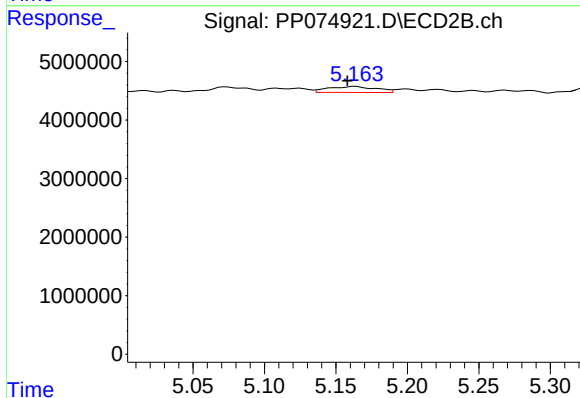


#19 AR-1242-4

R.T.: 5.164 min
Delta R.T.: 0.006 min
Response: 2416896
Conc: 14.12 ng/ml

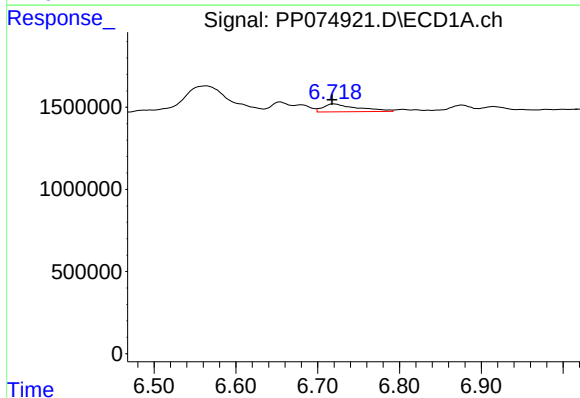


#20 AR-1242-5

R.T.: 6.720 min
Delta R.T.: 0.002 min
Response: 1393119
Conc: 38.62 ng/ml

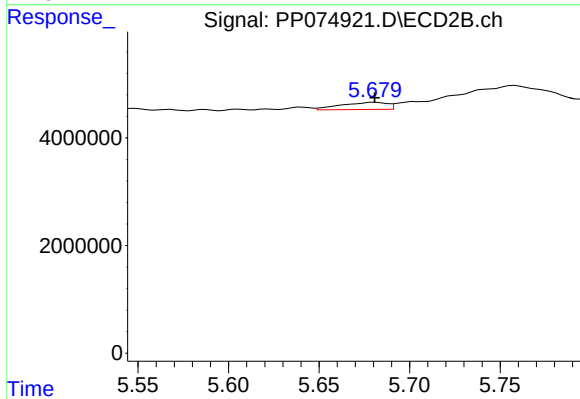

#20 AR-1242-5


R.T.: 5.681 min
Delta R.T.: 0.000 min
Response: 2391989
Conc: 12.92 ng/ml

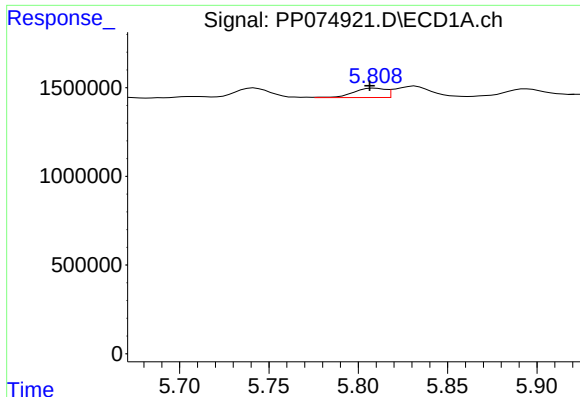

#21 AR-1248-1


R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 655693
Conc: 21.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

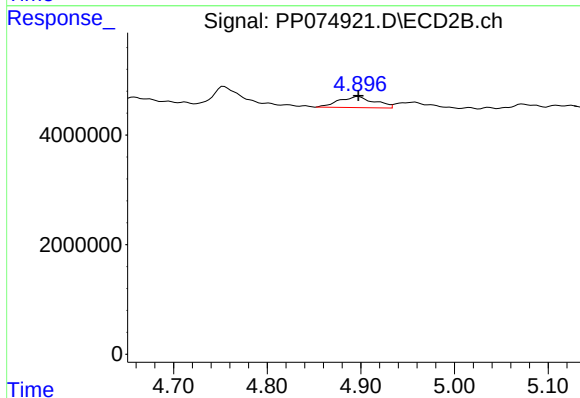


#21 AR-1248-1

R.T.: 4.898 min
Delta R.T.: 0.000 min
Response: 5310400
Conc: 19.23 ng/ml

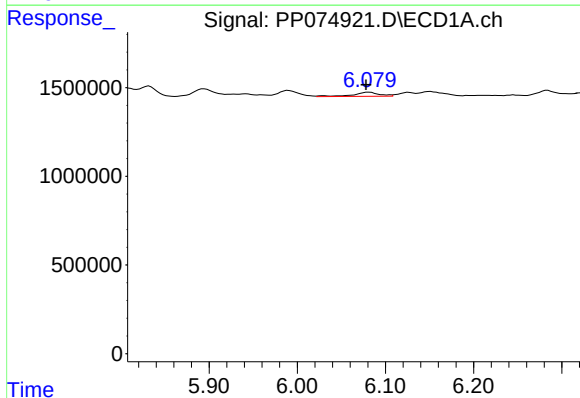


#22 AR-1248-2

R.T.: 6.081 min
Delta R.T.: 0.003 min
Response: 483461
Conc: 11.22 ng/ml

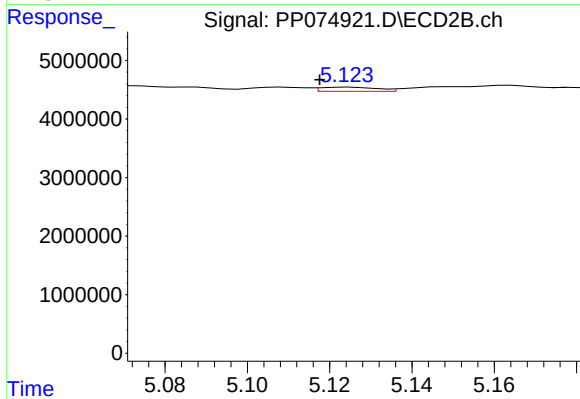

#22 AR-1248-2


R.T.: 5.125 min
Delta R.T.: 0.007 min
Response: 681455
Conc: 3.86 ng/ml

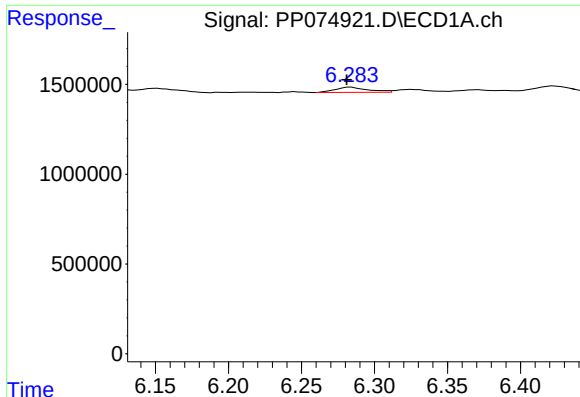

#23 AR-1248-3


R.T.: 6.284 min
Delta R.T.: 0.003 min
Response: 439298
Conc: 9.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

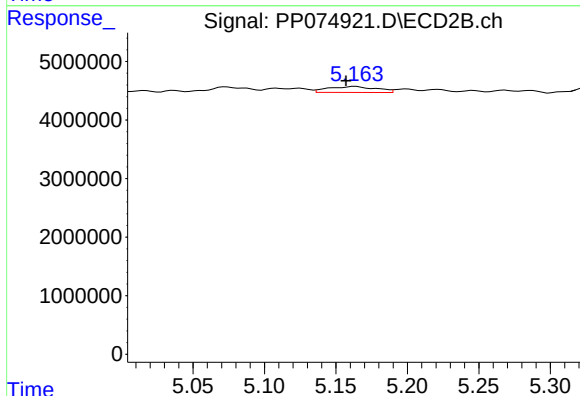


#23 AR-1248-3

R.T.: 5.164 min
Delta R.T.: 0.007 min
Response: 2416896
Conc: 10.64 ng/ml

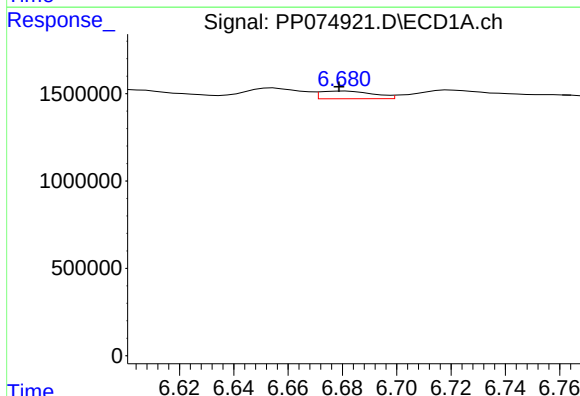


#24 AR-1248-4

R.T.: 6.681 min
Delta R.T.: 0.002 min
Response: 598892
Conc: 10.89 ng/ml

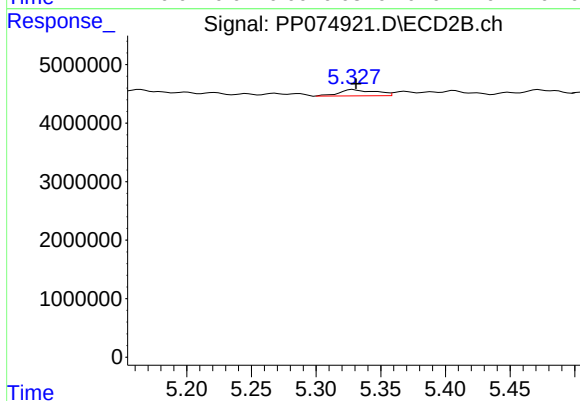

#24 AR-1248-4


R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 2042955
Conc: 9.37 ng/ml

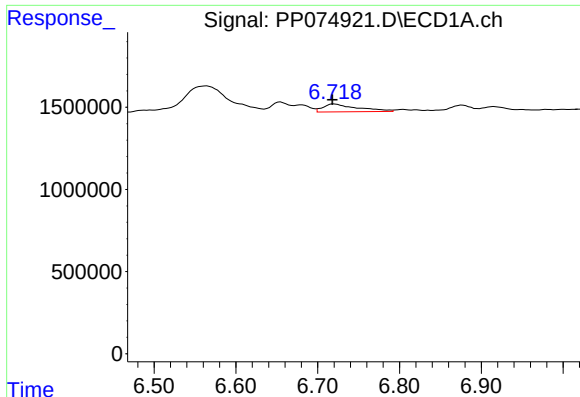

#25 AR-1248-5


R.T.: 6.720 min
Delta R.T.: 0.002 min
Response: 1393119
Conc: 25.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

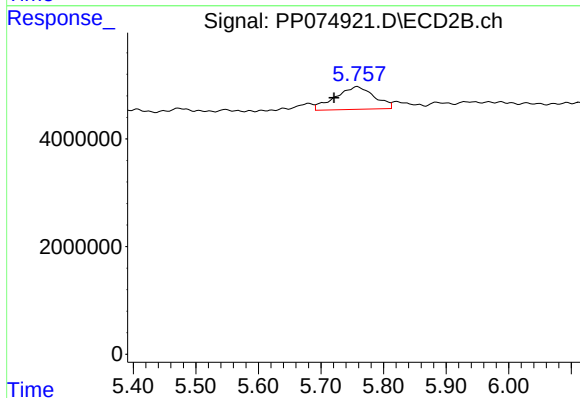


#25 AR-1248-5

R.T.: 5.758 min
Delta R.T.: 0.038 min
Response: 18228371
Conc: 49.63 ng/ml

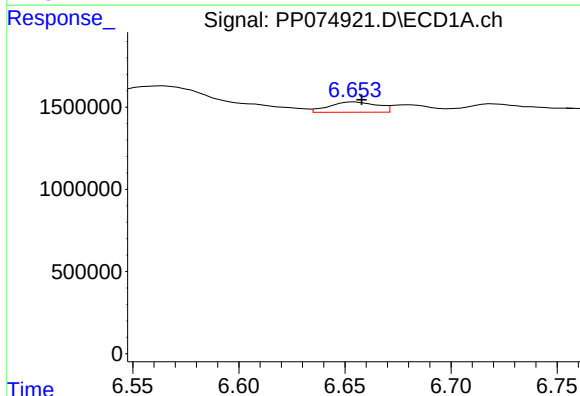


#26 AR-1254-1

R.T.: 6.655 min
Delta R.T.: -0.003 min
Response: 977659
Conc: 16.78 ng/ml

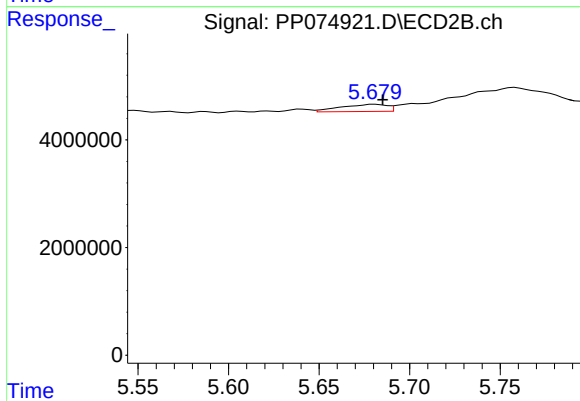

#26 AR-1254-1


R.T.: 5.681 min
Delta R.T.: -0.004 min
Response: 2391989
Conc: 5.02 ng/ml

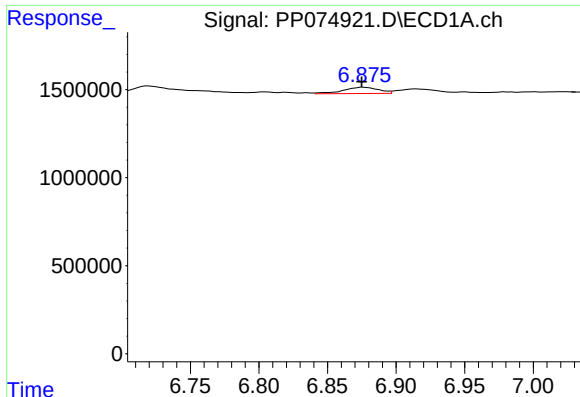

#27 AR-1254-2


R.T.: 6.877 min
Delta R.T.: 0.002 min
Response: 630703
Conc: 7.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

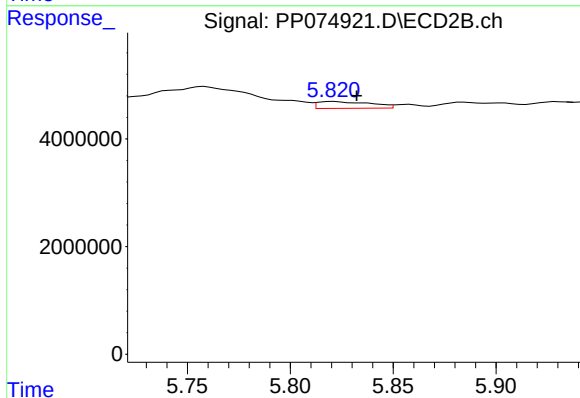


#27 AR-1254-2

R.T.: 5.821 min
Delta R.T.: -0.011 min
Response: 2270857
Conc: 6.45 ng/ml

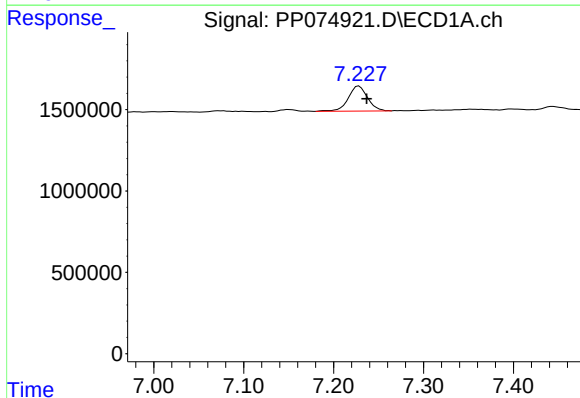


#28 AR-1254-3

R.T.: 7.228 min
Delta R.T.: -0.009 min
Response: 2295478
Conc: 25.73 ng/ml

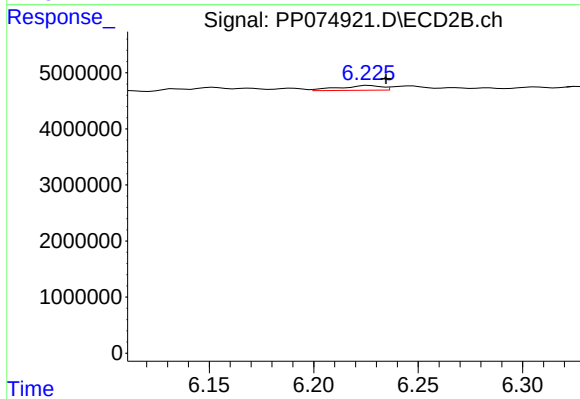

#28 AR-1254-3


R.T.: 6.227 min
Delta R.T.: -0.008 min
Response: 1217347
Conc: 1.96 ng/ml

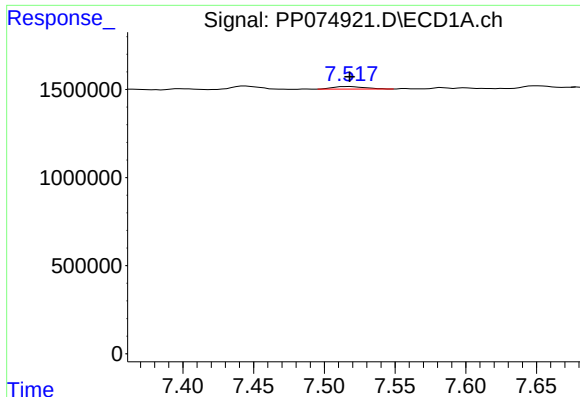

#29 AR-1254-4


R.T.: 7.518 min
Delta R.T.: 0.000 min
Response: 227530
Conc: 3.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

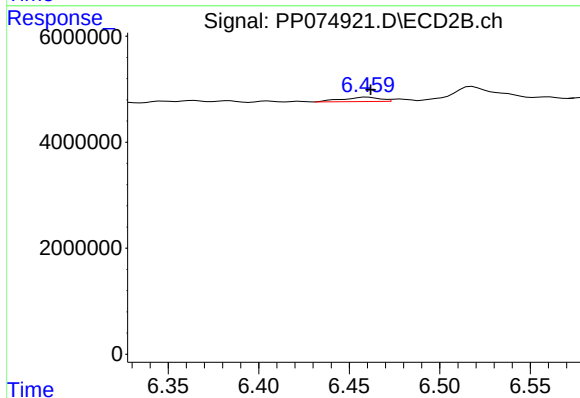


#29 AR-1254-4

R.T.: 6.460 min
Delta R.T.: -0.002 min
Response: 1186431
Conc: 2.53 ng/ml

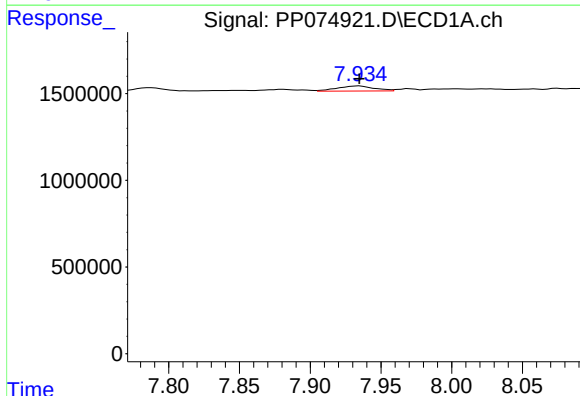


#30 AR-1254-5

R.T.: 7.935 min
Delta R.T.: 0.000 min
Response: 528031
Conc: 6.36 ng/ml

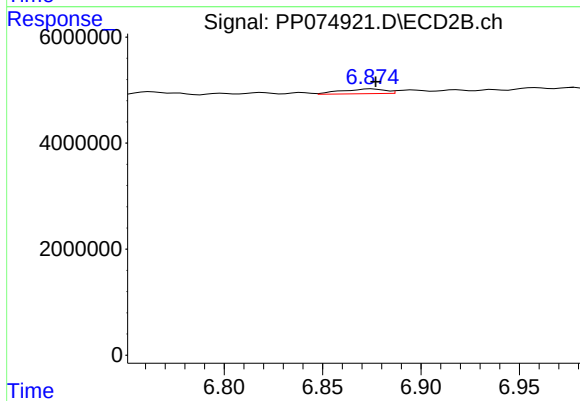

#30 AR-1254-5


R.T.: 6.875 min
Delta R.T.: -0.002 min
Response: 1381147
Conc: 2.82 ng/ml

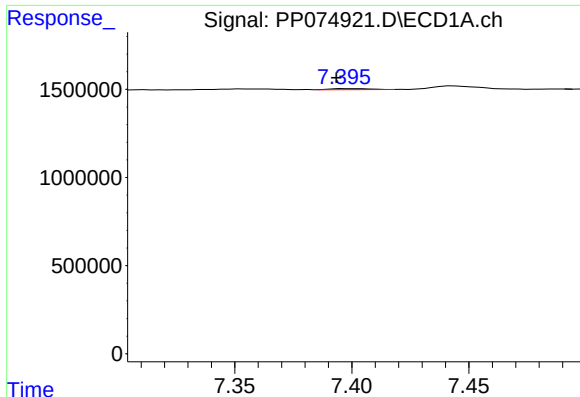

#31 AR-1260-1


R.T.: 7.397 min
Delta R.T.: 0.004 min
Response: 64511
Conc: 1.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

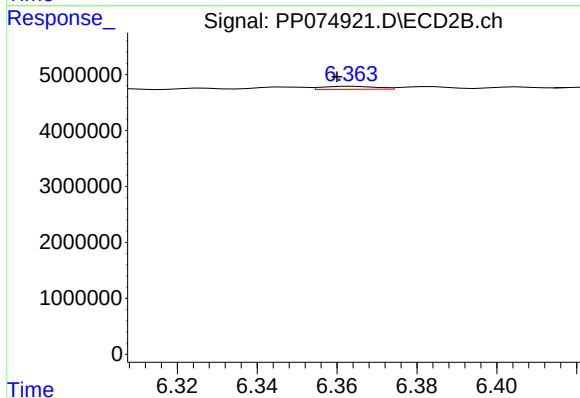


#31 AR-1260-1

R.T.: 6.364 min
Delta R.T.: 0.004 min
Response: 499167
Conc: 1.33 ng/ml

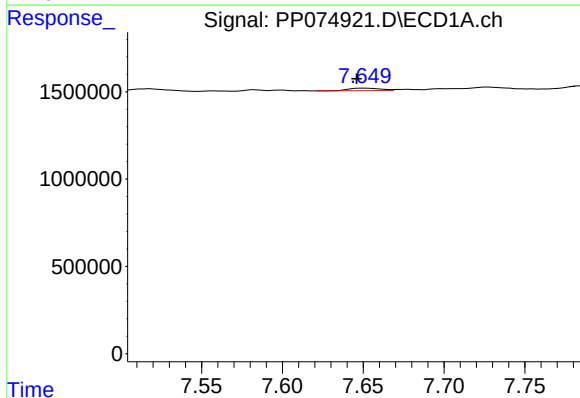


#32 AR-1260-2

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 207232
Conc: 3.01 ng/ml

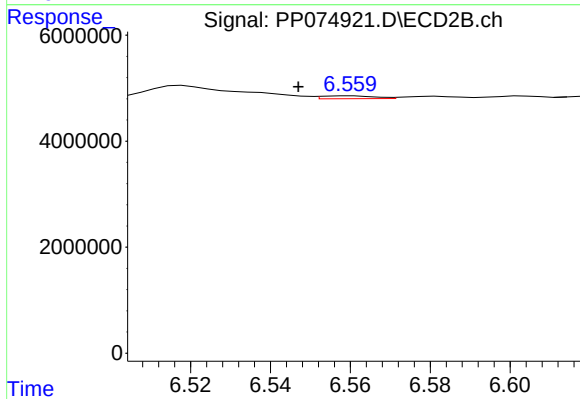

#32 AR-1260-2


R.T.: 6.560 min
Delta R.T.: 0.013 min
Response: 497368
Conc: 0.94 ng/ml

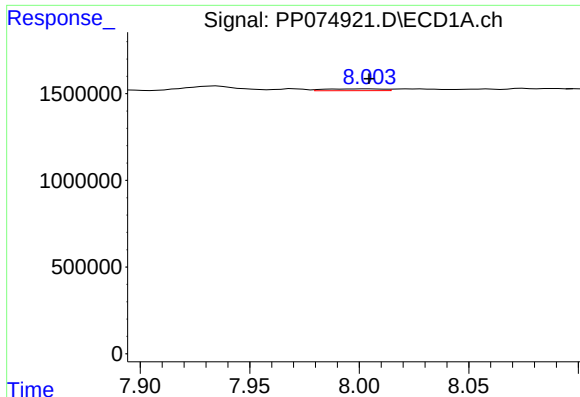

#33 AR-1260-3


R.T.: 8.004 min
Delta R.T.: 0.000 min
Response: 189184
Conc: 3.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

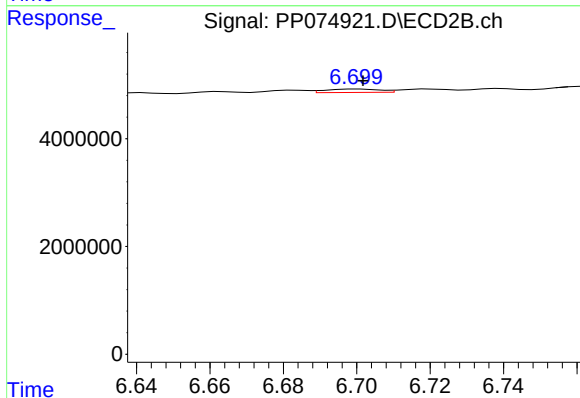


#33 AR-1260-3

R.T.: 6.700 min
Delta R.T.: -0.001 min
Response: 646341
Conc: 1.49 ng/ml

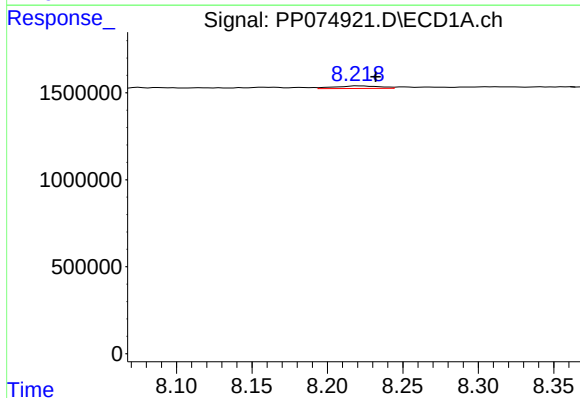


#34 AR-1260-4

R.T.: 8.220 min
Delta R.T.: -0.012 min
Response: 305311
Conc: 4.79 ng/ml

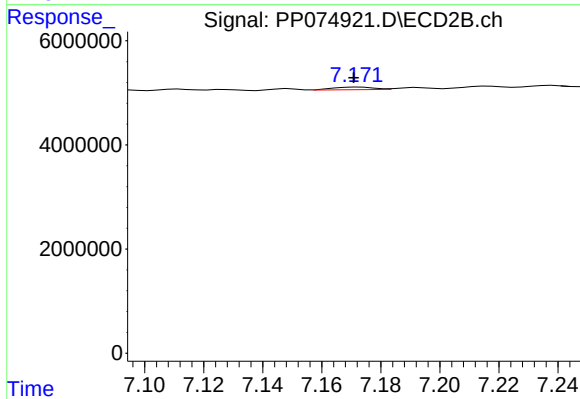

#34 AR-1260-4


R.T.: 7.173 min
Delta R.T.: 0.002 min
Response: 493617
Conc: 1.29 ng/ml

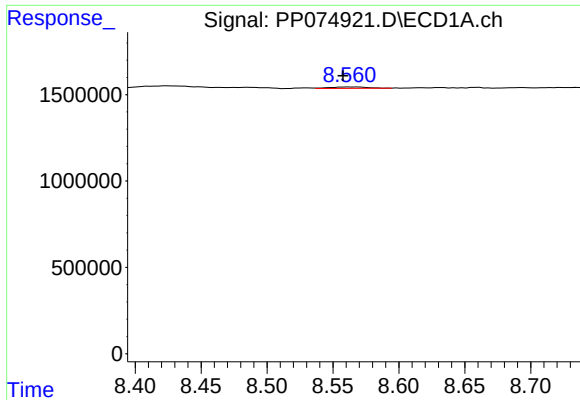

#35 AR-1260-5


R.T.: 8.561 min
Delta R.T.: 0.004 min
Response: 162011
Conc: 1.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

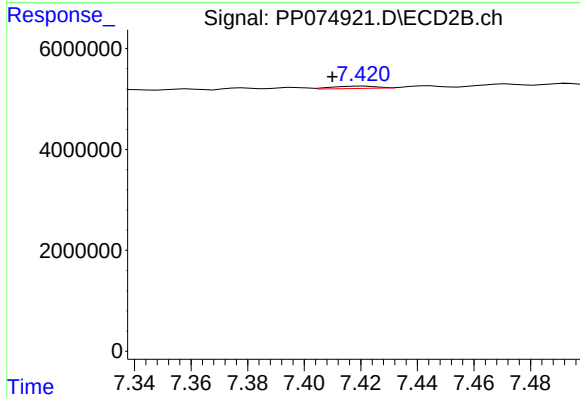


#35 AR-1260-5

R.T.: 7.421 min
Delta R.T.: 0.011 min
Response: 493468
Conc: 0.49 ng/ml

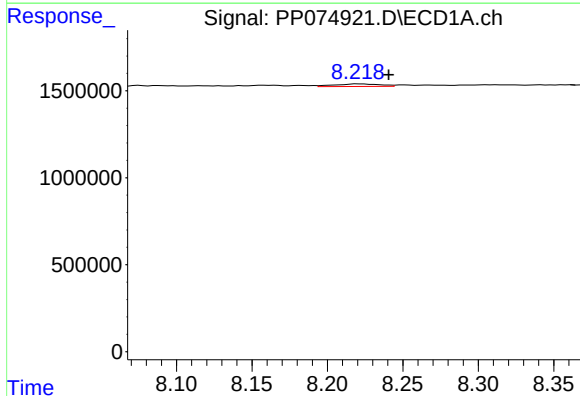


#36 AR-1262-1

R.T.: 8.220 min
Delta R.T.: -0.021 min
Response: 305311
Conc: 3.96 ng/ml

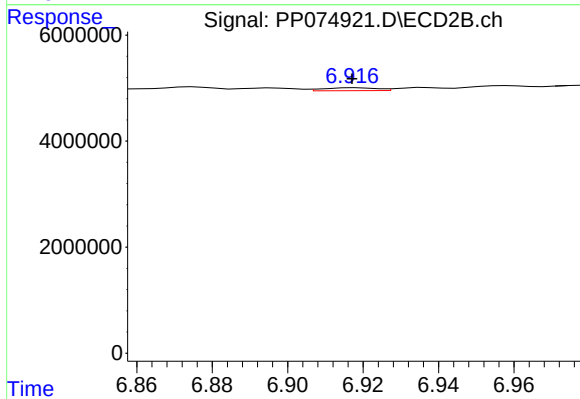

#36 AR-1262-1


R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 536017
Conc: 0.76 ng/ml

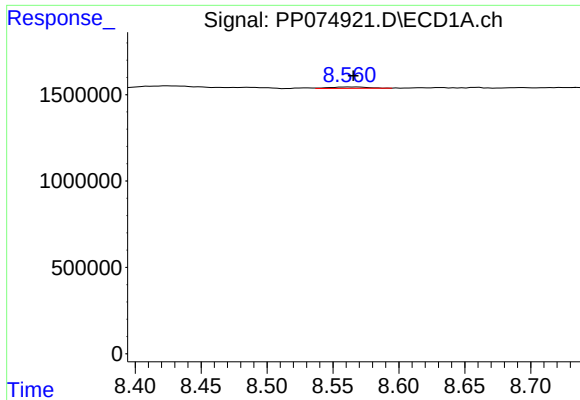

#37 AR-1262-2


R.T.: 8.561 min
Delta R.T.: -0.004 min
Response: 162011
Conc: 1.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

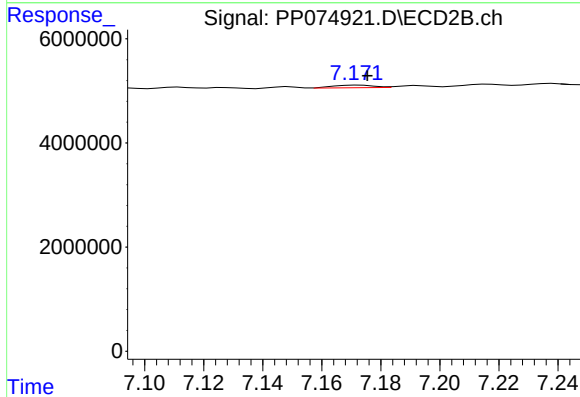


#37 AR-1262-2

R.T.: 7.173 min
Delta R.T.: -0.003 min
Response: 493617
Conc: 0.95 ng/ml

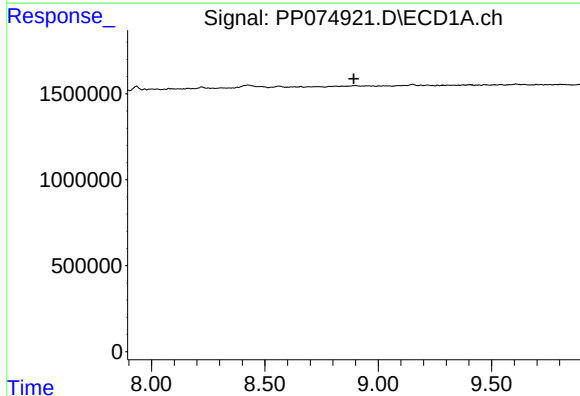


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

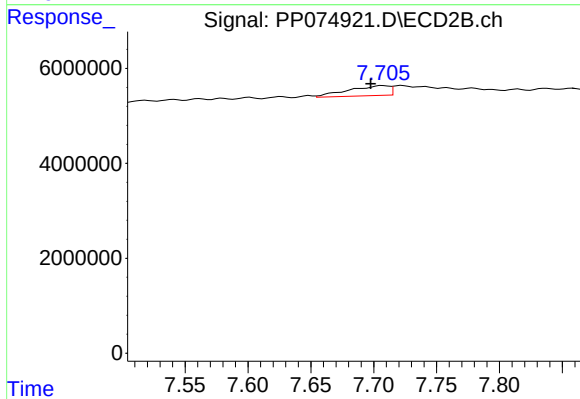

#38 AR-1262-3


R.T.: 7.707 min
Delta R.T.: 0.010 min
Response: 4698330
Conc: 10.08 ng/ml

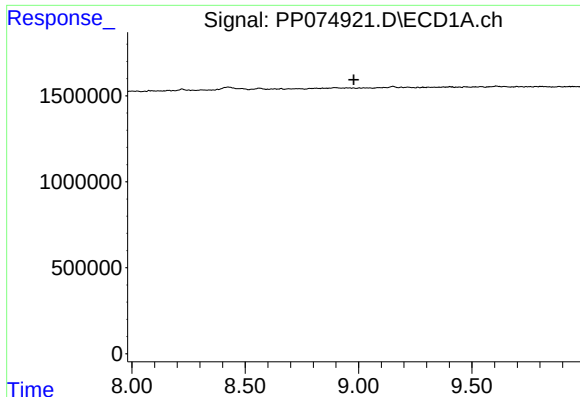

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

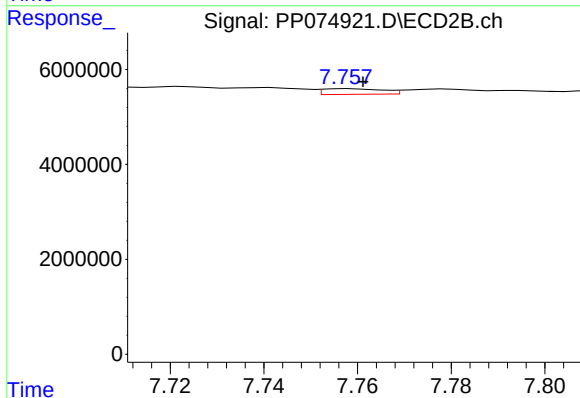


#39 AR-1262-4

R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 1065996
Conc: 1.30 ng/ml

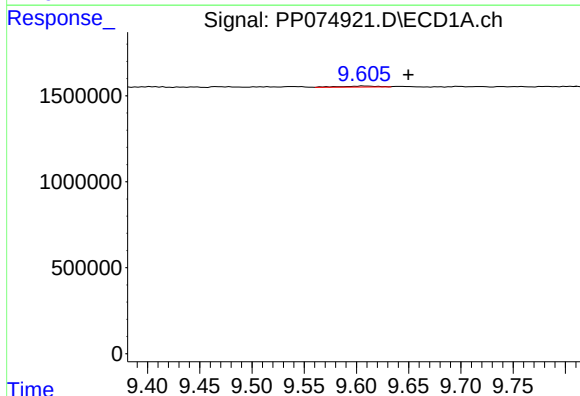


#40 AR-1262-5

R.T.: 9.606 min
Delta R.T.: -0.044 min
Response: 128730
Conc: 2.11 ng/ml

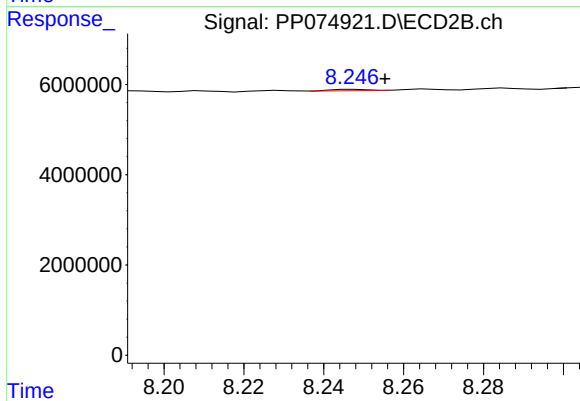

#40 AR-1262-5


R.T.: 8.248 min
Delta R.T.: -0.008 min
Response: 212505
Conc: 0.59 ng/ml

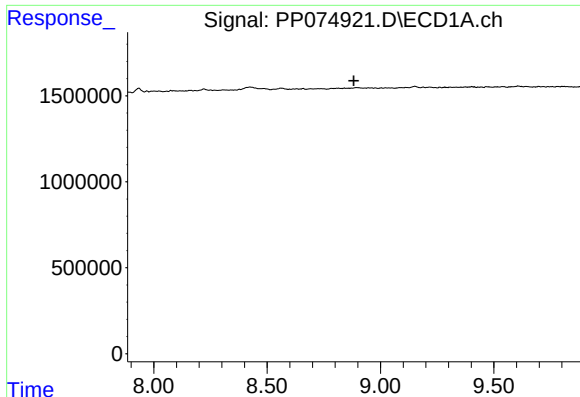

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

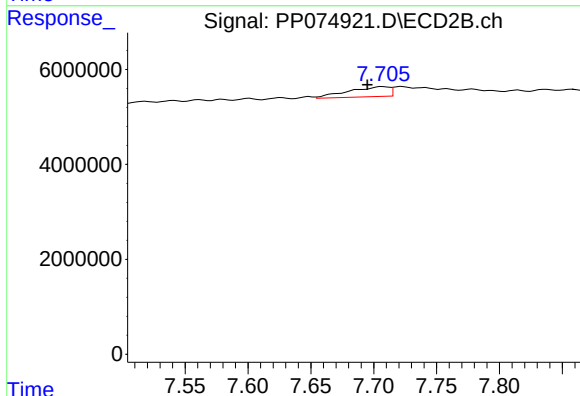


#41 AR-1268-1

R.T.: 7.707 min
Delta R.T.: 0.012 min
Response: 4698330
Conc: 3.33 ng/ml

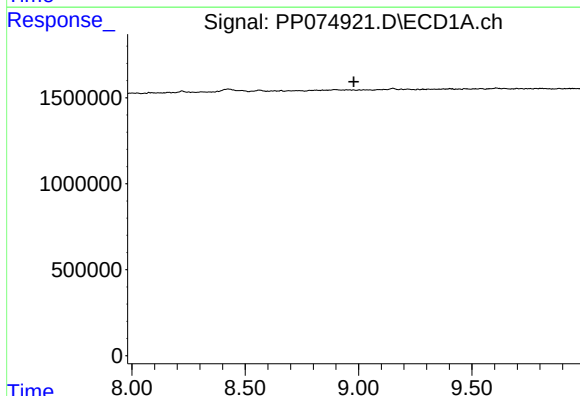


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 8.978 min
Response: 0
Conc: N.D.

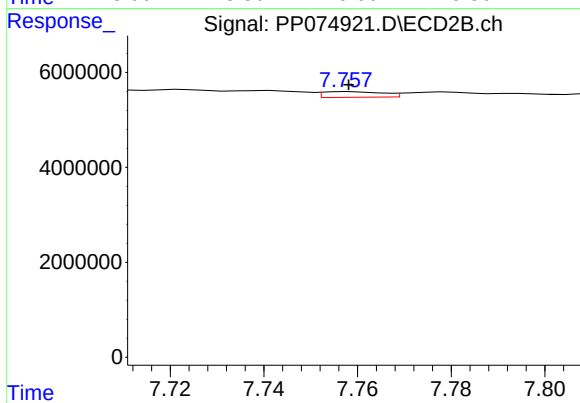

#42 AR-1268-2


R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 1065996
Conc: 0.78 ng/ml

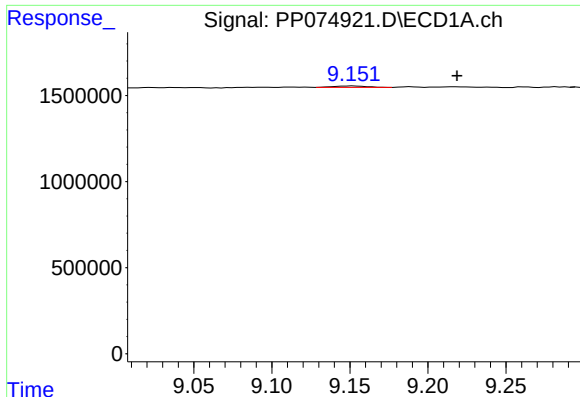

#43 AR-1268-3


R.T.: 9.152 min
Delta R.T.: -0.067 min
Response: 133506
Conc: 1.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

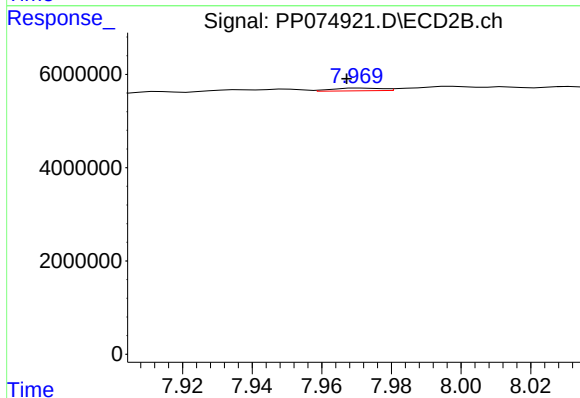


#43 AR-1268-3

R.T.: 7.971 min
Delta R.T.: 0.004 min
Response: 570921
Conc: 0.55 ng/ml

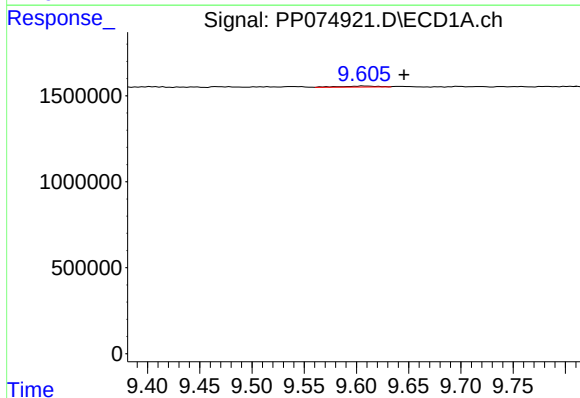


#44 AR-1268-4

R.T.: 9.606 min
Delta R.T.: -0.039 min
Response: 128730
Conc: 1.91 ng/ml

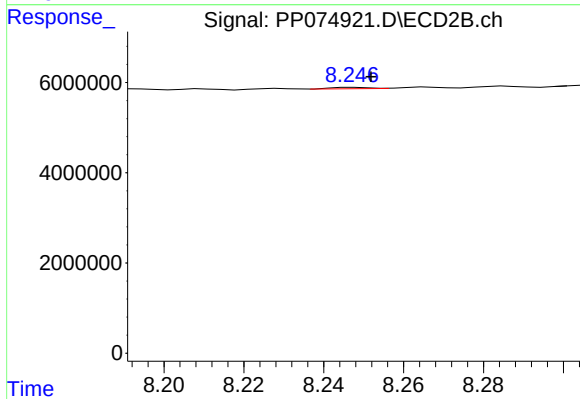

#44 AR-1268-4


R.T.: 8.248 min
Delta R.T.: -0.004 min
Response: 212505
Conc: 0.55 ng/ml

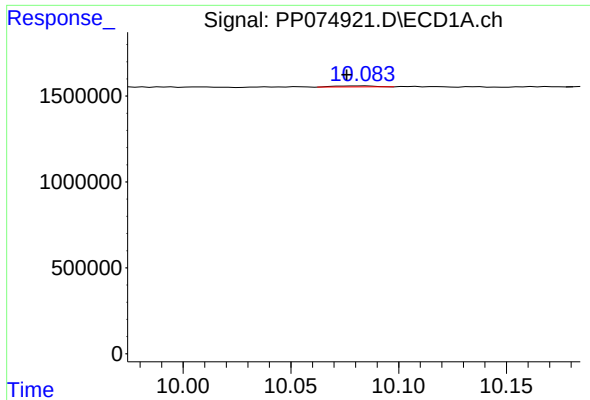

#45 AR-1268-5

R.T.: 10.084 min
Delta R.T.: 0.008 min
Response: 78951
Conc: 0.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

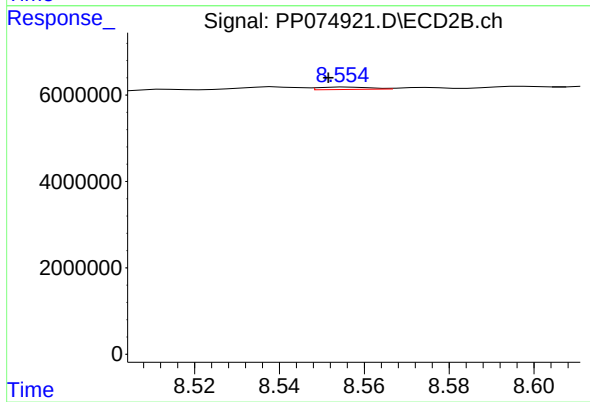

#45 AR-1268-5

R.T.: 8.556 min
Delta R.T.: 0.004 min
Response: 475639
Conc: 0.15 ng/ml