

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 21:00
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1242 WATER MDL 25PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:44:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.659	3.800	25712751	93737279	21.012	19.386
2)	SA Decachlor...	10.435	8.809	20647679	130.0E6	20.909	17.331
Target Compounds							
3)	L1 AR-1016-1	5.810	4.896	1845854	14080630	41.867	27.644 #
4)	L1 AR-1016-2	5.832	4.957	2384832	6204760	37.950	26.069 #
5)	L1 AR-1016-3	5.894	5.077	1582723	3615432	35.239	26.217 #
6)	L1 AR-1016-4	5.992	5.117	1388071	6595051	39.454	47.174
7)	L1 AR-1016-5	6.283	5.332	1925077	8275757	58.009	49.829
8)	L2 AR-1221-1	4.857	4.004	1023566	743055	58.181	12.010 #
9)	L2 AR-1221-2	4.959	4.095	667028	1230577	49.938	27.218 #
10)	L2 AR-1221-3	5.019	4.173	650373	1100621	17.154	6.699 #
11)	L3 AR-1232-1	5.019	4.173	650373	1100621	21.412	8.592 #
12)	L3 AR-1232-2	5.545	4.896	1040827	14080630	66.050	60.746
13)	L3 AR-1232-3	5.832	5.077	2384832	3615432	78.079	60.197
14)	L3 AR-1232-4	5.992	5.158	1388071	10899053	80.378	147.869 #
15)	L3 AR-1232-5	6.081	5.332	1808326	8275757	139.306	133.300
16)	L4 AR-1242-1	5.810	4.896	1845854	14080630	48.226	33.386 #
17)	L4 AR-1242-2	5.832	4.957	2384832	6204760	42.223	30.980 #
18)	L4 AR-1242-3	5.894	5.077	1582723	3615432	38.981	30.562
19)	L4 AR-1242-4	5.992	5.158	1388071	10899053	43.730	63.678 #
20)	L4 AR-1242-5	6.721	5.679	3039580	12144336	84.267	65.587
21)	L5 AR-1248-1	5.810	4.896	1845854	14080630	61.072	50.990
22)	L5 AR-1248-2	6.081	5.117	1808326	6595051	41.960	37.312
23)	L5 AR-1248-3	6.283	5.158	1925077	10899053	41.219	47.970
24)	L5 AR-1248-4	6.681	5.332	2439103	8275757	44.347	37.959
25)	L5 AR-1248-5	6.721	5.720	3039580	14573064	54.796	39.674 #
26)	L6 AR-1254-1	6.656	5.679	2262253	12144336	38.824	25.475 #
27)	L6 AR-1254-2	6.876	5.823	2281310	5573050	27.952	15.827 #
28)	L6 AR-1254-3	7.231	6.232	3440779	5535050	38.571	8.930 #
29)	L6 AR-1254-4	7.517	6.457	548456	4548638	8.321	9.706
30)	L6 AR-1254-5	7.933	6.871	480432	1421438	5.782	2.898 #
31)	L7 AR-1260-1	7.398	6.353	94542	995192	1.635	2.652 #
32)	L7 AR-1260-2	7.655	6.555	363499	539307	5.274	1.020 #
33)	L7 AR-1260-3	7.996	6.700	321808	1132001	6.202	2.614 #
34)	L7 AR-1260-4	8.220	7.175	487104	577196	7.636	1.513 #
35)	L7 AR-1260-5	8.562	7.412	260738	364175	2.299	0.363 #
36)	L8 AR-1262-1	8.220	6.910	487104	586020	6.325	0.829 #
37)	L8 AR-1262-2	8.562	7.175	260738	577196	1.970	1.108 #
38)	L8 AR-1262-3	8.900	7.705	73478	6059529	0.756	12.995 #
39)	L8 AR-1262-4	0.000	7.761	0	1967427	N.D.	2.394 #
40)	L8 AR-1262-5	9.604f	8.250	58074	210499	0.953	0.587 #
41)	L9 AR-1268-1	8.900	7.705	73478	6059529	0.453	4.296 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074922.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 21:00
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1242 WATER MDL 25PPB
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:44:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.761	0	1967427	N.D.	1.443 #
43) L9	AR-1268-3	9.156f	7.961	167382	625875	1.354	0.600 #
44) L9	AR-1268-4	9.604f	8.250	58074	210499	0.863	0.549 #
45) L9	AR-1268-5	10.078	8.547	101674	760957	0.275	0.243



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
Data File : PP074922.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 21:00
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1242 WATER MDL 25PPB
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:44:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

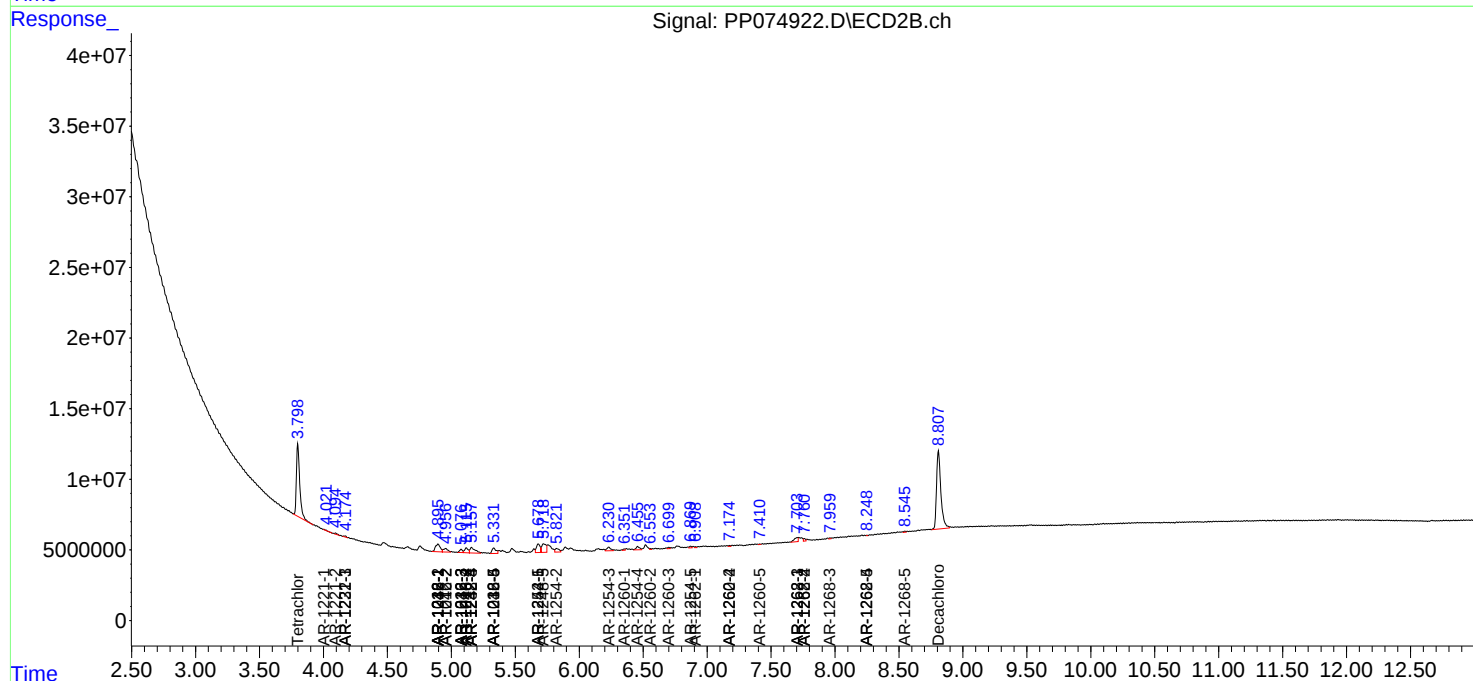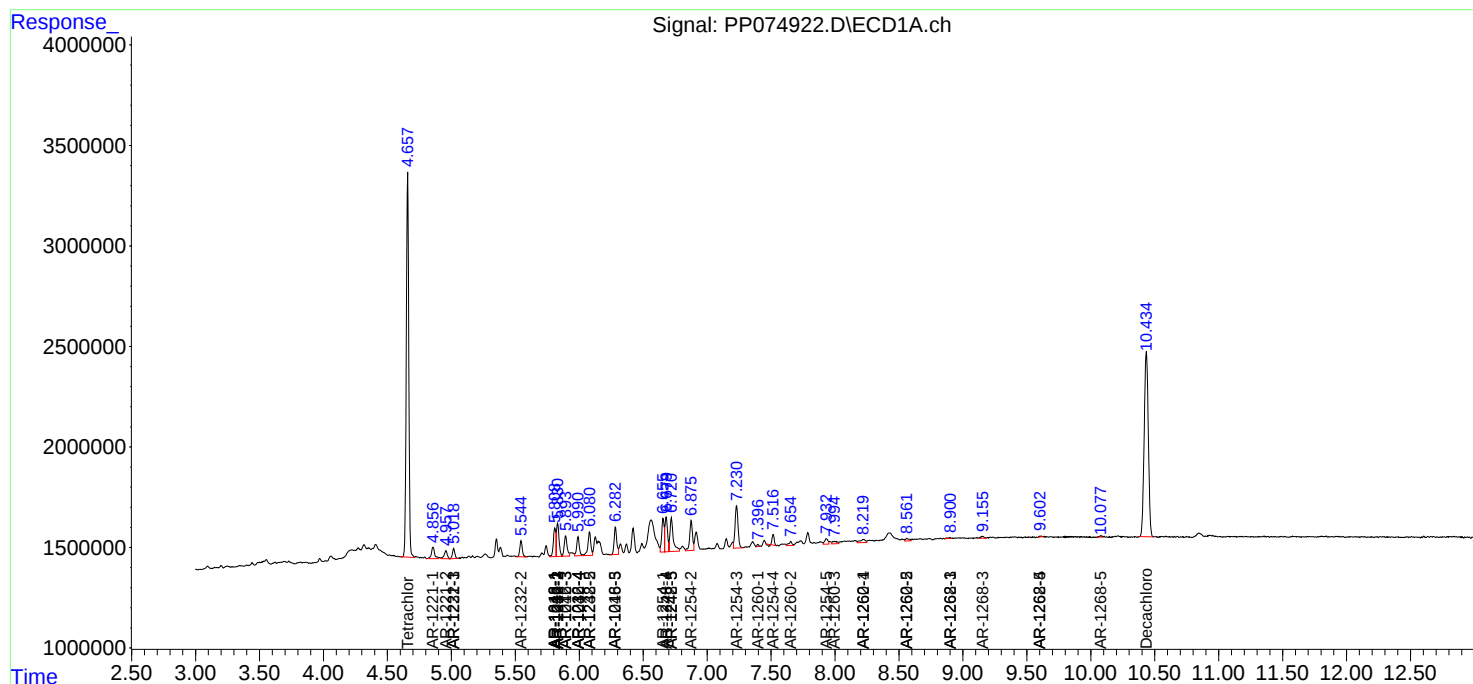


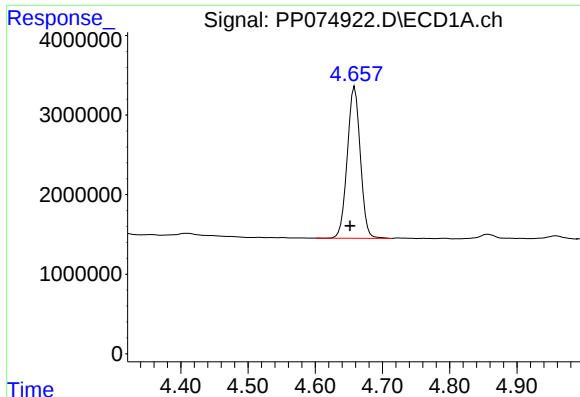

#1 Tetrachloro-m-xylene


R.T.: 4.659 min
Delta R.T.: 0.007 min
Response: 25712751
Conc: 21.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

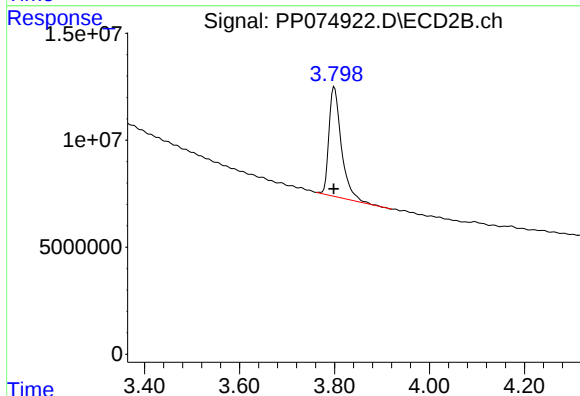


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 93737279
Conc: 19.39 ng/ml

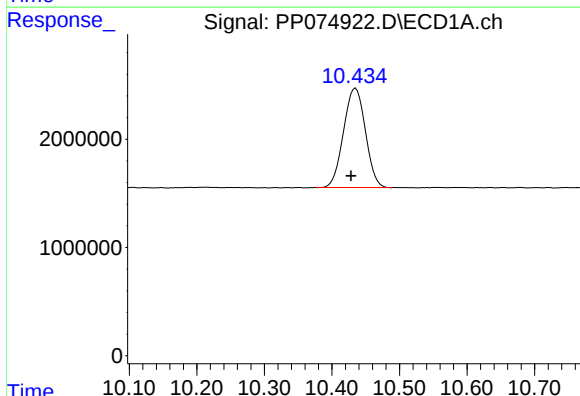


#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.007 min
Response: 20647679
Conc: 20.91 ng/ml

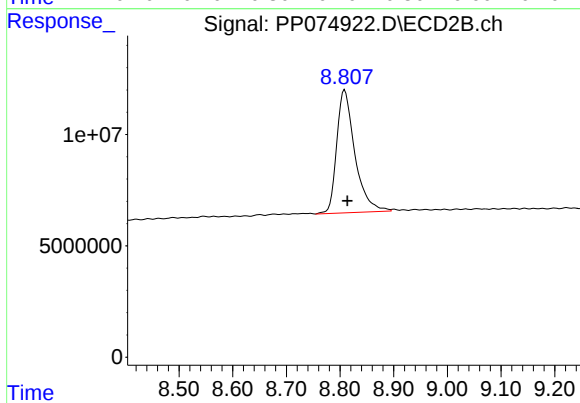

#2 Decachlorobiphenyl


R.T.: 8.809 min
Delta R.T.: -0.005 min
Response: 129971379
Conc: 17.33 ng/ml

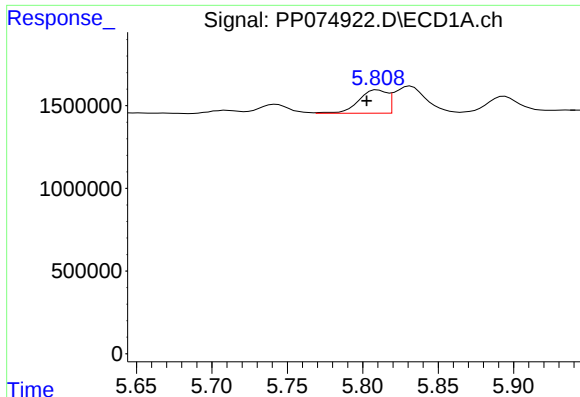

#3 AR-1016-1


R.T.: 5.810 min
Delta R.T.: 0.007 min
Response: 1845854
Conc: 41.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

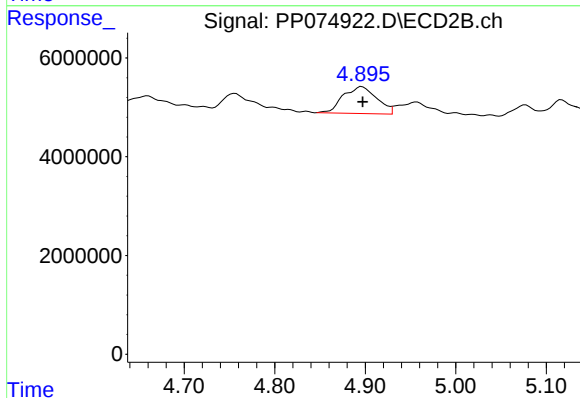


#3 AR-1016-1

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 14080630
Conc: 27.64 ng/ml

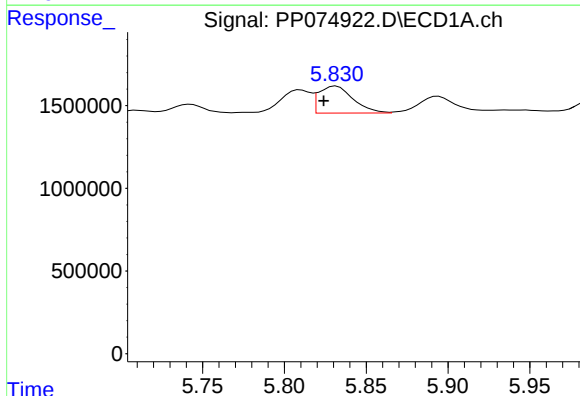


#4 AR-1016-2

R.T.: 5.832 min
Delta R.T.: 0.008 min
Response: 2384832
Conc: 37.95 ng/ml

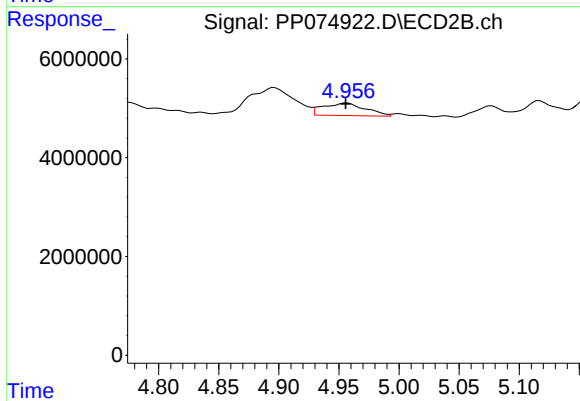

#4 AR-1016-2


R.T.: 4.957 min
Delta R.T.: 0.001 min
Response: 6204760
Conc: 26.07 ng/ml

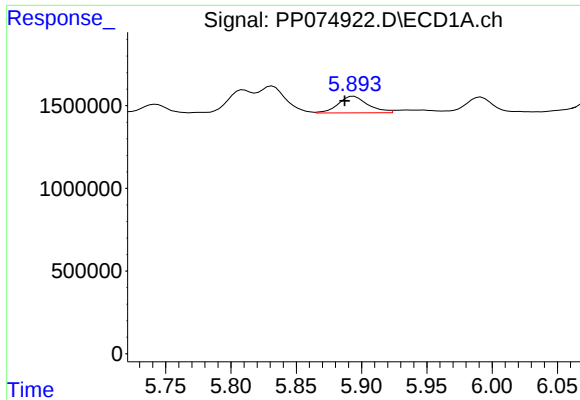

#5 AR-1016-3


R.T.: 5.894 min
Delta R.T.: 0.007 min
Response: 1582723
Conc: 35.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

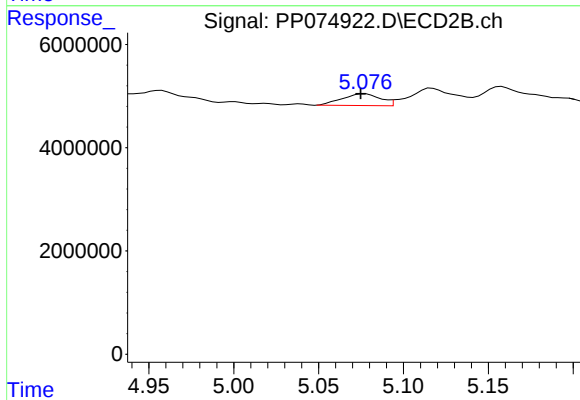


#5 AR-1016-3

R.T.: 5.077 min
Delta R.T.: 0.002 min
Response: 3615432
Conc: 26.22 ng/ml

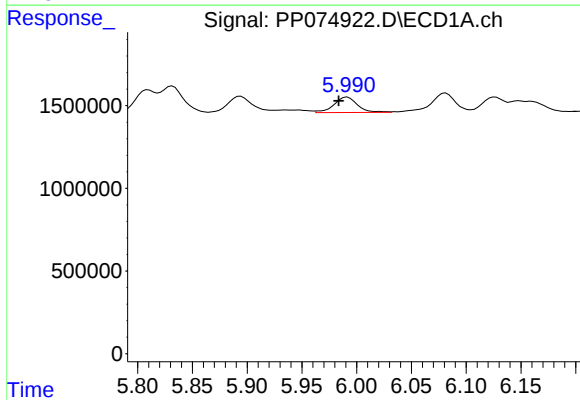


#6 AR-1016-4

R.T.: 5.992 min
Delta R.T.: 0.008 min
Response: 1388071
Conc: 39.45 ng/ml

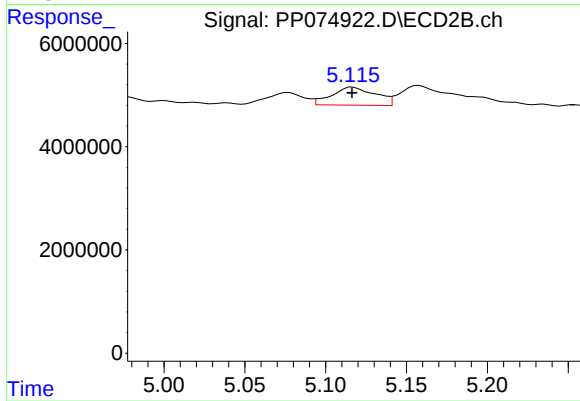

#6 AR-1016-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 6595051
Conc: 47.17 ng/ml

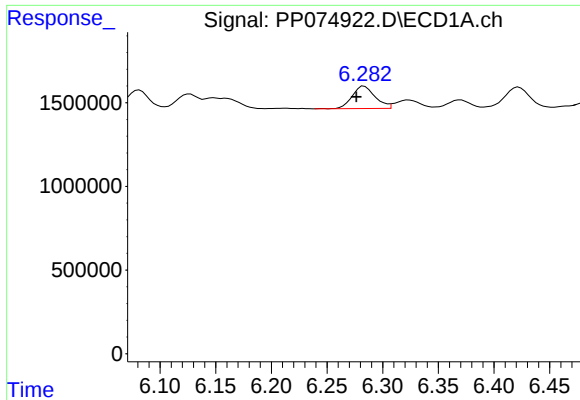

#7 AR-1016-5


R.T.: 6.283 min
Delta R.T.: 0.007 min
Response: 1925077
Conc: 58.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

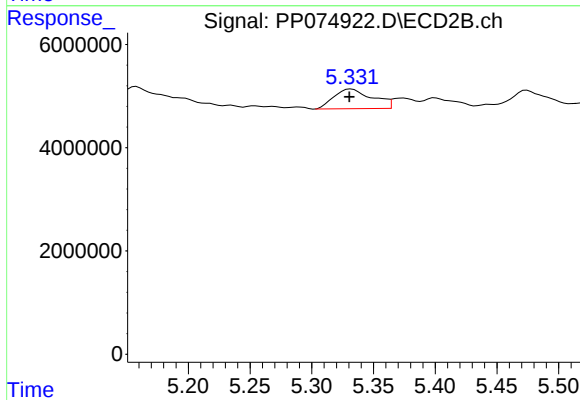


#7 AR-1016-5

R.T.: 5.332 min
Delta R.T.: 0.002 min
Response: 8275757
Conc: 49.83 ng/ml

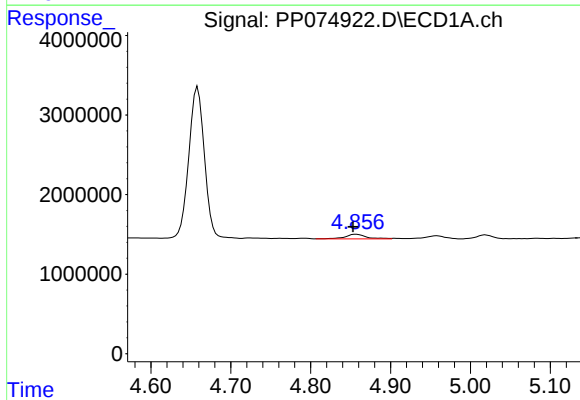


#8 AR-1221-1

R.T.: 4.857 min
Delta R.T.: 0.004 min
Response: 1023566
Conc: 58.18 ng/ml

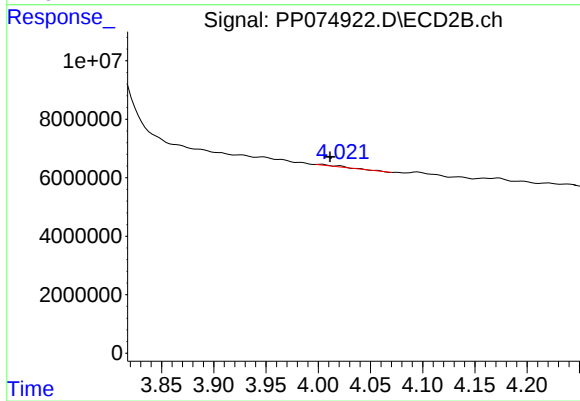

#8 AR-1221-1


R.T.: 4.004 min
Delta R.T.: -0.008 min
Response: 743055
Conc: 12.01 ng/ml

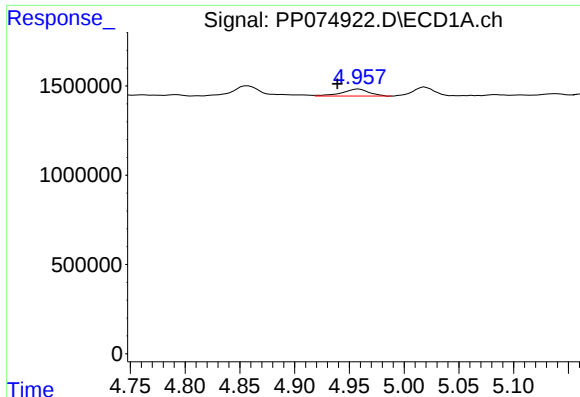

#9 AR-1221-2


R.T.: 4.959 min
Delta R.T.: 0.019 min
Response: 667028
Conc: 49.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

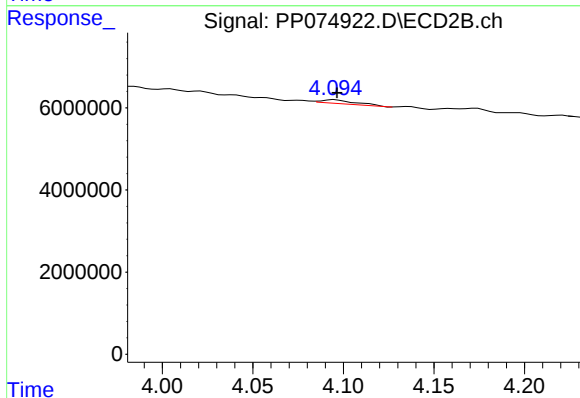


#9 AR-1221-2

R.T.: 4.095 min
Delta R.T.: -0.001 min
Response: 1230577
Conc: 27.22 ng/ml

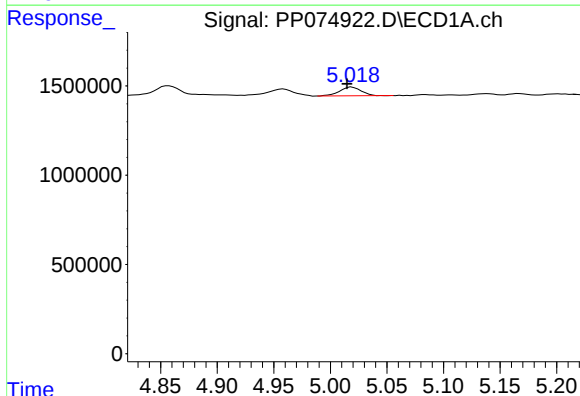


#10 AR-1221-3

R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 650373
Conc: 17.15 ng/ml

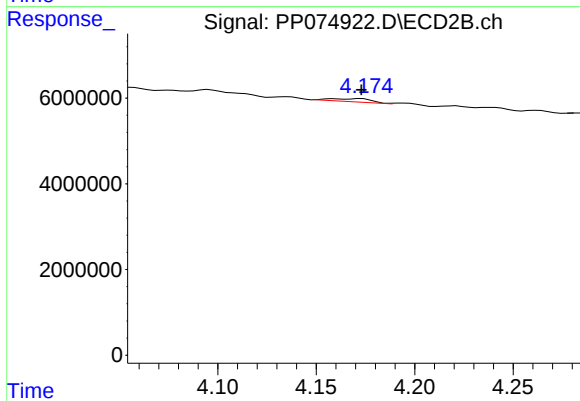

#10 AR-1221-3


R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 1100621
Conc: 6.70 ng/ml

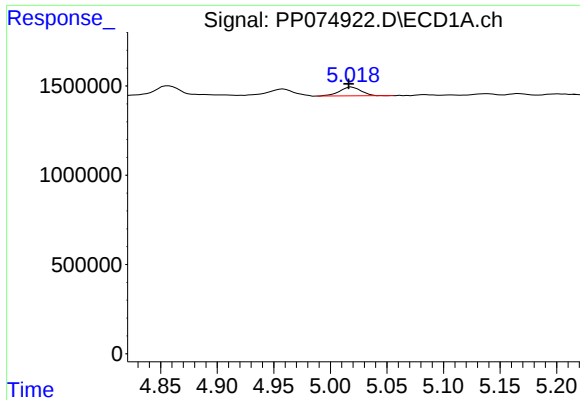

#11 AR-1232-1


R.T.: 5.019 min
Delta R.T.: 0.003 min
Response: 650373
Conc: 21.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

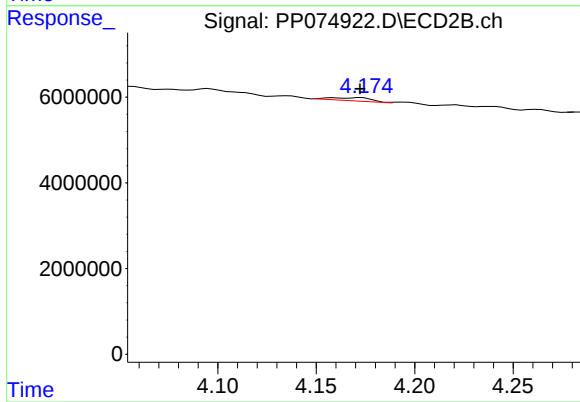


#11 AR-1232-1

R.T.: 4.173 min
Delta R.T.: 0.000 min
Response: 1100621
Conc: 8.59 ng/ml

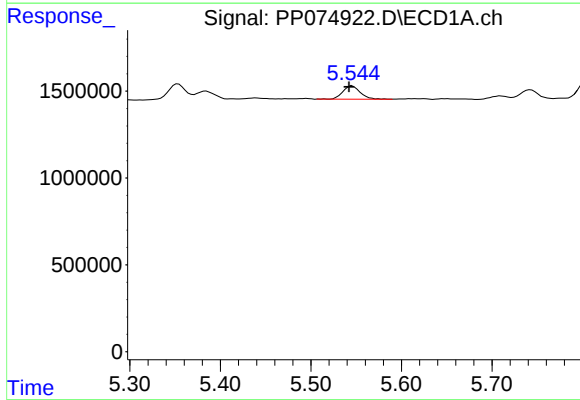


#12 AR-1232-2

R.T.: 5.545 min
Delta R.T.: 0.004 min
Response: 1040827
Conc: 66.05 ng/ml

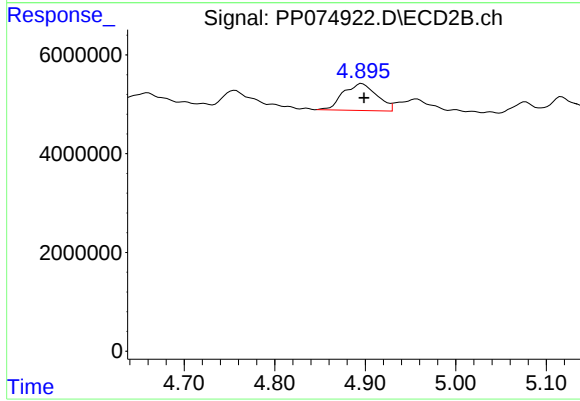

#12 AR-1232-2


R.T.: 4.896 min
Delta R.T.: -0.002 min
Response: 14080630
Conc: 60.75 ng/ml

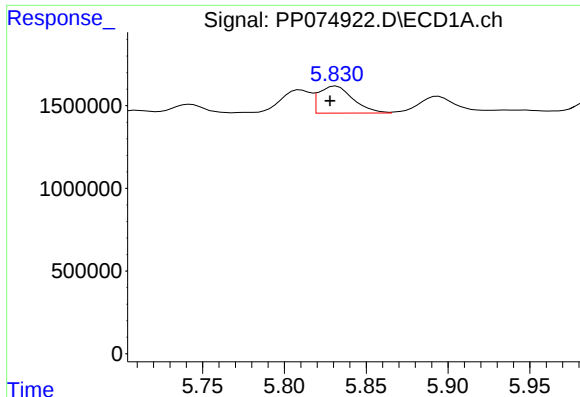

#13 AR-1232-3


R.T.: 5.832 min
Delta R.T.: 0.004 min
Response: 2384832
Conc: 78.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

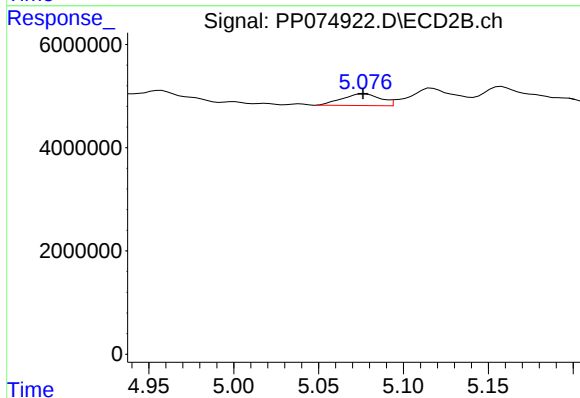


#13 AR-1232-3

R.T.: 5.077 min
Delta R.T.: 0.000 min
Response: 3615432
Conc: 60.20 ng/ml

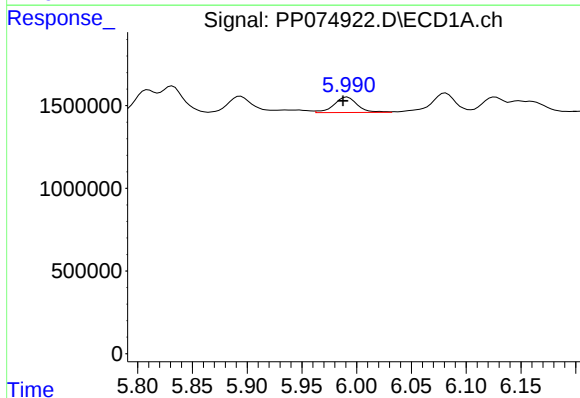


#14 AR-1232-4

R.T.: 5.992 min
Delta R.T.: 0.004 min
Response: 1388071
Conc: 80.38 ng/ml

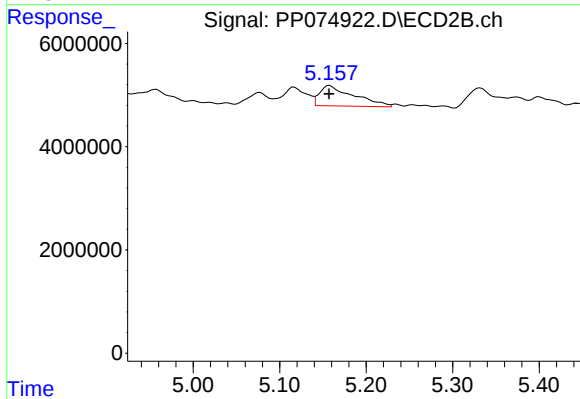

#14 AR-1232-4


R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 10899053
Conc: 147.87 ng/ml

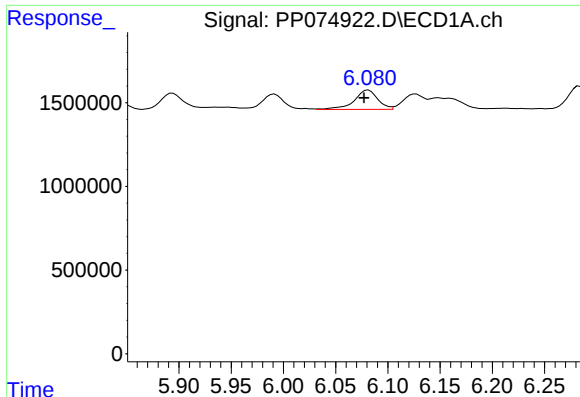

#15 AR-1232-5


R.T.: 6.081 min
Delta R.T.: 0.004 min
Response: 1808326
Conc: 139.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

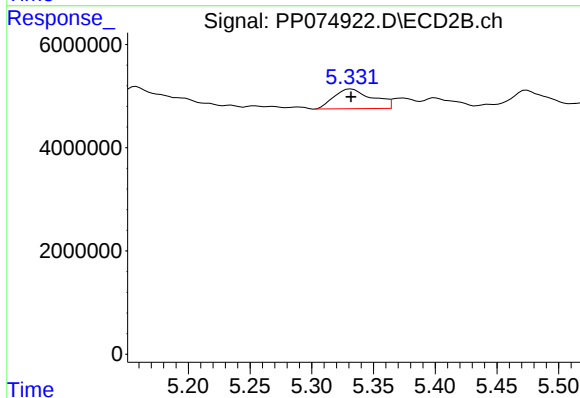


#15 AR-1232-5

R.T.: 5.332 min
Delta R.T.: 0.000 min
Response: 8275757
Conc: 133.30 ng/ml

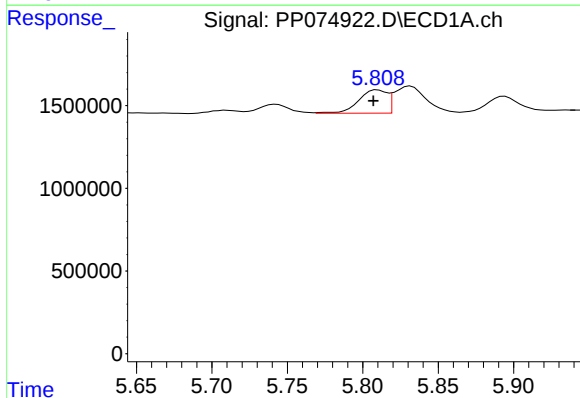


#16 AR-1242-1

R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 1845854
Conc: 48.23 ng/ml

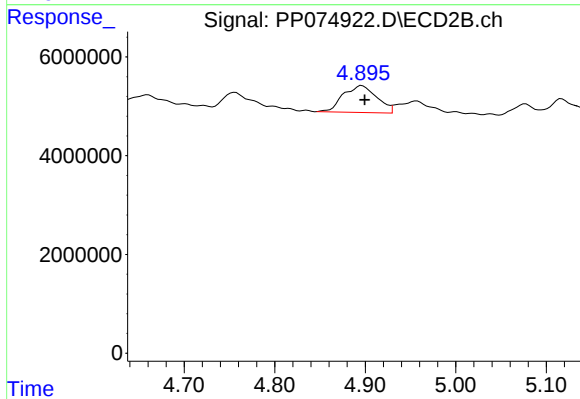

#16 AR-1242-1


R.T.: 4.896 min
Delta R.T.: -0.003 min
Response: 14080630
Conc: 33.39 ng/ml

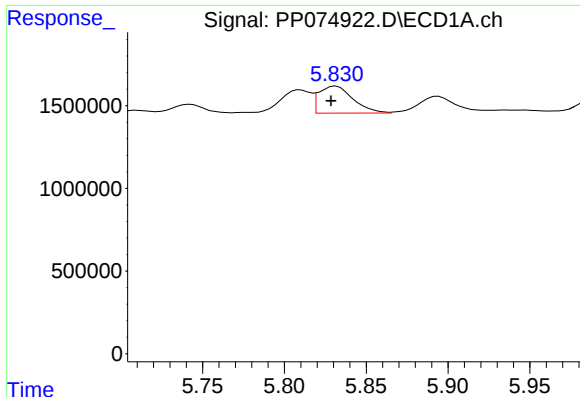

#17 AR-1242-2


R.T.: 5.832 min
Delta R.T.: 0.003 min
Response: 2384832
Conc: 42.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

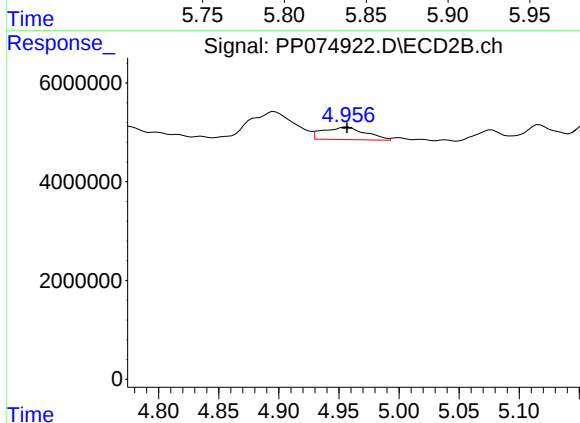


#17 AR-1242-2

R.T.: 4.957 min
Delta R.T.: 0.000 min
Response: 6204760
Conc: 30.98 ng/ml

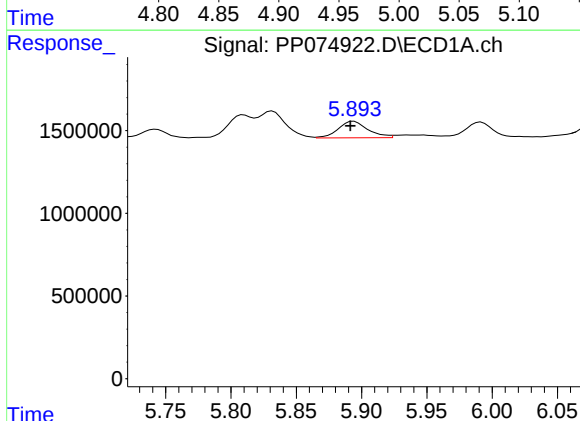


#18 AR-1242-3

R.T.: 5.894 min
Delta R.T.: 0.002 min
Response: 1582723
Conc: 38.98 ng/ml

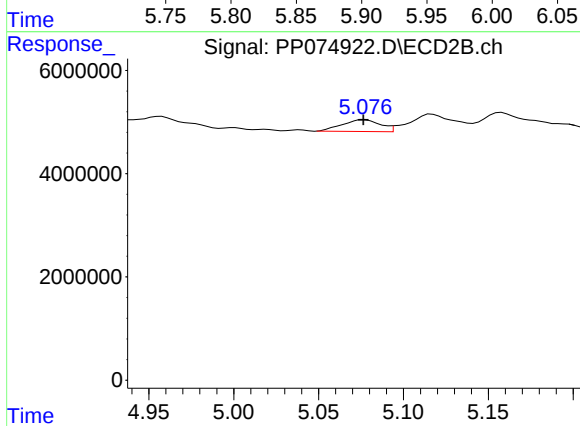

#18 AR-1242-3


R.T.: 5.077 min
Delta R.T.: 0.000 min
Response: 3615432
Conc: 30.56 ng/ml

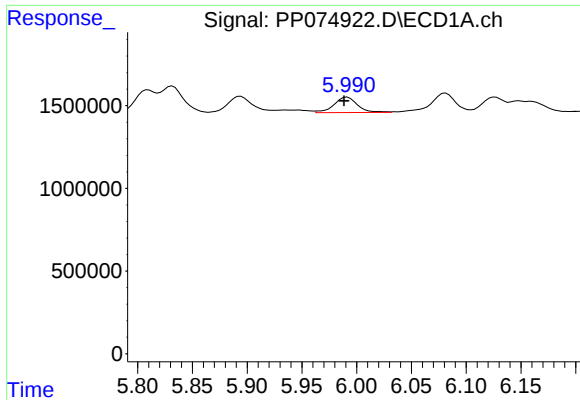

#19 AR-1242-4


R.T.: 5.992 min
Delta R.T.: 0.003 min
Response: 1388071
Conc: 43.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

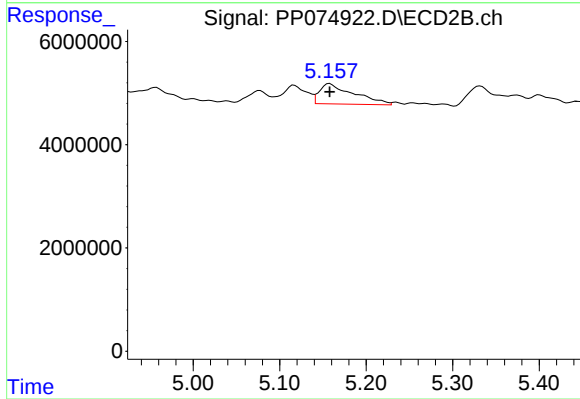


#19 AR-1242-4

R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 10899053
Conc: 63.68 ng/ml

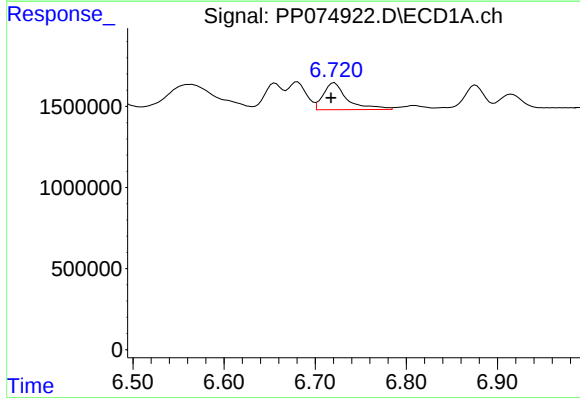


#20 AR-1242-5

R.T.: 6.721 min
Delta R.T.: 0.004 min
Response: 3039580
Conc: 84.27 ng/ml

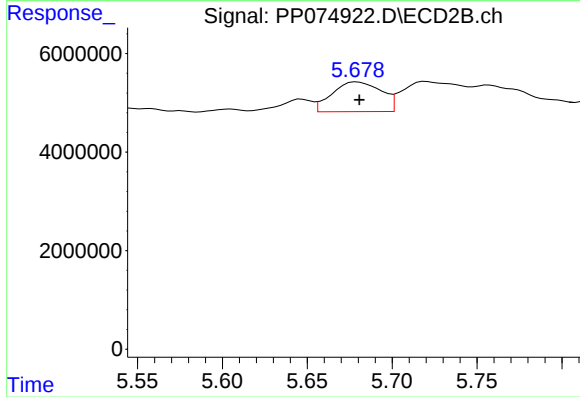

#20 AR-1242-5


R.T.: 5.679 min
Delta R.T.: -0.001 min
Response: 12144336
Conc: 65.59 ng/ml

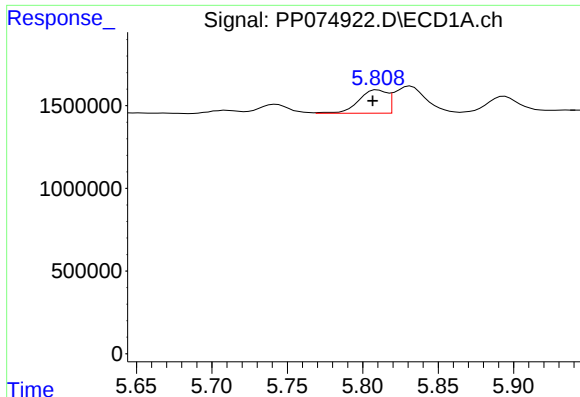

#21 AR-1248-1


R.T.: 5.810 min
Delta R.T.: 0.003 min
Response: 1845854
Conc: 61.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

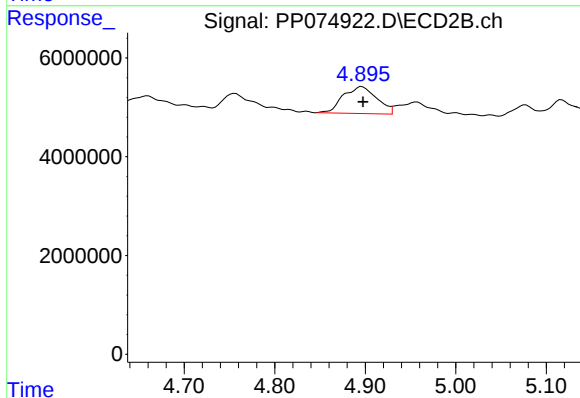


#21 AR-1248-1

R.T.: 4.896 min
Delta R.T.: 0.000 min
Response: 14080630
Conc: 50.99 ng/ml

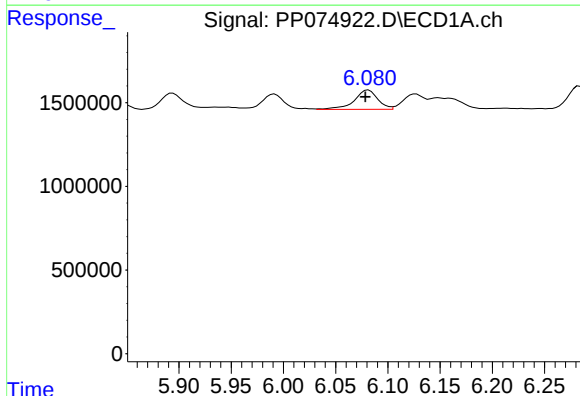


#22 AR-1248-2

R.T.: 6.081 min
Delta R.T.: 0.003 min
Response: 1808326
Conc: 41.96 ng/ml

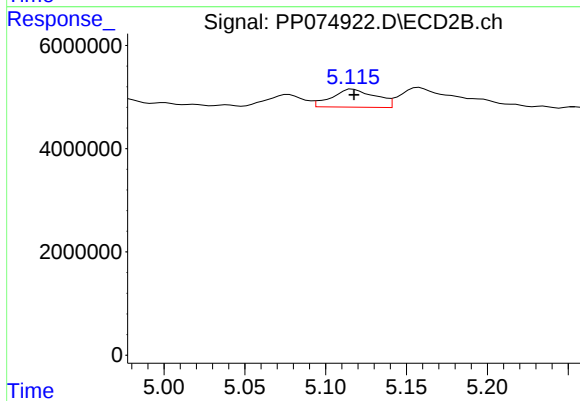

#22 AR-1248-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 6595051
Conc: 37.31 ng/ml

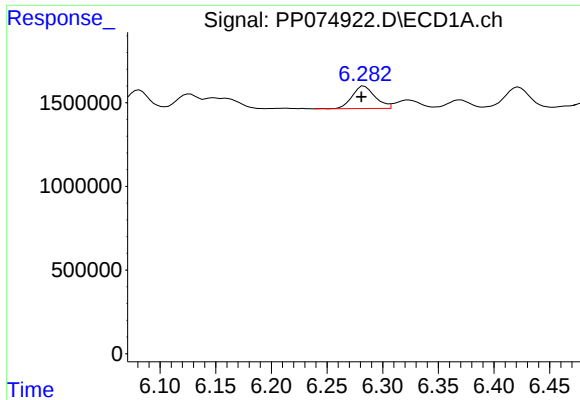

#23 AR-1248-3


R.T.: 6.283 min
Delta R.T.: 0.002 min
Response: 1925077
Conc: 41.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

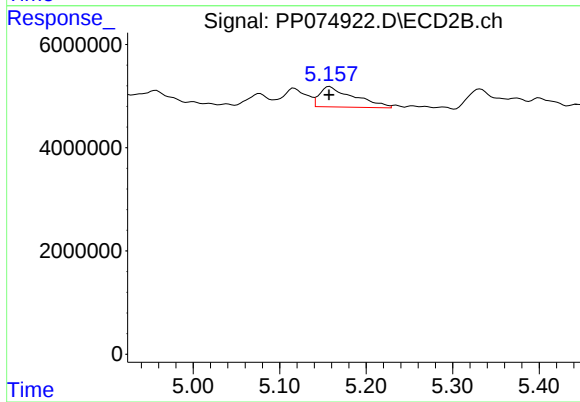


#23 AR-1248-3

R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 10899053
Conc: 47.97 ng/ml

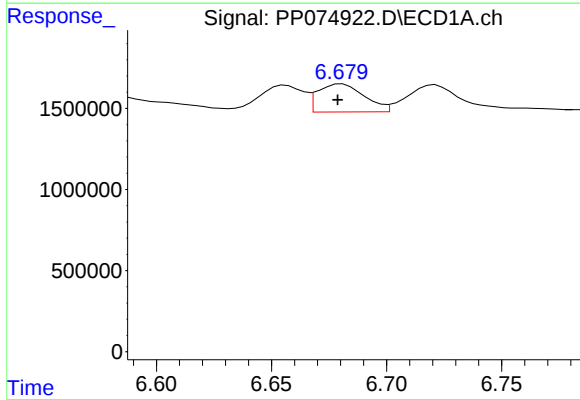


#24 AR-1248-4

R.T.: 6.681 min
Delta R.T.: 0.002 min
Response: 2439103
Conc: 44.35 ng/ml

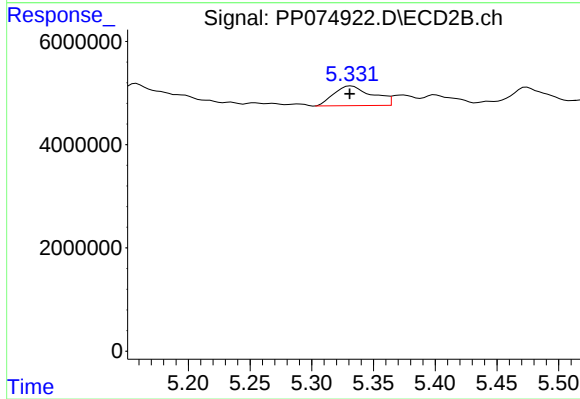

#24 AR-1248-4


R.T.: 5.332 min
Delta R.T.: 0.001 min
Response: 8275757
Conc: 37.96 ng/ml

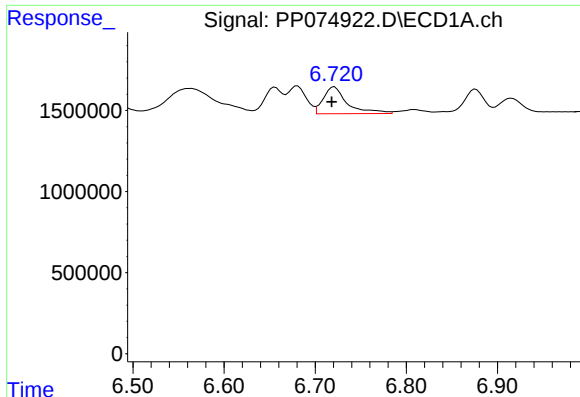

#25 AR-1248-5


R.T.: 6.721 min
Delta R.T.: 0.003 min
Response: 3039580
Conc: 54.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

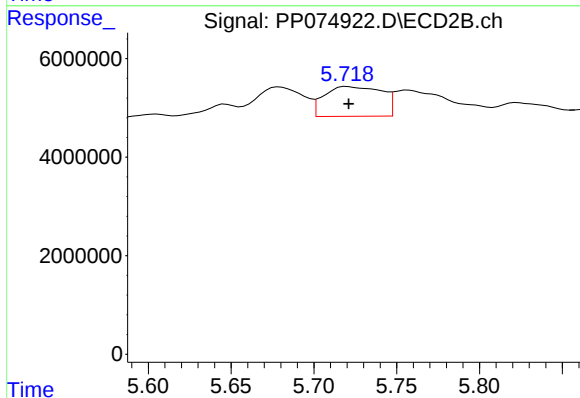


#25 AR-1248-5

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 14573064
Conc: 39.67 ng/ml

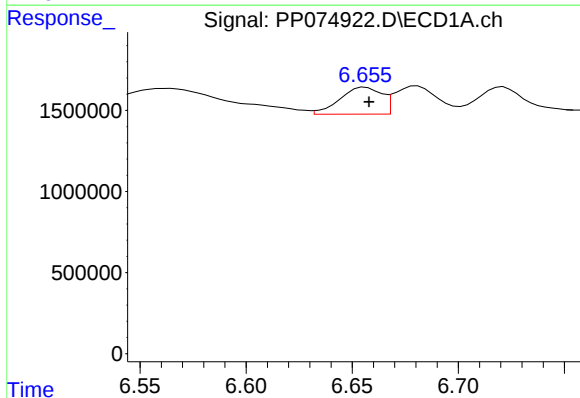


#26 AR-1254-1

R.T.: 6.656 min
Delta R.T.: -0.002 min
Response: 2262253
Conc: 38.82 ng/ml

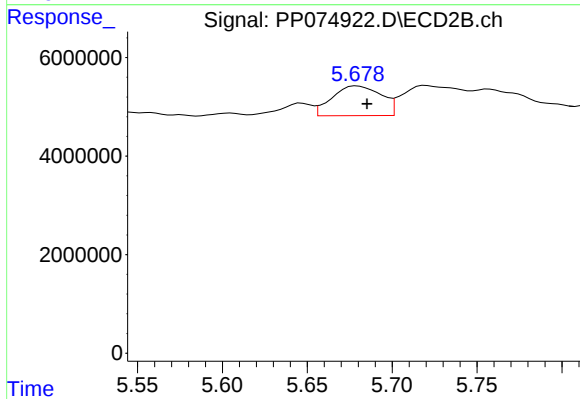

#26 AR-1254-1


R.T.: 5.679 min
Delta R.T.: -0.006 min
Response: 12144336
Conc: 25.48 ng/ml

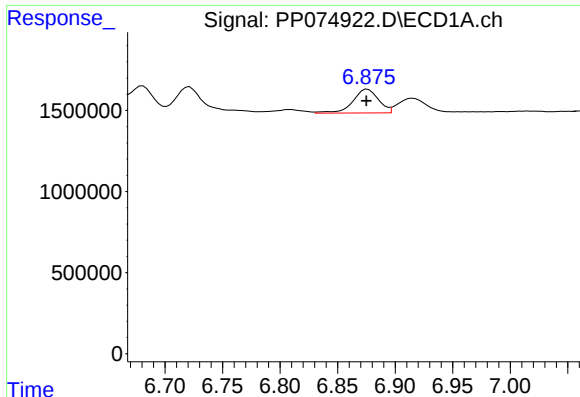

#27 AR-1254-2


R.T.: 6.876 min
Delta R.T.: 0.001 min
Response: 2281310
Conc: 27.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

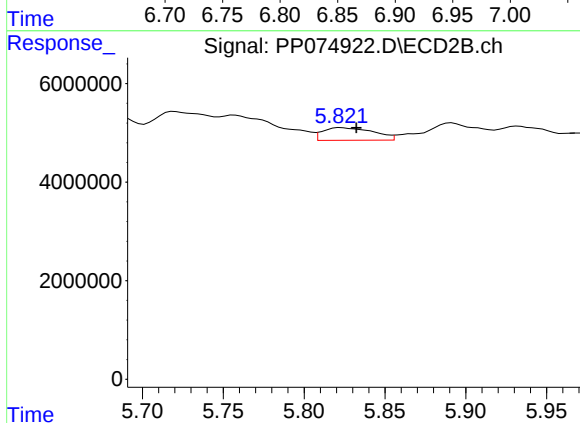


#27 AR-1254-2

R.T.: 5.823 min
Delta R.T.: -0.009 min
Response: 5573050
Conc: 15.83 ng/ml

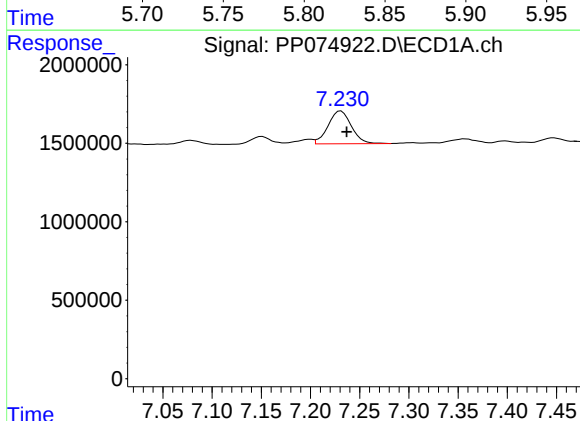


#28 AR-1254-3

R.T.: 7.231 min
Delta R.T.: -0.006 min
Response: 3440779
Conc: 38.57 ng/ml

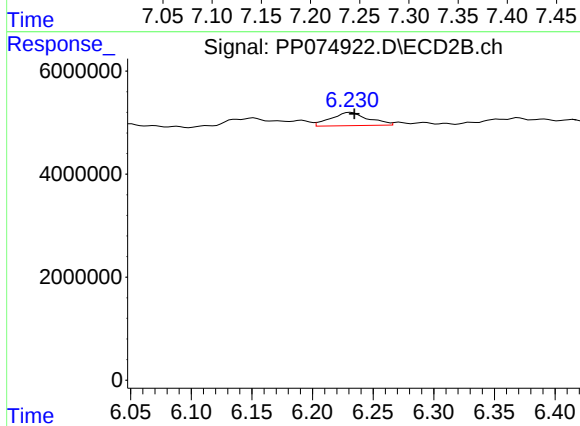

#28 AR-1254-3


R.T.: 6.232 min
Delta R.T.: -0.003 min
Response: 5535050
Conc: 8.93 ng/ml

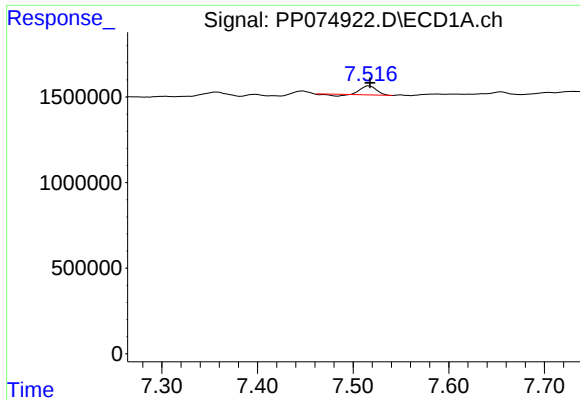

#29 AR-1254-4


R.T.: 7.517 min
Delta R.T.: 0.000 min
Response: 548456
Conc: 8.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

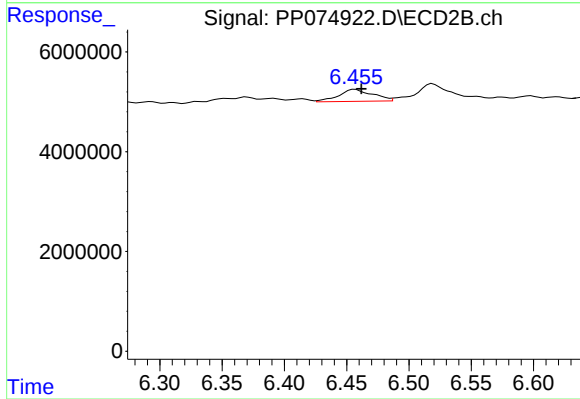


#29 AR-1254-4

R.T.: 6.457 min
Delta R.T.: -0.005 min
Response: 4548638
Conc: 9.71 ng/ml

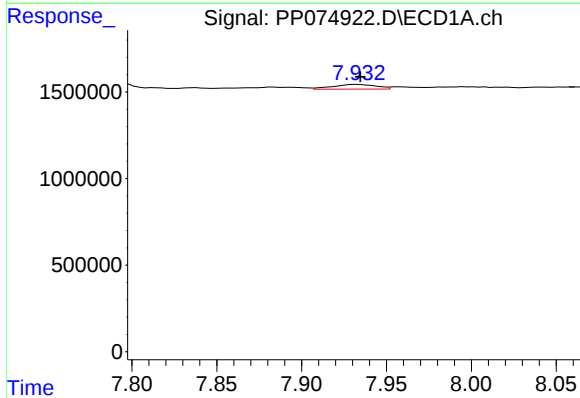


#30 AR-1254-5

R.T.: 7.933 min
Delta R.T.: -0.002 min
Response: 480432
Conc: 5.78 ng/ml

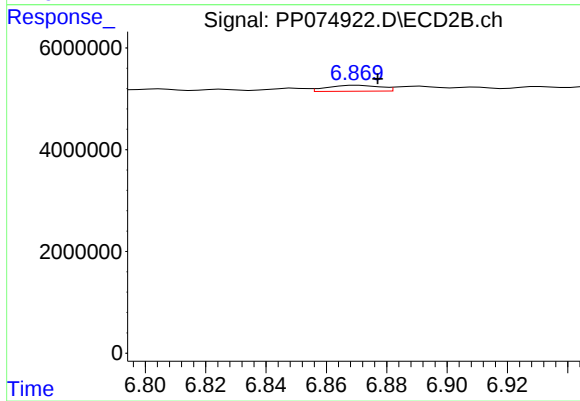

#30 AR-1254-5


R.T.: 6.871 min
Delta R.T.: -0.006 min
Response: 1421438
Conc: 2.90 ng/ml

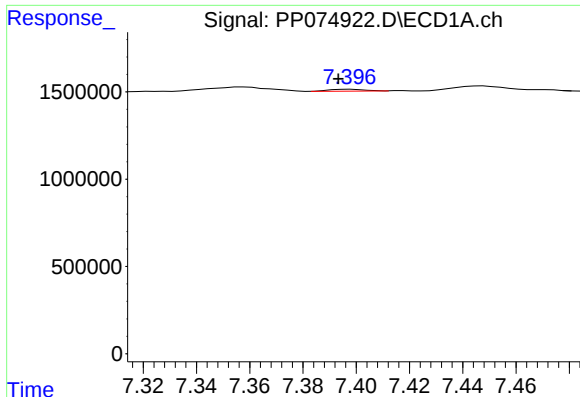

#31 AR-1260-1


R.T.: 7.398 min
Delta R.T.: 0.004 min
Response: 94542
Conc: 1.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

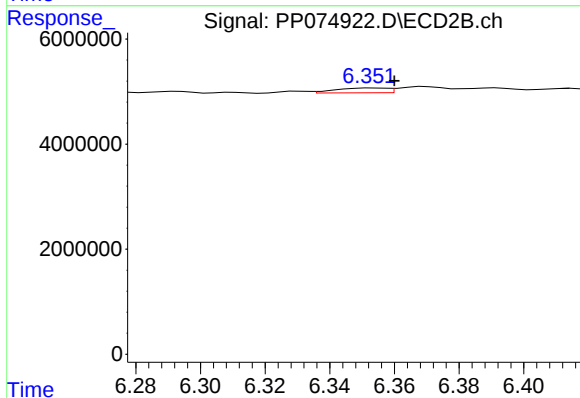


#31 AR-1260-1

R.T.: 6.353 min
Delta R.T.: -0.007 min
Response: 995192
Conc: 2.65 ng/ml

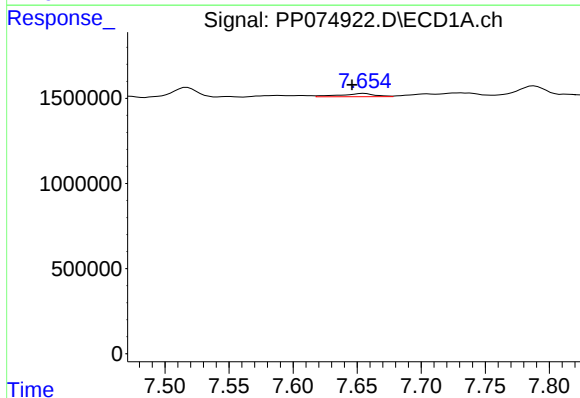


#32 AR-1260-2

R.T.: 7.655 min
Delta R.T.: 0.009 min
Response: 363499
Conc: 5.27 ng/ml

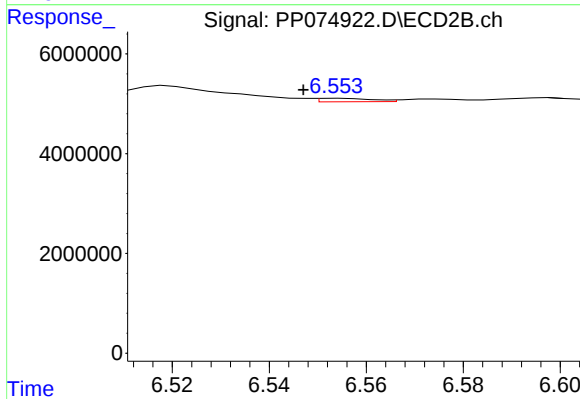

#32 AR-1260-2


R.T.: 6.555 min
Delta R.T.: 0.008 min
Response: 539307
Conc: 1.02 ng/ml

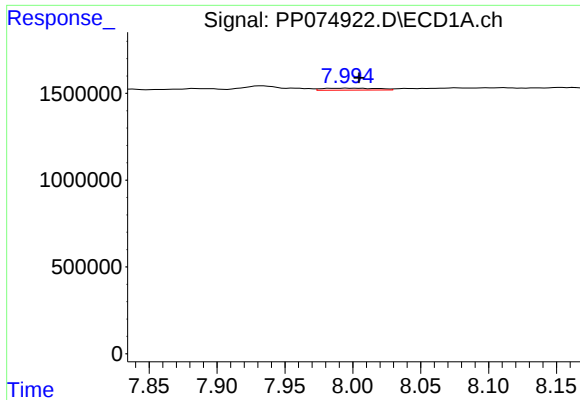

#33 AR-1260-3


R.T.: 7.996 min
Delta R.T.: -0.009 min
Response: 321808
Conc: 6.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

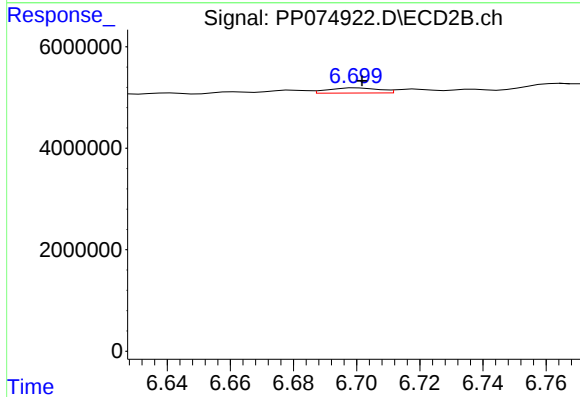


#33 AR-1260-3

R.T.: 6.700 min
Delta R.T.: -0.001 min
Response: 1132001
Conc: 2.61 ng/ml

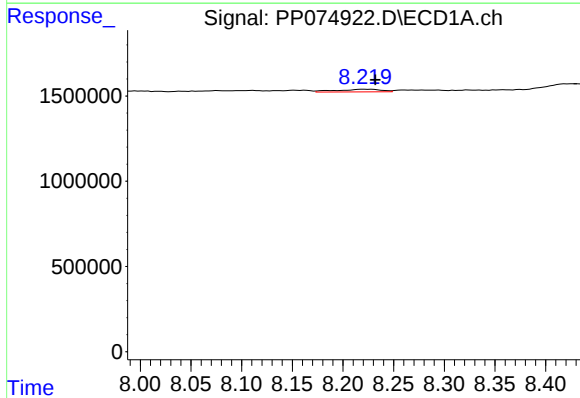


#34 AR-1260-4

R.T.: 8.220 min
Delta R.T.: -0.012 min
Response: 487104
Conc: 7.64 ng/ml

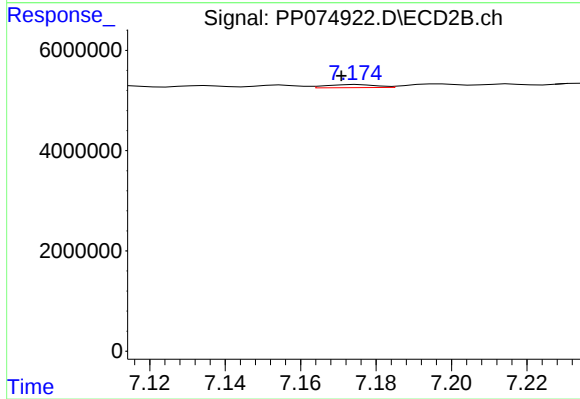

#34 AR-1260-4


R.T.: 7.175 min
Delta R.T.: 0.004 min
Response: 577196
Conc: 1.51 ng/ml

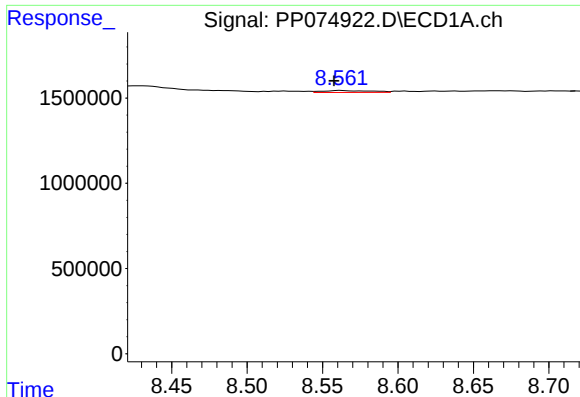

#35 AR-1260-5


R.T.: 8.562 min
Delta R.T.: 0.004 min
Response: 260738
Conc: 2.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

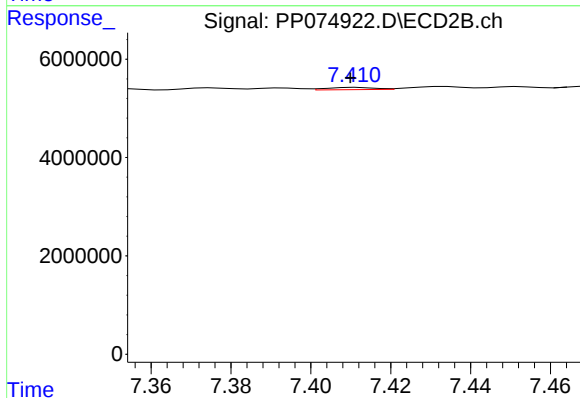


#35 AR-1260-5

R.T.: 7.412 min
Delta R.T.: 0.002 min
Response: 364175
Conc: 0.36 ng/ml

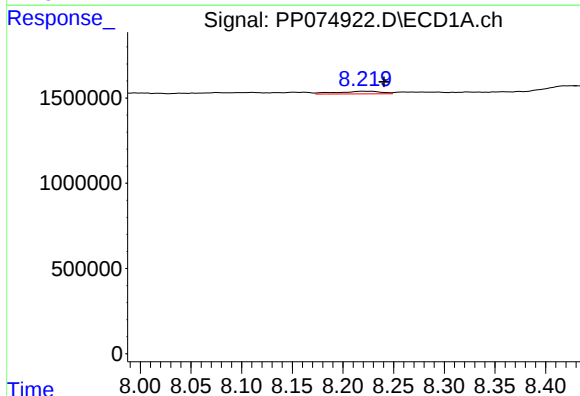


#36 AR-1262-1

R.T.: 8.220 min
Delta R.T.: -0.020 min
Response: 487104
Conc: 6.32 ng/ml

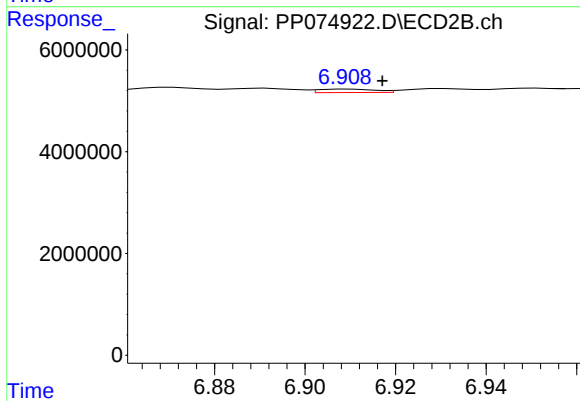

#36 AR-1262-1


R.T.: 6.910 min
Delta R.T.: -0.007 min
Response: 586020
Conc: 0.83 ng/ml

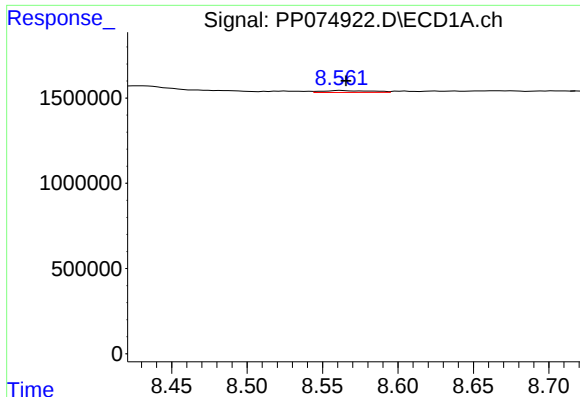

#37 AR-1262-2


R.T.: 8.562 min
Delta R.T.: -0.003 min
Response: 260738
Conc: 1.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

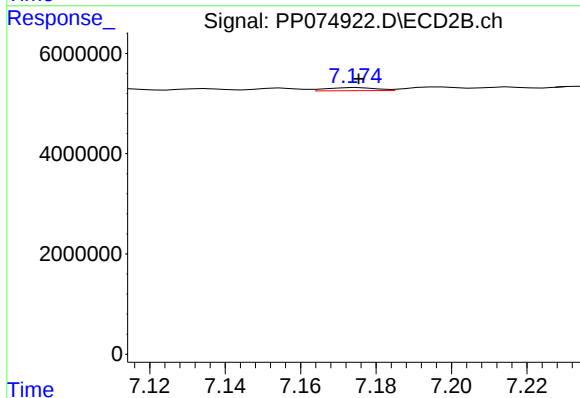


#37 AR-1262-2

R.T.: 7.175 min
Delta R.T.: 0.000 min
Response: 577196
Conc: 1.11 ng/ml

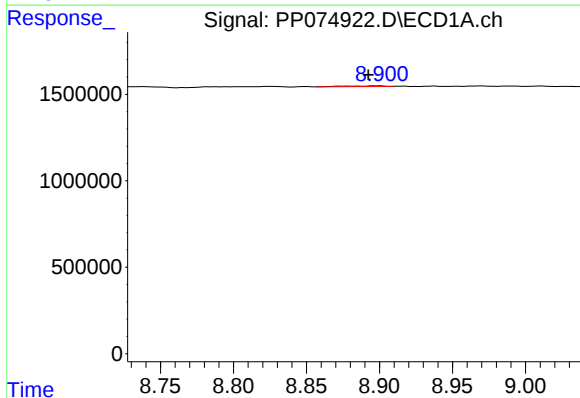


#38 AR-1262-3

R.T.: 8.900 min
Delta R.T.: 0.008 min
Response: 73478
Conc: 0.76 ng/ml

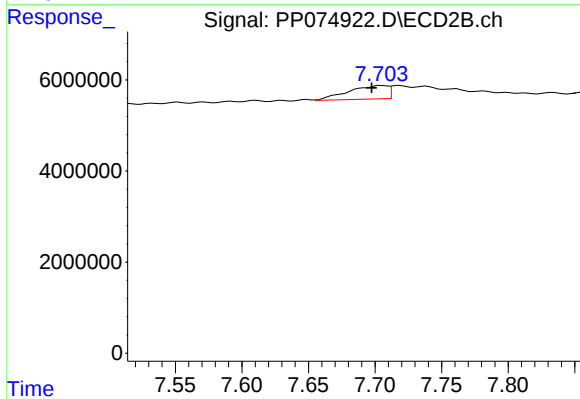

#38 AR-1262-3


R.T.: 7.705 min
Delta R.T.: 0.007 min
Response: 6059529
Conc: 12.99 ng/ml

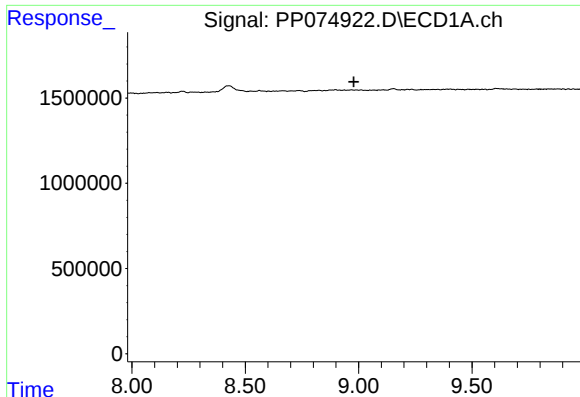

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

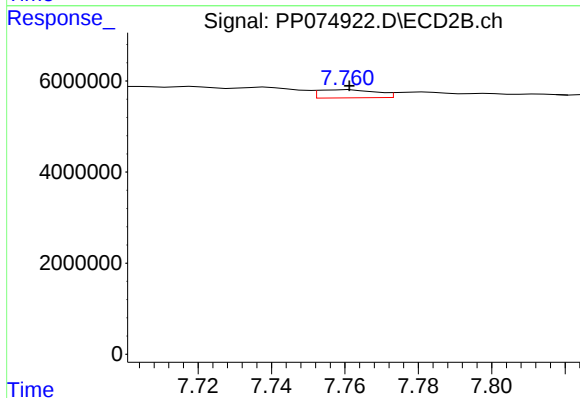


#39 AR-1262-4

R.T.: 7.761 min
Delta R.T.: 0.000 min
Response: 1967427
Conc: 2.39 ng/ml

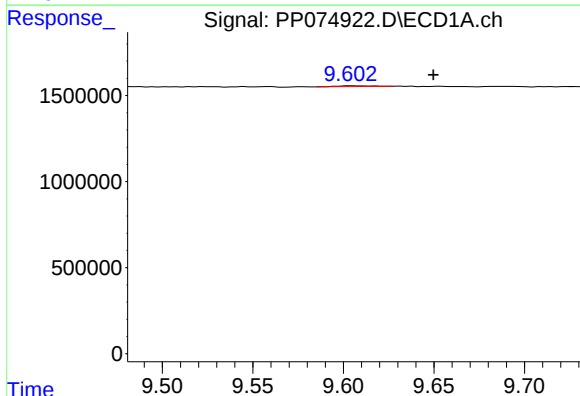


#40 AR-1262-5

R.T.: 9.604 min
Delta R.T.: -0.046 min
Response: 58074
Conc: 0.95 ng/ml

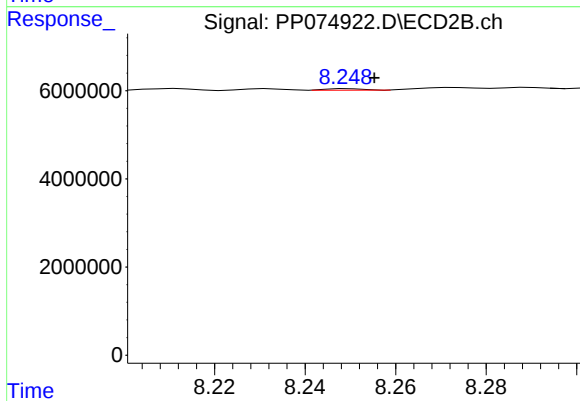

#40 AR-1262-5


R.T.: 8.250 min
Delta R.T.: -0.005 min
Response: 210499
Conc: 0.59 ng/ml

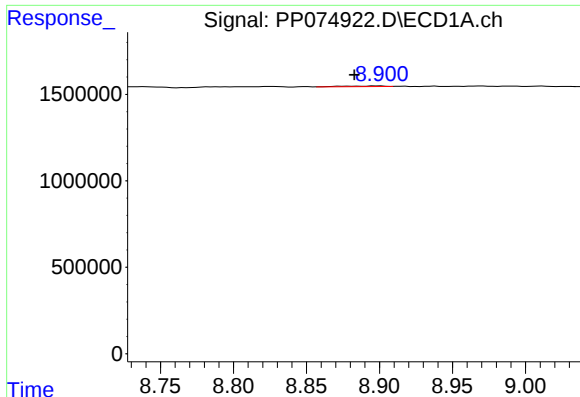

#41 AR-1268-1


R.T.: 8.900 min
Delta R.T.: 0.017 min
Response: 73478
Conc: 0.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

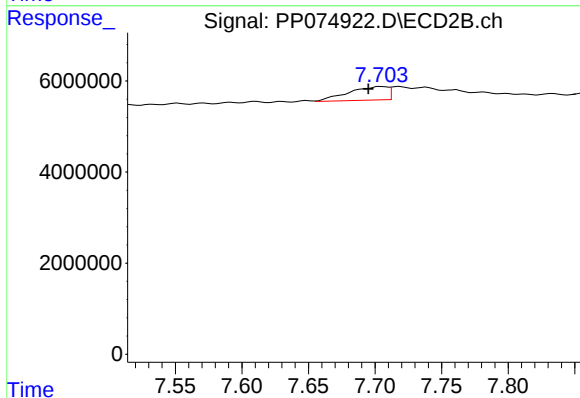


#41 AR-1268-1

R.T.: 7.705 min
Delta R.T.: 0.010 min
Response: 6059529
Conc: 4.30 ng/ml

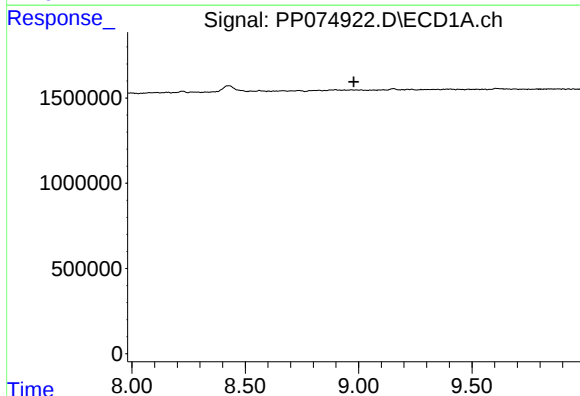


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.978 min
Response: 0
Conc: N.D.

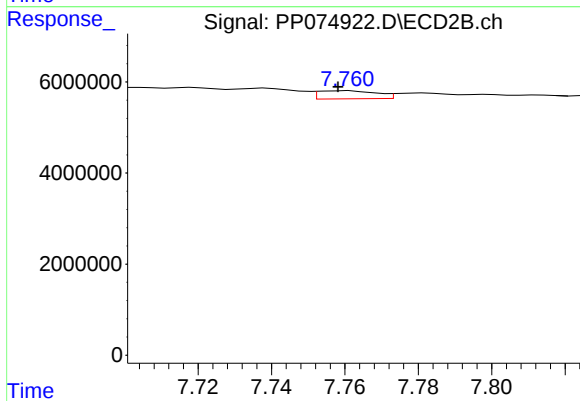

#42 AR-1268-2


R.T.: 7.761 min
Delta R.T.: 0.002 min
Response: 1967427
Conc: 1.44 ng/ml

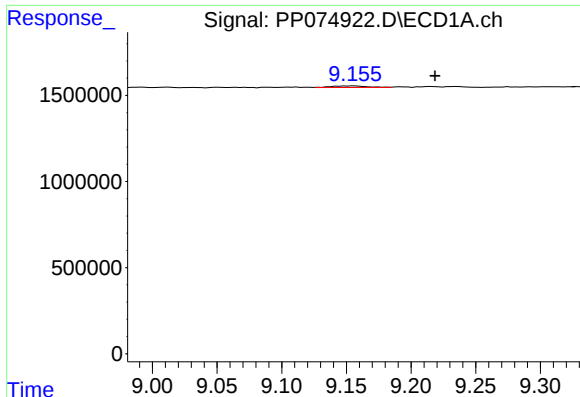

#43 AR-1268-3


R.T.: 9.156 min
Delta R.T.: -0.062 min
Response: 167382
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

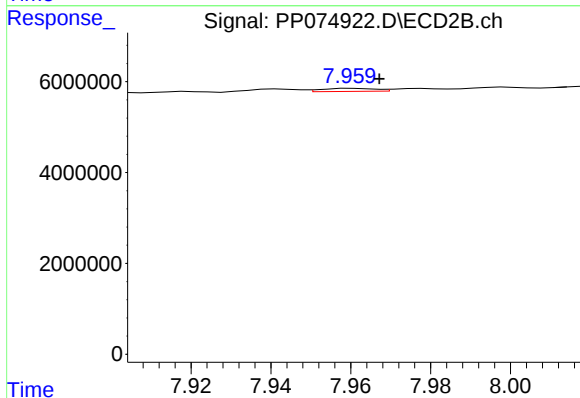


#43 AR-1268-3

R.T.: 7.961 min
Delta R.T.: -0.006 min
Response: 625875
Conc: 0.60 ng/ml

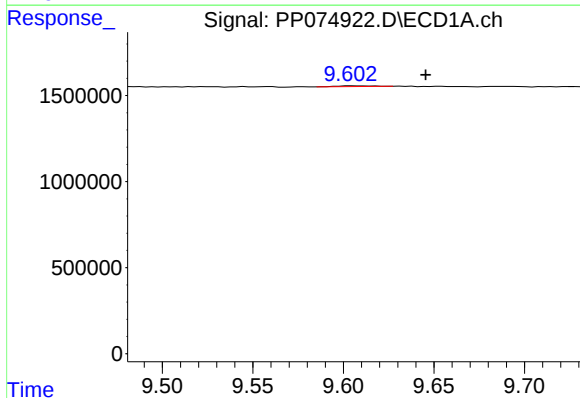


#44 AR-1268-4

R.T.: 9.604 min
Delta R.T.: -0.041 min
Response: 58074
Conc: 0.86 ng/ml

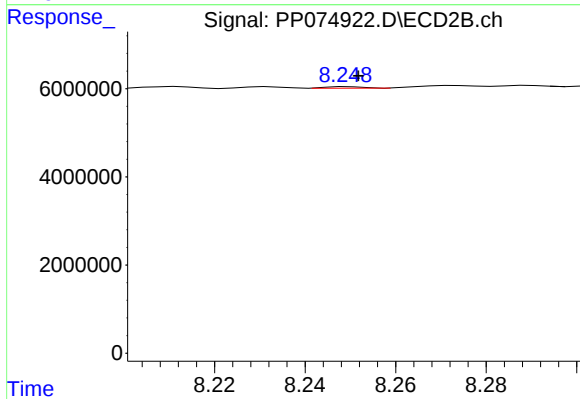

#44 AR-1268-4


R.T.: 8.250 min
Delta R.T.: -0.002 min
Response: 210499
Conc: 0.55 ng/ml

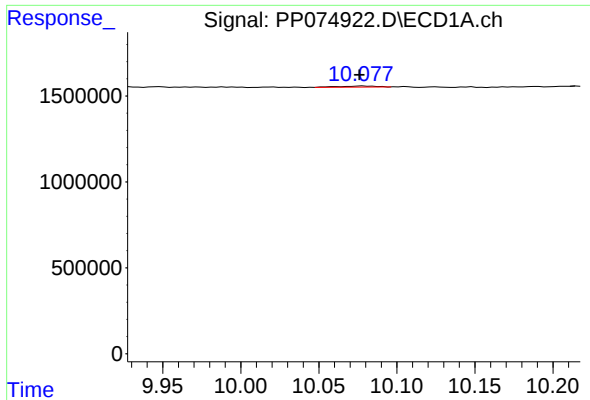

#45 AR-1268-5

R.T.: 10.078 min
Delta R.T.: 0.002 min
Response: 101674
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

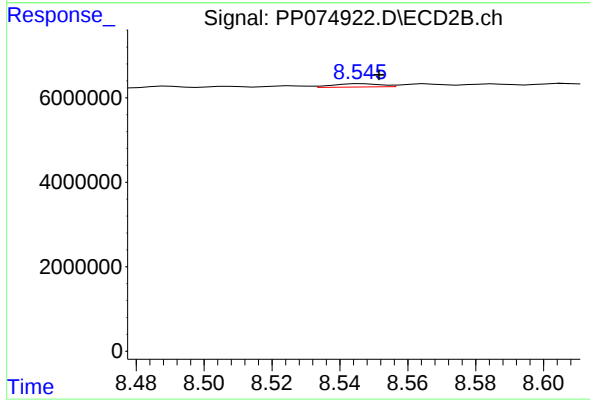

#45 AR-1268-5

R.T.: 8.547 min
Delta R.T.: -0.005 min
Response: 760957
Conc: 0.24 ng/ml