

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
 Data File : PP074924.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 05 Sep 2025 21:33
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1254 WATER MDL 25PPB
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 05 23:45:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.656	3.798	26228272	95617177	21.434	19.774
2)	SA Decachlor...	10.431	8.805	21155406	138.8E6	21.423	18.513
Target Compounds							
3)	L1 AR-1016-1	5.822	4.893	166048	231374	3.766	0.454 #
4)	L1 AR-1016-2	5.822	4.948	166048	255720	2.642	1.074 #
5)	L1 AR-1016-3	5.907	5.074	272134	226943	6.059	1.646 #
6)	L1 AR-1016-4	5.937f	5.115	444764	3967825	12.642	28.381 #
7)	L1 AR-1016-5	6.282	5.333	461232	1690052	13.898	10.176 #
8)	L2 AR-1221-1	4.854	4.013	187209	191187	10.641	3.090 #
9)	L2 AR-1221-2	4.957	4.089	601880	1759507	45.060	38.917
10)	L2 AR-1221-3	5.059f	4.172	84952	75064	2.241	0.457 #
11)	L3 AR-1232-1	5.059f	4.172	84952	75064	2.797	0.586 #
12)	L3 AR-1232-2	0.000	4.893	0	231374	N.D.	0.998 #
13)	L3 AR-1232-3	5.822	5.074	166048	226943	5.436	3.779 #
14)	L3 AR-1232-4	5.937f	5.155	444764	1086309	25.755	14.738 #
15)	L3 AR-1232-5	6.078	5.333	909124	1690052	70.035	27.222 #
16)	L4 AR-1242-1	5.822	4.893	166048	231374	4.338	0.549 #
17)	L4 AR-1242-2	5.822	4.965	166048	171590	2.940	0.857 #
18)	L4 AR-1242-3	5.907	5.074	272134	226943	6.702	1.918 #
19)	L4 AR-1242-4	5.937f	5.155	444764	1086309	14.012	6.347 #
20)	L4 AR-1242-5	6.724	5.678	1359375	10935778	37.687	59.060 #
21)	L5 AR-1248-1	5.822	4.893	166048	231374	5.494	0.838 #
22)	L5 AR-1248-2	6.078	5.115	909124	3967825	21.095	22.448
23)	L5 AR-1248-3	6.282	5.155	461232	1086309	9.876	4.781 #
24)	L5 AR-1248-4	6.655	5.333	2983434	1690052	54.243	7.752 #
25)	L5 AR-1248-5	6.724	5.764f	1359375	18968635	24.506	51.640 #
26)	L6 AR-1254-1	6.655	5.678	2983434	10935778	51.201	22.940 #
27)	L6 AR-1254-2	6.872	5.826	2452807	11089056	30.053	31.491
28)	L6 AR-1254-3	7.230	6.225	4053955	13543364	45.445	21.851 #
29)	L6 AR-1254-4	7.515	6.453	1540801	9831293	23.376	20.979
30)	L6 AR-1254-5	7.930	6.869	2201277	9525330	26.494	19.420 #
31)	L7 AR-1260-1	7.398	6.360	721671	6862438	12.484	18.289 #
32)	L7 AR-1260-2	7.651	6.539	1135323	5891697	16.474	11.141 #
33)	L7 AR-1260-3	7.991	6.693	611508	4222378	11.786	9.751
34)	L7 AR-1260-4	8.219	7.169	1261832	634358	19.780	1.663 #
35)	L7 AR-1260-5	8.562	7.408	432621	1121908	3.815	1.117 #
36)	L8 AR-1262-1	8.219	6.923	1261832	615237	16.384	0.870 #
37)	L8 AR-1262-2	8.562	7.169	432621	634358	3.268	1.218 #
38)	L8 AR-1262-3	8.893	7.703	211880	1972475	2.180	4.230 #
39)	L8 AR-1262-4	0.000	7.765	0	2049261	N.D.	2.493 #
40)	L8 AR-1262-5	9.600f	8.256	88804	224750	1.457	0.627 #
41)	L9 AR-1268-1	8.893	7.688	211880	2138088	1.308	1.516

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
Data File : PP074924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 21:33
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1254 WATER MDL 25PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:45:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	0.000	7.765	0	2049261	N.D.	1.503 #
43) L9	AR-1268-3	9.151f	7.963	119305	817302	0.965	0.783
44) L9	AR-1268-4	9.600f	8.256	88804	224750	1.320	0.587 #
45) L9	AR-1268-5	10.074	8.545	145793	801654	0.394	0.256 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090525\
Data File : PP074924.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 05 Sep 2025 21:33
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1254 WATER MDL 25PPB
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 05 23:45:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

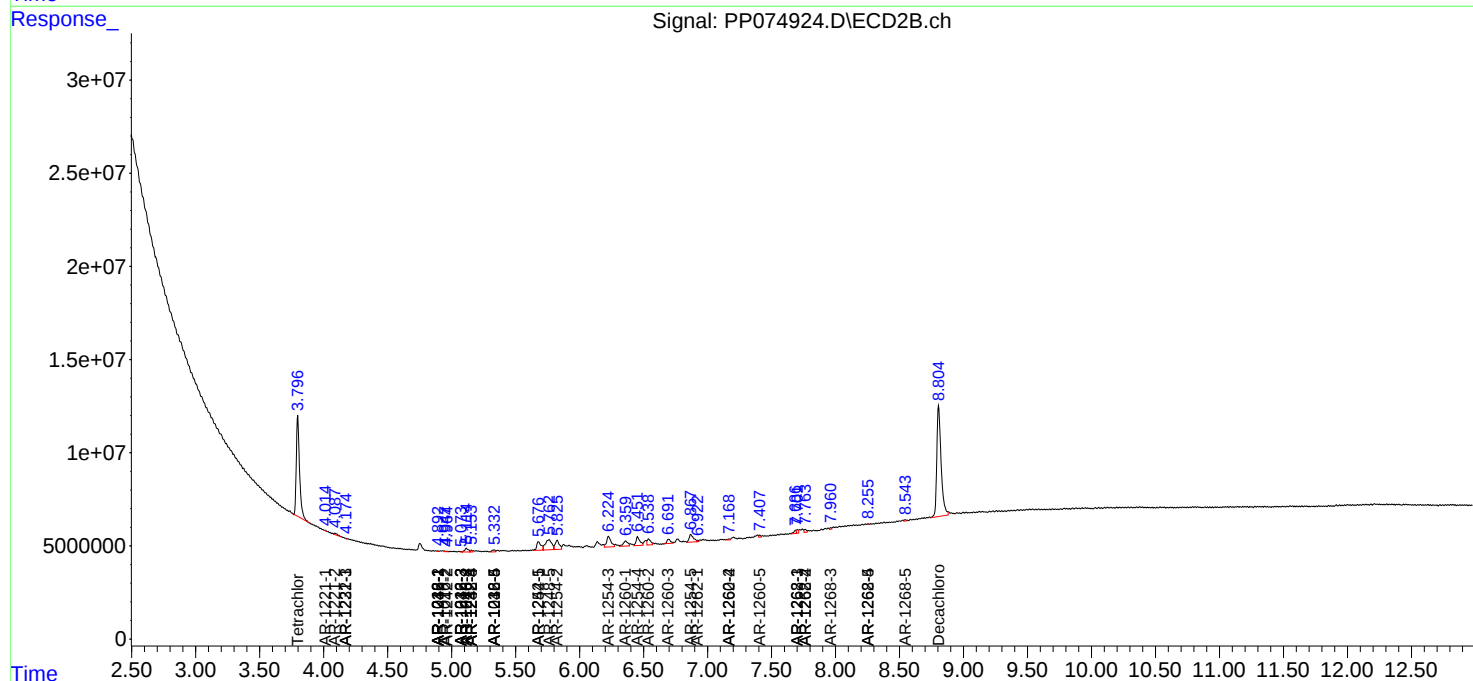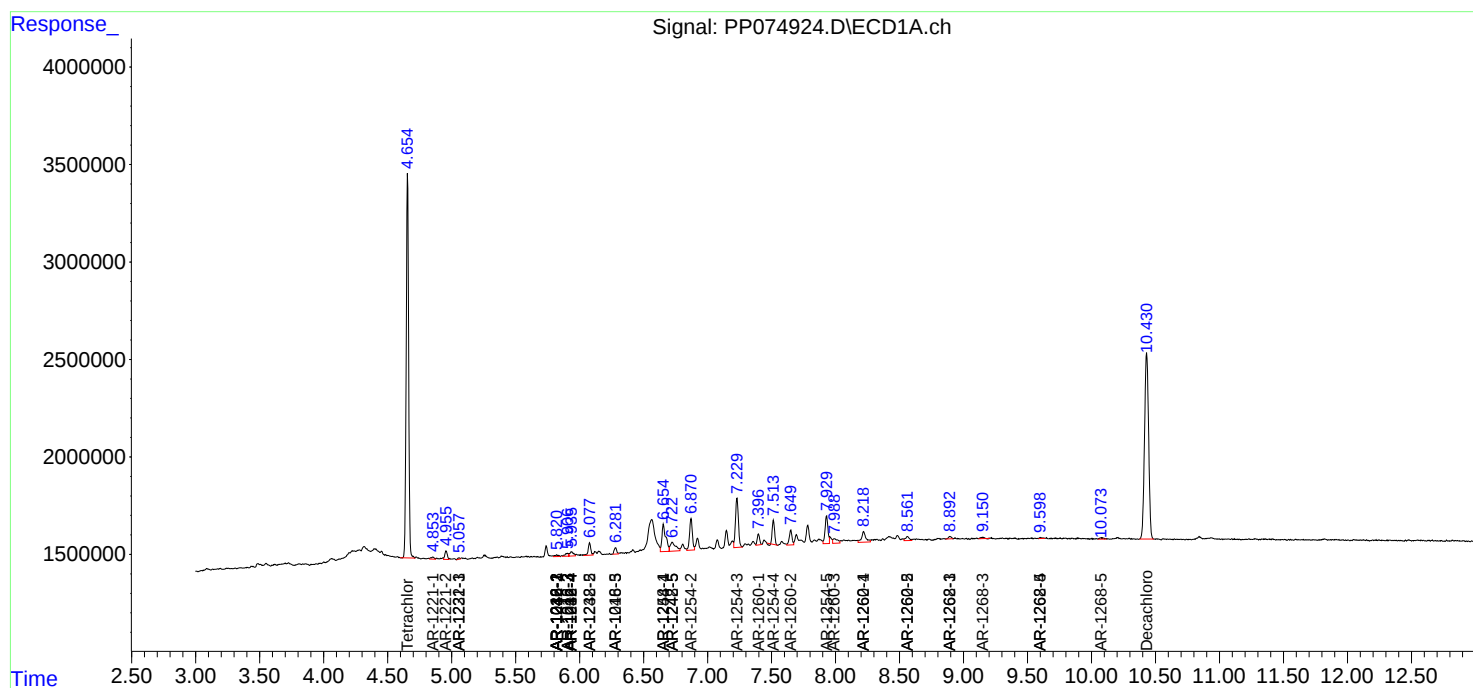


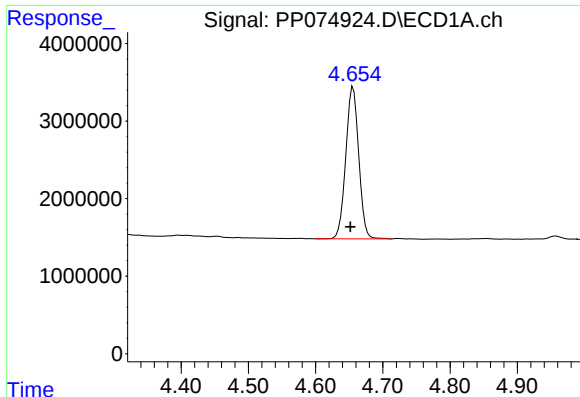

#1 Tetrachloro-m-xylene


R.T.: 4.656 min
Delta R.T.: 0.004 min
Response: 26228272
Conc: 21.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

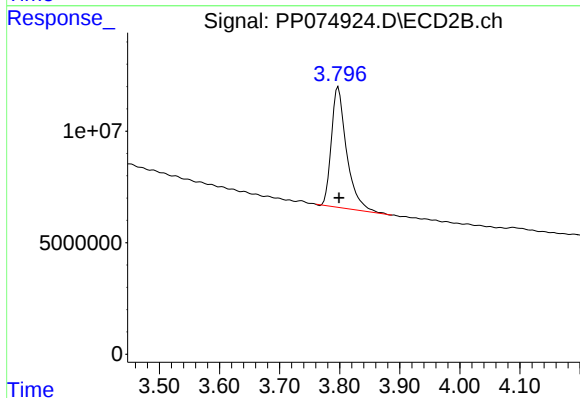


#1 Tetrachloro-m-xylene

R.T.: 3.798 min
Delta R.T.: -0.001 min
Response: 95617177
Conc: 19.77 ng/ml

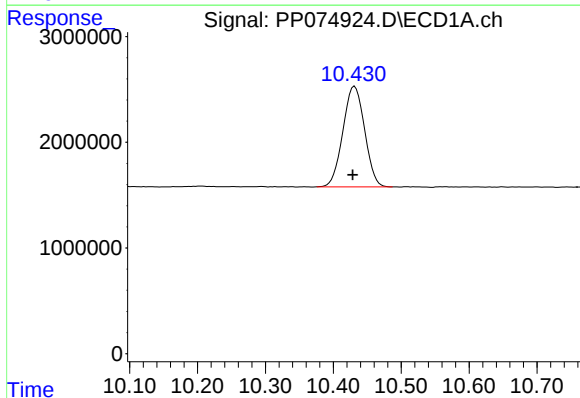


#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.003 min
Response: 21155406
Conc: 21.42 ng/ml

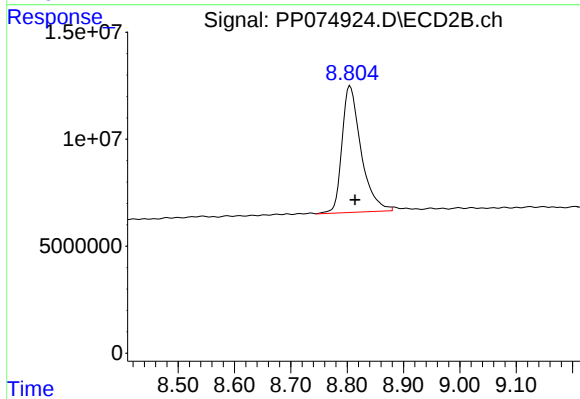

#2 Decachlorobiphenyl


R.T.: 8.805 min
Delta R.T.: -0.009 min
Response: 138832128
Conc: 18.51 ng/ml

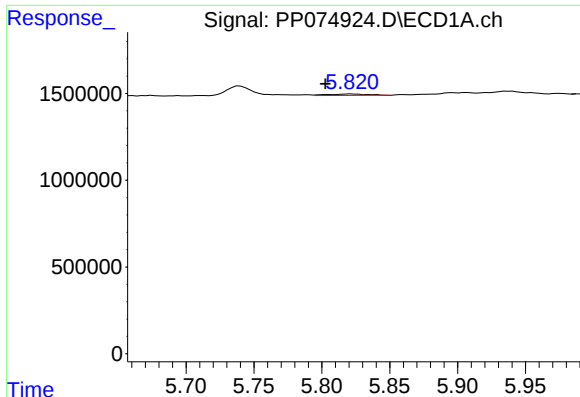

#3 AR-1016-1


R.T.: 5.822 min
Delta R.T.: 0.019 min
Response: 166048
Conc: 3.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

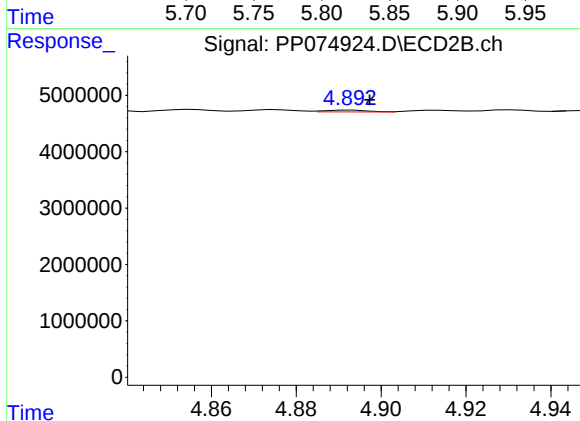


#3 AR-1016-1

R.T.: 4.893 min
Delta R.T.: -0.004 min
Response: 231374
Conc: 0.45 ng/ml

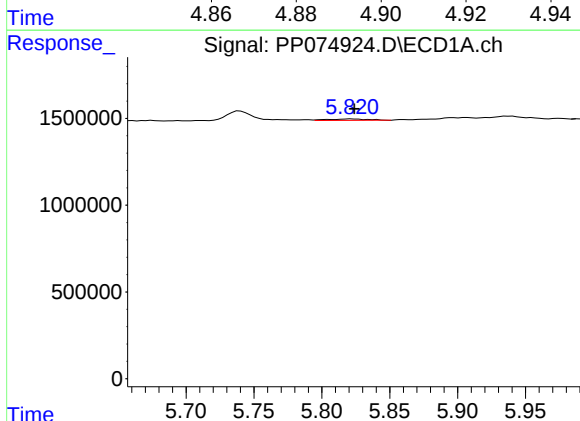


#4 AR-1016-2

R.T.: 5.822 min
Delta R.T.: -0.002 min
Response: 166048
Conc: 2.64 ng/ml

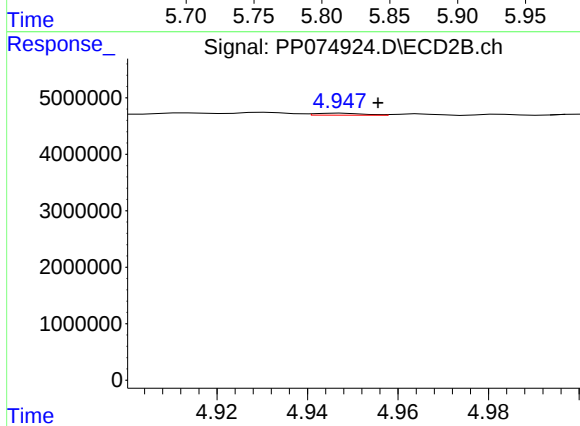

#4 AR-1016-2


R.T.: 4.948 min
Delta R.T.: -0.008 min
Response: 255720
Conc: 1.07 ng/ml

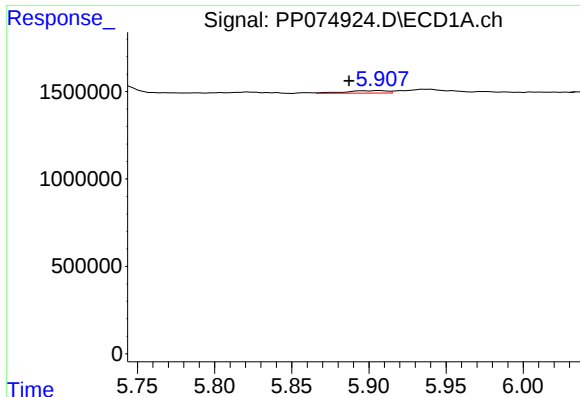

#5 AR-1016-3


R.T.: 5.907 min
Delta R.T.: 0.020 min
Response: 272134
Conc: 6.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

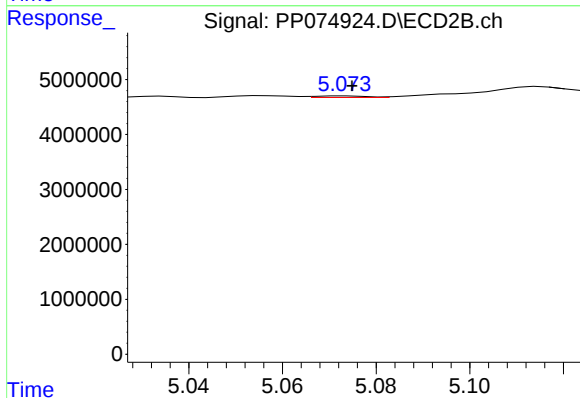


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 226943
Conc: 1.65 ng/ml

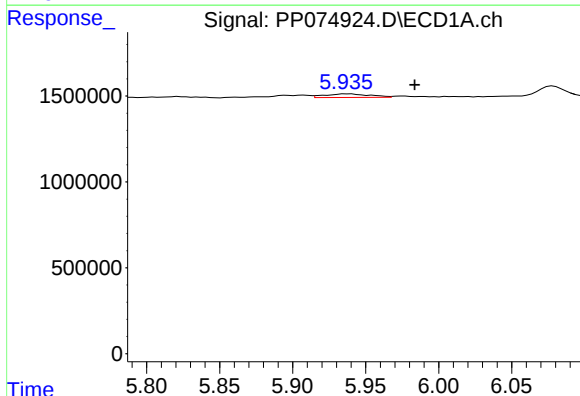


#6 AR-1016-4

R.T.: 5.937 min
Delta R.T.: -0.047 min
Response: 444764
Conc: 12.64 ng/ml

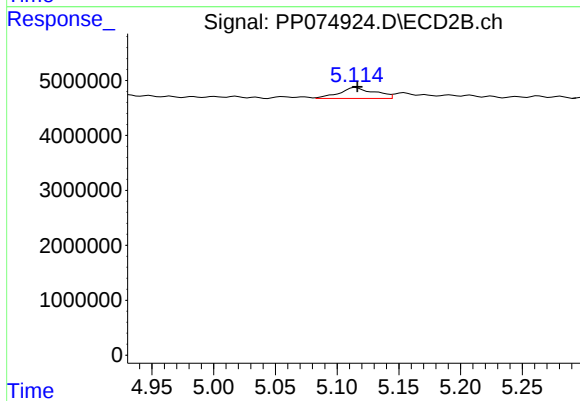

#6 AR-1016-4


R.T.: 5.115 min
Delta R.T.: -0.001 min
Response: 3967825
Conc: 28.38 ng/ml

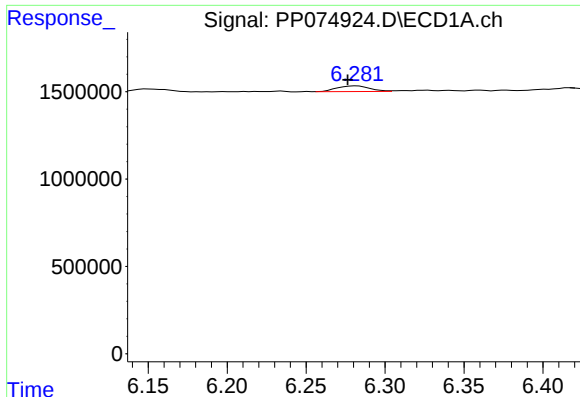

#7 AR-1016-5


R.T.: 6.282 min
Delta R.T.: 0.006 min
Response: 461232
Conc: 13.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

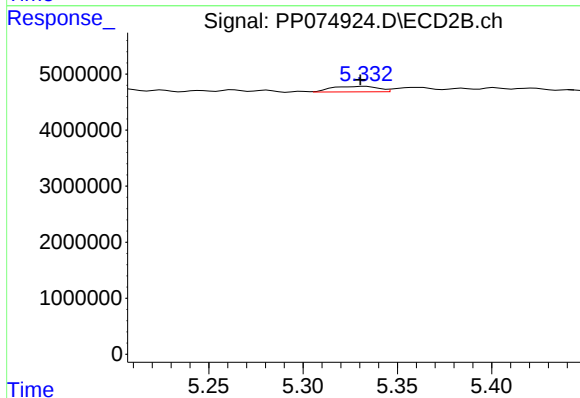


#7 AR-1016-5

R.T.: 5.333 min
Delta R.T.: 0.003 min
Response: 1690052
Conc: 10.18 ng/ml

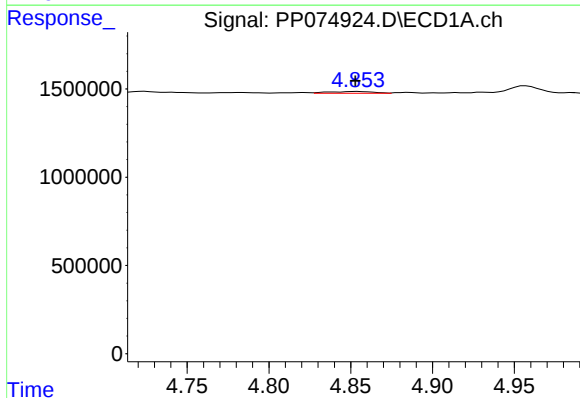


#8 AR-1221-1

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 187209
Conc: 10.64 ng/ml

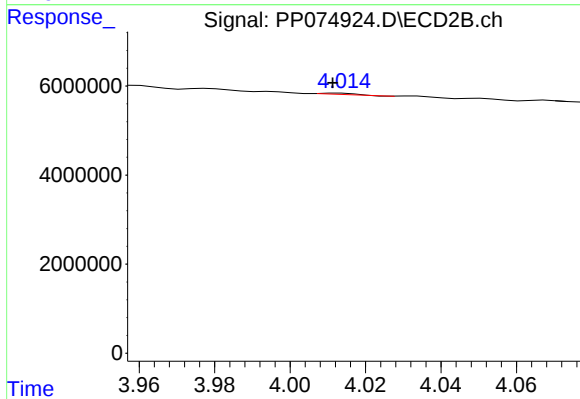

#8 AR-1221-1


R.T.: 4.013 min
Delta R.T.: 0.002 min
Response: 191187
Conc: 3.09 ng/ml

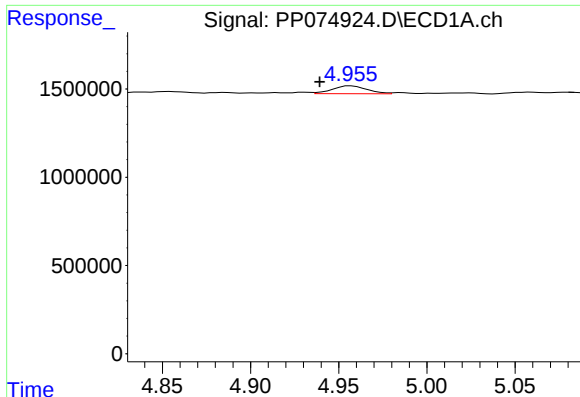

#9 AR-1221-2


R.T.: 4.957 min
Delta R.T.: 0.018 min
Response: 601880
Conc: 45.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

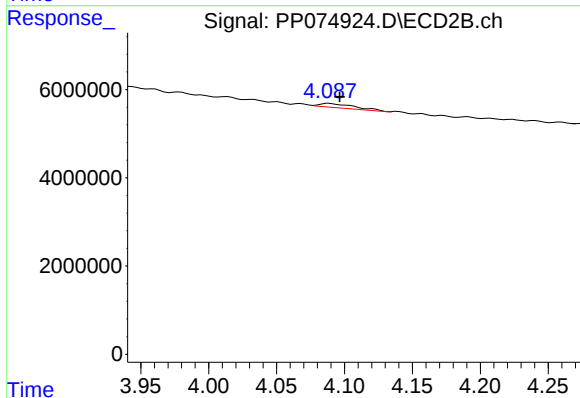


#9 AR-1221-2

R.T.: 4.089 min
Delta R.T.: -0.008 min
Response: 1759507
Conc: 38.92 ng/ml

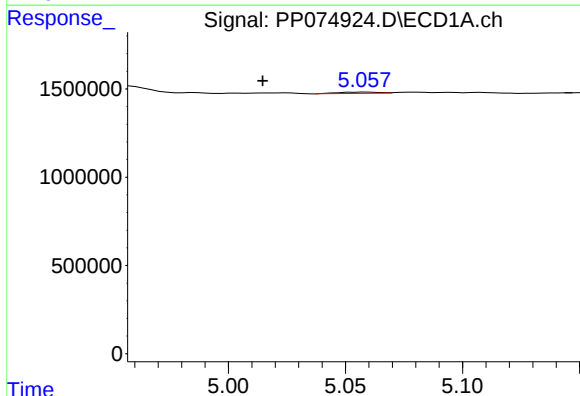


#10 AR-1221-3

R.T.: 5.059 min
Delta R.T.: 0.045 min
Response: 84952
Conc: 2.24 ng/ml

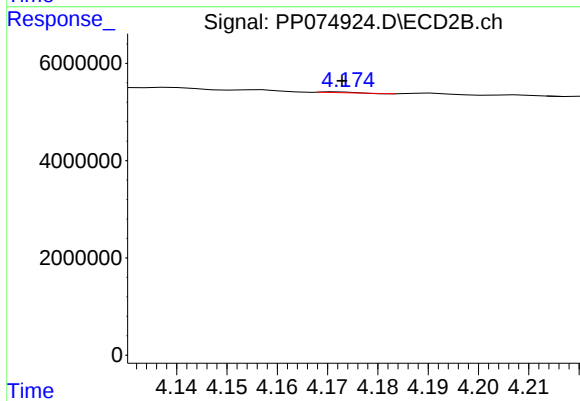

#10 AR-1221-3


R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 75064
Conc: 0.46 ng/ml

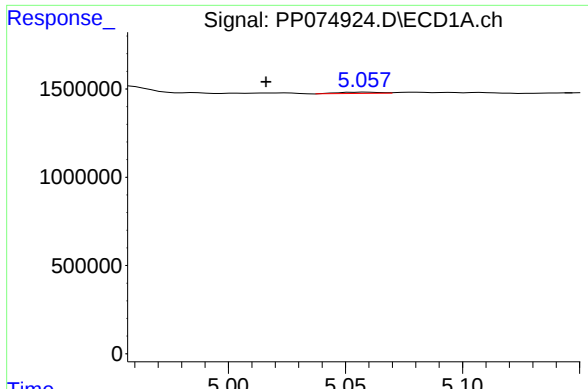

#11 AR-1232-1


R.T.: 5.059 min
Delta R.T.: 0.043 min
Response: 84952
Conc: 2.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

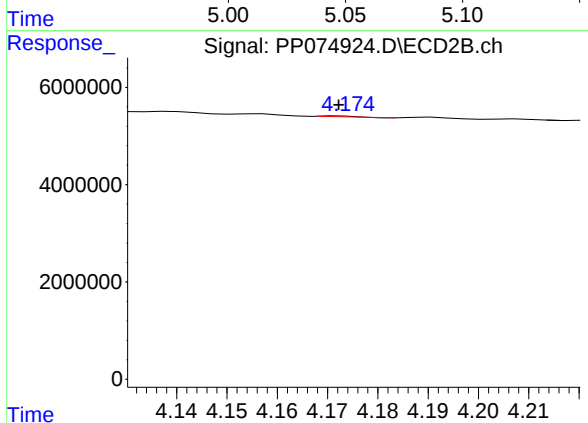


#11 AR-1232-1

R.T.: 4.172 min
Delta R.T.: 0.000 min
Response: 75064
Conc: 0.59 ng/ml

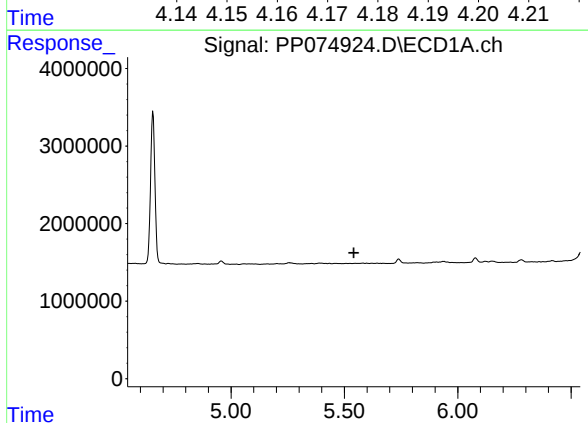


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.542 min
Response: 0
Conc: N.D.

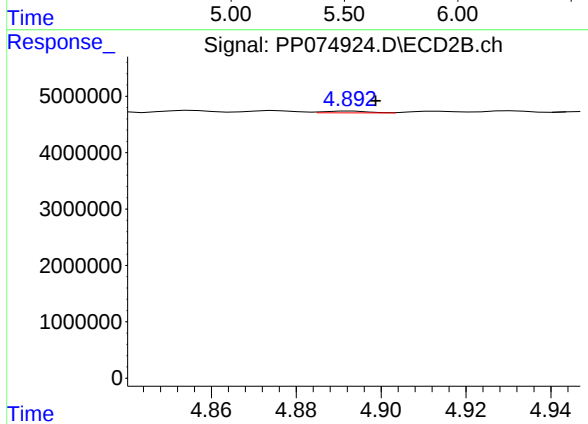

#12 AR-1232-2


R.T.: 4.893 min
Delta R.T.: -0.006 min
Response: 231374
Conc: 1.00 ng/ml

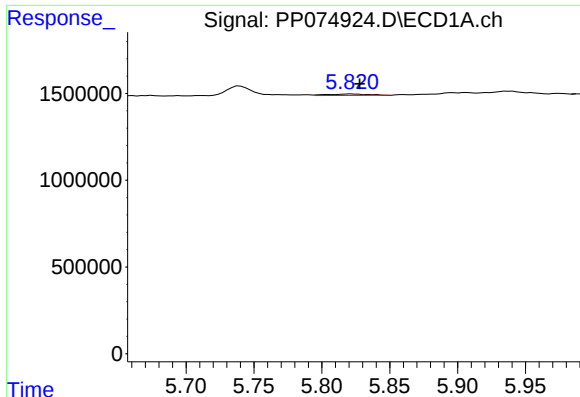

#13 AR-1232-3


R.T.: 5.822 min
Delta R.T.: -0.006 min
Response: 166048
Conc: 5.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

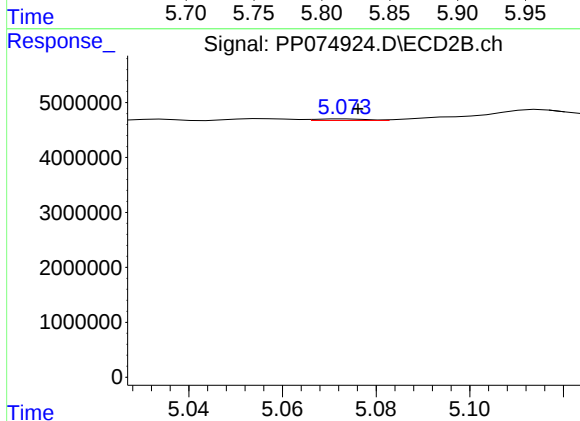


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 226943
Conc: 3.78 ng/ml

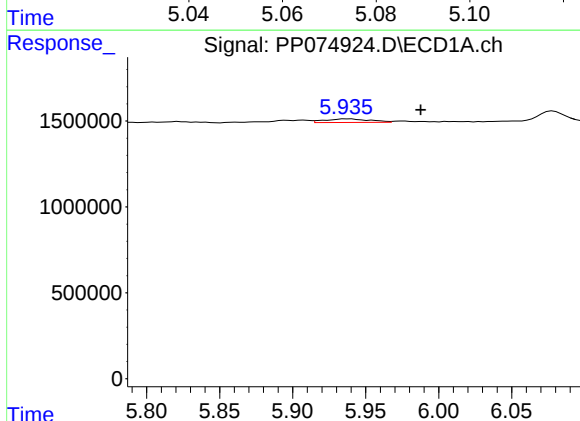


#14 AR-1232-4

R.T.: 5.937 min
Delta R.T.: -0.051 min
Response: 444764
Conc: 25.75 ng/ml

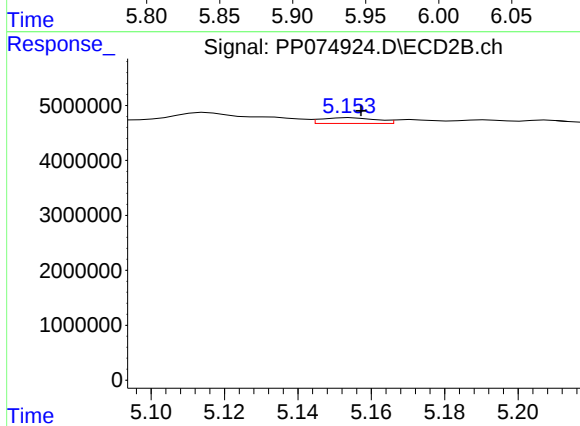

#14 AR-1232-4


R.T.: 5.155 min
Delta R.T.: -0.003 min
Response: 1086309
Conc: 14.74 ng/ml

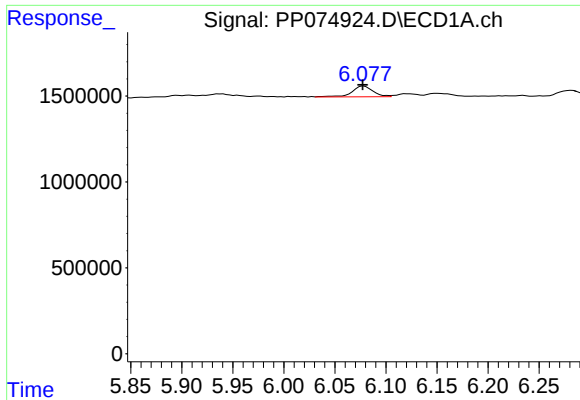

#15 AR-1232-5


R.T.: 6.078 min
Delta R.T.: 0.001 min
Response: 909124
Conc: 70.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

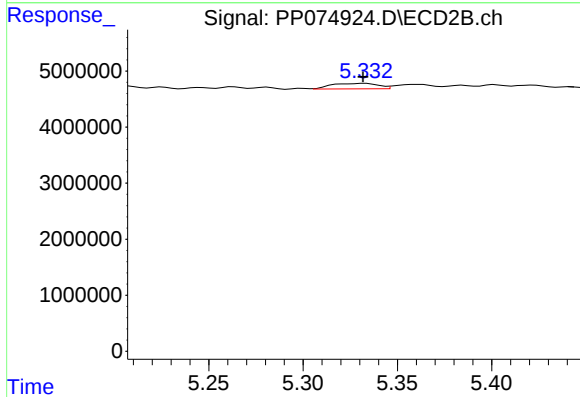


#15 AR-1232-5

R.T.: 5.333 min
Delta R.T.: 0.001 min
Response: 1690052
Conc: 27.22 ng/ml

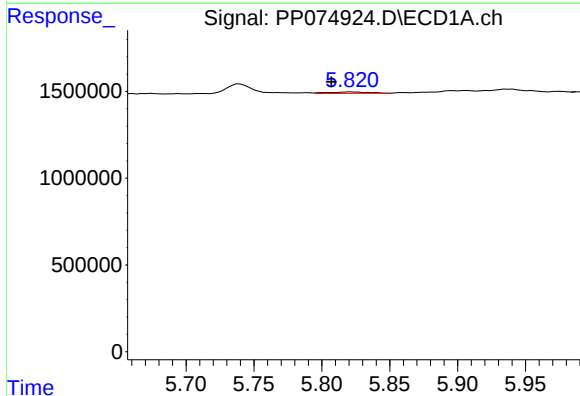


#16 AR-1242-1

R.T.: 5.822 min
Delta R.T.: 0.015 min
Response: 166048
Conc: 4.34 ng/ml

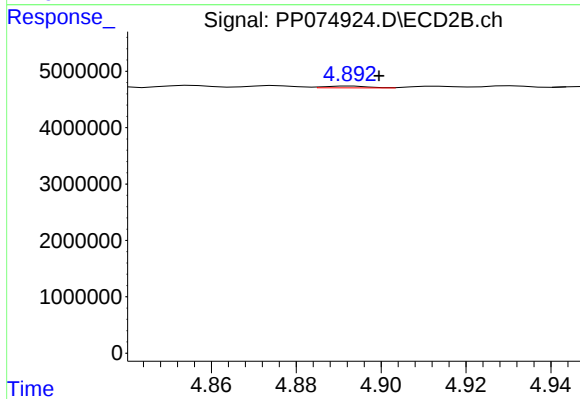

#16 AR-1242-1


R.T.: 4.893 min
Delta R.T.: -0.007 min
Response: 231374
Conc: 0.55 ng/ml

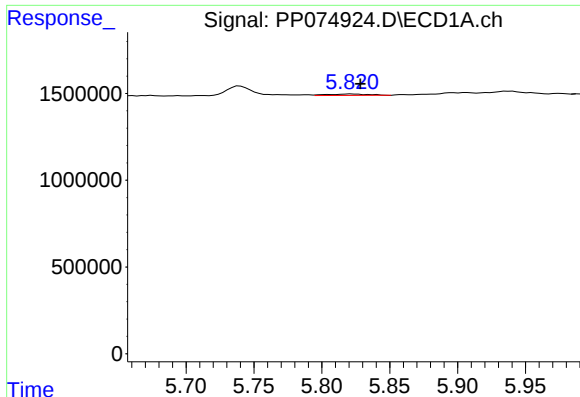

#17 AR-1242-2


R.T.: 5.822 min
Delta R.T.: -0.006 min
Response: 166048
Conc: 2.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

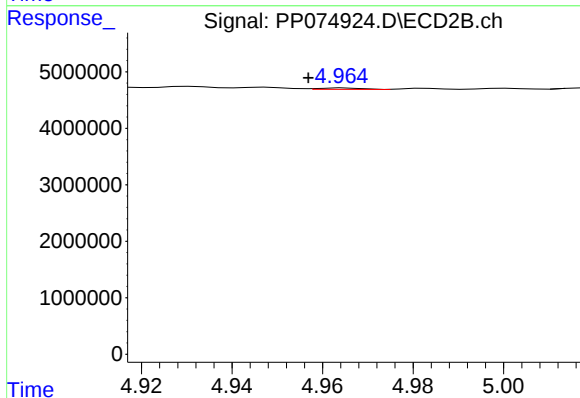


#17 AR-1242-2

R.T.: 4.965 min
Delta R.T.: 0.008 min
Response: 171590
Conc: 0.86 ng/ml

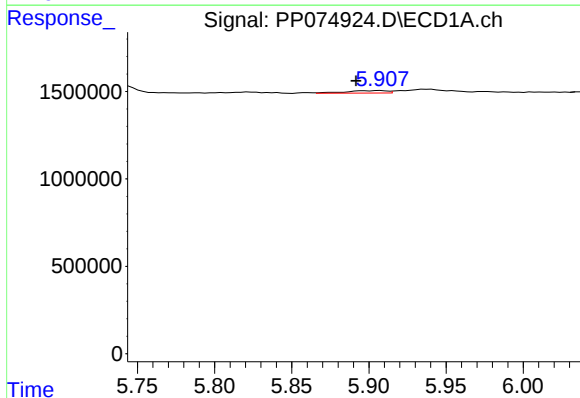


#18 AR-1242-3

R.T.: 5.907 min
Delta R.T.: 0.016 min
Response: 272134
Conc: 6.70 ng/ml

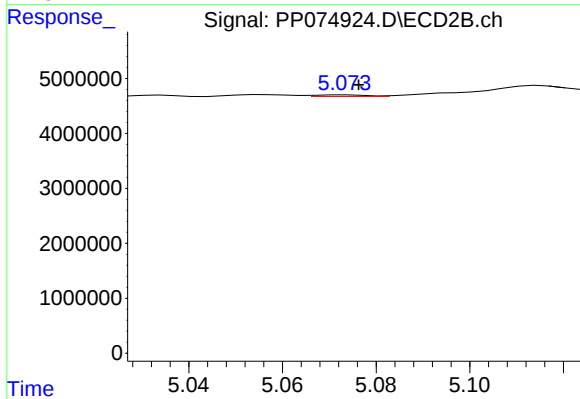

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 226943
Conc: 1.92 ng/ml

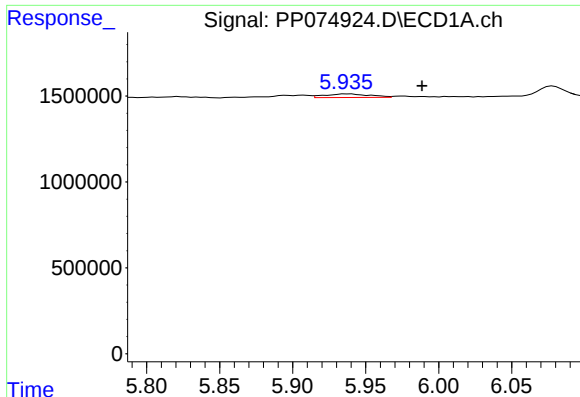

#19 AR-1242-4


R.T.: 5.937 min
Delta R.T.: -0.051 min
Response: 444764
Conc: 14.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

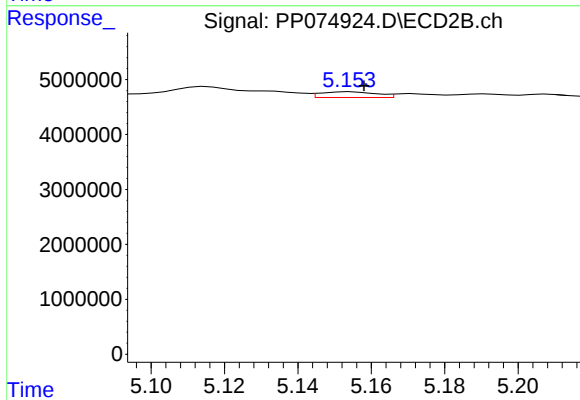


#19 AR-1242-4

R.T.: 5.155 min
Delta R.T.: -0.003 min
Response: 1086309
Conc: 6.35 ng/ml

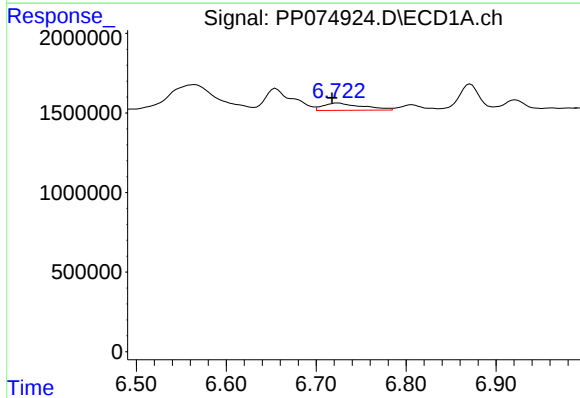


#20 AR-1242-5

R.T.: 6.724 min
Delta R.T.: 0.007 min
Response: 1359375
Conc: 37.69 ng/ml

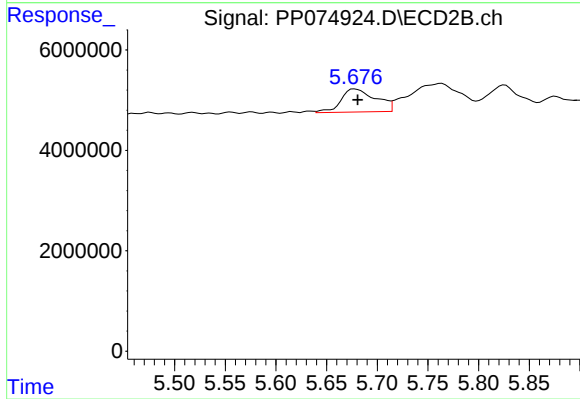

#20 AR-1242-5


R.T.: 5.678 min
Delta R.T.: -0.003 min
Response: 10935778
Conc: 59.06 ng/ml

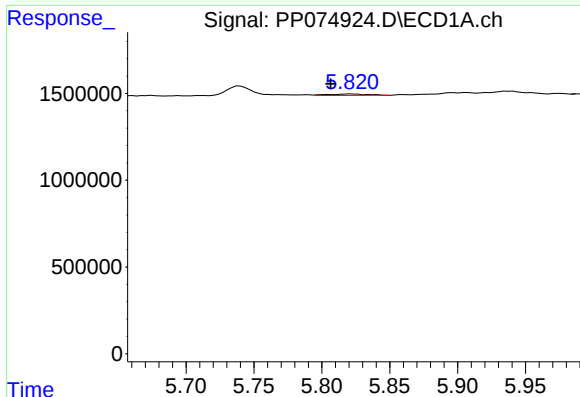

#21 AR-1248-1


R.T.: 5.822 min
Delta R.T.: 0.015 min
Response: 166048
Conc: 5.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

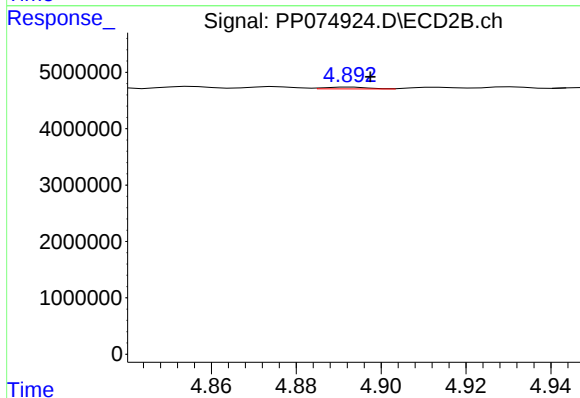


#21 AR-1248-1

R.T.: 4.893 min
Delta R.T.: -0.004 min
Response: 231374
Conc: 0.84 ng/ml

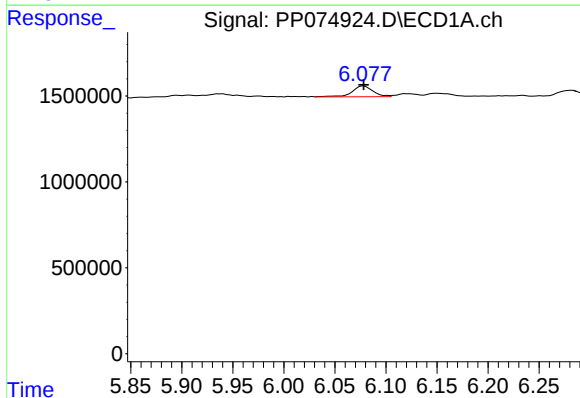


#22 AR-1248-2

R.T.: 6.078 min
Delta R.T.: 0.000 min
Response: 909124
Conc: 21.10 ng/ml

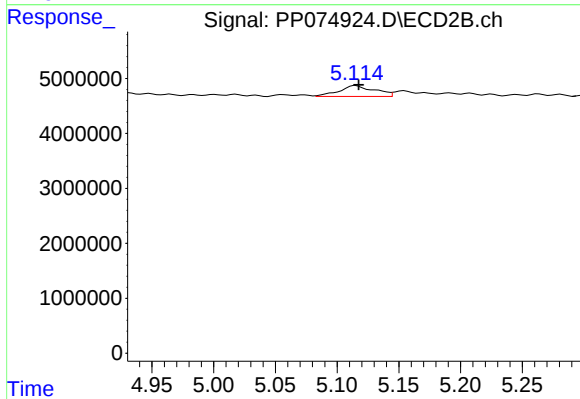

#22 AR-1248-2


R.T.: 5.115 min
Delta R.T.: -0.002 min
Response: 3967825
Conc: 22.45 ng/ml

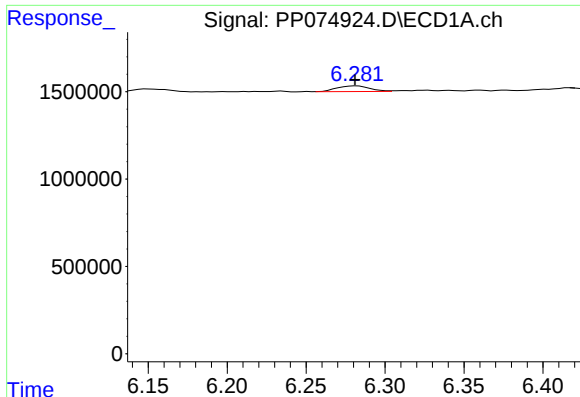

#23 AR-1248-3


R.T.: 6.282 min
Delta R.T.: 0.000 min
Response: 461232
Conc: 9.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

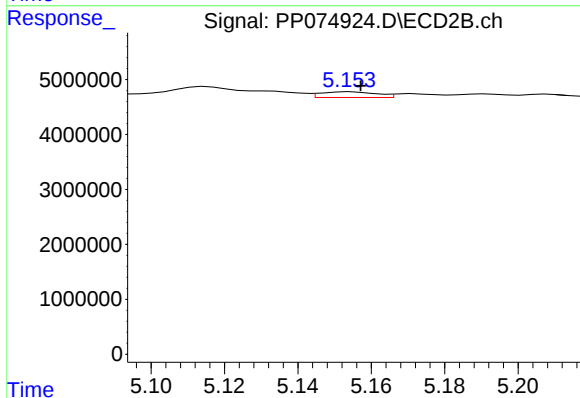


#23 AR-1248-3

R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 1086309
Conc: 4.78 ng/ml

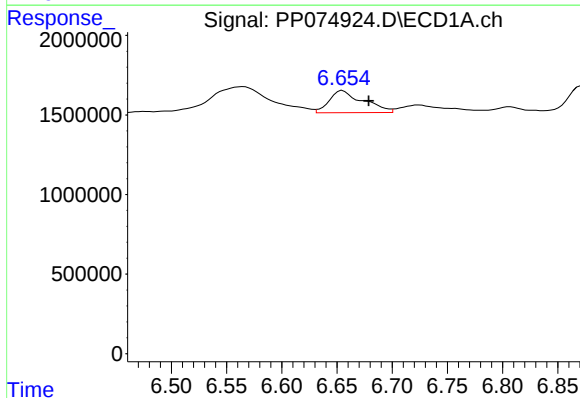


#24 AR-1248-4

R.T.: 6.655 min
Delta R.T.: -0.024 min
Response: 2983434
Conc: 54.24 ng/ml

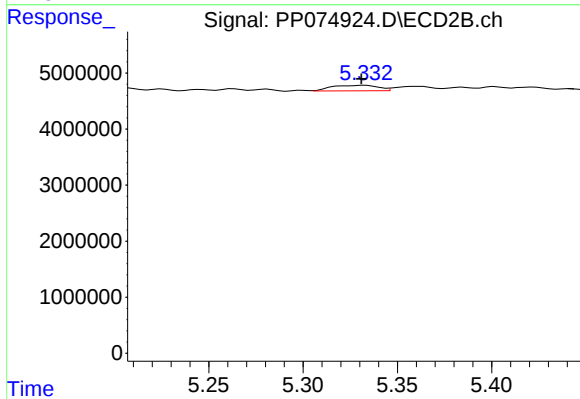

#24 AR-1248-4


R.T.: 5.333 min
Delta R.T.: 0.002 min
Response: 1690052
Conc: 7.75 ng/ml

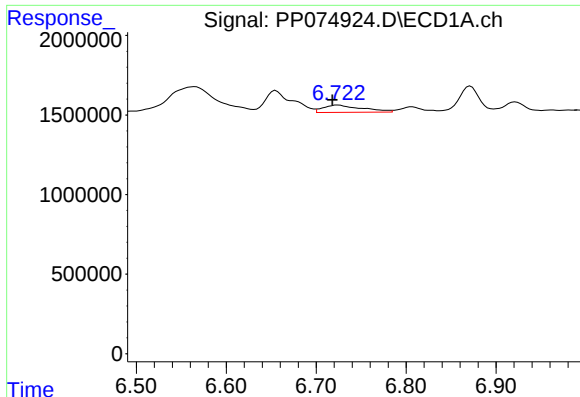

#25 AR-1248-5


R.T.: 6.724 min
Delta R.T.: 0.006 min
Response: 1359375
Conc: 24.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

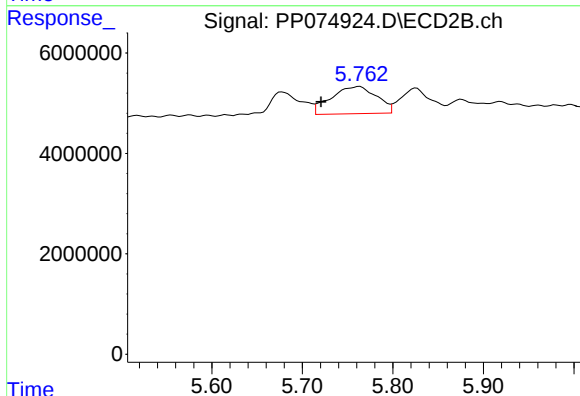


#25 AR-1248-5

R.T.: 5.764 min
Delta R.T.: 0.043 min
Response: 18968635
Conc: 51.64 ng/ml

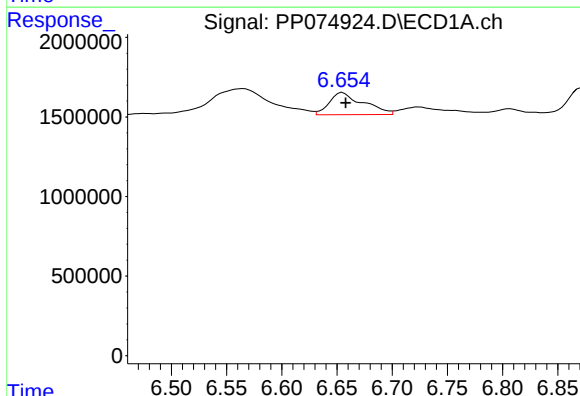


#26 AR-1254-1

R.T.: 6.655 min
Delta R.T.: -0.003 min
Response: 2983434
Conc: 51.20 ng/ml

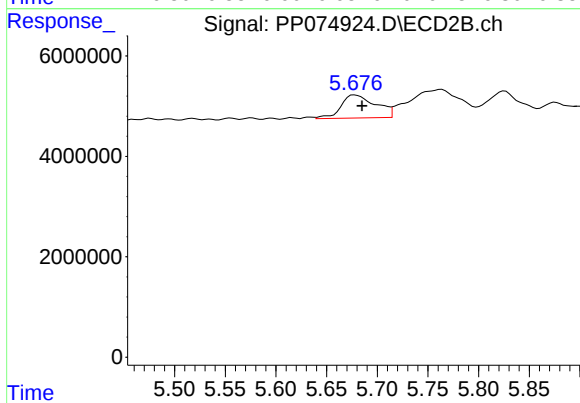

#26 AR-1254-1


R.T.: 5.678 min
Delta R.T.: -0.008 min
Response: 10935778
Conc: 22.94 ng/ml

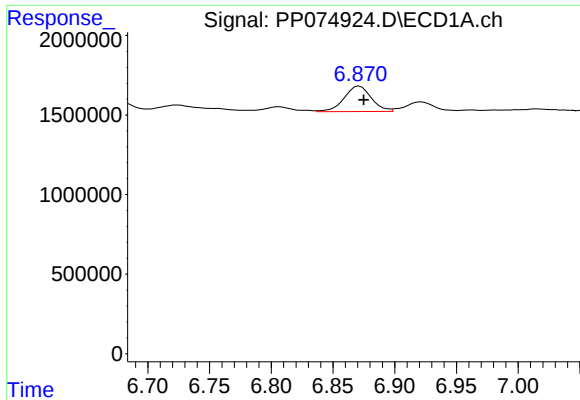

#27 AR-1254-2


R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 2452807
Conc: 30.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

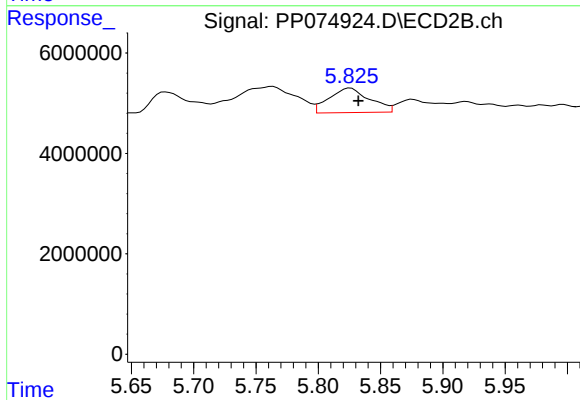


#27 AR-1254-2

R.T.: 5.826 min
Delta R.T.: -0.006 min
Response: 11089056
Conc: 31.49 ng/ml

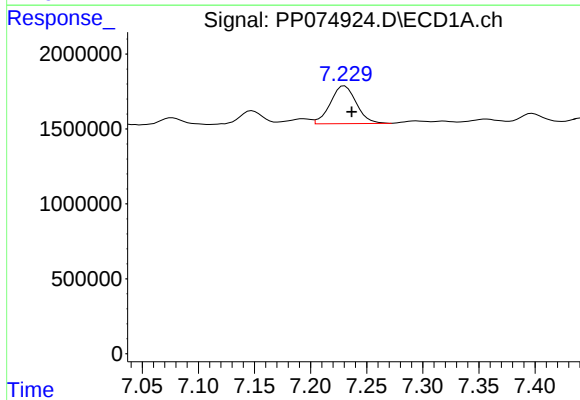


#28 AR-1254-3

R.T.: 7.230 min
Delta R.T.: -0.006 min
Response: 4053955
Conc: 45.44 ng/ml

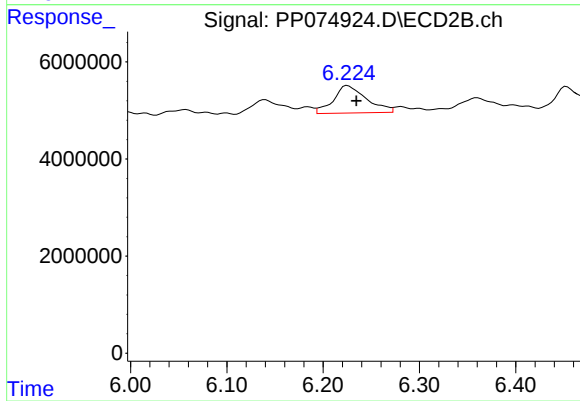

#28 AR-1254-3


R.T.: 6.225 min
Delta R.T.: -0.009 min
Response: 13543364
Conc: 21.85 ng/ml

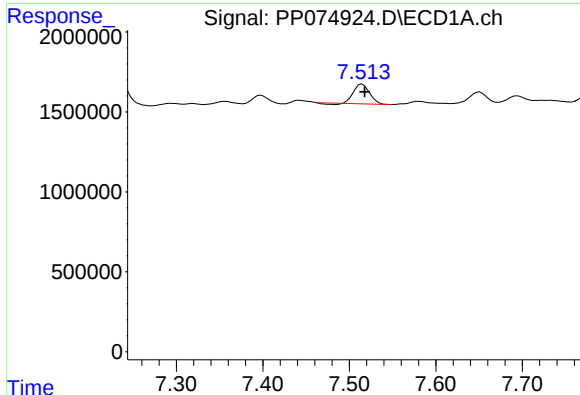

#29 AR-1254-4


R.T.: 7.515 min
Delta R.T.: -0.003 min
Response: 1540801
Conc: 23.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

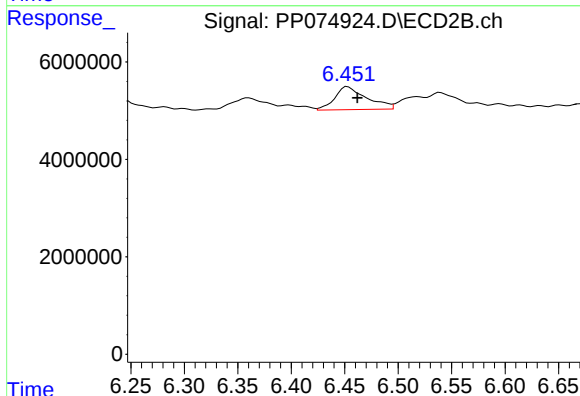


#29 AR-1254-4

R.T.: 6.453 min
Delta R.T.: -0.009 min
Response: 9831293
Conc: 20.98 ng/ml

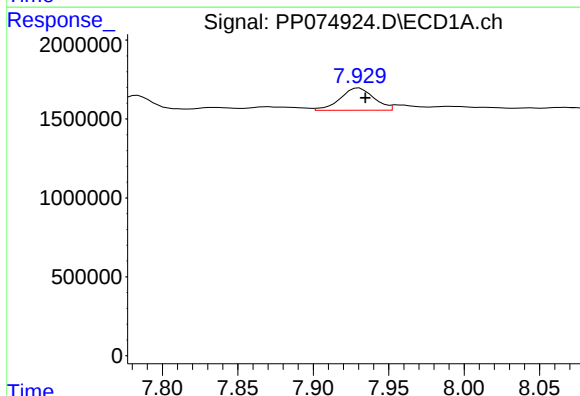


#30 AR-1254-5

R.T.: 7.930 min
Delta R.T.: -0.004 min
Response: 2201277
Conc: 26.49 ng/ml

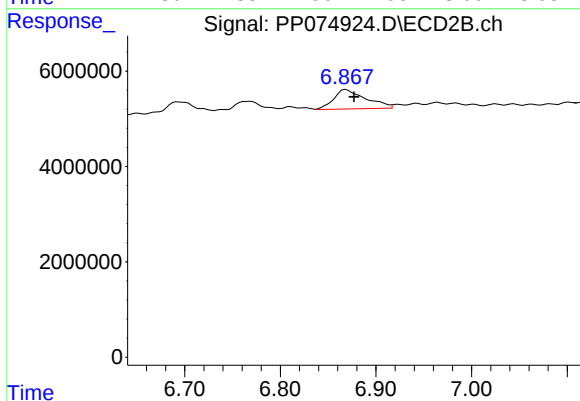

#30 AR-1254-5


R.T.: 6.869 min
Delta R.T.: -0.009 min
Response: 9525330
Conc: 19.42 ng/ml

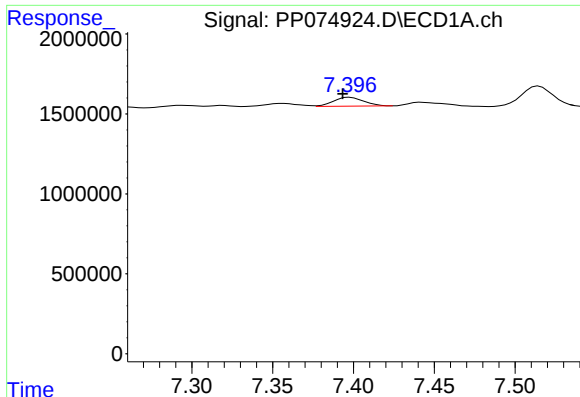

#31 AR-1260-1


R.T.: 7.398 min
Delta R.T.: 0.004 min
Response: 721671
Conc: 12.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

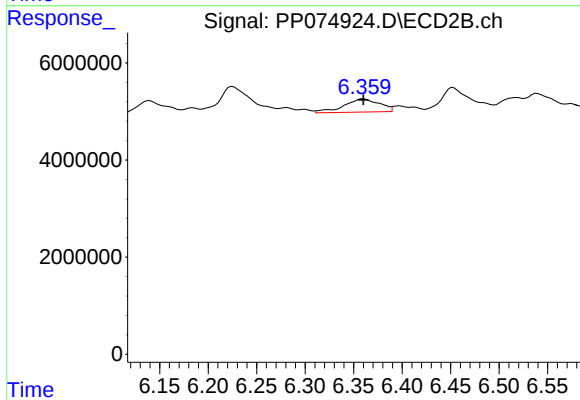


#31 AR-1260-1

R.T.: 6.360 min
Delta R.T.: 0.000 min
Response: 6862438
Conc: 18.29 ng/ml

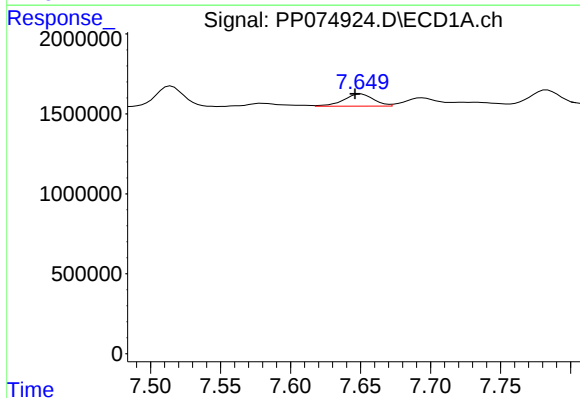


#32 AR-1260-2

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 1135323
Conc: 16.47 ng/ml

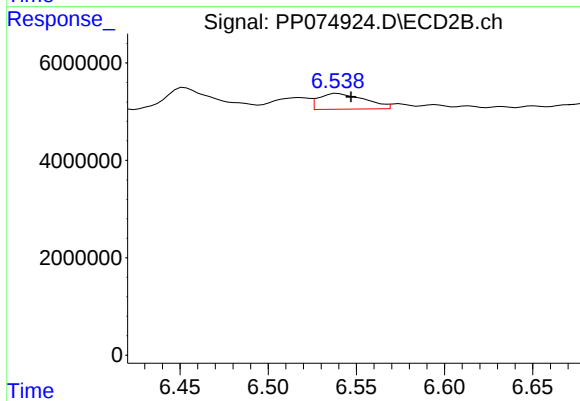

#32 AR-1260-2


R.T.: 6.539 min
Delta R.T.: -0.008 min
Response: 5891697
Conc: 11.14 ng/ml

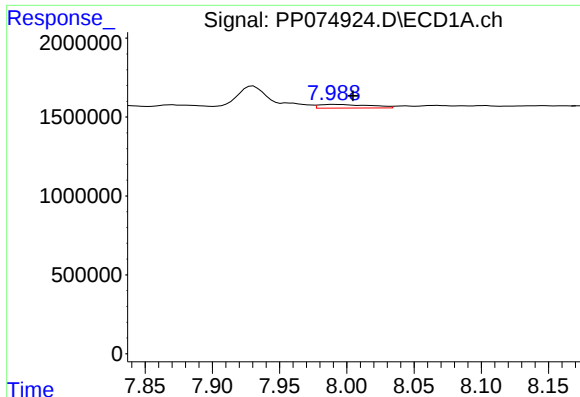

#33 AR-1260-3


R.T.: 7.991 min
Delta R.T.: -0.014 min
Response: 611508
Conc: 11.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

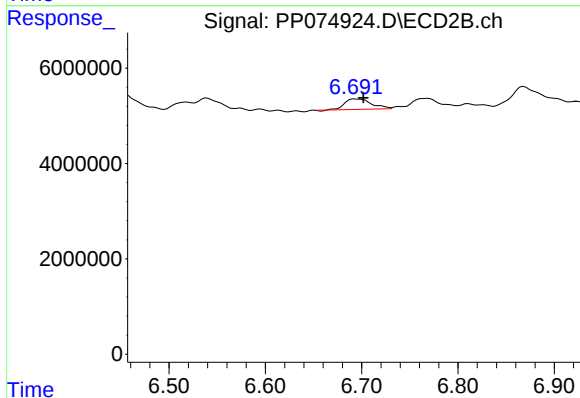


#33 AR-1260-3

R.T.: 6.693 min
Delta R.T.: -0.009 min
Response: 4222378
Conc: 9.75 ng/ml

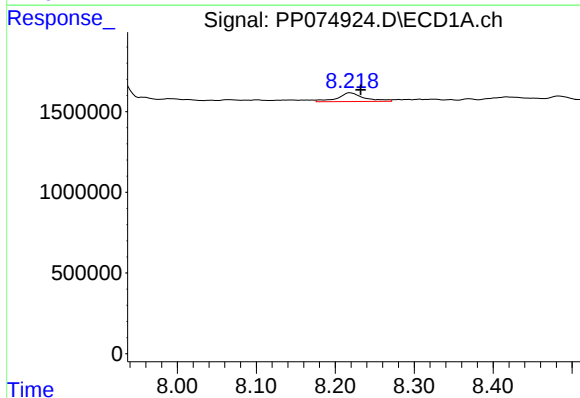


#34 AR-1260-4

R.T.: 8.219 min
Delta R.T.: -0.013 min
Response: 1261832
Conc: 19.78 ng/ml

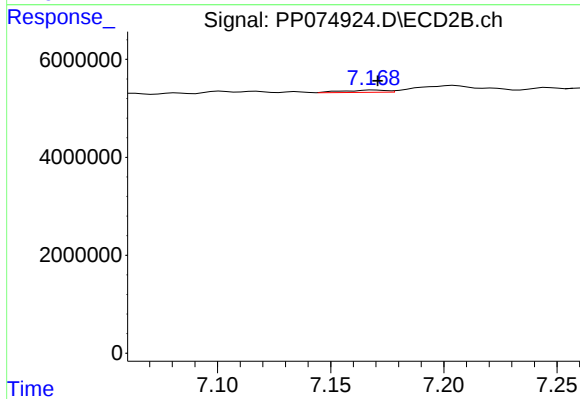

#34 AR-1260-4


R.T.: 7.169 min
Delta R.T.: -0.002 min
Response: 634358
Conc: 1.66 ng/ml

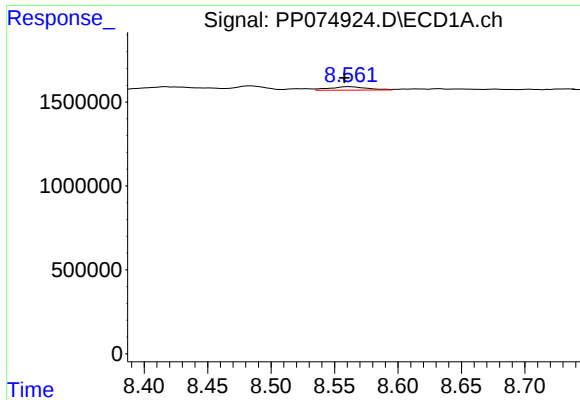

#35 AR-1260-5


R.T.: 8.562 min
Delta R.T.: 0.004 min
Response: 432621
Conc: 3.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

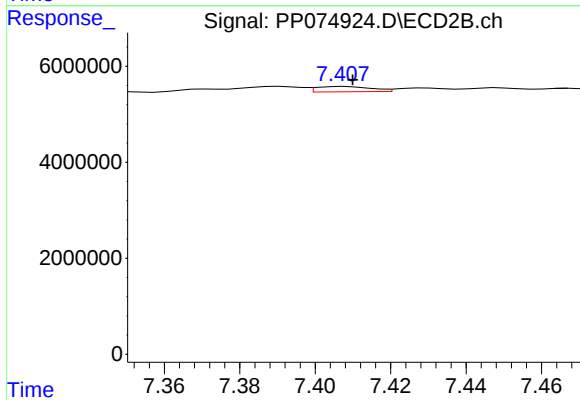


#35 AR-1260-5

R.T.: 7.408 min
Delta R.T.: -0.002 min
Response: 1121908
Conc: 1.12 ng/ml

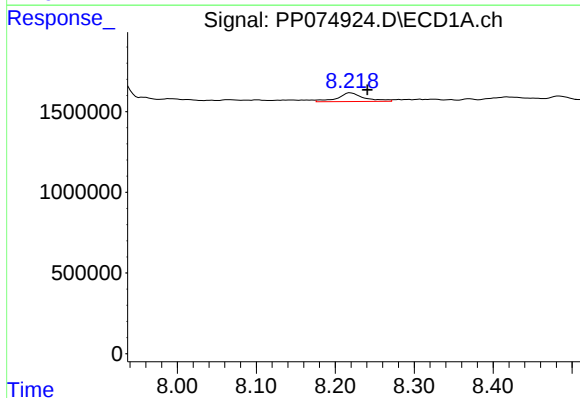


#36 AR-1262-1

R.T.: 8.219 min
Delta R.T.: -0.021 min
Response: 1261832
Conc: 16.38 ng/ml

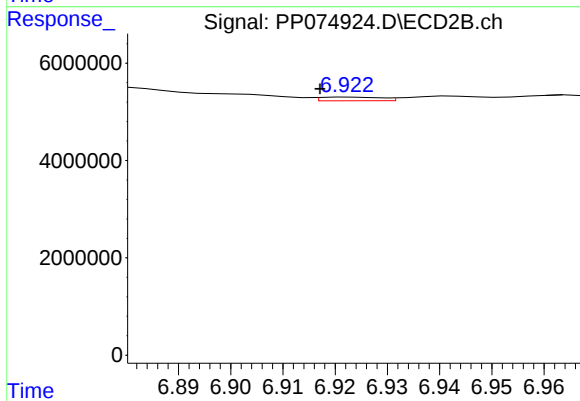

#36 AR-1262-1


R.T.: 6.923 min
Delta R.T.: 0.006 min
Response: 615237
Conc: 0.87 ng/ml

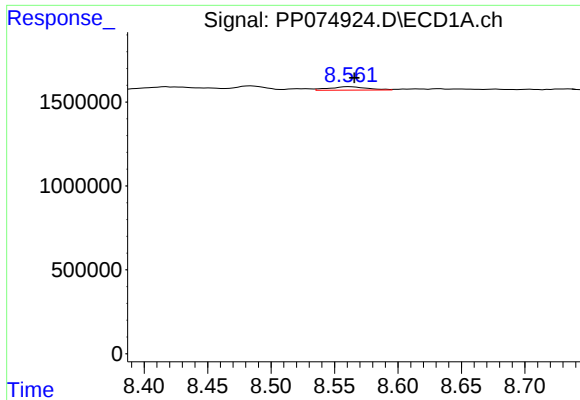

#37 AR-1262-2


R.T.: 8.562 min
Delta R.T.: -0.003 min
Response: 432621
Conc: 3.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

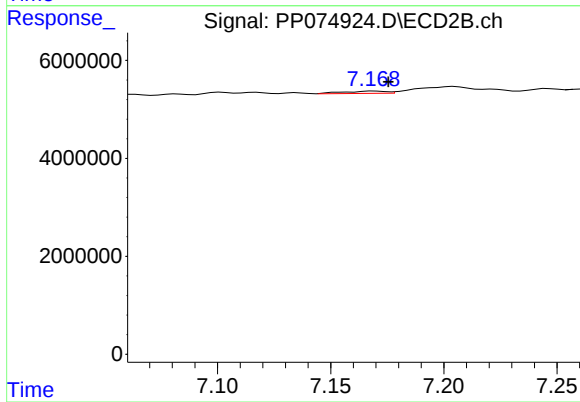


#37 AR-1262-2

R.T.: 7.169 min
Delta R.T.: -0.006 min
Response: 634358
Conc: 1.22 ng/ml

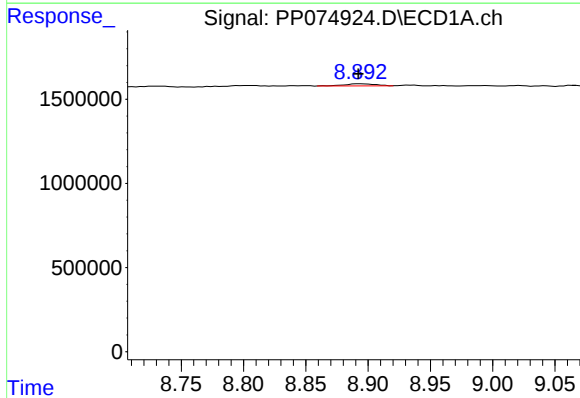


#38 AR-1262-3

R.T.: 8.893 min
Delta R.T.: 0.000 min
Response: 211880
Conc: 2.18 ng/ml

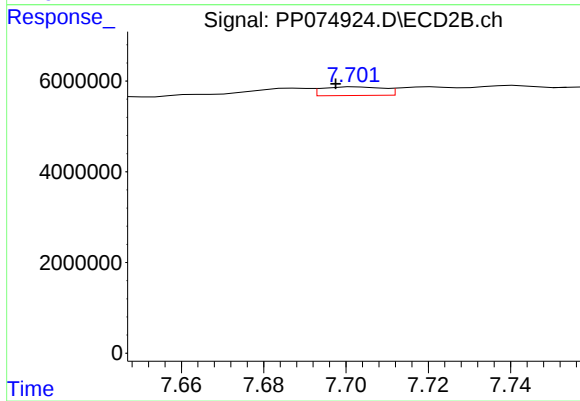

#38 AR-1262-3


R.T.: 7.703 min
Delta R.T.: 0.005 min
Response: 1972475
Conc: 4.23 ng/ml

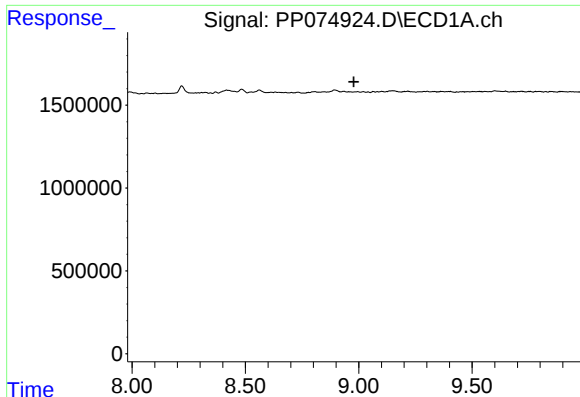

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 8.979 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

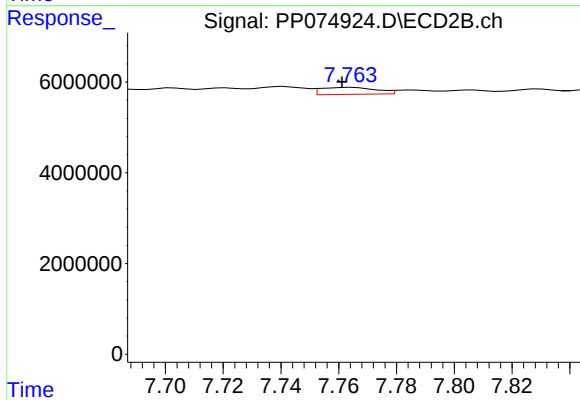


#39 AR-1262-4

R.T.: 7.765 min
Delta R.T.: 0.003 min
Response: 2049261
Conc: 2.49 ng/ml

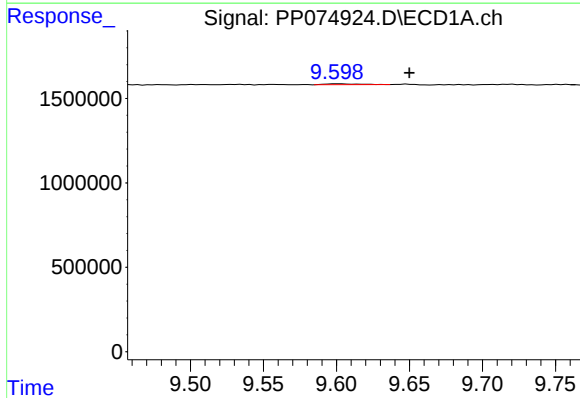


#40 AR-1262-5

R.T.: 9.600 min
Delta R.T.: -0.050 min
Response: 88804
Conc: 1.46 ng/ml

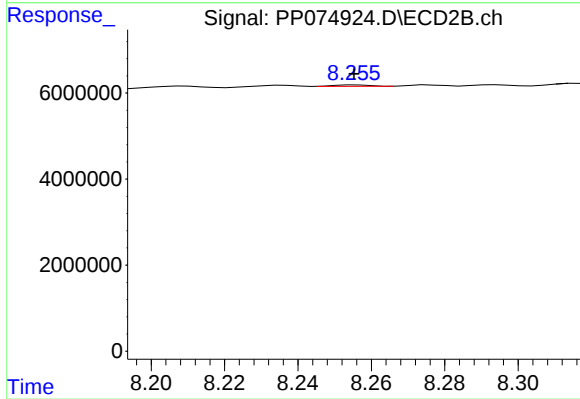

#40 AR-1262-5


R.T.: 8.256 min
Delta R.T.: 0.000 min
Response: 224750
Conc: 0.63 ng/ml

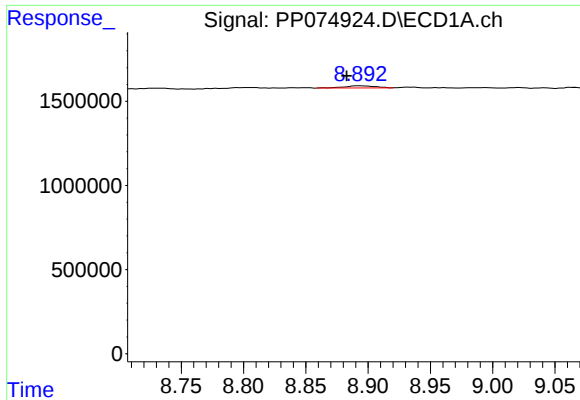

#41 AR-1268-1


R.T.: 8.893 min
Delta R.T.: 0.010 min
Response: 211880
Conc: 1.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

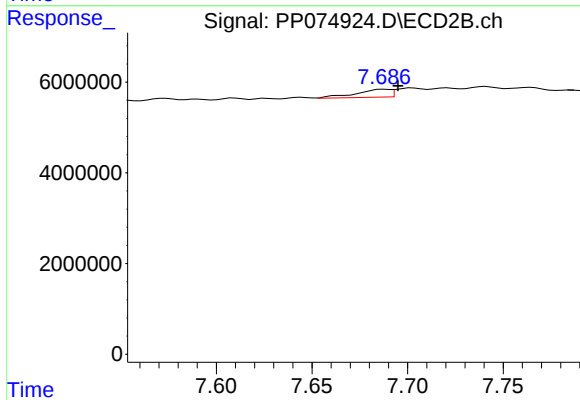


#41 AR-1268-1

R.T.: 7.688 min
Delta R.T.: -0.007 min
Response: 2138088
Conc: 1.52 ng/ml

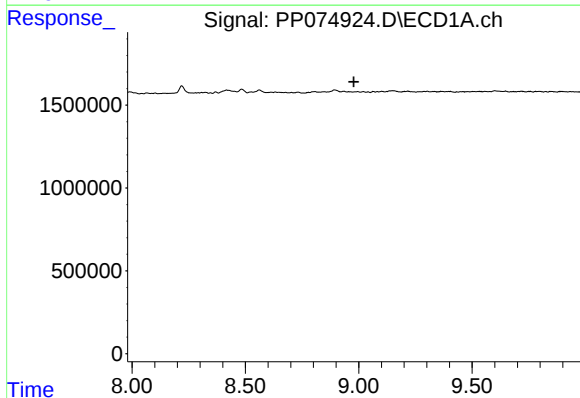


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 8.978 min
Response: 0
Conc: N.D.

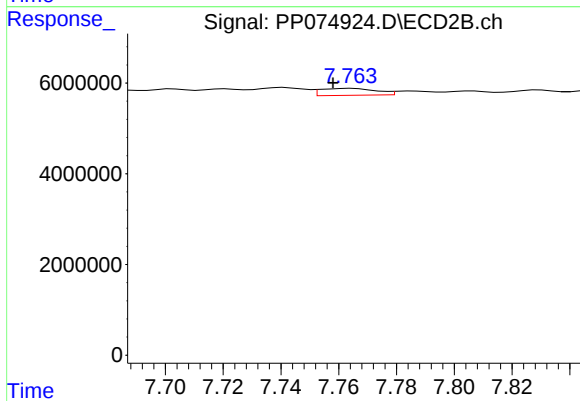

#42 AR-1268-2


R.T.: 7.765 min
Delta R.T.: 0.006 min
Response: 2049261
Conc: 1.50 ng/ml

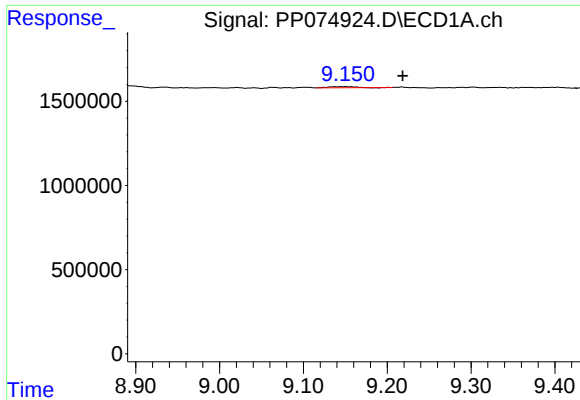

#43 AR-1268-3


R.T.: 9.151 min
Delta R.T.: -0.068 min
Response: 119305
Conc: 0.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

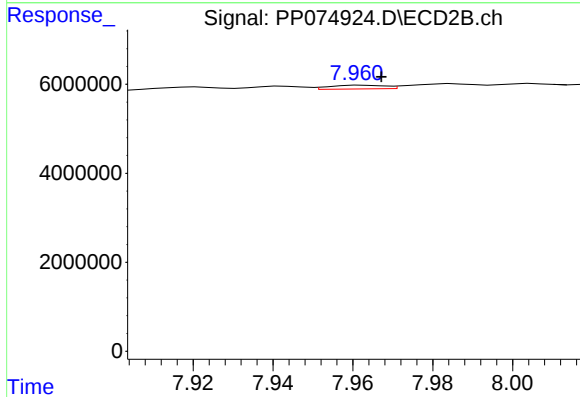


#43 AR-1268-3

R.T.: 7.963 min
Delta R.T.: -0.005 min
Response: 817302
Conc: 0.78 ng/ml

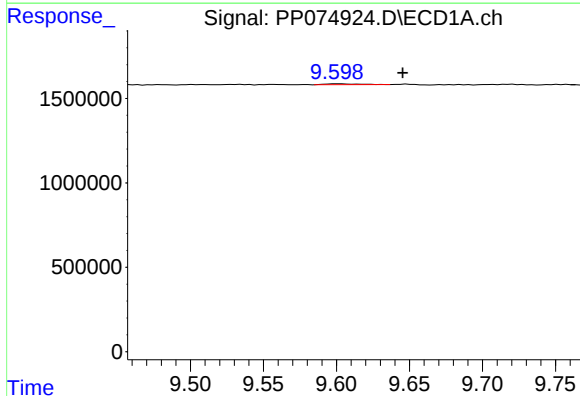


#44 AR-1268-4

R.T.: 9.600 min
Delta R.T.: -0.045 min
Response: 88804
Conc: 1.32 ng/ml

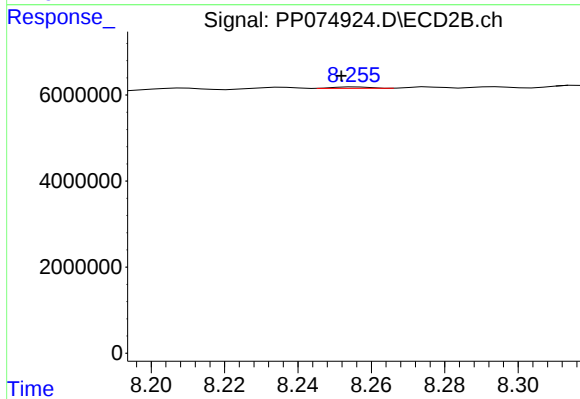

#44 AR-1268-4


R.T.: 8.256 min
Delta R.T.: 0.004 min
Response: 224750
Conc: 0.59 ng/ml

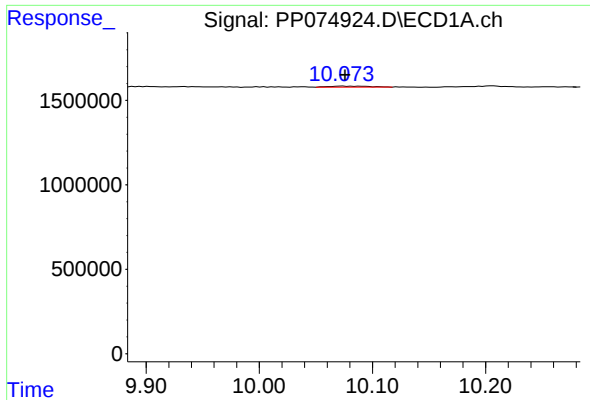

#45 AR-1268-5

R.T.: 10.074 min
Delta R.T.: -0.002 min
Response: 145793
Conc: 0.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

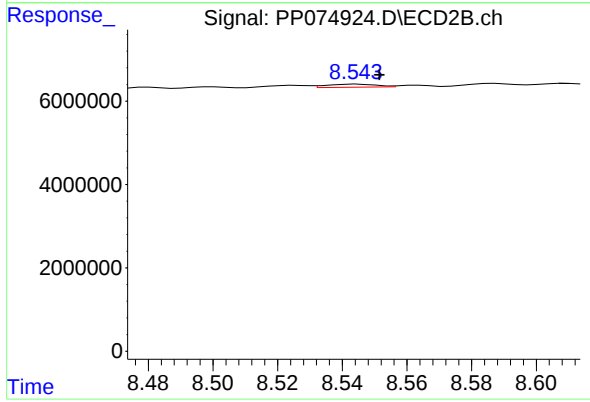

#45 AR-1268-5

R.T.: 8.545 min
Delta R.T.: -0.007 min
Response: 801654
Conc: 0.26 ng/ml