

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090623\
 Data File : PP059787.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Sep 2023 20:14
 Operator : YP\AJ
 Sample : 04297-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1683

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/07/2023
 Supervised By :Ankita Jodhani 09/07/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 07 00:26:06 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090623.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Sep 06 14:24:13 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.387	3.617	17804588	29276899	12.078m	14.822
2) SA Decachlor...	10.161	8.633	13141920	12194872	12.801	8.933 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090623\
Data File : PP059787.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Sep 2023 20:14
Operator : YP\AJ
Sample : 04297-02
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1683


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/07/2023
Supervised By :Ankita Jodhani 09/07/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 07 00:26:06 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090623.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Sep 06 14:24:13 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

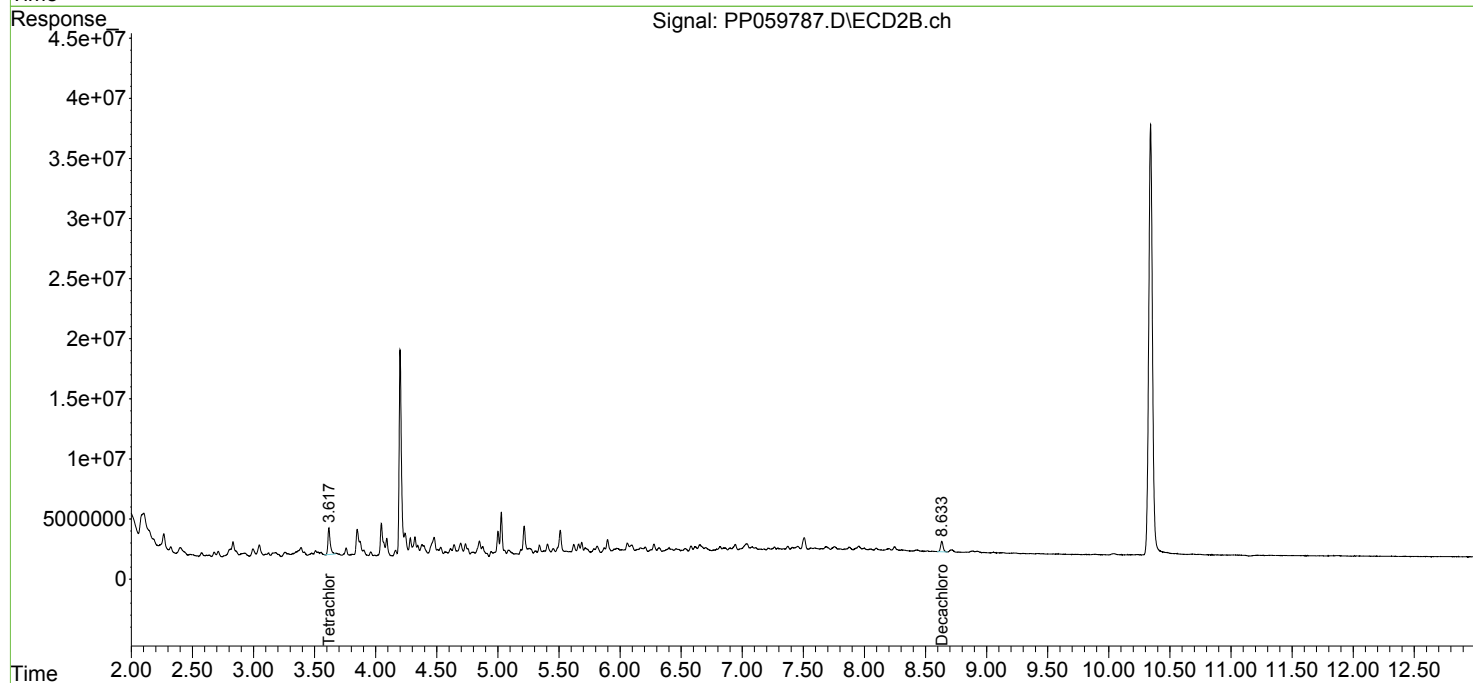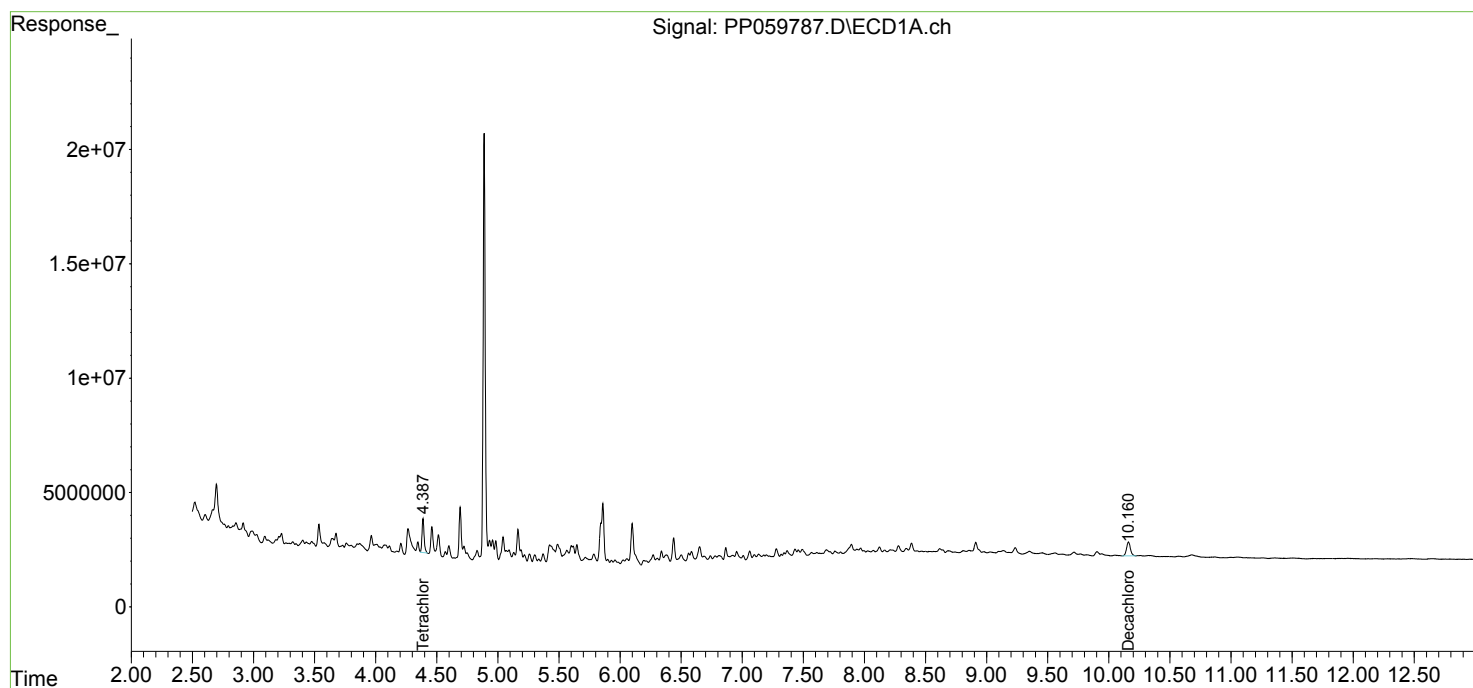

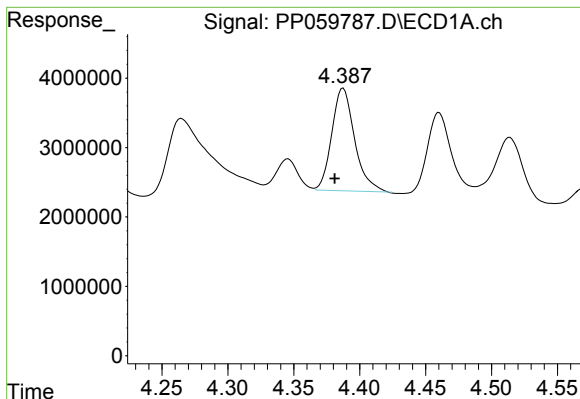

#1 Tetrachloro-m-xylene

R.T.: 4.387 min
Delta R.T.: 0.006 min
Response: 17804588
Conc: 12.08 ng/ml


Instrument :

ECD_P

ClientSampleId :
1683


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/07/2023
Supervised By :Ankita Jodhani 09/07/2023

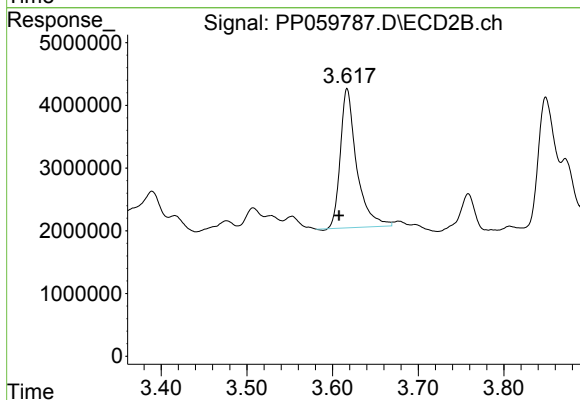


#1 Tetrachloro-m-xylene

R.T.: 3.617 min
Delta R.T.: 0.010 min
Response: 29276899
Conc: 14.82 ng/ml

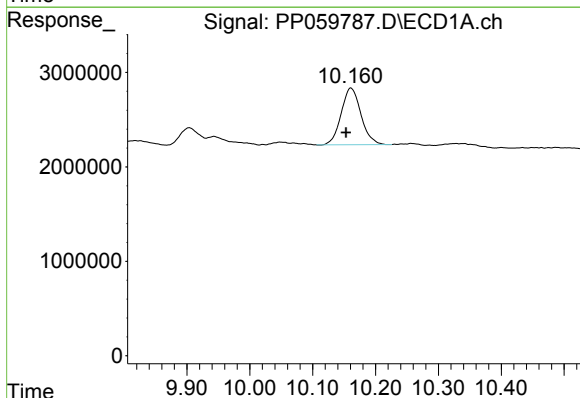

#2 Decachlorobiphenyl

R.T.: 10.161 min
Delta R.T.: 0.008 min
Response: 13141920
Conc: 12.80 ng/ml

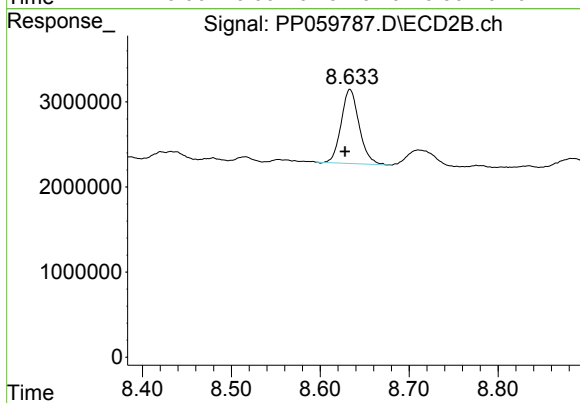

#2 Decachlorobiphenyl

R.T.: 8.633 min
Delta R.T.: 0.006 min
Response: 12194872
Conc: 8.93 ng/ml