

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
 Data File : PP039190.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2021 15:50
 Operator : AJ\MA
 Sample : PB138941BL
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 08:49:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.871	3.856	911520	552216	23.793	23.022
2)	SA Decachlor...	10.838	9.108	886078	566514	26.919	25.886
Target Compounds							
9)	L2 AR-1221-2	5.222	0.000	10967	0	29.532	N.D. #
20)	L4 AR-1242-5	7.191f	0.000	12962	0	15.885	N.D. #
25)	L5 AR-1248-5	7.191f	0.000	12962	0	9.236	N.D. #
28)	L6 AR-1254-3	7.736f	0.000	64256	0	26.254	N.D. #
32)	L7 AR-1260-2	8.120f	0.000	23365	0	11.762	N.D. #
34)	L7 AR-1260-4	8.745	0.000	16028	0	9.944	N.D. #
35)	L7 AR-1260-5	9.055	0.000	96202	0	34.729	N.D. #
37)	L8 AR-1262-2	9.055	0.000	96202	0	25.982	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
Data File : PP039190.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2021 15:50
Operator : AJ\MA
Sample : PB138941BL
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 08:49:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

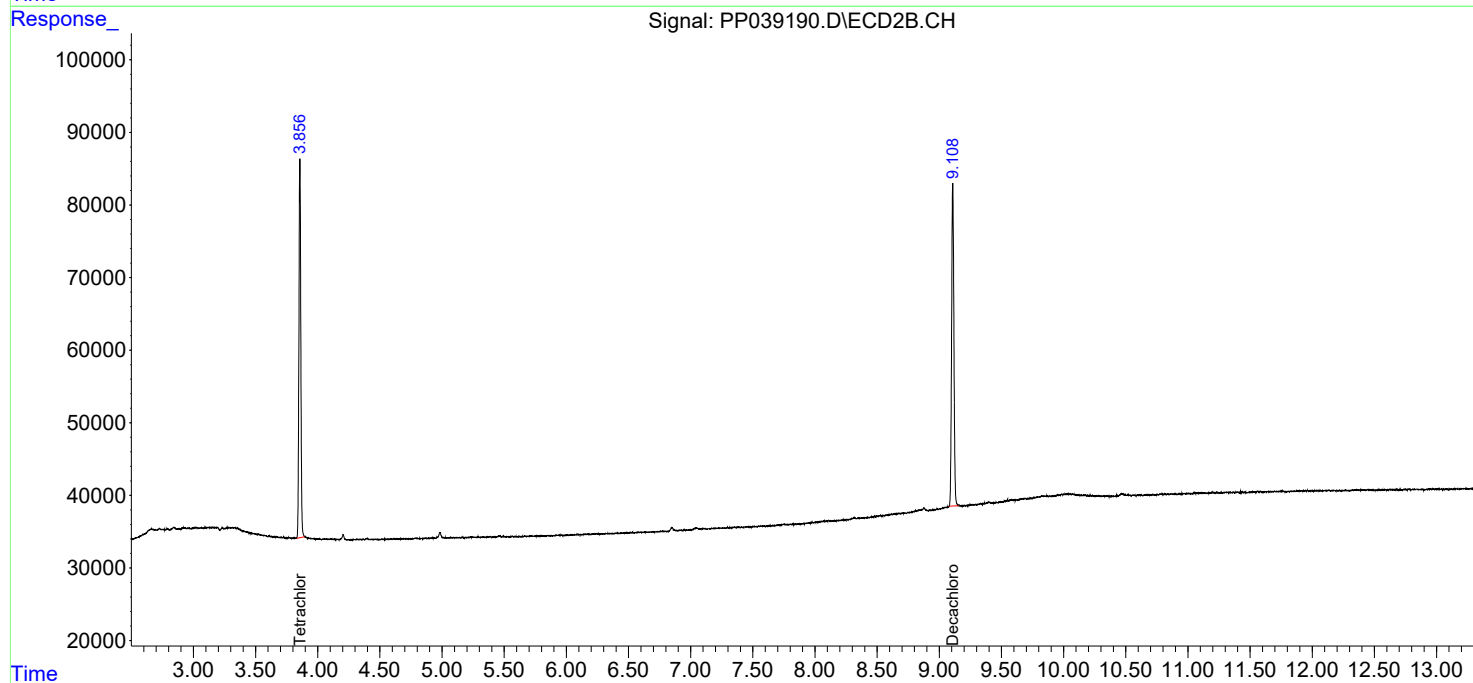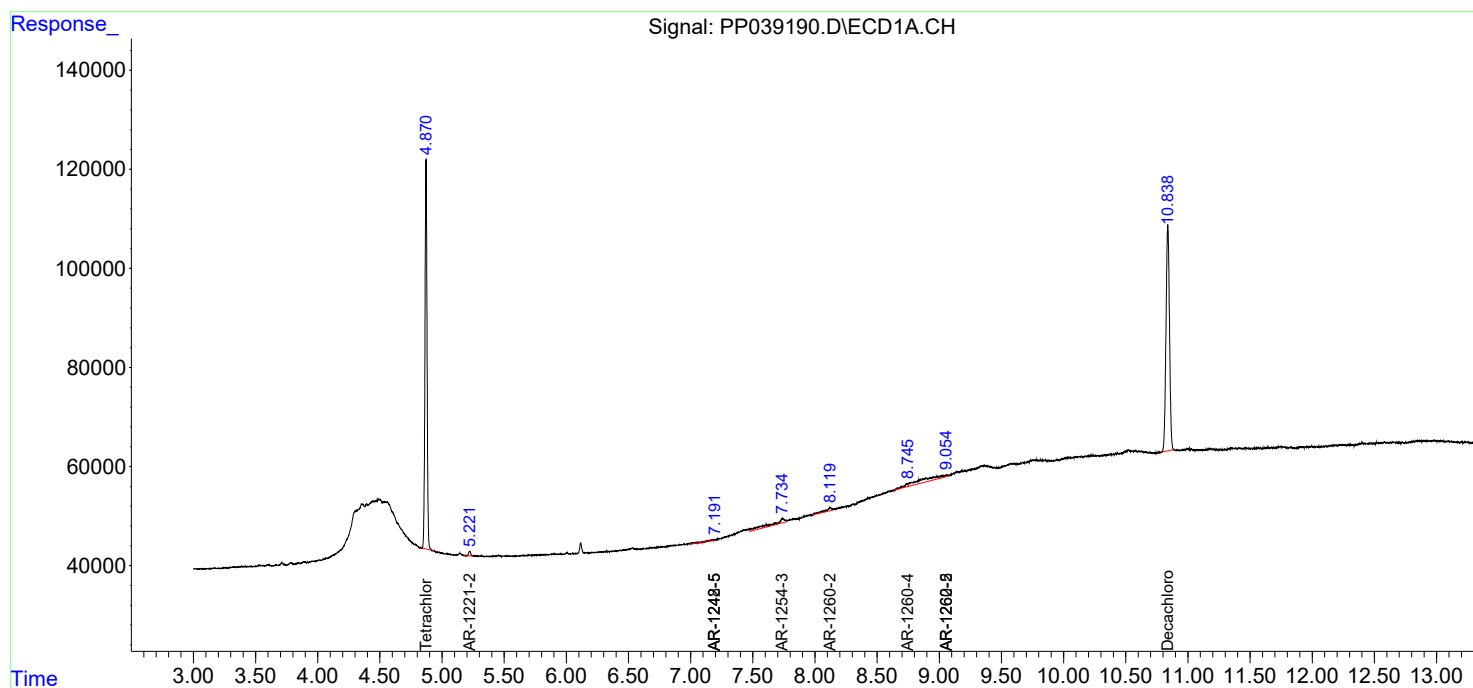


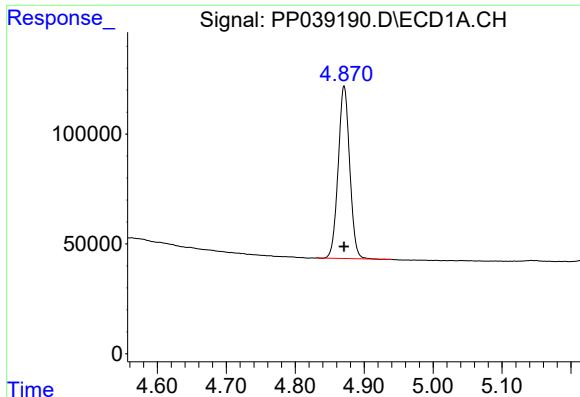

#1 Tetrachloro-m-xylene


R.T.: 4.871 min
Delta R.T.: 0.000 min
Response: 911520
Conc: 23.79 ng/ml

Instrument :
ECD_P
ClientSampleId :

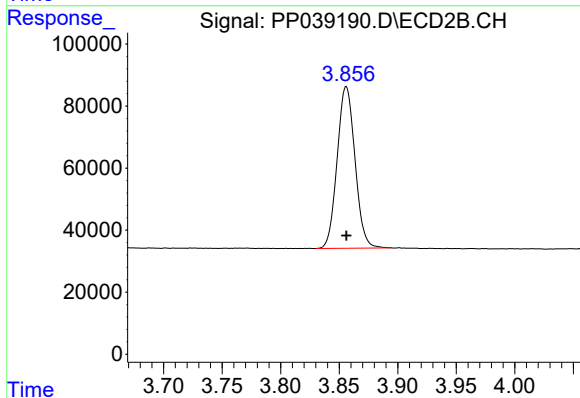


#1 Tetrachloro-m-xylene

R.T.: 3.856 min
Delta R.T.: 0.000 min
Response: 552216
Conc: 23.02 ng/ml

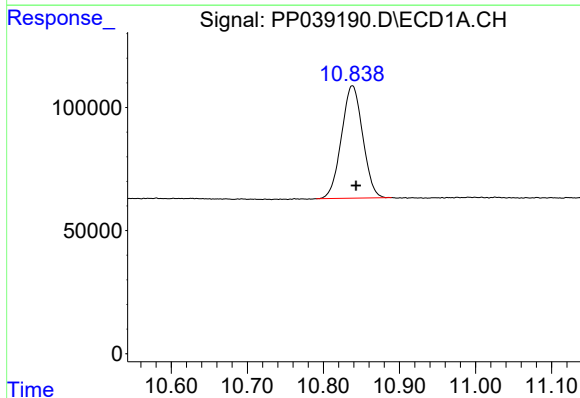


#2 Decachlorobiphenyl

R.T.: 10.838 min
Delta R.T.: -0.005 min
Response: 886078
Conc: 26.92 ng/ml

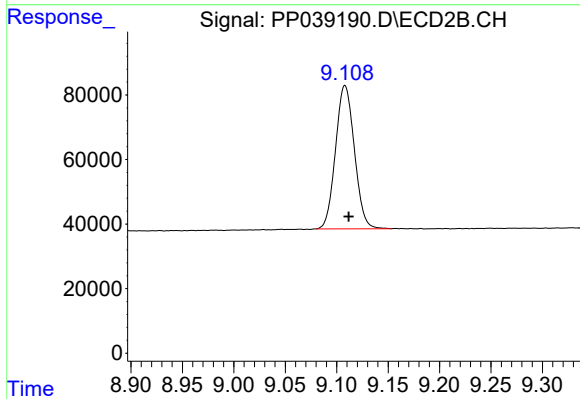

#2 Decachlorobiphenyl


R.T.: 9.108 min
Delta R.T.: -0.004 min
Response: 566514
Conc: 25.89 ng/ml

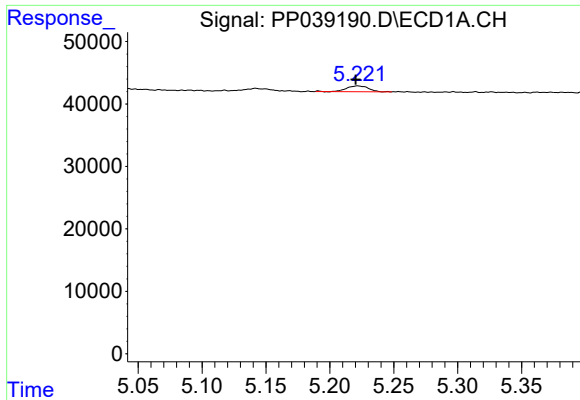

#9 AR-1221-2


R.T.: 5.222 min
Delta R.T.: 0.002 min
Response: 10967
Conc: 29.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

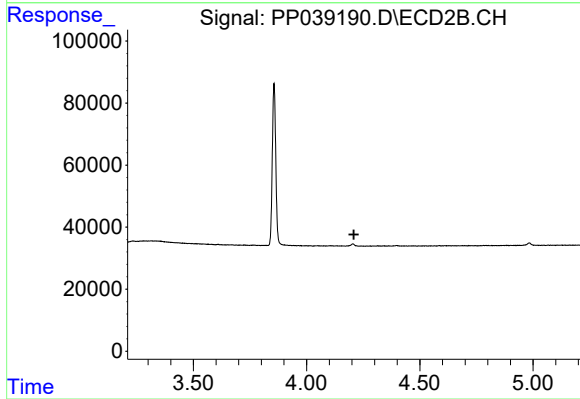


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

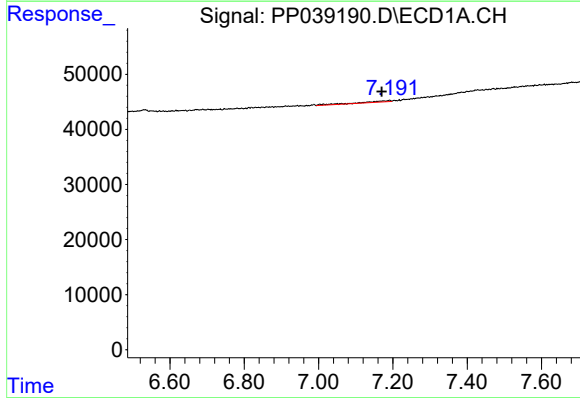


#20 AR-1242-5

R.T.: 7.191 min
Delta R.T.: 0.021 min
Response: 12962
Conc: 15.88 ng/ml

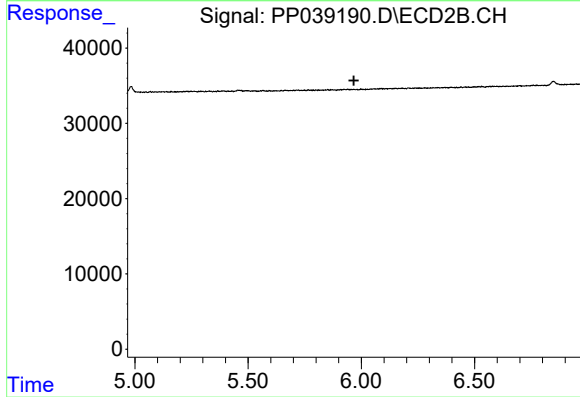

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.967 min
Response: 0
Conc: N.D.

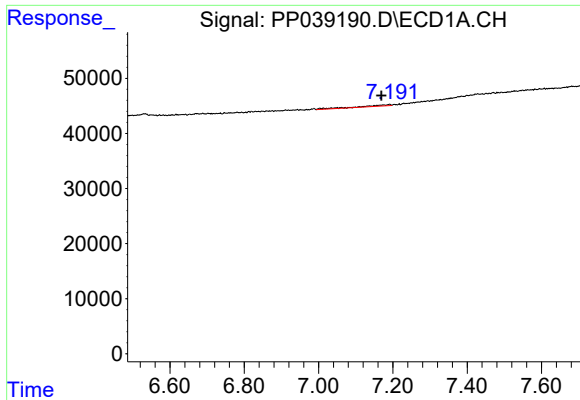

#25 AR-1248-5


R.T.: 7.191 min
Delta R.T.: 0.022 min
Response: 12962
Conc: 9.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

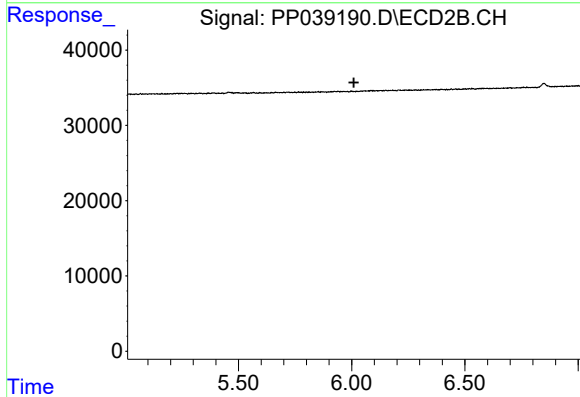


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 6.010 min
Response: 0
Conc: N.D.

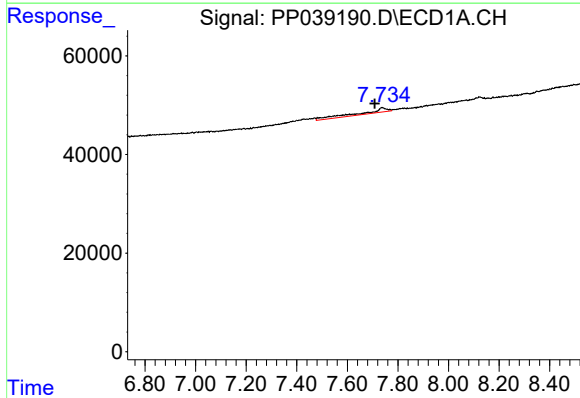


#28 AR-1254-3

R.T.: 7.736 min
Delta R.T.: 0.027 min
Response: 64256
Conc: 26.25 ng/ml

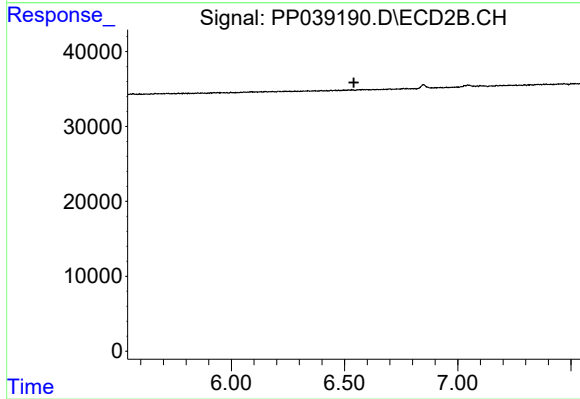

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

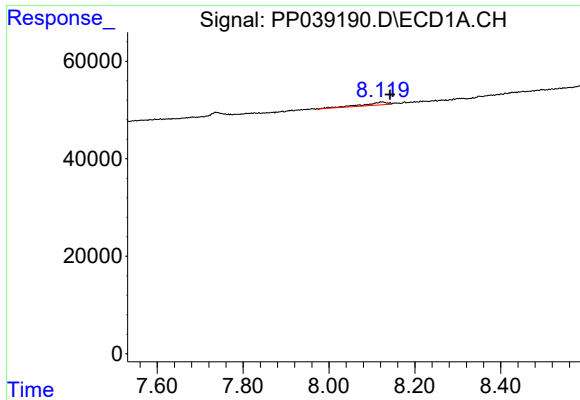

#32 AR-1260-2


R.T.: 8.120 min
Delta R.T.: -0.022 min
Response: 23365
Conc: 11.76 ng/ml

Instrument :
ECD_P
ClientSampleId :

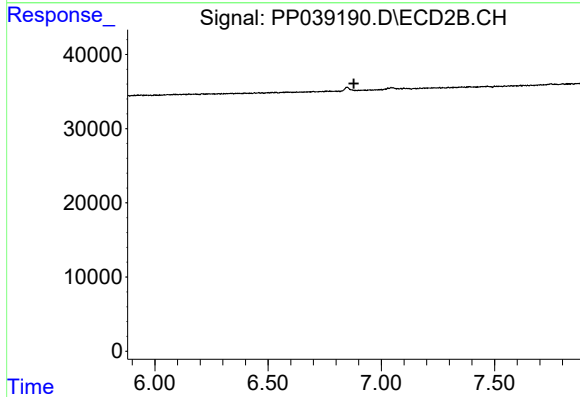


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 6.879 min
Response: 0
Conc: N.D.

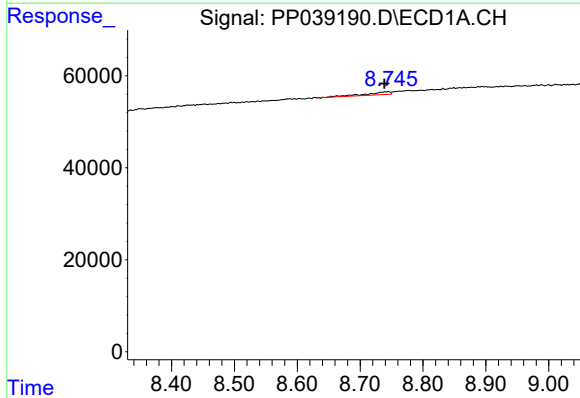


#34 AR-1260-4

R.T.: 8.745 min
Delta R.T.: 0.007 min
Response: 16028
Conc: 9.94 ng/ml

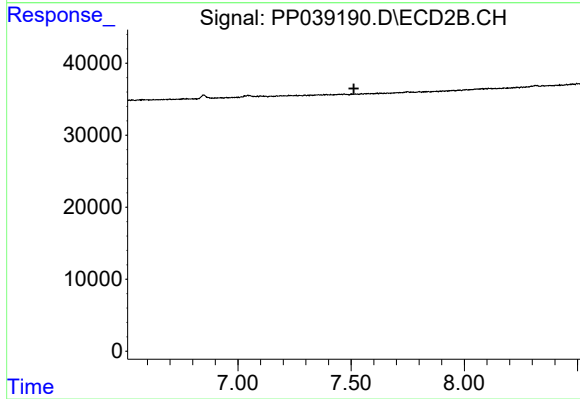

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T. : 7.512 min
Response: 0
Conc: N.D.

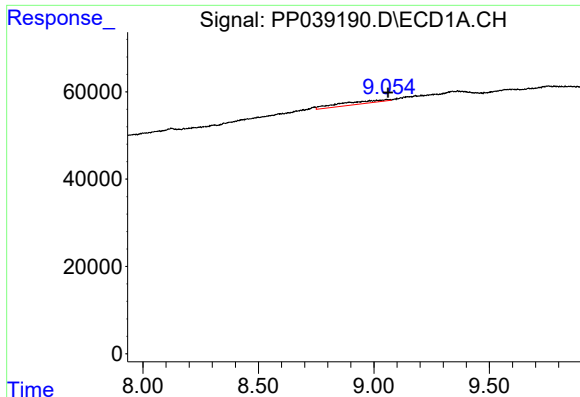

#35 AR-1260-5


R.T.: 9.055 min
Delta R.T.: -0.006 min
Response: 96202
Conc: 34.73 ng/ml

Instrument :
ECD_P
ClientSampleId :

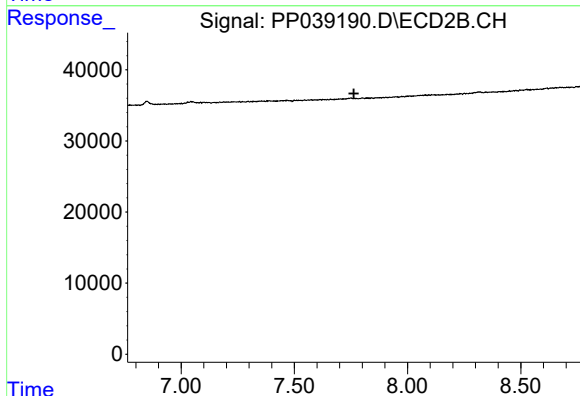


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T. : 7.763 min
Response: 0
Conc: N.D.

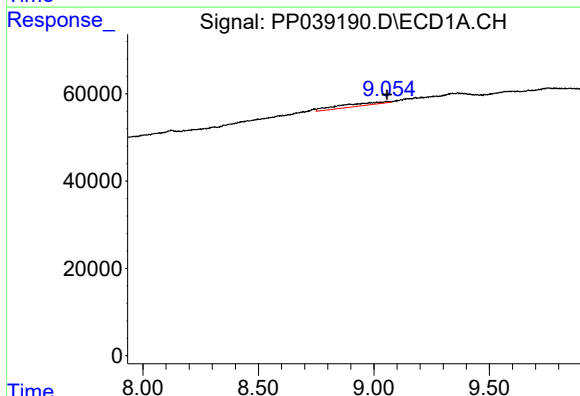

#37 AR-1262-2

R.T.: 9.055 min
Delta R.T.: -0.002 min
Response: 96202
Conc: 25.98 ng/ml

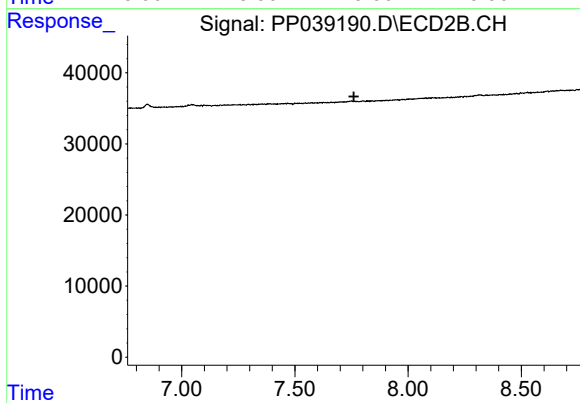

#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 7.760 min
Response: 0
Conc: N.D.