

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
 Data File : PP039214.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2021 23:09
 Operator : AJ\MA
 Sample : M3644-04
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 09:08:25 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.869	3.855	939359	546707	24.519	22.793
2)	SA Decachlor...	10.835	9.105	890584	559245	27.056	25.554
Target Compounds							
8)	L2 AR-1221-1	5.140f	0.000	17127	0	35.493	N.D. #
9)	L2 AR-1221-2	5.219	0.000	13615	0	36.662	N.D. #
15)	L3 AR-1232-5	6.479	0.000	7459	0	22.530	N.D. #
22)	L5 AR-1248-2	6.479	0.000	7459	0	6.991	N.D. #
30)	L6 AR-1254-5	8.446	0.000	883	0	0.443	N.D. #
32)	L7 AR-1260-2	8.134	0.000	2417	0	1.217	N.D. #
34)	L7 AR-1260-4	8.734	0.000	385	0	0.239	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
Data File : PP039214.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2021 23:09
Operator : AJ\MA
Sample : M3644-04
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 09:08:25 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

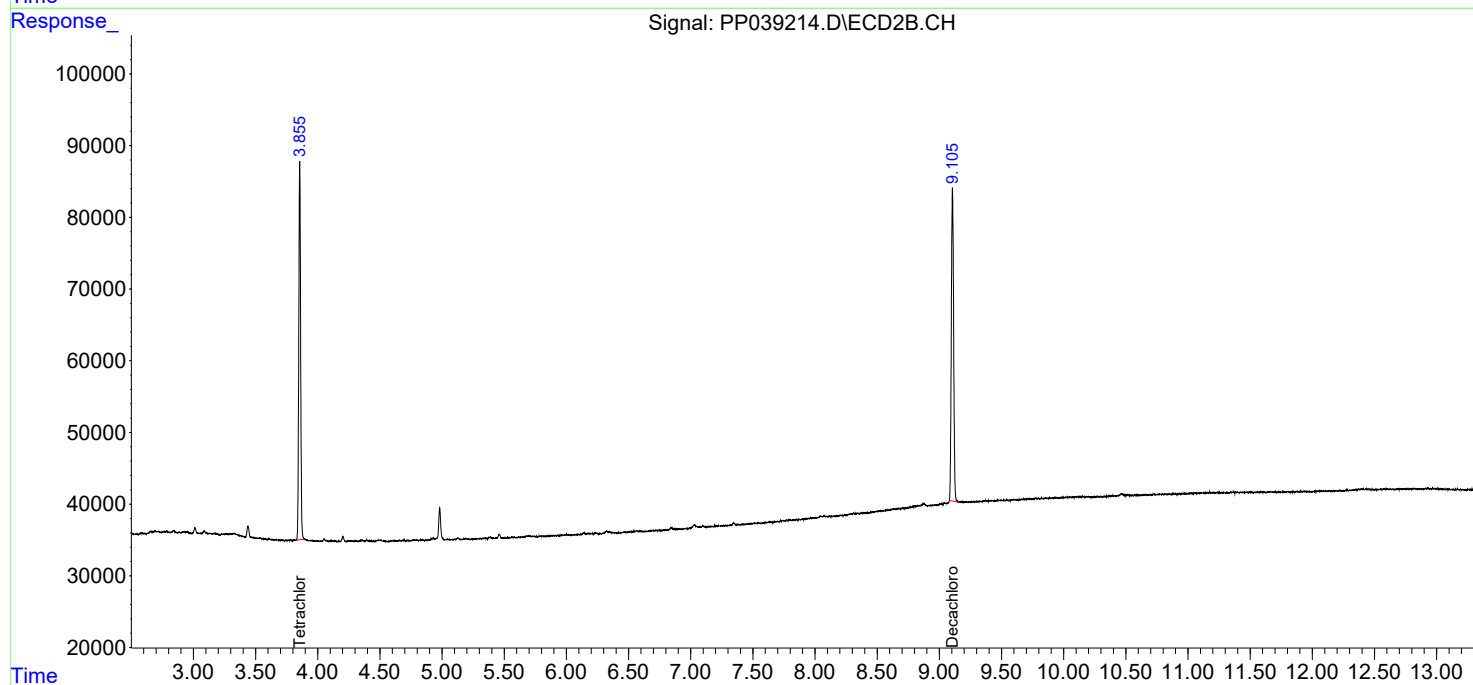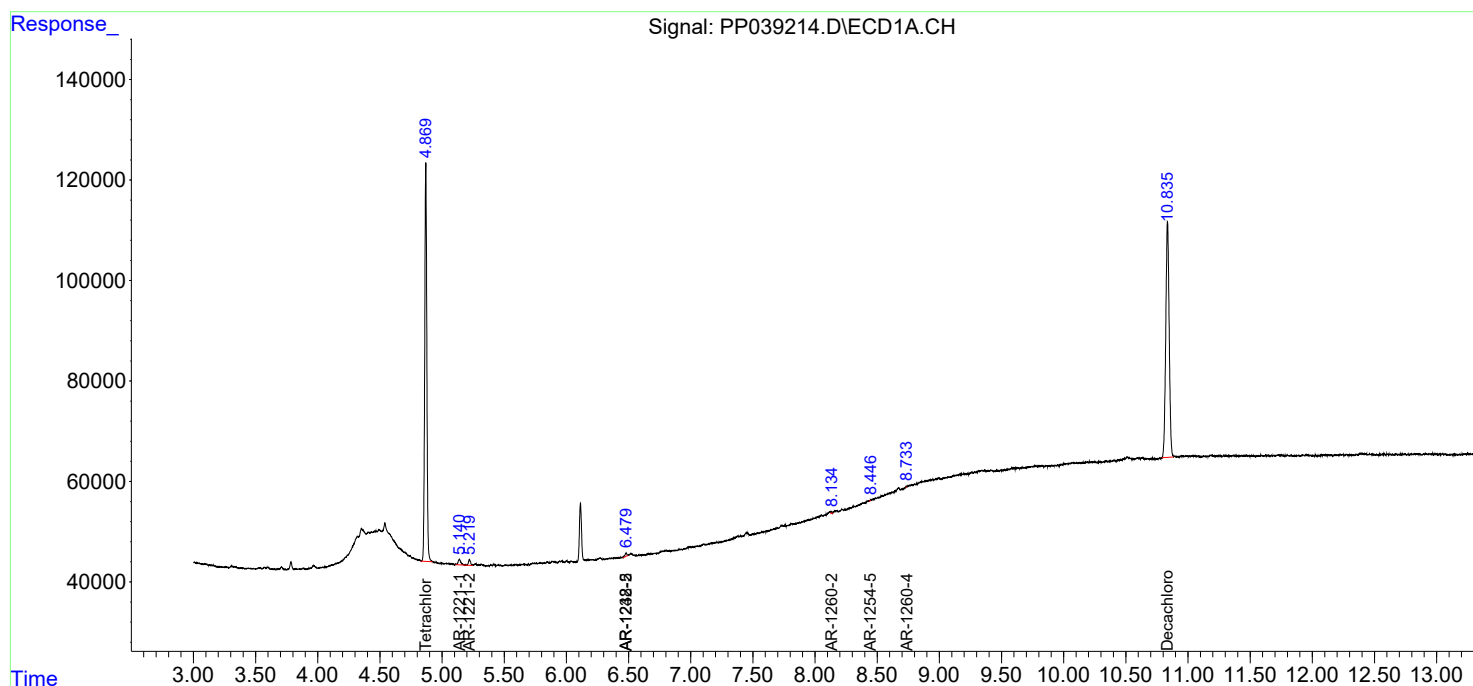


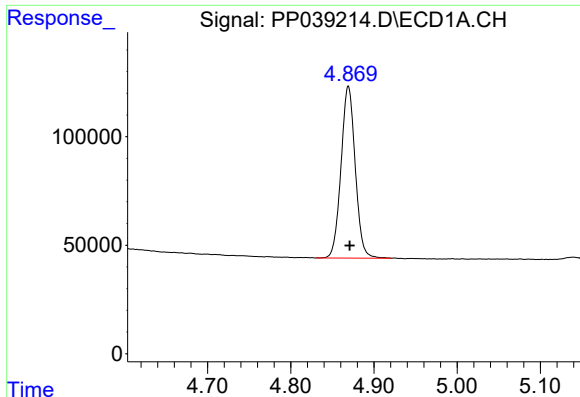

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 939359
Conc: 24.52 ng/ml

Instrument :
ECD_P
ClientSampleId :

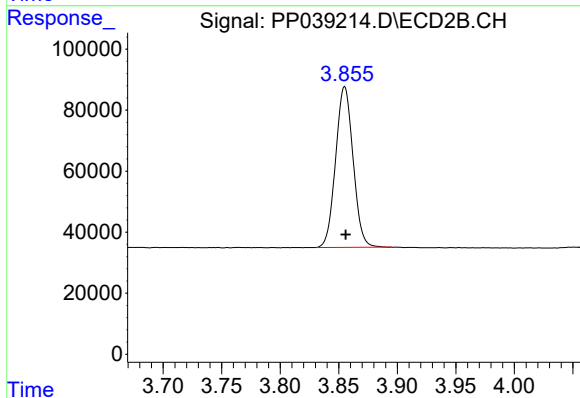


#1 Tetrachloro-m-xylene

R.T.: 3.855 min
Delta R.T.: 0.000 min
Response: 546707
Conc: 22.79 ng/ml

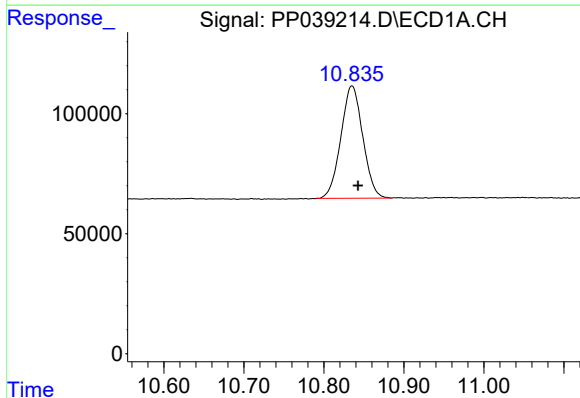


#2 Decachlorobiphenyl

R.T.: 10.835 min
Delta R.T.: -0.008 min
Response: 890584
Conc: 27.06 ng/ml

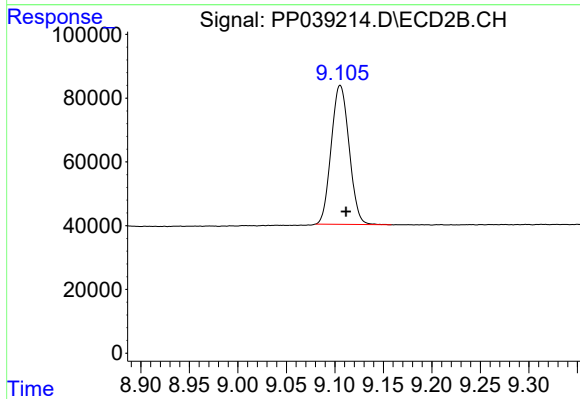

#2 Decachlorobiphenyl


R.T.: 9.105 min
Delta R.T.: -0.006 min
Response: 559245
Conc: 25.55 ng/ml

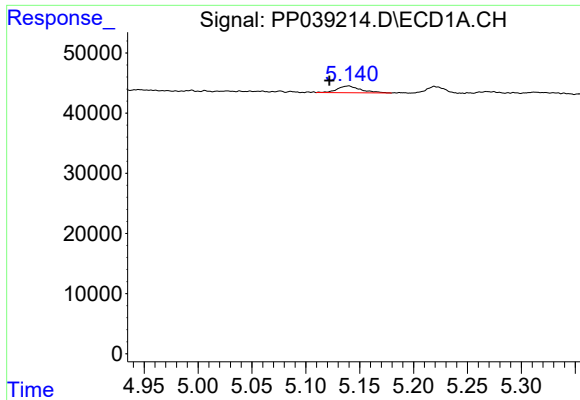

#8 AR-1221-1


R.T.: 5.140 min
Delta R.T.: 0.018 min
Response: 17127
Conc: 35.49 ng/ml

Instrument :
ECD_P
ClientSampleId :

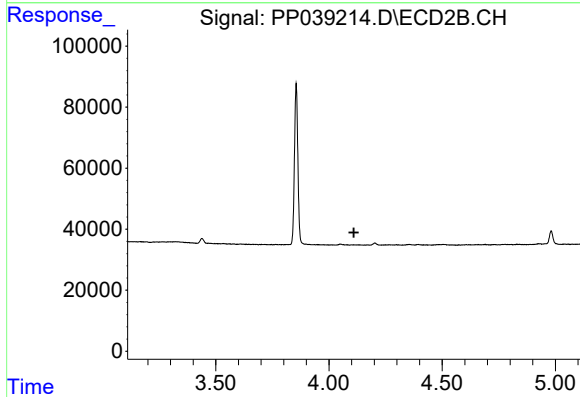


#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.110 min
Response: 0
Conc: N.D.

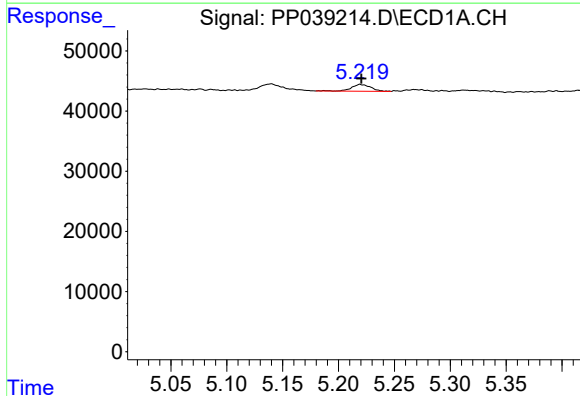


#9 AR-1221-2

R.T.: 5.219 min
Delta R.T.: -0.001 min
Response: 13615
Conc: 36.66 ng/ml

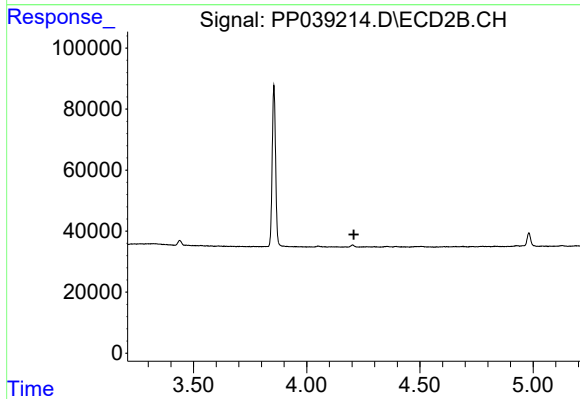

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

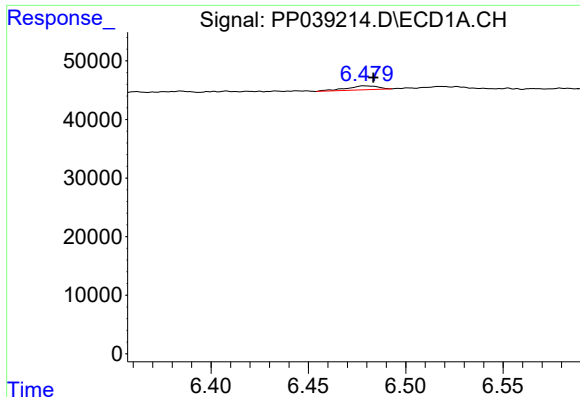

#15 AR-1232-5


R.T.: 6.479 min
Delta R.T.: -0.005 min
Response: 7459
Conc: 22.53 ng/ml

Instrument :
ECD_P
ClientSampleId :

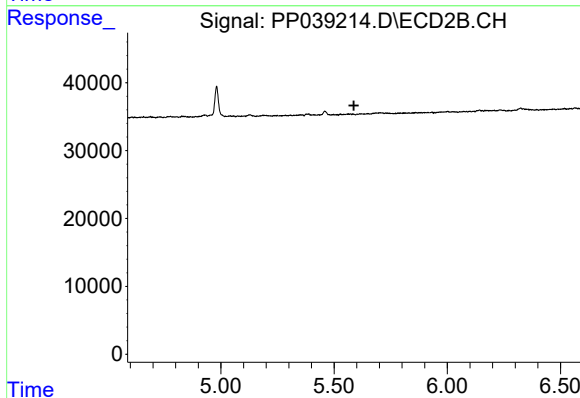


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 5.588 min
Response: 0
Conc: N.D.

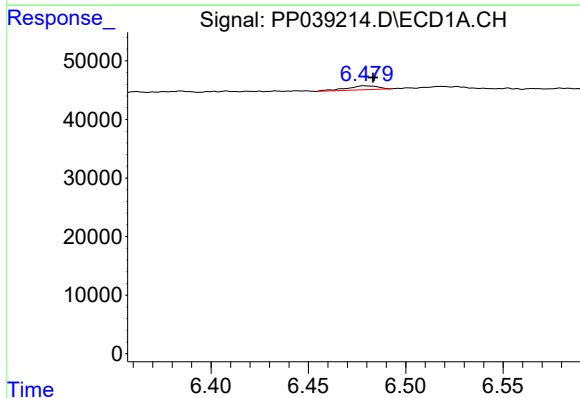


#22 AR-1248-2

R.T.: 6.479 min
Delta R.T.: -0.004 min
Response: 7459
Conc: 6.99 ng/ml

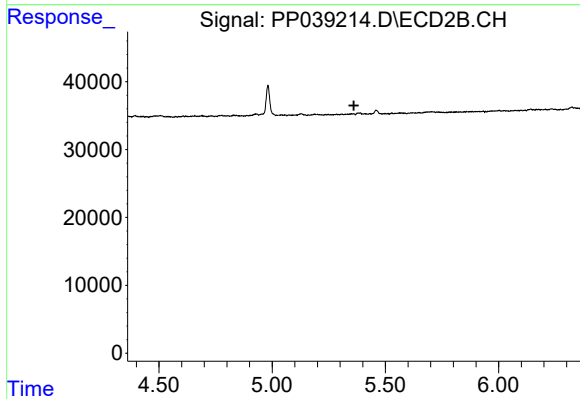

#22 AR-1248-2


R.T.: 0.000 min
Exp R.T. : 5.361 min
Response: 0
Conc: N.D.

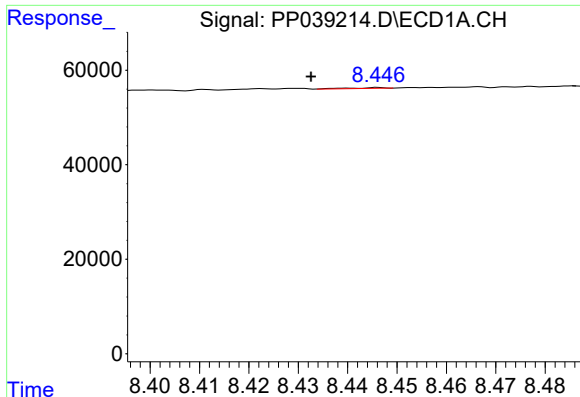

#30 AR-1254-5


R.T.: 8.446 min
Delta R.T.: 0.014 min
Response: 883
Conc: 0.44 ng/ml

Instrument :
ECD_P
ClientSampleId :

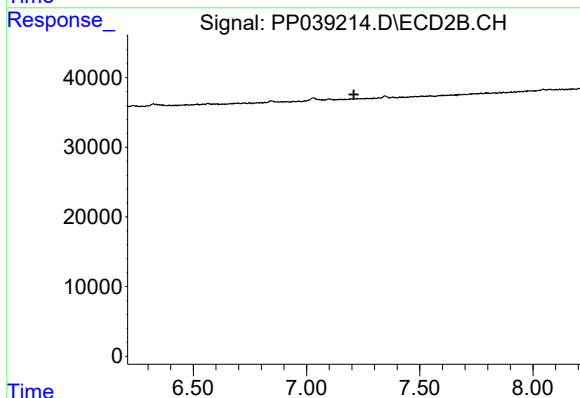


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 7.209 min
Response: 0
Conc: N.D.

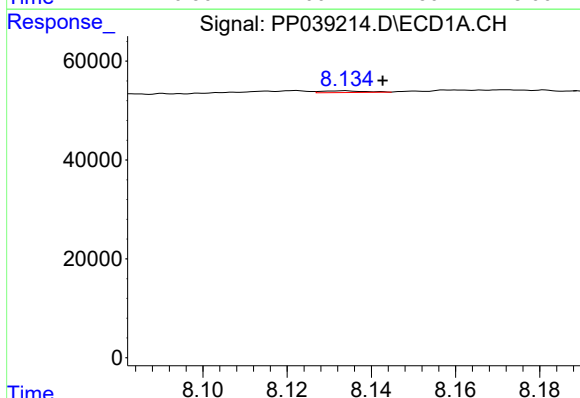


#32 AR-1260-2

R.T.: 8.134 min
Delta R.T.: -0.009 min
Response: 2417
Conc: 1.22 ng/ml

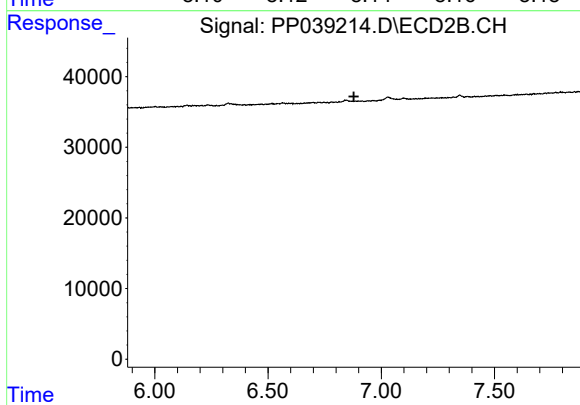

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 6.879 min
Response: 0
Conc: N.D.

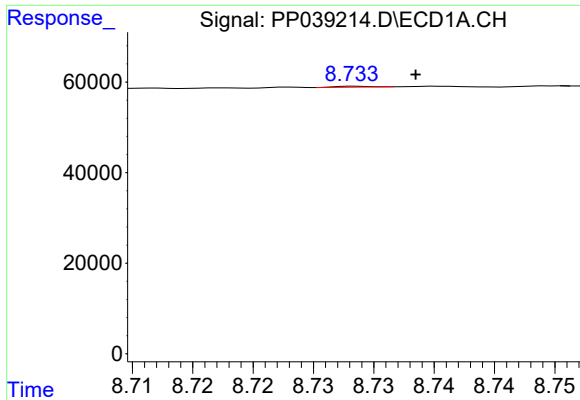

#34 AR-1260-4

R.T.: 8.734 min
Delta R.T.: -0.005 min
Response: 385
Conc: 0.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

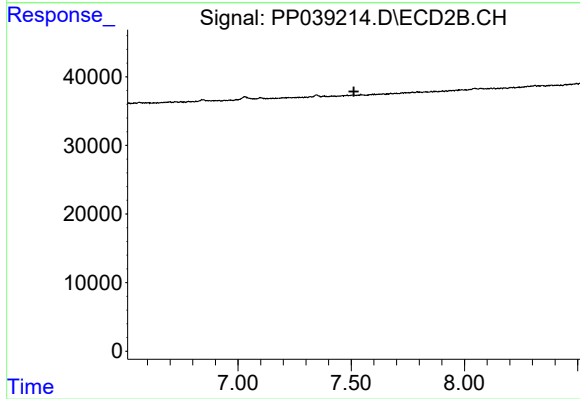

#34 AR-1260-4

R.T.: 0.000 min
Exp R.T. : 7.512 min
Response: 0
Conc: N.D.