

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
 Data File : PP039234.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Sep 2021 6:10
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 09:15:45 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.869	3.854	1003317	579310	26.189	24.152
2)	SA Decachlor...	10.835	9.105	955539	598027	29.029	27.326
Target Compounds							
9)	L2 AR-1221-2	5.218	0.000	12266	0	33.031	N.D. #
20)	L4 AR-1242-5	7.154f	0.000	5429	0	6.653	N.D. #
24)	L5 AR-1248-4	7.119	0.000	4477	0	3.334	N.D. #
25)	L5 AR-1248-5	7.154f	0.000	5429	0	3.868	N.D. #
26)	L6 AR-1254-1	7.088	0.000	14370	0	9.424	N.D. #
28)	L6 AR-1254-3	7.733f	0.000	31274	0	12.778	N.D. #
36)	L8 AR-1262-1	8.475f	0.000	3225	0	1.448	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
Data File : PP039234.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2021 6:10
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 09:15:45 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

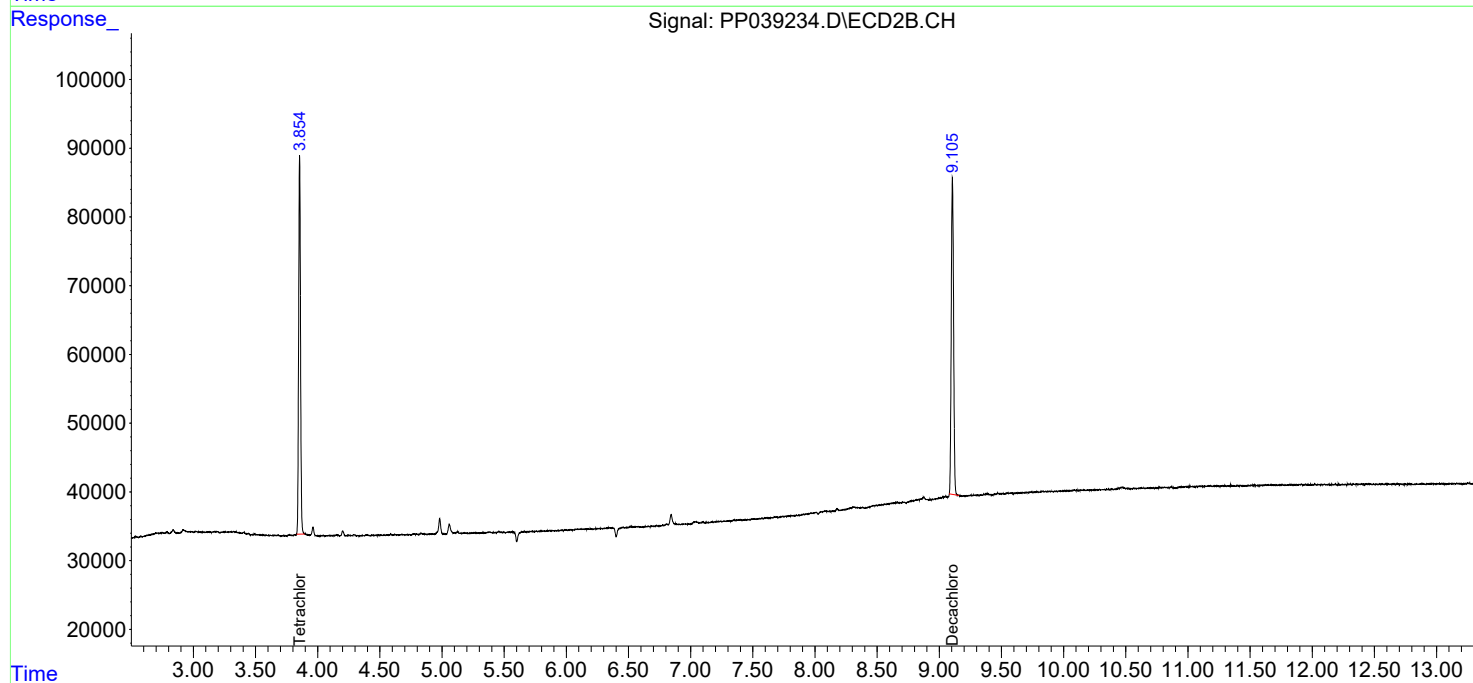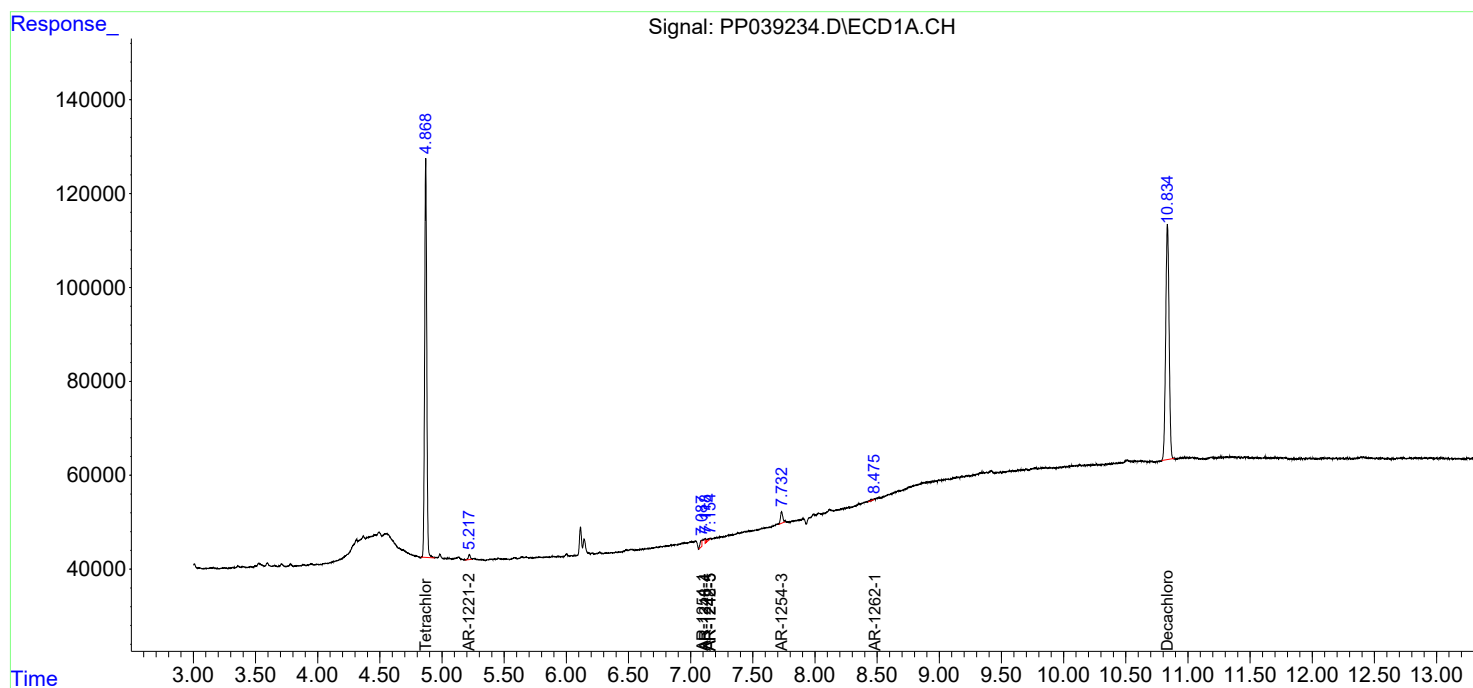


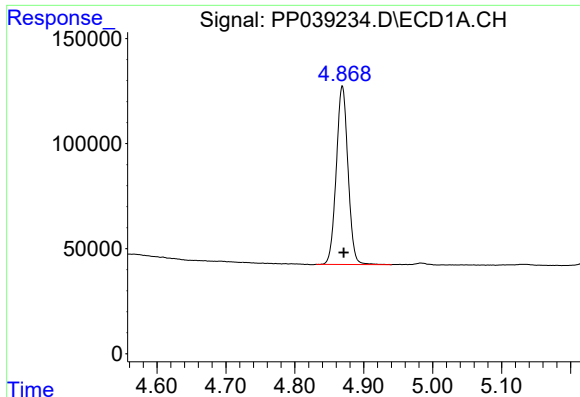

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 1003317
Conc: 26.19 ng/ml

Instrument :
ECD_P
ClientSampleId :

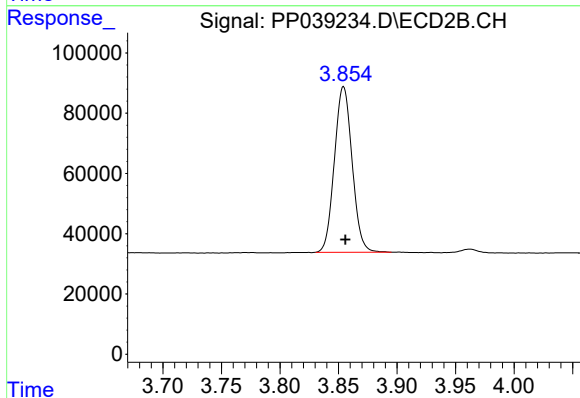


#1 Tetrachloro-m-xylene

R.T.: 3.854 min
Delta R.T.: -0.002 min
Response: 579310
Conc: 24.15 ng/ml

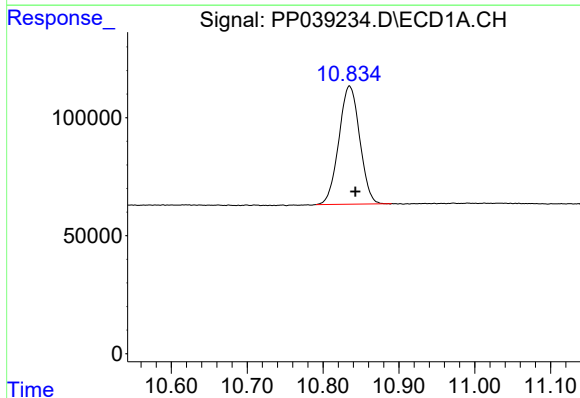


#2 Decachlorobiphenyl

R.T.: 10.835 min
Delta R.T.: -0.008 min
Response: 955539
Conc: 29.03 ng/ml

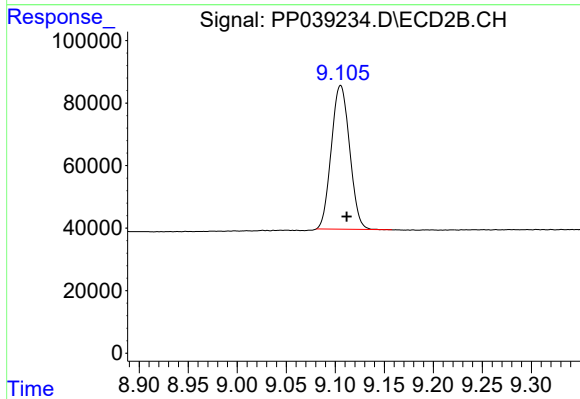

#2 Decachlorobiphenyl


R.T.: 9.105 min
Delta R.T.: -0.006 min
Response: 598027
Conc: 27.33 ng/ml

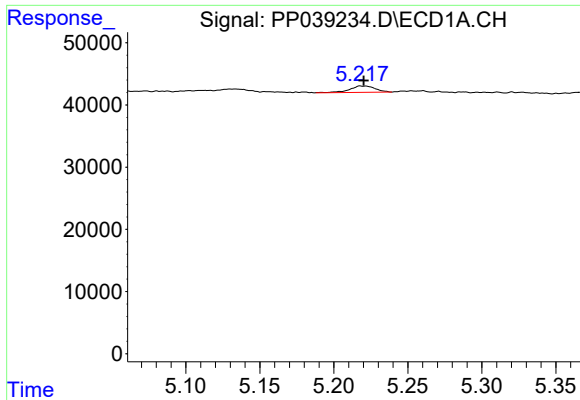

#9 AR-1221-2


R.T.: 5.218 min
Delta R.T.: -0.002 min
Response: 12266
Conc: 33.03 ng/ml

Instrument :
ECD_P
ClientSampleId :

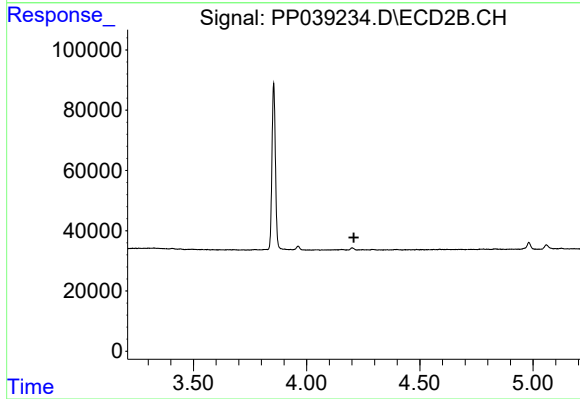


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.209 min
Response: 0
Conc: N.D.

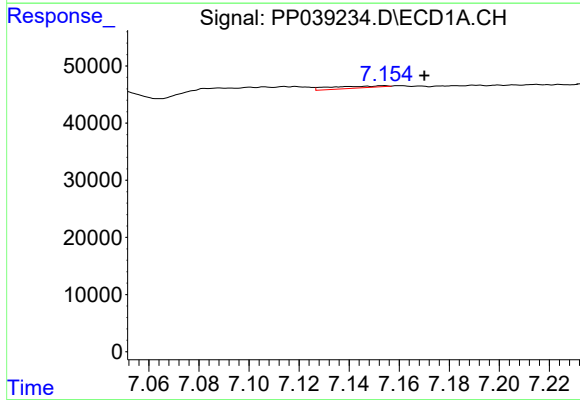


#20 AR-1242-5

R.T.: 7.154 min
Delta R.T.: -0.016 min
Response: 5429
Conc: 6.65 ng/ml

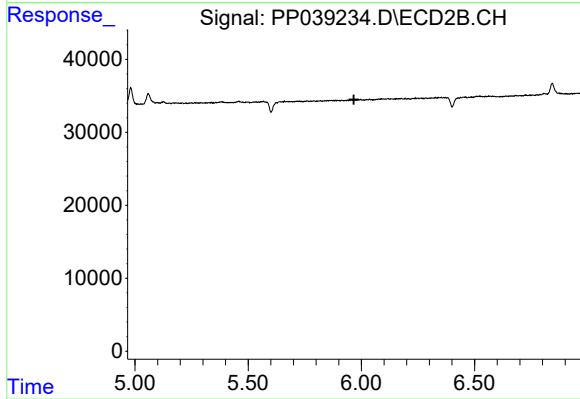

#20 AR-1242-5


R.T.: 0.000 min
Exp R.T. : 5.967 min
Response: 0
Conc: N.D.

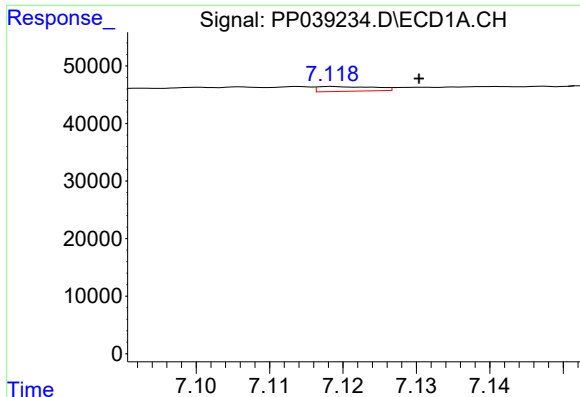

#24 AR-1248-4


R.T.: 7.119 min
Delta R.T.: -0.012 min
Response: 4477
Conc: 3.33 ng/ml

Instrument :
ECD_P
ClientSampleId :

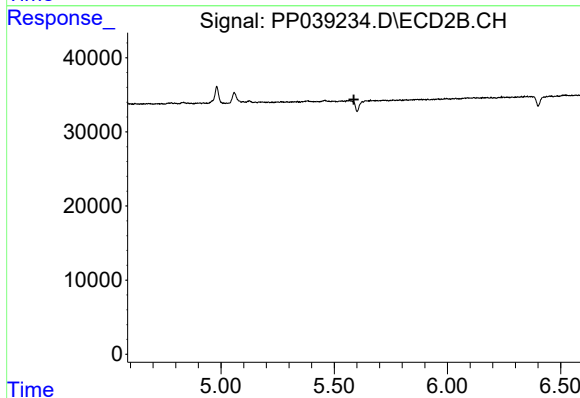


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.587 min
Response: 0
Conc: N.D.

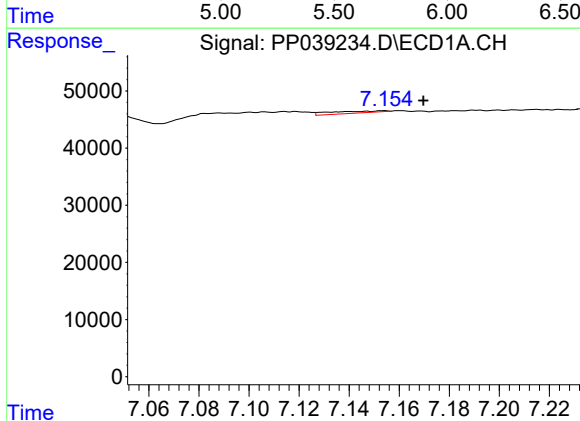


#25 AR-1248-5

R.T.: 7.154 min
Delta R.T.: -0.016 min
Response: 5429
Conc: 3.87 ng/ml

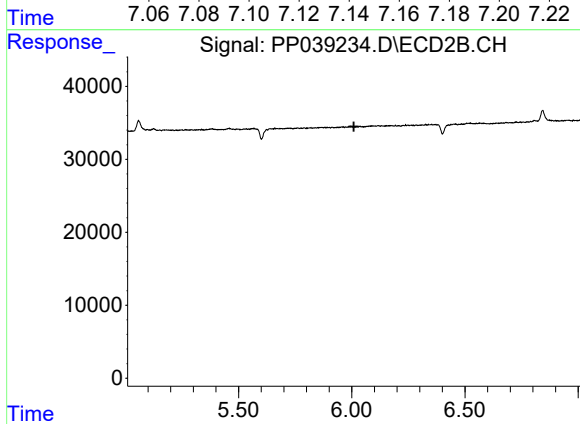

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 6.010 min
Response: 0
Conc: N.D.

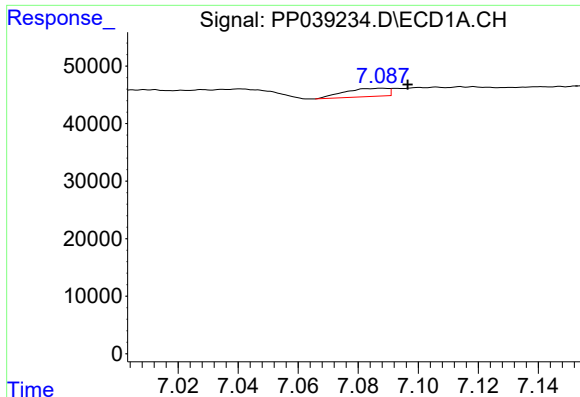

#26 AR-1254-1


R.T.: 7.088 min
Delta R.T.: -0.008 min
Response: 14370
Conc: 9.42 ng/ml

Instrument :
ECD_P
ClientSampleId :

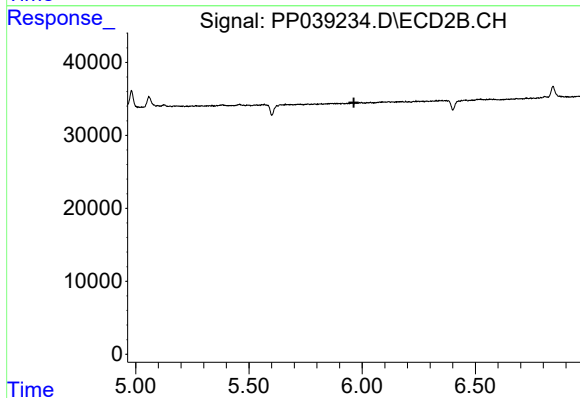


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 5.964 min
Response: 0
Conc: N.D.

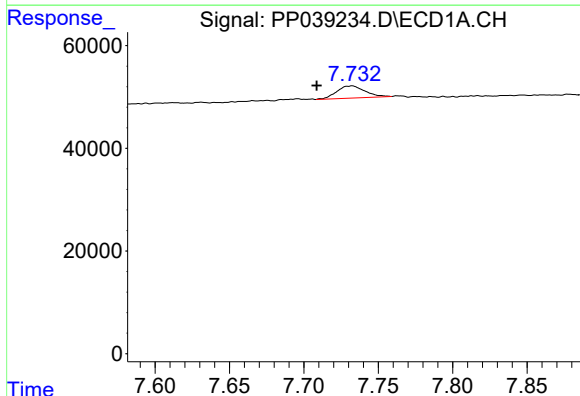


#28 AR-1254-3

R.T.: 7.733 min
Delta R.T.: 0.024 min
Response: 31274
Conc: 12.78 ng/ml

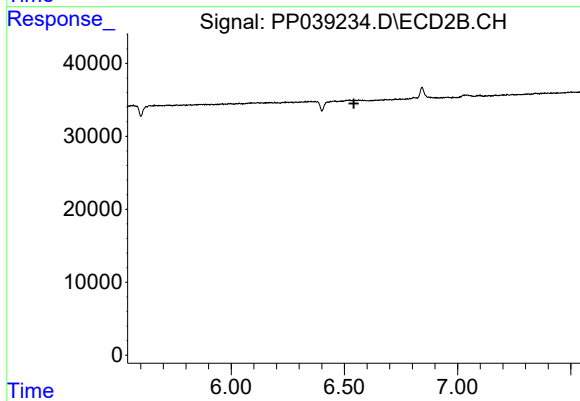

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.542 min
Response: 0
Conc: N.D.

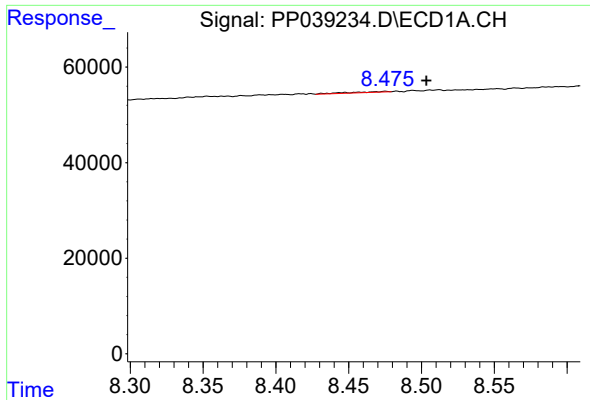

#36 AR-1262-1

R.T.: 8.475 min
Delta R.T.: -0.028 min
Response: 3225
Conc: 1.45 ng/ml

Instrument :
ECD_P
ClientSampleId :

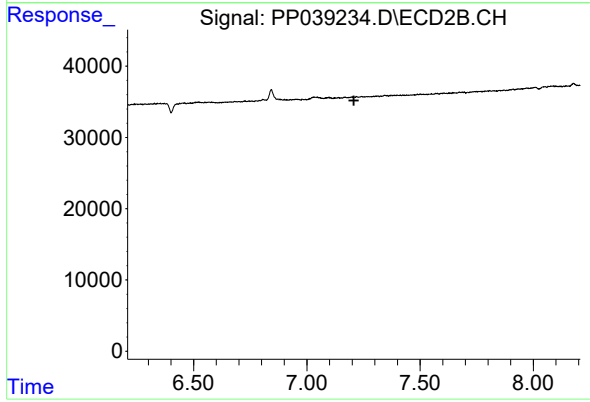

#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 7.208 min
Response: 0
Conc: N.D.