

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
 Data File : PP039197.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 07 Sep 2021 17:48
 Operator : AJ\MA
 Sample : M3658-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CHRT-24029

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 08:52:27 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.870	3.856	845524	486708	22.070	20.291
2)	SA Decachlor...	10.837	9.107	965808	594045	29.341	27.144
Target Compounds							
31)	L7 AR-1260-1	7.873	6.677	202743	132089	117.994	109.780
32)	L7 AR-1260-2	8.138	6.877	307247	141178	154.672	100.958 #
33)	L7 AR-1260-3	8.502	7.027	163505	130198	121.133	95.342
34)	L7 AR-1260-4	8.732	7.509	227971	82684	141.429	85.066 #
35)	L7 AR-1260-5	9.056	7.759	326660	229511	117.926	111.116



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
Data File : PP039197.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 07 Sep 2021 17:48
Operator : AJ\MA
Sample : M3658-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CHRT-24029

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 08:52:27 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

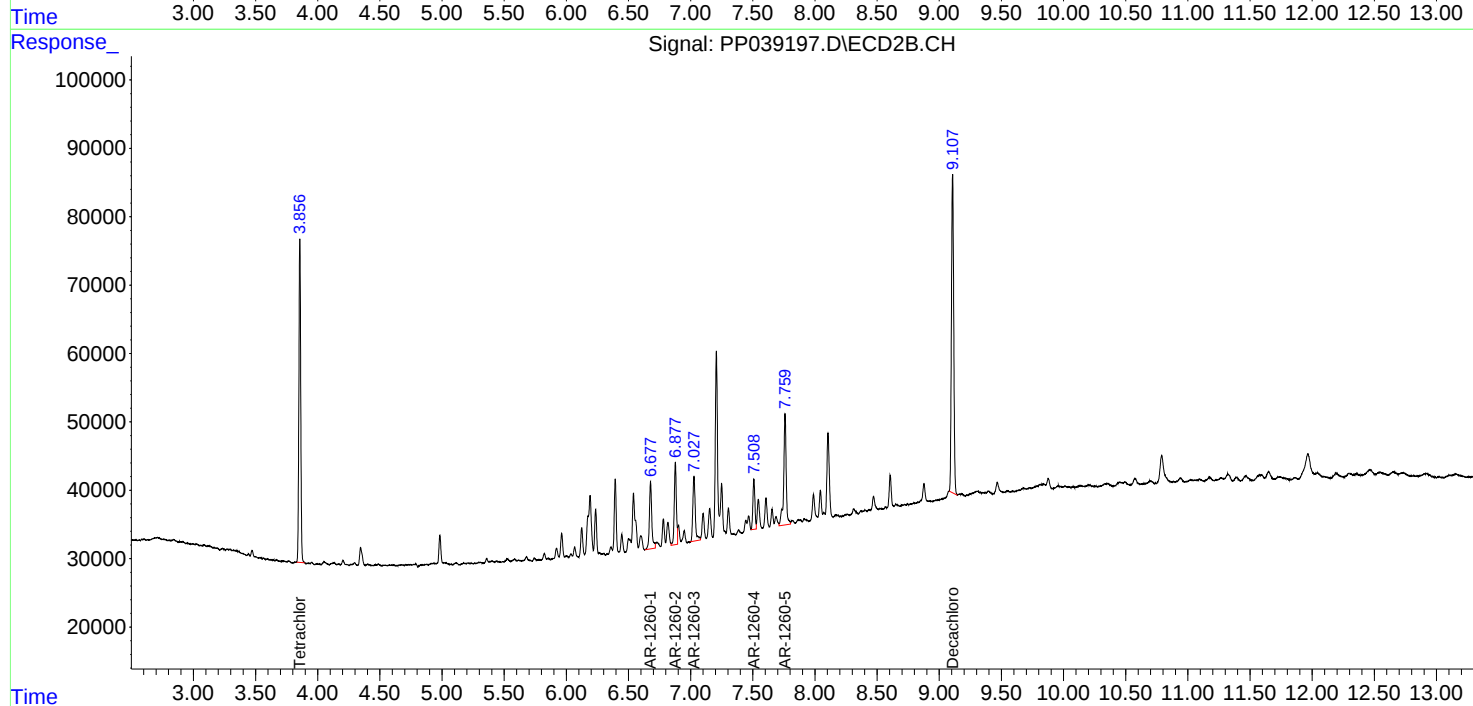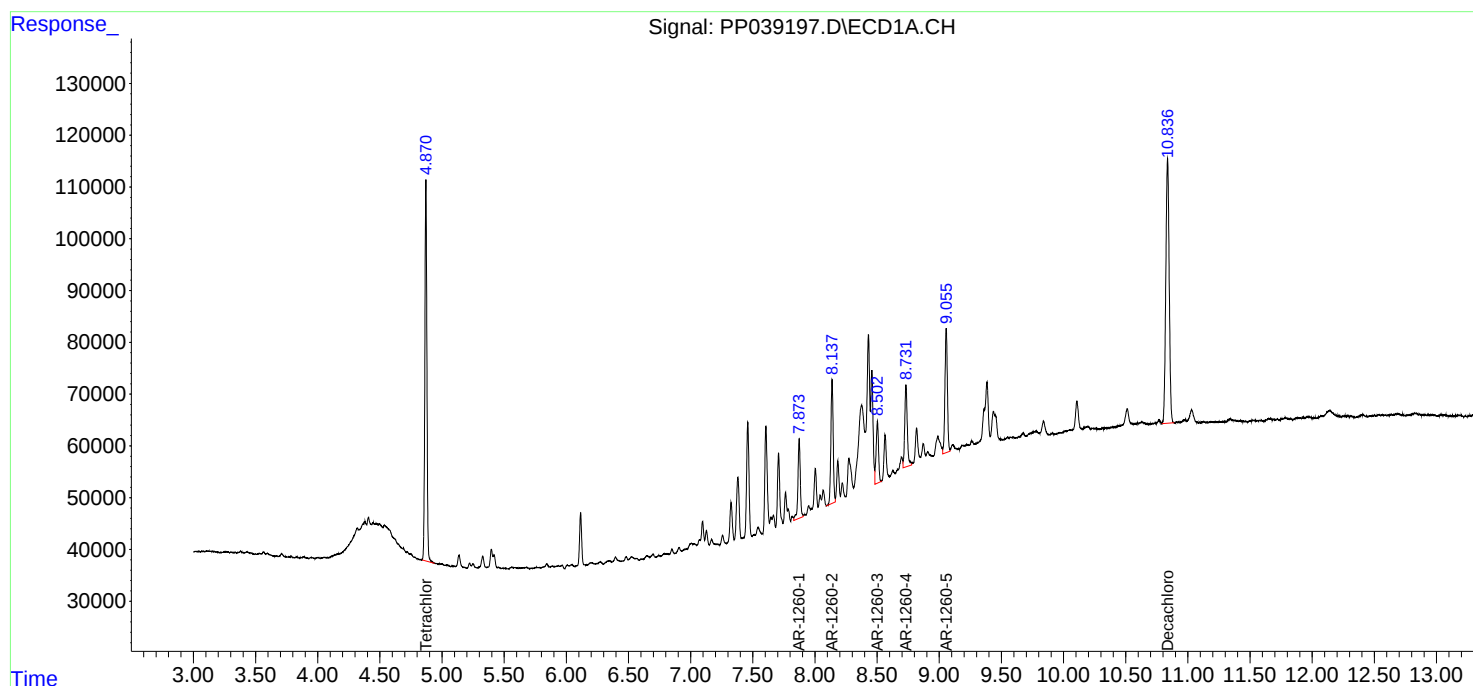


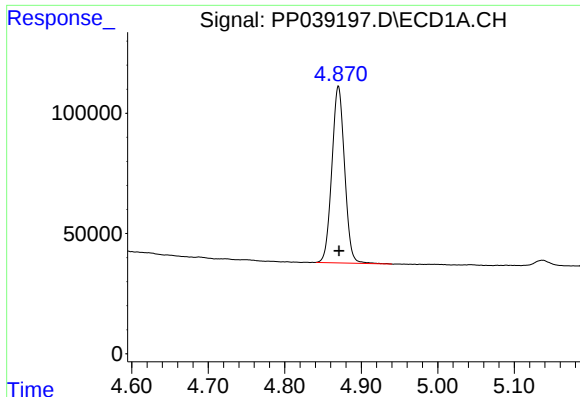

#1 Tetrachloro-m-xylene


R.T.: 4.870 min
Delta R.T.: 0.000 min
Response: 845524
Conc: 22.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24029

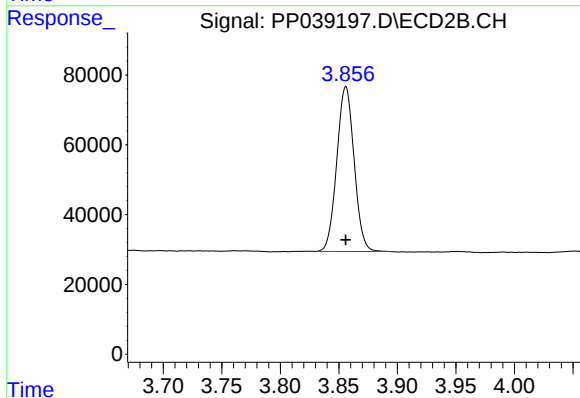


#1 Tetrachloro-m-xylene

R.T.: 3.856 min
Delta R.T.: 0.000 min
Response: 486708
Conc: 20.29 ng/ml

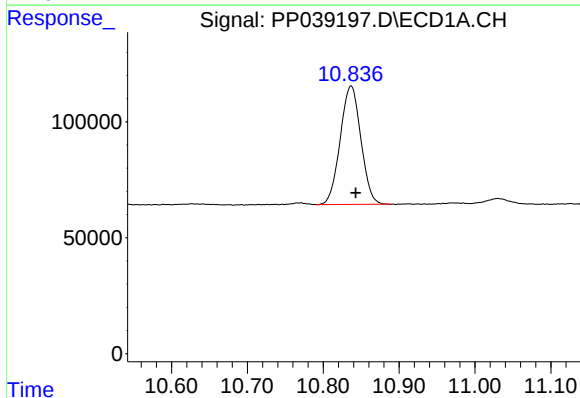


#2 Decachlorobiphenyl

R.T.: 10.837 min
Delta R.T.: -0.006 min
Response: 965808
Conc: 29.34 ng/ml

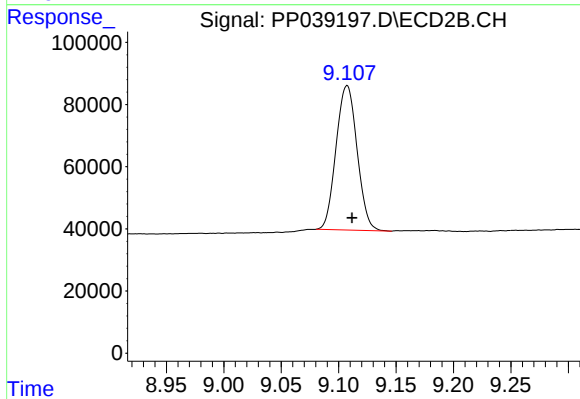

#2 Decachlorobiphenyl


R.T.: 9.107 min
Delta R.T.: -0.004 min
Response: 594045
Conc: 27.14 ng/ml

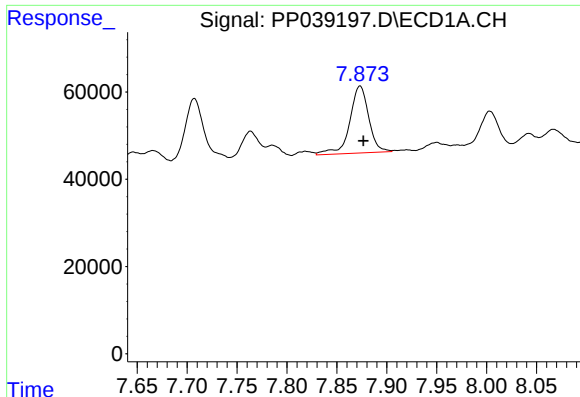

#31 AR-1260-1


R.T.: 7.873 min
Delta R.T.: -0.003 min
Response: 202743
Conc: 117.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24029

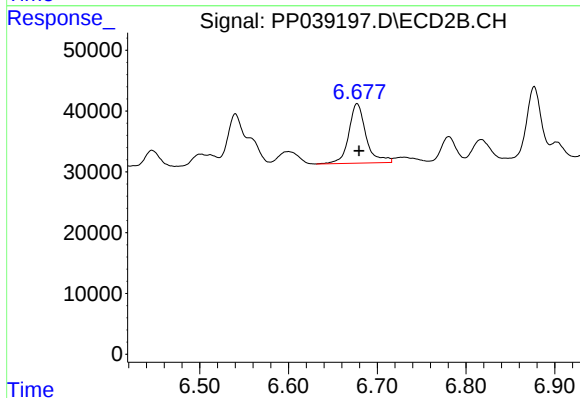


#31 AR-1260-1

R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 132089
Conc: 109.78 ng/ml

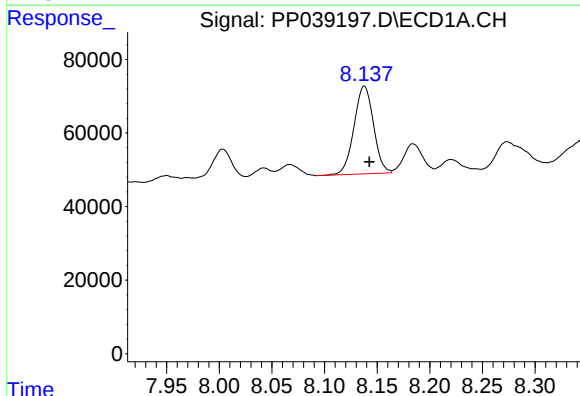


#32 AR-1260-2

R.T.: 8.138 min
Delta R.T.: -0.005 min
Response: 307247
Conc: 154.67 ng/ml

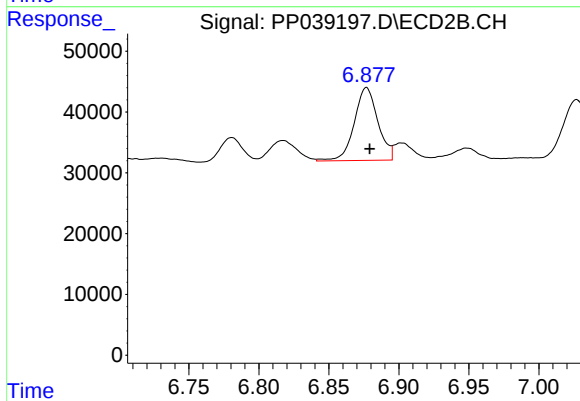

#32 AR-1260-2


R.T.: 6.877 min
Delta R.T.: -0.002 min
Response: 141178
Conc: 100.96 ng/ml

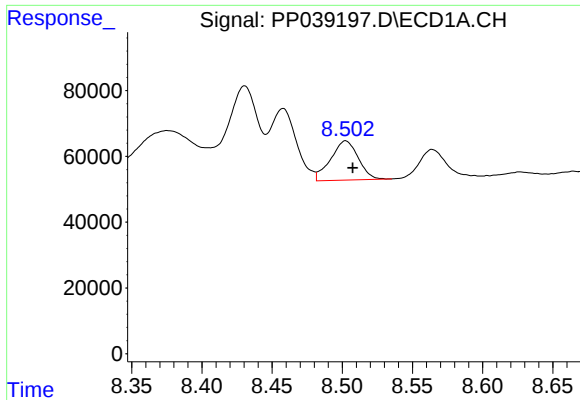

#33 AR-1260-3


R.T.: 8.502 min
Delta R.T.: -0.005 min
Response: 163505
Conc: 121.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24029

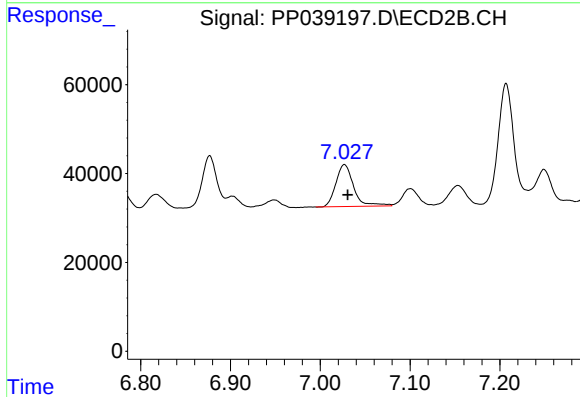


#33 AR-1260-3

R.T.: 7.027 min
Delta R.T.: -0.003 min
Response: 130198
Conc: 95.34 ng/ml

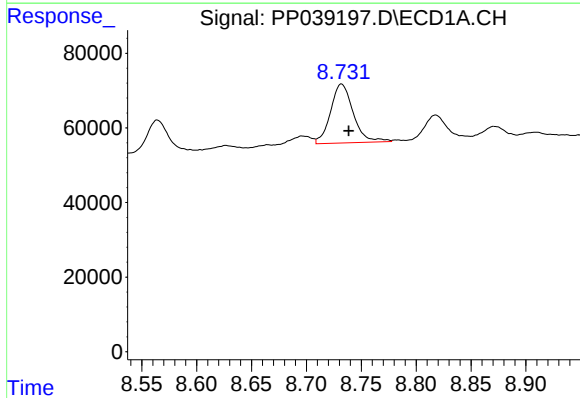


#34 AR-1260-4

R.T.: 8.732 min
Delta R.T.: -0.007 min
Response: 227971
Conc: 141.43 ng/ml

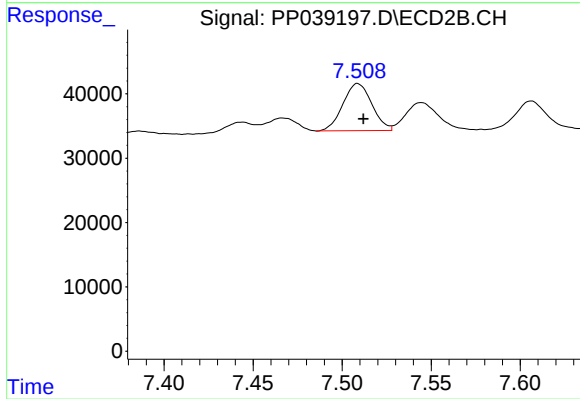

#34 AR-1260-4


R.T.: 7.509 min
Delta R.T.: -0.003 min
Response: 82684
Conc: 85.07 ng/ml

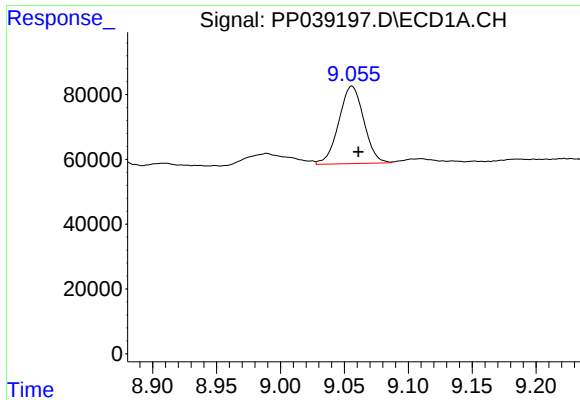

#35 AR-1260-5

R.T.: 9.056 min
Delta R.T.: -0.005 min
Response: 326660
Conc: 117.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
CHRT-24029

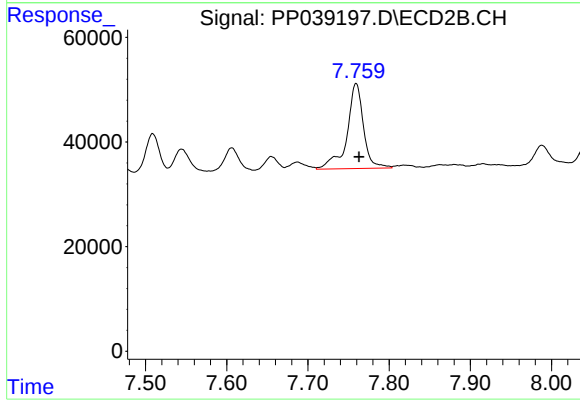

#35 AR-1260-5

R.T.: 7.759 min
Delta R.T.: -0.004 min
Response: 229511
Conc: 111.12 ng/ml