

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
 Data File : PP039222.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 08 Sep 2021 1:58
 Operator : AJ\MA
 Sample : M3659-01
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TREMONT-AVE-STATION-DRUM-10

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 08 09:11:12 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.869	3.853	1107041	593434	28.896	24.741
2) SA Decachlor...	10.836	9.106	982844	570045	29.859	26.047

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090721\
Data File : PP039222.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 08 Sep 2021 1:58
Operator : AJ\MA
Sample : M3659-01
Misc :
ALS Vial : 39 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-STATION-DRUM-10

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 08 09:11:12 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

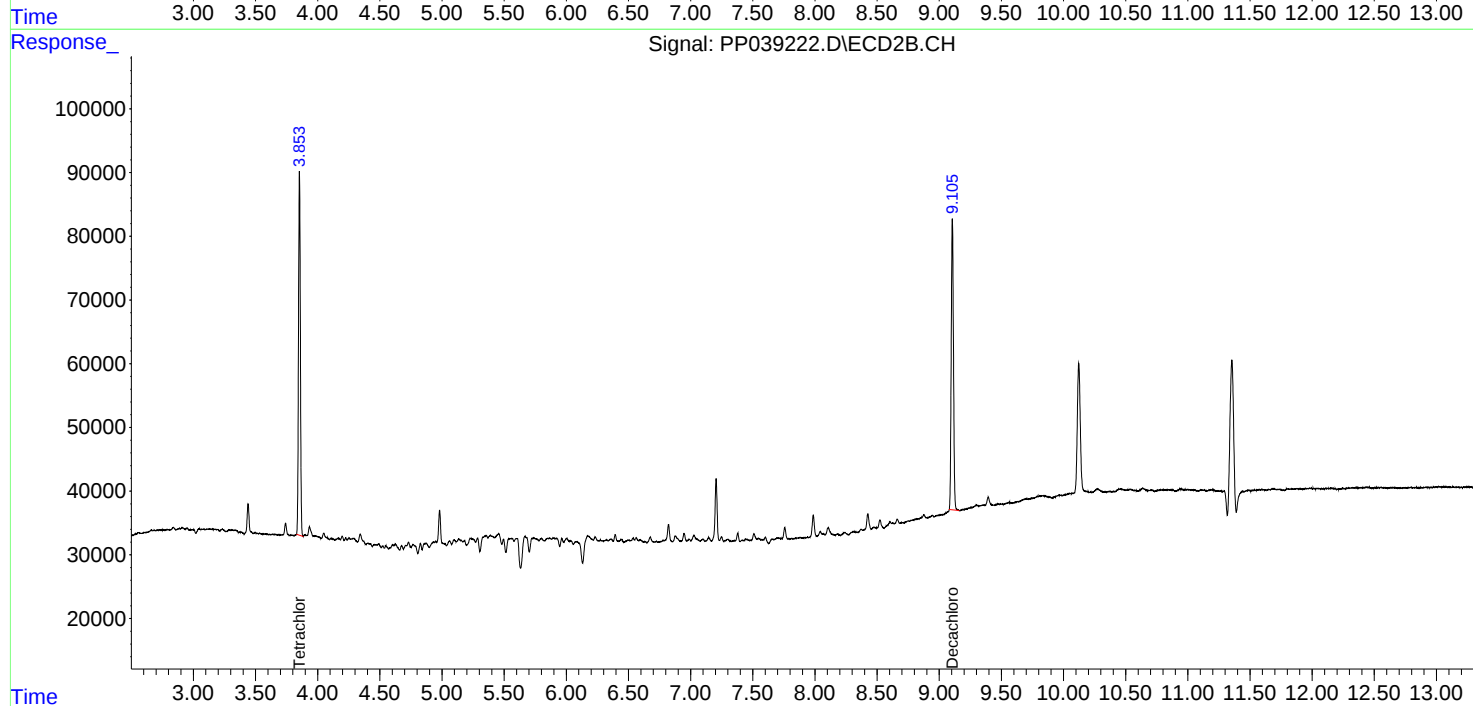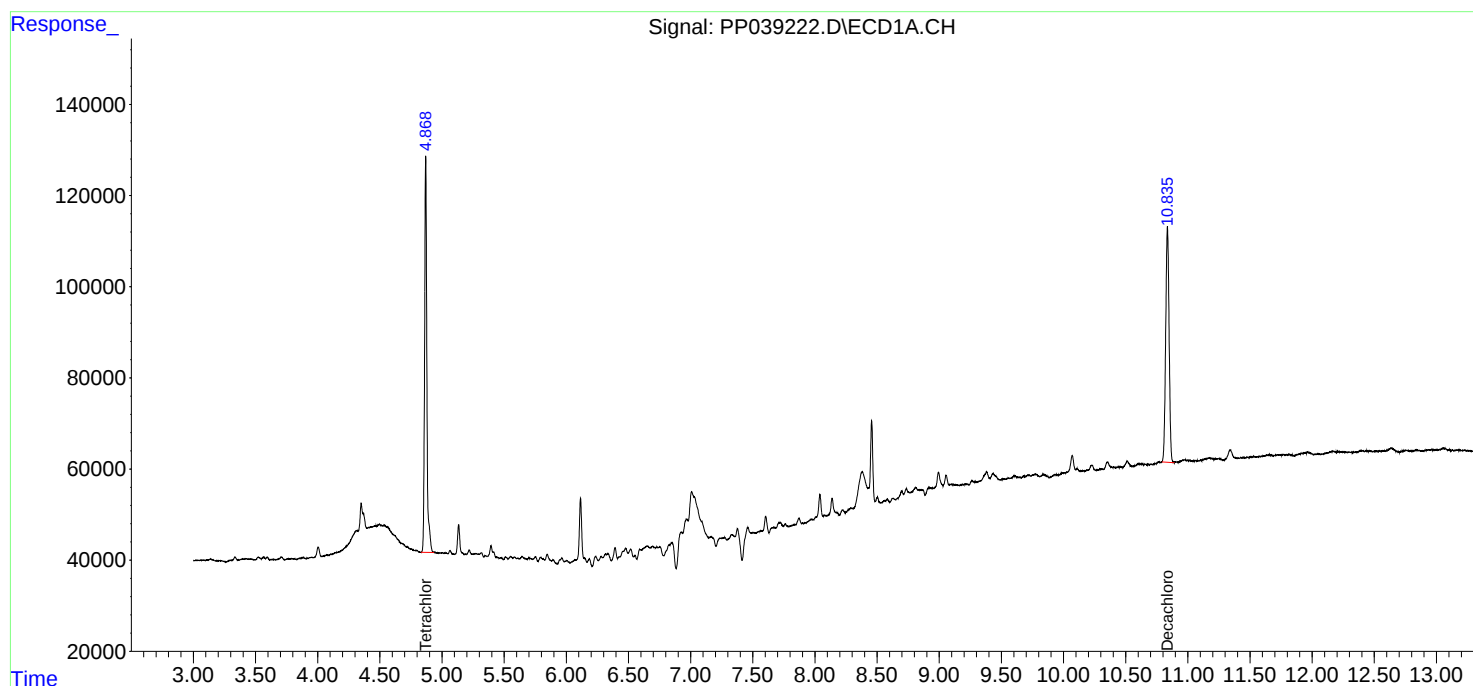


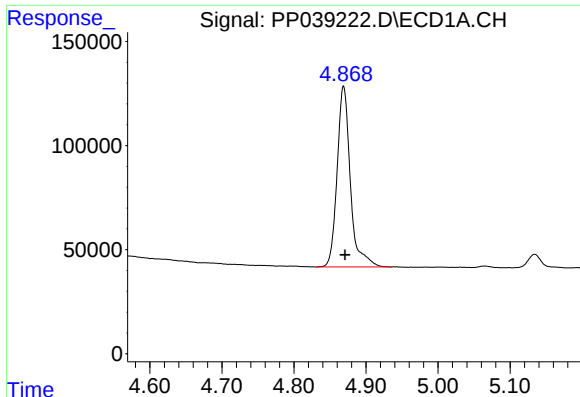

#1 Tetrachloro-m-xylene


R.T.: 4.869 min
Delta R.T.: -0.002 min
Response: 1107041
Conc: 28.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
TREMONT-AVE-STATION-DRUM-10

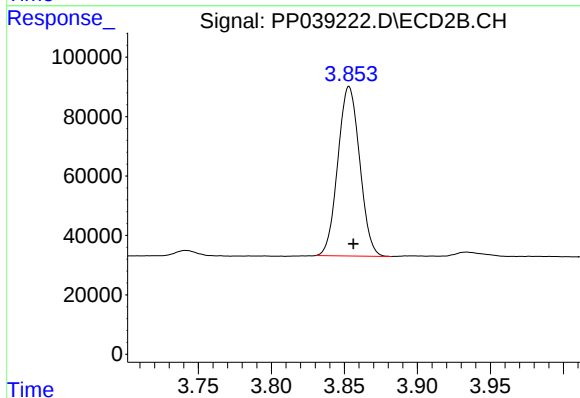


#1 Tetrachloro-m-xylene

R.T.: 3.853 min
Delta R.T.: -0.003 min
Response: 593434
Conc: 24.74 ng/ml

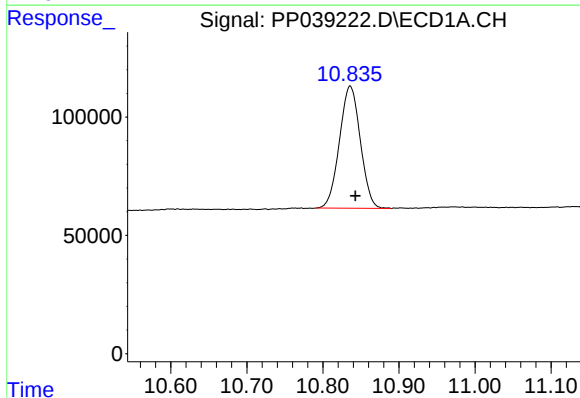

#2 Decachlorobiphenyl

R.T.: 10.836 min
Delta R.T.: -0.007 min
Response: 982844
Conc: 29.86 ng/ml

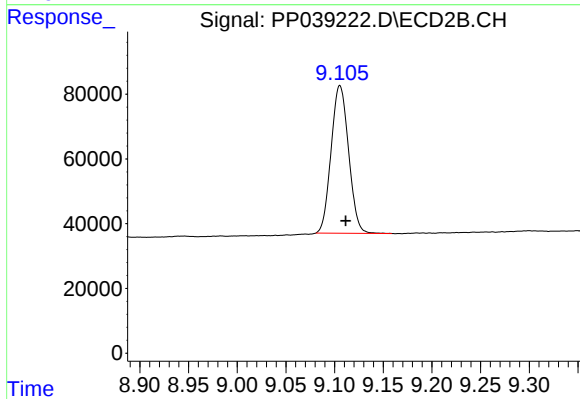

#2 Decachlorobiphenyl

R.T.: 9.106 min
Delta R.T.: -0.006 min
Response: 570045
Conc: 26.05 ng/ml