

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090825\
 Data File : PP074945.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2025 10:30
 Operator : YP\AJ
 Sample : Q2893-09
 Misc : AR1242 WATER MDL 25PPB
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 06:03:10 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.656	3.795	24103833	87301397	19.698	18.055
2)	SA Decachlor...	10.429	8.804	19668318	119.9E6	19.917	15.994
Target Compounds							
3)	L1 AR-1016-1	5.808	4.891	949296	6943942	21.531	13.633 #
4)	L1 AR-1016-2	5.829	4.949	1562458	3812501	24.863	16.018 #
5)	L1 AR-1016-3	5.891	5.074	1080723	2618962	24.062	18.991
6)	L1 AR-1016-4	5.989	5.115	674946	1945463	19.185	13.916 #
7)	L1 AR-1016-5	6.281	5.328	749801	2305336	22.594	13.881 #
8)	L2 AR-1221-1	4.854	4.008	457047	318426	25.979	5.147 #
9)	L2 AR-1221-2	4.956	4.084	570920	1489557	42.743	32.946
10)	L2 AR-1221-3	5.018	4.166	552361	1742909	14.569	10.608 #
11)	L3 AR-1232-1	5.018	4.166	552361	1742909	18.185	13.606 #
12)	L3 AR-1232-2	5.543	4.891	691202	6943942	43.863	29.957 #
13)	L3 AR-1232-3	5.829	5.074	1562458	2618962	51.155	43.606
14)	L3 AR-1232-4	5.989	5.157	674946	2113045	39.084	28.668 #
15)	L3 AR-1232-5	6.075	5.328	632352	2305336	48.714	37.133
16)	L4 AR-1242-1	5.808	4.891	949296	6943942	24.802	16.464 #
17)	L4 AR-1242-2	5.829	4.949	1562458	3812501	27.663	19.036 #
18)	L4 AR-1242-3	5.891	5.074	1080723	2618962	26.617	22.139
19)	L4 AR-1242-4	5.989	5.157	674946	2113045	21.264	12.345 #
20)	L4 AR-1242-5	6.718	5.686	1585199	6043103	43.947	32.636 #
21)	L5 AR-1248-1	5.808	4.891	949296	6943942	31.409	25.146
22)	L5 AR-1248-2	6.075	5.115	632352	1945463	14.673	11.007
23)	L5 AR-1248-3	6.281	5.157	749801	2113045	16.054	9.300 #
24)	L5 AR-1248-4	6.679	5.328	1063396	2305336	19.334	10.574 #
25)	L5 AR-1248-5	6.718	5.717	1585199	12796305	28.577	34.837
26)	L6 AR-1254-1	6.652	5.686	1023674	6043103	17.568	12.677 #
27)	L6 AR-1254-2	6.873	5.835	1023430	853211	12.540	2.423 #
28)	L6 AR-1254-3	7.226	6.233	2650995	938929	29.718	1.515 #
29)	L6 AR-1254-4	7.513	6.464	374830	841006	5.687	1.795 #
30)	L6 AR-1254-5	7.928	6.879	866436	707351	10.428	1.442 #
31)	L7 AR-1260-1	7.399	6.363	90850	564269	1.572	1.504
32)	L7 AR-1260-2	7.651	6.562	314028	304310	4.557	0.575 #
33)	L7 AR-1260-3	0.000	6.709	0	636872	N.D.	1.471 #
34)	L7 AR-1260-4	8.216	7.162	488274	230238	7.654	0.604 #
35)	L7 AR-1260-5	8.559	7.411	385196	331185	3.396	0.330 #
36)	L8 AR-1262-1	8.216	6.920	488274	369795	6.340	0.523 #
37)	L8 AR-1262-2	8.559	7.182	385196	175056	2.910	0.336 #
38)	L8 AR-1262-3	0.000	7.696	0	1182839	N.D.	2.537 #
39)	L8 AR-1262-4	8.992	7.756	138220	1096541	1.835	1.334 #
40)	L8 AR-1262-5	9.596f	8.252	140356	287398	2.303	0.802 #
41)	L9 AR-1268-1	8.813f	7.696	33290	1182839	0.205	0.839 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090825\
Data File : PP074945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2025 10:30
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1242 WATER MDL 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 06:03:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.992	7.756	138220	1096541	0.942	0.804
43)	L9 AR-1268-3	0.000	7.970	0	683335	N.D.	0.655 #
44)	L9 AR-1268-4	9.596f	8.252	140356	287398	2.087	0.750 #
45)	L9 AR-1268-5	10.076	8.558	162325	428178	0.439	0.137 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090825\
Data File : PP074945.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2025 10:30
Operator : YP\AJ
Sample : Q2893-09
Misc : AR1242 WATER MDL 25PPB
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 06:03:10 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

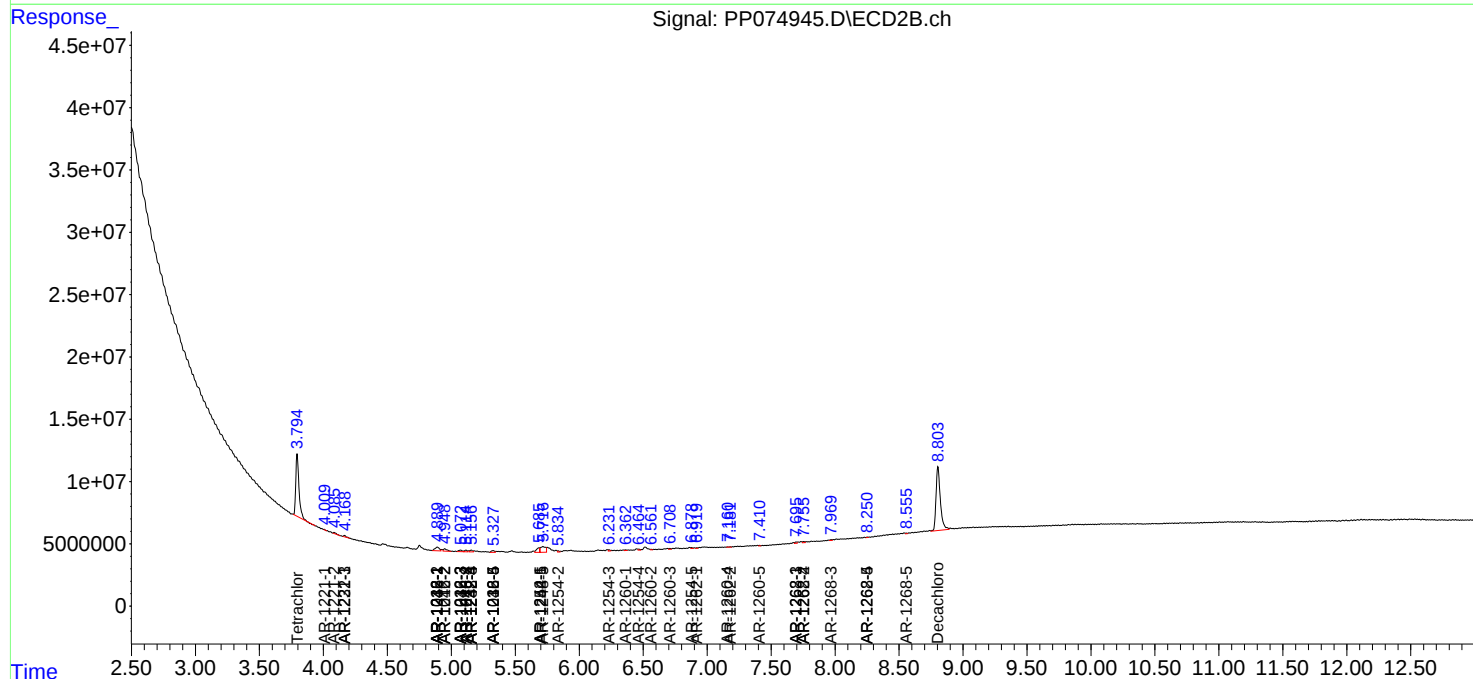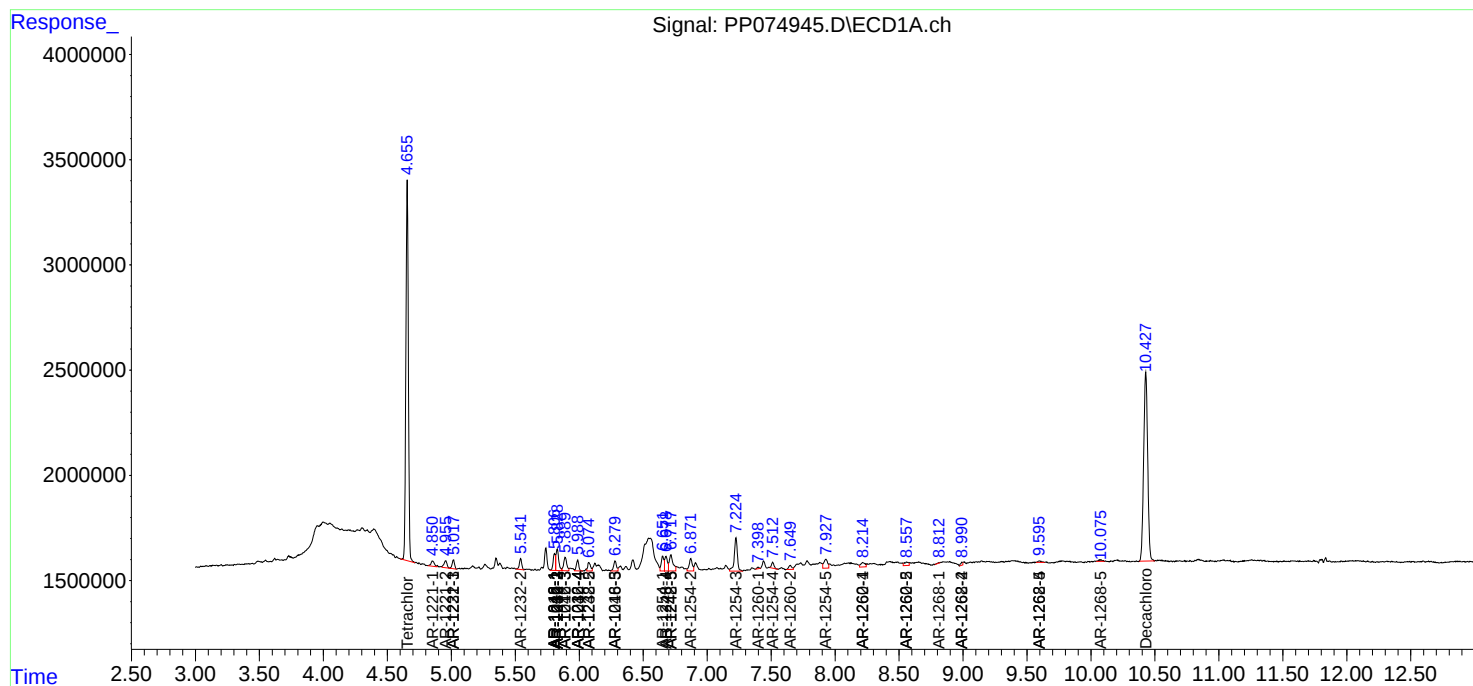


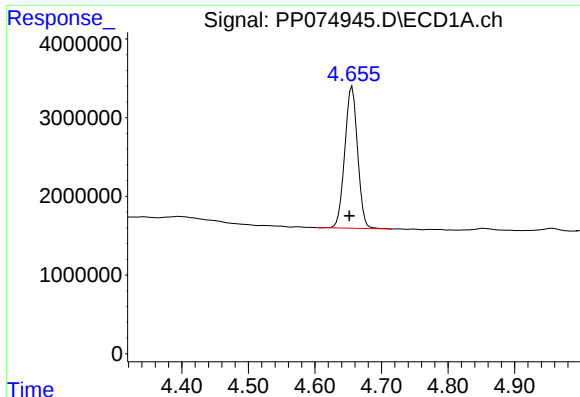

#1 Tetrachloro-m-xylene


R.T.: 4.656 min
Delta R.T.: 0.004 min
Response: 24103833
Conc: 19.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

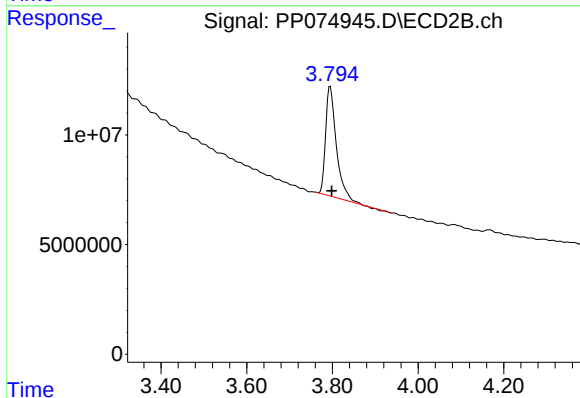


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: -0.004 min
Response: 87301397
Conc: 18.05 ng/ml

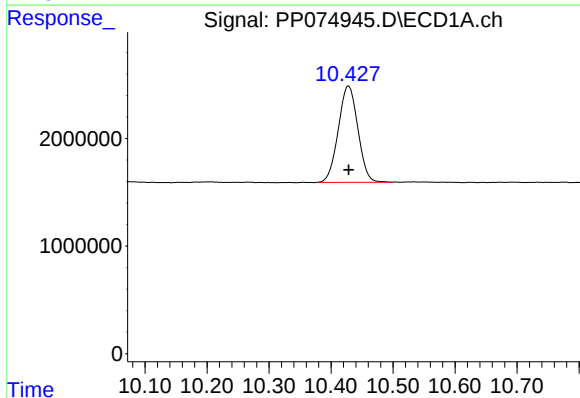


#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: 0.000 min
Response: 19668318
Conc: 19.92 ng/ml

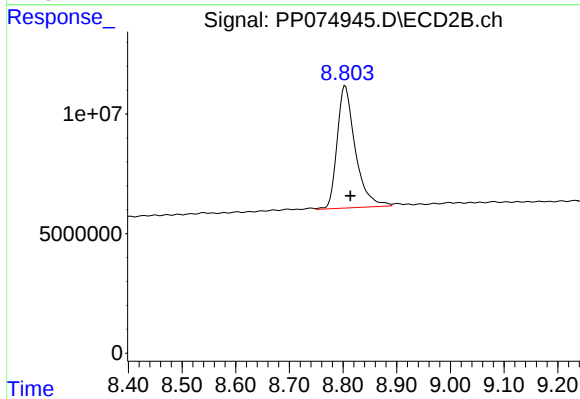

#2 Decachlorobiphenyl


R.T.: 8.804 min
Delta R.T.: -0.010 min
Response: 119944398
Conc: 15.99 ng/ml

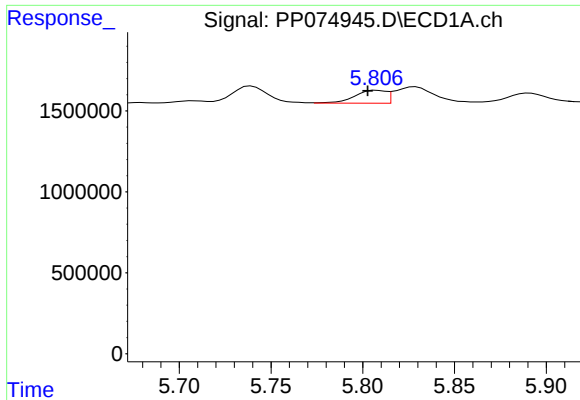

#3 AR-1016-1


R.T.: 5.808 min
Delta R.T.: 0.005 min
Response: 949296
Conc: 21.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

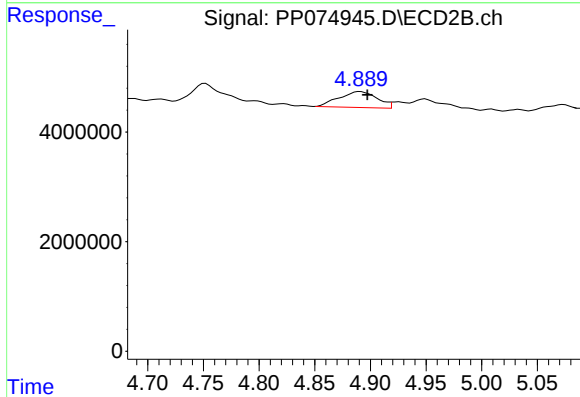


#3 AR-1016-1

R.T.: 4.891 min
Delta R.T.: -0.007 min
Response: 6943942
Conc: 13.63 ng/ml

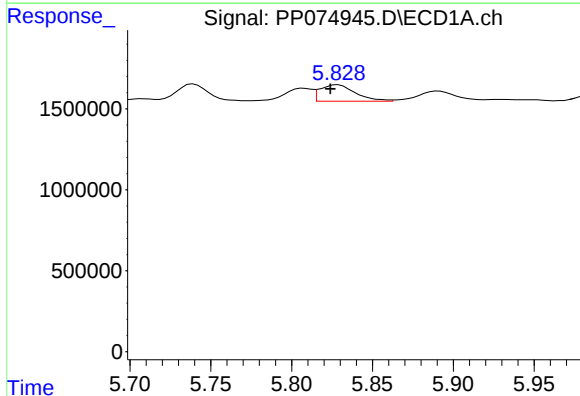


#4 AR-1016-2

R.T.: 5.829 min
Delta R.T.: 0.005 min
Response: 1562458
Conc: 24.86 ng/ml

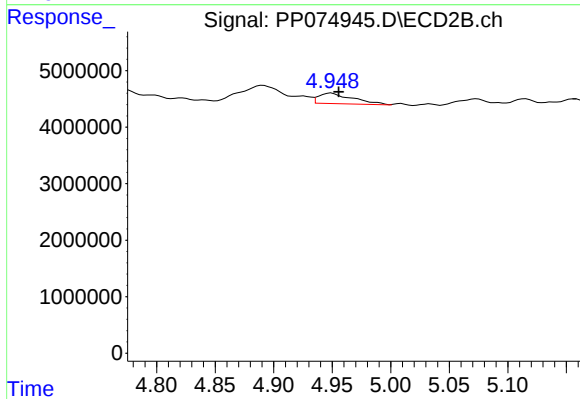

#4 AR-1016-2


R.T.: 4.949 min
Delta R.T.: -0.006 min
Response: 3812501
Conc: 16.02 ng/ml

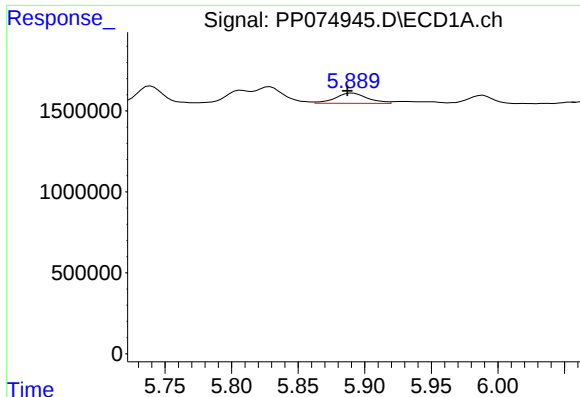

#5 AR-1016-3


R.T.: 5.891 min
Delta R.T.: 0.004 min
Response: 1080723
Conc: 24.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

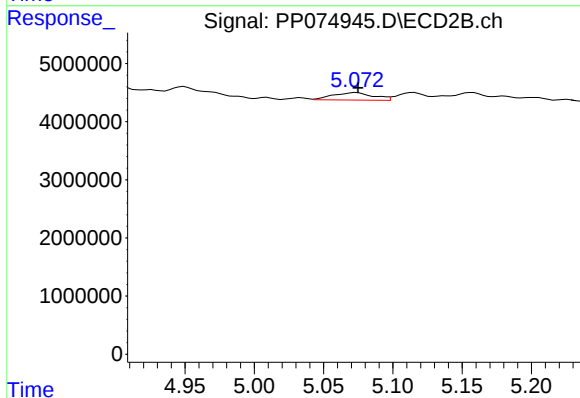


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 2618962
Conc: 18.99 ng/ml

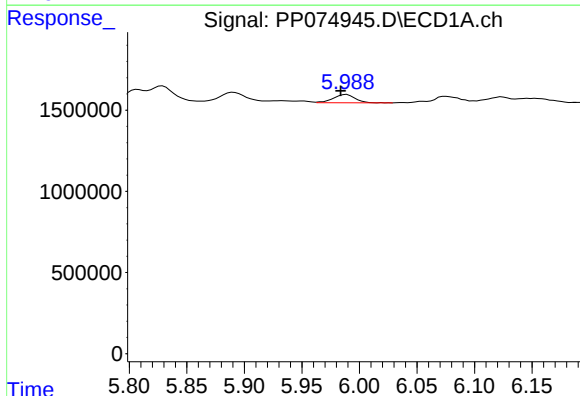


#6 AR-1016-4

R.T.: 5.989 min
Delta R.T.: 0.005 min
Response: 674946
Conc: 19.18 ng/ml

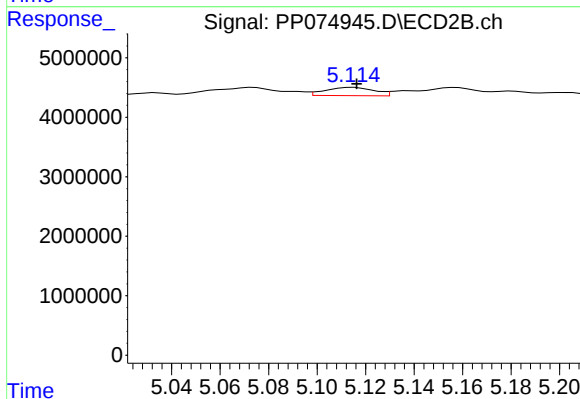

#6 AR-1016-4


R.T.: 5.115 min
Delta R.T.: -0.001 min
Response: 1945463
Conc: 13.92 ng/ml

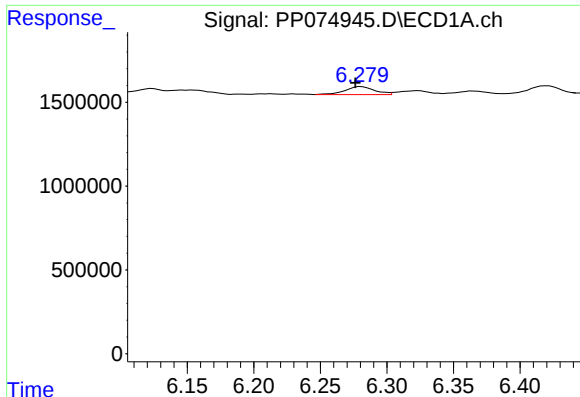

#7 AR-1016-5


R.T.: 6.281 min
Delta R.T.: 0.004 min
Response: 749801
Conc: 22.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

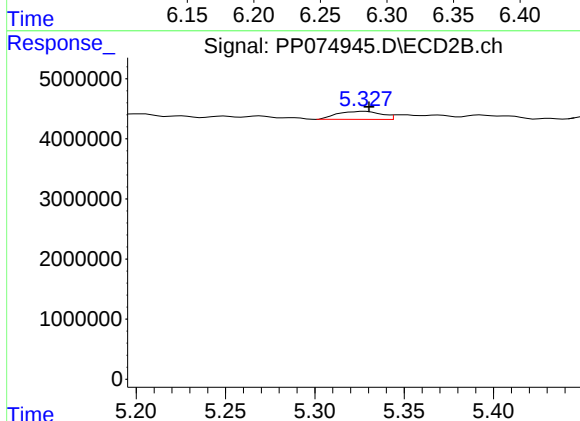


#7 AR-1016-5

R.T.: 5.328 min
Delta R.T.: -0.002 min
Response: 2305336
Conc: 13.88 ng/ml

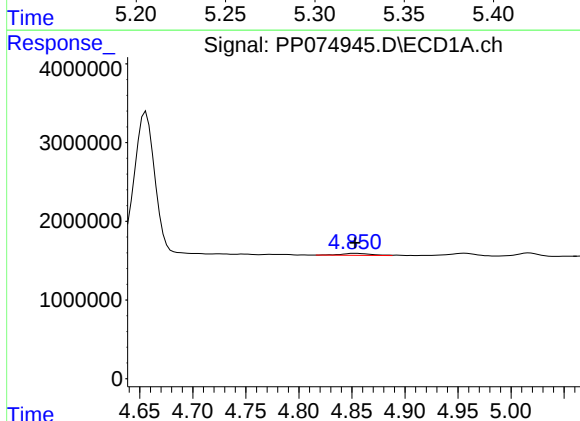


#8 AR-1221-1

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 457047
Conc: 25.98 ng/ml

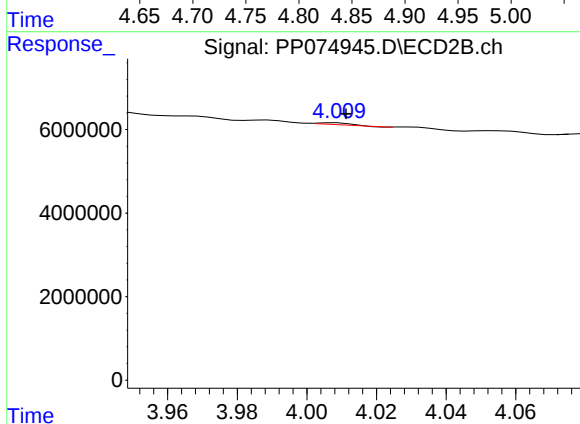

#8 AR-1221-1


R.T.: 4.008 min
Delta R.T.: -0.003 min
Response: 318426
Conc: 5.15 ng/ml

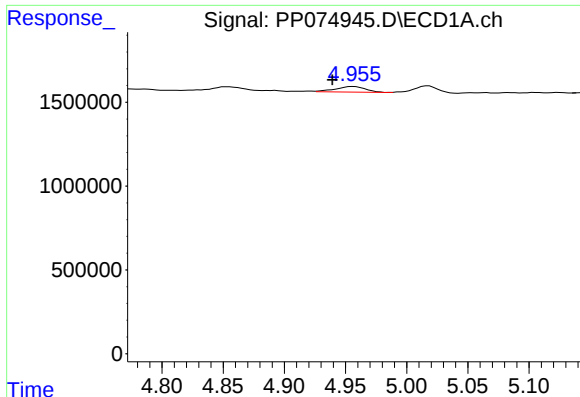

#9 AR-1221-2


R.T.: 4.956 min
Delta R.T.: 0.017 min
Response: 570920
Conc: 42.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

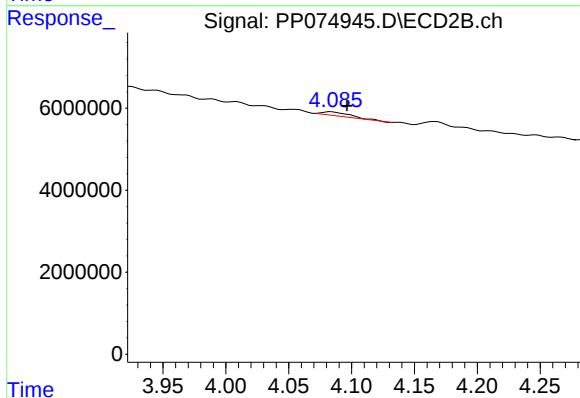


#9 AR-1221-2

R.T.: 4.084 min
Delta R.T.: -0.012 min
Response: 1489557
Conc: 32.95 ng/ml

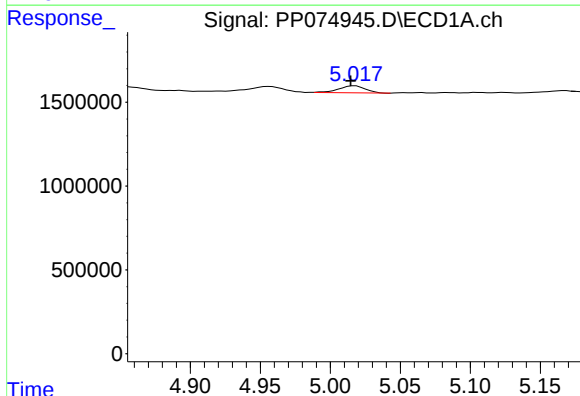


#10 AR-1221-3

R.T.: 5.018 min
Delta R.T.: 0.003 min
Response: 552361
Conc: 14.57 ng/ml

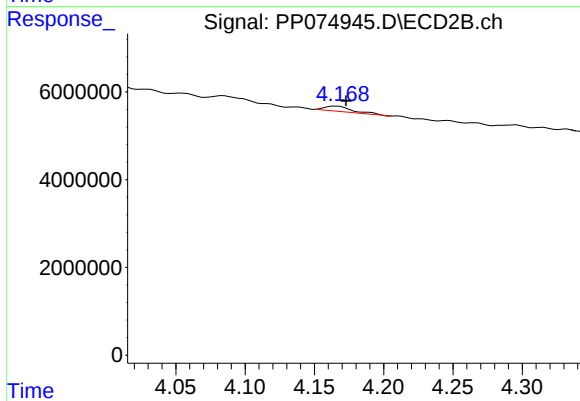

#10 AR-1221-3


R.T.: 4.166 min
Delta R.T.: -0.007 min
Response: 1742909
Conc: 10.61 ng/ml

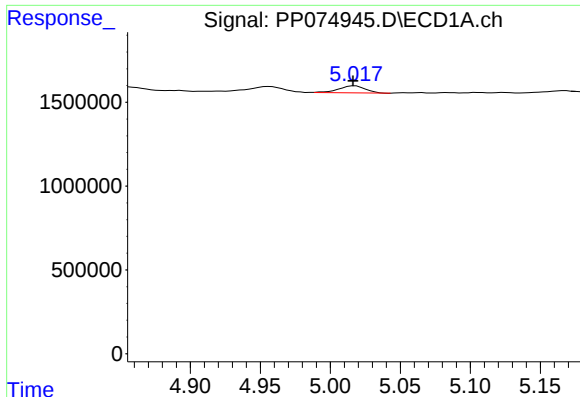

#11 AR-1232-1


R.T.: 5.018 min
Delta R.T.: 0.002 min
Response: 552361
Conc: 18.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

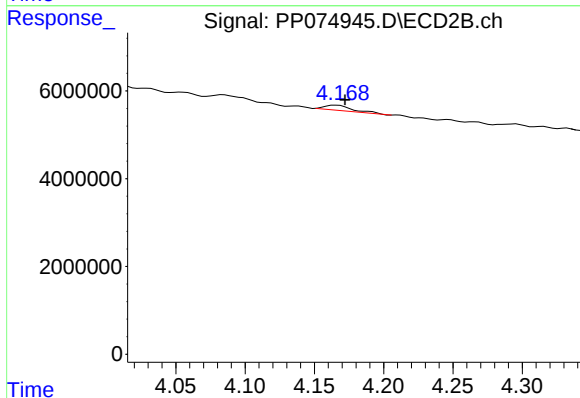


#11 AR-1232-1

R.T.: 4.166 min
Delta R.T.: -0.006 min
Response: 1742909
Conc: 13.61 ng/ml

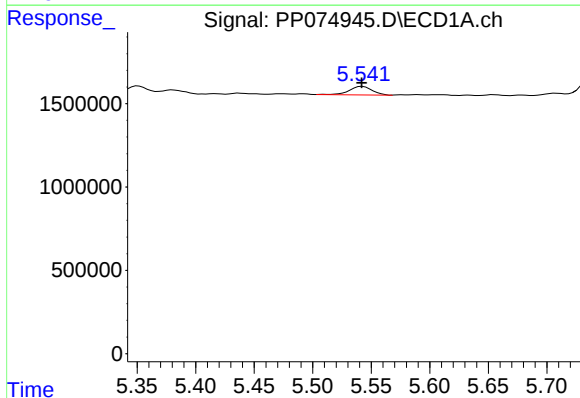


#12 AR-1232-2

R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 691202
Conc: 43.86 ng/ml

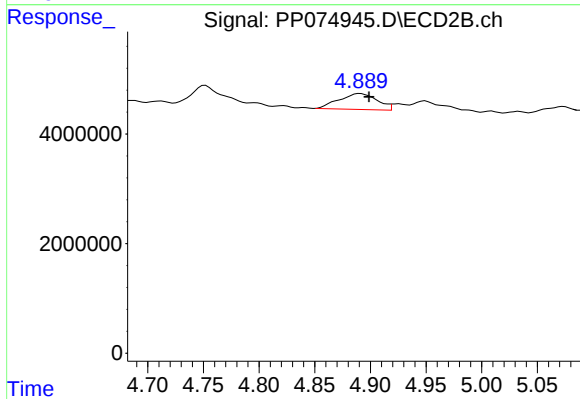

#12 AR-1232-2


R.T.: 4.891 min
Delta R.T.: -0.008 min
Response: 6943942
Conc: 29.96 ng/ml

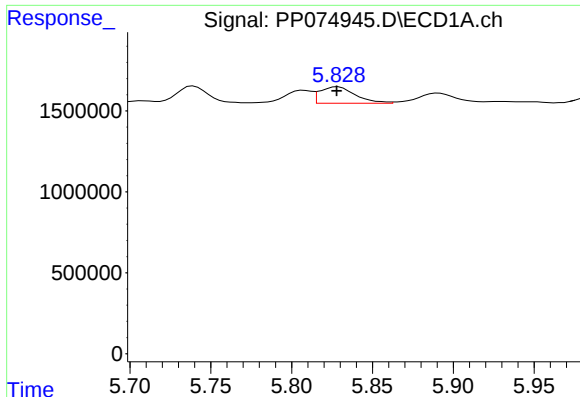

#13 AR-1232-3


R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 1562458
Conc: 51.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

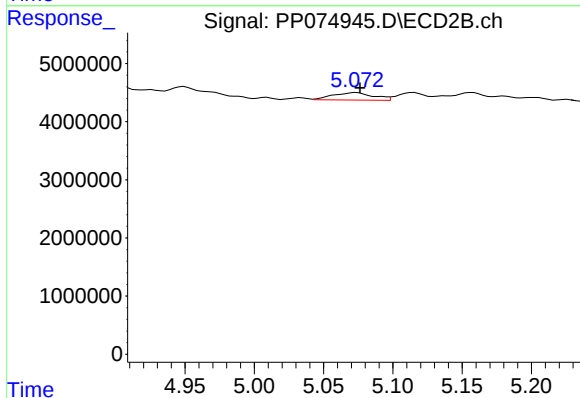


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 2618962
Conc: 43.61 ng/ml

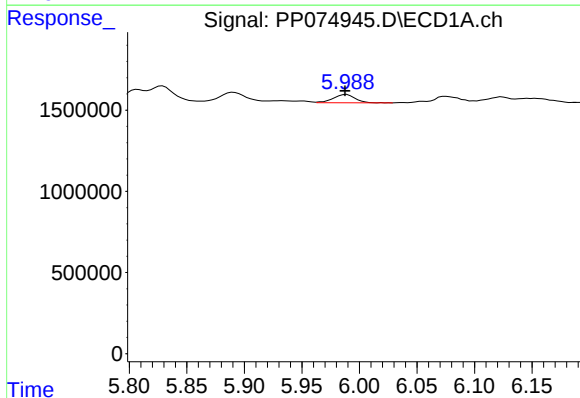


#14 AR-1232-4

R.T.: 5.989 min
Delta R.T.: 0.001 min
Response: 674946
Conc: 39.08 ng/ml

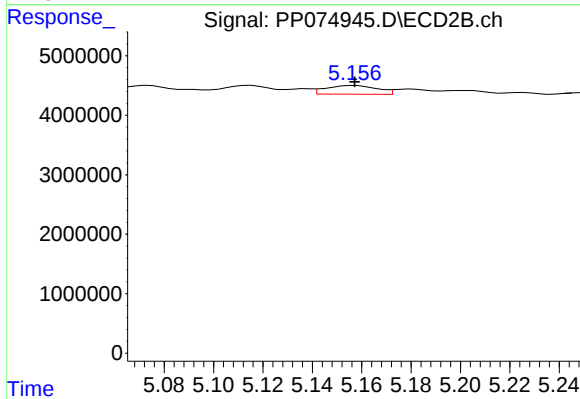

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 2113045
Conc: 28.67 ng/ml

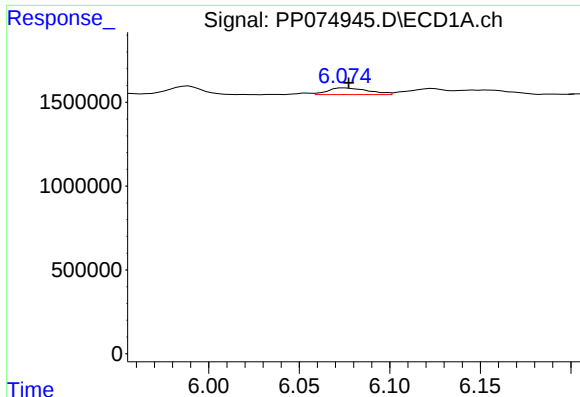

#15 AR-1232-5


R.T.: 6.075 min
Delta R.T.: -0.002 min
Response: 632352
Conc: 48.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

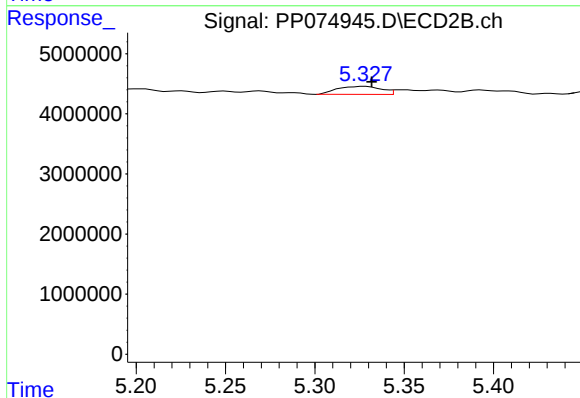


#15 AR-1232-5

R.T.: 5.328 min
Delta R.T.: -0.004 min
Response: 2305336
Conc: 37.13 ng/ml

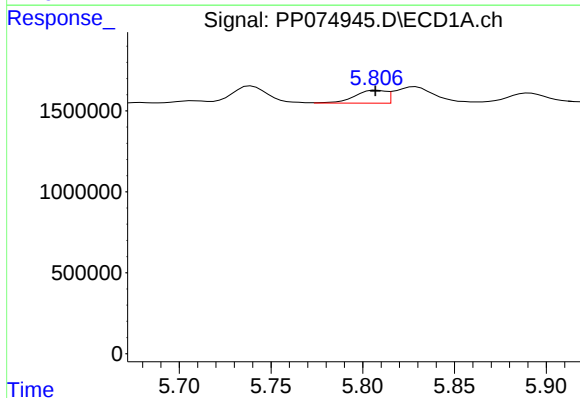


#16 AR-1242-1

R.T.: 5.808 min
Delta R.T.: 0.000 min
Response: 949296
Conc: 24.80 ng/ml

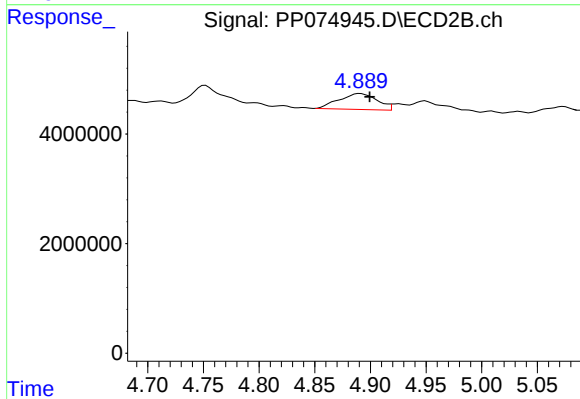

#16 AR-1242-1


R.T.: 4.891 min
Delta R.T.: -0.009 min
Response: 6943942
Conc: 16.46 ng/ml

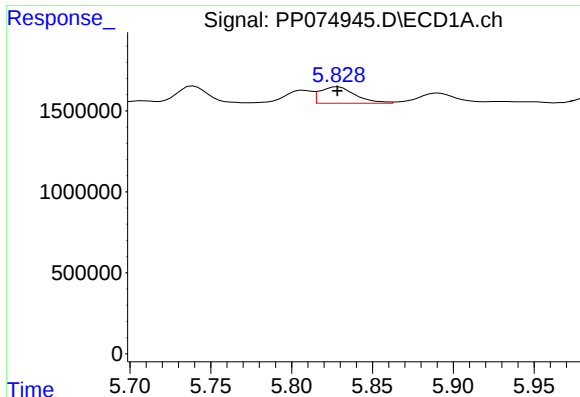

#17 AR-1242-2


R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 1562458
Conc: 27.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

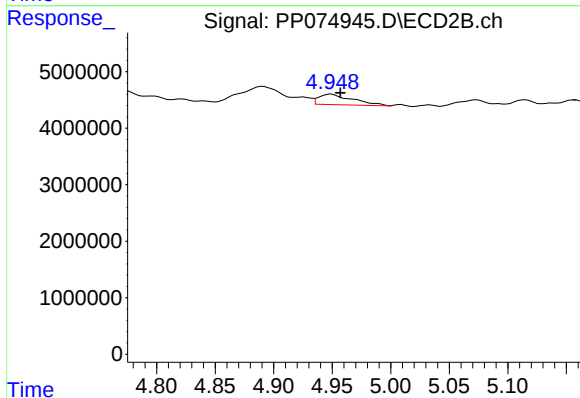


#17 AR-1242-2

R.T.: 4.949 min
Delta R.T.: -0.007 min
Response: 3812501
Conc: 19.04 ng/ml

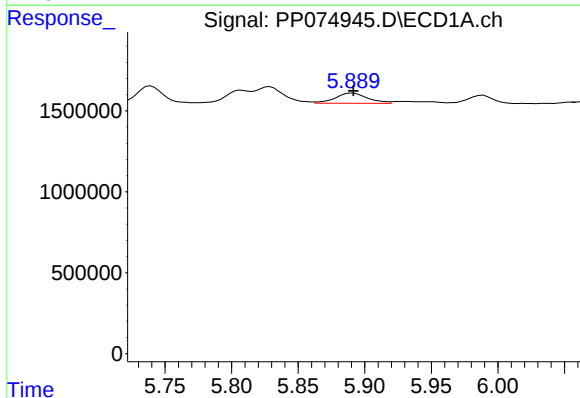


#18 AR-1242-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 1080723
Conc: 26.62 ng/ml

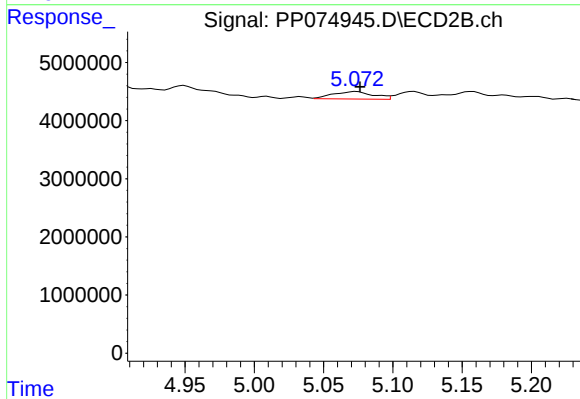

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: -0.003 min
Response: 2618962
Conc: 22.14 ng/ml

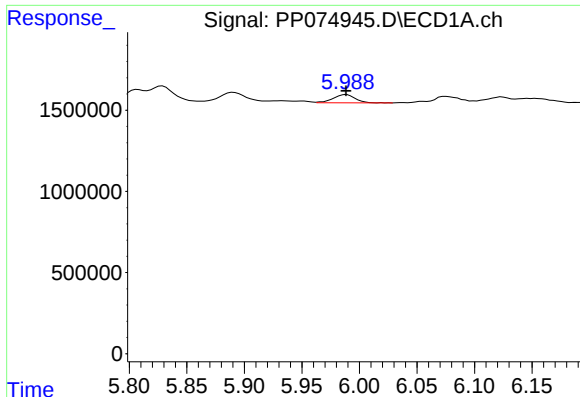

#19 AR-1242-4


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 674946
Conc: 21.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

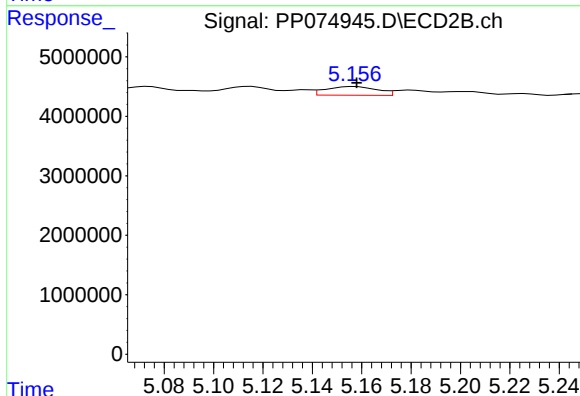


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 2113045
Conc: 12.35 ng/ml

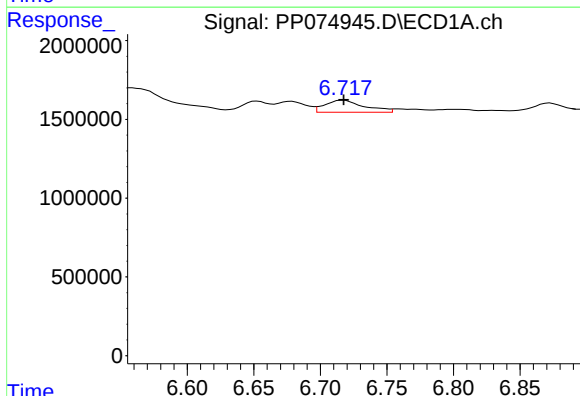


#20 AR-1242-5

R.T.: 6.718 min
Delta R.T.: 0.000 min
Response: 1585199
Conc: 43.95 ng/ml

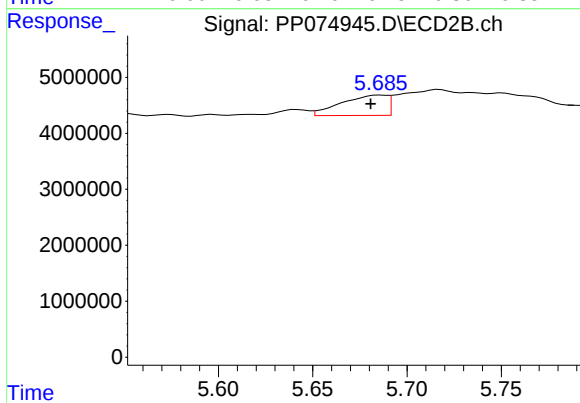

#20 AR-1242-5


R.T.: 5.686 min
Delta R.T.: 0.005 min
Response: 6043103
Conc: 32.64 ng/ml

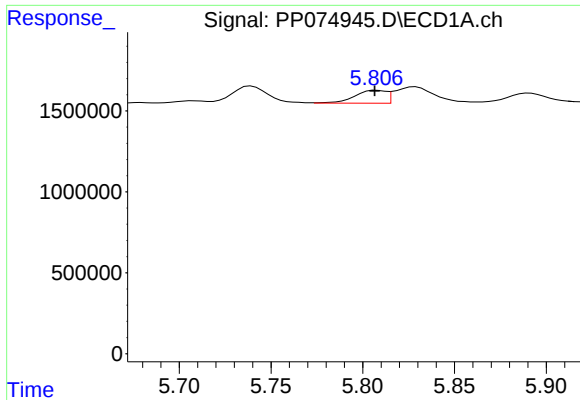

#21 AR-1248-1


R.T.: 5.808 min
Delta R.T.: 0.001 min
Response: 949296
Conc: 31.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

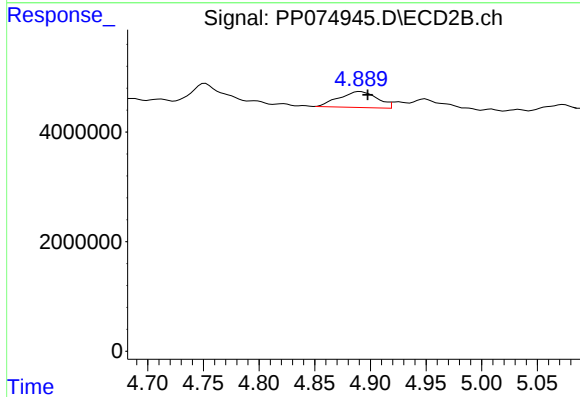


#21 AR-1248-1

R.T.: 4.891 min
Delta R.T.: -0.007 min
Response: 6943942
Conc: 25.15 ng/ml

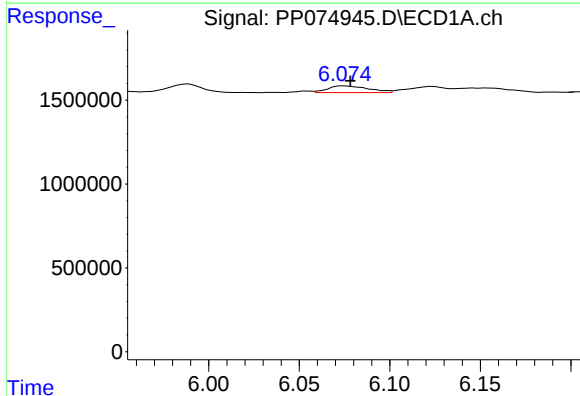


#22 AR-1248-2

R.T.: 6.075 min
Delta R.T.: -0.003 min
Response: 632352
Conc: 14.67 ng/ml

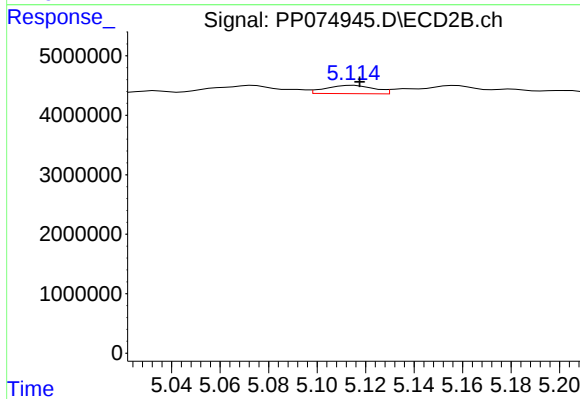

#22 AR-1248-2


R.T.: 5.115 min
Delta R.T.: -0.003 min
Response: 1945463
Conc: 11.01 ng/ml

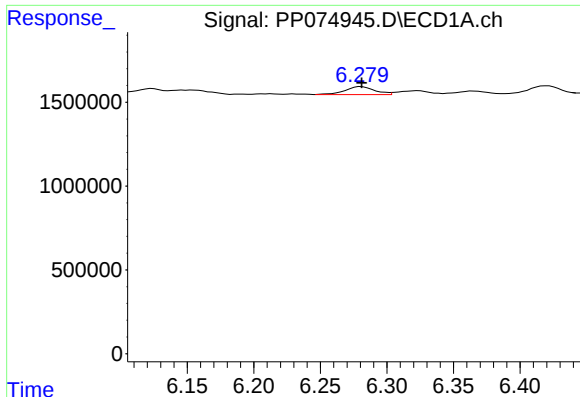

#23 AR-1248-3


R.T.: 6.281 min
Delta R.T.: 0.000 min
Response: 749801
Conc: 16.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

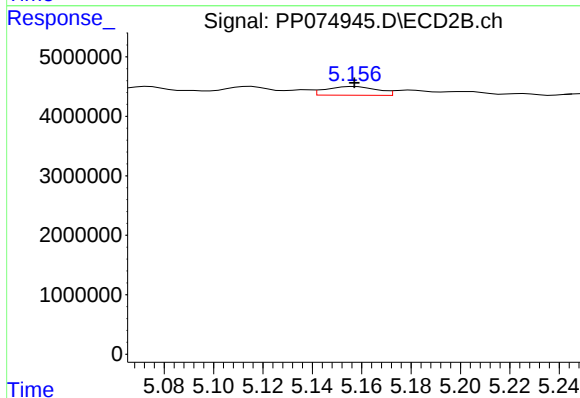


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 2113045
Conc: 9.30 ng/ml

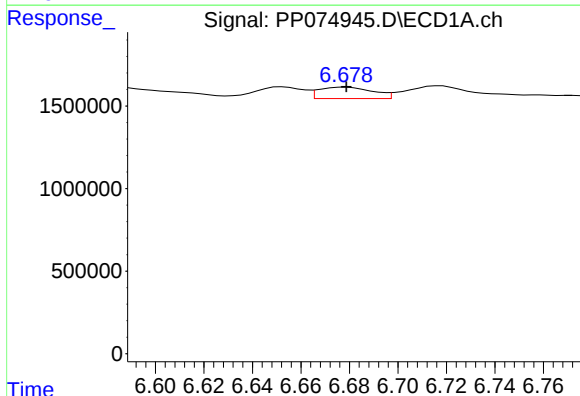


#24 AR-1248-4

R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 1063396
Conc: 19.33 ng/ml

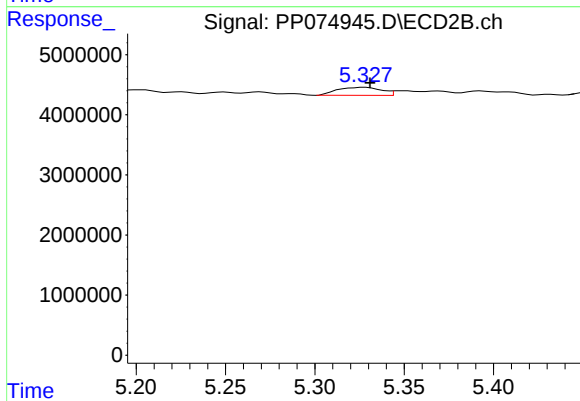

#24 AR-1248-4


R.T.: 5.328 min
Delta R.T.: -0.003 min
Response: 2305336
Conc: 10.57 ng/ml

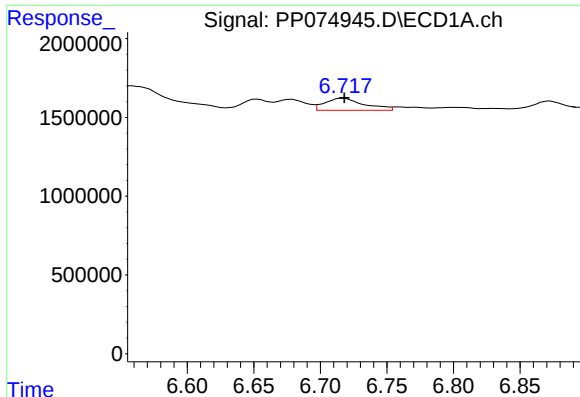

#25 AR-1248-5


R.T.: 6.718 min
Delta R.T.: 0.000 min
Response: 1585199
Conc: 28.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

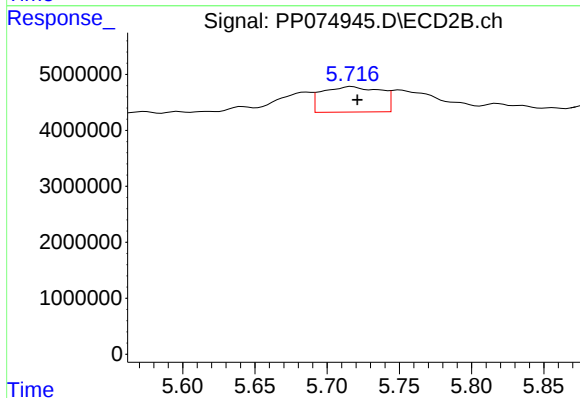


#25 AR-1248-5

R.T.: 5.717 min
Delta R.T.: -0.004 min
Response: 12796305
Conc: 34.84 ng/ml

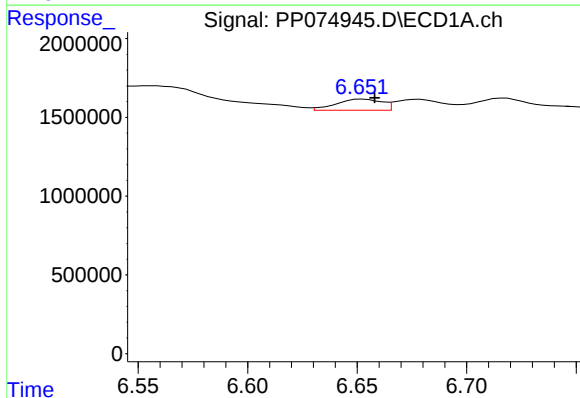


#26 AR-1254-1

R.T.: 6.652 min
Delta R.T.: -0.006 min
Response: 1023674
Conc: 17.57 ng/ml

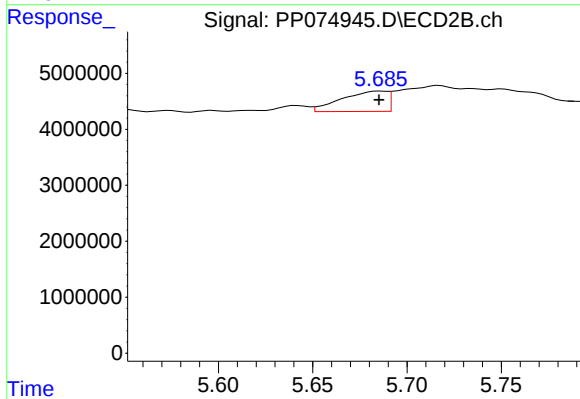

#26 AR-1254-1


R.T.: 5.686 min
Delta R.T.: 0.001 min
Response: 6043103
Conc: 12.68 ng/ml

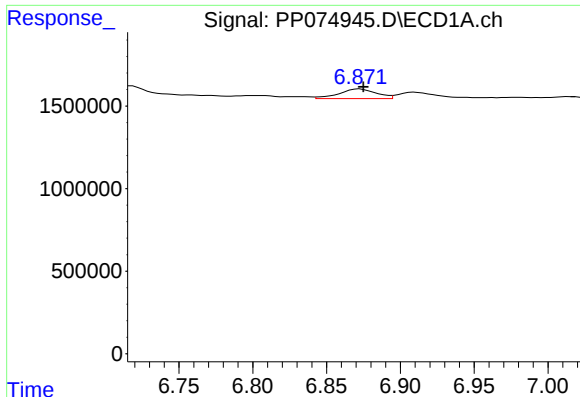

#27 AR-1254-2


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 1023430
Conc: 12.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

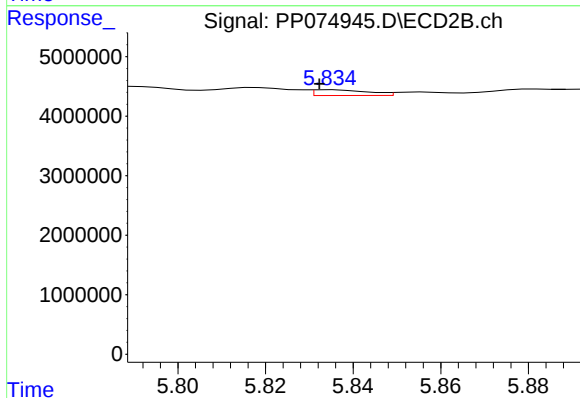


#27 AR-1254-2

R.T.: 5.835 min
Delta R.T.: 0.003 min
Response: 853211
Conc: 2.42 ng/ml

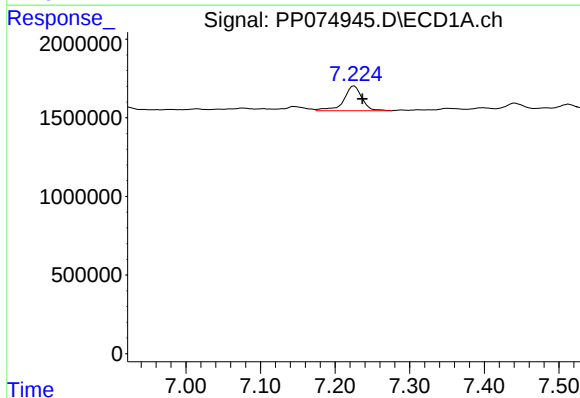


#28 AR-1254-3

R.T.: 7.226 min
Delta R.T.: -0.011 min
Response: 2650995
Conc: 29.72 ng/ml

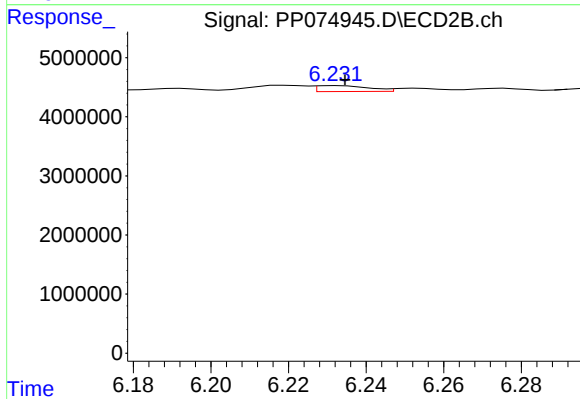

#28 AR-1254-3


R.T.: 6.233 min
Delta R.T.: -0.002 min
Response: 938929
Conc: 1.51 ng/ml

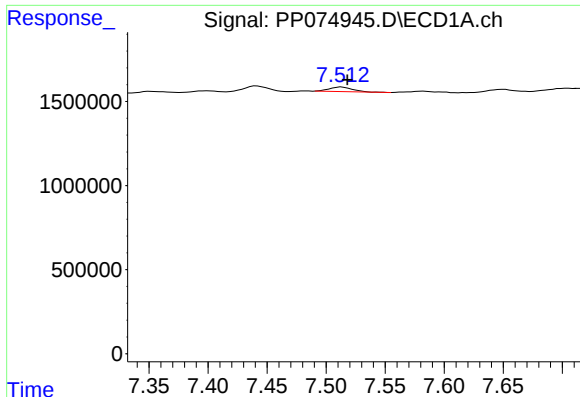

#29 AR-1254-4


R.T.: 7.513 min
Delta R.T.: -0.005 min
Response: 374830
Conc: 5.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

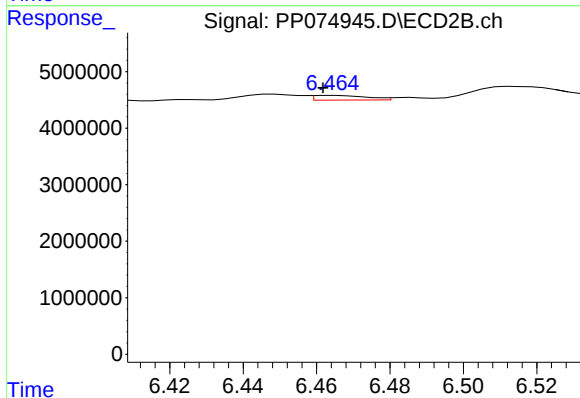


#29 AR-1254-4

R.T.: 6.464 min
Delta R.T.: 0.002 min
Response: 841006
Conc: 1.79 ng/ml

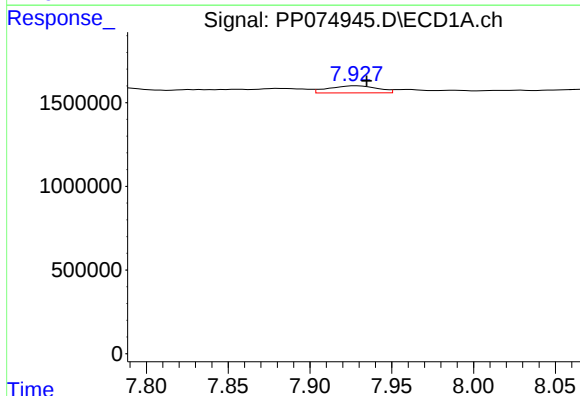


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.006 min
Response: 866436
Conc: 10.43 ng/ml

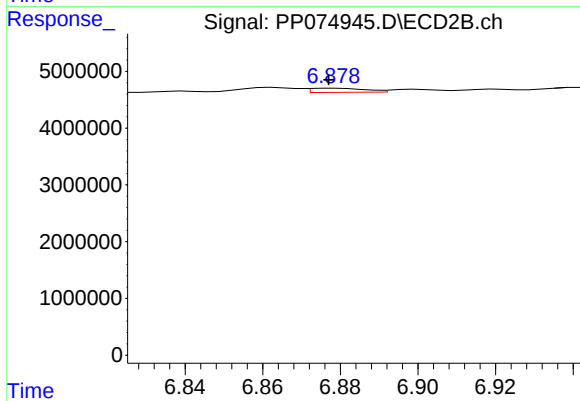

#30 AR-1254-5


R.T.: 6.879 min
Delta R.T.: 0.002 min
Response: 707351
Conc: 1.44 ng/ml

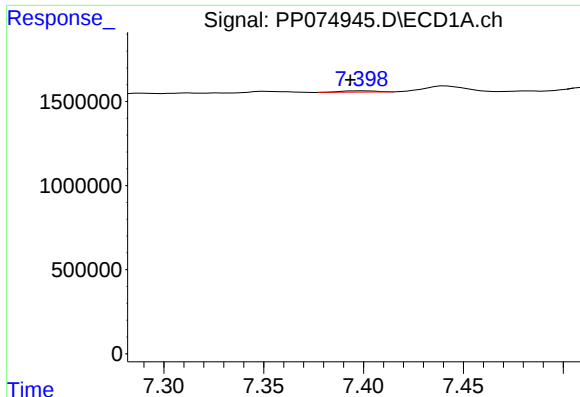

#31 AR-1260-1


R.T.: 7.399 min
Delta R.T.: 0.005 min
Response: 90850
Conc: 1.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

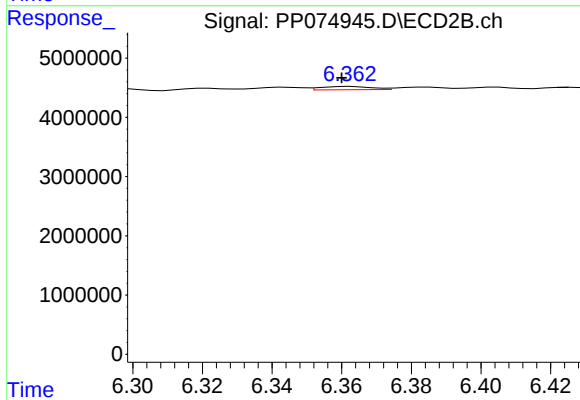


#31 AR-1260-1

R.T.: 6.363 min
Delta R.T.: 0.003 min
Response: 564269
Conc: 1.50 ng/ml

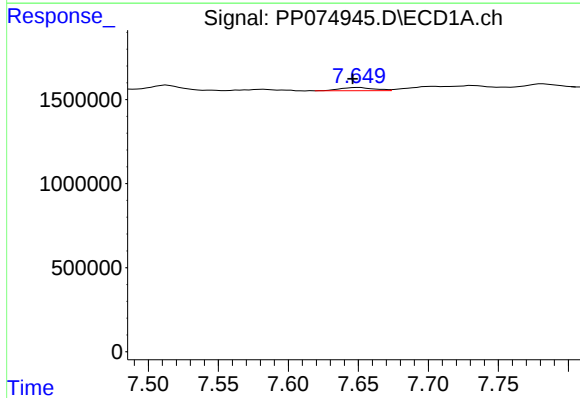


#32 AR-1260-2

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 314028
Conc: 4.56 ng/ml

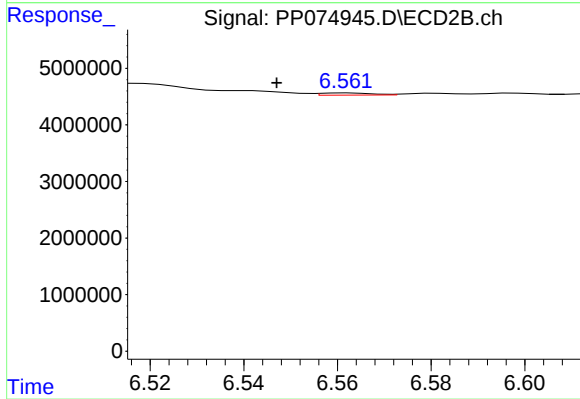

#32 AR-1260-2


R.T.: 6.562 min
Delta R.T.: 0.015 min
Response: 304310
Conc: 0.58 ng/ml

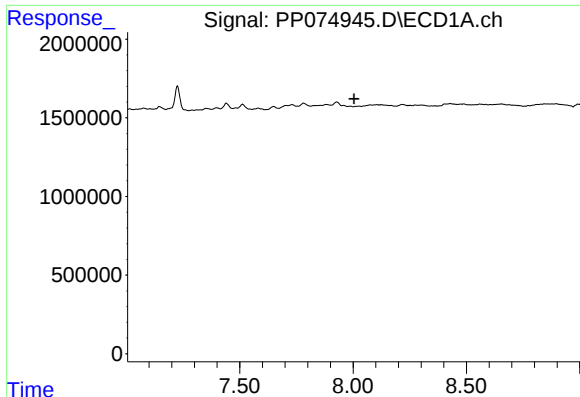

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

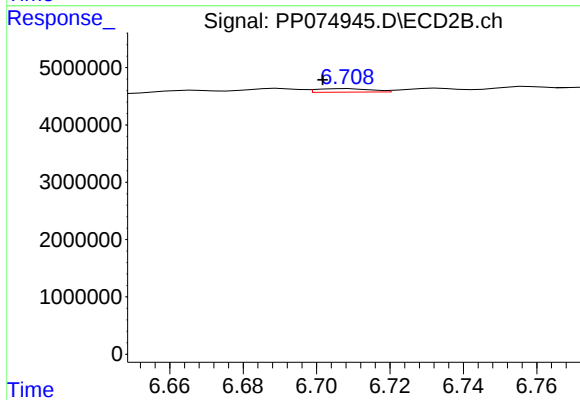


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: 0.007 min
Response: 636872
Conc: 1.47 ng/ml

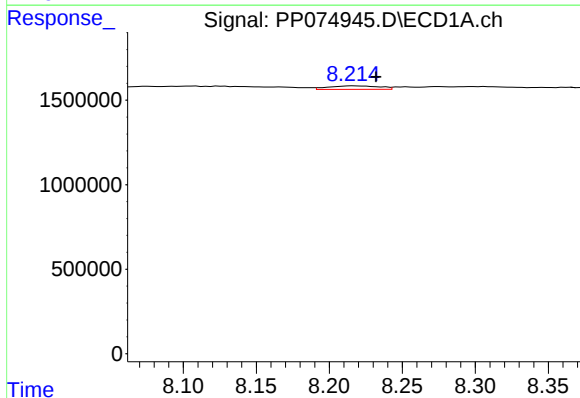


#34 AR-1260-4

R.T.: 8.216 min
Delta R.T.: -0.016 min
Response: 488274
Conc: 7.65 ng/ml

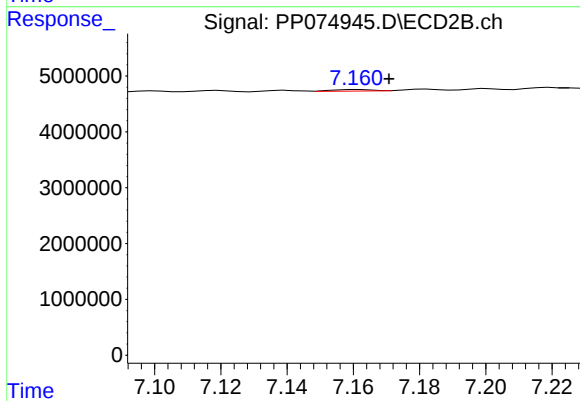

#34 AR-1260-4


R.T.: 7.162 min
Delta R.T.: -0.009 min
Response: 230238
Conc: 0.60 ng/ml

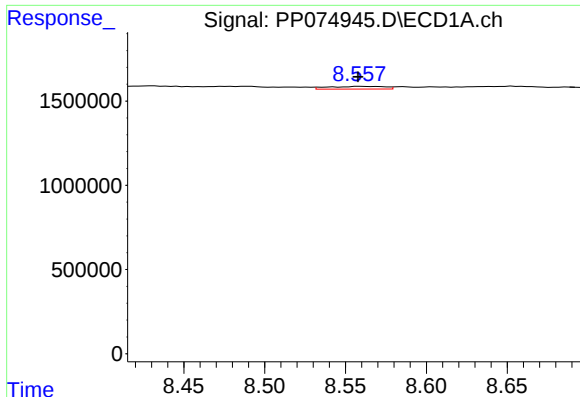

#35 AR-1260-5


R.T.: 8.559 min
Delta R.T.: 0.001 min
Response: 385196
Conc: 3.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

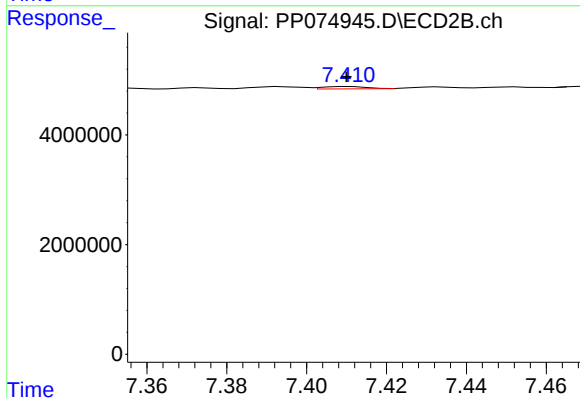


#35 AR-1260-5

R.T.: 7.411 min
Delta R.T.: 0.000 min
Response: 331185
Conc: 0.33 ng/ml

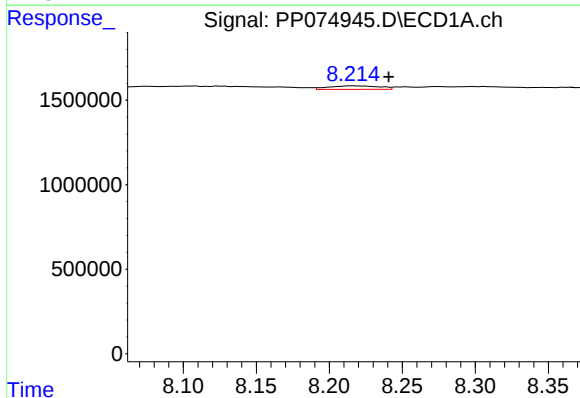


#36 AR-1262-1

R.T.: 8.216 min
Delta R.T.: -0.025 min
Response: 488274
Conc: 6.34 ng/ml

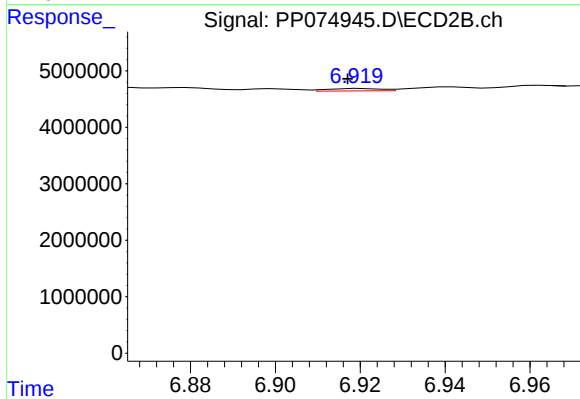

#36 AR-1262-1


R.T.: 6.920 min
Delta R.T.: 0.003 min
Response: 369795
Conc: 0.52 ng/ml

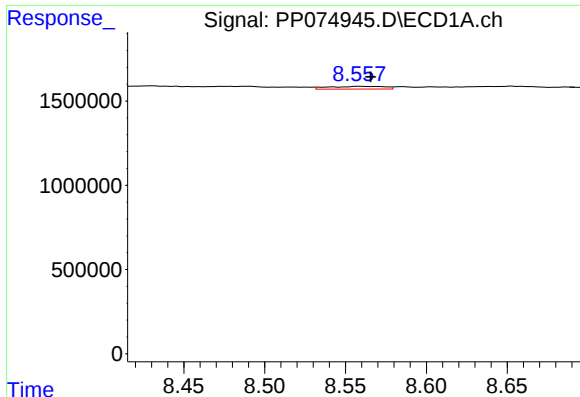

#37 AR-1262-2


R.T.: 8.559 min
Delta R.T.: -0.007 min
Response: 385196
Conc: 2.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

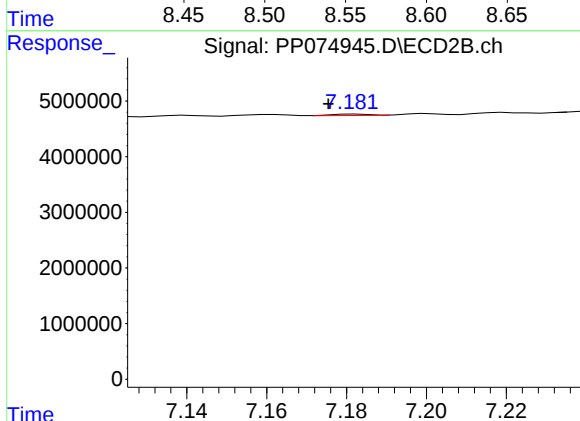


#37 AR-1262-2

R.T.: 7.182 min
Delta R.T.: 0.007 min
Response: 175056
Conc: 0.34 ng/ml

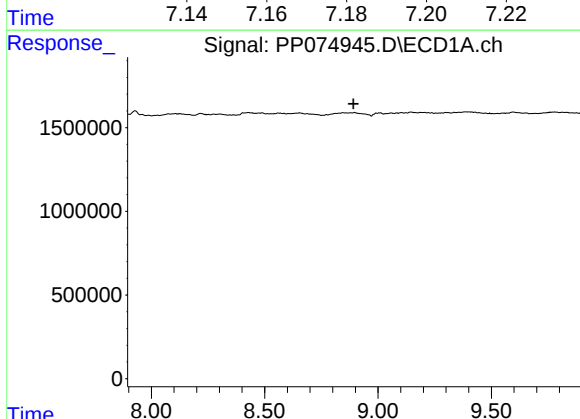


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

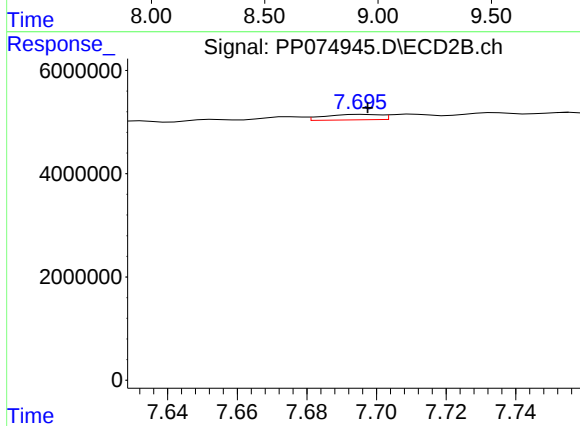

#38 AR-1262-3


R.T.: 7.696 min
Delta R.T.: -0.001 min
Response: 1182839
Conc: 2.54 ng/ml

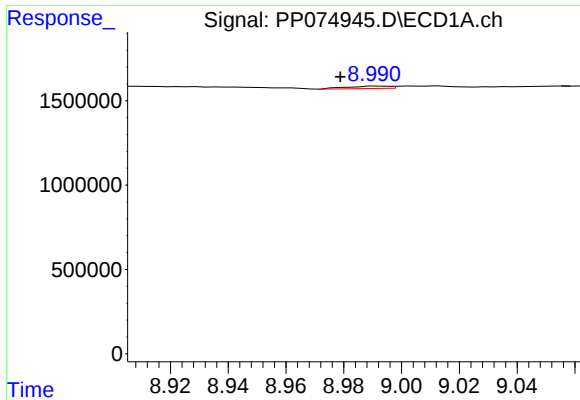

#39 AR-1262-4


R.T.: 8.992 min
Delta R.T.: 0.013 min
Response: 138220
Conc: 1.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

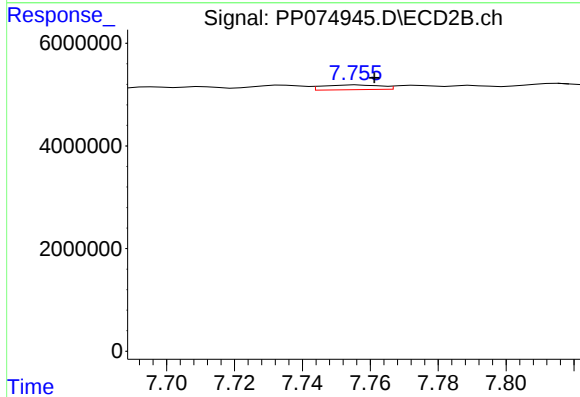


#39 AR-1262-4

R.T.: 7.756 min
Delta R.T.: -0.005 min
Response: 1096541
Conc: 1.33 ng/ml

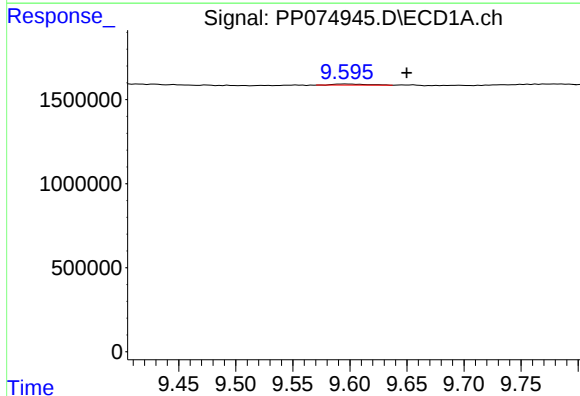


#40 AR-1262-5

R.T.: 9.596 min
Delta R.T.: -0.054 min
Response: 140356
Conc: 2.30 ng/ml

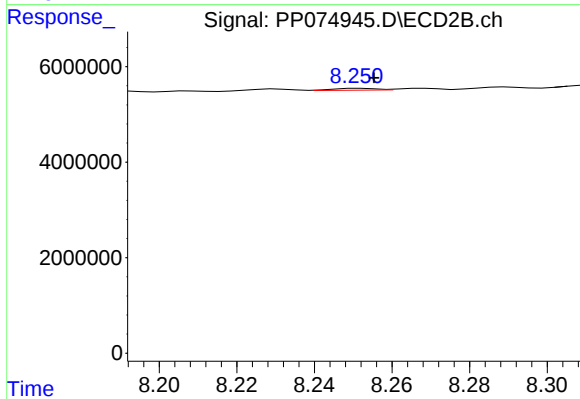

#40 AR-1262-5


R.T.: 8.252 min
Delta R.T.: -0.004 min
Response: 287398
Conc: 0.80 ng/ml

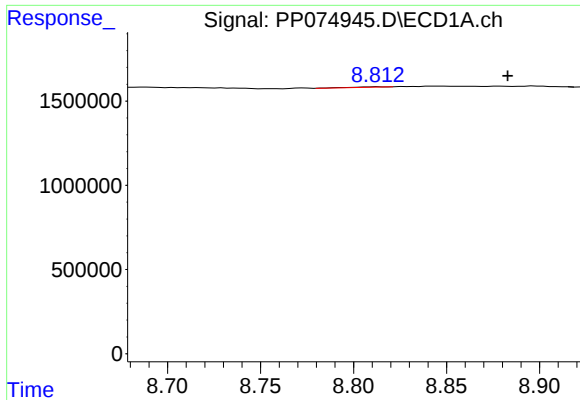

#41 AR-1268-1


R.T.: 8.813 min
Delta R.T.: -0.070 min
Response: 33290
Conc: 0.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

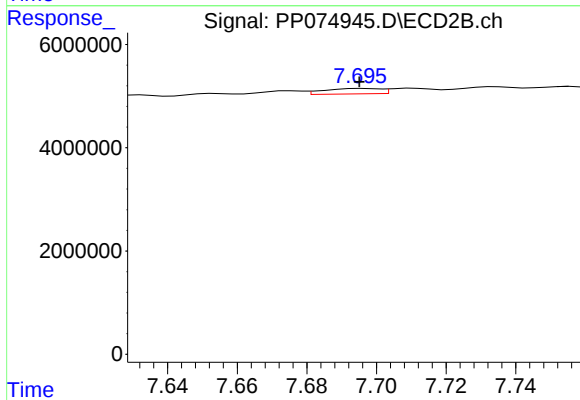


#41 AR-1268-1

R.T.: 7.696 min
Delta R.T.: 0.001 min
Response: 1182839
Conc: 0.84 ng/ml

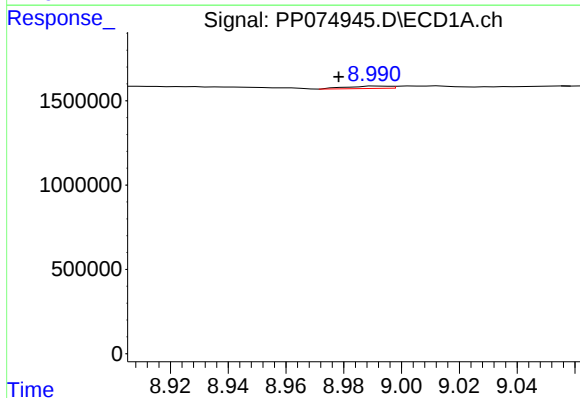


#42 AR-1268-2

R.T.: 8.992 min
Delta R.T.: 0.013 min
Response: 138220
Conc: 0.94 ng/ml

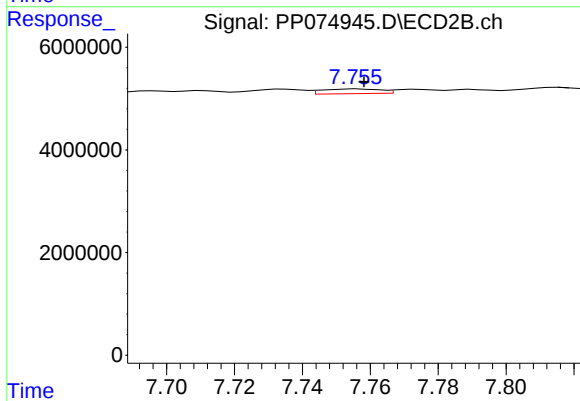

#42 AR-1268-2


R.T.: 7.756 min
Delta R.T.: -0.002 min
Response: 1096541
Conc: 0.80 ng/ml

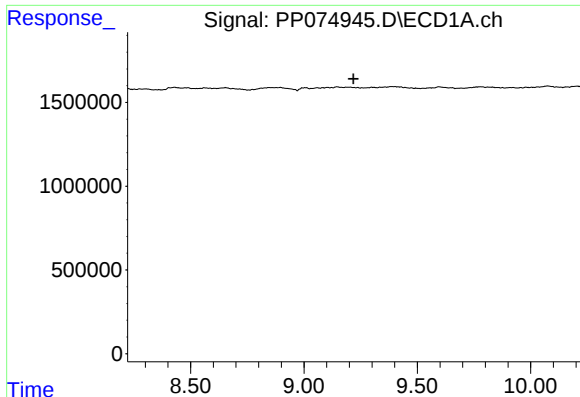

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

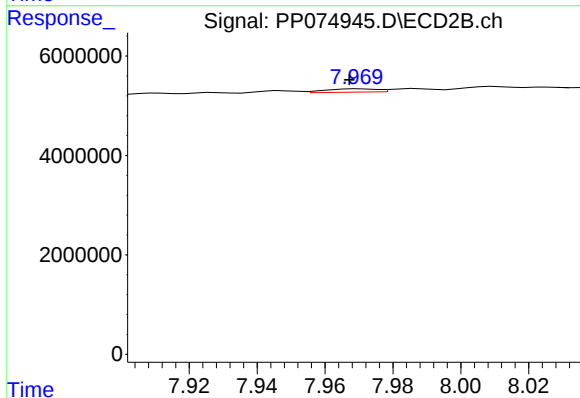


#43 AR-1268-3

R.T.: 7.970 min
Delta R.T.: 0.003 min
Response: 683335
Conc: 0.66 ng/ml

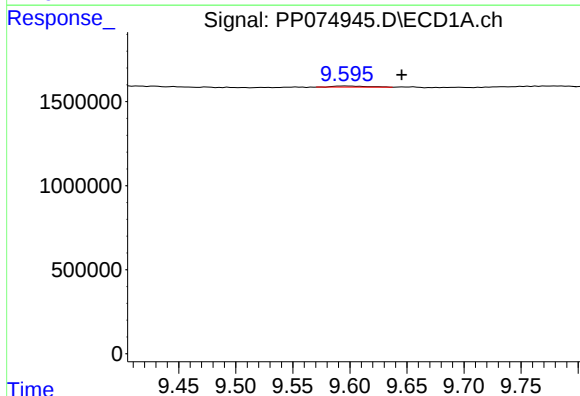


#44 AR-1268-4

R.T.: 9.596 min
Delta R.T.: -0.049 min
Response: 140356
Conc: 2.09 ng/ml

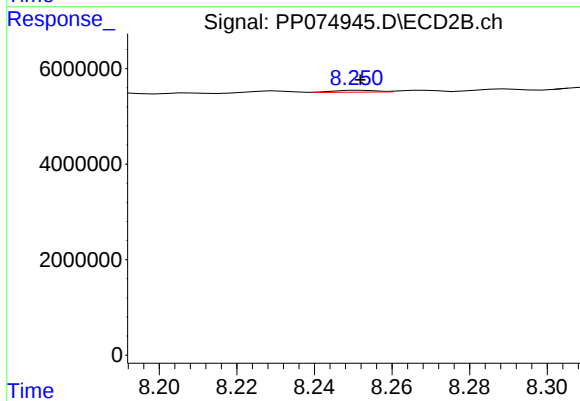

#44 AR-1268-4


R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 287398
Conc: 0.75 ng/ml

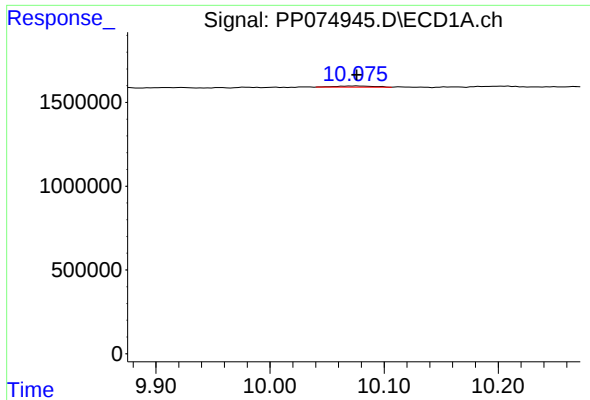

#45 AR-1268-5

R.T.: 10.076 min
Delta R.T.: 0.000 min
Response: 162325
Conc: 0.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
MDL-WATER-03-QT3-2025

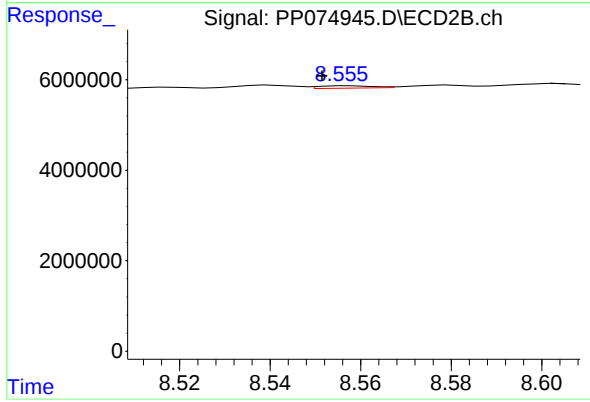

#45 AR-1268-5

R.T.: 8.558 min
Delta R.T.: 0.006 min
Response: 428178
Conc: 0.14 ng/ml