

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090825\
 Data File : PP074972.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Sep 2025 20:24
 Operator : YP\AJ
 Sample : Q3043-03 10X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC258874-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/09/2025
 Supervised By :mohammad ahmed 09/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 09 06:09:38 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.655	3.795	3062149	6721988	2.502	1.390m#
2) SA Decachlor...	10.426	8.806	2234776	11235404	2.263m	1.498 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090825\
Data File : PP074972.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Sep 2025 20:24
Operator : YP\AJ
Sample : Q3043-03 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC258874-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/09/2025
Supervised By :mohammad ahmed 09/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 09 06:09:38 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

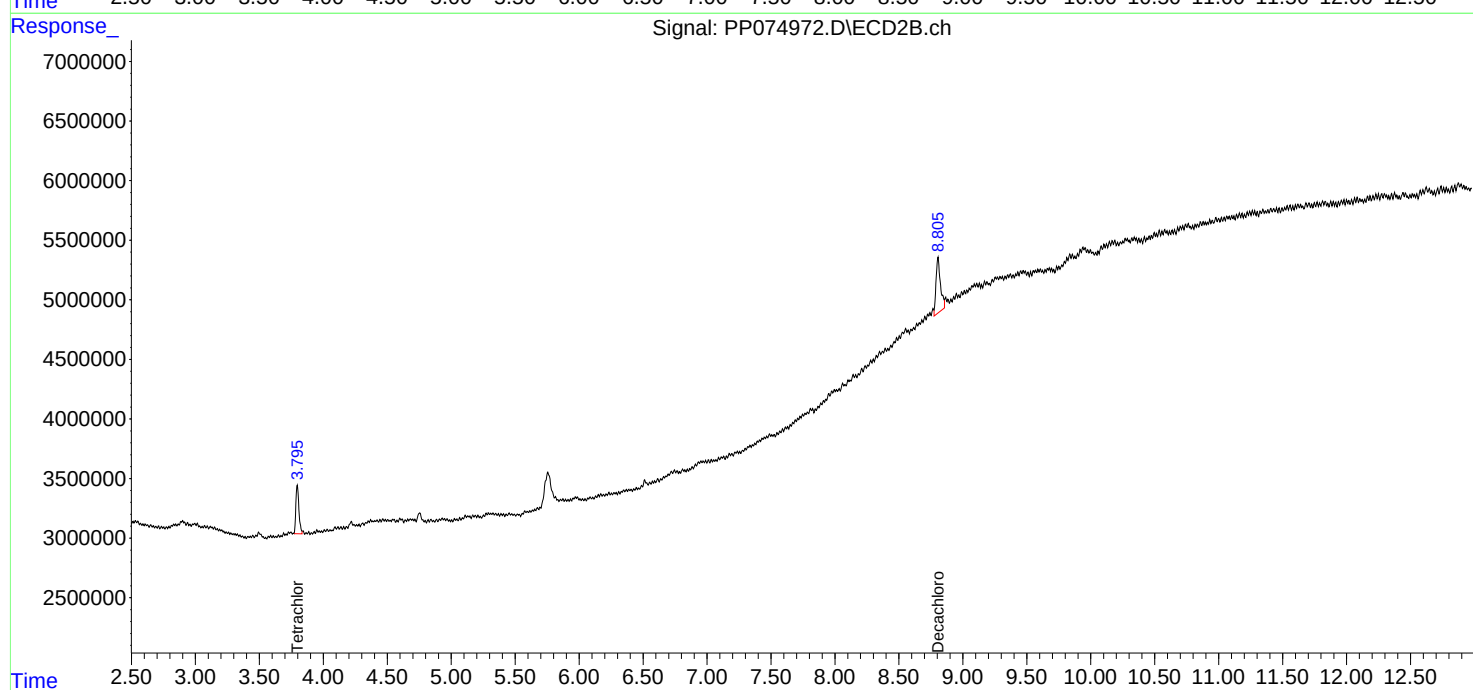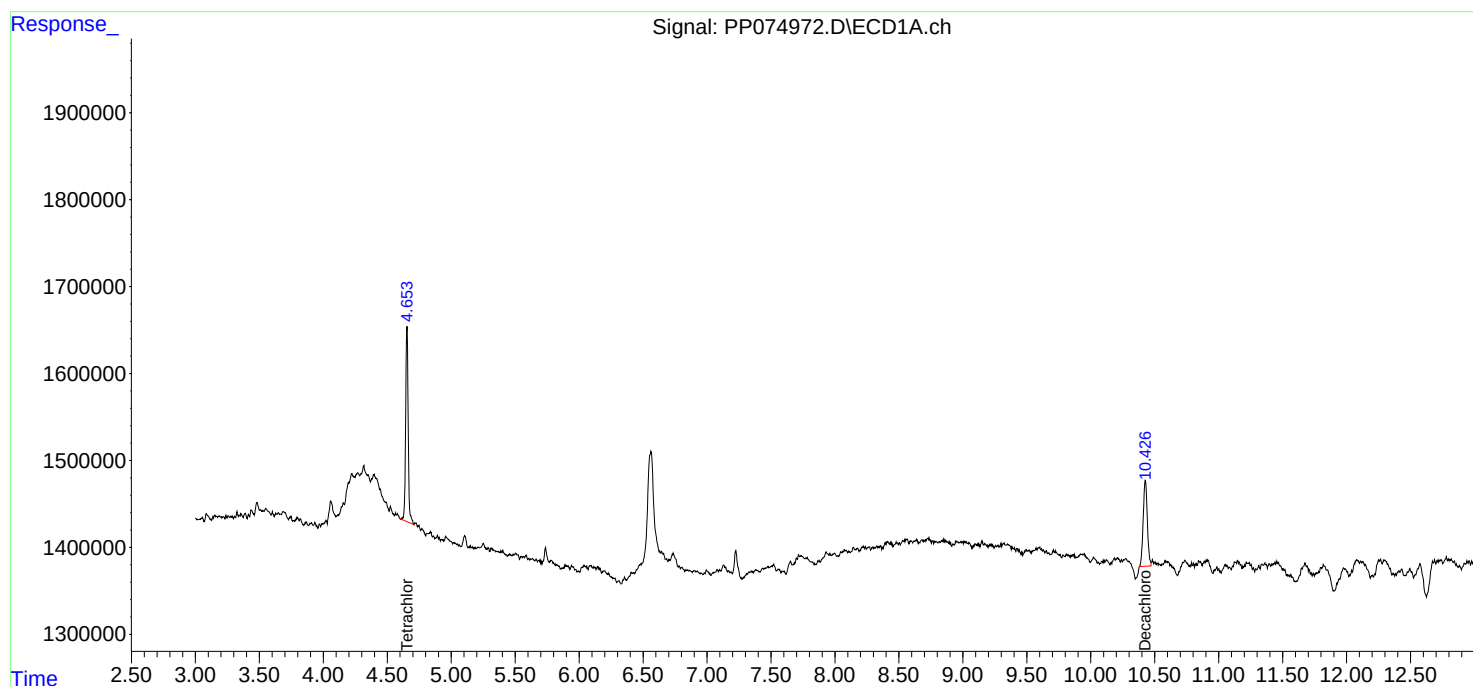

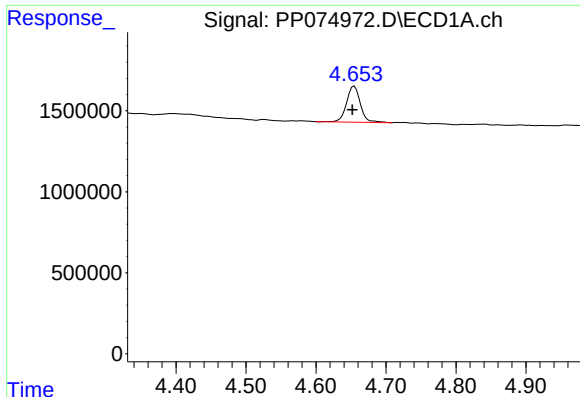


#1 Tetrachloro-m-xylene

R.T.: 4.655 min
Delta R.T.: 0.003 min
Response: 3062149
Conc: 2.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258874-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/09/2025
Supervised By :mohammad ahmed 09/12/2025

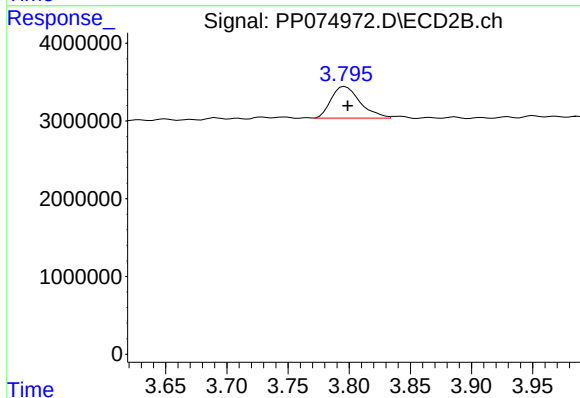


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: -0.004 min
Response: 6721988
Conc: 1.39 ng/ml m

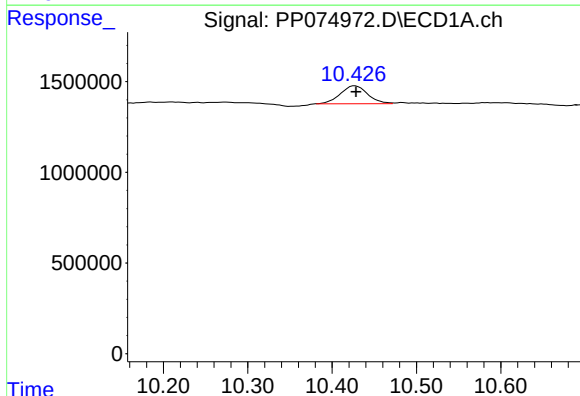

#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.003 min
Response: 2234776
Conc: 2.26 ng/ml m

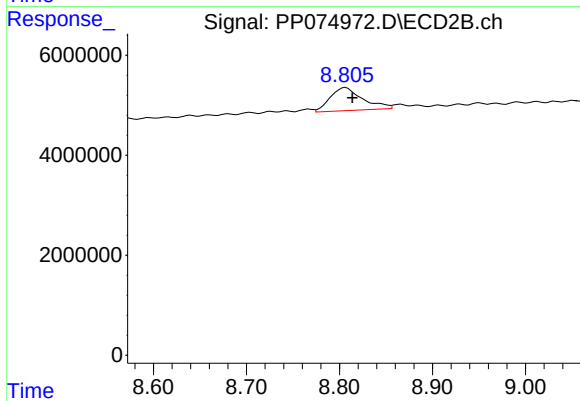

#2 Decachlorobiphenyl

R.T.: 8.806 min
Delta R.T.: -0.007 min
Response: 11235404
Conc: 1.50 ng/ml