

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090921\
 Data File : PP039278.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 09 Sep 2021 19:16
 Operator : AJ\MA
 Sample : M3671-01
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FILTER-MEDIA-FILTERS

Manual Integrations
 APPROVED

mohammad
 9/10/2021 10:57:18 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 05:06:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Sep 03 04:15:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.867	3.853	110611	68265	2.887m	2.846
2) SA Decachlor...	10.839	9.087f	922950	126415	28.039	5.776 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090921\
Data File : PP039278.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 09 Sep 2021 19:16
Operator : AJ\MA
Sample : M3671-01
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FILTER-MEDIA-FILTERS


Manual Integrations
APPROVED

mohammad
9/10/2021 10:57:18 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 05:06:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP090221.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Sep 03 04:15:14 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

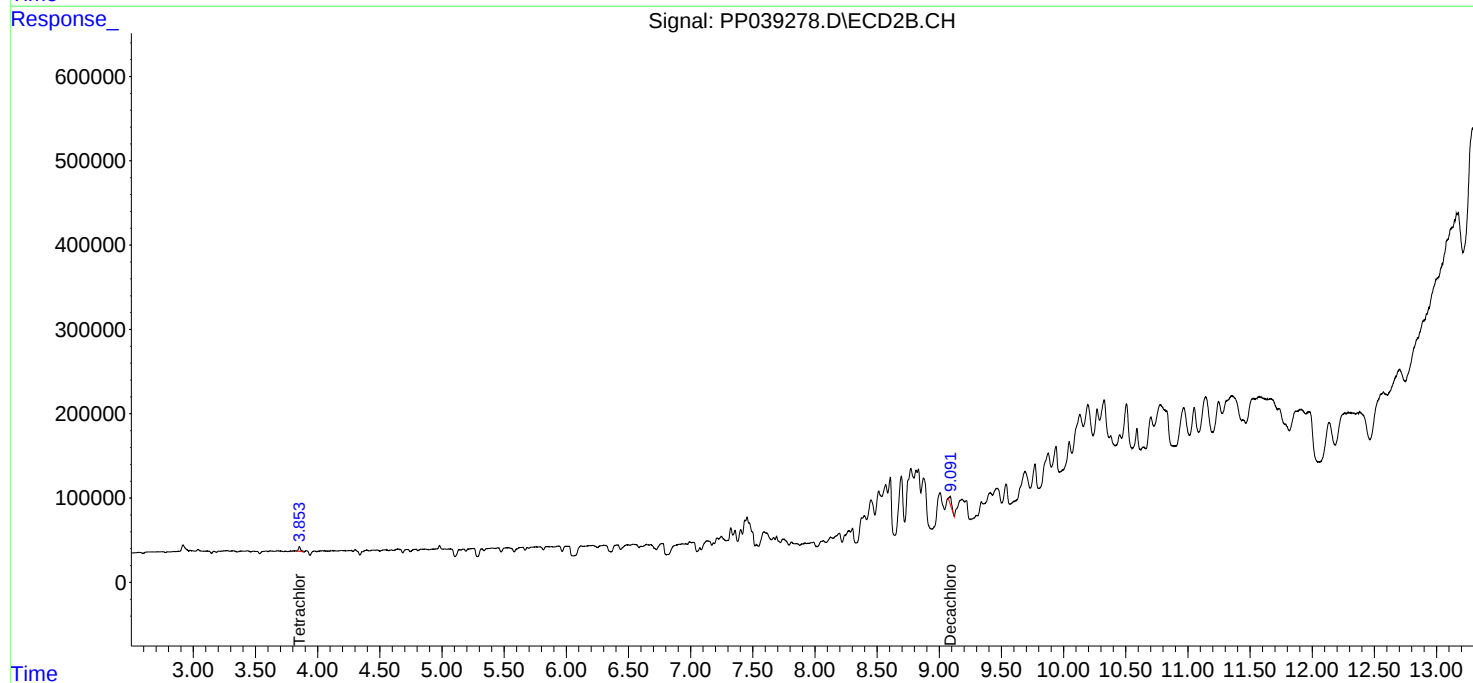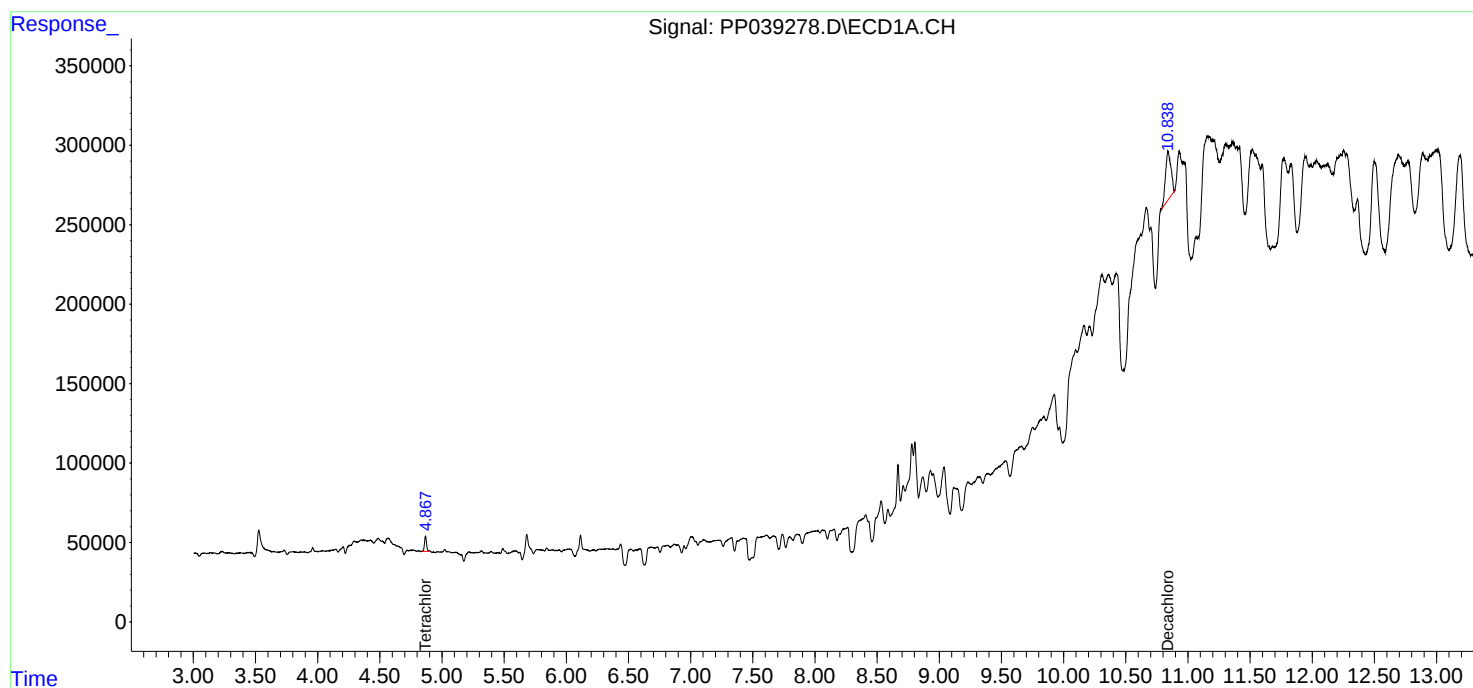

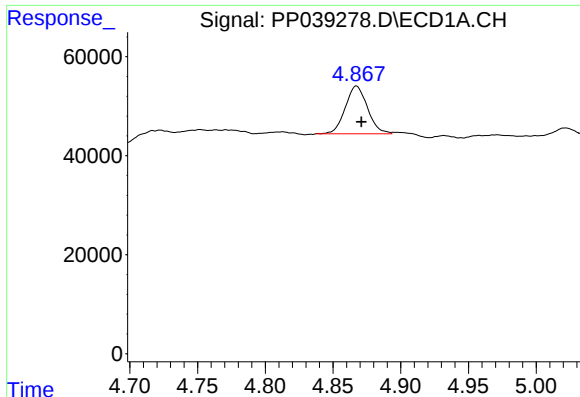


#1 Tetrachloro-m-xylene

R.T.: 4.867 min
Delta R.T.: -0.004 min
Response: 110611
Conc: 2.89 ng/ml m

Instrument :
ECD_P
ClientSampleId :
FILTER-MEDIA-FILTERS


Manual Integrations
APPROVED

mohammad
9/10/2021 10:57:18 AM

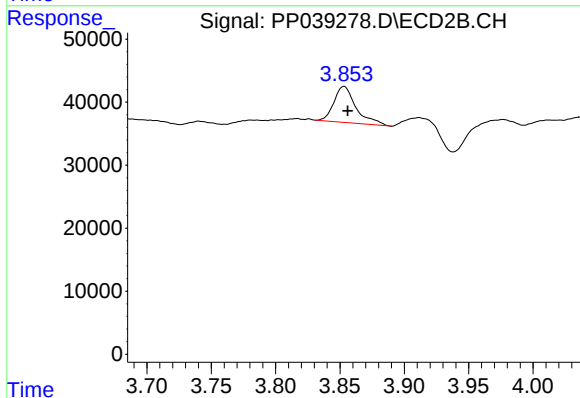


#1 Tetrachloro-m-xylene

R.T.: 3.853 min
Delta R.T.: -0.003 min
Response: 68265
Conc: 2.85 ng/ml

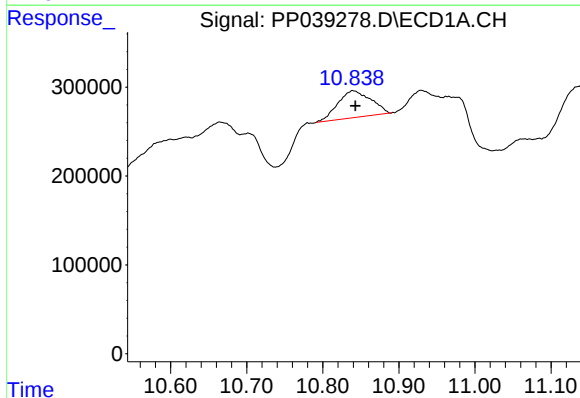

#2 Decachlorobiphenyl

R.T.: 10.839 min
Delta R.T.: -0.003 min
Response: 922950
Conc: 28.04 ng/ml

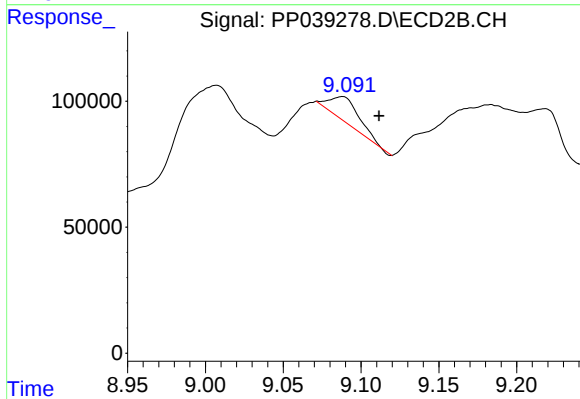

#2 Decachlorobiphenyl

R.T.: 9.087 min
Delta R.T.: -0.025 min
Response: 126415
Conc: 5.78 ng/ml