

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075002.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 13:36
 Operator : YP\AJ
 Sample : Q3034-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:48:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	3.800	26350497	97438013	21.534	20.151
2)	SA Decachlor...	10.429	8.808	21833882	130.7E6	22.110	17.432
Target Compounds							
3)	L1 AR-1016-1	5.805	4.896	3479417	28670469	78.918	56.288 #
4)	L1 AR-1016-2	5.826	4.955	5517998	13921176	87.808	58.489 #
5)	L1 AR-1016-3	5.889	5.074	4115962	9483505	91.641	68.769
6)	L1 AR-1016-4	5.986	5.115	3770586	11052108	107.174	79.055 #
7)	L1 AR-1016-5	6.279	5.330	4571986	15688686	137.768	94.463 #
8)	L2 AR-1221-1	4.852	4.014	1863950	427956	105.949	6.917 #
9)	L2 AR-1221-2	4.955	4.097	532928	2037481	39.898	45.065
10)	L2 AR-1221-3	5.016	4.169	174560	632208	4.604	3.848
11)	L3 AR-1232-1	5.016	4.169	174560	632208	5.747	4.935
12)	L3 AR-1232-2	5.540	4.896	1737008	28670469	110.229	123.690
13)	L3 AR-1232-3	5.826	5.074	5517998	9483505	180.659	157.901
14)	L3 AR-1232-4	5.986	5.158	3770586	18149005	218.341	246.230
15)	L3 AR-1232-5	6.076	5.330	3636794	15688686	280.164	252.702
16)	L4 AR-1242-1	5.805	4.896	3479417	28670469	90.905	67.979 #
17)	L4 AR-1242-2	5.826	4.955	5517998	13921176	97.695	69.508 #
18)	L4 AR-1242-3	5.889	5.074	4115962	9483505	101.371	80.166
19)	L4 AR-1242-4	5.986	5.158	3770586	18149005	118.789	106.036
20)	L4 AR-1242-5	6.715	5.679	3015388	13824388	83.597	74.660
21)	L5 AR-1248-1	5.805	4.896	3479417	28670469	115.121	103.825
22)	L5 AR-1248-2	6.076	5.115	3636794	11052108	84.388	62.528 #
23)	L5 AR-1248-3	6.279	5.158	4571986	18149005	97.894	79.880
24)	L5 AR-1248-4	6.676	5.330	2687345	15688686	48.860	71.960 #
25)	L5 AR-1248-5	6.715	5.721	3015388	12909829	54.360	35.146 #
26)	L6 AR-1254-1	6.651	5.679	2526317	13824388	43.356	29.000 #
27)	L6 AR-1254-2	6.872	5.820	1892751	2935738	23.191	8.337 #
28)	L6 AR-1254-3	7.226	6.230	538824	792334	6.040	1.278 #
29)	L6 AR-1254-4	7.516	6.455	334685	170313	5.078	0.363 #
30)	L6 AR-1254-5	7.918	6.874	559837	267057	6.738	0.544 #
31)	L7 AR-1260-1	0.000	6.358	0	359409	N.D.	0.958 #
32)	L7 AR-1260-2	7.651	6.543	390608	575726	5.668	1.089 #
33)	L7 AR-1260-3	8.000	6.704	104464	238755	2.013	0.551 #
34)	L7 AR-1260-4	8.246	7.178	207319	405676	3.250	1.063 #
35)	L7 AR-1260-5	8.558	7.419	45165	217302	0.398	0.216 #
36)	L8 AR-1262-1	8.246	6.915	207319	187093	2.692	0.265 #
37)	L8 AR-1262-2	8.558	7.178	45165	405676	0.341	0.779 #
38)	L8 AR-1262-3	0.000	7.694	0	458647	N.D.	0.984 #
39)	L8 AR-1262-4	8.973	7.754	149115	685040	1.979	0.834 #
40)	L8 AR-1262-5	9.606f	8.259	154426	390780	2.533	1.091 #
41)	L9 AR-1268-1	0.000	7.694	0	458647	N.D.	0.325 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 13:36
Operator : YP\AJ
Sample : Q3034-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:48:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.973	7.754	149115	685040	1.016	0.502 #
43)	L9 AR-1268-3	0.000	7.967	0	671001	N.D.	0.643 #
44)	L9 AR-1268-4	9.606f	8.259	154426	390780	2.296	1.020 #
45)	L9 AR-1268-5	10.076	8.550	107377	655156	0.290	0.209 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075002.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 13:36
Operator : YP\AJ
Sample : Q3034-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:48:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

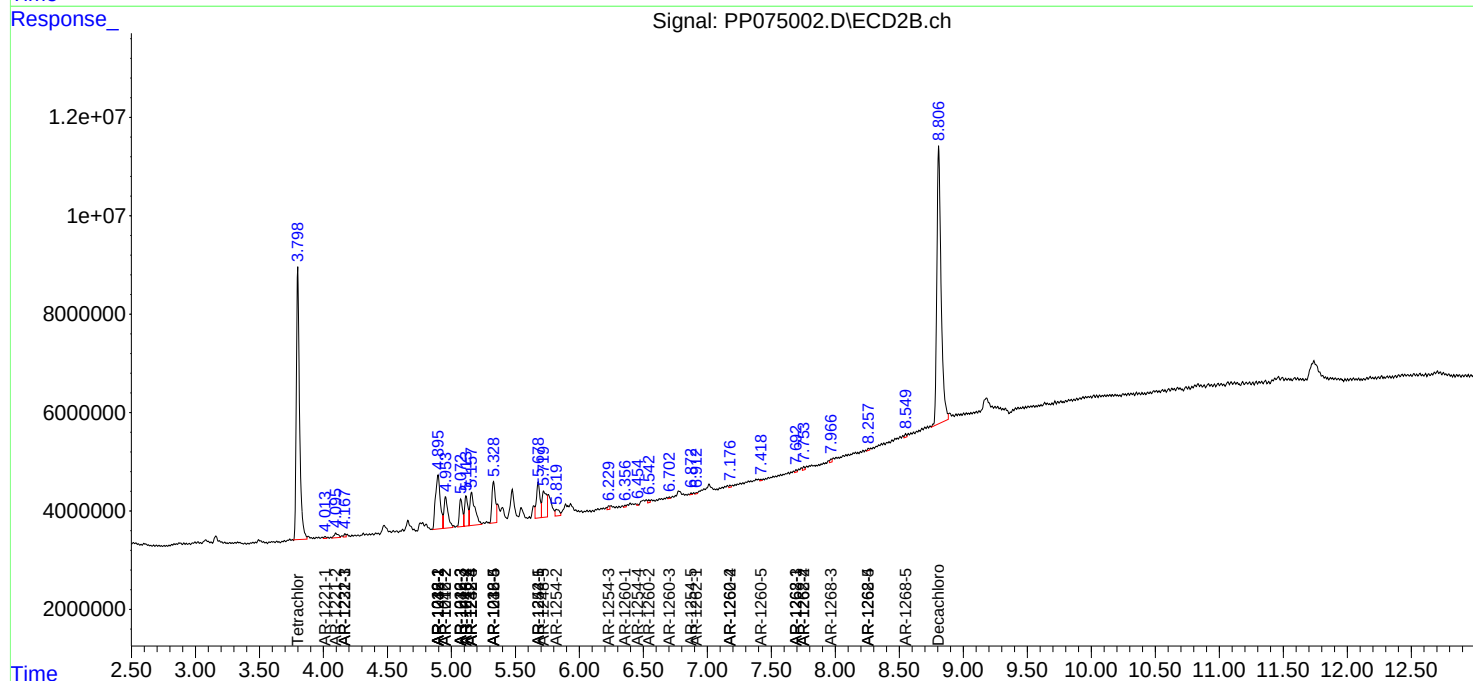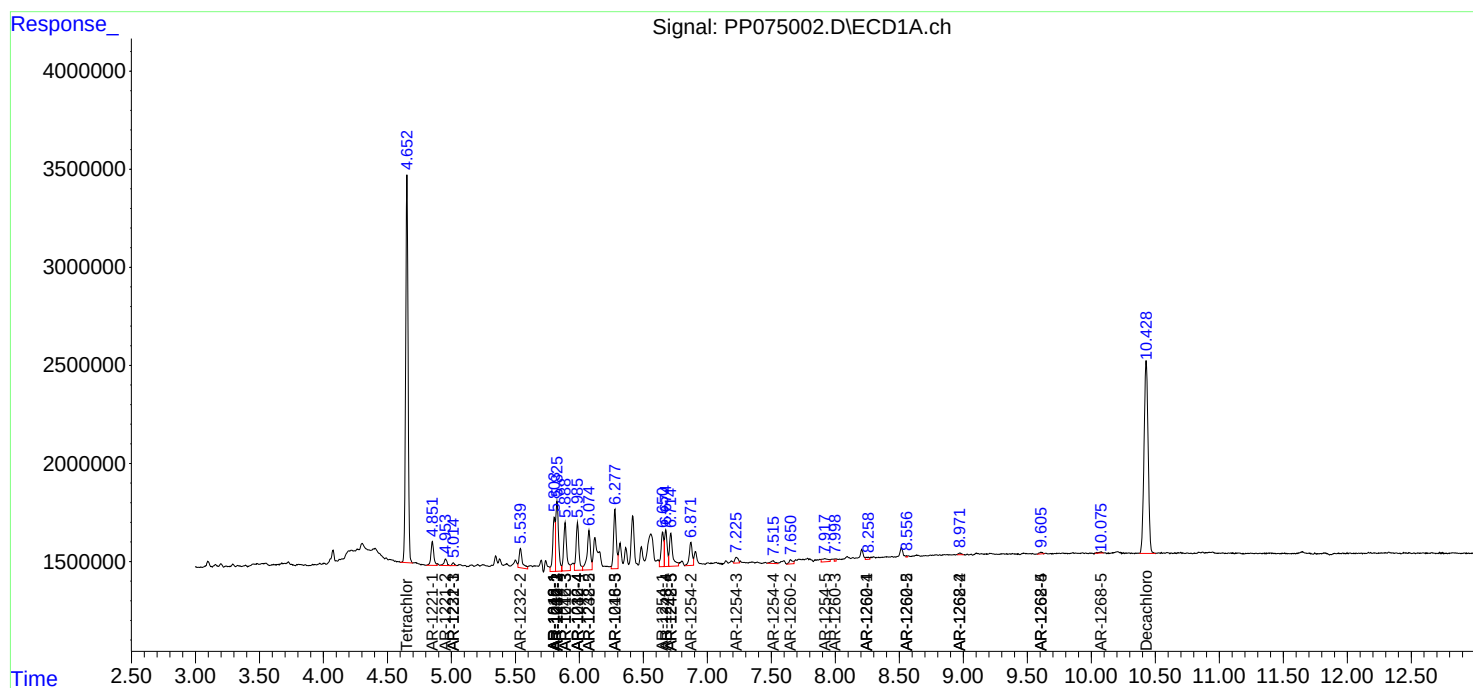


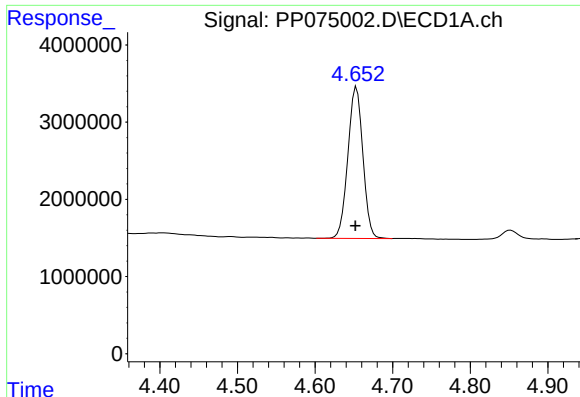

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.002 min
Response: 26350497
Conc: 21.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

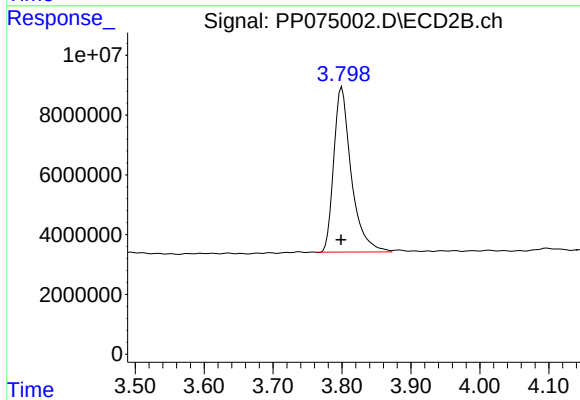


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.001 min
Response: 97438013
Conc: 20.15 ng/ml

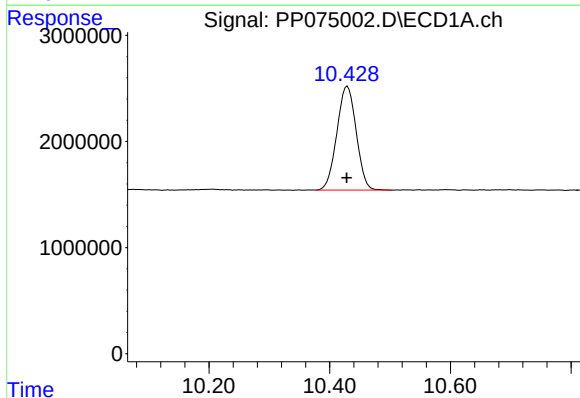


#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: 0.001 min
Response: 21833882
Conc: 22.11 ng/ml

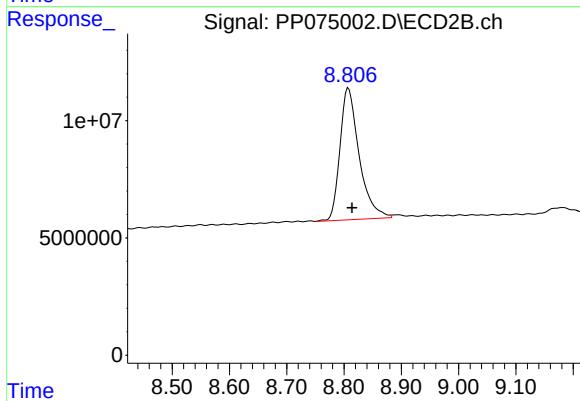

#2 Decachlorobiphenyl


R.T.: 8.808 min
Delta R.T.: -0.006 min
Response: 130729344
Conc: 17.43 ng/ml

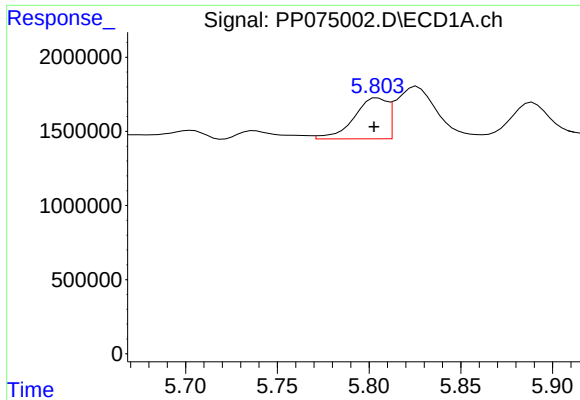

#3 AR-1016-1


R.T.: 5.805 min
Delta R.T.: 0.002 min
Response: 3479417
Conc: 78.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

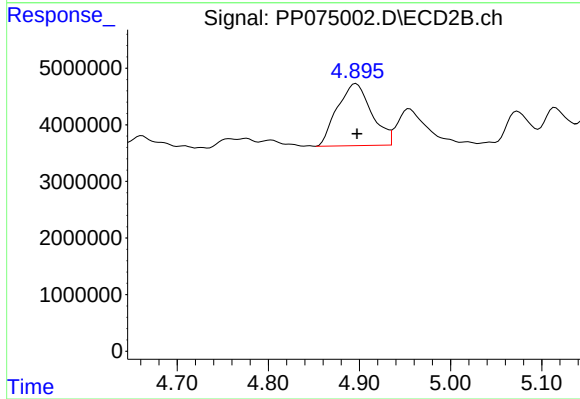


#3 AR-1016-1

R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 28670469
Conc: 56.29 ng/ml

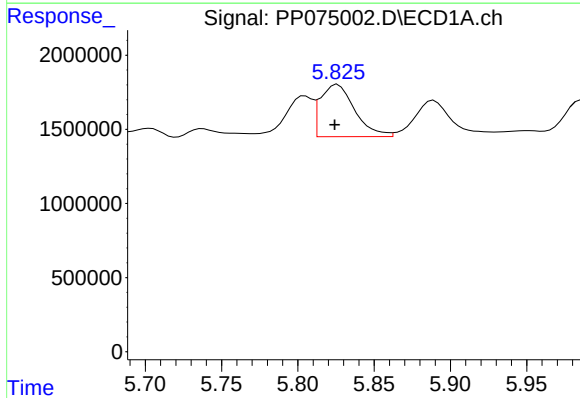


#4 AR-1016-2

R.T.: 5.826 min
Delta R.T.: 0.002 min
Response: 5517998
Conc: 87.81 ng/ml

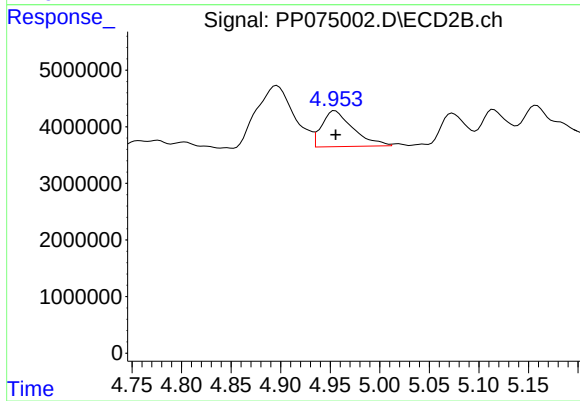

#4 AR-1016-2


R.T.: 4.955 min
Delta R.T.: 0.000 min
Response: 13921176
Conc: 58.49 ng/ml

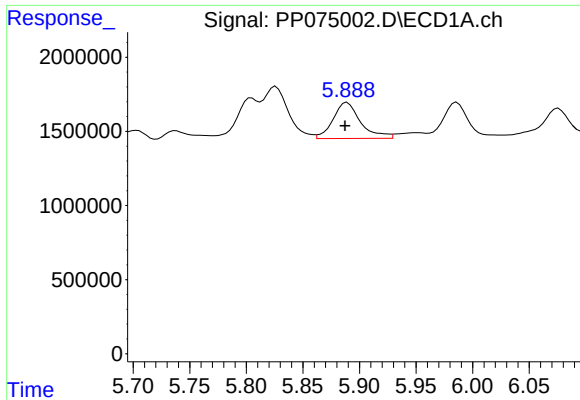

#5 AR-1016-3


R.T.: 5.889 min
Delta R.T.: 0.002 min
Response: 4115962
Conc: 91.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

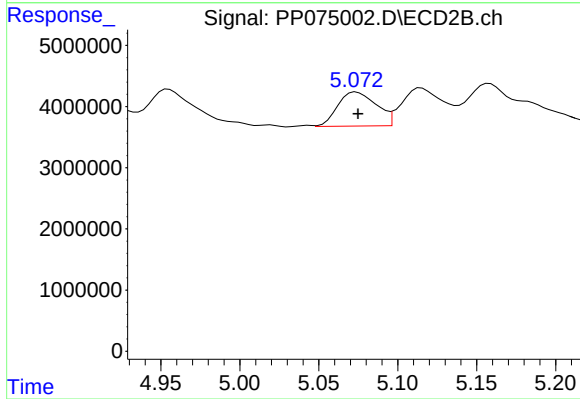


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 9483505
Conc: 68.77 ng/ml

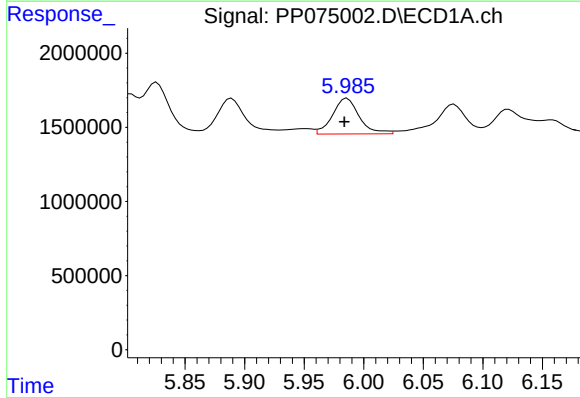


#6 AR-1016-4

R.T.: 5.986 min
Delta R.T.: 0.002 min
Response: 3770586
Conc: 107.17 ng/ml

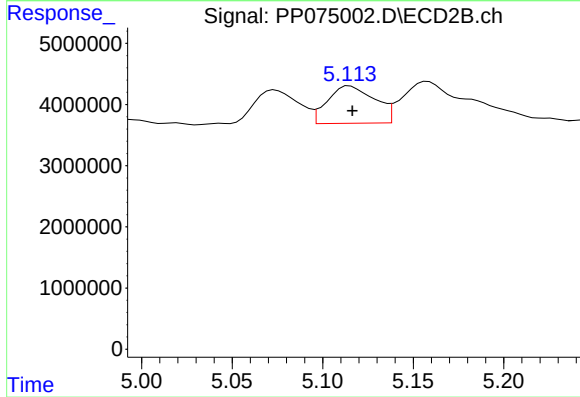

#6 AR-1016-4


R.T.: 5.115 min
Delta R.T.: -0.001 min
Response: 11052108
Conc: 79.05 ng/ml

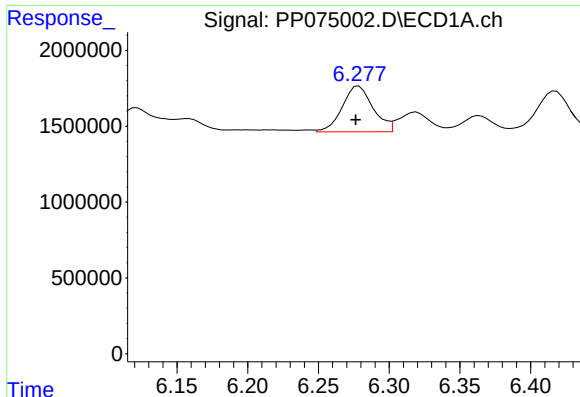

#7 AR-1016-5


R.T.: 6.279 min
Delta R.T.: 0.002 min
Response: 4571986
Conc: 137.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

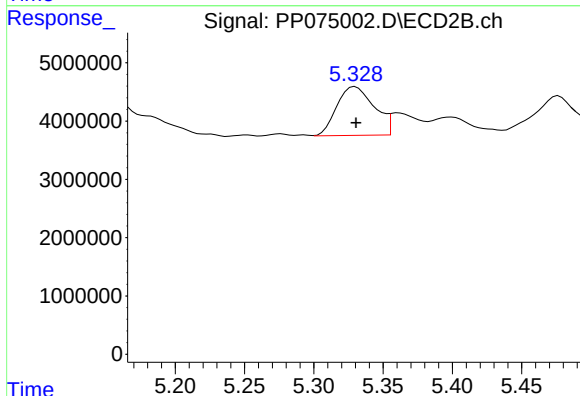


#7 AR-1016-5

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 15688686
Conc: 94.46 ng/ml

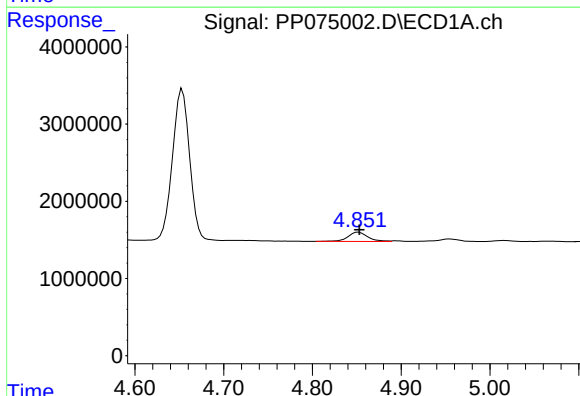


#8 AR-1221-1

R.T.: 4.852 min
Delta R.T.: -0.001 min
Response: 1863950
Conc: 105.95 ng/ml

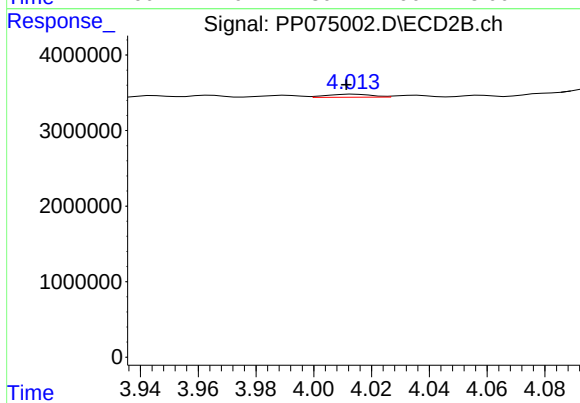

#8 AR-1221-1


R.T.: 4.014 min
Delta R.T.: 0.003 min
Response: 427956
Conc: 6.92 ng/ml

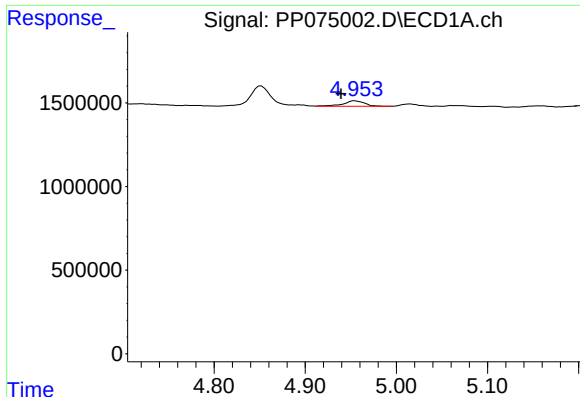

#9 AR-1221-2


R.T.: 4.955 min
Delta R.T.: 0.016 min
Response: 532928
Conc: 39.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

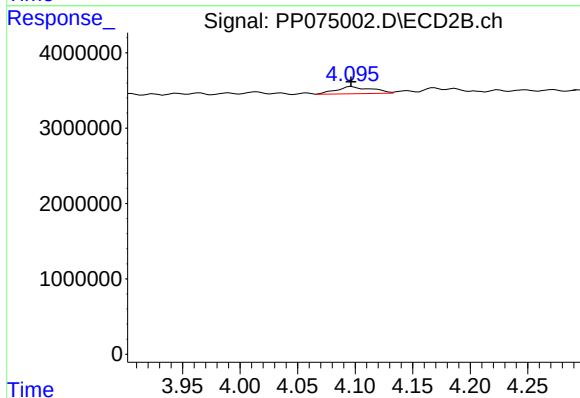


#9 AR-1221-2

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 2037481
Conc: 45.06 ng/ml

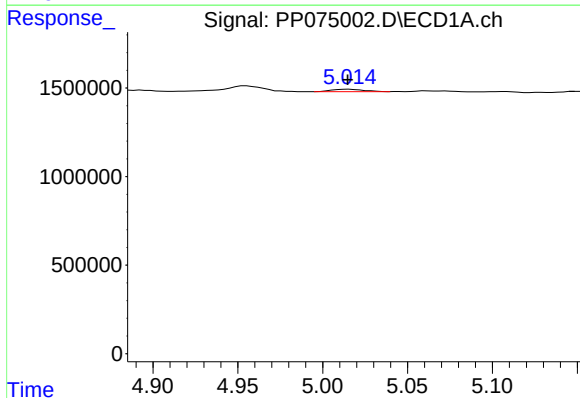


#10 AR-1221-3

R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 174560
Conc: 4.60 ng/ml

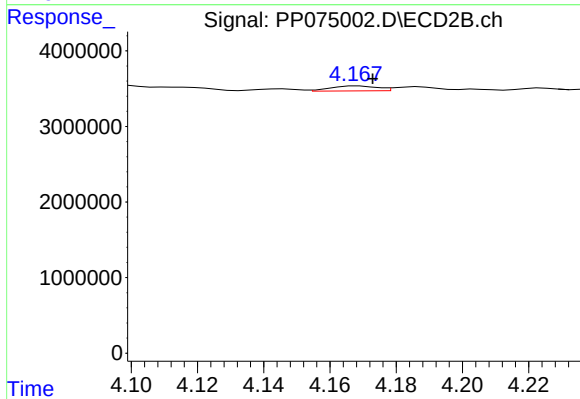

#10 AR-1221-3


R.T.: 4.169 min
Delta R.T.: -0.004 min
Response: 632208
Conc: 3.85 ng/ml

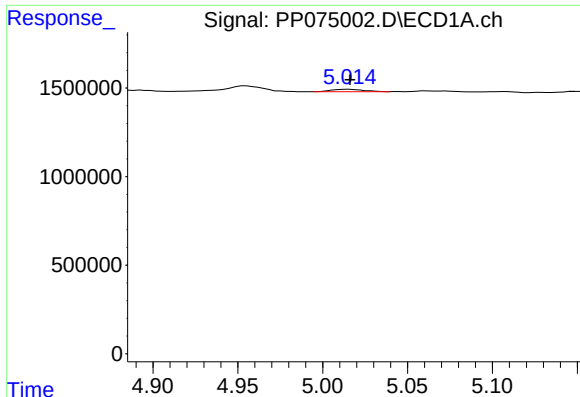

#11 AR-1232-1


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 174560
Conc: 5.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

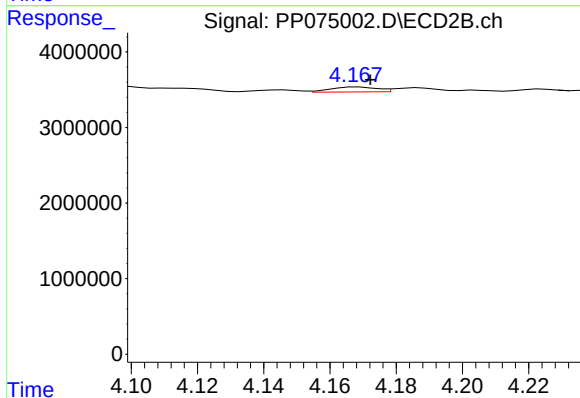


#11 AR-1232-1

R.T.: 4.169 min
Delta R.T.: -0.004 min
Response: 632208
Conc: 4.94 ng/ml

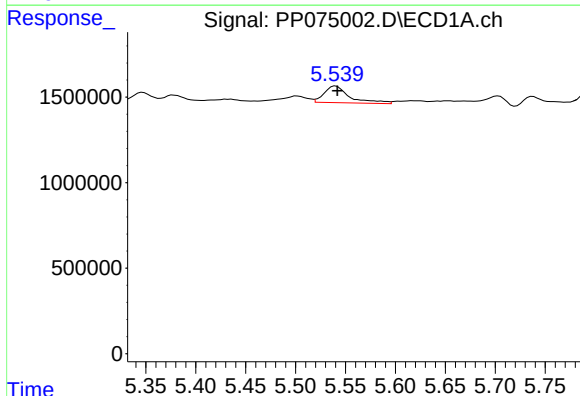


#12 AR-1232-2

R.T.: 5.540 min
Delta R.T.: -0.002 min
Response: 1737008
Conc: 110.23 ng/ml

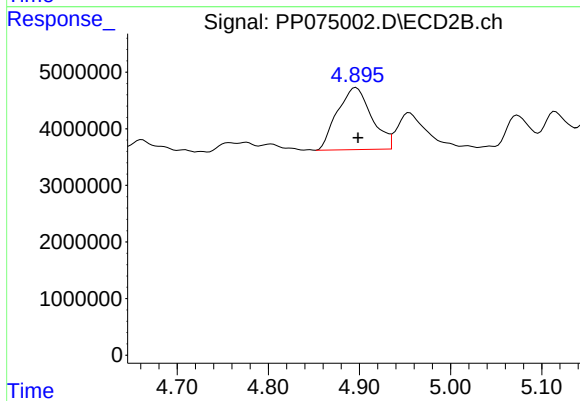

#12 AR-1232-2


R.T.: 4.896 min
Delta R.T.: -0.002 min
Response: 28670469
Conc: 123.69 ng/ml

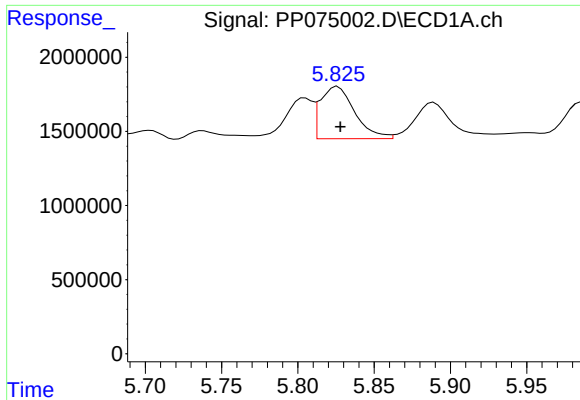

#13 AR-1232-3


R.T.: 5.826 min
Delta R.T.: -0.002 min
Response: 5517998
Conc: 180.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

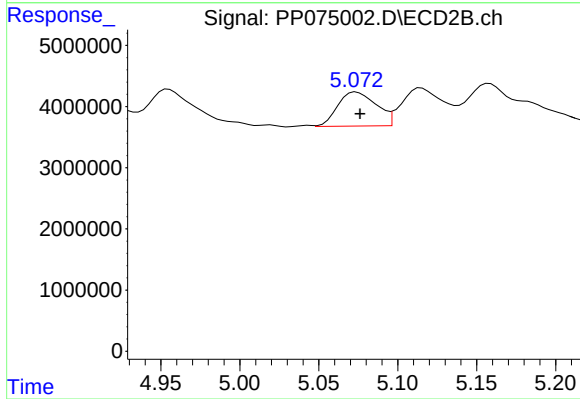


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 9483505
Conc: 157.90 ng/ml

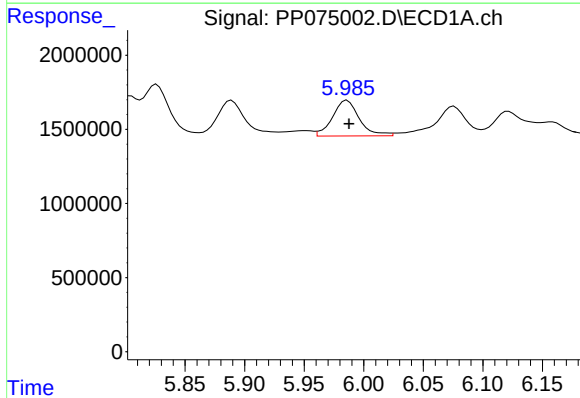


#14 AR-1232-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 3770586
Conc: 218.34 ng/ml

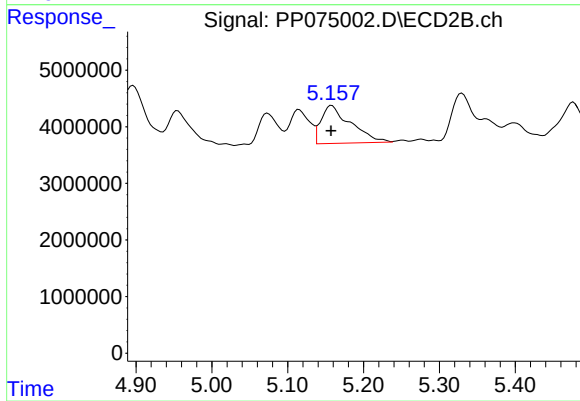

#14 AR-1232-4


R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 18149005
Conc: 246.23 ng/ml

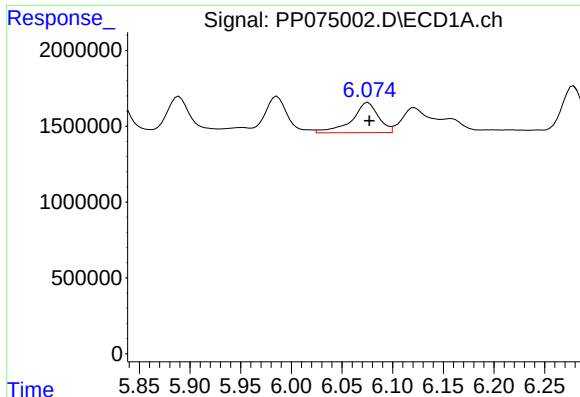

#15 AR-1232-5


R.T.: 6.076 min
Delta R.T.: -0.001 min
Response: 3636794
Conc: 280.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

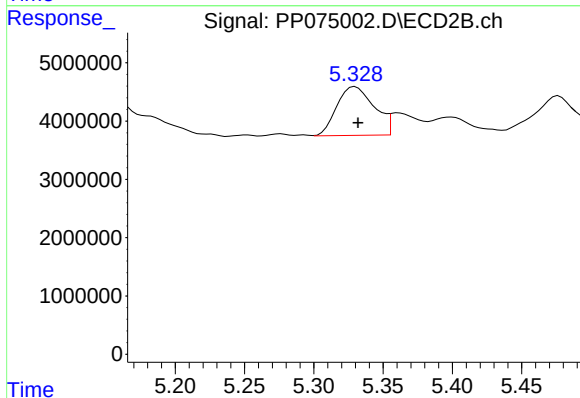


#15 AR-1232-5

R.T.: 5.330 min
Delta R.T.: -0.002 min
Response: 15688686
Conc: 252.70 ng/ml

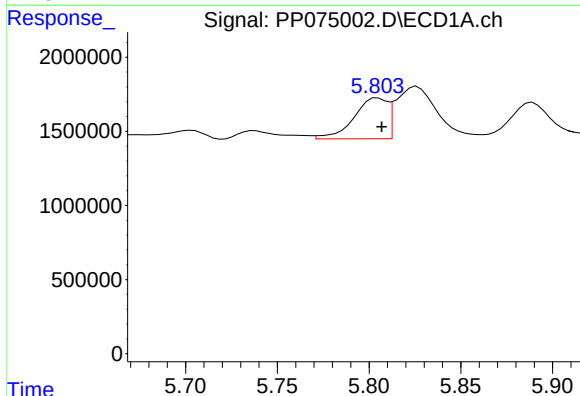


#16 AR-1242-1

R.T.: 5.805 min
Delta R.T.: -0.002 min
Response: 3479417
Conc: 90.91 ng/ml

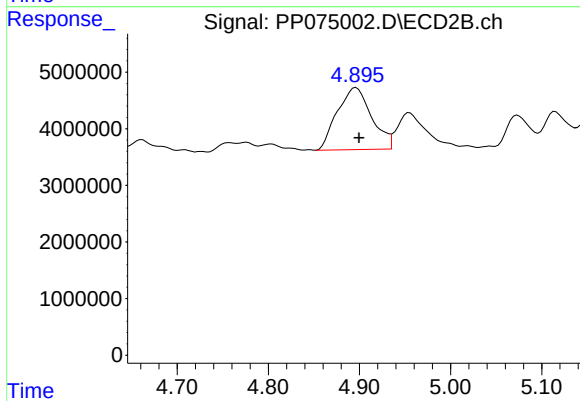

#16 AR-1242-1


R.T.: 4.896 min
Delta R.T.: -0.003 min
Response: 28670469
Conc: 67.98 ng/ml

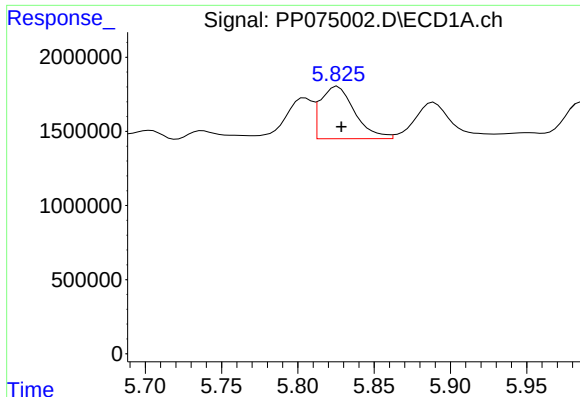

#17 AR-1242-2


R.T.: 5.826 min
Delta R.T.: -0.002 min
Response: 5517998
Conc: 97.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

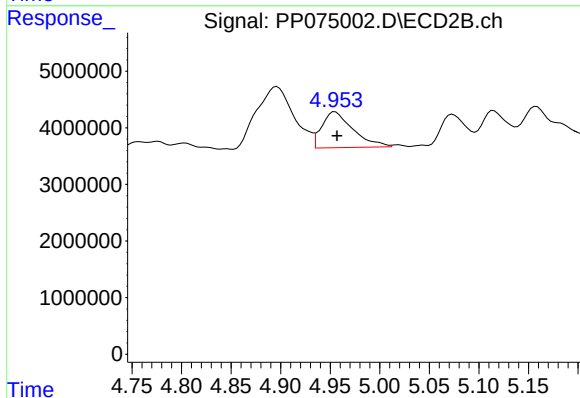


#17 AR-1242-2

R.T.: 4.955 min
Delta R.T.: -0.002 min
Response: 13921176
Conc: 69.51 ng/ml

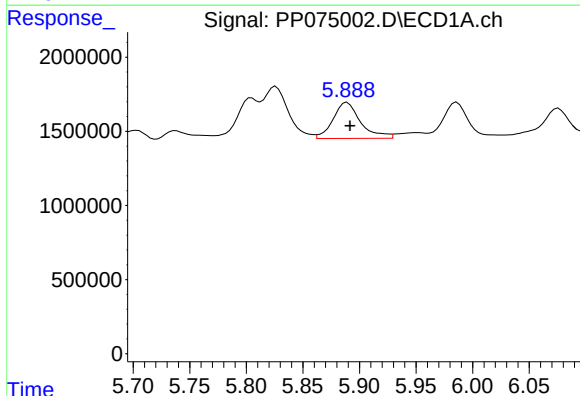


#18 AR-1242-3

R.T.: 5.889 min
Delta R.T.: -0.002 min
Response: 4115962
Conc: 101.37 ng/ml

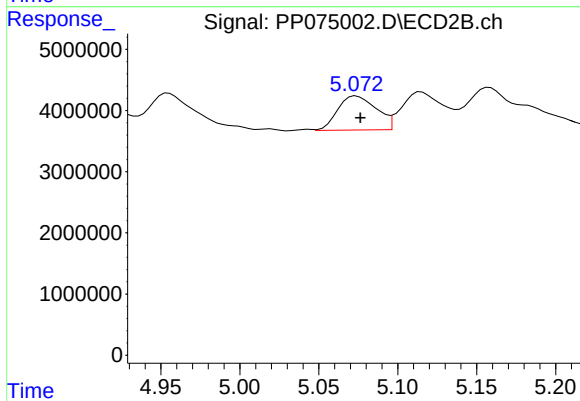

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: -0.003 min
Response: 9483505
Conc: 80.17 ng/ml

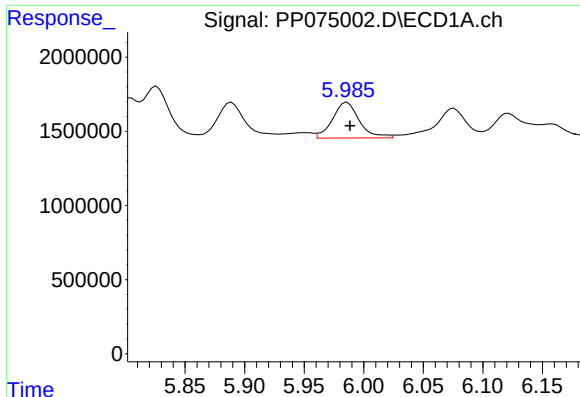

#19 AR-1242-4


R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 3770586
Conc: 118.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

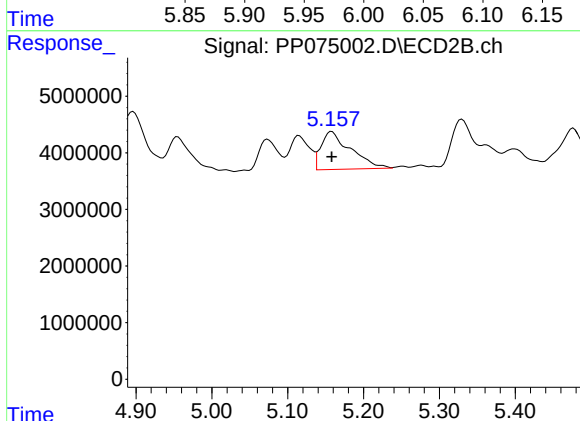


#19 AR-1242-4

R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 18149005
Conc: 106.04 ng/ml

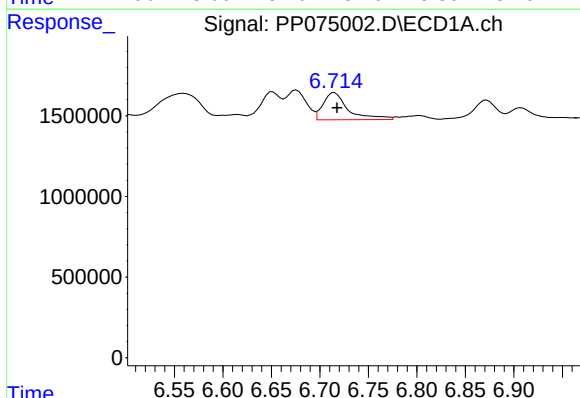


#20 AR-1242-5

R.T.: 6.715 min
Delta R.T.: -0.002 min
Response: 3015388
Conc: 83.60 ng/ml

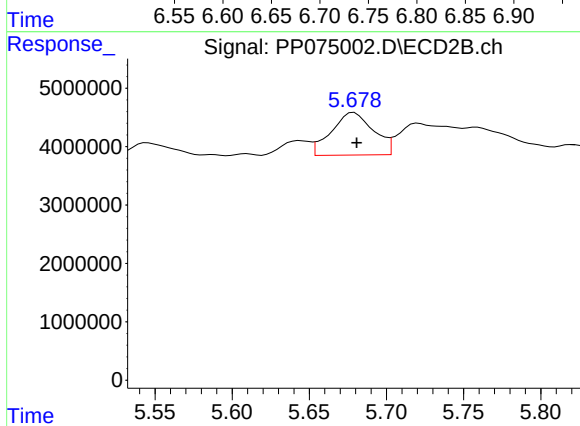

#20 AR-1242-5


R.T.: 5.679 min
Delta R.T.: -0.002 min
Response: 13824388
Conc: 74.66 ng/ml

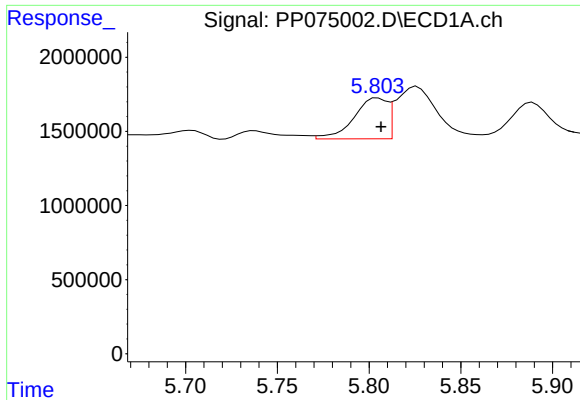

#21 AR-1248-1


R.T.: 5.805 min
Delta R.T.: -0.002 min
Response: 3479417
Conc: 115.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

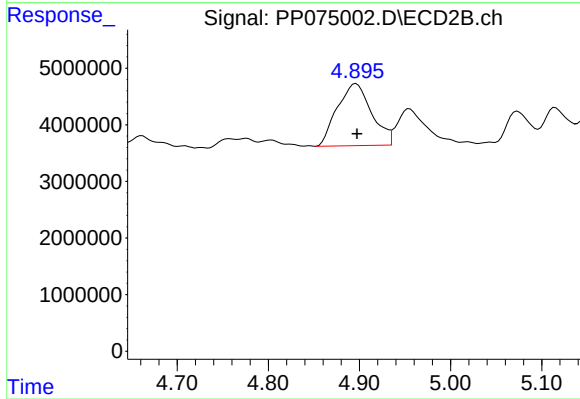


#21 AR-1248-1

R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 28670469
Conc: 103.82 ng/ml

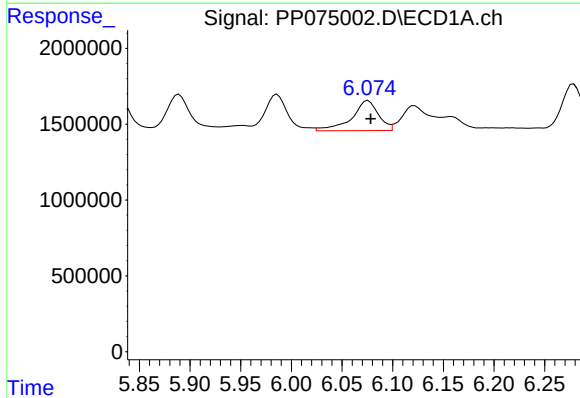


#22 AR-1248-2

R.T.: 6.076 min
Delta R.T.: -0.002 min
Response: 3636794
Conc: 84.39 ng/ml

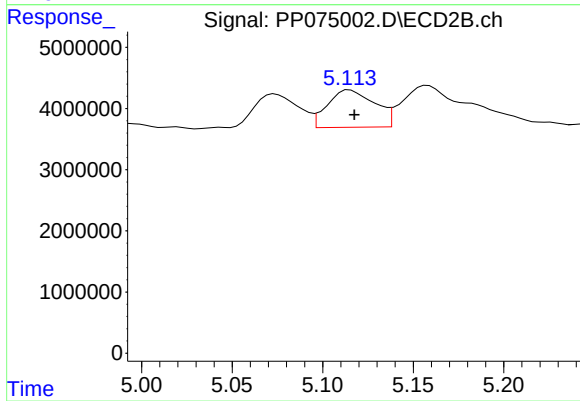

#22 AR-1248-2


R.T.: 5.115 min
Delta R.T.: -0.003 min
Response: 11052108
Conc: 62.53 ng/ml

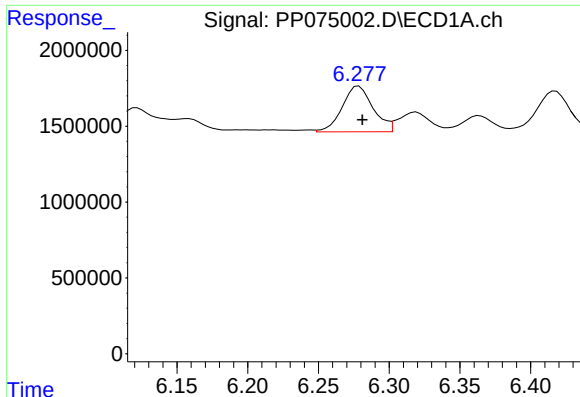

#23 AR-1248-3


R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 4571986
Conc: 97.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

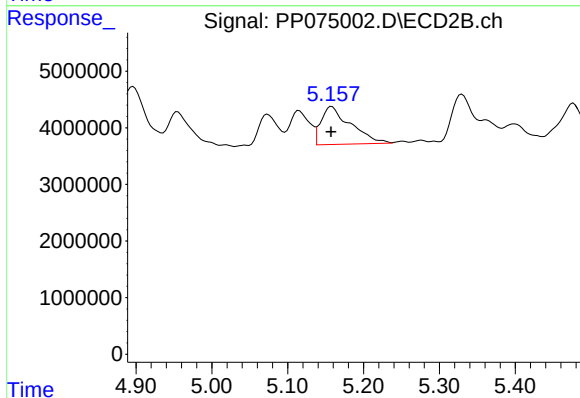


#23 AR-1248-3

R.T.: 5.158 min
Delta R.T.: 0.001 min
Response: 18149005
Conc: 79.88 ng/ml

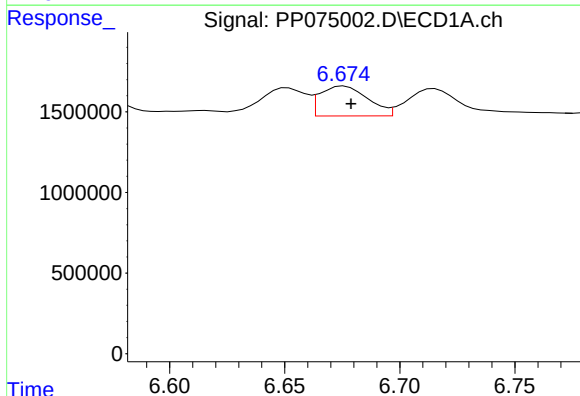


#24 AR-1248-4

R.T.: 6.676 min
Delta R.T.: -0.003 min
Response: 2687345
Conc: 48.86 ng/ml

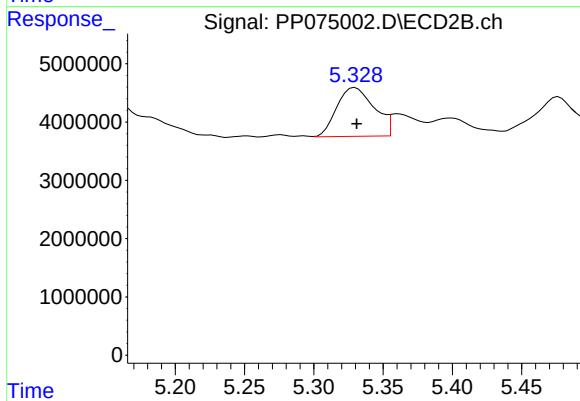

#24 AR-1248-4


R.T.: 5.330 min
Delta R.T.: -0.001 min
Response: 15688686
Conc: 71.96 ng/ml

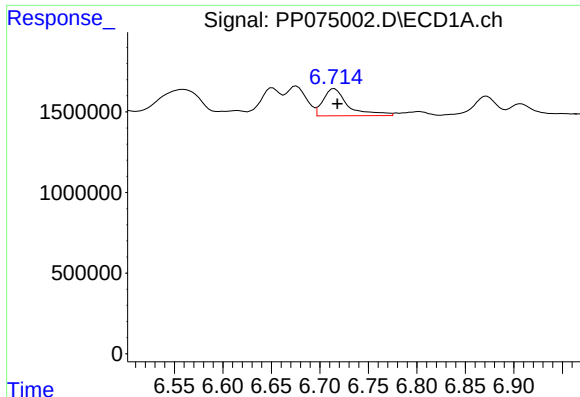

#25 AR-1248-5


R.T.: 6.715 min
Delta R.T.: -0.003 min
Response: 3015388
Conc: 54.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

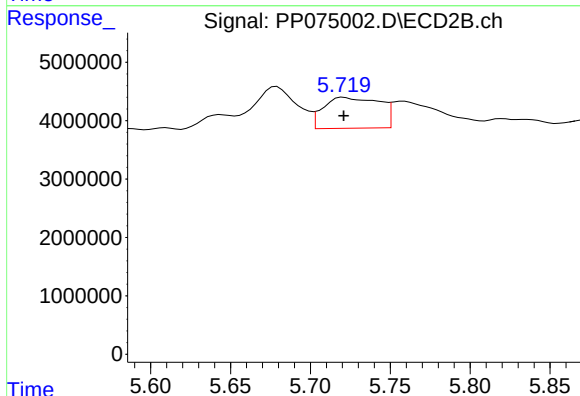


#25 AR-1248-5

R.T.: 5.721 min
Delta R.T.: 0.000 min
Response: 12909829
Conc: 35.15 ng/ml

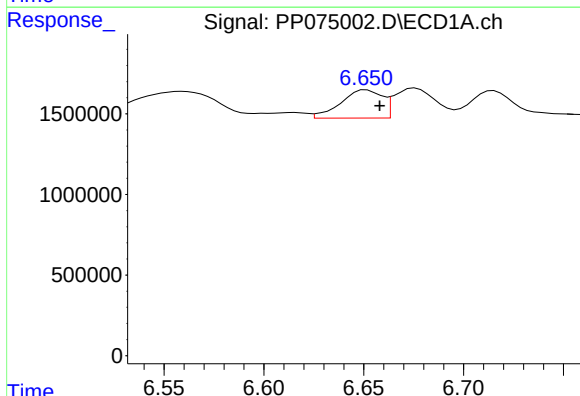


#26 AR-1254-1

R.T.: 6.651 min
Delta R.T.: -0.007 min
Response: 2526317
Conc: 43.36 ng/ml

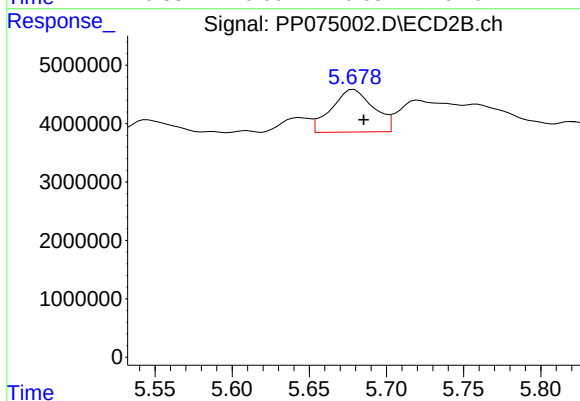

#26 AR-1254-1


R.T.: 5.679 min
Delta R.T.: -0.006 min
Response: 13824388
Conc: 29.00 ng/ml

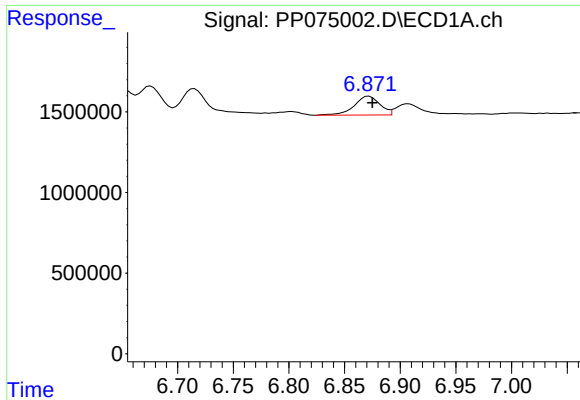

#27 AR-1254-2


R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 1892751
Conc: 23.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

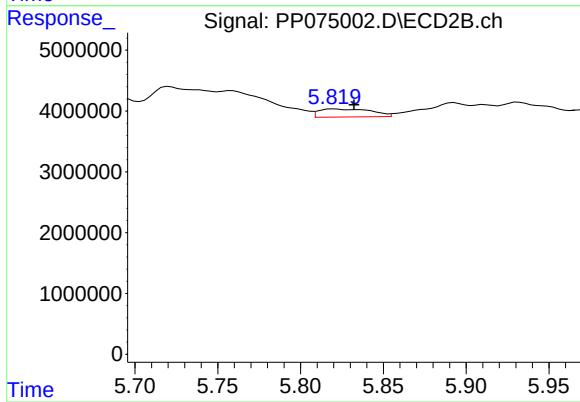


#27 AR-1254-2

R.T.: 5.820 min
Delta R.T.: -0.012 min
Response: 2935738
Conc: 8.34 ng/ml

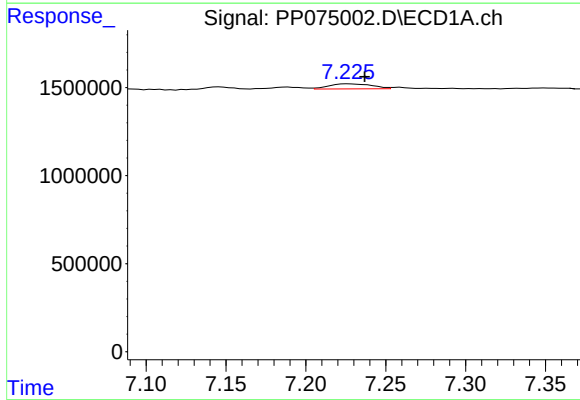


#28 AR-1254-3

R.T.: 7.226 min
Delta R.T.: -0.011 min
Response: 538824
Conc: 6.04 ng/ml

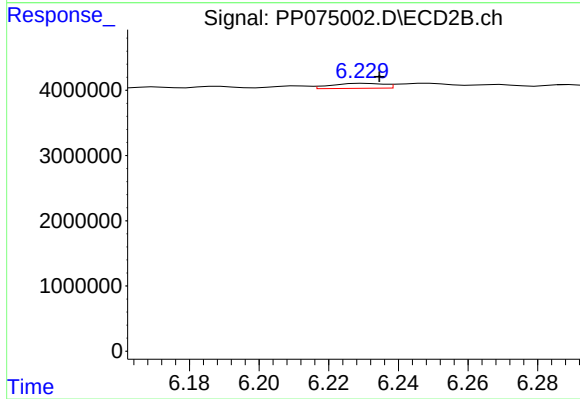

#28 AR-1254-3


R.T.: 6.230 min
Delta R.T.: -0.004 min
Response: 792334
Conc: 1.28 ng/ml

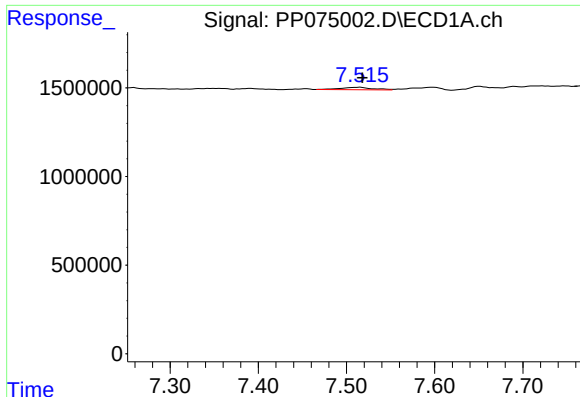

#29 AR-1254-4


R.T.: 7.516 min
Delta R.T.: -0.002 min
Response: 334685
Conc: 5.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

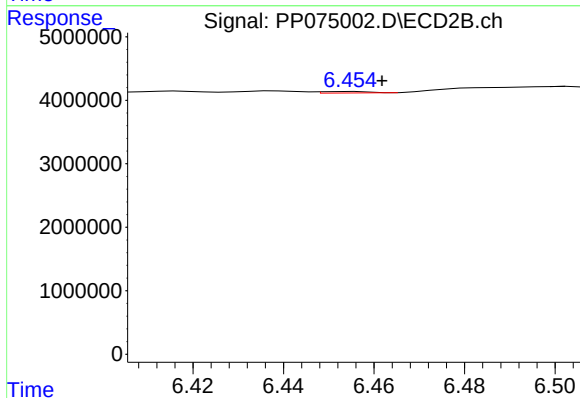


#29 AR-1254-4

R.T.: 6.455 min
Delta R.T.: -0.006 min
Response: 170313
Conc: 0.36 ng/ml

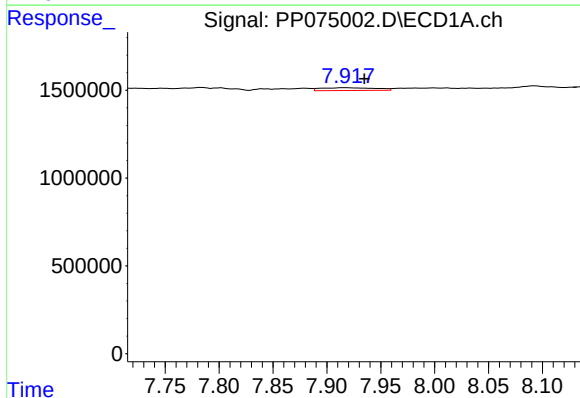


#30 AR-1254-5

R.T.: 7.918 min
Delta R.T.: -0.016 min
Response: 559837
Conc: 6.74 ng/ml

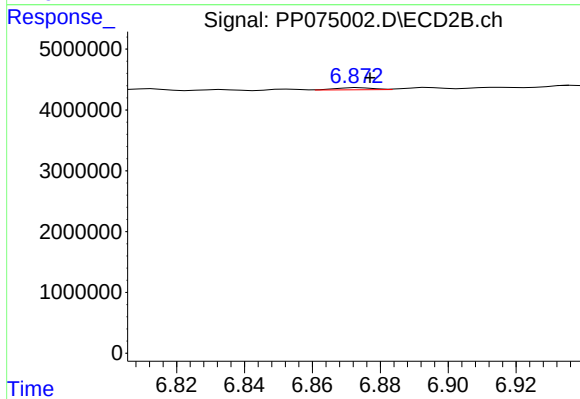

#30 AR-1254-5


R.T.: 6.874 min
Delta R.T.: -0.003 min
Response: 267057
Conc: 0.54 ng/ml

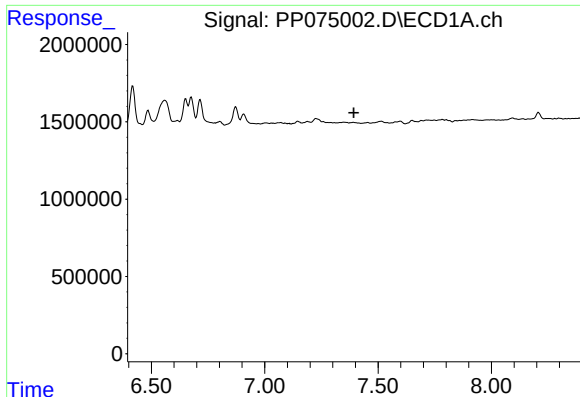

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

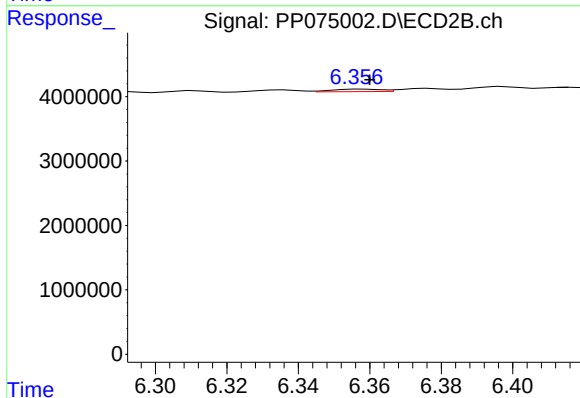


#31 AR-1260-1

R.T.: 6.358 min
Delta R.T.: -0.002 min
Response: 359409
Conc: 0.96 ng/ml

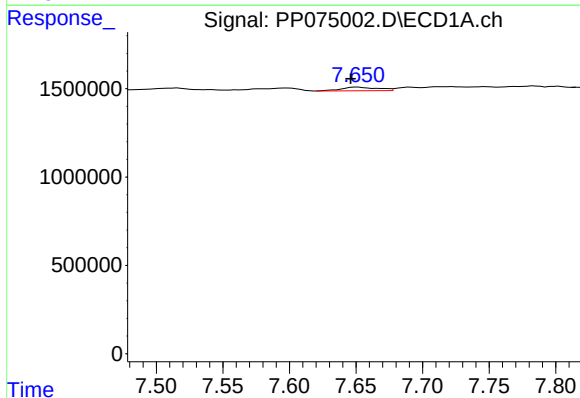


#32 AR-1260-2

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 390608
Conc: 5.67 ng/ml

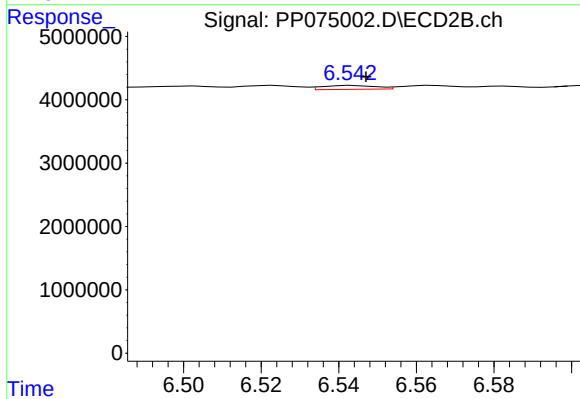

#32 AR-1260-2


R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 575726
Conc: 1.09 ng/ml

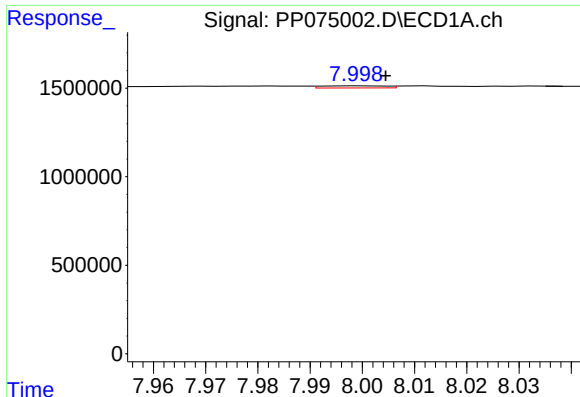

#33 AR-1260-3


R.T.: 8.000 min
Delta R.T.: -0.005 min
Response: 104464
Conc: 2.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

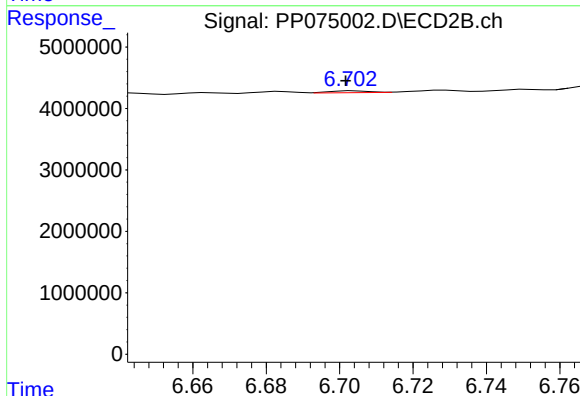


#33 AR-1260-3

R.T.: 6.704 min
Delta R.T.: 0.002 min
Response: 238755
Conc: 0.55 ng/ml

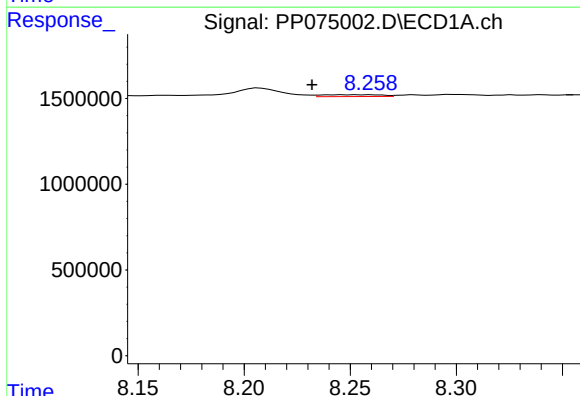


#34 AR-1260-4

R.T.: 8.246 min
Delta R.T.: 0.014 min
Response: 207319
Conc: 3.25 ng/ml

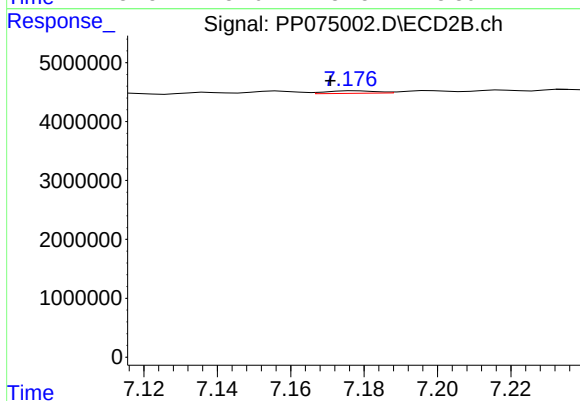

#34 AR-1260-4


R.T.: 7.178 min
Delta R.T.: 0.007 min
Response: 405676
Conc: 1.06 ng/ml

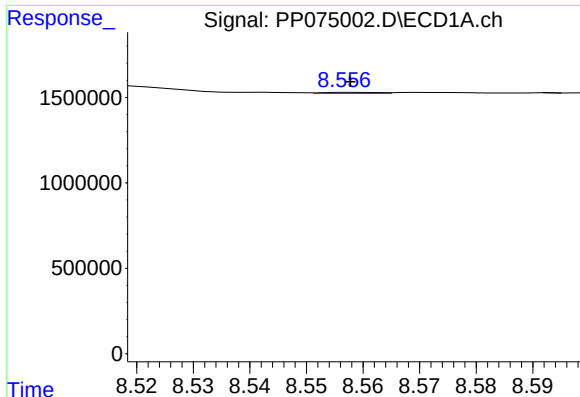

#35 AR-1260-5


R.T.: 8.558 min
Delta R.T.: 0.000 min
Response: 45165
Conc: 0.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

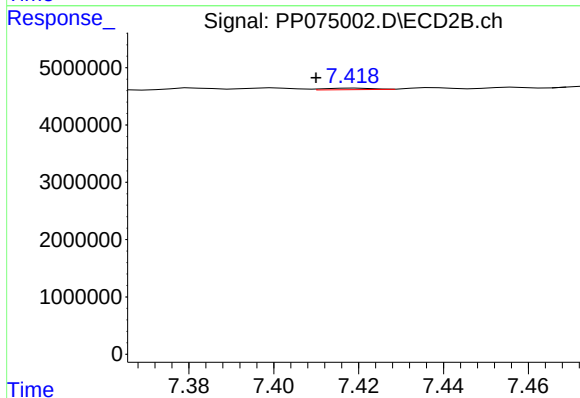


#35 AR-1260-5

R.T.: 7.419 min
Delta R.T.: 0.009 min
Response: 217302
Conc: 0.22 ng/ml

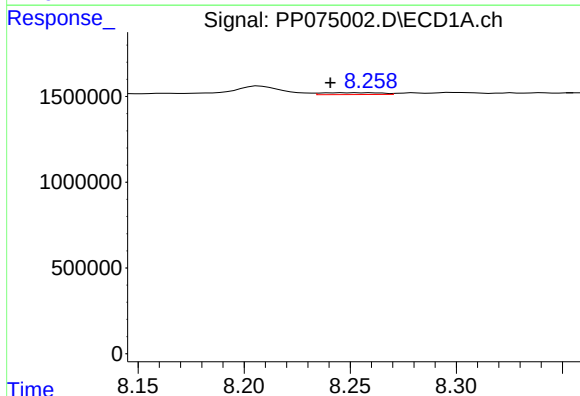


#36 AR-1262-1

R.T.: 8.246 min
Delta R.T.: 0.005 min
Response: 207319
Conc: 2.69 ng/ml

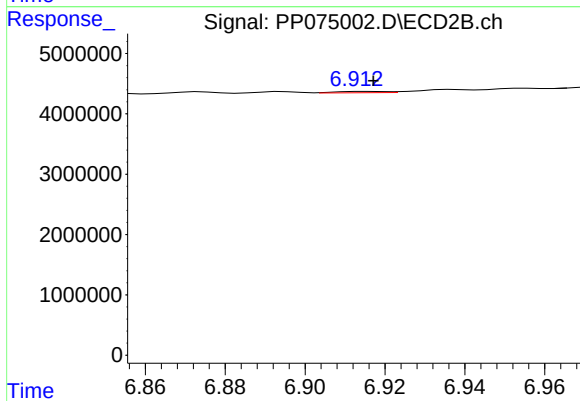

#36 AR-1262-1


R.T.: 6.915 min
Delta R.T.: -0.002 min
Response: 187093
Conc: 0.26 ng/ml

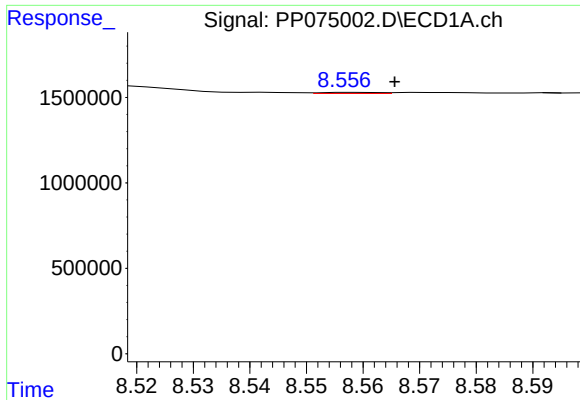

#37 AR-1262-2


R.T.: 8.558 min
Delta R.T.: -0.008 min
Response: 45165
Conc: 0.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

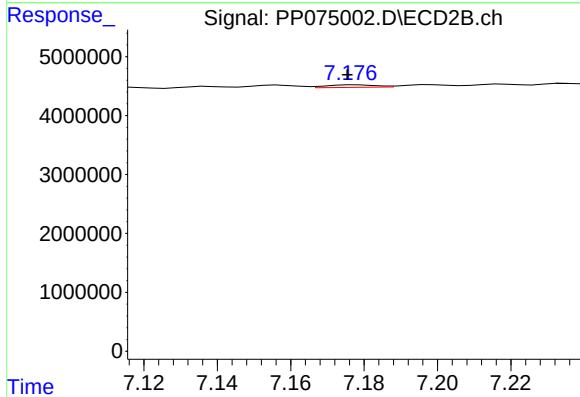


#37 AR-1262-2

R.T.: 7.178 min
Delta R.T.: 0.003 min
Response: 405676
Conc: 0.78 ng/ml

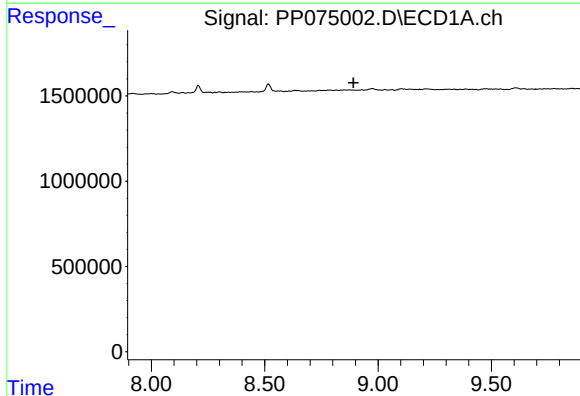


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

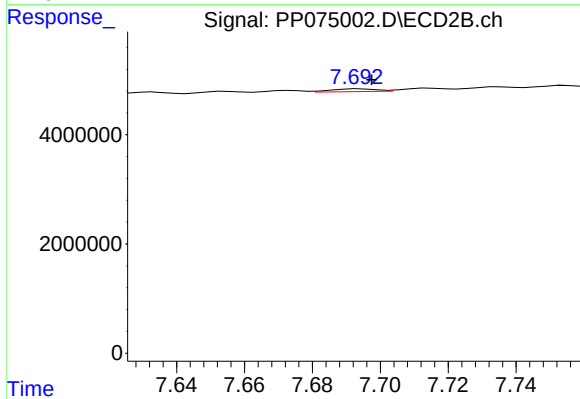

#38 AR-1262-3


R.T.: 7.694 min
Delta R.T.: -0.004 min
Response: 458647
Conc: 0.98 ng/ml

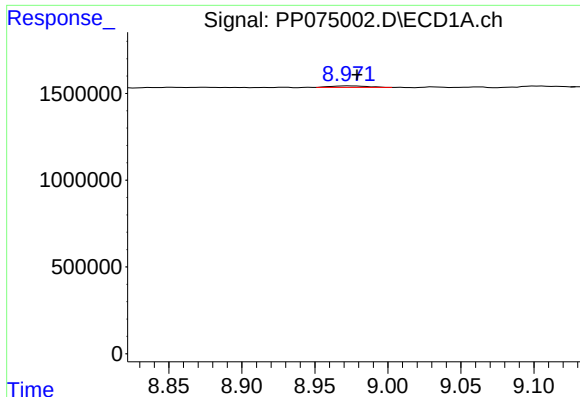

#39 AR-1262-4


R.T.: 8.973 min
Delta R.T.: -0.006 min
Response: 149115
Conc: 1.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

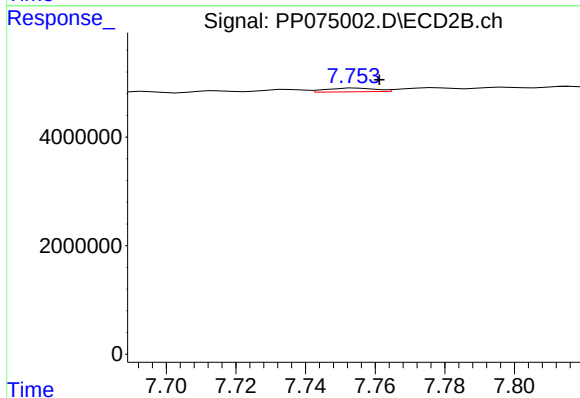


#39 AR-1262-4

R.T.: 7.754 min
Delta R.T.: -0.007 min
Response: 685040
Conc: 0.83 ng/ml

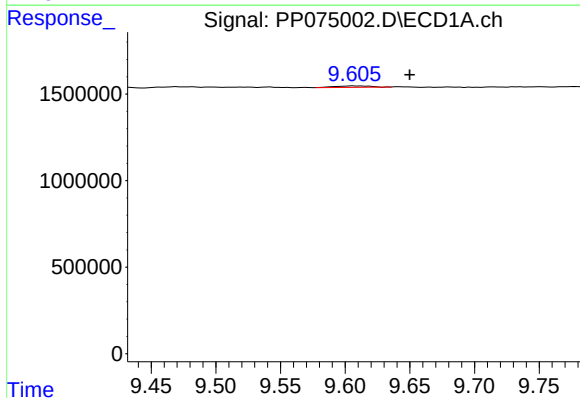


#40 AR-1262-5

R.T.: 9.606 min
Delta R.T.: -0.044 min
Response: 154426
Conc: 2.53 ng/ml

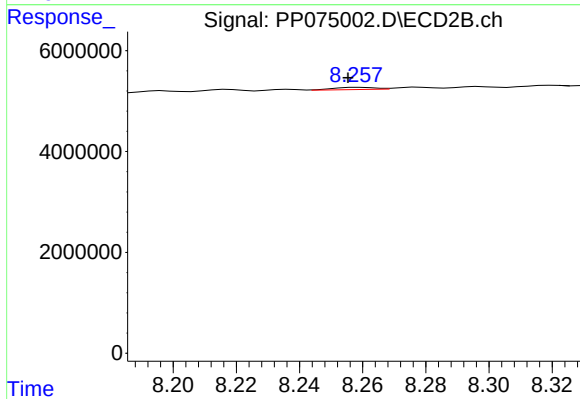

#40 AR-1262-5


R.T.: 8.259 min
Delta R.T.: 0.003 min
Response: 390780
Conc: 1.09 ng/ml

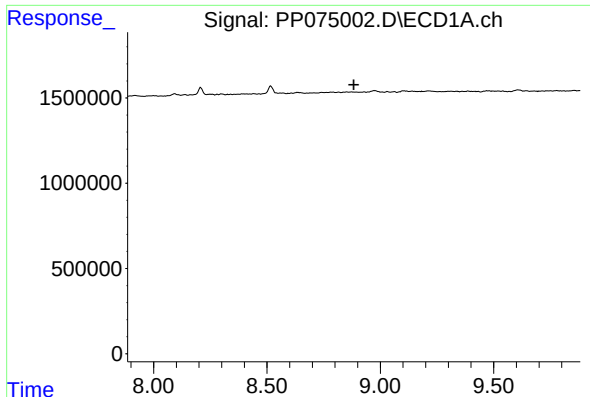

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

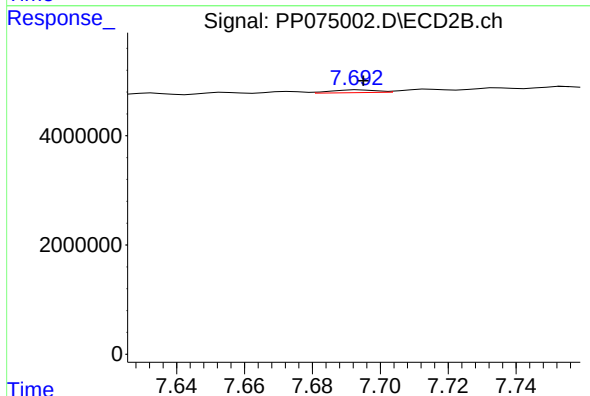


#41 AR-1268-1

R.T.: 7.694 min
Delta R.T.: -0.001 min
Response: 458647
Conc: 0.33 ng/ml

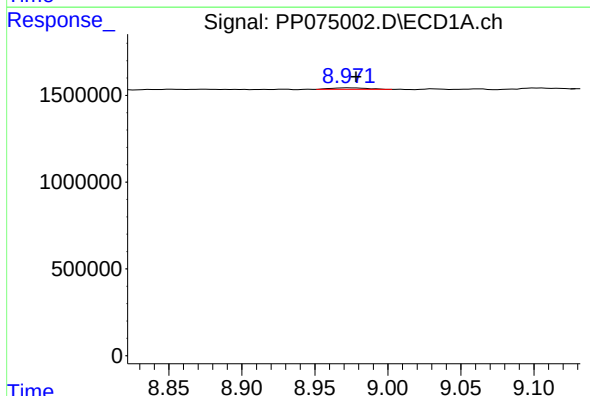


#42 AR-1268-2

R.T.: 8.973 min
Delta R.T.: -0.005 min
Response: 149115
Conc: 1.02 ng/ml

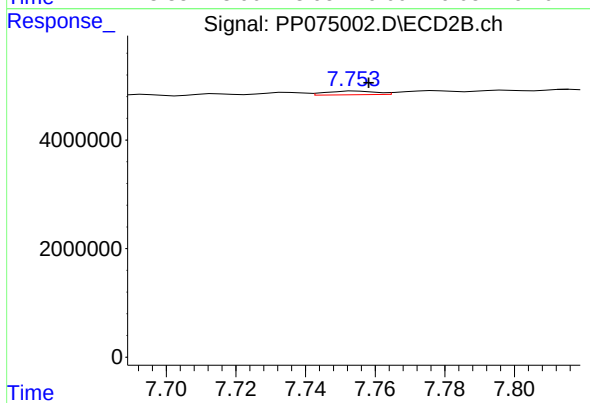

#42 AR-1268-2


R.T.: 7.754 min
Delta R.T.: -0.004 min
Response: 685040
Conc: 0.50 ng/ml

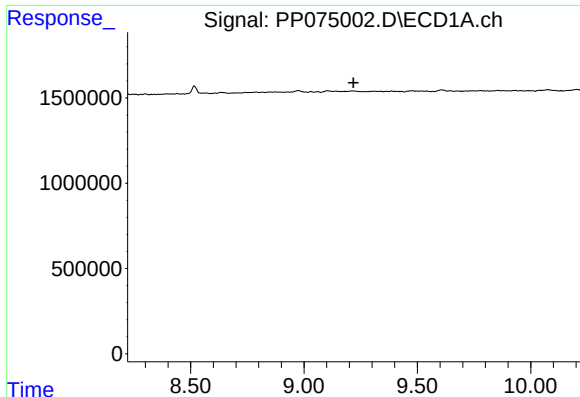

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

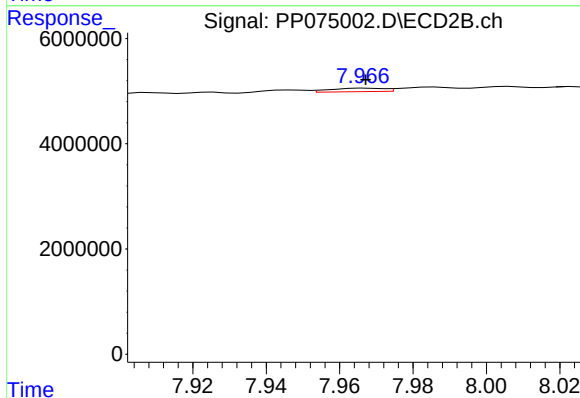


#43 AR-1268-3

R.T.: 7.967 min
Delta R.T.: 0.000 min
Response: 671001
Conc: 0.64 ng/ml

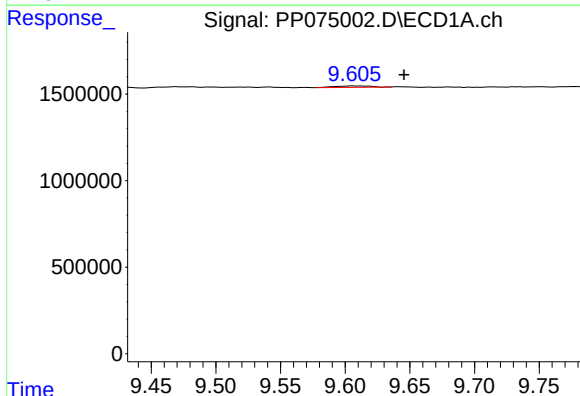


#44 AR-1268-4

R.T.: 9.606 min
Delta R.T.: -0.039 min
Response: 154426
Conc: 2.30 ng/ml

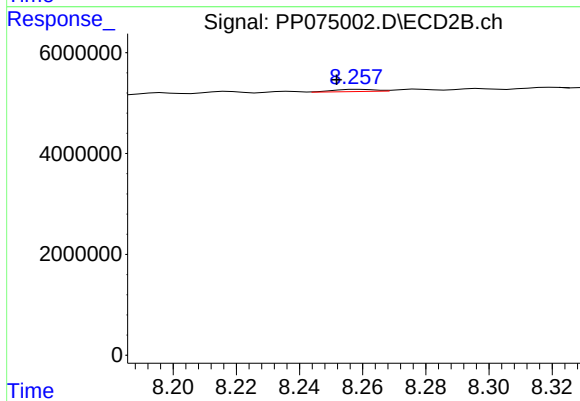

#44 AR-1268-4


R.T.: 8.259 min
Delta R.T.: 0.007 min
Response: 390780
Conc: 1.02 ng/ml

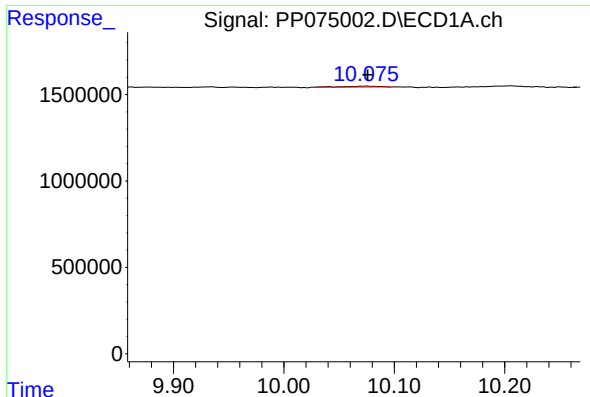

#45 AR-1268-5

R.T.: 10.076 min
Delta R.T.: 0.000 min
Response: 107377
Conc: 0.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-A

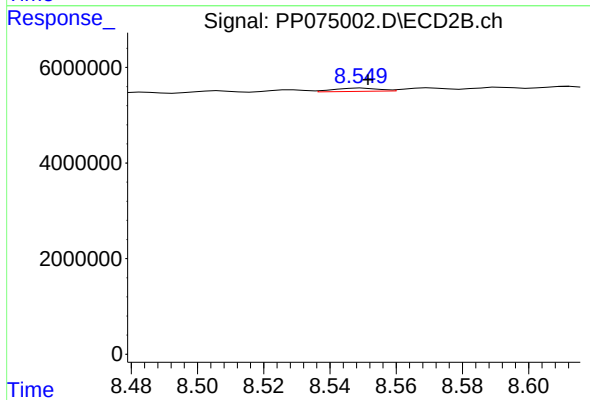

#45 AR-1268-5

R.T.: 8.550 min
Delta R.T.: -0.002 min
Response: 655156
Conc: 0.21 ng/ml