

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075003.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 13:52
 Operator : YP\AJ
 Sample : Q3034-02
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:49:07 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.656	3.795	25554451	96620501	20.883	19.982
2) SA Decachlor...	10.432	8.804	20773304	125.0E6	21.036	16.668
Target Compounds						
3) L1 AR-1016-1	5.807	4.894	1608601	13267273	36.485	26.047 #
4) L1 AR-1016-2	5.829	4.951	2500724	6213726	39.794	26.106 #
5) L1 AR-1016-3	5.892	5.070	1944651	4462508	43.297	32.360 #
6) L1 AR-1016-4	5.989	5.111	1585142	4277636	45.056	30.598 #
7) L1 AR-1016-5	6.281	5.326	1757504	6752779	52.959	40.659
8) L2 AR-1221-1	4.855	4.014	2231438	399823	126.838	6.463 #
9) L2 AR-1221-2	4.958	4.099	540628	1760734	40.475	38.944
10) L2 AR-1221-3	5.019	4.169	200456	475536	5.287	2.894 #
11) L3 AR-1232-1	5.019	4.169	200456	475536	6.600	3.712 #
12) L3 AR-1232-2	5.542	4.894	703895	13267273	44.668	57.238 #
13) L3 AR-1232-3	5.829	5.070	2500724	4462508	81.874	74.301
14) L3 AR-1232-4	5.989	5.155	1585142	7718813	91.790	104.722
15) L3 AR-1232-5	6.079	5.326	1440593	6752779	110.977	108.769
16) L4 AR-1242-1	5.807	4.894	1608601	13267273	42.027	31.457 #
17) L4 AR-1242-2	5.829	4.951	2500724	6213726	44.275	31.025 #
18) L4 AR-1242-3	5.892	5.070	1944651	4462508	47.894	37.723
19) L4 AR-1242-4	5.989	5.155	1585142	7718813	49.939	45.097
20) L4 AR-1242-5	6.718	5.673	1163865	5065282	32.266	27.356
21) L5 AR-1248-1	5.807	4.894	1608601	13267273	53.223	48.045
22) L5 AR-1248-2	6.079	5.111	1440593	4277636	33.427	24.201 #
23) L5 AR-1248-3	6.281	5.155	1757504	7718813	37.631	33.973
24) L5 AR-1248-4	6.679	5.326	1189002	6752779	21.618	30.973 #
25) L5 AR-1248-5	6.718	5.754	1163865	17890702	20.982	48.706 #
26) L6 AR-1254-1	6.654	5.673	1228857	5065282	21.089	10.625 #
27) L6 AR-1254-2	6.876	5.841	761679	920239	9.332	2.613 #
28) L6 AR-1254-3	7.228	6.237	219467	636761	2.460	1.027 #
29) L6 AR-1254-4	0.000	6.450	0	200181	N.D.	0.427 #
30) L6 AR-1254-5	7.934	6.887	209030	229587	2.516	0.468 #
31) L7 AR-1260-1	0.000	6.365	0	331415	N.D.	0.883 #
32) L7 AR-1260-2	7.653	6.517	178123	708667	2.585	1.340 #
33) L7 AR-1260-3	7.995	6.704	218141	587059	4.204	1.356 #
34) L7 AR-1260-4	8.210	7.177	850389	167631	13.330	0.439 #
35) L7 AR-1260-5	8.520f	7.416	824248	164408	7.268	0.164 #
36) L8 AR-1262-1	8.257	6.910	133005	298683	1.727	0.422 #
37) L8 AR-1262-2	8.520f	7.177	824248	167631	6.226	0.322 #
38) L8 AR-1262-3	8.885	7.692	93051	282851	0.957	0.607 #
39) L8 AR-1262-4	8.976	7.752	216844	552829	2.879	0.673 #
40) L8 AR-1262-5	9.624	8.247	62676	147296	1.028	0.411 #
41) L9 AR-1268-1	8.885	7.692	93051	282851	0.574	0.201 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 13:52
Operator : YP\AJ
Sample : Q3034-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.976	7.752	216844	552829	1.478	0.405 #
43)	L9 AR-1268-3	0.000	7.968	0	1086791	N.D.	1.042 #
44)	L9 AR-1268-4	9.624	8.247	62676	147296	0.932	0.384 #
45)	L9 AR-1268-5	10.080	8.564	44057	898381	0.119	0.286 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075003.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 13:52
Operator : YP\AJ
Sample : Q3034-02
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:07 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

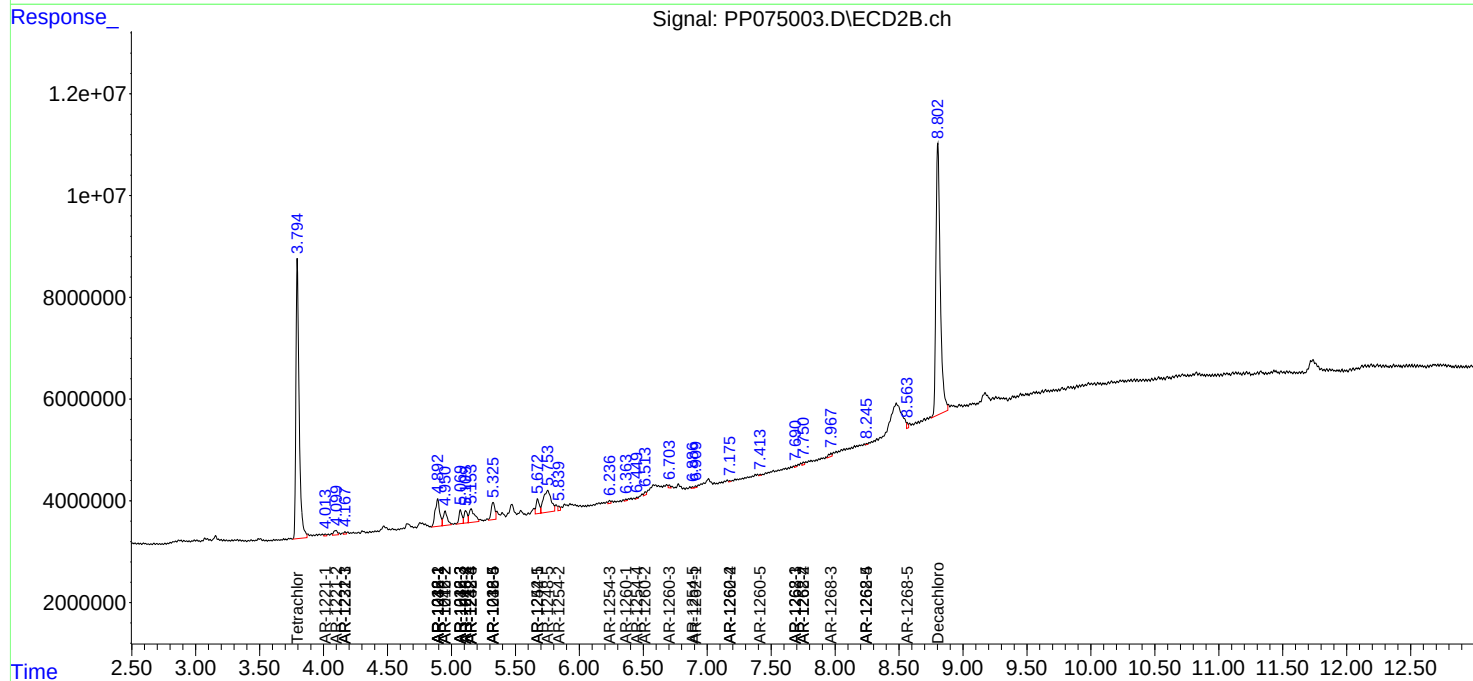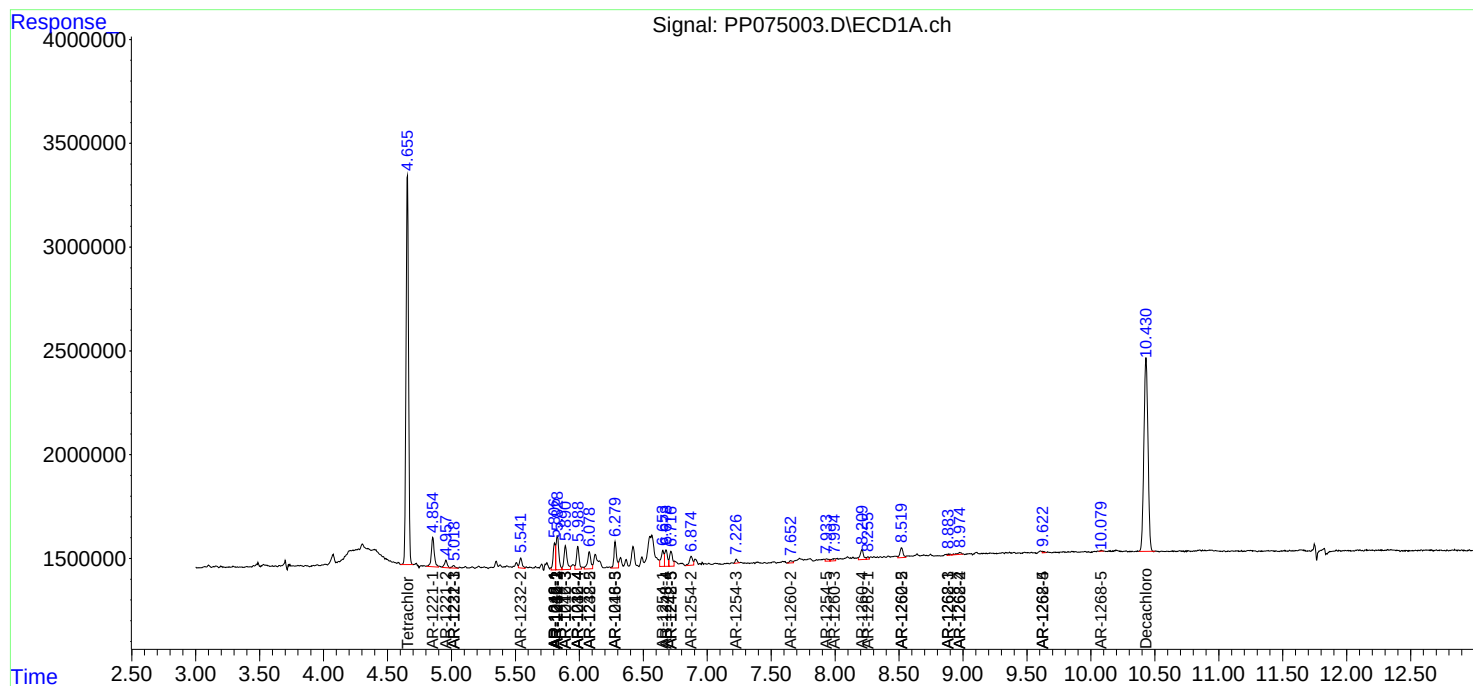


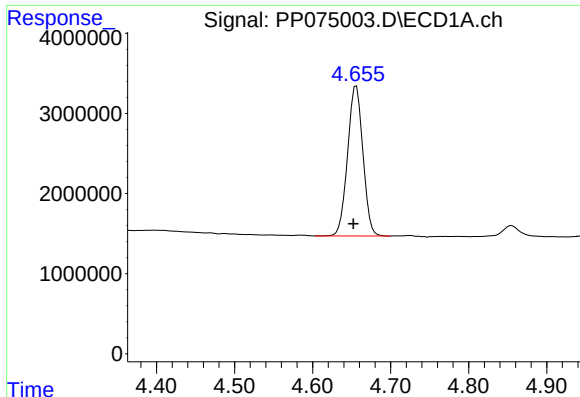

#1 Tetrachloro-m-xylene


R.T.: 4.656 min
Delta R.T.: 0.004 min
Response: 25554451
Conc: 20.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

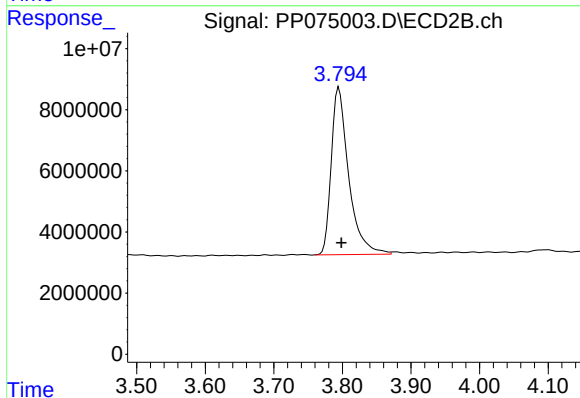


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: -0.004 min
Response: 96620501
Conc: 19.98 ng/ml

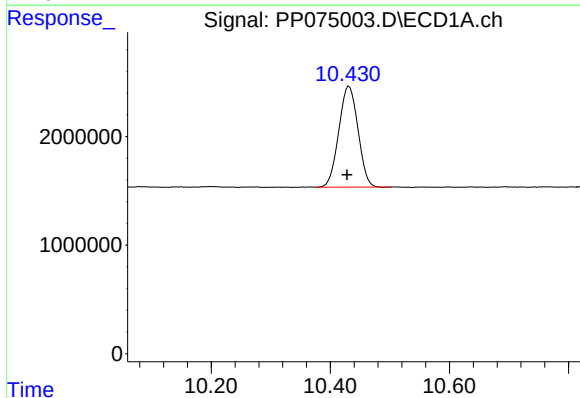


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.003 min
Response: 20773304
Conc: 21.04 ng/ml

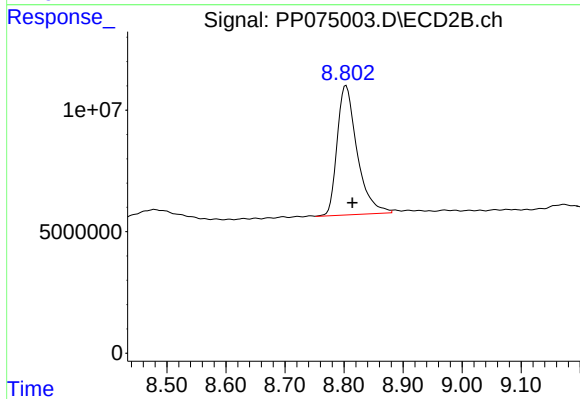

#2 Decachlorobiphenyl


R.T.: 8.804 min
Delta R.T.: -0.010 min
Response: 124993136
Conc: 16.67 ng/ml

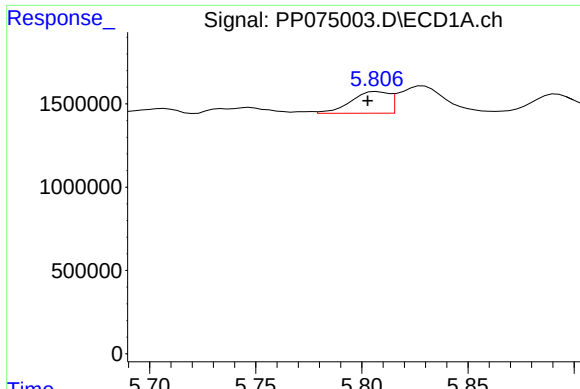

#3 AR-1016-1


R.T.: 5.807 min
Delta R.T.: 0.005 min
Response: 1608601
Conc: 36.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

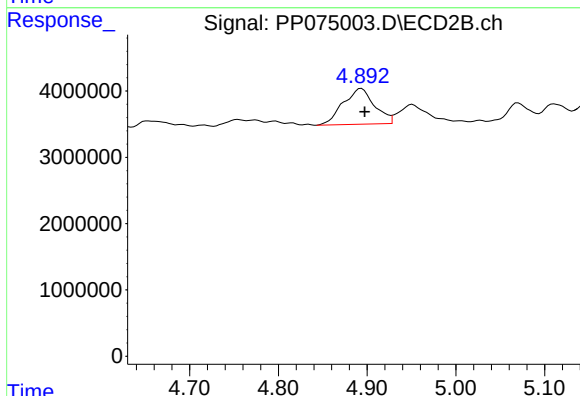


#3 AR-1016-1

R.T.: 4.894 min
Delta R.T.: -0.004 min
Response: 13267273
Conc: 26.05 ng/ml

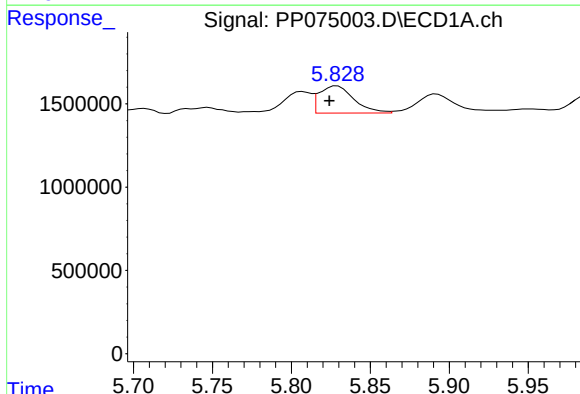


#4 AR-1016-2

R.T.: 5.829 min
Delta R.T.: 0.005 min
Response: 2500724
Conc: 39.79 ng/ml

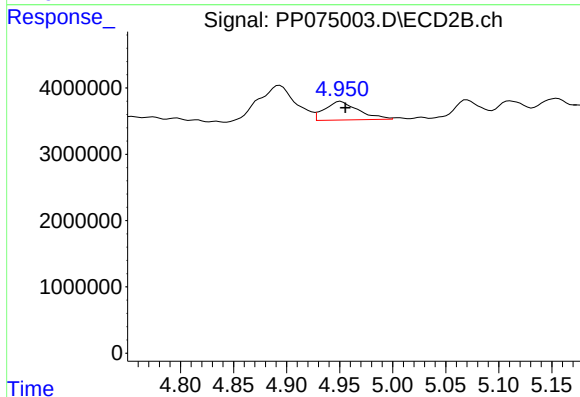

#4 AR-1016-2


R.T.: 4.951 min
Delta R.T.: -0.004 min
Response: 6213726
Conc: 26.11 ng/ml

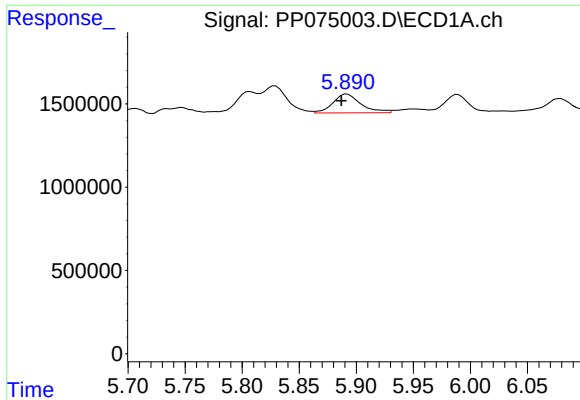

#5 AR-1016-3


R.T.: 5.892 min
Delta R.T.: 0.005 min
Response: 1944651
Conc: 43.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

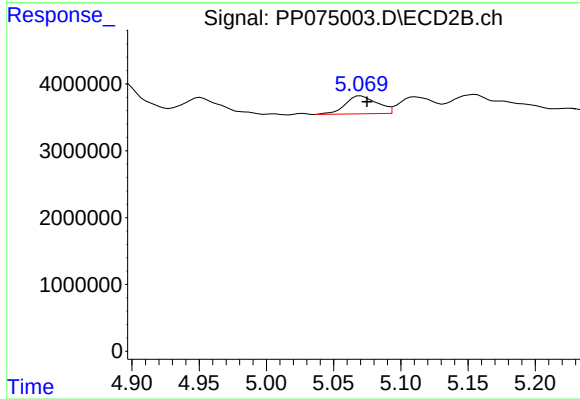


#5 AR-1016-3

R.T.: 5.070 min
Delta R.T.: -0.005 min
Response: 4462508
Conc: 32.36 ng/ml

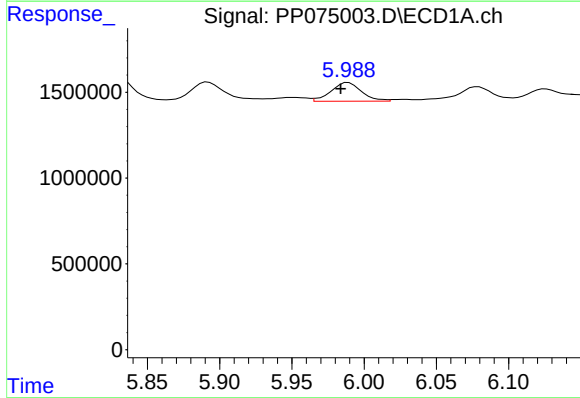


#6 AR-1016-4

R.T.: 5.989 min
Delta R.T.: 0.005 min
Response: 1585142
Conc: 45.06 ng/ml

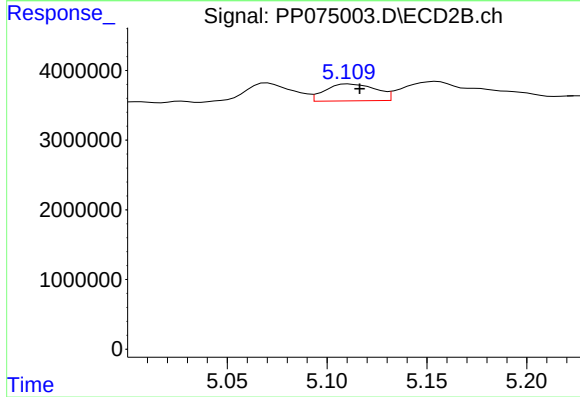

#6 AR-1016-4


R.T.: 5.111 min
Delta R.T.: -0.005 min
Response: 4277636
Conc: 30.60 ng/ml

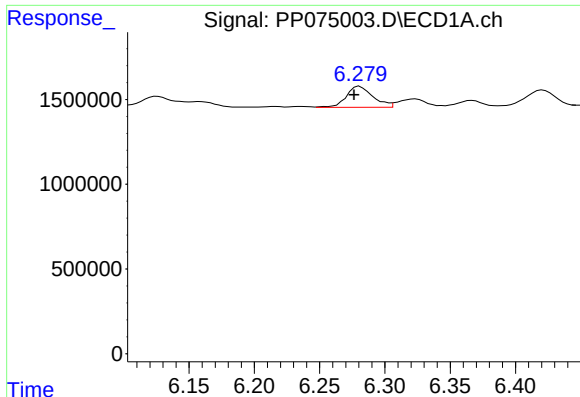

#7 AR-1016-5


R.T.: 6.281 min
Delta R.T.: 0.004 min
Response: 1757504
Conc: 52.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

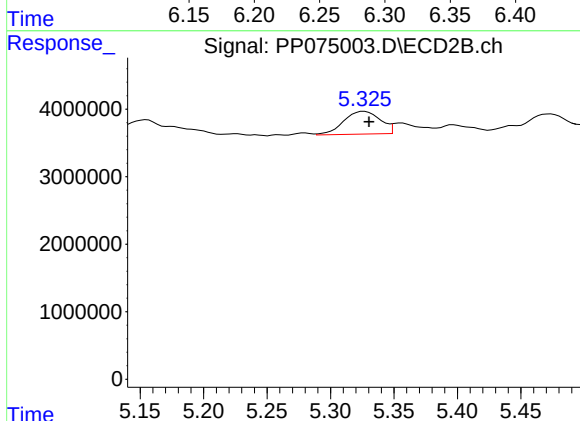


#7 AR-1016-5

R.T.: 5.326 min
Delta R.T.: -0.004 min
Response: 6752779
Conc: 40.66 ng/ml

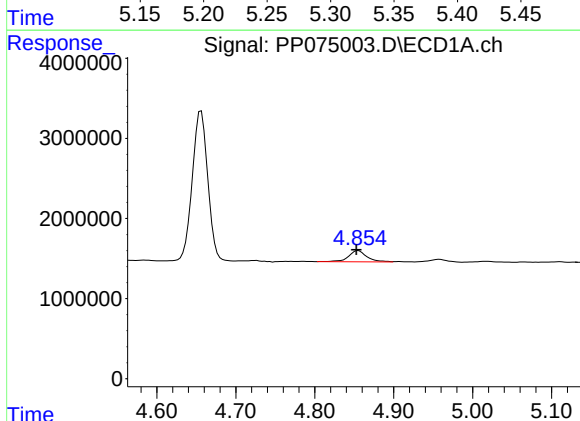


#8 AR-1221-1

R.T.: 4.855 min
Delta R.T.: 0.002 min
Response: 2231438
Conc: 126.84 ng/ml

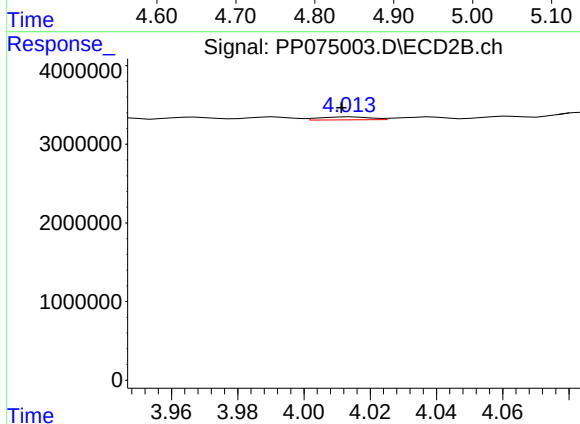

#8 AR-1221-1


R.T.: 4.014 min
Delta R.T.: 0.003 min
Response: 399823
Conc: 6.46 ng/ml

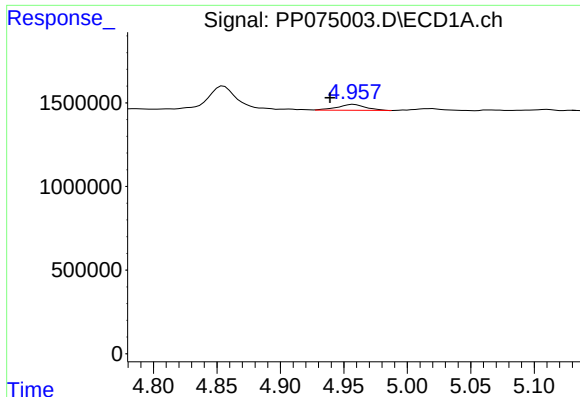

#9 AR-1221-2


R.T.: 4.958 min
Delta R.T.: 0.019 min
Response: 540628
Conc: 40.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

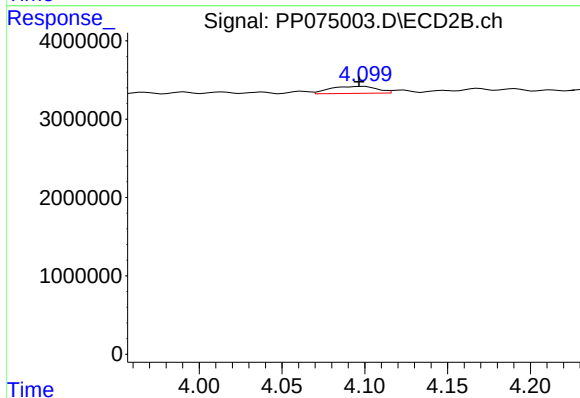


#9 AR-1221-2

R.T.: 4.099 min
Delta R.T.: 0.003 min
Response: 1760734
Conc: 38.94 ng/ml

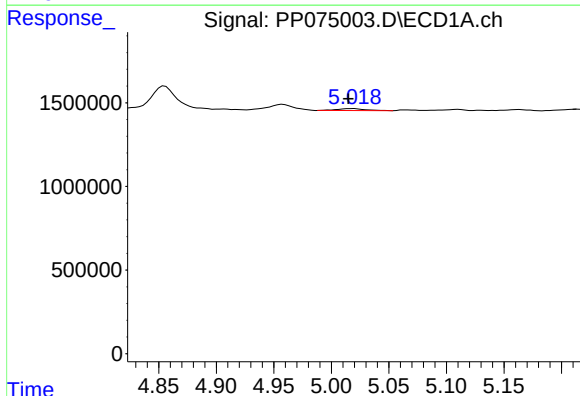


#10 AR-1221-3

R.T.: 5.019 min
Delta R.T.: 0.004 min
Response: 200456
Conc: 5.29 ng/ml

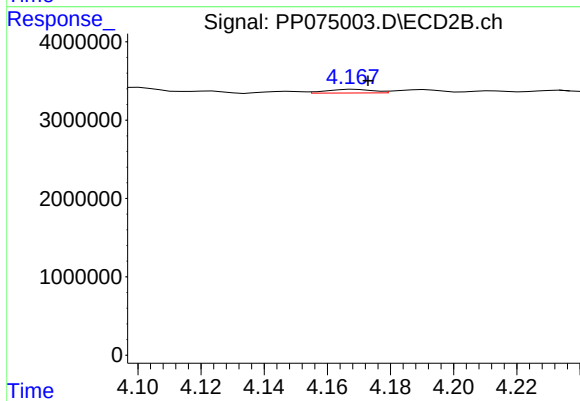

#10 AR-1221-3


R.T.: 4.169 min
Delta R.T.: -0.004 min
Response: 475536
Conc: 2.89 ng/ml

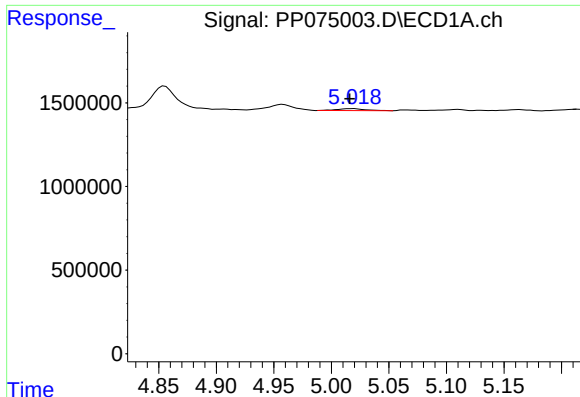

#11 AR-1232-1


R.T.: 5.019 min
Delta R.T.: 0.003 min
Response: 200456
Conc: 6.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

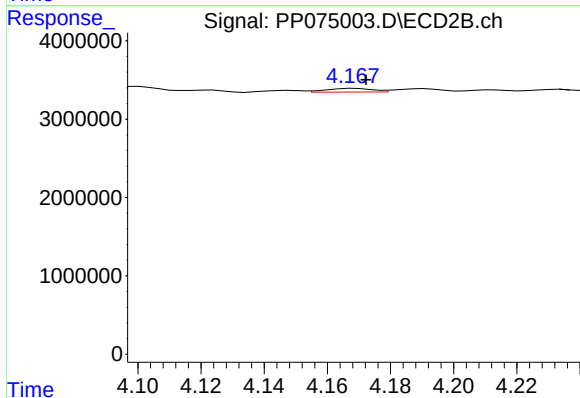


#11 AR-1232-1

R.T.: 4.169 min
Delta R.T.: -0.004 min
Response: 475536
Conc: 3.71 ng/ml

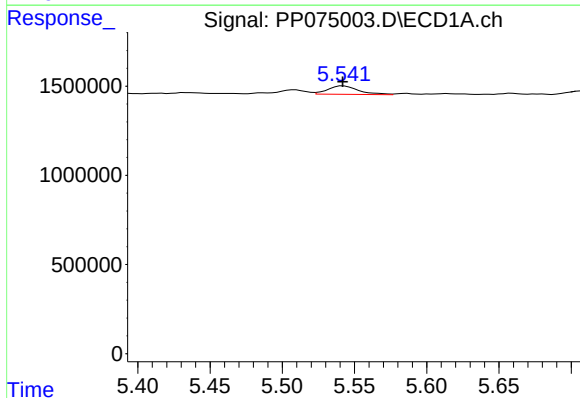


#12 AR-1232-2

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 703895
Conc: 44.67 ng/ml

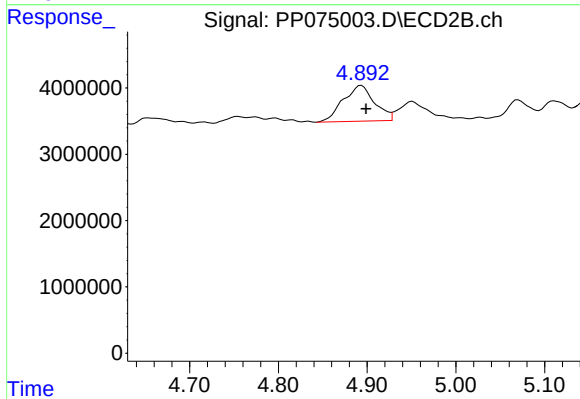

#12 AR-1232-2


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 13267273
Conc: 57.24 ng/ml

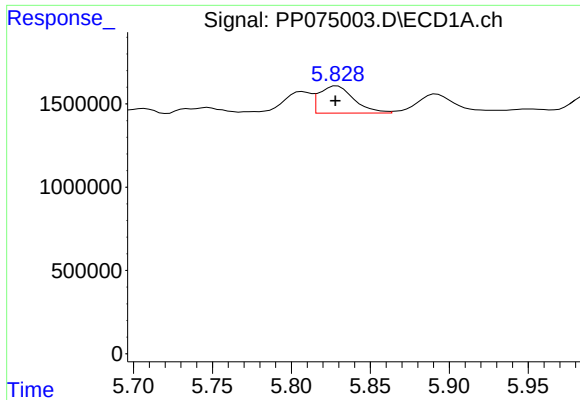

#13 AR-1232-3


R.T.: 5.829 min
Delta R.T.: 0.001 min
Response: 2500724
Conc: 81.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

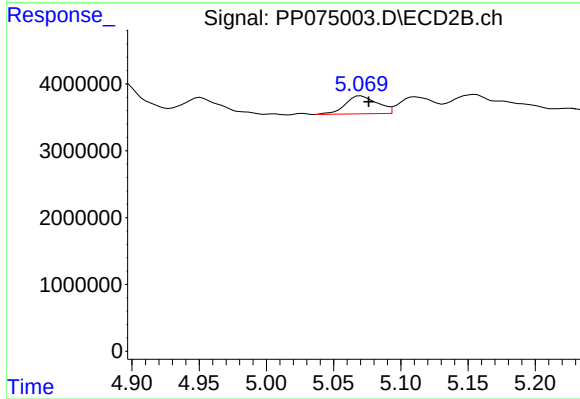


#13 AR-1232-3

R.T.: 5.070 min
Delta R.T.: -0.006 min
Response: 4462508
Conc: 74.30 ng/ml

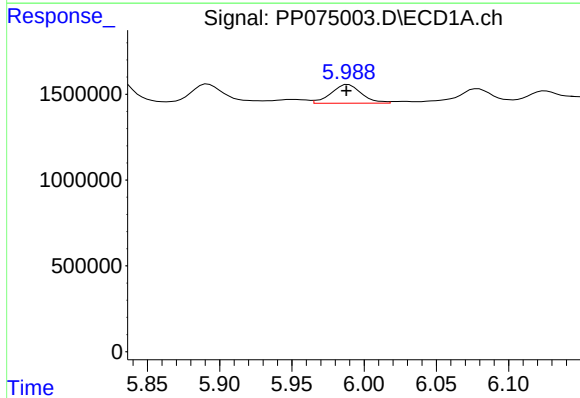


#14 AR-1232-4

R.T.: 5.989 min
Delta R.T.: 0.001 min
Response: 1585142
Conc: 91.79 ng/ml

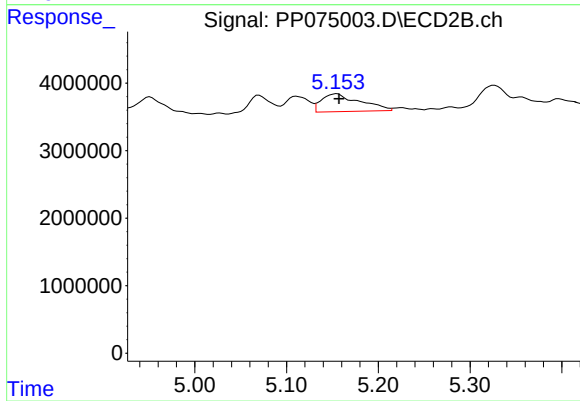

#14 AR-1232-4


R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 7718813
Conc: 104.72 ng/ml

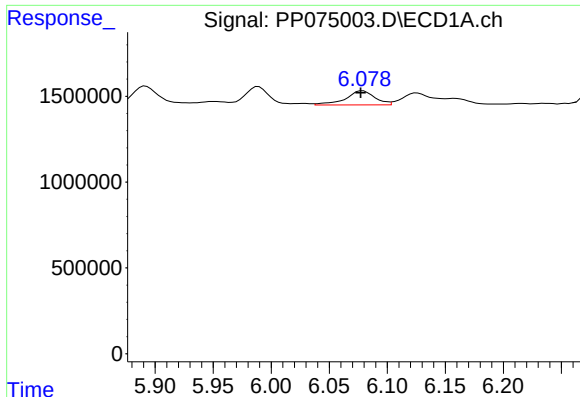

#15 AR-1232-5


R.T.: 6.079 min
Delta R.T.: 0.002 min
Response: 1440593
Conc: 110.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

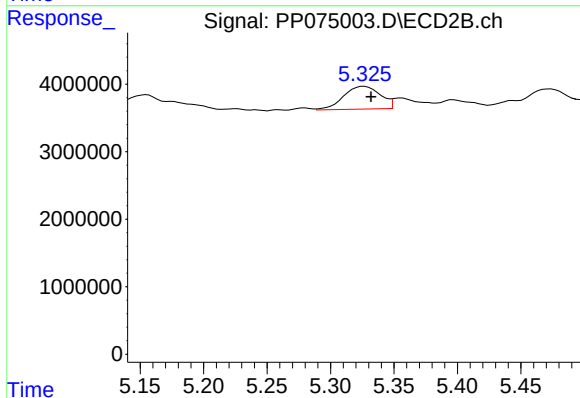


#15 AR-1232-5

R.T.: 5.326 min
Delta R.T.: -0.005 min
Response: 6752779
Conc: 108.77 ng/ml

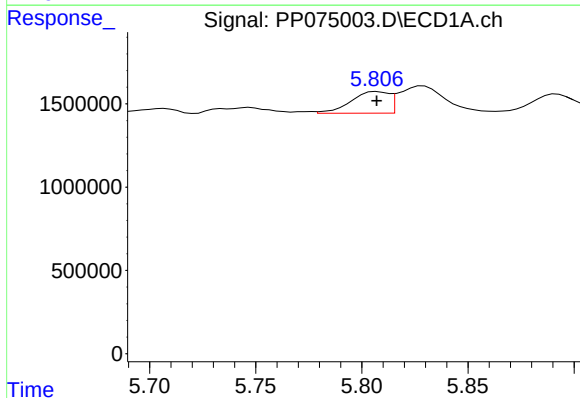


#16 AR-1242-1

R.T.: 5.807 min
Delta R.T.: 0.000 min
Response: 1608601
Conc: 42.03 ng/ml

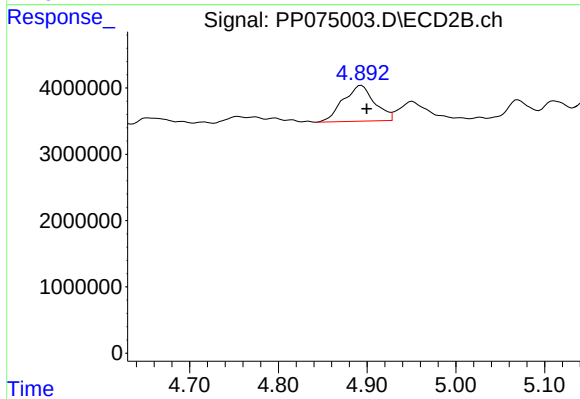

#16 AR-1242-1


R.T.: 4.894 min
Delta R.T.: -0.006 min
Response: 13267273
Conc: 31.46 ng/ml

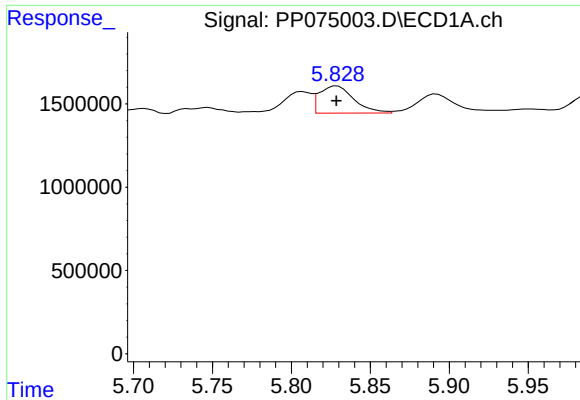

#17 AR-1242-2


R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 2500724
Conc: 44.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

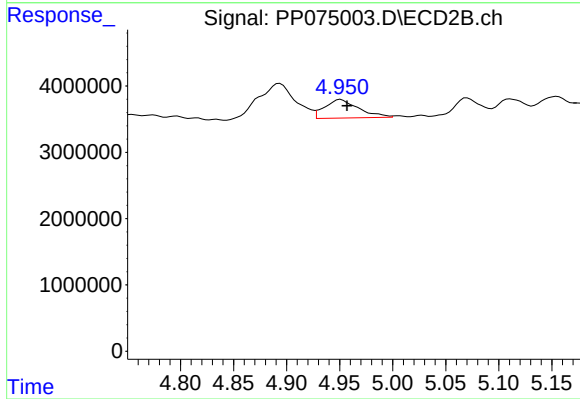


#17 AR-1242-2

R.T.: 4.951 min
Delta R.T.: -0.006 min
Response: 6213726
Conc: 31.02 ng/ml

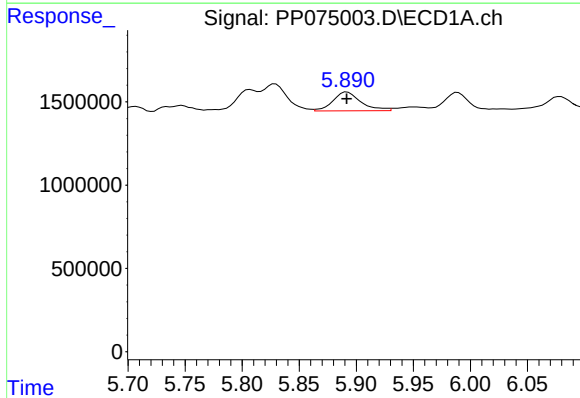


#18 AR-1242-3

R.T.: 5.892 min
Delta R.T.: 0.000 min
Response: 1944651
Conc: 47.89 ng/ml

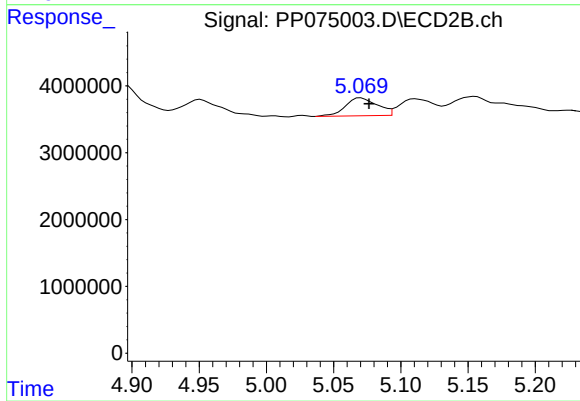

#18 AR-1242-3


R.T.: 5.070 min
Delta R.T.: -0.006 min
Response: 4462508
Conc: 37.72 ng/ml

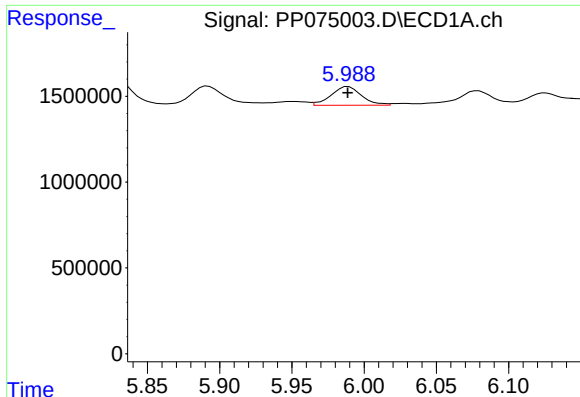

#19 AR-1242-4


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 1585142
Conc: 49.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

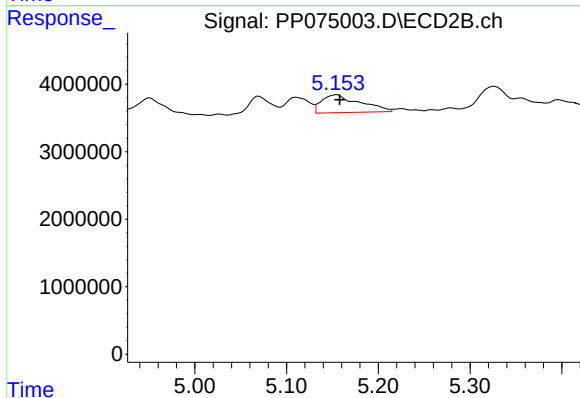


#19 AR-1242-4

R.T.: 5.155 min
Delta R.T.: -0.003 min
Response: 7718813
Conc: 45.10 ng/ml

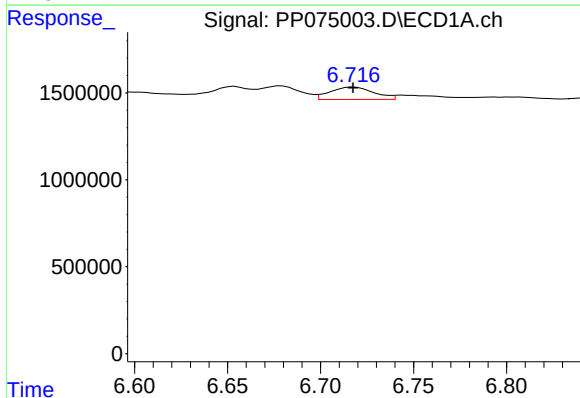


#20 AR-1242-5

R.T.: 6.718 min
Delta R.T.: 0.000 min
Response: 1163865
Conc: 32.27 ng/ml

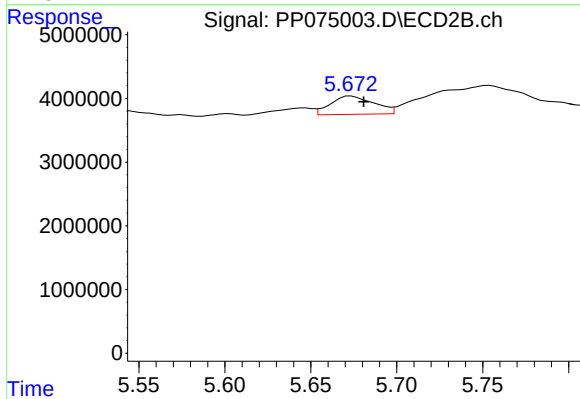

#20 AR-1242-5


R.T.: 5.673 min
Delta R.T.: -0.007 min
Response: 5065282
Conc: 27.36 ng/ml

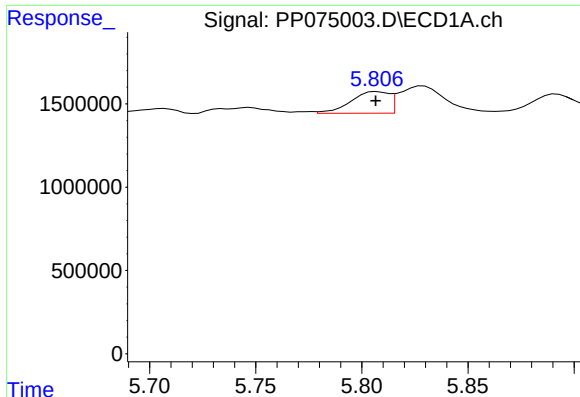

#21 AR-1248-1


R.T.: 5.807 min
Delta R.T.: 0.000 min
Response: 1608601
Conc: 53.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

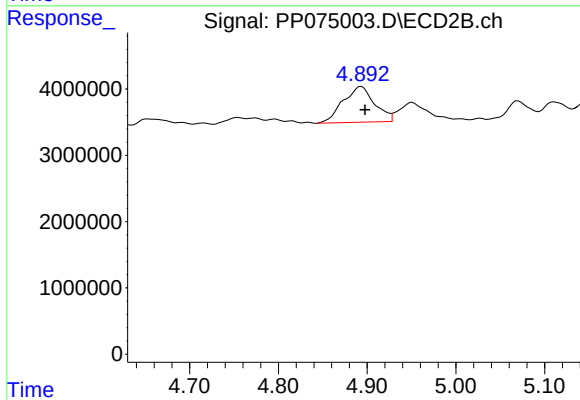


#21 AR-1248-1

R.T.: 4.894 min
Delta R.T.: -0.004 min
Response: 13267273
Conc: 48.04 ng/ml

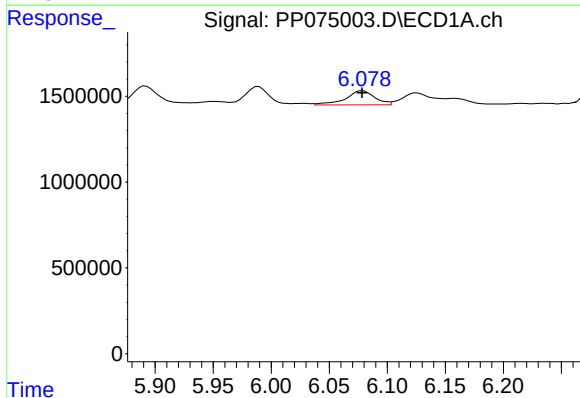


#22 AR-1248-2

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 1440593
Conc: 33.43 ng/ml

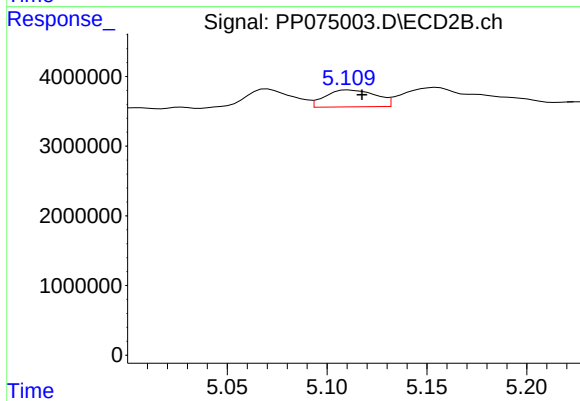

#22 AR-1248-2


R.T.: 5.111 min
Delta R.T.: -0.007 min
Response: 4277636
Conc: 24.20 ng/ml

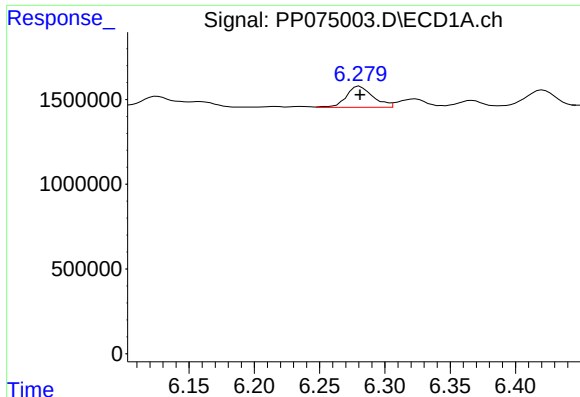

#23 AR-1248-3


R.T.: 6.281 min
Delta R.T.: 0.000 min
Response: 1757504
Conc: 37.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

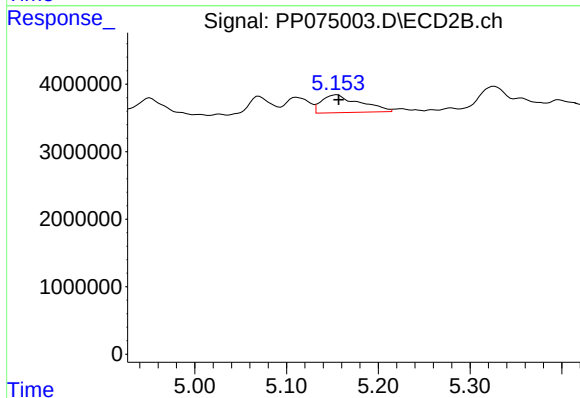


#23 AR-1248-3

R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 7718813
Conc: 33.97 ng/ml

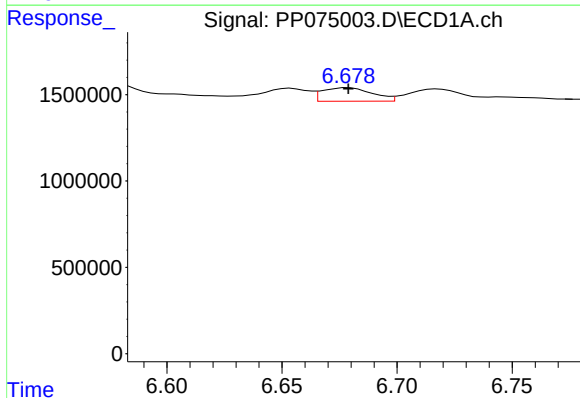


#24 AR-1248-4

R.T.: 6.679 min
Delta R.T.: 0.000 min
Response: 1189002
Conc: 21.62 ng/ml

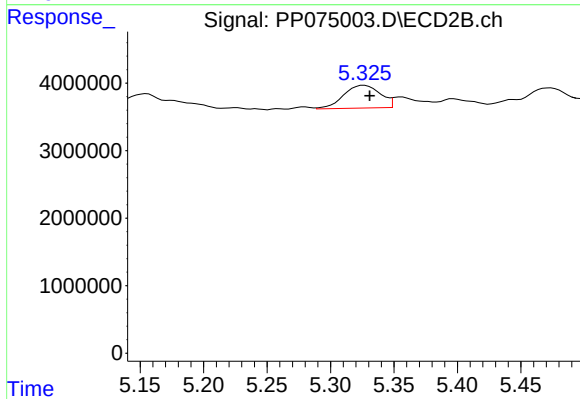

#24 AR-1248-4


R.T.: 5.326 min
Delta R.T.: -0.005 min
Response: 6752779
Conc: 30.97 ng/ml

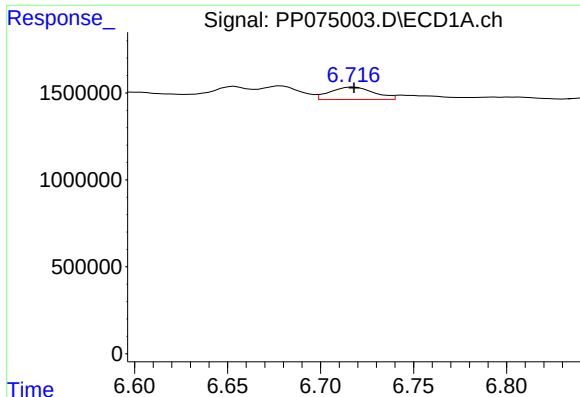

#25 AR-1248-5


R.T.: 6.718 min
Delta R.T.: 0.000 min
Response: 1163865
Conc: 20.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

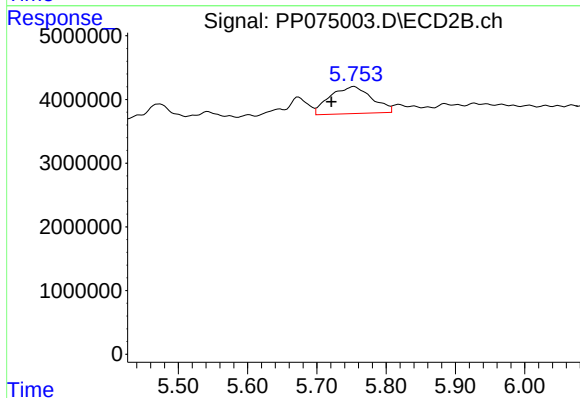


#25 AR-1248-5

R.T.: 5.754 min
Delta R.T.: 0.033 min
Response: 17890702
Conc: 48.71 ng/ml

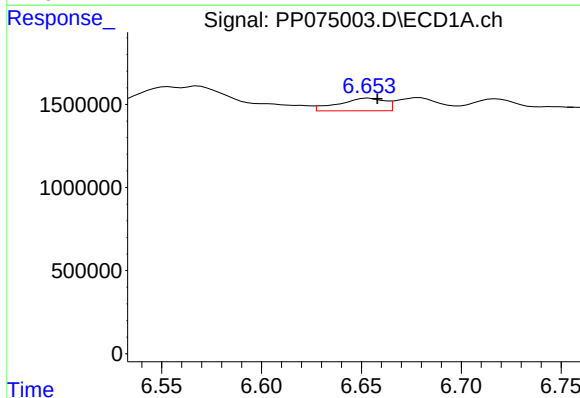


#26 AR-1254-1

R.T.: 6.654 min
Delta R.T.: -0.004 min
Response: 1228857
Conc: 21.09 ng/ml

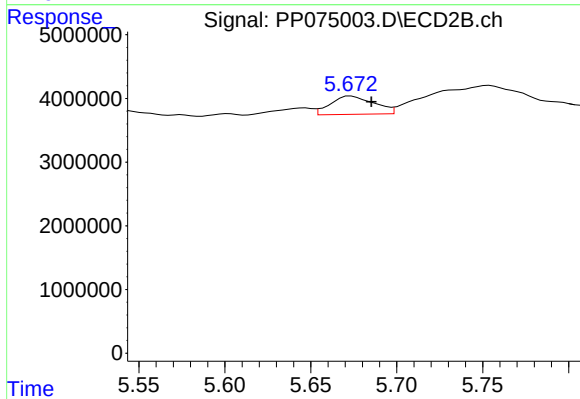

#26 AR-1254-1


R.T.: 5.673 min
Delta R.T.: -0.012 min
Response: 5065282
Conc: 10.63 ng/ml

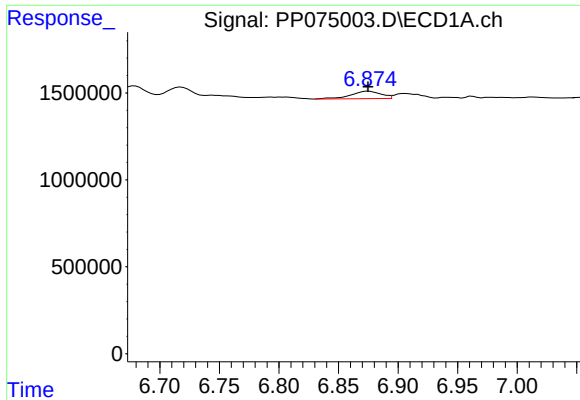

#27 AR-1254-2


R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 761679
Conc: 9.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

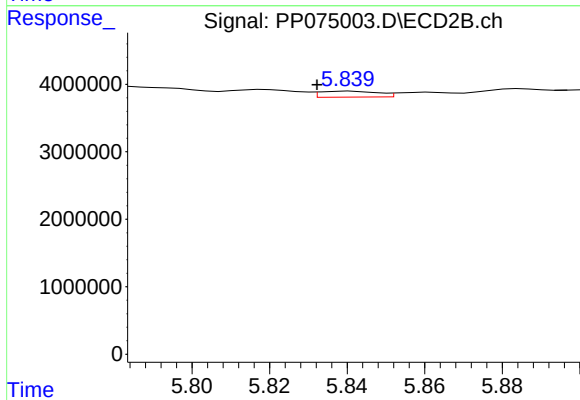


#27 AR-1254-2

R.T.: 5.841 min
Delta R.T.: 0.009 min
Response: 920239
Conc: 2.61 ng/ml

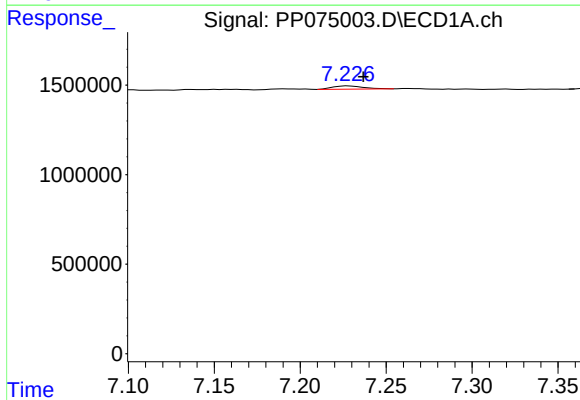


#28 AR-1254-3

R.T.: 7.228 min
Delta R.T.: -0.009 min
Response: 219467
Conc: 2.46 ng/ml

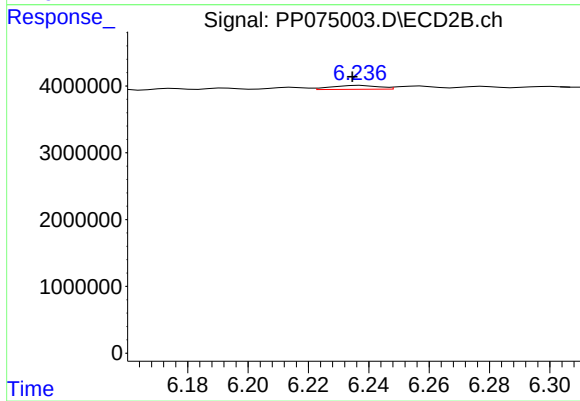

#28 AR-1254-3


R.T.: 6.237 min
Delta R.T.: 0.003 min
Response: 636761
Conc: 1.03 ng/ml

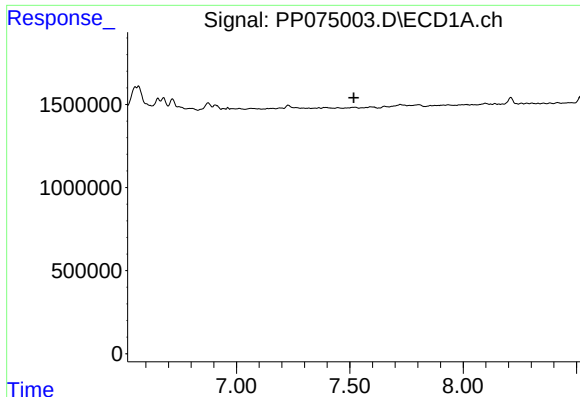

#29 AR-1254-4


R.T.: 0.000 min
Exp R.T.: 7.518 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

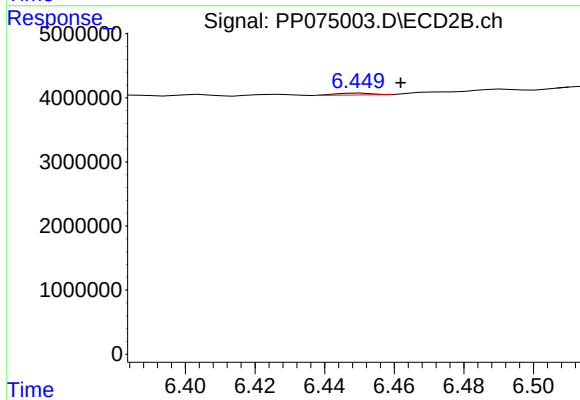


#29 AR-1254-4

R.T.: 6.450 min
Delta R.T.: -0.012 min
Response: 200181
Conc: 0.43 ng/ml

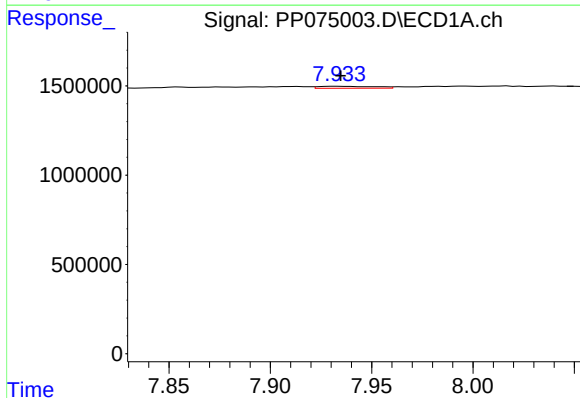


#30 AR-1254-5

R.T.: 7.934 min
Delta R.T.: 0.000 min
Response: 209030
Conc: 2.52 ng/ml

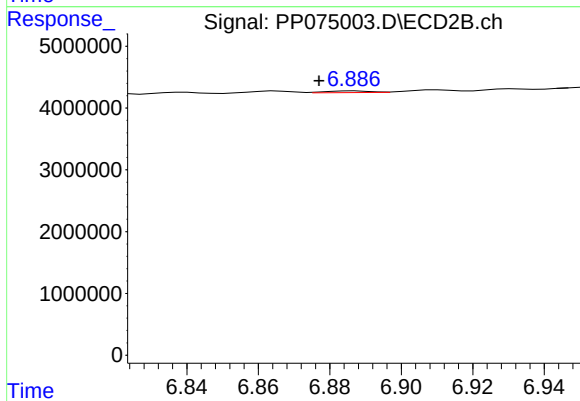

#30 AR-1254-5


R.T.: 6.887 min
Delta R.T.: 0.010 min
Response: 229587
Conc: 0.47 ng/ml

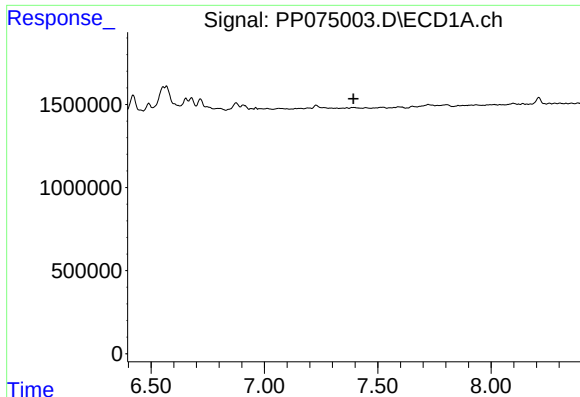

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

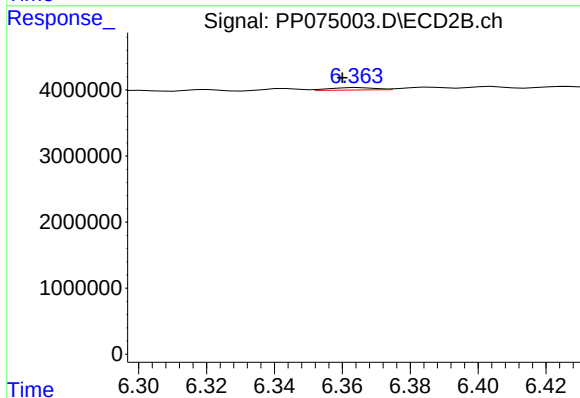


#31 AR-1260-1

R.T.: 6.365 min
Delta R.T.: 0.005 min
Response: 331415
Conc: 0.88 ng/ml

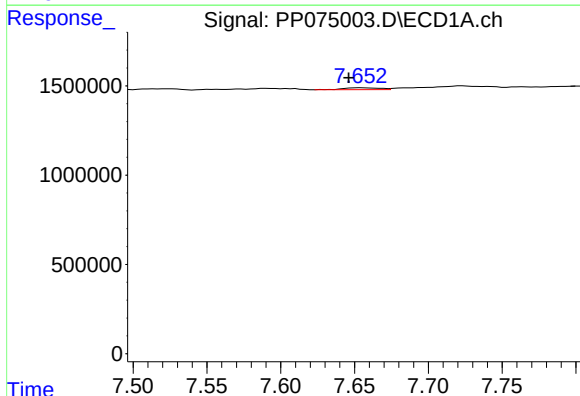


#32 AR-1260-2

R.T.: 7.653 min
Delta R.T.: 0.007 min
Response: 178123
Conc: 2.58 ng/ml

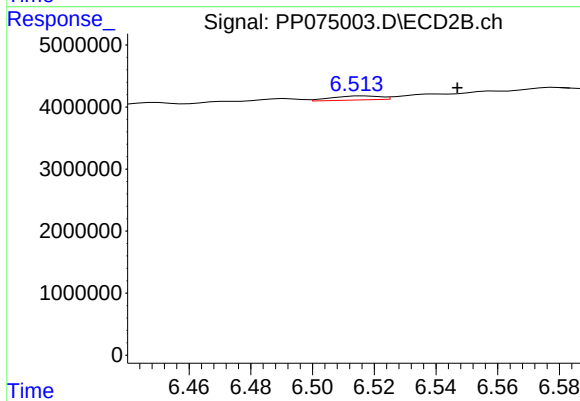

#32 AR-1260-2


R.T.: 6.517 min
Delta R.T.: -0.030 min
Response: 708667
Conc: 1.34 ng/ml

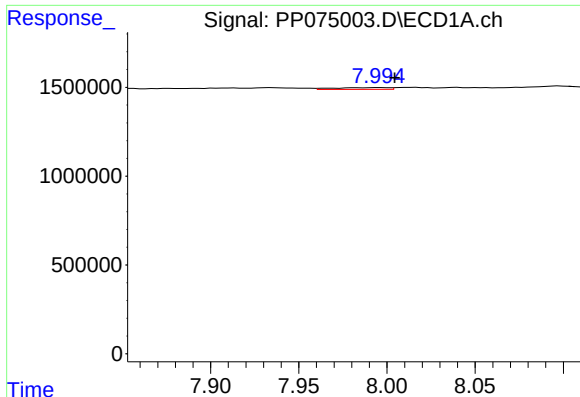

#33 AR-1260-3


R.T.: 7.995 min
Delta R.T.: -0.009 min
Response: 218141
Conc: 4.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

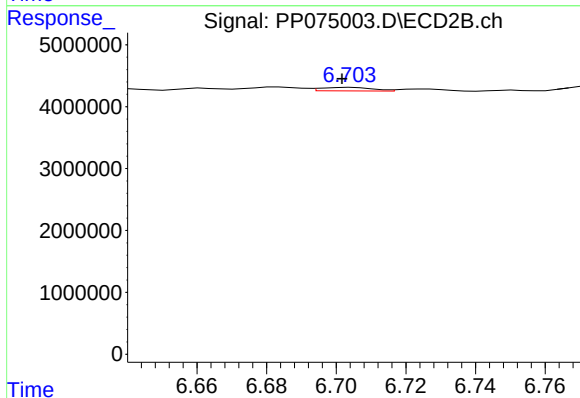


#33 AR-1260-3

R.T.: 6.704 min
Delta R.T.: 0.003 min
Response: 587059
Conc: 1.36 ng/ml

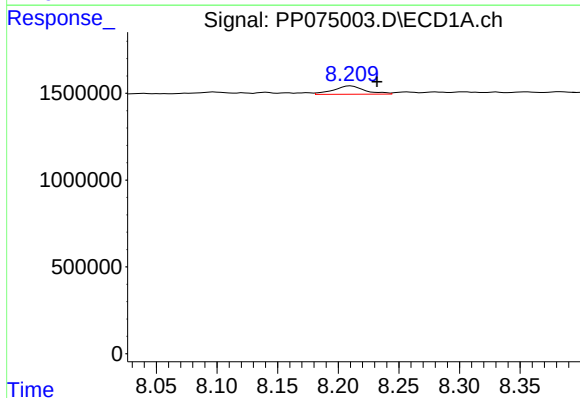


#34 AR-1260-4

R.T.: 8.210 min
Delta R.T.: -0.022 min
Response: 850389
Conc: 13.33 ng/ml

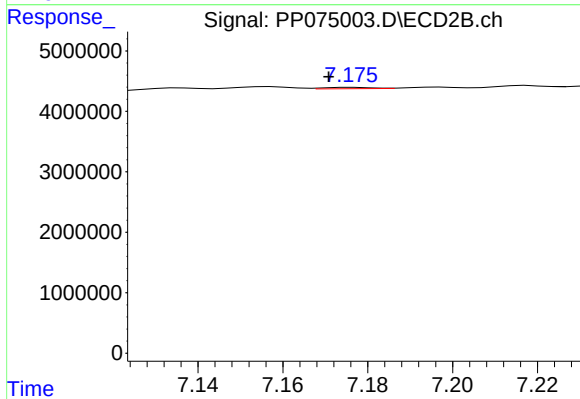

#34 AR-1260-4


R.T.: 7.177 min
Delta R.T.: 0.006 min
Response: 167631
Conc: 0.44 ng/ml

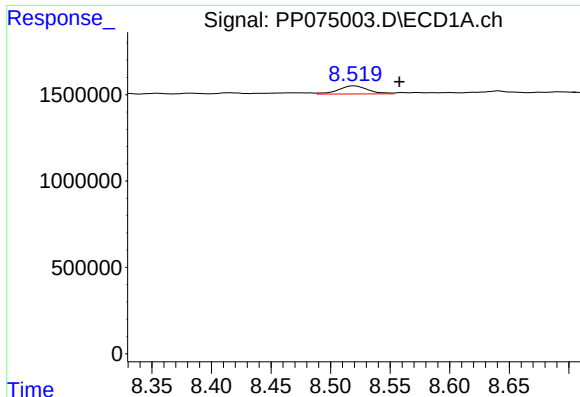

#35 AR-1260-5


R.T.: 8.520 min
Delta R.T.: -0.038 min
Response: 824248
Conc: 7.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

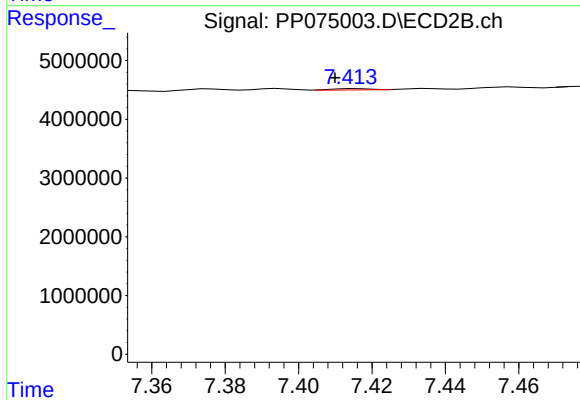


#35 AR-1260-5

R.T.: 7.416 min
Delta R.T.: 0.006 min
Response: 164408
Conc: 0.16 ng/ml

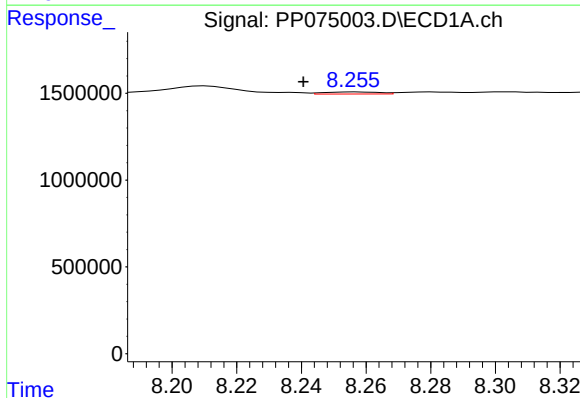


#36 AR-1262-1

R.T.: 8.257 min
Delta R.T.: 0.016 min
Response: 133005
Conc: 1.73 ng/ml

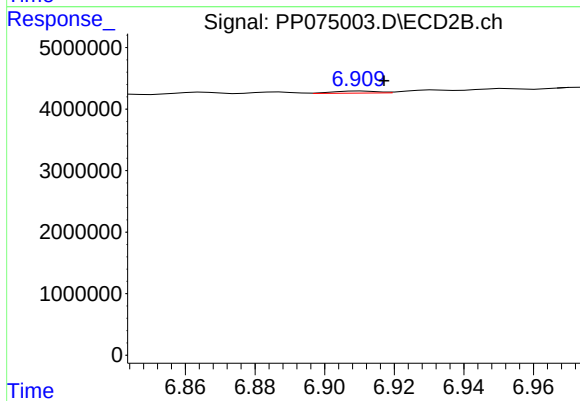

#36 AR-1262-1


R.T.: 6.910 min
Delta R.T.: -0.007 min
Response: 298683
Conc: 0.42 ng/ml

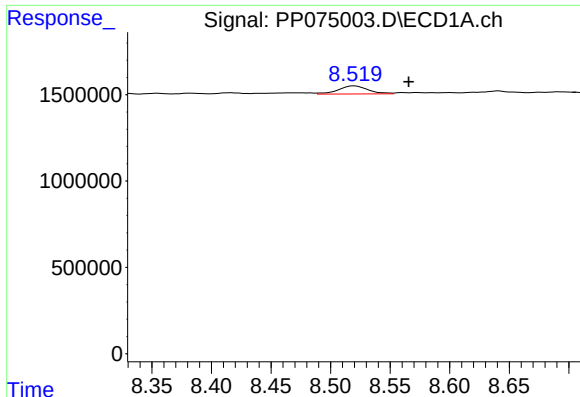

#37 AR-1262-2


R.T.: 8.520 min
Delta R.T.: -0.046 min
Response: 824248
Conc: 6.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

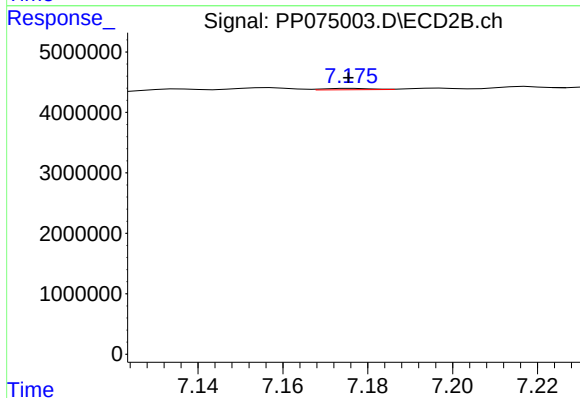


#37 AR-1262-2

R.T.: 7.177 min
Delta R.T.: 0.001 min
Response: 167631
Conc: 0.32 ng/ml

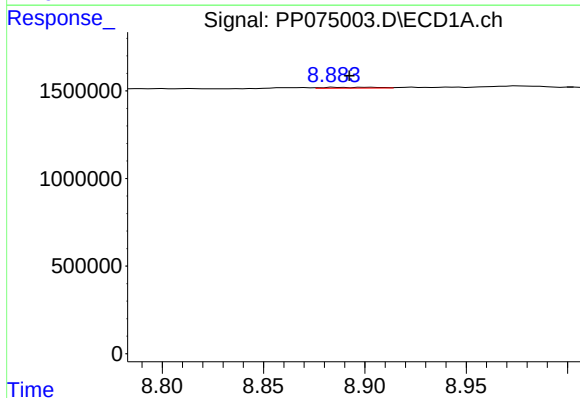


#38 AR-1262-3

R.T.: 8.885 min
Delta R.T.: -0.008 min
Response: 93051
Conc: 0.96 ng/ml

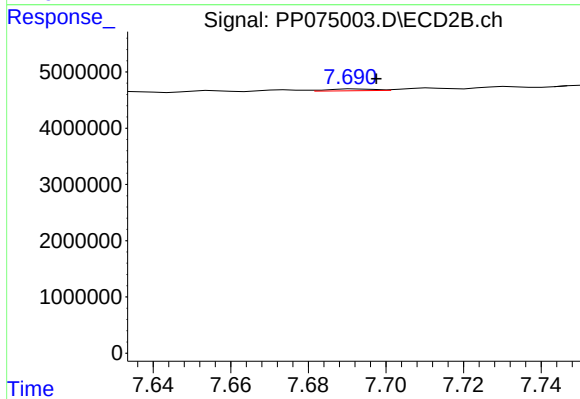

#38 AR-1262-3


R.T.: 7.692 min
Delta R.T.: -0.005 min
Response: 282851
Conc: 0.61 ng/ml

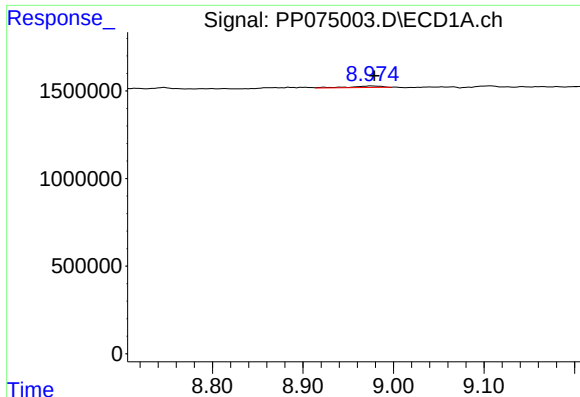

#39 AR-1262-4


R.T.: 8.976 min
Delta R.T.: -0.003 min
Response: 216844
Conc: 2.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

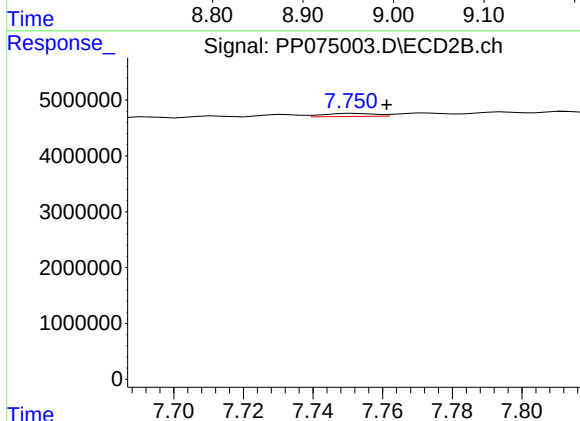


#39 AR-1262-4

R.T.: 7.752 min
Delta R.T.: -0.009 min
Response: 552829
Conc: 0.67 ng/ml

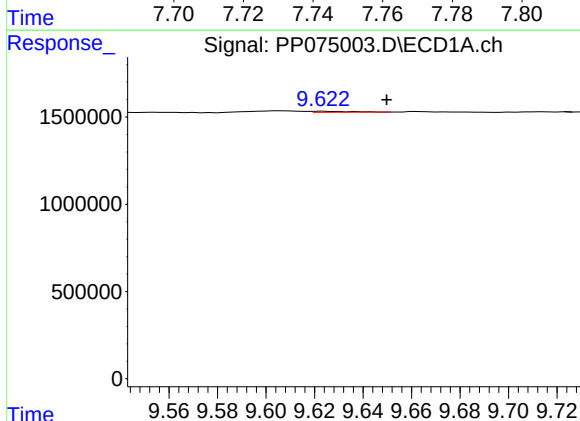


#40 AR-1262-5

R.T.: 9.624 min
Delta R.T.: -0.026 min
Response: 62676
Conc: 1.03 ng/ml

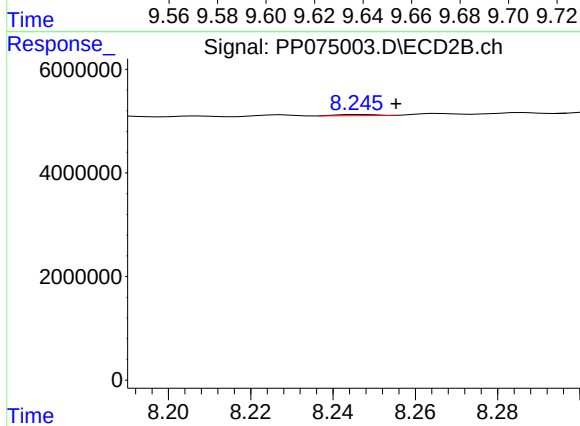

#40 AR-1262-5


R.T.: 8.247 min
Delta R.T.: -0.009 min
Response: 147296
Conc: 0.41 ng/ml

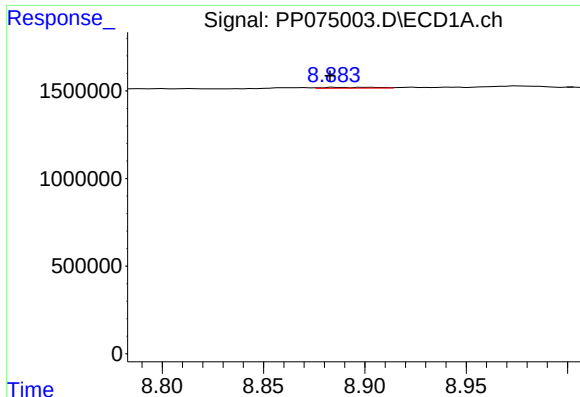

#41 AR-1268-1


R.T.: 8.885 min
Delta R.T.: 0.002 min
Response: 93051
Conc: 0.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

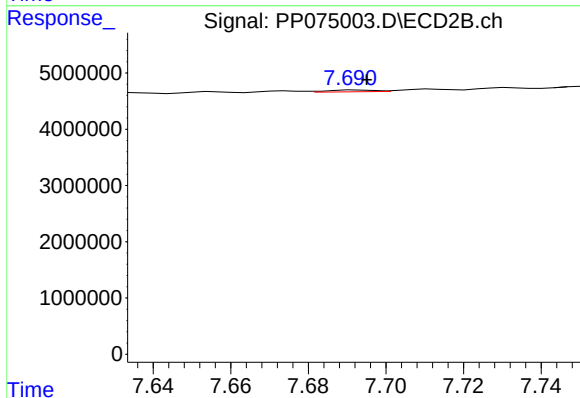


#41 AR-1268-1

R.T.: 7.692 min
Delta R.T.: -0.003 min
Response: 282851
Conc: 0.20 ng/ml

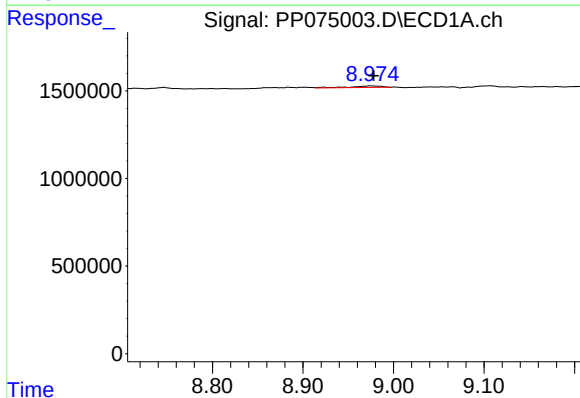


#42 AR-1268-2

R.T.: 8.976 min
Delta R.T.: -0.003 min
Response: 216844
Conc: 1.48 ng/ml

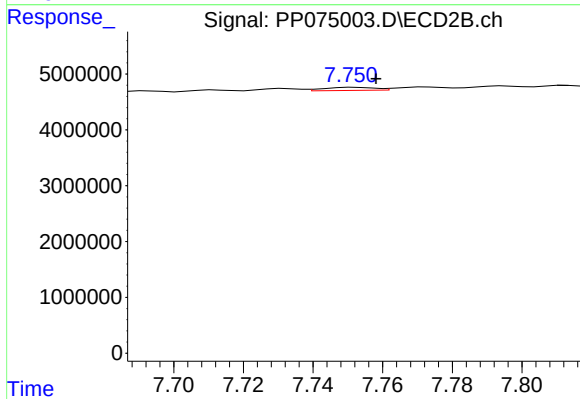

#42 AR-1268-2


R.T.: 7.752 min
Delta R.T.: -0.006 min
Response: 552829
Conc: 0.41 ng/ml

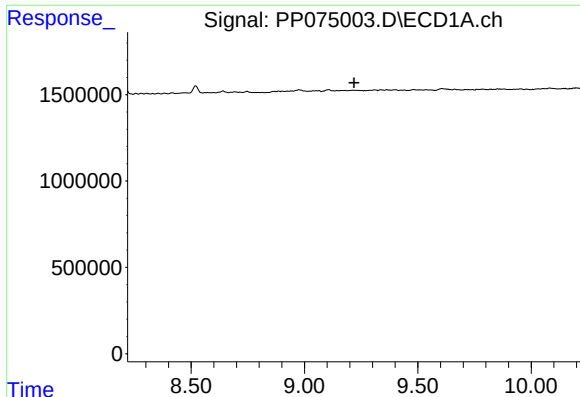

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

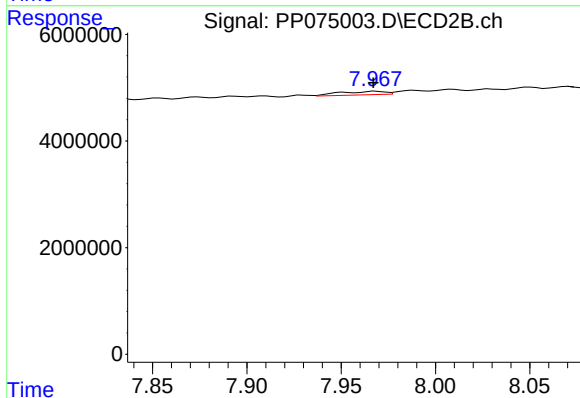


#43 AR-1268-3

R.T.: 7.968 min
Delta R.T.: 0.001 min
Response: 1086791
Conc: 1.04 ng/ml

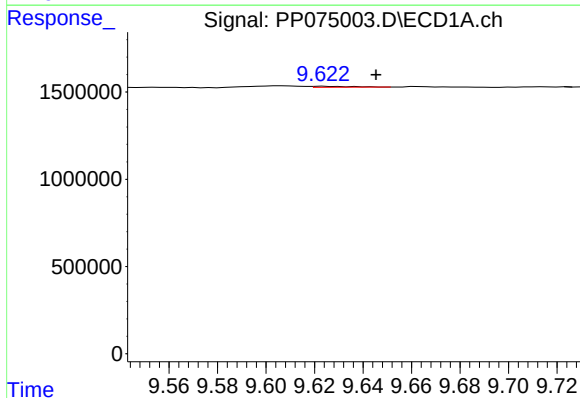


#44 AR-1268-4

R.T.: 9.624 min
Delta R.T.: -0.022 min
Response: 62676
Conc: 0.93 ng/ml

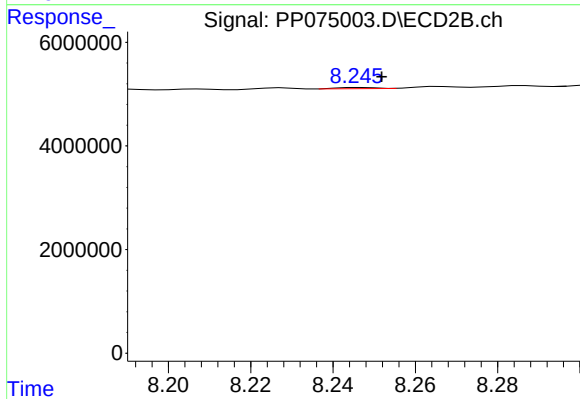

#44 AR-1268-4


R.T.: 8.247 min
Delta R.T.: -0.005 min
Response: 147296
Conc: 0.38 ng/ml

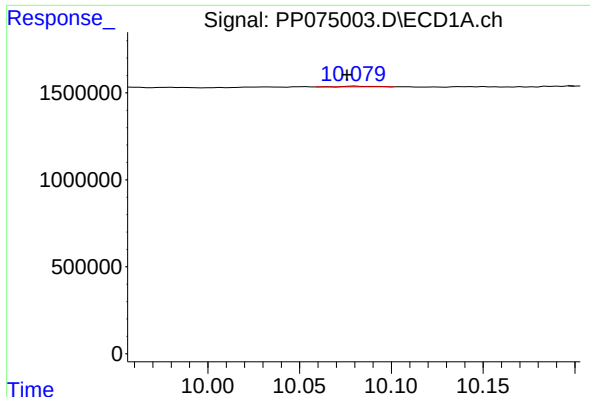

#45 AR-1268-5

R.T.: 10.080 min
Delta R.T.: 0.005 min
Response: 44057
Conc: 0.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-B

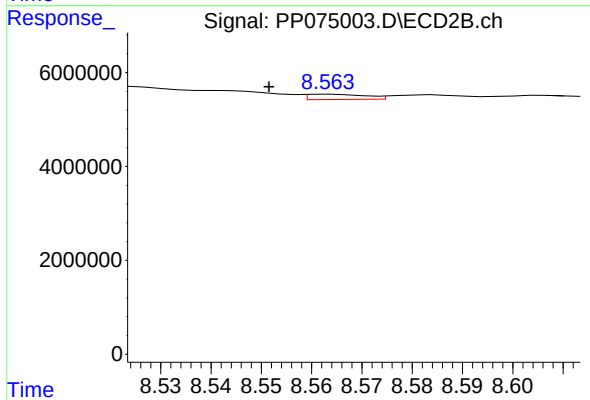

#45 AR-1268-5

R.T.: 8.564 min
Delta R.T.: 0.012 min
Response: 898381
Conc: 0.29 ng/ml