

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 14:08
 Operator : YP\AJ
 Sample : Q3034-03
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-C

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:49:20 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.655	3.797	27527751	103.9E6	22.496	21.486
2)	SA Decachlor...	10.429	8.805	22700418	137.8E6	22.988	18.371
Target Compounds							
3)	L1 AR-1016-1	5.806	4.894	26665718	272.8E6	604.818	535.603
4)	L1 AR-1016-2	5.828	4.952	39531291	146.3E6	629.062	614.487
5)	L1 AR-1016-3	5.890	5.072	26956477	86253503	600.181	625.462
6)	L1 AR-1016-4	5.987	5.114	26176446	93492287	744.033	668.742
7)	L1 AR-1016-5	6.279	5.327	31754552	131.9E6	956.864	794.363
8)	L2 AR-1221-1	4.853	4.019	1016582	840836	57.784	13.591 #
9)	L2 AR-1221-2	4.941	4.097	1130860	2568555	84.663	56.811 #
10)	L2 AR-1221-3	5.016	4.169	2798202	9785012	73.806	59.558
11)	L3 AR-1232-1	5.016	4.169	2798202	9785012	92.125	76.388
12)	L3 AR-1232-2	5.542	4.894	13556582	272.8E6	860.286	1176.959 #
13)	L3 AR-1232-3	5.828	5.072	39531291	86253503	1294.254	1436.128
14)	L3 AR-1232-4	5.987	5.156	26176446	155.4E6	1515.782	2108.606 #
15)	L3 AR-1232-5	6.077	5.327	22804631	131.9E6	1756.776	2125.039
16)	L4 AR-1242-1	5.806	4.894	26665718	272.8E6	696.684	646.851
17)	L4 AR-1242-2	5.828	4.952	39531291	146.3E6	699.892	730.255
18)	L4 AR-1242-3	5.890	5.072	26956477	86253503	663.905	729.119
19)	L4 AR-1242-4	5.987	5.156	26176446	155.4E6	824.667	908.041
20)	L4 AR-1242-5	6.716	5.677	18048277	110.1E6	500.360	594.342
21)	L5 AR-1248-1	5.806	4.894	26665718	272.8E6	882.269	987.936
22)	L5 AR-1248-2	6.077	5.114	22804631	93492287	529.158	528.936
23)	L5 AR-1248-3	6.279	5.156	31754552	155.4E6	679.916	684.056
24)	L5 AR-1248-4	6.677	5.327	18143074	131.9E6	329.869	605.127 #
25)	L5 AR-1248-5	6.716	5.717	18048277	102.1E6	325.367	277.833
26)	L6 AR-1254-1	6.652	5.677	14560283	110.1E6	249.879	230.854
27)	L6 AR-1254-2	6.873	5.822	12114687	15860016	148.435	45.040 #
28)	L6 AR-1254-3	7.232	6.225	1738102	6868152	19.484	11.081 #
29)	L6 AR-1254-4	7.512	6.459	705454	2119804	10.703	4.523 #
30)	L6 AR-1254-5	7.928	6.869	388891	604493	4.681	1.232 #
31)	L7 AR-1260-1	7.395	6.362	232802	1202680	4.027	3.205
32)	L7 AR-1260-2	7.651	6.552	347133	2310707	5.037	4.370
33)	L7 AR-1260-3	8.006	6.697	256013	794962	4.934	1.836 #
34)	L7 AR-1260-4	8.246	7.160	61594	965538	0.966	2.531 #
35)	L7 AR-1260-5	8.554	7.414	248980	796975	2.195	0.793 #
36)	L8 AR-1262-1	8.246	6.908	61594	275243	0.800	0.389 #
37)	L8 AR-1262-2	8.554	7.182	248980	657752	1.881	1.263 #
38)	L8 AR-1262-3	8.895	7.697	71132	815285	0.732	1.748 #
39)	L8 AR-1262-4	8.974	7.758	162459	517086	2.157	0.629 #
40)	L8 AR-1262-5	9.611f	8.253	303316	192039	4.976	0.536 #
41)	L9 AR-1268-1	8.874	7.697	78497	815285	0.484	0.578

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 14:08
Operator : YP\AJ
Sample : Q3034-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.974	7.758	162459	517086	1.107	0.379 #
43)	L9 AR-1268-3	0.000	7.960	0	768367	N.D.	0.737 #
44)	L9 AR-1268-4	9.611	8.253	303316	192039	4.509	0.501 #
45)	L9 AR-1268-5	10.078	8.556	178366	1207061	0.482	0.385



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 14:08
Operator : YP\AJ
Sample : Q3034-03
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:20 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

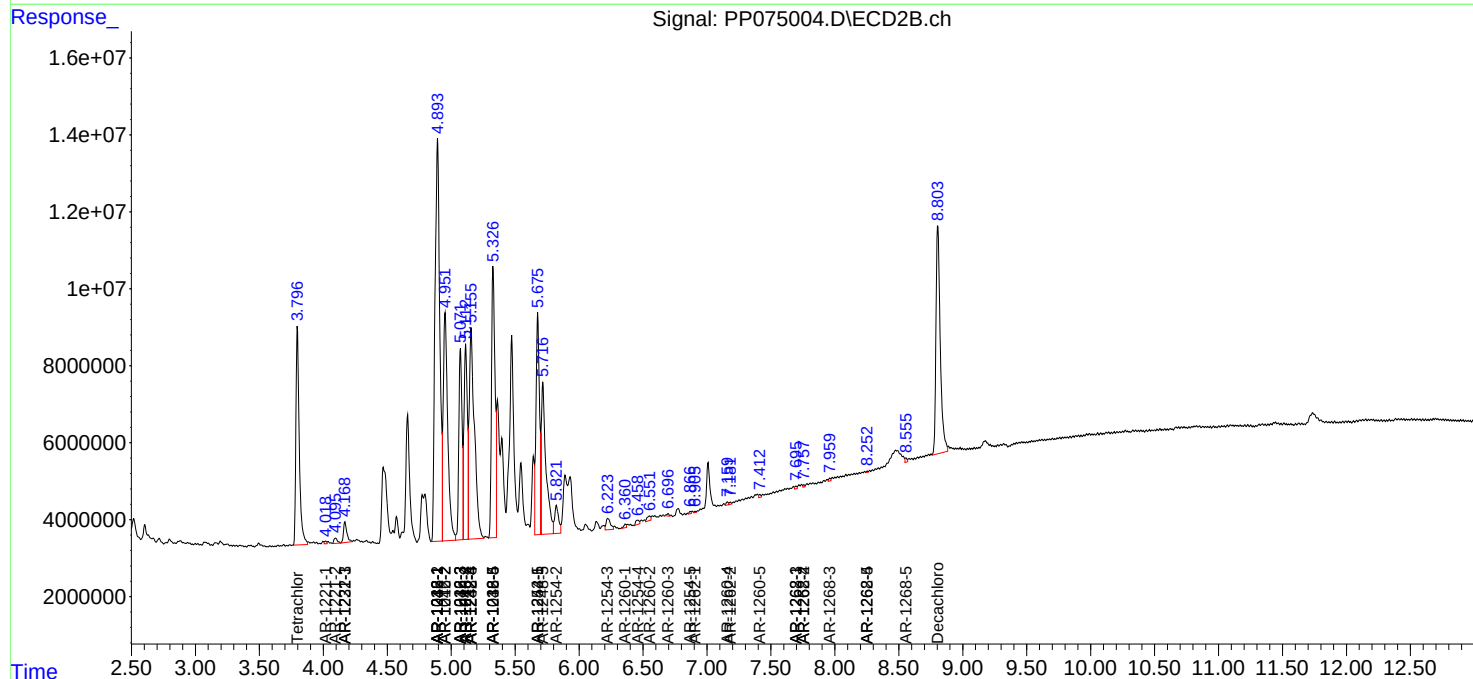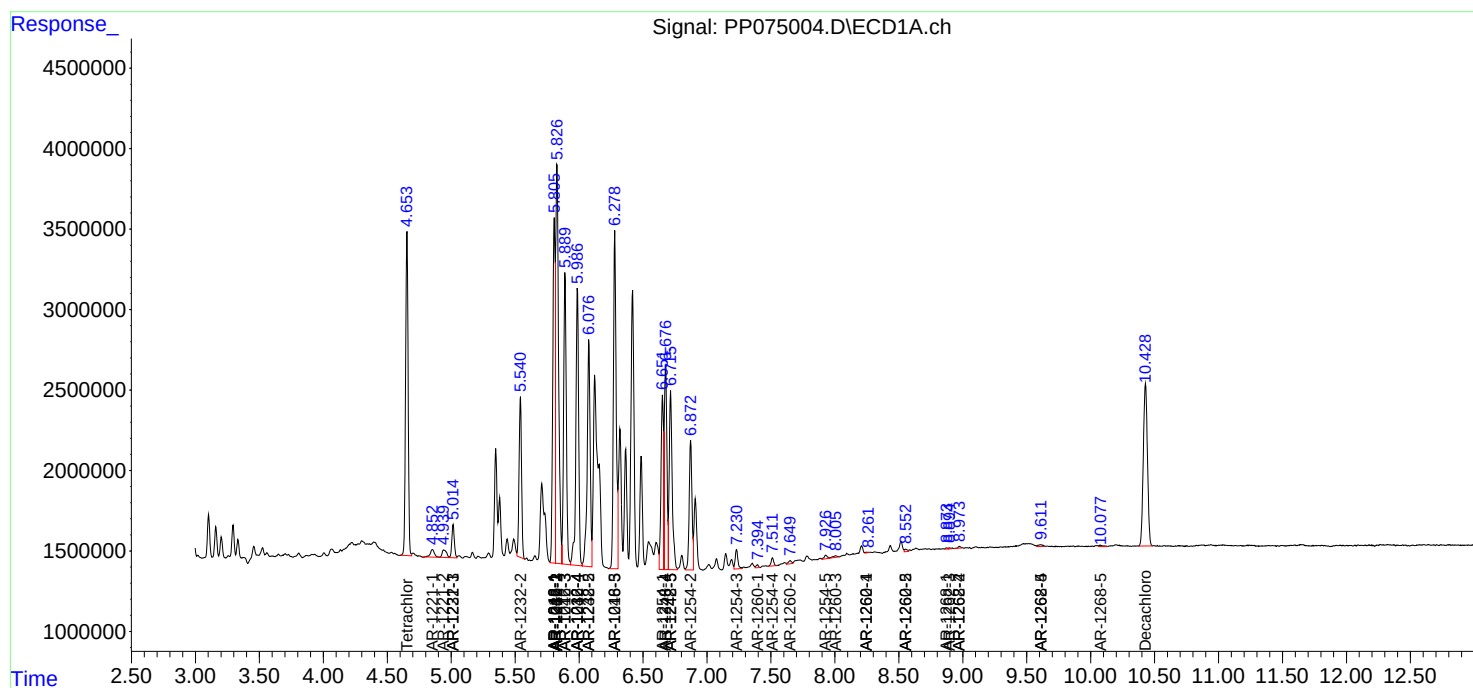


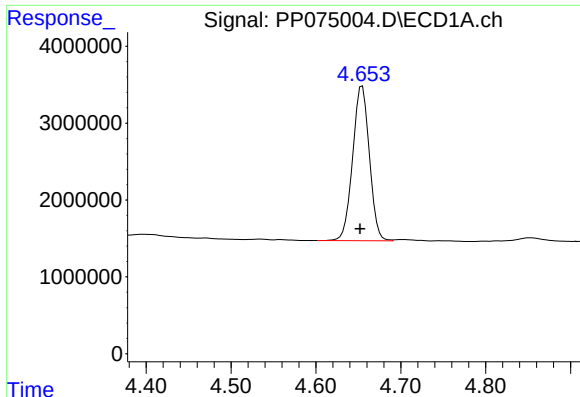

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: 0.003 min
Response: 27527751
Conc: 22.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

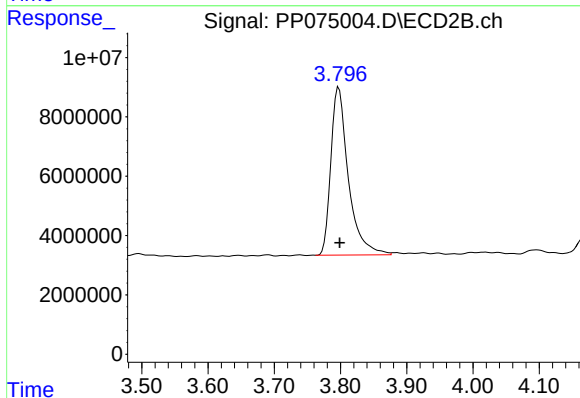


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: -0.001 min
Response: 103893638
Conc: 21.49 ng/ml

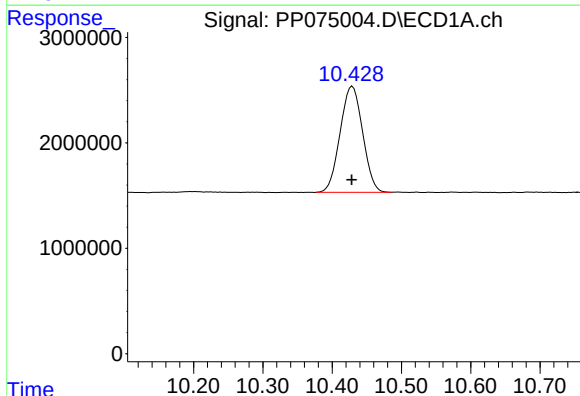


#2 Decachlorobiphenyl

R.T.: 10.429 min
Delta R.T.: 0.001 min
Response: 22700418
Conc: 22.99 ng/ml

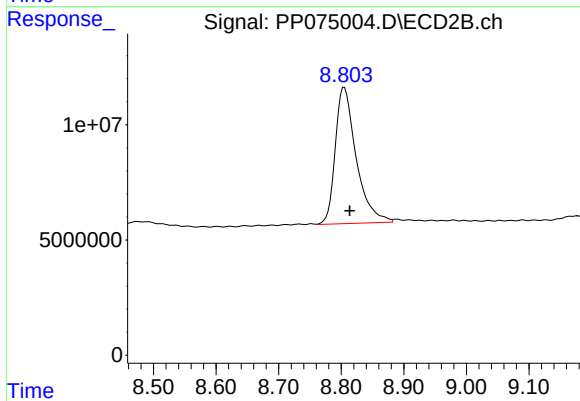

#2 Decachlorobiphenyl


R.T.: 8.805 min
Delta R.T.: -0.009 min
Response: 137768633
Conc: 18.37 ng/ml

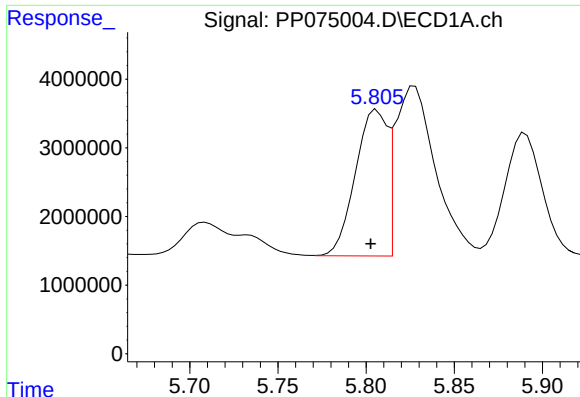

#3 AR-1016-1


R.T.: 5.806 min
Delta R.T.: 0.003 min
Response: 26665718
Conc: 604.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

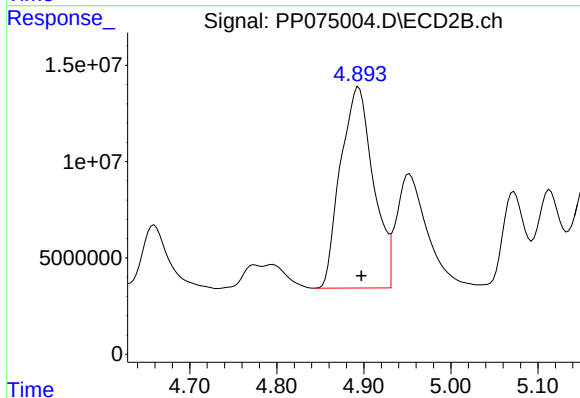


#3 AR-1016-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 272811386
Conc: 535.60 ng/ml

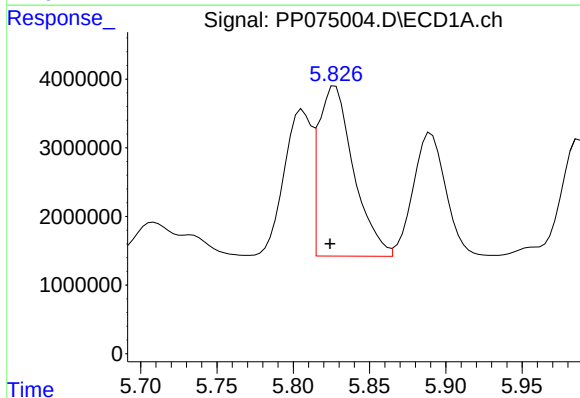


#4 AR-1016-2

R.T.: 5.828 min
Delta R.T.: 0.004 min
Response: 39531291
Conc: 629.06 ng/ml

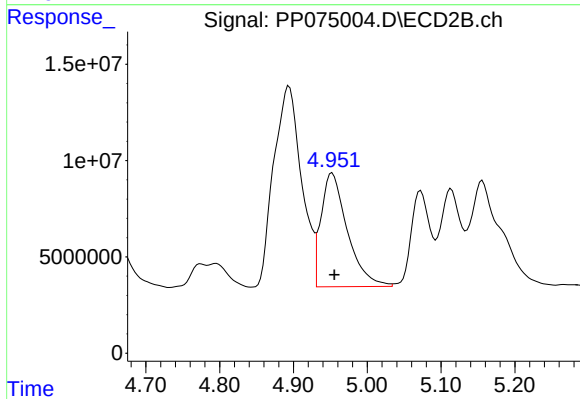

#4 AR-1016-2


R.T.: 4.952 min
Delta R.T.: -0.003 min
Response: 146257450
Conc: 614.49 ng/ml

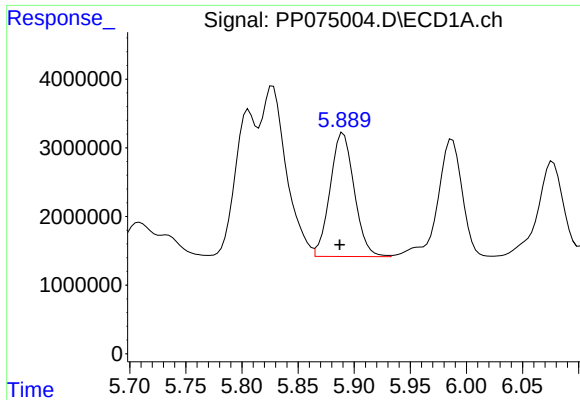

#5 AR-1016-3


R.T.: 5.890 min
Delta R.T.: 0.003 min
Response: 26956477
Conc: 600.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

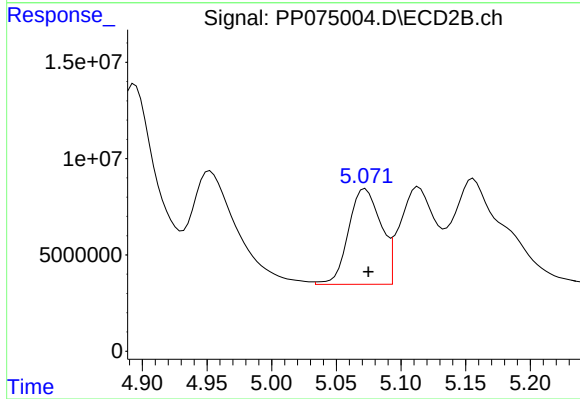


#5 AR-1016-3

R.T.: 5.072 min
Delta R.T.: -0.002 min
Response: 86253503
Conc: 625.46 ng/ml

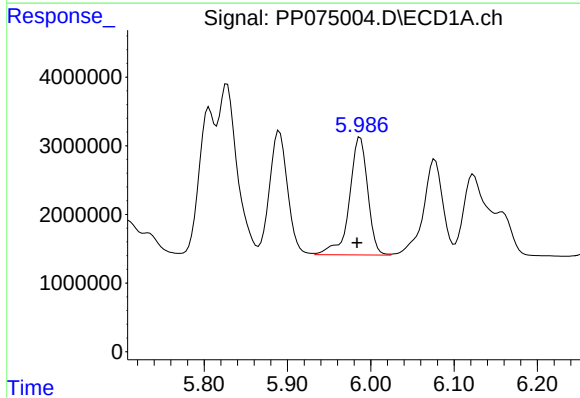


#6 AR-1016-4

R.T.: 5.987 min
Delta R.T.: 0.004 min
Response: 26176446
Conc: 744.03 ng/ml

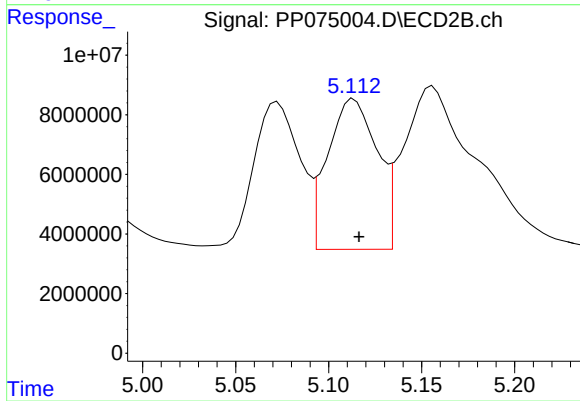

#6 AR-1016-4


R.T.: 5.114 min
Delta R.T.: -0.003 min
Response: 93492287
Conc: 668.74 ng/ml

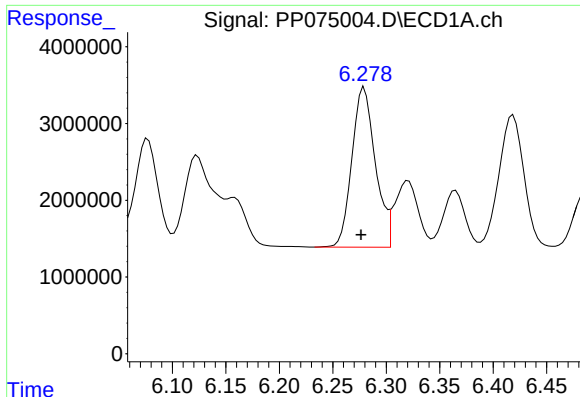

#7 AR-1016-5


R.T.: 6.279 min
Delta R.T.: 0.003 min
Response: 31754552
Conc: 956.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

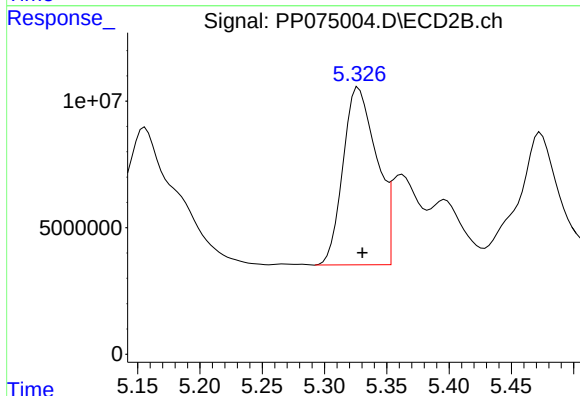


#7 AR-1016-5

R.T.: 5.327 min
Delta R.T.: -0.003 min
Response: 131930478
Conc: 794.36 ng/ml

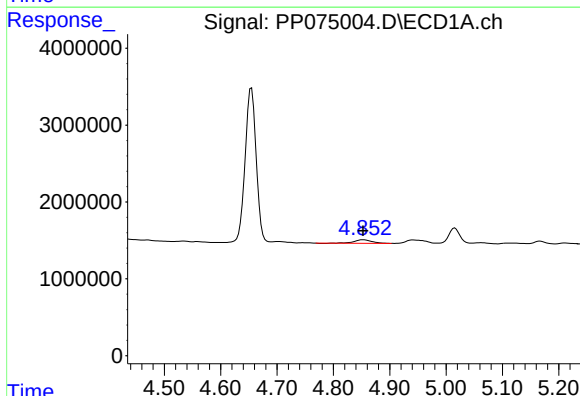


#8 AR-1221-1

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 1016582
Conc: 57.78 ng/ml

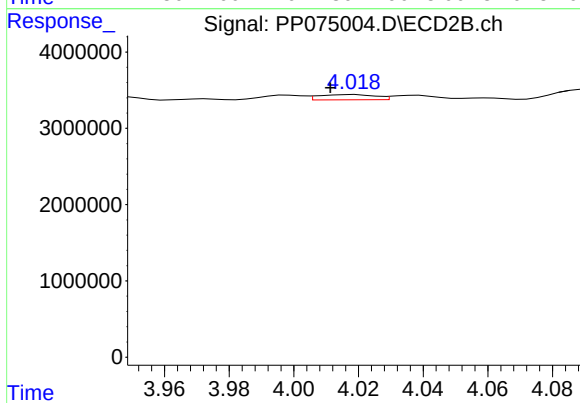

#8 AR-1221-1


R.T.: 4.019 min
Delta R.T.: 0.007 min
Response: 840836
Conc: 13.59 ng/ml

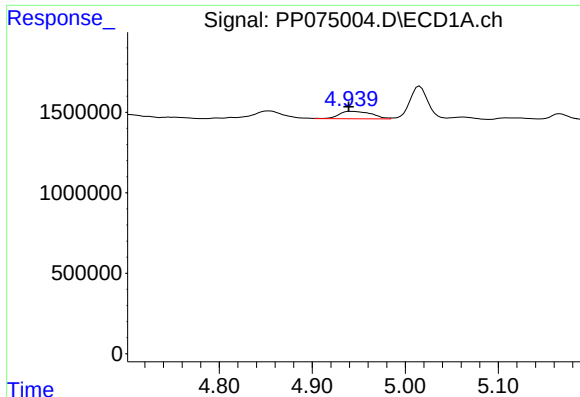

#9 AR-1221-2


R.T.: 4.941 min
Delta R.T.: 0.002 min
Response: 1130860
Conc: 84.66 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

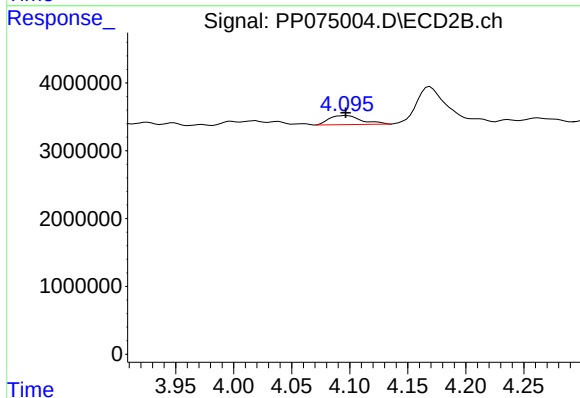


#9 AR-1221-2

R.T.: 4.097 min
Delta R.T.: 0.000 min
Response: 2568555
Conc: 56.81 ng/ml

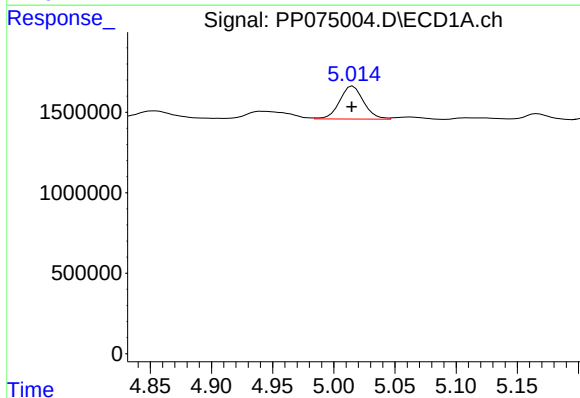


#10 AR-1221-3

R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 2798202
Conc: 73.81 ng/ml

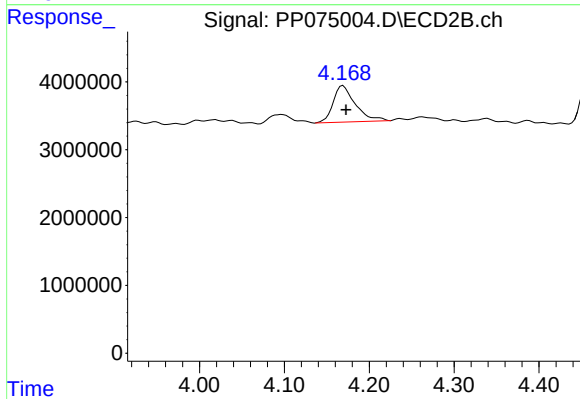

#10 AR-1221-3


R.T.: 4.169 min
Delta R.T.: -0.004 min
Response: 9785012
Conc: 59.56 ng/ml

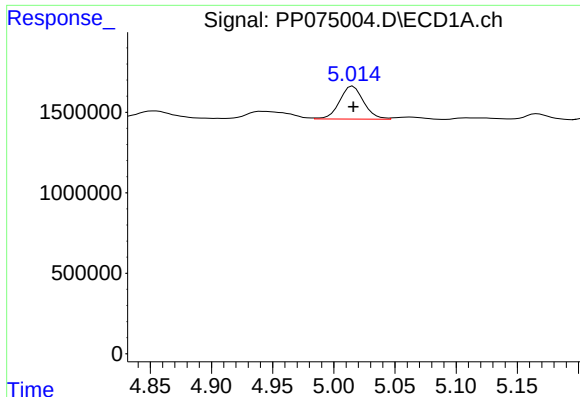

#11 AR-1232-1


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 2798202
Conc: 92.13 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

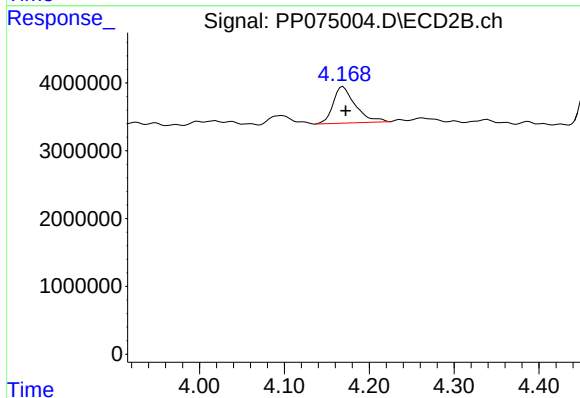


#11 AR-1232-1

R.T.: 4.169 min
Delta R.T.: -0.003 min
Response: 9785012
Conc: 76.39 ng/ml

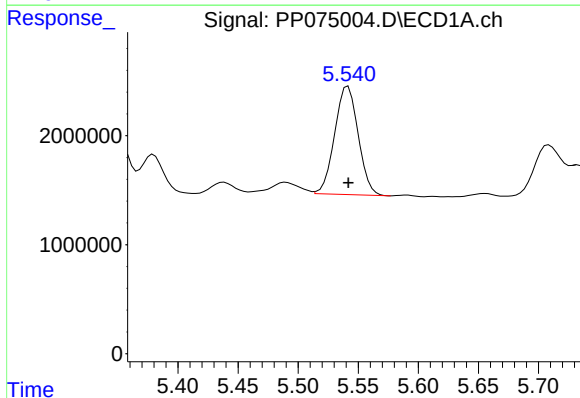


#12 AR-1232-2

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 13556582
Conc: 860.29 ng/ml

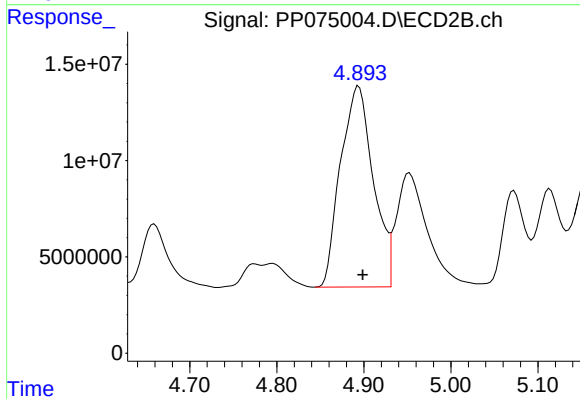

#12 AR-1232-2


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 272811386
Conc: 1176.96 ng/ml

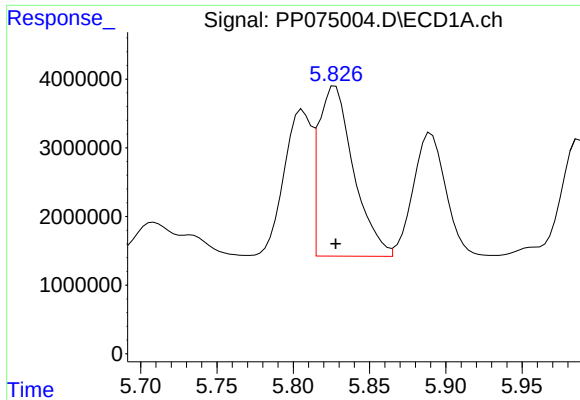

#13 AR-1232-3


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 39531291
Conc: 1294.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

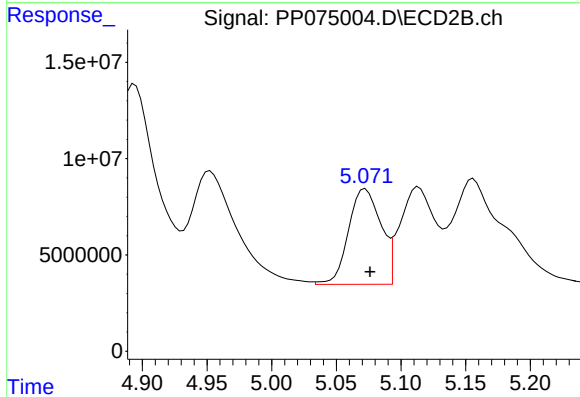


#13 AR-1232-3

R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 86253503
Conc: 1436.13 ng/ml

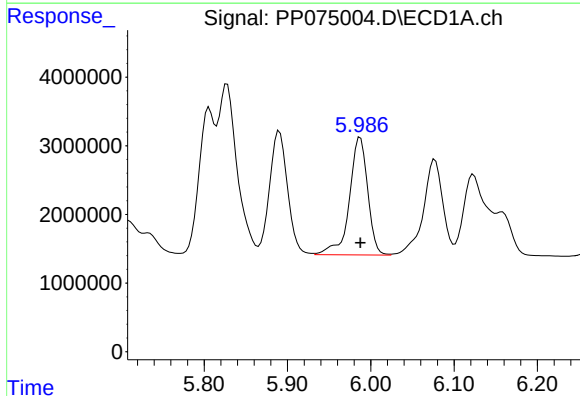


#14 AR-1232-4

R.T.: 5.987 min
Delta R.T.: 0.000 min
Response: 26176446
Conc: 1515.78 ng/ml

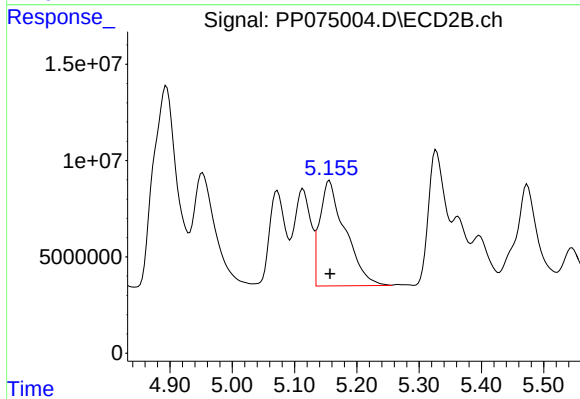

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: -0.001 min
Response: 155419815
Conc: 2108.61 ng/ml

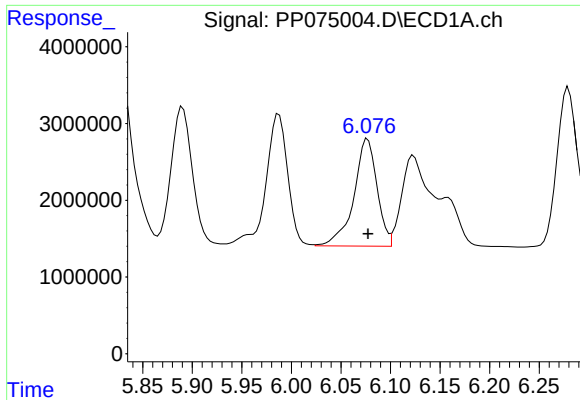

#15 AR-1232-5


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 22804631
Conc: 1756.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

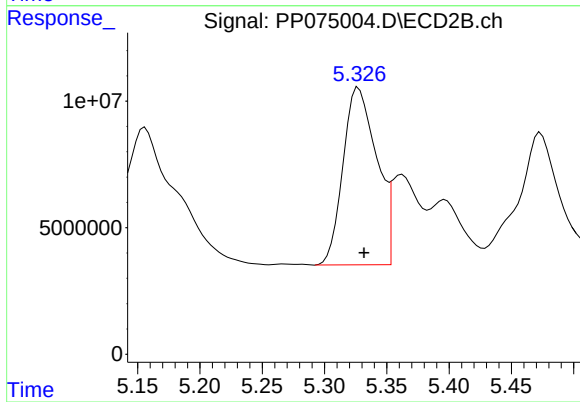


#15 AR-1232-5

R.T.: 5.327 min
Delta R.T.: -0.005 min
Response: 131930478
Conc: 2125.04 ng/ml

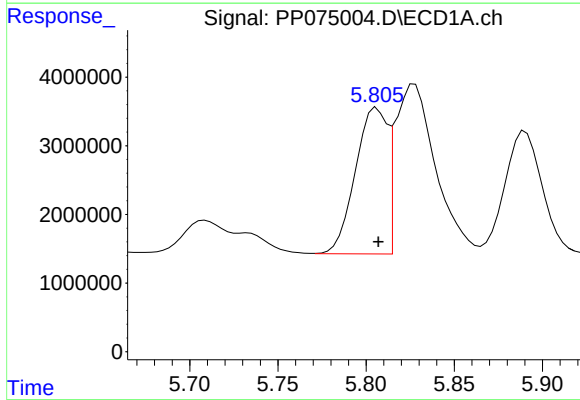


#16 AR-1242-1

R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 26665718
Conc: 696.68 ng/ml

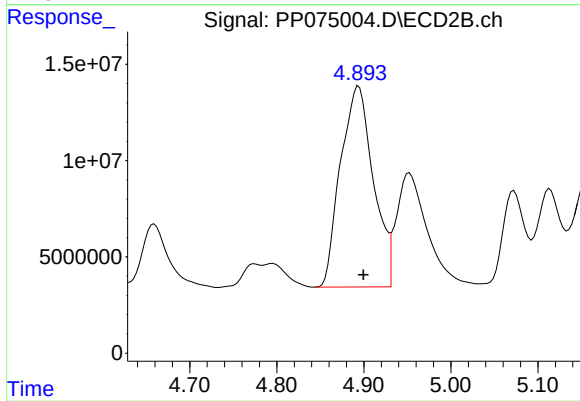

#16 AR-1242-1


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 272811386
Conc: 646.85 ng/ml

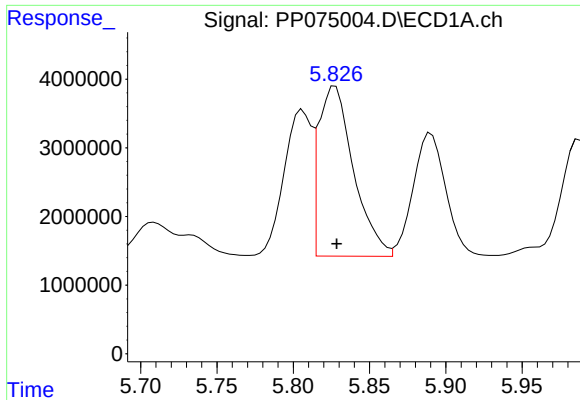

#17 AR-1242-2


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 39531291
Conc: 699.89 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

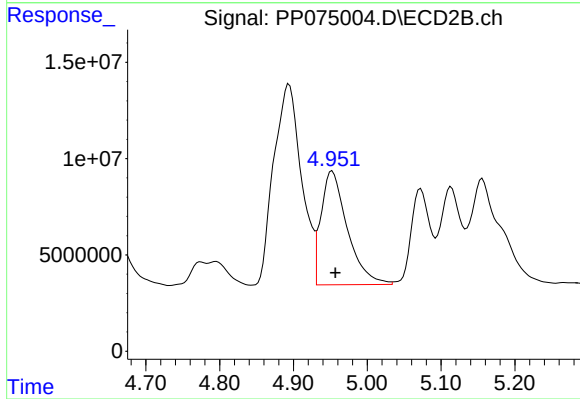


#17 AR-1242-2

R.T.: 4.952 min
Delta R.T.: -0.004 min
Response: 146257450
Conc: 730.26 ng/ml

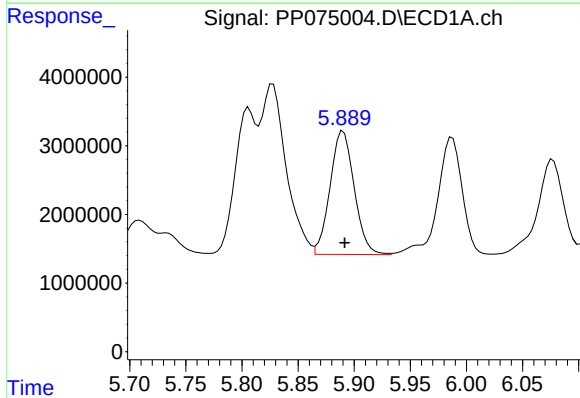


#18 AR-1242-3

R.T.: 5.890 min
Delta R.T.: -0.001 min
Response: 26956477
Conc: 663.91 ng/ml

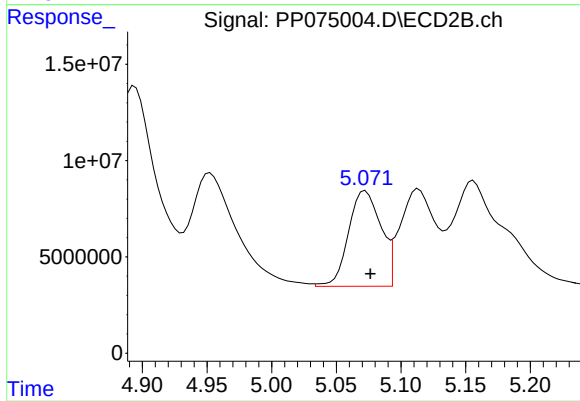

#18 AR-1242-3


R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 86253503
Conc: 729.12 ng/ml

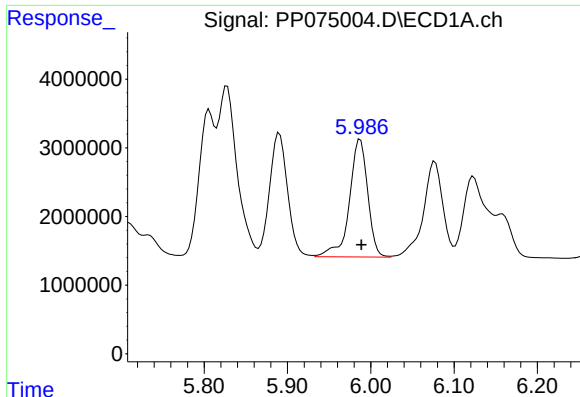

#19 AR-1242-4


R.T.: 5.987 min
Delta R.T.: -0.001 min
Response: 26176446
Conc: 824.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

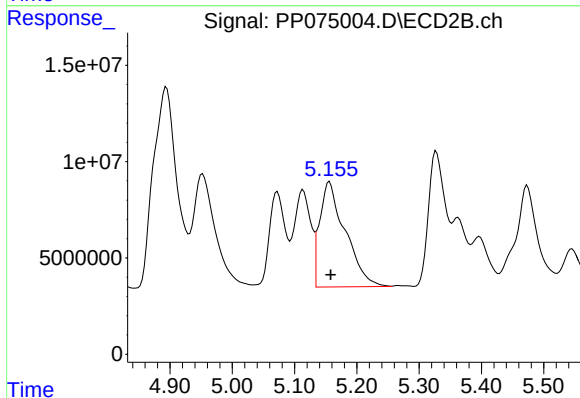


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 155419815
Conc: 908.04 ng/ml

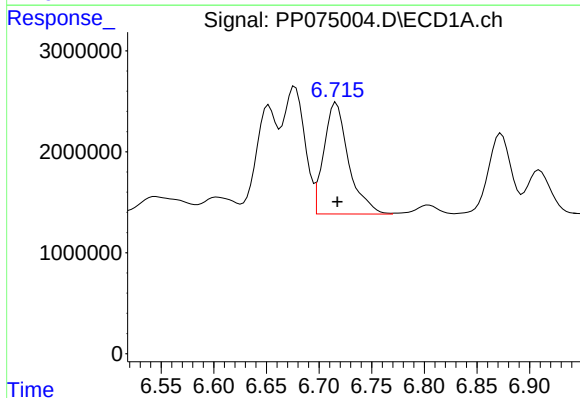


#20 AR-1242-5

R.T.: 6.716 min
Delta R.T.: -0.001 min
Response: 18048277
Conc: 500.36 ng/ml

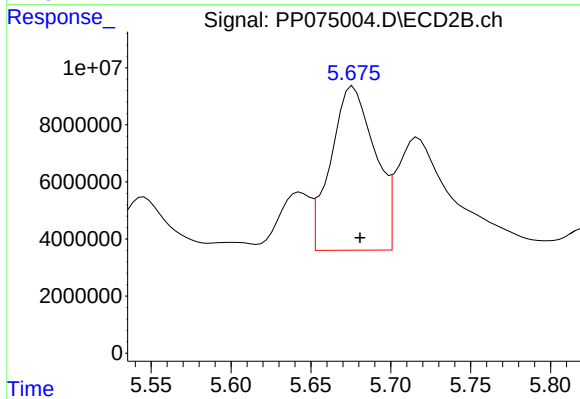

#20 AR-1242-5


R.T.: 5.677 min
Delta R.T.: -0.004 min
Response: 110050729
Conc: 594.34 ng/ml

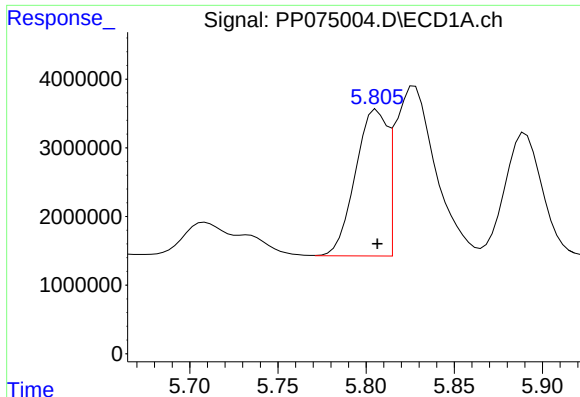

#21 AR-1248-1


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 26665718
Conc: 882.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

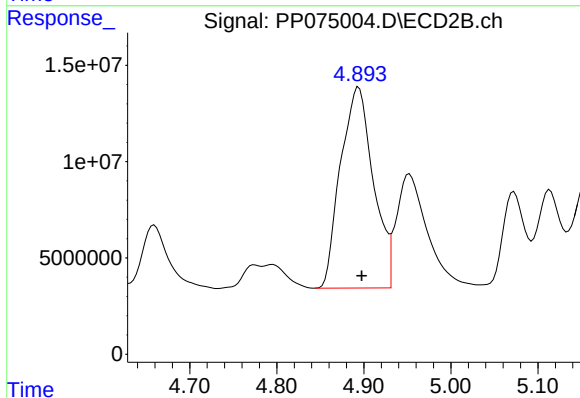


#21 AR-1248-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 272811386
Conc: 987.94 ng/ml

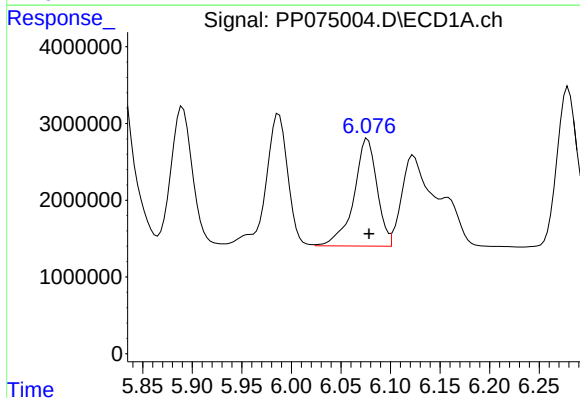


#22 AR-1248-2

R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 22804631
Conc: 529.16 ng/ml

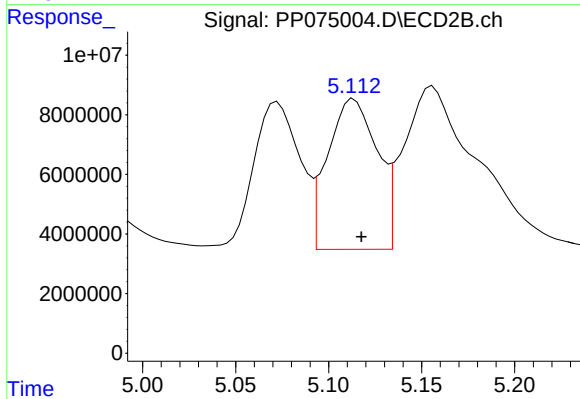

#22 AR-1248-2


R.T.: 5.114 min
Delta R.T.: -0.004 min
Response: 93492287
Conc: 528.94 ng/ml

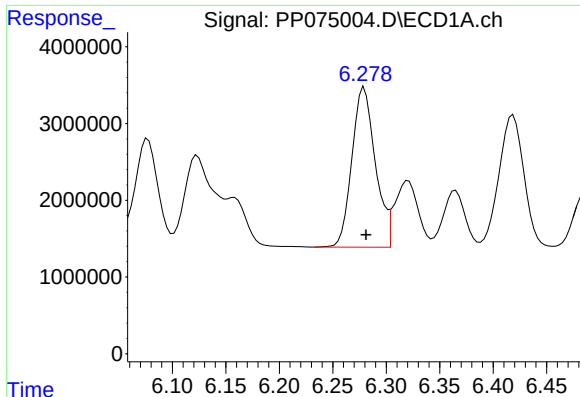

#23 AR-1248-3


R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 31754552
Conc: 679.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

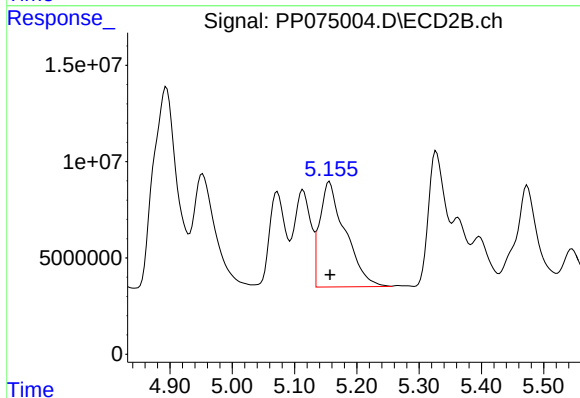


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: -0.001 min
Response: 155419815
Conc: 684.06 ng/ml

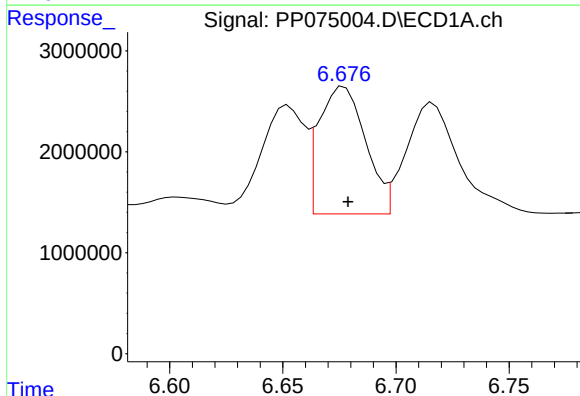


#24 AR-1248-4

R.T.: 6.677 min
Delta R.T.: -0.002 min
Response: 18143074
Conc: 329.87 ng/ml

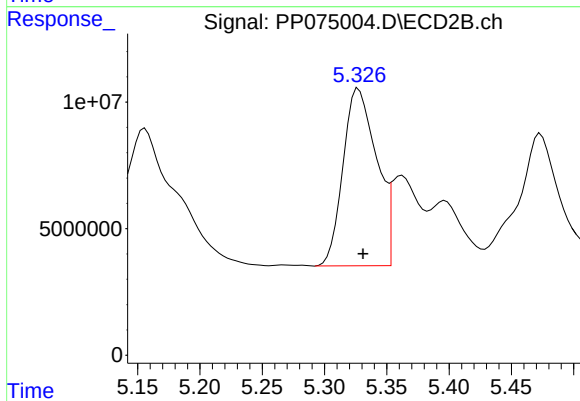

#24 AR-1248-4


R.T.: 5.327 min
Delta R.T.: -0.004 min
Response: 131930478
Conc: 605.13 ng/ml

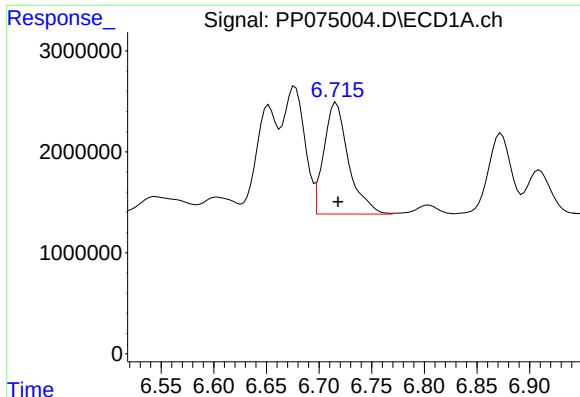

#25 AR-1248-5


R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 18048277
Conc: 325.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

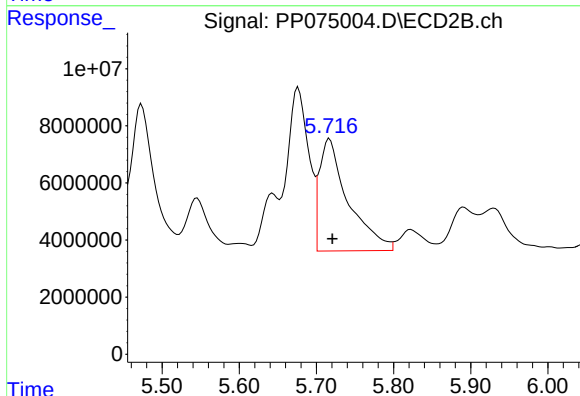


#25 AR-1248-5

R.T.: 5.717 min
Delta R.T.: -0.004 min
Response: 102054183
Conc: 277.83 ng/ml

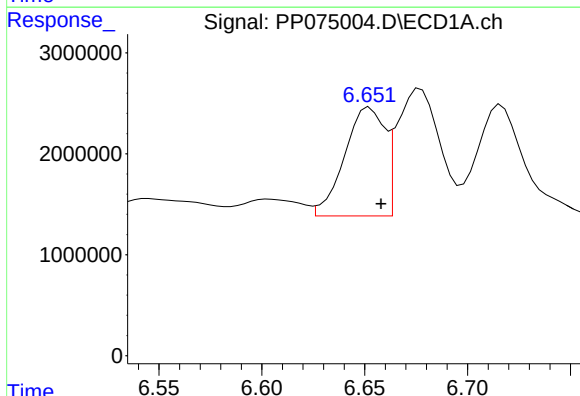


#26 AR-1254-1

R.T.: 6.652 min
Delta R.T.: -0.006 min
Response: 14560283
Conc: 249.88 ng/ml

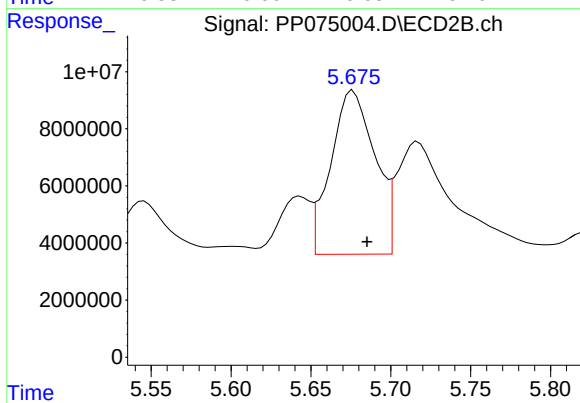

#26 AR-1254-1


R.T.: 5.677 min
Delta R.T.: -0.009 min
Response: 110050729
Conc: 230.85 ng/ml

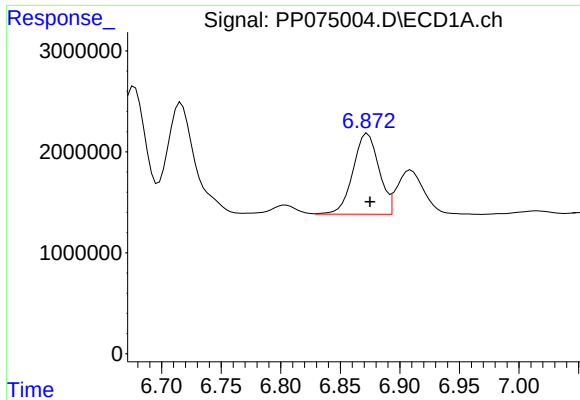

#27 AR-1254-2


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 12114687
Conc: 148.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

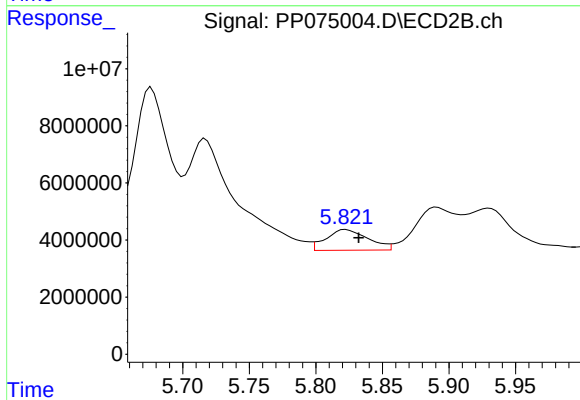


#27 AR-1254-2

R.T.: 5.822 min
Delta R.T.: -0.010 min
Response: 15860016
Conc: 45.04 ng/ml

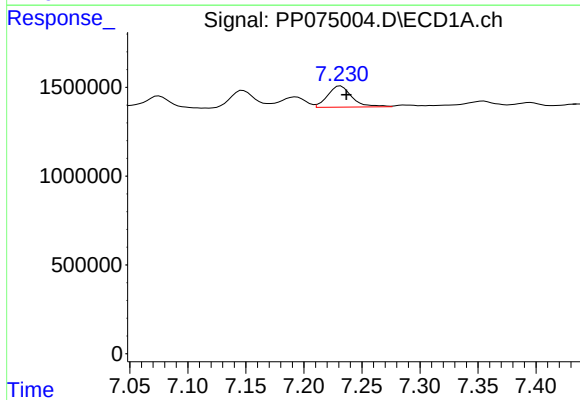


#28 AR-1254-3

R.T.: 7.232 min
Delta R.T.: -0.005 min
Response: 1738102
Conc: 19.48 ng/ml

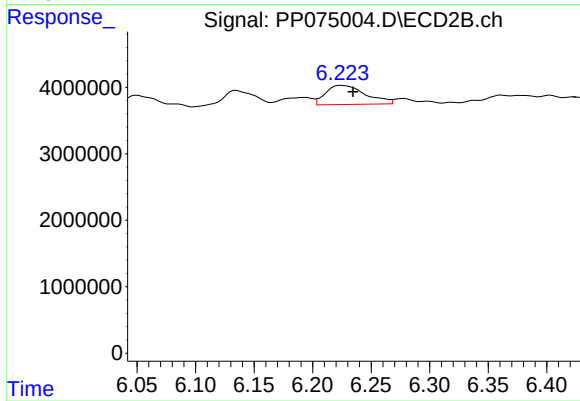

#28 AR-1254-3


R.T.: 6.225 min
Delta R.T.: -0.010 min
Response: 6868152
Conc: 11.08 ng/ml

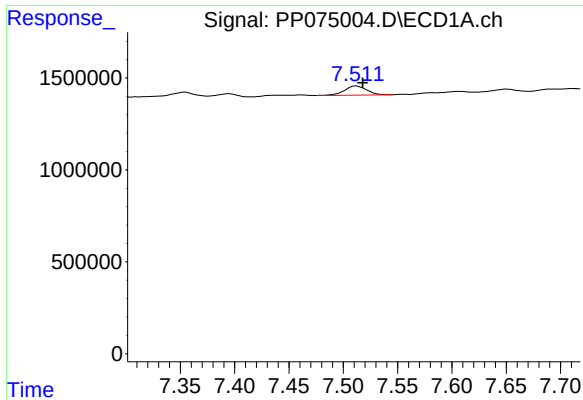

#29 AR-1254-4


R.T.: 7.512 min
Delta R.T.: -0.006 min
Response: 705454
Conc: 10.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

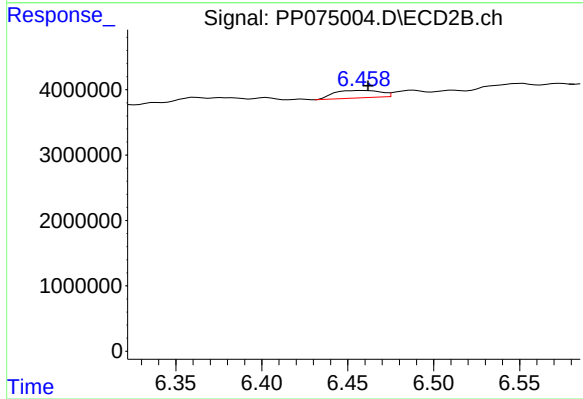


#29 AR-1254-4

R.T.: 6.459 min
Delta R.T.: -0.003 min
Response: 2119804
Conc: 4.52 ng/ml

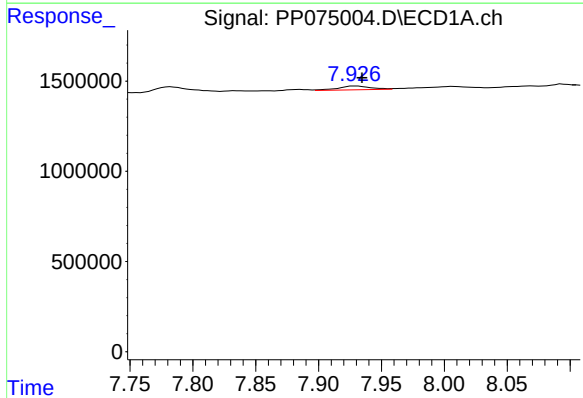


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.006 min
Response: 388891
Conc: 4.68 ng/ml

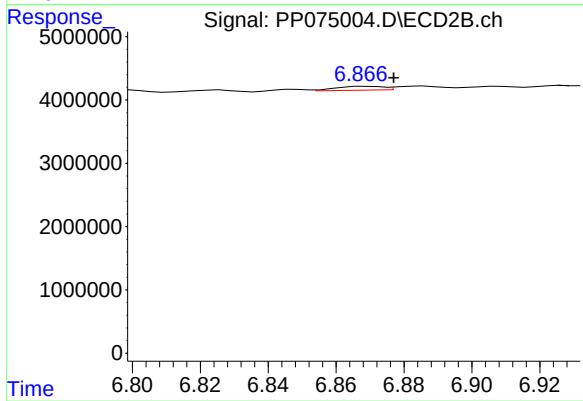

#30 AR-1254-5


R.T.: 6.869 min
Delta R.T.: -0.008 min
Response: 604493
Conc: 1.23 ng/ml

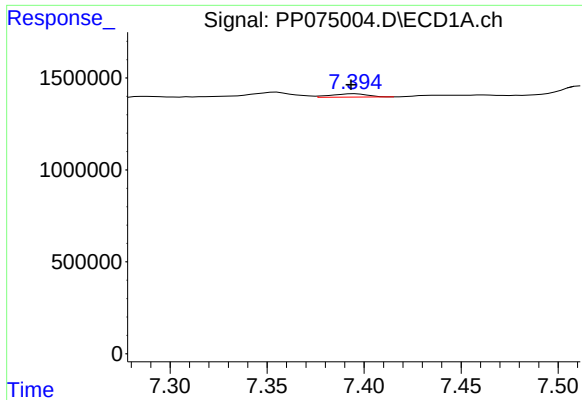

#31 AR-1260-1


R.T.: 7.395 min
Delta R.T.: 0.002 min
Response: 232802
Conc: 4.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

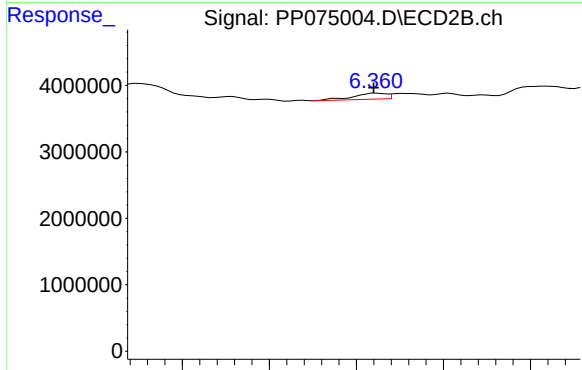


#31 AR-1260-1

R.T.: 6.362 min
Delta R.T.: 0.002 min
Response: 1202680
Conc: 3.21 ng/ml

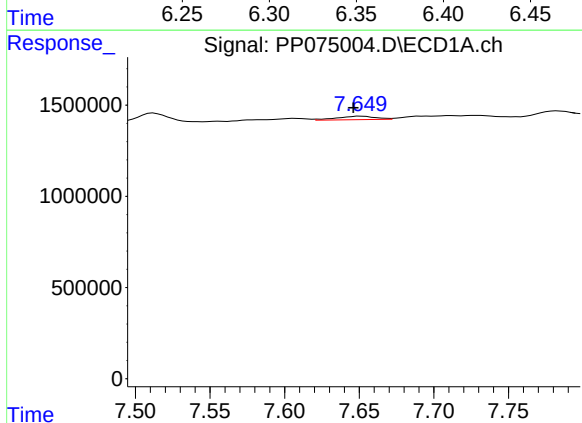


#32 AR-1260-2

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 347133
Conc: 5.04 ng/ml

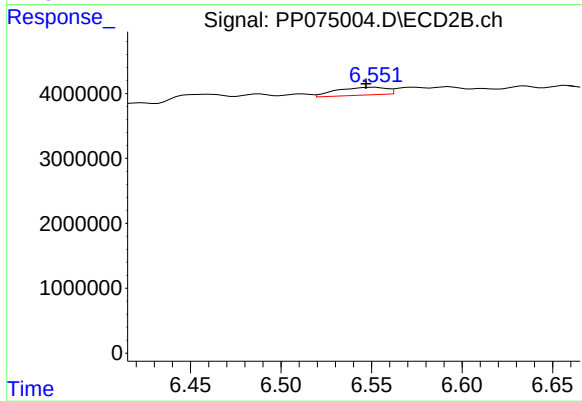

#32 AR-1260-2


R.T.: 6.552 min
Delta R.T.: 0.005 min
Response: 2310707
Conc: 4.37 ng/ml

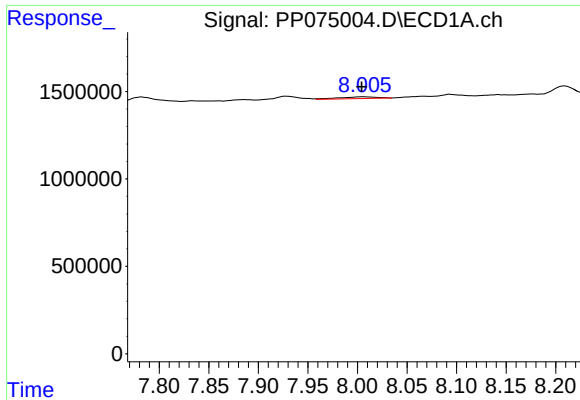

#33 AR-1260-3


R.T.: 8.006 min
Delta R.T.: 0.002 min
Response: 256013
Conc: 4.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

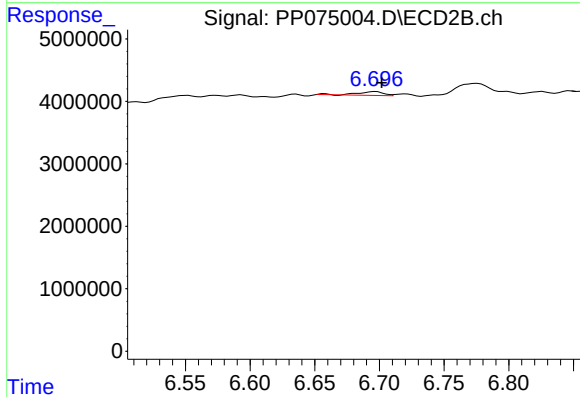


#33 AR-1260-3

R.T.: 6.697 min
Delta R.T.: -0.005 min
Response: 794962
Conc: 1.84 ng/ml

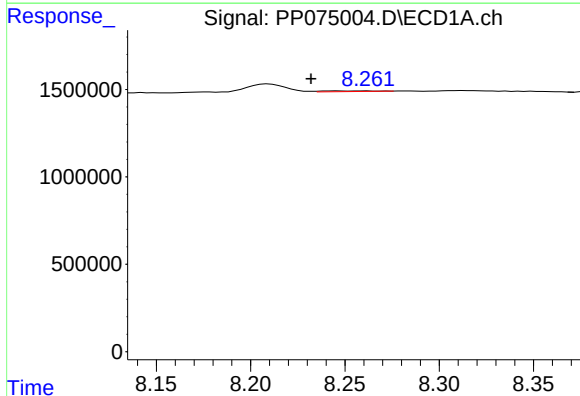


#34 AR-1260-4

R.T.: 8.246 min
Delta R.T.: 0.014 min
Response: 61594
Conc: 0.97 ng/ml

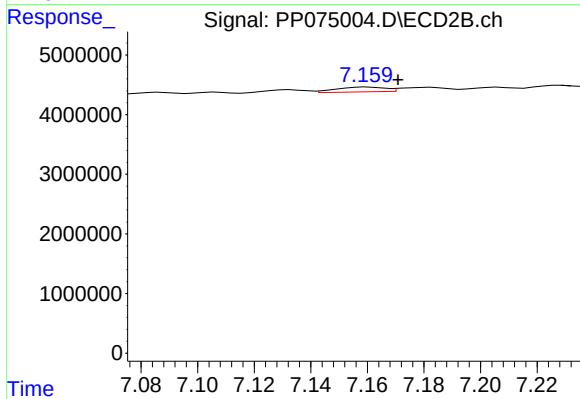

#34 AR-1260-4


R.T.: 7.160 min
Delta R.T.: -0.011 min
Response: 965538
Conc: 2.53 ng/ml

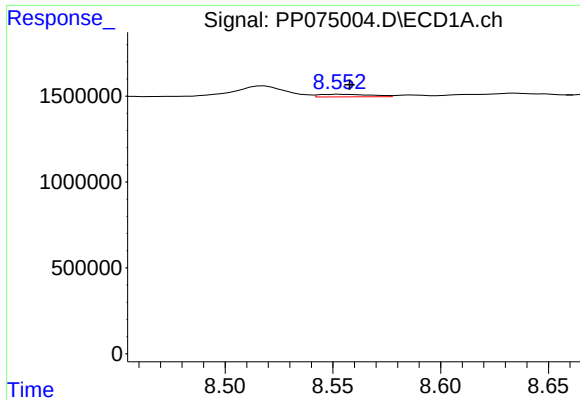

#35 AR-1260-5


R.T.: 8.554 min
Delta R.T.: -0.004 min
Response: 248980
Conc: 2.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

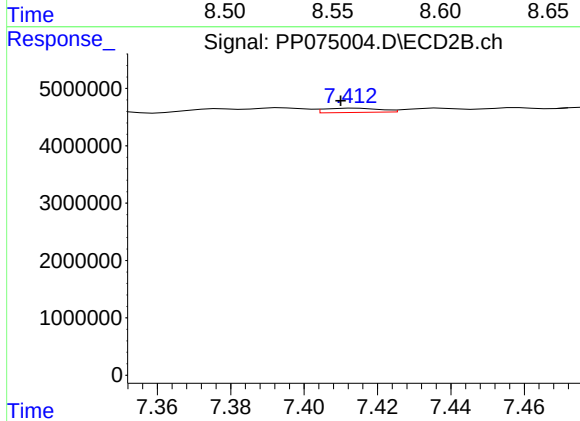


#35 AR-1260-5

R.T.: 7.414 min
Delta R.T.: 0.004 min
Response: 796975
Conc: 0.79 ng/ml

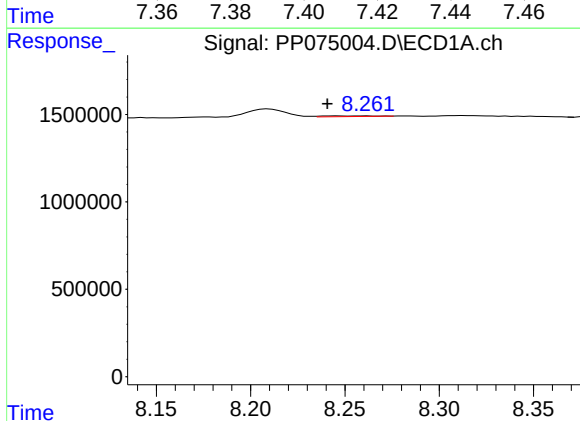


#36 AR-1262-1

R.T.: 8.246 min
Delta R.T.: 0.005 min
Response: 61594
Conc: 0.80 ng/ml

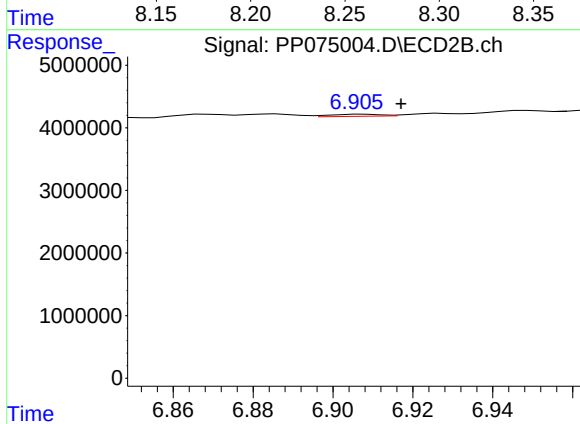

#36 AR-1262-1


R.T.: 6.908 min
Delta R.T.: -0.009 min
Response: 275243
Conc: 0.39 ng/ml

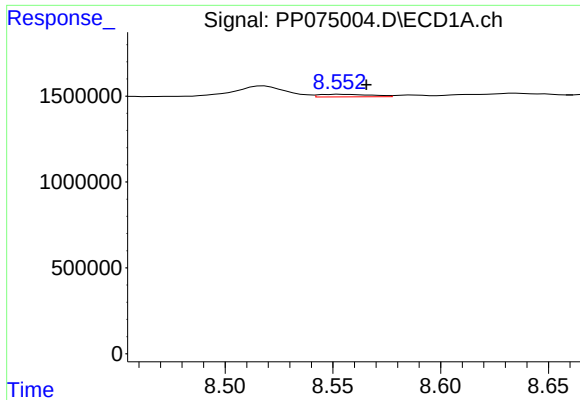

#37 AR-1262-2


R.T.: 8.554 min
Delta R.T.: -0.012 min
Response: 248980
Conc: 1.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

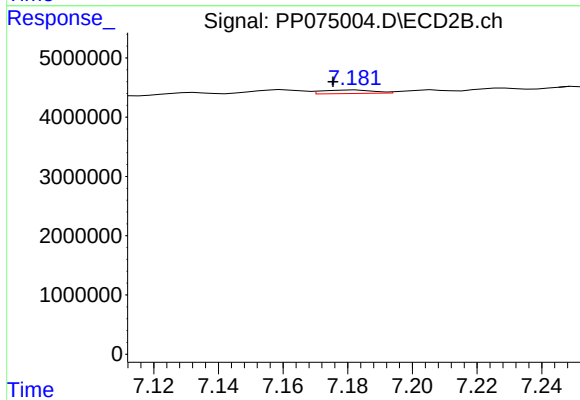


#37 AR-1262-2

R.T.: 7.182 min
Delta R.T.: 0.007 min
Response: 657752
Conc: 1.26 ng/ml

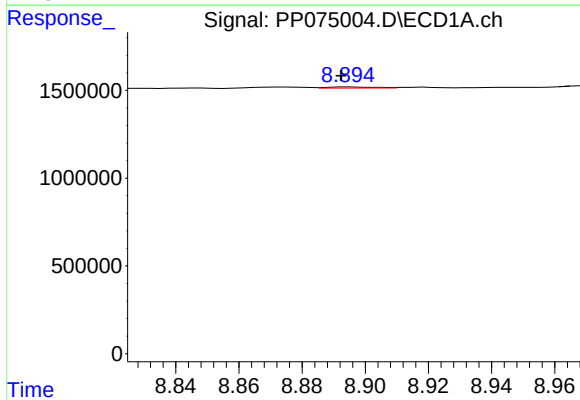


#38 AR-1262-3

R.T.: 8.895 min
Delta R.T.: 0.003 min
Response: 71132
Conc: 0.73 ng/ml

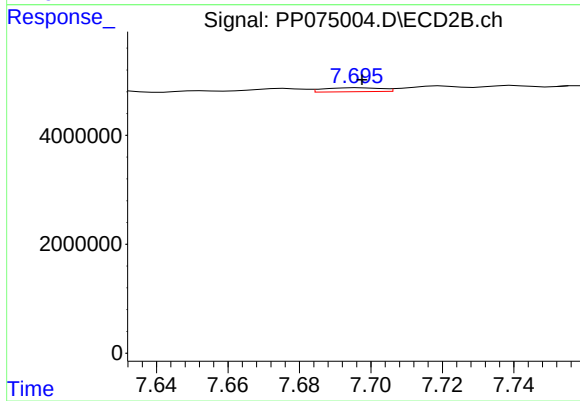

#38 AR-1262-3


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 815285
Conc: 1.75 ng/ml

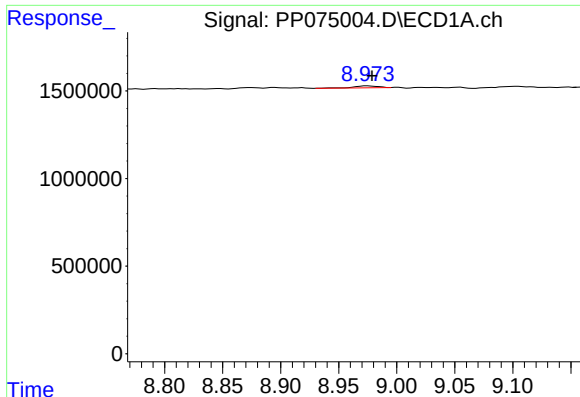

#39 AR-1262-4


R.T.: 8.974 min
Delta R.T.: -0.004 min
Response: 162459
Conc: 2.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

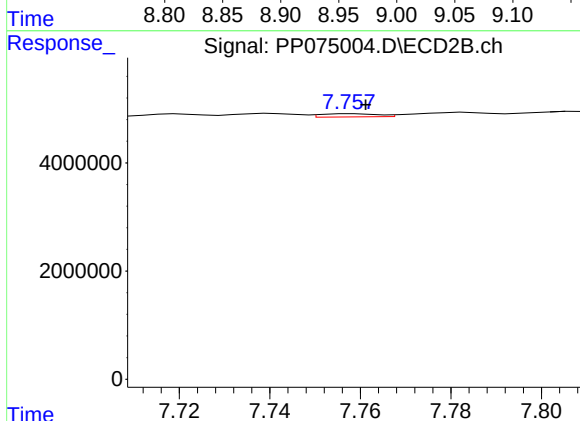


#39 AR-1262-4

R.T.: 7.758 min
Delta R.T.: -0.003 min
Response: 517086
Conc: 0.63 ng/ml

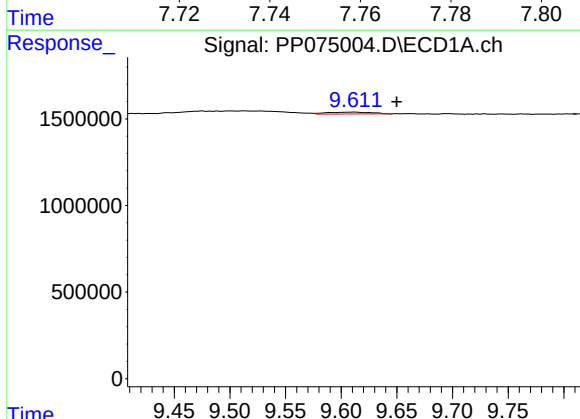


#40 AR-1262-5

R.T.: 9.611 min
Delta R.T.: -0.039 min
Response: 303316
Conc: 4.98 ng/ml

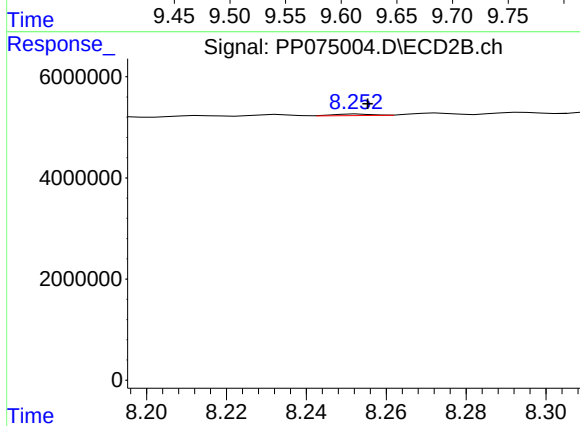

#40 AR-1262-5


R.T.: 8.253 min
Delta R.T.: -0.002 min
Response: 192039
Conc: 0.54 ng/ml

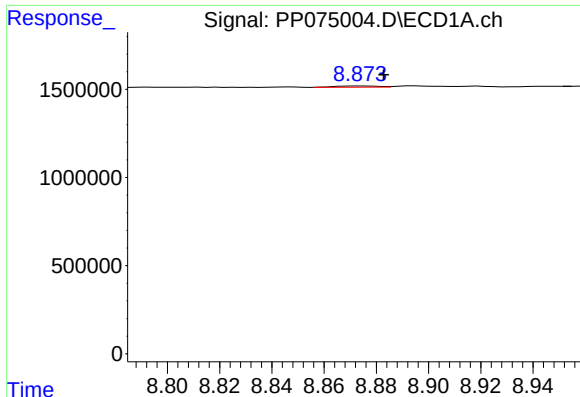

#41 AR-1268-1


R.T.: 8.874 min
Delta R.T.: -0.009 min
Response: 78497
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

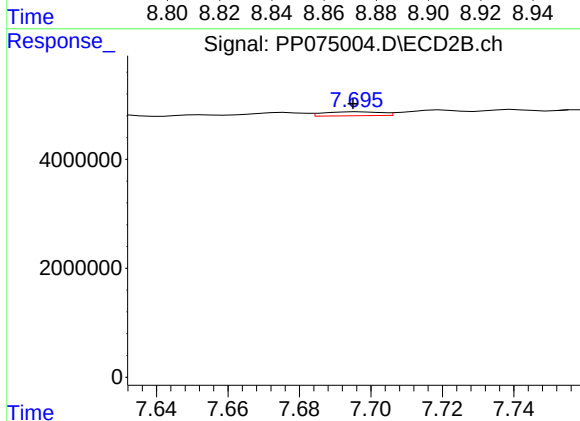


#41 AR-1268-1

R.T.: 7.697 min
Delta R.T.: 0.002 min
Response: 815285
Conc: 0.58 ng/ml

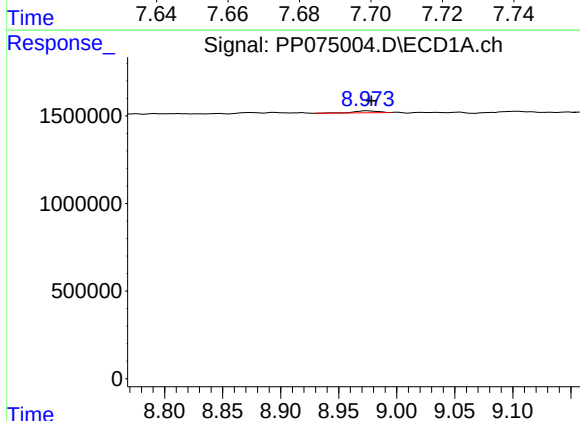


#42 AR-1268-2

R.T.: 8.974 min
Delta R.T.: -0.004 min
Response: 162459
Conc: 1.11 ng/ml

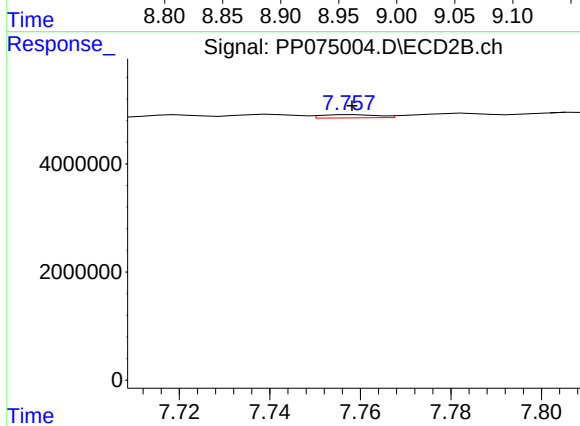

#42 AR-1268-2


R.T.: 7.758 min
Delta R.T.: 0.000 min
Response: 517086
Conc: 0.38 ng/ml

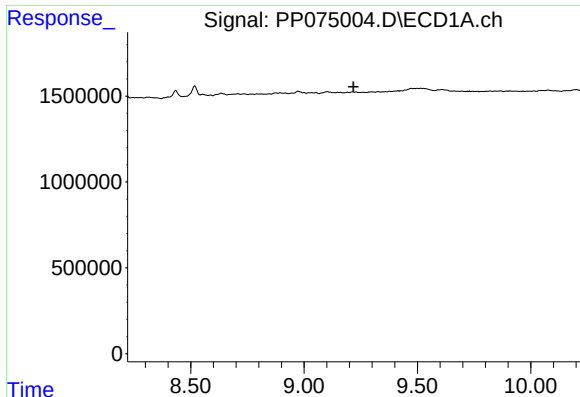

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

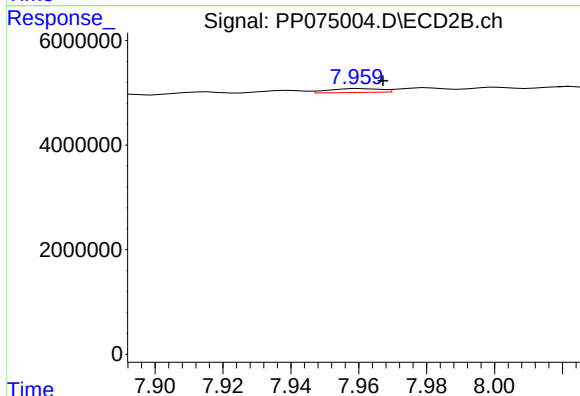


#43 AR-1268-3

R.T.: 7.960 min
Delta R.T.: -0.007 min
Response: 768367
Conc: 0.74 ng/ml

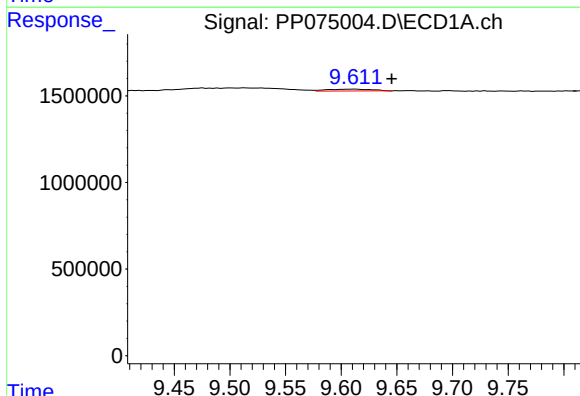


#44 AR-1268-4

R.T.: 9.611 min
Delta R.T.: -0.034 min
Response: 303316
Conc: 4.51 ng/ml

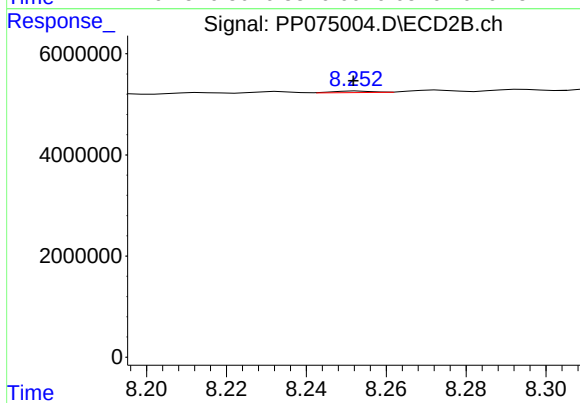

#44 AR-1268-4


R.T.: 8.253 min
Delta R.T.: 0.001 min
Response: 192039
Conc: 0.50 ng/ml

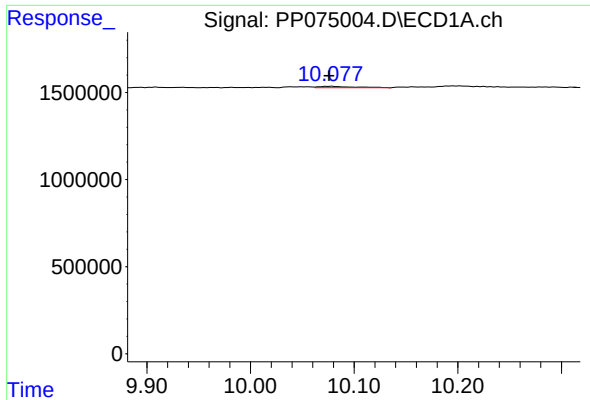

#45 AR-1268-5

R.T.: 10.078 min
Delta R.T.: 0.002 min
Response: 178366
Conc: 0.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-C

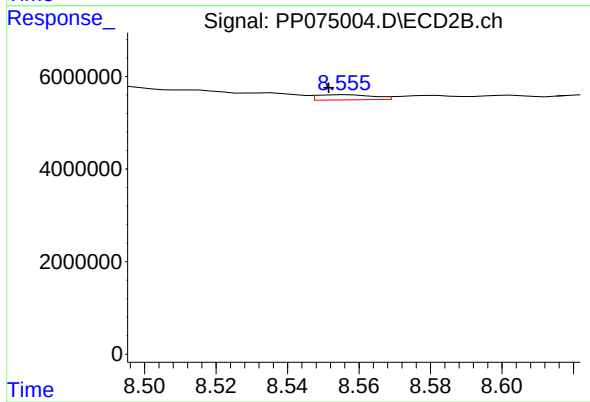

#45 AR-1268-5

R.T.: 8.556 min
Delta R.T.: 0.005 min
Response: 1207061
Conc: 0.38 ng/ml