

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 14:25
 Operator : YP\AJ
 Sample : Q3034-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:49:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.655	3.797	28528314	110.6E6	23.313	22.881
2)	SA Decachlor...	10.431	8.805	23195316	140.1E6	23.489	18.685
Target Compounds							
3)	L1 AR-1016-1	5.806	4.894	2934611	25368919	66.561	49.806 #
4)	L1 AR-1016-2	5.827	4.952	4369525	13621956	69.532	57.231
5)	L1 AR-1016-3	5.890	5.072	3254236	9107679	72.455	66.044
6)	L1 AR-1016-4	5.988	5.114	2876855	10011257	81.771	71.610
7)	L1 AR-1016-5	6.280	5.328	3658794	18213663	110.251	109.666
8)	L2 AR-1221-1	4.854	4.018	605057	144232	34.392	2.331 #
9)	L2 AR-1221-2	4.956	4.101	604715	2106778	45.273	46.598
10)	L2 AR-1221-3	5.016	4.179	276426	366584	7.291	2.231 #
11)	L3 AR-1232-1	5.016	4.165	276426	565357	9.101	4.414 #
12)	L3 AR-1232-2	5.541	4.894	1463796	25368919	92.891	109.446
13)	L3 AR-1232-3	5.827	5.072	4369525	9107679	143.058	151.644
14)	L3 AR-1232-4	5.988	5.156	2876855	16647506	166.588	225.859 #
15)	L3 AR-1232-5	6.077	5.328	2816418	18213663	216.965	293.372 #
16)	L4 AR-1242-1	5.806	4.894	2934611	25368919	76.671	60.151
17)	L4 AR-1242-2	5.827	4.952	4369525	13621956	77.361	68.014
18)	L4 AR-1242-3	5.890	5.072	3254236	9107679	80.148	76.989
19)	L4 AR-1242-4	5.988	5.156	2876855	16647506	90.633	97.263
20)	L4 AR-1242-5	6.717	5.675	2314121	10481678	64.155	56.607
21)	L5 AR-1248-1	5.806	4.894	2934611	25368919	97.095	91.869
22)	L5 AR-1248-2	6.077	5.114	2816418	10011257	65.352	56.639
23)	L5 AR-1248-3	6.280	5.156	3658794	16647506	78.341	73.271
24)	L5 AR-1248-4	6.678	5.328	2097396	18213663	38.134	83.541 #
25)	L5 AR-1248-5	6.717	5.720	2314121	5842597	41.718	15.906 #
26)	L6 AR-1254-1	6.653	5.675	1901082	10481678	32.626	21.988 #
27)	L6 AR-1254-2	6.872	5.823	1454681	2690211	17.823	7.640 #
28)	L6 AR-1254-3	7.225	6.229	837846	549482	9.392	0.887 #
29)	L6 AR-1254-4	7.517	6.455	107740	206725	1.635	0.441 #
30)	L6 AR-1254-5	7.884f	6.867	197634	179370	2.379	0.366 #
31)	L7 AR-1260-1	7.389	6.351	56379	168034	0.975	0.448 #
32)	L7 AR-1260-2	7.652	6.543	144801	659404	2.101	1.247 #
33)	L7 AR-1260-3	0.000	6.700	0	338783	N.D.	0.782 #
34)	L7 AR-1260-4	8.249	7.164	314507	231399	4.930	0.607 #
35)	L7 AR-1260-5	8.578	7.411	134684	196226	1.188	0.195 #
36)	L8 AR-1262-1	8.249	6.909	314507	183637	4.084	0.260 #
37)	L8 AR-1262-2	8.578	7.164	134684	231399	1.017	0.444 #
38)	L8 AR-1262-3	0.000	7.702	0	459707	N.D.	0.986 #
39)	L8 AR-1262-4	8.975	7.760	262439	551292	3.484	0.671 #
40)	L8 AR-1262-5	9.610f	8.261	442767	301244	7.264	0.841 #
41)	L9 AR-1268-1	0.000	7.702	0	459707	N.D.	0.326 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 14:25
 Operator : YP\AJ
 Sample : Q3034-04
 Misc :
 ALS Vial : 13 Sample Multiplier: 1


Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-D

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:49:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.975	7.760	262439	551292	1.788	0.404 #
43) L9	AR-1268-3	0.000	7.964	0	578737	N.D.	0.555 #
44) L9	AR-1268-4	9.610f	8.261	442767	301244	6.583	0.786 #
45) L9	AR-1268-5	10.079	8.570	44867	1044106	0.121	0.333 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

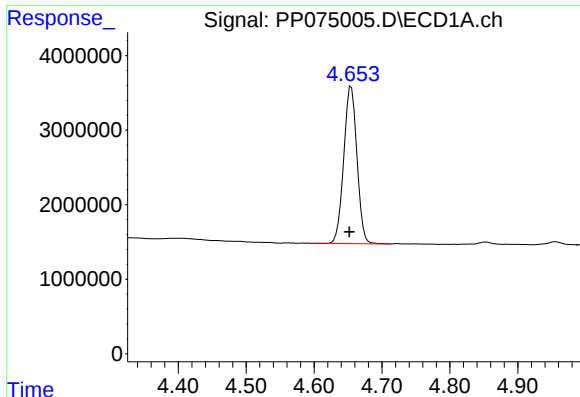

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: 0.003 min
Response: 28528314
Conc: 23.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

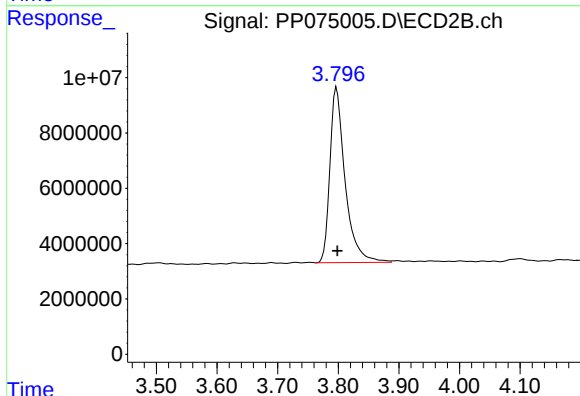


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: -0.001 min
Response: 110638408
Conc: 22.88 ng/ml

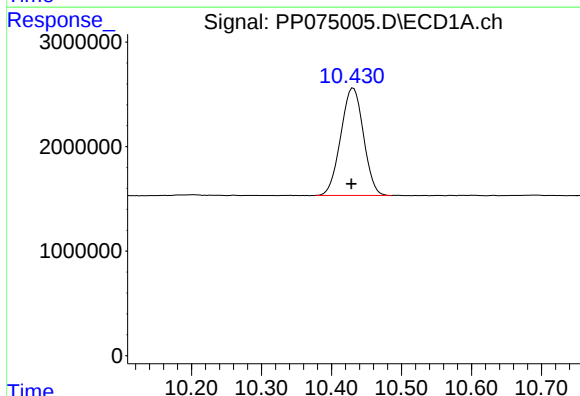


#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.003 min
Response: 23195316
Conc: 23.49 ng/ml

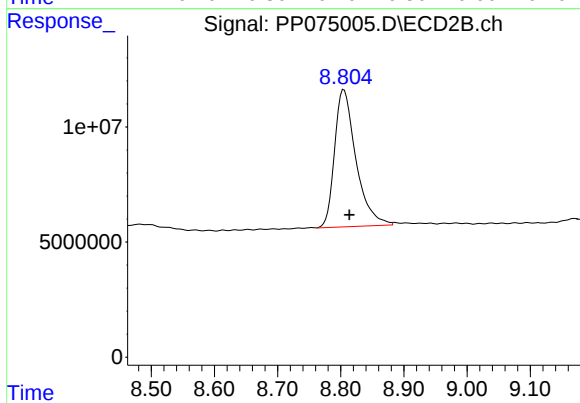

#2 Decachlorobiphenyl


R.T.: 8.805 min
Delta R.T.: -0.009 min
Response: 140123881
Conc: 18.69 ng/ml

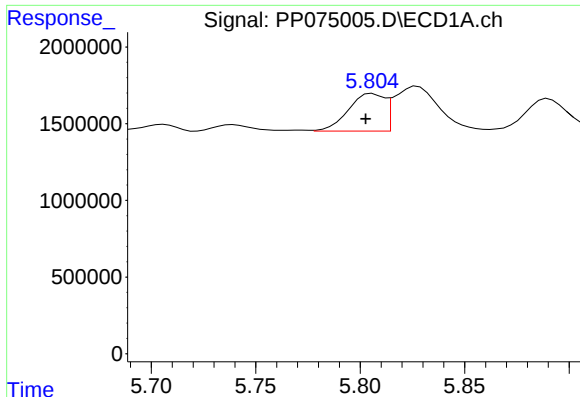

#3 AR-1016-1


R.T.: 5.806 min
Delta R.T.: 0.003 min
Response: 2934611
Conc: 66.56 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

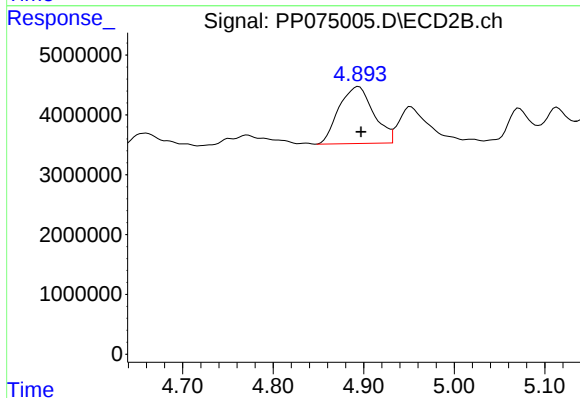


#3 AR-1016-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 25368919
Conc: 49.81 ng/ml

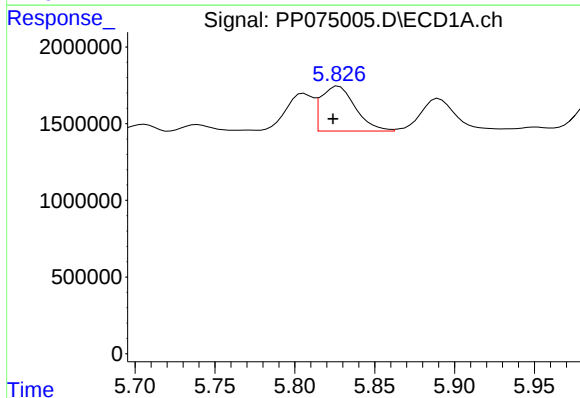


#4 AR-1016-2

R.T.: 5.827 min
Delta R.T.: 0.003 min
Response: 4369525
Conc: 69.53 ng/ml

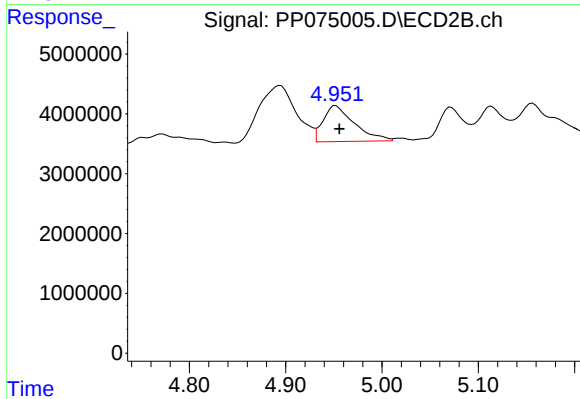

#4 AR-1016-2


R.T.: 4.952 min
Delta R.T.: -0.004 min
Response: 13621956
Conc: 57.23 ng/ml

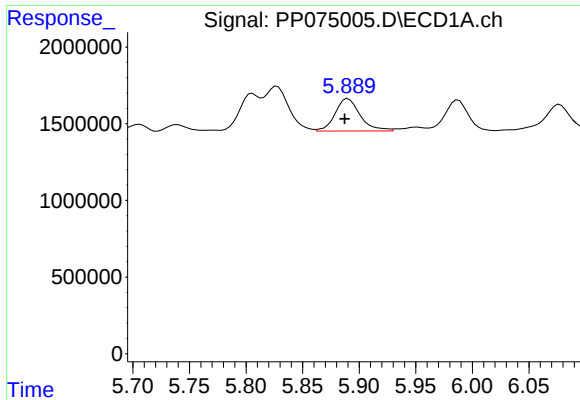

#5 AR-1016-3


R.T.: 5.890 min
Delta R.T.: 0.003 min
Response: 3254236
Conc: 72.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

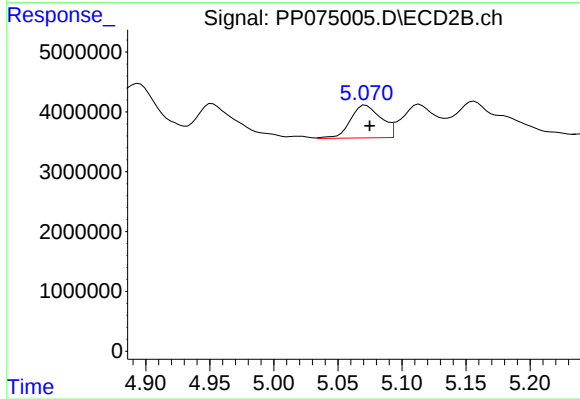


#5 AR-1016-3

R.T.: 5.072 min
Delta R.T.: -0.003 min
Response: 9107679
Conc: 66.04 ng/ml

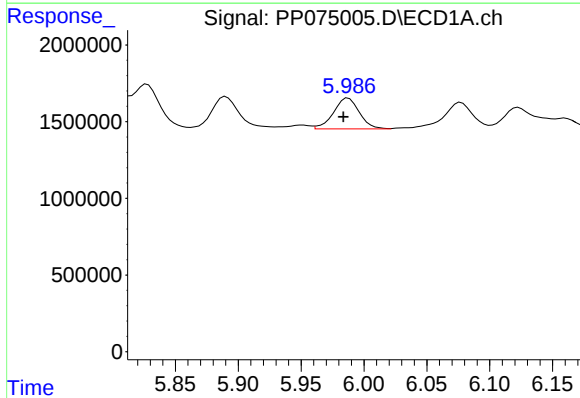


#6 AR-1016-4

R.T.: 5.988 min
Delta R.T.: 0.004 min
Response: 2876855
Conc: 81.77 ng/ml

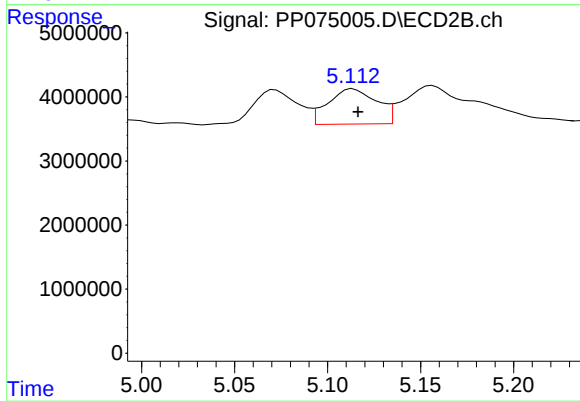

#6 AR-1016-4


R.T.: 5.114 min
Delta R.T.: -0.003 min
Response: 10011257
Conc: 71.61 ng/ml

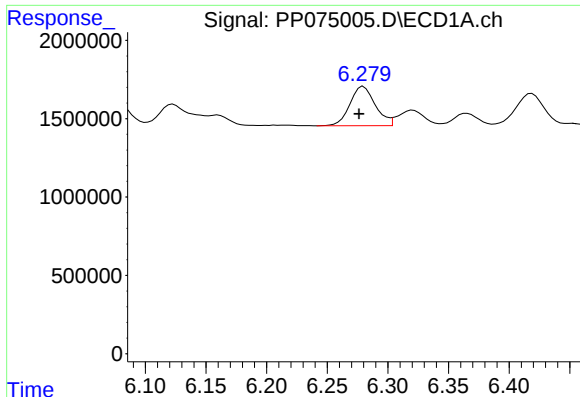

#7 AR-1016-5


R.T.: 6.280 min
Delta R.T.: 0.004 min
Response: 3658794
Conc: 110.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

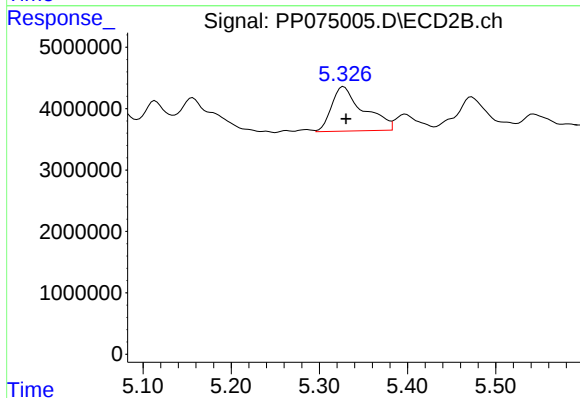


#7 AR-1016-5

R.T.: 5.328 min
Delta R.T.: -0.003 min
Response: 18213663
Conc: 109.67 ng/ml

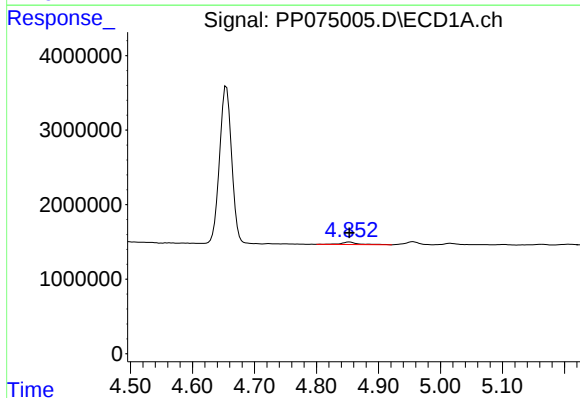


#8 AR-1221-1

R.T.: 4.854 min
Delta R.T.: 0.000 min
Response: 605057
Conc: 34.39 ng/ml

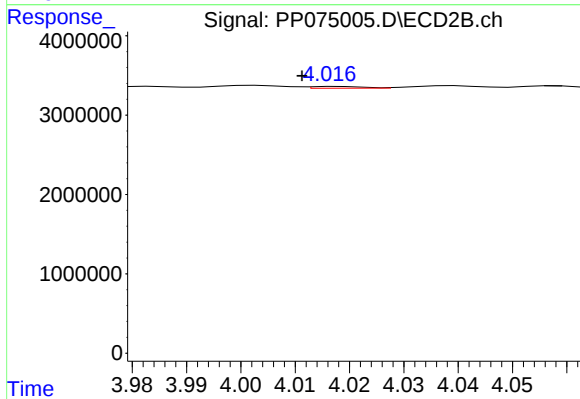

#8 AR-1221-1


R.T.: 4.018 min
Delta R.T.: 0.007 min
Response: 144232
Conc: 2.33 ng/ml

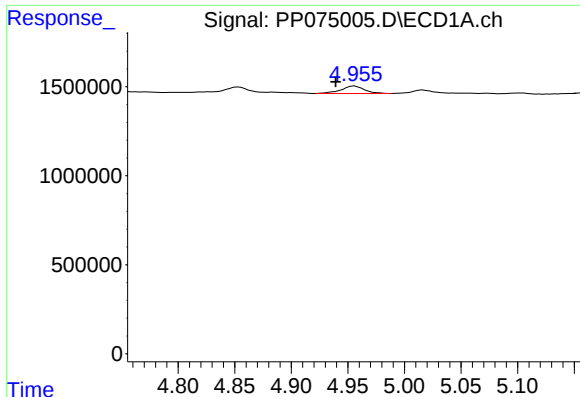

#9 AR-1221-2


R.T.: 4.956 min
Delta R.T.: 0.017 min
Response: 604715
Conc: 45.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

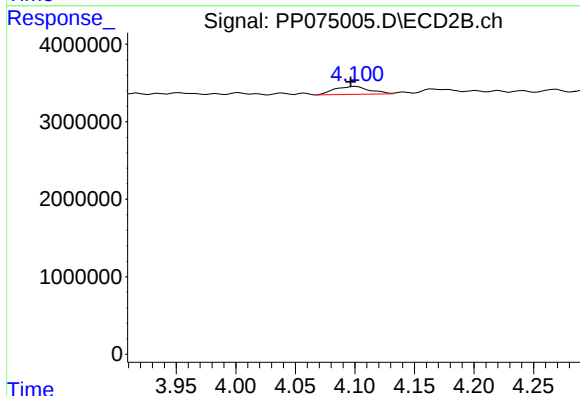


#9 AR-1221-2

R.T.: 4.101 min
Delta R.T.: 0.004 min
Response: 2106778
Conc: 46.60 ng/ml

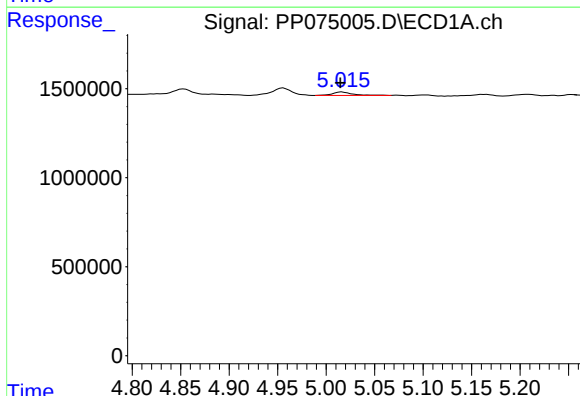


#10 AR-1221-3

R.T.: 5.016 min
Delta R.T.: 0.002 min
Response: 276426
Conc: 7.29 ng/ml

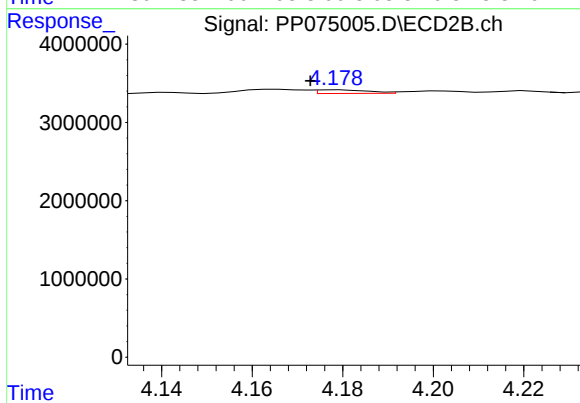

#10 AR-1221-3


R.T.: 4.179 min
Delta R.T.: 0.006 min
Response: 366584
Conc: 2.23 ng/ml

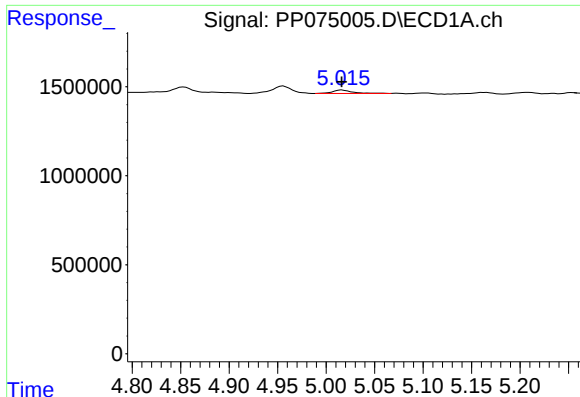

#11 AR-1232-1


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 276426
Conc: 9.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

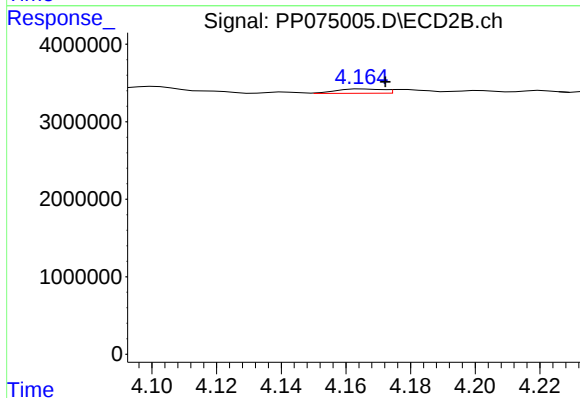


#11 AR-1232-1

R.T.: 4.165 min
Delta R.T.: -0.007 min
Response: 565357
Conc: 4.41 ng/ml

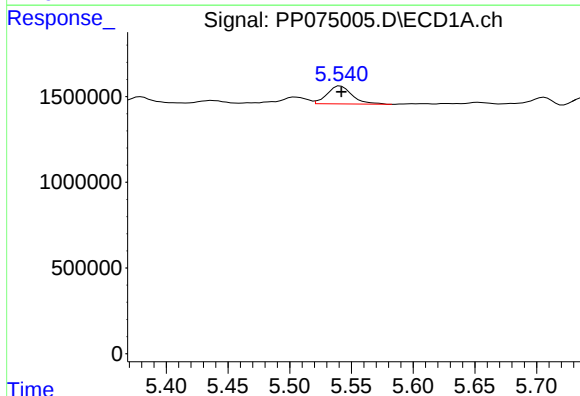


#12 AR-1232-2

R.T.: 5.541 min
Delta R.T.: 0.000 min
Response: 1463796
Conc: 92.89 ng/ml

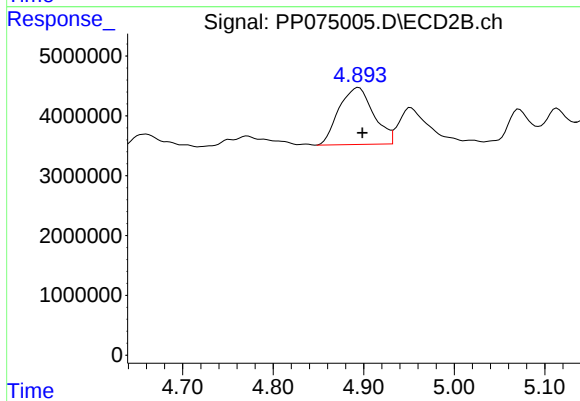

#12 AR-1232-2


R.T.: 4.894 min
Delta R.T.: -0.004 min
Response: 25368919
Conc: 109.45 ng/ml

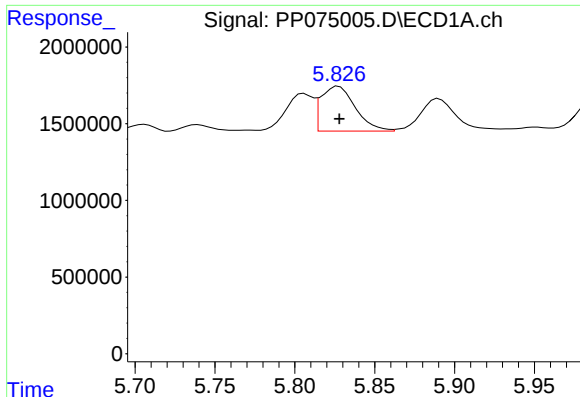

#13 AR-1232-3


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 4369525
Conc: 143.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

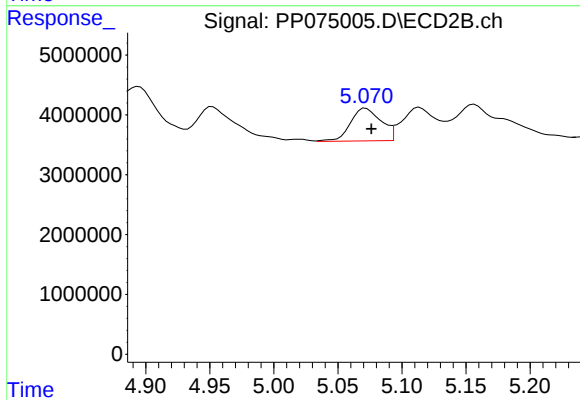


#13 AR-1232-3

R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 9107679
Conc: 151.64 ng/ml

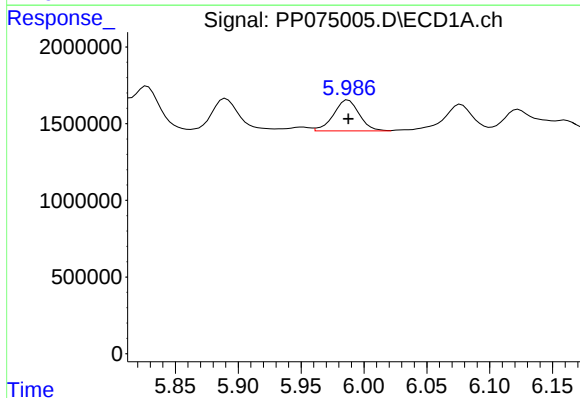


#14 AR-1232-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 2876855
Conc: 166.59 ng/ml

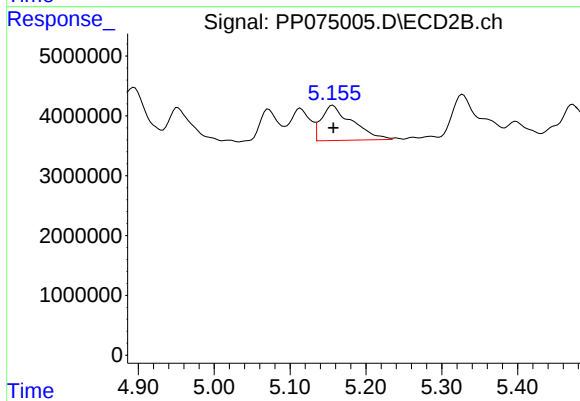

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: 0.000 min
Response: 16647506
Conc: 225.86 ng/ml

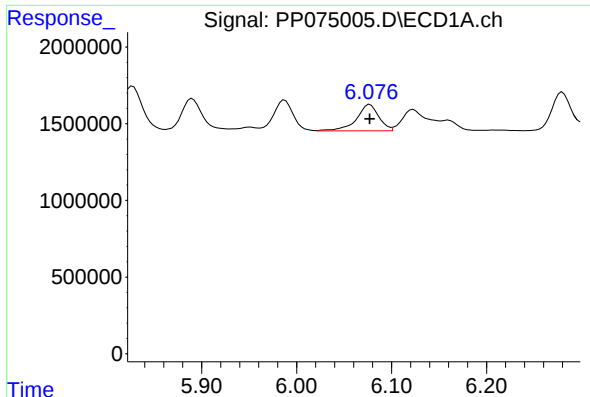

#15 AR-1232-5


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 2816418
Conc: 216.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

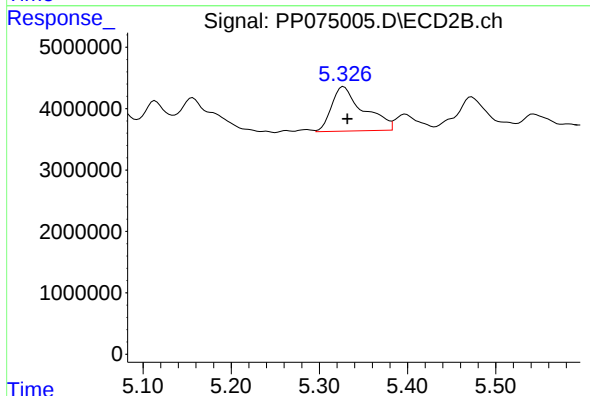


#15 AR-1232-5

R.T.: 5.328 min
Delta R.T.: -0.004 min
Response: 18213663
Conc: 293.37 ng/ml

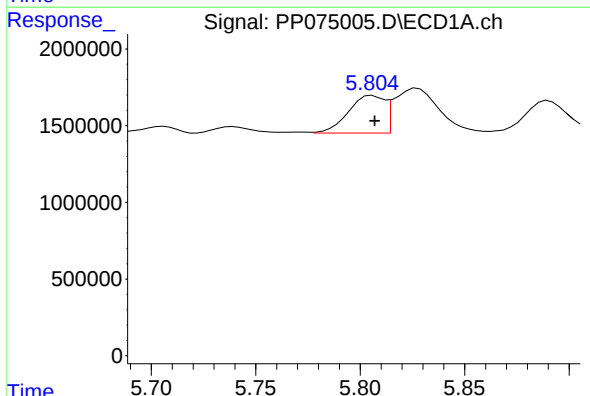


#16 AR-1242-1

R.T.: 5.806 min
Delta R.T.: -0.001 min
Response: 2934611
Conc: 76.67 ng/ml

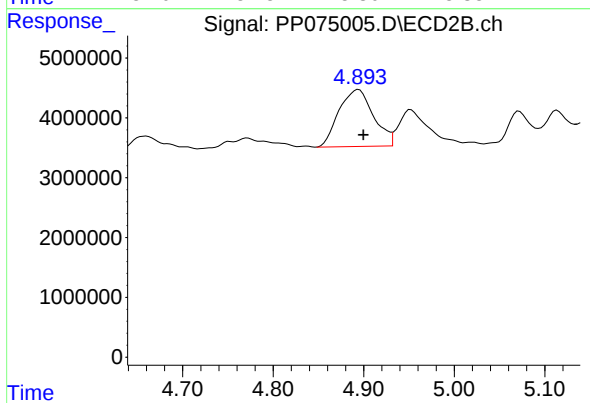

#16 AR-1242-1


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 25368919
Conc: 60.15 ng/ml

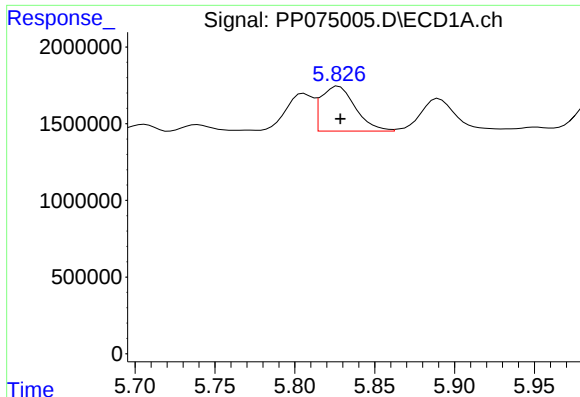

#17 AR-1242-2


R.T.: 5.827 min
Delta R.T.: 0.000 min
Response: 4369525
Conc: 77.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

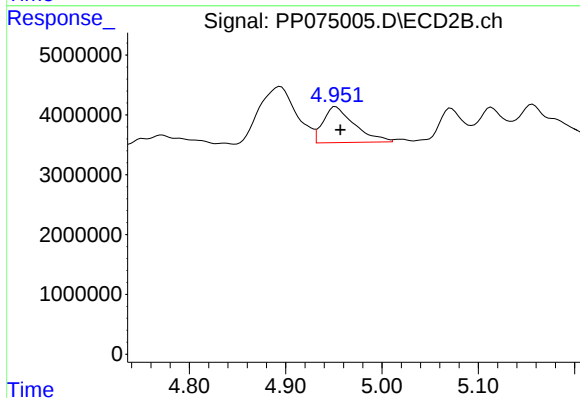


#17 AR-1242-2

R.T.: 4.952 min
Delta R.T.: -0.005 min
Response: 13621956
Conc: 68.01 ng/ml

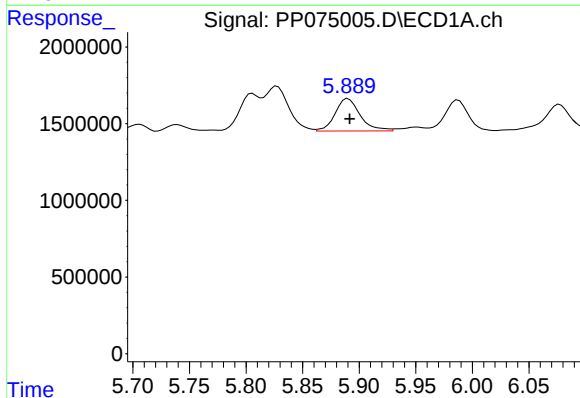


#18 AR-1242-3

R.T.: 5.890 min
Delta R.T.: -0.001 min
Response: 3254236
Conc: 80.15 ng/ml

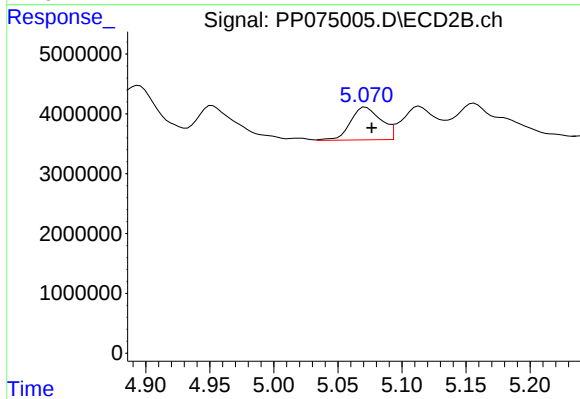

#18 AR-1242-3


R.T.: 5.072 min
Delta R.T.: -0.005 min
Response: 9107679
Conc: 76.99 ng/ml

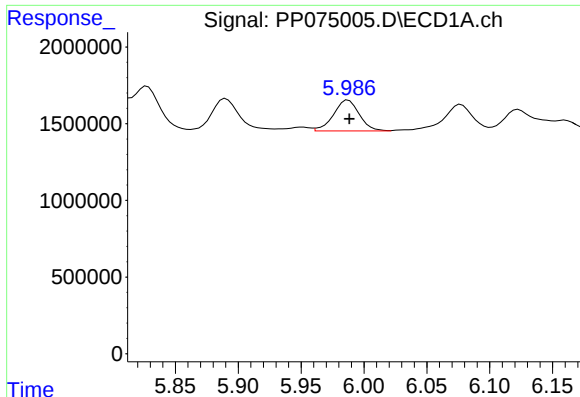

#19 AR-1242-4


R.T.: 5.988 min
Delta R.T.: -0.001 min
Response: 2876855
Conc: 90.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

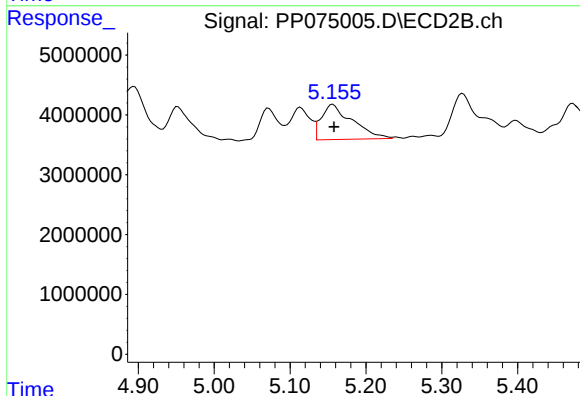


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 16647506
Conc: 97.26 ng/ml

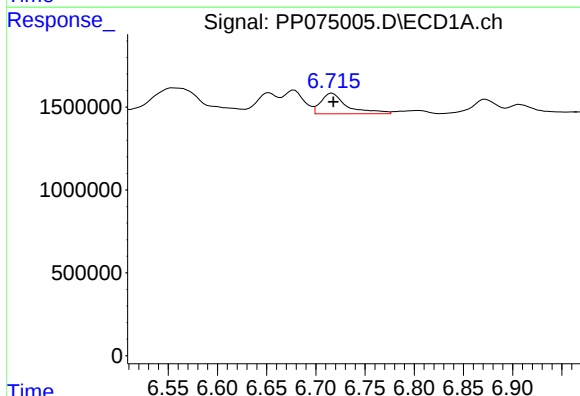


#20 AR-1242-5

R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 2314121
Conc: 64.16 ng/ml

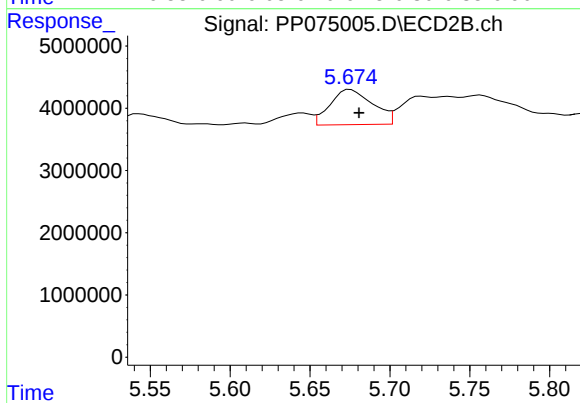

#20 AR-1242-5


R.T.: 5.675 min
Delta R.T.: -0.005 min
Response: 10481678
Conc: 56.61 ng/ml

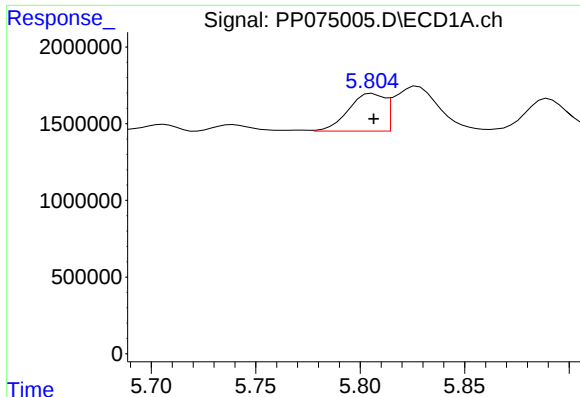

#21 AR-1248-1


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 2934611
Conc: 97.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

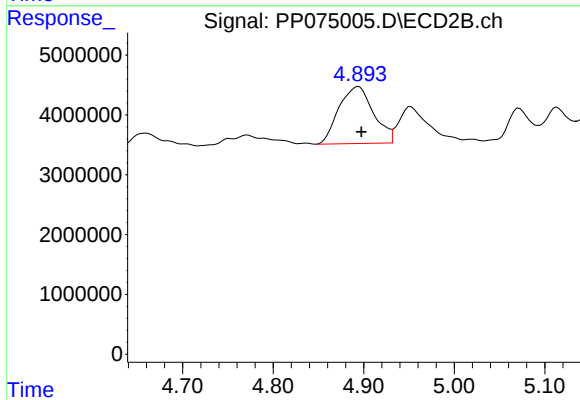


#21 AR-1248-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 25368919
Conc: 91.87 ng/ml

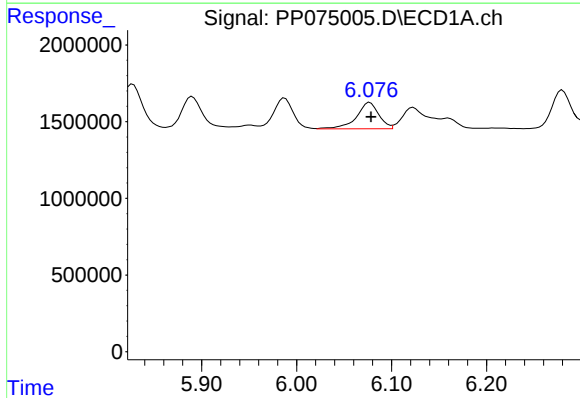


#22 AR-1248-2

R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 2816418
Conc: 65.35 ng/ml

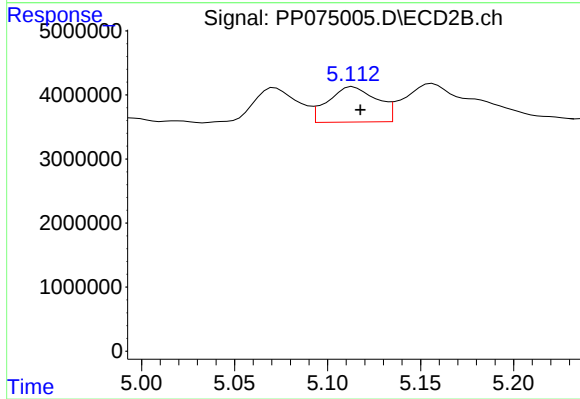

#22 AR-1248-2


R.T.: 5.114 min
Delta R.T.: -0.004 min
Response: 10011257
Conc: 56.64 ng/ml

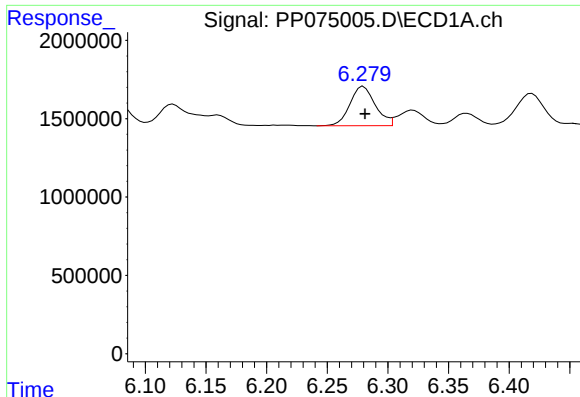

#23 AR-1248-3


R.T.: 6.280 min
Delta R.T.: -0.001 min
Response: 3658794
Conc: 78.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

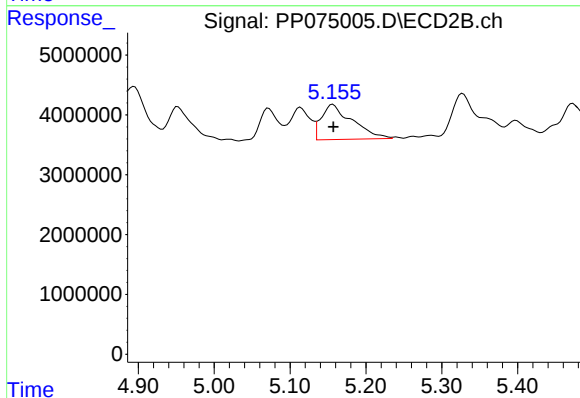


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: 0.000 min
Response: 16647506
Conc: 73.27 ng/ml

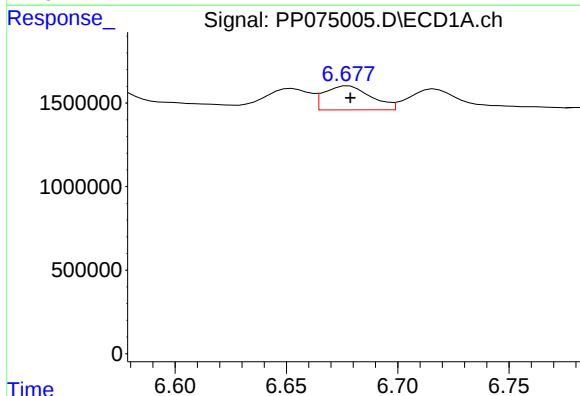


#24 AR-1248-4

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 2097396
Conc: 38.13 ng/ml

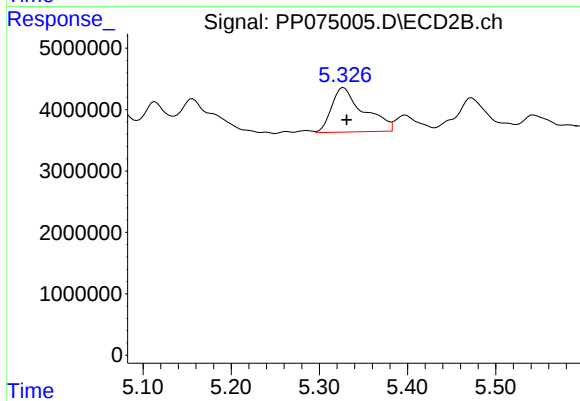

#24 AR-1248-4


R.T.: 5.328 min
Delta R.T.: -0.003 min
Response: 18213663
Conc: 83.54 ng/ml

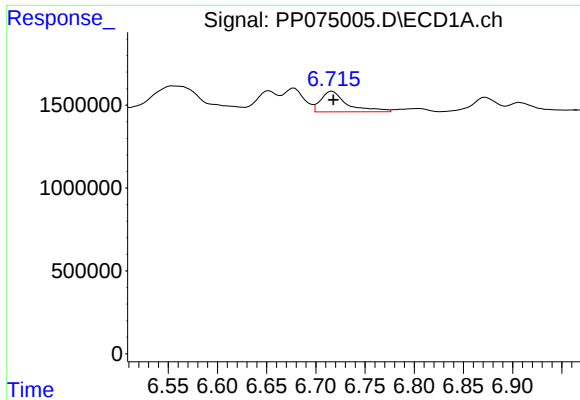

#25 AR-1248-5


R.T.: 6.717 min
Delta R.T.: -0.001 min
Response: 2314121
Conc: 41.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

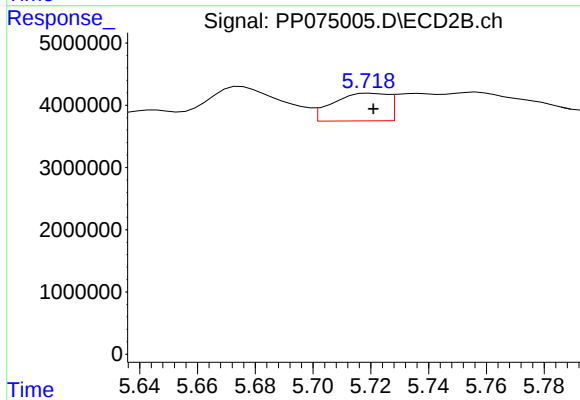


#25 AR-1248-5

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 5842597
Conc: 15.91 ng/ml

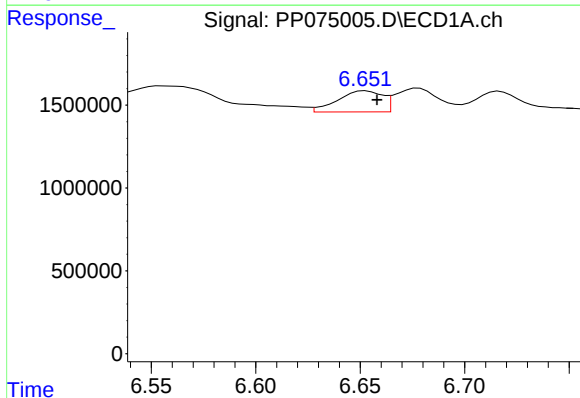


#26 AR-1254-1

R.T.: 6.653 min
Delta R.T.: -0.005 min
Response: 1901082
Conc: 32.63 ng/ml

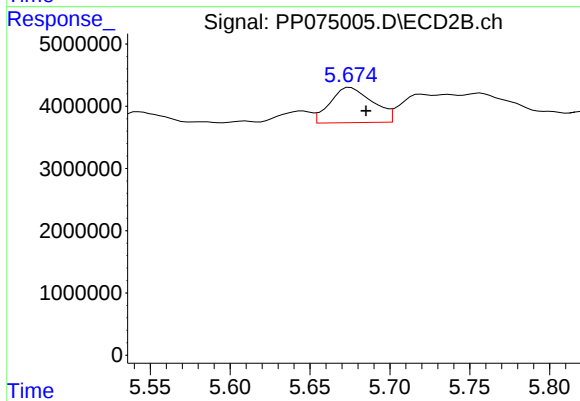

#26 AR-1254-1


R.T.: 5.675 min
Delta R.T.: -0.010 min
Response: 10481678
Conc: 21.99 ng/ml

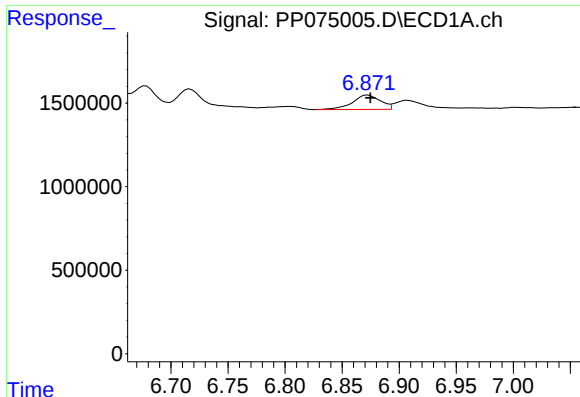

#27 AR-1254-2


R.T.: 6.872 min
Delta R.T.: -0.002 min
Response: 1454681
Conc: 17.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

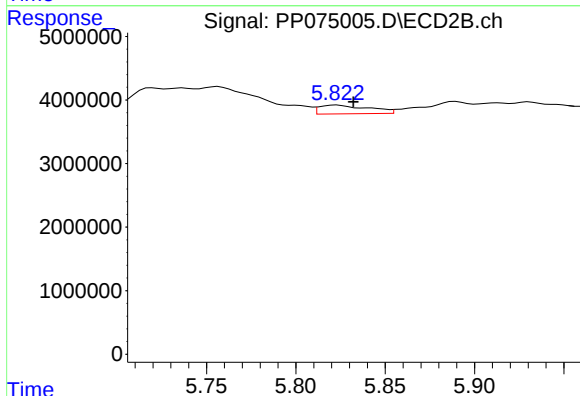


#27 AR-1254-2

R.T.: 5.823 min
Delta R.T.: -0.009 min
Response: 2690211
Conc: 7.64 ng/ml

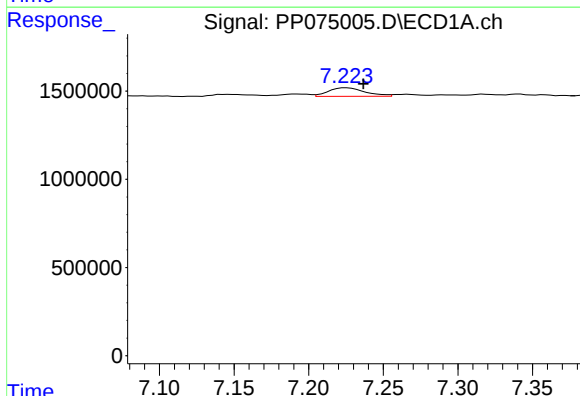


#28 AR-1254-3

R.T.: 7.225 min
Delta R.T.: -0.012 min
Response: 837846
Conc: 9.39 ng/ml

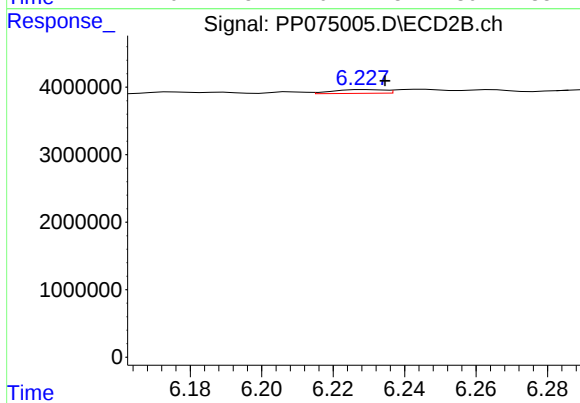

#28 AR-1254-3


R.T.: 6.229 min
Delta R.T.: -0.005 min
Response: 549482
Conc: 0.89 ng/ml

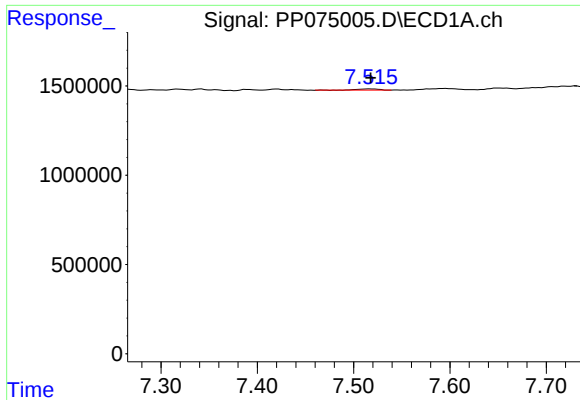

#29 AR-1254-4


R.T.: 7.517 min
Delta R.T.: -0.001 min
Response: 107740
Conc: 1.63 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

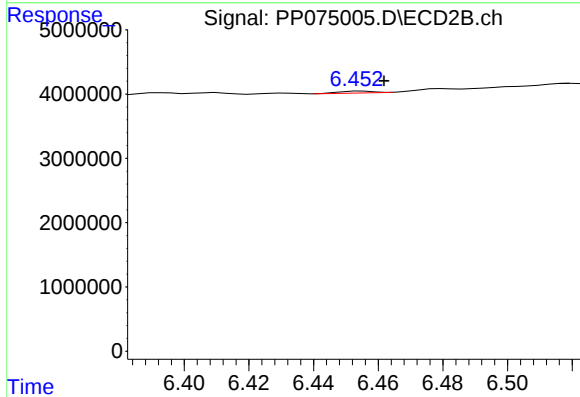


#29 AR-1254-4

R.T.: 6.455 min
Delta R.T.: -0.007 min
Response: 206725
Conc: 0.44 ng/ml

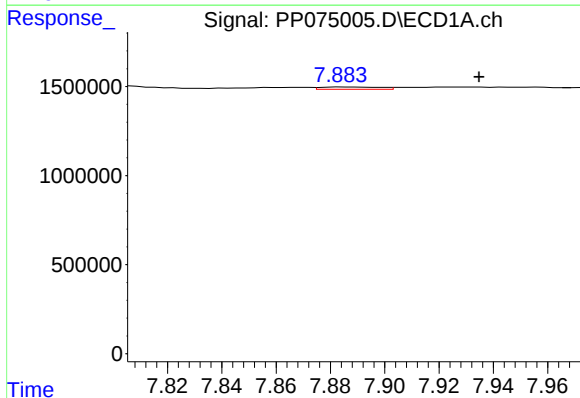


#30 AR-1254-5

R.T.: 7.884 min
Delta R.T.: -0.050 min
Response: 197634
Conc: 2.38 ng/ml

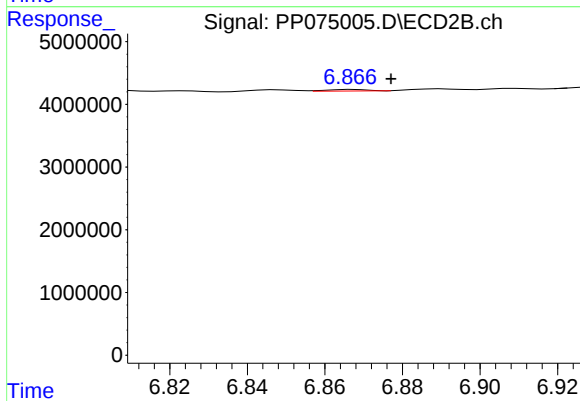

#30 AR-1254-5


R.T.: 6.867 min
Delta R.T.: -0.010 min
Response: 179370
Conc: 0.37 ng/ml

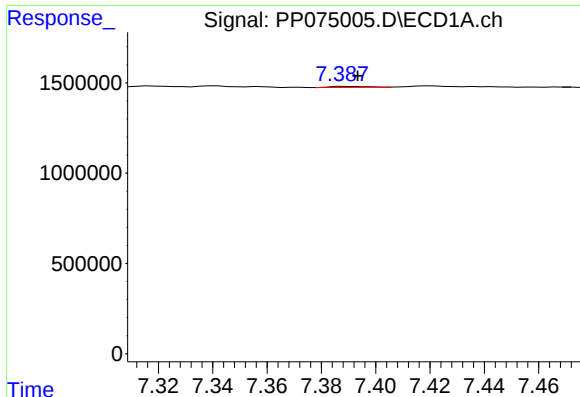

#31 AR-1260-1


R.T.: 7.389 min
Delta R.T.: -0.005 min
Response: 56379
Conc: 0.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

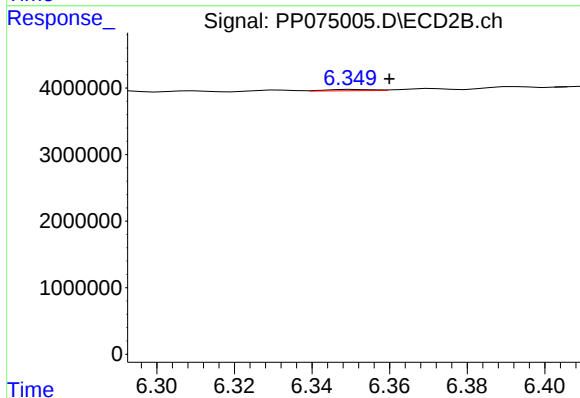


#31 AR-1260-1

R.T.: 6.351 min
Delta R.T.: -0.009 min
Response: 168034
Conc: 0.45 ng/ml

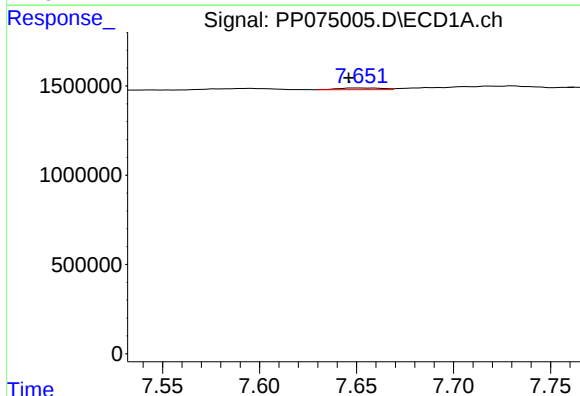


#32 AR-1260-2

R.T.: 7.652 min
Delta R.T.: 0.006 min
Response: 144801
Conc: 2.10 ng/ml

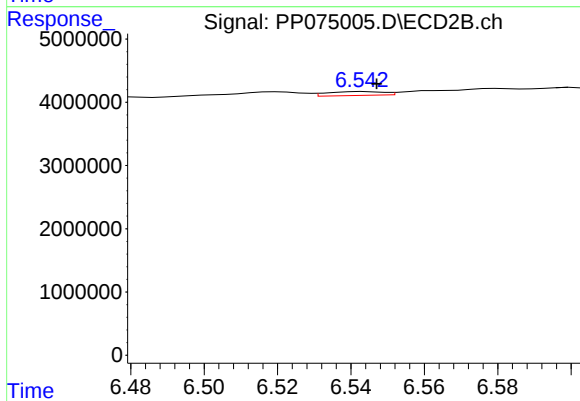

#32 AR-1260-2


R.T.: 6.543 min
Delta R.T.: -0.004 min
Response: 659404
Conc: 1.25 ng/ml

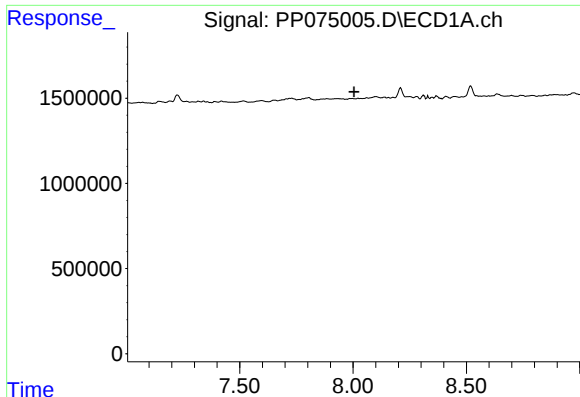

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.005 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

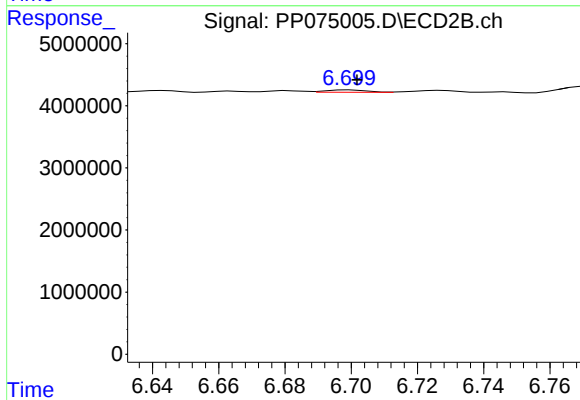


#33 AR-1260-3

R.T.: 6.700 min
Delta R.T.: -0.002 min
Response: 338783
Conc: 0.78 ng/ml

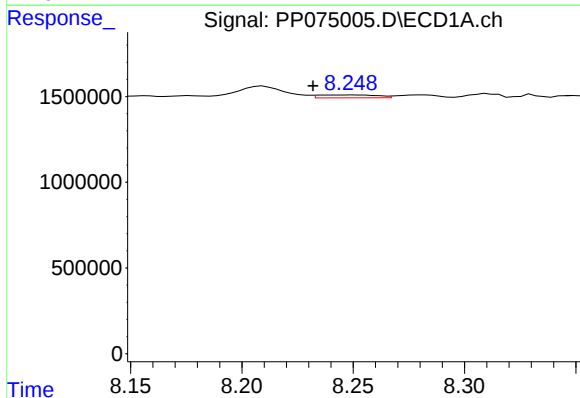


#34 AR-1260-4

R.T.: 8.249 min
Delta R.T.: 0.017 min
Response: 314507
Conc: 4.93 ng/ml

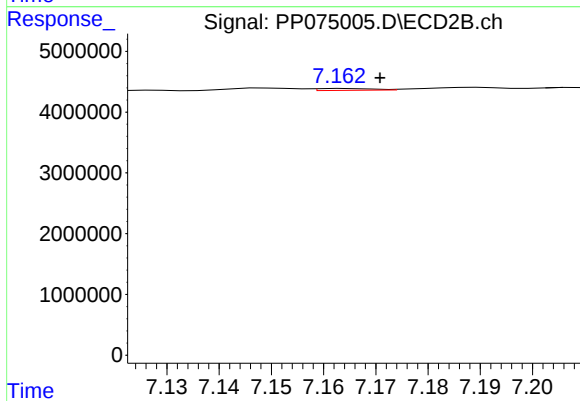

#34 AR-1260-4


R.T.: 7.164 min
Delta R.T.: -0.007 min
Response: 231399
Conc: 0.61 ng/ml

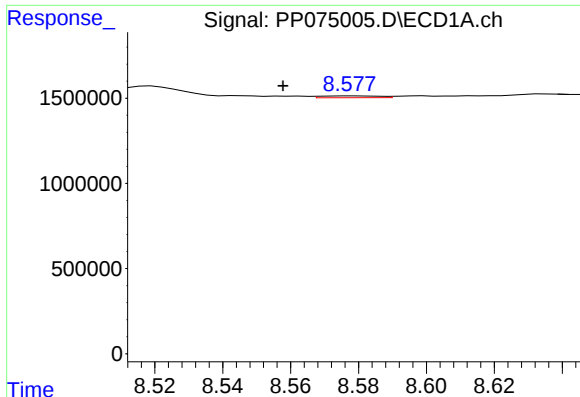

#35 AR-1260-5


R.T.: 8.578 min
Delta R.T.: 0.020 min
Response: 134684
Conc: 1.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

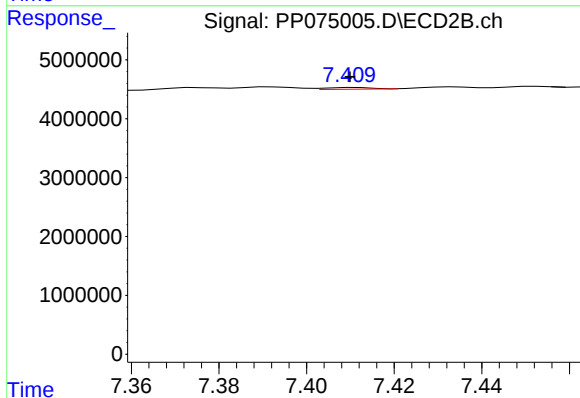


#35 AR-1260-5

R.T.: 7.411 min
Delta R.T.: 0.001 min
Response: 196226
Conc: 0.20 ng/ml

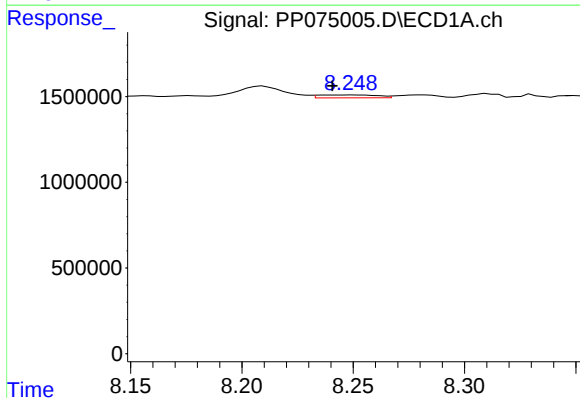


#36 AR-1262-1

R.T.: 8.249 min
Delta R.T.: 0.008 min
Response: 314507
Conc: 4.08 ng/ml

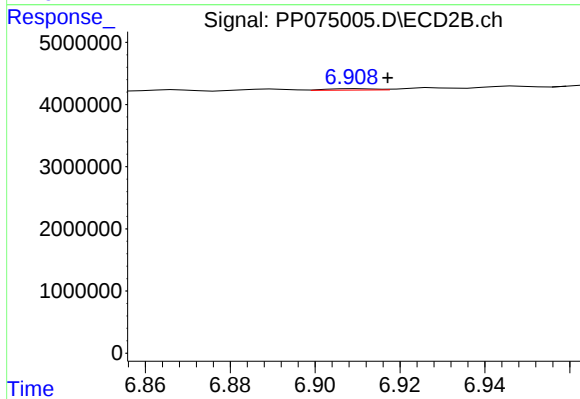

#36 AR-1262-1


R.T.: 6.909 min
Delta R.T.: -0.008 min
Response: 183637
Conc: 0.26 ng/ml

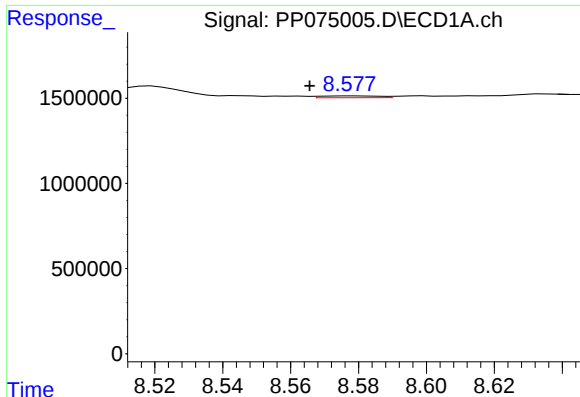

#37 AR-1262-2


R.T.: 8.578 min
Delta R.T.: 0.012 min
Response: 134684
Conc: 1.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

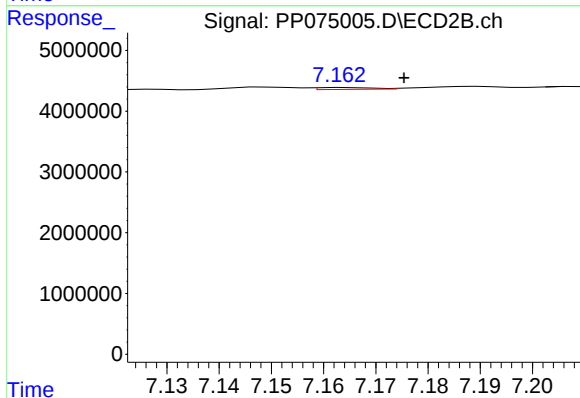


#37 AR-1262-2

R.T.: 7.164 min
Delta R.T.: -0.011 min
Response: 231399
Conc: 0.44 ng/ml

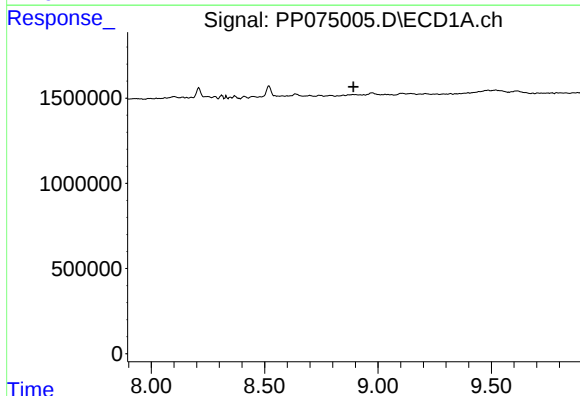


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

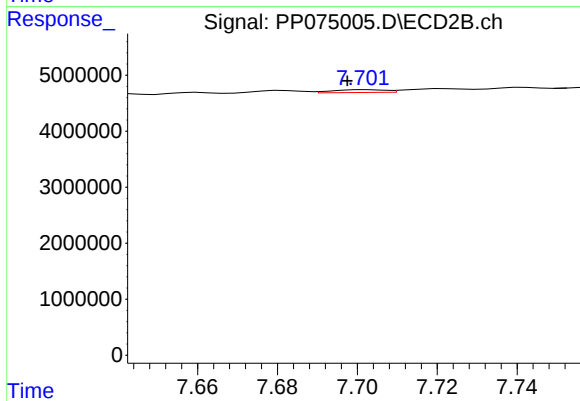

#38 AR-1262-3


R.T.: 7.702 min
Delta R.T.: 0.005 min
Response: 459707
Conc: 0.99 ng/ml

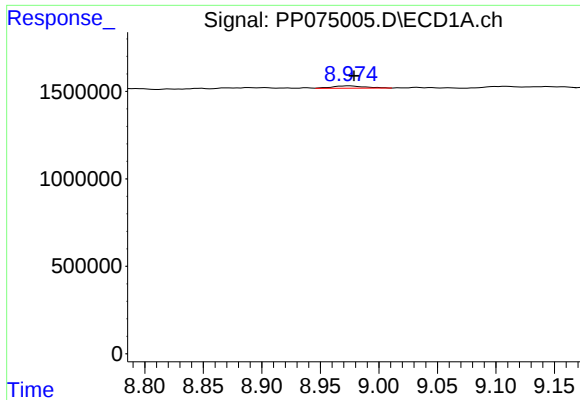

#39 AR-1262-4


R.T.: 8.975 min
Delta R.T.: -0.004 min
Response: 262439
Conc: 3.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

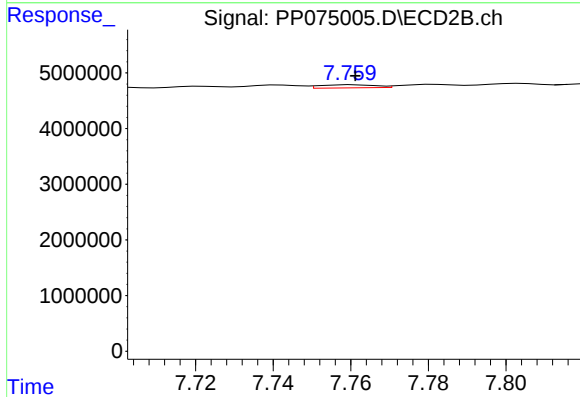


#39 AR-1262-4

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 551292
Conc: 0.67 ng/ml

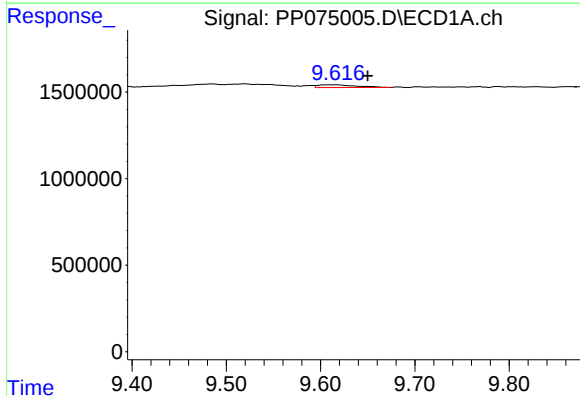


#40 AR-1262-5

R.T.: 9.610 min
Delta R.T.: -0.040 min
Response: 442767
Conc: 7.26 ng/ml

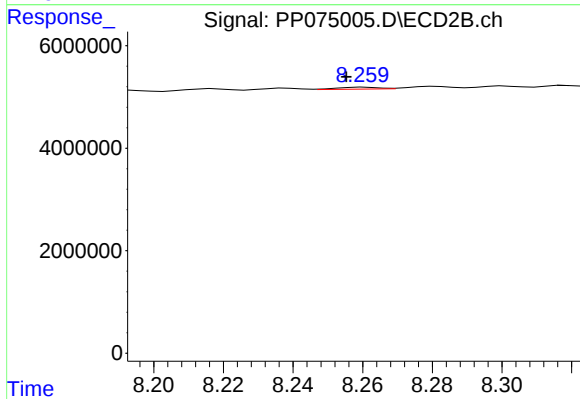

#40 AR-1262-5


R.T.: 8.261 min
Delta R.T.: 0.005 min
Response: 301244
Conc: 0.84 ng/ml

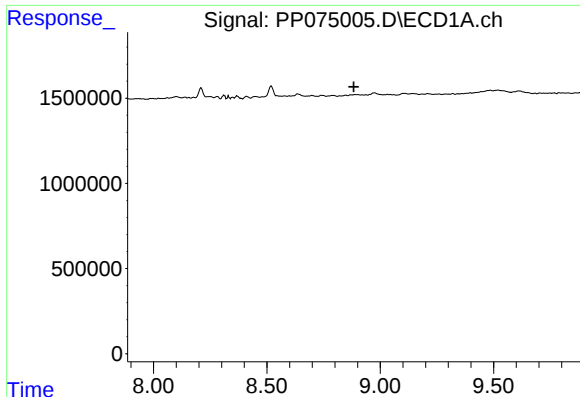

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

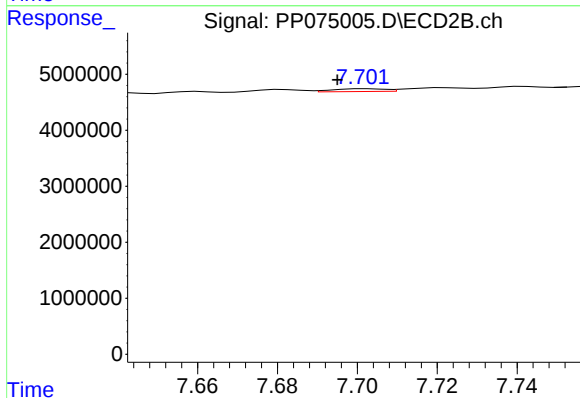


#41 AR-1268-1

R.T.: 7.702 min
Delta R.T.: 0.007 min
Response: 459707
Conc: 0.33 ng/ml

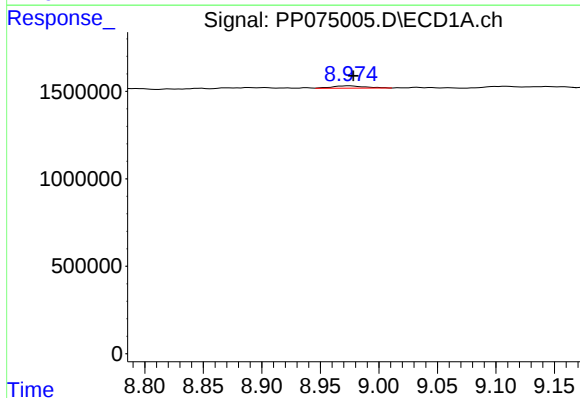


#42 AR-1268-2

R.T.: 8.975 min
Delta R.T.: -0.003 min
Response: 262439
Conc: 1.79 ng/ml

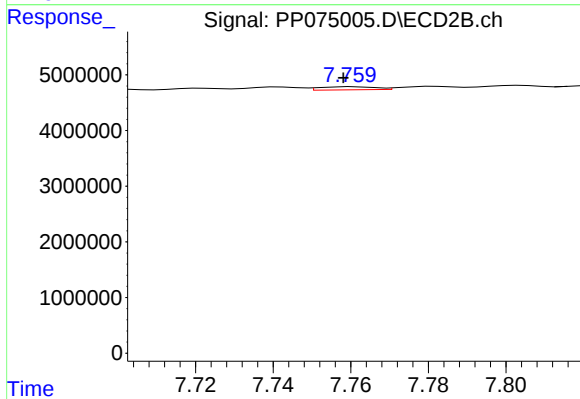

#42 AR-1268-2


R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 551292
Conc: 0.40 ng/ml

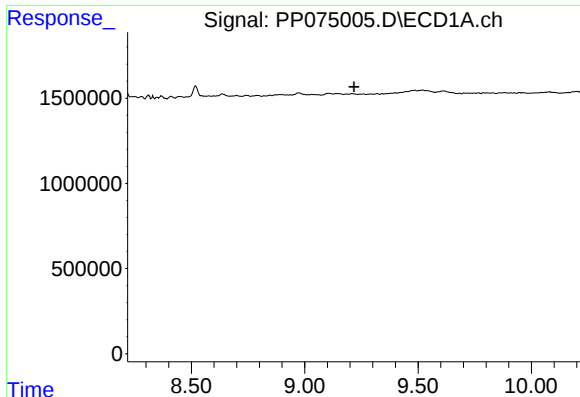

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

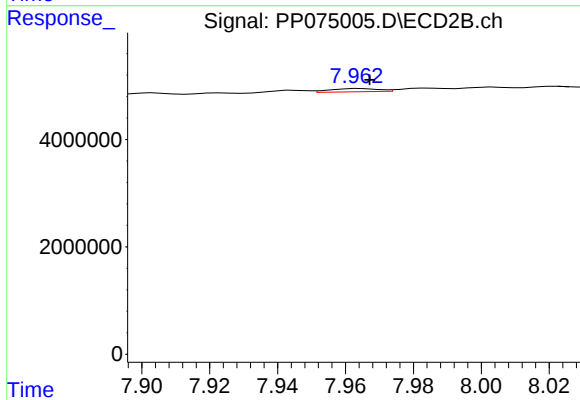


#43 AR-1268-3

R.T.: 7.964 min
Delta R.T.: -0.003 min
Response: 578737
Conc: 0.55 ng/ml

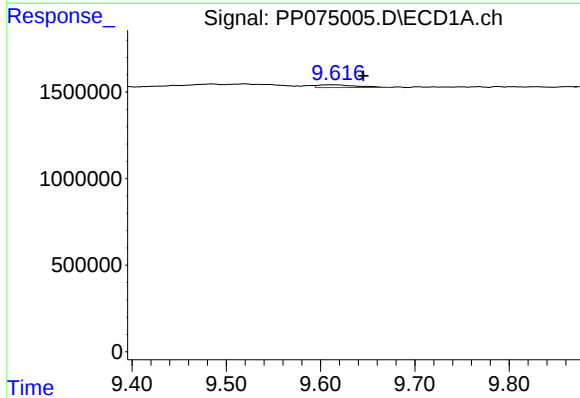


#44 AR-1268-4

R.T.: 9.610 min
Delta R.T.: -0.036 min
Response: 442767
Conc: 6.58 ng/ml

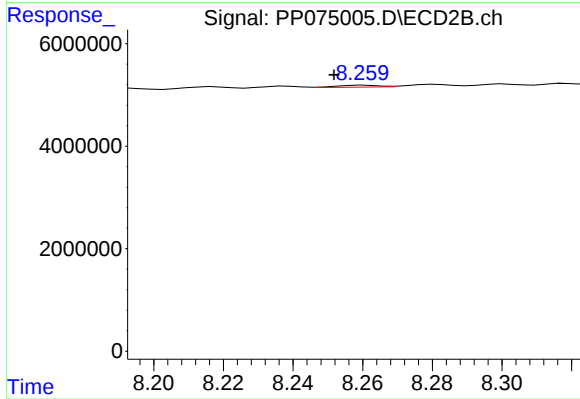

#44 AR-1268-4


R.T.: 8.261 min
Delta R.T.: 0.009 min
Response: 301244
Conc: 0.79 ng/ml

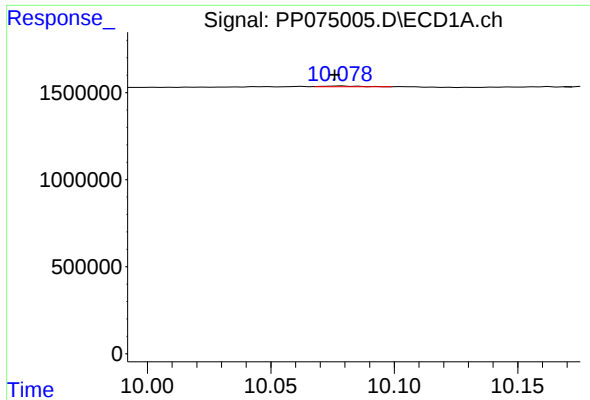

#45 AR-1268-5

R.T.: 10.079 min
Delta R.T.: 0.003 min
Response: 44867
Conc: 0.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-D

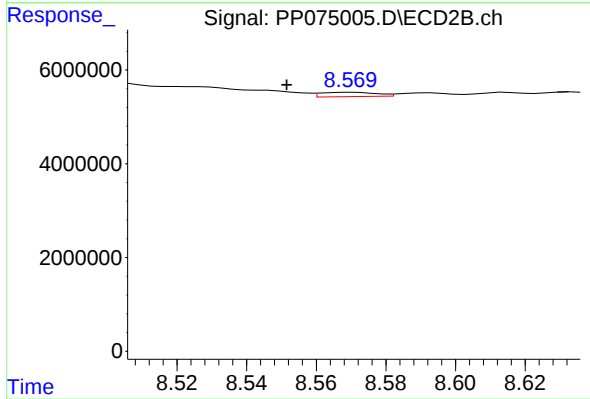

#45 AR-1268-5

R.T.: 8.570 min
Delta R.T.: 0.019 min
Response: 1044106
Conc: 0.33 ng/ml