

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075006.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 14:41
 Operator : YP\AJ
 Sample : Q3034-05
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-E

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:49:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.657	3.800	28862502	111.4E6	23.586	23.037
2)	SA Decachlor...	10.432	8.808	23445389	144.3E6	23.742	19.247
Target Compounds							
3)	L1 AR-1016-1	5.808	4.897	2771336	20906962	62.858	41.046 #
4)	L1 AR-1016-2	5.830	4.954	4046437	10729106	64.391	45.077 #
5)	L1 AR-1016-3	5.892	5.075	3527786	7022778	78.545	50.925 #
6)	L1 AR-1016-4	5.989	5.117	2967603	8004472	84.350	57.255 #
7)	L1 AR-1016-5	6.282	5.330	4138867	12383729	124.717	74.563 #
8)	L2 AR-1221-1	4.855	4.017	792218	503142	45.031	8.133 #
9)	L2 AR-1221-2	4.958	4.103	587826	2292730	44.008	50.711
10)	L2 AR-1221-3	5.018	4.171	332522	852815	8.771	5.191 #
11)	L3 AR-1232-1	5.018	4.171	332522	852815	10.948	6.658 #
12)	L3 AR-1232-2	5.544	4.897	1712558	20906962	108.677	90.197
13)	L3 AR-1232-3	5.830	5.075	4046437	7022778	132.480	116.930
14)	L3 AR-1232-4	5.989	5.158	2967603	13577788	171.843	184.212
15)	L3 AR-1232-5	6.079	5.330	2968057	12383729	228.647	199.468
16)	L4 AR-1242-1	5.808	4.897	2771336	20906962	72.406	49.572 #
17)	L4 AR-1242-2	5.830	4.954	4046437	10729106	71.641	53.570 #
18)	L4 AR-1242-3	5.892	5.075	3527786	7022778	86.885	59.365 #
19)	L4 AR-1242-4	5.989	5.158	2967603	13577788	93.492	79.328
20)	L4 AR-1242-5	6.719	5.679	3029590	11264242	83.991	60.834 #
21)	L5 AR-1248-1	5.808	4.897	2771336	20906962	91.693	75.711
22)	L5 AR-1248-2	6.079	5.117	2968057	8004472	68.871	45.286 #
23)	L5 AR-1248-3	6.282	5.158	4138867	13577788	88.620	59.760 #
24)	L5 AR-1248-4	6.680	5.330	2548407	12383729	46.334	56.801
25)	L5 AR-1248-5	6.719	5.723	3029590	7281139	54.616	19.822 #
26)	L6 AR-1254-1	6.654	5.679	2015482	11264242	34.589	23.629 #
27)	L6 AR-1254-2	6.875	5.828	1947140	1906548	23.857	5.414 #
28)	L6 AR-1254-3	7.231	6.225	786018	774121	8.811	1.249 #
29)	L6 AR-1254-4	7.513	6.469	218964	274271	3.322	0.585 #
30)	L6 AR-1254-5	7.936	6.872	946126	252753	11.387	0.515 #
31)	L7 AR-1260-1	0.000	6.355	0	168159	N.D.	0.448 #
32)	L7 AR-1260-2	7.656	6.551	509122	368750	7.387	0.697 #
33)	L7 AR-1260-3	8.007	6.698	249316	306595	4.805	0.708 #
34)	L7 AR-1260-4	8.212	7.163	1215643	333086	19.056	0.873 #
35)	L7 AR-1260-5	8.557	7.419	107222	275278	0.945	0.274 #
36)	L8 AR-1262-1	8.212	6.917	1215643	358398	15.784	0.507 #
37)	L8 AR-1262-2	8.571	7.184	132173	278030	0.998	0.534 #
38)	L8 AR-1262-3	8.886	7.697	193931	377151	1.995	0.809 #
39)	L8 AR-1262-4	8.966	7.763	513447	507226	6.816	0.617 #
40)	L8 AR-1262-5	9.613f	8.252	370012	111362	6.070	0.311 #
41)	L9 AR-1268-1	8.886	7.697	193931	377151	1.197	0.267 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 14:41
Operator : YP\AJ
Sample : Q3034-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.966	7.763	513447	507226	3.499	0.372 #
43)	L9 AR-1268-3	9.223	7.966	385850	821963	3.122	0.788 #
44)	L9 AR-1268-4	9.613	8.252	370012	111362	5.501	0.291 #
45)	L9 AR-1268-5	10.081	8.541	95984	1679634	0.259	0.536 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075006.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 14:41
Operator : YP\AJ
Sample : Q3034-05
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:49:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

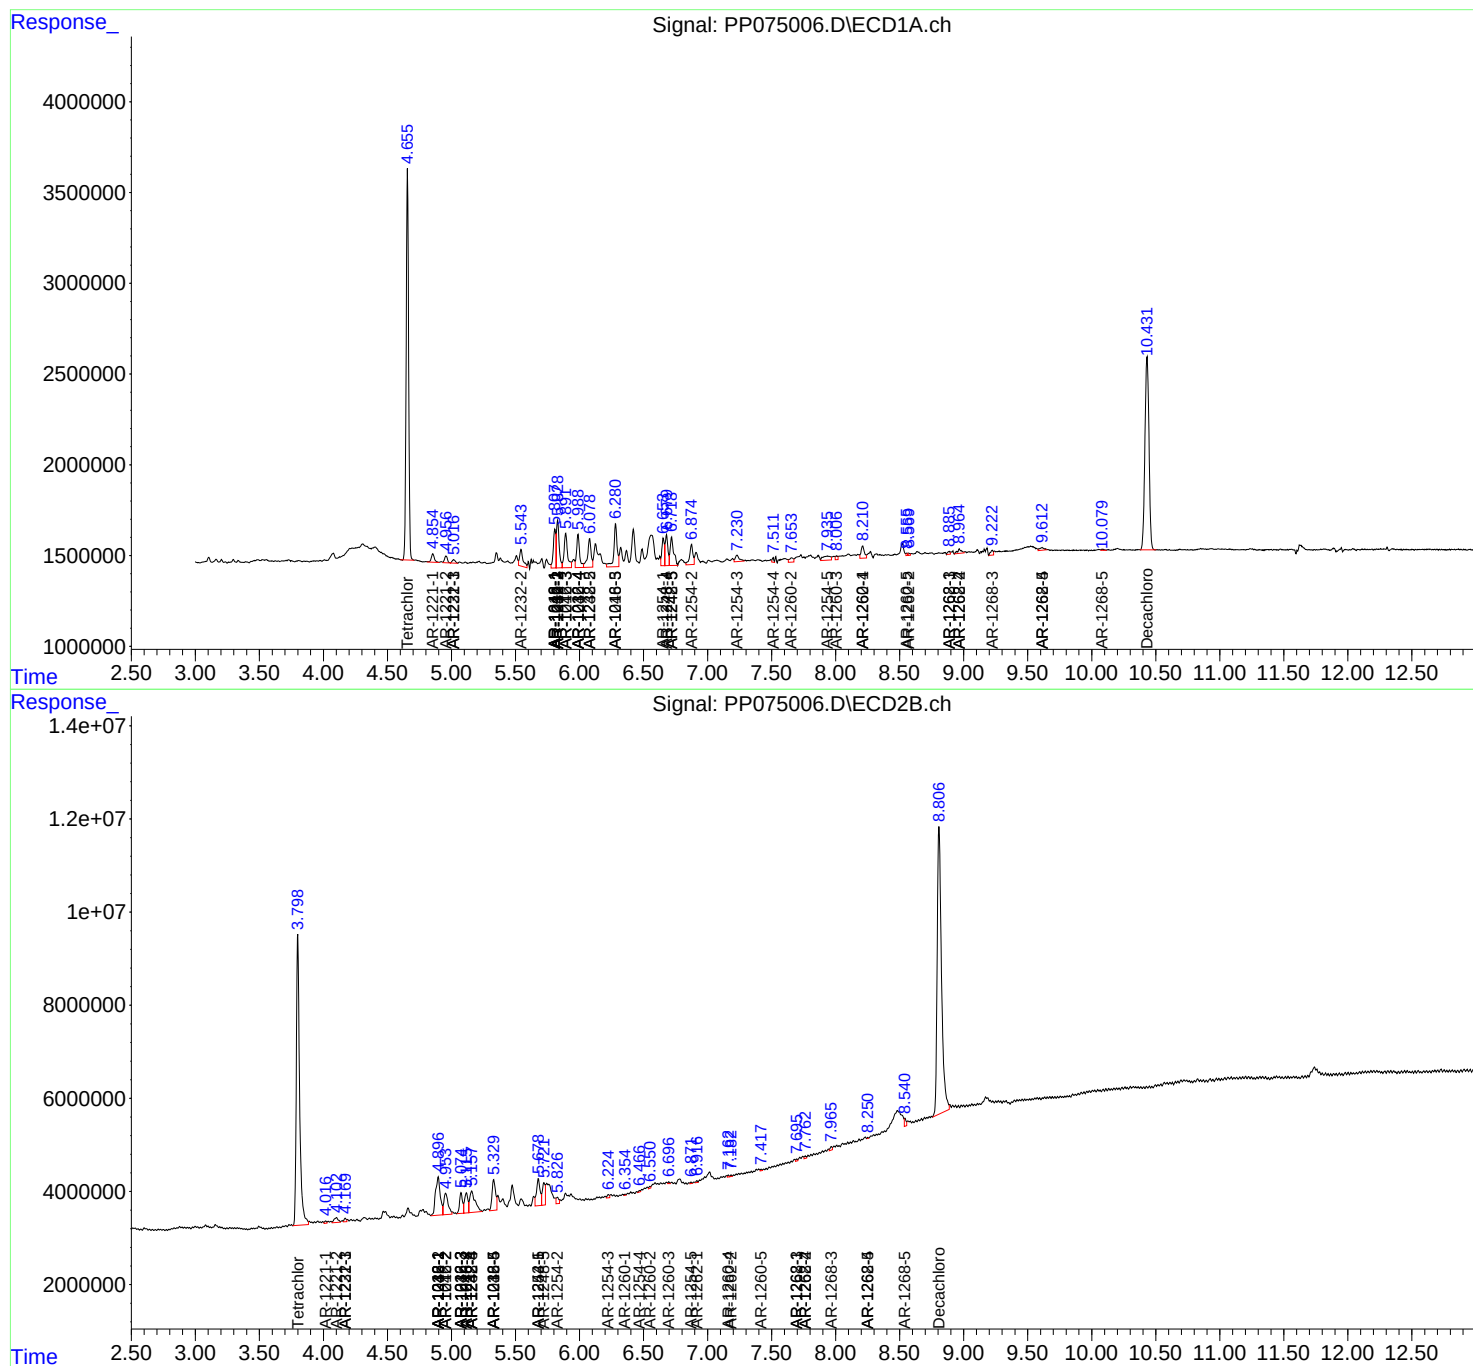


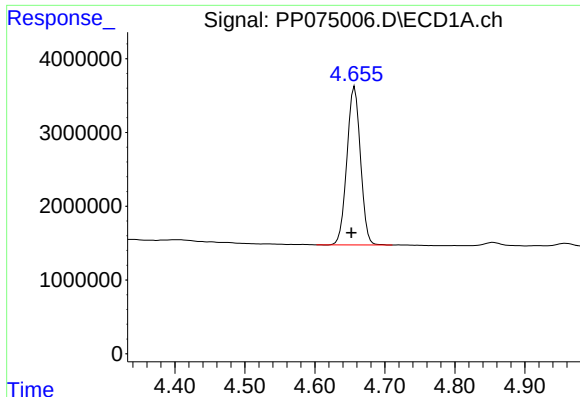

#1 Tetrachloro-m-xylene


R.T.: 4.657 min
Delta R.T.: 0.005 min
Response: 28862502
Conc: 23.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

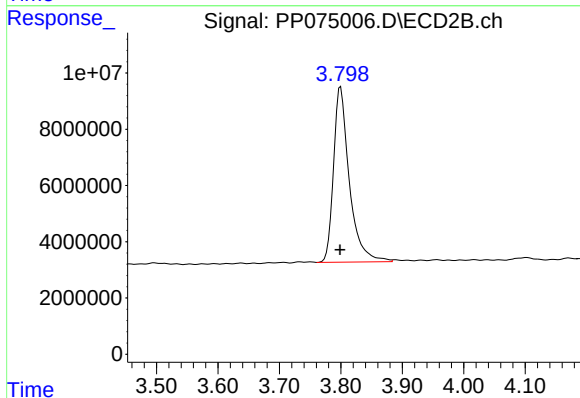


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.000 min
Response: 111393251
Conc: 23.04 ng/ml

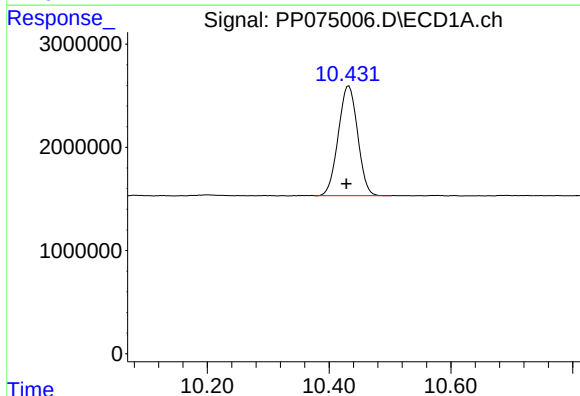


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.004 min
Response: 23445389
Conc: 23.74 ng/ml

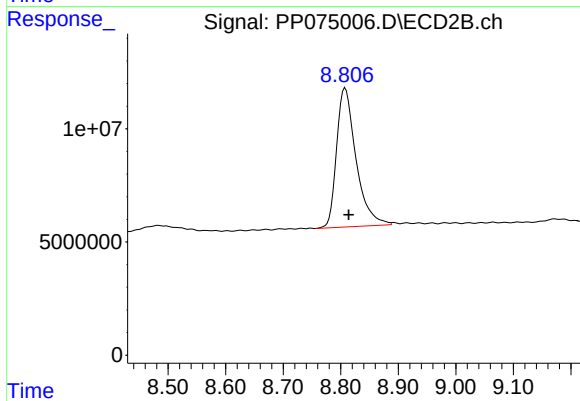

#2 Decachlorobiphenyl


R.T.: 8.808 min
Delta R.T.: -0.006 min
Response: 144337488
Conc: 19.25 ng/ml

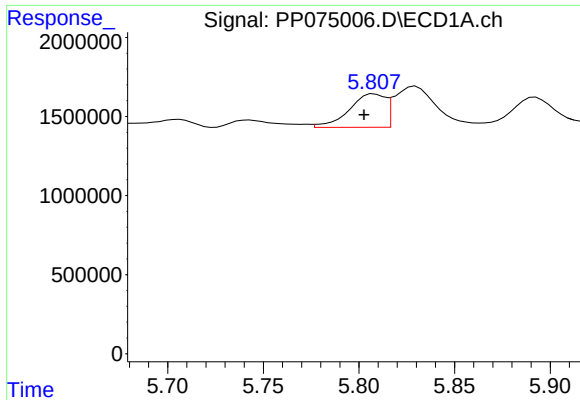

#3 AR-1016-1


R.T.: 5.808 min
Delta R.T.: 0.005 min
Response: 2771336
Conc: 62.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

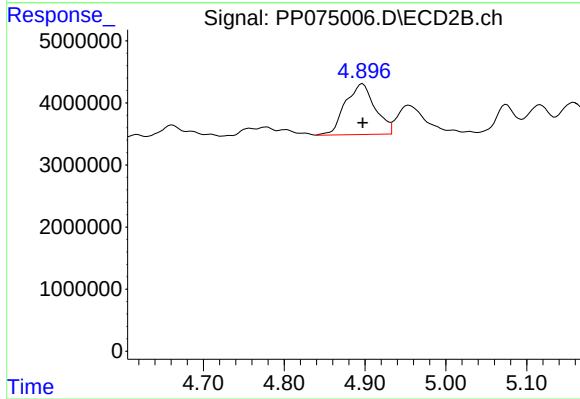


#3 AR-1016-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 20906962
Conc: 41.05 ng/ml

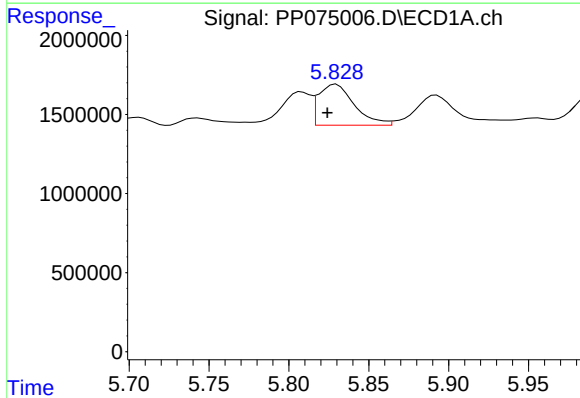


#4 AR-1016-2

R.T.: 5.830 min
Delta R.T.: 0.005 min
Response: 4046437
Conc: 64.39 ng/ml

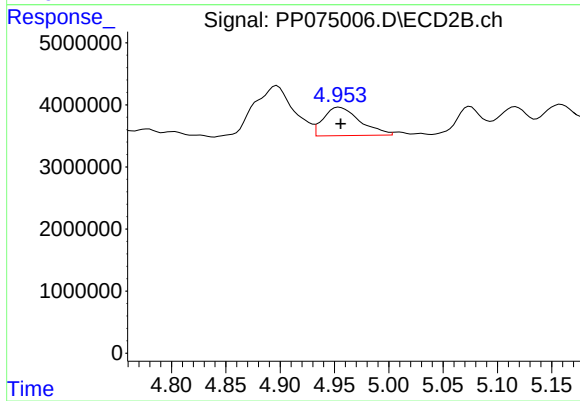

#4 AR-1016-2


R.T.: 4.954 min
Delta R.T.: -0.001 min
Response: 10729106
Conc: 45.08 ng/ml

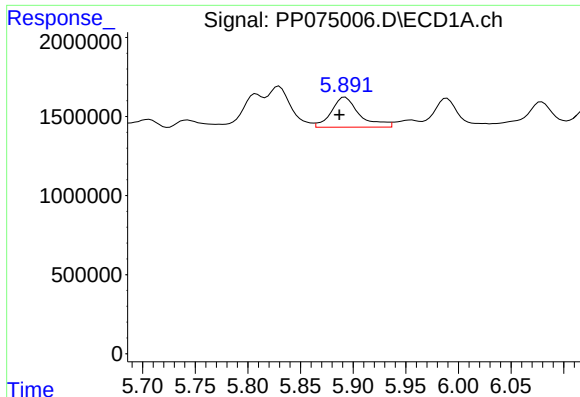

#5 AR-1016-3


R.T.: 5.892 min
Delta R.T.: 0.005 min
Response: 3527786
Conc: 78.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

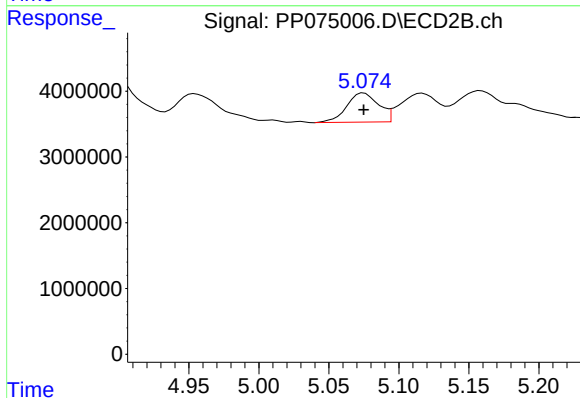


#5 AR-1016-3

R.T.: 5.075 min
Delta R.T.: 0.000 min
Response: 7022778
Conc: 50.93 ng/ml

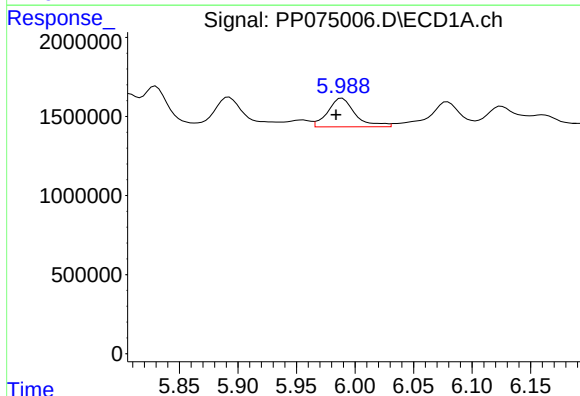


#6 AR-1016-4

R.T.: 5.989 min
Delta R.T.: 0.005 min
Response: 2967603
Conc: 84.35 ng/ml

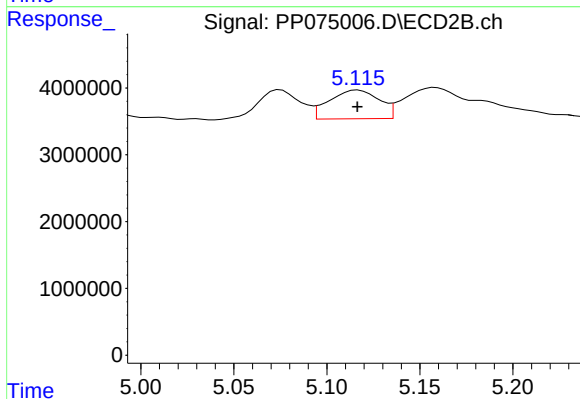

#6 AR-1016-4


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 8004472
Conc: 57.26 ng/ml

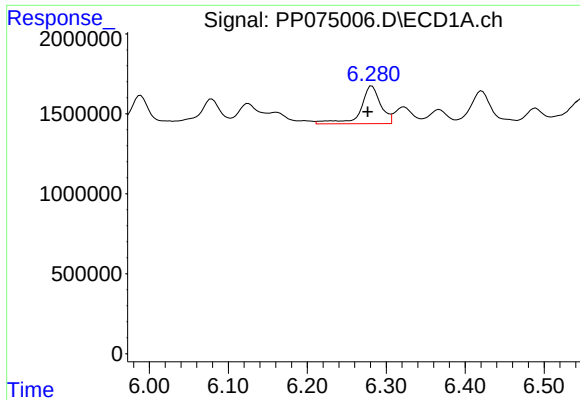

#7 AR-1016-5


R.T.: 6.282 min
Delta R.T.: 0.006 min
Response: 4138867
Conc: 124.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

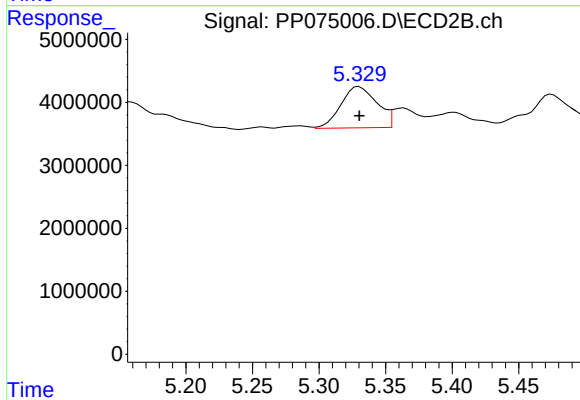


#7 AR-1016-5

R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 12383729
Conc: 74.56 ng/ml

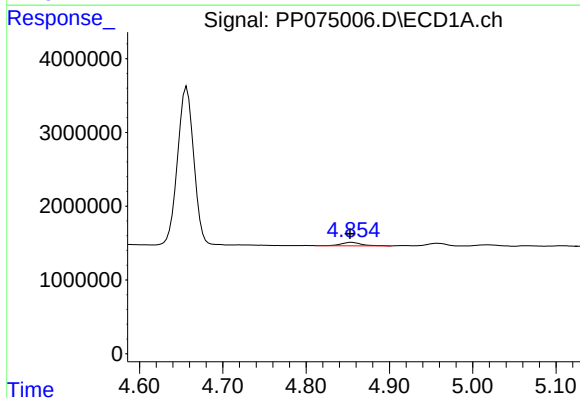


#8 AR-1221-1

R.T.: 4.855 min
Delta R.T.: 0.002 min
Response: 792218
Conc: 45.03 ng/ml

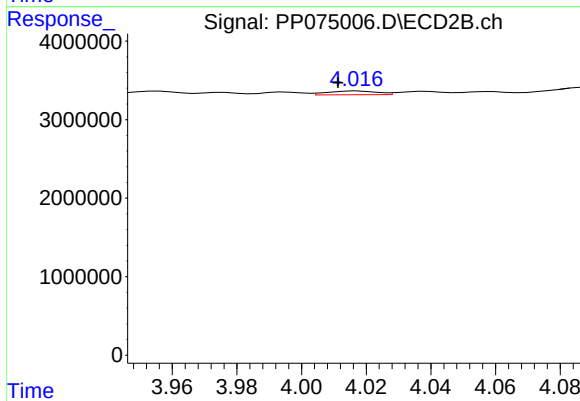

#8 AR-1221-1


R.T.: 4.017 min
Delta R.T.: 0.006 min
Response: 503142
Conc: 8.13 ng/ml

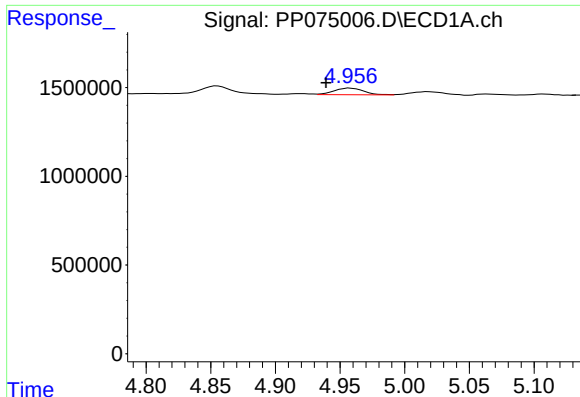

#9 AR-1221-2


R.T.: 4.958 min
Delta R.T.: 0.019 min
Response: 587826
Conc: 44.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

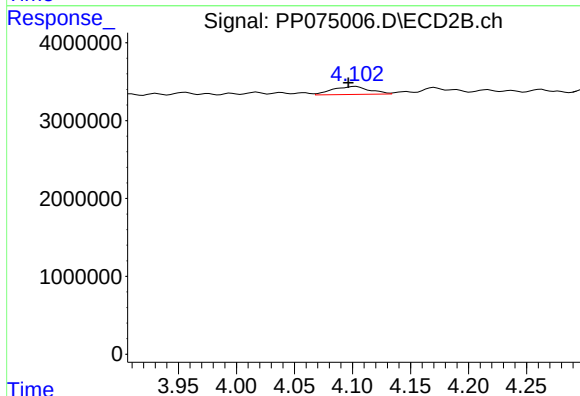


#9 AR-1221-2

R.T.: 4.103 min
Delta R.T.: 0.006 min
Response: 2292730
Conc: 50.71 ng/ml

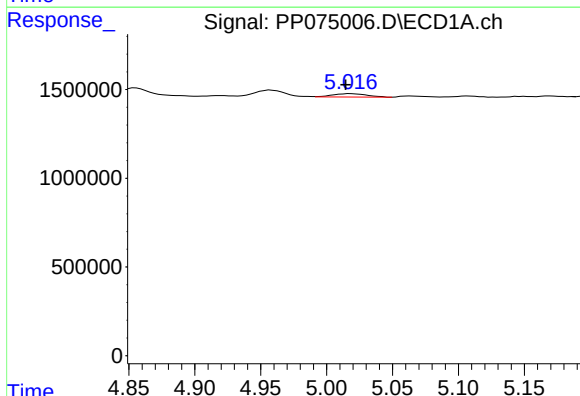


#10 AR-1221-3

R.T.: 5.018 min
Delta R.T.: 0.003 min
Response: 332522
Conc: 8.77 ng/ml

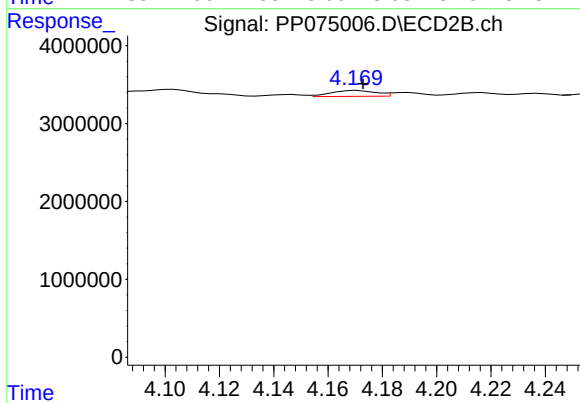

#10 AR-1221-3


R.T.: 4.171 min
Delta R.T.: -0.002 min
Response: 852815
Conc: 5.19 ng/ml

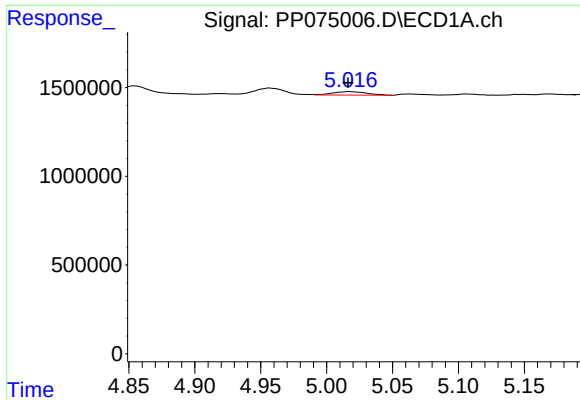

#11 AR-1232-1


R.T.: 5.018 min
 Delta R.T.: 0.002 min
 Response: 332522
 Conc: 10.95 ng/ml

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-E

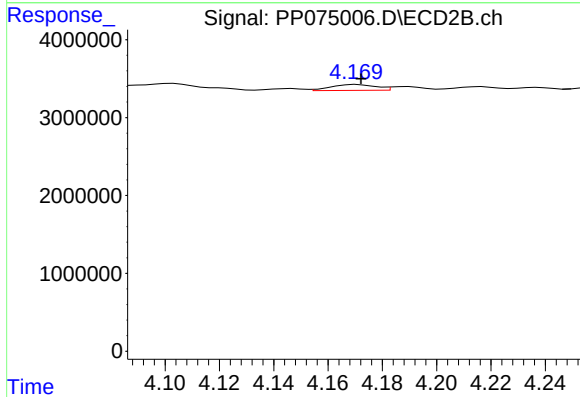


#11 AR-1232-1

R.T.: 4.171 min
 Delta R.T.: -0.002 min
 Response: 852815
 Conc: 6.66 ng/ml

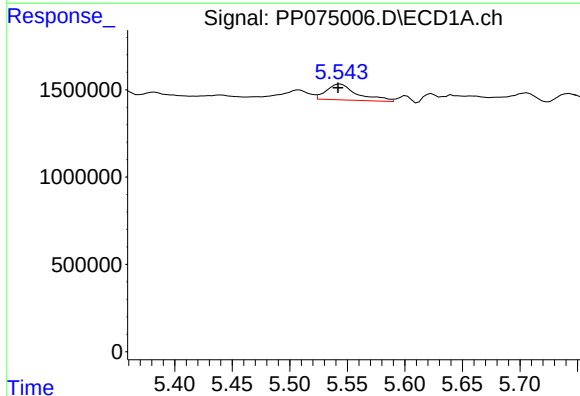


#12 AR-1232-2

R.T.: 5.544 min
 Delta R.T.: 0.002 min
 Response: 1712558
 Conc: 108.68 ng/ml

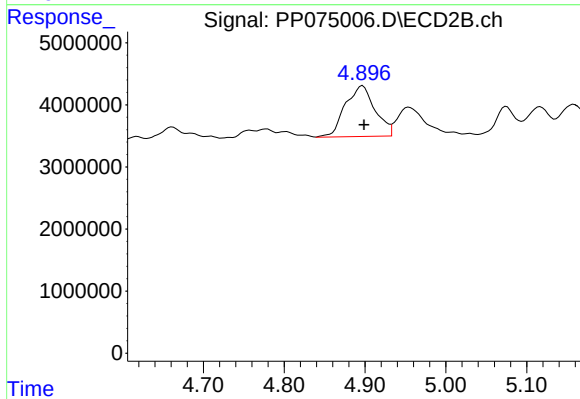

#12 AR-1232-2


R.T.: 4.897 min
 Delta R.T.: -0.002 min
 Response: 20906962
 Conc: 90.20 ng/ml

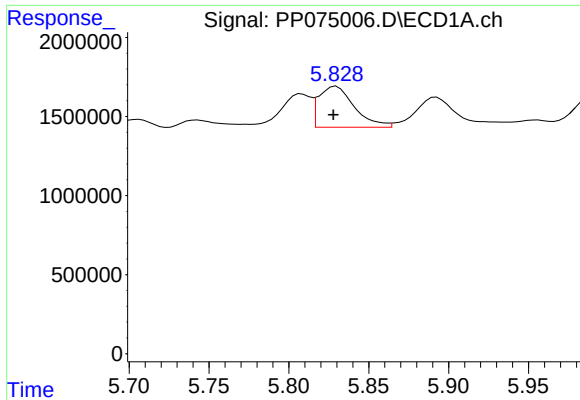

#13 AR-1232-3


R.T.: 5.830 min
Delta R.T.: 0.002 min
Response: 4046437
Conc: 132.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

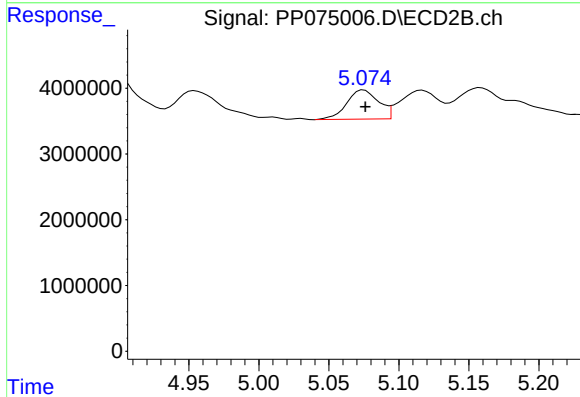


#13 AR-1232-3

R.T.: 5.075 min
Delta R.T.: -0.001 min
Response: 7022778
Conc: 116.93 ng/ml

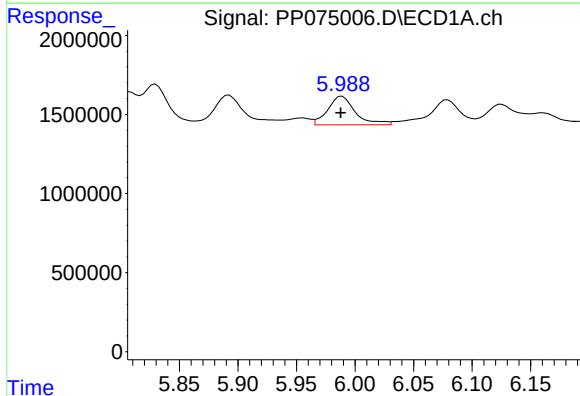


#14 AR-1232-4

R.T.: 5.989 min
Delta R.T.: 0.001 min
Response: 2967603
Conc: 171.84 ng/ml

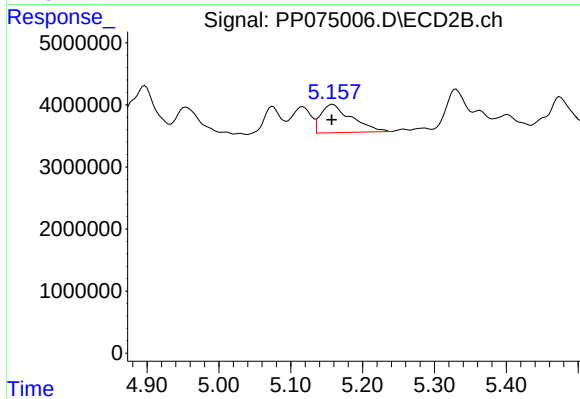

#14 AR-1232-4


R.T.: 5.158 min
Delta R.T.: 0.001 min
Response: 13577788
Conc: 184.21 ng/ml

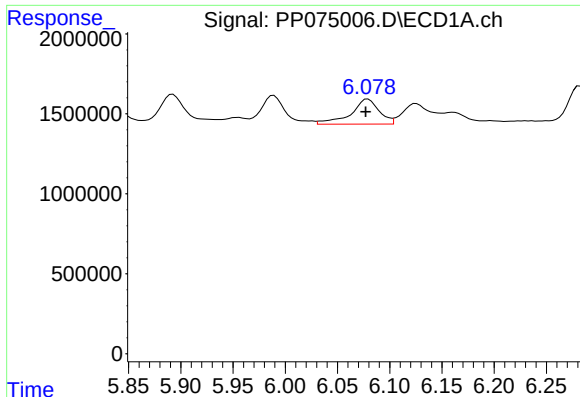

#15 AR-1232-5


R.T.: 6.079 min
Delta R.T.: 0.002 min
Response: 2968057
Conc: 228.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

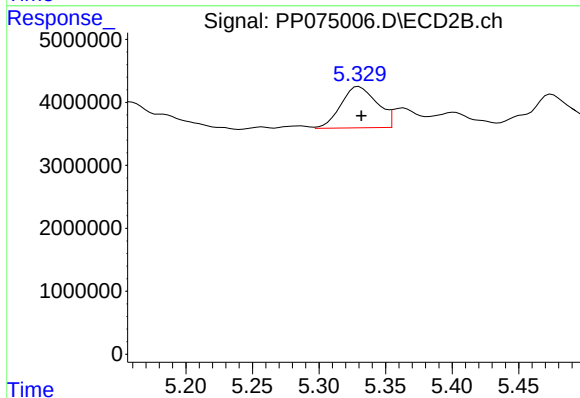


#15 AR-1232-5

R.T.: 5.330 min
Delta R.T.: -0.002 min
Response: 12383729
Conc: 199.47 ng/ml

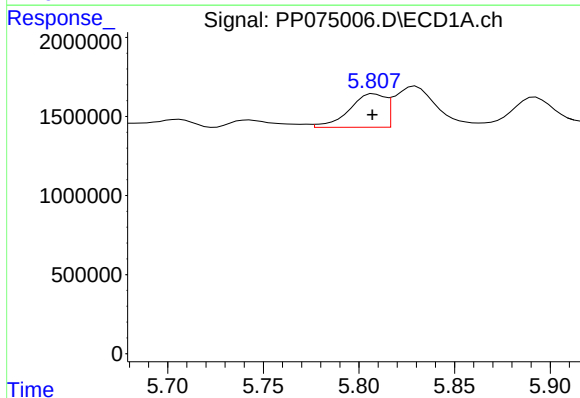


#16 AR-1242-1

R.T.: 5.808 min
Delta R.T.: 0.001 min
Response: 2771336
Conc: 72.41 ng/ml

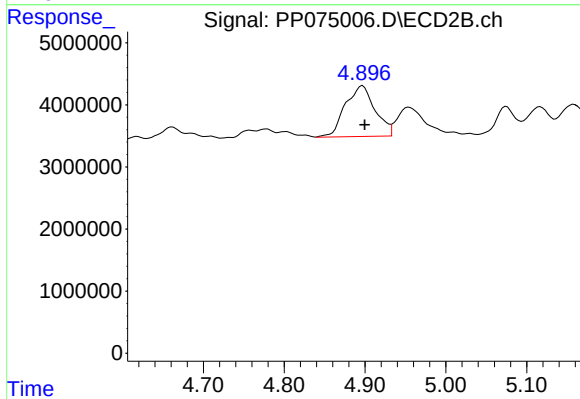

#16 AR-1242-1


R.T.: 4.897 min
Delta R.T.: -0.002 min
Response: 20906962
Conc: 49.57 ng/ml

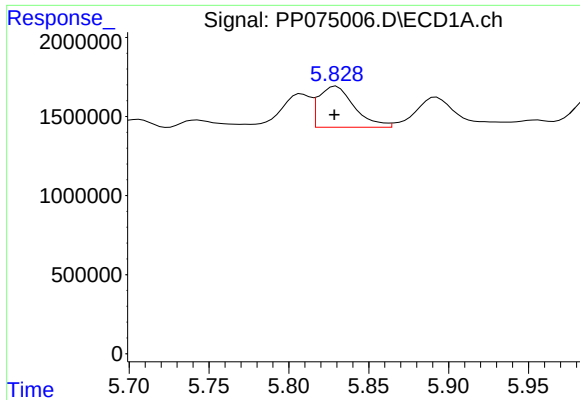

#17 AR-1242-2


R.T.: 5.830 min
Delta R.T.: 0.001 min
Response: 4046437
Conc: 71.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

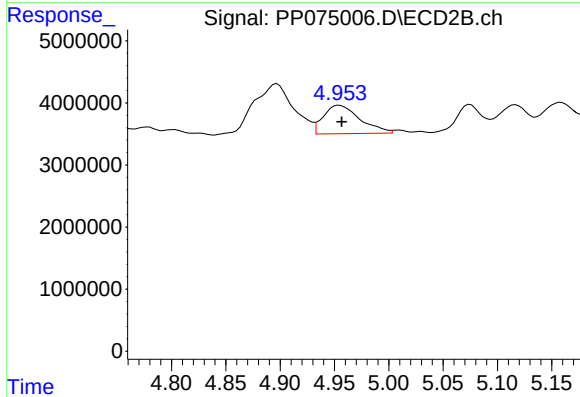


#17 AR-1242-2

R.T.: 4.954 min
Delta R.T.: -0.002 min
Response: 10729106
Conc: 53.57 ng/ml

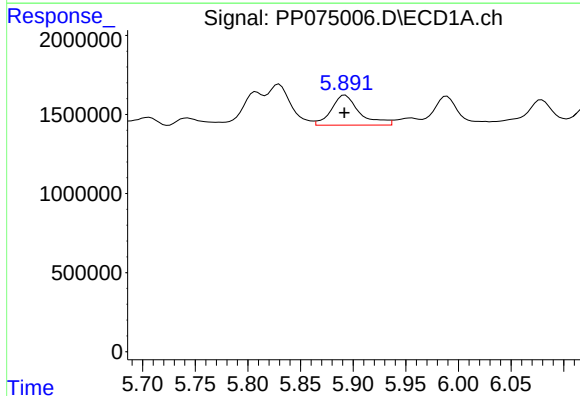


#18 AR-1242-3

R.T.: 5.892 min
Delta R.T.: 0.000 min
Response: 3527786
Conc: 86.89 ng/ml

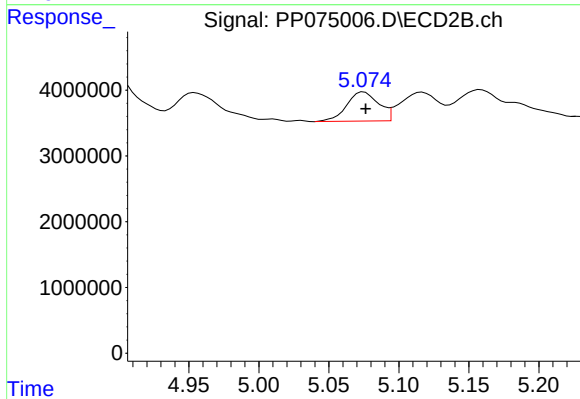

#18 AR-1242-3


R.T.: 5.075 min
Delta R.T.: -0.001 min
Response: 7022778
Conc: 59.37 ng/ml

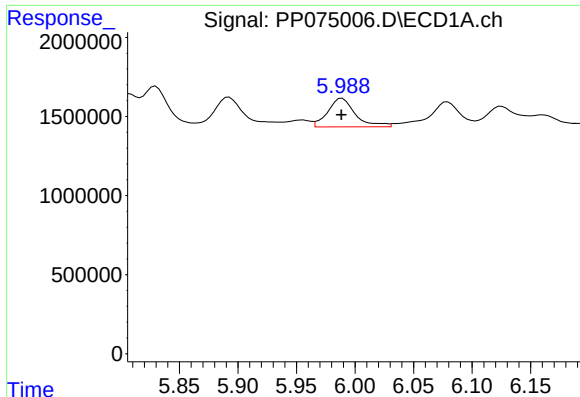

#19 AR-1242-4


R.T.: 5.989 min
Delta R.T.: 0.000 min
Response: 2967603
Conc: 93.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

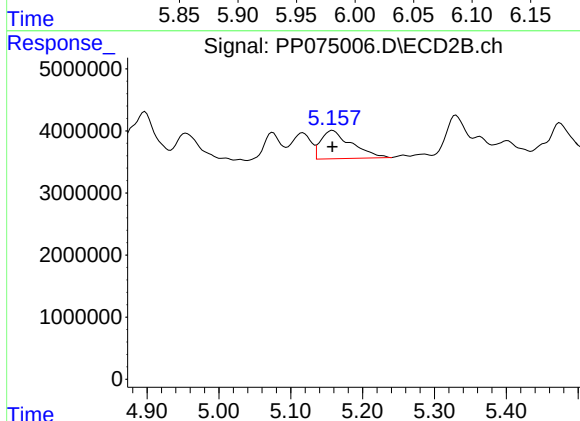


#19 AR-1242-4

R.T.: 5.158 min
Delta R.T.: 0.000 min
Response: 13577788
Conc: 79.33 ng/ml

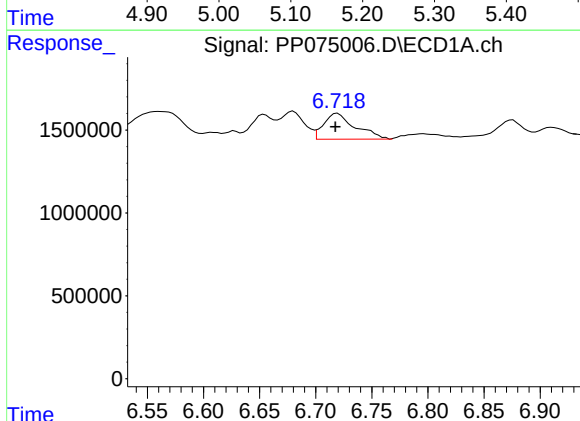


#20 AR-1242-5

R.T.: 6.719 min
Delta R.T.: 0.002 min
Response: 3029590
Conc: 83.99 ng/ml

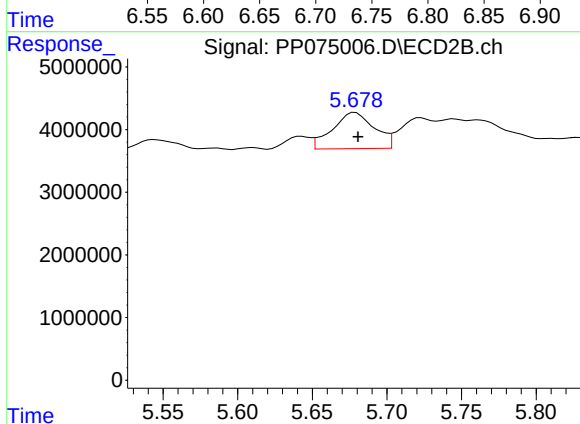

#20 AR-1242-5


R.T.: 5.679 min
Delta R.T.: -0.002 min
Response: 11264242
Conc: 60.83 ng/ml

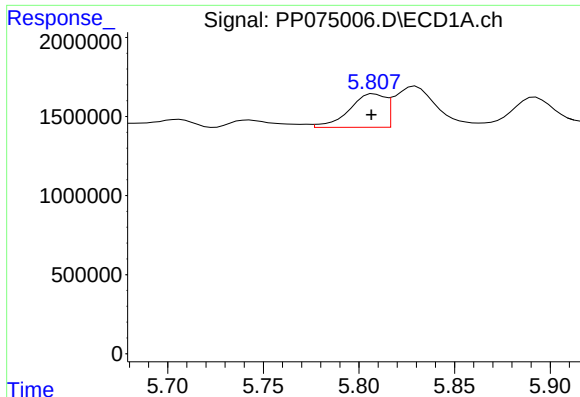

#21 AR-1248-1


R.T.: 5.808 min
Delta R.T.: 0.002 min
Response: 2771336
Conc: 91.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

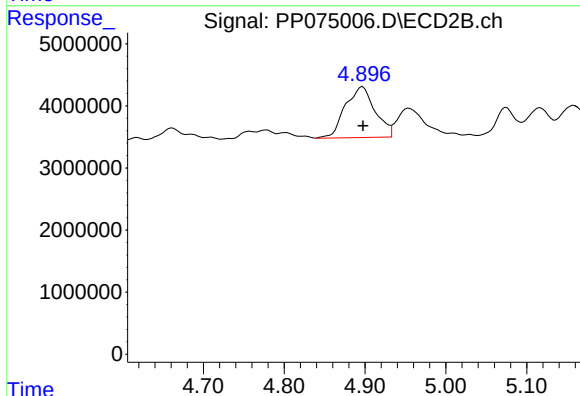


#21 AR-1248-1

R.T.: 4.897 min
Delta R.T.: 0.000 min
Response: 20906962
Conc: 75.71 ng/ml

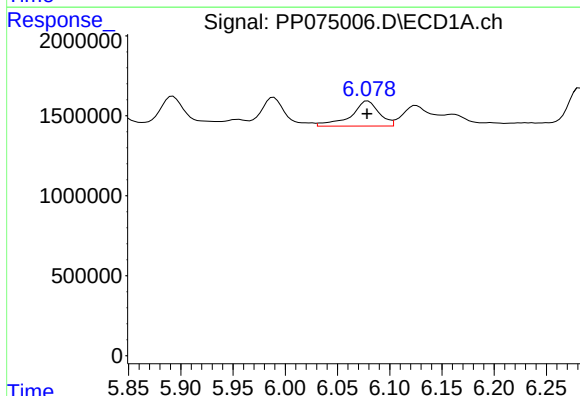


#22 AR-1248-2

R.T.: 6.079 min
Delta R.T.: 0.000 min
Response: 2968057
Conc: 68.87 ng/ml

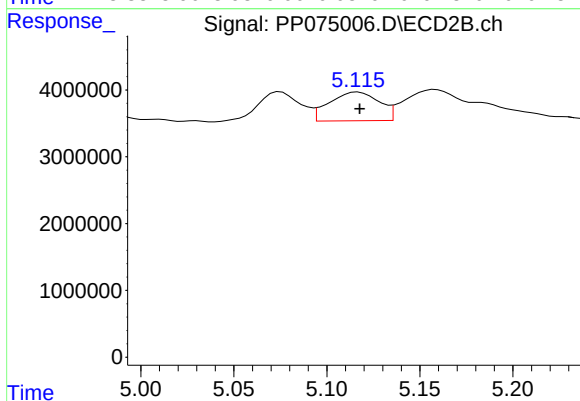

#22 AR-1248-2


R.T.: 5.117 min
Delta R.T.: 0.000 min
Response: 8004472
Conc: 45.29 ng/ml

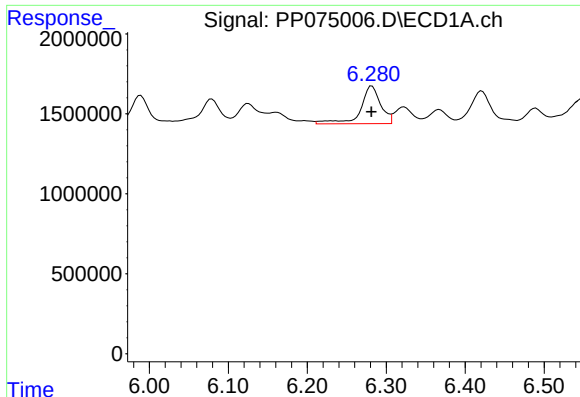

#23 AR-1248-3


R.T.: 6.282 min
Delta R.T.: 0.000 min
Response: 4138867
Conc: 88.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

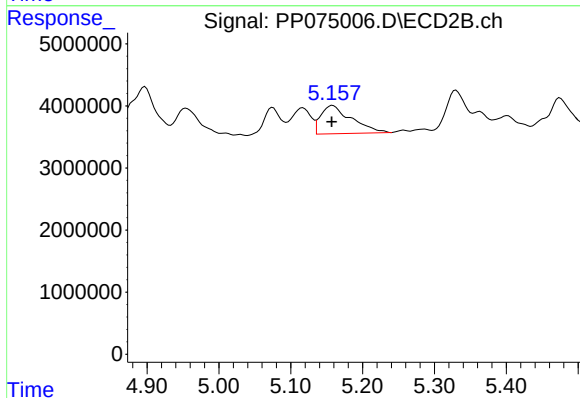


#23 AR-1248-3

R.T.: 5.158 min
Delta R.T.: 0.001 min
Response: 13577788
Conc: 59.76 ng/ml

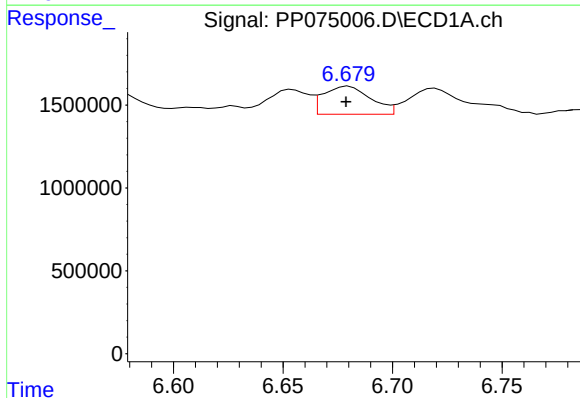


#24 AR-1248-4

R.T.: 6.680 min
Delta R.T.: 0.001 min
Response: 2548407
Conc: 46.33 ng/ml

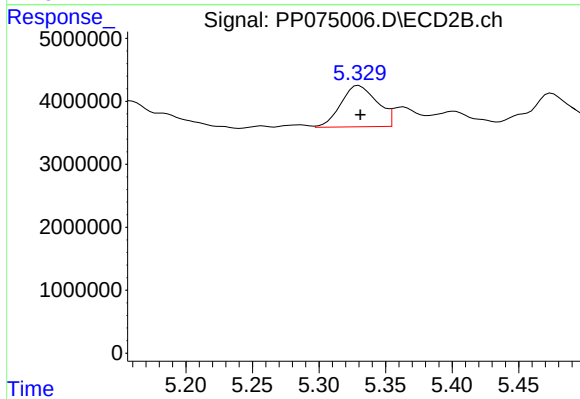

#24 AR-1248-4


R.T.: 5.330 min
Delta R.T.: 0.000 min
Response: 12383729
Conc: 56.80 ng/ml

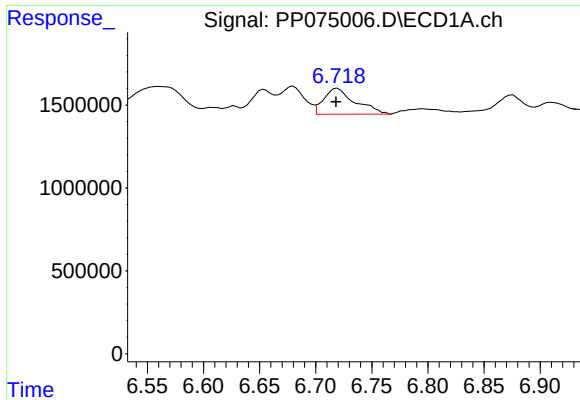

#25 AR-1248-5


R.T.: 6.719 min
Delta R.T.: 0.001 min
Response: 3029590
Conc: 54.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

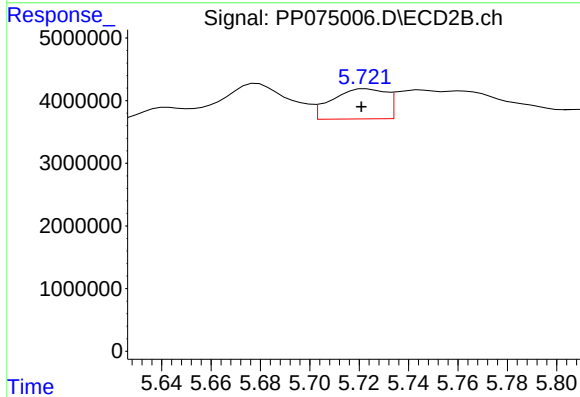


#25 AR-1248-5

R.T.: 5.723 min
Delta R.T.: 0.002 min
Response: 7281139
Conc: 19.82 ng/ml

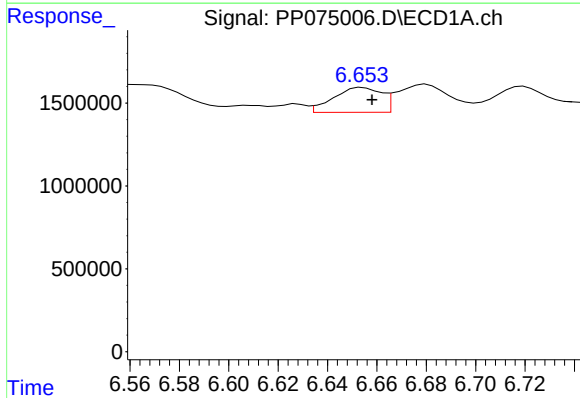


#26 AR-1254-1

R.T.: 6.654 min
Delta R.T.: -0.004 min
Response: 2015482
Conc: 34.59 ng/ml

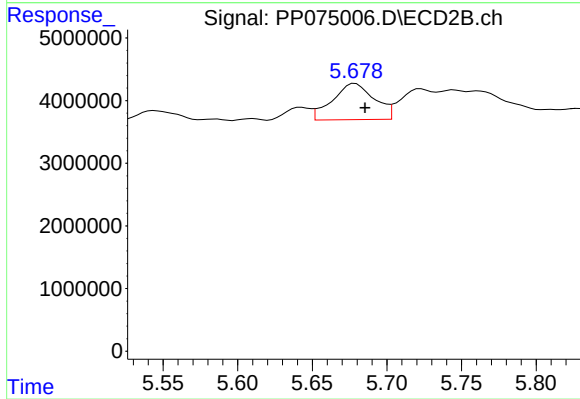

#26 AR-1254-1


R.T.: 5.679 min
Delta R.T.: -0.006 min
Response: 11264242
Conc: 23.63 ng/ml

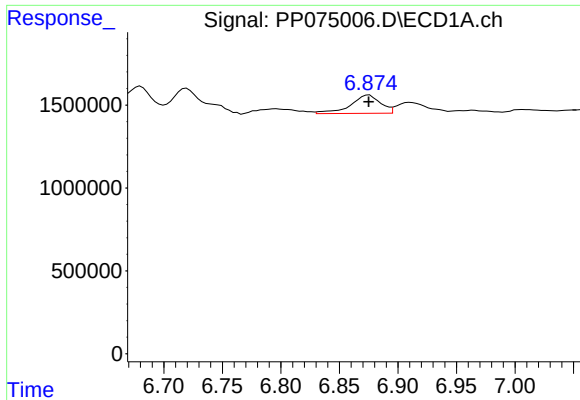

#27 AR-1254-2


R.T.: 6.875 min
Delta R.T.: 0.000 min
Response: 1947140
Conc: 23.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

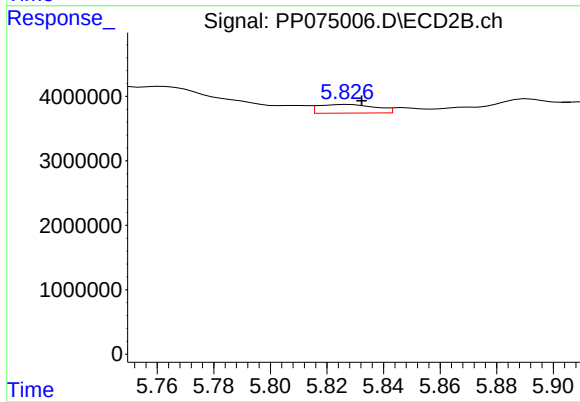


#27 AR-1254-2

R.T.: 5.828 min
Delta R.T.: -0.005 min
Response: 1906548
Conc: 5.41 ng/ml

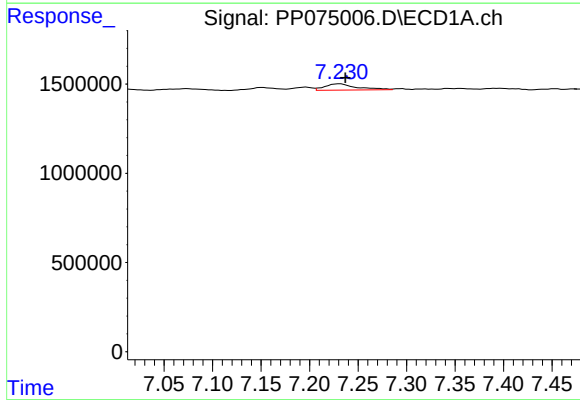


#28 AR-1254-3

R.T.: 7.231 min
Delta R.T.: -0.005 min
Response: 786018
Conc: 8.81 ng/ml

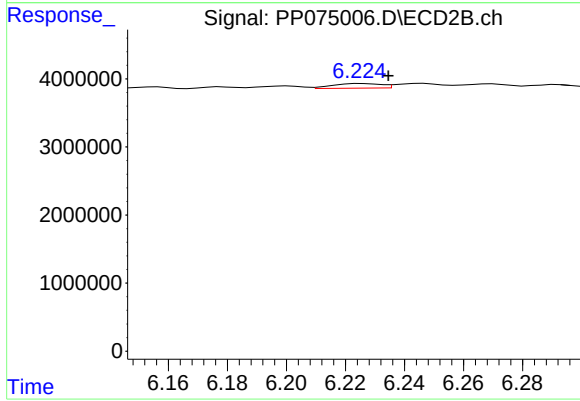

#28 AR-1254-3


R.T.: 6.225 min
Delta R.T.: -0.009 min
Response: 774121
Conc: 1.25 ng/ml

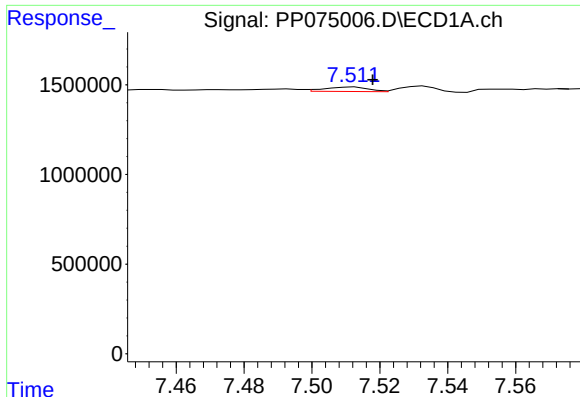

#29 AR-1254-4


R.T.: 7.513 min
Delta R.T.: -0.005 min
Response: 218964
Conc: 3.32 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

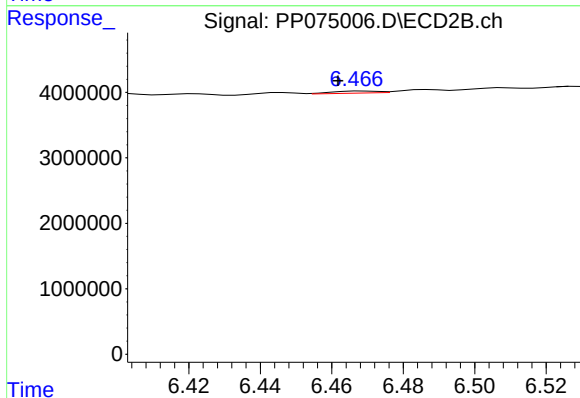


#29 AR-1254-4

R.T.: 6.469 min
Delta R.T.: 0.007 min
Response: 274271
Conc: 0.59 ng/ml

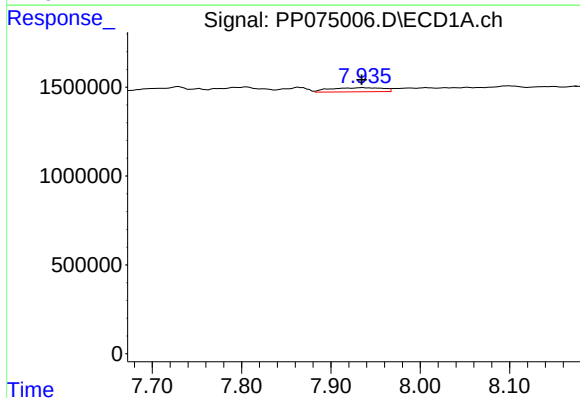


#30 AR-1254-5

R.T.: 7.936 min
Delta R.T.: 0.001 min
Response: 946126
Conc: 11.39 ng/ml

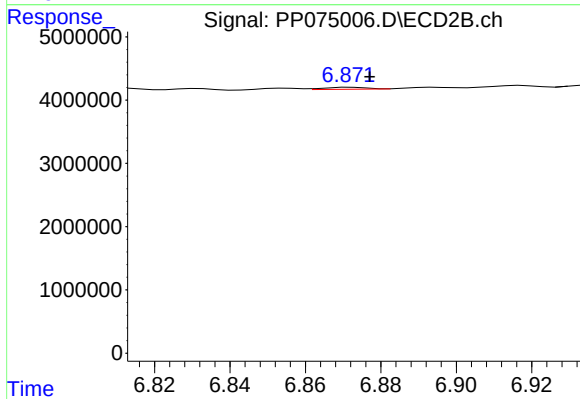

#30 AR-1254-5


R.T.: 6.872 min
Delta R.T.: -0.005 min
Response: 252753
Conc: 0.52 ng/ml

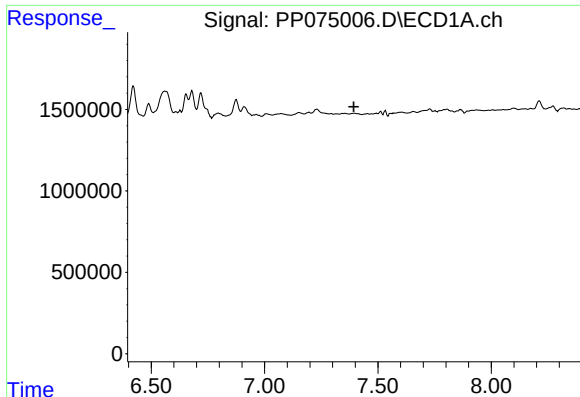

#31 AR-1260-1


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

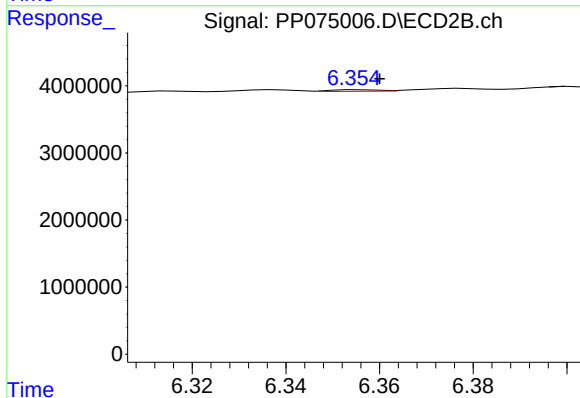


#31 AR-1260-1

R.T.: 6.355 min
Delta R.T.: -0.005 min
Response: 168159
Conc: 0.45 ng/ml

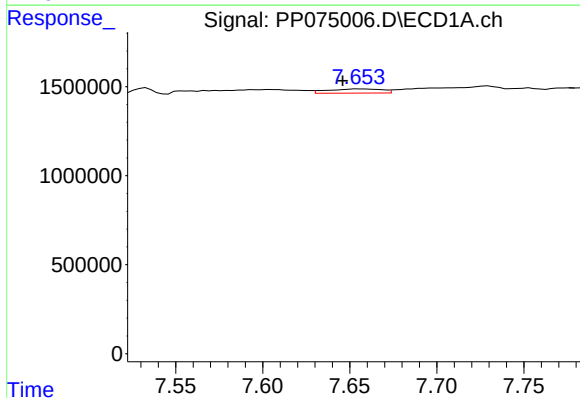


#32 AR-1260-2

R.T.: 7.656 min
Delta R.T.: 0.010 min
Response: 509122
Conc: 7.39 ng/ml

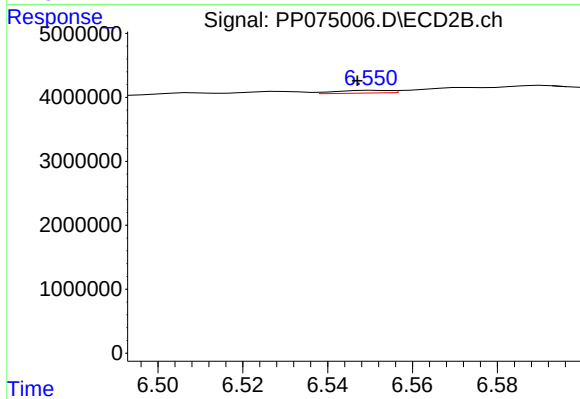

#32 AR-1260-2


R.T.: 6.551 min
Delta R.T.: 0.004 min
Response: 368750
Conc: 0.70 ng/ml

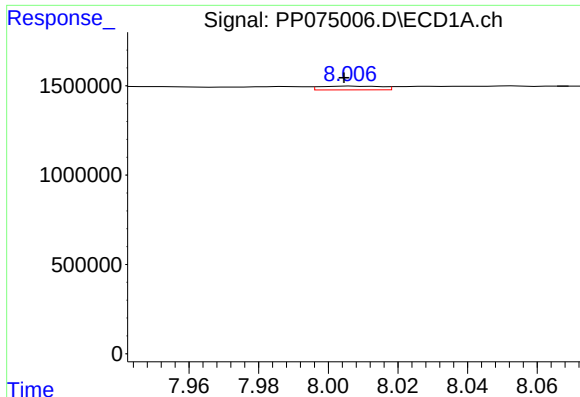

#33 AR-1260-3


R.T.: 8.007 min
Delta R.T.: 0.002 min
Response: 249316
Conc: 4.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

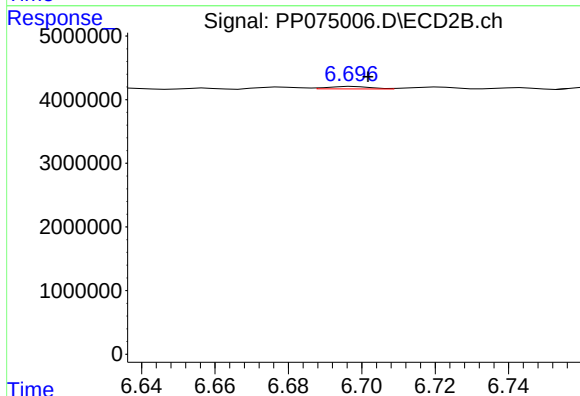


#33 AR-1260-3

R.T.: 6.698 min
Delta R.T.: -0.004 min
Response: 306595
Conc: 0.71 ng/ml

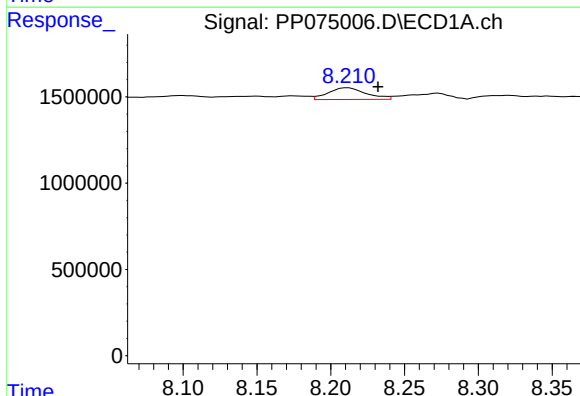


#34 AR-1260-4

R.T.: 8.212 min
Delta R.T.: -0.021 min
Response: 1215643
Conc: 19.06 ng/ml

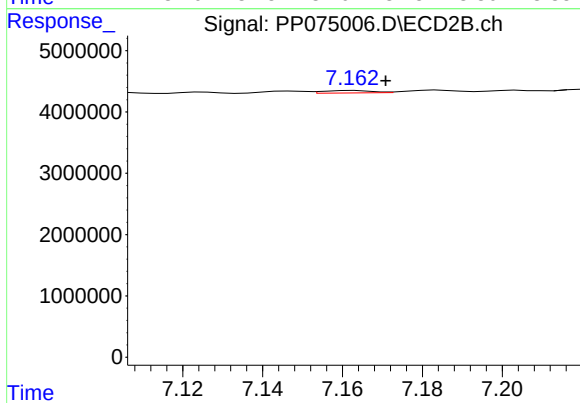

#34 AR-1260-4


R.T.: 7.163 min
Delta R.T.: -0.008 min
Response: 333086
Conc: 0.87 ng/ml

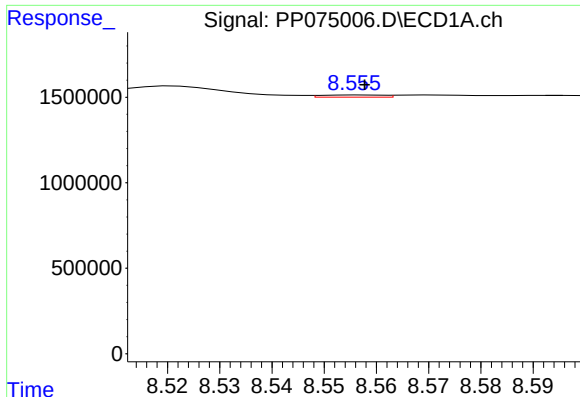

#35 AR-1260-5


R.T.: 8.557 min
Delta R.T.: -0.001 min
Response: 107222
Conc: 0.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

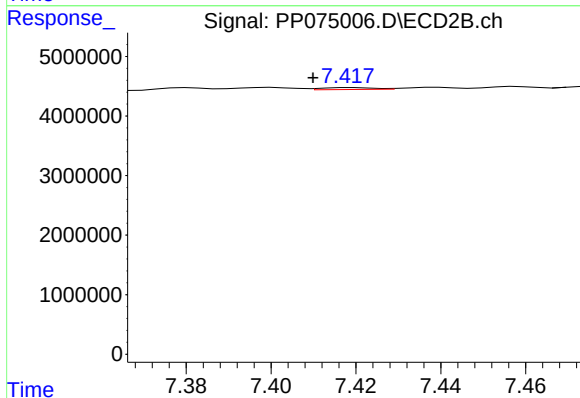


#35 AR-1260-5

R.T.: 7.419 min
Delta R.T.: 0.009 min
Response: 275278
Conc: 0.27 ng/ml

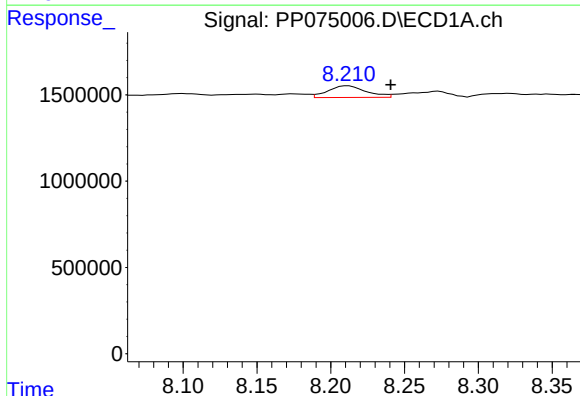


#36 AR-1262-1

R.T.: 8.212 min
Delta R.T.: -0.029 min
Response: 1215643
Conc: 15.78 ng/ml

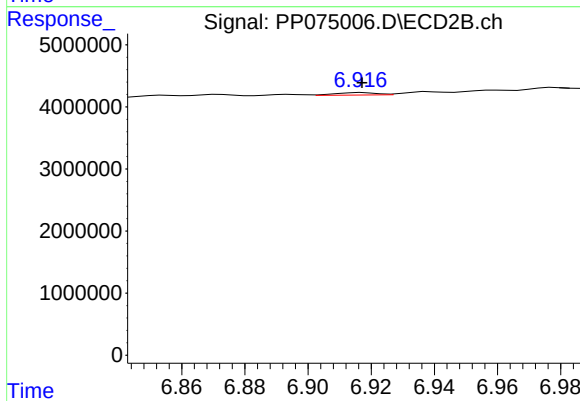

#36 AR-1262-1


R.T.: 6.917 min
Delta R.T.: 0.000 min
Response: 358398
Conc: 0.51 ng/ml

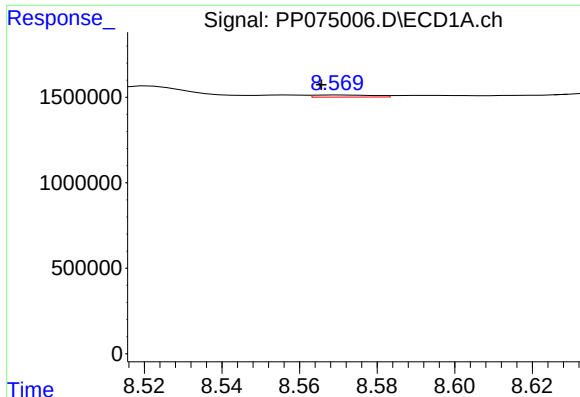

#37 AR-1262-2


R.T.: 8.571 min
Delta R.T.: 0.005 min
Response: 132173
Conc: 1.00 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

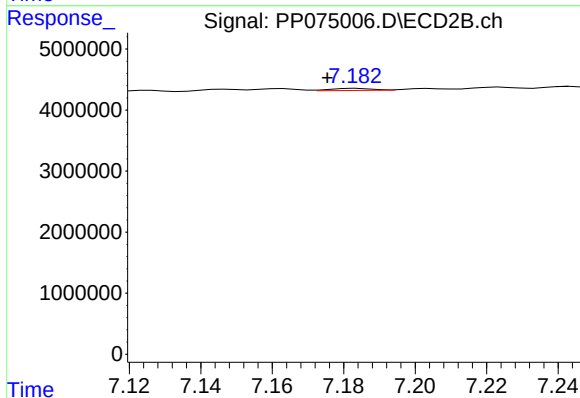


#37 AR-1262-2

R.T.: 7.184 min
Delta R.T.: 0.008 min
Response: 278030
Conc: 0.53 ng/ml

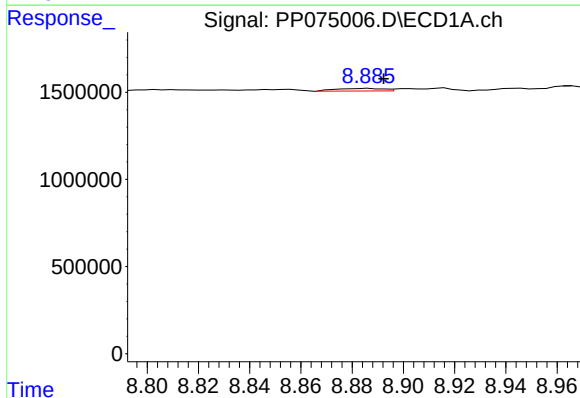


#38 AR-1262-3

R.T.: 8.886 min
Delta R.T.: -0.006 min
Response: 193931
Conc: 1.99 ng/ml

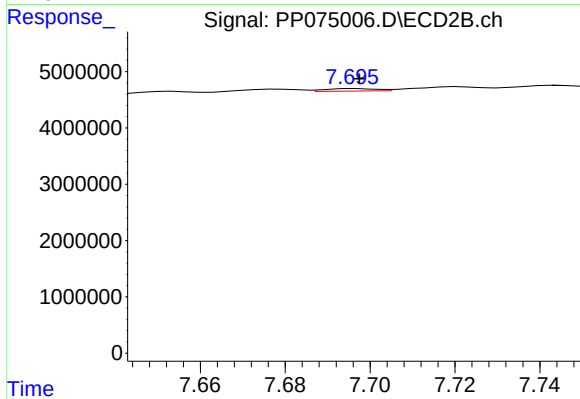

#38 AR-1262-3


R.T.: 7.697 min
Delta R.T.: 0.000 min
Response: 377151
Conc: 0.81 ng/ml

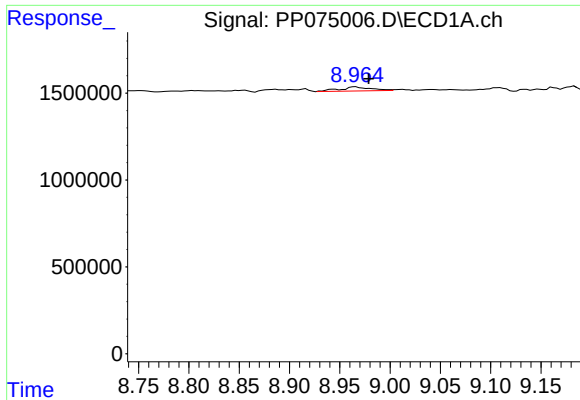

#39 AR-1262-4


R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 513447
Conc: 6.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

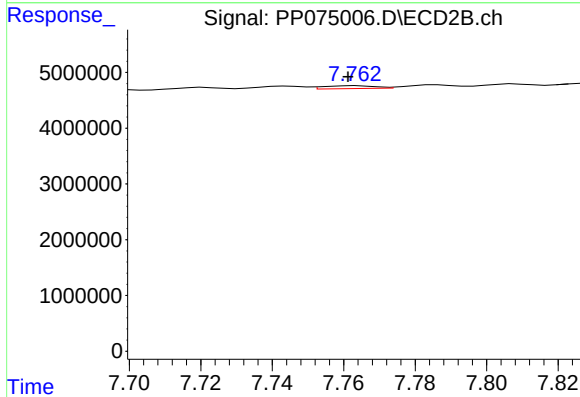


#39 AR-1262-4

R.T.: 7.763 min
Delta R.T.: 0.002 min
Response: 507226
Conc: 0.62 ng/ml

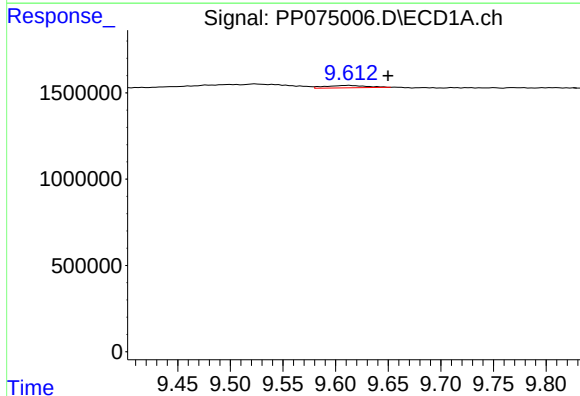


#40 AR-1262-5

R.T.: 9.613 min
Delta R.T.: -0.037 min
Response: 370012
Conc: 6.07 ng/ml

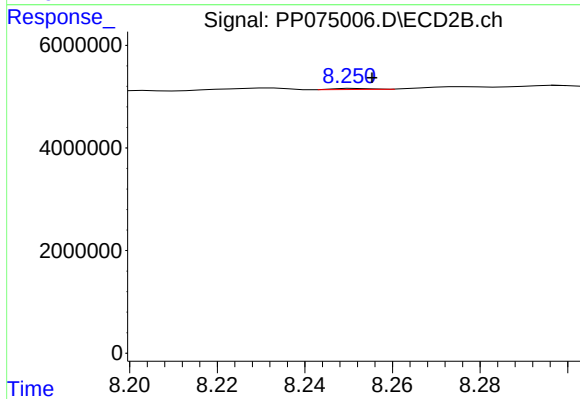

#40 AR-1262-5


R.T.: 8.252 min
Delta R.T.: -0.004 min
Response: 111362
Conc: 0.31 ng/ml

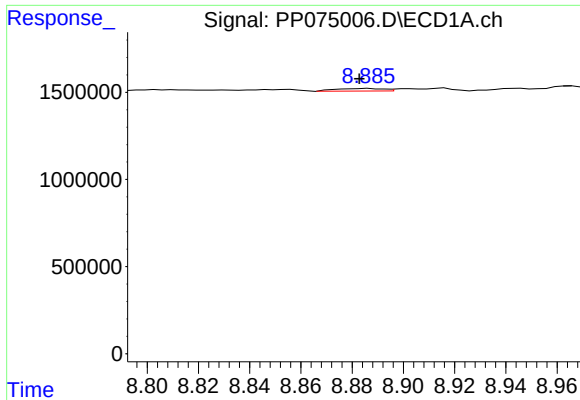

#41 AR-1268-1


R.T.: 8.886 min
Delta R.T.: 0.003 min
Response: 193931
Conc: 1.20 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

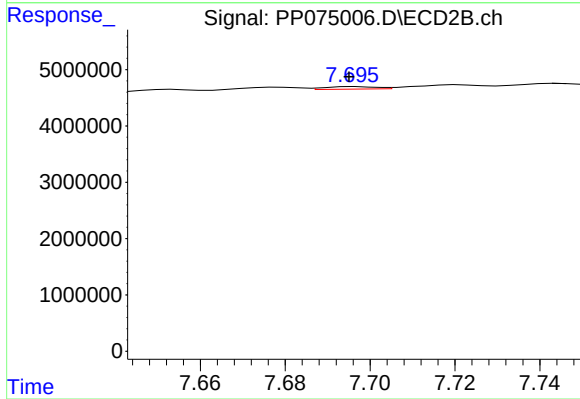


#41 AR-1268-1

R.T.: 7.697 min
Delta R.T.: 0.002 min
Response: 377151
Conc: 0.27 ng/ml

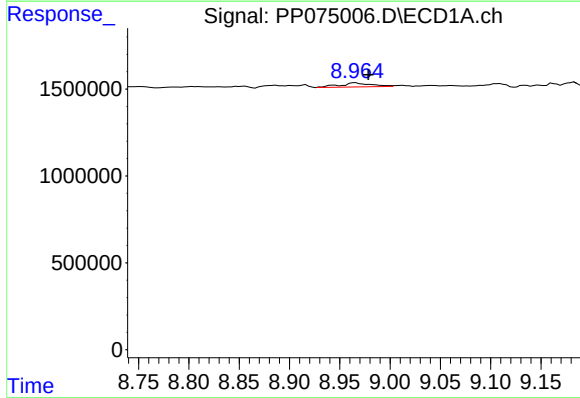


#42 AR-1268-2

R.T.: 8.966 min
Delta R.T.: -0.013 min
Response: 513447
Conc: 3.50 ng/ml

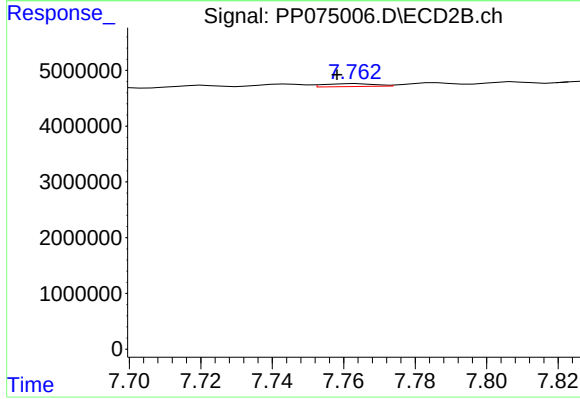

#42 AR-1268-2


R.T.: 7.763 min
Delta R.T.: 0.005 min
Response: 507226
Conc: 0.37 ng/ml

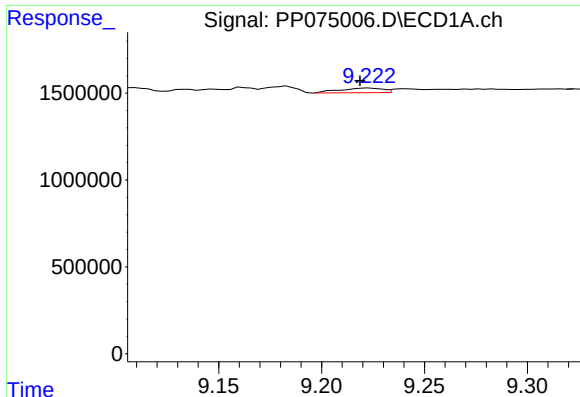

#43 AR-1268-3


R.T.: 9.223 min
Delta R.T.: 0.004 min
Response: 385850
Conc: 3.12 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

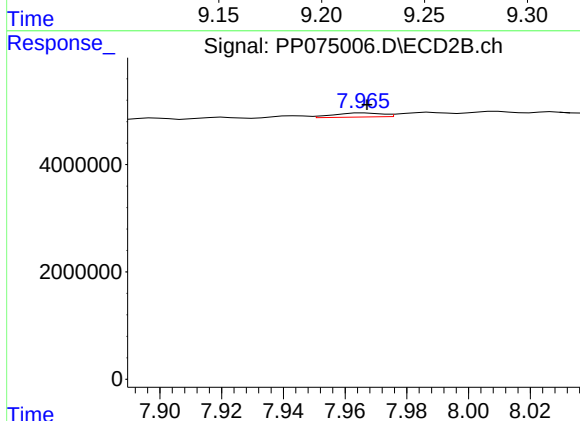


#43 AR-1268-3

R.T.: 7.966 min
Delta R.T.: 0.000 min
Response: 821963
Conc: 0.79 ng/ml

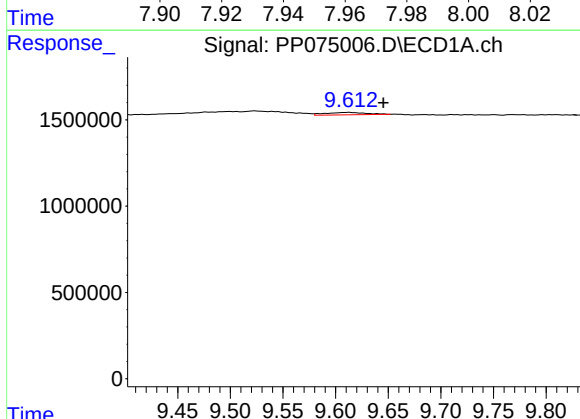


#44 AR-1268-4

R.T.: 9.613 min
Delta R.T.: -0.032 min
Response: 370012
Conc: 5.50 ng/ml

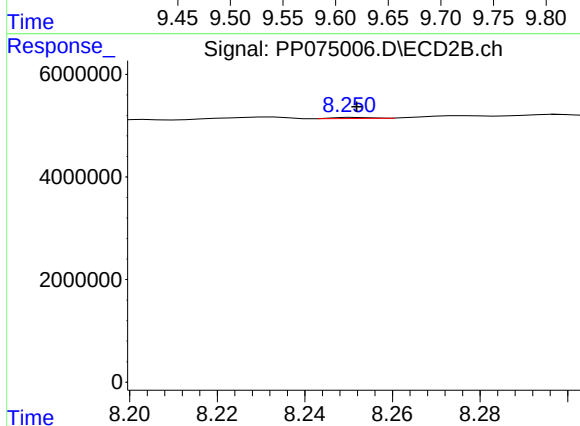

#44 AR-1268-4


R.T.: 8.252 min
Delta R.T.: 0.000 min
Response: 111362
Conc: 0.29 ng/ml

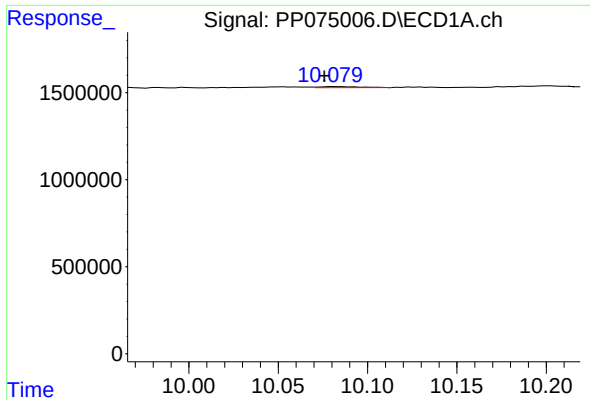

#45 AR-1268-5

R.T.: 10.081 min
Delta R.T.: 0.005 min
Response: 95984
Conc: 0.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-E

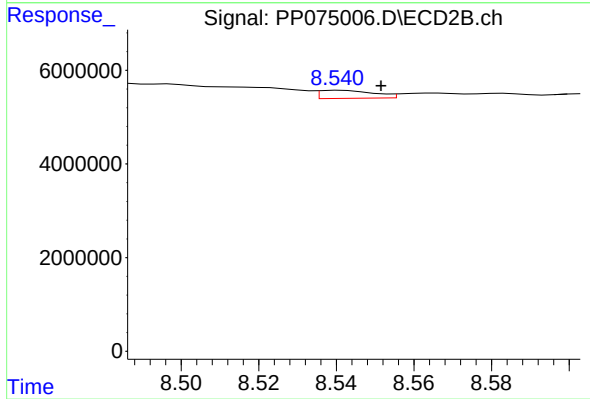

#45 AR-1268-5

R.T.: 8.541 min
Delta R.T.: -0.010 min
Response: 1679634
Conc: 0.54 ng/ml