

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075007.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 14:57
 Operator : YP\AJ
 Sample : Q3034-06
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-F

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:50:00 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	3.797	28272862	106.5E6	23.105	22.016
2)	SA Decachlor...	10.426	8.803	23081763	141.0E6	23.374	18.799
Target Compounds							
3)	L1 AR-1016-1	5.805	4.894	8359918	79888374	189.615	156.843
4)	L1 AR-1016-2	5.827	4.953	12025104	41261894	191.356	173.358
5)	L1 AR-1016-3	5.890	5.072	8946301	26724074	199.188	193.788
6)	L1 AR-1016-4	5.987	5.113	8216304	29789417	233.538	213.081
7)	L1 AR-1016-5	6.279	5.327	10768811	43613684	324.498	262.601
8)	L2 AR-1221-1	4.853	4.010	555269	345065	31.562	5.577 #
9)	L2 AR-1221-2	4.956	4.099	647517	1875375	48.477	41.480
10)	L2 AR-1221-3	5.016	4.167	646039	2588619	17.040	15.756
11)	L3 AR-1232-1	5.016	4.167	646039	2588619	21.270	20.209
12)	L3 AR-1232-2	5.541	4.894	4326033	79888374	274.525	344.653 #
13)	L3 AR-1232-3	5.827	5.072	12025104	26724074	393.702	444.958
14)	L3 AR-1232-4	5.987	5.155	8216304	47030671	475.776	638.073 #
15)	L3 AR-1232-5	6.076	5.327	7607617	43613684	586.060	702.497
16)	L4 AR-1242-1	5.805	4.894	8359918	79888374	218.416	189.420
17)	L4 AR-1242-2	5.827	4.953	12025104	41261894	212.902	206.018
18)	L4 AR-1242-3	5.890	5.072	8946301	26724074	220.336	225.904
19)	L4 AR-1242-4	5.987	5.155	8216304	47030671	258.848	274.777
20)	L4 AR-1242-5	6.716	5.675	5404627	30272752	149.835	163.491
21)	L5 AR-1248-1	5.805	4.894	8359918	79888374	276.598	289.301
22)	L5 AR-1248-2	6.076	5.113	7607617	29789417	176.527	168.535
23)	L5 AR-1248-3	6.279	5.155	10768811	47030671	230.578	206.998
24)	L5 AR-1248-4	6.676	5.327	5443235	43613684	98.966	200.043 #
25)	L5 AR-1248-5	6.716	5.717	5404627	22629311	97.433	61.606 #
26)	L6 AR-1254-1	6.651	5.675	4741089	30272752	81.365	63.503
27)	L6 AR-1254-2	6.872	5.824	3800593	5424298	46.567	15.404 #
28)	L6 AR-1254-3	7.228	6.235	803152	1095422	9.003	1.767 #
29)	L6 AR-1254-4	7.511	6.467	115547	348971	1.753	0.745 #
30)	L6 AR-1254-5	7.927	6.871	320026	267272	3.852	0.545 #
31)	L7 AR-1260-1	7.392	6.365	125768	306452	2.176	0.817 #
32)	L7 AR-1260-2	7.654	6.546	134093	490054	1.946	0.927 #
33)	L7 AR-1260-3	8.011	6.692	226507	500719	4.366	1.156 #
34)	L7 AR-1260-4	8.245	7.172	188773	202780	2.959	0.532 #
35)	L7 AR-1260-5	8.550	7.414	235150	566050	2.073	0.564 #
36)	L8 AR-1262-1	8.245	6.909	188773	322982	2.451	0.457 #
37)	L8 AR-1262-2	8.550	7.172	235150	202780	1.776	0.389 #
38)	L8 AR-1262-3	0.000	7.692	0	790009	N.D.	1.694 #
39)	L8 AR-1262-4	8.970	7.754	176052	482758	2.337	0.587 #
40)	L8 AR-1262-5	9.606f	8.260	788231	226488	12.931	0.632 #
41)	L9 AR-1268-1	0.000	7.692	0	790009	N.D.	0.560 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 14:57
Operator : YP\AJ
Sample : Q3034-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:50:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.970	7.754	176052	482758	1.200	0.354 #
43)	L9 AR-1268-3	9.282f	7.959	44200	392411	0.358	0.376
44)	L9 AR-1268-4	9.606f	8.260	788231	226488	11.719	0.591 #
45)	L9 AR-1268-5	10.076	8.568	411652	667903	1.112	0.213 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075007.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 14:57
Operator : YP\AJ
Sample : Q3034-06
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:50:00 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

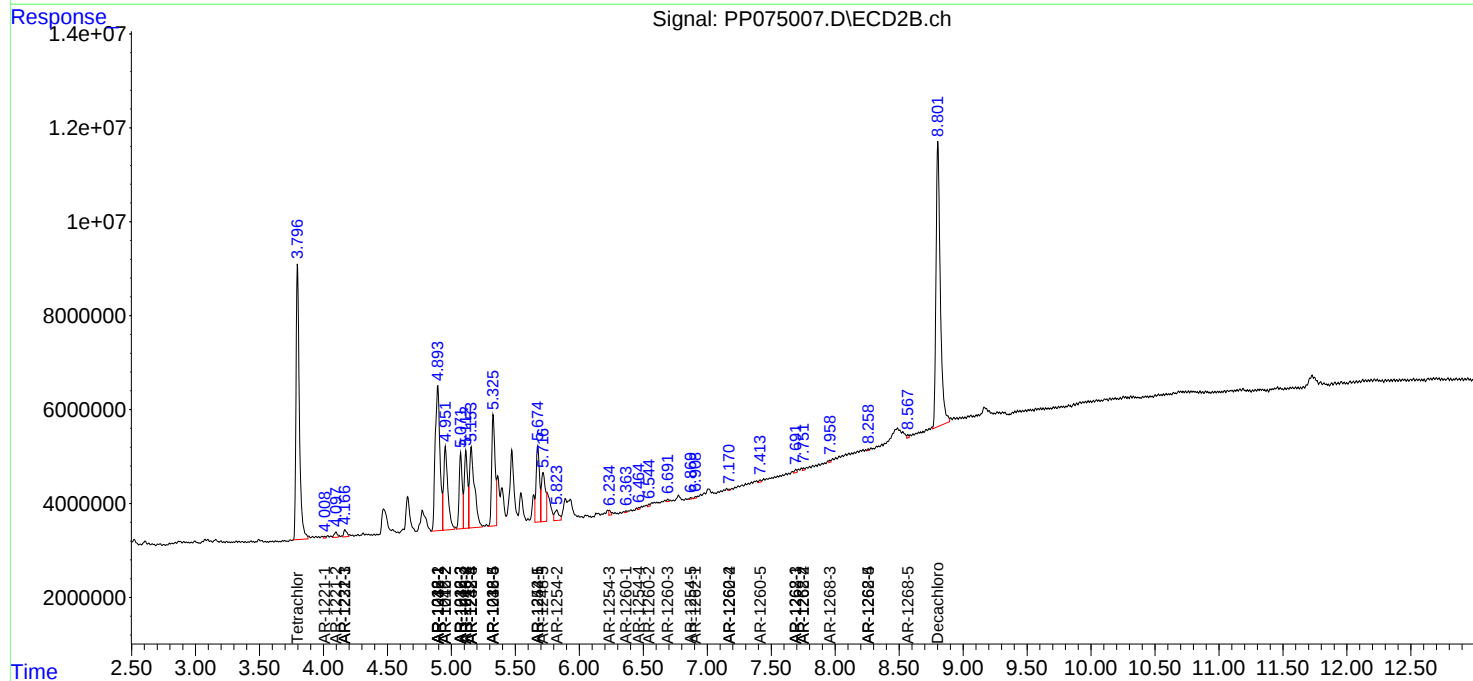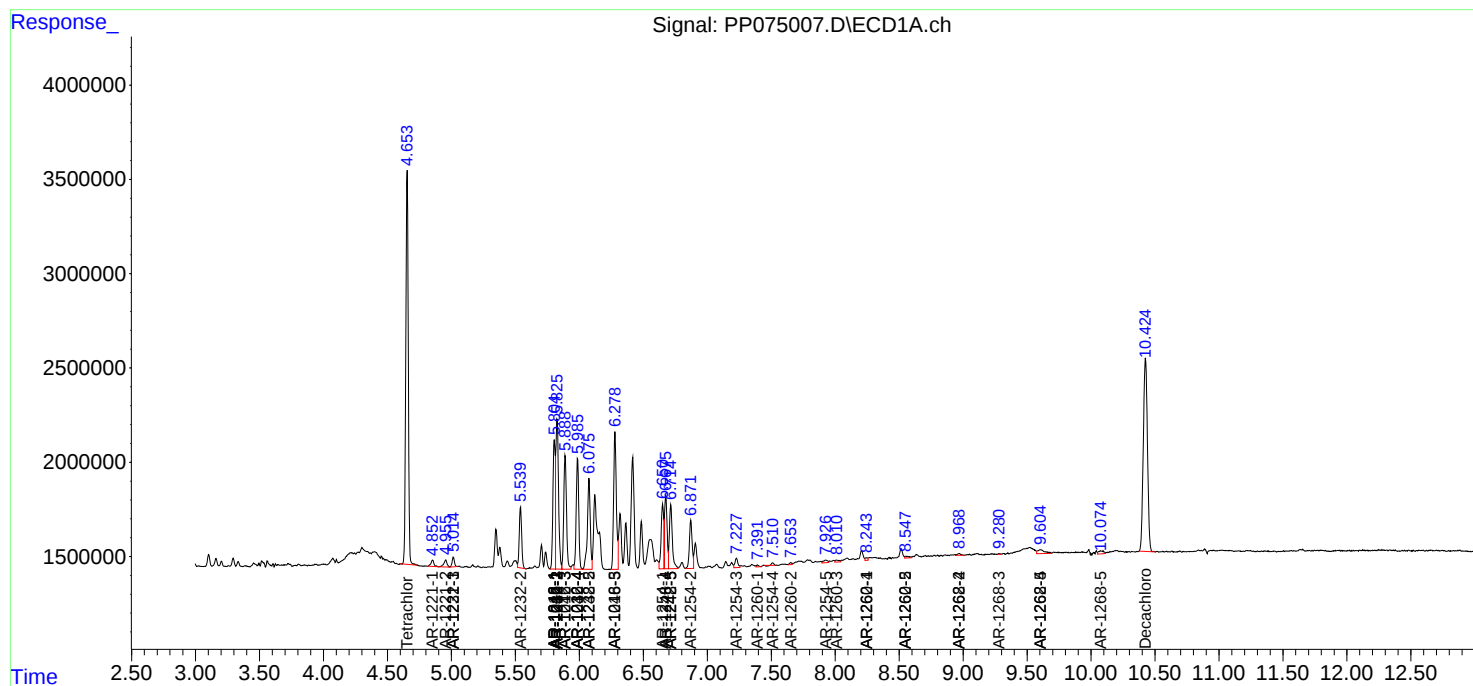


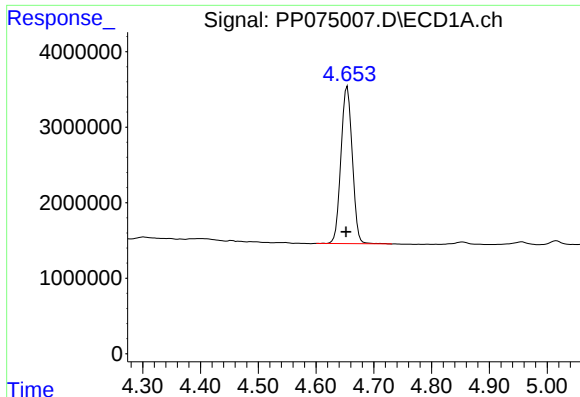

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.002 min
Response: 28272862
Conc: 23.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

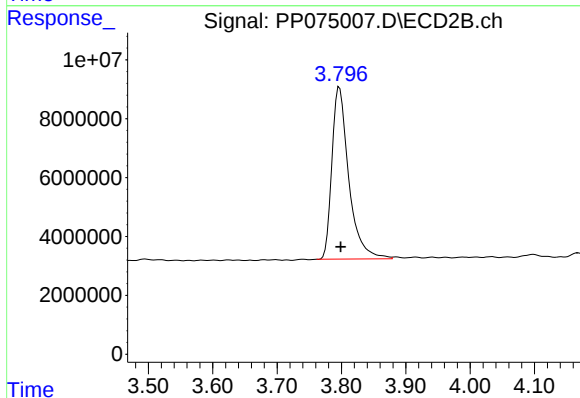


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: -0.002 min
Response: 106454627
Conc: 22.02 ng/ml

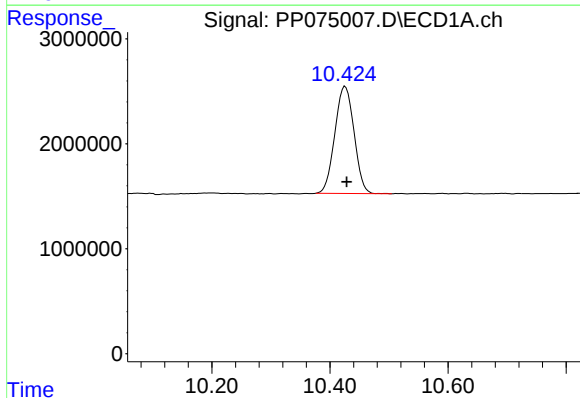


#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.002 min
Response: 23081763
Conc: 23.37 ng/ml

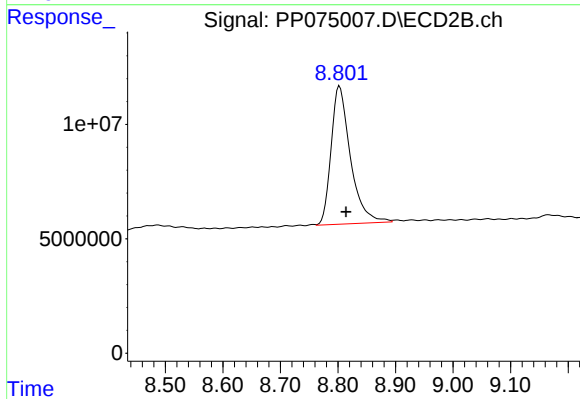

#2 Decachlorobiphenyl


R.T.: 8.803 min
Delta R.T.: -0.011 min
Response: 140976077
Conc: 18.80 ng/ml

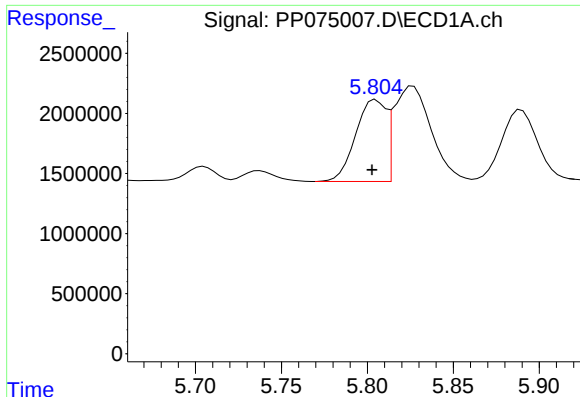

#3 AR-1016-1


R.T.: 5.805 min
Delta R.T.: 0.002 min
Response: 8359918
Conc: 189.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

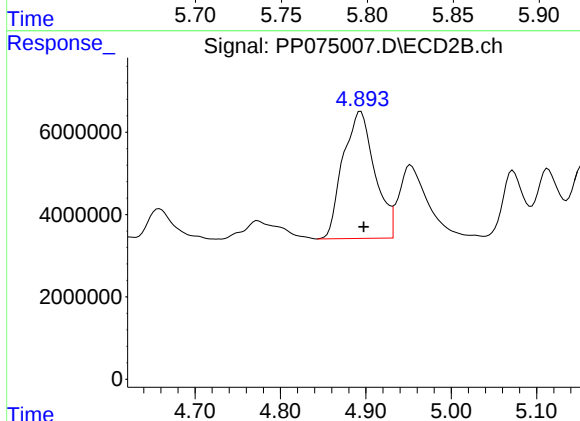


#3 AR-1016-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 79888374
Conc: 156.84 ng/ml

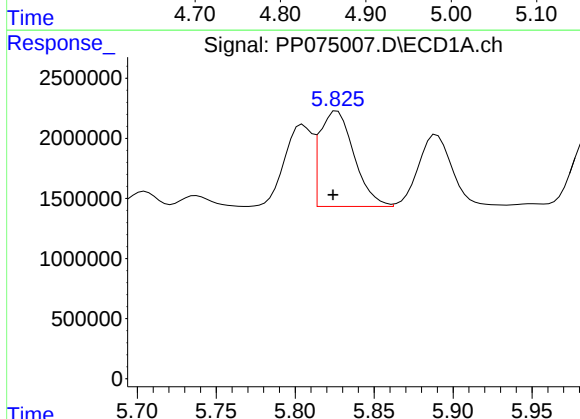


#4 AR-1016-2

R.T.: 5.827 min
Delta R.T.: 0.003 min
Response: 12025104
Conc: 191.36 ng/ml

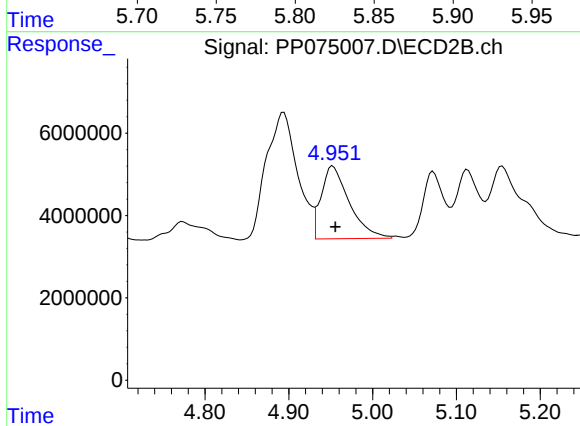

#4 AR-1016-2


R.T.: 4.953 min
Delta R.T.: -0.003 min
Response: 41261894
Conc: 173.36 ng/ml

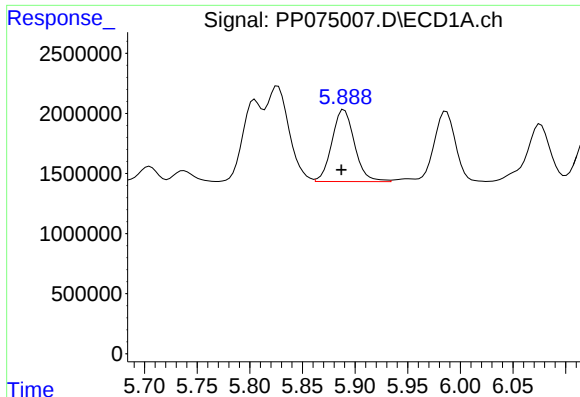

#5 AR-1016-3


R.T.: 5.890 min
Delta R.T.: 0.003 min
Response: 8946301
Conc: 199.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

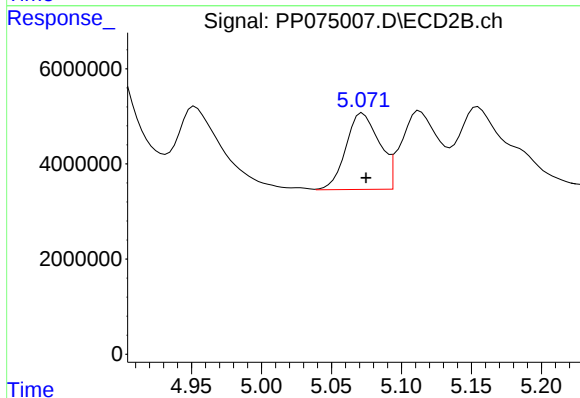


#5 AR-1016-3

R.T.: 5.072 min
Delta R.T.: -0.002 min
Response: 26724074
Conc: 193.79 ng/ml

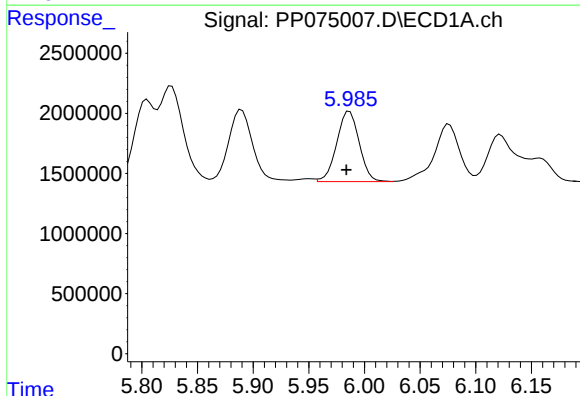


#6 AR-1016-4

R.T.: 5.987 min
Delta R.T.: 0.003 min
Response: 8216304
Conc: 233.54 ng/ml

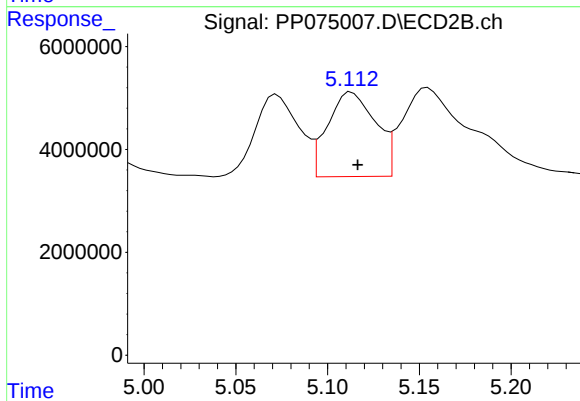

#6 AR-1016-4


R.T.: 5.113 min
Delta R.T.: -0.003 min
Response: 29789417
Conc: 213.08 ng/ml

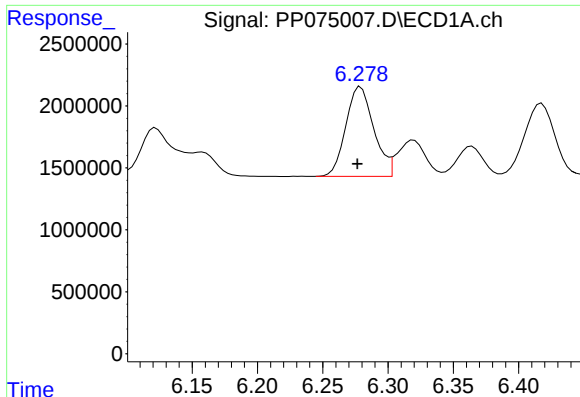

#7 AR-1016-5


R.T.: 6.279 min
Delta R.T.: 0.003 min
Response: 10768811
Conc: 324.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

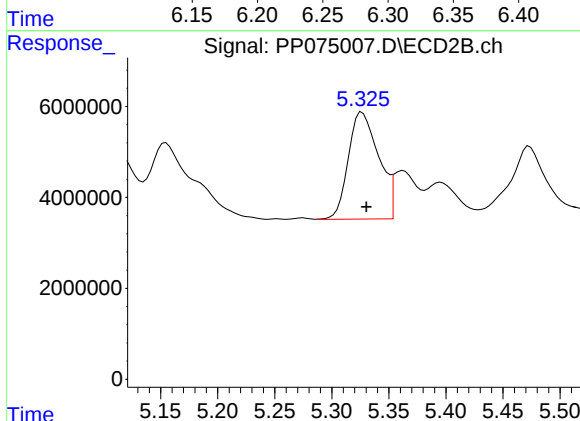


#7 AR-1016-5

R.T.: 5.327 min
Delta R.T.: -0.004 min
Response: 43613684
Conc: 262.60 ng/ml

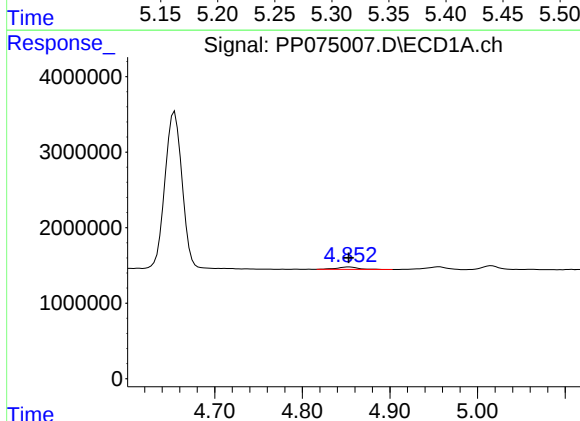


#8 AR-1221-1

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 555269
Conc: 31.56 ng/ml

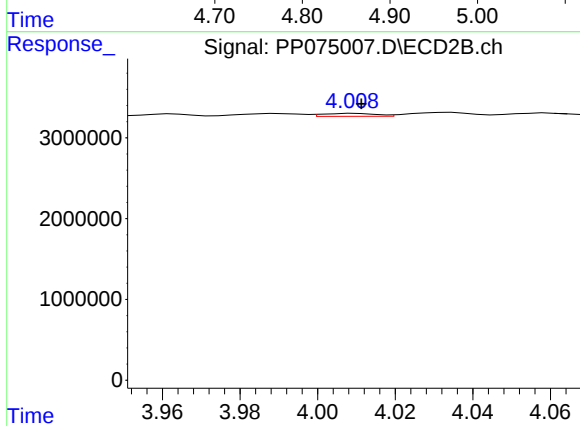

#8 AR-1221-1


R.T.: 4.010 min
Delta R.T.: -0.002 min
Response: 345065
Conc: 5.58 ng/ml

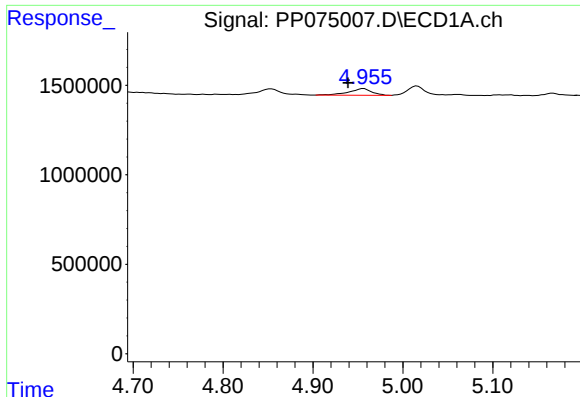

#9 AR-1221-2


R.T.: 4.956 min
Delta R.T.: 0.017 min
Response: 647517
Conc: 48.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

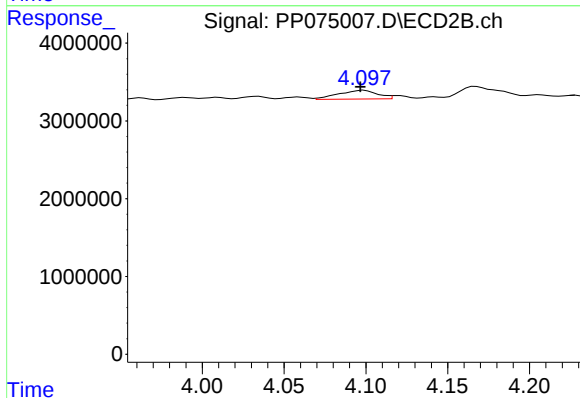


#9 AR-1221-2

R.T.: 4.099 min
Delta R.T.: 0.002 min
Response: 1875375
Conc: 41.48 ng/ml

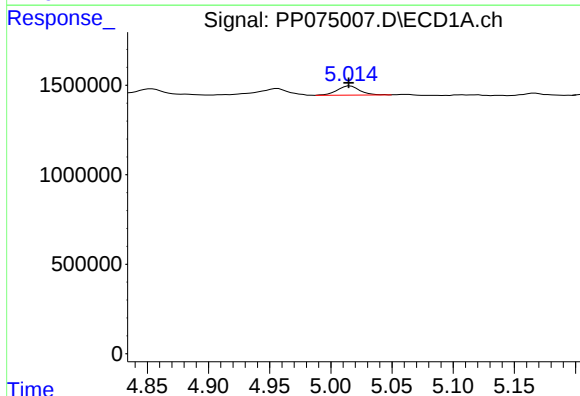


#10 AR-1221-3

R.T.: 5.016 min
Delta R.T.: 0.001 min
Response: 646039
Conc: 17.04 ng/ml

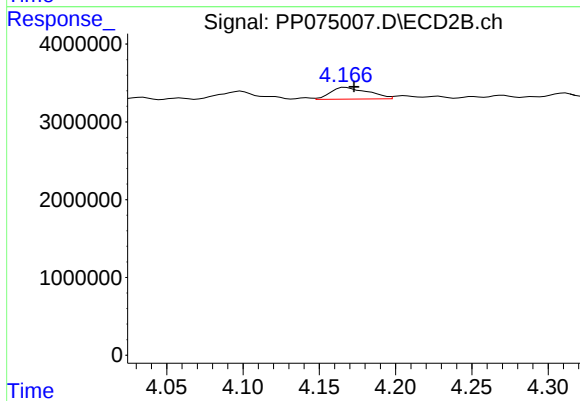

#10 AR-1221-3


R.T.: 4.167 min
Delta R.T.: -0.006 min
Response: 2588619
Conc: 15.76 ng/ml

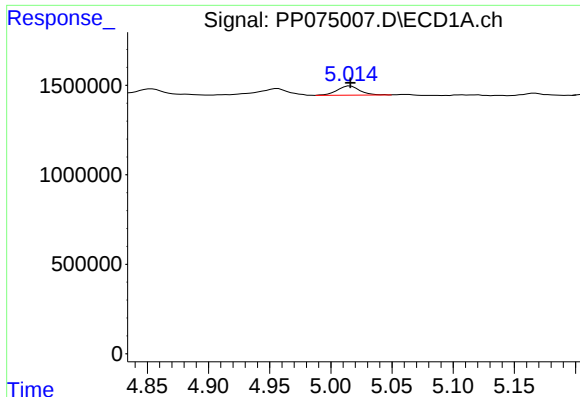

#11 AR-1232-1


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 646039
Conc: 21.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

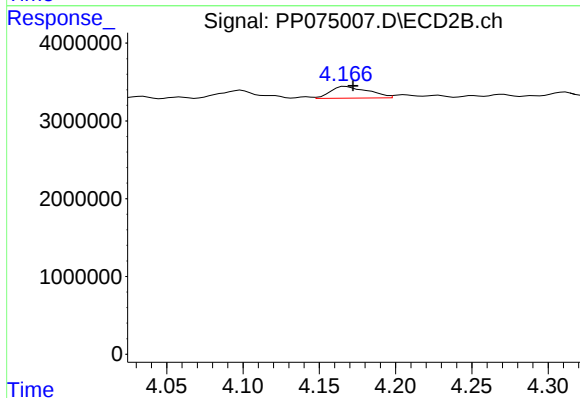


#11 AR-1232-1

R.T.: 4.167 min
Delta R.T.: -0.005 min
Response: 2588619
Conc: 20.21 ng/ml

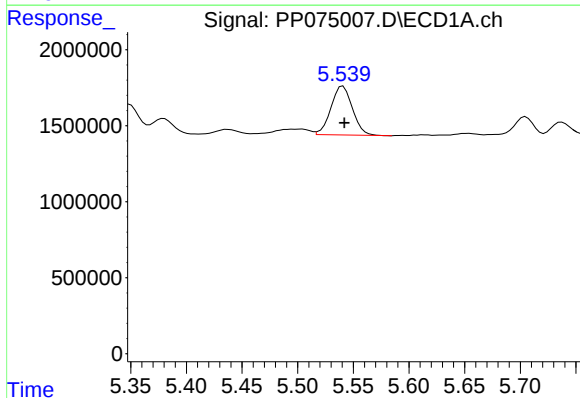


#12 AR-1232-2

R.T.: 5.541 min
Delta R.T.: -0.001 min
Response: 4326033
Conc: 274.53 ng/ml

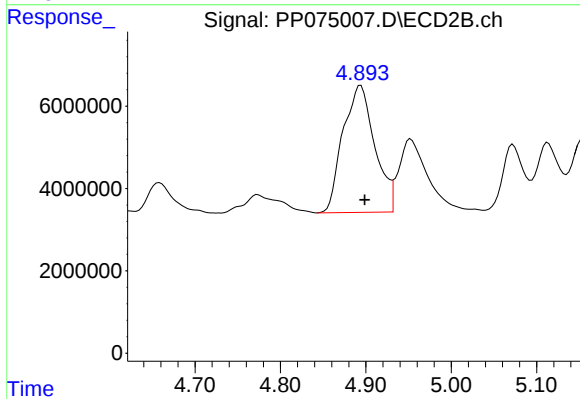

#12 AR-1232-2


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 79888374
Conc: 344.65 ng/ml

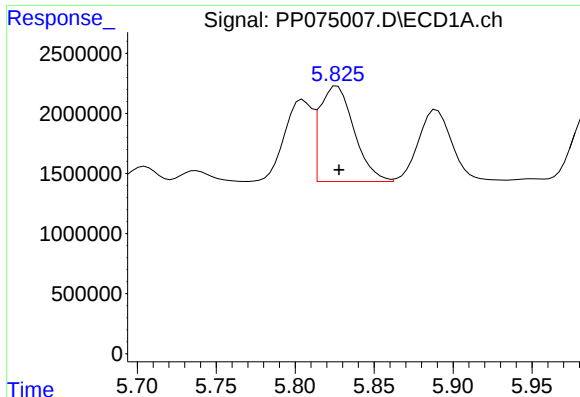

#13 AR-1232-3


R.T.: 5.827 min
Delta R.T.: -0.001 min
Response: 12025104
Conc: 393.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

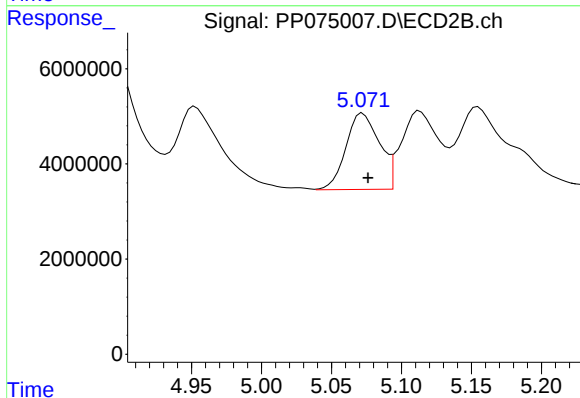


#13 AR-1232-3

R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 26724074
Conc: 444.96 ng/ml

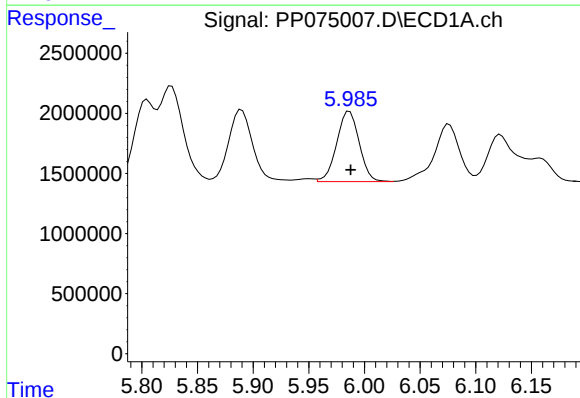


#14 AR-1232-4

R.T.: 5.987 min
Delta R.T.: -0.001 min
Response: 8216304
Conc: 475.78 ng/ml

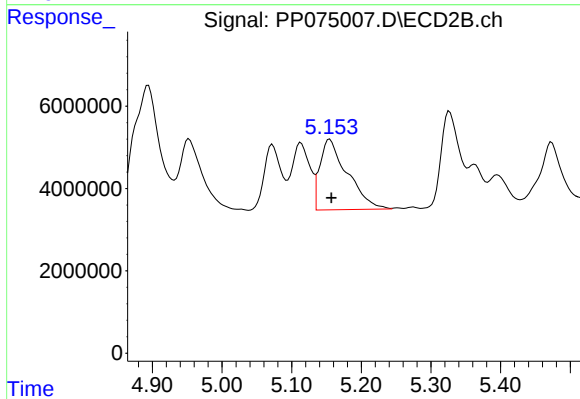

#14 AR-1232-4


R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 47030671
Conc: 638.07 ng/ml

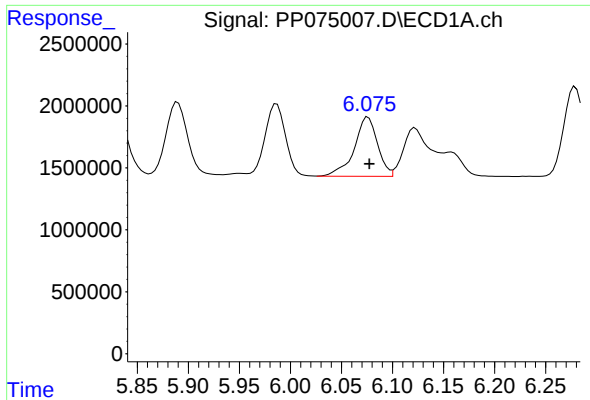

#15 AR-1232-5


R.T.: 6.076 min
Delta R.T.: -0.001 min
Response: 7607617
Conc: 586.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

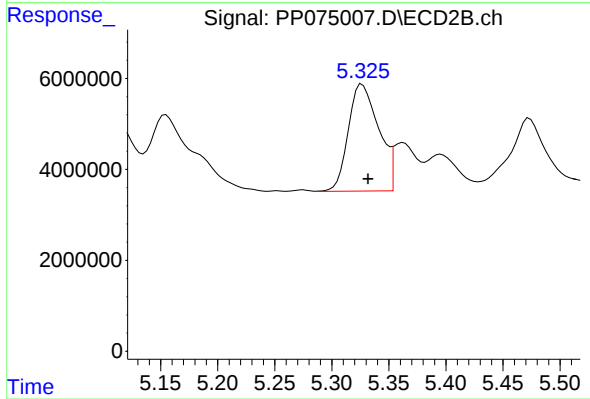


#15 AR-1232-5

R.T.: 5.327 min
Delta R.T.: -0.005 min
Response: 43613684
Conc: 702.50 ng/ml

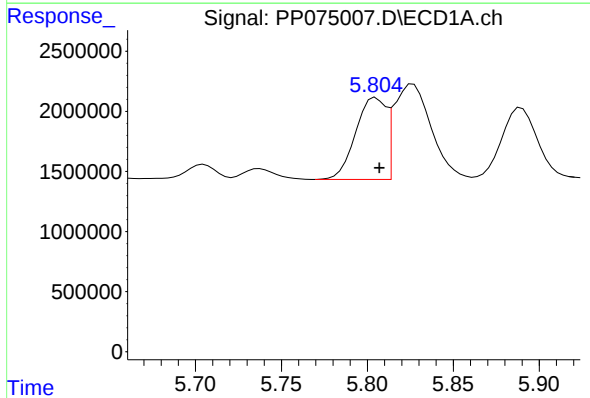


#16 AR-1242-1

R.T.: 5.805 min
Delta R.T.: -0.002 min
Response: 8359918
Conc: 218.42 ng/ml

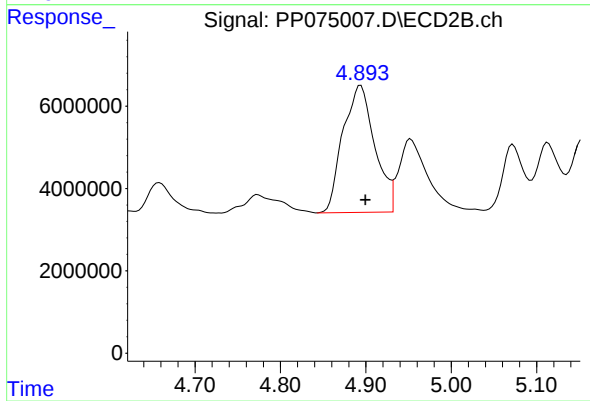

#16 AR-1242-1


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 79888374
Conc: 189.42 ng/ml

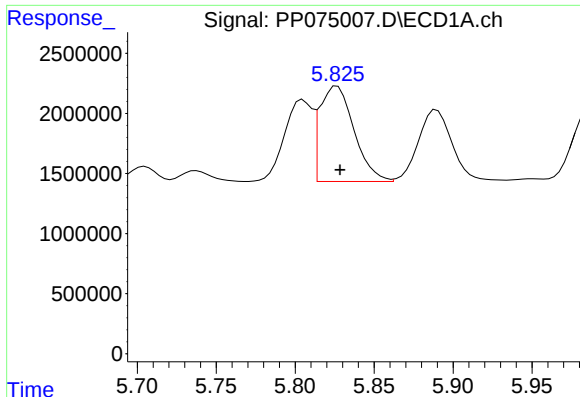

#17 AR-1242-2


R.T.: 5.827 min
Delta R.T.: -0.002 min
Response: 12025104
Conc: 212.90 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

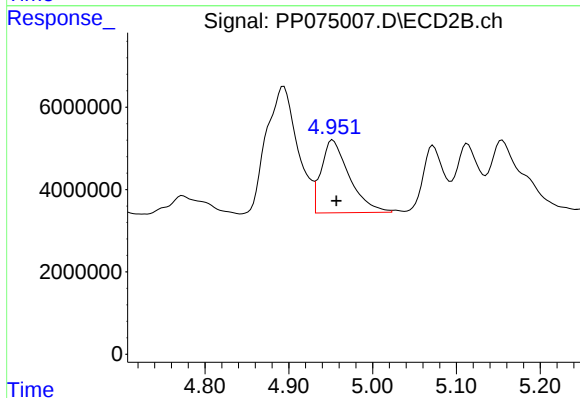


#17 AR-1242-2

R.T.: 4.953 min
Delta R.T.: -0.004 min
Response: 41261894
Conc: 206.02 ng/ml

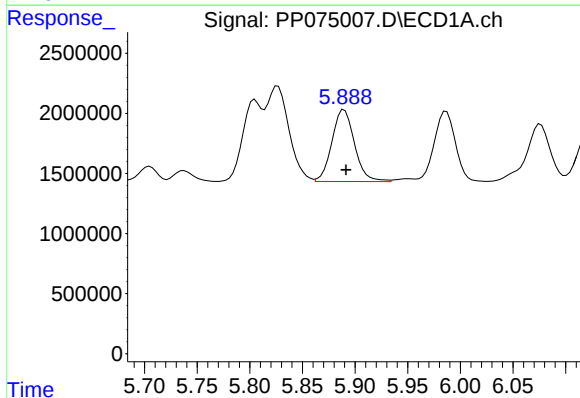


#18 AR-1242-3

R.T.: 5.890 min
Delta R.T.: -0.002 min
Response: 8946301
Conc: 220.34 ng/ml

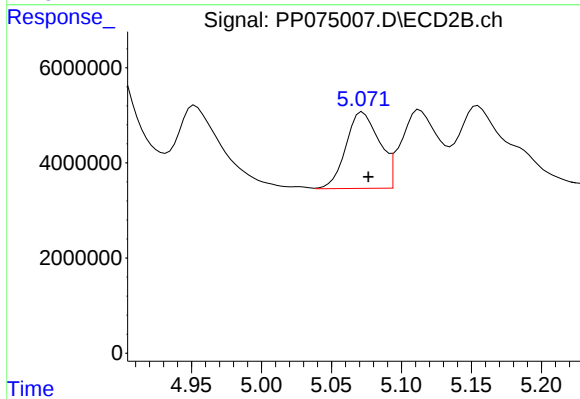

#18 AR-1242-3


R.T.: 5.072 min
Delta R.T.: -0.004 min
Response: 26724074
Conc: 225.90 ng/ml

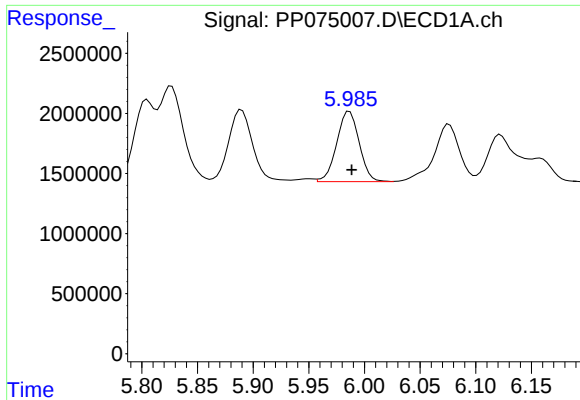

#19 AR-1242-4


R.T.: 5.987 min
Delta R.T.: -0.002 min
Response: 8216304
Conc: 258.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

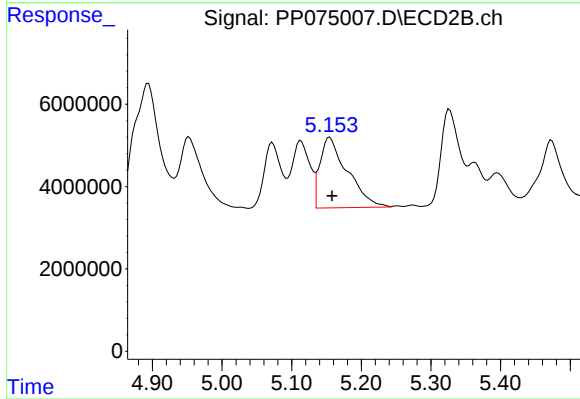


#19 AR-1242-4

R.T.: 5.155 min
Delta R.T.: -0.003 min
Response: 47030671
Conc: 274.78 ng/ml

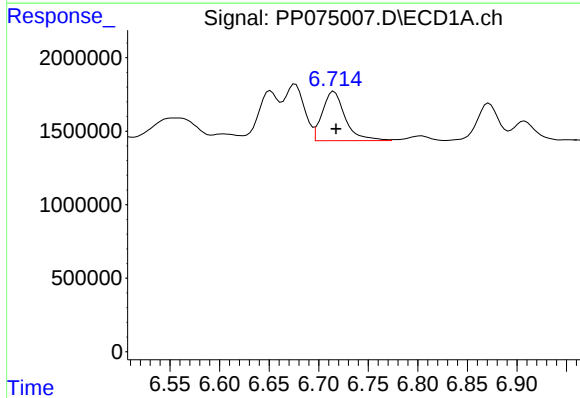


#20 AR-1242-5

R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 5404627
Conc: 149.83 ng/ml

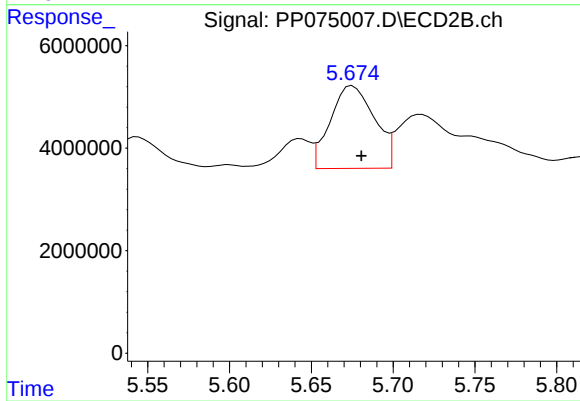

#20 AR-1242-5


R.T.: 5.675 min
Delta R.T.: -0.006 min
Response: 30272752
Conc: 163.49 ng/ml

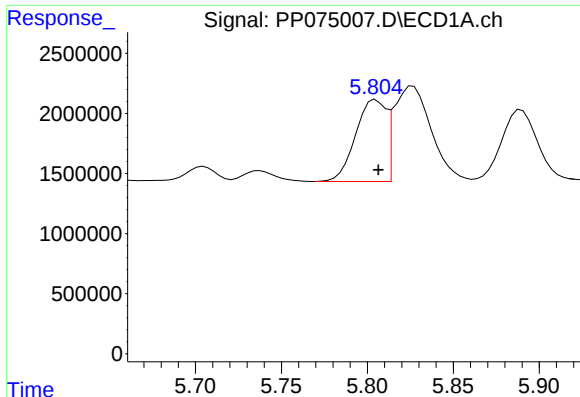

#21 AR-1248-1


R.T.: 5.805 min
Delta R.T.: -0.001 min
Response: 8359918
Conc: 276.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

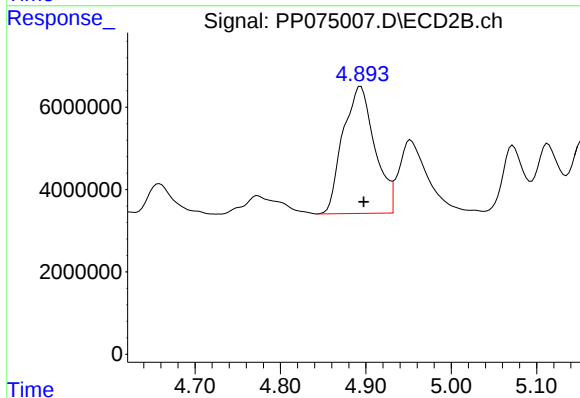


#21 AR-1248-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 79888374
Conc: 289.30 ng/ml

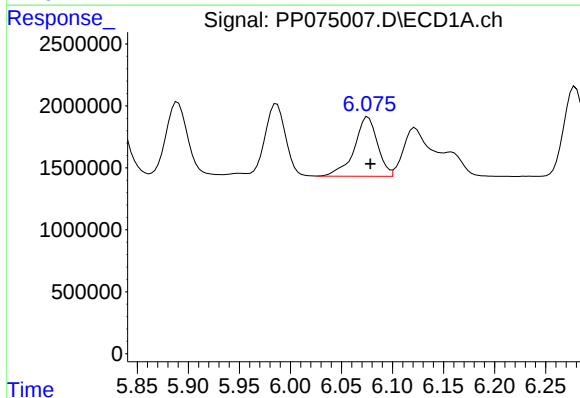


#22 AR-1248-2

R.T.: 6.076 min
Delta R.T.: -0.002 min
Response: 7607617
Conc: 176.53 ng/ml

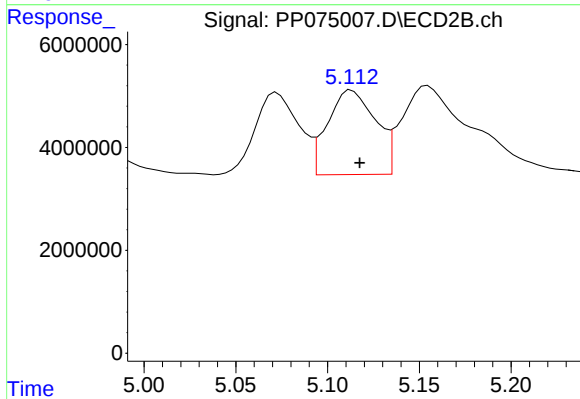

#22 AR-1248-2


R.T.: 5.113 min
Delta R.T.: -0.004 min
Response: 29789417
Conc: 168.53 ng/ml

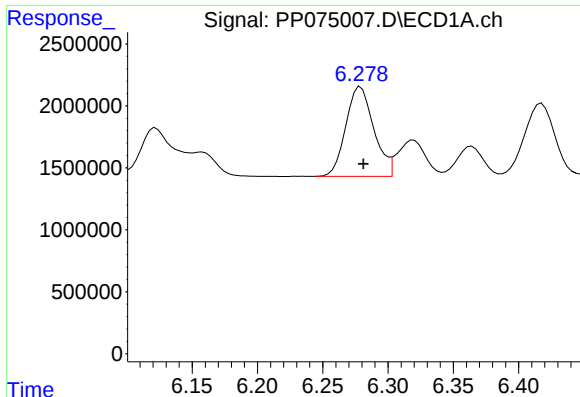

#23 AR-1248-3


R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 10768811
Conc: 230.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

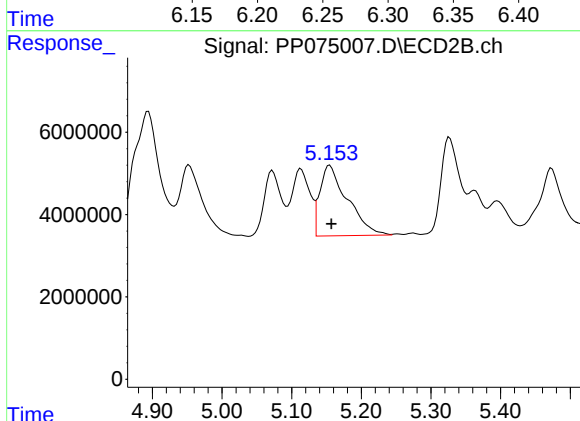


#23 AR-1248-3

R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 47030671
Conc: 207.00 ng/ml

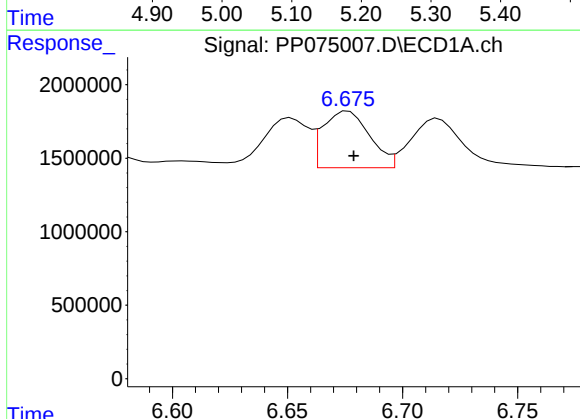


#24 AR-1248-4

R.T.: 6.676 min
Delta R.T.: -0.002 min
Response: 5443235
Conc: 98.97 ng/ml

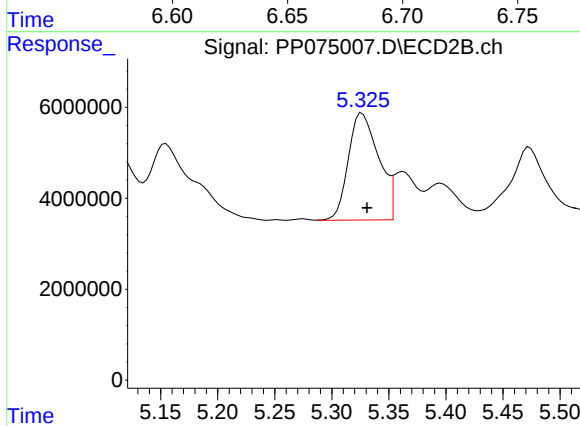

#24 AR-1248-4


R.T.: 5.327 min
Delta R.T.: -0.004 min
Response: 43613684
Conc: 200.04 ng/ml

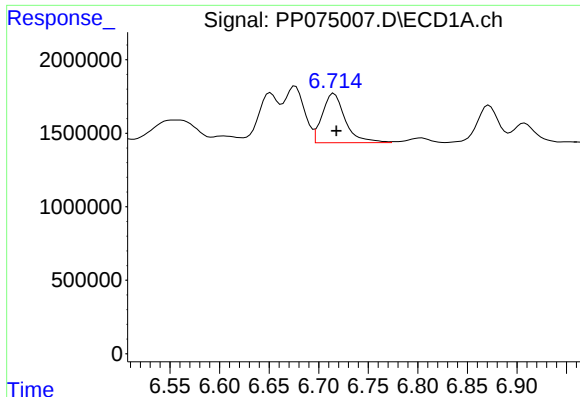

#25 AR-1248-5


R.T.: 6.716 min
Delta R.T.: -0.002 min
Response: 5404627
Conc: 97.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

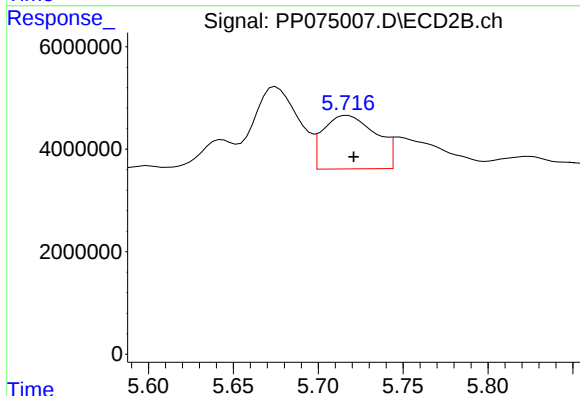


#25 AR-1248-5

R.T.: 5.717 min
Delta R.T.: -0.004 min
Response: 22629311
Conc: 61.61 ng/ml

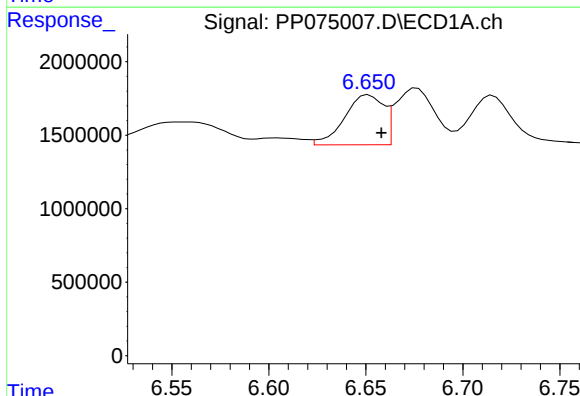


#26 AR-1254-1

R.T.: 6.651 min
Delta R.T.: -0.007 min
Response: 4741089
Conc: 81.36 ng/ml

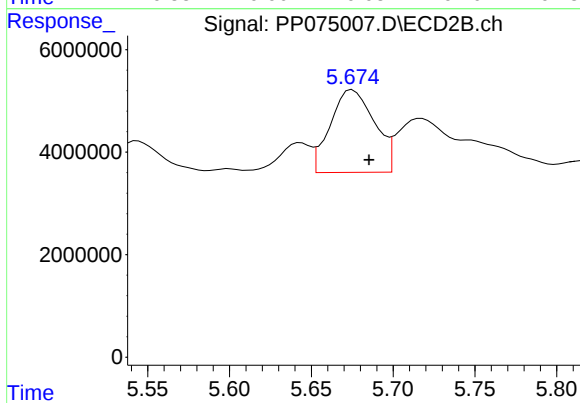

#26 AR-1254-1


R.T.: 5.675 min
Delta R.T.: -0.010 min
Response: 30272752
Conc: 63.50 ng/ml

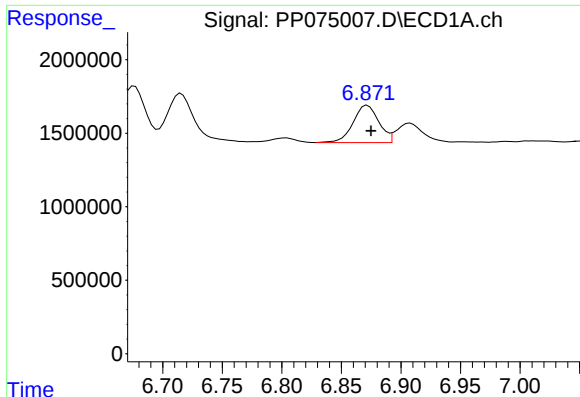

#27 AR-1254-2


R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 3800593
Conc: 46.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

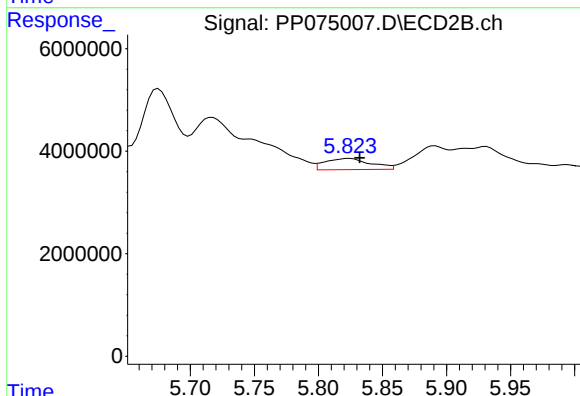


#27 AR-1254-2

R.T.: 5.824 min
Delta R.T.: -0.008 min
Response: 5424298
Conc: 15.40 ng/ml

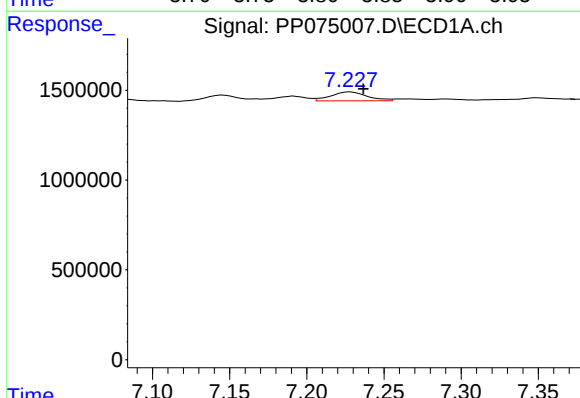


#28 AR-1254-3

R.T.: 7.228 min
Delta R.T.: -0.009 min
Response: 803152
Conc: 9.00 ng/ml

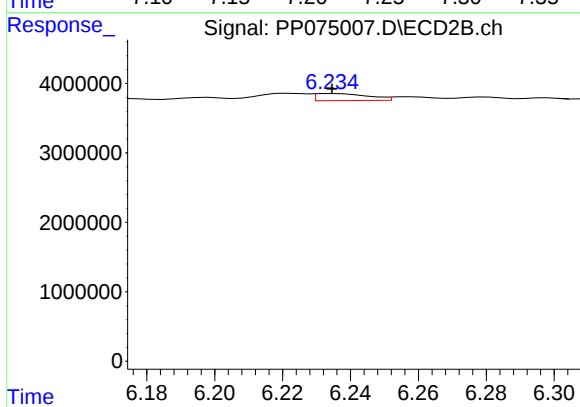

#28 AR-1254-3


R.T.: 6.235 min
Delta R.T.: 0.000 min
Response: 1095422
Conc: 1.77 ng/ml

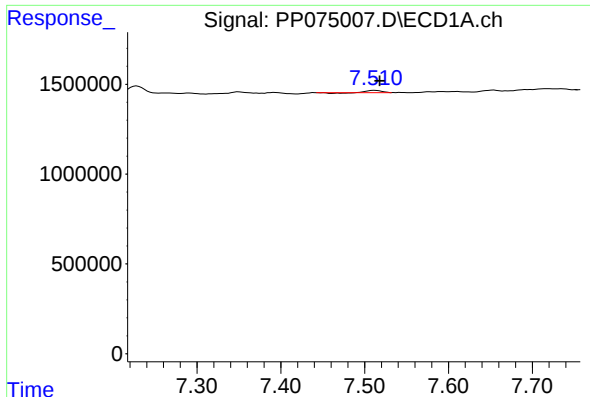

#29 AR-1254-4


R.T.: 7.511 min
Delta R.T.: -0.006 min
Response: 115547
Conc: 1.75 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

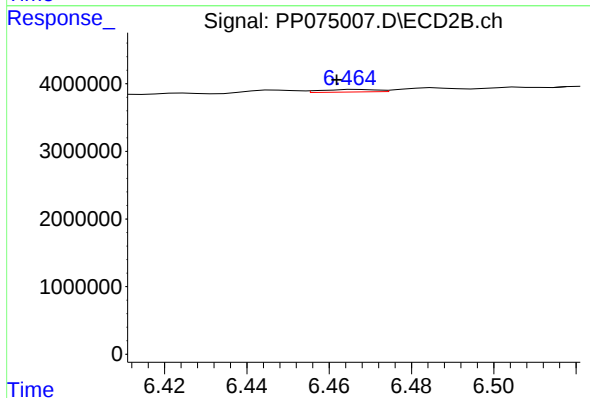


#29 AR-1254-4

R.T.: 6.467 min
Delta R.T.: 0.005 min
Response: 348971
Conc: 0.74 ng/ml

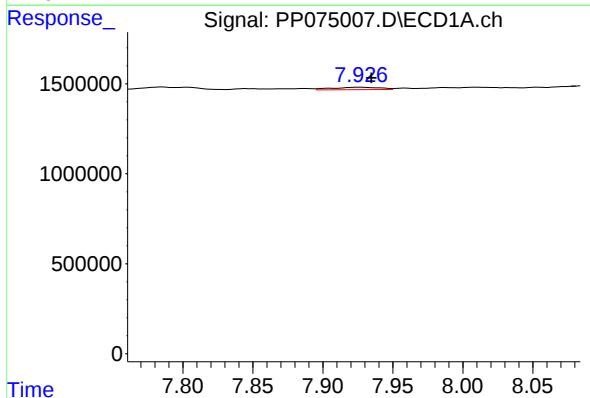


#30 AR-1254-5

R.T.: 7.927 min
Delta R.T.: -0.008 min
Response: 320026
Conc: 3.85 ng/ml

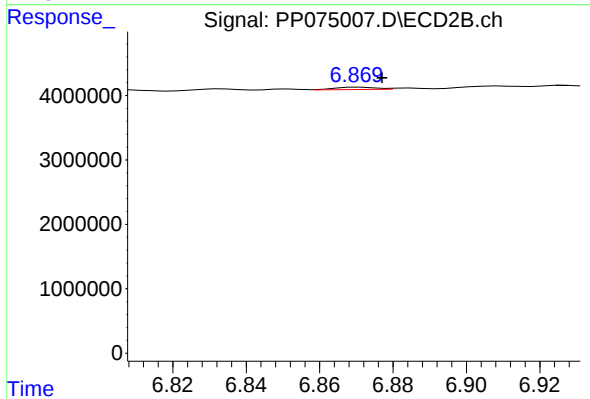

#30 AR-1254-5


R.T.: 6.871 min
Delta R.T.: -0.006 min
Response: 267272
Conc: 0.54 ng/ml

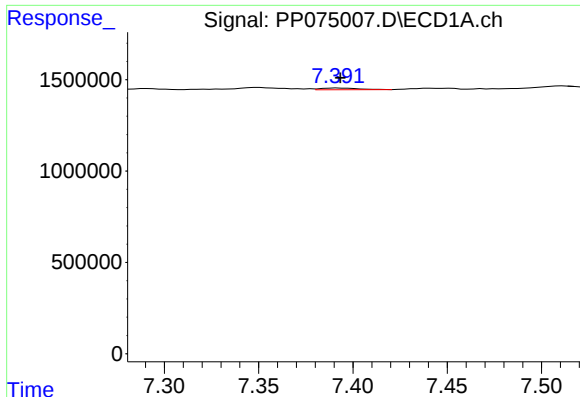

#31 AR-1260-1


R.T.: 7.392 min
Delta R.T.: -0.001 min
Response: 125768
Conc: 2.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

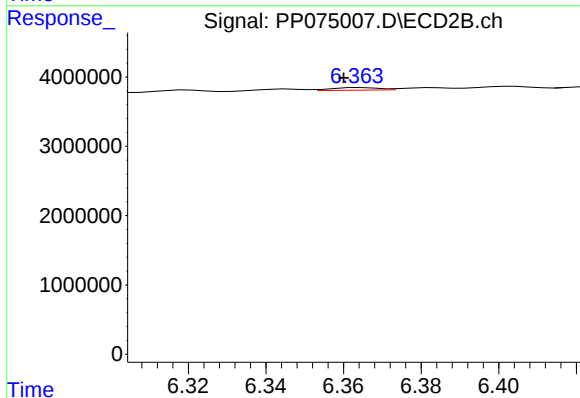


#31 AR-1260-1

R.T.: 6.365 min
Delta R.T.: 0.005 min
Response: 306452
Conc: 0.82 ng/ml

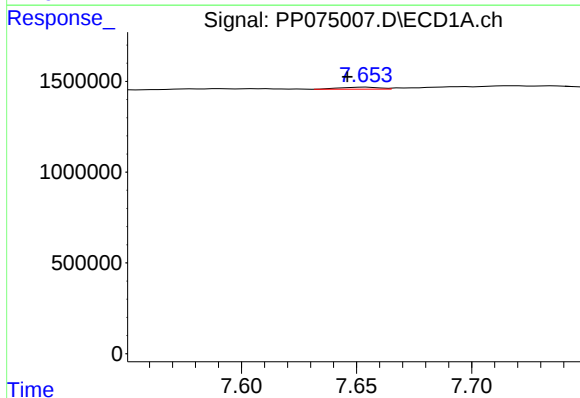


#32 AR-1260-2

R.T.: 7.654 min
Delta R.T.: 0.008 min
Response: 134093
Conc: 1.95 ng/ml

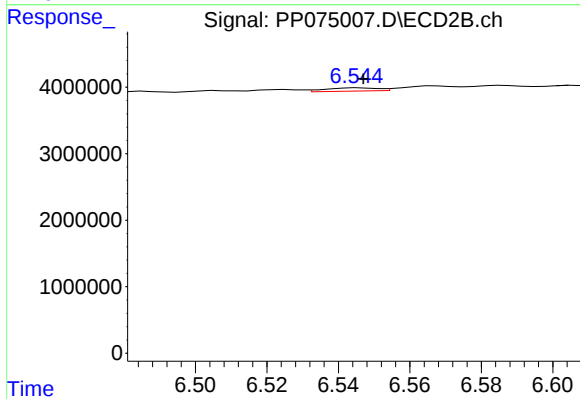

#32 AR-1260-2


R.T.: 6.546 min
Delta R.T.: -0.001 min
Response: 490054
Conc: 0.93 ng/ml

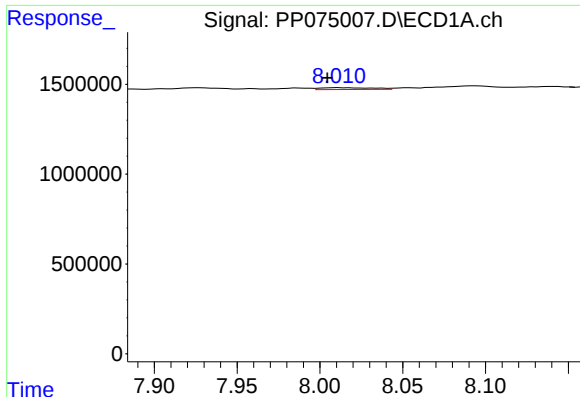

#33 AR-1260-3


R.T.: 8.011 min
Delta R.T.: 0.006 min
Response: 226507
Conc: 4.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

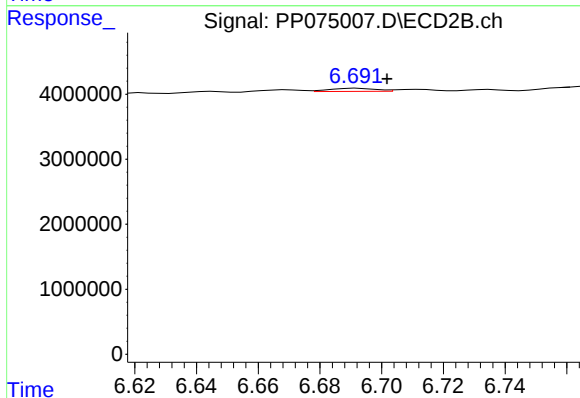


#33 AR-1260-3

R.T.: 6.692 min
Delta R.T.: -0.010 min
Response: 500719
Conc: 1.16 ng/ml

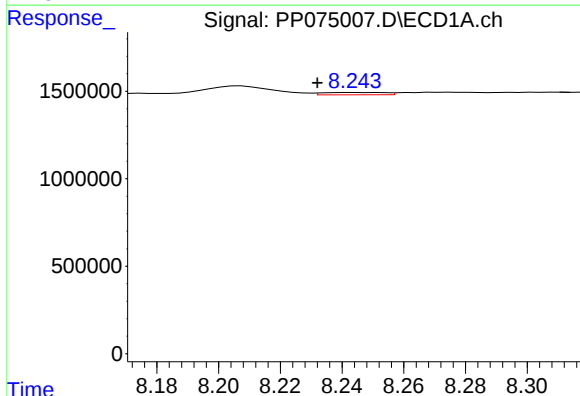


#34 AR-1260-4

R.T.: 8.245 min
Delta R.T.: 0.013 min
Response: 188773
Conc: 2.96 ng/ml

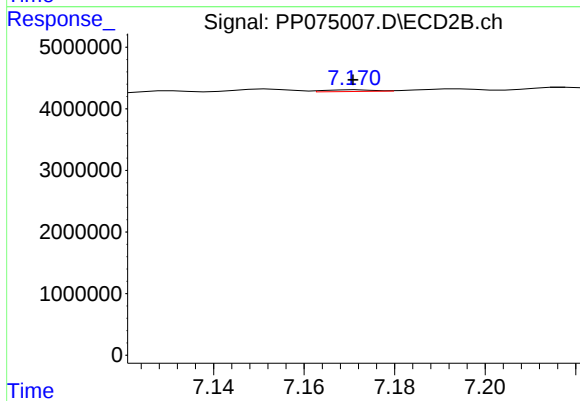

#34 AR-1260-4


R.T.: 7.172 min
Delta R.T.: 0.000 min
Response: 202780
Conc: 0.53 ng/ml

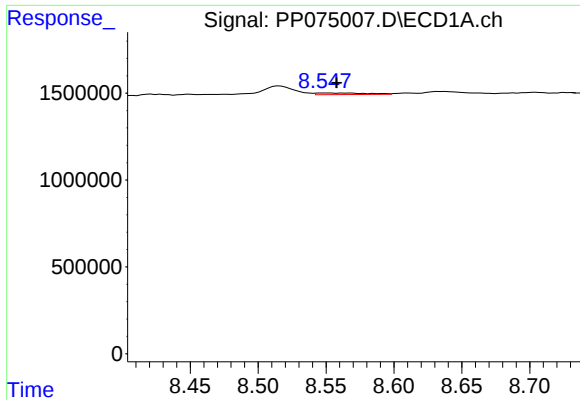

#35 AR-1260-5


R.T.: 8.550 min
Delta R.T.: -0.008 min
Response: 235150
Conc: 2.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

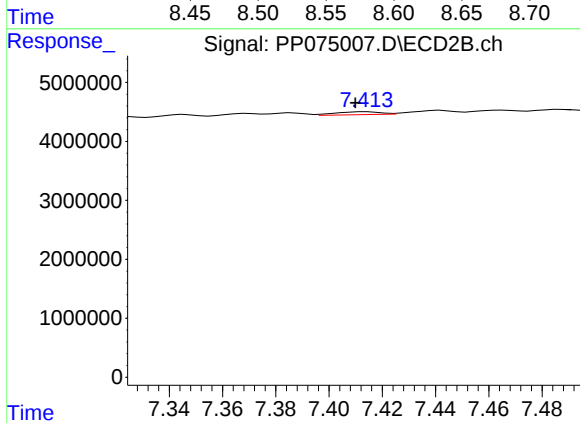


#35 AR-1260-5

R.T.: 7.414 min
Delta R.T.: 0.004 min
Response: 566050
Conc: 0.56 ng/ml

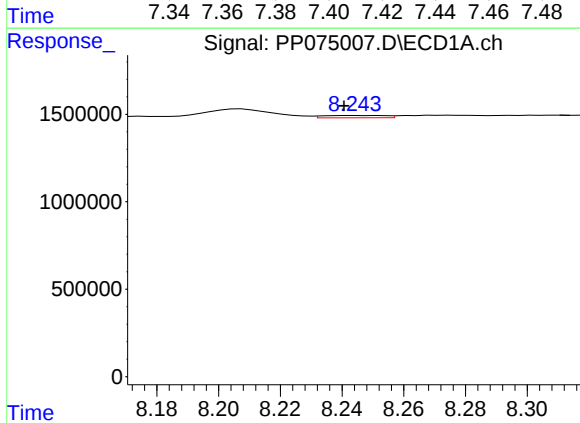


#36 AR-1262-1

R.T.: 8.245 min
Delta R.T.: 0.004 min
Response: 188773
Conc: 2.45 ng/ml

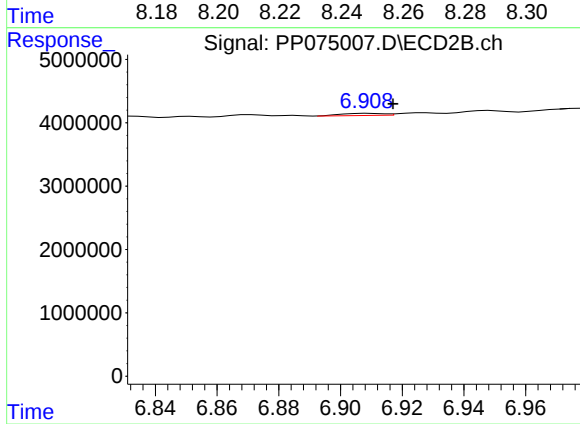

#36 AR-1262-1


R.T.: 6.909 min
Delta R.T.: -0.008 min
Response: 322982
Conc: 0.46 ng/ml

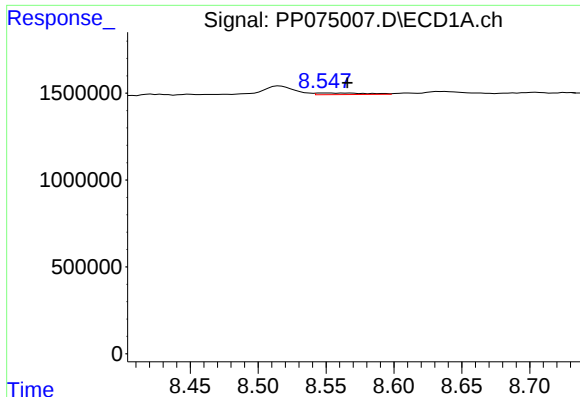

#37 AR-1262-2


R.T.: 8.550 min
Delta R.T.: -0.016 min
Response: 235150
Conc: 1.78 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

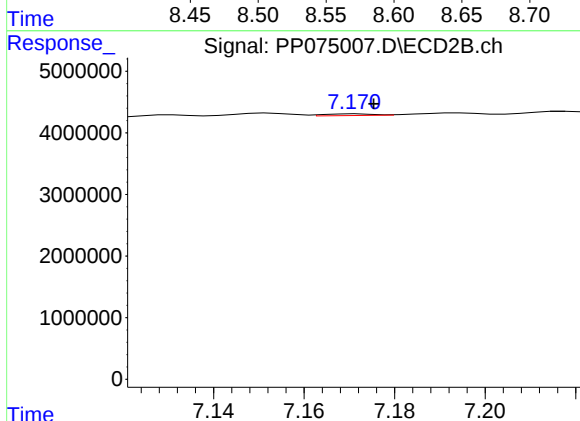


#37 AR-1262-2

R.T.: 7.172 min
Delta R.T.: -0.004 min
Response: 202780
Conc: 0.39 ng/ml

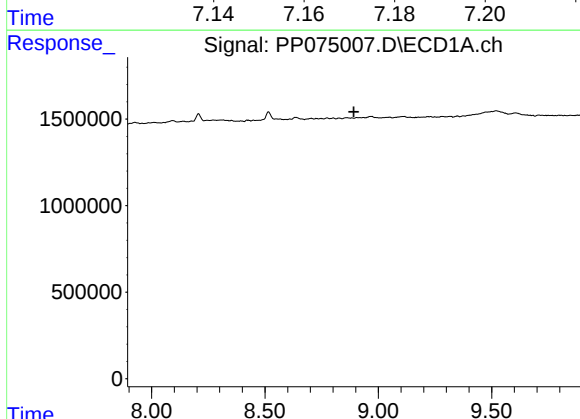


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

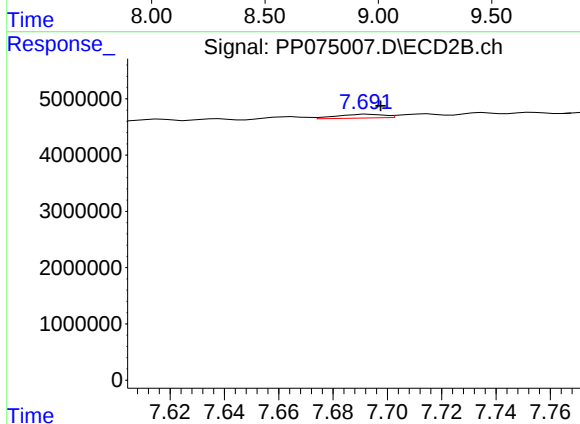

#38 AR-1262-3


R.T.: 7.692 min
Delta R.T.: -0.005 min
Response: 790009
Conc: 1.69 ng/ml

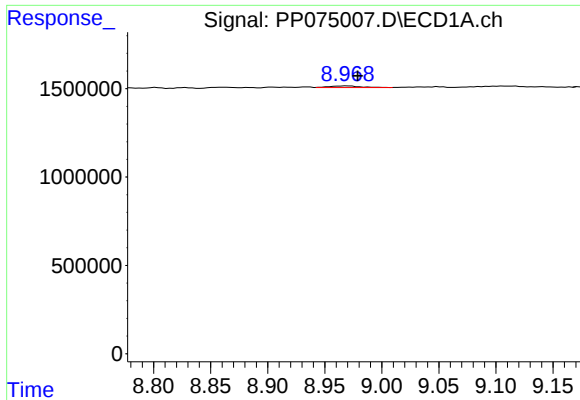

#39 AR-1262-4


R.T.: 8.970 min
Delta R.T.: -0.009 min
Response: 176052
Conc: 2.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

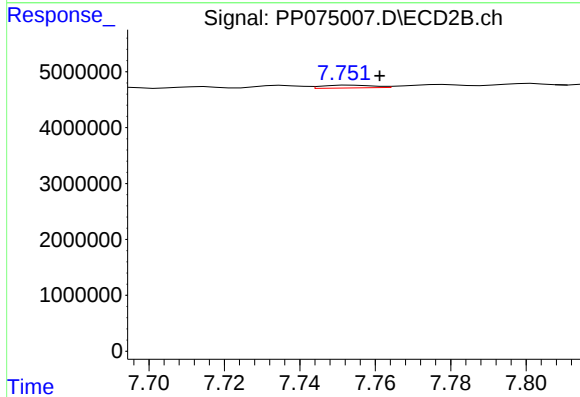


#39 AR-1262-4

R.T.: 7.754 min
Delta R.T.: -0.008 min
Response: 482758
Conc: 0.59 ng/ml

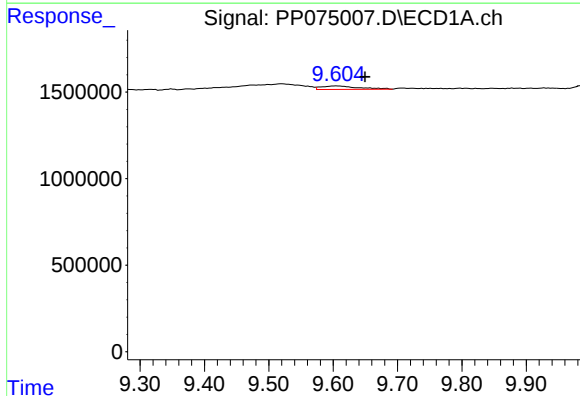


#40 AR-1262-5

R.T.: 9.606 min
Delta R.T.: -0.044 min
Response: 788231
Conc: 12.93 ng/ml

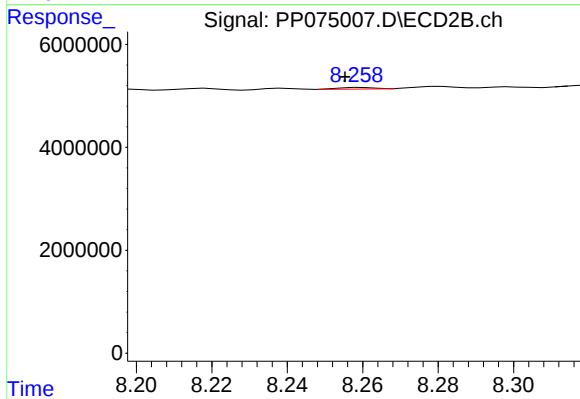

#40 AR-1262-5


R.T.: 8.260 min
Delta R.T.: 0.004 min
Response: 226488
Conc: 0.63 ng/ml

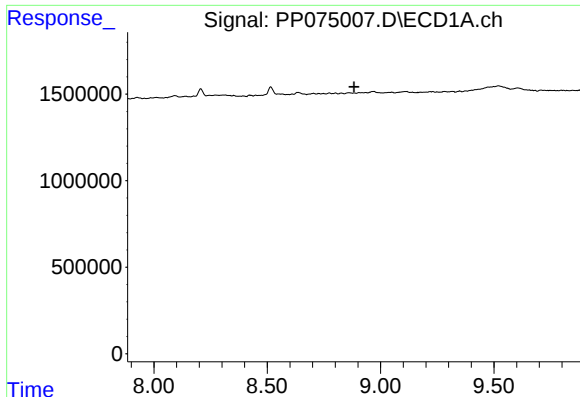

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

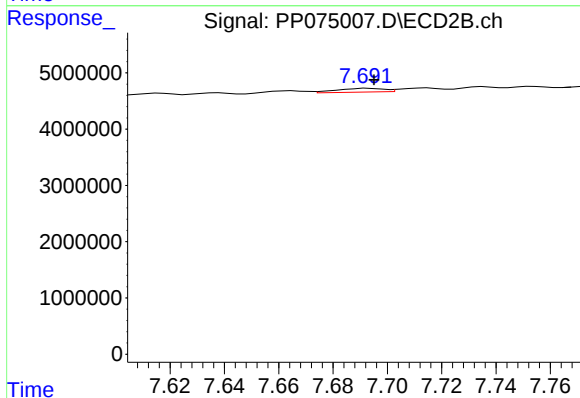


#41 AR-1268-1

R.T.: 7.692 min
Delta R.T.: -0.003 min
Response: 790009
Conc: 0.56 ng/ml

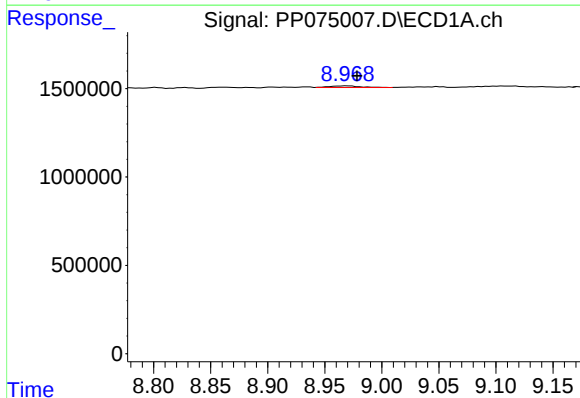


#42 AR-1268-2

R.T.: 8.970 min
Delta R.T.: -0.008 min
Response: 176052
Conc: 1.20 ng/ml

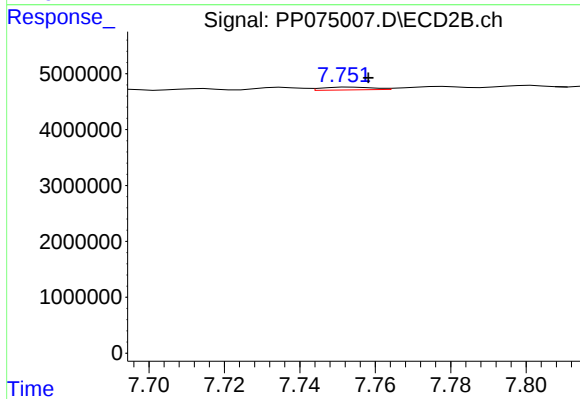

#42 AR-1268-2


R.T.: 7.754 min
Delta R.T.: -0.005 min
Response: 482758
Conc: 0.35 ng/ml

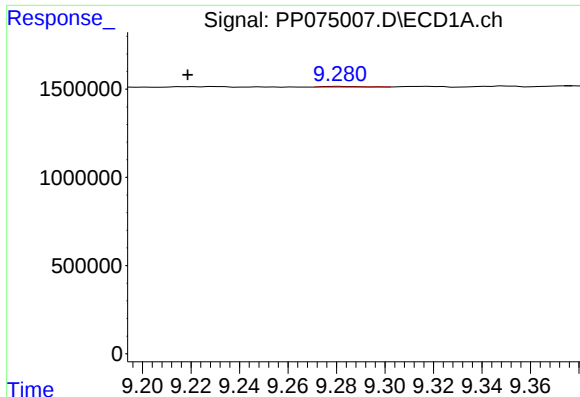

#43 AR-1268-3


R.T.: 9.282 min
Delta R.T.: 0.063 min
Response: 44200
Conc: 0.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

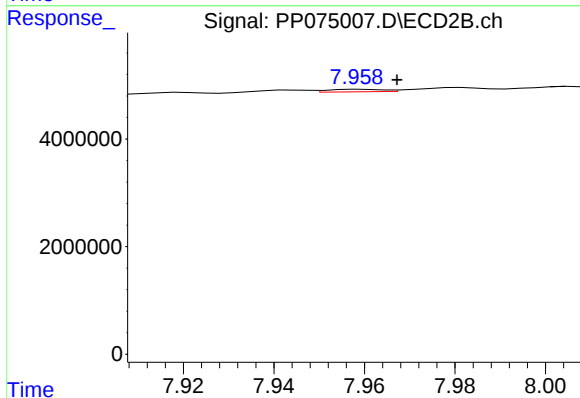


#43 AR-1268-3

R.T.: 7.959 min
Delta R.T.: -0.008 min
Response: 392411
Conc: 0.38 ng/ml

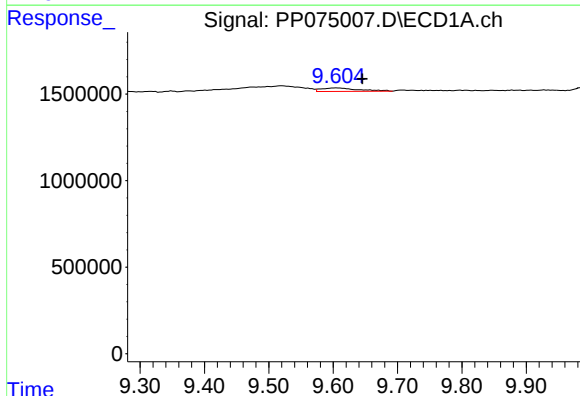


#44 AR-1268-4

R.T.: 9.606 min
Delta R.T.: -0.040 min
Response: 788231
Conc: 11.72 ng/ml

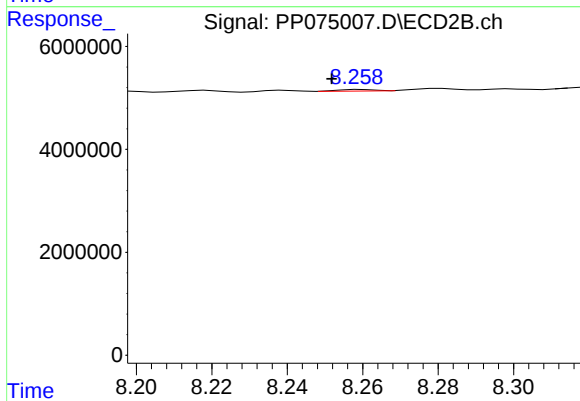

#44 AR-1268-4


R.T.: 8.260 min
Delta R.T.: 0.008 min
Response: 226488
Conc: 0.59 ng/ml

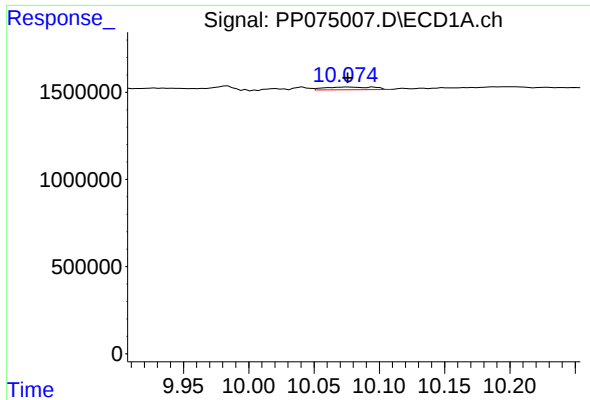

#45 AR-1268-5

R.T.: 10.076 min
Delta R.T.: 0.000 min
Response: 411652
Conc: 1.11 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-F

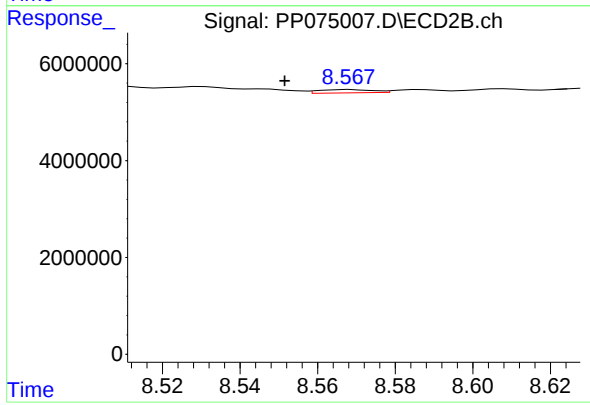

#45 AR-1268-5

R.T.: 8.568 min
Delta R.T.: 0.017 min
Response: 667903
Conc: 0.21 ng/ml