

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075008.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 15:13
 Operator : YP\AJ
 Sample : Q3034-07
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-G

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:50:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.654	3.797	27535002	104.9E6	22.502	21.695
2)	SA Decachlor...	10.426	8.803	22336709	140.4E6	22.619	18.719
Target Compounds							
3)	L1 AR-1016-1	5.805	4.894	4053119	34462978	91.931	67.660 #
4)	L1 AR-1016-2	5.827	4.952	5784567	18086073	92.050	75.987
5)	L1 AR-1016-3	5.890	5.071	4605328	11982571	102.537	86.891
6)	L1 AR-1016-4	5.986	5.113	4239001	15907462	120.488	113.785
7)	L1 AR-1016-5	6.279	5.326	6664696	25262373	200.828	152.107
8)	L2 AR-1221-1	4.853	4.007	866531	307876	49.255	4.976 #
9)	L2 AR-1221-2	4.955	4.093	762643	1269794	57.096	28.085 #
10)	L2 AR-1221-3	5.014	4.176	250286	521520	6.602	3.174 #
11)	L3 AR-1232-1	5.014	4.176	250286	521520	8.240	4.071 #
12)	L3 AR-1232-2	5.541	4.894	1925184	34462978	122.170	148.680
13)	L3 AR-1232-3	5.827	5.071	5784567	11982571	189.387	199.511
14)	L3 AR-1232-4	5.986	5.156	4239001	26259585	245.465	356.268 #
15)	L3 AR-1232-5	6.075	5.326	4580324	25262373	352.850	406.908
16)	L4 AR-1242-1	5.805	4.894	4053119	34462978	105.894	81.714
17)	L4 AR-1242-2	5.827	4.952	5784567	18086073	102.414	90.303
18)	L4 AR-1242-3	5.890	5.071	4605328	11982571	113.424	101.291
19)	L4 AR-1242-4	5.986	5.156	4239001	26259585	133.546	153.422
20)	L4 AR-1242-5	6.715	5.676	4420379	23967318	122.548	129.438
21)	L5 AR-1248-1	5.805	4.894	4053119	34462978	134.103	124.801
22)	L5 AR-1248-2	6.075	5.113	4580324	15907462	106.282	89.997
23)	L5 AR-1248-3	6.279	5.156	6664696	26259585	142.702	115.577
24)	L5 AR-1248-4	6.676	5.326	4294769	25262373	78.086	115.871 #
25)	L5 AR-1248-5	6.715	5.718	4420379	19918206	79.689	54.225 #
26)	L6 AR-1254-1	6.651	5.676	3659038	23967318	62.795	50.276
27)	L6 AR-1254-2	6.872	5.826	3202612	5825182	39.240	16.543 #
28)	L6 AR-1254-3	7.231	6.227	1285856	1824036	14.414	2.943 #
29)	L6 AR-1254-4	7.511	6.457	263205	892014	3.993	1.903 #
30)	L6 AR-1254-5	7.930	6.872	570087	649281	6.861	1.324 #
31)	L7 AR-1260-1	7.393	6.356	159906	311618	2.766	0.830 #
32)	L7 AR-1260-2	7.651	6.539	205832	1010425	2.987	1.911 #
33)	L7 AR-1260-3	8.005	6.697	531592	202378	10.246	0.467 #
34)	L7 AR-1260-4	8.208	7.176	1386043	379136	21.727	0.994 #
35)	L7 AR-1260-5	8.553	7.403	309580	385993	2.730	0.384 #
36)	L8 AR-1262-1	8.261	6.918	308833	489574	4.010	0.692 #
37)	L8 AR-1262-2	8.553	7.176	309580	379136	2.339	0.728 #
38)	L8 AR-1262-3	0.000	7.692	0	788101	N.D.	1.690 #
39)	L8 AR-1262-4	8.970	7.760	215018	863589	2.854	1.051 #
40)	L8 AR-1262-5	9.604f	8.249	195077	285208	3.200	0.796 #
41)	L9 AR-1268-1	0.000	7.692	0	788101	N.D.	0.559 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 15:13
Operator : YP\AJ
Sample : Q3034-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:50:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.970	7.760	215018	863589	1.465	0.633 #
43)	L9 AR-1268-3	0.000	7.965	0	807192	N.D.	0.774 #
44)	L9 AR-1268-4	9.604f	8.249	195077	285208	2.900	0.744 #
45)	L9 AR-1268-5	10.075	8.548	500162	822462	1.351	0.262 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075008.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 15:13
Operator : YP\AJ
Sample : Q3034-07
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:50:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

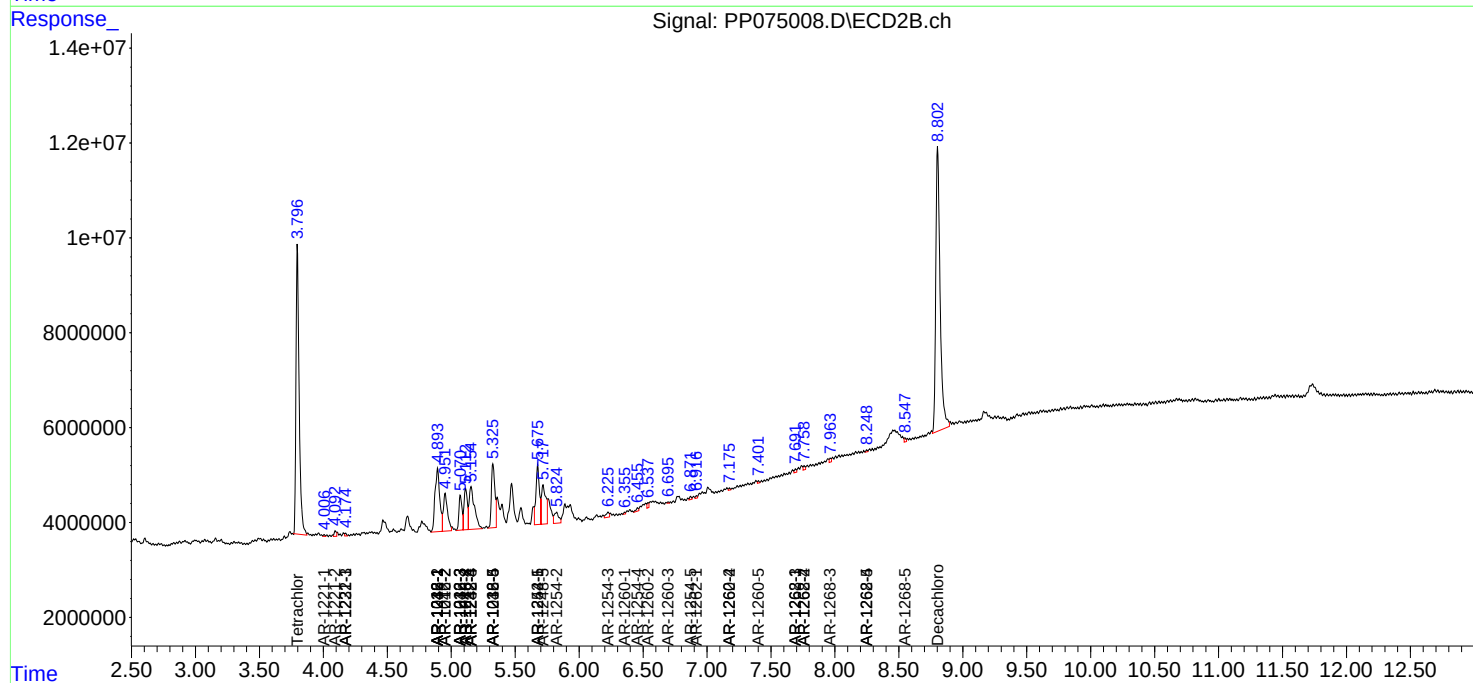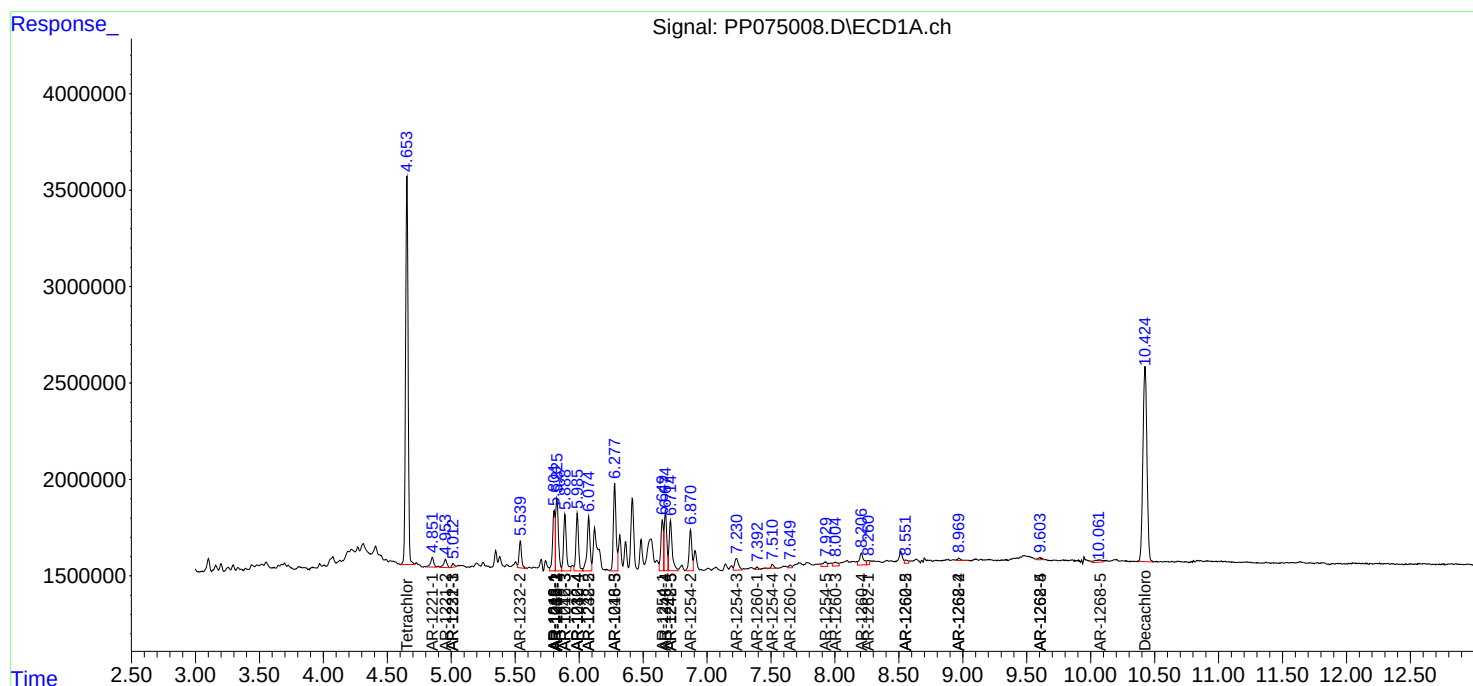


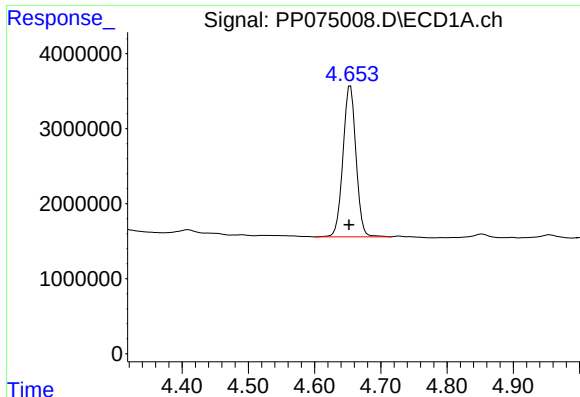

#1 Tetrachloro-m-xylene


R.T.: 4.654 min
Delta R.T.: 0.002 min
Response: 27535002
Conc: 22.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

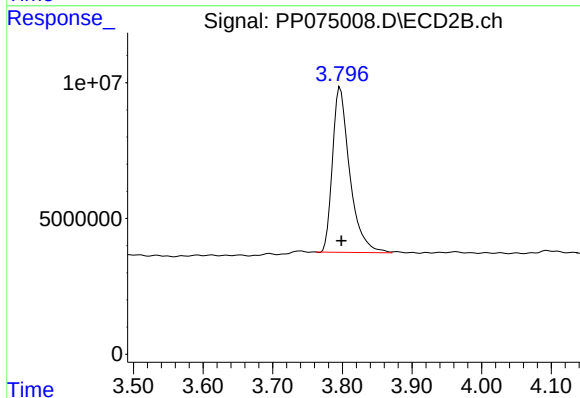


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: -0.002 min
Response: 104905840
Conc: 21.70 ng/ml

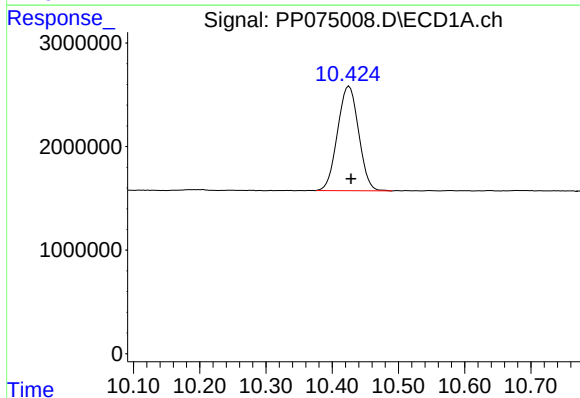


#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.003 min
Response: 22336709
Conc: 22.62 ng/ml

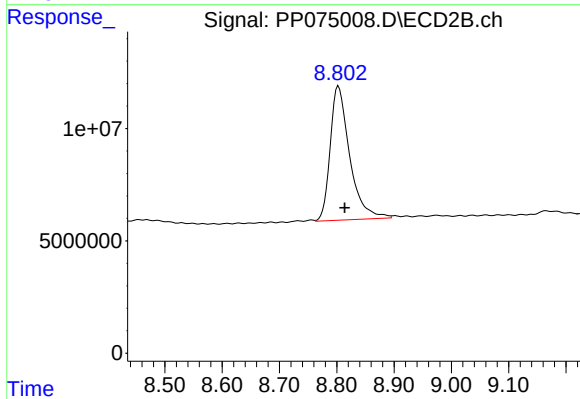

#2 Decachlorobiphenyl


R.T.: 8.803 min
Delta R.T.: -0.011 min
Response: 140375273
Conc: 18.72 ng/ml

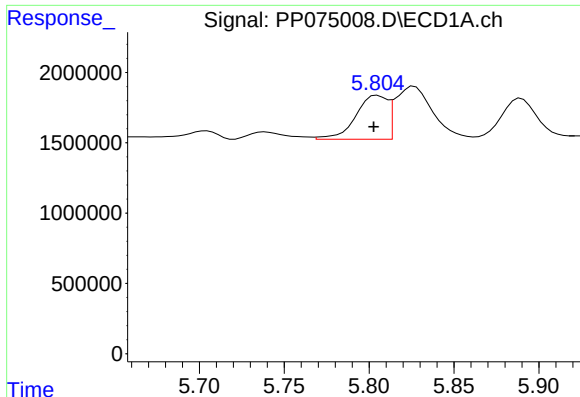

#3 AR-1016-1


R.T.: 5.805 min
Delta R.T.: 0.002 min
Response: 4053119
Conc: 91.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

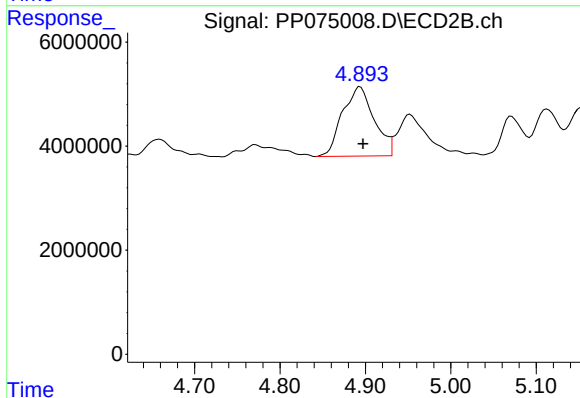


#3 AR-1016-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 34462978
Conc: 67.66 ng/ml

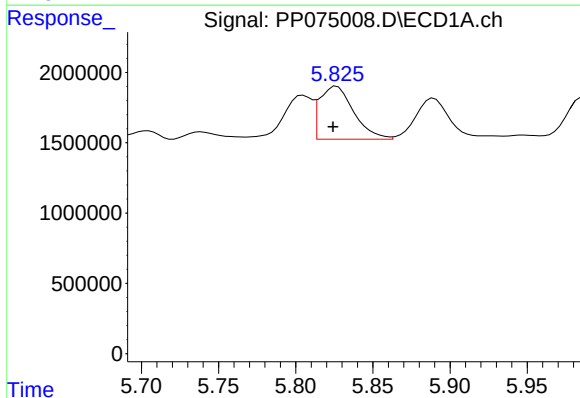


#4 AR-1016-2

R.T.: 5.827 min
Delta R.T.: 0.003 min
Response: 5784567
Conc: 92.05 ng/ml

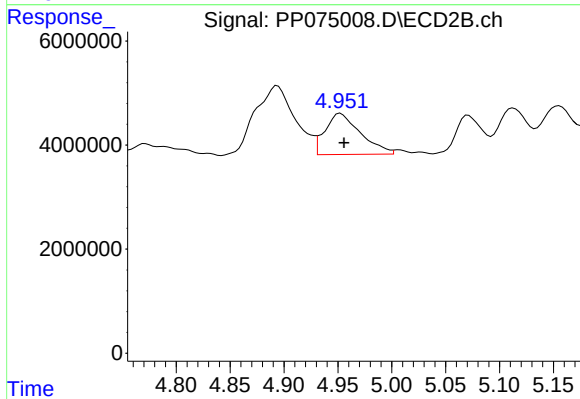

#4 AR-1016-2


R.T.: 4.952 min
Delta R.T.: -0.003 min
Response: 18086073
Conc: 75.99 ng/ml

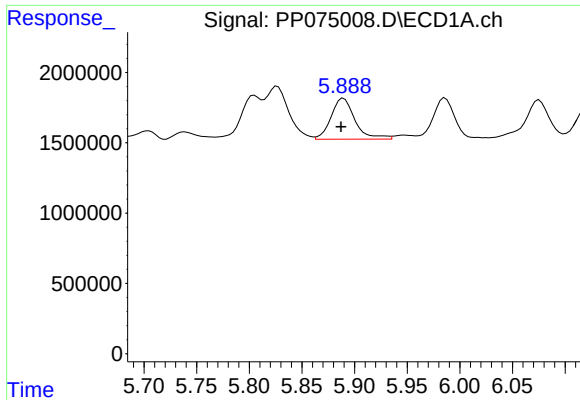

#5 AR-1016-3


R.T.: 5.890 min
Delta R.T.: 0.003 min
Response: 4605328
Conc: 102.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

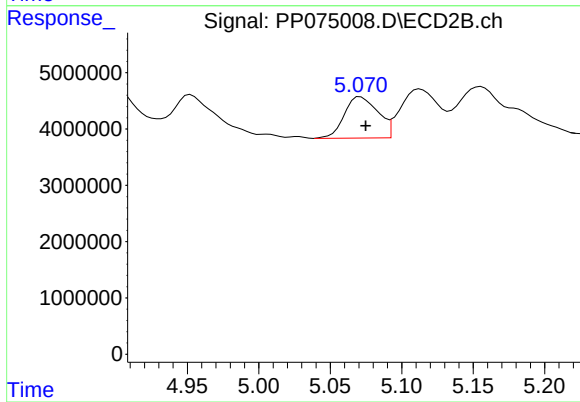


#5 AR-1016-3

R.T.: 5.071 min
Delta R.T.: -0.004 min
Response: 11982571
Conc: 86.89 ng/ml

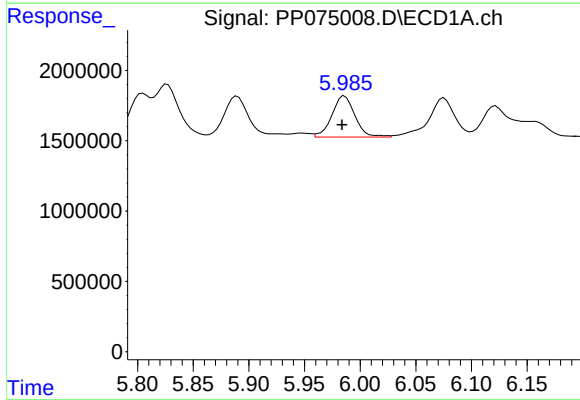


#6 AR-1016-4

R.T.: 5.986 min
Delta R.T.: 0.002 min
Response: 4239001
Conc: 120.49 ng/ml

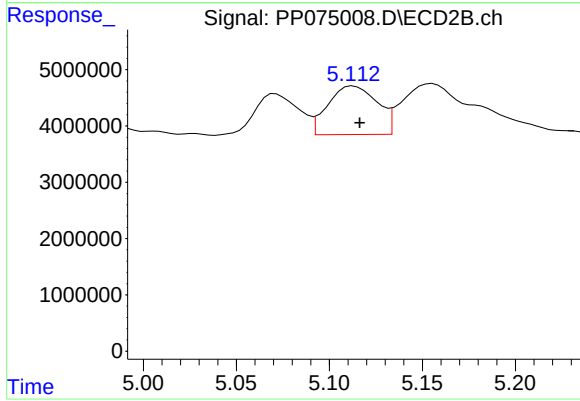

#6 AR-1016-4


R.T.: 5.113 min
Delta R.T.: -0.003 min
Response: 15907462
Conc: 113.78 ng/ml

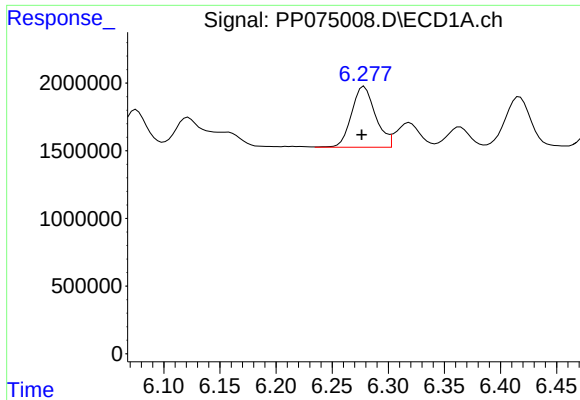

#7 AR-1016-5


R.T.: 6.279 min
Delta R.T.: 0.002 min
Response: 6664696
Conc: 200.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

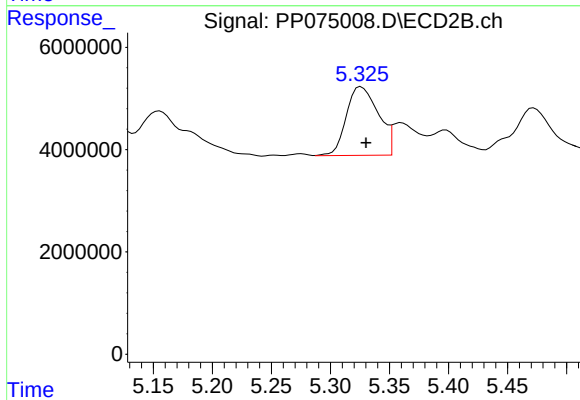


#7 AR-1016-5

R.T.: 5.326 min
Delta R.T.: -0.004 min
Response: 25262373
Conc: 152.11 ng/ml

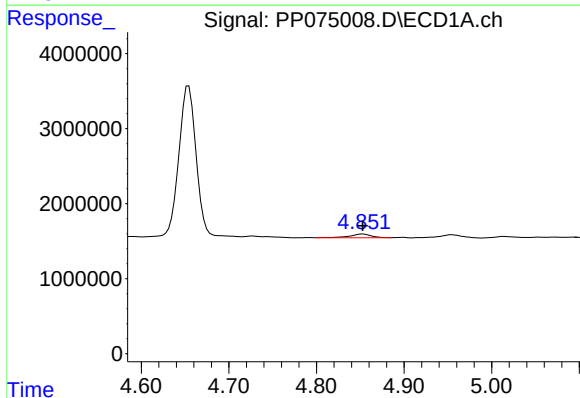


#8 AR-1221-1

R.T.: 4.853 min
Delta R.T.: 0.000 min
Response: 866531
Conc: 49.25 ng/ml

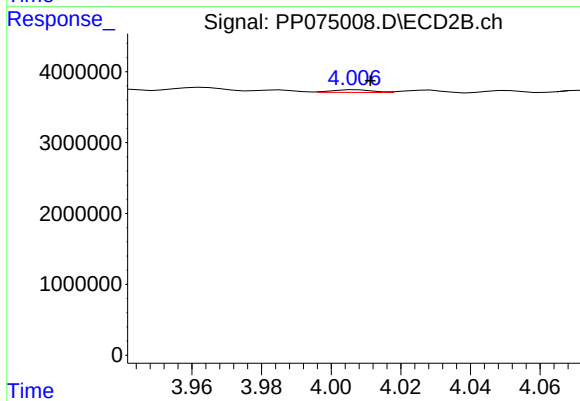

#8 AR-1221-1


R.T.: 4.007 min
Delta R.T.: -0.004 min
Response: 307876
Conc: 4.98 ng/ml

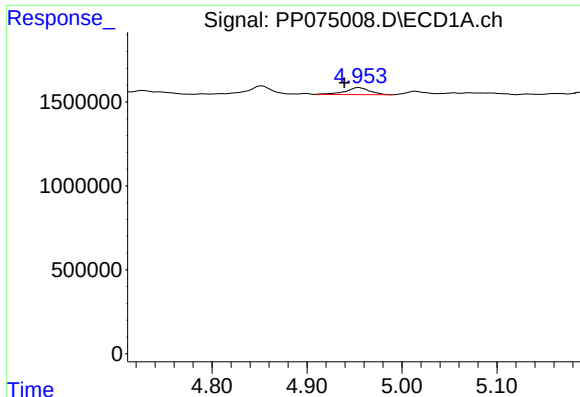

#9 AR-1221-2


R.T.: 4.955 min
Delta R.T.: 0.016 min
Response: 762643
Conc: 57.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

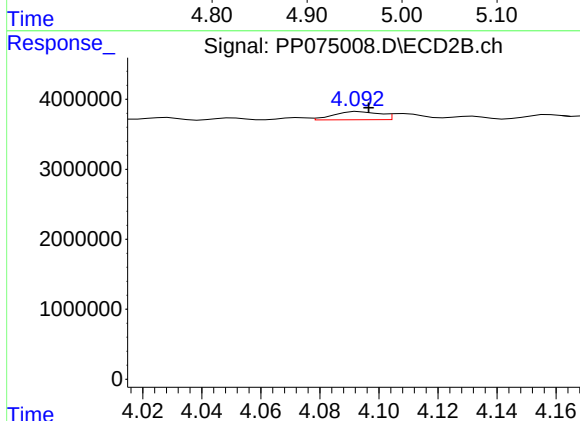


#9 AR-1221-2

R.T.: 4.093 min
Delta R.T.: -0.003 min
Response: 1269794
Conc: 28.09 ng/ml

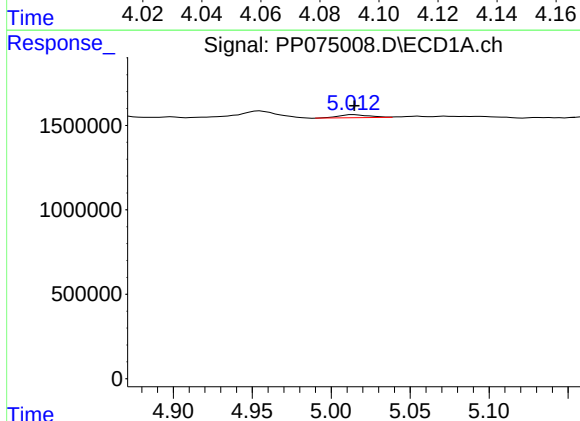


#10 AR-1221-3

R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 250286
Conc: 6.60 ng/ml

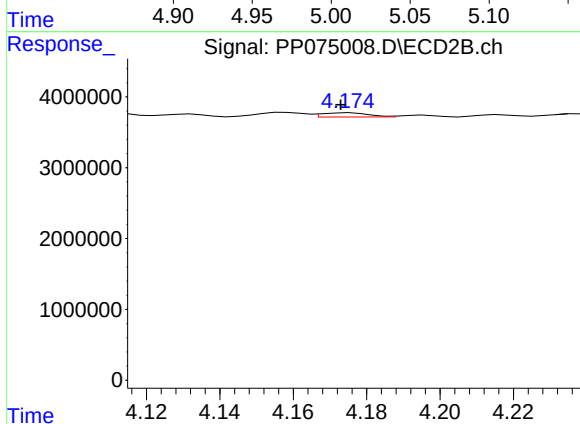

#10 AR-1221-3


R.T.: 4.176 min
Delta R.T.: 0.003 min
Response: 521520
Conc: 3.17 ng/ml

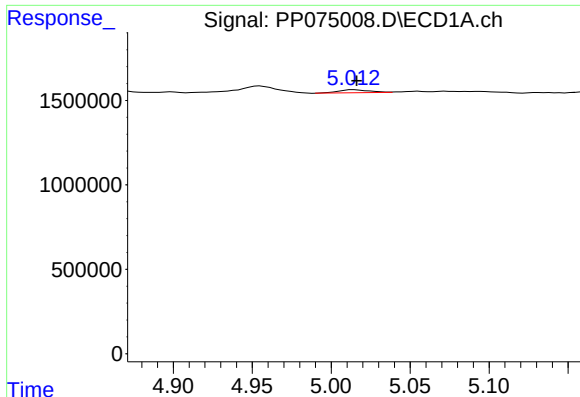

#11 AR-1232-1


R.T.: 5.014 min
Delta R.T.: -0.002 min
Response: 250286
Conc: 8.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

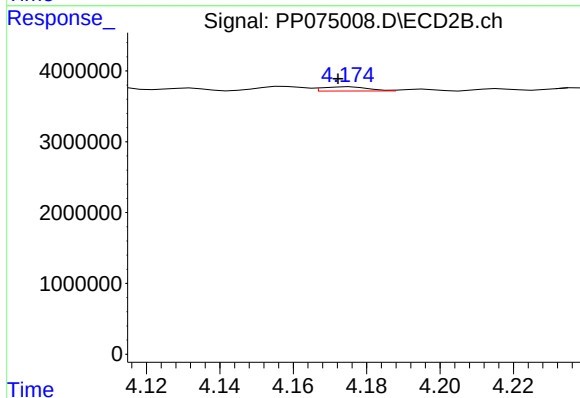


#11 AR-1232-1

R.T.: 4.176 min
Delta R.T.: 0.003 min
Response: 521520
Conc: 4.07 ng/ml

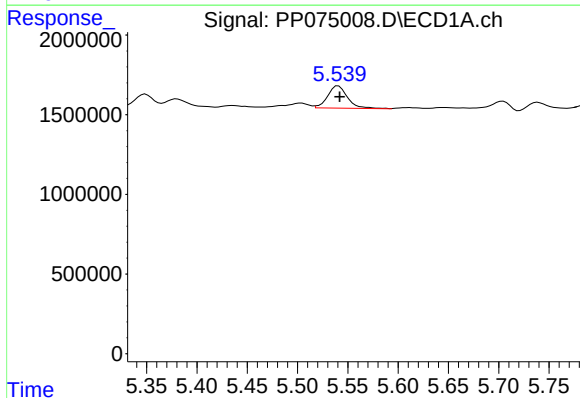


#12 AR-1232-2

R.T.: 5.541 min
Delta R.T.: -0.001 min
Response: 1925184
Conc: 122.17 ng/ml

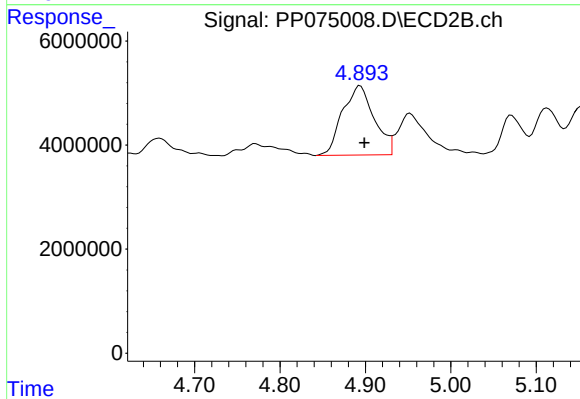

#12 AR-1232-2


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 34462978
Conc: 148.68 ng/ml

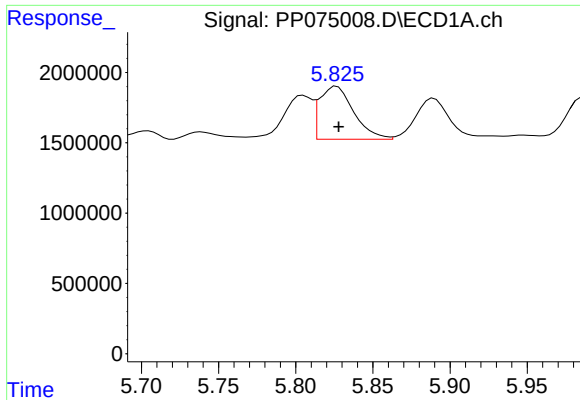

#13 AR-1232-3


R.T.: 5.827 min
Delta R.T.: -0.001 min
Response: 5784567
Conc: 189.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

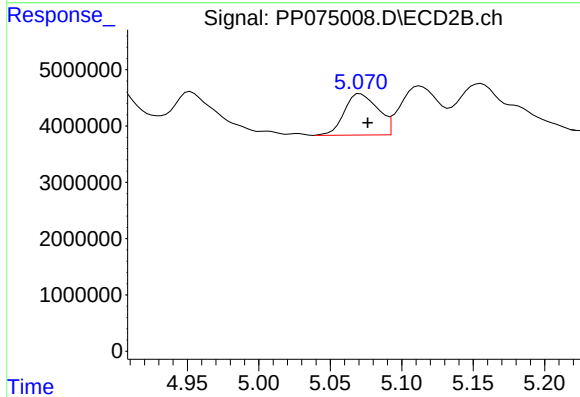


#13 AR-1232-3

R.T.: 5.071 min
Delta R.T.: -0.005 min
Response: 11982571
Conc: 199.51 ng/ml

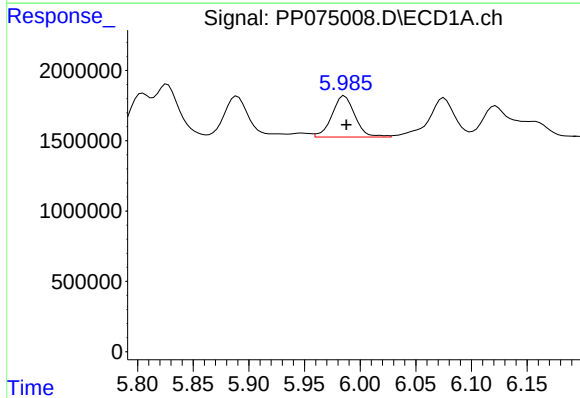


#14 AR-1232-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 4239001
Conc: 245.46 ng/ml

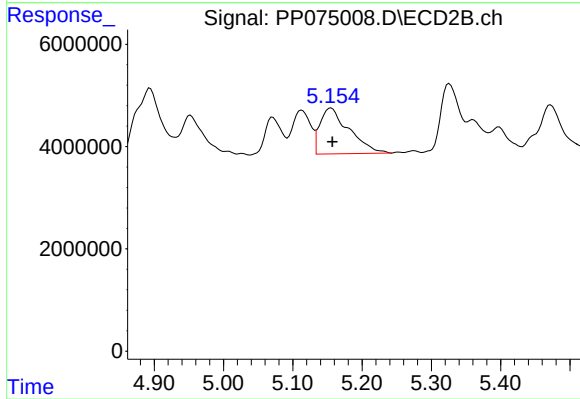

#14 AR-1232-4


R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 26259585
Conc: 356.27 ng/ml

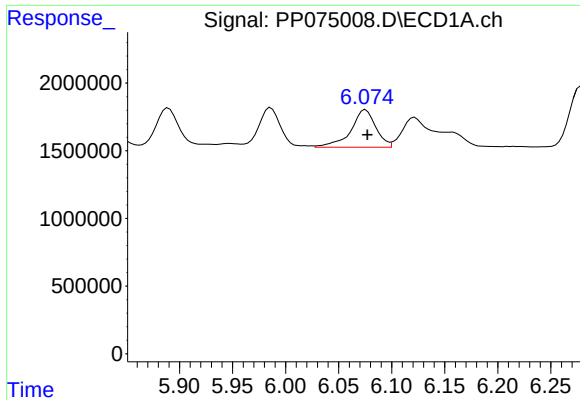

#15 AR-1232-5


R.T.: 6.075 min
Delta R.T.: -0.002 min
Response: 4580324
Conc: 352.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

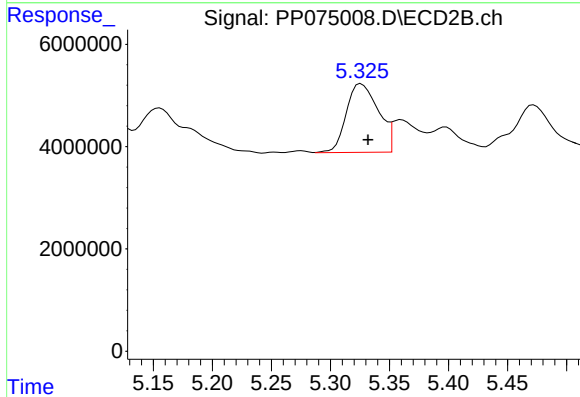


#15 AR-1232-5

R.T.: 5.326 min
Delta R.T.: -0.006 min
Response: 25262373
Conc: 406.91 ng/ml

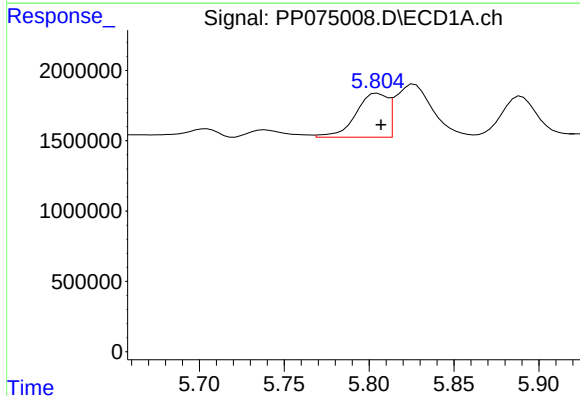


#16 AR-1242-1

R.T.: 5.805 min
Delta R.T.: -0.002 min
Response: 4053119
Conc: 105.89 ng/ml

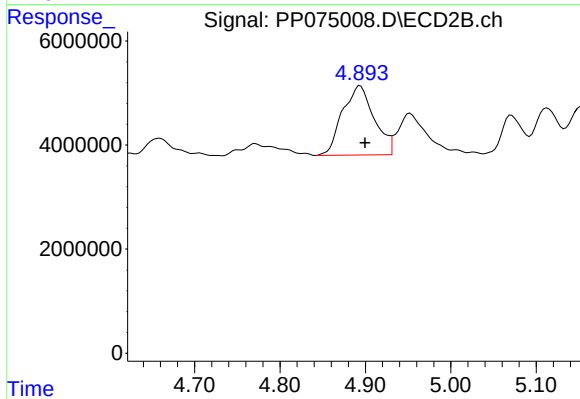

#16 AR-1242-1


R.T.: 4.894 min
Delta R.T.: -0.006 min
Response: 34462978
Conc: 81.71 ng/ml

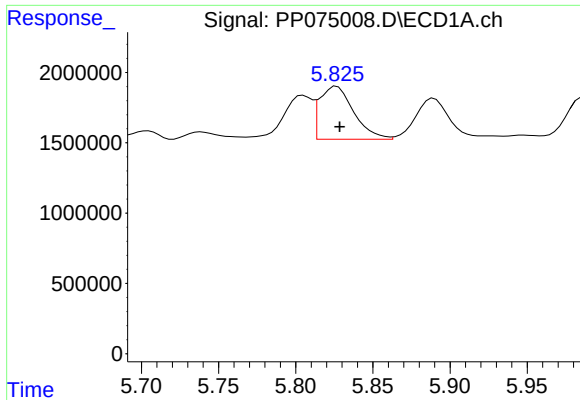

#17 AR-1242-2


R.T.: 5.827 min
Delta R.T.: -0.002 min
Response: 5784567
Conc: 102.41 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

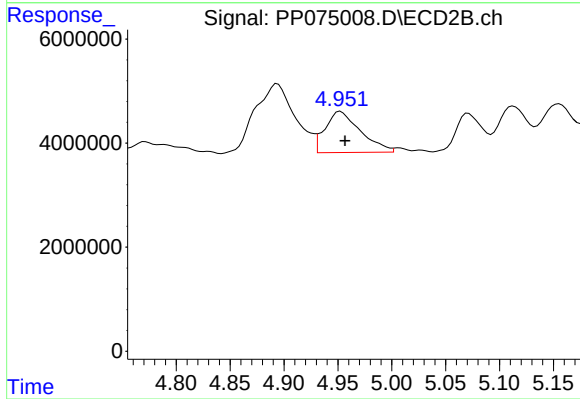


#17 AR-1242-2

R.T.: 4.952 min
Delta R.T.: -0.004 min
Response: 18086073
Conc: 90.30 ng/ml

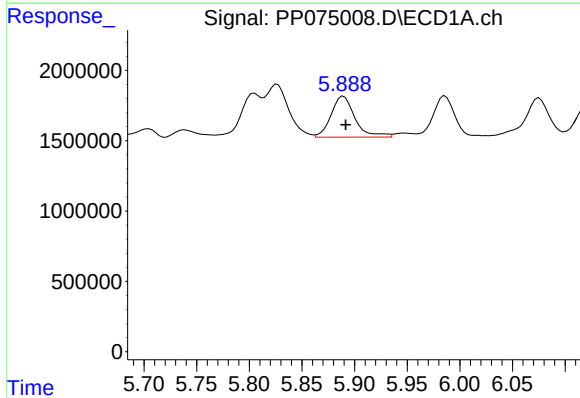


#18 AR-1242-3

R.T.: 5.890 min
Delta R.T.: -0.002 min
Response: 4605328
Conc: 113.42 ng/ml

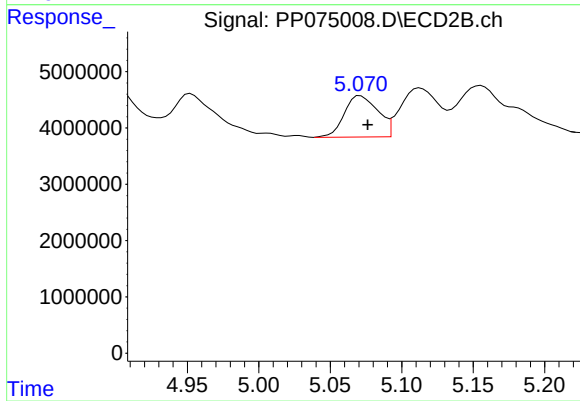

#18 AR-1242-3


R.T.: 5.071 min
Delta R.T.: -0.005 min
Response: 11982571
Conc: 101.29 ng/ml

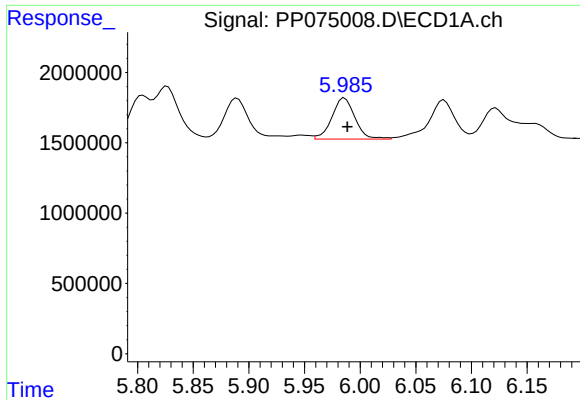

#19 AR-1242-4


R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 4239001
Conc: 133.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

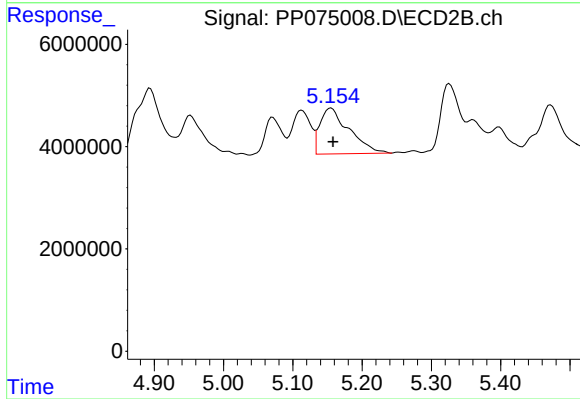


#19 AR-1242-4

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 26259585
Conc: 153.42 ng/ml

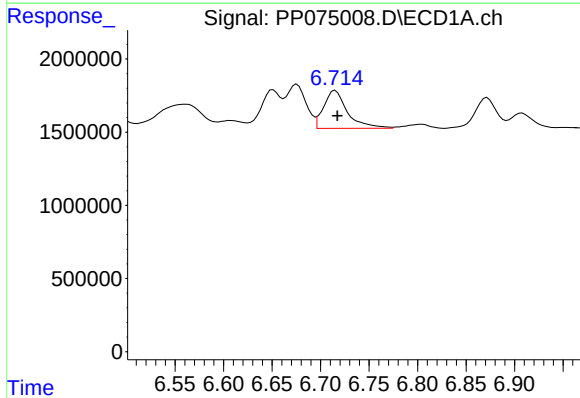


#20 AR-1242-5

R.T.: 6.715 min
Delta R.T.: -0.002 min
Response: 4420379
Conc: 122.55 ng/ml

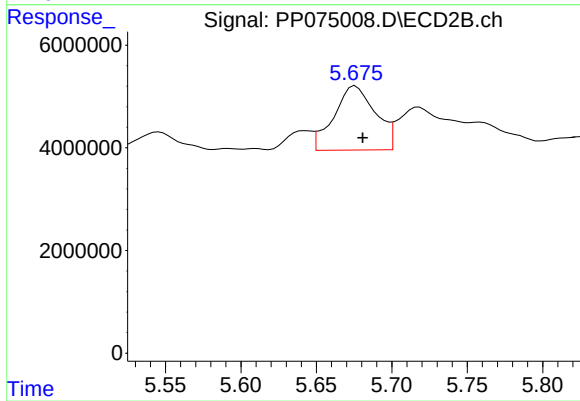

#20 AR-1242-5


R.T.: 5.676 min
Delta R.T.: -0.005 min
Response: 23967318
Conc: 129.44 ng/ml

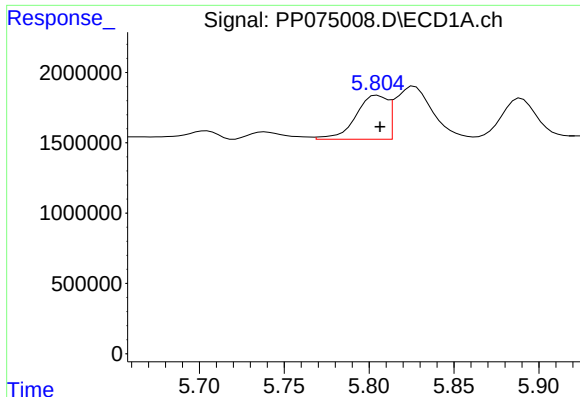

#21 AR-1248-1


R.T.: 5.805 min
Delta R.T.: -0.001 min
Response: 4053119
Conc: 134.10 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

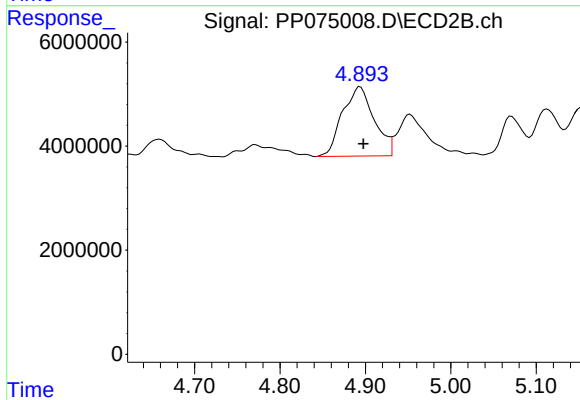


#21 AR-1248-1

R.T.: 4.894 min
Delta R.T.: -0.003 min
Response: 34462978
Conc: 124.80 ng/ml

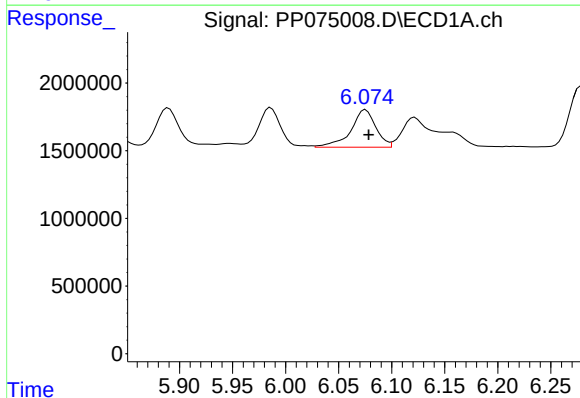


#22 AR-1248-2

R.T.: 6.075 min
Delta R.T.: -0.003 min
Response: 4580324
Conc: 106.28 ng/ml

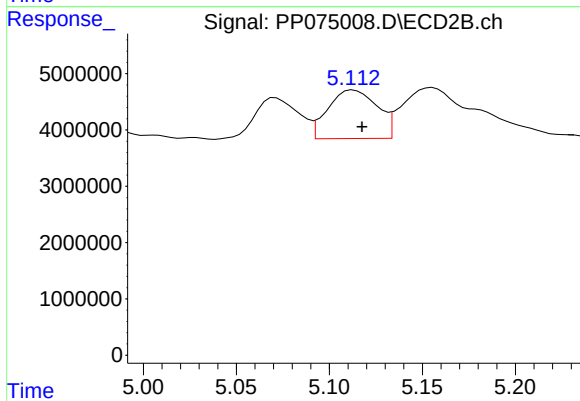

#22 AR-1248-2


R.T.: 5.113 min
Delta R.T.: -0.005 min
Response: 15907462
Conc: 90.00 ng/ml

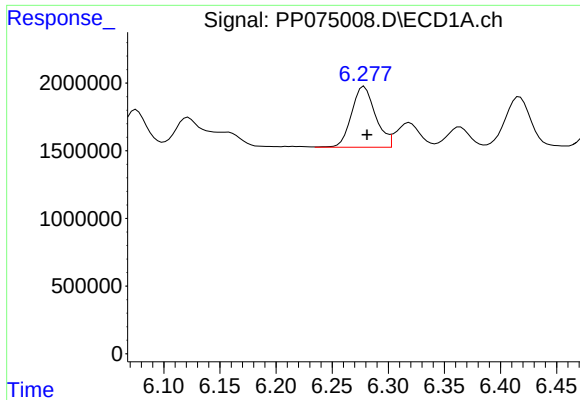

#23 AR-1248-3


R.T.: 6.279 min
Delta R.T.: -0.002 min
Response: 6664696
Conc: 142.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

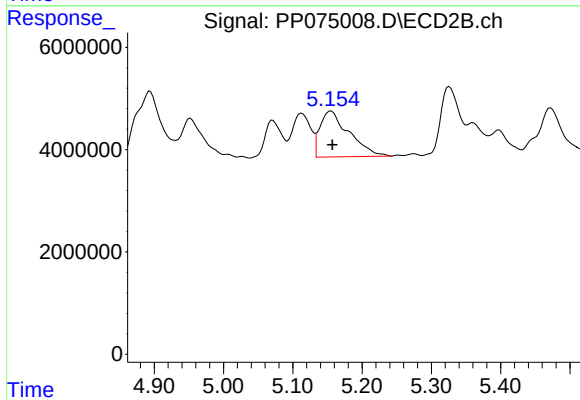


#23 AR-1248-3

R.T.: 5.156 min
Delta R.T.: -0.002 min
Response: 26259585
Conc: 115.58 ng/ml

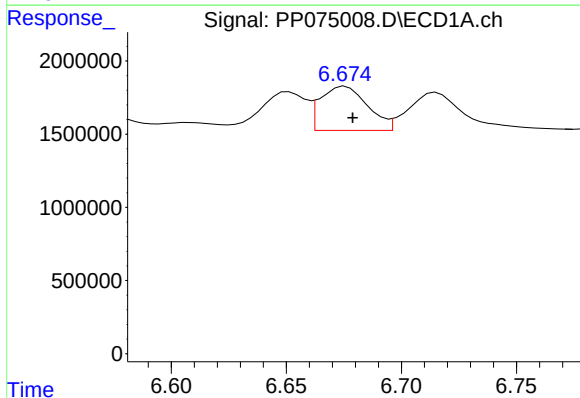


#24 AR-1248-4

R.T.: 6.676 min
Delta R.T.: -0.003 min
Response: 4294769
Conc: 78.09 ng/ml

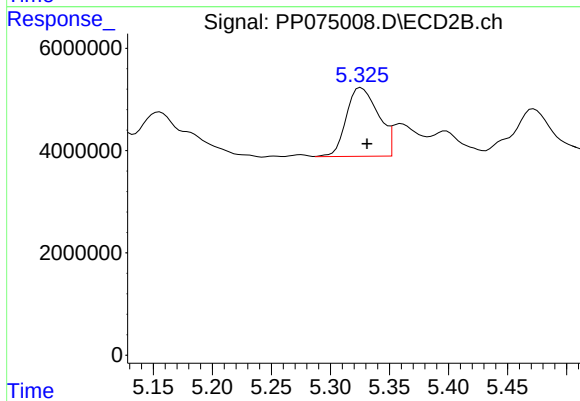

#24 AR-1248-4


R.T.: 5.326 min
Delta R.T.: -0.005 min
Response: 25262373
Conc: 115.87 ng/ml

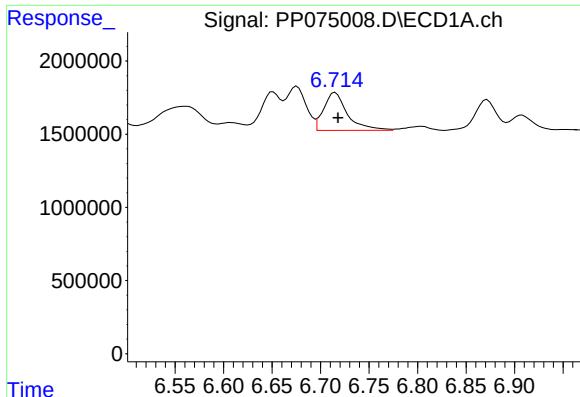

#25 AR-1248-5


R.T.: 6.715 min
Delta R.T.: -0.003 min
Response: 4420379
Conc: 79.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

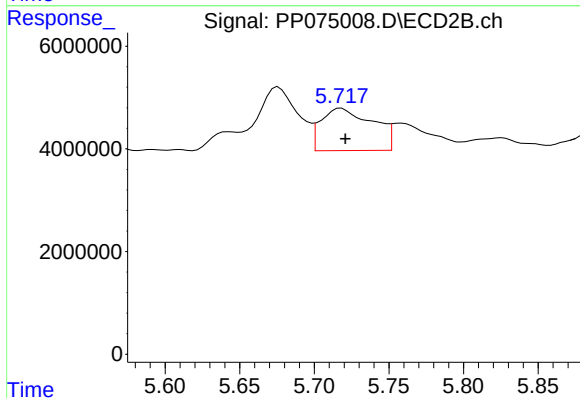


#25 AR-1248-5

R.T.: 5.718 min
Delta R.T.: -0.003 min
Response: 19918206
Conc: 54.23 ng/ml

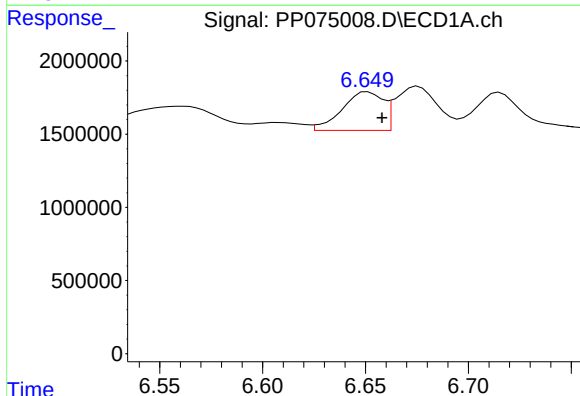


#26 AR-1254-1

R.T.: 6.651 min
Delta R.T.: -0.007 min
Response: 3659038
Conc: 62.80 ng/ml

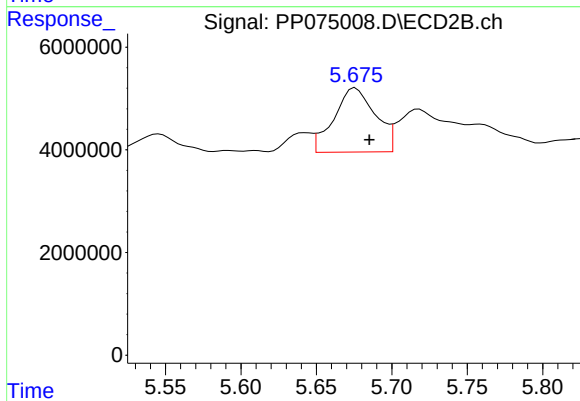

#26 AR-1254-1


R.T.: 5.676 min
Delta R.T.: -0.009 min
Response: 23967318
Conc: 50.28 ng/ml

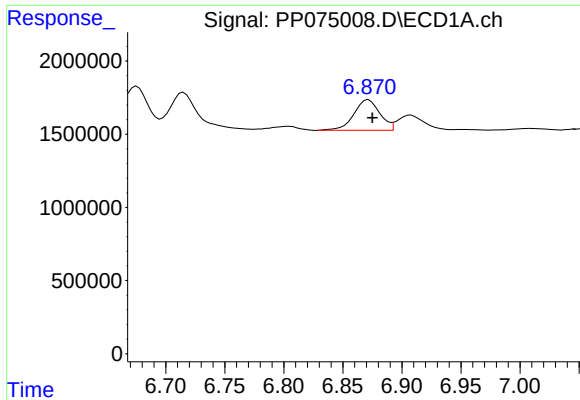

#27 AR-1254-2


R.T.: 6.872 min
Delta R.T.: -0.003 min
Response: 3202612
Conc: 39.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

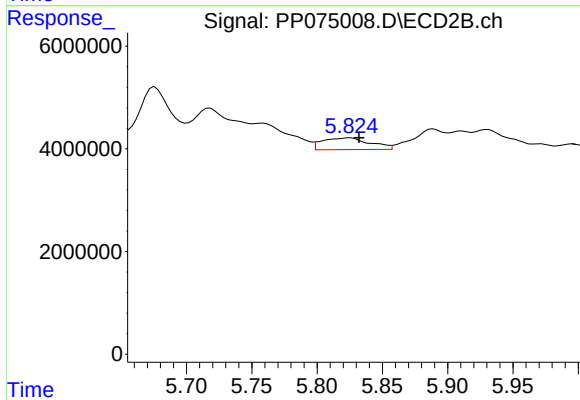


#27 AR-1254-2

R.T.: 5.826 min
Delta R.T.: -0.007 min
Response: 5825182
Conc: 16.54 ng/ml

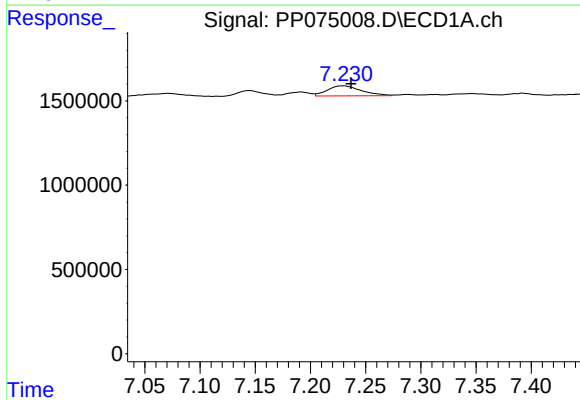


#28 AR-1254-3

R.T.: 7.231 min
Delta R.T.: -0.006 min
Response: 1285856
Conc: 14.41 ng/ml

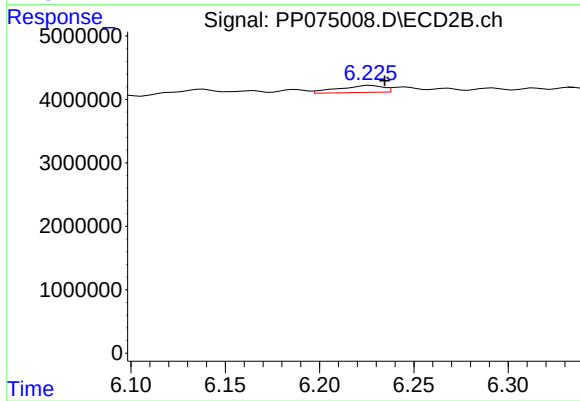

#28 AR-1254-3


R.T.: 6.227 min
Delta R.T.: -0.008 min
Response: 1824036
Conc: 2.94 ng/ml

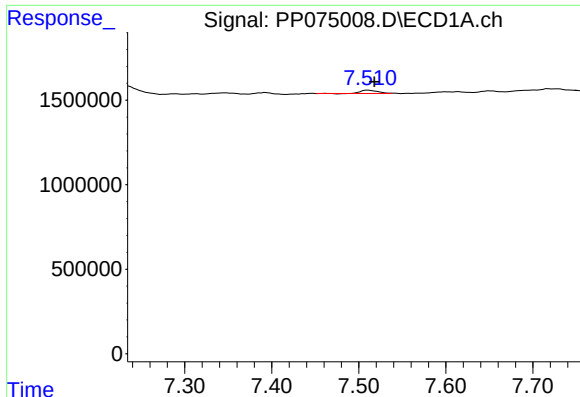

#29 AR-1254-4


R.T.: 7.511 min
Delta R.T.: -0.007 min
Response: 263205
Conc: 3.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

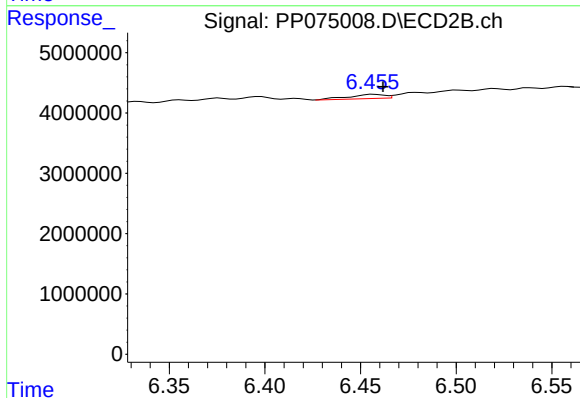


#29 AR-1254-4

R.T.: 6.457 min
Delta R.T.: -0.005 min
Response: 892014
Conc: 1.90 ng/ml

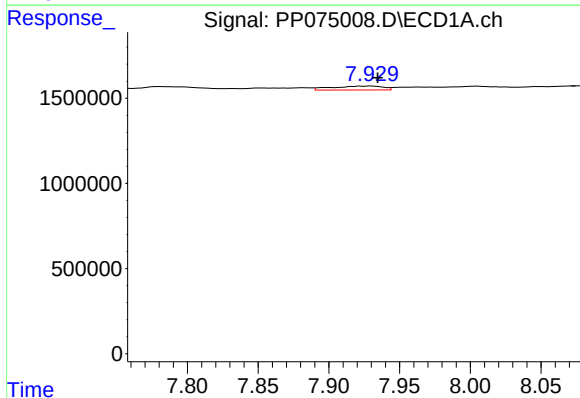


#30 AR-1254-5

R.T.: 7.930 min
Delta R.T.: -0.005 min
Response: 570087
Conc: 6.86 ng/ml

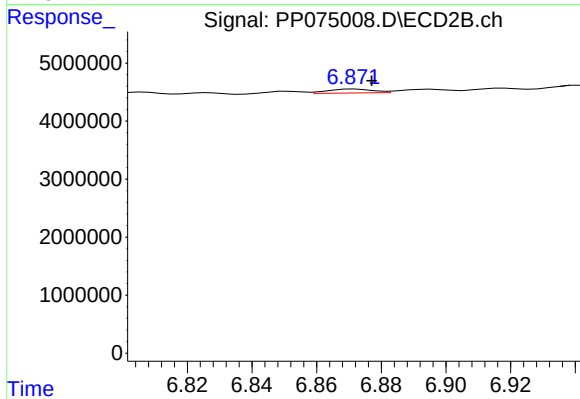

#30 AR-1254-5


R.T.: 6.872 min
Delta R.T.: -0.005 min
Response: 649281
Conc: 1.32 ng/ml

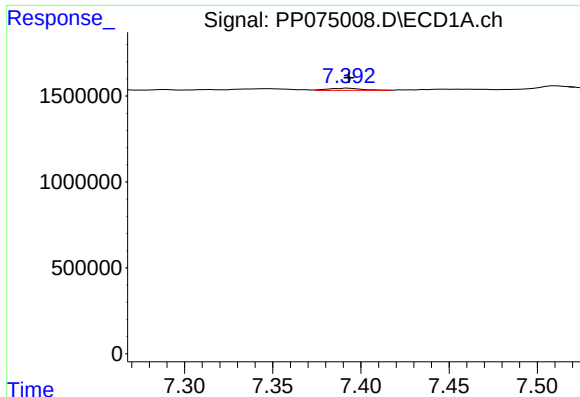

#31 AR-1260-1


R.T.: 7.393 min
Delta R.T.: 0.000 min
Response: 159906
Conc: 2.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

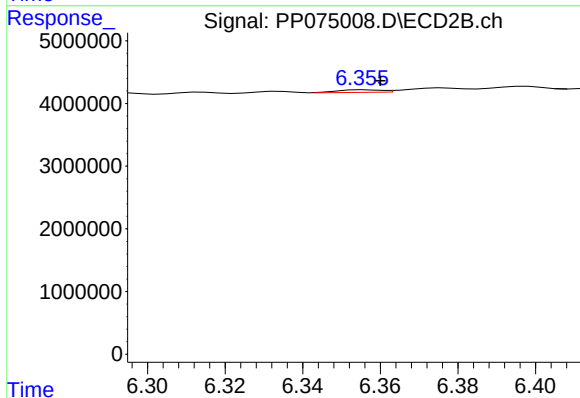


#31 AR-1260-1

R.T.: 6.356 min
Delta R.T.: -0.004 min
Response: 311618
Conc: 0.83 ng/ml

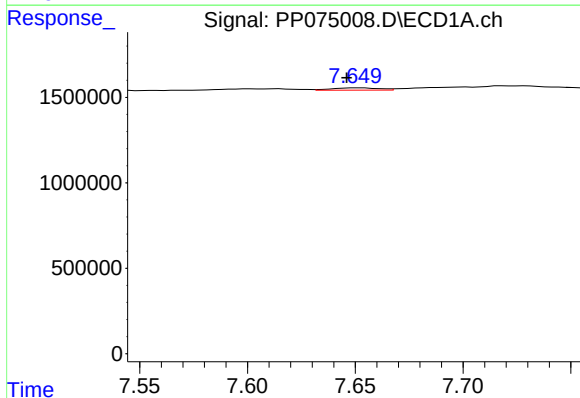


#32 AR-1260-2

R.T.: 7.651 min
Delta R.T.: 0.005 min
Response: 205832
Conc: 2.99 ng/ml

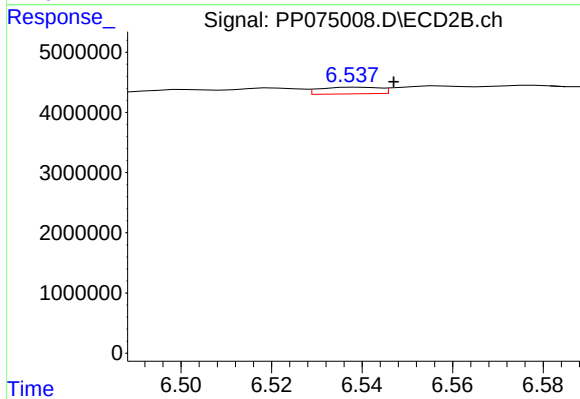

#32 AR-1260-2


R.T.: 6.539 min
Delta R.T.: -0.008 min
Response: 1010425
Conc: 1.91 ng/ml

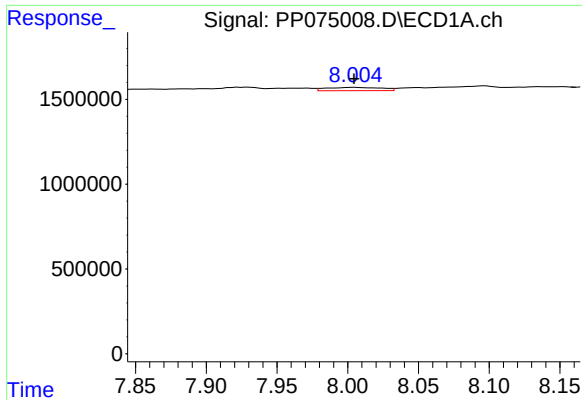

#33 AR-1260-3


R.T.: 8.005 min
Delta R.T.: 0.000 min
Response: 531592
Conc: 10.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

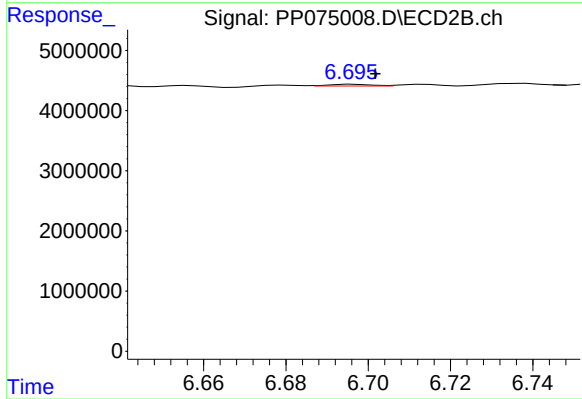


#33 AR-1260-3

R.T.: 6.697 min
Delta R.T.: -0.005 min
Response: 202378
Conc: 0.47 ng/ml

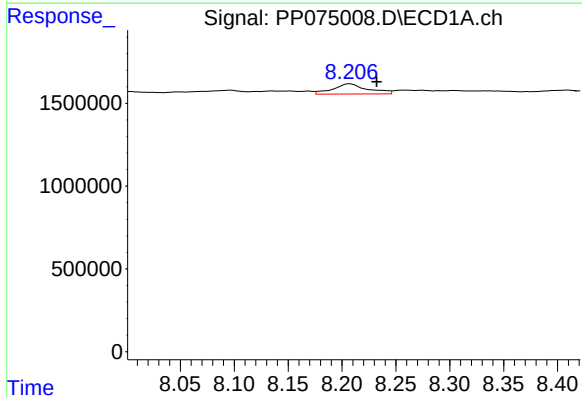


#34 AR-1260-4

R.T.: 8.208 min
Delta R.T.: -0.024 min
Response: 1386043
Conc: 21.73 ng/ml

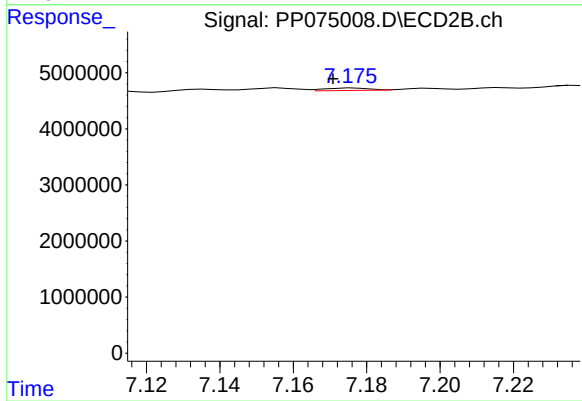

#34 AR-1260-4


R.T.: 7.176 min
Delta R.T.: 0.006 min
Response: 379136
Conc: 0.99 ng/ml

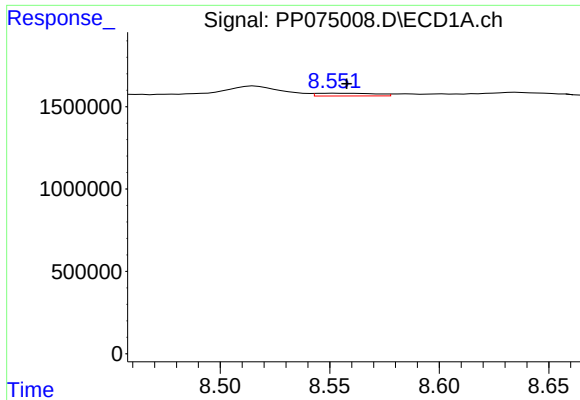

#35 AR-1260-5


R.T.: 8.553 min
Delta R.T.: -0.005 min
Response: 309580
Conc: 2.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

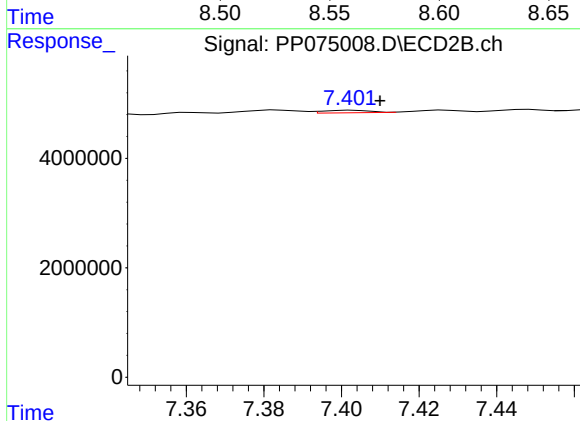


#35 AR-1260-5

R.T.: 7.403 min
Delta R.T.: -0.007 min
Response: 385993
Conc: 0.38 ng/ml

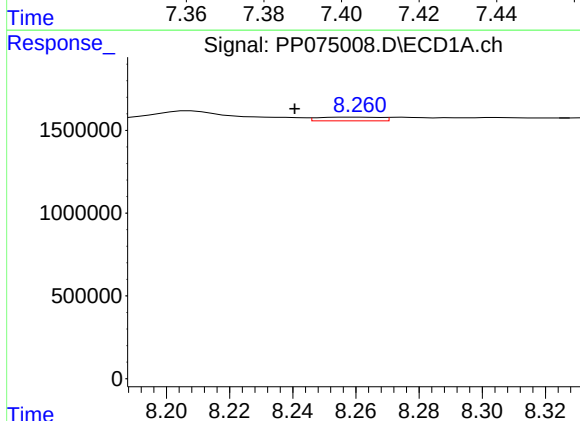


#36 AR-1262-1

R.T.: 8.261 min
Delta R.T.: 0.021 min
Response: 308833
Conc: 4.01 ng/ml

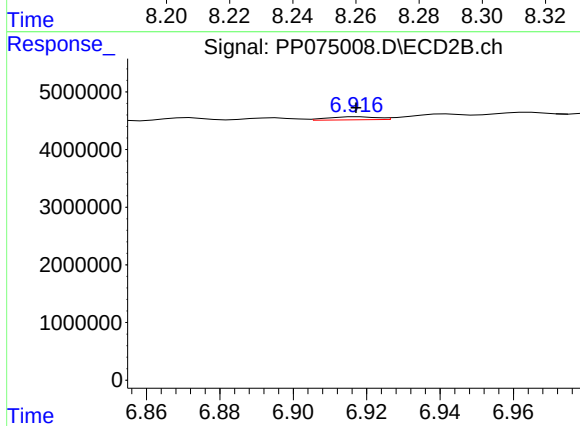

#36 AR-1262-1


R.T.: 6.918 min
Delta R.T.: 0.000 min
Response: 489574
Conc: 0.69 ng/ml

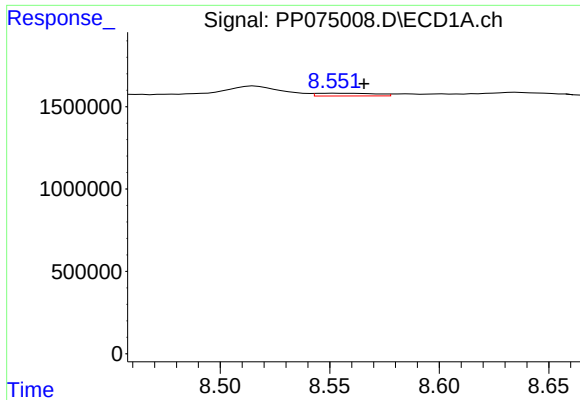

#37 AR-1262-2


R.T.: 8.553 min
Delta R.T.: -0.013 min
Response: 309580
Conc: 2.34 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

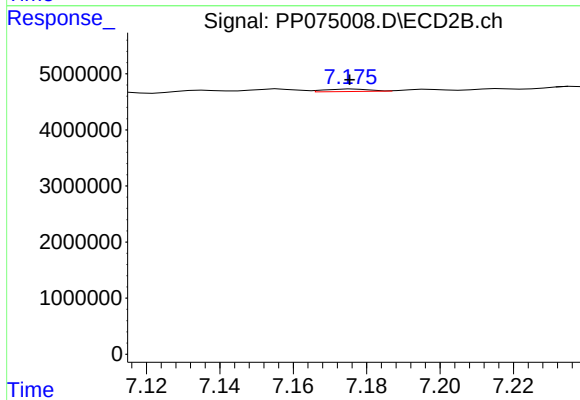


#37 AR-1262-2

R.T.: 7.176 min
Delta R.T.: 0.001 min
Response: 379136
Conc: 0.73 ng/ml

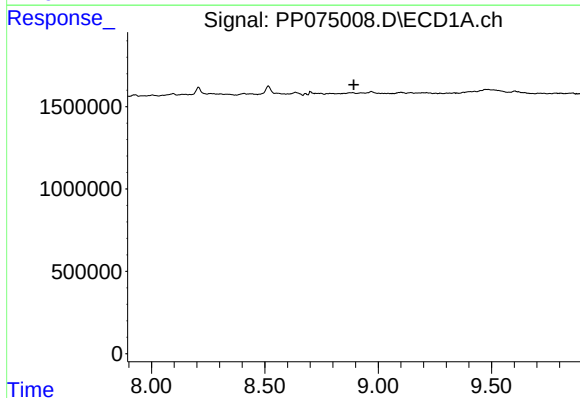


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

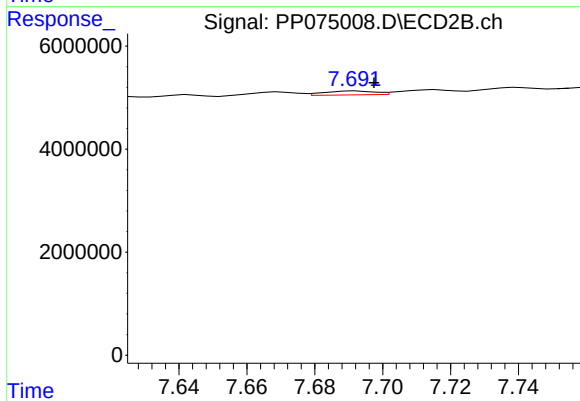

#38 AR-1262-3


R.T.: 7.692 min
Delta R.T.: -0.005 min
Response: 788101
Conc: 1.69 ng/ml

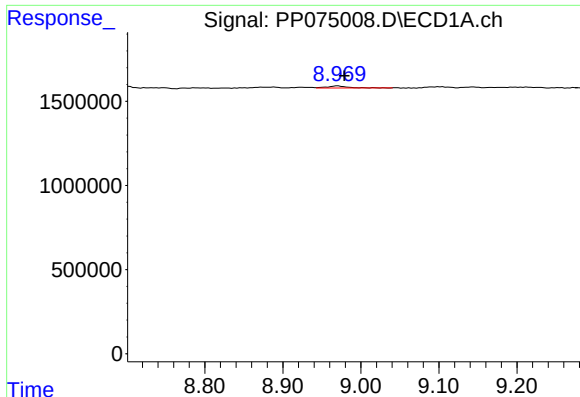

#39 AR-1262-4


R.T.: 8.970 min
Delta R.T.: -0.008 min
Response: 215018
Conc: 2.85 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

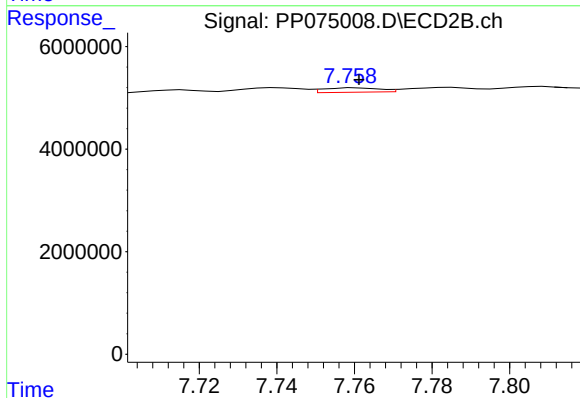


#39 AR-1262-4

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 863589
Conc: 1.05 ng/ml

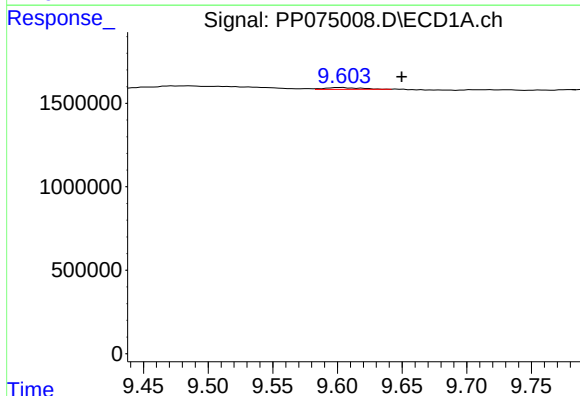


#40 AR-1262-5

R.T.: 9.604 min
Delta R.T.: -0.046 min
Response: 195077
Conc: 3.20 ng/ml

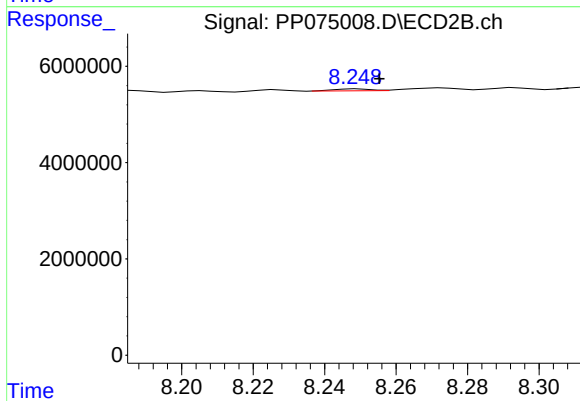

#40 AR-1262-5


R.T.: 8.249 min
Delta R.T.: -0.006 min
Response: 285208
Conc: 0.80 ng/ml

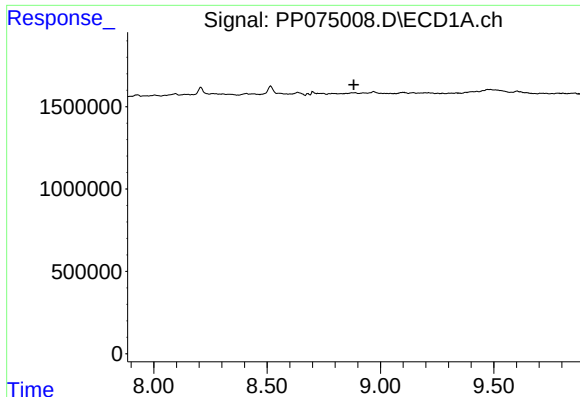

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

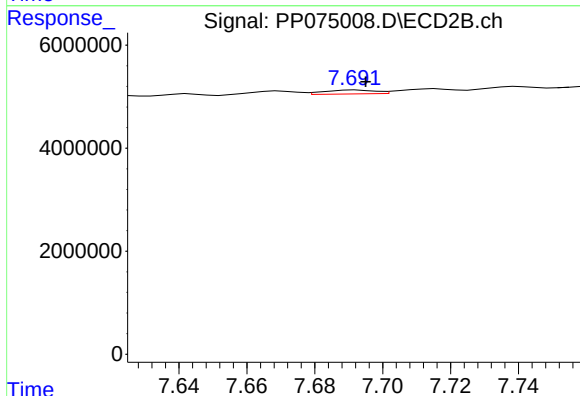


#41 AR-1268-1

R.T.: 7.692 min
Delta R.T.: -0.003 min
Response: 788101
Conc: 0.56 ng/ml

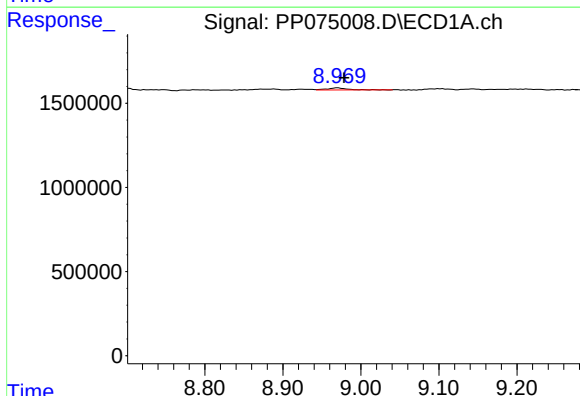


#42 AR-1268-2

R.T.: 8.970 min
Delta R.T.: -0.008 min
Response: 215018
Conc: 1.47 ng/ml

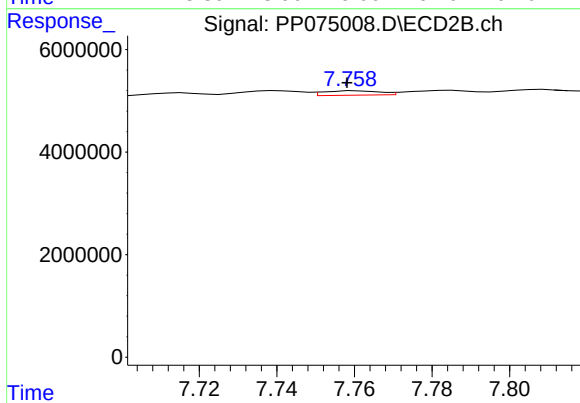

#42 AR-1268-2


R.T.: 7.760 min
Delta R.T.: 0.002 min
Response: 863589
Conc: 0.63 ng/ml

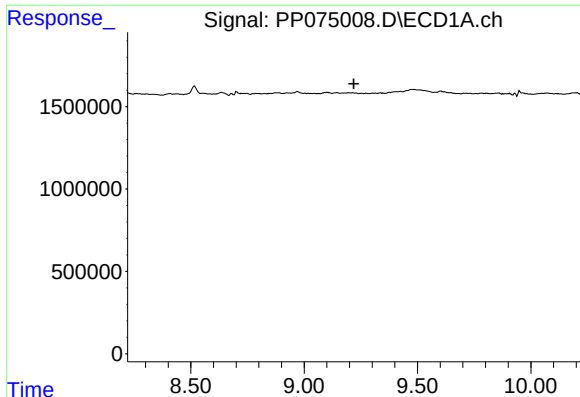

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

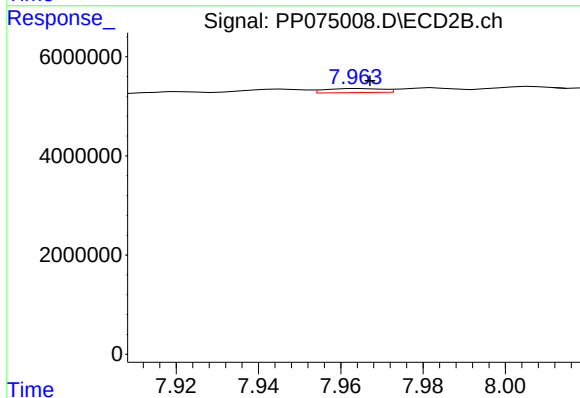


#43 AR-1268-3

R.T.: 7.965 min
Delta R.T.: -0.003 min
Response: 807192
Conc: 0.77 ng/ml

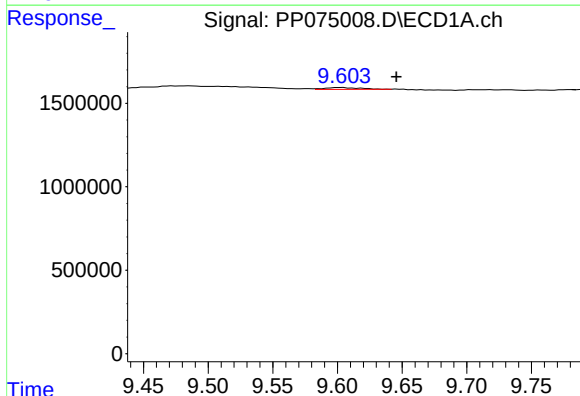


#44 AR-1268-4

R.T.: 9.604 min
Delta R.T.: -0.041 min
Response: 195077
Conc: 2.90 ng/ml

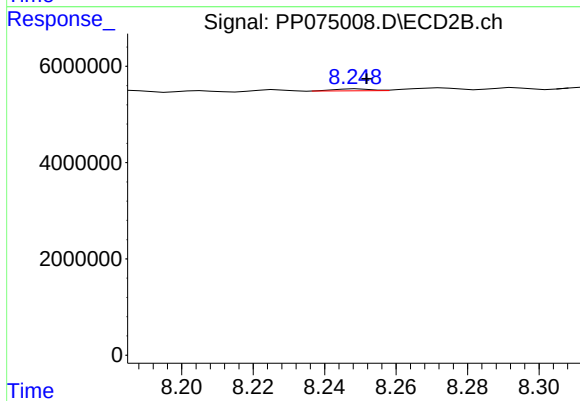

#44 AR-1268-4


R.T.: 8.249 min
Delta R.T.: -0.003 min
Response: 285208
Conc: 0.74 ng/ml

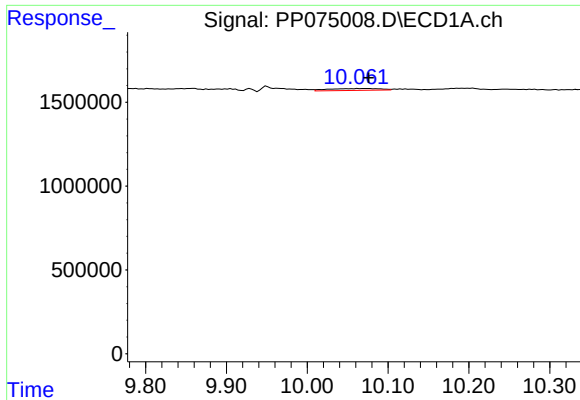

#45 AR-1268-5

R.T.: 10.075 min
Delta R.T.: 0.000 min
Response: 500162
Conc: 1.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-G

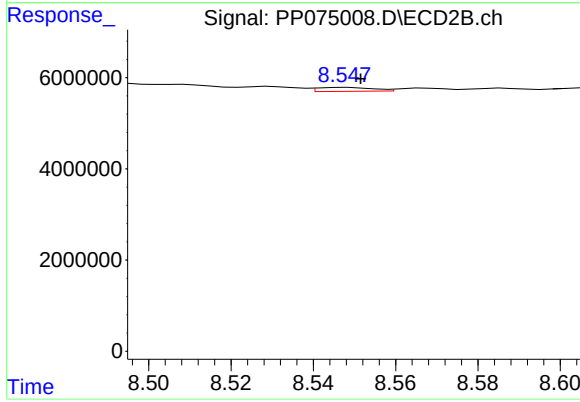

#45 AR-1268-5

R.T.: 8.548 min
Delta R.T.: -0.003 min
Response: 822462
Conc: 0.26 ng/ml