

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075009.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 15:30
 Operator : YP\AJ
 Sample : Q3034-08
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-H

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:50:28 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.653	3.799	20102162	77487714	16.427	16.025
2)	SA Decachlor...	10.425	8.805	16554860	97212354	16.764	12.963
Target Compounds							
3)	L1 AR-1016-1	5.804	4.896	47516344	546.1E6	1077.741	1072.069
4)	L1 AR-1016-2	5.825	4.955	66918377	293.4E6	1064.873	1232.874
5)	L1 AR-1016-3	5.888	5.074	48964358	175.2E6	1090.182	1270.706
6)	L1 AR-1016-4	5.986	5.115	45370529	194.5E6	1289.602	1391.552
7)	L1 AR-1016-5	6.278	5.329	59359871	281.0E6	1788.698	1691.980
8)	L2 AR-1221-1	4.850	4.012	1140122	2001485	64.806	32.351 #
9)	L2 AR-1221-2	4.938	4.093	1494130	3904624	111.860	86.362
10)	L2 AR-1221-3	5.014	4.171	4749600	18198892	125.277	110.770
11)	L3 AR-1232-1	5.014	4.171	4749600	18198892	156.371	142.073
12)	L3 AR-1232-2	5.540	4.896	22511327	546.1E6	1428.544	2355.815 #
13)	L3 AR-1232-3	5.825	5.074	66918377	175.2E6	2190.907	2917.676 #
14)	L3 AR-1232-4	5.986	5.157	45370529	333.6E6	2627.240	4525.894 #
15)	L3 AR-1232-5	6.075	5.329	41085843	281.0E6	3165.086	4526.296 #
16)	L4 AR-1242-1	5.804	4.896	47516344	546.1E6	1241.439	1294.745
17)	L4 AR-1242-2	5.825	4.955	66918377	293.4E6	1184.774	1465.145
18)	L4 AR-1242-3	5.888	5.074	48964358	175.2E6	1205.932	1481.298
19)	L4 AR-1242-4	5.986	5.157	45370529	333.6E6	1429.360	1949.012 #
20)	L4 AR-1242-5	6.714	5.678	30010017	216.2E6	831.980	1167.805 #
21)	L5 AR-1248-1	5.804	4.896	47516344	546.1E6	1572.139	1977.463 #
22)	L5 AR-1248-2	6.075	5.115	41085843	194.5E6	953.355	1100.636
23)	L5 AR-1248-3	6.278	5.157	59359871	333.6E6	1270.991	1468.252
24)	L5 AR-1248-4	6.675	5.329	31964857	281.0E6	581.171	1288.911 #
25)	L5 AR-1248-5	6.714	5.719	30010017	202.5E6	541.009	551.264
26)	L6 AR-1254-1	6.650	5.678	25545791	216.2E6	438.408	453.599
27)	L6 AR-1254-2	6.871	5.824	21290815	32301576	260.866	91.731 #
28)	L6 AR-1254-3	7.229	6.227	3089726	12775294	34.636	20.612 #
29)	L6 AR-1254-4	7.511	6.456	1215525	3761043	18.441	8.026 #
30)	L6 AR-1254-5	7.928	6.876	970367	1231463	11.679	2.511 #
31)	L7 AR-1260-1	7.393	6.371	351249	2812002	6.076	7.494
32)	L7 AR-1260-2	7.646	6.541	647498	1650584	9.395	3.121 #
33)	L7 AR-1260-3	8.003	6.698	1137550	998844	21.924	2.307 #
34)	L7 AR-1260-4	8.207	7.177	2419637	379220	37.930	0.994 #
35)	L7 AR-1260-5	8.593	7.419	195517	419464	1.724	0.418 #
36)	L8 AR-1262-1	8.261	6.914	251952	338450	3.271	0.479 #
37)	L8 AR-1262-2	8.593	7.177	195517	379220	1.477	0.728 #
38)	L8 AR-1262-3	0.000	7.689	0	1178466	N.D.	2.527 #
39)	L8 AR-1262-4	8.976	7.767	162318	670805	2.155	0.816 #
40)	L8 AR-1262-5	9.603f	8.255	239929	124137	3.936	0.346 #
41)	L9 AR-1268-1	0.000	7.689	0	1178466	N.D.	0.835 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 15:30
Operator : YP\AJ
Sample : Q3034-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:50:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.976	7.749	162318	790422	1.106	0.580 #
43)	L9 AR-1268-3	0.000	7.959	0	955694	N.D.	0.916 #
44)	L9 AR-1268-4	9.603f	8.255	239929	124137	3.567	0.324 #
45)	L9 AR-1268-5	0.000	8.546	0	1076391	N.D.	0.343 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075009.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 15:30
Operator : YP\AJ
Sample : Q3034-08
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:50:28 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

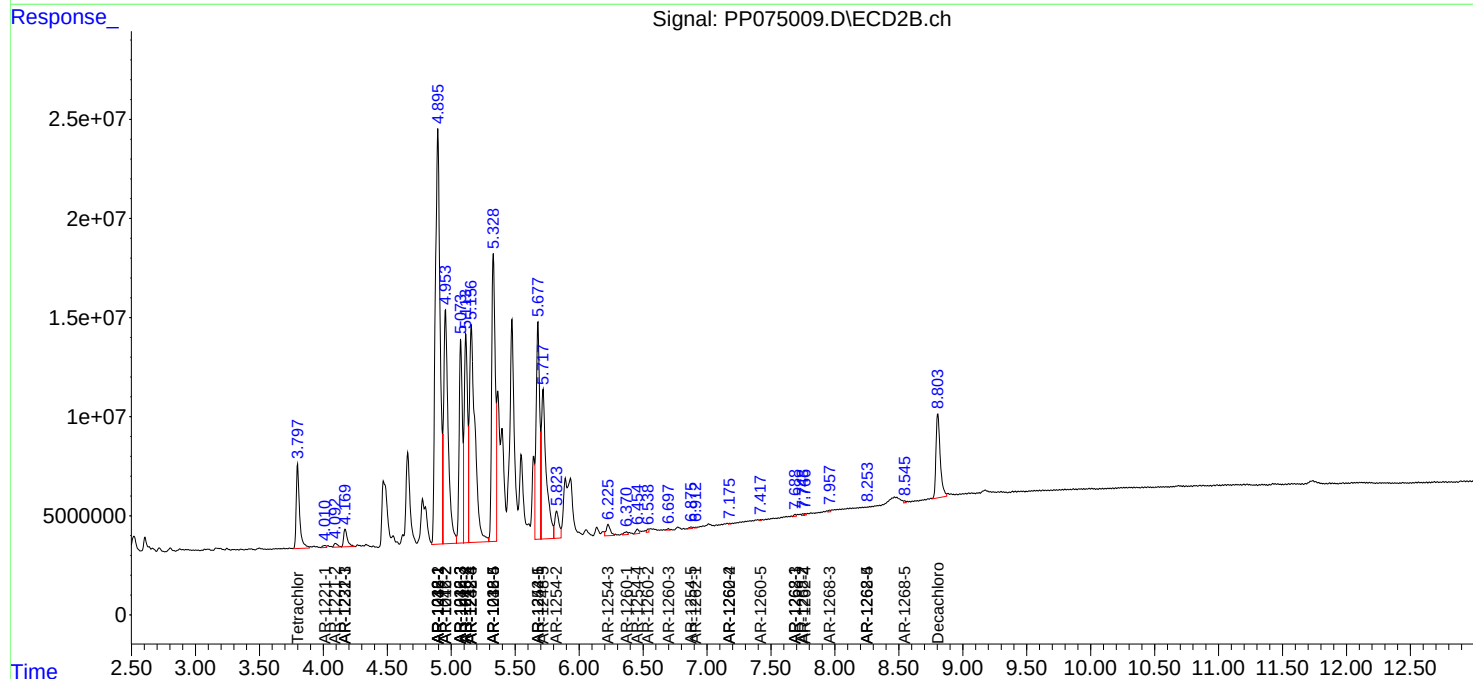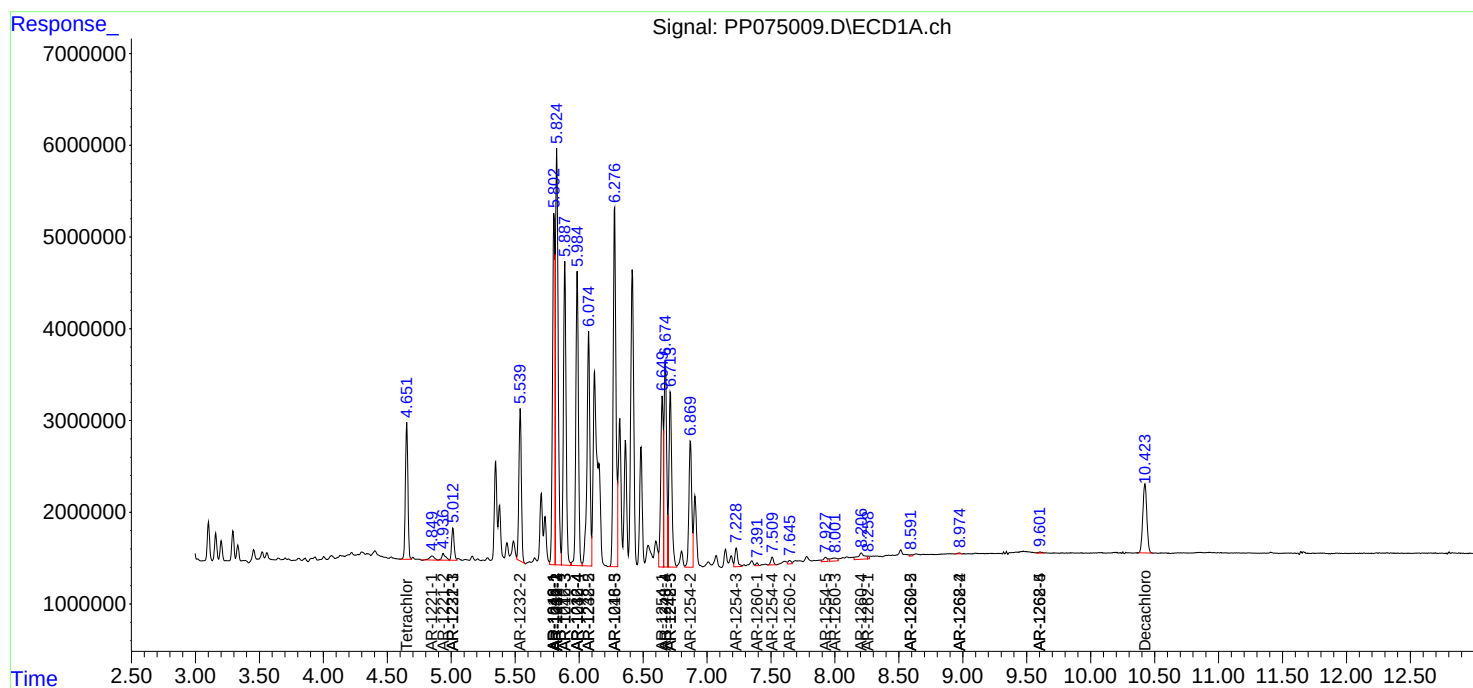


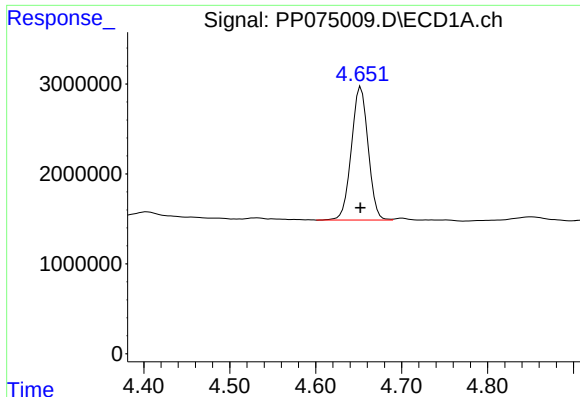

#1 Tetrachloro-m-xylene


R.T.: 4.653 min
Delta R.T.: 0.000 min
Response: 20102162
Conc: 16.43 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

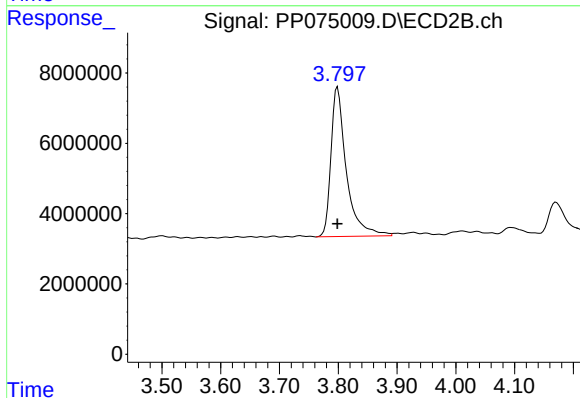


#1 Tetrachloro-m-xylene

R.T.: 3.799 min
Delta R.T.: 0.000 min
Response: 77487714
Conc: 16.03 ng/ml

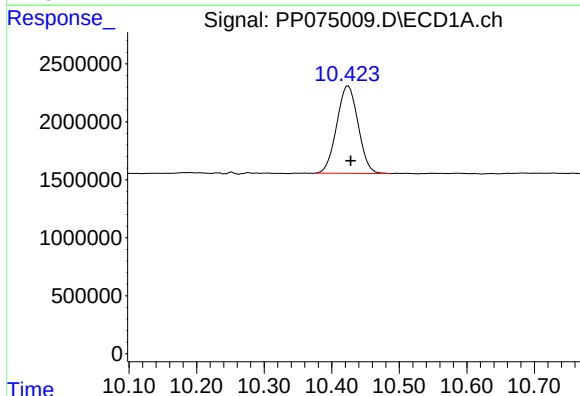


#2 Decachlorobiphenyl

R.T.: 10.425 min
Delta R.T.: -0.004 min
Response: 16554860
Conc: 16.76 ng/ml

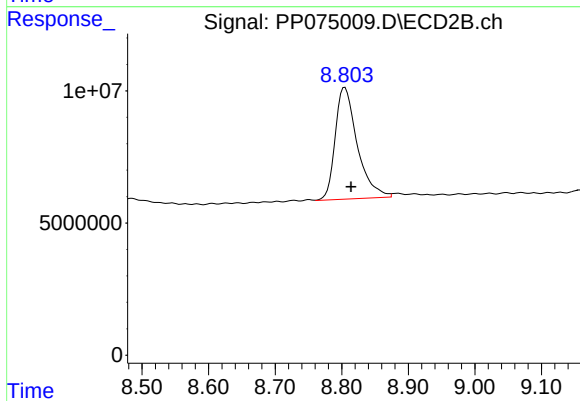

#2 Decachlorobiphenyl


R.T.: 8.805 min
Delta R.T.: -0.009 min
Response: 97212354
Conc: 12.96 ng/ml

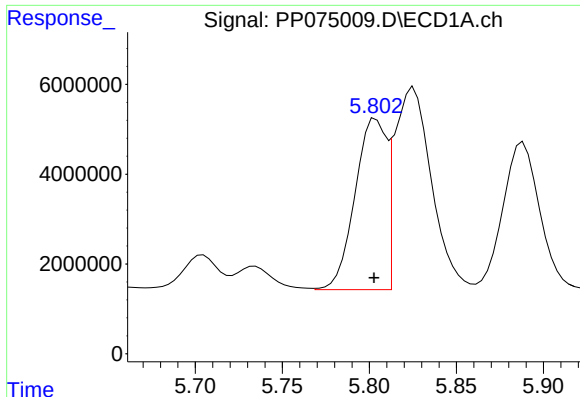

#3 AR-1016-1


R.T.: 5.804 min
Delta R.T.: 0.001 min
Response: 47516344
Conc: 1077.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

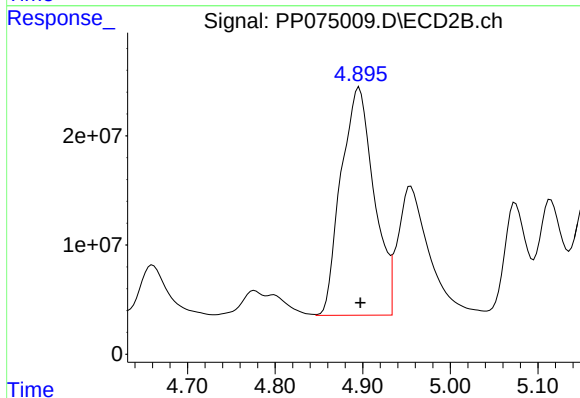


#3 AR-1016-1

R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 546062224
Conc: 1072.07 ng/ml

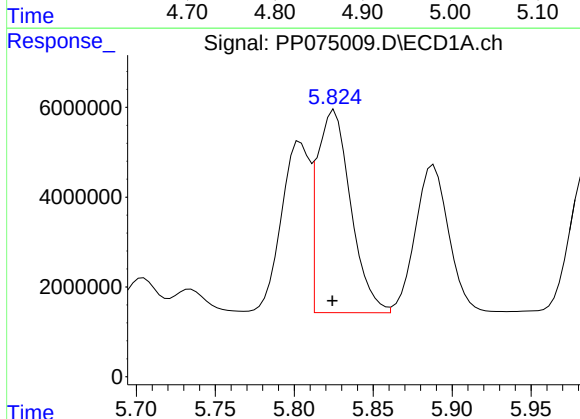


#4 AR-1016-2

R.T.: 5.825 min
Delta R.T.: 0.001 min
Response: 66918377
Conc: 1064.87 ng/ml

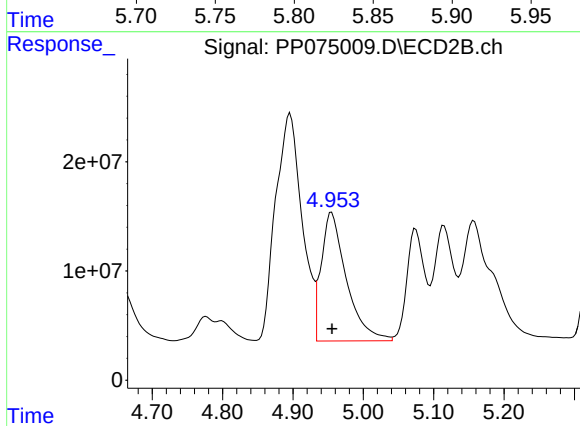

#4 AR-1016-2


R.T.: 4.955 min
Delta R.T.: 0.000 min
Response: 293442945
Conc: 1232.87 ng/ml

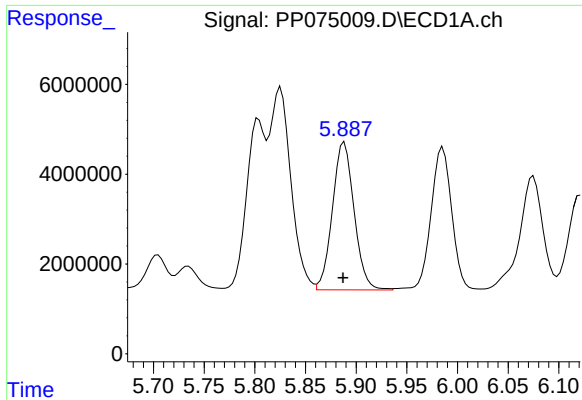

#5 AR-1016-3


R.T.: 5.888 min
Delta R.T.: 0.001 min
Response: 48964358
Conc: 1090.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

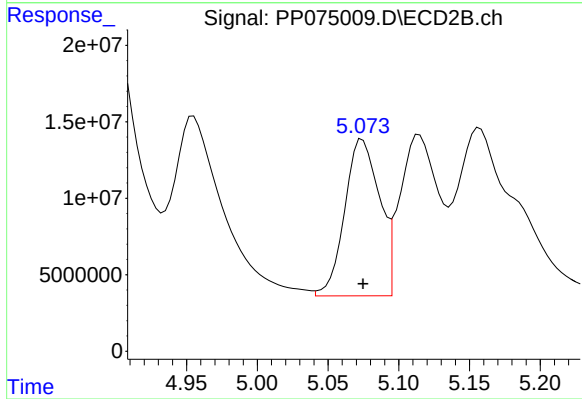


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: 0.000 min
Response: 175234918
Conc: 1270.71 ng/ml

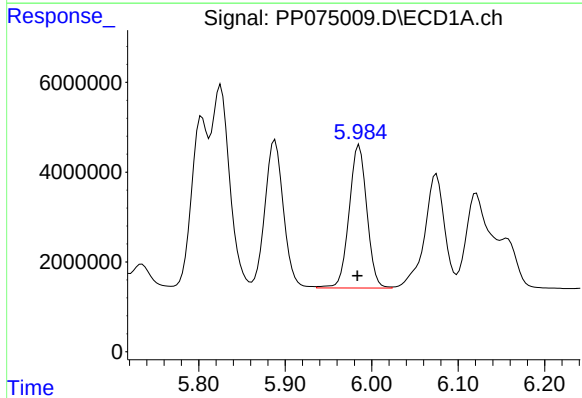


#6 AR-1016-4

R.T.: 5.986 min
Delta R.T.: 0.002 min
Response: 45370529
Conc: 1289.60 ng/ml

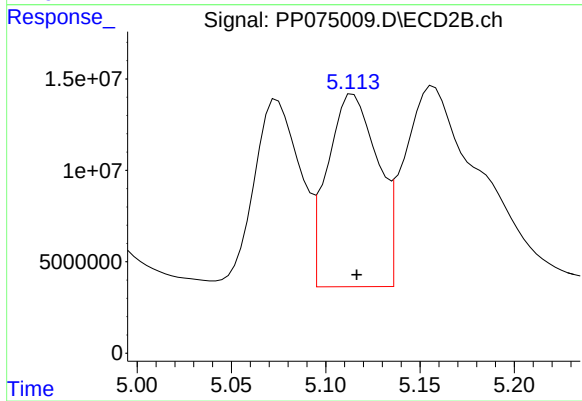

#6 AR-1016-4


R.T.: 5.115 min
Delta R.T.: -0.002 min
Response: 194543508
Conc: 1391.55 ng/ml

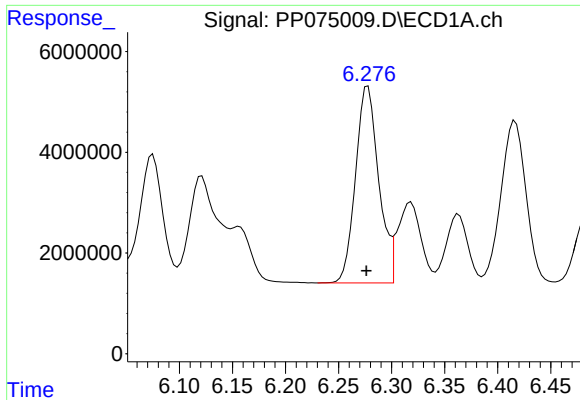

#7 AR-1016-5


R.T.: 6.278 min
Delta R.T.: 0.001 min
Response: 59359871
Conc: 1788.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

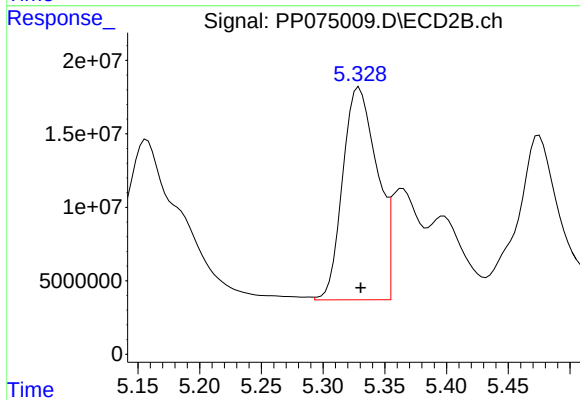


#7 AR-1016-5

R.T.: 5.329 min
Delta R.T.: -0.001 min
Response: 281009667
Conc: 1691.98 ng/ml

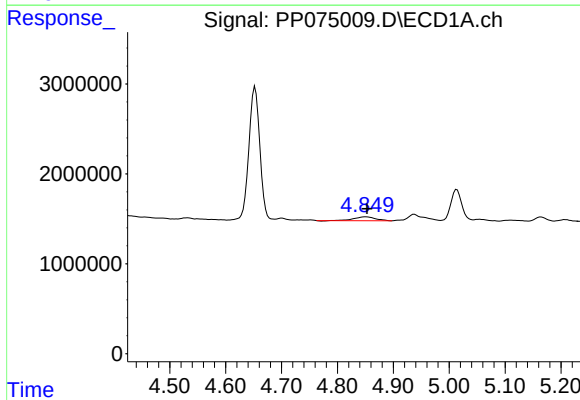


#8 AR-1221-1

R.T.: 4.850 min
Delta R.T.: -0.003 min
Response: 1140122
Conc: 64.81 ng/ml

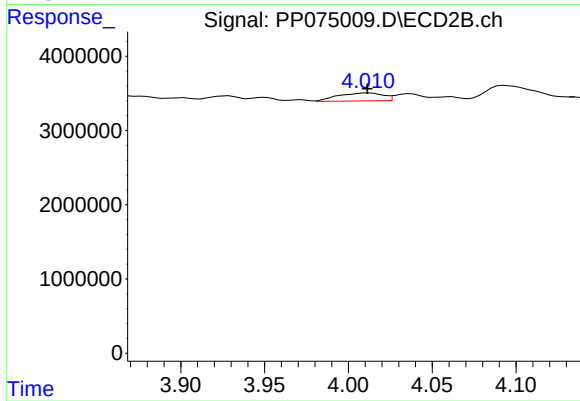

#8 AR-1221-1


R.T.: 4.012 min
Delta R.T.: 0.000 min
Response: 2001485
Conc: 32.35 ng/ml

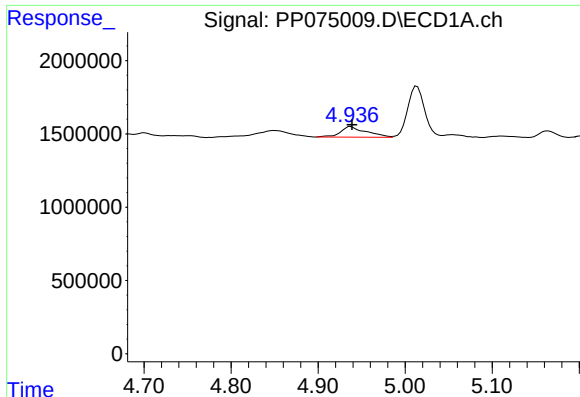

#9 AR-1221-2


R.T.: 4.938 min
Delta R.T.: -0.002 min
Response: 1494130
Conc: 111.86 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

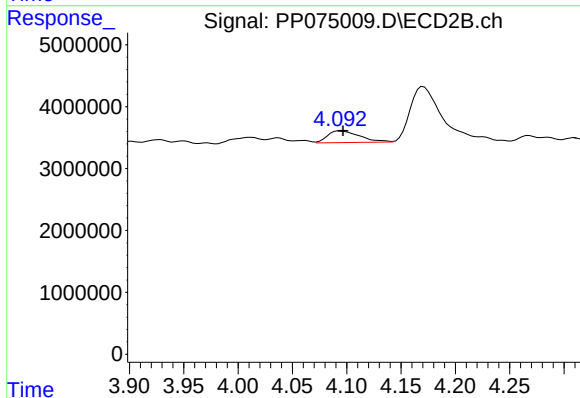


#9 AR-1221-2

R.T.: 4.093 min
Delta R.T.: -0.003 min
Response: 3904624
Conc: 86.36 ng/ml

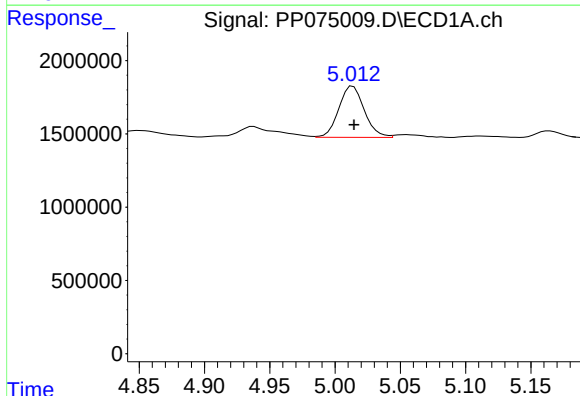


#10 AR-1221-3

R.T.: 5.014 min
Delta R.T.: 0.000 min
Response: 4749600
Conc: 125.28 ng/ml

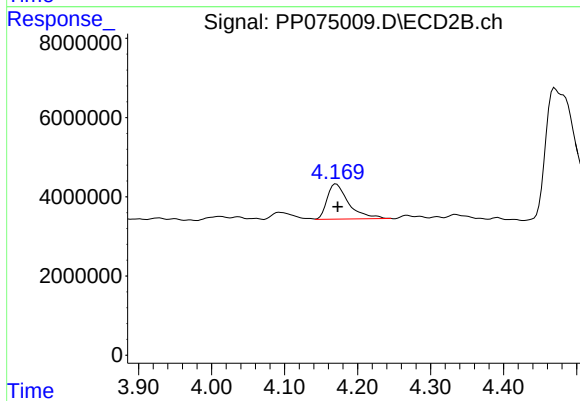

#10 AR-1221-3


R.T.: 4.171 min
Delta R.T.: -0.002 min
Response: 18198892
Conc: 110.77 ng/ml

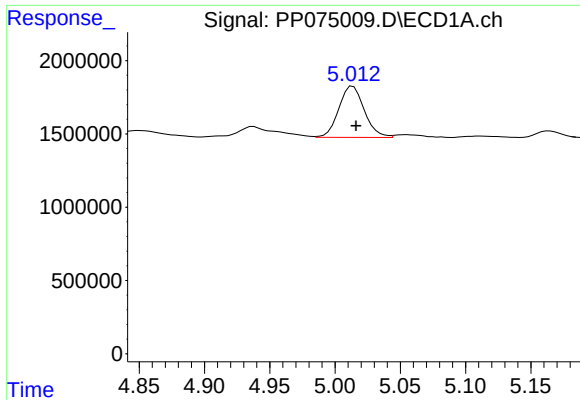

#11 AR-1232-1


R.T.: 5.014 min
Delta R.T.: -0.002 min
Response: 4749600
Conc: 156.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

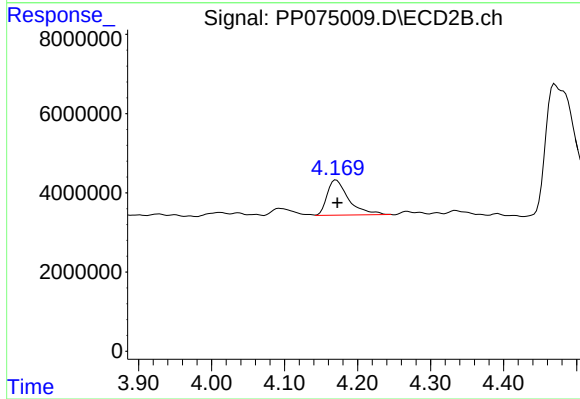


#11 AR-1232-1

R.T.: 4.171 min
Delta R.T.: -0.002 min
Response: 18198892
Conc: 142.07 ng/ml

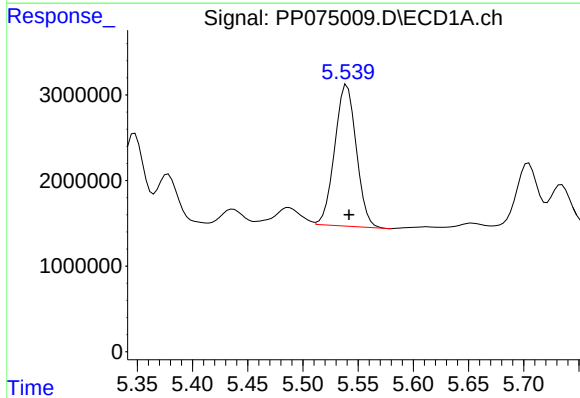


#12 AR-1232-2

R.T.: 5.540 min
Delta R.T.: -0.002 min
Response: 22511327
Conc: 1428.54 ng/ml

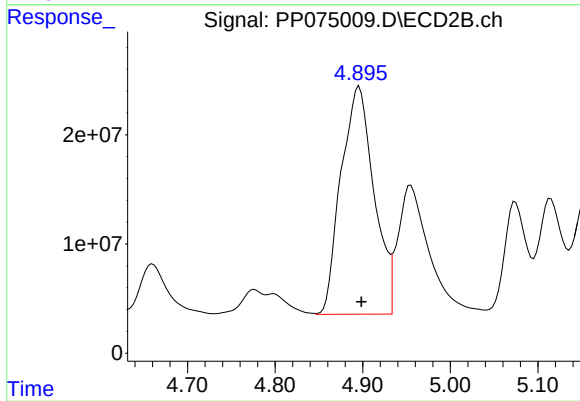

#12 AR-1232-2


R.T.: 4.896 min
Delta R.T.: -0.003 min
Response: 546062224
Conc: 2355.81 ng/ml

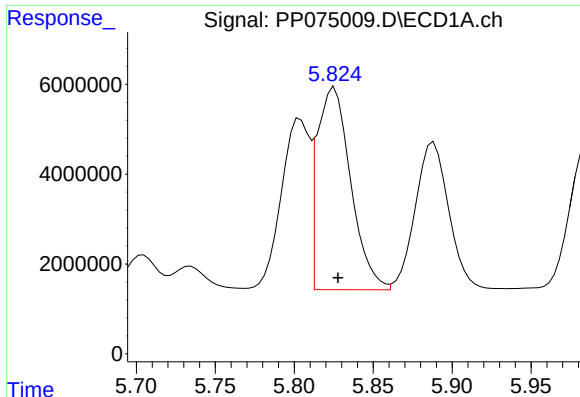

#13 AR-1232-3


R.T.: 5.825 min
Delta R.T.: -0.002 min
Response: 66918377
Conc: 2190.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

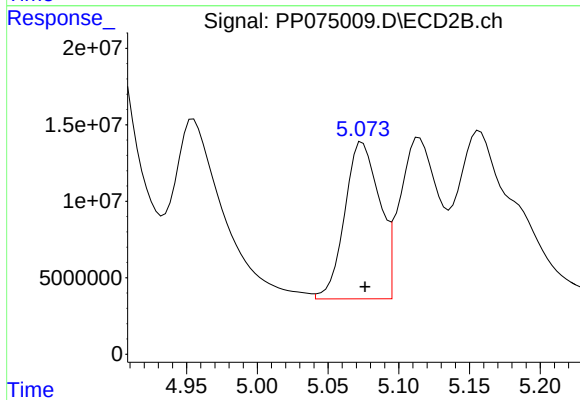


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 175234918
Conc: 2917.68 ng/ml

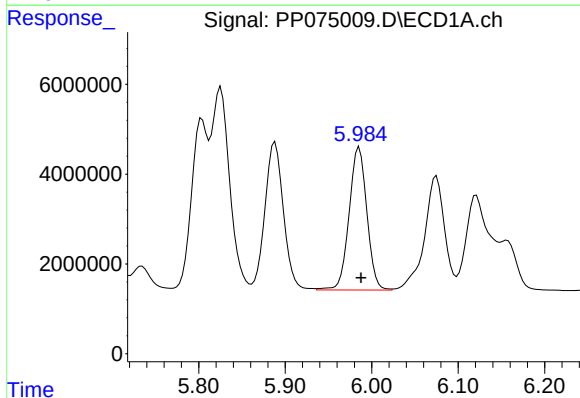


#14 AR-1232-4

R.T.: 5.986 min
Delta R.T.: -0.002 min
Response: 45370529
Conc: 2627.24 ng/ml

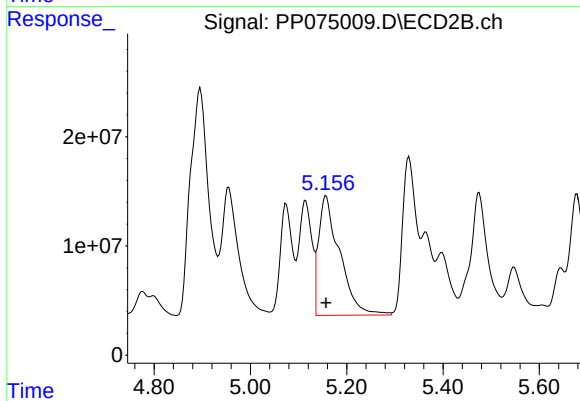

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 333591795
Conc: 4525.89 ng/ml

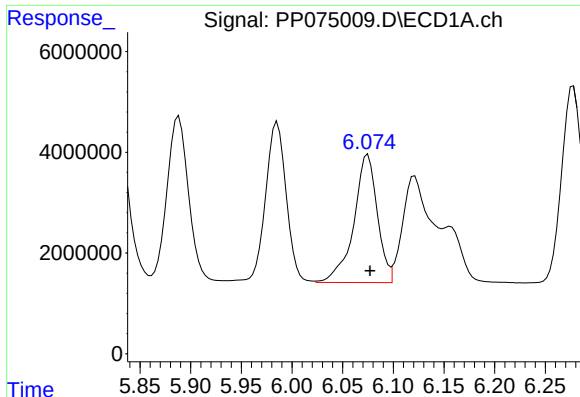

#15 AR-1232-5


R.T.: 6.075 min
Delta R.T.: -0.002 min
Response: 41085843
Conc: 3165.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

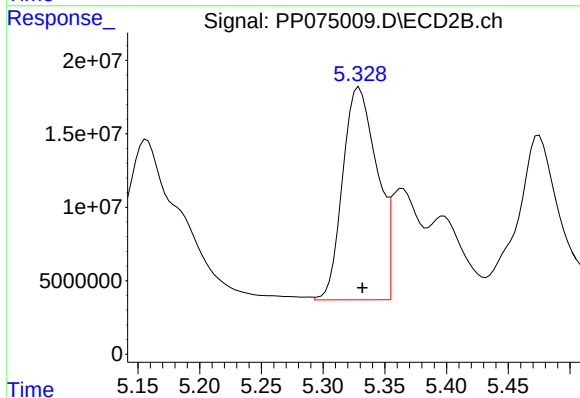


#15 AR-1232-5

R.T.: 5.329 min
Delta R.T.: -0.003 min
Response: 281009667
Conc: 4526.30 ng/ml

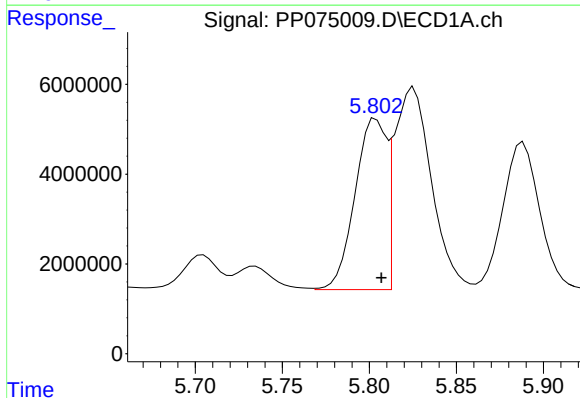


#16 AR-1242-1

R.T.: 5.804 min
Delta R.T.: -0.003 min
Response: 47516344
Conc: 1241.44 ng/ml

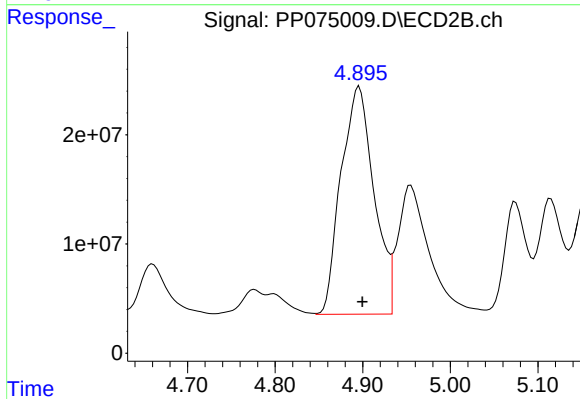

#16 AR-1242-1


R.T.: 4.896 min
Delta R.T.: -0.003 min
Response: 546062224
Conc: 1294.74 ng/ml

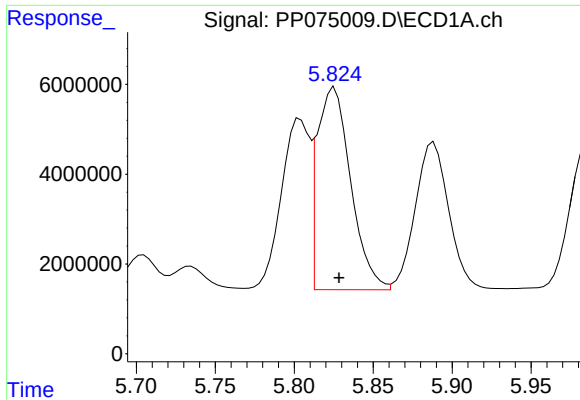

#17 AR-1242-2


R.T.: 5.825 min
Delta R.T.: -0.003 min
Response: 66918377
Conc: 1184.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

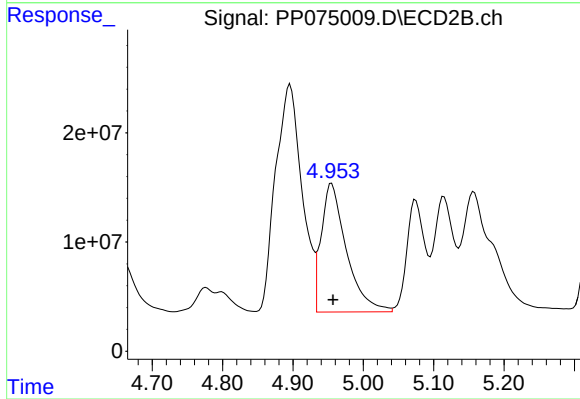


#17 AR-1242-2

R.T.: 4.955 min
Delta R.T.: -0.002 min
Response: 293442945
Conc: 1465.14 ng/ml

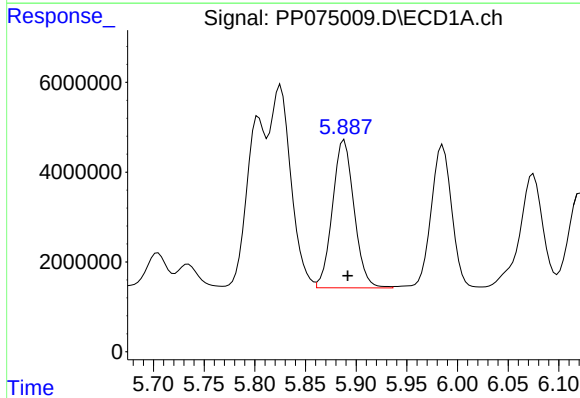


#18 AR-1242-3

R.T.: 5.888 min
Delta R.T.: -0.003 min
Response: 48964358
Conc: 1205.93 ng/ml

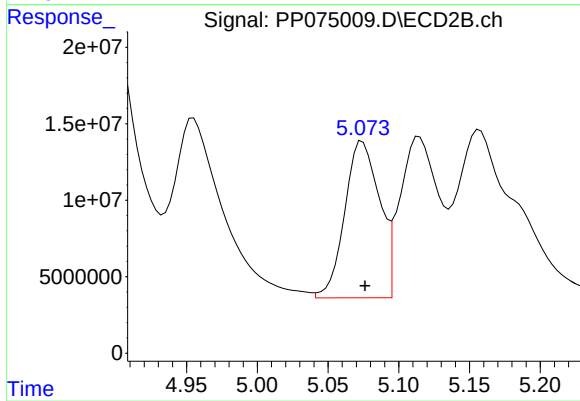

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 175234918
Conc: 1481.30 ng/ml

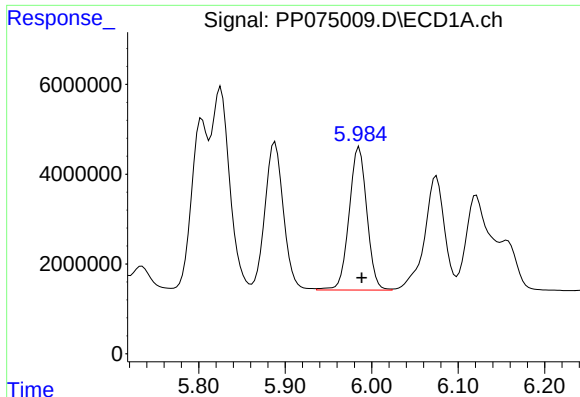

#19 AR-1242-4


R.T.: 5.986 min
Delta R.T.: -0.003 min
Response: 45370529
Conc: 1429.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

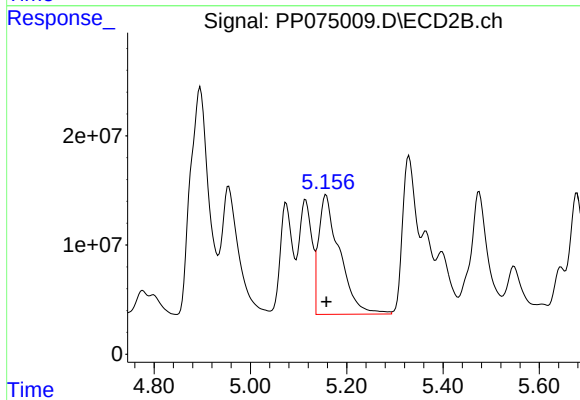


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 333591795
Conc: 1949.01 ng/ml

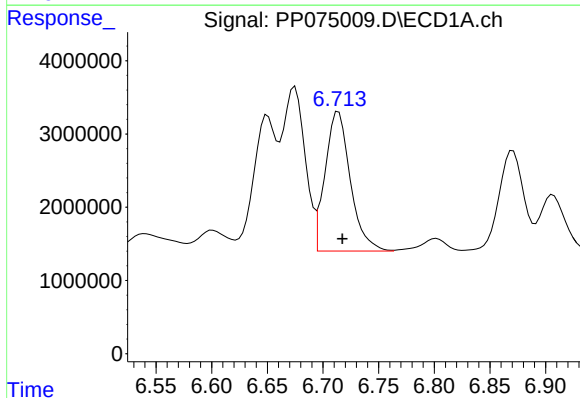


#20 AR-1242-5

R.T.: 6.714 min
Delta R.T.: -0.004 min
Response: 30010017
Conc: 831.98 ng/ml

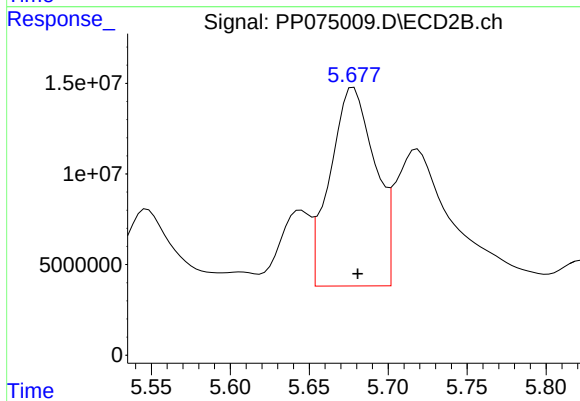

#20 AR-1242-5


R.T.: 5.678 min
Delta R.T.: -0.003 min
Response: 216235514
Conc: 1167.80 ng/ml

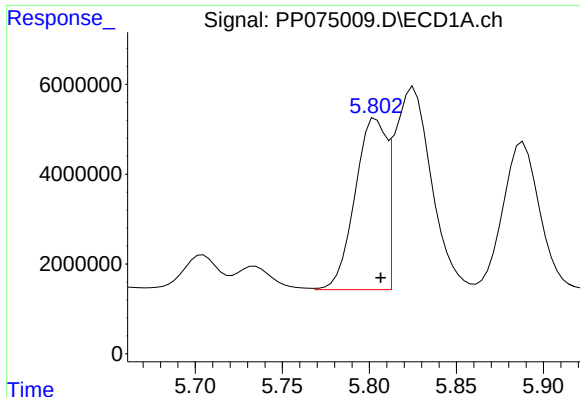

#21 AR-1248-1


R.T.: 5.804 min
Delta R.T.: -0.003 min
Response: 47516344
Conc: 1572.14 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

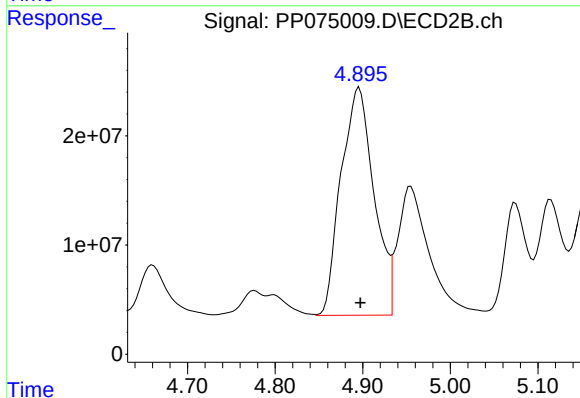


#21 AR-1248-1

R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 546062224
Conc: 1977.46 ng/ml

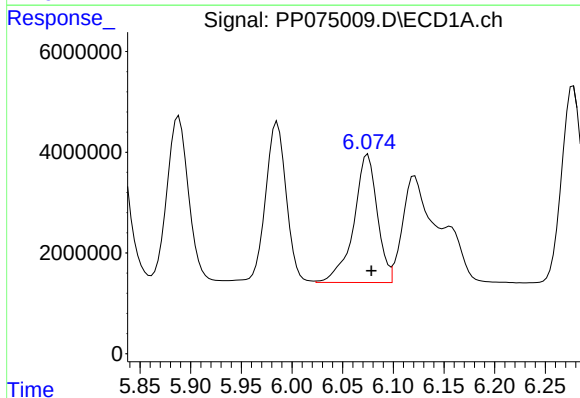


#22 AR-1248-2

R.T.: 6.075 min
Delta R.T.: -0.003 min
Response: 41085843
Conc: 953.36 ng/ml

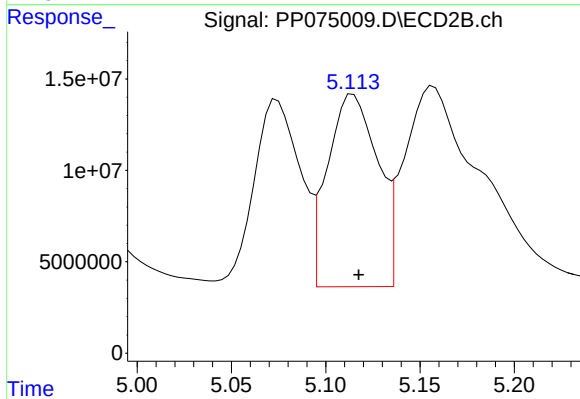

#22 AR-1248-2


R.T.: 5.115 min
Delta R.T.: -0.003 min
Response: 194543508
Conc: 1100.64 ng/ml

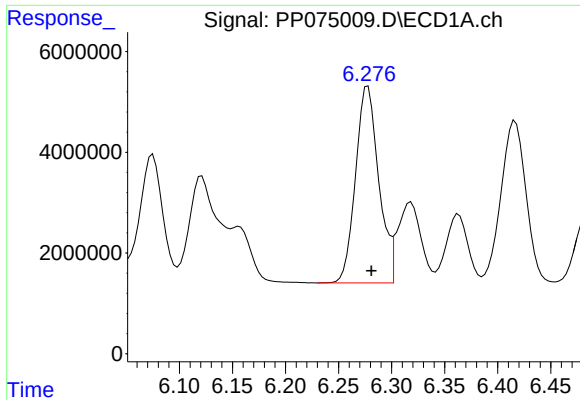

#23 AR-1248-3


R.T.: 6.278 min
Delta R.T.: -0.003 min
Response: 59359871
Conc: 1270.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

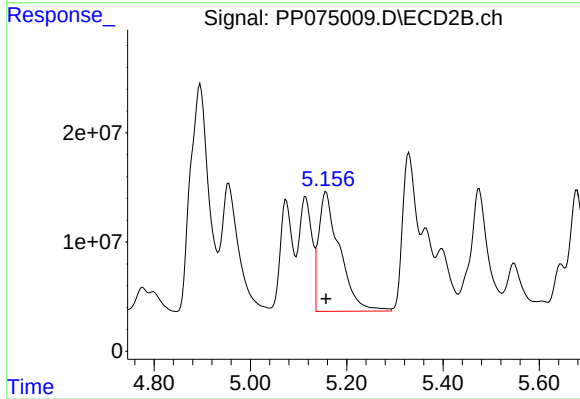


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 333591795
Conc: 1468.25 ng/ml

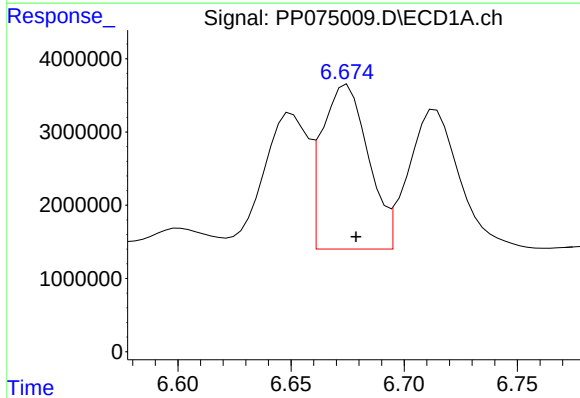


#24 AR-1248-4

R.T.: 6.675 min
Delta R.T.: -0.004 min
Response: 31964857
Conc: 581.17 ng/ml

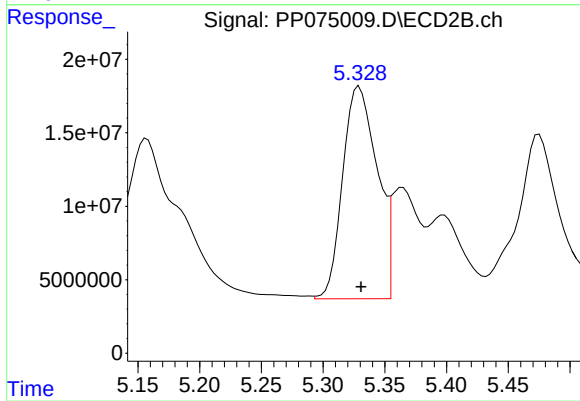

#24 AR-1248-4


R.T.: 5.329 min
Delta R.T.: -0.002 min
Response: 281009667
Conc: 1288.91 ng/ml

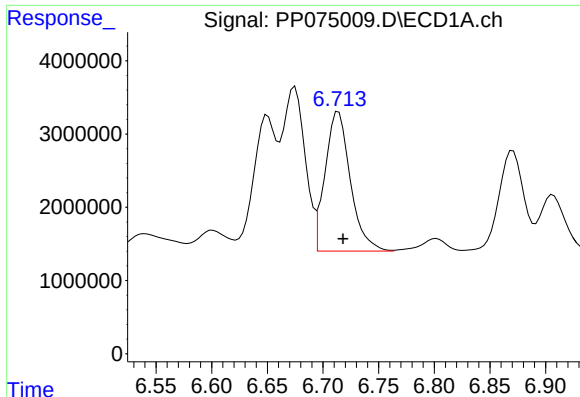

#25 AR-1248-5


R.T.: 6.714 min
Delta R.T.: -0.004 min
Response: 30010017
Conc: 541.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

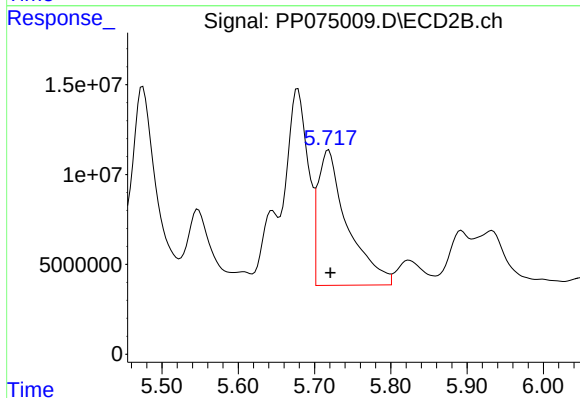


#25 AR-1248-5

R.T.: 5.719 min
Delta R.T.: -0.002 min
Response: 202491284
Conc: 551.26 ng/ml

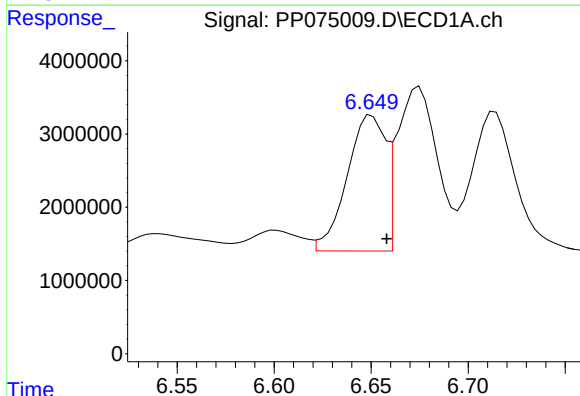


#26 AR-1254-1

R.T.: 6.650 min
Delta R.T.: -0.008 min
Response: 25545791
Conc: 438.41 ng/ml

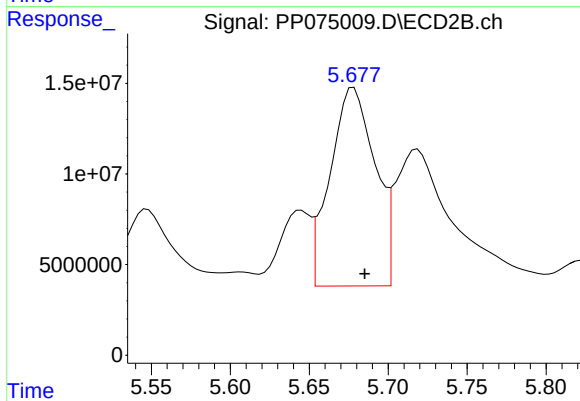

#26 AR-1254-1


R.T.: 5.678 min
Delta R.T.: -0.007 min
Response: 216235514
Conc: 453.60 ng/ml

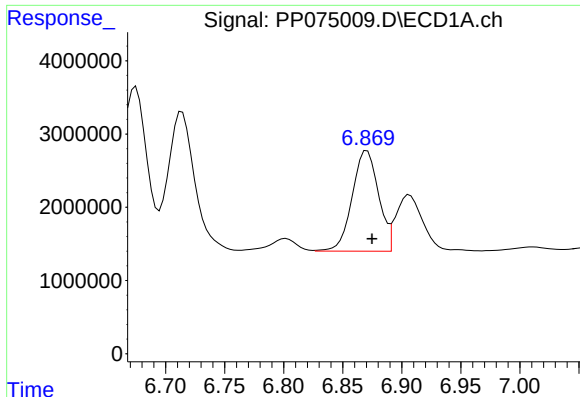

#27 AR-1254-2


R.T.: 6.871 min
Delta R.T.: -0.004 min
Response: 21290815
Conc: 260.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

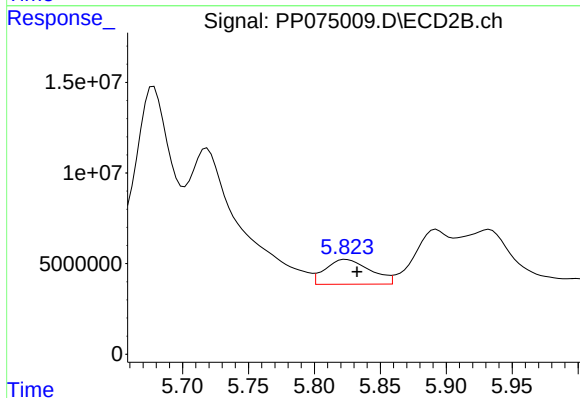


#27 AR-1254-2

R.T.: 5.824 min
Delta R.T.: -0.008 min
Response: 32301576
Conc: 91.73 ng/ml

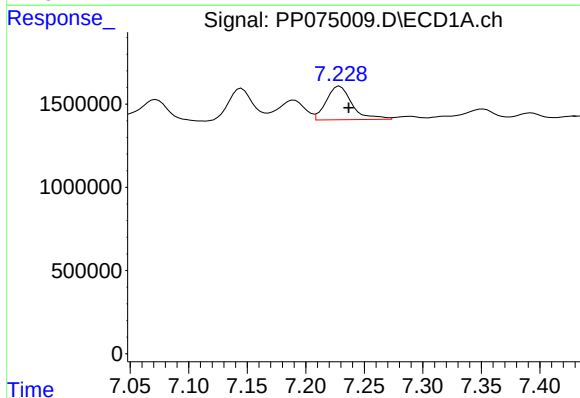


#28 AR-1254-3

R.T.: 7.229 min
Delta R.T.: -0.008 min
Response: 3089726
Conc: 34.64 ng/ml

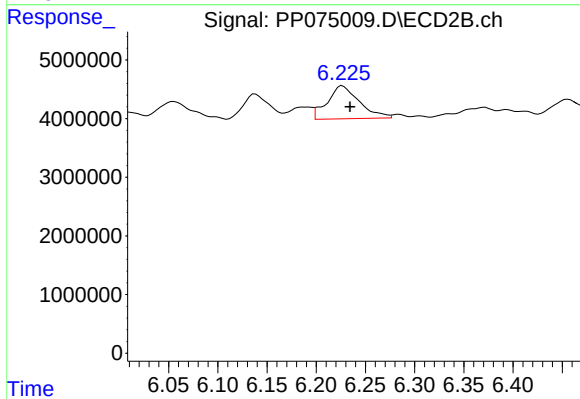

#28 AR-1254-3


R.T.: 6.227 min
Delta R.T.: -0.008 min
Response: 12775294
Conc: 20.61 ng/ml

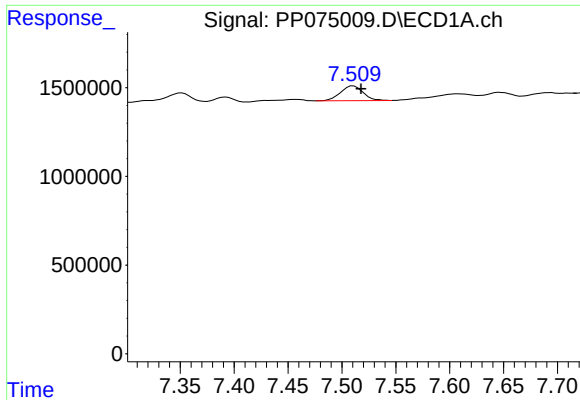

#29 AR-1254-4


R.T.: 7.511 min
Delta R.T.: -0.007 min
Response: 1215525
Conc: 18.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

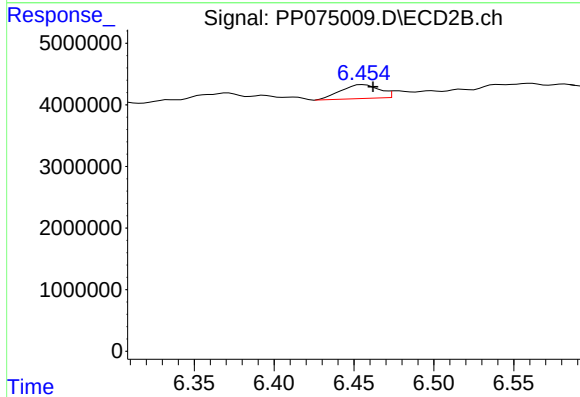


#29 AR-1254-4

R.T.: 6.456 min
Delta R.T.: -0.006 min
Response: 3761043
Conc: 8.03 ng/ml

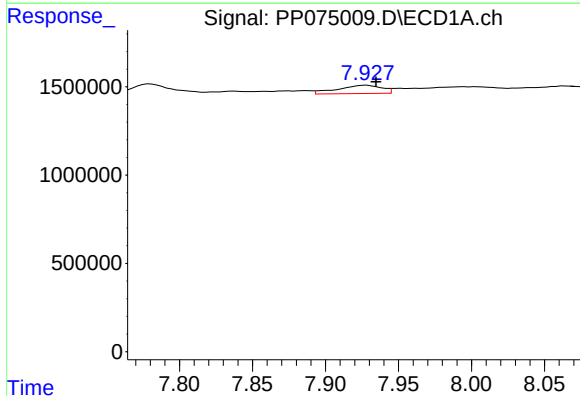


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.006 min
Response: 970367
Conc: 11.68 ng/ml

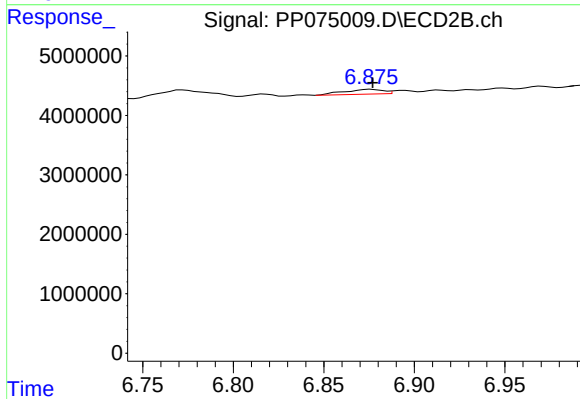

#30 AR-1254-5


R.T.: 6.876 min
Delta R.T.: 0.000 min
Response: 1231463
Conc: 2.51 ng/ml

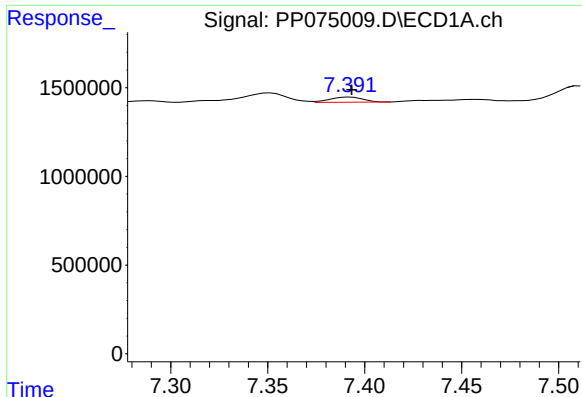

#31 AR-1260-1


R.T.: 7.393 min
Delta R.T.: 0.000 min
Response: 351249
Conc: 6.08 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

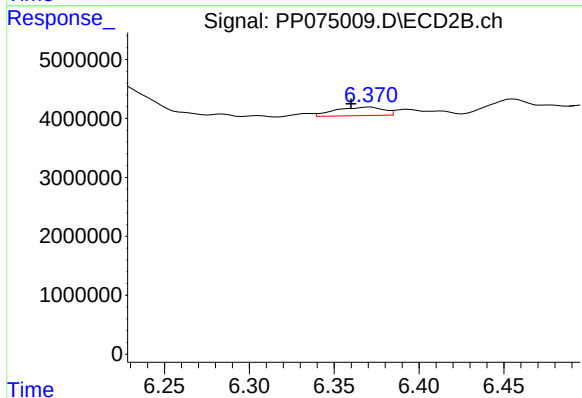


#31 AR-1260-1

R.T.: 6.371 min
Delta R.T.: 0.011 min
Response: 2812002
Conc: 7.49 ng/ml

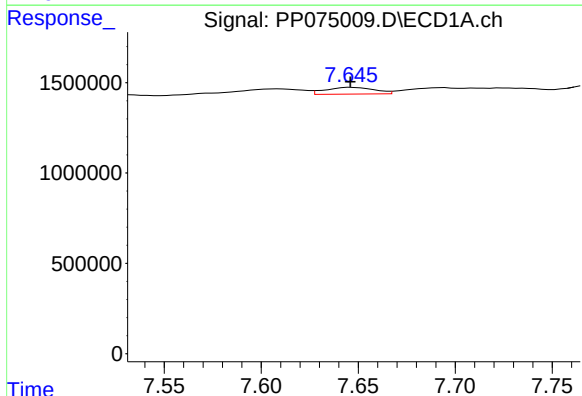


#32 AR-1260-2

R.T.: 7.646 min
Delta R.T.: 0.000 min
Response: 647498
Conc: 9.40 ng/ml

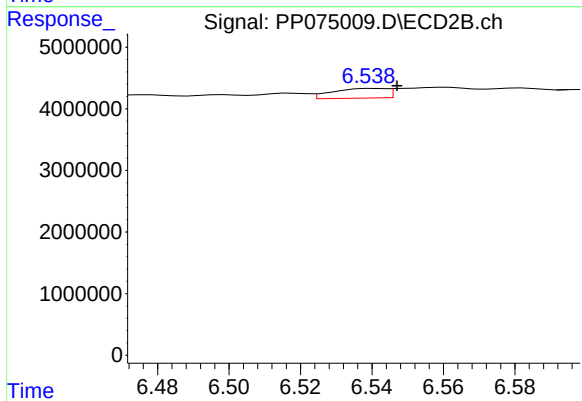

#32 AR-1260-2


R.T.: 6.541 min
Delta R.T.: -0.006 min
Response: 1650584
Conc: 3.12 ng/ml

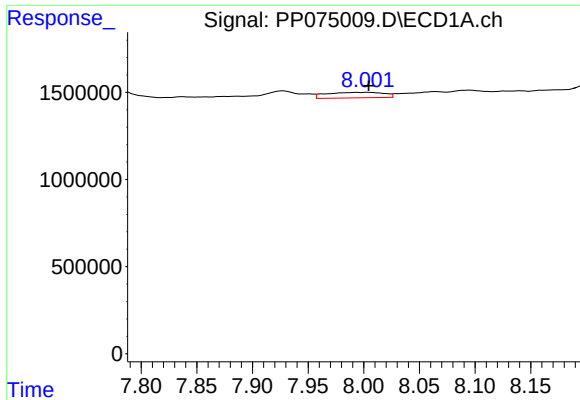

#33 AR-1260-3


R.T.: 8.003 min
Delta R.T.: -0.001 min
Response: 1137550
Conc: 21.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

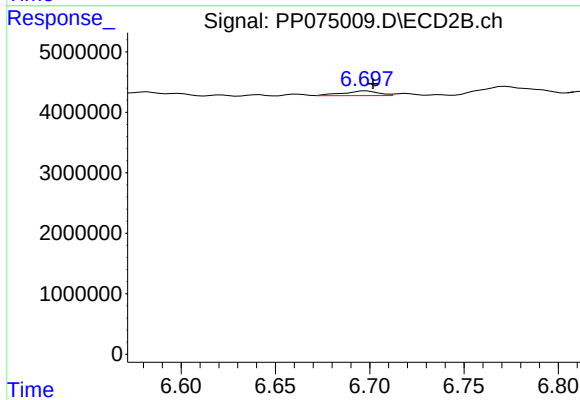


#33 AR-1260-3

R.T.: 6.698 min
Delta R.T.: -0.003 min
Response: 998844
Conc: 2.31 ng/ml

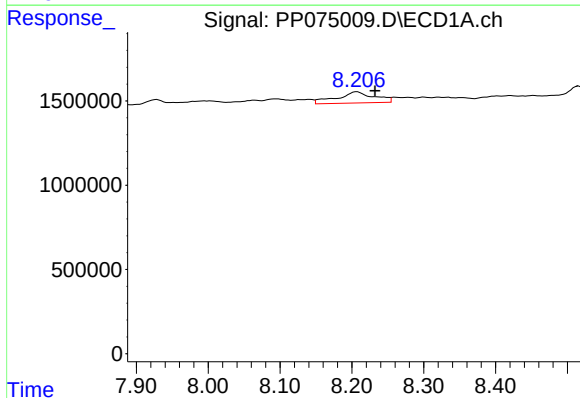


#34 AR-1260-4

R.T.: 8.207 min
Delta R.T.: -0.025 min
Response: 2419637
Conc: 37.93 ng/ml

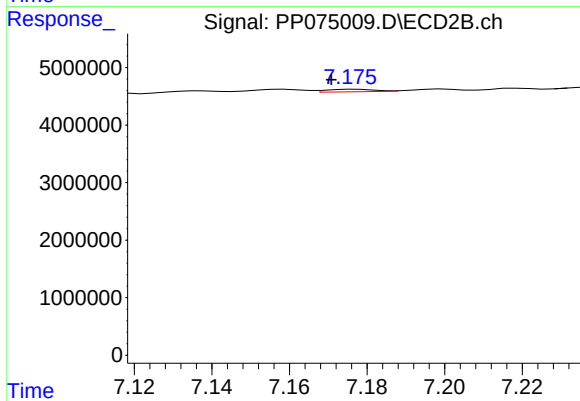

#34 AR-1260-4


R.T.: 7.177 min
Delta R.T.: 0.006 min
Response: 379220
Conc: 0.99 ng/ml

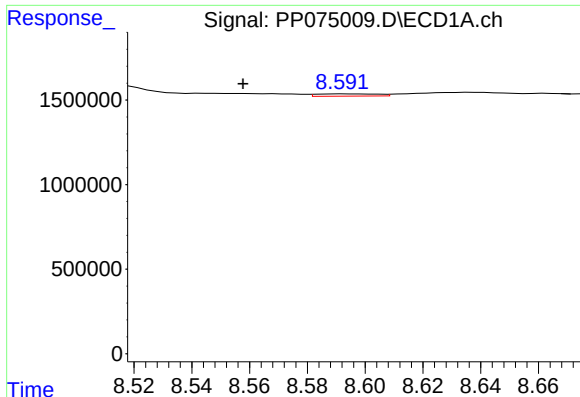

#35 AR-1260-5


R.T.: 8.593 min
Delta R.T.: 0.035 min
Response: 195517
Conc: 1.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

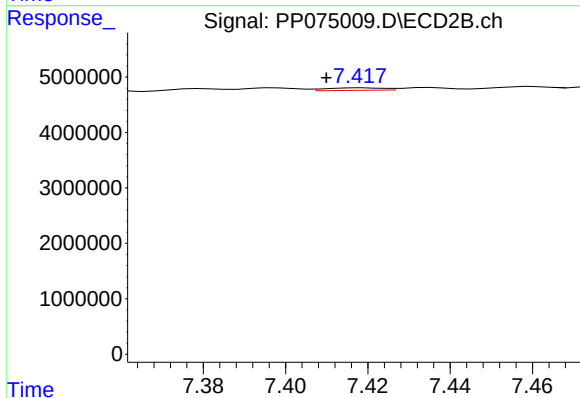


#35 AR-1260-5

R.T.: 7.419 min
Delta R.T.: 0.009 min
Response: 419464
Conc: 0.42 ng/ml

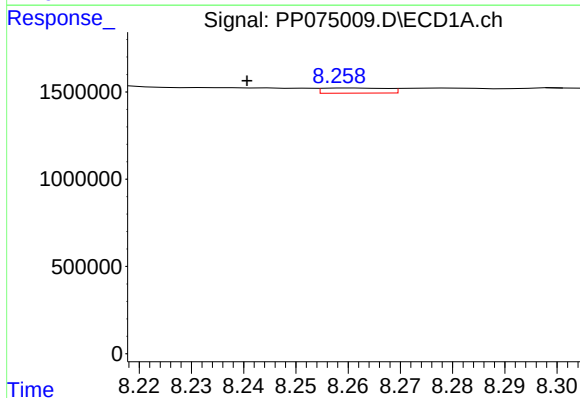


#36 AR-1262-1

R.T.: 8.261 min
Delta R.T.: 0.020 min
Response: 251952
Conc: 3.27 ng/ml

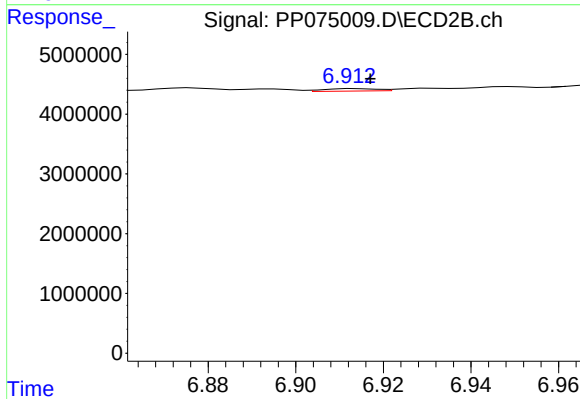

#36 AR-1262-1


R.T.: 6.914 min
Delta R.T.: -0.003 min
Response: 338450
Conc: 0.48 ng/ml

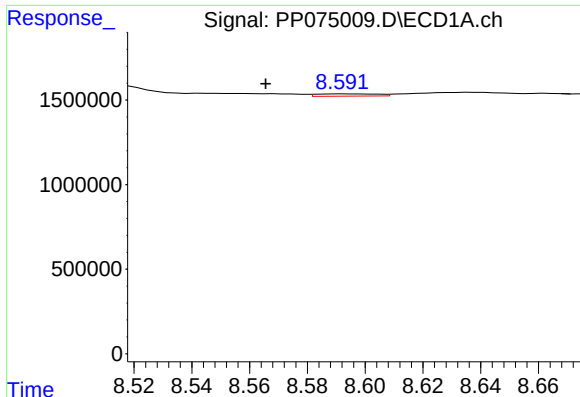

#37 AR-1262-2


R.T.: 8.593 min
Delta R.T.: 0.027 min
Response: 195517
Conc: 1.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

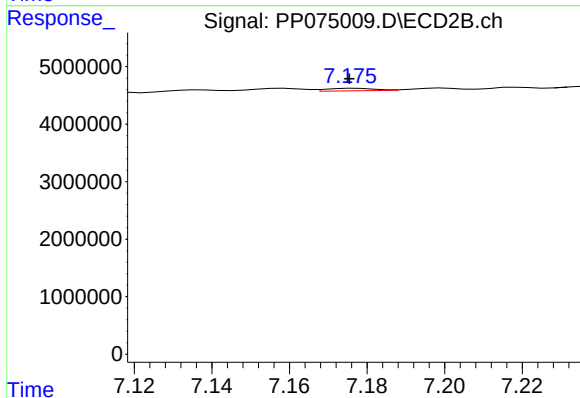


#37 AR-1262-2

R.T.: 7.177 min
Delta R.T.: 0.002 min
Response: 379220
Conc: 0.73 ng/ml

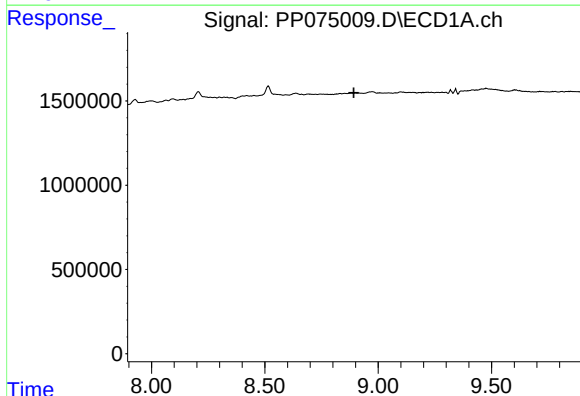


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

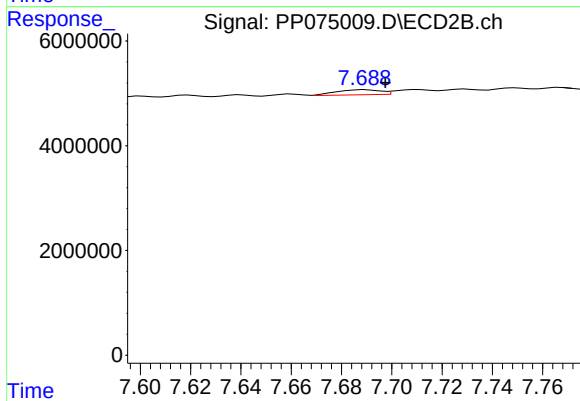

#38 AR-1262-3


R.T.: 7.689 min
Delta R.T.: -0.008 min
Response: 1178466
Conc: 2.53 ng/ml

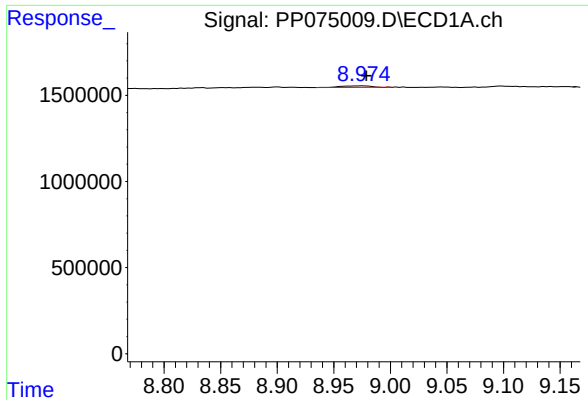

#39 AR-1262-4


R.T.: 8.976 min
Delta R.T.: -0.003 min
Response: 162318
Conc: 2.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

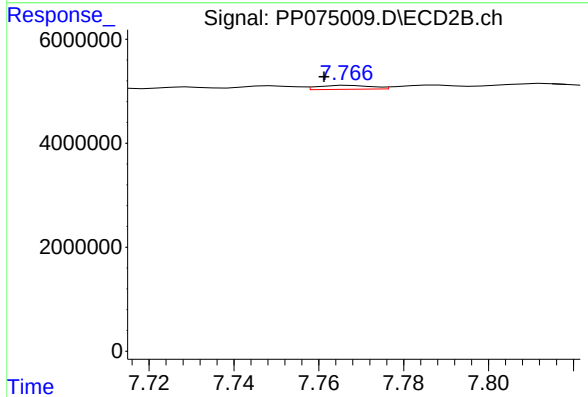


#39 AR-1262-4

R.T.: 7.767 min
Delta R.T.: 0.006 min
Response: 670805
Conc: 0.82 ng/ml

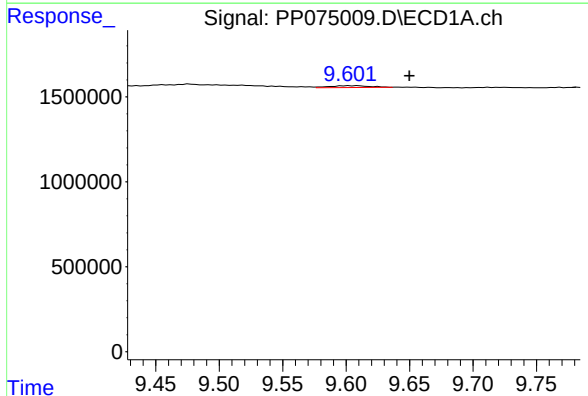


#40 AR-1262-5

R.T.: 9.603 min
Delta R.T.: -0.047 min
Response: 239929
Conc: 3.94 ng/ml

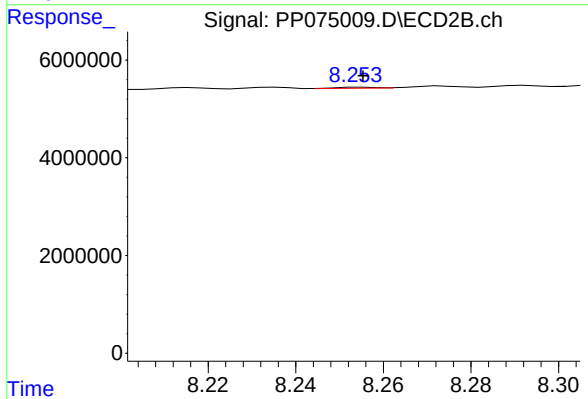

#40 AR-1262-5


R.T.: 8.255 min
Delta R.T.: 0.000 min
Response: 124137
Conc: 0.35 ng/ml

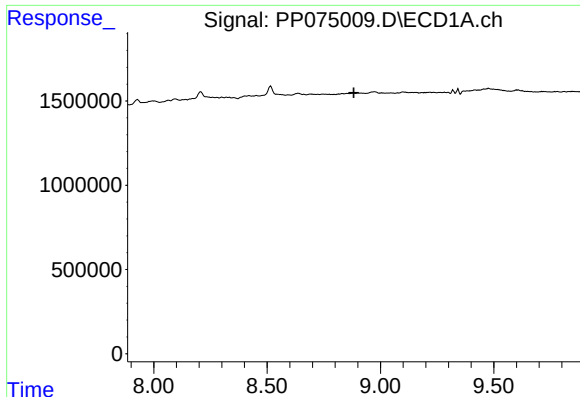

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

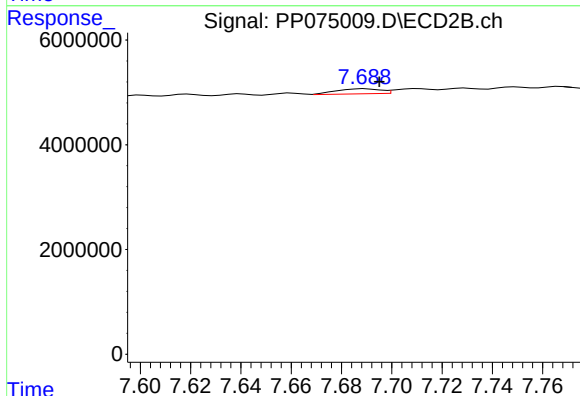


#41 AR-1268-1

R.T.: 7.689 min
Delta R.T.: -0.006 min
Response: 1178466
Conc: 0.84 ng/ml

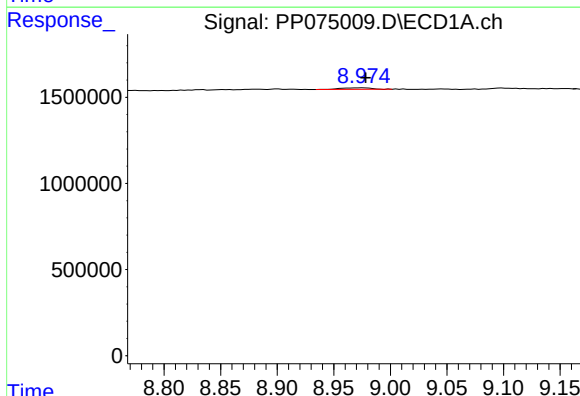


#42 AR-1268-2

R.T.: 8.976 min
Delta R.T.: -0.003 min
Response: 162318
Conc: 1.11 ng/ml

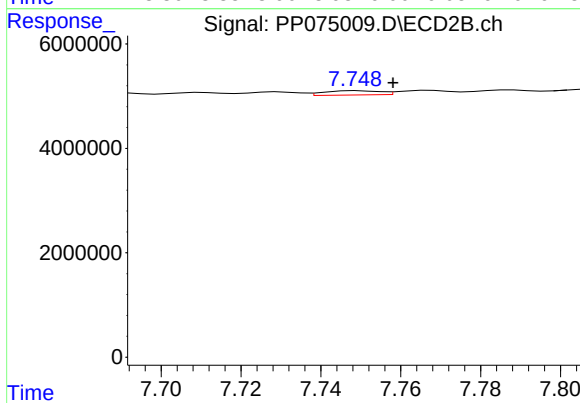

#42 AR-1268-2


R.T.: 7.749 min
Delta R.T.: -0.009 min
Response: 790422
Conc: 0.58 ng/ml

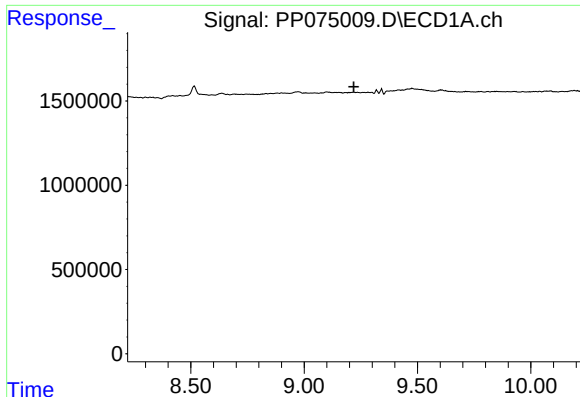

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

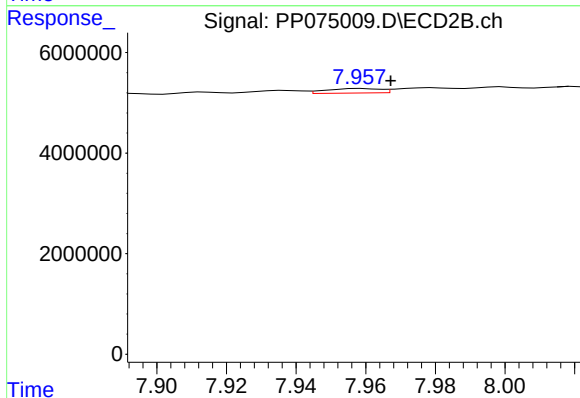


#43 AR-1268-3

R.T.: 7.959 min
Delta R.T.: -0.008 min
Response: 955694
Conc: 0.92 ng/ml

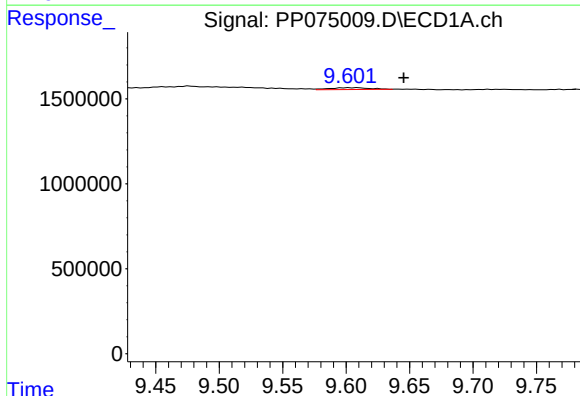


#44 AR-1268-4

R.T.: 9.603 min
Delta R.T.: -0.043 min
Response: 239929
Conc: 3.57 ng/ml

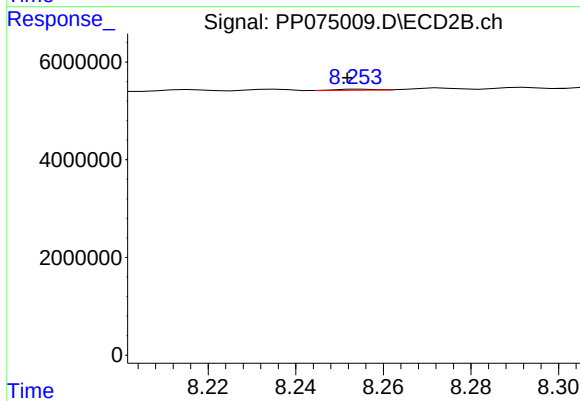

#44 AR-1268-4


R.T.: 8.255 min
Delta R.T.: 0.003 min
Response: 124137
Conc: 0.32 ng/ml

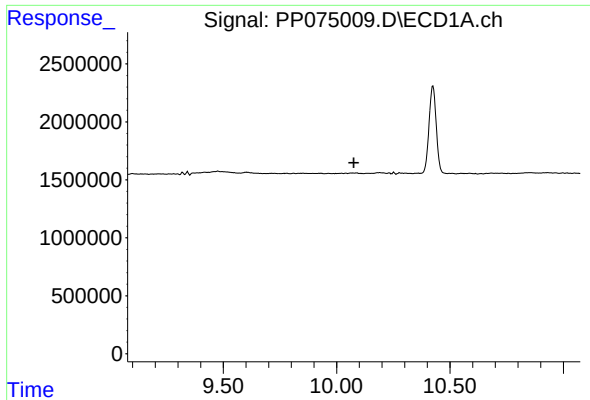

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-H

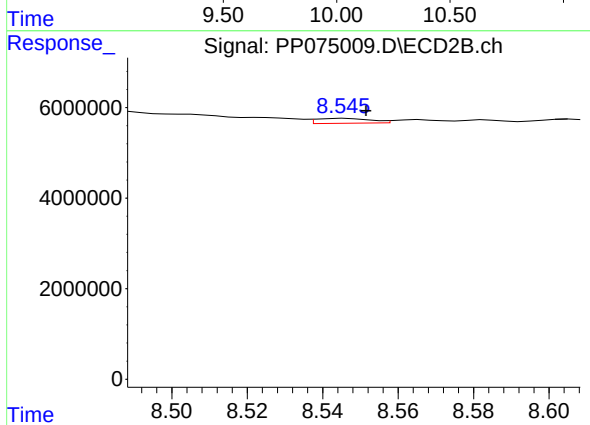

#45 AR-1268-5

R.T.: 8.546 min
Delta R.T.: -0.005 min
Response: 1076391
Conc: 0.34 ng/ml