

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 18:12
 Operator : YP\AJ
 Sample : Q3034-09
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-I

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:51:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.652	3.795	20836667	74462775	17.028	15.399
2)	SA Decachlor...	10.426	8.801	16966779	101.2E6	17.181	13.496
Target Compounds							
3)	L1 AR-1016-1	5.803	4.892	19502703	199.6E6	442.350	391.885
4)	L1 AR-1016-2	5.825	4.950	27223410	105.0E6	433.207	441.067
5)	L1 AR-1016-3	5.887	5.070	20115990	64882428	447.879	470.491
6)	L1 AR-1016-4	5.984	5.111	18671728	72715524	530.721	520.128
7)	L1 AR-1016-5	6.277	5.325	25044466	108.3E6	754.668	652.016
8)	L2 AR-1221-1	4.848	4.009	412981	921365	23.474	14.893 #
9)	L2 AR-1221-2	4.937	4.092	366715	2593614	27.455	57.366 #
10)	L2 AR-1221-3	5.013	4.168	1761246	6463183	46.455	39.339
11)	L3 AR-1232-1	5.013	4.168	1761246	6463183	57.985	50.456
12)	L3 AR-1232-2	5.539	4.892	9069629	199.6E6	575.549	861.147 #
13)	L3 AR-1232-3	5.825	5.070	27223410	64882428	891.294	1080.298
14)	L3 AR-1232-4	5.984	5.154	18671728	121.0E6	1081.211	1641.718 #
15)	L3 AR-1232-5	6.074	5.325	17544020	108.3E6	1351.520	1744.238 #
16)	L4 AR-1242-1	5.803	4.892	19502703	199.6E6	509.539	473.282
17)	L4 AR-1242-2	5.825	4.950	27223410	105.0E6	481.984	524.163
18)	L4 AR-1242-3	5.887	5.070	20115990	64882428	495.432	548.465
19)	L4 AR-1242-4	5.984	5.154	18671728	121.0E6	588.237	706.982
20)	L4 AR-1242-5	6.714	5.674	12976396	83221863	359.750	449.449
21)	L5 AR-1248-1	5.803	4.892	19502703	199.6E6	645.272	722.844
22)	L5 AR-1248-2	6.074	5.111	17544020	72715524	407.091	411.390
23)	L5 AR-1248-3	6.277	5.154	25044466	121.0E6	536.243	532.592
24)	L5 AR-1248-4	6.674	5.325	13847021	108.3E6	251.760	496.690 #
25)	L5 AR-1248-5	6.714	5.714	12976396	78837307	233.933	214.627
26)	L6 AR-1254-1	6.649	5.674	11476399	83221863	196.954	174.575
27)	L6 AR-1254-2	6.870	5.820	9270122	11651766	113.582	33.089 #
28)	L6 AR-1254-3	7.228	6.224	1934978	5056932	21.691	8.159 #
29)	L6 AR-1254-4	7.510	6.458	574800	2113498	8.721	4.510 #
30)	L6 AR-1254-5	7.928	6.867	863839	433712	10.397	0.884 #
31)	L7 AR-1260-1	7.392	6.358	268531	884902	4.645	2.358 #
32)	L7 AR-1260-2	7.648	6.544	398330	721058	5.780	1.364 #
33)	L7 AR-1260-3	8.007	6.701	503913	490222	9.712	1.132 #
34)	L7 AR-1260-4	8.206	7.176	1456278	729488	22.828	1.912 #
35)	L7 AR-1260-5	8.515f	7.408	903382	711735	7.965	0.709 #
36)	L8 AR-1262-1	8.266	6.921	449053	909165	5.831	1.285 #
37)	L8 AR-1262-2	8.515f	7.176	903382	729488	6.824	1.401 #
38)	L8 AR-1262-3	0.000	7.691	0	1280198	N.D.	2.745 #
39)	L8 AR-1262-4	8.971	7.755	174018	980342	2.310	1.193 #
40)	L8 AR-1262-5	9.608f	8.262	102868	338851	1.688	0.946 #
41)	L9 AR-1268-1	0.000	7.691	0	1280198	N.D.	0.908 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 18:12
Operator : YP\AJ
Sample : Q3034-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:51:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.971	7.755	174018	980342	1.186	0.719 #
43)	L9 AR-1268-3	0.000	7.961	0	872947	N.D.	0.837 #
44)	L9 AR-1268-4	9.608f	8.243	102868	171236	1.529	0.447 #
45)	L9 AR-1268-5	0.000	8.559	0	305800	N.D.	0.098 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 18:12
Operator : YP\AJ
Sample : Q3034-09
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:51:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

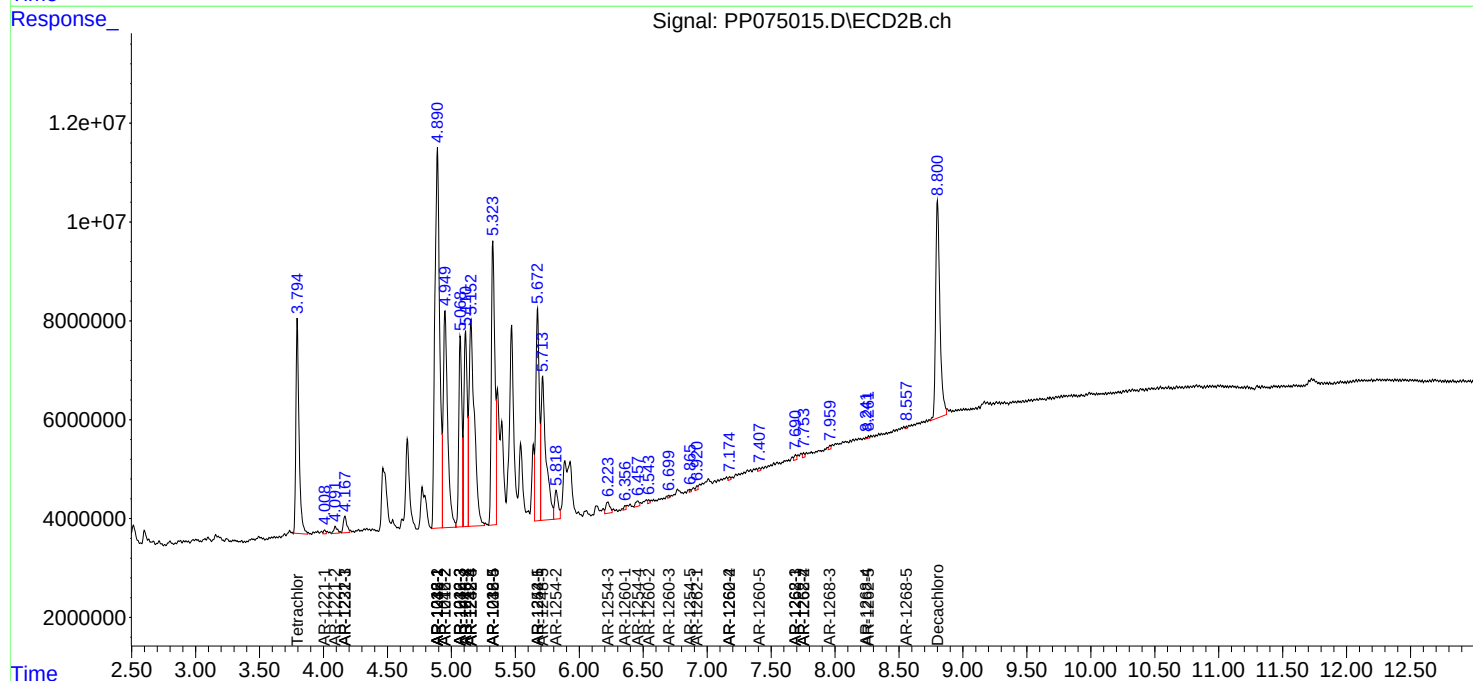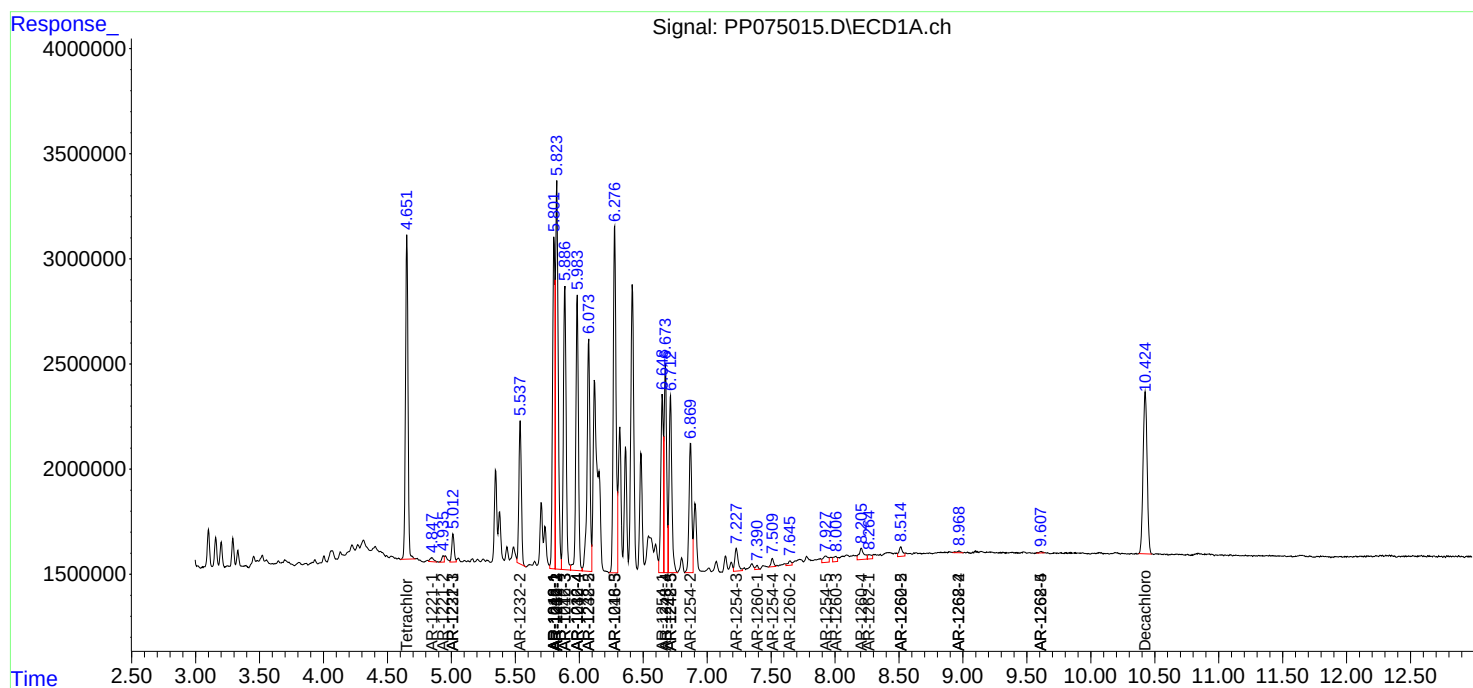


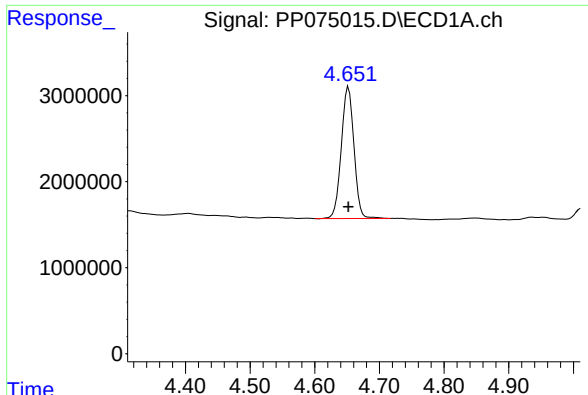

#1 Tetrachloro-m-xylene


R.T.: 4.652 min
Delta R.T.: 0.000 min
Response: 20836667
Conc: 17.03 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

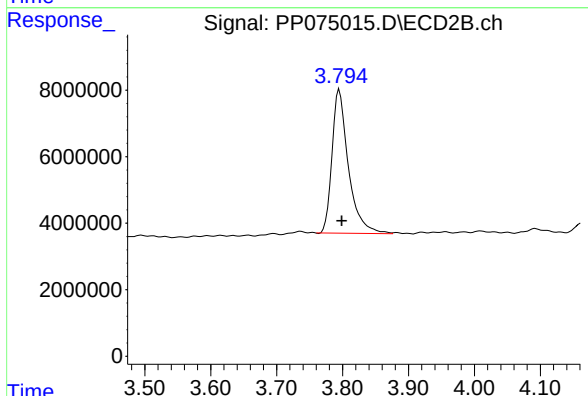


#1 Tetrachloro-m-xylene

R.T.: 3.795 min
Delta R.T.: -0.004 min
Response: 74462775
Conc: 15.40 ng/ml

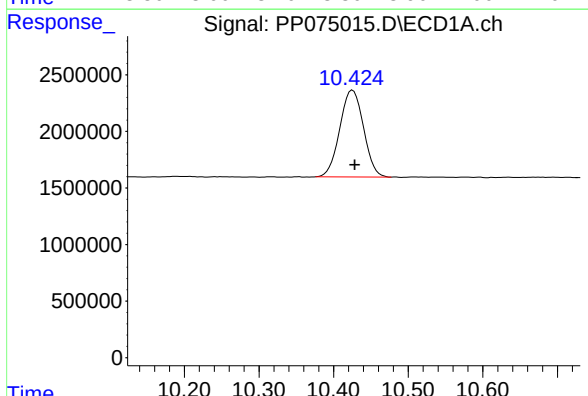


#2 Decachlorobiphenyl

R.T.: 10.426 min
Delta R.T.: -0.003 min
Response: 16966779
Conc: 17.18 ng/ml

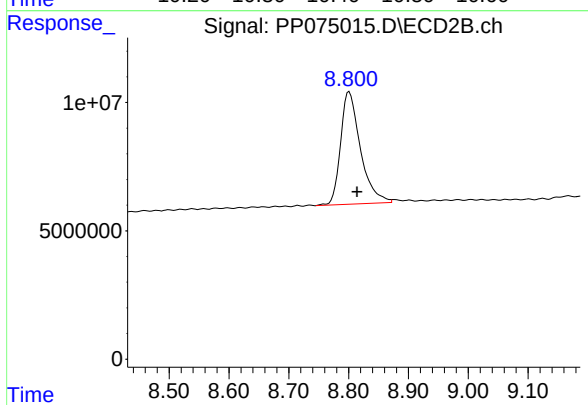

#2 Decachlorobiphenyl


R.T.: 8.801 min
Delta R.T.: -0.013 min
Response: 101211689
Conc: 13.50 ng/ml

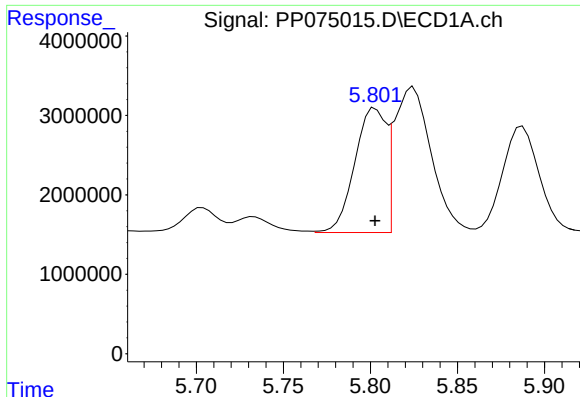

#3 AR-1016-1


R.T.: 5.803 min
Delta R.T.: 0.000 min
Response: 19502703
Conc: 442.35 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

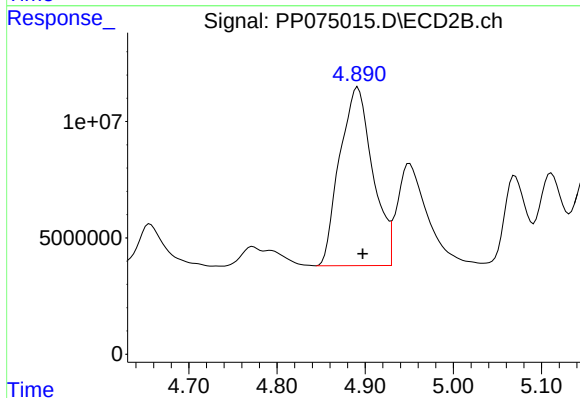


#3 AR-1016-1

R.T.: 4.892 min
Delta R.T.: -0.006 min
Response: 199608105
Conc: 391.88 ng/ml

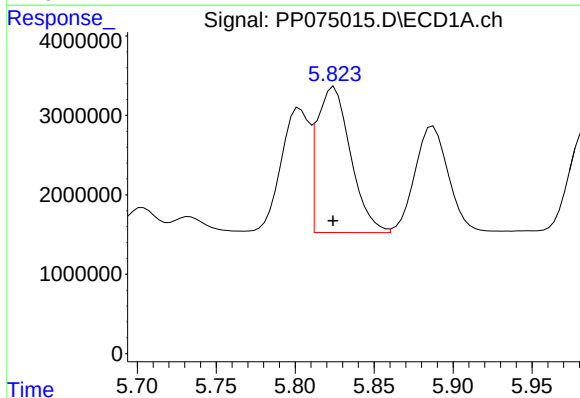


#4 AR-1016-2

R.T.: 5.825 min
Delta R.T.: 0.000 min
Response: 27223410
Conc: 433.21 ng/ml

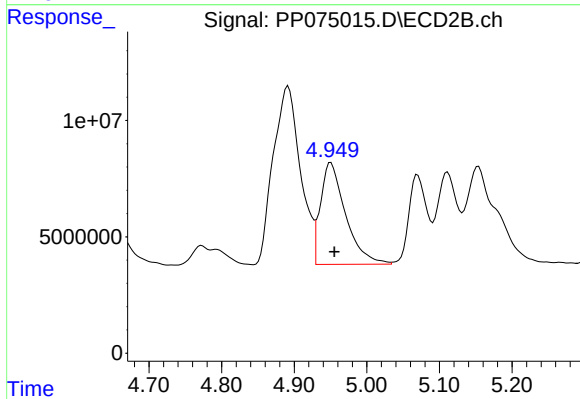

#4 AR-1016-2


R.T.: 4.950 min
Delta R.T.: -0.005 min
Response: 104980685
Conc: 441.07 ng/ml

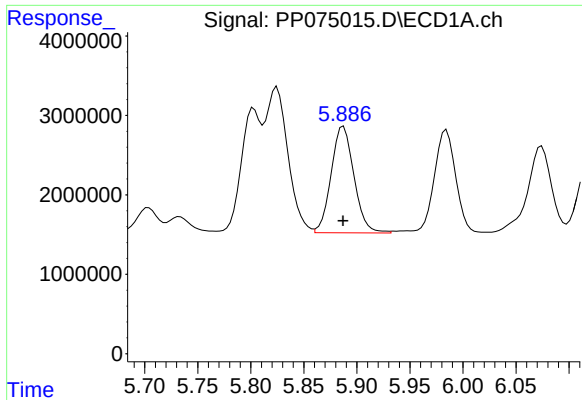

#5 AR-1016-3


R.T.: 5.887 min
Delta R.T.: 0.000 min
Response: 20115990
Conc: 447.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

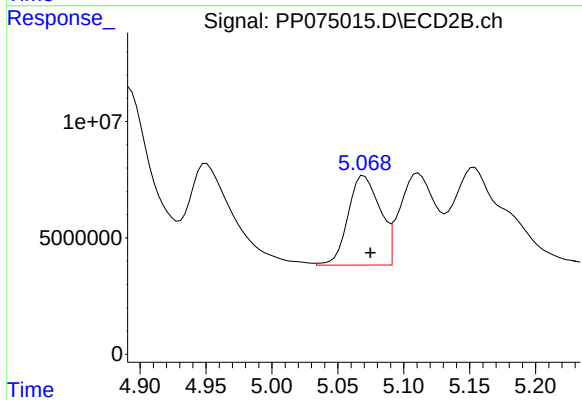


#5 AR-1016-3

R.T.: 5.070 min
Delta R.T.: -0.005 min
Response: 64882428
Conc: 470.49 ng/ml

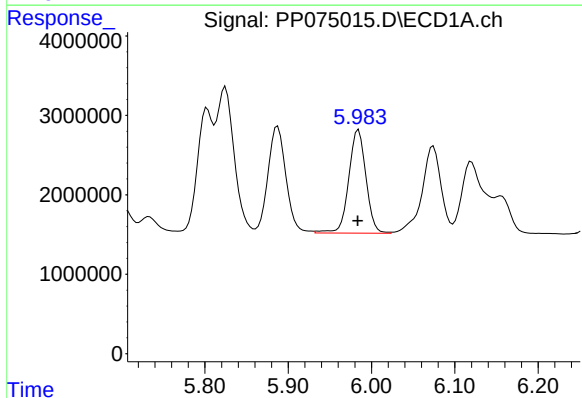


#6 AR-1016-4

R.T.: 5.984 min
Delta R.T.: 0.000 min
Response: 18671728
Conc: 530.72 ng/ml

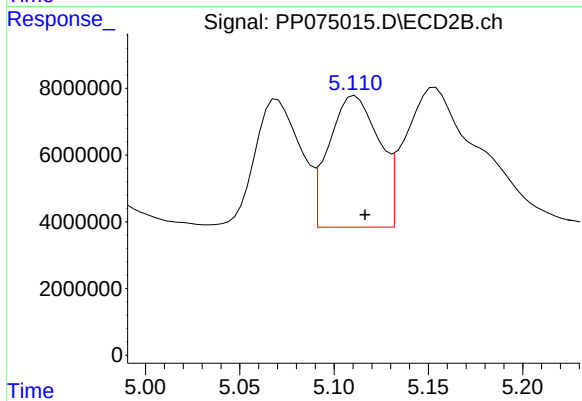

#6 AR-1016-4


R.T.: 5.111 min
Delta R.T.: -0.005 min
Response: 72715524
Conc: 520.13 ng/ml

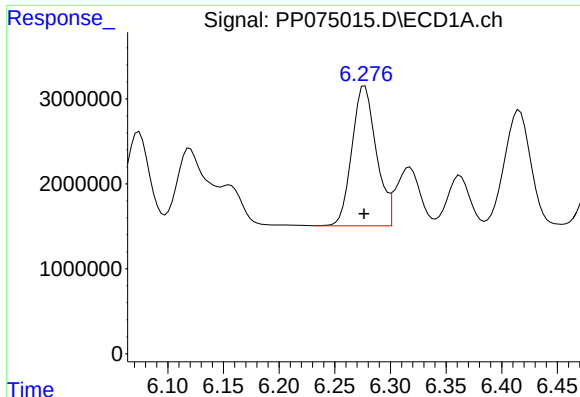

#7 AR-1016-5


R.T.: 6.277 min
Delta R.T.: 0.000 min
Response: 25044466
Conc: 754.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

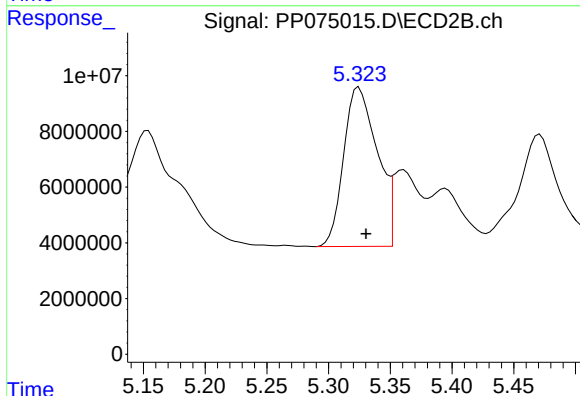


#7 AR-1016-5

R.T.: 5.325 min
Delta R.T.: -0.006 min
Response: 108288931
Conc: 652.02 ng/ml

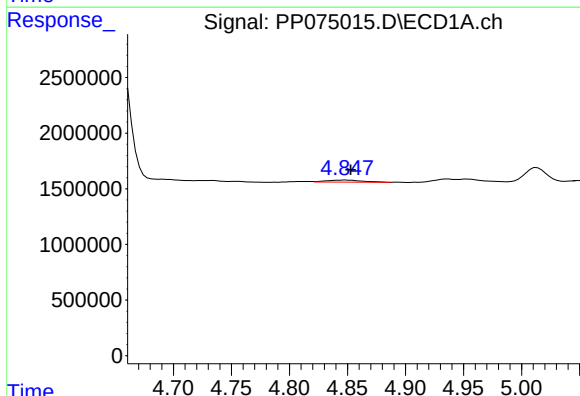


#8 AR-1221-1

R.T.: 4.848 min
Delta R.T.: -0.004 min
Response: 412981
Conc: 23.47 ng/ml

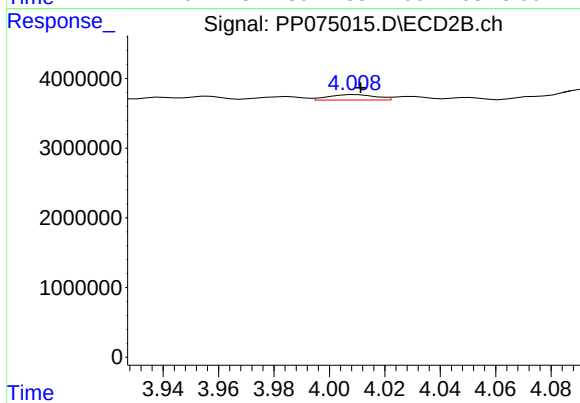

#8 AR-1221-1


R.T.: 4.009 min
Delta R.T.: -0.002 min
Response: 921365
Conc: 14.89 ng/ml

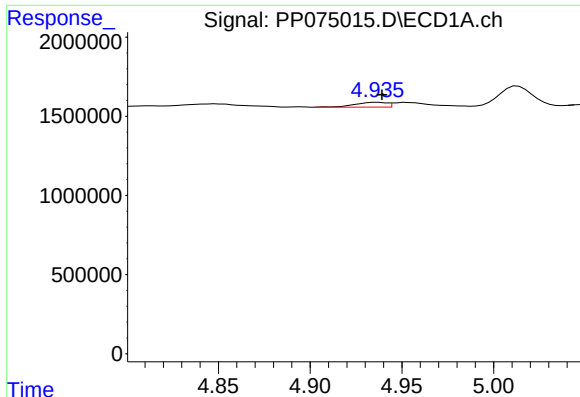

#9 AR-1221-2


R.T.: 4.937 min
Delta R.T.: -0.003 min
Response: 366715
Conc: 27.45 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

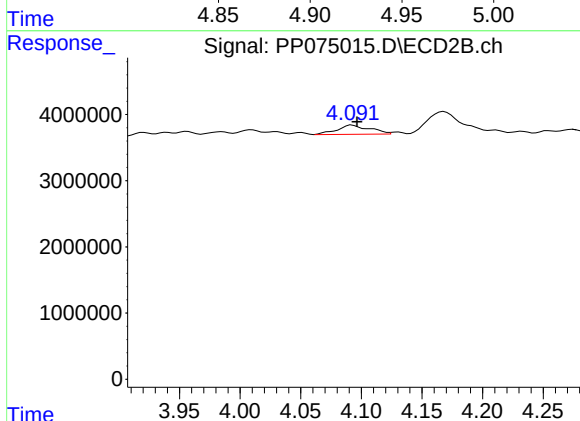


#9 AR-1221-2

R.T.: 4.092 min
Delta R.T.: -0.004 min
Response: 2593614
Conc: 57.37 ng/ml

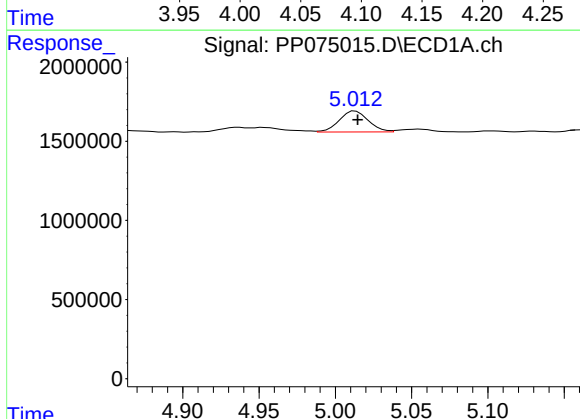


#10 AR-1221-3

R.T.: 5.013 min
Delta R.T.: -0.002 min
Response: 1761246
Conc: 46.46 ng/ml

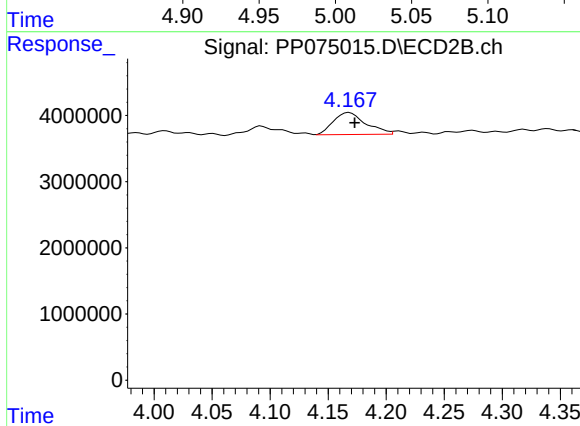

#10 AR-1221-3


R.T.: 4.168 min
Delta R.T.: -0.005 min
Response: 6463183
Conc: 39.34 ng/ml

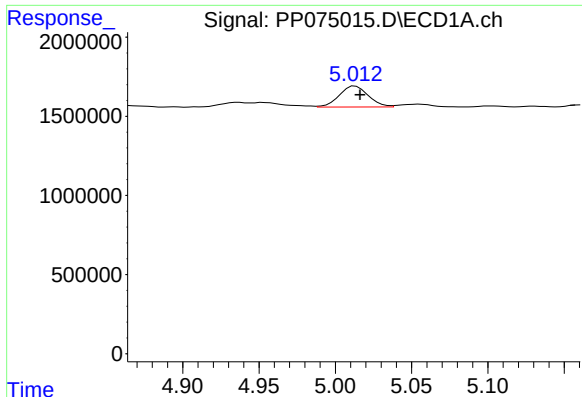

#11 AR-1232-1


R.T.: 5.013 min
Delta R.T.: -0.003 min
Response: 1761246
Conc: 57.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

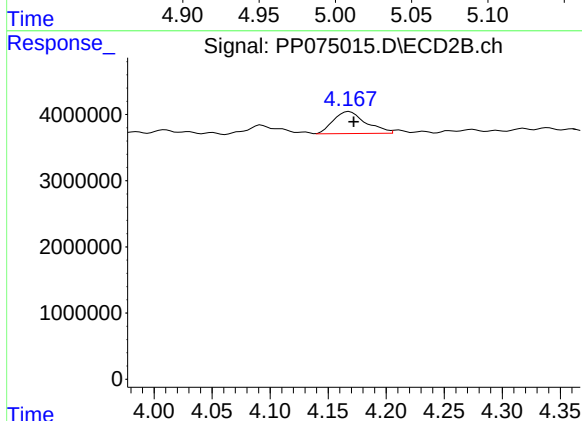


#11 AR-1232-1

R.T.: 4.168 min
Delta R.T.: -0.004 min
Response: 6463183
Conc: 50.46 ng/ml

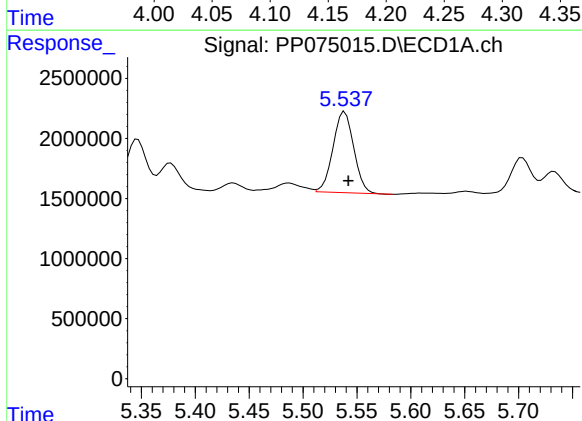


#12 AR-1232-2

R.T.: 5.539 min
Delta R.T.: -0.003 min
Response: 9069629
Conc: 575.55 ng/ml

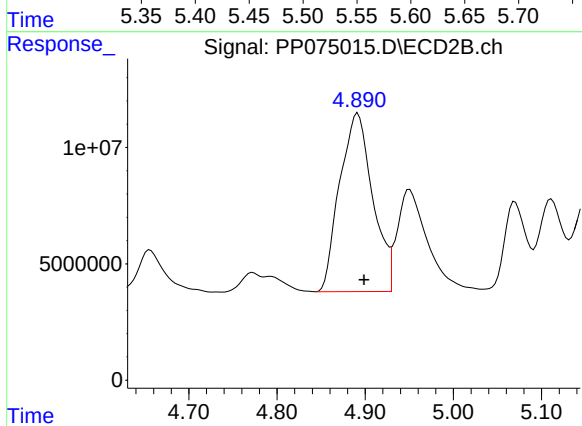

#12 AR-1232-2


R.T.: 4.892 min
Delta R.T.: -0.007 min
Response: 199608105
Conc: 861.15 ng/ml

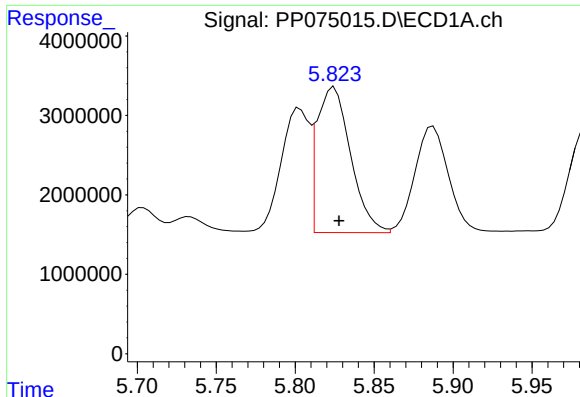

#13 AR-1232-3


R.T.: 5.825 min
Delta R.T.: -0.003 min
Response: 27223410
Conc: 891.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

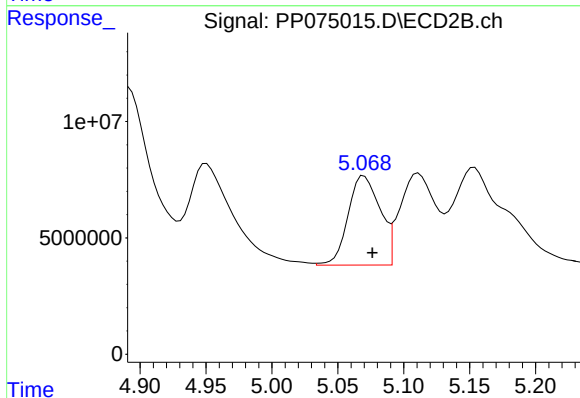


#13 AR-1232-3

R.T.: 5.070 min
Delta R.T.: -0.006 min
Response: 64882428
Conc: 1080.30 ng/ml

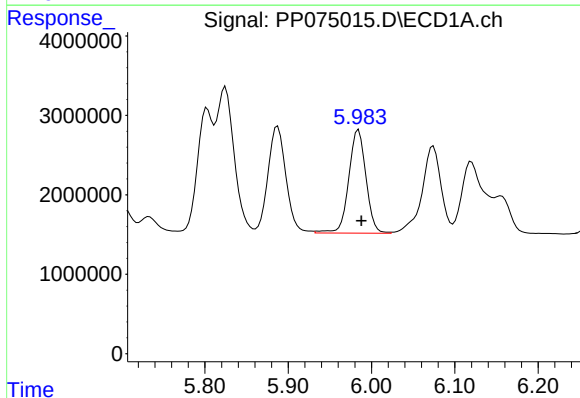


#14 AR-1232-4

R.T.: 5.984 min
Delta R.T.: -0.003 min
Response: 18671728
Conc: 1081.21 ng/ml

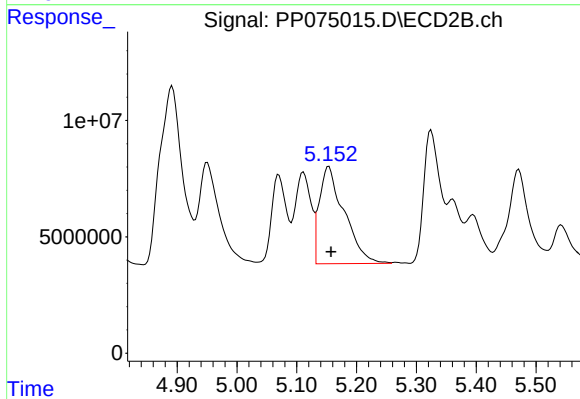

#14 AR-1232-4


R.T.: 5.154 min
Delta R.T.: -0.004 min
Response: 121006740
Conc: 1641.72 ng/ml

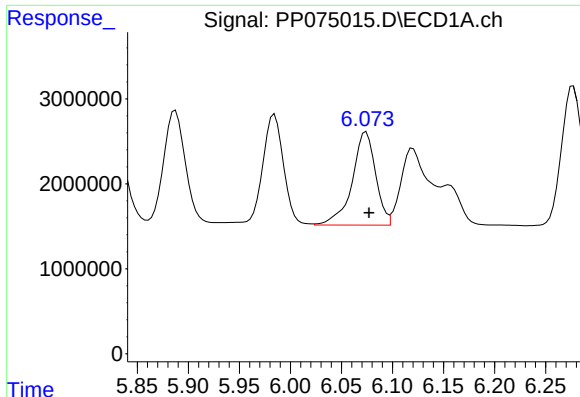

#15 AR-1232-5


R.T.: 6.074 min
Delta R.T.: -0.003 min
Response: 17544020
Conc: 1351.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

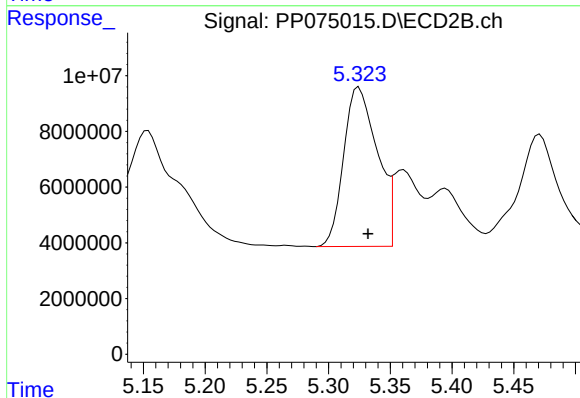


#15 AR-1232-5

R.T.: 5.325 min
Delta R.T.: -0.007 min
Response: 108288931
Conc: 1744.24 ng/ml

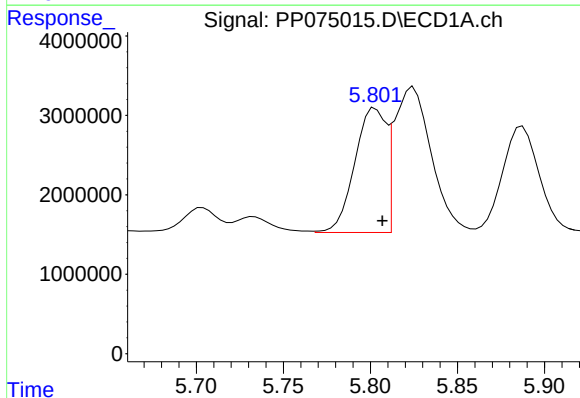


#16 AR-1242-1

R.T.: 5.803 min
Delta R.T.: -0.004 min
Response: 19502703
Conc: 509.54 ng/ml

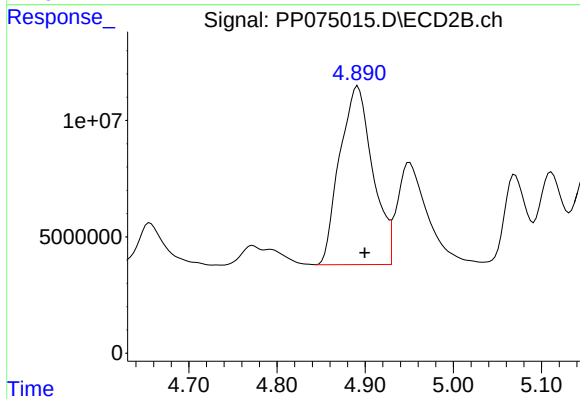

#16 AR-1242-1


R.T.: 4.892 min
Delta R.T.: -0.008 min
Response: 199608105
Conc: 473.28 ng/ml

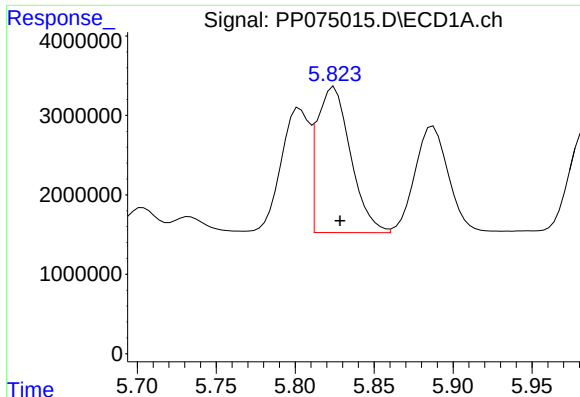

#17 AR-1242-2


R.T.: 5.825 min
Delta R.T.: -0.004 min
Response: 27223410
Conc: 481.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

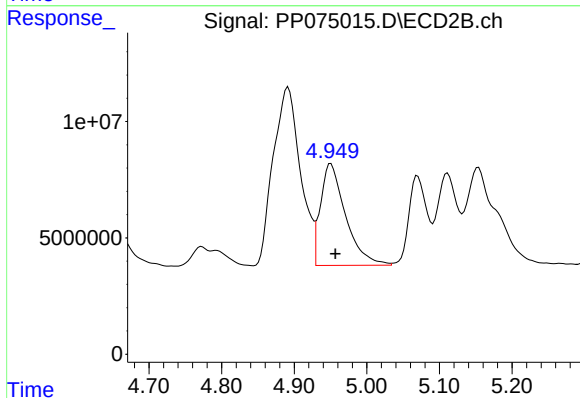


#17 AR-1242-2

R.T.: 4.950 min
Delta R.T.: -0.006 min
Response: 104980685
Conc: 524.16 ng/ml

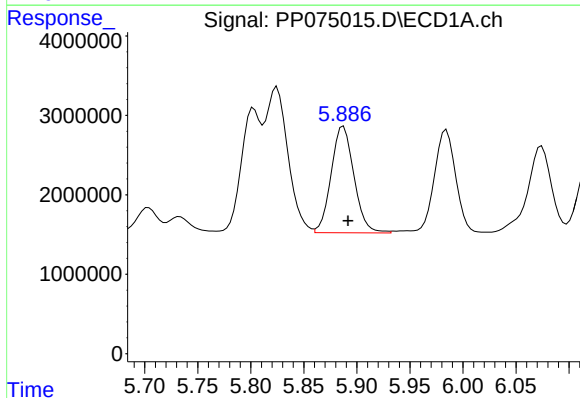


#18 AR-1242-3

R.T.: 5.887 min
Delta R.T.: -0.004 min
Response: 20115990
Conc: 495.43 ng/ml

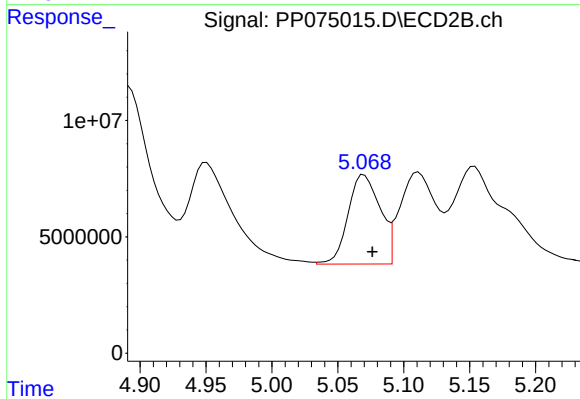

#18 AR-1242-3


R.T.: 5.070 min
Delta R.T.: -0.006 min
Response: 64882428
Conc: 548.46 ng/ml

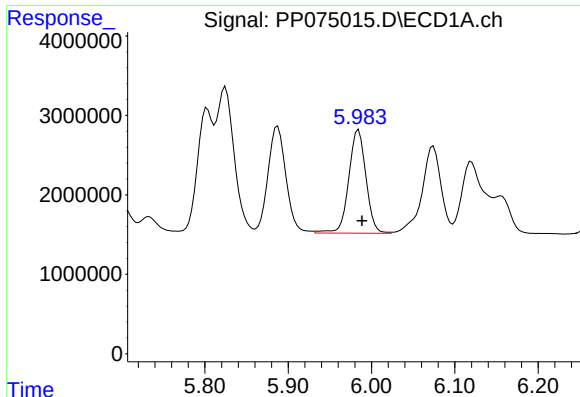

#19 AR-1242-4


R.T.: 5.984 min
Delta R.T.: -0.004 min
Response: 18671728
Conc: 588.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

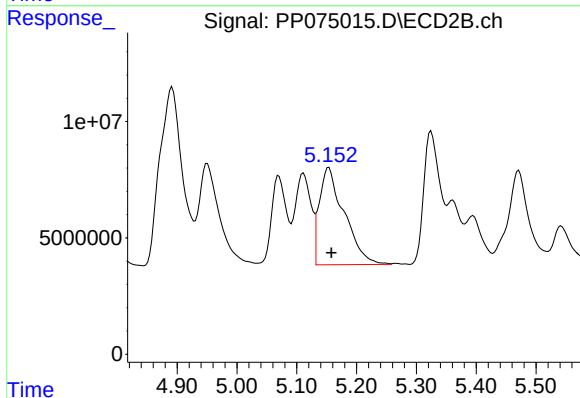


#19 AR-1242-4

R.T.: 5.154 min
Delta R.T.: -0.004 min
Response: 121006740
Conc: 706.98 ng/ml

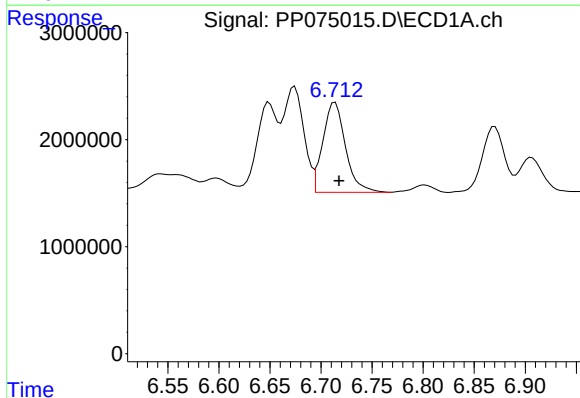


#20 AR-1242-5

R.T.: 6.714 min
Delta R.T.: -0.004 min
Response: 12976396
Conc: 359.75 ng/ml

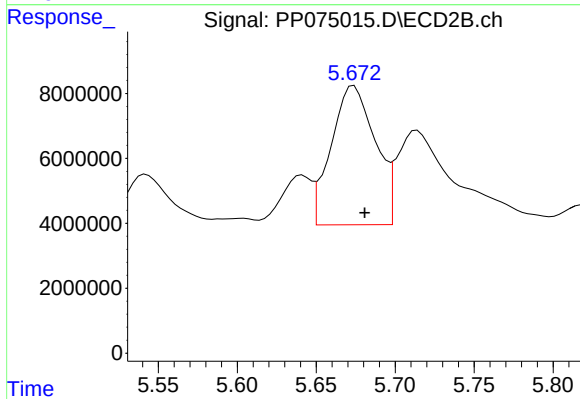

#20 AR-1242-5


R.T.: 5.674 min
Delta R.T.: -0.007 min
Response: 83221863
Conc: 449.45 ng/ml

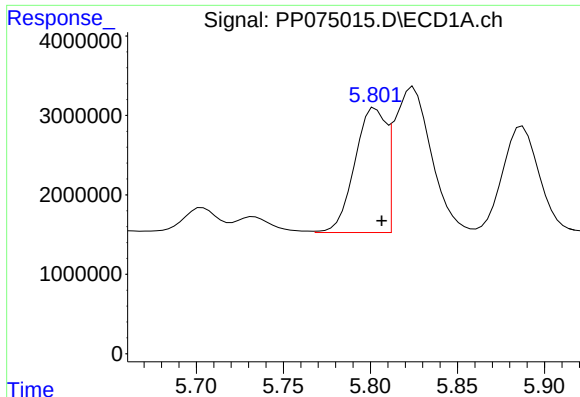

#21 AR-1248-1


R.T.: 5.803 min
Delta R.T.: -0.004 min
Response: 19502703
Conc: 645.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

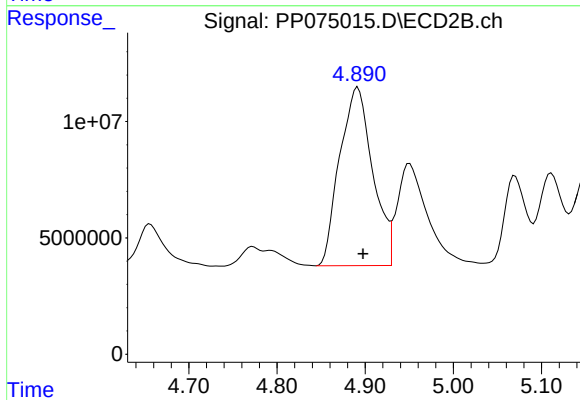


#21 AR-1248-1

R.T.: 4.892 min
Delta R.T.: -0.006 min
Response: 199608105
Conc: 722.84 ng/ml

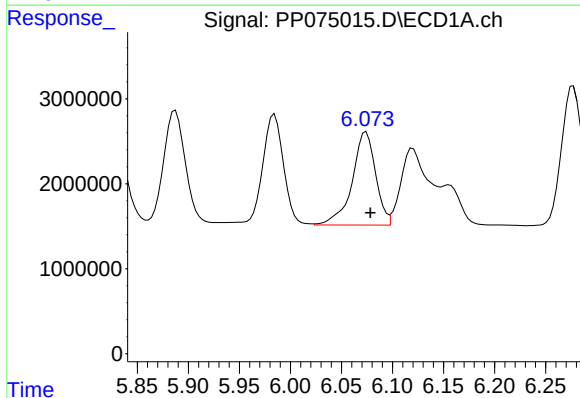


#22 AR-1248-2

R.T.: 6.074 min
Delta R.T.: -0.004 min
Response: 17544020
Conc: 407.09 ng/ml

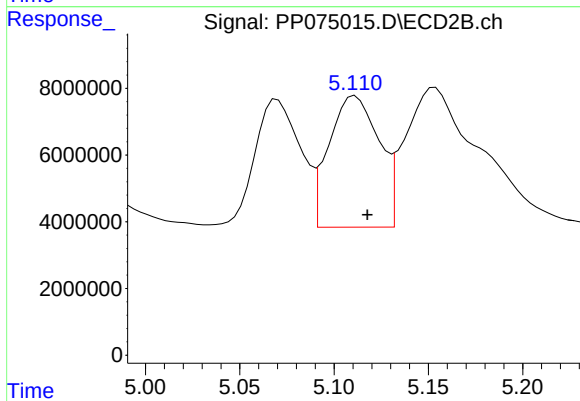

#22 AR-1248-2


R.T.: 5.111 min
Delta R.T.: -0.006 min
Response: 72715524
Conc: 411.39 ng/ml

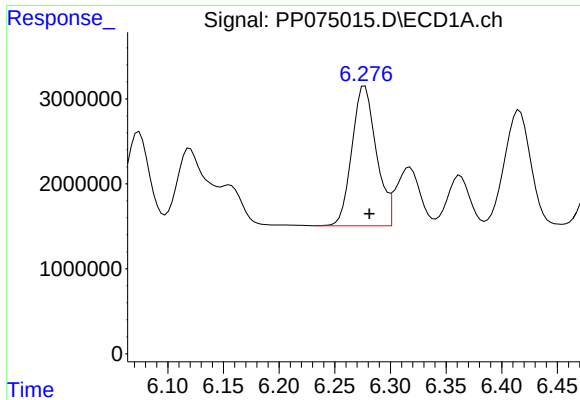

#23 AR-1248-3


R.T.: 6.277 min
Delta R.T.: -0.004 min
Response: 25044466
Conc: 536.24 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

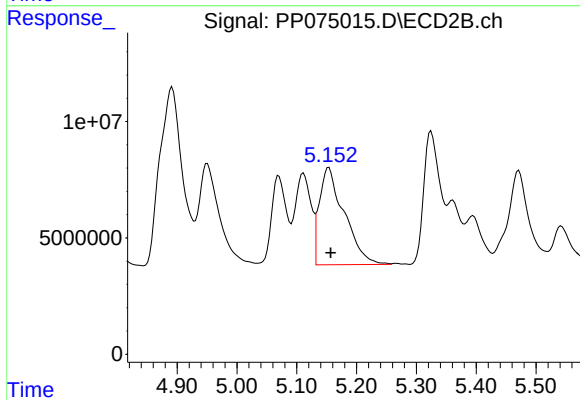


#23 AR-1248-3

R.T.: 5.154 min
Delta R.T.: -0.003 min
Response: 121006740
Conc: 532.59 ng/ml

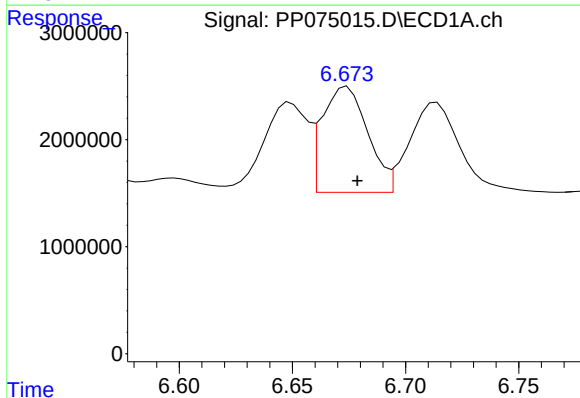


#24 AR-1248-4

R.T.: 6.674 min
Delta R.T.: -0.005 min
Response: 13847021
Conc: 251.76 ng/ml

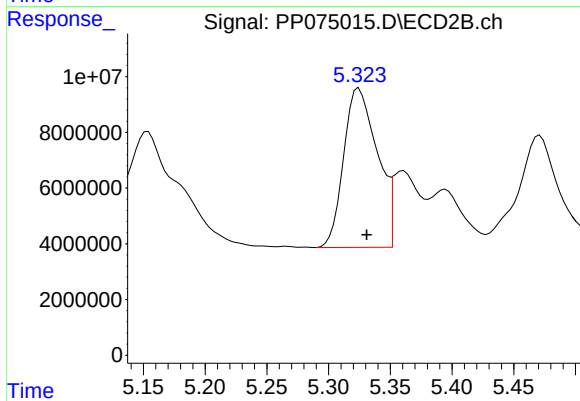

#24 AR-1248-4


R.T.: 5.325 min
Delta R.T.: -0.006 min
Response: 108288931
Conc: 496.69 ng/ml

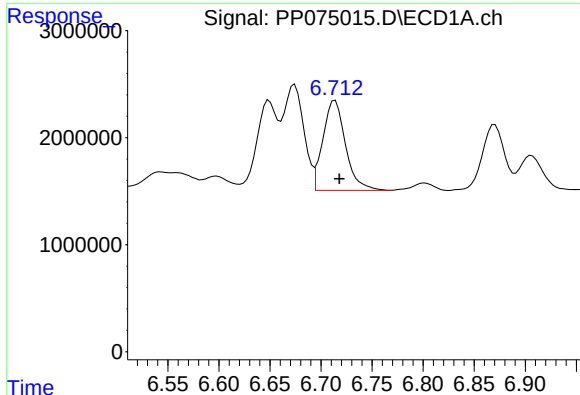

#25 AR-1248-5


R.T.: 6.714 min
Delta R.T.: -0.004 min
Response: 12976396
Conc: 233.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

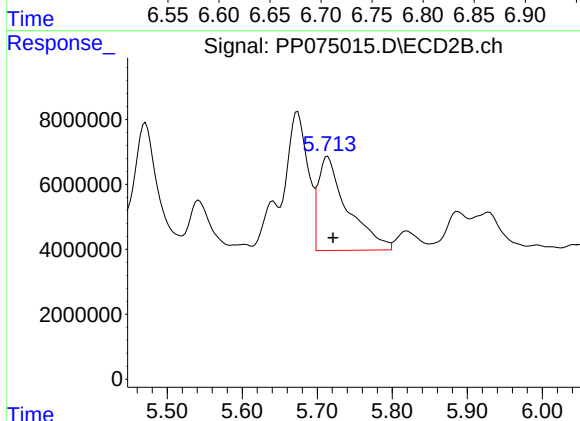


#25 AR-1248-5

R.T.: 5.714 min
Delta R.T.: -0.007 min
Response: 78837307
Conc: 214.63 ng/ml

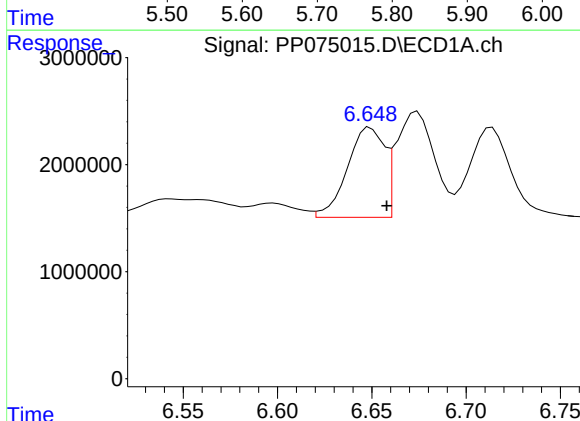


#26 AR-1254-1

R.T.: 6.649 min
Delta R.T.: -0.009 min
Response: 11476399
Conc: 196.95 ng/ml

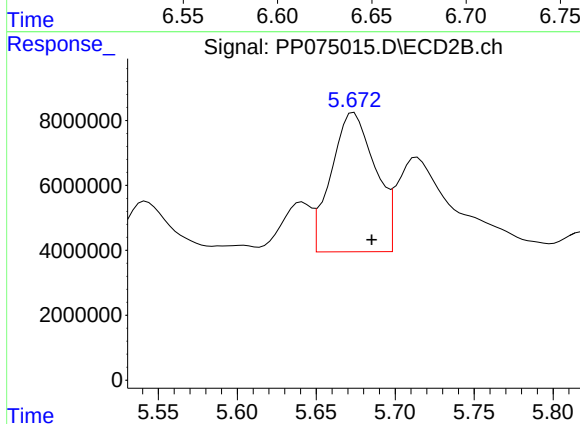

#26 AR-1254-1


R.T.: 5.674 min
Delta R.T.: -0.011 min
Response: 83221863
Conc: 174.58 ng/ml

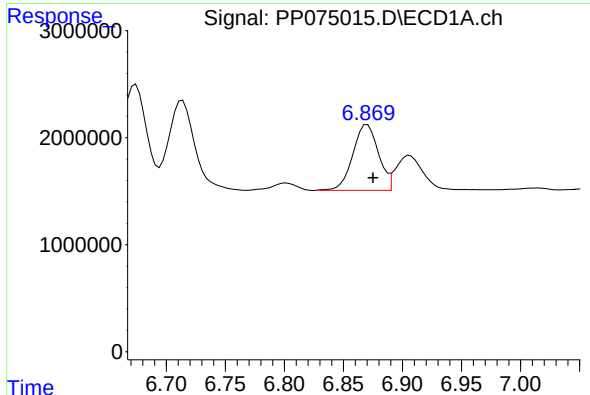

#27 AR-1254-2


R.T.: 6.870 min
Delta R.T.: -0.005 min
Response: 9270122
Conc: 113.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

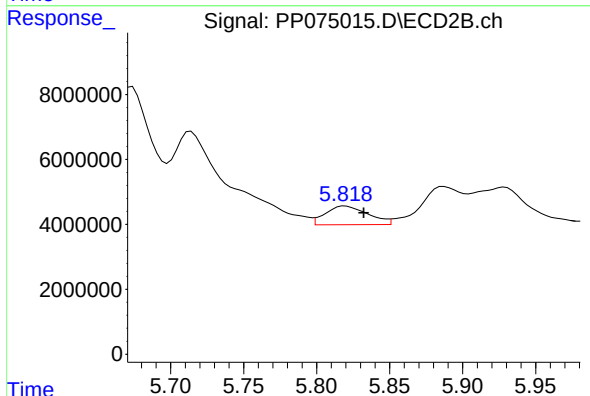


#27 AR-1254-2

R.T.: 5.820 min
Delta R.T.: -0.013 min
Response: 11651766
Conc: 33.09 ng/ml

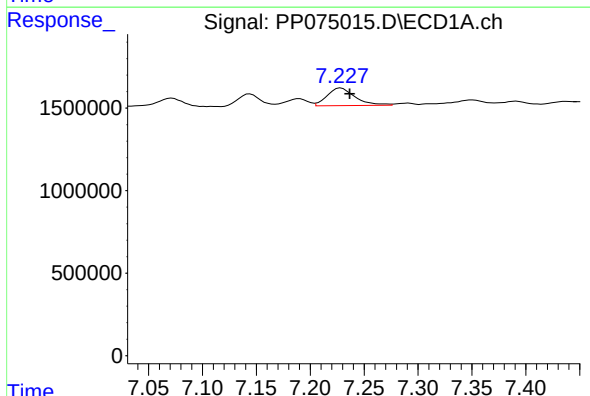


#28 AR-1254-3

R.T.: 7.228 min
Delta R.T.: -0.008 min
Response: 1934978
Conc: 21.69 ng/ml

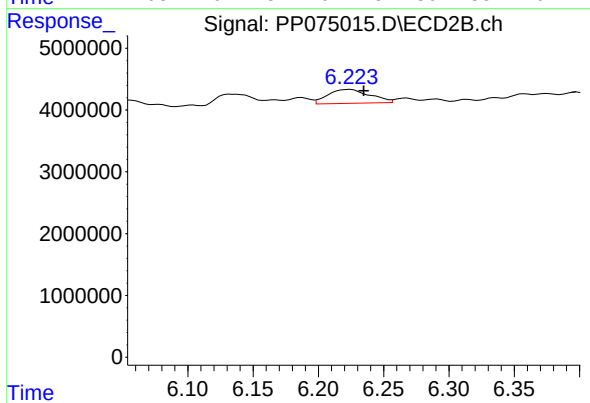

#28 AR-1254-3


R.T.: 6.224 min
Delta R.T.: -0.010 min
Response: 5056932
Conc: 8.16 ng/ml

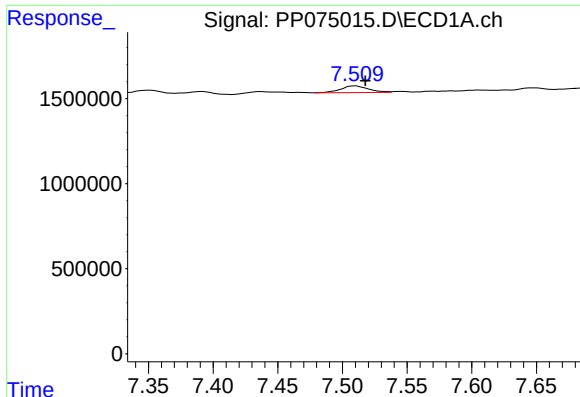

#29 AR-1254-4


R.T.: 7.510 min
Delta R.T.: -0.007 min
Response: 574800
Conc: 8.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

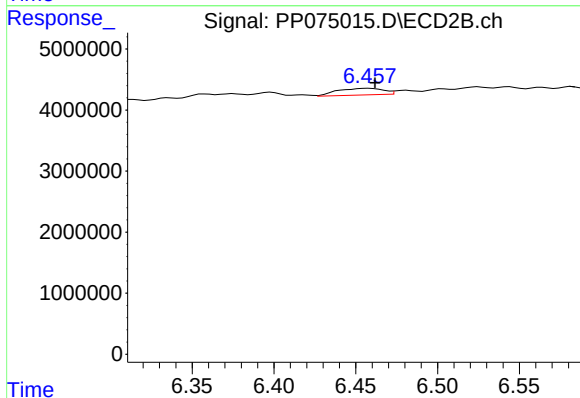


#29 AR-1254-4

R.T.: 6.458 min
Delta R.T.: -0.004 min
Response: 2113498
Conc: 4.51 ng/ml

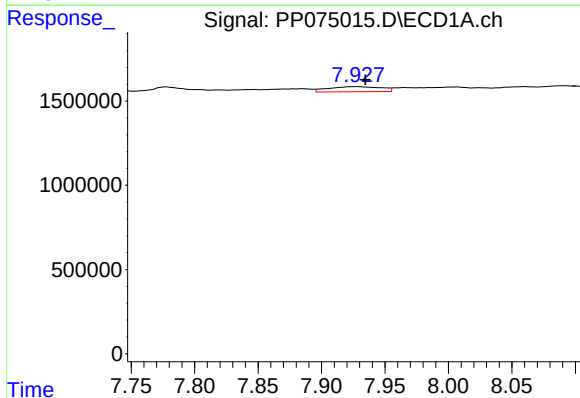


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.006 min
Response: 863839
Conc: 10.40 ng/ml

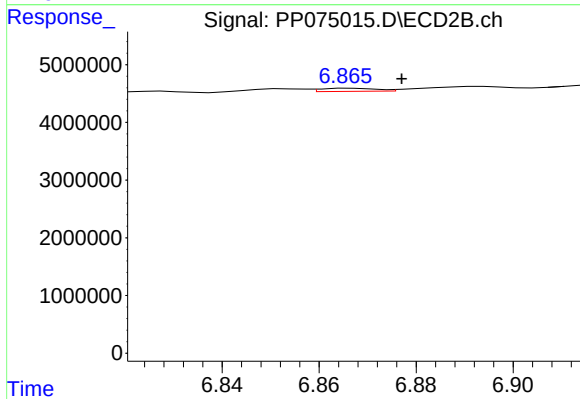

#30 AR-1254-5


R.T.: 6.867 min
Delta R.T.: -0.010 min
Response: 433712
Conc: 0.88 ng/ml

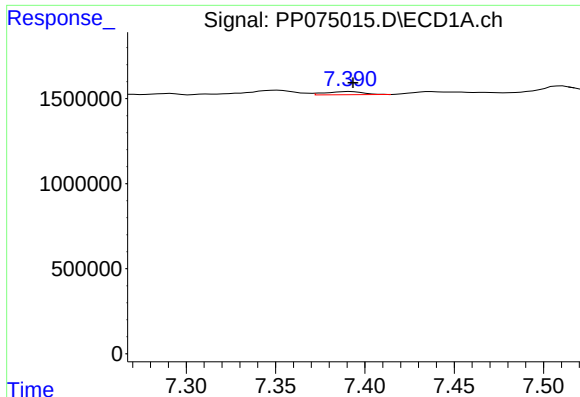

#31 AR-1260-1


R.T.: 7.392 min
Delta R.T.: -0.002 min
Response: 268531
Conc: 4.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

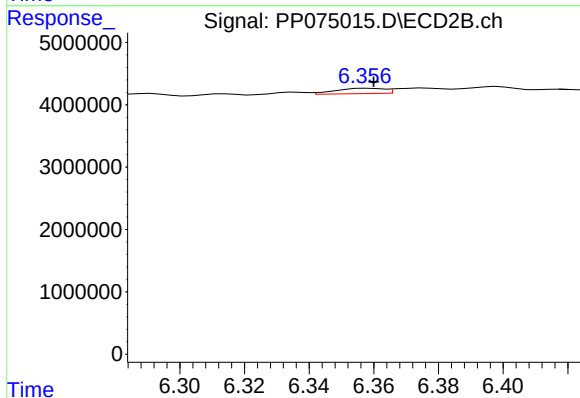


#31 AR-1260-1

R.T.: 6.358 min
Delta R.T.: -0.002 min
Response: 884902
Conc: 2.36 ng/ml

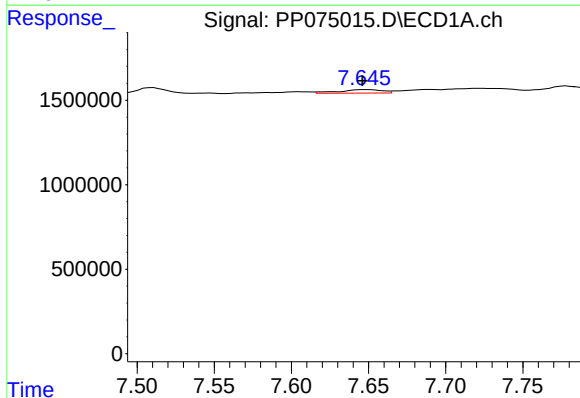


#32 AR-1260-2

R.T.: 7.648 min
Delta R.T.: 0.002 min
Response: 398330
Conc: 5.78 ng/ml

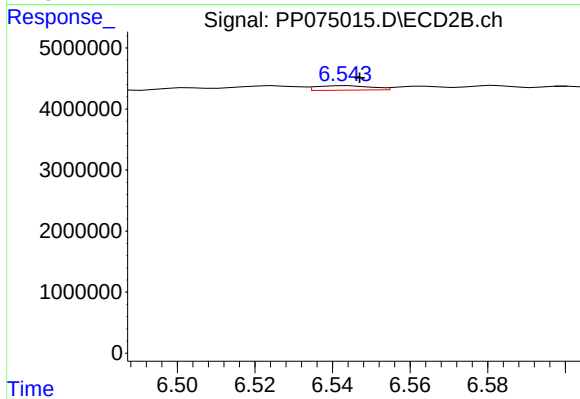

#32 AR-1260-2


R.T.: 6.544 min
Delta R.T.: -0.003 min
Response: 721058
Conc: 1.36 ng/ml

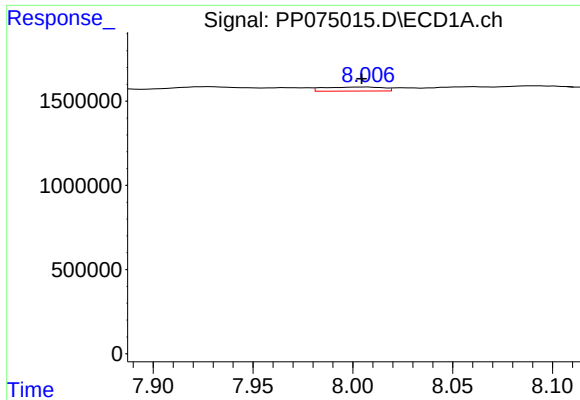

#33 AR-1260-3


R.T.: 8.007 min
Delta R.T.: 0.002 min
Response: 503913
Conc: 9.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

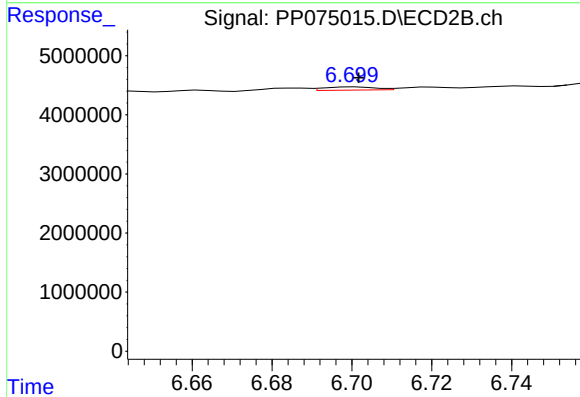


#33 AR-1260-3

R.T.: 6.701 min
Delta R.T.: 0.000 min
Response: 490222
Conc: 1.13 ng/ml

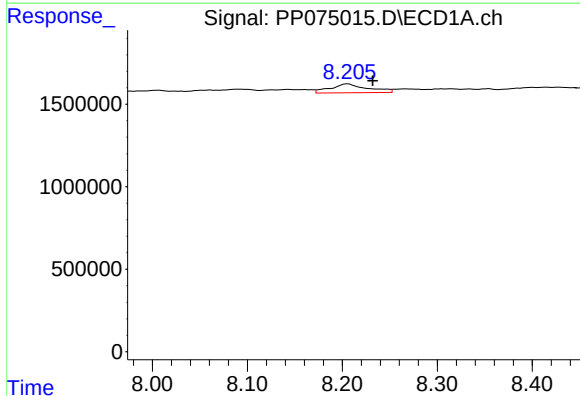


#34 AR-1260-4

R.T.: 8.206 min
Delta R.T.: -0.026 min
Response: 1456278
Conc: 22.83 ng/ml

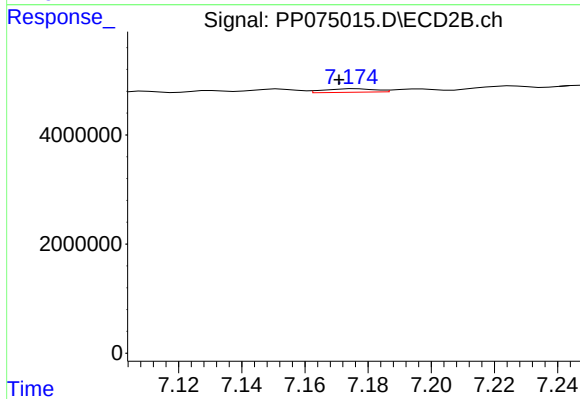

#34 AR-1260-4


R.T.: 7.176 min
Delta R.T.: 0.006 min
Response: 729488
Conc: 1.91 ng/ml

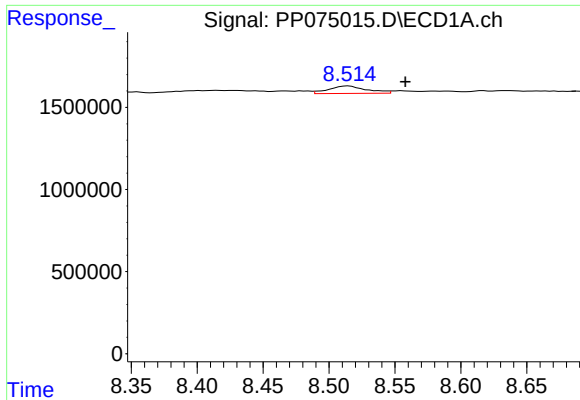

#35 AR-1260-5


R.T.: 8.515 min
Delta R.T.: -0.043 min
Response: 903382
Conc: 7.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

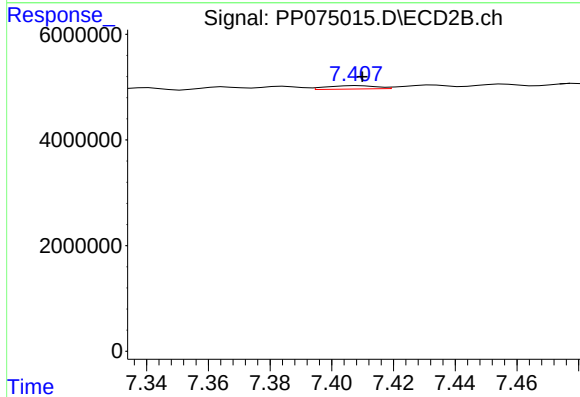


#35 AR-1260-5

R.T.: 7.408 min
Delta R.T.: -0.002 min
Response: 711735
Conc: 0.71 ng/ml

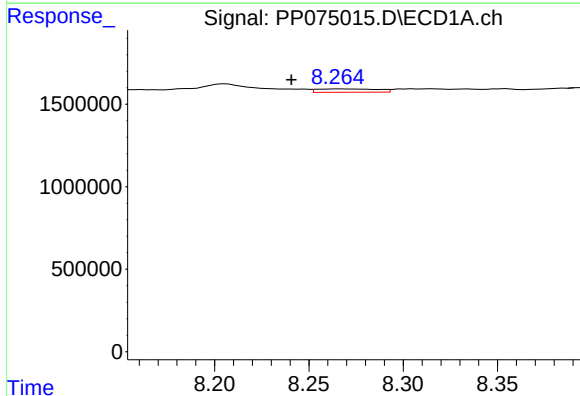


#36 AR-1262-1

R.T.: 8.266 min
Delta R.T.: 0.025 min
Response: 449053
Conc: 5.83 ng/ml

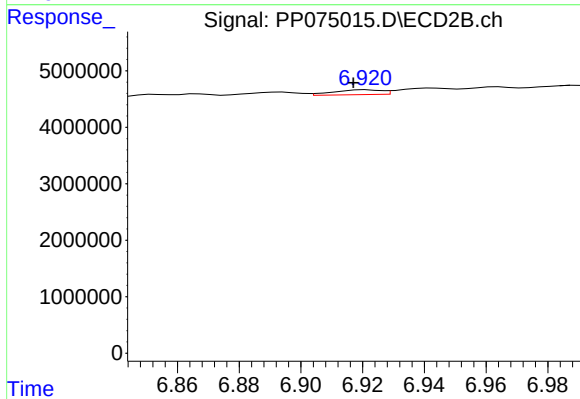

#36 AR-1262-1


R.T.: 6.921 min
Delta R.T.: 0.004 min
Response: 909165
Conc: 1.29 ng/ml

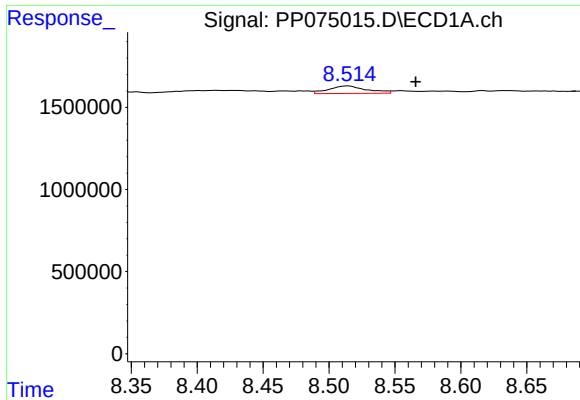

#37 AR-1262-2


R.T.: 8.515 min
Delta R.T.: -0.051 min
Response: 903382
Conc: 6.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

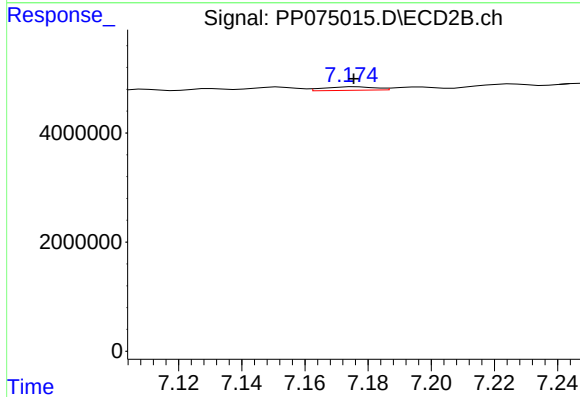


#37 AR-1262-2

R.T.: 7.176 min
Delta R.T.: 0.000 min
Response: 729488
Conc: 1.40 ng/ml

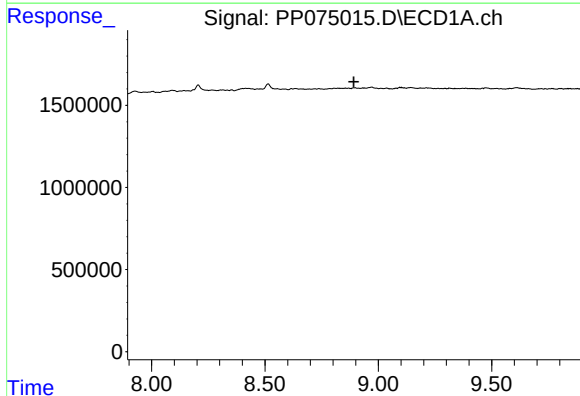


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

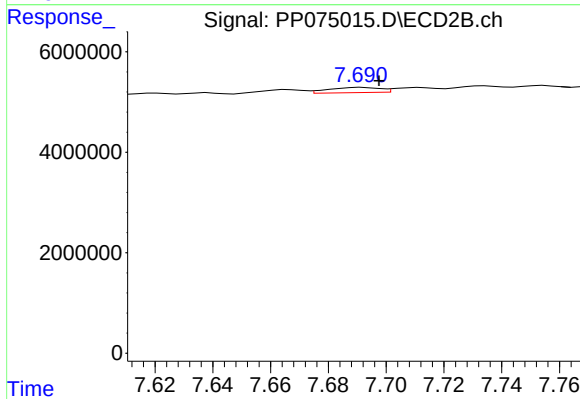

#38 AR-1262-3


R.T.: 7.691 min
Delta R.T.: -0.006 min
Response: 1280198
Conc: 2.75 ng/ml

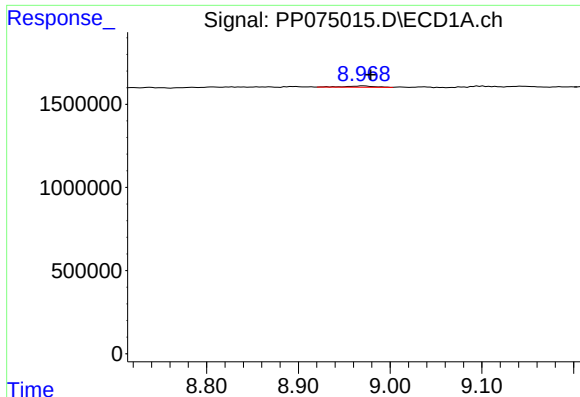

#39 AR-1262-4


R.T.: 8.971 min
Delta R.T.: -0.008 min
Response: 174018
Conc: 2.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

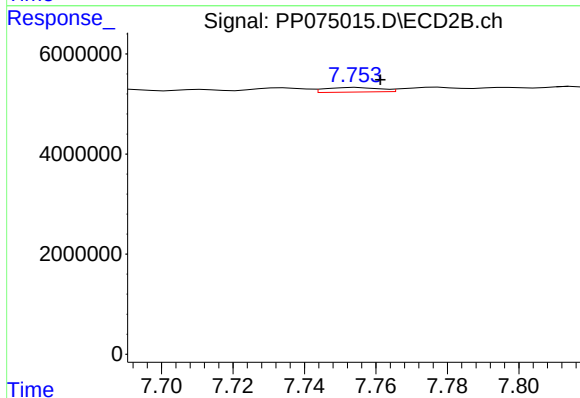


#39 AR-1262-4

R.T.: 7.755 min
Delta R.T.: -0.007 min
Response: 980342
Conc: 1.19 ng/ml

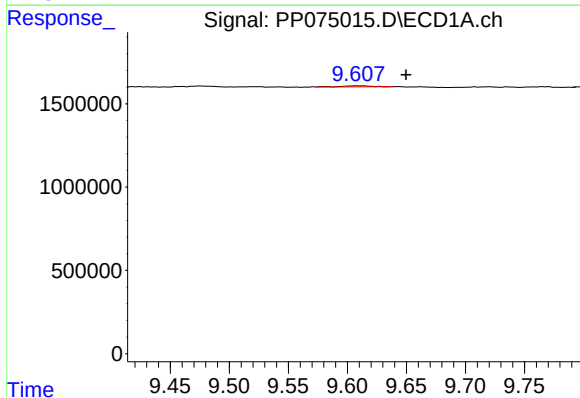


#40 AR-1262-5

R.T.: 9.608 min
Delta R.T.: -0.042 min
Response: 102868
Conc: 1.69 ng/ml

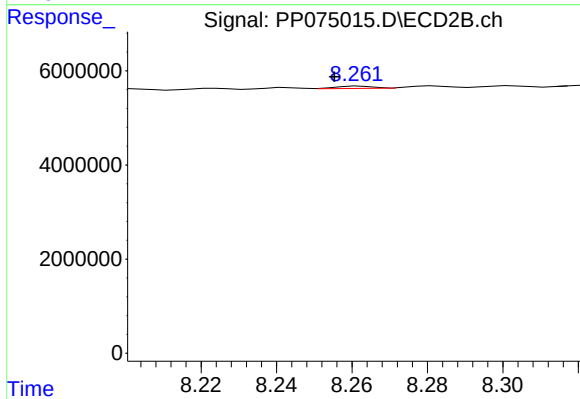

#40 AR-1262-5


R.T.: 8.262 min
Delta R.T.: 0.007 min
Response: 338851
Conc: 0.95 ng/ml

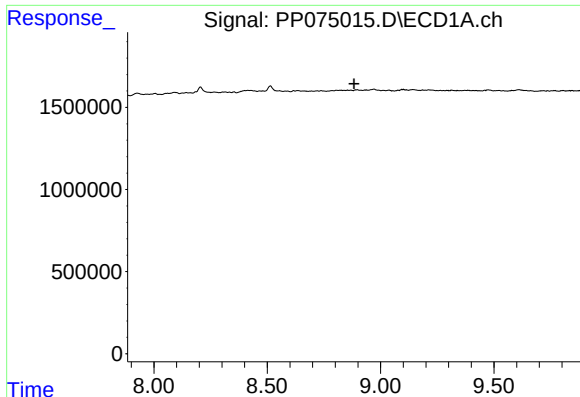

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

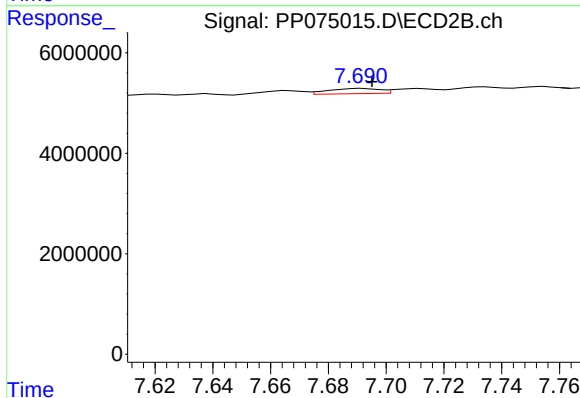


#41 AR-1268-1

R.T.: 7.691 min
Delta R.T.: -0.004 min
Response: 1280198
Conc: 0.91 ng/ml

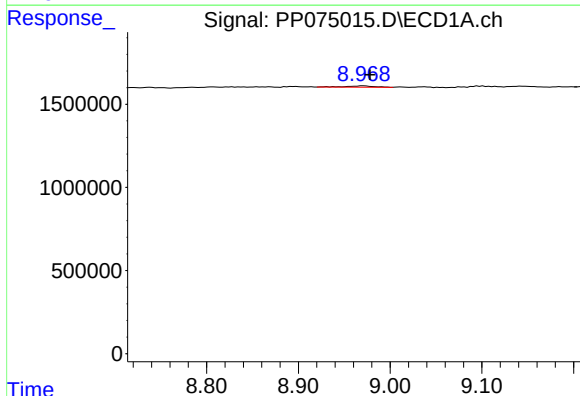


#42 AR-1268-2

R.T.: 8.971 min
Delta R.T.: -0.007 min
Response: 174018
Conc: 1.19 ng/ml

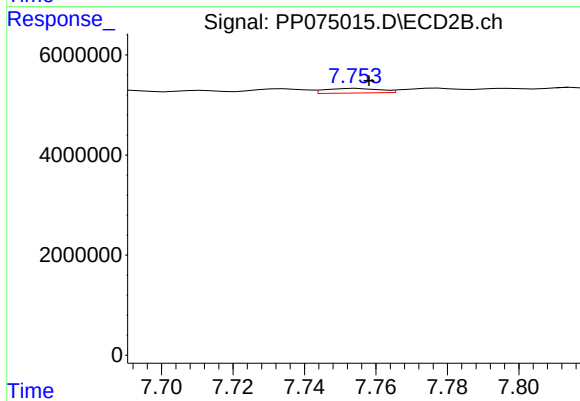

#42 AR-1268-2


R.T.: 7.755 min
Delta R.T.: -0.003 min
Response: 980342
Conc: 0.72 ng/ml

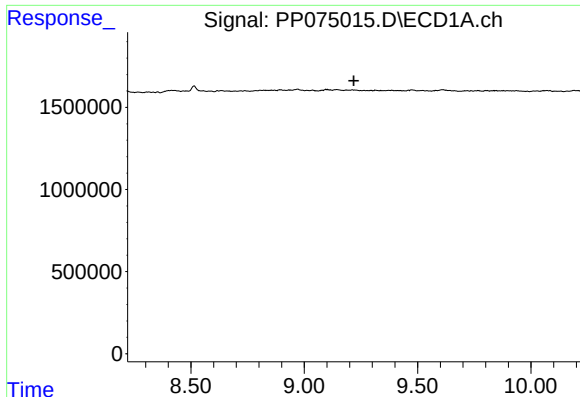

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

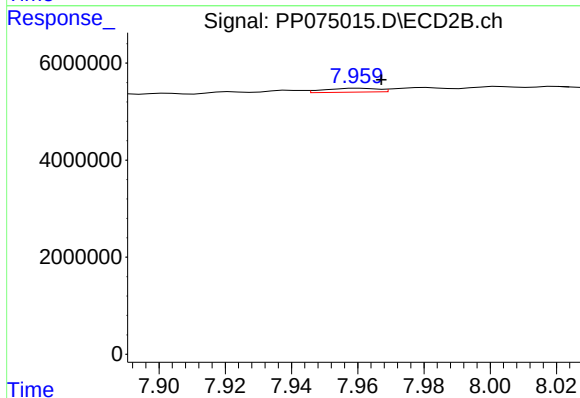


#43 AR-1268-3

R.T.: 7.961 min
Delta R.T.: -0.007 min
Response: 872947
Conc: 0.84 ng/ml

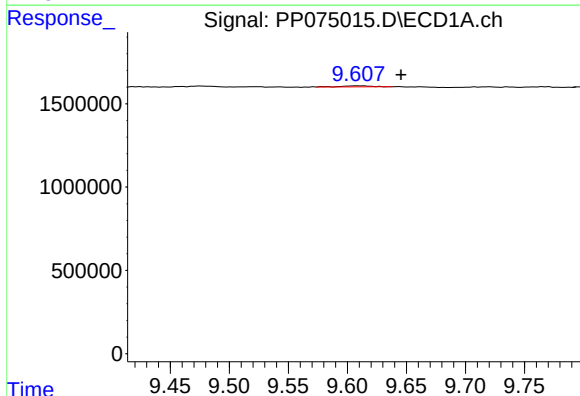


#44 AR-1268-4

R.T.: 9.608 min
Delta R.T.: -0.037 min
Response: 102868
Conc: 1.53 ng/ml

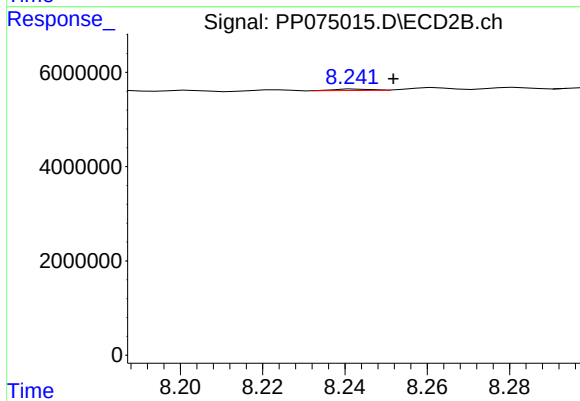

#44 AR-1268-4


R.T.: 8.243 min
Delta R.T.: -0.009 min
Response: 171236
Conc: 0.45 ng/ml

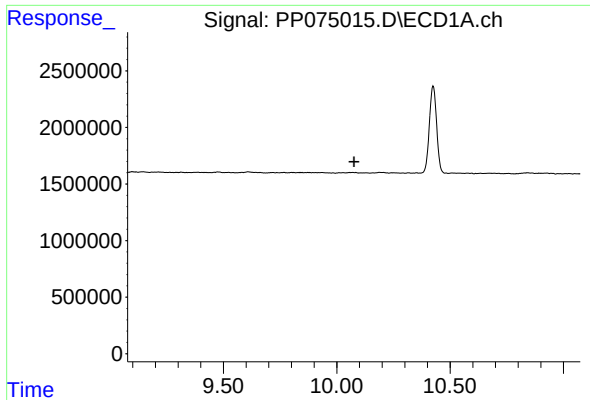

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-I

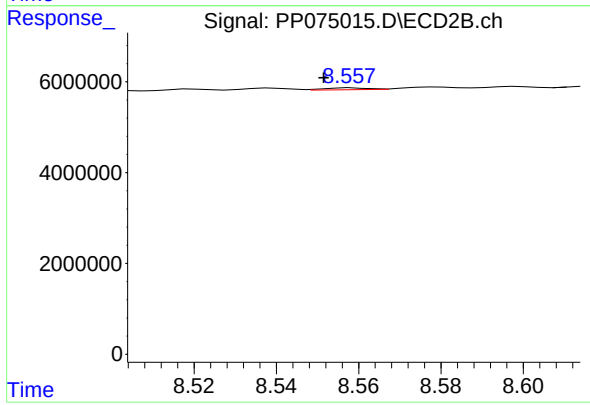

#45 AR-1268-5

R.T.: 8.559 min
Delta R.T.: 0.007 min
Response: 305800
Conc: 0.10 ng/ml