

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP090925\  
 Data File : PP075016.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 09 Sep 2025 18:28  
 Operator : YP\AJ  
 Sample : Q3034-10  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 PASSAIC-J

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 10 01:52:02 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP081925.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Wed Aug 20 06:20:44 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml   | ng/ml     |
|-----------------------------|-----------------|--------|-------|----------|----------|---------|-----------|
| -----                       |                 |        |       |          |          |         |           |
| System Monitoring Compounds |                 |        |       |          |          |         |           |
| 1)                          | SA Tetrachlo... | 4.656  | 3.798 | 28960406 | 110.3E6  | 23.666  | 22.802    |
| 2)                          | SA Decachlor... | 10.427 | 8.803 | 23644988 | 147.3E6  | 23.944  | 19.638    |
| Target Compounds            |                 |        |       |          |          |         |           |
| 3)                          | L1 AR-1016-1    | 5.806  | 4.895 | 5643397  | 48668451 | 128.001 | 95.549 #  |
| 4)                          | L1 AR-1016-2    | 5.828  | 4.952 | 8303455  | 25551257 | 132.133 | 107.351   |
| 5)                          | L1 AR-1016-3    | 5.891  | 5.073 | 6280796  | 15964868 | 139.841 | 115.768   |
| 6)                          | L1 AR-1016-4    | 5.988  | 5.113 | 5668000  | 18070894 | 161.106 | 129.259   |
| 7)                          | L1 AR-1016-5    | 6.280  | 5.327 | 6866703  | 25863010 | 206.915 | 155.723   |
| 8)                          | L2 AR-1221-1    | 4.850  | 4.015 | 348039   | 229504   | 19.783  | 3.710 #   |
| 9)                          | L2 AR-1221-2    | 4.957  | 4.096 | 571692   | 1910365  | 42.800  | 42.253    |
| 10)                         | L2 AR-1221-3    | 5.017  | 4.166 | 471952   | 1792256  | 12.448  | 10.909    |
| 11)                         | L3 AR-1232-1    | 5.017  | 4.166 | 471952   | 1792256  | 15.538  | 13.992    |
| 12)                         | L3 AR-1232-2    | 5.543  | 4.895 | 2710759  | 48668451 | 172.022 | 209.965   |
| 13)                         | L3 AR-1232-3    | 5.828  | 5.073 | 8303455  | 15964868 | 271.855 | 265.816   |
| 14)                         | L3 AR-1232-4    | 5.988  | 5.156 | 5668000  | 28818850 | 328.213 | 390.990   |
| 15)                         | L3 AR-1232-5    | 6.078  | 5.327 | 5150198  | 25863010 | 396.750 | 416.582   |
| 16)                         | L4 AR-1242-1    | 5.806  | 4.895 | 5643397  | 48668451 | 147.443 | 115.396   |
| 17)                         | L4 AR-1242-2    | 5.828  | 4.952 | 8303455  | 25551257 | 147.011 | 127.576   |
| 18)                         | L4 AR-1242-3    | 5.891  | 5.073 | 6280796  | 15964868 | 154.688 | 134.954   |
| 19)                         | L4 AR-1242-4    | 5.988  | 5.156 | 5668000  | 28818850 | 178.566 | 168.374   |
| 20)                         | L4 AR-1242-5    | 6.717  | 5.676 | 4277274  | 20060497 | 118.581 | 108.339   |
| 21)                         | L5 AR-1248-1    | 5.806  | 4.895 | 5643397  | 48668451 | 186.719 | 176.244   |
| 22)                         | L5 AR-1248-2    | 6.078  | 5.113 | 5150198  | 18070894 | 119.505 | 102.237   |
| 23)                         | L5 AR-1248-3    | 6.280  | 5.156 | 6866703  | 28818850 | 147.027 | 126.842   |
| 24)                         | L5 AR-1248-4    | 6.677  | 5.327 | 3912189  | 25863010 | 71.130  | 118.626 # |
| 25)                         | L5 AR-1248-5    | 6.717  | 5.720 | 4277274  | 17412101 | 77.109  | 47.403 #  |
| 26)                         | L6 AR-1254-1    | 6.652  | 5.676 | 3465870  | 20060497 | 59.480  | 42.081 #  |
| 27)                         | L6 AR-1254-2    | 6.873  | 5.822 | 2741295  | 4102820  | 33.588  | 11.651 #  |
| 28)                         | L6 AR-1254-3    | 7.228  | 6.232 | 898249   | 1520768  | 10.069  | 2.454 #   |
| 29)                         | L6 AR-1254-4    | 7.514  | 6.457 | 189869   | 428551   | 2.881   | 0.914 #   |
| 30)                         | L6 AR-1254-5    | 7.931  | 6.882 | 319869   | 368334   | 3.850   | 0.751 #   |
| 31)                         | L7 AR-1260-1    | 7.393  | 6.356 | 193762   | 287534   | 3.352   | 0.766 #   |
| 32)                         | L7 AR-1260-2    | 7.652  | 6.539 | 152204   | 605120   | 2.208   | 1.144 #   |
| 33)                         | L7 AR-1260-3    | 8.002  | 6.710 | 198870   | 345456   | 3.833   | 0.798 #   |
| 34)                         | L7 AR-1260-4    | 8.256  | 7.163 | 116458   | 361691   | 1.826   | 0.948 #   |
| 35)                         | L7 AR-1260-5    | 8.516f | 7.409 | 1064641  | 335756   | 9.387   | 0.334 #   |
| 36)                         | L8 AR-1262-1    | 8.256  | 6.910 | 116458   | 528477   | 1.512   | 0.747 #   |
| 37)                         | L8 AR-1262-2    | 8.516f | 7.182 | 1064641  | 187227   | 8.042   | 0.360 #   |
| 38)                         | L8 AR-1262-3    | 0.000  | 7.698 | 0        | 413228   | N.D.    | 0.886 #   |
| 39)                         | L8 AR-1262-4    | 8.973  | 7.760 | 187151   | 463706   | 2.484   | 0.564 #   |
| 40)                         | L8 AR-1262-5    | 9.607f | 8.264 | 247292   | 216360   | 4.057   | 0.604 #   |
| 41)                         | L9 AR-1268-1    | 0.000  | 7.698 | 0        | 413228   | N.D.    | 0.293 #   |

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP090925\  
Data File : PP075016.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 09 Sep 2025 18:28  
Operator : YP\AJ  
Sample : Q3034-10  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 10 01:52:02 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP081925.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Aug 20 06:20:44 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

|     | Compound     | RT#1   | RT#2  | Resp#1 | Resp#2 | ng/ml | ng/ml   |
|-----|--------------|--------|-------|--------|--------|-------|---------|
| 42) | L9 AR-1268-2 | 8.973  | 7.760 | 187151 | 463706 | 1.275 | 0.340 # |
| 43) | L9 AR-1268-3 | 0.000  | 7.964 | 0      | 519125 | N.D.  | 0.498 # |
| 44) | L9 AR-1268-4 | 9.607f | 8.244 | 247292 | 130537 | 3.676 | 0.341 # |
| 45) | L9 AR-1268-5 | 10.074 | 8.551 | 141514 | 830763 | 0.382 | 0.265 # |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP090925\  
Data File : PP075016.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 09 Sep 2025 18:28  
Operator : YP\AJ  
Sample : Q3034-10  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 10 01:52:02 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP081925.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Wed Aug 20 06:20:44 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

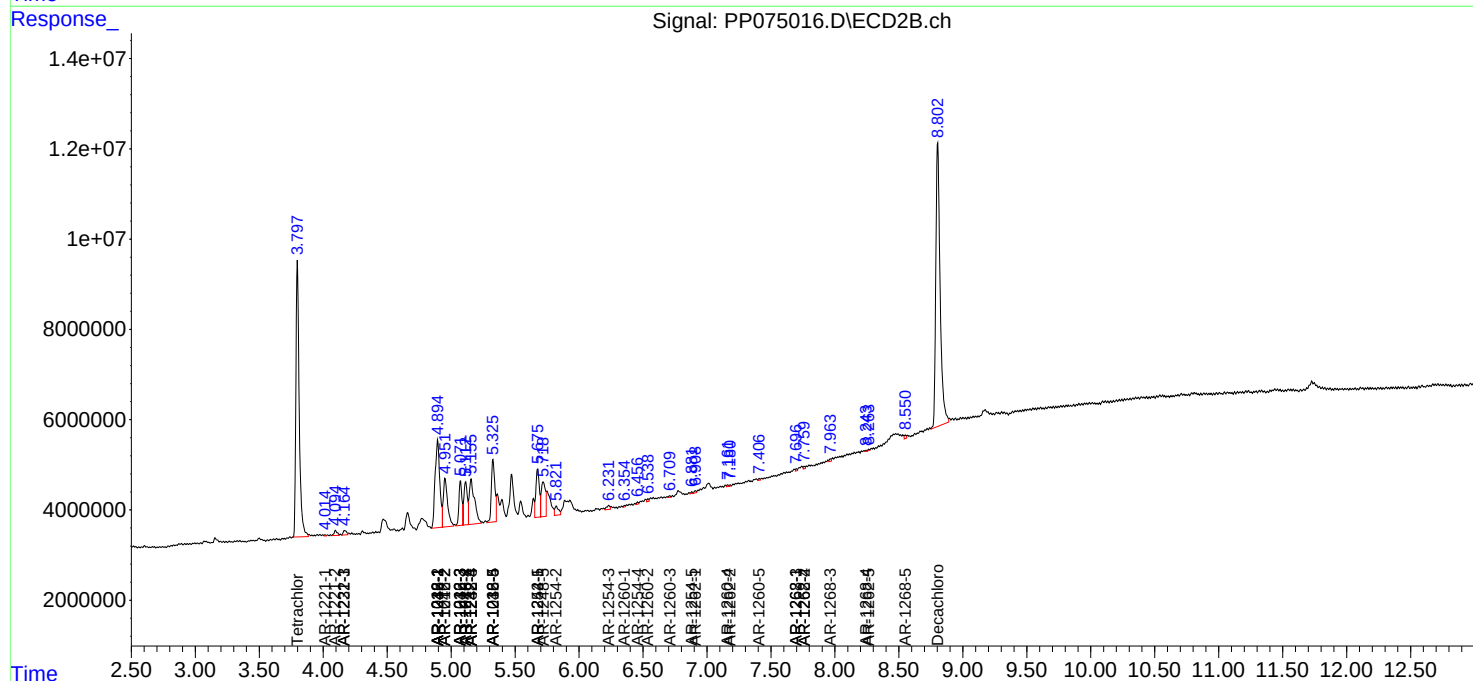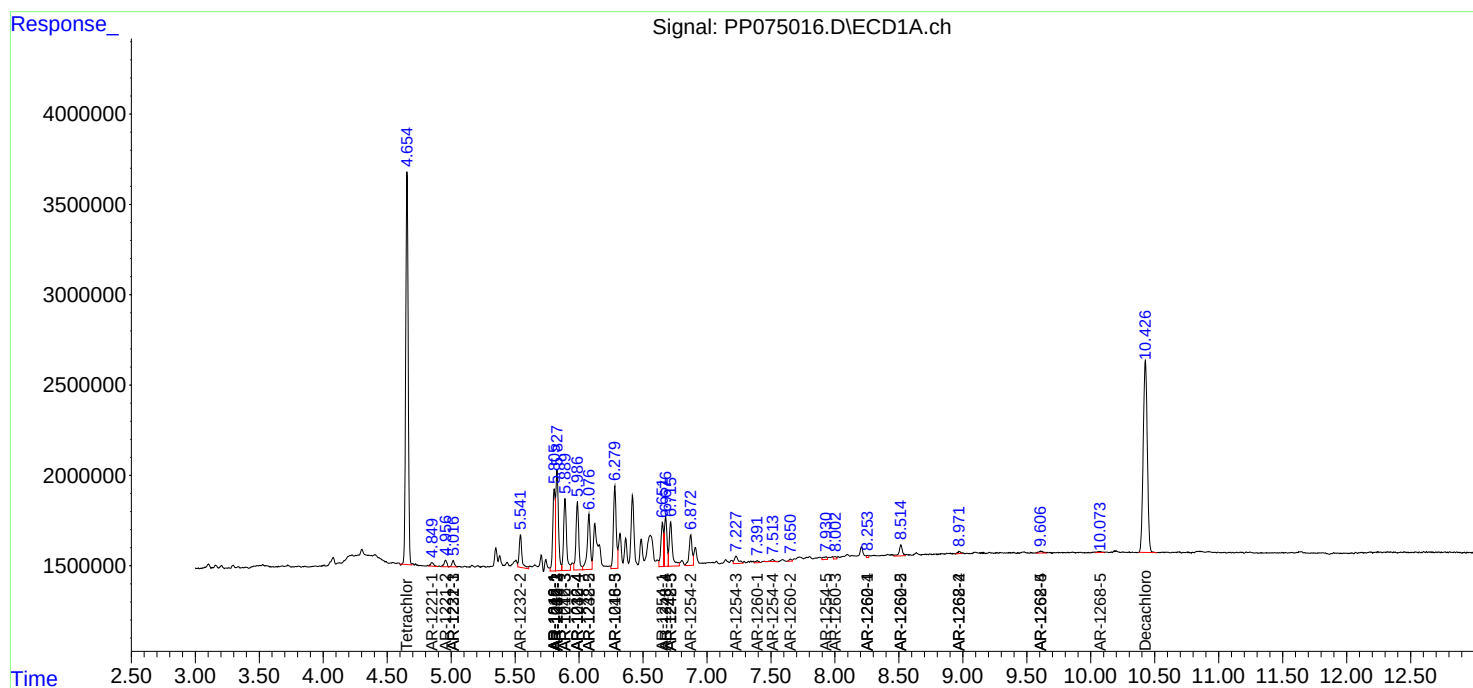


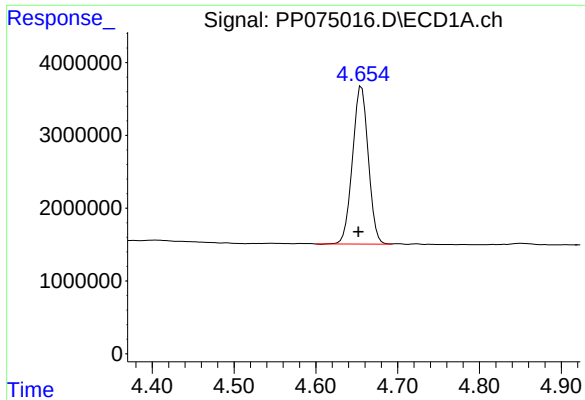

#1 Tetrachloro-m-xylene


R.T.: 4.656 min  
Delta R.T.: 0.004 min  
Response: 28960406  
Conc: 23.67 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

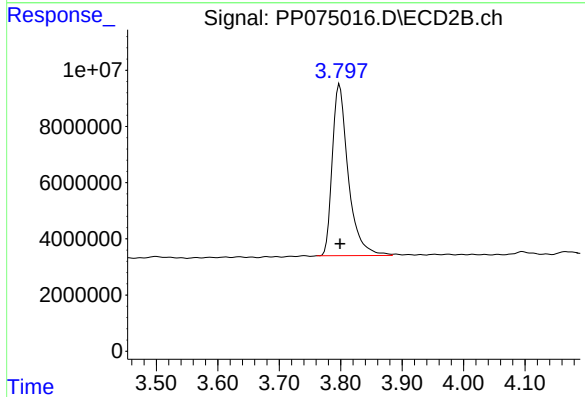


#1 Tetrachloro-m-xylene

R.T.: 3.798 min  
Delta R.T.: 0.000 min  
Response: 110256783  
Conc: 22.80 ng/ml

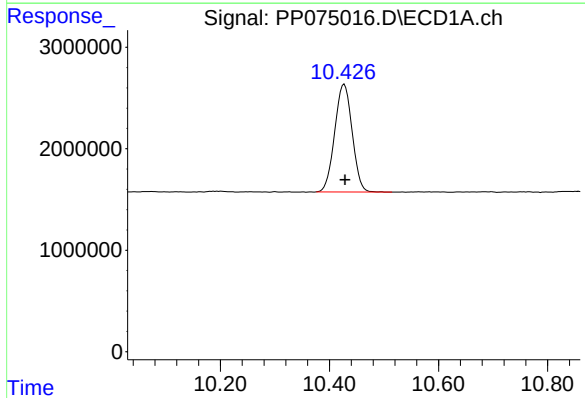


#2 Decachlorobiphenyl

R.T.: 10.427 min  
Delta R.T.: -0.001 min  
Response: 23644988  
Conc: 23.94 ng/ml

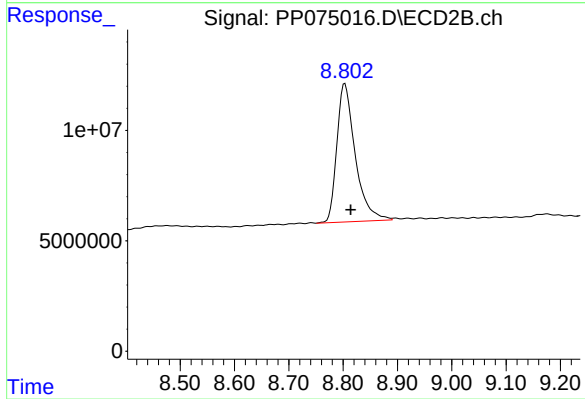

#2 Decachlorobiphenyl


R.T.: 8.803 min  
Delta R.T.: -0.011 min  
Response: 147272354  
Conc: 19.64 ng/ml

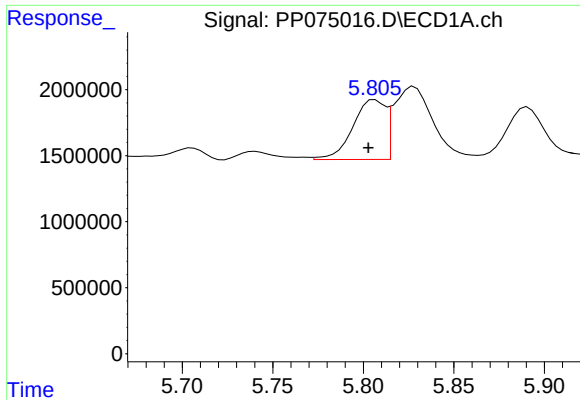

#3 AR-1016-1


R.T.: 5.806 min  
Delta R.T.: 0.004 min  
Response: 5643397  
Conc: 128.00 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

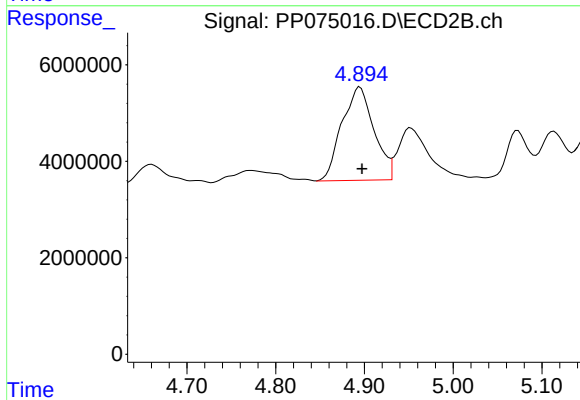


#3 AR-1016-1

R.T.: 4.895 min  
Delta R.T.: -0.002 min  
Response: 48668451  
Conc: 95.55 ng/ml

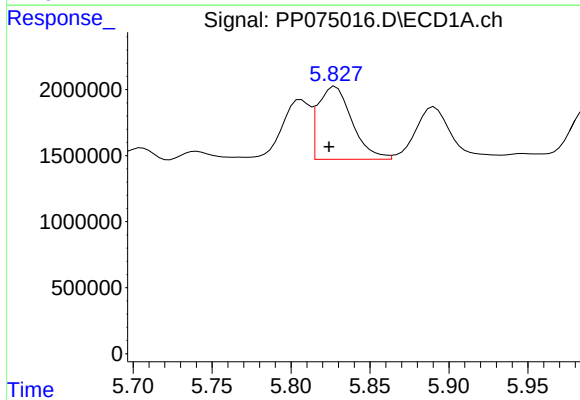


#4 AR-1016-2

R.T.: 5.828 min  
Delta R.T.: 0.004 min  
Response: 8303455  
Conc: 132.13 ng/ml

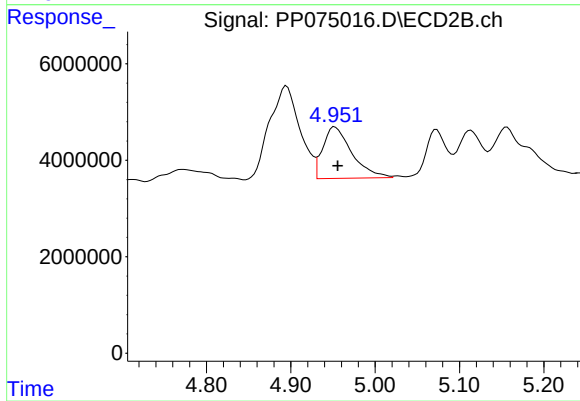

#4 AR-1016-2


R.T.: 4.952 min  
Delta R.T.: -0.003 min  
Response: 25551257  
Conc: 107.35 ng/ml

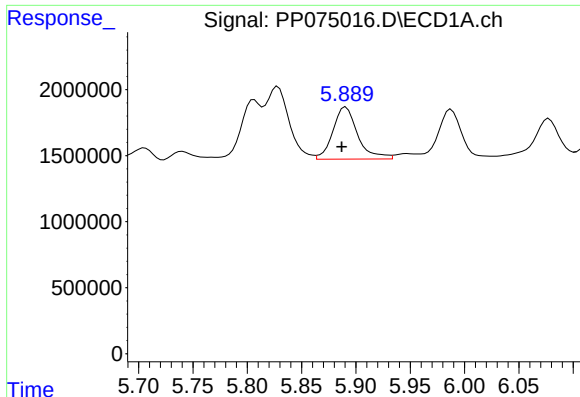

#5 AR-1016-3


R.T.: 5.891 min  
Delta R.T.: 0.004 min  
Response: 6280796  
Conc: 139.84 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

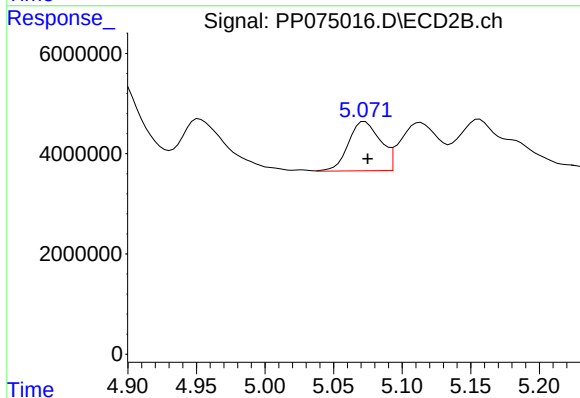


#5 AR-1016-3

R.T.: 5.073 min  
Delta R.T.: -0.002 min  
Response: 15964868  
Conc: 115.77 ng/ml

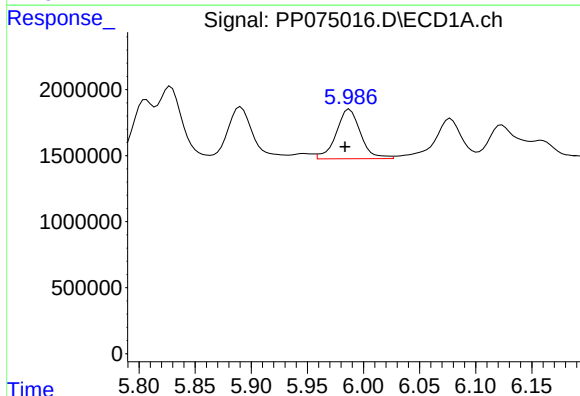


#6 AR-1016-4

R.T.: 5.988 min  
Delta R.T.: 0.004 min  
Response: 5668000  
Conc: 161.11 ng/ml

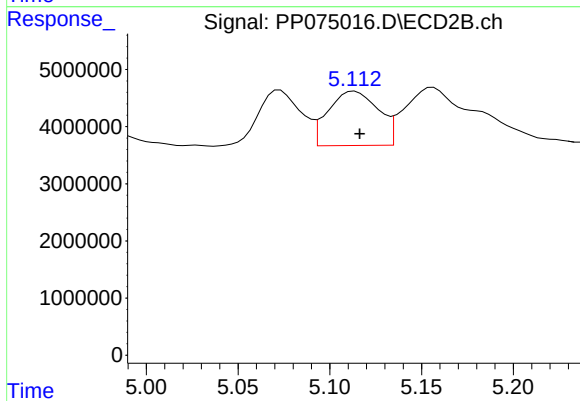

#6 AR-1016-4


R.T.: 5.113 min  
Delta R.T.: -0.003 min  
Response: 18070894  
Conc: 129.26 ng/ml

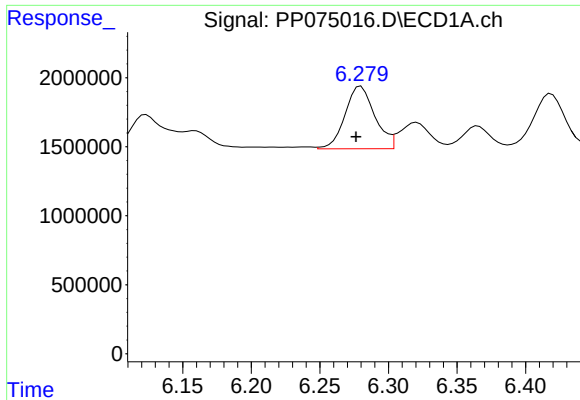

#7 AR-1016-5


R.T.: 6.280 min  
Delta R.T.: 0.004 min  
Response: 6866703  
Conc: 206.92 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

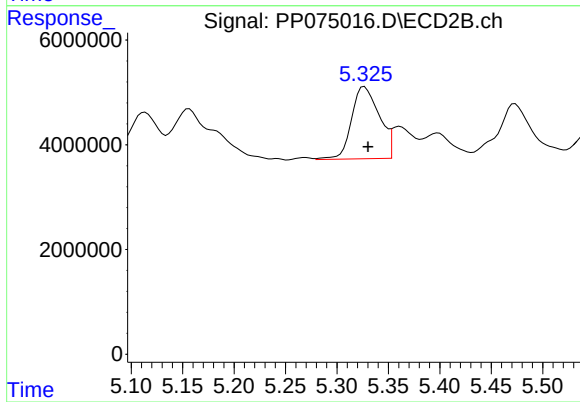


#7 AR-1016-5

R.T.: 5.327 min  
Delta R.T.: -0.004 min  
Response: 25863010  
Conc: 155.72 ng/ml

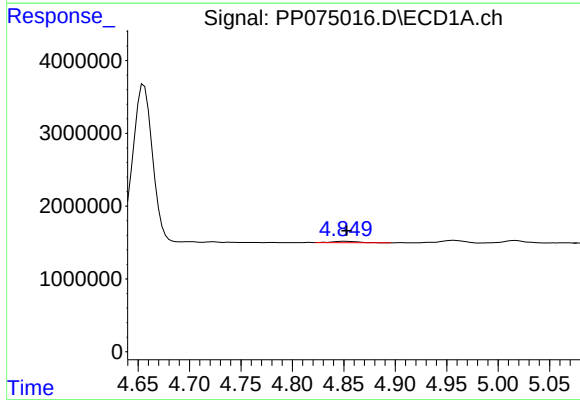


#8 AR-1221-1

R.T.: 4.850 min  
Delta R.T.: -0.003 min  
Response: 348039  
Conc: 19.78 ng/ml

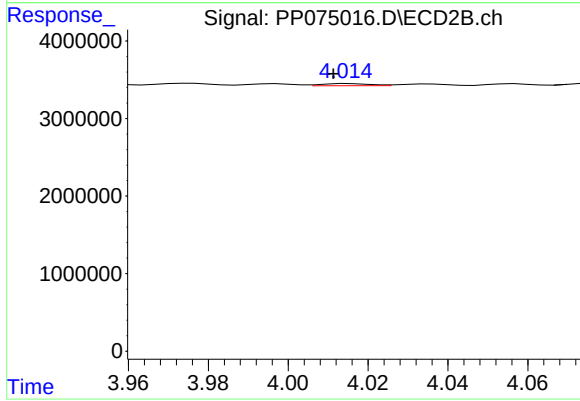

#8 AR-1221-1


R.T.: 4.015 min  
Delta R.T.: 0.004 min  
Response: 229504  
Conc: 3.71 ng/ml

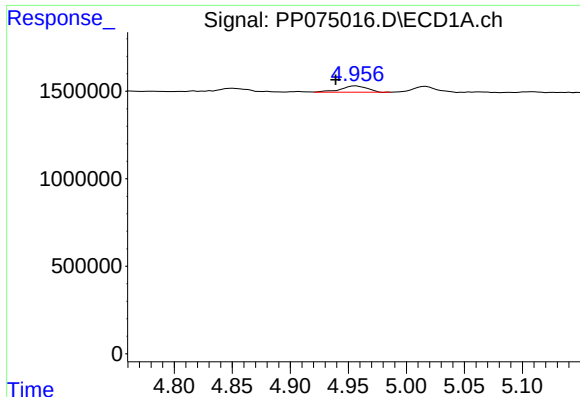

#9 AR-1221-2


R.T.: 4.957 min  
Delta R.T.: 0.018 min  
Response: 571692  
Conc: 42.80 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

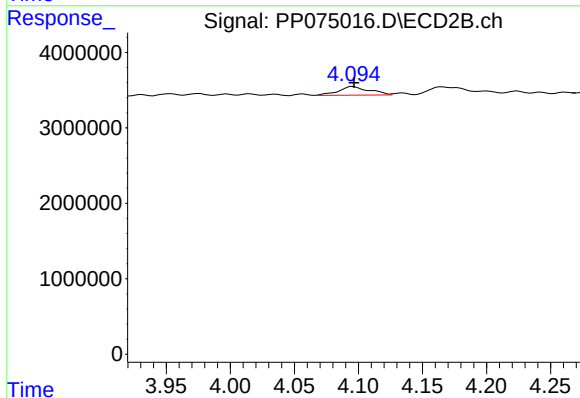


#9 AR-1221-2

R.T.: 4.096 min  
Delta R.T.: 0.000 min  
Response: 1910365  
Conc: 42.25 ng/ml

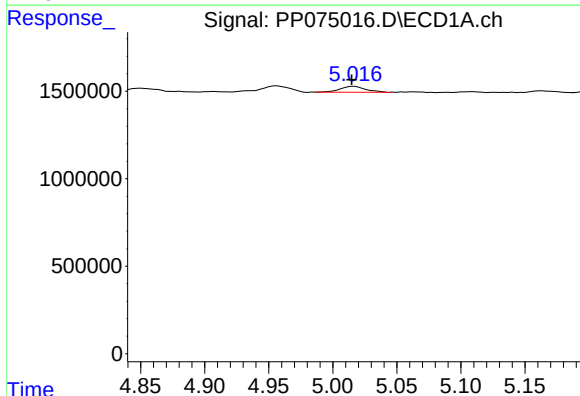

#10 AR-1221-3


R.T.: 5.017 min  
Delta R.T.: 0.002 min  
Response: 471952  
Conc: 12.45 ng/ml

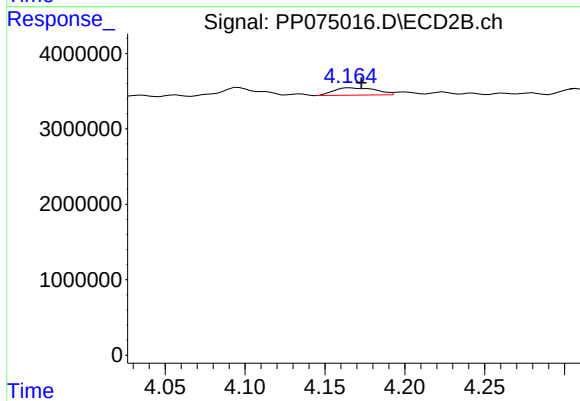

#10 AR-1221-3

R.T.: 4.166 min  
Delta R.T.: -0.007 min  
Response: 1792256  
Conc: 10.91 ng/ml




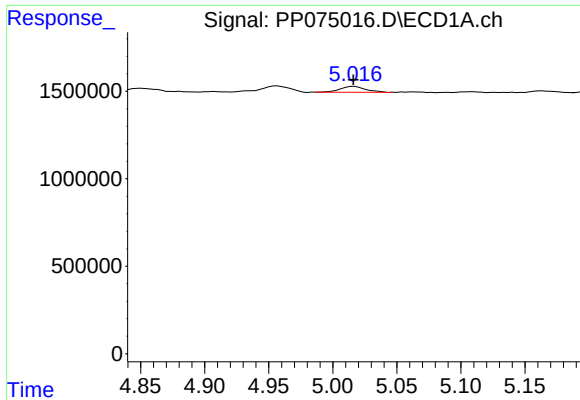

#11 AR-1232-1


R.T.: 5.017 min  
Delta R.T.: 0.000 min  
Response: 471952  
Conc: 15.54 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

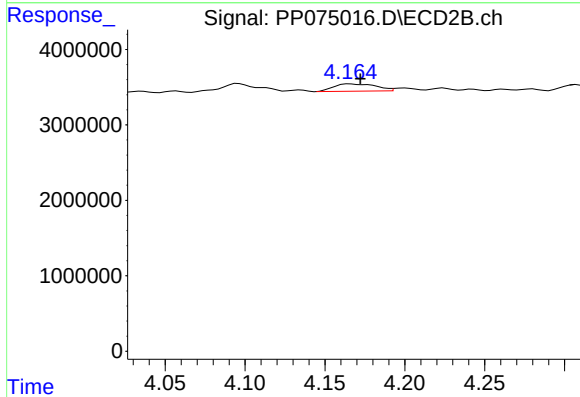


#11 AR-1232-1

R.T.: 4.166 min  
Delta R.T.: -0.007 min  
Response: 1792256  
Conc: 13.99 ng/ml

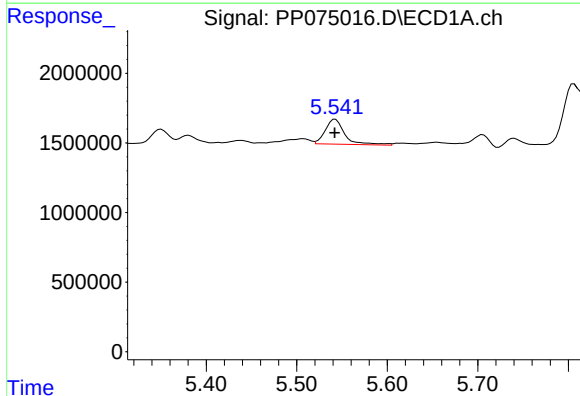


#12 AR-1232-2

R.T.: 5.543 min  
Delta R.T.: 0.000 min  
Response: 2710759  
Conc: 172.02 ng/ml

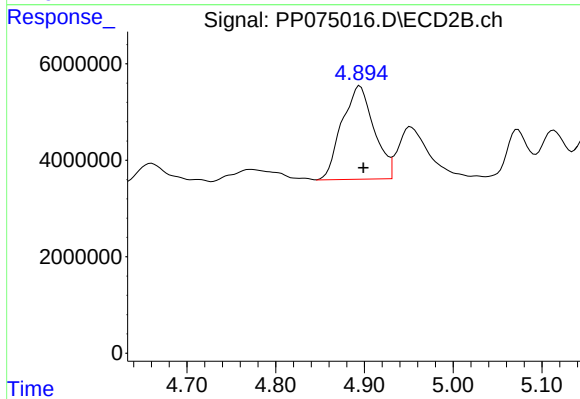

#12 AR-1232-2


R.T.: 4.895 min  
Delta R.T.: -0.004 min  
Response: 48668451  
Conc: 209.96 ng/ml

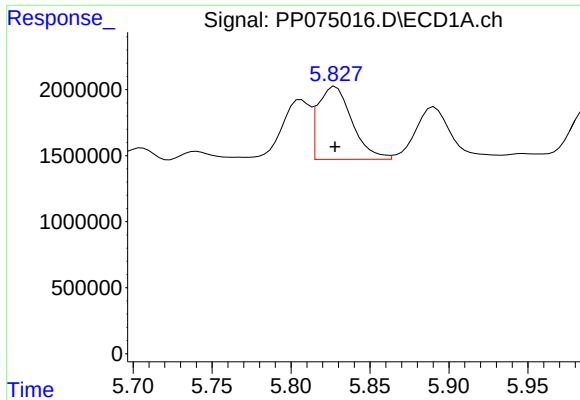

#13 AR-1232-3


R.T.: 5.828 min  
Delta R.T.: 0.000 min  
Response: 8303455  
Conc: 271.85 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

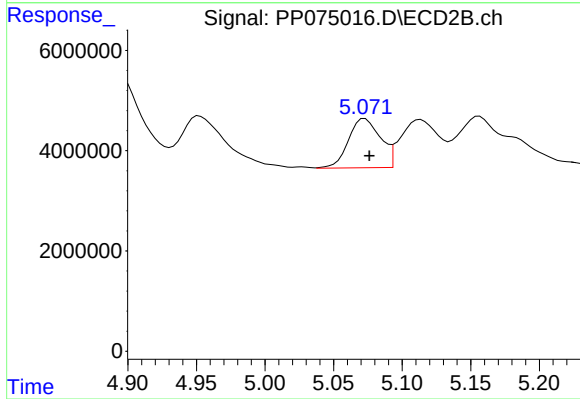


#13 AR-1232-3

R.T.: 5.073 min  
Delta R.T.: -0.003 min  
Response: 15964868  
Conc: 265.82 ng/ml

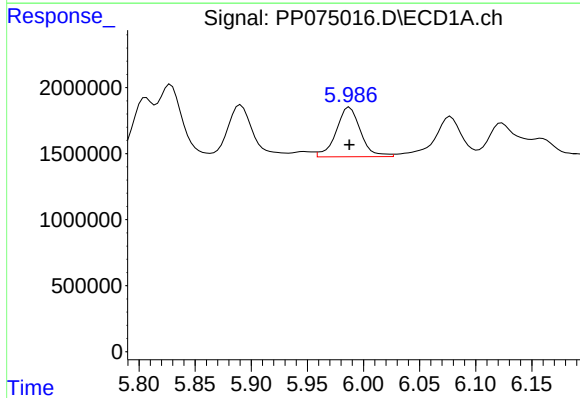


#14 AR-1232-4

R.T.: 5.988 min  
Delta R.T.: 0.000 min  
Response: 5668000  
Conc: 328.21 ng/ml

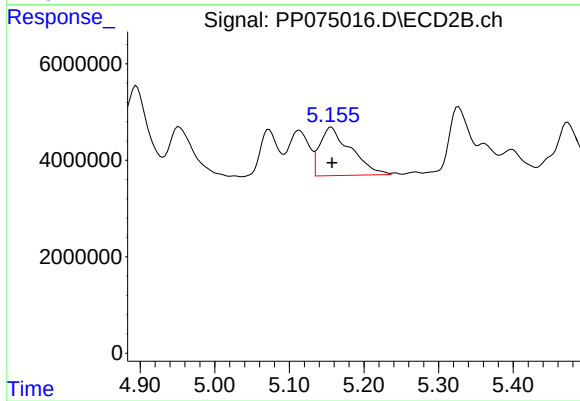

#14 AR-1232-4


R.T.: 5.156 min  
Delta R.T.: 0.000 min  
Response: 28818850  
Conc: 390.99 ng/ml

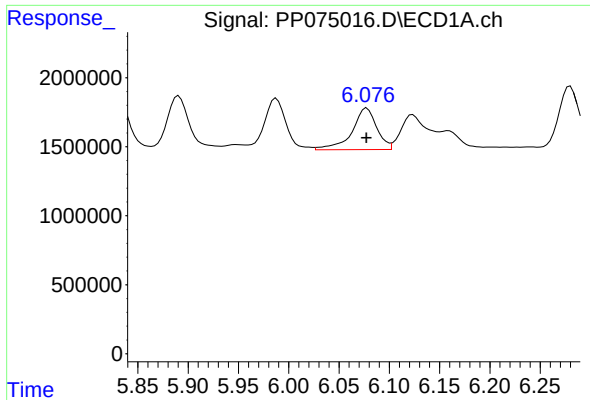

#15 AR-1232-5


R.T.: 6.078 min  
Delta R.T.: 0.000 min  
Response: 5150198  
Conc: 396.75 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

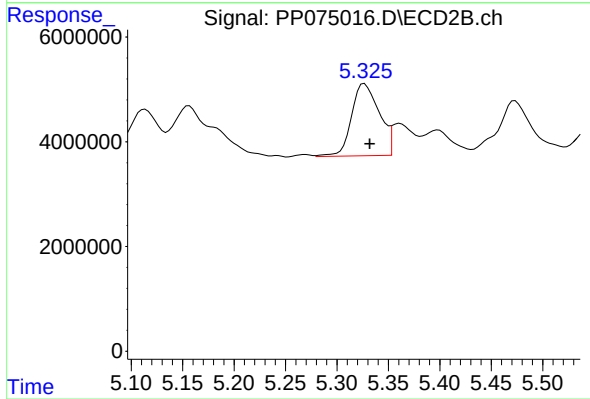


#15 AR-1232-5

R.T.: 5.327 min  
Delta R.T.: -0.005 min  
Response: 25863010  
Conc: 416.58 ng/ml

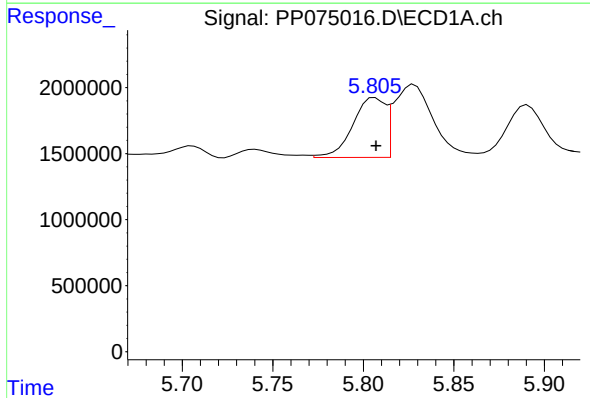


#16 AR-1242-1

R.T.: 5.806 min  
Delta R.T.: 0.000 min  
Response: 5643397  
Conc: 147.44 ng/ml

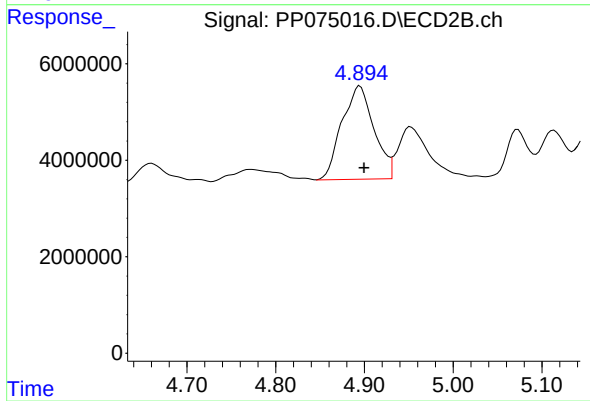

#16 AR-1242-1


R.T.: 4.895 min  
Delta R.T.: -0.005 min  
Response: 48668451  
Conc: 115.40 ng/ml

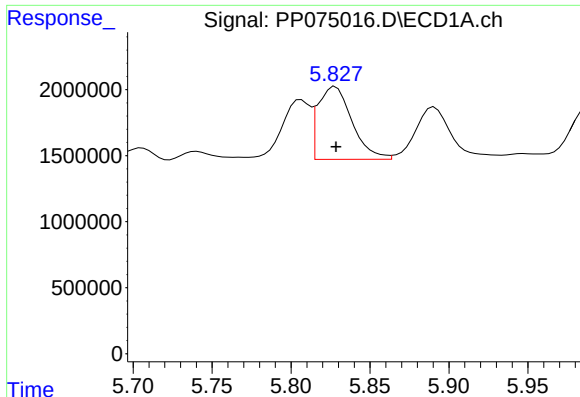

#17 AR-1242-2


R.T.: 5.828 min  
Delta R.T.: 0.000 min  
Response: 8303455  
Conc: 147.01 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

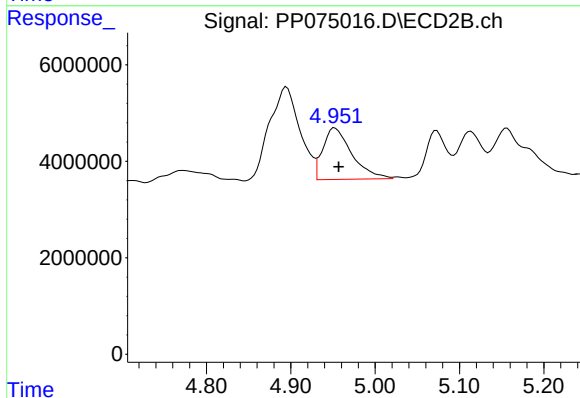


#17 AR-1242-2

R.T.: 4.952 min  
Delta R.T.: -0.005 min  
Response: 25551257  
Conc: 127.58 ng/ml

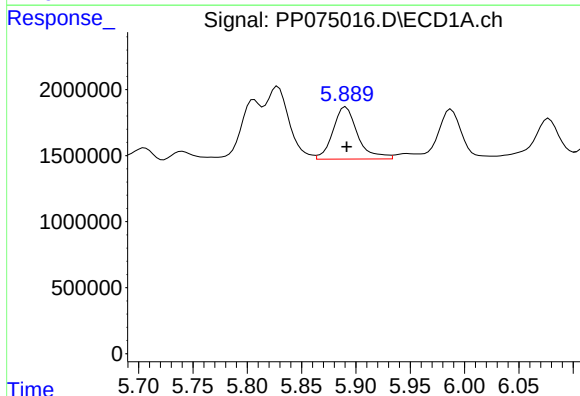


#18 AR-1242-3

R.T.: 5.891 min  
Delta R.T.: 0.000 min  
Response: 6280796  
Conc: 154.69 ng/ml

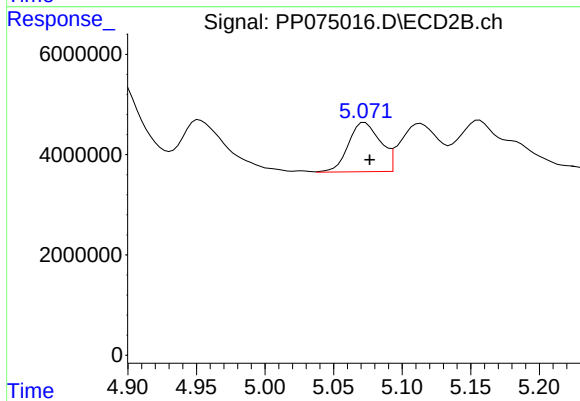

#18 AR-1242-3


R.T.: 5.073 min  
Delta R.T.: -0.003 min  
Response: 15964868  
Conc: 134.95 ng/ml

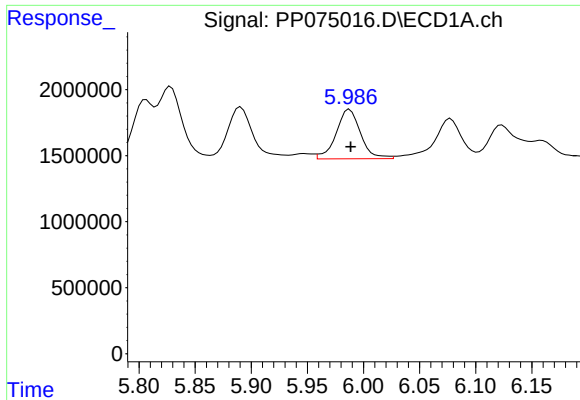

#19 AR-1242-4


R.T.: 5.988 min  
Delta R.T.: 0.000 min  
Response: 5668000  
Conc: 178.57 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

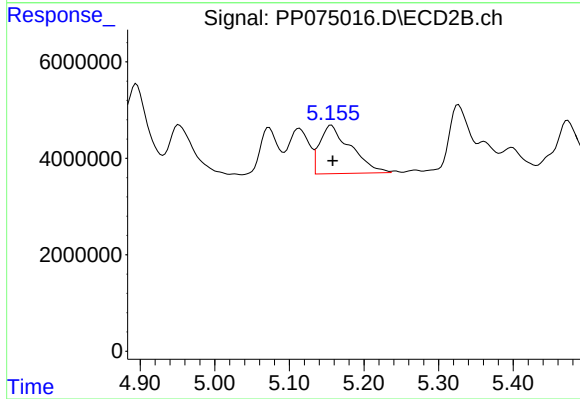


#19 AR-1242-4

R.T.: 5.156 min  
Delta R.T.: -0.002 min  
Response: 28818850  
Conc: 168.37 ng/ml

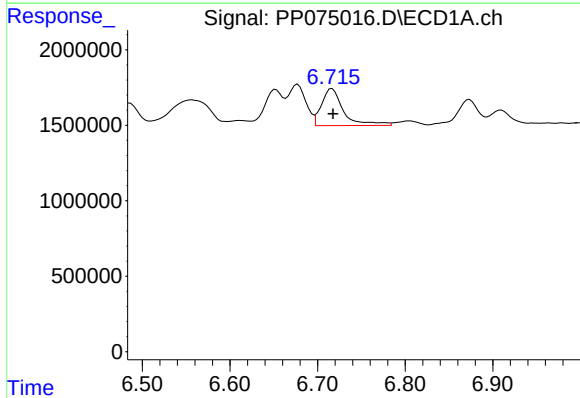


#20 AR-1242-5

R.T.: 6.717 min  
Delta R.T.: 0.000 min  
Response: 4277274  
Conc: 118.58 ng/ml

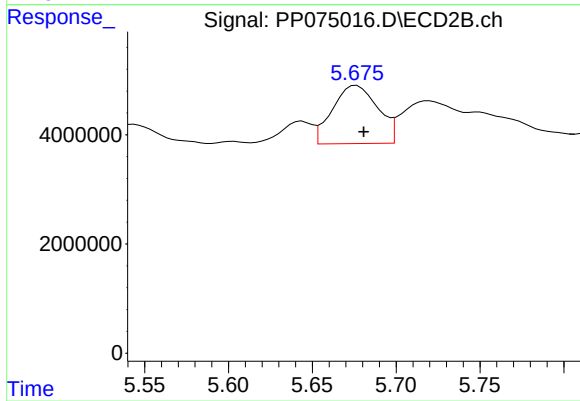

#20 AR-1242-5


R.T.: 5.676 min  
Delta R.T.: -0.004 min  
Response: 20060497  
Conc: 108.34 ng/ml

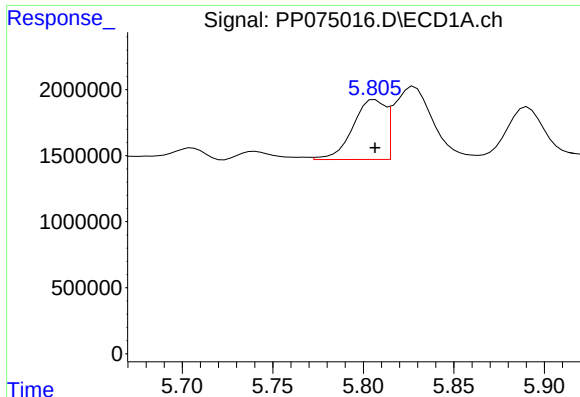

#21 AR-1248-1


R.T.: 5.806 min  
Delta R.T.: 0.000 min  
Response: 5643397  
Conc: 186.72 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

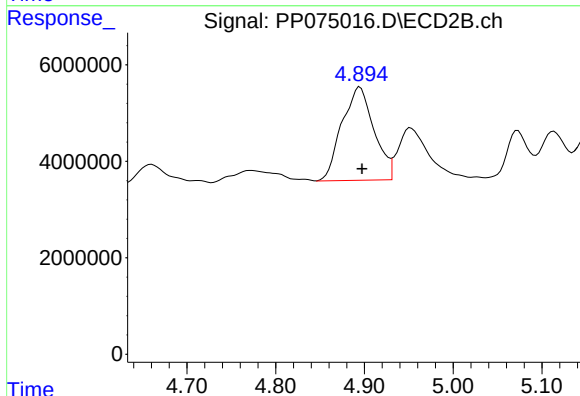


#21 AR-1248-1

R.T.: 4.895 min  
Delta R.T.: -0.003 min  
Response: 48668451  
Conc: 176.24 ng/ml

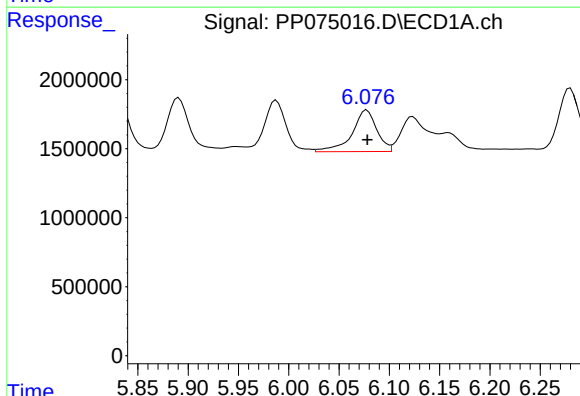


#22 AR-1248-2

R.T.: 6.078 min  
Delta R.T.: 0.000 min  
Response: 5150198  
Conc: 119.51 ng/ml

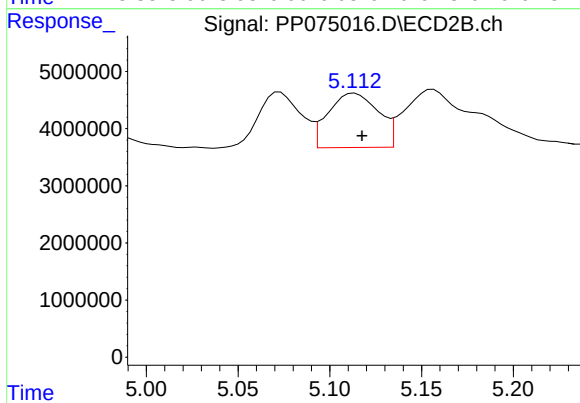

#22 AR-1248-2


R.T.: 5.113 min  
Delta R.T.: -0.004 min  
Response: 18070894  
Conc: 102.24 ng/ml

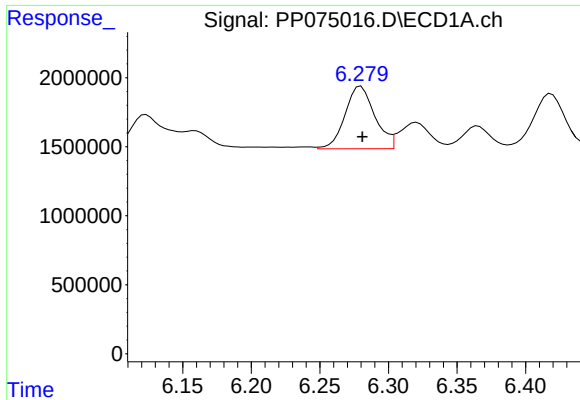

#23 AR-1248-3


R.T.: 6.280 min  
Delta R.T.: -0.001 min  
Response: 6866703  
Conc: 147.03 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

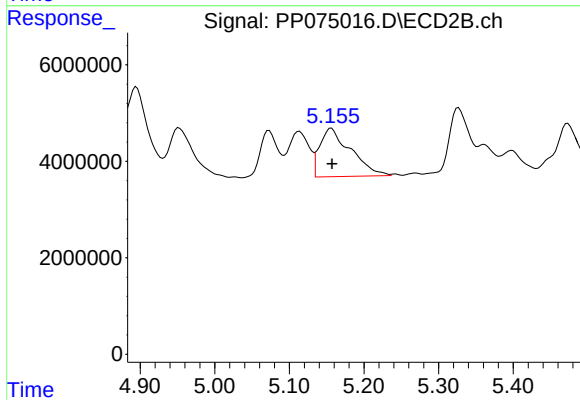


#23 AR-1248-3

R.T.: 5.156 min  
Delta R.T.: 0.000 min  
Response: 28818850  
Conc: 126.84 ng/ml

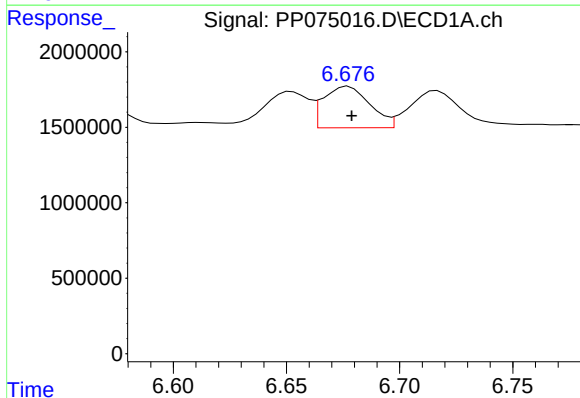


#24 AR-1248-4

R.T.: 6.677 min  
Delta R.T.: -0.002 min  
Response: 3912189  
Conc: 71.13 ng/ml

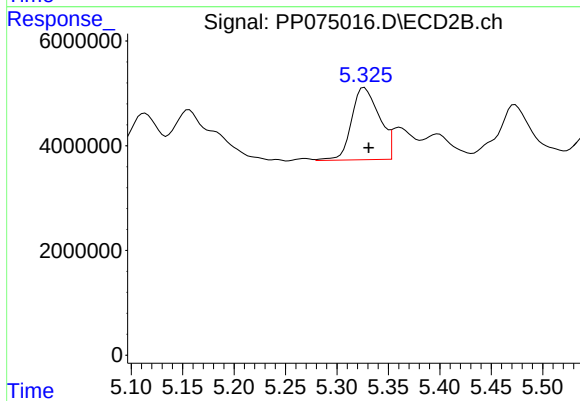

#24 AR-1248-4


R.T.: 5.327 min  
Delta R.T.: -0.004 min  
Response: 25863010  
Conc: 118.63 ng/ml

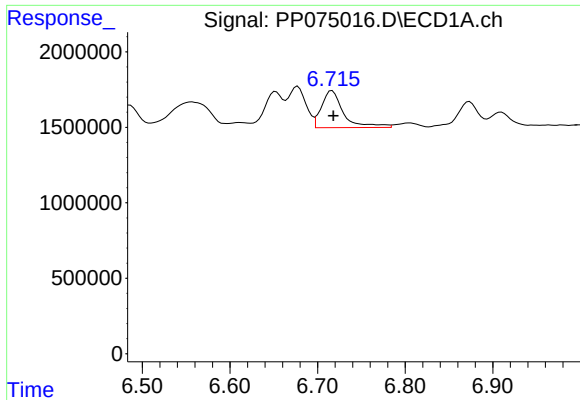

#25 AR-1248-5


R.T.: 6.717 min  
Delta R.T.: -0.001 min  
Response: 4277274  
Conc: 77.11 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

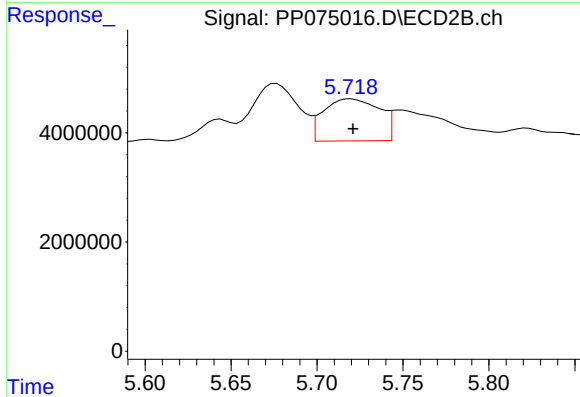


#25 AR-1248-5

R.T.: 5.720 min  
Delta R.T.: -0.001 min  
Response: 17412101  
Conc: 47.40 ng/ml

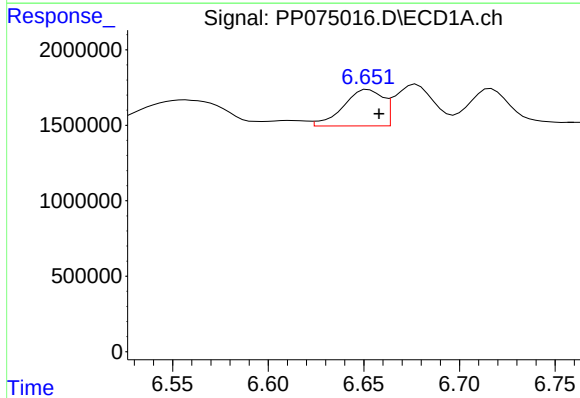

#26 AR-1254-1


R.T.: 6.652 min  
Delta R.T.: -0.006 min  
Response: 3465870  
Conc: 59.48 ng/ml

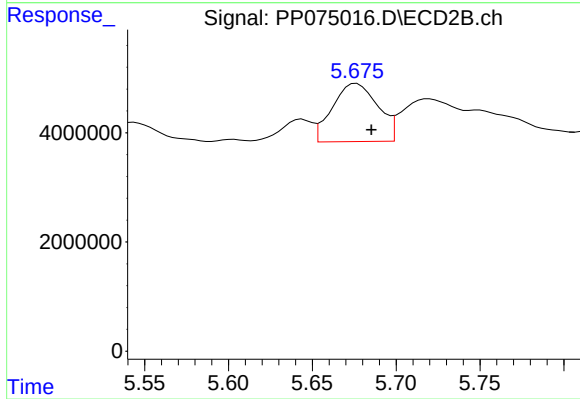

#26 AR-1254-1

R.T.: 5.676 min  
Delta R.T.: -0.009 min  
Response: 20060497  
Conc: 42.08 ng/ml




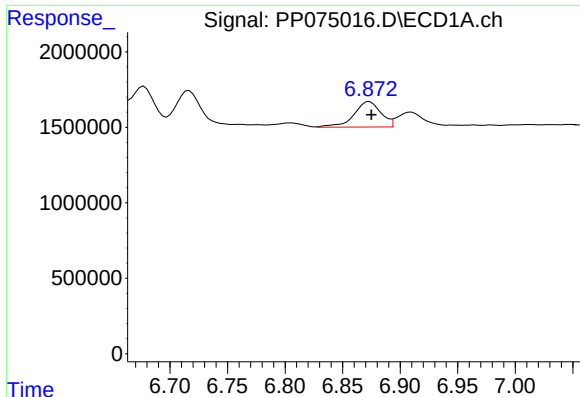

#27 AR-1254-2


R.T.: 6.873 min  
Delta R.T.: -0.001 min  
Response: 2741295  
Conc: 33.59 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

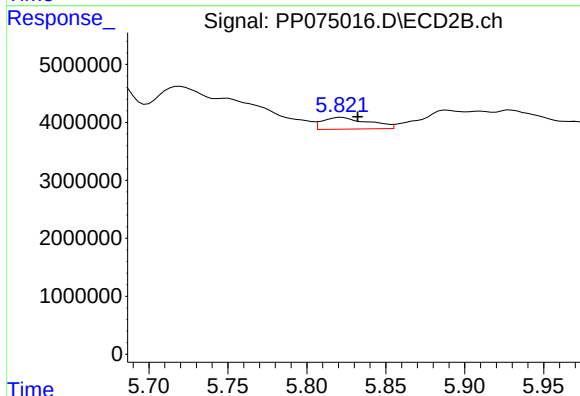


#27 AR-1254-2

R.T.: 5.822 min  
Delta R.T.: -0.010 min  
Response: 4102820  
Conc: 11.65 ng/ml

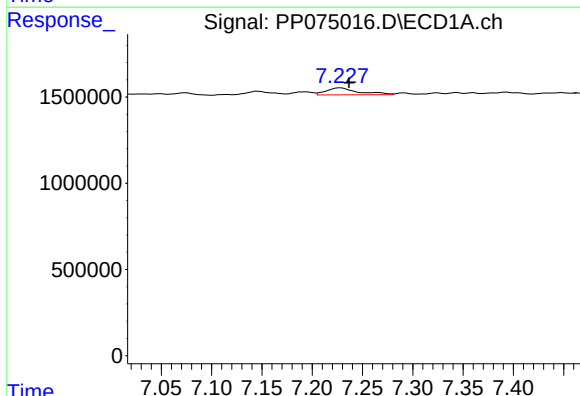


#28 AR-1254-3

R.T.: 7.228 min  
Delta R.T.: -0.009 min  
Response: 898249  
Conc: 10.07 ng/ml

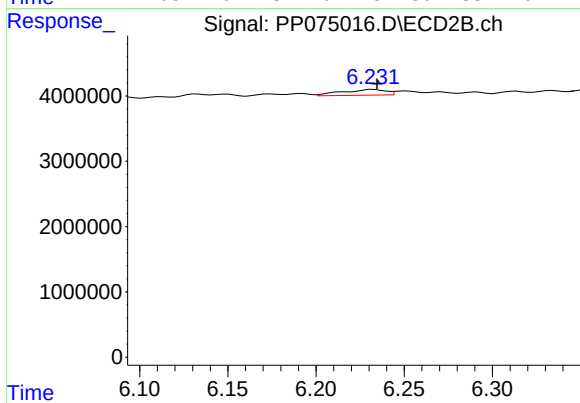

#28 AR-1254-3


R.T.: 6.232 min  
Delta R.T.: -0.002 min  
Response: 1520768  
Conc: 2.45 ng/ml

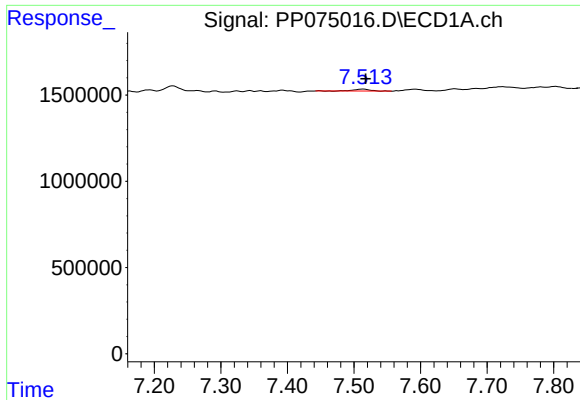

#29 AR-1254-4


R.T.: 7.514 min  
Delta R.T.: -0.004 min  
Response: 189869  
Conc: 2.88 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

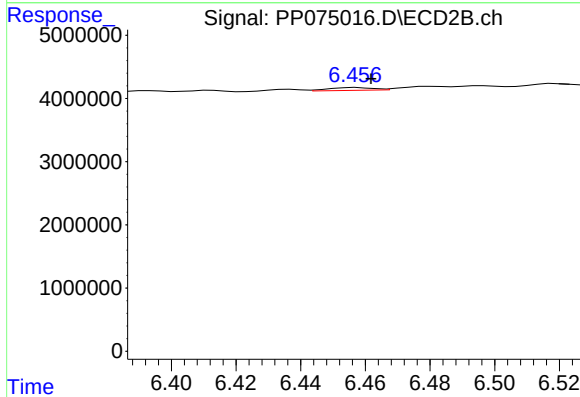


#29 AR-1254-4

R.T.: 6.457 min  
Delta R.T.: -0.005 min  
Response: 428551  
Conc: 0.91 ng/ml

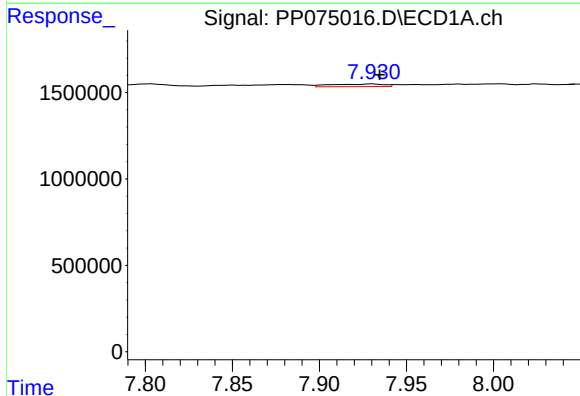


#30 AR-1254-5

R.T.: 7.931 min  
Delta R.T.: -0.004 min  
Response: 319869  
Conc: 3.85 ng/ml

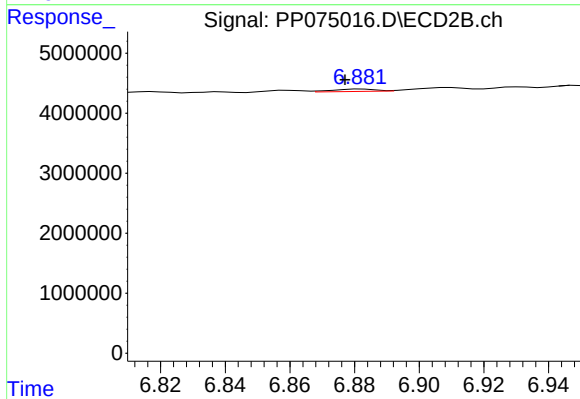

#30 AR-1254-5


R.T.: 6.882 min  
Delta R.T.: 0.005 min  
Response: 368334  
Conc: 0.75 ng/ml

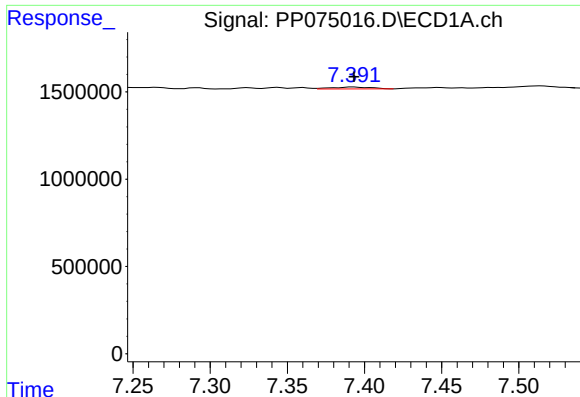

#31 AR-1260-1


R.T.: 7.393 min  
Delta R.T.: 0.000 min  
Response: 193762  
Conc: 3.35 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

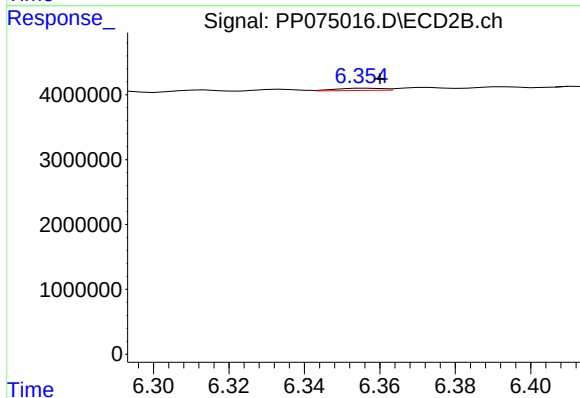


#31 AR-1260-1

R.T.: 6.356 min  
Delta R.T.: -0.004 min  
Response: 287534  
Conc: 0.77 ng/ml

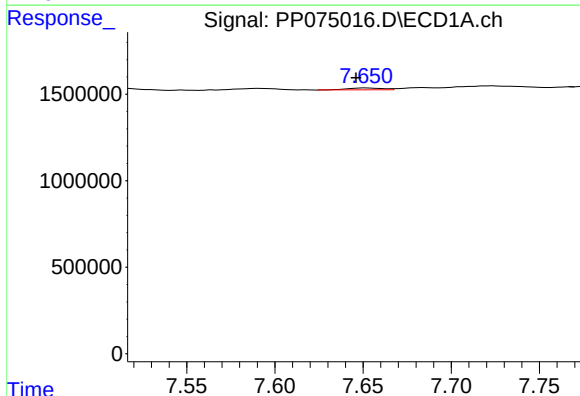


#32 AR-1260-2

R.T.: 7.652 min  
Delta R.T.: 0.006 min  
Response: 152204  
Conc: 2.21 ng/ml

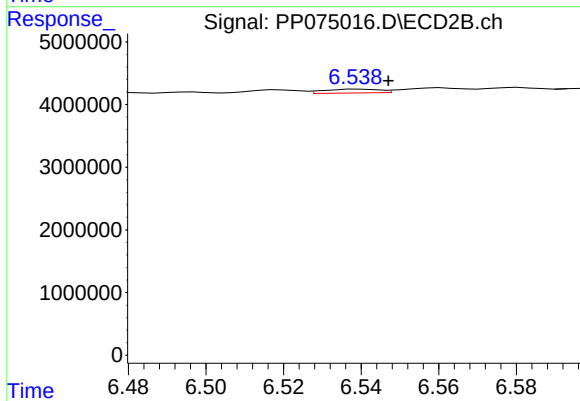

#32 AR-1260-2


R.T.: 6.539 min  
Delta R.T.: -0.008 min  
Response: 605120  
Conc: 1.14 ng/ml

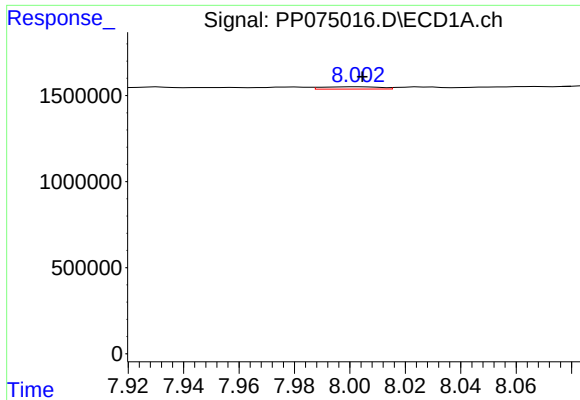

#33 AR-1260-3


R.T.: 8.002 min  
Delta R.T.: -0.002 min  
Response: 198870  
Conc: 3.83 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

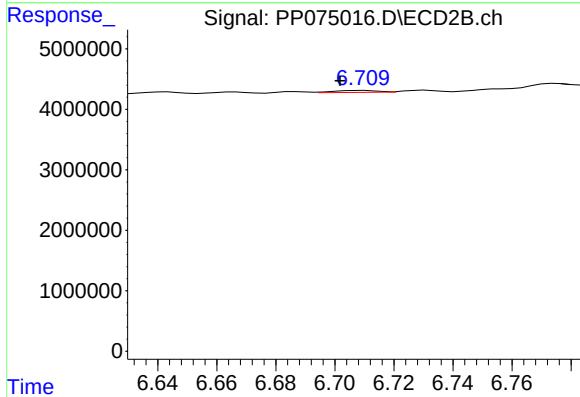


#33 AR-1260-3

R.T.: 6.710 min  
Delta R.T.: 0.008 min  
Response: 345456  
Conc: 0.80 ng/ml

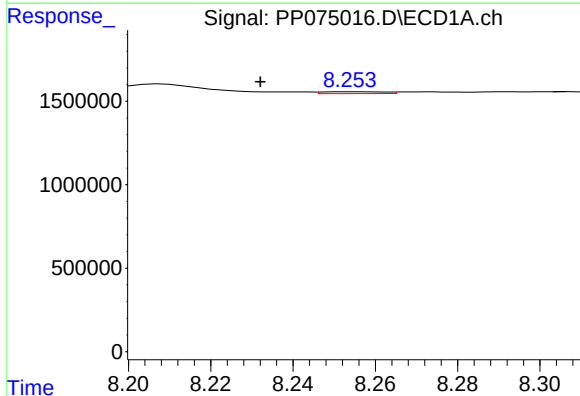


#34 AR-1260-4

R.T.: 8.256 min  
Delta R.T.: 0.024 min  
Response: 116458  
Conc: 1.83 ng/ml

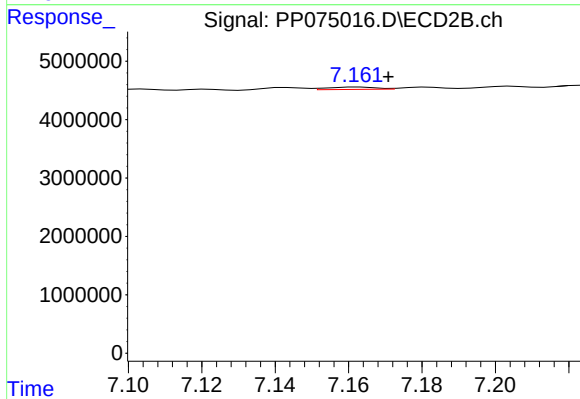

#34 AR-1260-4


R.T.: 7.163 min  
Delta R.T.: -0.008 min  
Response: 361691  
Conc: 0.95 ng/ml

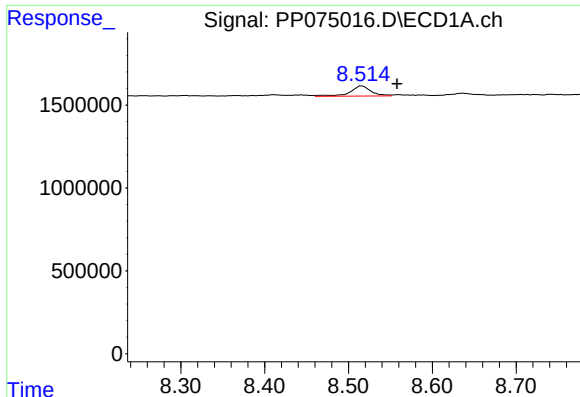

#35 AR-1260-5


R.T.: 8.516 min  
Delta R.T.: -0.041 min  
Response: 1064641  
Conc: 9.39 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

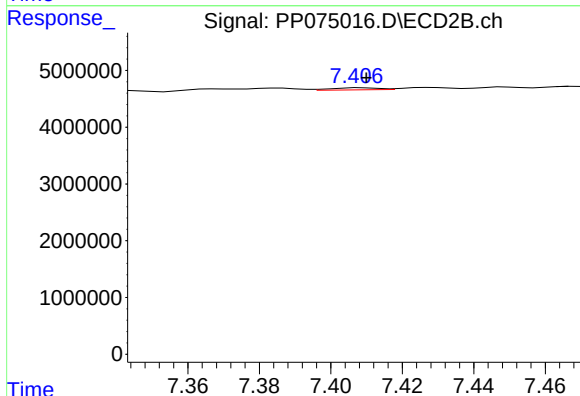


#35 AR-1260-5

R.T.: 7.409 min  
Delta R.T.: -0.001 min  
Response: 335756  
Conc: 0.33 ng/ml

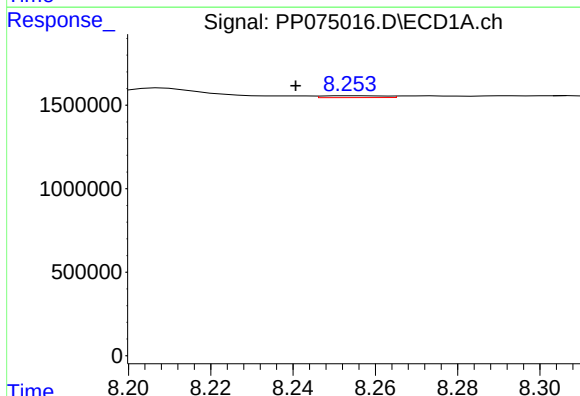


#36 AR-1262-1

R.T.: 8.256 min  
Delta R.T.: 0.015 min  
Response: 116458  
Conc: 1.51 ng/ml

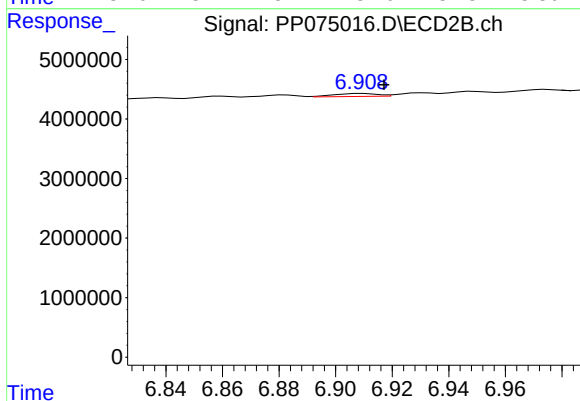

#36 AR-1262-1


R.T.: 6.910 min  
Delta R.T.: -0.008 min  
Response: 528477  
Conc: 0.75 ng/ml

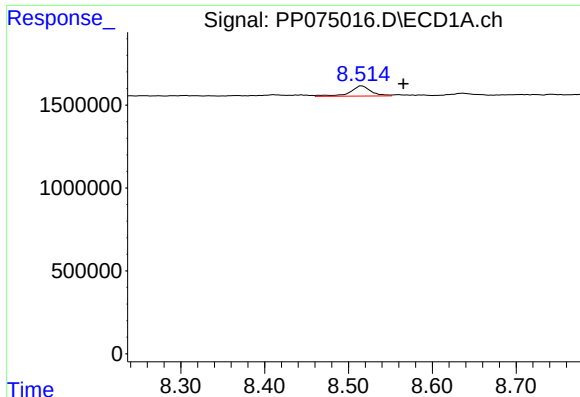

#37 AR-1262-2


R.T.: 8.516 min  
Delta R.T.: -0.049 min  
Response: 1064641  
Conc: 8.04 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

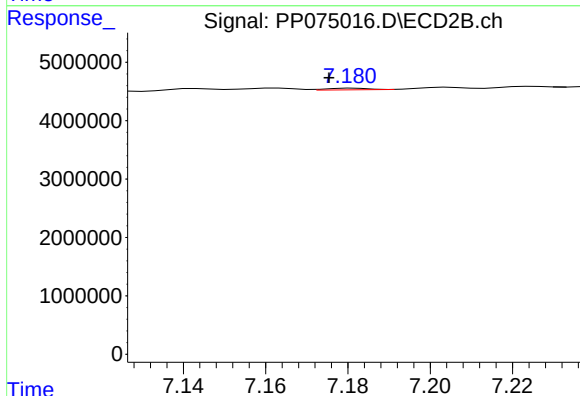


#37 AR-1262-2

R.T.: 7.182 min  
Delta R.T.: 0.006 min  
Response: 187227  
Conc: 0.36 ng/ml

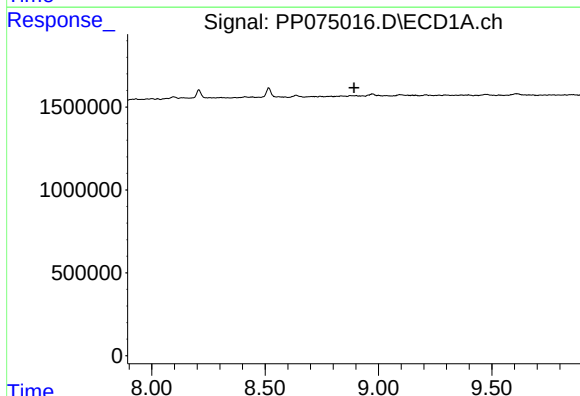


#38 AR-1262-3

R.T.: 0.000 min  
Exp R.T. : 8.892 min  
Response: 0  
Conc: N.D.

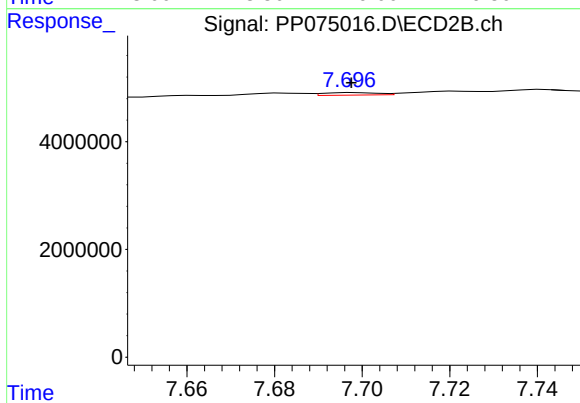

#38 AR-1262-3


R.T.: 7.698 min  
Delta R.T.: 0.000 min  
Response: 413228  
Conc: 0.89 ng/ml

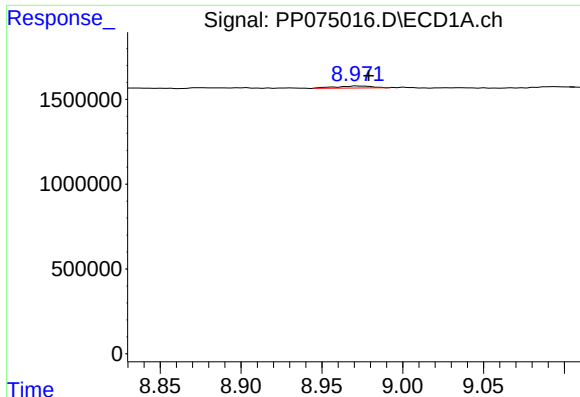

#39 AR-1262-4


R.T.: 8.973 min  
Delta R.T.: -0.005 min  
Response: 187151  
Conc: 2.48 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

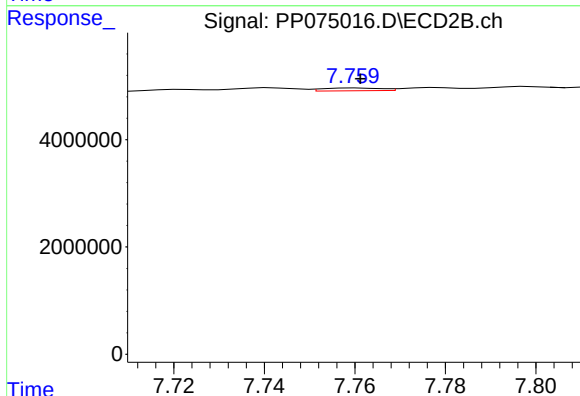


#39 AR-1262-4

R.T.: 7.760 min  
Delta R.T.: 0.000 min  
Response: 463706  
Conc: 0.56 ng/ml

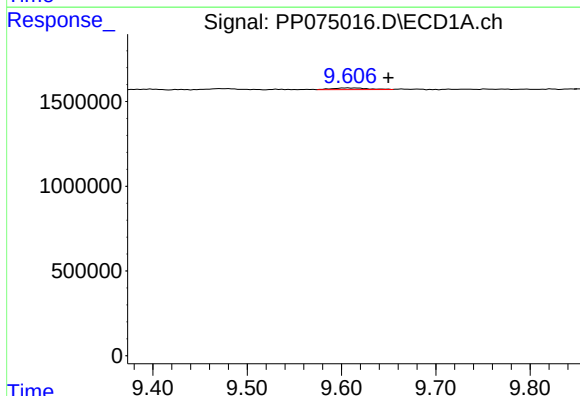


#40 AR-1262-5

R.T.: 9.607 min  
Delta R.T.: -0.043 min  
Response: 247292  
Conc: 4.06 ng/ml

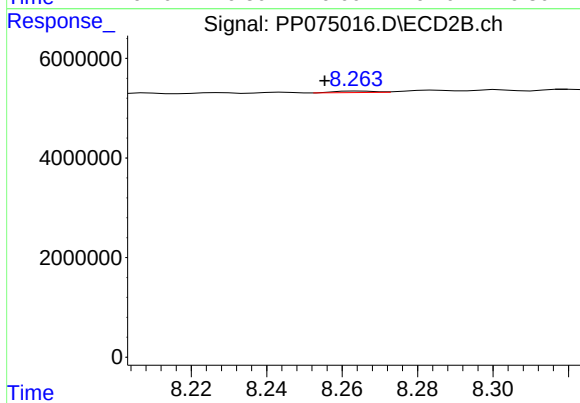

#40 AR-1262-5


R.T.: 8.264 min  
Delta R.T.: 0.009 min  
Response: 216360  
Conc: 0.60 ng/ml

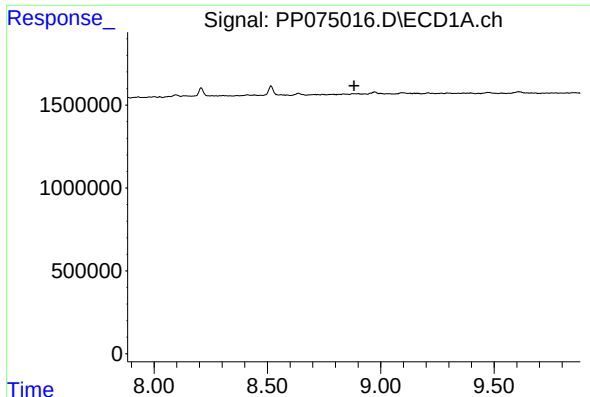

#41 AR-1268-1


R.T.: 0.000 min  
Exp R.T.: 8.883 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

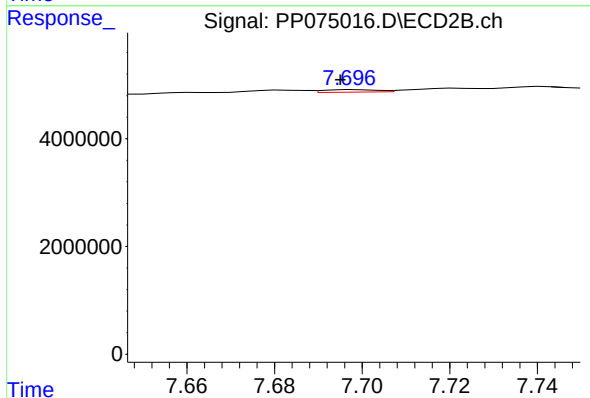


#41 AR-1268-1

R.T.: 7.698 min  
Delta R.T.: 0.003 min  
Response: 413228  
Conc: 0.29 ng/ml

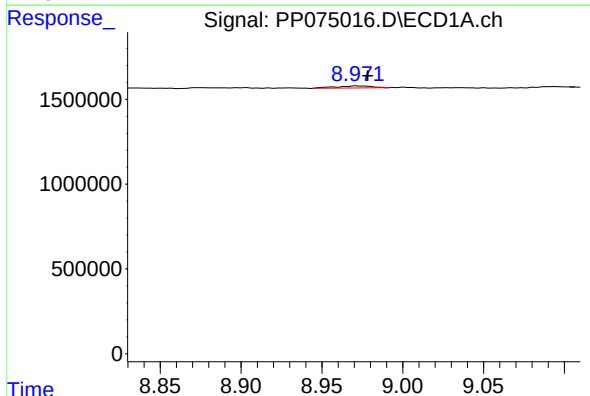

#42 AR-1268-2


R.T.: 8.973 min  
Delta R.T.: -0.005 min  
Response: 187151  
Conc: 1.28 ng/ml

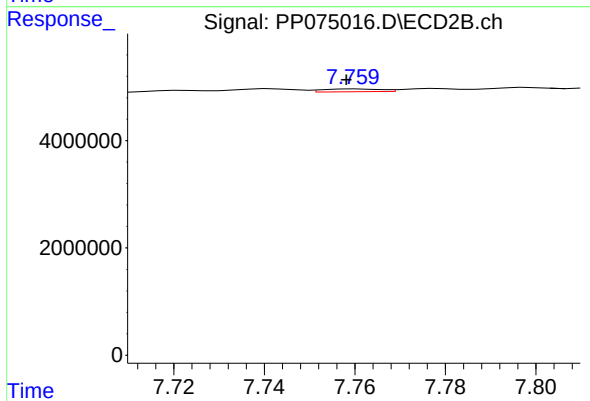

#42 AR-1268-2

R.T.: 7.760 min  
Delta R.T.: 0.002 min  
Response: 463706  
Conc: 0.34 ng/ml




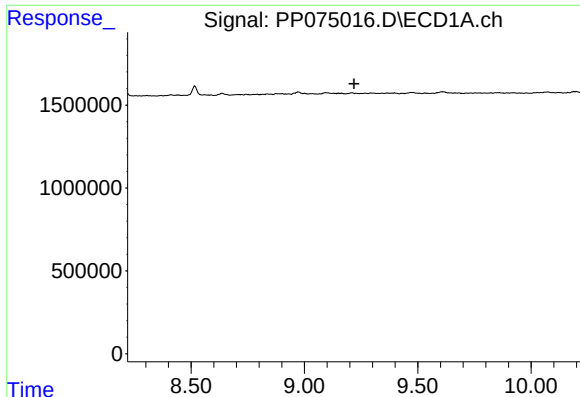

#43 AR-1268-3


R.T.: 0.000 min  
Exp R.T.: 9.219 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

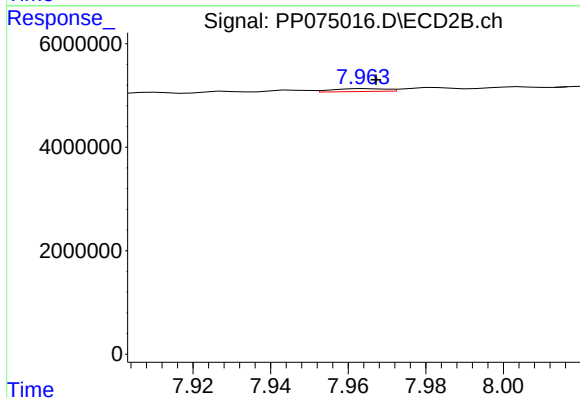


#43 AR-1268-3

R.T.: 7.964 min  
Delta R.T.: -0.003 min  
Response: 519125  
Conc: 0.50 ng/ml

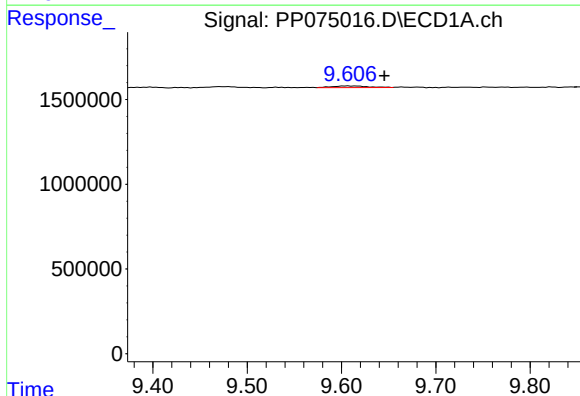


#44 AR-1268-4

R.T.: 9.607 min  
Delta R.T.: -0.038 min  
Response: 247292  
Conc: 3.68 ng/ml

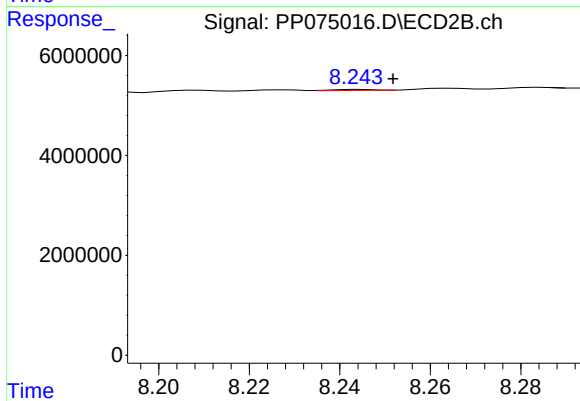

#44 AR-1268-4


R.T.: 8.244 min  
Delta R.T.: -0.007 min  
Response: 130537  
Conc: 0.34 ng/ml

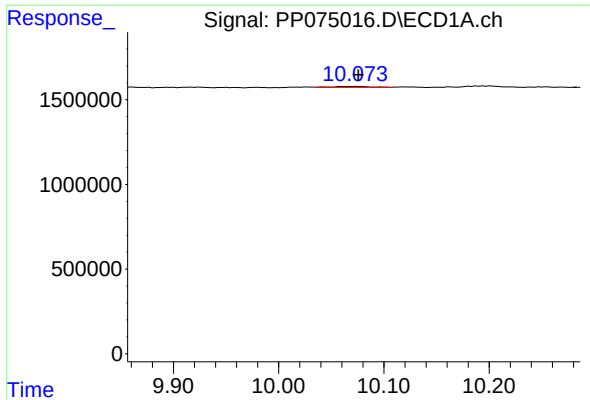

#45 AR-1268-5

R.T.: 10.074 min  
Delta R.T.: -0.002 min  
Response: 141514  
Conc: 0.38 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
PASSAIC-J

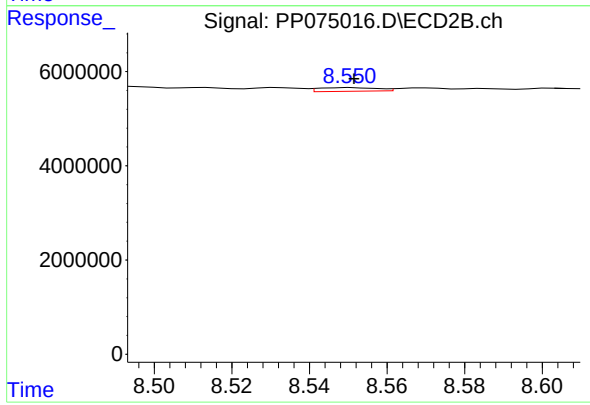

#45 AR-1268-5

R.T.: 8.551 min  
Delta R.T.: 0.000 min  
Response: 830763  
Conc: 0.26 ng/ml