

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
 Data File : PP075017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Sep 2025 18:44
 Operator : YP\AJ
 Sample : Q3034-11
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-K

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 10 01:52:15 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.656	3.798	29022696	110.7E6	23.717	22.903
2)	SA Decachlor...	10.428	8.804	23457727	147.7E6	23.754	19.695
Target Compounds							
3)	L1 AR-1016-1	5.807	4.896	4538895	42710422	102.949	83.852
4)	L1 AR-1016-2	5.828	4.954	7036102	21670190	111.966	91.045
5)	L1 AR-1016-3	5.891	5.074	4355974	14398504	96.985	104.410
6)	L1 AR-1016-4	5.988	5.115	4563318	15600365	129.707	111.588
7)	L1 AR-1016-5	6.280	5.328	5720197	30108660	172.367	181.286
8)	L2 AR-1221-1	4.854	4.003	207315	170602	11.784	2.758 #
9)	L2 AR-1221-2	4.958	4.102	620592	1679909	46.461	37.156
10)	L2 AR-1221-3	5.018	4.171	359556	1561501	9.484	9.504
11)	L3 AR-1232-1	5.018	4.171	359556	1561501	11.838	12.190
12)	L3 AR-1232-2	5.543	4.896	2013471	42710422	127.773	184.261 #
13)	L3 AR-1232-3	5.828	5.074	7036102	14398504	230.362	239.736
14)	L3 AR-1232-4	5.988	5.157	4563318	26430125	264.245	358.582 #
15)	L3 AR-1232-5	6.077	5.328	4076786	30108660	314.059	484.968 #
16)	L4 AR-1242-1	5.807	4.896	4538895	42710422	118.586	101.269
17)	L4 AR-1242-2	5.828	4.954	7036102	21670190	124.573	108.198
18)	L4 AR-1242-3	5.891	5.074	4355974	14398504	107.282	121.714
19)	L4 AR-1242-4	5.988	5.157	4563318	26430125	143.763	154.418
20)	L4 AR-1242-5	6.717	5.677	3546149	17459361	98.311	94.291
21)	L5 AR-1248-1	5.807	4.896	4538895	42710422	150.175	154.668
22)	L5 AR-1248-2	6.077	5.115	4076786	15600365	94.598	88.260
23)	L5 AR-1248-3	6.280	5.157	5720197	26430125	122.479	116.328
24)	L5 AR-1248-4	6.677	5.328	3227654	30108660	58.684	138.100 #
25)	L5 AR-1248-5	6.717	5.720	3546149	16928309	63.929	46.086 #
26)	L6 AR-1254-1	6.653	5.677	3050910	17459361	52.359	36.625 #
27)	L6 AR-1254-2	6.873	5.827	2225020	2467660	27.262	7.008 #
28)	L6 AR-1254-3	7.227	6.243	1046932	692304	11.736	1.117 #
29)	L6 AR-1254-4	7.516	6.468	171114	218423	2.596	0.466 #
30)	L6 AR-1254-5	7.940	6.869	482701	335721	5.810	0.684 #
31)	L7 AR-1260-1	7.394	6.368	93607	436503	1.619	1.163 #
32)	L7 AR-1260-2	7.659	6.547	217786	719897	3.160	1.361 #
33)	L7 AR-1260-3	7.998	6.700	215700	314582	4.157	0.727 #
34)	L7 AR-1260-4	8.252	7.173	409222	339682	6.415	0.890 #
35)	L7 AR-1260-5	8.518f	7.414	933320	340268	8.229	0.339 #
36)	L8 AR-1262-1	8.252	6.911	409222	228272	5.313	0.323 #
37)	L8 AR-1262-2	8.518f	7.173	933320	339682	7.050	0.652 #
38)	L8 AR-1262-3	0.000	7.691	0	393840	N.D.	0.845 #
39)	L8 AR-1262-4	8.974	7.765	171110	357844	2.271	0.435 #
40)	L8 AR-1262-5	0.000	8.251	0	111947	N.D.	0.312 #
41)	L9 AR-1268-1	0.000	7.691	0	393840	N.D.	0.279 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP090925\
Data File : PP075017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Sep 2025 18:44
Operator : YP\AJ
Sample : Q3034-11
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 10 01:52:15 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	8.974	7.765	171110	357844	1.166	0.262 #
43)	L9 AR-1268-3	0.000	7.959	0	707584	N.D.	0.678 #
44)	L9 AR-1268-4	0.000	8.251	0	111947	N.D.	0.292 #
45)	L9 AR-1268-5	10.079	8.547	98428	987427	0.266	0.315


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

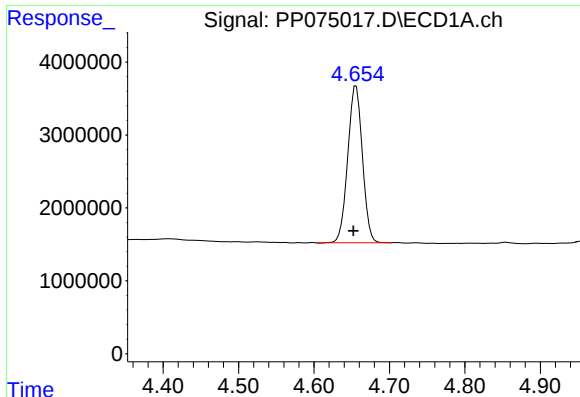

#1 Tetrachloro-m-xylene


R.T.: 4.656 min
Delta R.T.: 0.004 min
Response: 29022696
Conc: 23.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

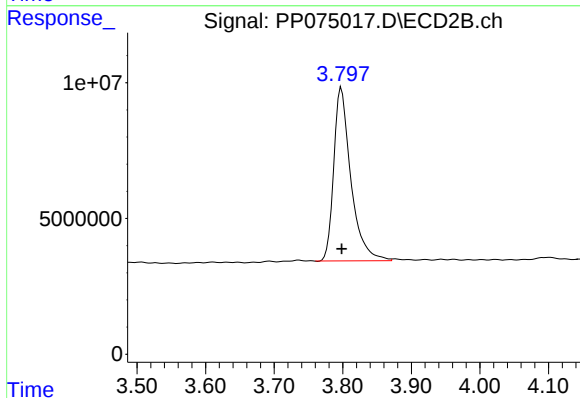


#1 Tetrachloro-m-xylene

R.T.: 3.798 min
Delta R.T.: 0.000 min
Response: 110743874
Conc: 22.90 ng/ml

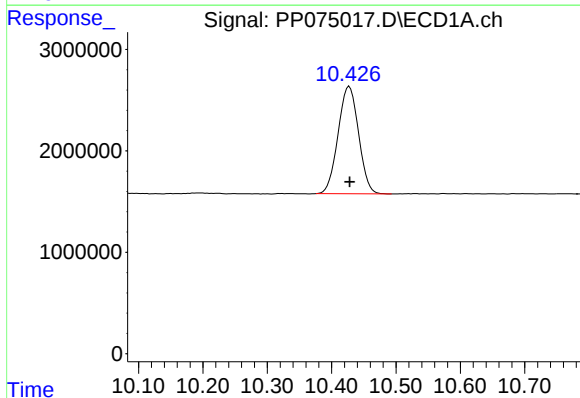


#2 Decachlorobiphenyl

R.T.: 10.428 min
Delta R.T.: 0.000 min
Response: 23457727
Conc: 23.75 ng/ml

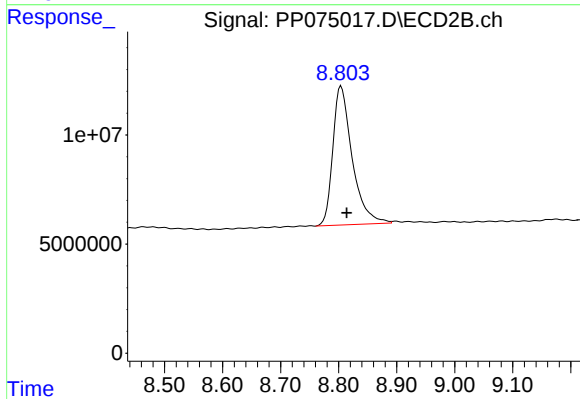

#2 Decachlorobiphenyl


R.T.: 8.804 min
Delta R.T.: -0.010 min
Response: 147694841
Conc: 19.69 ng/ml

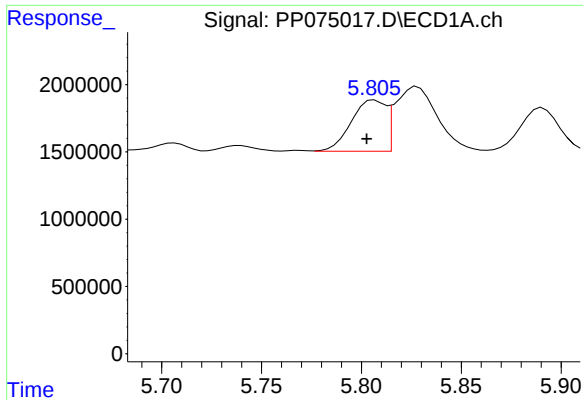

#3 AR-1016-1


R.T.: 5.807 min
Delta R.T.: 0.004 min
Response: 4538895
Conc: 102.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

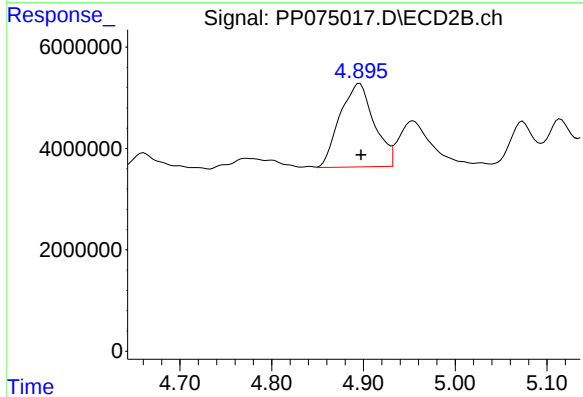


#3 AR-1016-1

R.T.: 4.896 min
Delta R.T.: -0.001 min
Response: 42710422
Conc: 83.85 ng/ml

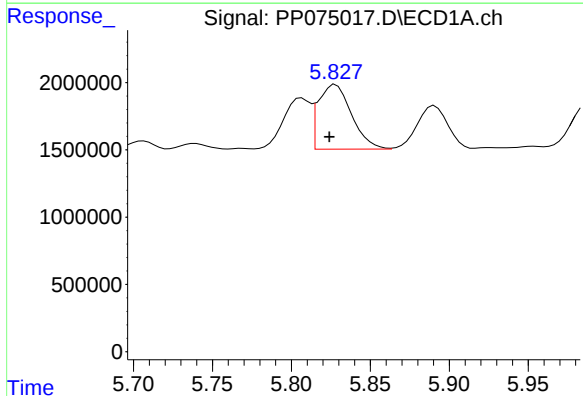


#4 AR-1016-2

R.T.: 5.828 min
Delta R.T.: 0.004 min
Response: 7036102
Conc: 111.97 ng/ml

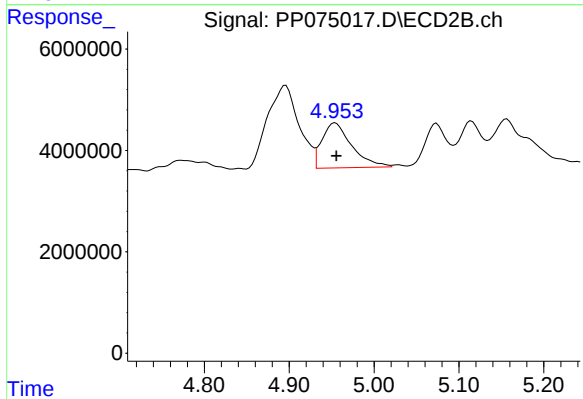

#4 AR-1016-2


R.T.: 4.954 min
Delta R.T.: -0.001 min
Response: 21670190
Conc: 91.05 ng/ml

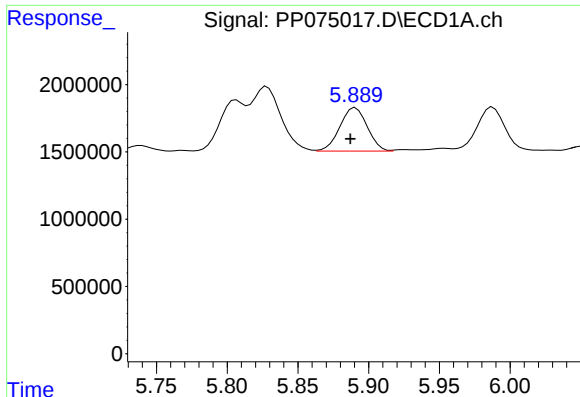

#5 AR-1016-3


R.T.: 5.891 min
Delta R.T.: 0.004 min
Response: 4355974
Conc: 96.98 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

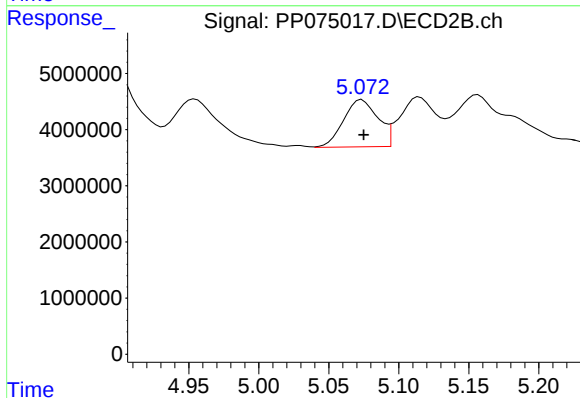


#5 AR-1016-3

R.T.: 5.074 min
Delta R.T.: -0.001 min
Response: 14398504
Conc: 104.41 ng/ml

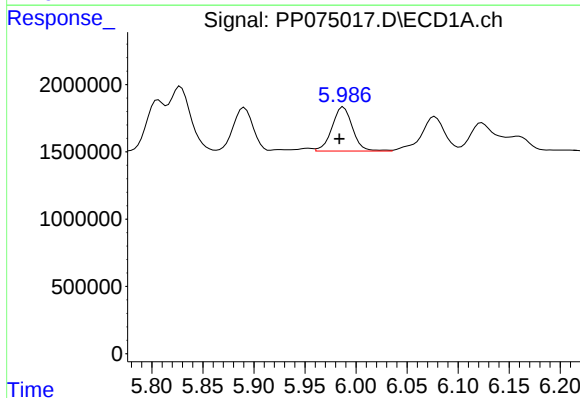


#6 AR-1016-4

R.T.: 5.988 min
Delta R.T.: 0.004 min
Response: 4563318
Conc: 129.71 ng/ml

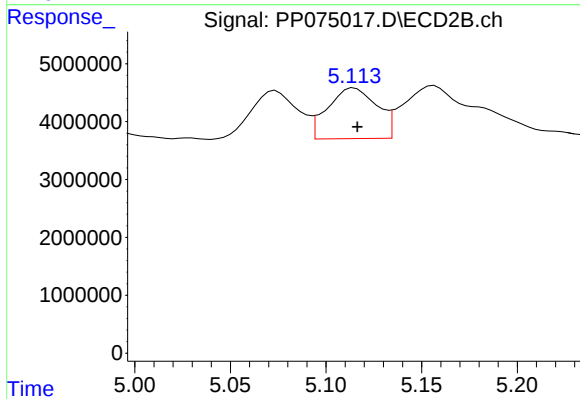

#6 AR-1016-4


R.T.: 5.115 min
Delta R.T.: -0.002 min
Response: 15600365
Conc: 111.59 ng/ml

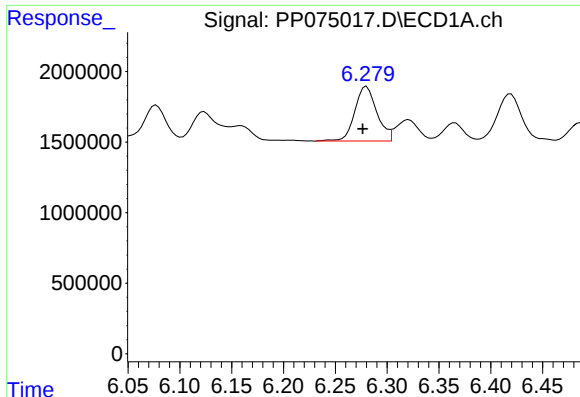

#7 AR-1016-5


R.T.: 6.280 min
Delta R.T.: 0.004 min
Response: 5720197
Conc: 172.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

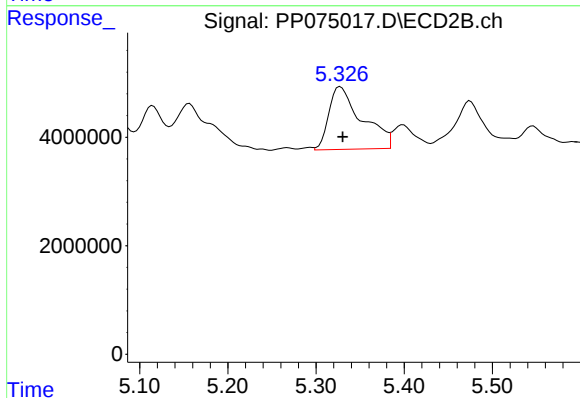


#7 AR-1016-5

R.T.: 5.328 min
Delta R.T.: -0.003 min
Response: 30108660
Conc: 181.29 ng/ml

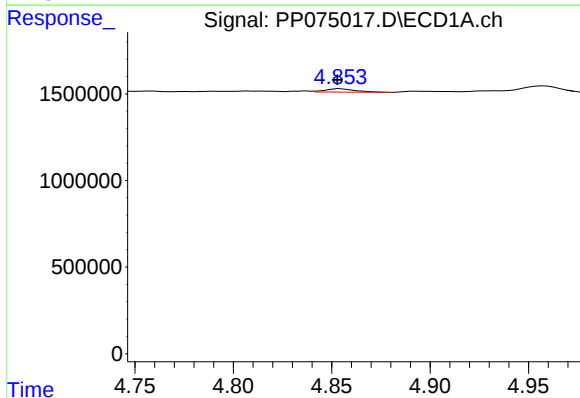


#8 AR-1221-1

R.T.: 4.854 min
Delta R.T.: 0.001 min
Response: 207315
Conc: 11.78 ng/ml

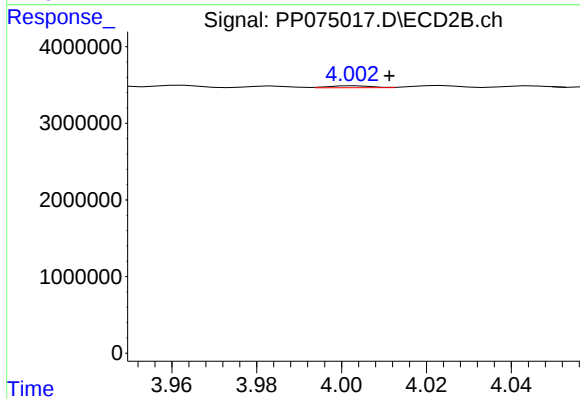

#8 AR-1221-1


R.T.: 4.003 min
Delta R.T.: -0.008 min
Response: 170602
Conc: 2.76 ng/ml

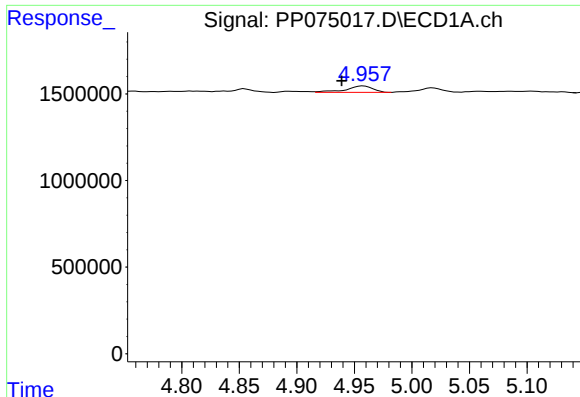

#9 AR-1221-2


R.T.: 4.958 min
Delta R.T.: 0.019 min
Response: 620592
Conc: 46.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

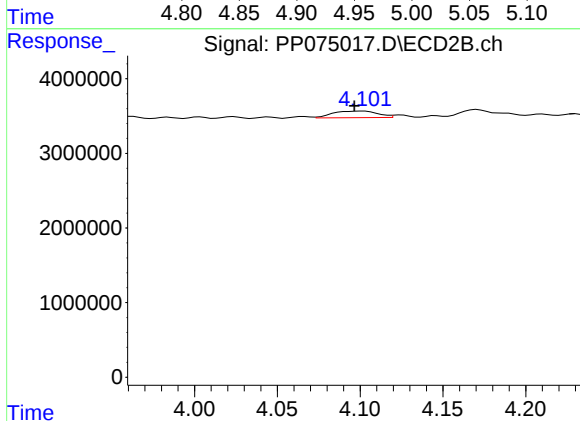


#9 AR-1221-2

R.T.: 4.102 min
Delta R.T.: 0.005 min
Response: 1679909
Conc: 37.16 ng/ml

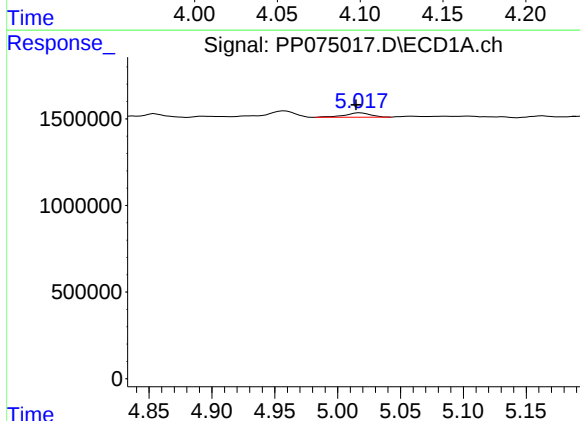


#10 AR-1221-3

R.T.: 5.018 min
Delta R.T.: 0.003 min
Response: 359556
Conc: 9.48 ng/ml

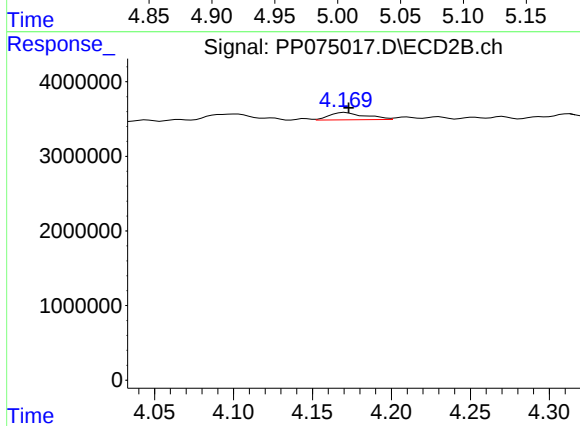

#10 AR-1221-3


R.T.: 4.171 min
Delta R.T.: -0.002 min
Response: 1561501
Conc: 9.50 ng/ml

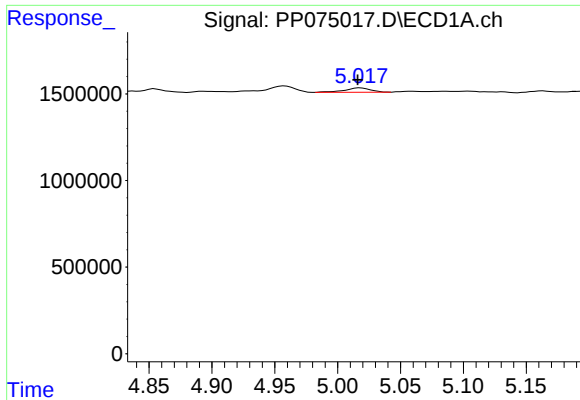

#11 AR-1232-1


R.T.: 5.018 min
Delta R.T.: 0.002 min
Response: 359556
Conc: 11.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

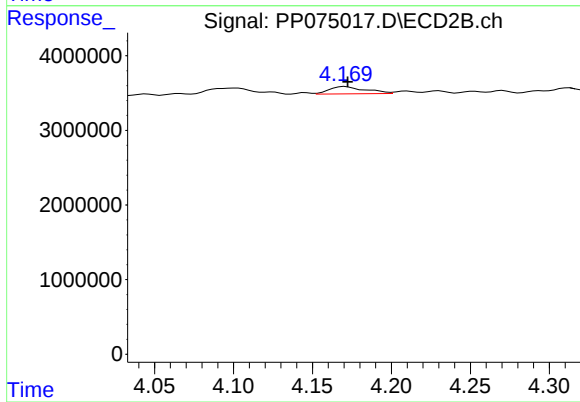


#11 AR-1232-1

R.T.: 4.171 min
Delta R.T.: -0.001 min
Response: 1561501
Conc: 12.19 ng/ml

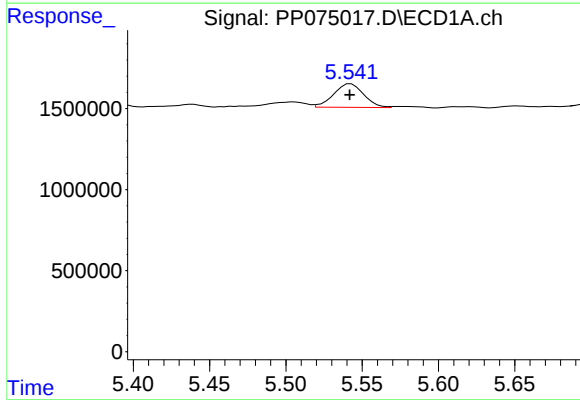


#12 AR-1232-2

R.T.: 5.543 min
Delta R.T.: 0.000 min
Response: 2013471
Conc: 127.77 ng/ml

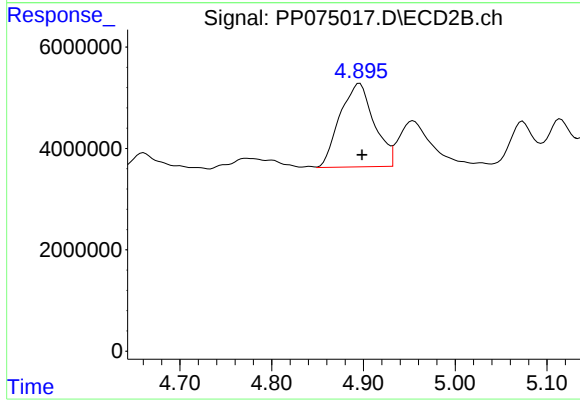

#12 AR-1232-2


R.T.: 4.896 min
Delta R.T.: -0.003 min
Response: 42710422
Conc: 184.26 ng/ml

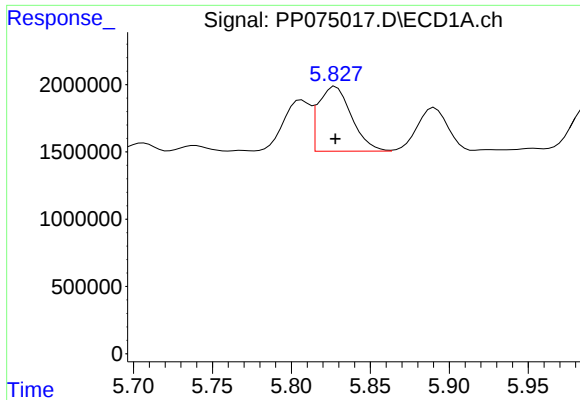

#13 AR-1232-3


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 7036102
Conc: 230.36 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

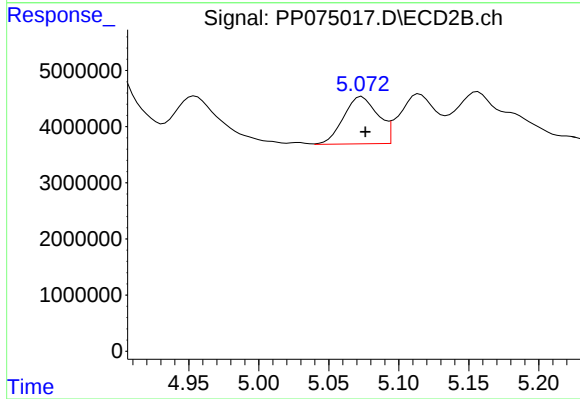


#13 AR-1232-3

R.T.: 5.074 min
Delta R.T.: -0.002 min
Response: 14398504
Conc: 239.74 ng/ml

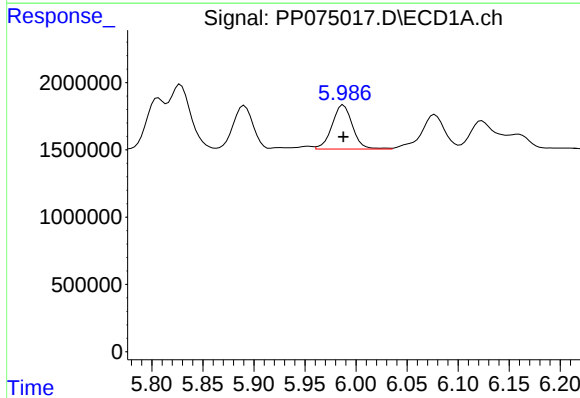


#14 AR-1232-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 4563318
Conc: 264.24 ng/ml

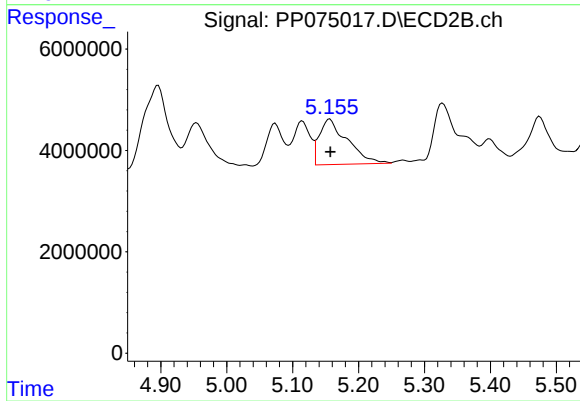

#14 AR-1232-4


R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 26430125
Conc: 358.58 ng/ml

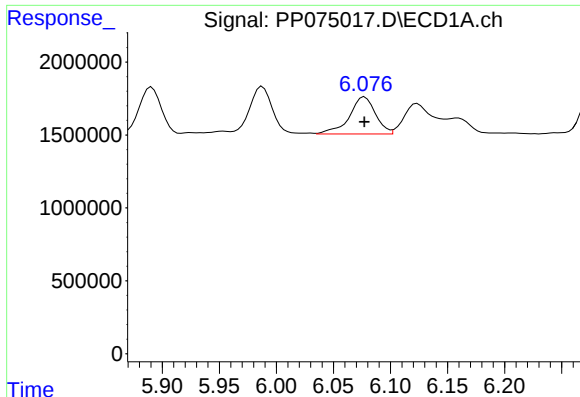

#15 AR-1232-5


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 4076786
Conc: 314.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

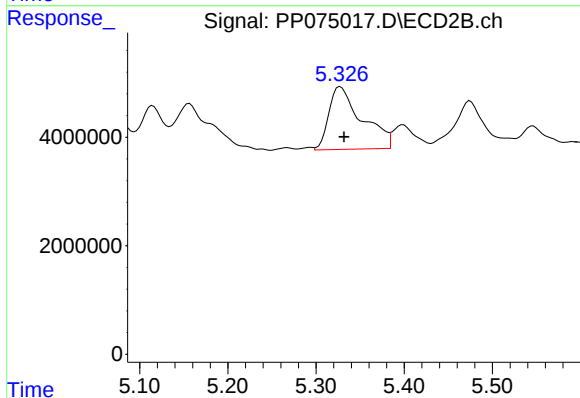


#15 AR-1232-5

R.T.: 5.328 min
Delta R.T.: -0.004 min
Response: 30108660
Conc: 484.97 ng/ml

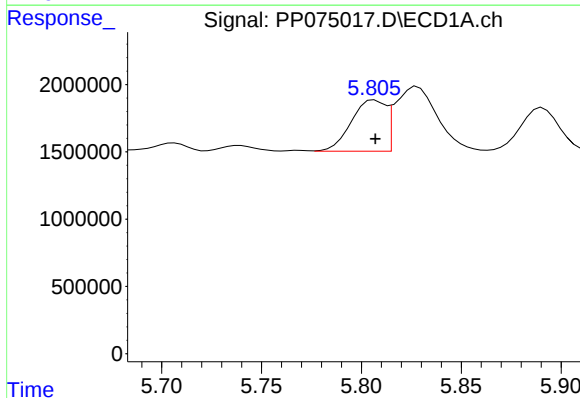


#16 AR-1242-1

R.T.: 5.807 min
Delta R.T.: 0.000 min
Response: 4538895
Conc: 118.59 ng/ml

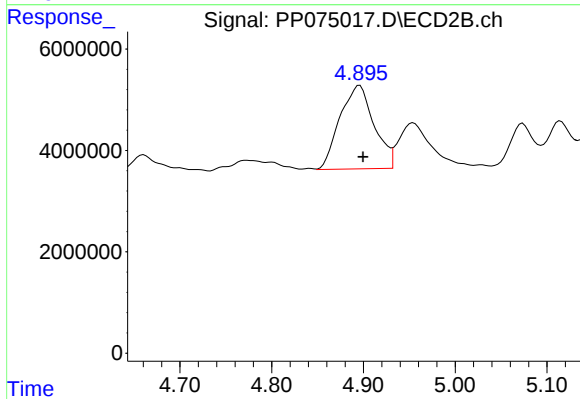

#16 AR-1242-1


R.T.: 4.896 min
Delta R.T.: -0.004 min
Response: 42710422
Conc: 101.27 ng/ml

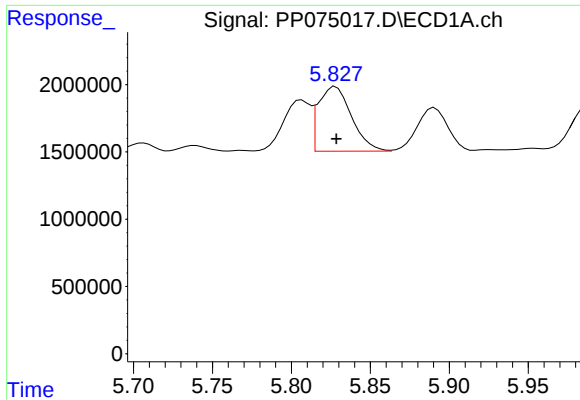

#17 AR-1242-2


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 7036102
Conc: 124.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

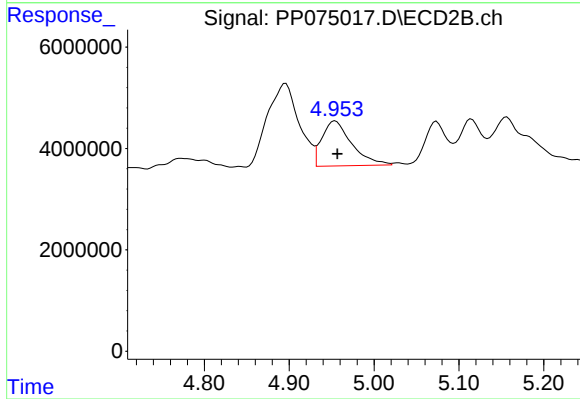


#17 AR-1242-2

R.T.: 4.954 min
Delta R.T.: -0.002 min
Response: 21670190
Conc: 108.20 ng/ml

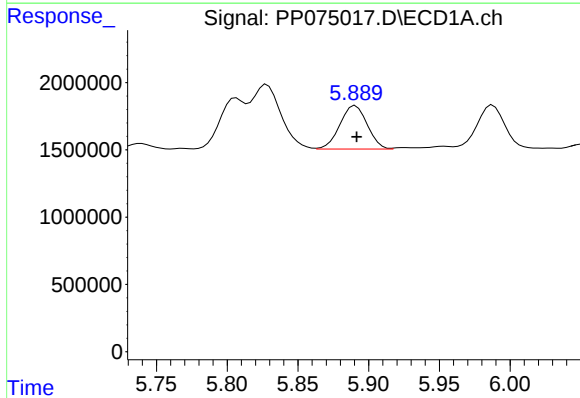


#18 AR-1242-3

R.T.: 5.891 min
Delta R.T.: 0.000 min
Response: 4355974
Conc: 107.28 ng/ml

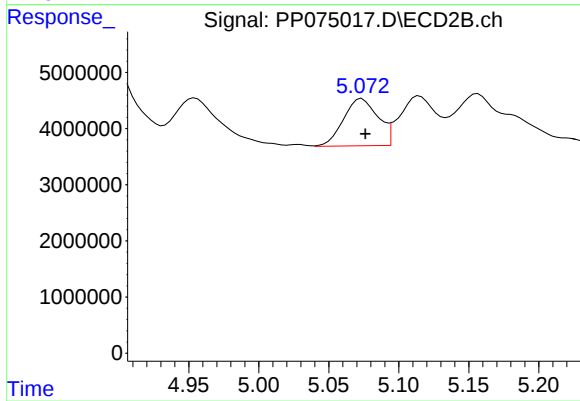

#18 AR-1242-3


R.T.: 5.074 min
Delta R.T.: -0.003 min
Response: 14398504
Conc: 121.71 ng/ml

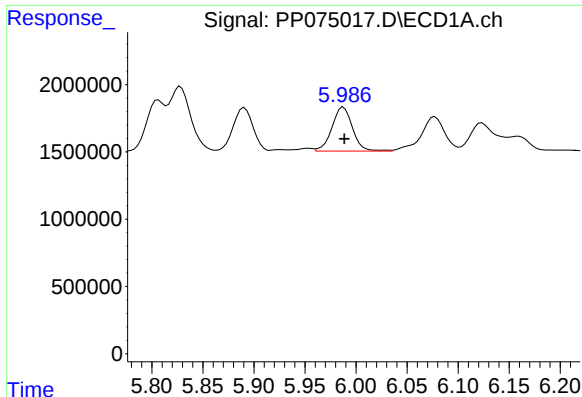

#19 AR-1242-4


R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 4563318
Conc: 143.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

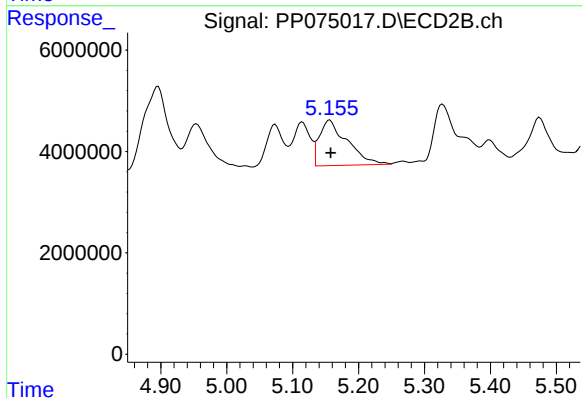


#19 AR-1242-4

R.T.: 5.157 min
Delta R.T.: -0.001 min
Response: 26430125
Conc: 154.42 ng/ml

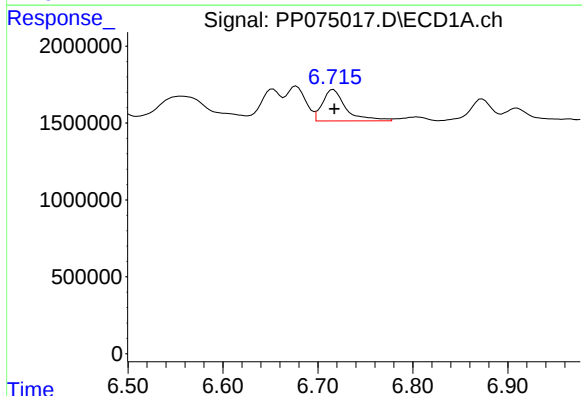


#20 AR-1242-5

R.T.: 6.717 min
Delta R.T.: -0.001 min
Response: 3546149
Conc: 98.31 ng/ml

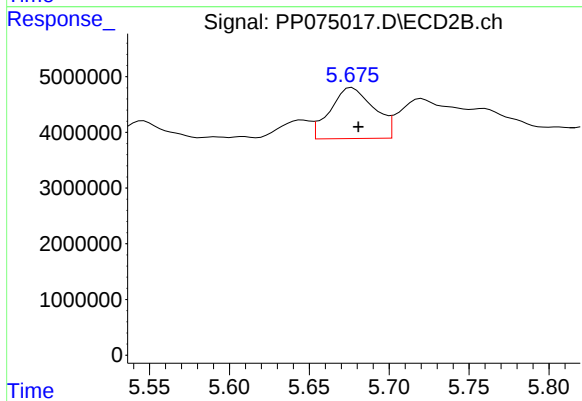

#20 AR-1242-5


R.T.: 5.677 min
Delta R.T.: -0.004 min
Response: 17459361
Conc: 94.29 ng/ml

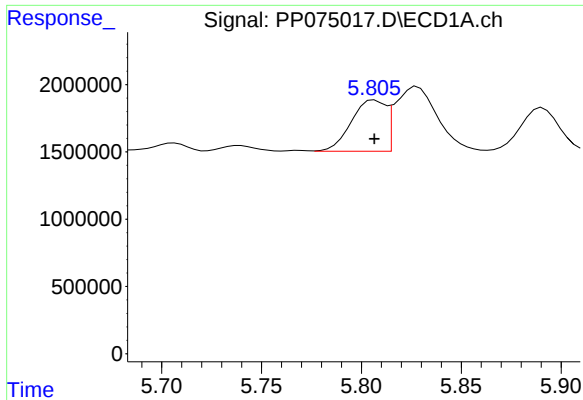

#21 AR-1248-1


R.T.: 5.807 min
Delta R.T.: 0.000 min
Response: 4538895
Conc: 150.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

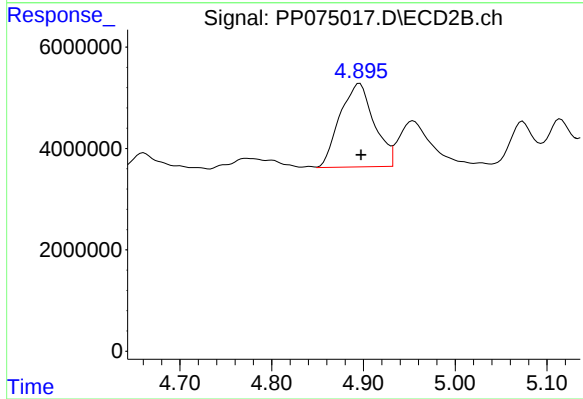


#21 AR-1248-1

R.T.: 4.896 min
Delta R.T.: -0.002 min
Response: 42710422
Conc: 154.67 ng/ml

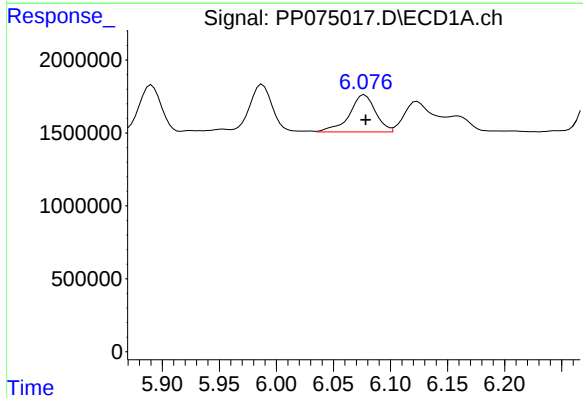


#22 AR-1248-2

R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 4076786
Conc: 94.60 ng/ml

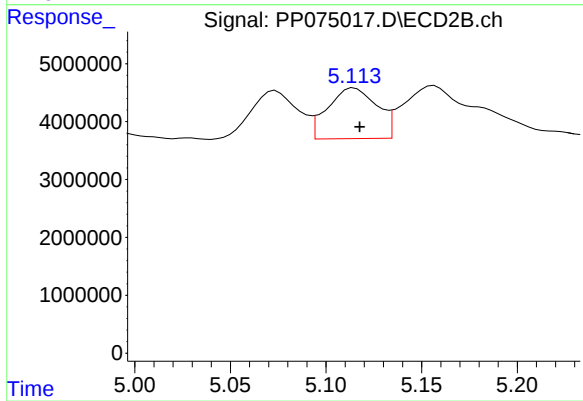

#22 AR-1248-2


R.T.: 5.115 min
Delta R.T.: -0.003 min
Response: 15600365
Conc: 88.26 ng/ml

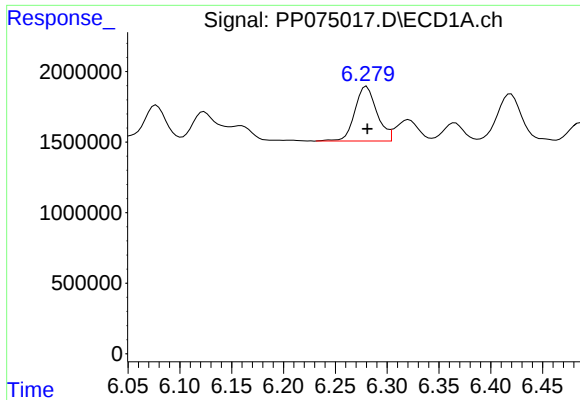

#23 AR-1248-3


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 5720197
Conc: 122.48 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

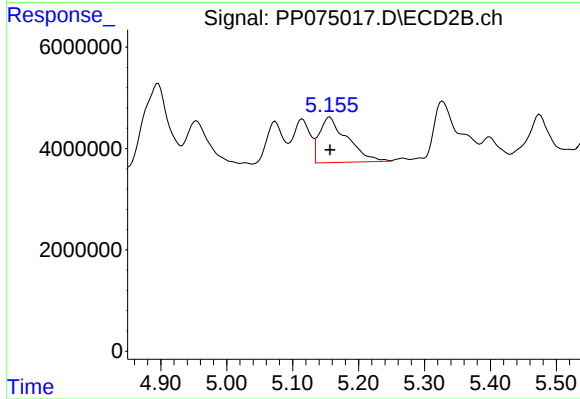


#23 AR-1248-3

R.T.: 5.157 min
Delta R.T.: 0.000 min
Response: 26430125
Conc: 116.33 ng/ml

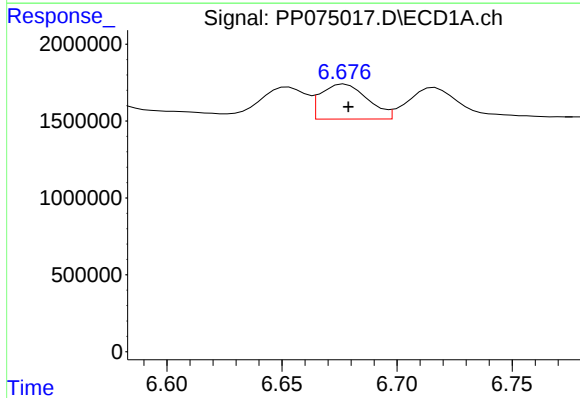


#24 AR-1248-4

R.T.: 6.677 min
Delta R.T.: -0.001 min
Response: 3227654
Conc: 58.68 ng/ml

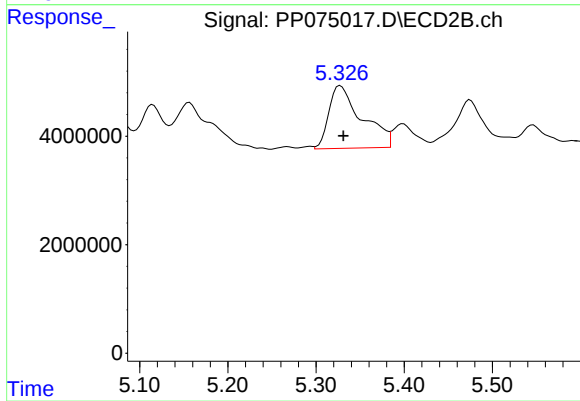

#24 AR-1248-4


R.T.: 5.328 min
Delta R.T.: -0.003 min
Response: 30108660
Conc: 138.10 ng/ml

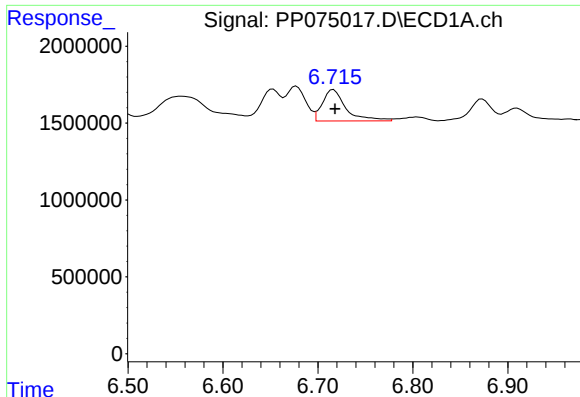

#25 AR-1248-5


R.T.: 6.717 min
Delta R.T.: -0.001 min
Response: 3546149
Conc: 63.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

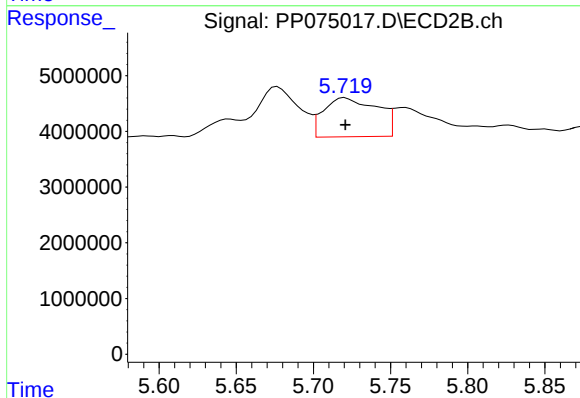


#25 AR-1248-5

R.T.: 5.720 min
Delta R.T.: 0.000 min
Response: 16928309
Conc: 46.09 ng/ml

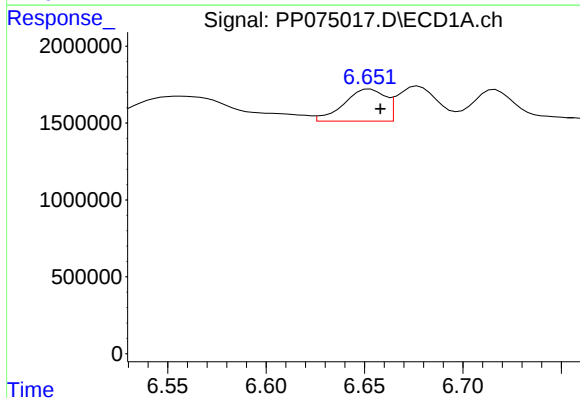


#26 AR-1254-1

R.T.: 6.653 min
Delta R.T.: -0.005 min
Response: 3050910
Conc: 52.36 ng/ml

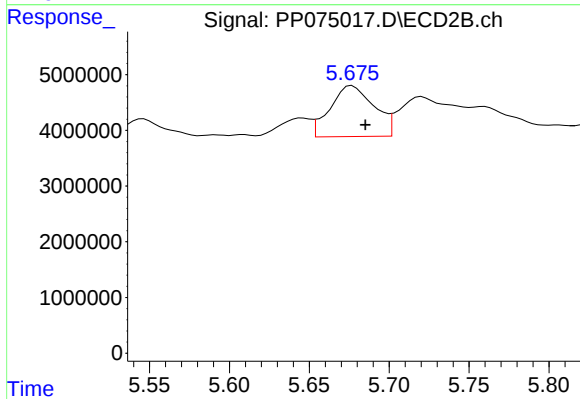

#26 AR-1254-1


R.T.: 5.677 min
Delta R.T.: -0.008 min
Response: 17459361
Conc: 36.62 ng/ml

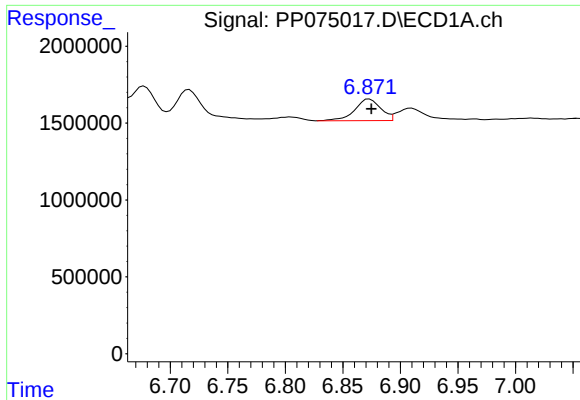

#27 AR-1254-2


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 2225020
Conc: 27.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

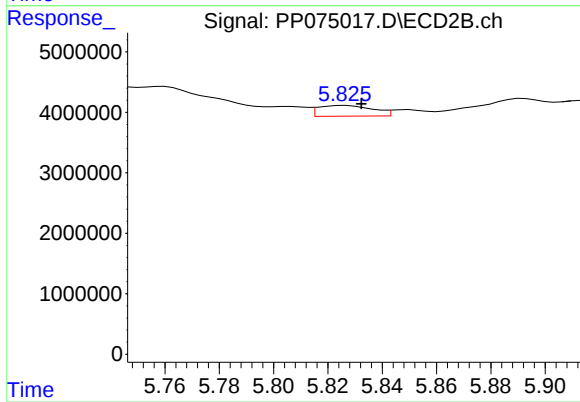


#27 AR-1254-2

R.T.: 5.827 min
Delta R.T.: -0.006 min
Response: 2467660
Conc: 7.01 ng/ml

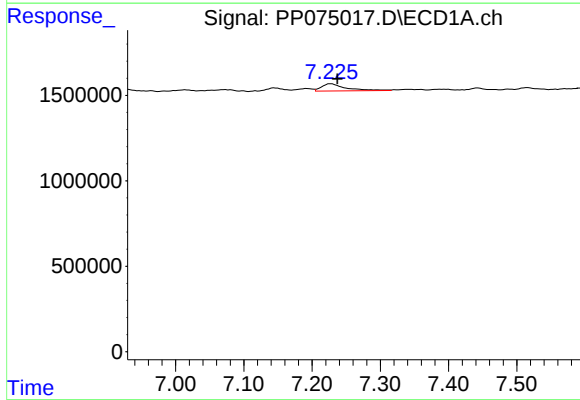


#28 AR-1254-3

R.T.: 7.227 min
Delta R.T.: -0.009 min
Response: 1046932
Conc: 11.74 ng/ml

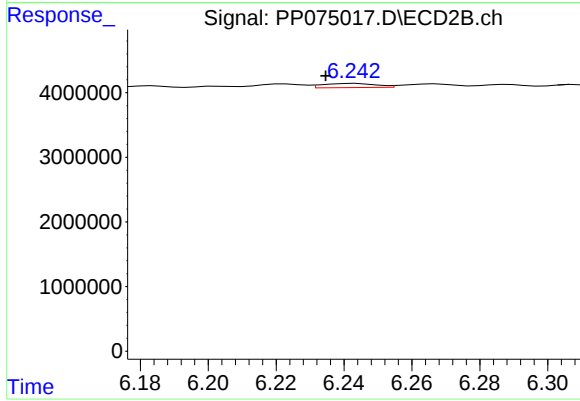

#28 AR-1254-3


R.T.: 6.243 min
Delta R.T.: 0.009 min
Response: 692304
Conc: 1.12 ng/ml

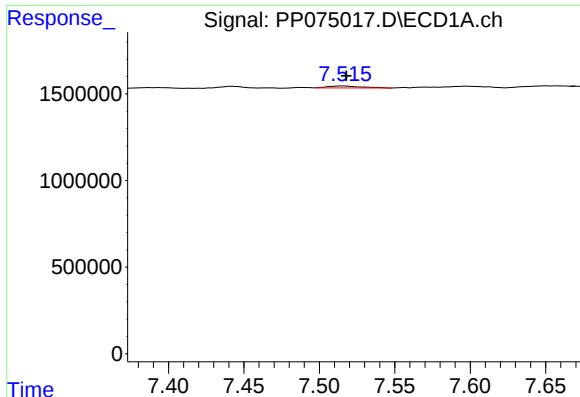

#29 AR-1254-4


R.T.: 7.516 min
Delta R.T.: -0.001 min
Response: 171114
Conc: 2.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

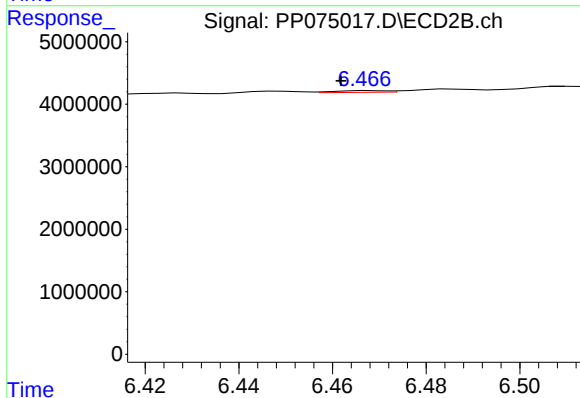


#29 AR-1254-4

R.T.: 6.468 min
Delta R.T.: 0.007 min
Response: 218423
Conc: 0.47 ng/ml

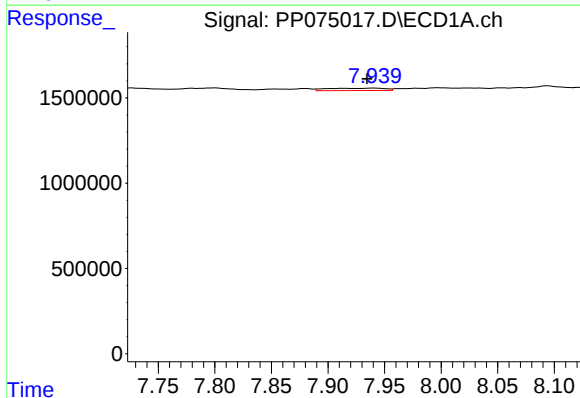


#30 AR-1254-5

R.T.: 7.940 min
Delta R.T.: 0.006 min
Response: 482701
Conc: 5.81 ng/ml

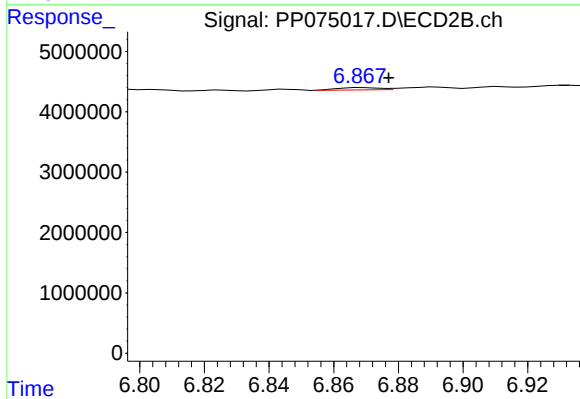

#30 AR-1254-5


R.T.: 6.869 min
Delta R.T.: -0.008 min
Response: 335721
Conc: 0.68 ng/ml

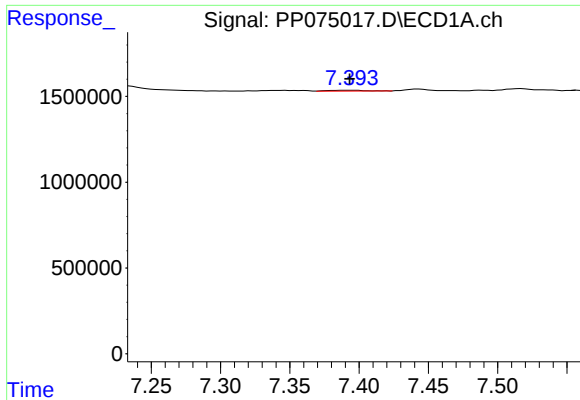

#31 AR-1260-1


R.T.: 7.394 min
Delta R.T.: 0.000 min
Response: 93607
Conc: 1.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

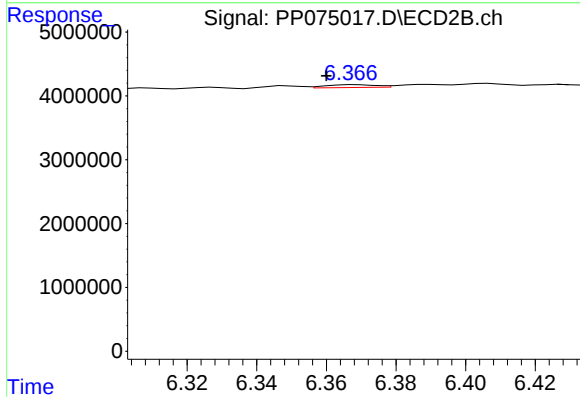


#31 AR-1260-1

R.T.: 6.368 min
Delta R.T.: 0.008 min
Response: 436503
Conc: 1.16 ng/ml

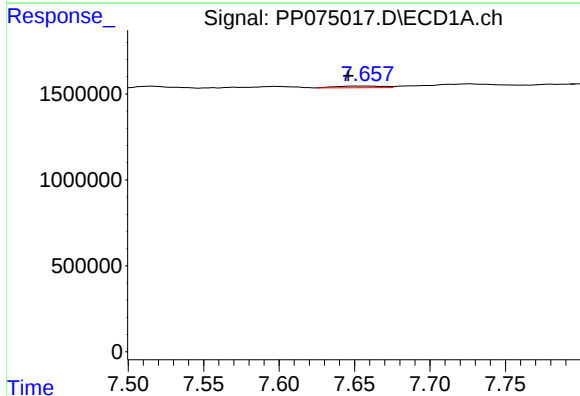


#32 AR-1260-2

R.T.: 7.659 min
Delta R.T.: 0.013 min
Response: 217786
Conc: 3.16 ng/ml

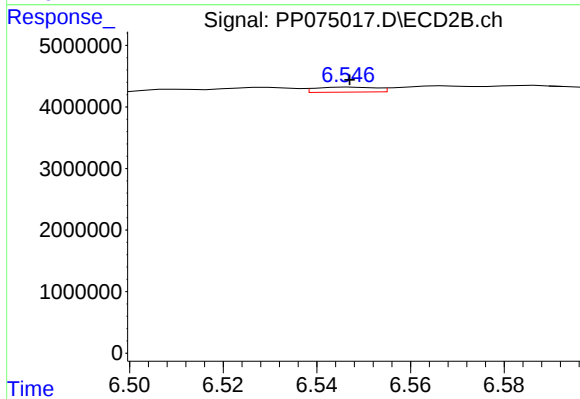

#32 AR-1260-2


R.T.: 6.547 min
Delta R.T.: 0.000 min
Response: 719897
Conc: 1.36 ng/ml

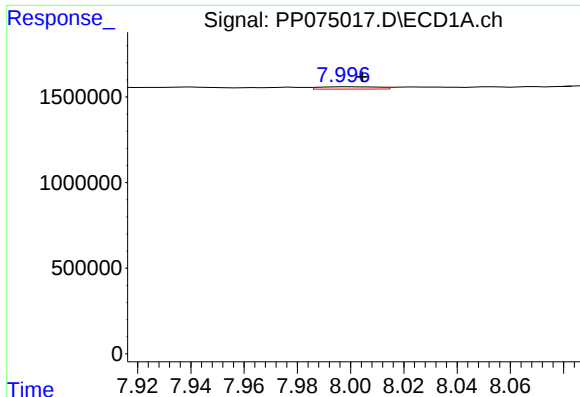

#33 AR-1260-3


R.T.: 7.998 min
Delta R.T.: -0.006 min
Response: 215700
Conc: 4.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

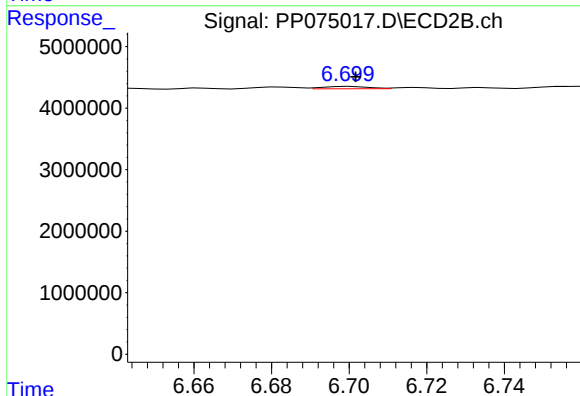


#33 AR-1260-3

R.T.: 6.700 min
Delta R.T.: -0.002 min
Response: 314582
Conc: 0.73 ng/ml

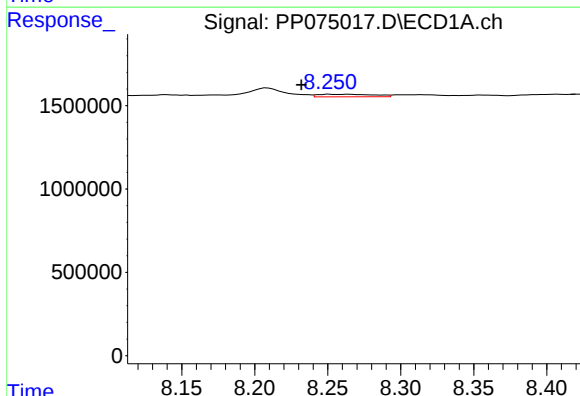


#34 AR-1260-4

R.T.: 8.252 min
Delta R.T.: 0.020 min
Response: 409222
Conc: 6.41 ng/ml

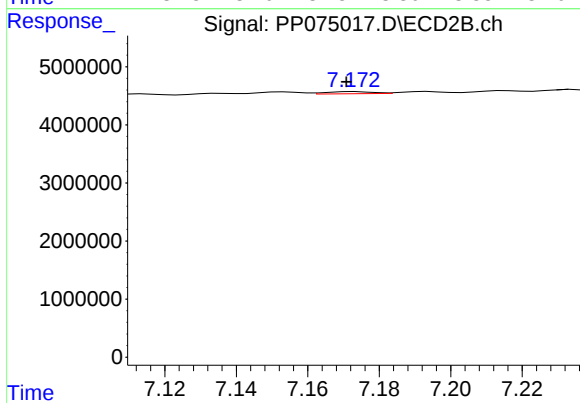

#34 AR-1260-4


R.T.: 7.173 min
Delta R.T.: 0.002 min
Response: 339682
Conc: 0.89 ng/ml

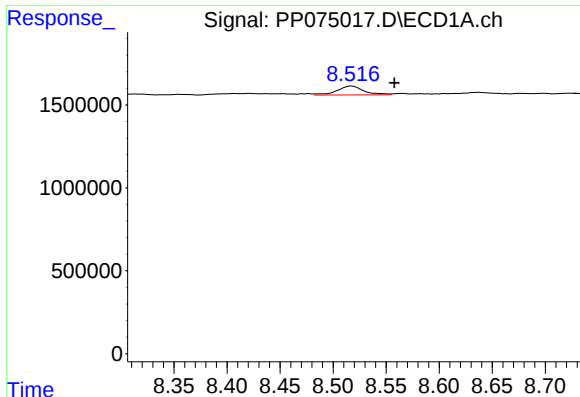

#35 AR-1260-5


R.T.: 8.518 min
Delta R.T.: -0.040 min
Response: 933320
Conc: 8.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

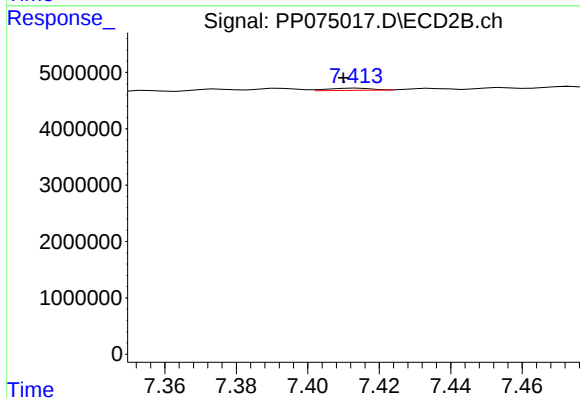


#35 AR-1260-5

R.T.: 7.414 min
Delta R.T.: 0.004 min
Response: 340268
Conc: 0.34 ng/ml

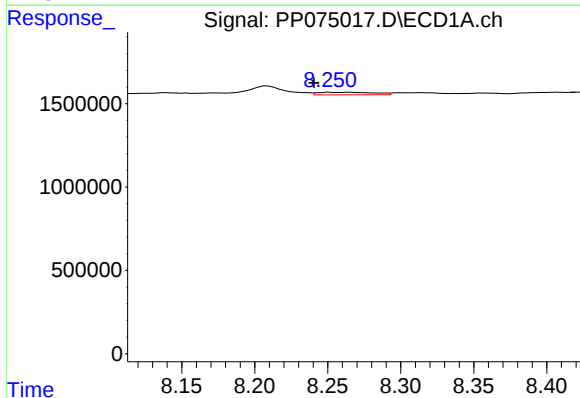


#36 AR-1262-1

R.T.: 8.252 min
Delta R.T.: 0.011 min
Response: 409222
Conc: 5.31 ng/ml

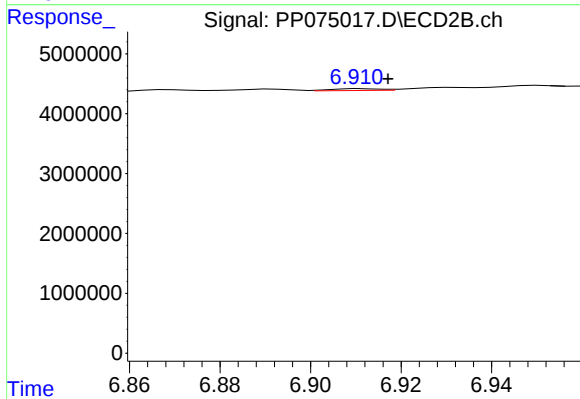

#36 AR-1262-1


R.T.: 6.911 min
Delta R.T.: -0.006 min
Response: 228272
Conc: 0.32 ng/ml

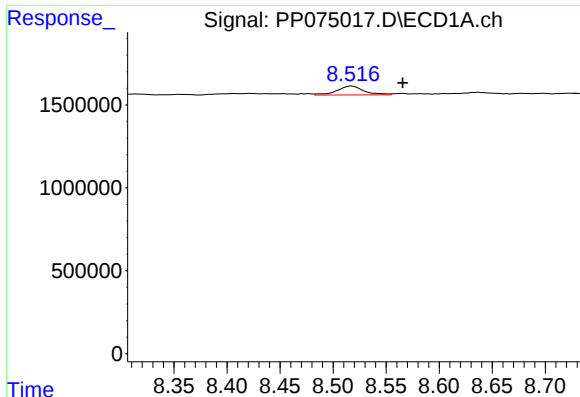

#37 AR-1262-2


R.T.: 8.518 min
Delta R.T.: -0.048 min
Response: 933320
Conc: 7.05 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

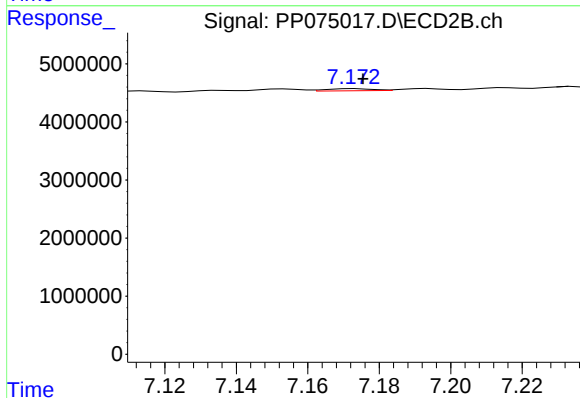


#37 AR-1262-2

R.T.: 7.173 min
Delta R.T.: -0.002 min
Response: 339682
Conc: 0.65 ng/ml

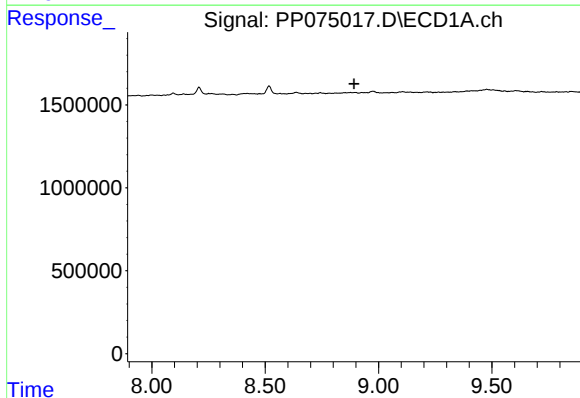


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

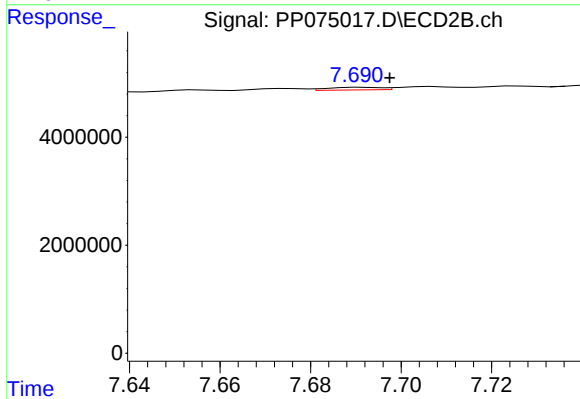

#38 AR-1262-3


R.T.: 7.691 min
Delta R.T.: -0.006 min
Response: 393840
Conc: 0.84 ng/ml

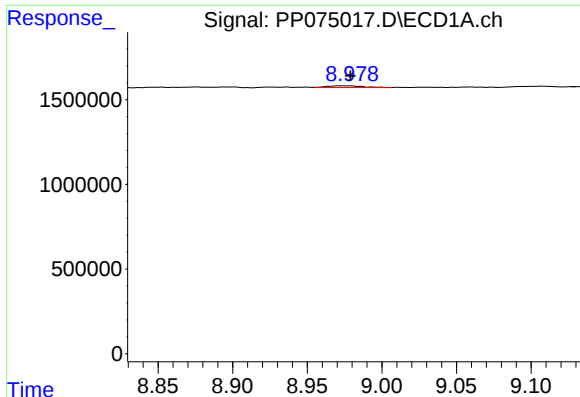

#39 AR-1262-4


R.T.: 8.974 min
Delta R.T.: -0.005 min
Response: 171110
Conc: 2.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

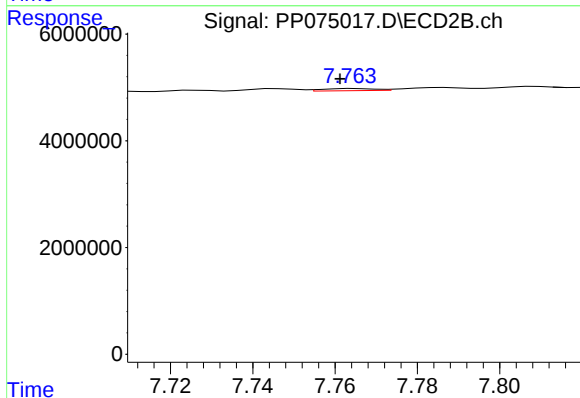


#39 AR-1262-4

R.T.: 7.765 min
Delta R.T.: 0.004 min
Response: 357844
Conc: 0.44 ng/ml

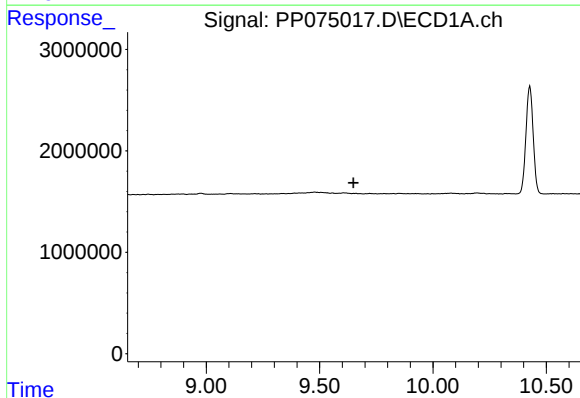


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.650 min
Response: 0
Conc: N.D.

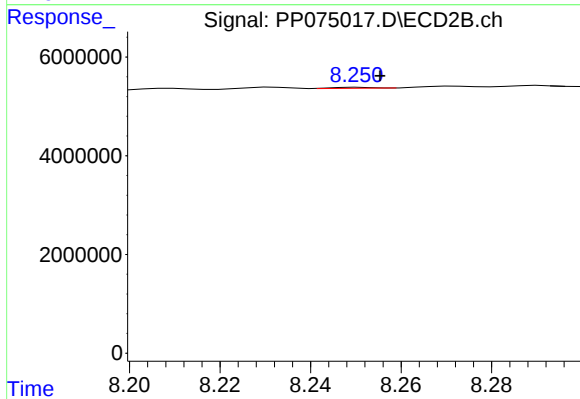

#40 AR-1262-5


R.T.: 8.251 min
Delta R.T.: -0.005 min
Response: 111947
Conc: 0.31 ng/ml

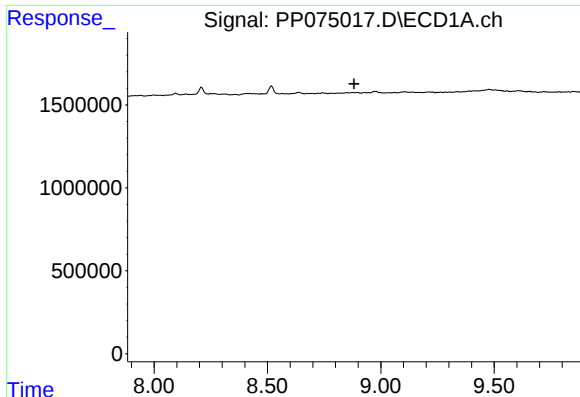

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

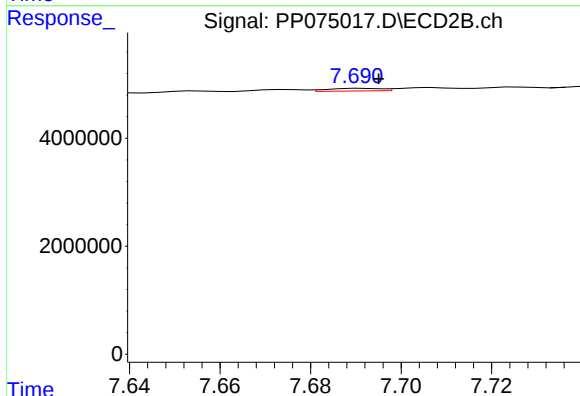


#41 AR-1268-1

R.T.: 7.691 min
Delta R.T.: -0.004 min
Response: 393840
Conc: 0.28 ng/ml

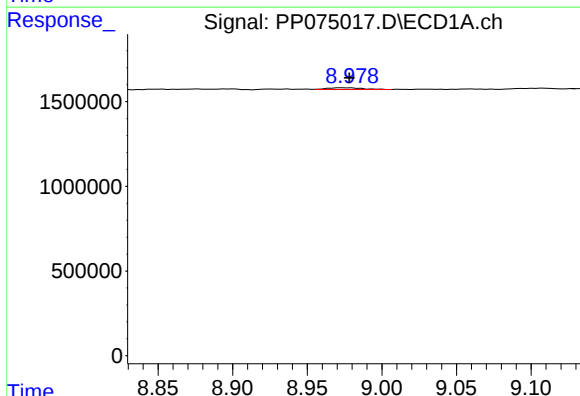


#42 AR-1268-2

R.T.: 8.974 min
Delta R.T.: -0.004 min
Response: 171110
Conc: 1.17 ng/ml

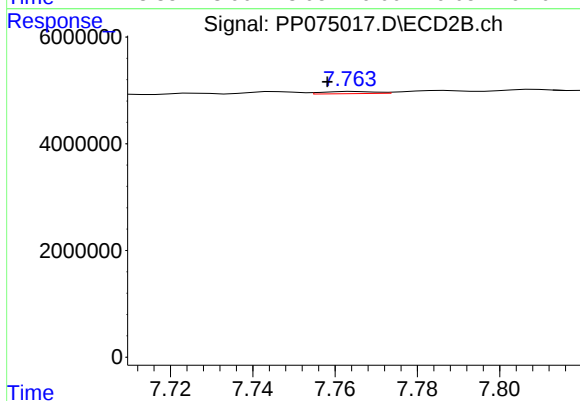

#42 AR-1268-2


R.T.: 7.765 min
Delta R.T.: 0.007 min
Response: 357844
Conc: 0.26 ng/ml

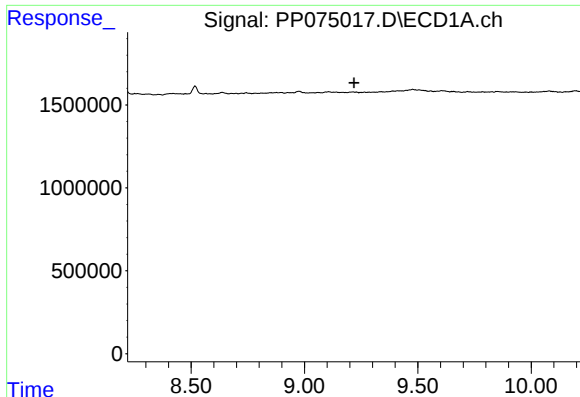

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

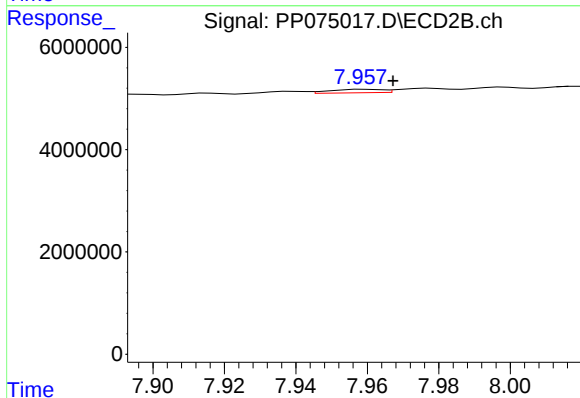


#43 AR-1268-3

R.T.: 7.959 min
Delta R.T.: -0.008 min
Response: 707584
Conc: 0.68 ng/ml

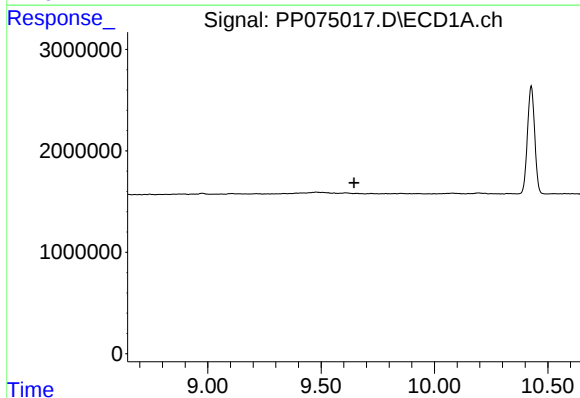


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.645 min
Response: 0
Conc: N.D.

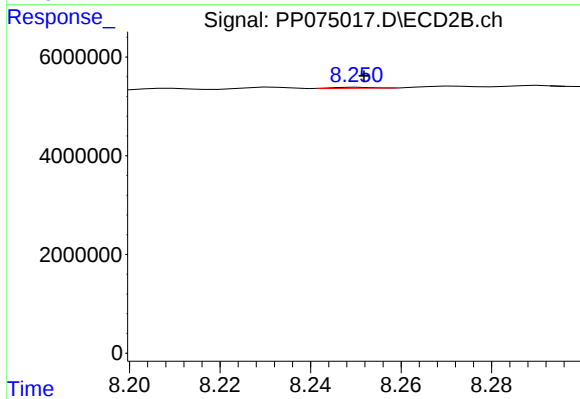

#44 AR-1268-4


R.T.: 8.251 min
Delta R.T.: -0.001 min
Response: 111947
Conc: 0.29 ng/ml

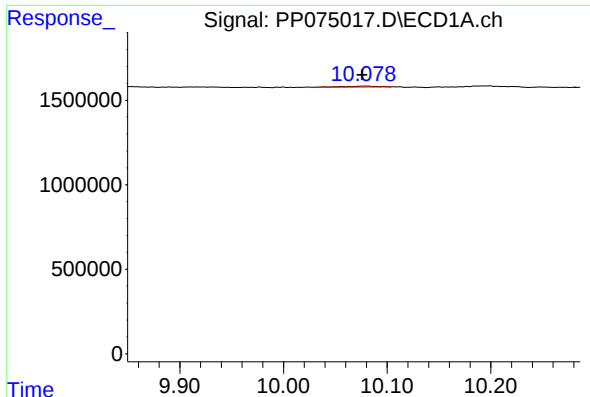

#45 AR-1268-5

R.T.: 10.079 min
Delta R.T.: 0.003 min
Response: 98428
Conc: 0.27 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-K

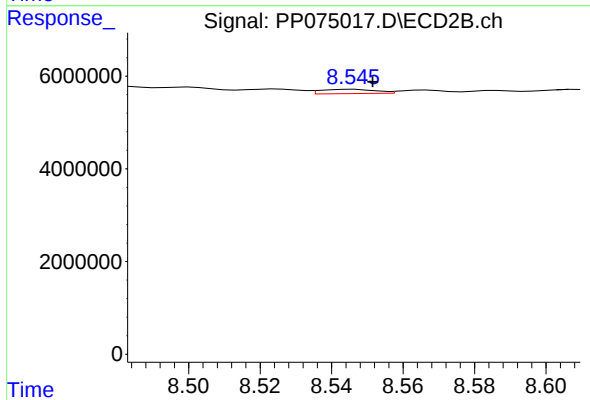

#45 AR-1268-5

R.T.: 8.547 min
Delta R.T.: -0.005 min
Response: 987427
Conc: 0.31 ng/ml