

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
 Data File : PP075029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 10:39
 Operator : YP\AJ
 Sample : Q3034-08DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-HDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:29:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.655	3.796	10128055	30507975	8.277	6.309
2)	SA Decachlor...	10.432	8.803	7915721	46667533	8.016	6.223
Target Compounds							
3)	L1 AR-1016-1	5.806	4.894	24857481	262.6E6	563.804	515.637
4)	L1 AR-1016-2	5.828	4.953	35278252	143.3E6	561.383	602.253
5)	L1 AR-1016-3	5.890	5.073	26091570	85090812	580.924	617.031
6)	L1 AR-1016-4	5.988	5.113	23829643	92719706	677.328	663.216
7)	L1 AR-1016-5	6.280	5.327	31683019	139.6E6	954.708	840.246
8)	L2 AR-1221-1	4.855	4.016	475963	451476	27.054	7.297 #
9)	L2 AR-1221-2	4.941	4.095	715233	2307031	53.547	51.027
10)	L2 AR-1221-3	5.016	4.170	2026363	7502323	53.448	45.664
11)	L3 AR-1232-1	5.016	4.170	2026363	7502323	66.714	58.568
12)	L3 AR-1232-2	5.542	4.894	11767059	262.6E6	746.725	1133.086 #
13)	L3 AR-1232-3	5.828	5.073	35278252	85090812	1155.009	1416.769
14)	L3 AR-1232-4	5.988	5.155	23829643	159.1E6	1379.887	2157.974 #
15)	L3 AR-1232-5	6.077	5.327	22100453	139.6E6	1702.529	2247.782 #
16)	L4 AR-1242-1	5.806	4.894	24857481	262.6E6	649.441	622.739
17)	L4 AR-1242-2	5.828	4.953	35278252	143.3E6	624.593	715.716
18)	L4 AR-1242-3	5.890	5.073	26091570	85090812	642.603	719.291
19)	L4 AR-1242-4	5.988	5.155	23829643	159.1E6	750.733	929.301
20)	L4 AR-1242-5	6.717	5.676	16215429	107.3E6	449.547	579.434 #
21)	L5 AR-1248-1	5.806	4.894	24857481	262.6E6	822.441	951.108
22)	L5 AR-1248-2	6.077	5.113	22100453	92719706	512.818	524.565
23)	L5 AR-1248-3	6.280	5.155	31683019	159.1E6	678.385	700.071
24)	L5 AR-1248-4	6.678	5.327	16977122	139.6E6	308.670	640.080 #
25)	L5 AR-1248-5	6.717	5.716	16215429	102.9E6	292.325	280.187
26)	L6 AR-1254-1	6.653	5.676	14062671	107.3E6	241.339	225.064
27)	L6 AR-1254-2	6.873	5.824	11365007	15968662	139.250	45.348 #
28)	L6 AR-1254-3	7.227	6.223	5372805	6352189	60.229	10.249 #
29)	L6 AR-1254-4	7.514	6.446	513834	1213325	7.796	2.589 #
30)	L6 AR-1254-5	7.928	6.882	1140239	850091	13.724	1.733 #
31)	L7 AR-1260-1	7.397	6.359	315792	694969	5.463	1.852 #
32)	L7 AR-1260-2	7.655	6.574	856313	576064	12.425	1.089 #
33)	L7 AR-1260-3	8.018	6.709	671576	809941	12.943	1.871 #
34)	L7 AR-1260-4	8.210	7.163	1120009	514679	17.557	1.349 #
35)	L7 AR-1260-5	8.520f	7.404	374607	738724	3.303	0.735 #
36)	L8 AR-1262-1	8.269	6.929	376292	864108	4.886	1.222 #
37)	L8 AR-1262-2	8.520f	7.183	374607	397885	2.830	0.764 #
38)	L8 AR-1262-3	0.000	7.693	0	5604793	N.D.	12.020 #
39)	L8 AR-1262-4	8.981	7.753	48092	2383545	0.638	2.900 #
40)	L8 AR-1262-5	9.601f	8.259	117051	843103	1.920	2.353
41)	L9 AR-1268-1	0.000	7.693	0	5604793	N.D.	3.974 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
 Data File : PP075029.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 10:39
 Operator : YP\AJ
 Sample : Q3034-08DL 2X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PASSAIC-HDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:29:21 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42) L9	AR-1268-2	8.981	7.753	48092	2383545	0.328	1.748 #
43) L9	AR-1268-3	0.000	7.963	0	931362	N.D.	0.893 #
44) L9	AR-1268-4	9.601f	8.259	117051	843103	1.740	2.201 #
45) L9	AR-1268-5	0.000	8.552	0	801283	N.D.	0.255 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
Data File : PP075029.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 10:39
Operator : YP\AJ
Sample : Q3034-08DL 2X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:29:21 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

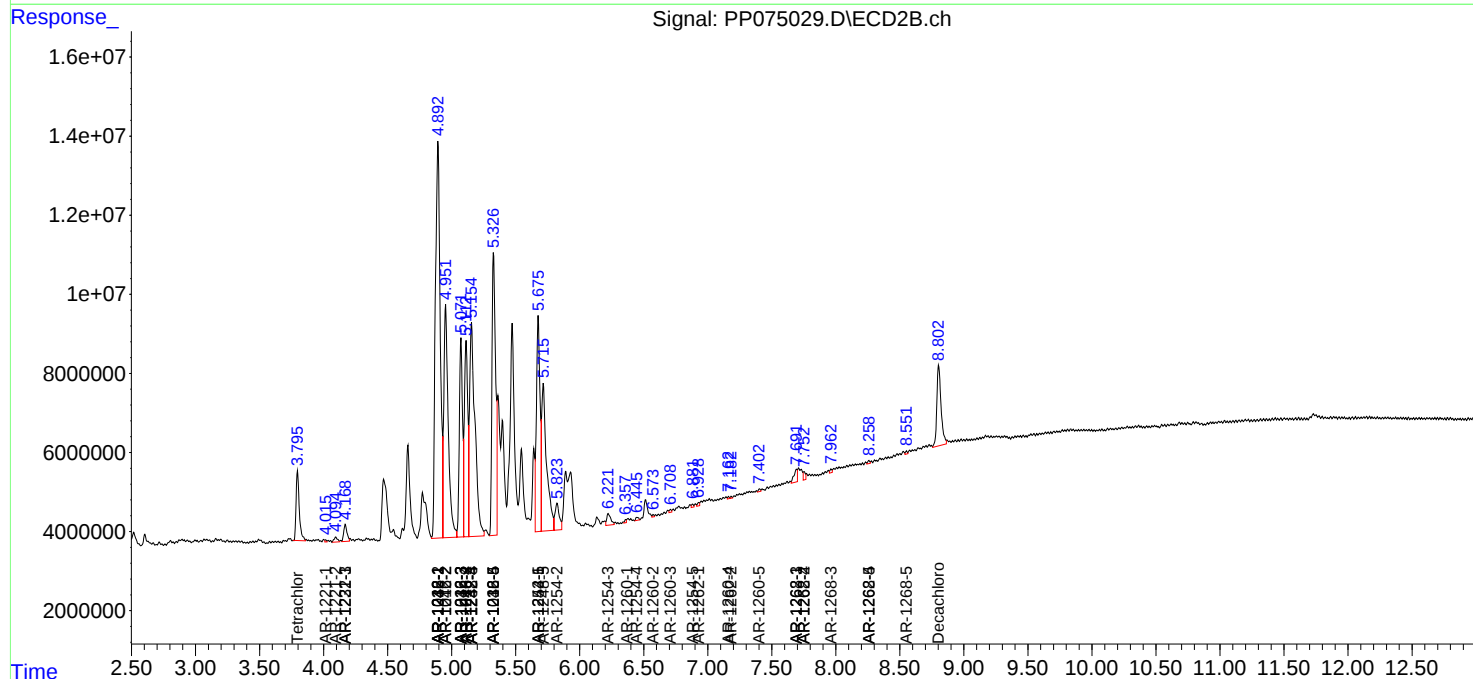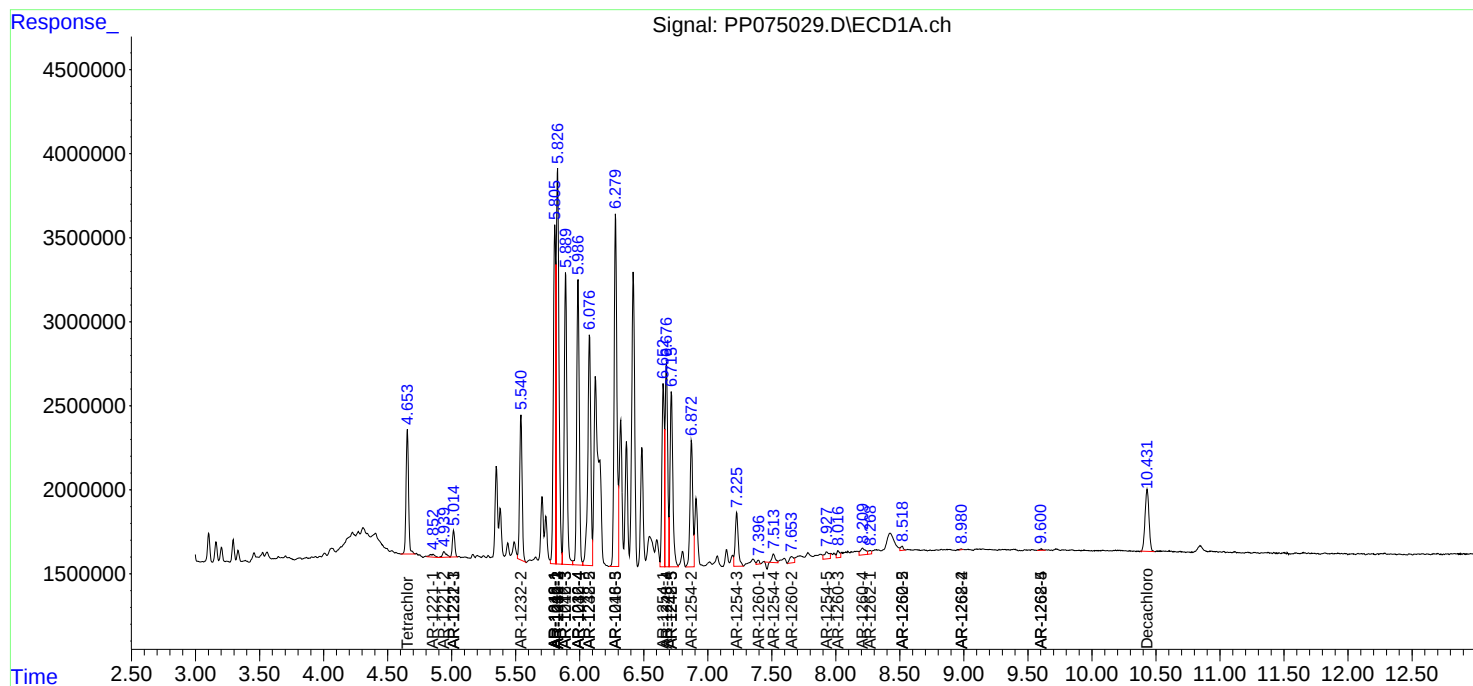


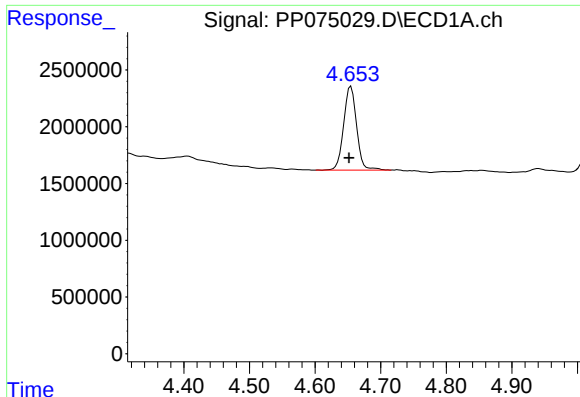

#1 Tetrachloro-m-xylene


R.T.: 4.655 min
Delta R.T.: 0.003 min
Response: 10128055
Conc: 8.28 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

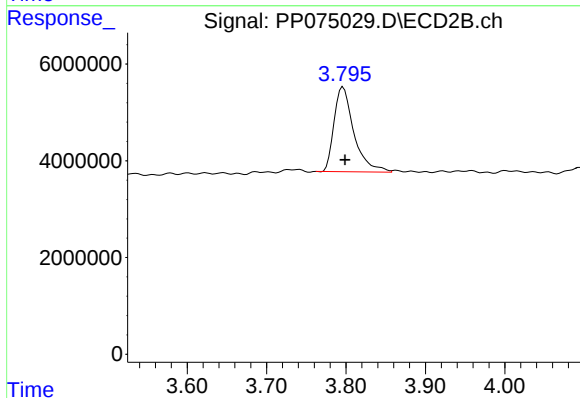


#1 Tetrachloro-m-xylene

R.T.: 3.796 min
Delta R.T.: -0.002 min
Response: 30507975
Conc: 6.31 ng/ml

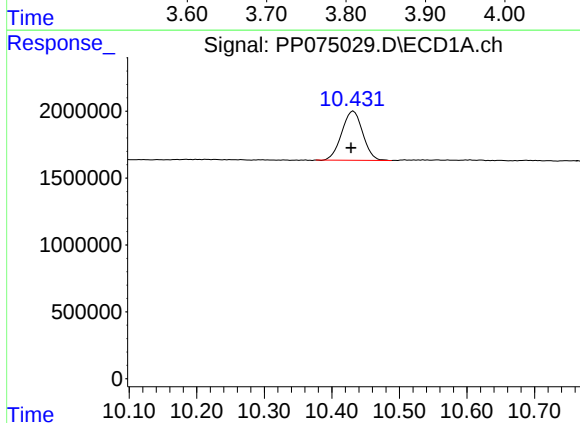


#2 Decachlorobiphenyl

R.T.: 10.432 min
Delta R.T.: 0.004 min
Response: 7915721
Conc: 8.02 ng/ml

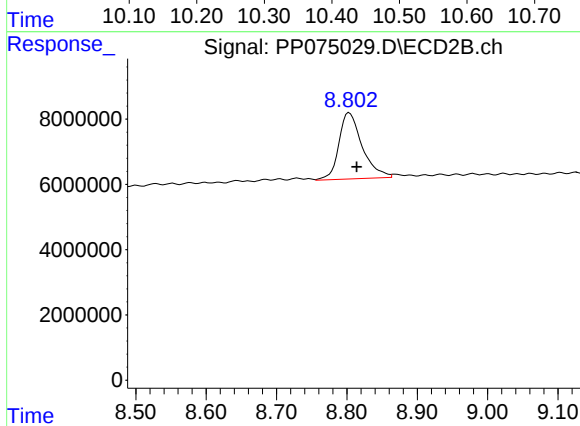

#2 Decachlorobiphenyl


R.T.: 8.803 min
Delta R.T.: -0.011 min
Response: 46667533
Conc: 6.22 ng/ml

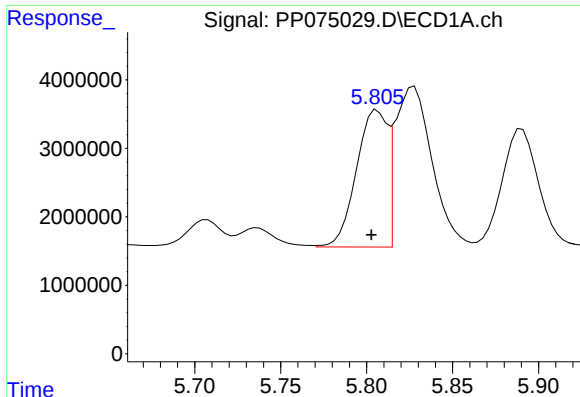

#3 AR-1016-1


R.T.: 5.806 min
Delta R.T.: 0.004 min
Response: 24857481
Conc: 563.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

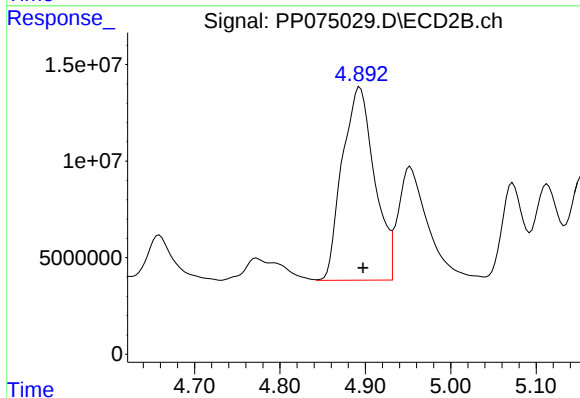


#3 AR-1016-1

R.T.: 4.894 min
Delta R.T.: -0.004 min
Response: 262641770
Conc: 515.64 ng/ml

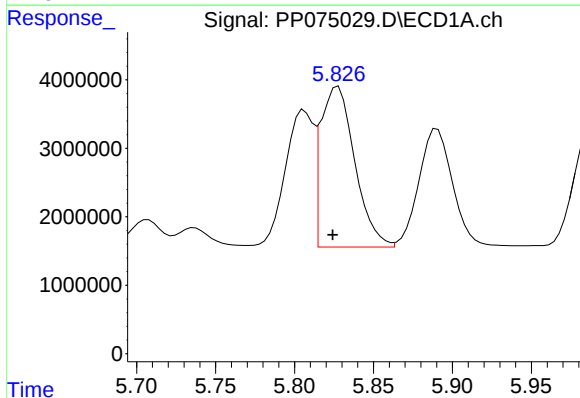


#4 AR-1016-2

R.T.: 5.828 min
Delta R.T.: 0.004 min
Response: 35278252
Conc: 561.38 ng/ml

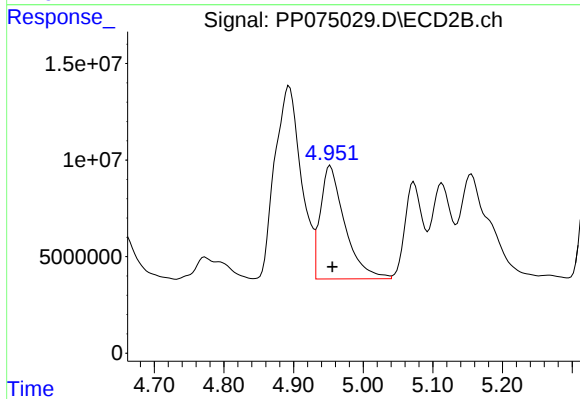

#4 AR-1016-2


R.T.: 4.953 min
Delta R.T.: -0.003 min
Response: 143345547
Conc: 602.25 ng/ml

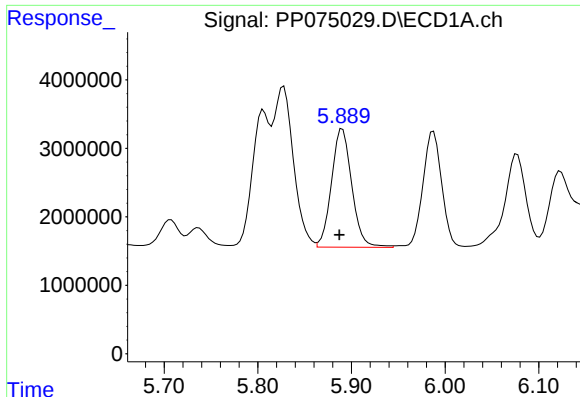

#5 AR-1016-3


R.T.: 5.890 min
Delta R.T.: 0.003 min
Response: 26091570
Conc: 580.92 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

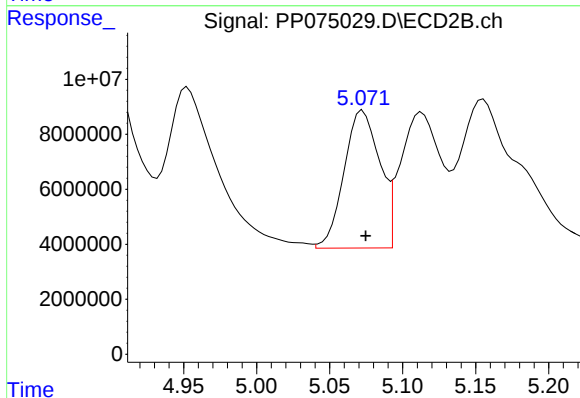


#5 AR-1016-3

R.T.: 5.073 min
Delta R.T.: -0.002 min
Response: 85090812
Conc: 617.03 ng/ml

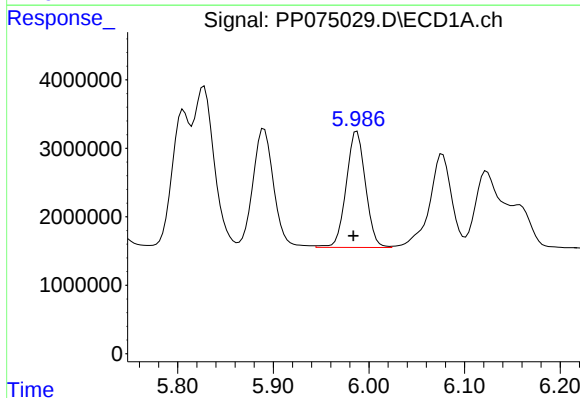


#6 AR-1016-4

R.T.: 5.988 min
Delta R.T.: 0.004 min
Response: 23829643
Conc: 677.33 ng/ml

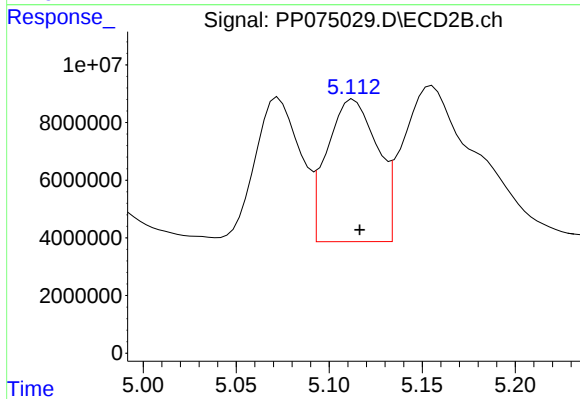

#6 AR-1016-4


R.T.: 5.113 min
Delta R.T.: -0.003 min
Response: 92719706
Conc: 663.22 ng/ml

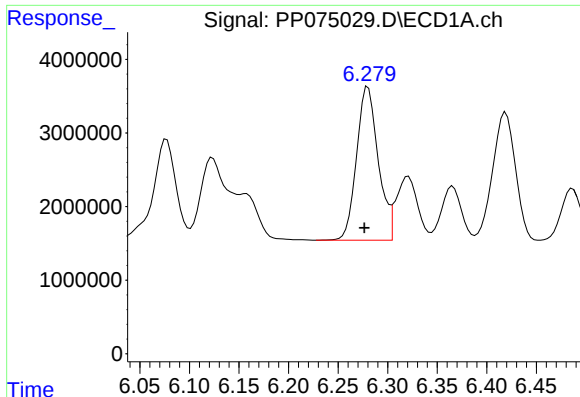

#7 AR-1016-5


R.T.: 6.280 min
Delta R.T.: 0.004 min
Response: 31683019
Conc: 954.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

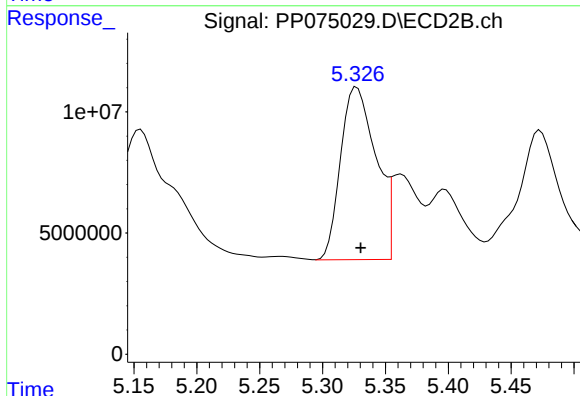


#7 AR-1016-5

R.T.: 5.327 min
Delta R.T.: -0.003 min
Response: 139550828
Conc: 840.25 ng/ml

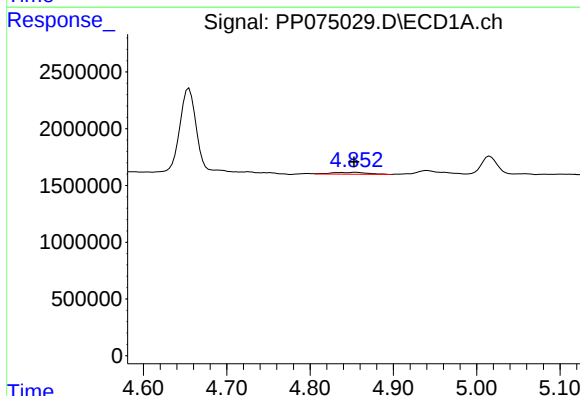


#8 AR-1221-1

R.T.: 4.855 min
Delta R.T.: 0.002 min
Response: 475963
Conc: 27.05 ng/ml

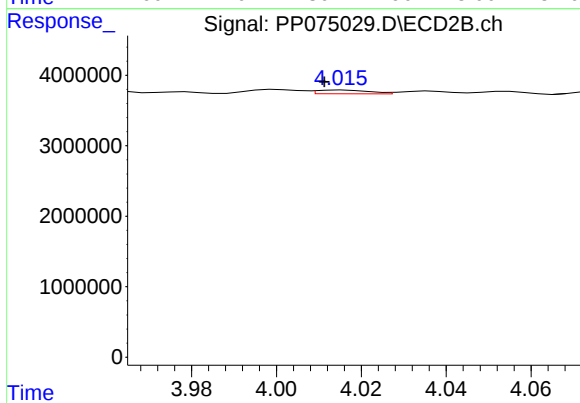

#8 AR-1221-1


R.T.: 4.016 min
Delta R.T.: 0.004 min
Response: 451476
Conc: 7.30 ng/ml

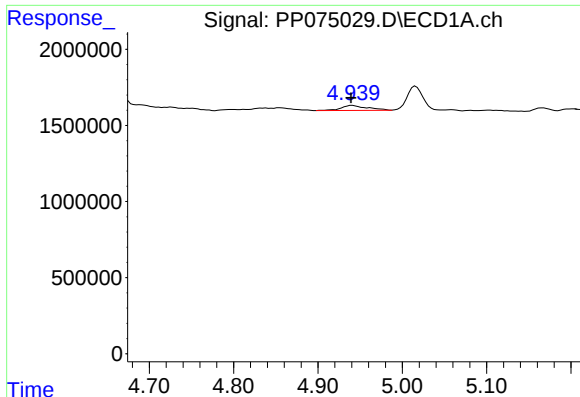

#9 AR-1221-2


R.T.: 4.941 min
Delta R.T.: 0.001 min
Response: 715233
Conc: 53.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

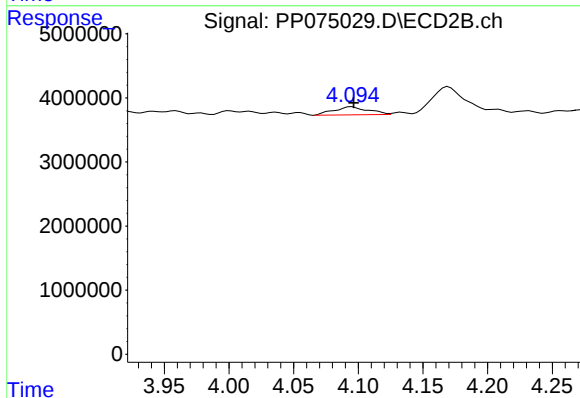


#9 AR-1221-2

R.T.: 4.095 min
Delta R.T.: -0.002 min
Response: 2307031
Conc: 51.03 ng/ml

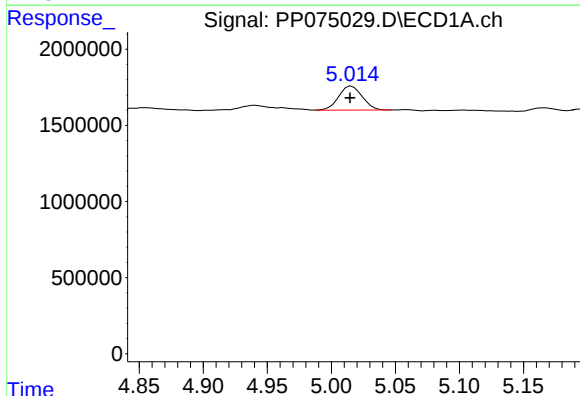


#10 AR-1221-3

R.T.: 5.016 min
Delta R.T.: 0.001 min
Response: 2026363
Conc: 53.45 ng/ml

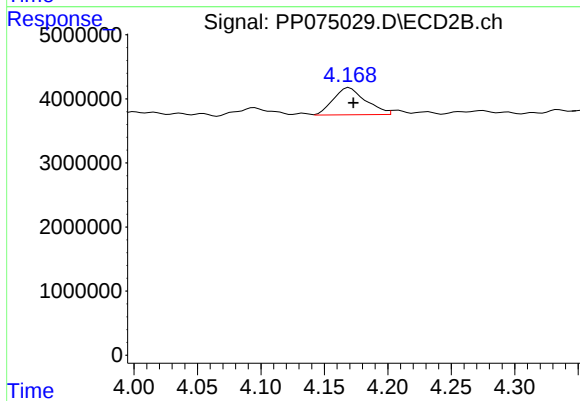

#10 AR-1221-3


R.T.: 4.170 min
Delta R.T.: -0.003 min
Response: 7502323
Conc: 45.66 ng/ml

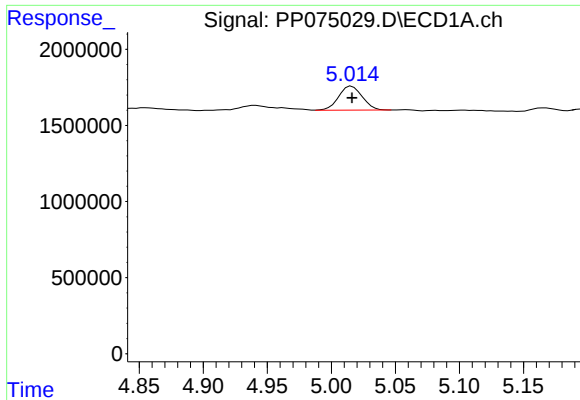

#11 AR-1232-1


R.T.: 5.016 min
Delta R.T.: 0.000 min
Response: 2026363
Conc: 66.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

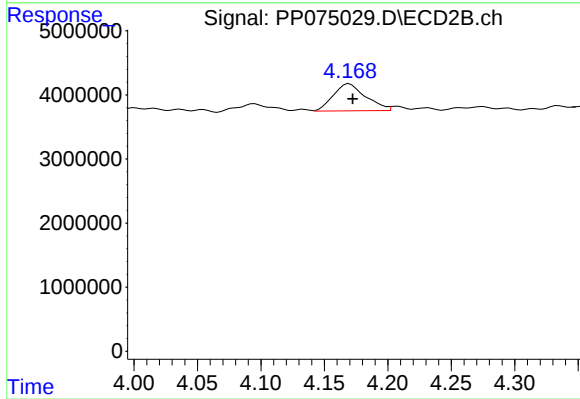


#11 AR-1232-1

R.T.: 4.170 min
Delta R.T.: -0.003 min
Response: 7502323
Conc: 58.57 ng/ml

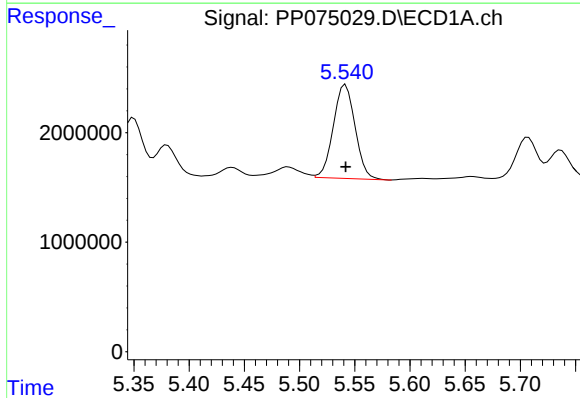


#12 AR-1232-2

R.T.: 5.542 min
Delta R.T.: 0.000 min
Response: 11767059
Conc: 746.72 ng/ml

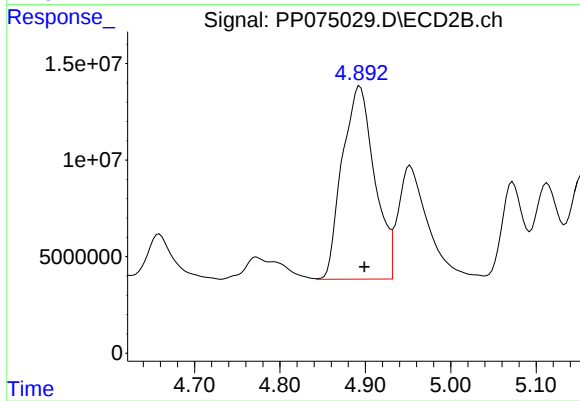

#12 AR-1232-2


R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 262641770
Conc: 1133.09 ng/ml

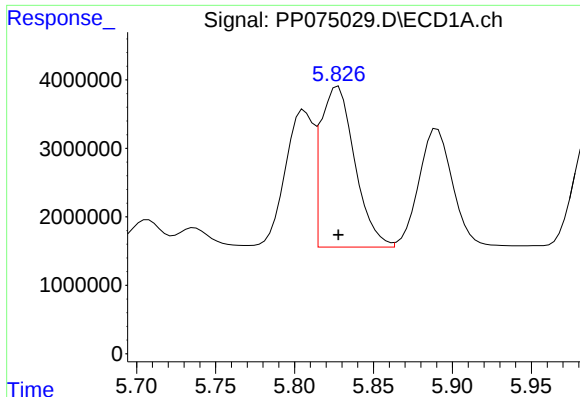

#13 AR-1232-3


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 35278252
Conc: 1155.01 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

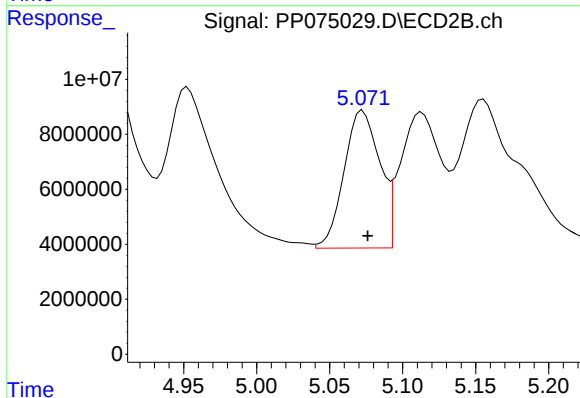


#13 AR-1232-3

R.T.: 5.073 min
Delta R.T.: -0.003 min
Response: 85090812
Conc: 1416.77 ng/ml

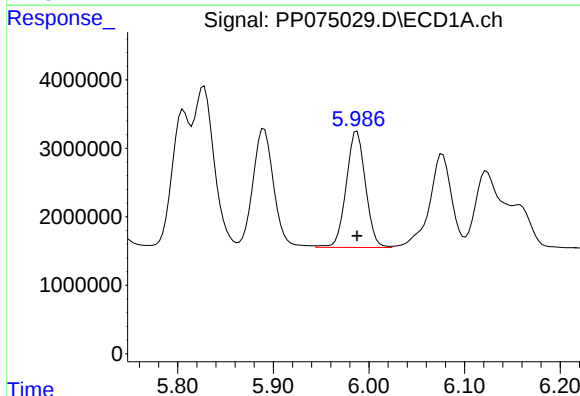


#14 AR-1232-4

R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 23829643
Conc: 1379.89 ng/ml

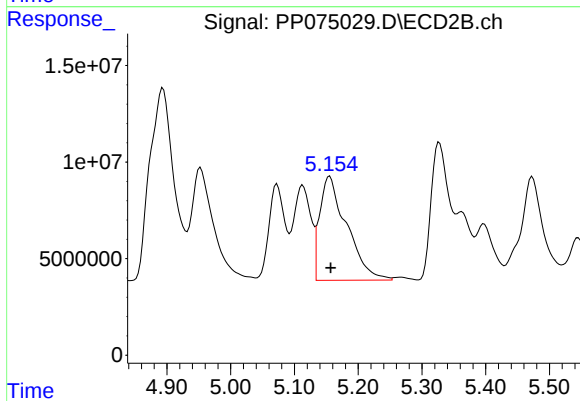

#14 AR-1232-4


R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 159058606
Conc: 2157.97 ng/ml

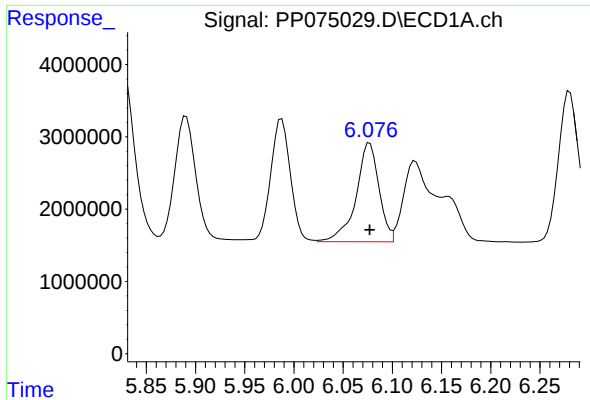

#15 AR-1232-5


R.T.: 6.077 min
Delta R.T.: 0.000 min
Response: 22100453
Conc: 1702.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

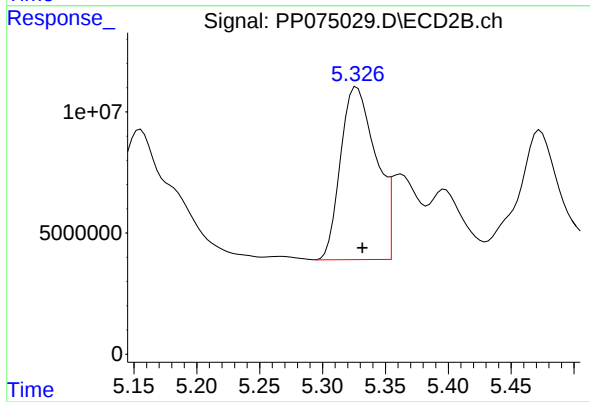


#15 AR-1232-5

R.T.: 5.327 min
Delta R.T.: -0.005 min
Response: 139550828
Conc: 2247.78 ng/ml

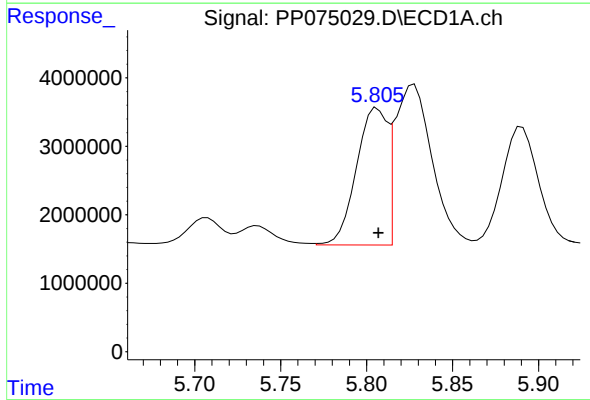


#16 AR-1242-1

R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 24857481
Conc: 649.44 ng/ml

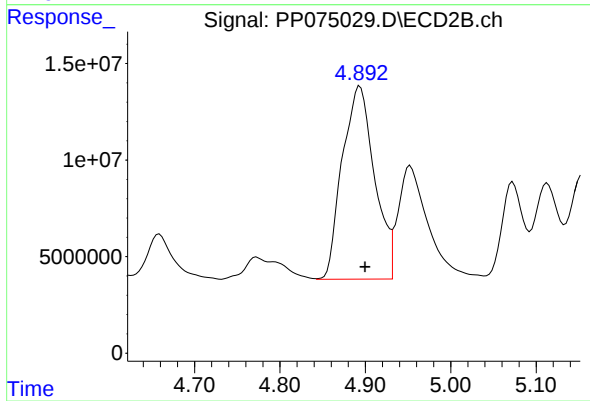

#16 AR-1242-1


R.T.: 4.894 min
Delta R.T.: -0.006 min
Response: 262641770
Conc: 622.74 ng/ml

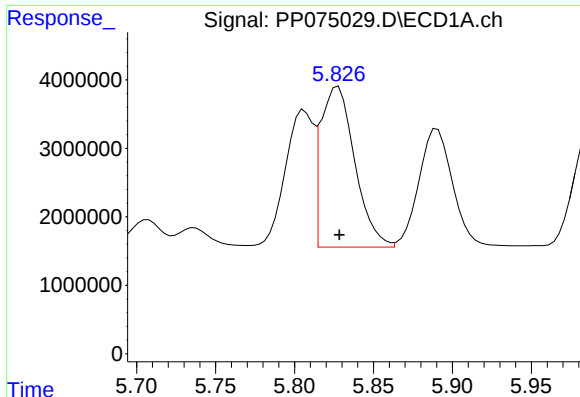

#17 AR-1242-2


R.T.: 5.828 min
Delta R.T.: 0.000 min
Response: 35278252
Conc: 624.59 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

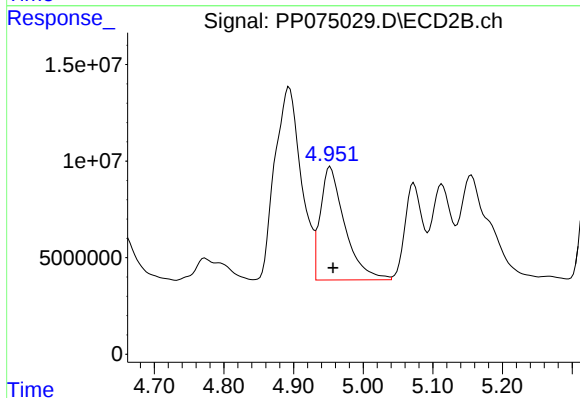


#17 AR-1242-2

R.T.: 4.953 min
Delta R.T.: -0.004 min
Response: 143345547
Conc: 715.72 ng/ml

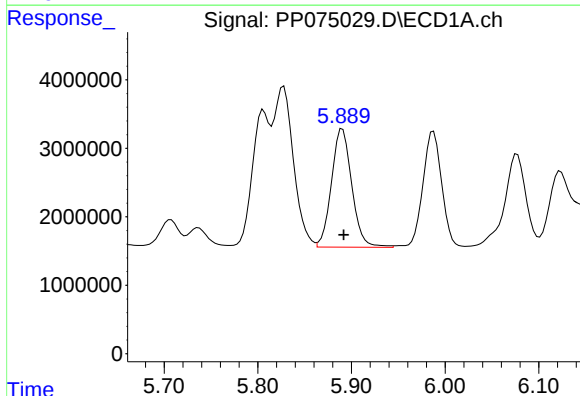


#18 AR-1242-3

R.T.: 5.890 min
Delta R.T.: -0.001 min
Response: 26091570
Conc: 642.60 ng/ml

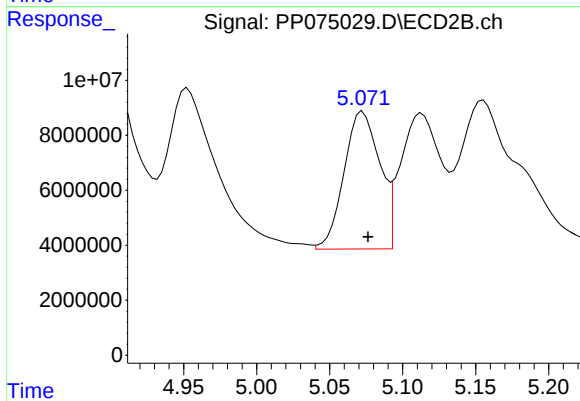

#18 AR-1242-3


R.T.: 5.073 min
Delta R.T.: -0.004 min
Response: 85090812
Conc: 719.29 ng/ml

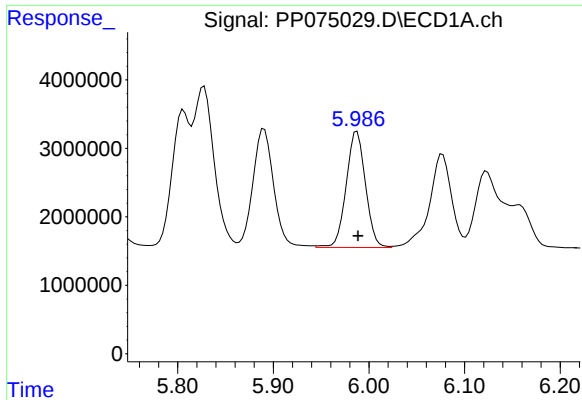

#19 AR-1242-4


R.T.: 5.988 min
Delta R.T.: 0.000 min
Response: 23829643
Conc: 750.73 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

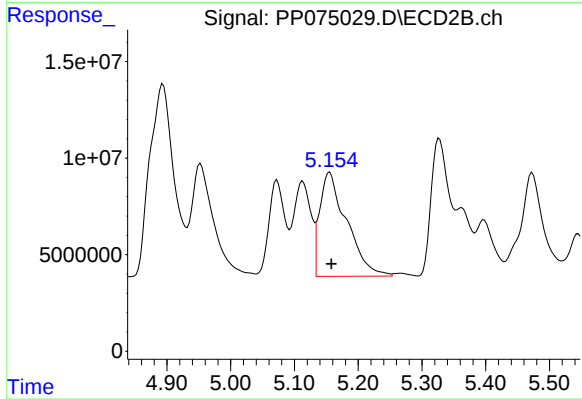


#19 AR-1242-4

R.T.: 5.155 min
Delta R.T.: -0.003 min
Response: 159058606
Conc: 929.30 ng/ml

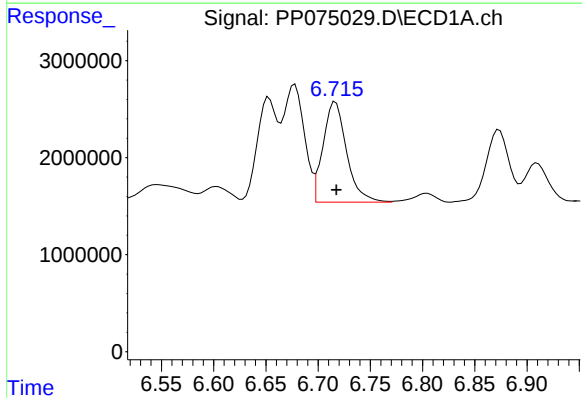


#20 AR-1242-5

R.T.: 6.717 min
Delta R.T.: 0.000 min
Response: 16215429
Conc: 449.55 ng/ml

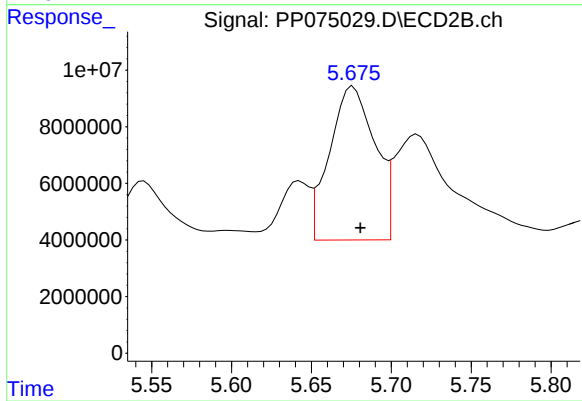

#20 AR-1242-5


R.T.: 5.676 min
Delta R.T.: -0.005 min
Response: 107290309
Conc: 579.43 ng/ml

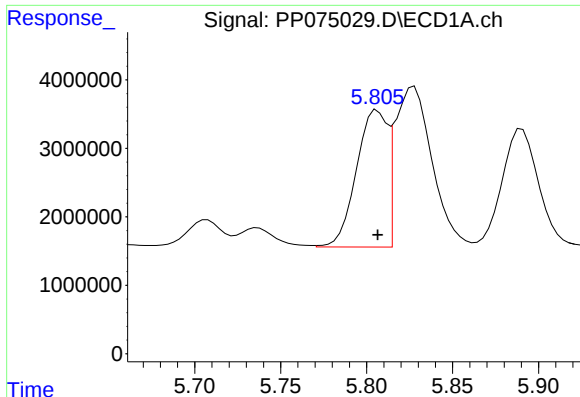

#21 AR-1248-1


R.T.: 5.806 min
Delta R.T.: 0.000 min
Response: 24857481
Conc: 822.44 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

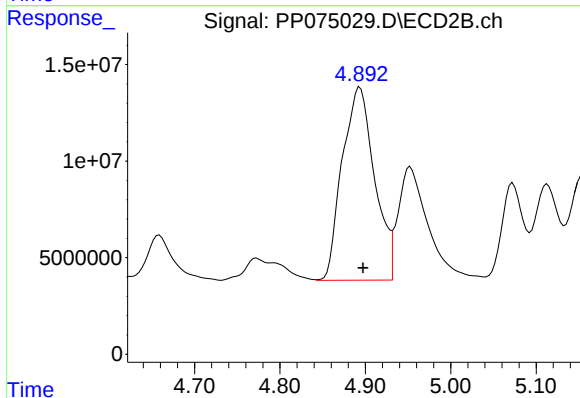


#21 AR-1248-1

R.T.: 4.894 min
Delta R.T.: -0.004 min
Response: 262641770
Conc: 951.11 ng/ml

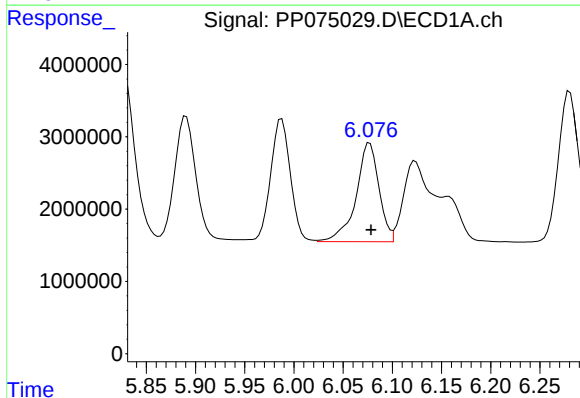


#22 AR-1248-2

R.T.: 6.077 min
Delta R.T.: -0.001 min
Response: 22100453
Conc: 512.82 ng/ml

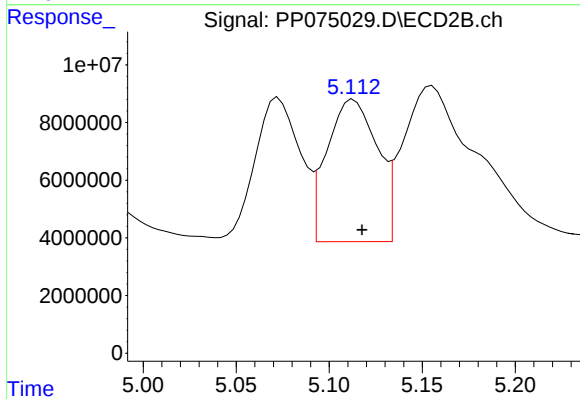

#22 AR-1248-2


R.T.: 5.113 min
Delta R.T.: -0.005 min
Response: 92719706
Conc: 524.56 ng/ml

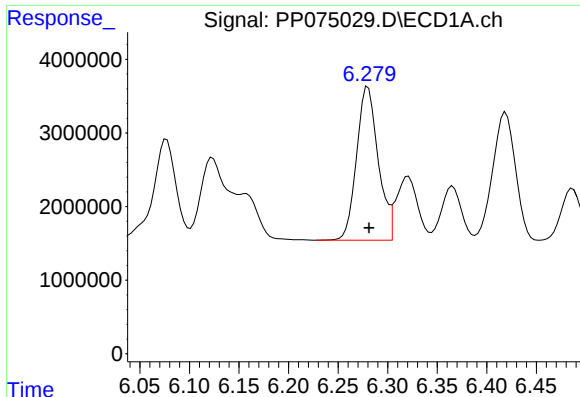

#23 AR-1248-3


R.T.: 6.280 min
Delta R.T.: 0.000 min
Response: 31683019
Conc: 678.38 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

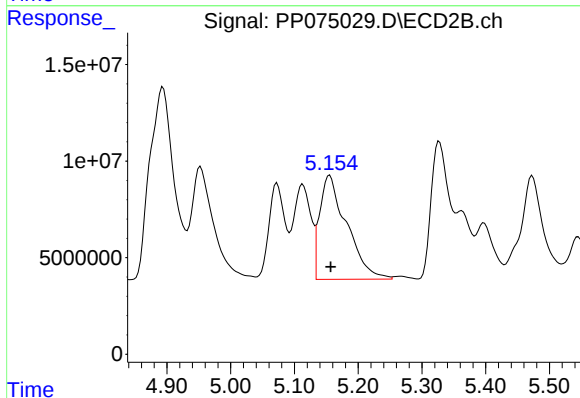


#23 AR-1248-3

R.T.: 5.155 min
Delta R.T.: -0.002 min
Response: 159058606
Conc: 700.07 ng/ml

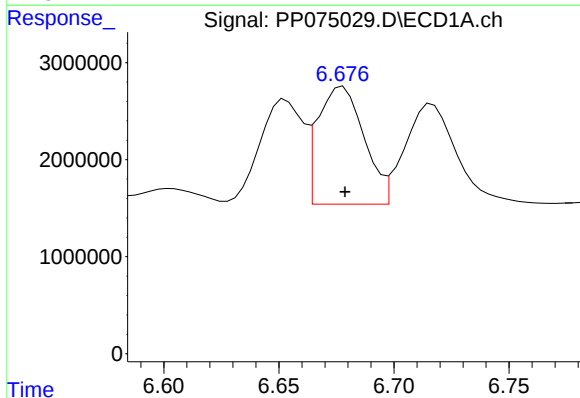


#24 AR-1248-4

R.T.: 6.678 min
Delta R.T.: 0.000 min
Response: 16977122
Conc: 308.67 ng/ml

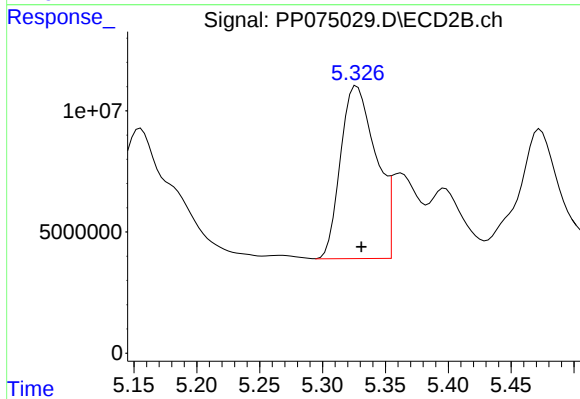

#24 AR-1248-4


R.T.: 5.327 min
Delta R.T.: -0.004 min
Response: 139550828
Conc: 640.08 ng/ml

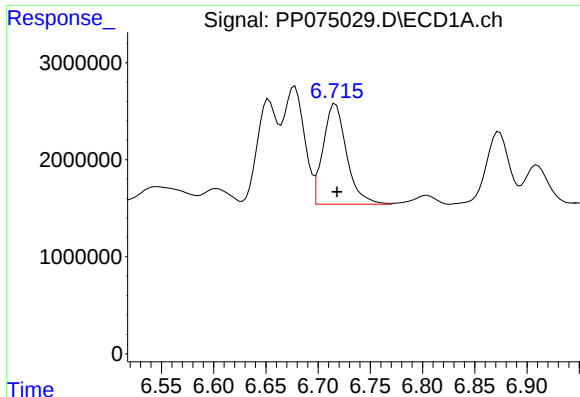

#25 AR-1248-5


R.T.: 6.717 min
Delta R.T.: -0.001 min
Response: 16215429
Conc: 292.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

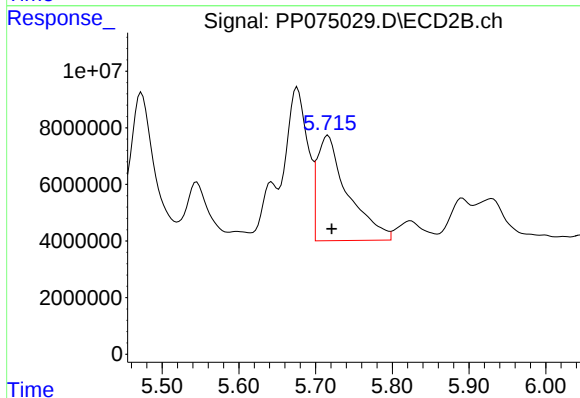


#25 AR-1248-5

R.T.: 5.716 min
Delta R.T.: -0.005 min
Response: 102918865
Conc: 280.19 ng/ml

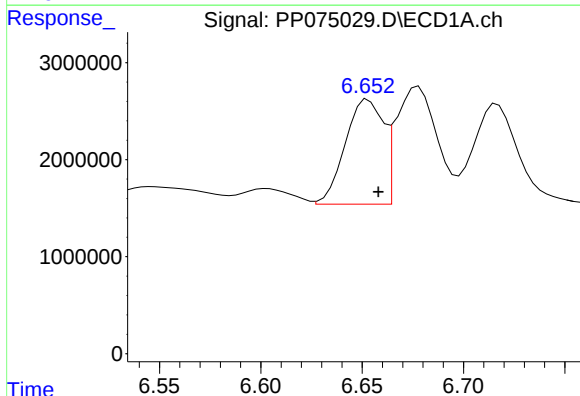


#26 AR-1254-1

R.T.: 6.653 min
Delta R.T.: -0.005 min
Response: 14062671
Conc: 241.34 ng/ml

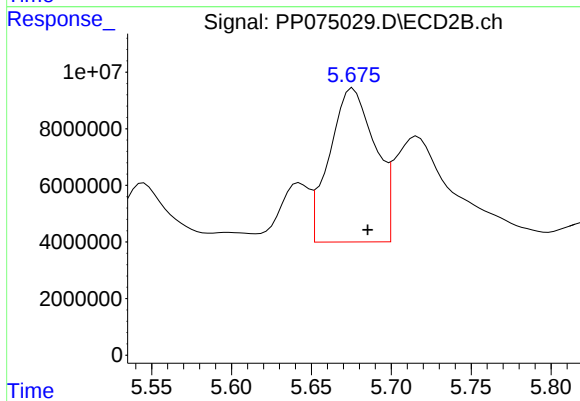

#26 AR-1254-1


R.T.: 5.676 min
Delta R.T.: -0.009 min
Response: 107290309
Conc: 225.06 ng/ml

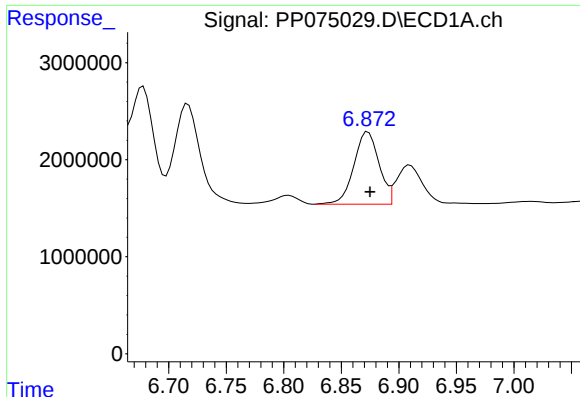

#27 AR-1254-2


R.T.: 6.873 min
Delta R.T.: -0.002 min
Response: 11365007
Conc: 139.25 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

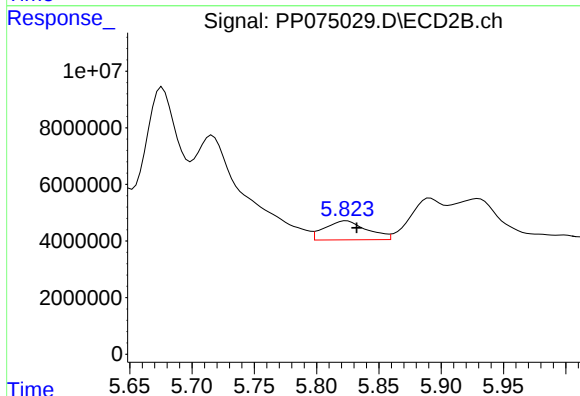


#27 AR-1254-2

R.T.: 5.824 min
Delta R.T.: -0.008 min
Response: 15968662
Conc: 45.35 ng/ml

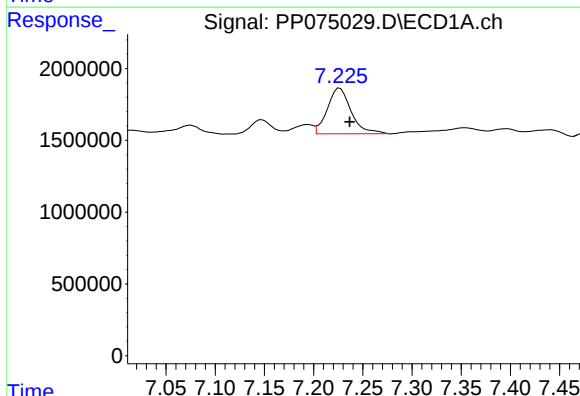


#28 AR-1254-3

R.T.: 7.227 min
Delta R.T.: -0.010 min
Response: 5372805
Conc: 60.23 ng/ml

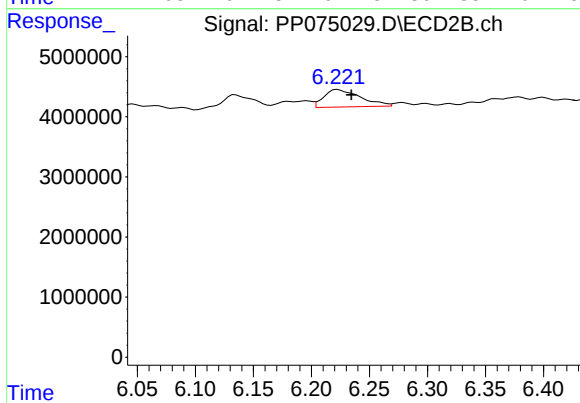

#28 AR-1254-3


R.T.: 6.223 min
Delta R.T.: -0.012 min
Response: 6352189
Conc: 10.25 ng/ml

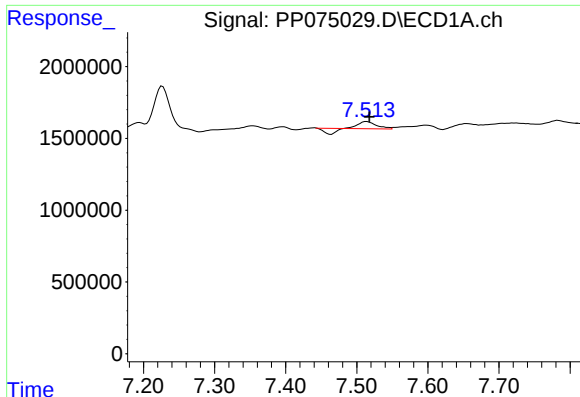

#29 AR-1254-4


R.T.: 7.514 min
Delta R.T.: -0.004 min
Response: 513834
Conc: 7.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

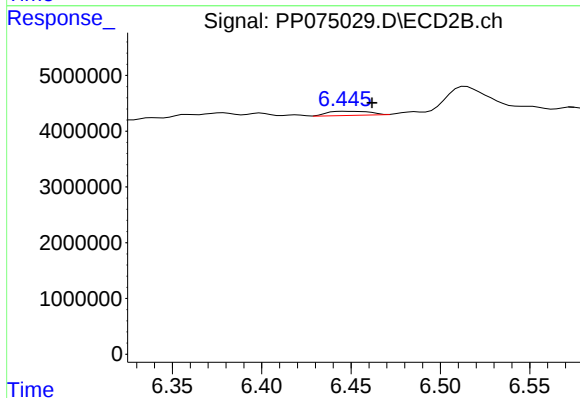


#29 AR-1254-4

R.T.: 6.446 min
Delta R.T.: -0.016 min
Response: 1213325
Conc: 2.59 ng/ml

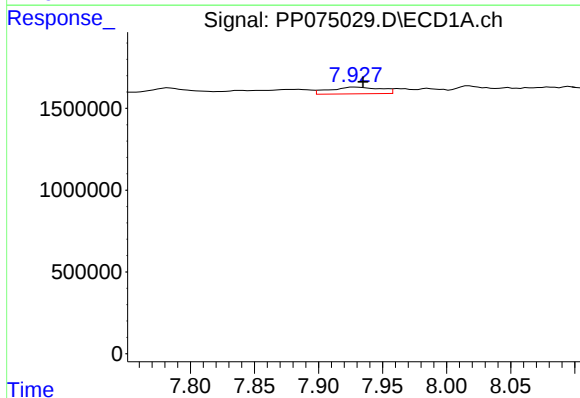


#30 AR-1254-5

R.T.: 7.928 min
Delta R.T.: -0.006 min
Response: 1140239
Conc: 13.72 ng/ml

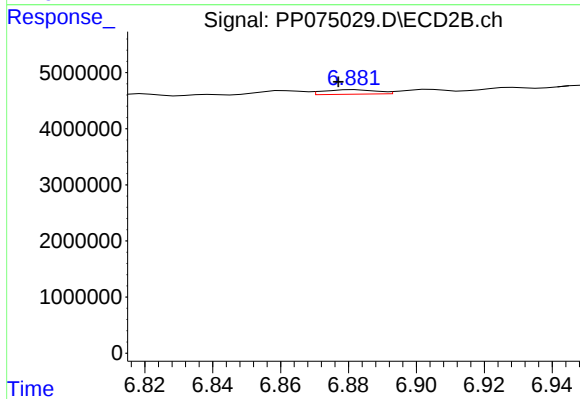

#30 AR-1254-5


R.T.: 6.882 min
Delta R.T.: 0.005 min
Response: 850091
Conc: 1.73 ng/ml

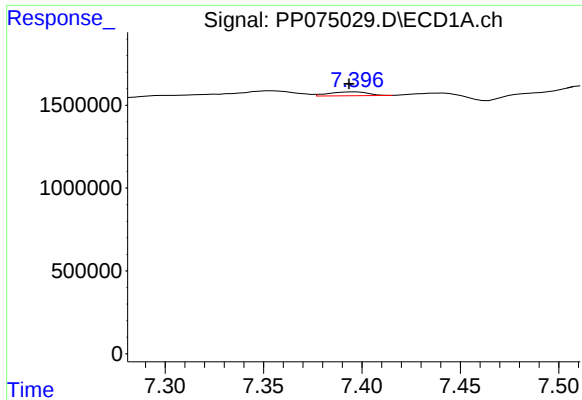

#31 AR-1260-1


R.T.: 7.397 min
Delta R.T.: 0.004 min
Response: 315792
Conc: 5.46 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

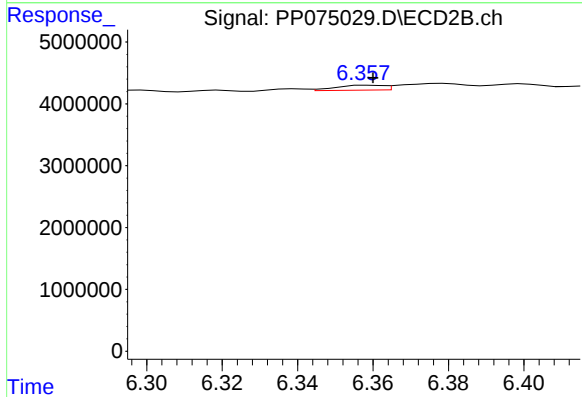


#31 AR-1260-1

R.T.: 6.359 min
Delta R.T.: 0.000 min
Response: 694969
Conc: 1.85 ng/ml

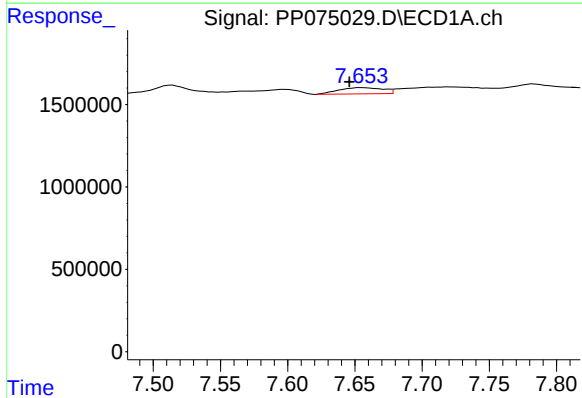


#32 AR-1260-2

R.T.: 7.655 min
Delta R.T.: 0.009 min
Response: 856313
Conc: 12.43 ng/ml

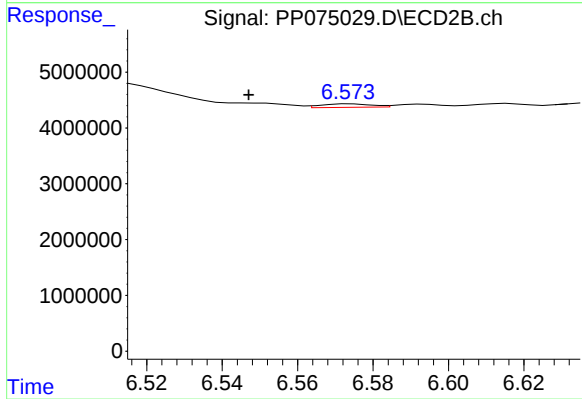

#32 AR-1260-2


R.T.: 6.574 min
Delta R.T.: 0.027 min
Response: 576064
Conc: 1.09 ng/ml

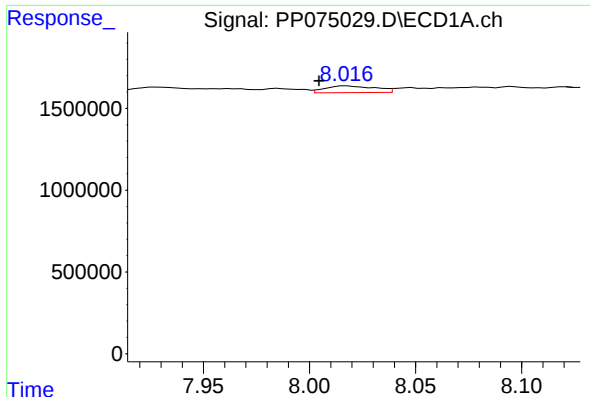

#33 AR-1260-3


R.T.: 8.018 min
Delta R.T.: 0.013 min
Response: 671576
Conc: 12.94 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

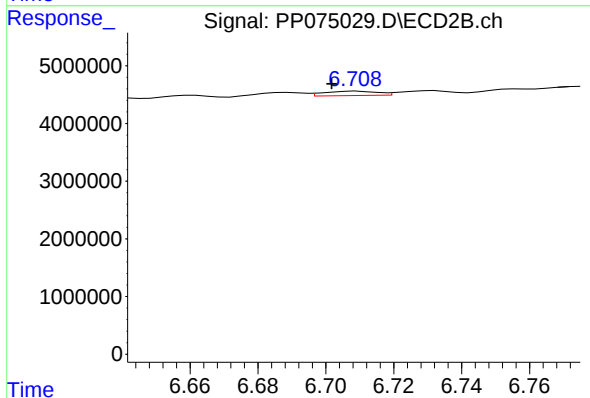


#33 AR-1260-3

R.T.: 6.709 min
Delta R.T.: 0.007 min
Response: 809941
Conc: 1.87 ng/ml

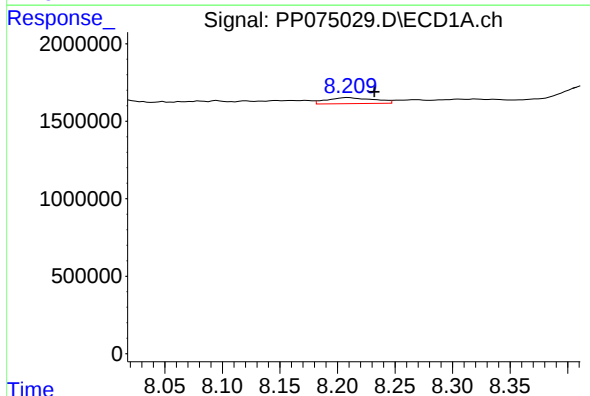


#34 AR-1260-4

R.T.: 8.210 min
Delta R.T.: -0.022 min
Response: 1120009
Conc: 17.56 ng/ml

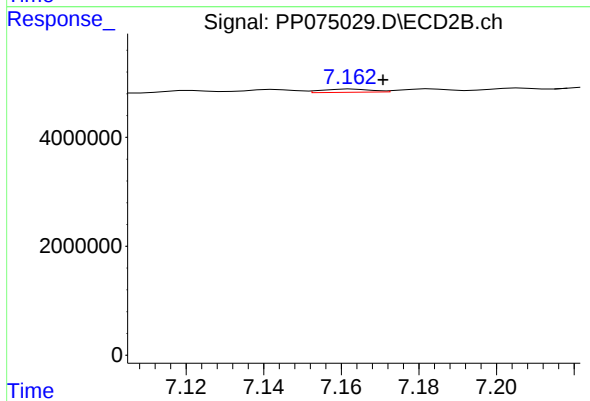

#34 AR-1260-4


R.T.: 7.163 min
Delta R.T.: -0.008 min
Response: 514679
Conc: 1.35 ng/ml

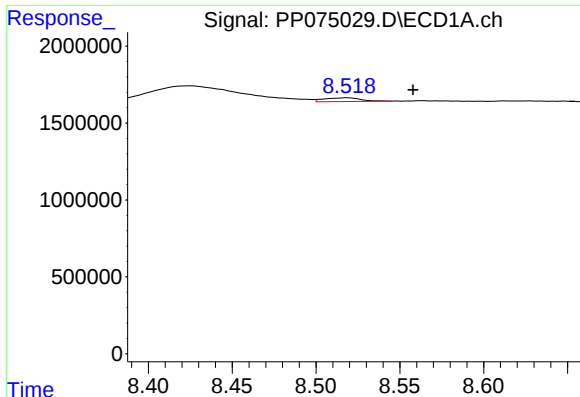

#35 AR-1260-5


R.T.: 8.520 min
Delta R.T.: -0.038 min
Response: 374607
Conc: 3.30 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

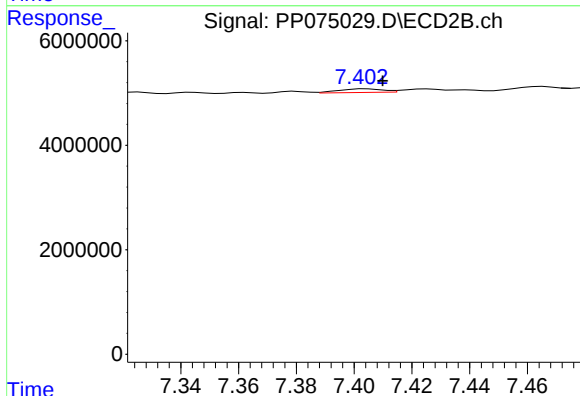


#35 AR-1260-5

R.T.: 7.404 min
Delta R.T.: -0.006 min
Response: 738724
Conc: 0.74 ng/ml

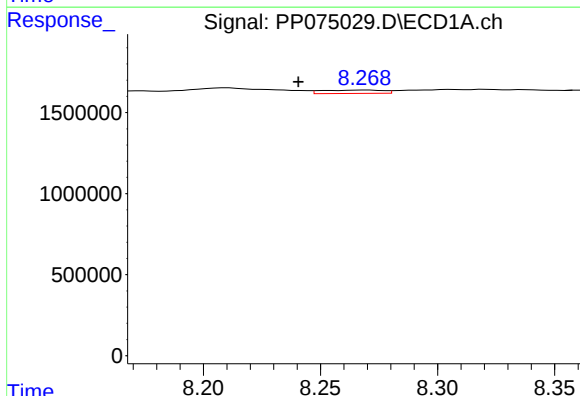


#36 AR-1262-1

R.T.: 8.269 min
Delta R.T.: 0.028 min
Response: 376292
Conc: 4.89 ng/ml

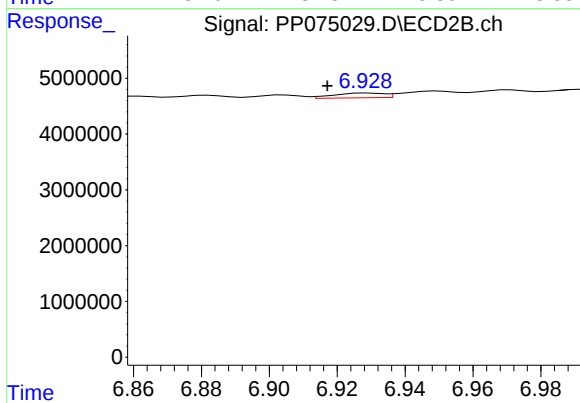

#36 AR-1262-1


R.T.: 6.929 min
Delta R.T.: 0.012 min
Response: 864108
Conc: 1.22 ng/ml

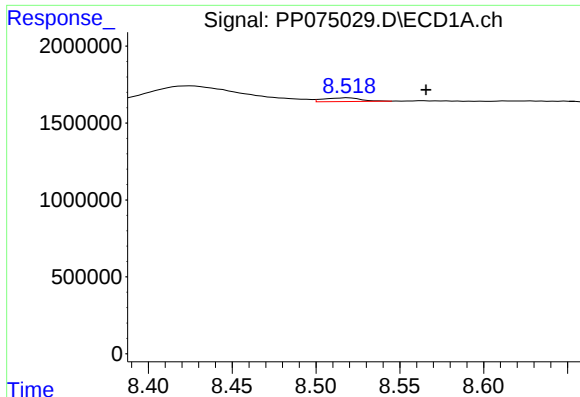

#37 AR-1262-2


R.T.: 8.520 min
Delta R.T.: -0.046 min
Response: 374607
Conc: 2.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

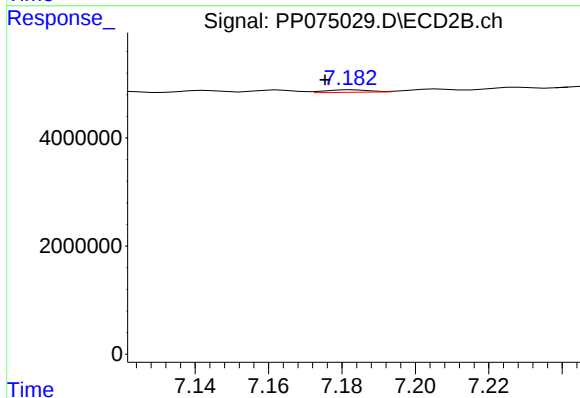


#37 AR-1262-2

R.T.: 7.183 min
Delta R.T.: 0.008 min
Response: 397885
Conc: 0.76 ng/ml

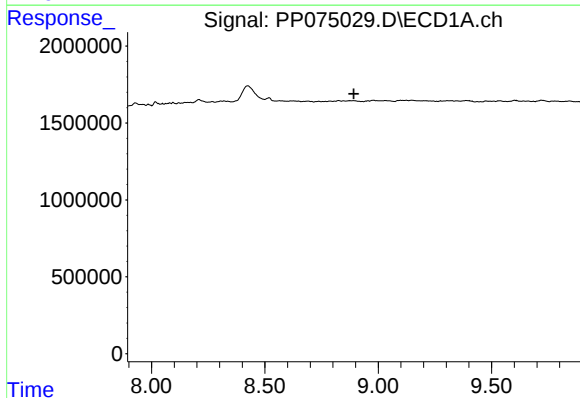


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.892 min
Response: 0
Conc: N.D.

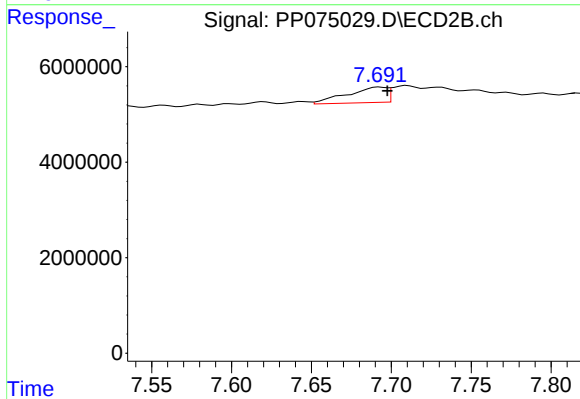

#38 AR-1262-3


R.T.: 7.693 min
Delta R.T.: -0.005 min
Response: 5604793
Conc: 12.02 ng/ml

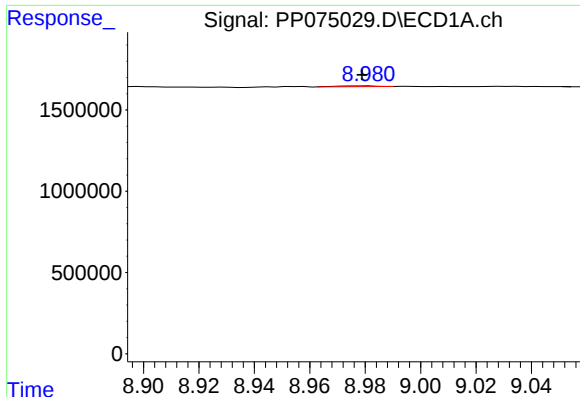

#39 AR-1262-4


R.T.: 8.981 min
Delta R.T.: 0.002 min
Response: 48092
Conc: 0.64 ng/ml

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

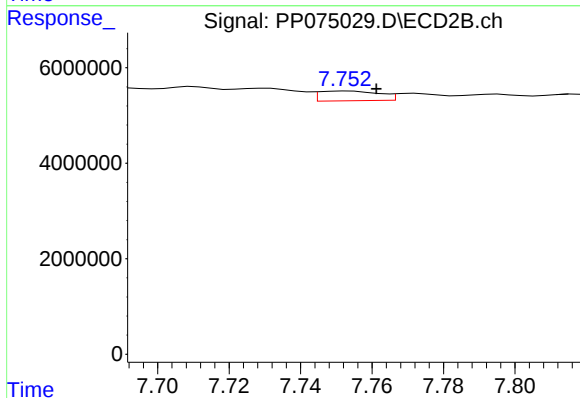


#39 AR-1262-4

R.T.: 7.753 min
Delta R.T.: -0.008 min
Response: 2383545
Conc: 2.90 ng/ml

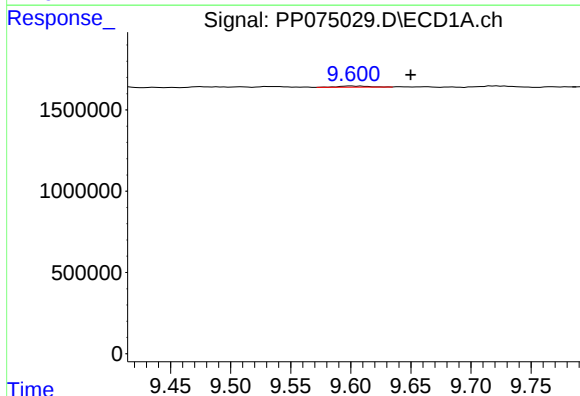


#40 AR-1262-5

R.T.: 9.601 min
Delta R.T.: -0.049 min
Response: 117051
Conc: 1.92 ng/ml

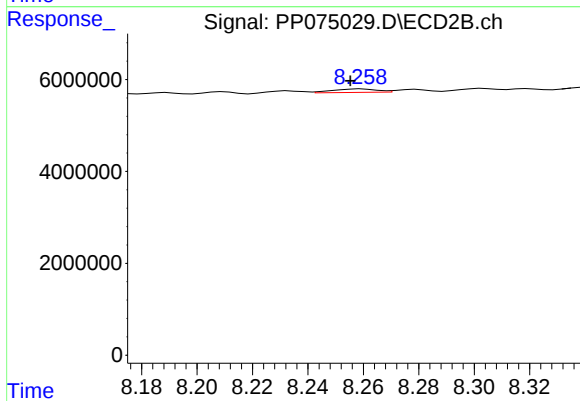

#40 AR-1262-5


R.T.: 8.259 min
Delta R.T.: 0.004 min
Response: 843103
Conc: 2.35 ng/ml

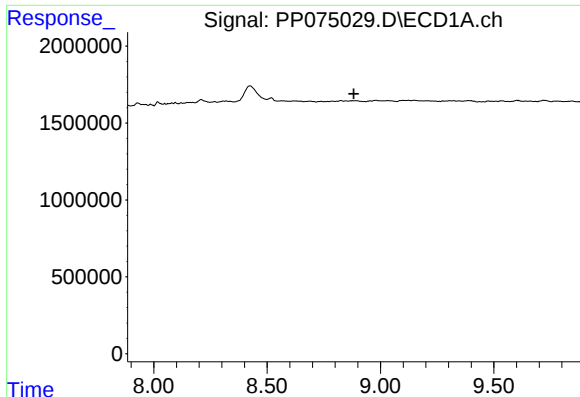

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 8.883 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

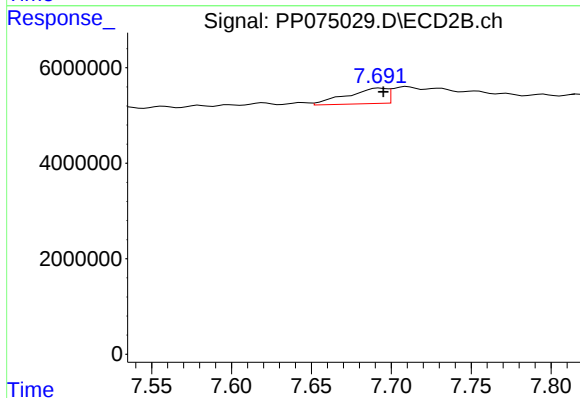


#41 AR-1268-1

R.T.: 7.693 min
Delta R.T.: -0.002 min
Response: 5604793
Conc: 3.97 ng/ml

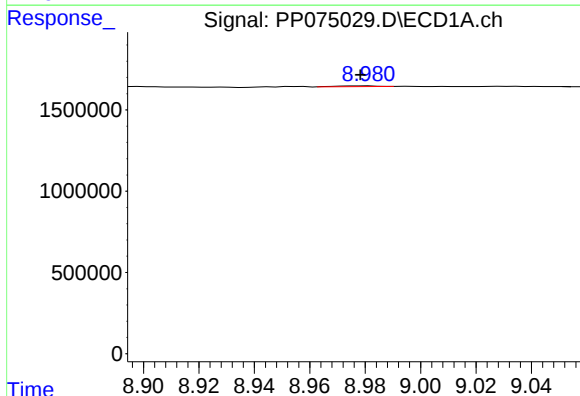


#42 AR-1268-2

R.T.: 8.981 min
Delta R.T.: 0.003 min
Response: 48092
Conc: 0.33 ng/ml

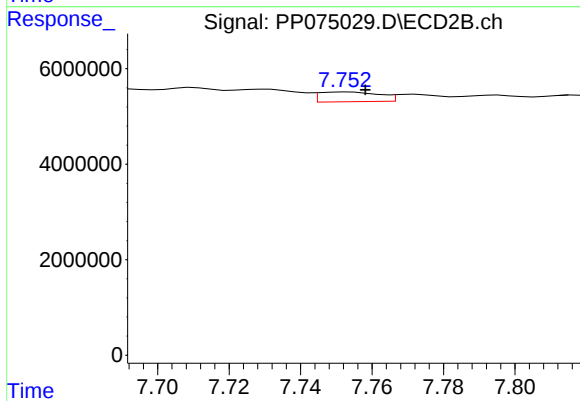

#42 AR-1268-2


R.T.: 7.753 min
Delta R.T.: -0.005 min
Response: 2383545
Conc: 1.75 ng/ml

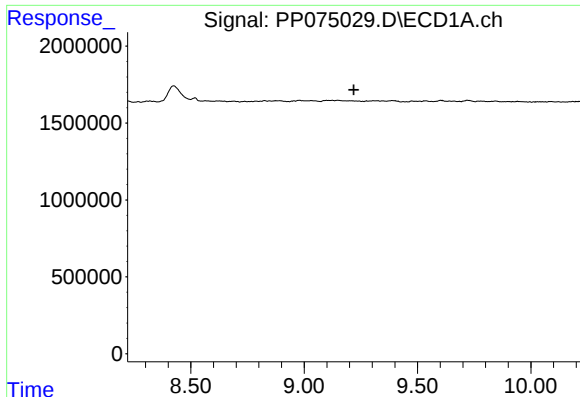

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.219 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

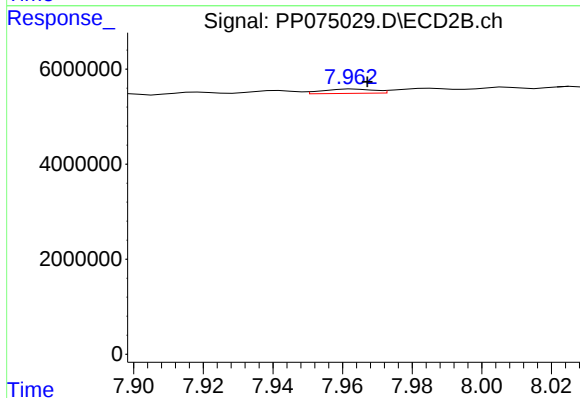


#43 AR-1268-3

R.T.: 7.963 min
Delta R.T.: -0.004 min
Response: 931362
Conc: 0.89 ng/ml

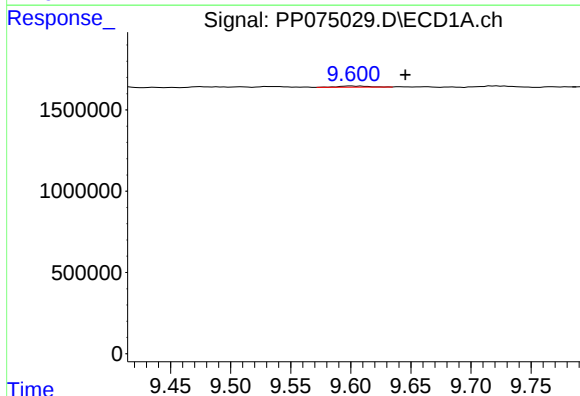


#44 AR-1268-4

R.T.: 9.601 min
Delta R.T.: -0.044 min
Response: 117051
Conc: 1.74 ng/ml

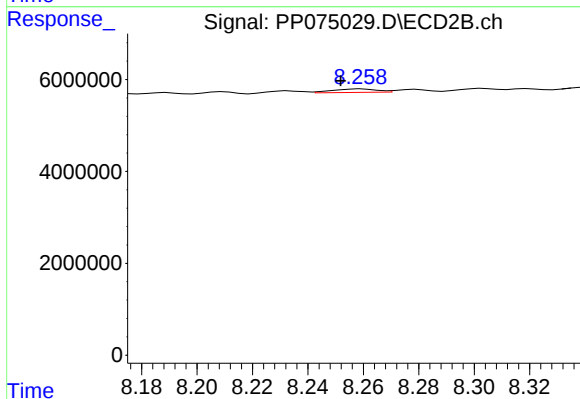

#44 AR-1268-4


R.T.: 8.259 min
Delta R.T.: 0.008 min
Response: 843103
Conc: 2.20 ng/ml

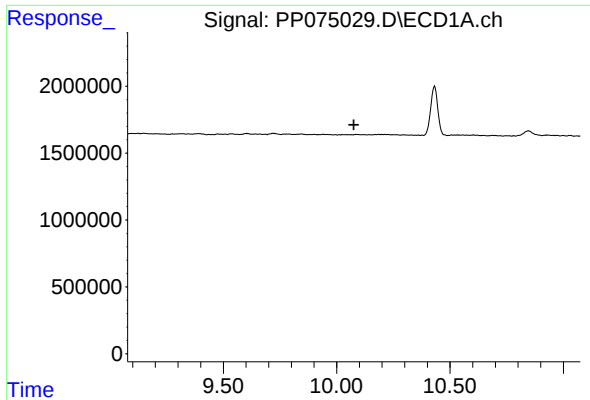

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PASSAIC-HDL

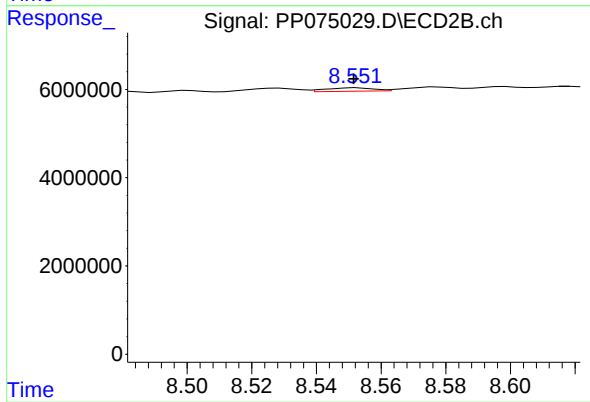

#45 AR-1268-5

R.T.: 8.552 min
Delta R.T.: 0.000 min
Response: 801283
Conc: 0.26 ng/ml