

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
 Data File : PP075048.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 16:41
 Operator : YP\AJ
 Sample : Q3048-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 VNJ-258

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2025
 Supervised By :mohammad ahmed 09/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:33:47 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.654	3.800	23240250	88753908	18.992	18.355
2) SA Decachlor...	10.427	8.805	15548125	81843556	15.745m	10.914 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
Data File : PP075048.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 16:41
Operator : YP\AJ
Sample : Q3048-01
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
VNJ-258


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:33:47 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

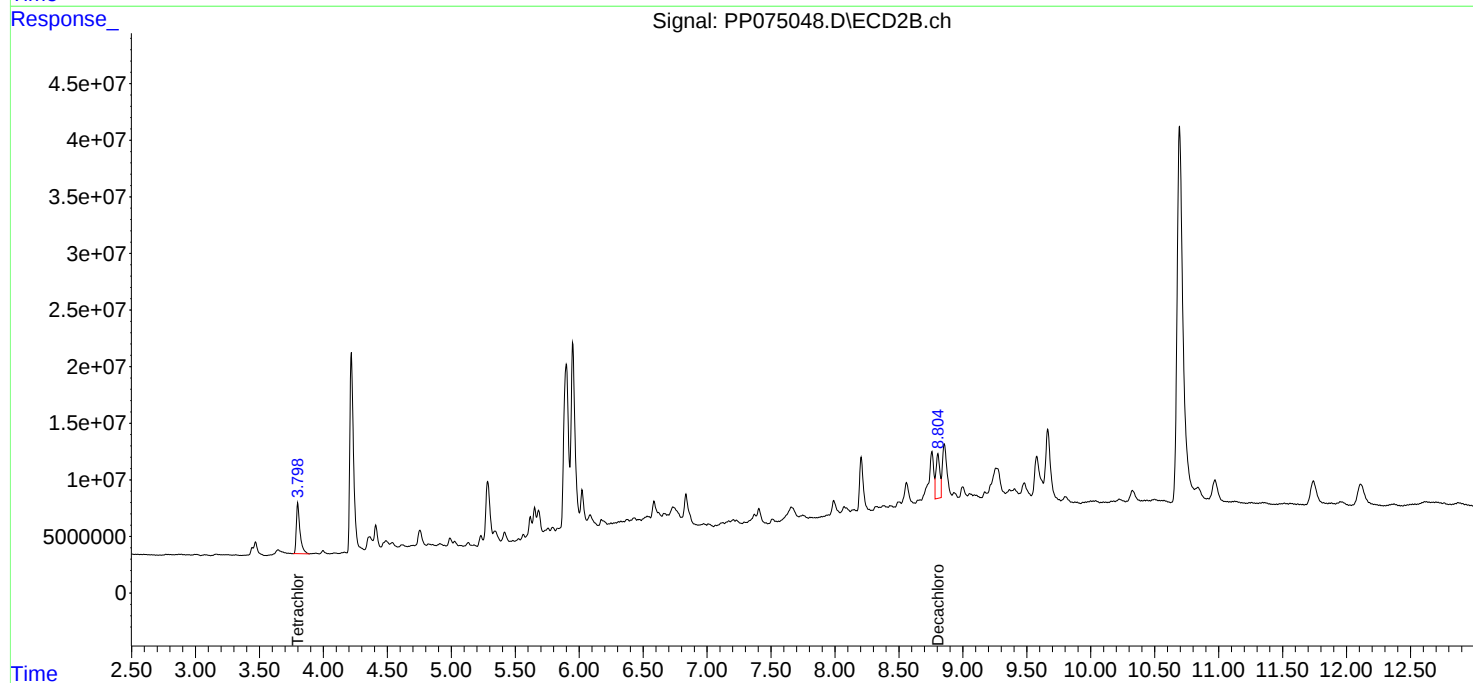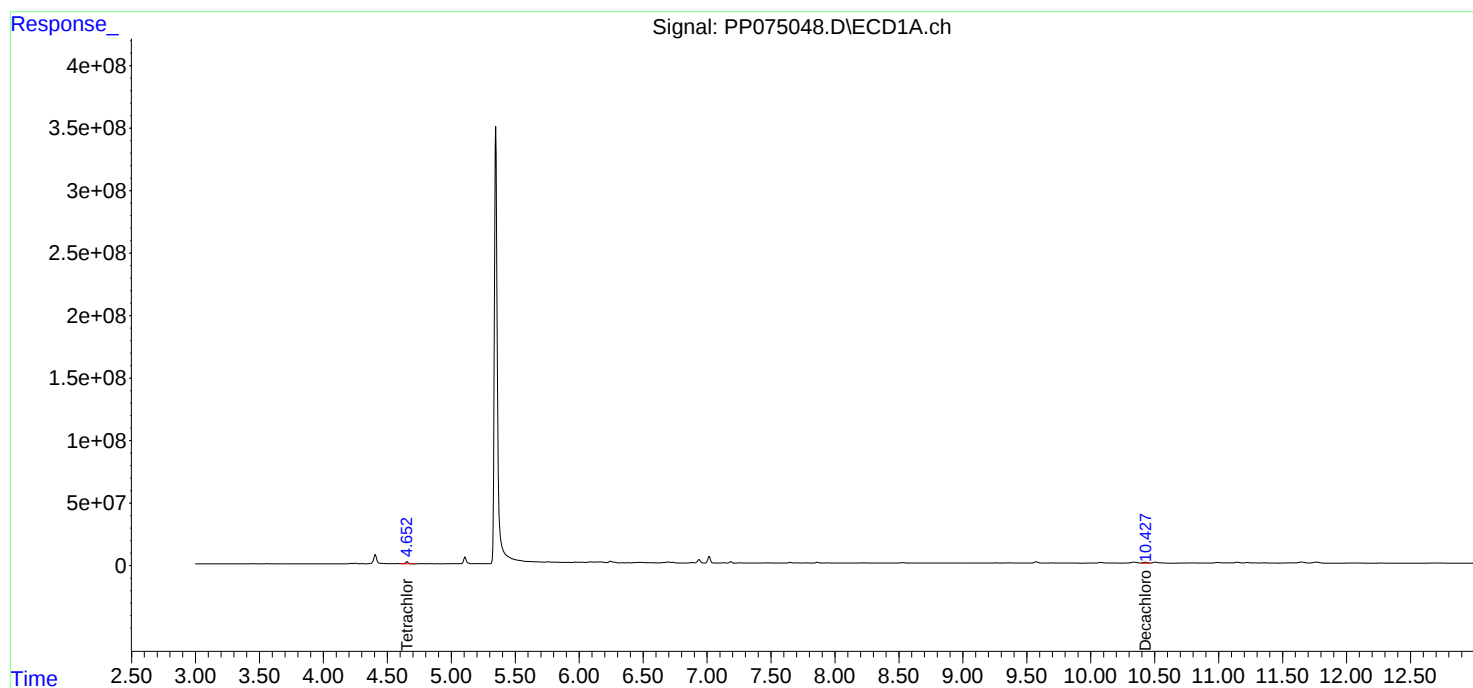

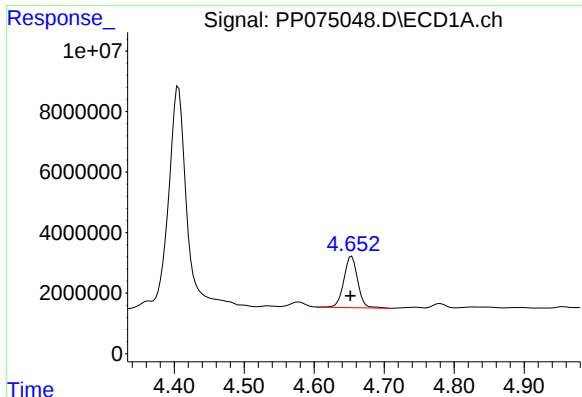


#1 Tetrachloro-m-xylene

R.T.: 4.654 min
Delta R.T.: 0.002 min
Response: 23240250
Conc: 18.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
VNJ-258


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/12/2025

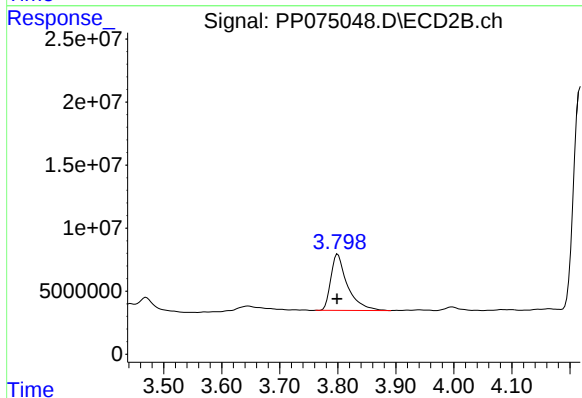


#1 Tetrachloro-m-xylene

R.T.: 3.800 min
Delta R.T.: 0.001 min
Response: 88753908
Conc: 18.35 ng/ml

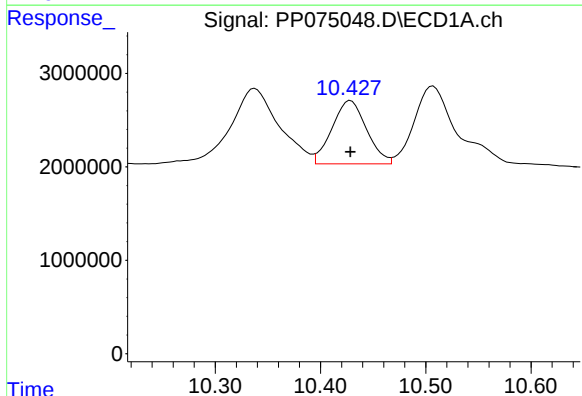

#2 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 15548125
Conc: 15.74 ng/ml m

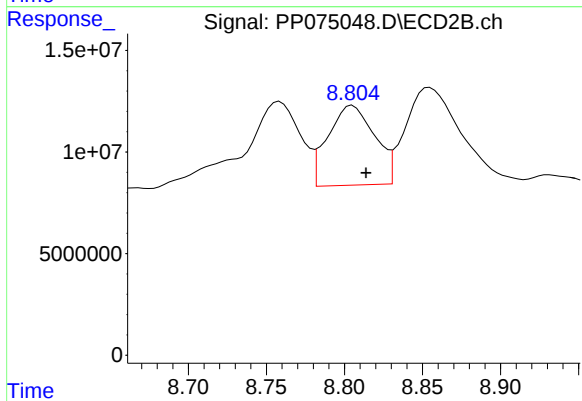

#2 Decachlorobiphenyl

R.T.: 8.805 min
Delta R.T.: -0.009 min
Response: 81843556
Conc: 10.91 ng/ml