

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
 Data File : PP075051.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Sep 2025 17:30
 Operator : YP\AJ
 Sample : Q3050-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 72-11939

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/11/2025
 Supervised By :mohammad ahmed 09/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 11 05:34:31 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.657	3.797	18802325	64273565	15.365	13.292m
2) SA Decachlor...	10.430	8.806	13149788	82613786	13.316	11.016

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091025\
Data File : PP075051.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Sep 2025 17:30
Operator : YP\AJ
Sample : Q3050-01
Misc :
ALS Vial : 24 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
72-11939


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 11 05:34:31 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

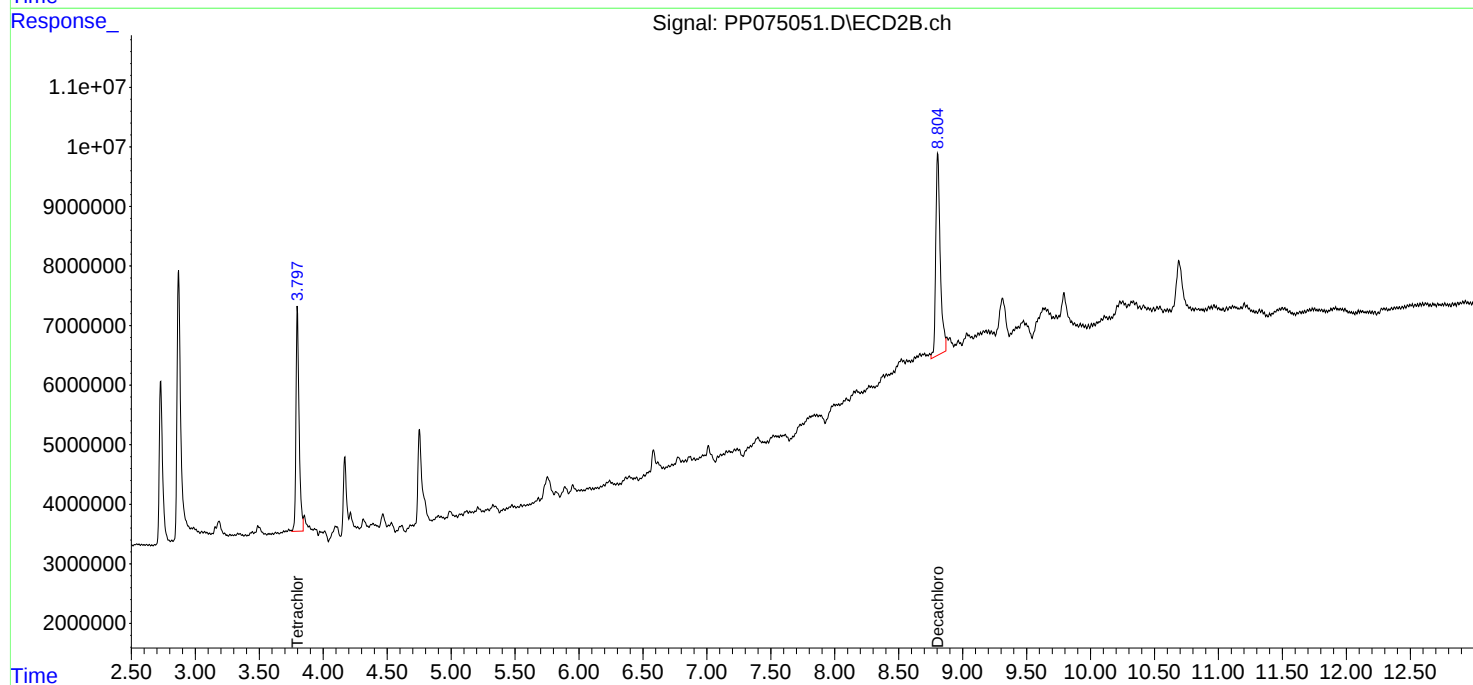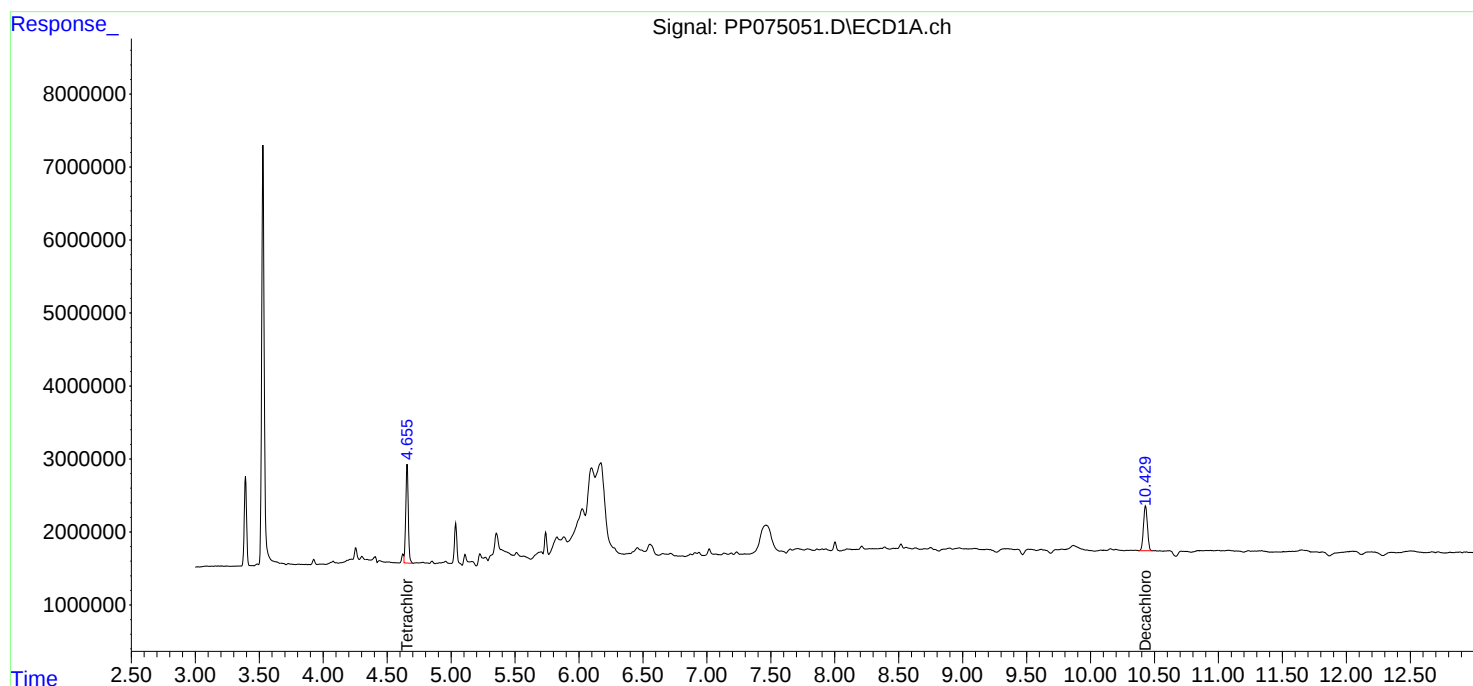

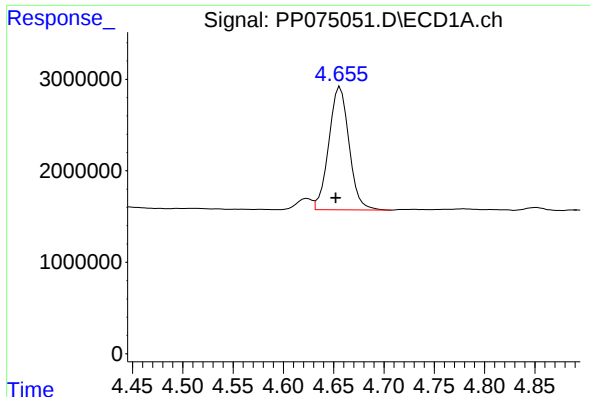


#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.005 min
Response: 18802325
Conc: 15.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
72-11939


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/11/2025
Supervised By :mohammad ahmed 09/12/2025

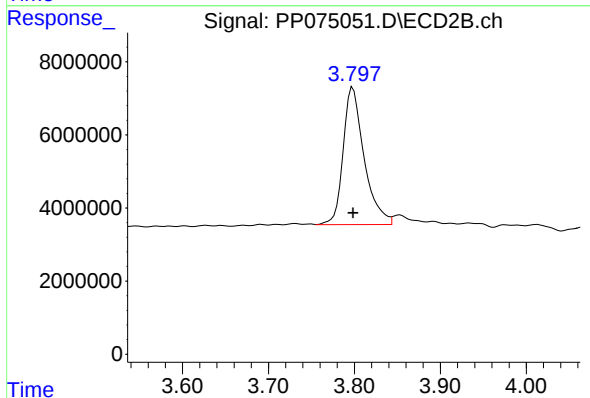


#1 Tetrachloro-m-xylene

R.T.: 3.797 min
Delta R.T.: -0.002 min
Response: 64273565
Conc: 13.29 ng/ml m

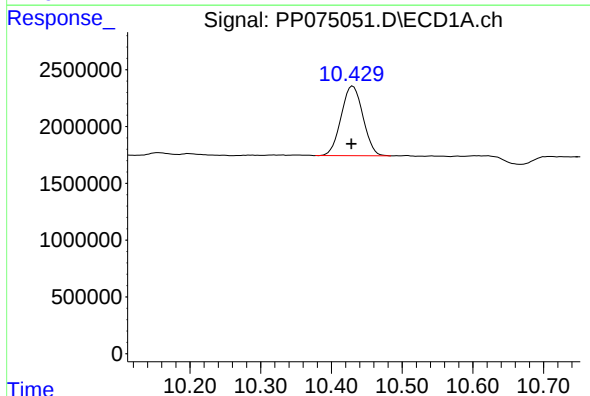

#2 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: 0.002 min
Response: 13149788
Conc: 13.32 ng/ml

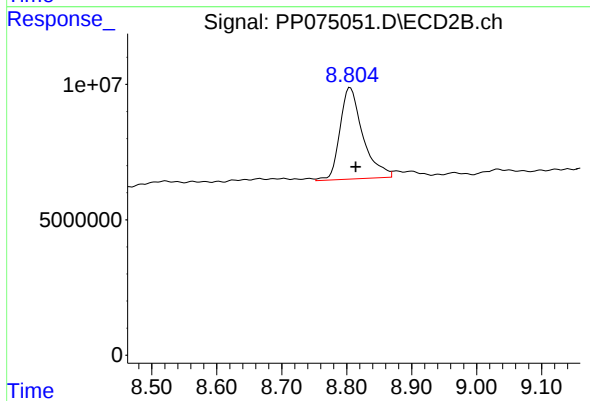

#2 Decachlorobiphenyl

R.T.: 8.806 min
Delta R.T.: -0.008 min
Response: 82613786
Conc: 11.02 ng/ml