

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091123\
 Data File : PP059850.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Sep 2023 03:49
 Operator : YP\AJ
 Sample : 04343-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SAMPLE-2-23RD-ST

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 04:43:43 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 12 04:36:26 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.380	3.605	26744523	37835340	17.212	17.064
2) SA Decachlor...	10.151	8.618	18862103	25188442	15.437	13.809

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091123\
Data File : PP059850.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Sep 2023 03:49
Operator : YP\AJ
Sample : 04343-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-23RD-ST

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 04:43:43 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091123.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 12 04:36:26 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

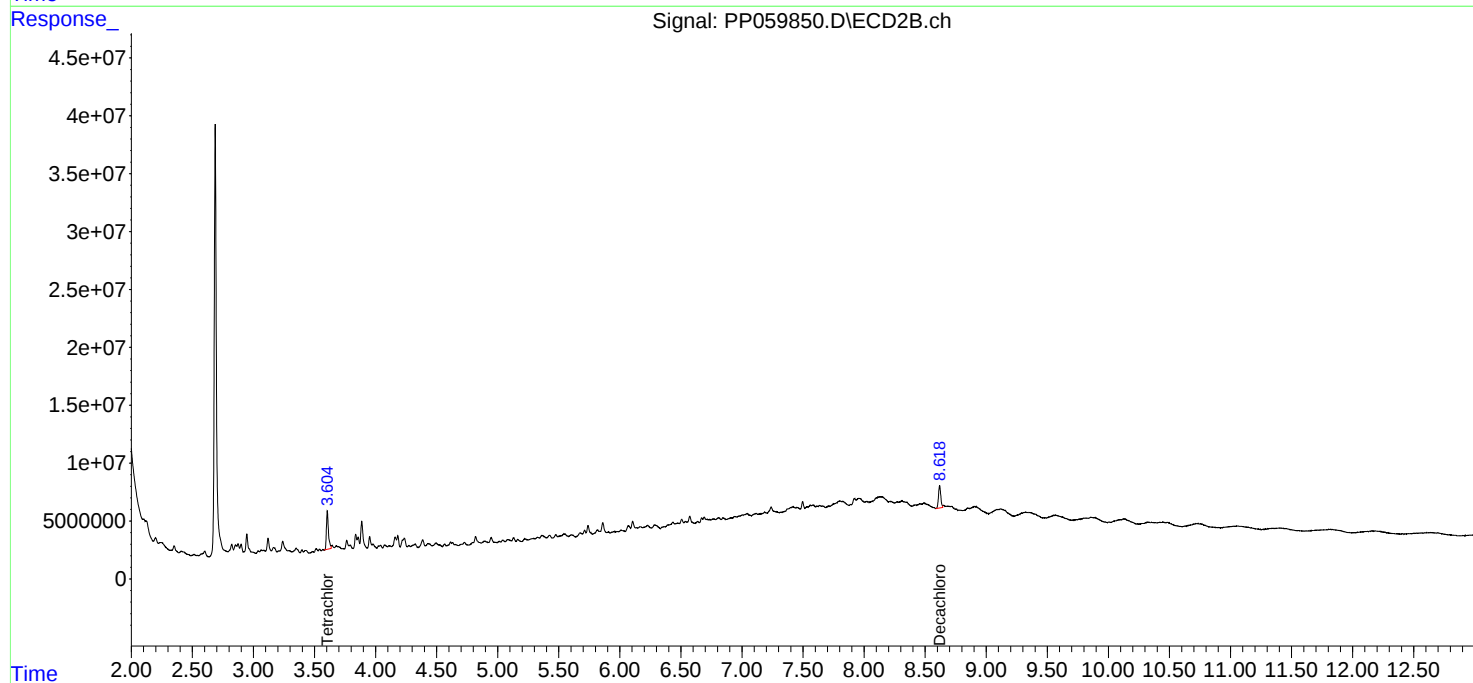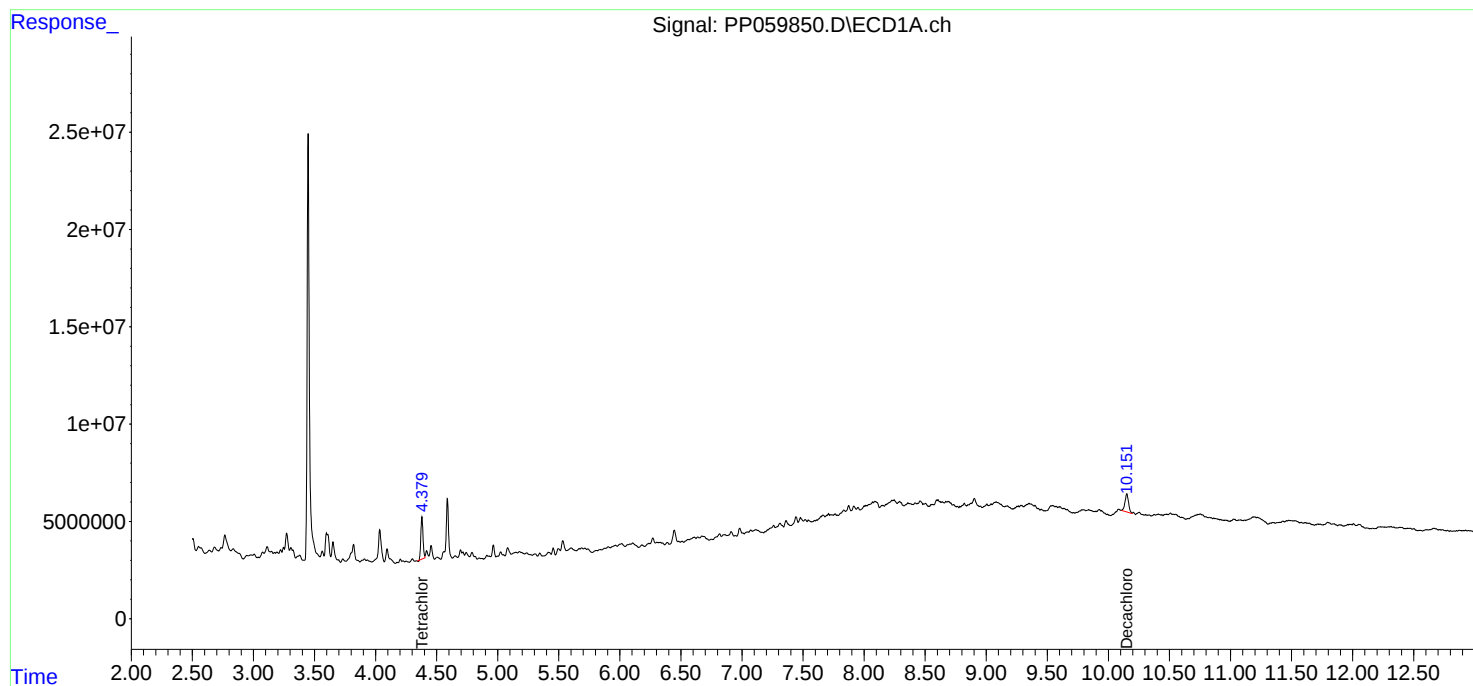


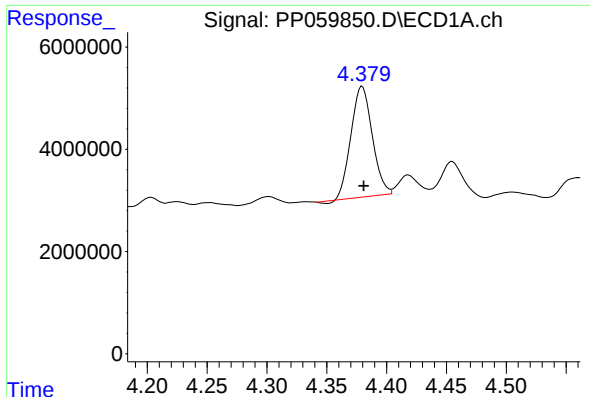

#1 Tetrachloro-m-xylene


R.T.: 4.380 min
Delta R.T.: -0.001 min
Response: 26744523
Conc: 17.21 ng/ml

Instrument :
ECD_P
ClientSampleId :
SAMPLE-2-23RD-ST

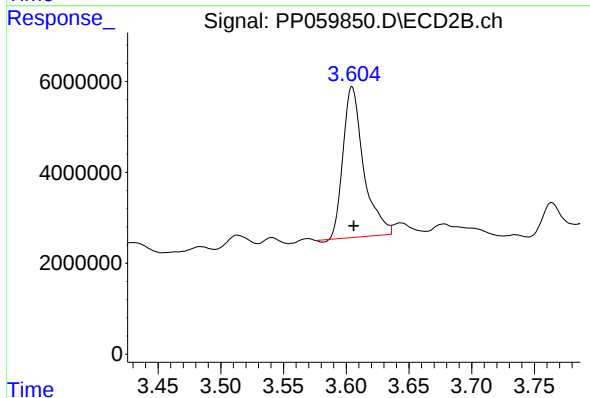


#1 Tetrachloro-m-xylene

R.T.: 3.605 min
Delta R.T.: -0.001 min
Response: 37835340
Conc: 17.06 ng/ml

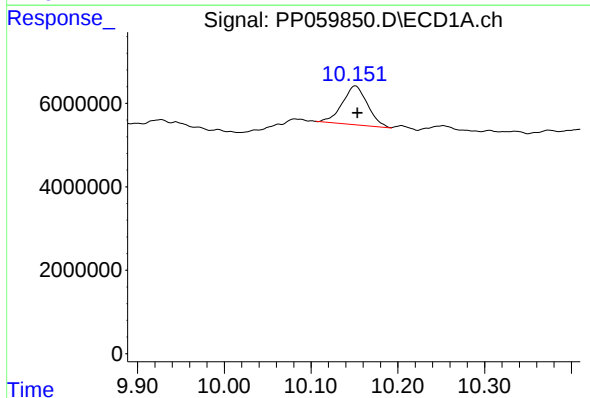

#2 Decachlorobiphenyl

R.T.: 10.151 min
Delta R.T.: -0.002 min
Response: 18862103
Conc: 15.44 ng/ml

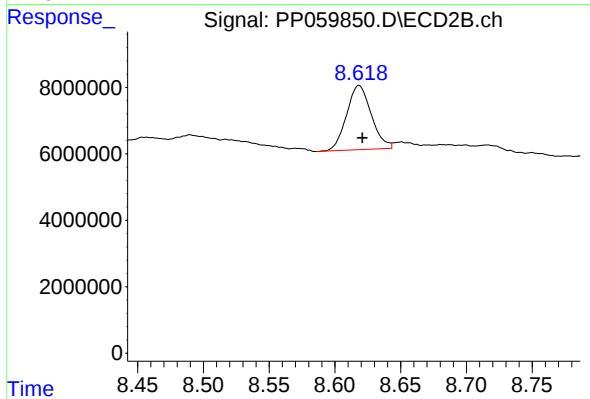

#2 Decachlorobiphenyl

R.T.: 8.618 min
Delta R.T.: -0.003 min
Response: 25188442
Conc: 13.81 ng/ml