

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091125\
 Data File : PP075080.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Sep 2025 18:00
 Operator : YP\AJ
 Sample : Q3074-01 10X
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-25-0141

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/12/2025
 Supervised By :mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 12 01:31:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Aug 20 06:20:44 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.657	3.794	3081352	6950814	2.518	1.437m#
2) SA Decachlor...	10.431	8.800	2292528	11117422	2.322m	1.482m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091125\
Data File : PP075080.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Sep 2025 18:00
Operator : YP\AJ
Sample : Q3074-01 10X
Misc :
ALS Vial : 17 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
MOO-25-0141


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2025
Supervised By :mohammad ahmed 09/15/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 12 01:31:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP081925.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Aug 20 06:20:44 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

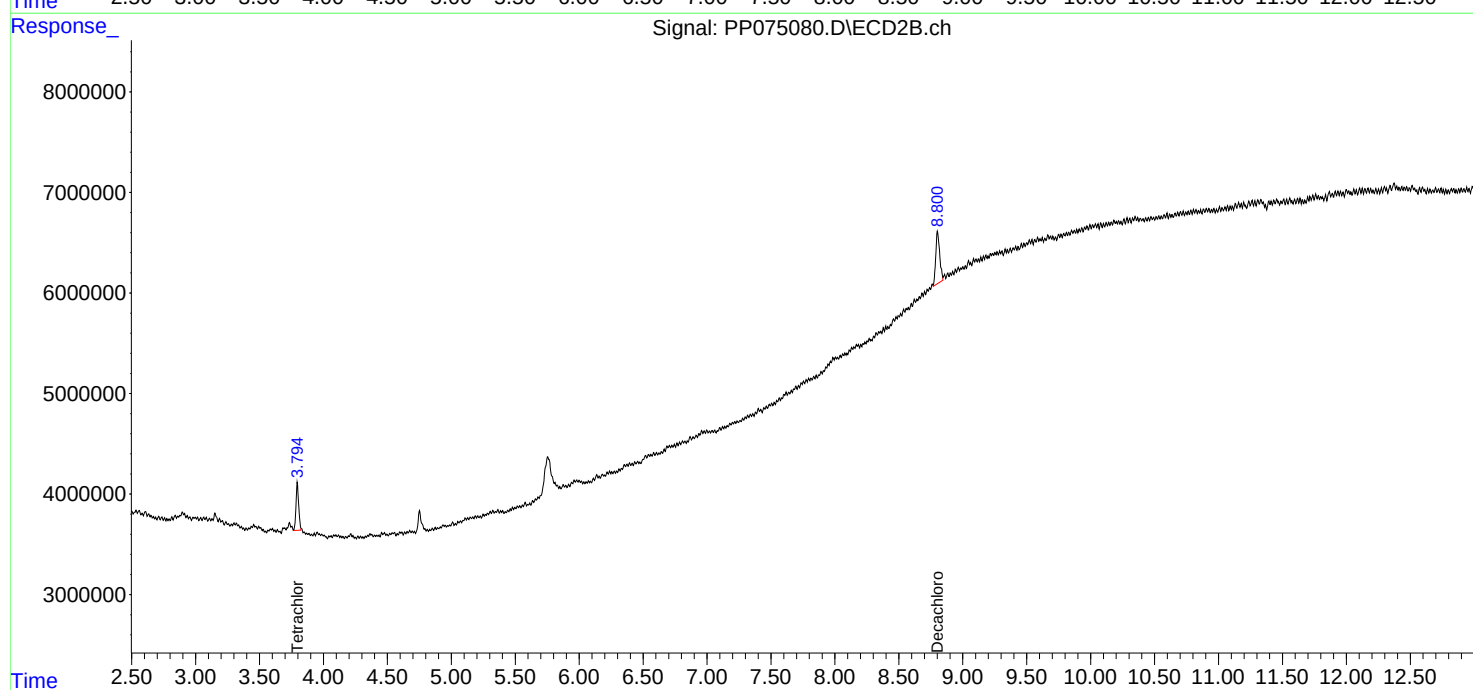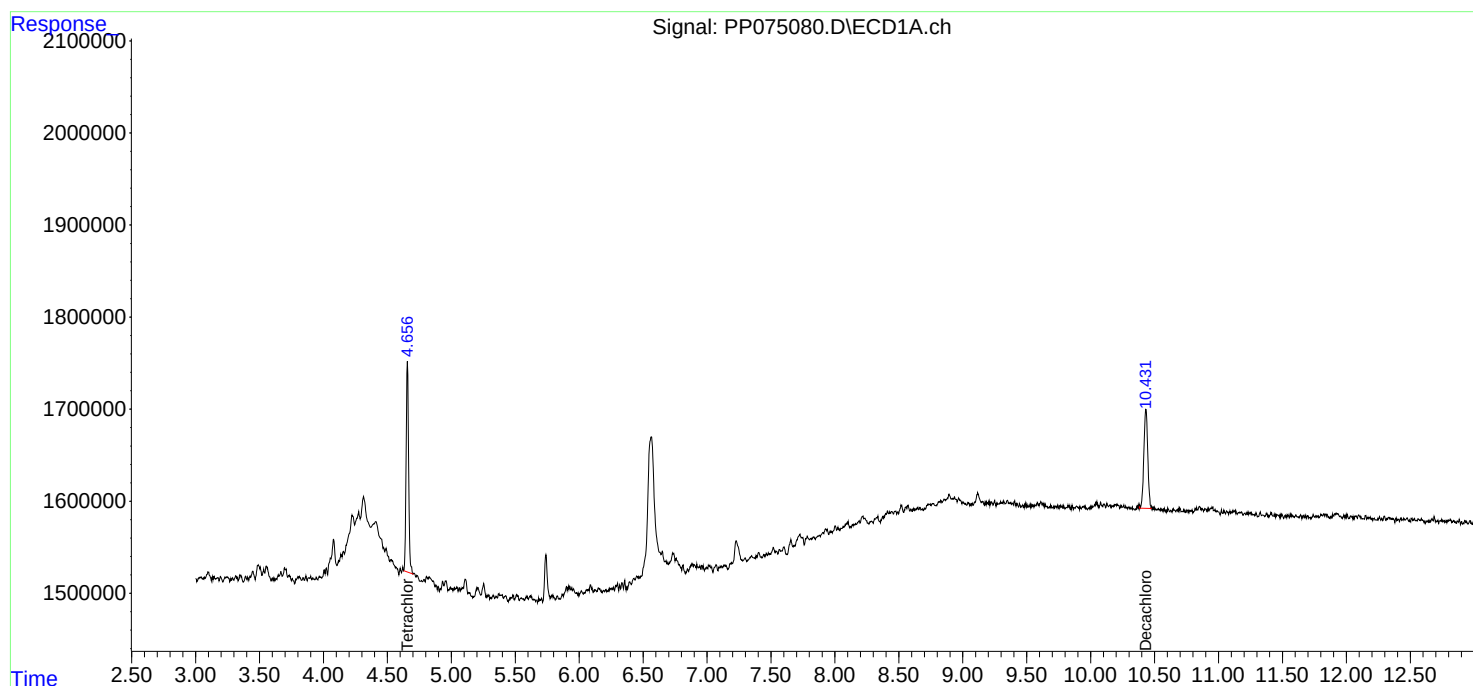

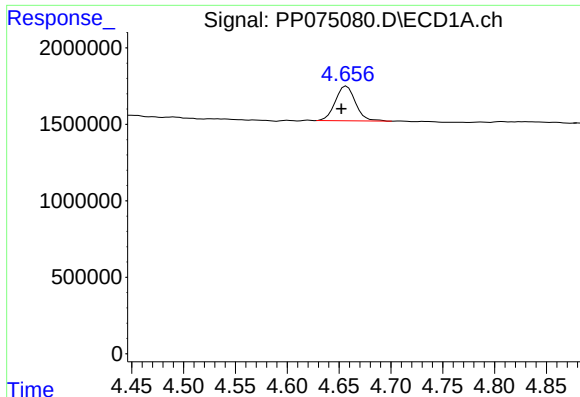


#1 Tetrachloro-m-xylene

R.T.: 4.657 min
Delta R.T.: 0.005 min
Response: 3081352
Conc: 2.52 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-25-0141


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/12/2025
Supervised By :mohammad ahmed 09/15/2025

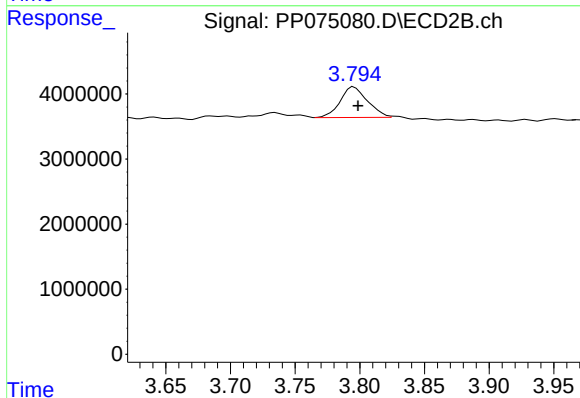


#1 Tetrachloro-m-xylene

R.T.: 3.794 min
Delta R.T.: -0.005 min
Response: 6950814
Conc: 1.44 ng/ml m

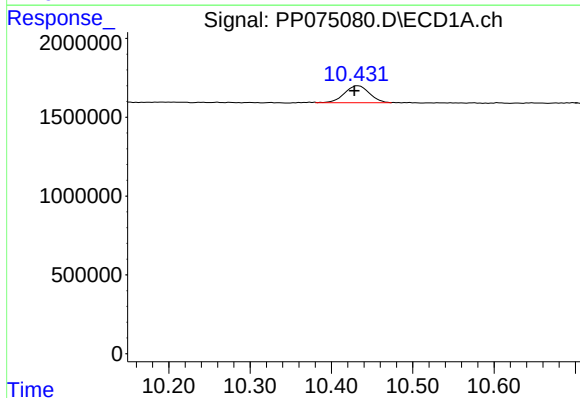

#2 Decachlorobiphenyl

R.T.: 10.431 min
Delta R.T.: 0.003 min
Response: 2292528
Conc: 2.32 ng/ml m

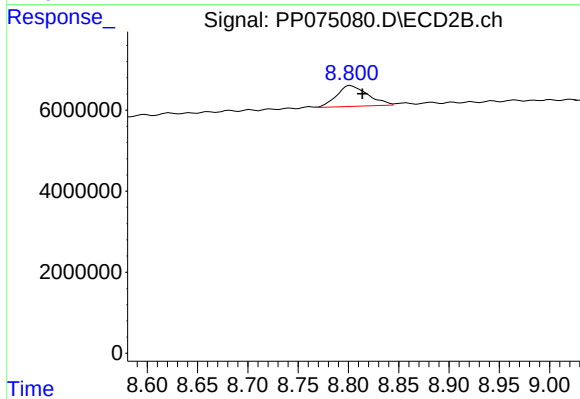

#2 Decachlorobiphenyl

R.T.: 8.800 min
Delta R.T.: -0.014 min
Response: 11117422
Conc: 1.48 ng/ml m