

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091625\
 Data File : PP075188.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2025 22:58
 Operator : YP\AJ
 Sample : DDT ANALOG
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 DDT ANALOG

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:41:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 16 19:36:38 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.682f	3.791	732089	303010	0.569	0.054 #
2)	SA Decachlor...	10.421	8.800	580517	1329090	0.506	0.164 #
Target Compounds							
3)	L1 AR-1016-1	5.736f	4.893	1159449	1392021	24.158	2.544 #
4)	L1 AR-1016-2	0.000	4.948	0	1833152	N.D.	6.753 #
5)	L1 AR-1016-3	5.899	5.070	1514629	1816854	31.990	12.971 #
6)	L1 AR-1016-4	5.936f	5.086	1504180	1884628	42.495	13.325 #
7)	L1 AR-1016-5	6.249	5.345	605655	6674187	16.704	42.177 #
8)	L2 AR-1221-1	4.842	4.001	282180	478824	14.971	6.232 #
9)	L2 AR-1221-2	4.956	4.088	384057	796980	26.878	14.575 #
10)	L2 AR-1221-3	4.956f	4.155	384057	315634	9.205	1.627 #
11)	L3 AR-1232-1	4.956f	4.155	384057	315634	10.088	2.160 #
12)	L3 AR-1232-2	0.000	4.893	0	1392021	N.D.	5.551 #
13)	L3 AR-1232-3	0.000	5.070	0	1816854	N.D.	29.218 #
14)	L3 AR-1232-4	5.936f	5.140	1504180	4909681	82.422	69.095
15)	L3 AR-1232-5	6.057	5.345	661359	6674187	50.510	105.509 #
16)	L4 AR-1242-1	5.736f	4.893	1159449	1392021	28.397	3.002 #
17)	L4 AR-1242-2	0.000	4.948	0	1833152	N.D.	8.530 #
18)	L4 AR-1242-3	5.899	5.070	1514629	1816854	35.885	15.276 #
19)	L4 AR-1242-4	5.936f	5.160	1504180	3185884	45.603	20.758 #
20)	L4 AR-1242-5	6.745	5.691	2684201	22135419	73.089	113.679 #
21)	L5 AR-1248-1	0.000	4.893	0	1392021	N.D.	4.632 #
22)	L5 AR-1248-2	6.095	5.086	712768	1884628	15.784	9.423 #
23)	L5 AR-1248-3	6.299	5.140	1036799	4909681	20.974	20.577
24)	L5 AR-1248-4	6.648	5.345	4811206	6674187	80.074	28.502 #
25)	L5 AR-1248-5	6.745	5.691	2684201	22135419	44.948	56.506 #
26)	L6 AR-1254-1	6.648	5.691	4811206	22135419	73.545	40.695 #
27)	L6 AR-1254-2	6.860	5.837	4242169	13233540	49.800	36.327 #
28)	L6 AR-1254-3	7.222	6.230	9444068	42740551	99.253	72.450 #
29)	L6 AR-1254-4	7.514	6.427	822233	3481592	11.327	7.021 #
30)	L6 AR-1254-5	7.944	6.860	479.8E6	3418.3E6	5859.740	6723.375
31)	L7 AR-1260-1	7.396	6.353	919897	4973359	14.665	11.979
32)	L7 AR-1260-2	7.630	6.535	693.9E6	5842847	9068.055	10.500 #
33)	L7 AR-1260-3	7.944f	0.000	479.8E6	0	8148.485	N.D. #
34)	L7 AR-1260-4	8.244	7.164	188413	257550	2.787	0.650 #
35)	L7 AR-1260-5	0.000	7.405	0	614506	N.D.	0.598 #
36)	L8 AR-1262-1	8.244	6.860f	188413	3418.3E6	2.332	4520.395 #
37)	L8 AR-1262-2	0.000	7.164	0	257550	N.D.	0.467 #
38)	L8 AR-1262-3	8.906	7.706	93155	88089473	0.878	180.934 #
39)	L8 AR-1262-4	9.004	7.706f	96171	88089473	1.152	99.016 #
40)	L8 AR-1262-5	9.682f	8.242	98390	276607	1.638	0.696 #
41)	L9 AR-1268-1	8.860	7.706	481285	88089473	2.683	59.472 #

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091625\
Data File : PP075188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 22:58
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:41:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 19:36:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
42)	L9 AR-1268-2	9.004	7.706f	96171	88089473	0.578	61.159 #
43)	L9 AR-1268-3	0.000	7.957	0	655536	N.D.	0.591 #
44)	L9 AR-1268-4	9.599f	8.242	811619	276607	11.775	0.654 #
45)	L9 AR-1268-5	10.061	8.543	301851	617886	0.715	0.185 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091625\
Data File : PP075188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 22:58
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:41:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 19:36:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

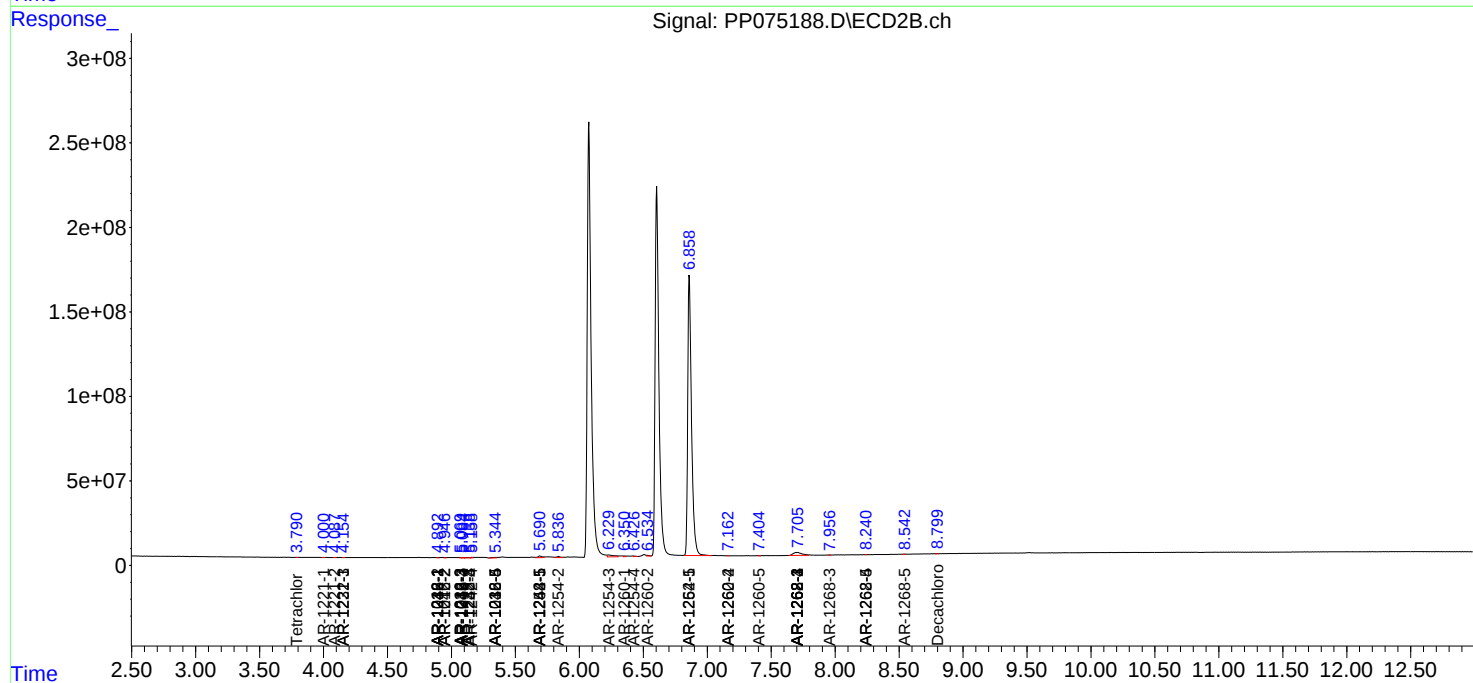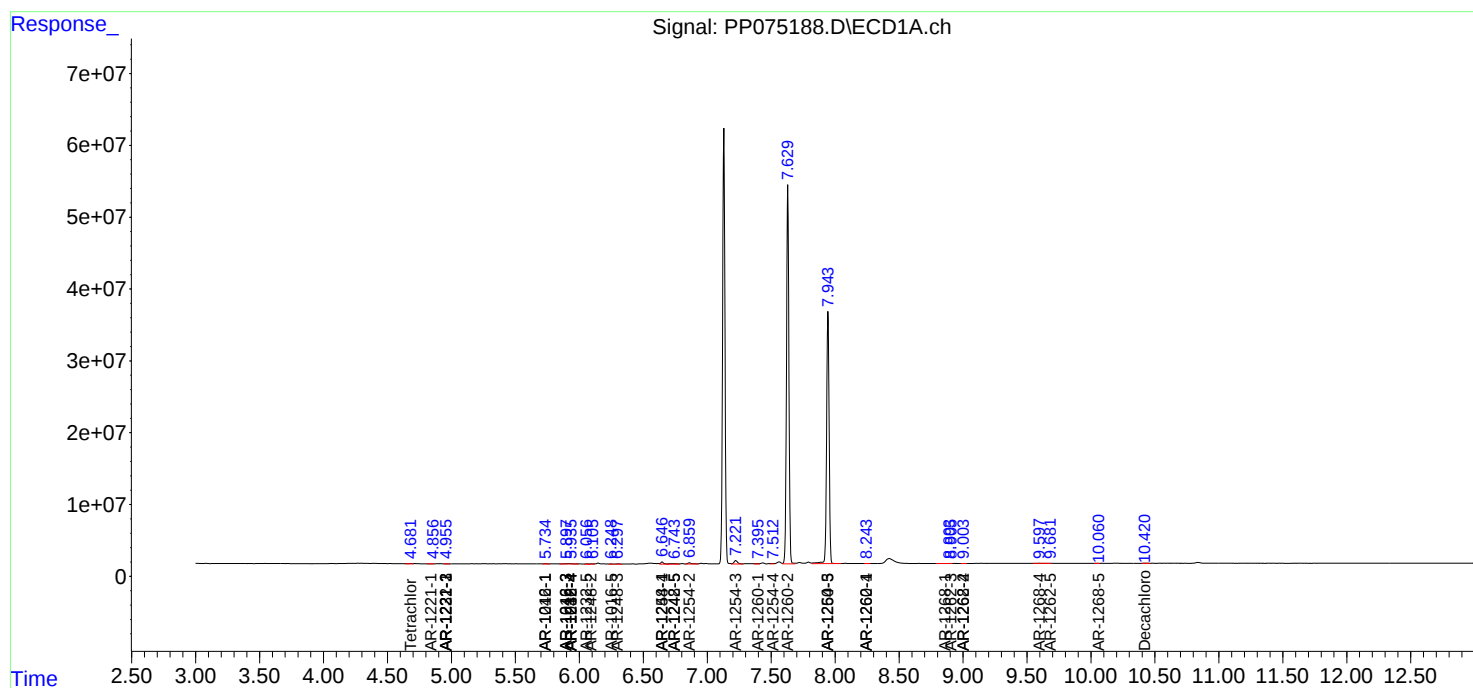


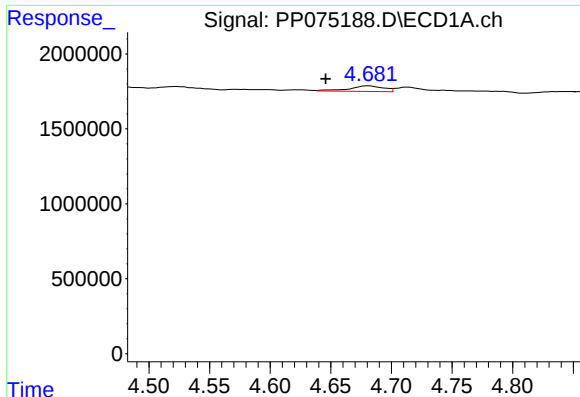

#1 Tetrachloro-m-xylene


R.T.: 4.682 min
Delta R.T.: 0.036 min
Response: 732089
Conc: 0.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

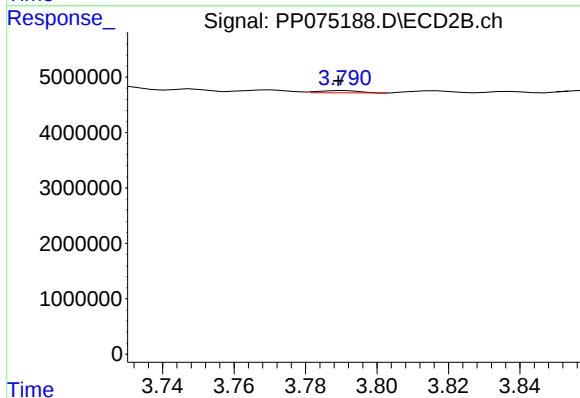


#1 Tetrachloro-m-xylene

R.T.: 3.791 min
Delta R.T.: 0.002 min
Response: 303010
Conc: 0.05 ng/ml

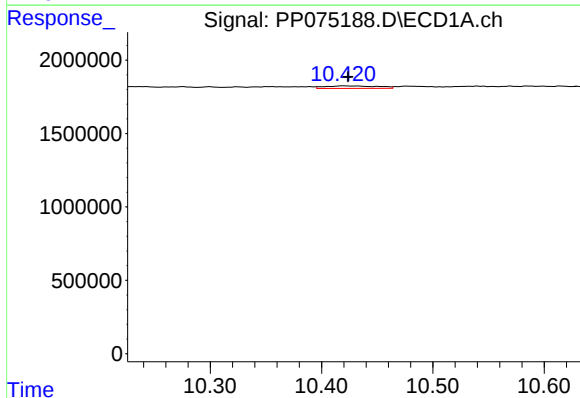


#2 Decachlorobiphenyl

R.T.: 10.421 min
Delta R.T.: -0.002 min
Response: 580517
Conc: 0.51 ng/ml

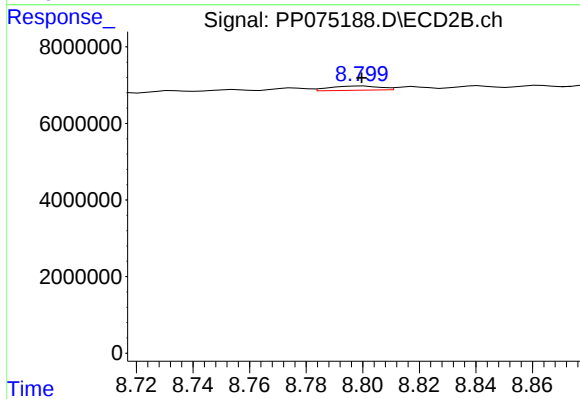

#2 Decachlorobiphenyl


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 1329090
Conc: 0.16 ng/ml

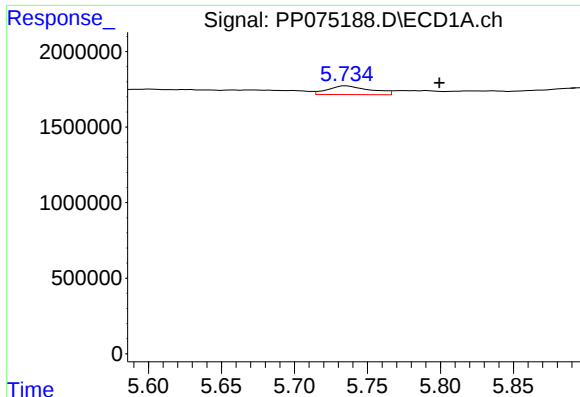

#3 AR-1016-1


R.T.: 5.736 min
Delta R.T.: -0.064 min
Response: 1159449
Conc: 24.16 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

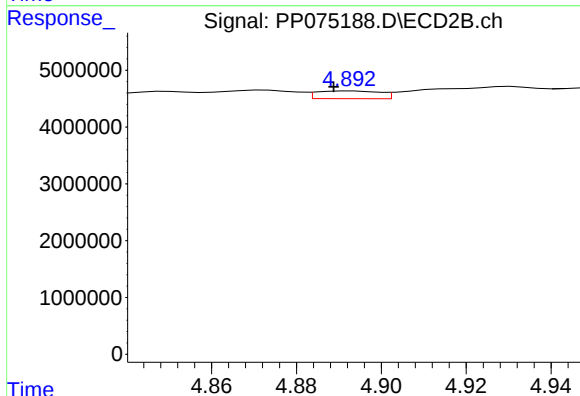


#3 AR-1016-1

R.T.: 4.893 min
Delta R.T.: 0.004 min
Response: 1392021
Conc: 2.54 ng/ml

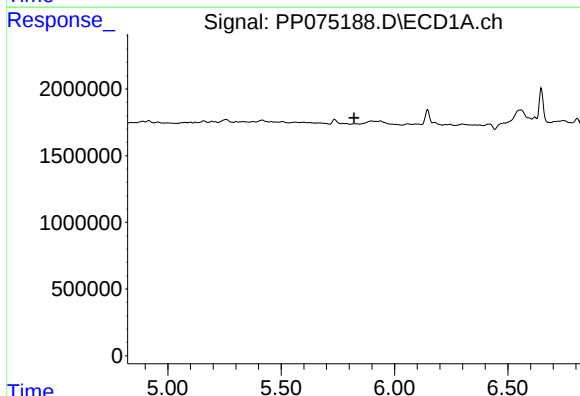


#4 AR-1016-2

R.T.: 0.000 min
Exp R.T. : 5.821 min
Response: 0
Conc: N.D.

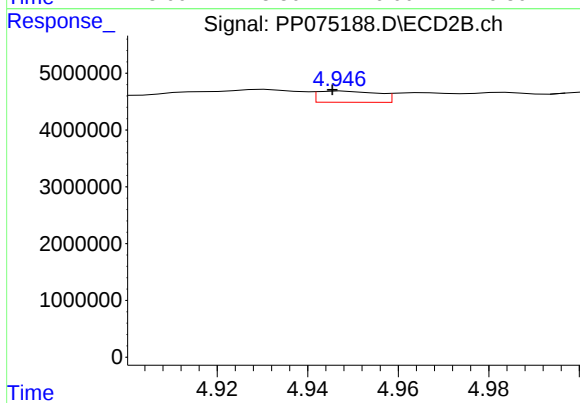

#4 AR-1016-2


R.T.: 4.948 min
Delta R.T.: 0.002 min
Response: 1833152
Conc: 6.75 ng/ml

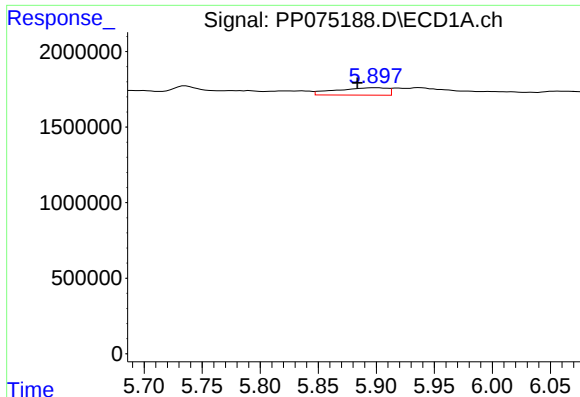

#5 AR-1016-3


R.T.: 5.899 min
Delta R.T.: 0.015 min
Response: 1514629
Conc: 31.99 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

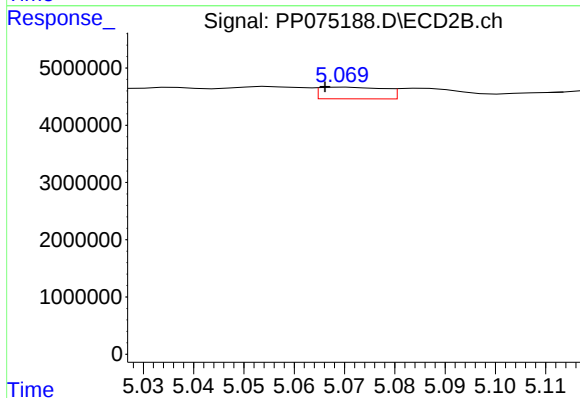


#5 AR-1016-3

R.T.: 5.070 min
Delta R.T.: 0.004 min
Response: 1816854
Conc: 12.97 ng/ml

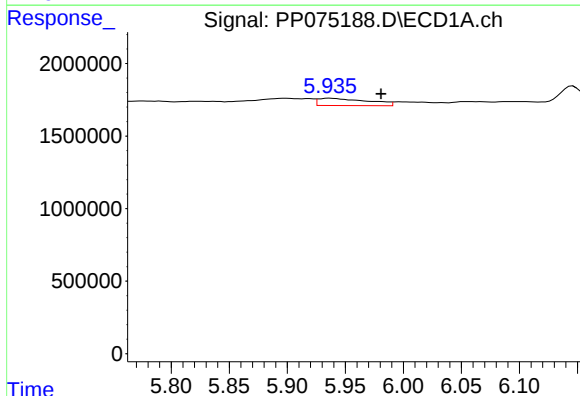


#6 AR-1016-4

R.T.: 5.936 min
Delta R.T.: -0.044 min
Response: 1504180
Conc: 42.50 ng/ml

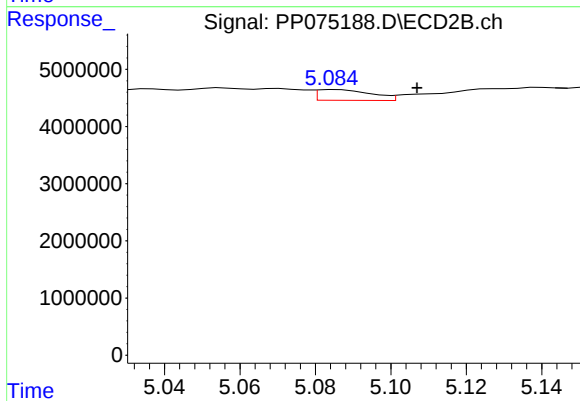

#6 AR-1016-4


R.T.: 5.086 min
Delta R.T.: -0.021 min
Response: 1884628
Conc: 13.33 ng/ml

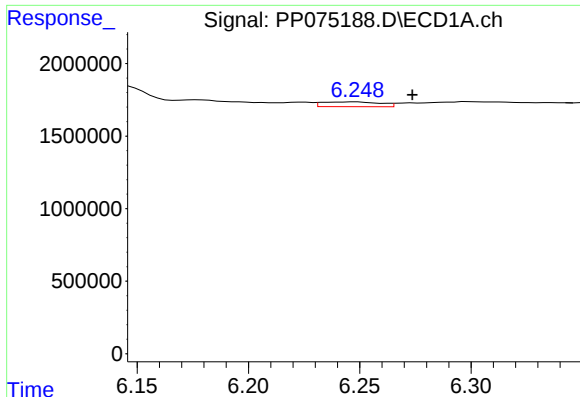

#7 AR-1016-5


R.T.: 6.249 min
Delta R.T.: -0.025 min
Response: 605655
Conc: 16.70 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

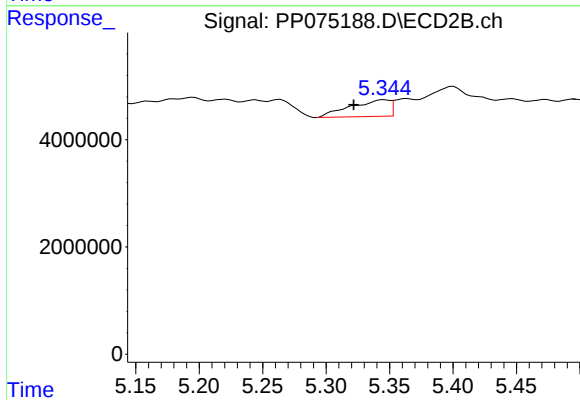


#7 AR-1016-5

R.T.: 5.345 min
Delta R.T.: 0.024 min
Response: 6674187
Conc: 42.18 ng/ml

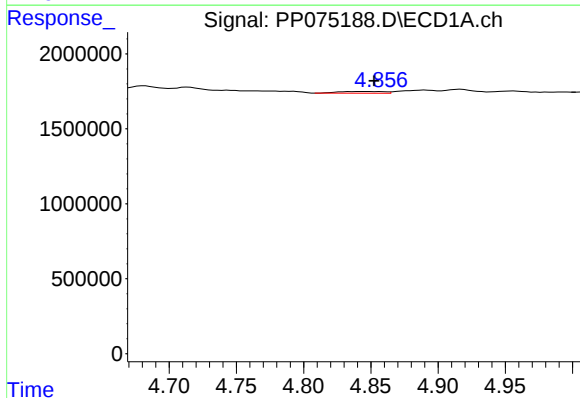


#8 AR-1221-1

R.T.: 4.842 min
Delta R.T.: -0.010 min
Response: 282180
Conc: 14.97 ng/ml

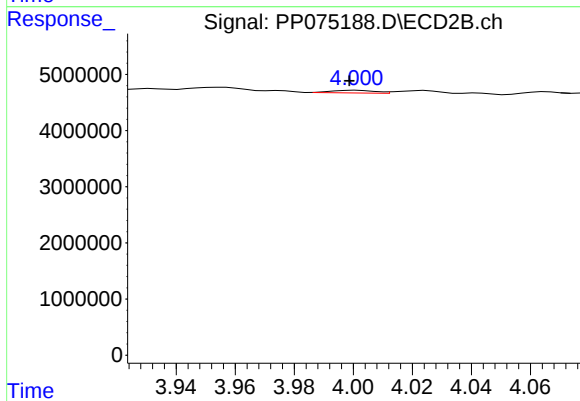

#8 AR-1221-1


R.T.: 4.001 min
Delta R.T.: 0.003 min
Response: 478824
Conc: 6.23 ng/ml

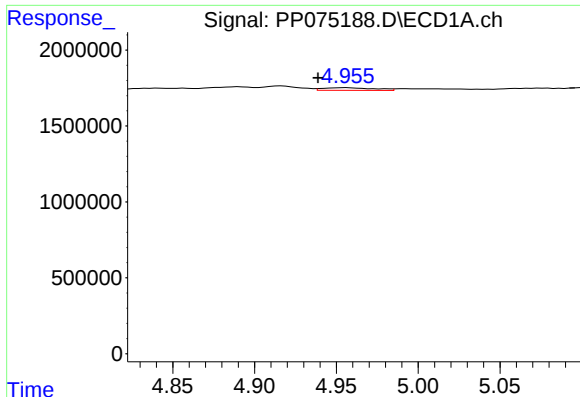

#9 AR-1221-2


R.T.: 4.956 min
Delta R.T.: 0.018 min
Response: 384057
Conc: 26.88 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

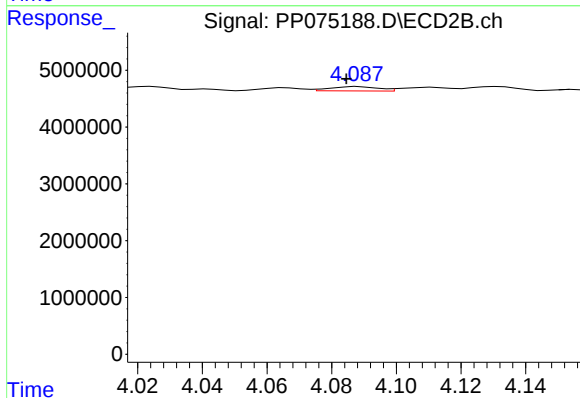


#9 AR-1221-2

R.T.: 4.088 min
Delta R.T.: 0.004 min
Response: 796980
Conc: 14.57 ng/ml

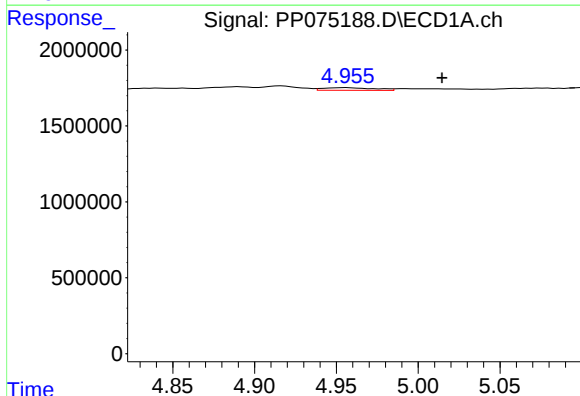


#10 AR-1221-3

R.T.: 4.956 min
Delta R.T.: -0.058 min
Response: 384057
Conc: 9.21 ng/ml

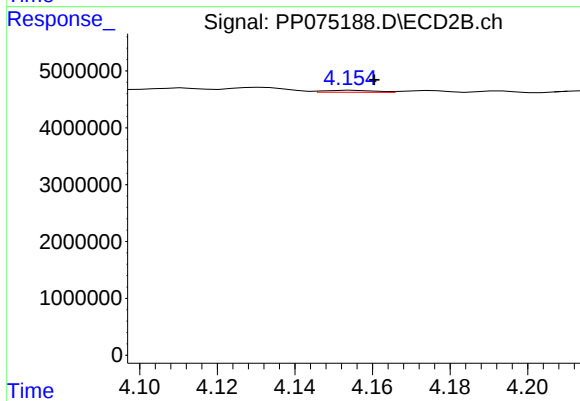

#10 AR-1221-3


R.T.: 4.155 min
Delta R.T.: -0.006 min
Response: 315634
Conc: 1.63 ng/ml

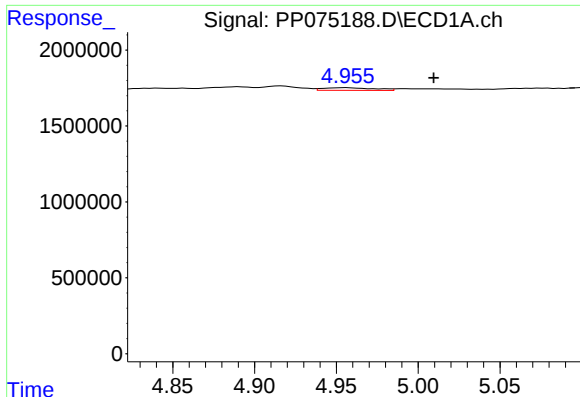

#11 AR-1232-1


R.T.: 4.956 min
Delta R.T.: -0.053 min
Response: 384057
Conc: 10.09 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

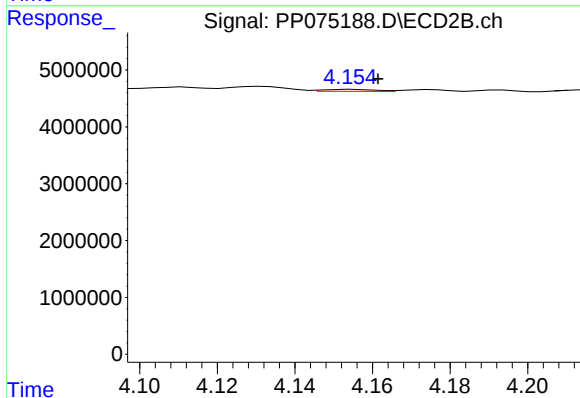


#11 AR-1232-1

R.T.: 4.155 min
Delta R.T.: -0.006 min
Response: 315634
Conc: 2.16 ng/ml

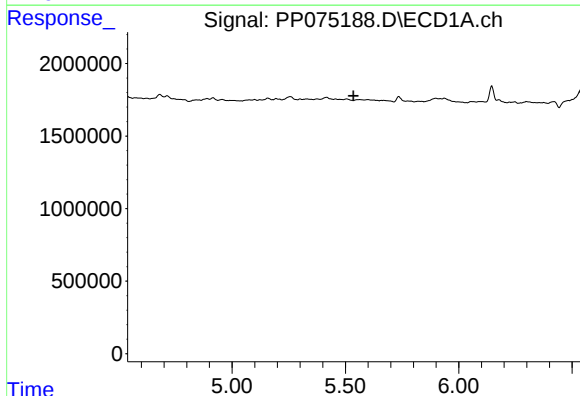


#12 AR-1232-2

R.T.: 0.000 min
Exp R.T. : 5.536 min
Response: 0
Conc: N.D.

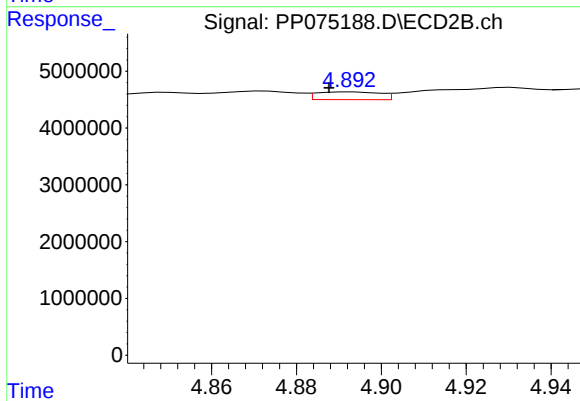

#12 AR-1232-2


R.T.: 4.893 min
Delta R.T.: 0.005 min
Response: 1392021
Conc: 5.55 ng/ml

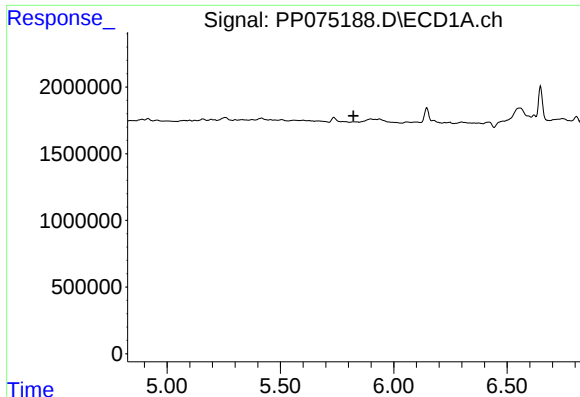

#13 AR-1232-3


R.T.: 0.000 min
Exp R.T.: 5.823 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

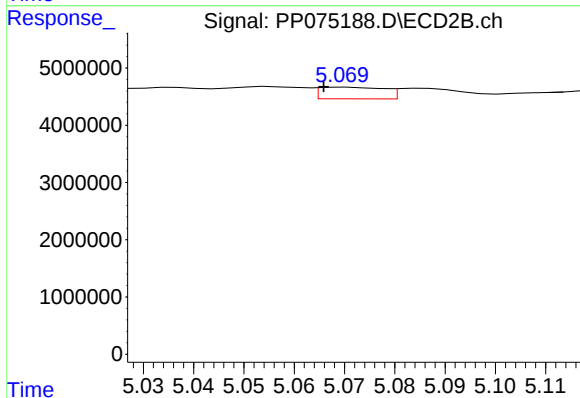


#13 AR-1232-3

R.T.: 5.070 min
Delta R.T.: 0.004 min
Response: 1816854
Conc: 29.22 ng/ml

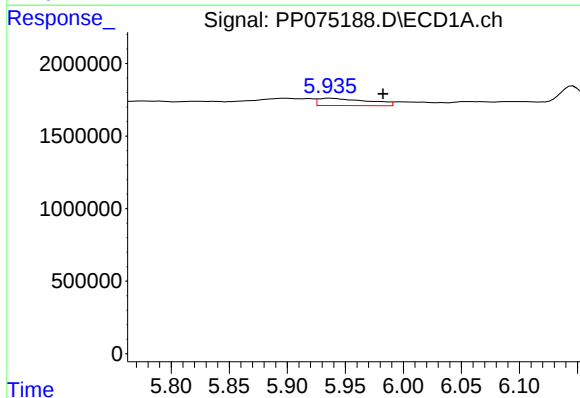


#14 AR-1232-4

R.T.: 5.936 min
Delta R.T.: -0.046 min
Response: 1504180
Conc: 82.42 ng/ml

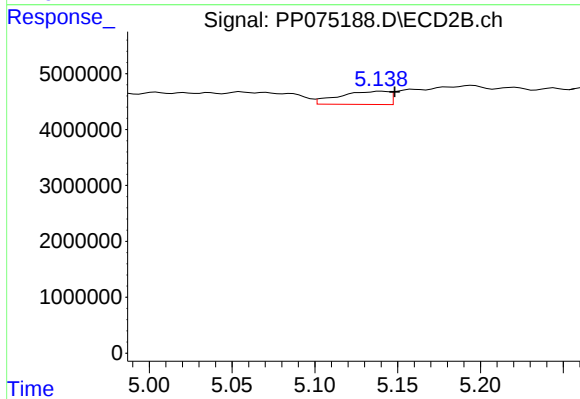

#14 AR-1232-4


R.T.: 5.140 min
Delta R.T.: -0.008 min
Response: 4909681
Conc: 69.09 ng/ml

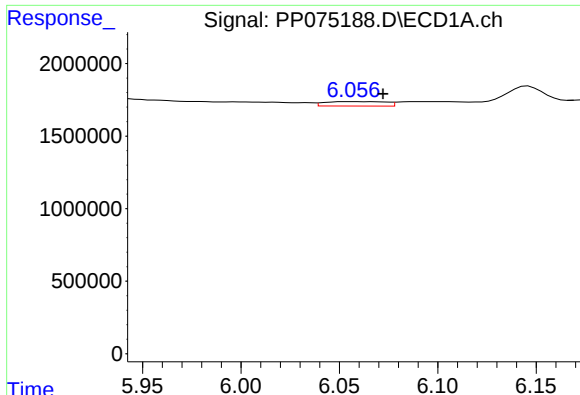

#15 AR-1232-5


R.T.: 6.057 min
Delta R.T.: -0.015 min
Response: 661359
Conc: 50.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

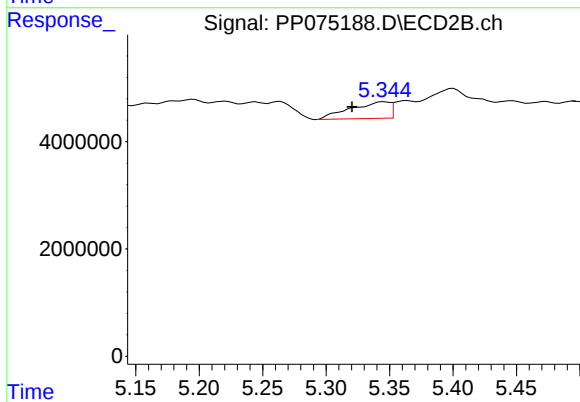


#15 AR-1232-5

R.T.: 5.345 min
Delta R.T.: 0.025 min
Response: 6674187
Conc: 105.51 ng/ml

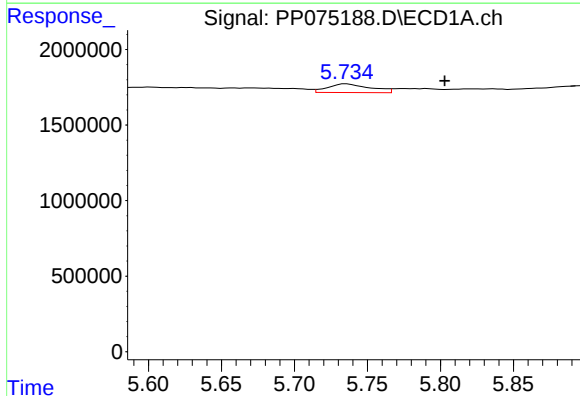


#16 AR-1242-1

R.T.: 5.736 min
Delta R.T.: -0.067 min
Response: 1159449
Conc: 28.40 ng/ml

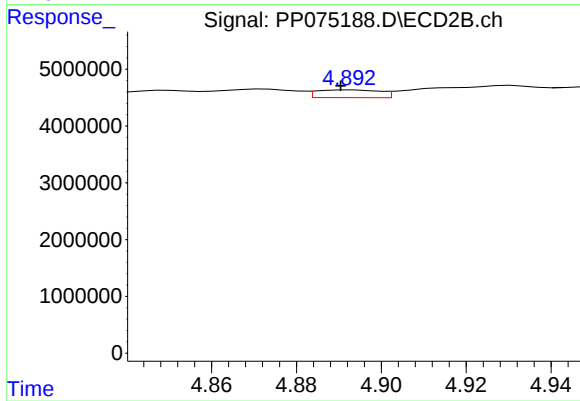

#16 AR-1242-1


R.T.: 4.893 min
Delta R.T.: 0.002 min
Response: 1392021
Conc: 3.00 ng/ml

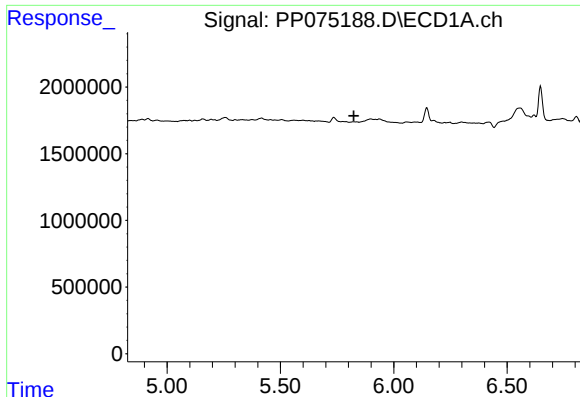

#17 AR-1242-2


R.T.: 0.000 min
Exp R.T.: 5.824 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

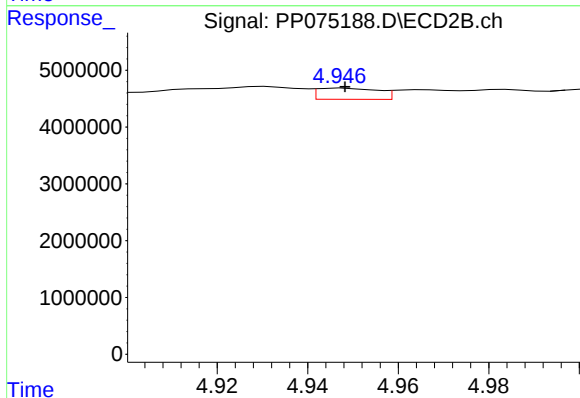


#17 AR-1242-2

R.T.: 4.948 min
Delta R.T.: 0.000 min
Response: 1833152
Conc: 8.53 ng/ml

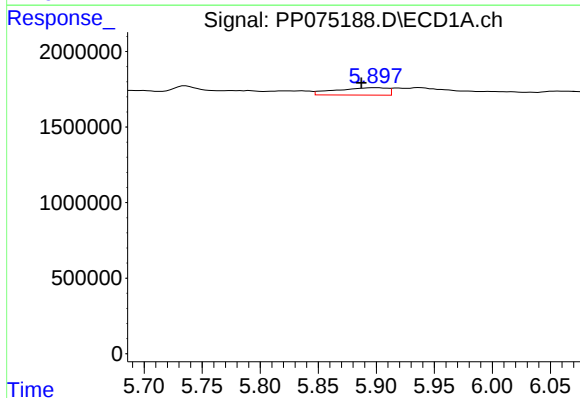


#18 AR-1242-3

R.T.: 5.899 min
Delta R.T.: 0.011 min
Response: 1514629
Conc: 35.88 ng/ml

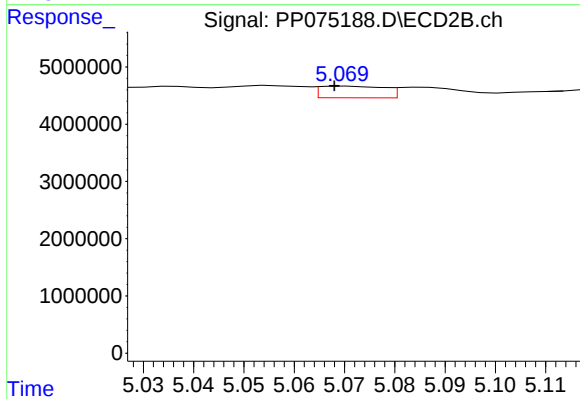

#18 AR-1242-3


R.T.: 5.070 min
Delta R.T.: 0.002 min
Response: 1816854
Conc: 15.28 ng/ml

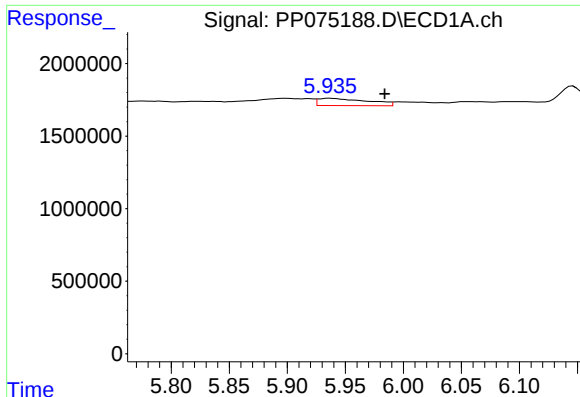

#19 AR-1242-4


R.T.: 5.936 min
Delta R.T.: -0.048 min
Response: 1504180
Conc: 45.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

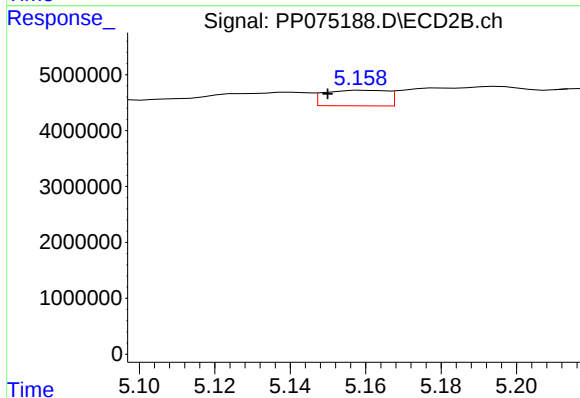


#19 AR-1242-4

R.T.: 5.160 min
Delta R.T.: 0.010 min
Response: 3185884
Conc: 20.76 ng/ml

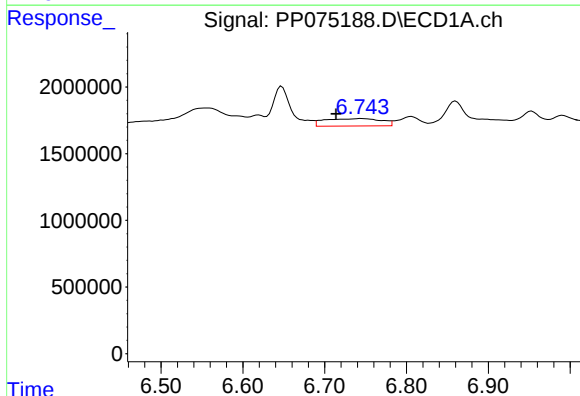


#20 AR-1242-5

R.T.: 6.745 min
Delta R.T.: 0.031 min
Response: 2684201
Conc: 73.09 ng/ml

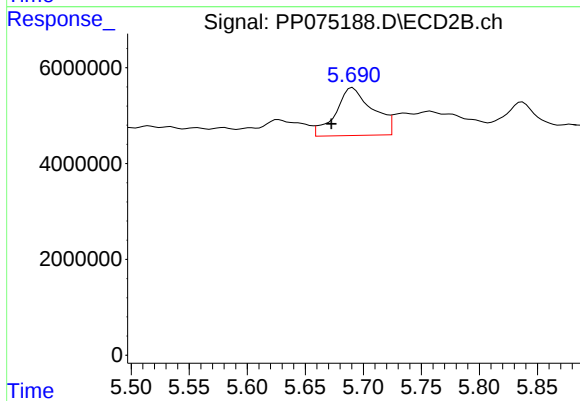

#20 AR-1242-5


R.T.: 5.691 min
Delta R.T.: 0.018 min
Response: 22135419
Conc: 113.68 ng/ml

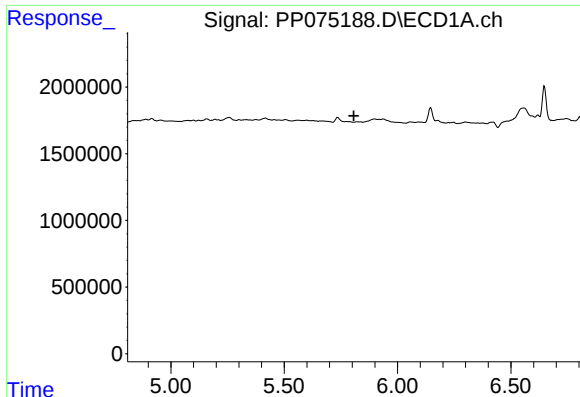

#21 AR-1248-1


R.T.: 0.000 min
Exp R.T.: 5.807 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

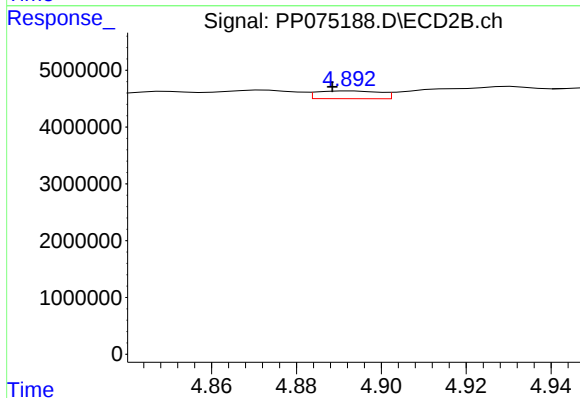


#21 AR-1248-1

R.T.: 4.893 min
Delta R.T.: 0.004 min
Response: 1392021
Conc: 4.63 ng/ml

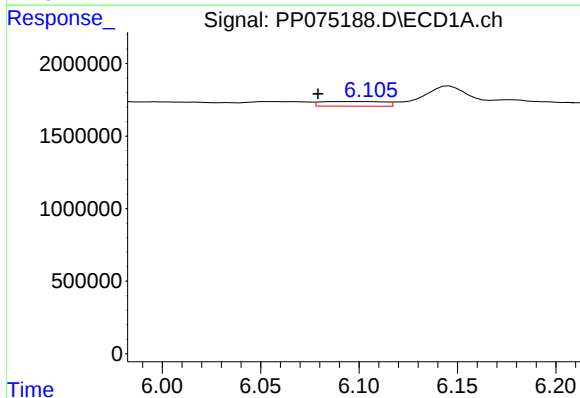


#22 AR-1248-2

R.T.: 6.095 min
Delta R.T.: 0.015 min
Response: 712768
Conc: 15.78 ng/ml

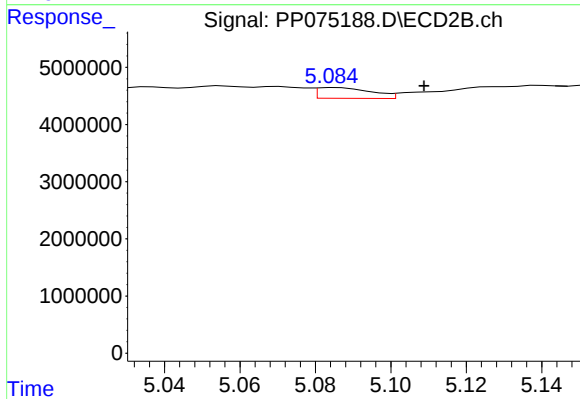

#22 AR-1248-2


R.T.: 5.086 min
Delta R.T.: -0.023 min
Response: 1884628
Conc: 9.42 ng/ml

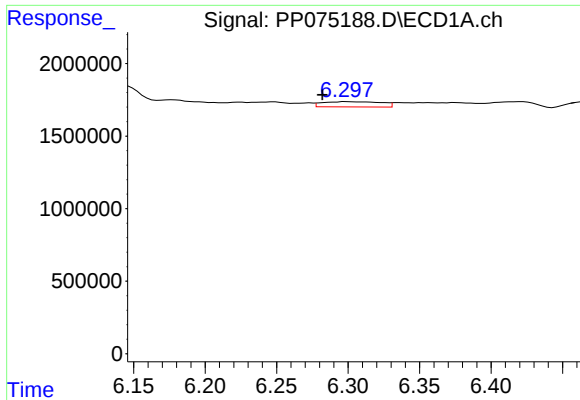

#23 AR-1248-3


R.T.: 6.299 min
Delta R.T.: 0.017 min
Response: 1036799
Conc: 20.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

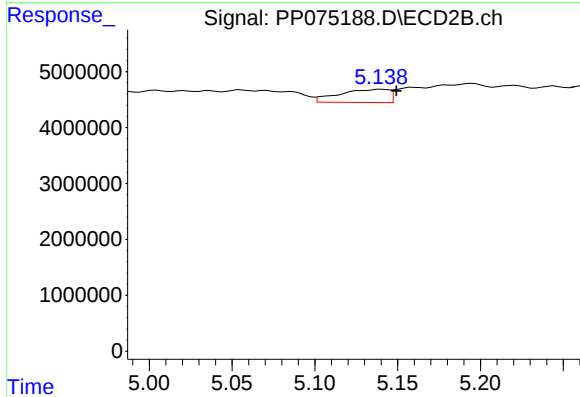


#23 AR-1248-3

R.T.: 5.140 min
Delta R.T.: -0.009 min
Response: 4909681
Conc: 20.58 ng/ml

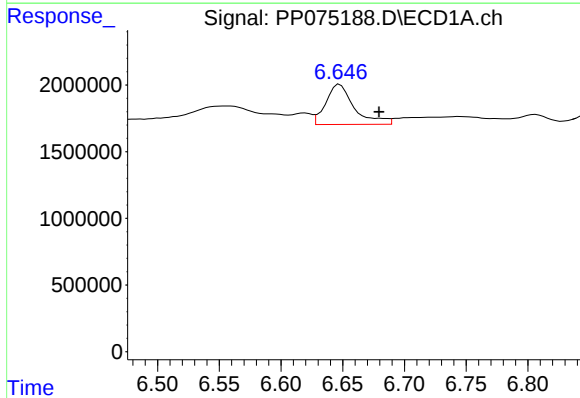


#24 AR-1248-4

R.T.: 6.648 min
Delta R.T.: -0.032 min
Response: 4811206
Conc: 80.07 ng/ml

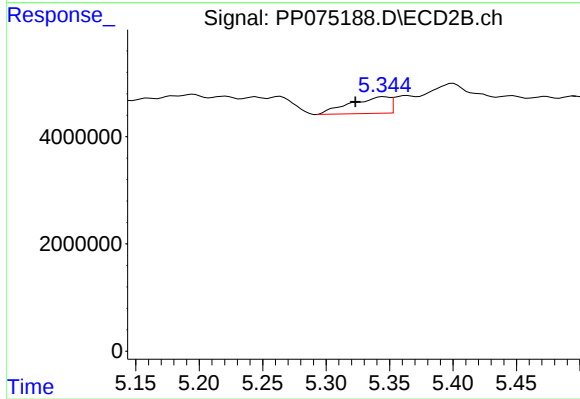

#24 AR-1248-4


R.T.: 5.345 min
Delta R.T.: 0.022 min
Response: 6674187
Conc: 28.50 ng/ml

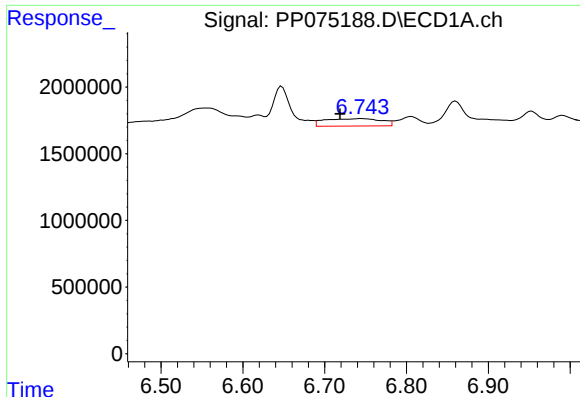

#25 AR-1248-5


R.T.: 6.745 min
Delta R.T.: 0.026 min
Response: 2684201
Conc: 44.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

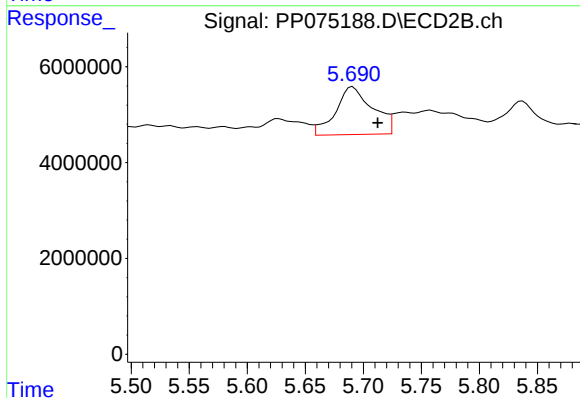


#25 AR-1248-5

R.T.: 5.691 min
Delta R.T.: -0.022 min
Response: 22135419
Conc: 56.51 ng/ml

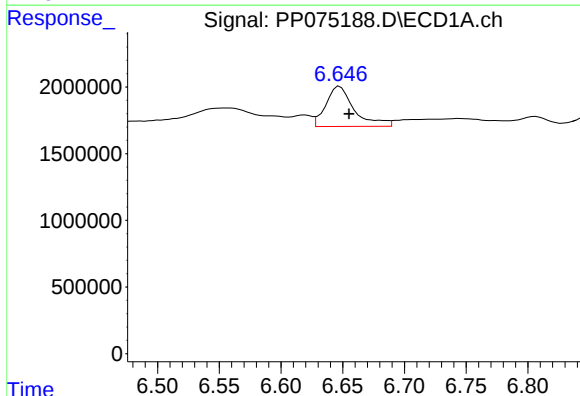


#26 AR-1254-1

R.T.: 6.648 min
Delta R.T.: -0.007 min
Response: 4811206
Conc: 73.55 ng/ml

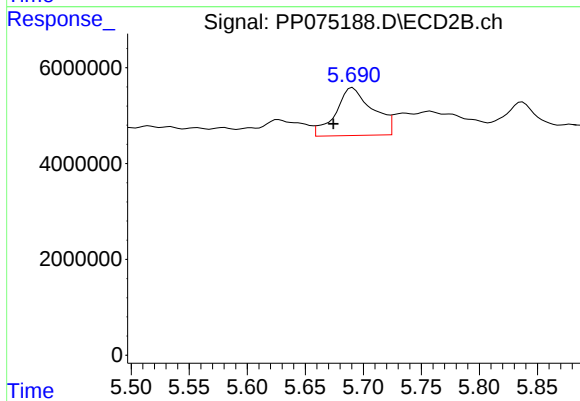

#26 AR-1254-1


R.T.: 5.691 min
Delta R.T.: 0.017 min
Response: 22135419
Conc: 40.69 ng/ml

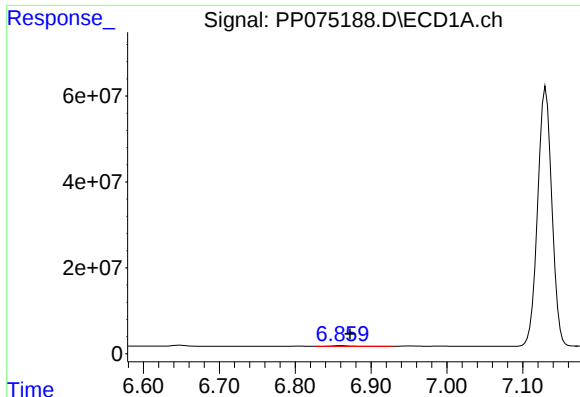

#27 AR-1254-2


R.T.: 6.860 min
Delta R.T.: -0.012 min
Response: 4242169
Conc: 49.80 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

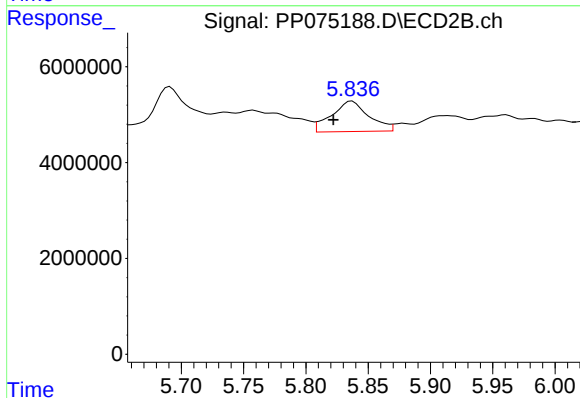


#27 AR-1254-2

R.T.: 5.837 min
Delta R.T.: 0.015 min
Response: 13233540
Conc: 36.33 ng/ml

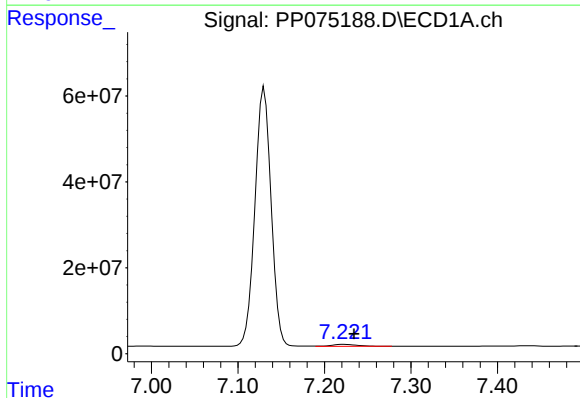


#28 AR-1254-3

R.T.: 7.222 min
Delta R.T.: -0.012 min
Response: 9444068
Conc: 99.25 ng/ml

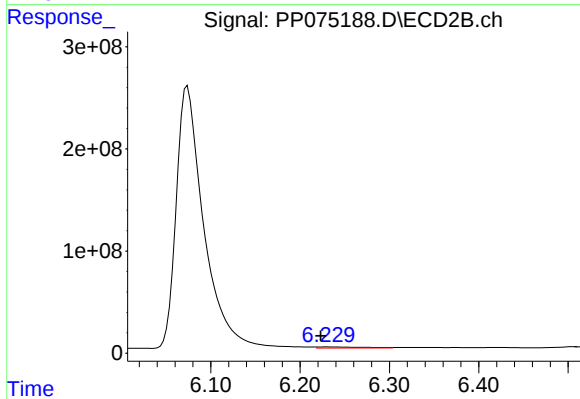

#28 AR-1254-3


R.T.: 6.230 min
Delta R.T.: 0.007 min
Response: 42740551
Conc: 72.45 ng/ml

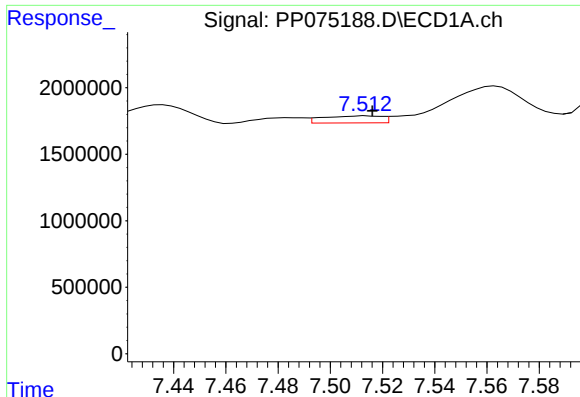

#29 AR-1254-4


R.T.: 7.514 min
Delta R.T.: -0.002 min
Response: 822233
Conc: 11.33 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

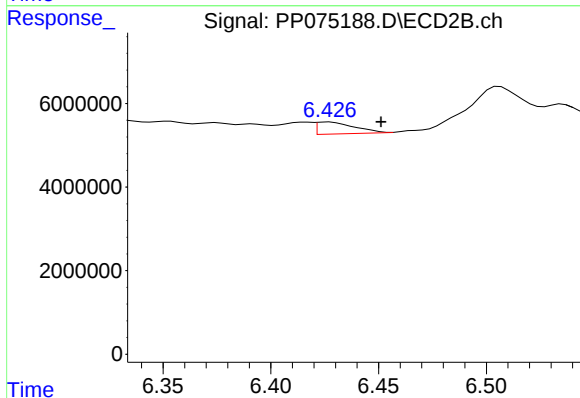


#29 AR-1254-4

R.T.: 6.427 min
Delta R.T.: -0.024 min
Response: 3481592
Conc: 7.02 ng/ml

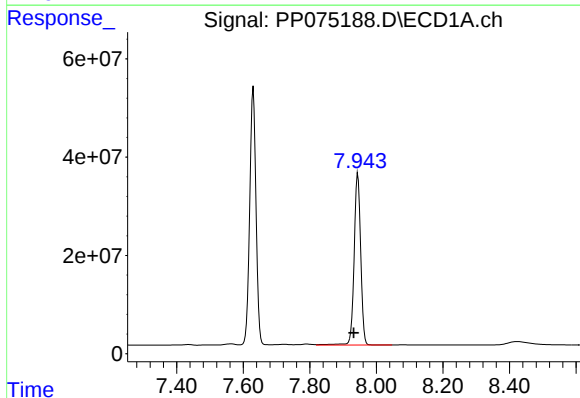


#30 AR-1254-5

R.T.: 7.944 min
Delta R.T.: 0.012 min
Response: 479830444
Conc: 5859.74 ng/ml

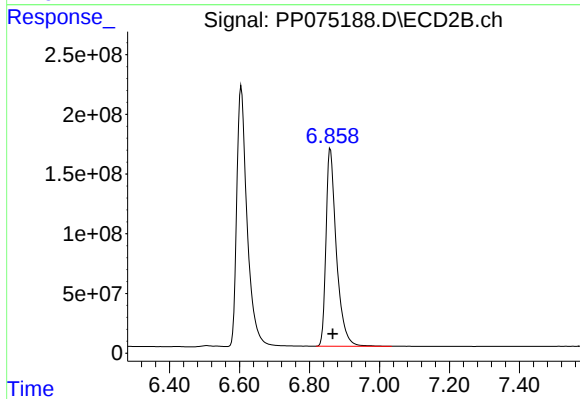

#30 AR-1254-5


R.T.: 6.860 min
Delta R.T.: -0.007 min
Response: 3418275524
Conc: 6723.37 ng/ml

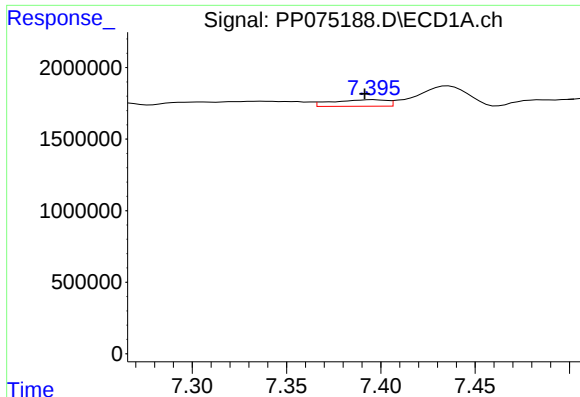

#31 AR-1260-1


R.T.: 7.396 min
Delta R.T.: 0.005 min
Response: 919897
Conc: 14.67 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

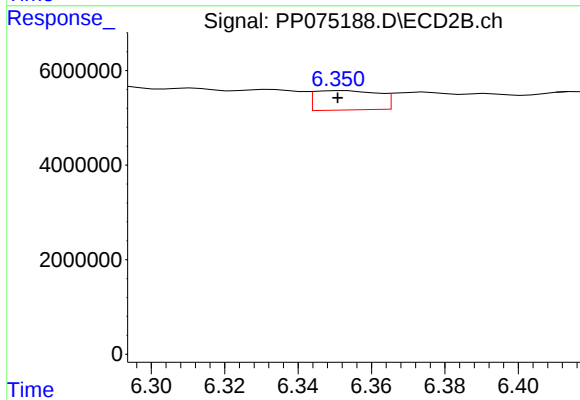


#31 AR-1260-1

R.T.: 6.353 min
Delta R.T.: 0.002 min
Response: 4973359
Conc: 11.98 ng/ml

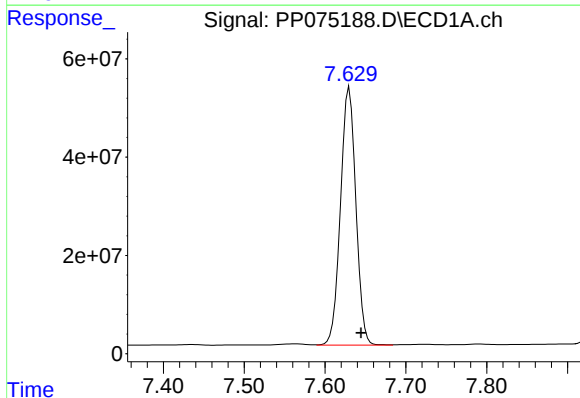


#32 AR-1260-2

R.T.: 7.630 min
Delta R.T.: -0.014 min
Response: 693915491
Conc: 9068.05 ng/ml

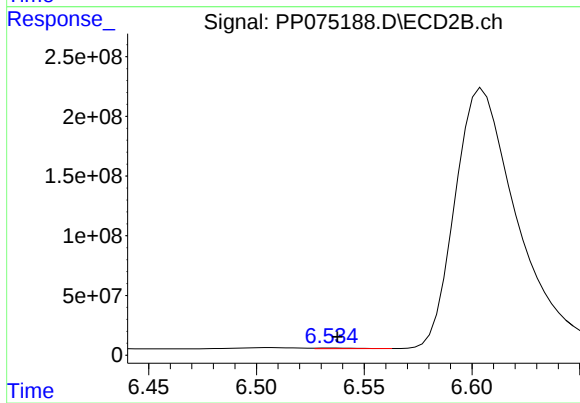

#32 AR-1260-2


R.T.: 6.535 min
Delta R.T.: -0.002 min
Response: 5842847
Conc: 10.50 ng/ml

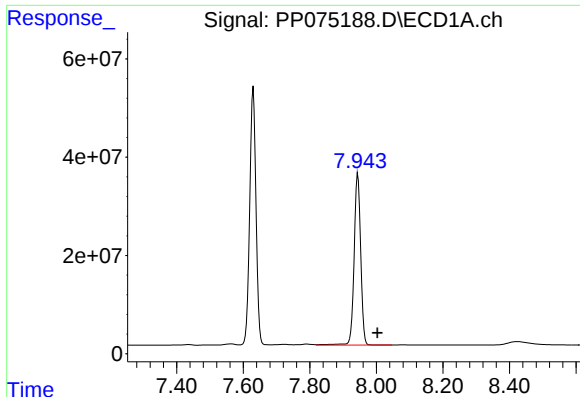

#33 AR-1260-3


R.T.: 7.944 min
Delta R.T.: -0.059 min
Response: 479830444
Conc: 8148.49 ng/m

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

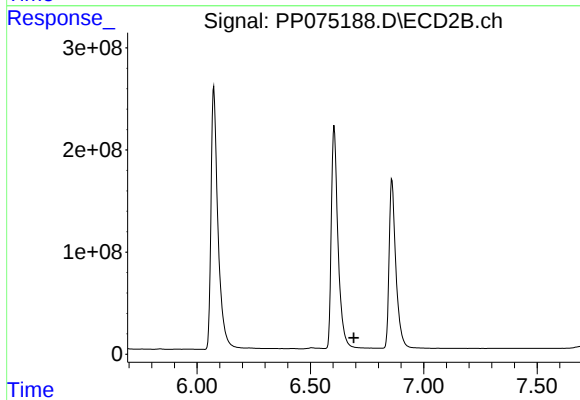


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 6.691 min
Response: 0
Conc: N.D.

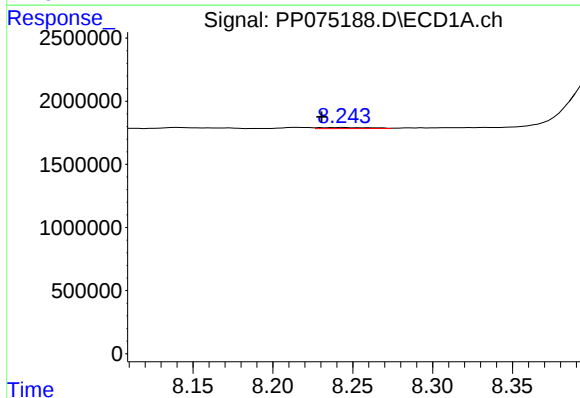


#34 AR-1260-4

R.T.: 8.244 min
Delta R.T.: 0.014 min
Response: 188413
Conc: 2.79 ng/ml

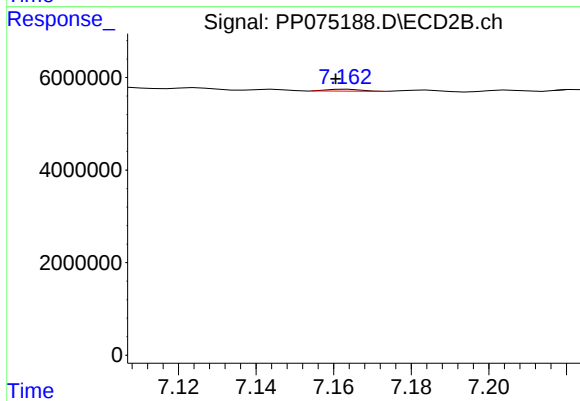

#34 AR-1260-4


R.T.: 7.164 min
Delta R.T.: 0.003 min
Response: 257550
Conc: 0.65 ng/ml

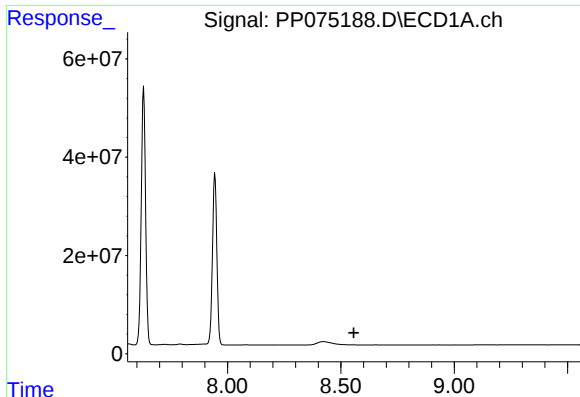

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.556 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

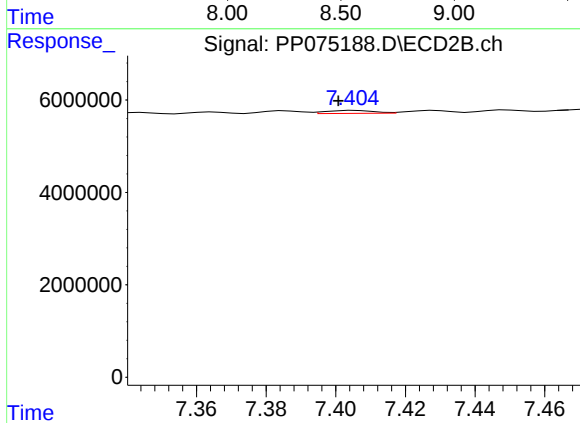


#35 AR-1260-5

R.T.: 7.405 min
Delta R.T.: 0.005 min
Response: 614506
Conc: 0.60 ng/ml

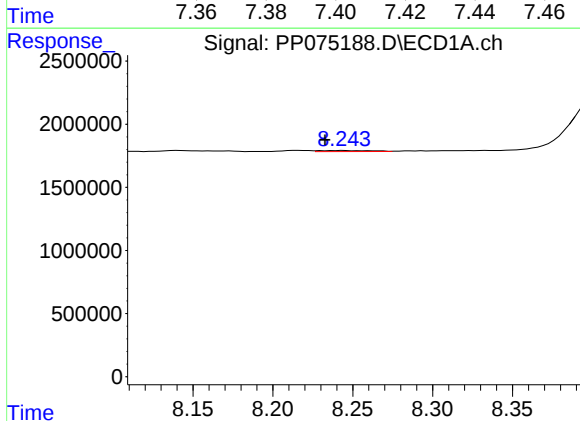


#36 AR-1262-1

R.T.: 8.244 min
Delta R.T.: 0.012 min
Response: 188413
Conc: 2.33 ng/ml

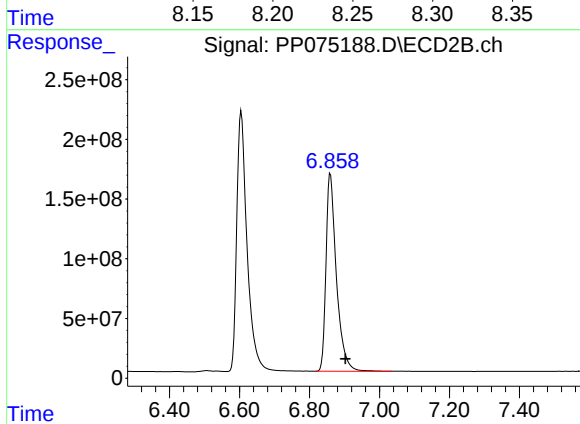

#36 AR-1262-1


R.T.: 6.860 min
Delta R.T.: -0.043 min
Response: 3418275524
Conc: 4520.40 ng/ml

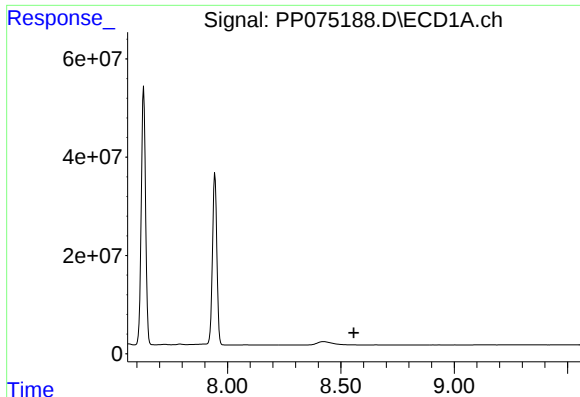

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.557 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

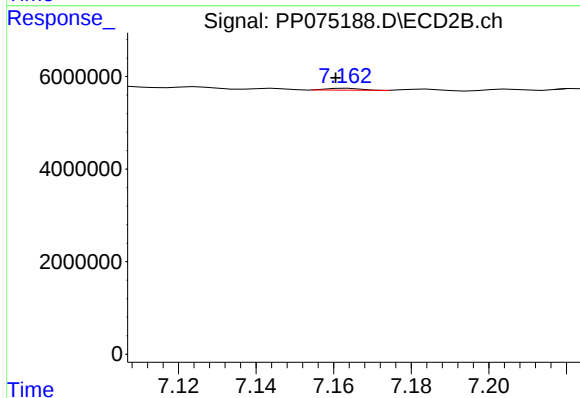


#37 AR-1262-2

R.T.: 7.164 min
Delta R.T.: 0.003 min
Response: 257550
Conc: 0.47 ng/ml

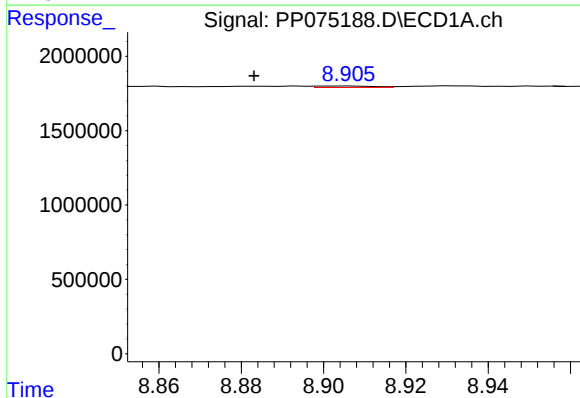


#38 AR-1262-3

R.T.: 8.906 min
Delta R.T.: 0.023 min
Response: 93155
Conc: 0.88 ng/ml

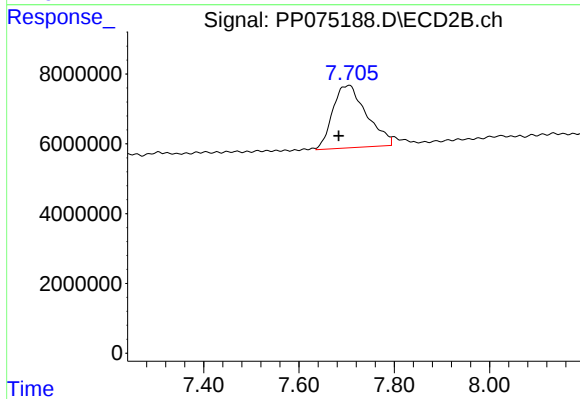

#38 AR-1262-3


R.T.: 7.706 min
Delta R.T.: 0.023 min
Response: 88089473
Conc: 180.93 ng/ml

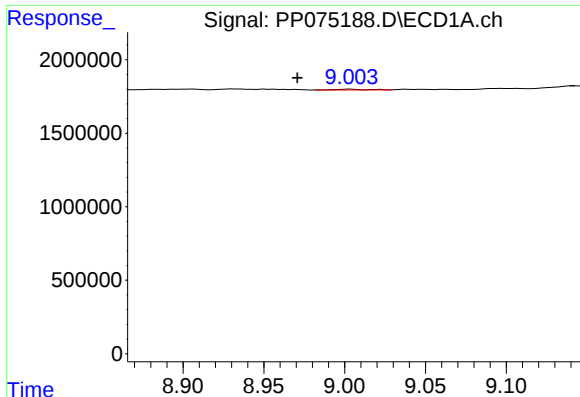

#39 AR-1262-4


R.T.: 9.004 min
Delta R.T.: 0.033 min
Response: 96171
Conc: 1.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

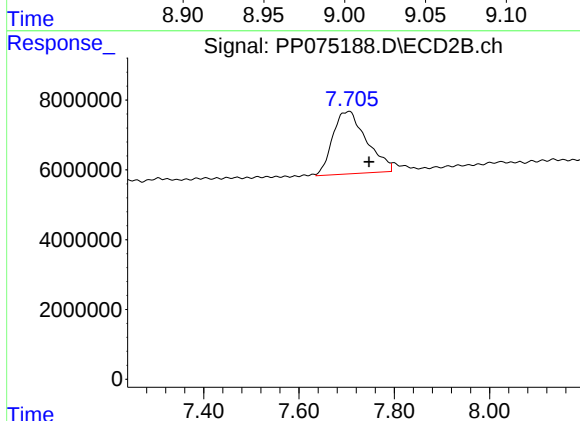


#39 AR-1262-4

R.T.: 7.706 min
Delta R.T.: -0.040 min
Response: 88089473
Conc: 99.02 ng/ml

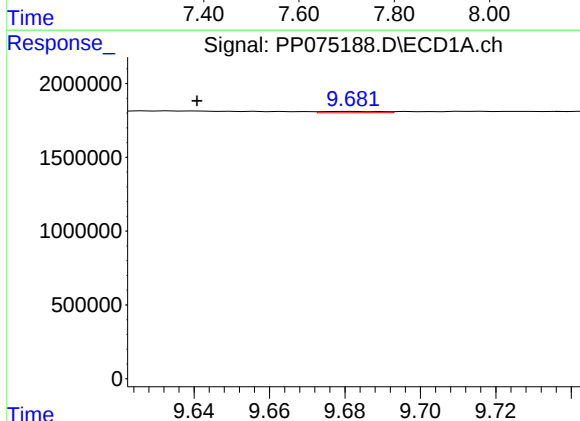


#40 AR-1262-5

R.T.: 9.682 min
Delta R.T.: 0.041 min
Response: 98390
Conc: 1.64 ng/ml

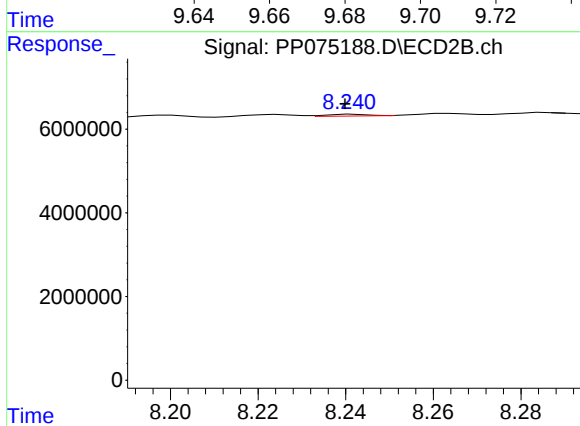

#40 AR-1262-5


R.T.: 8.242 min
Delta R.T.: 0.002 min
Response: 276607
Conc: 0.70 ng/ml

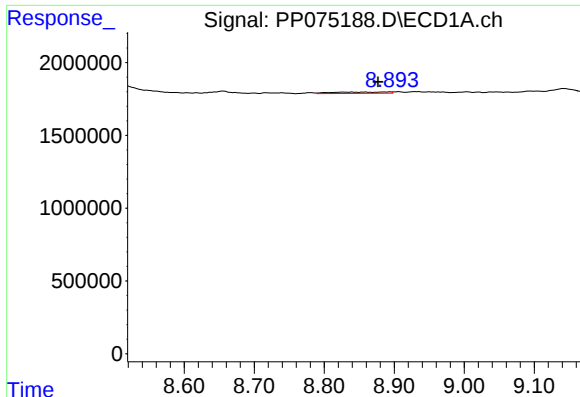

#41 AR-1268-1


R.T.: 8.860 min
Delta R.T.: -0.017 min
Response: 481285
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

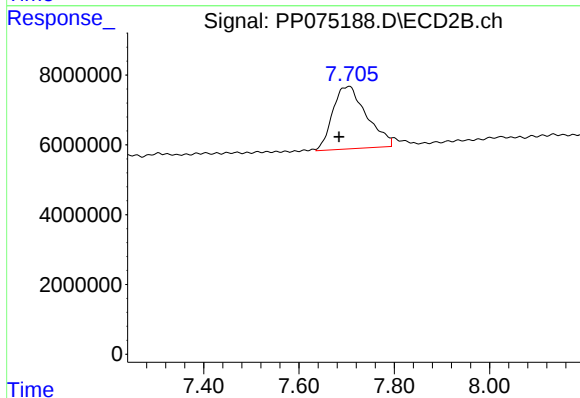


#41 AR-1268-1

R.T.: 7.706 min
Delta R.T.: 0.022 min
Response: 88089473
Conc: 59.47 ng/ml

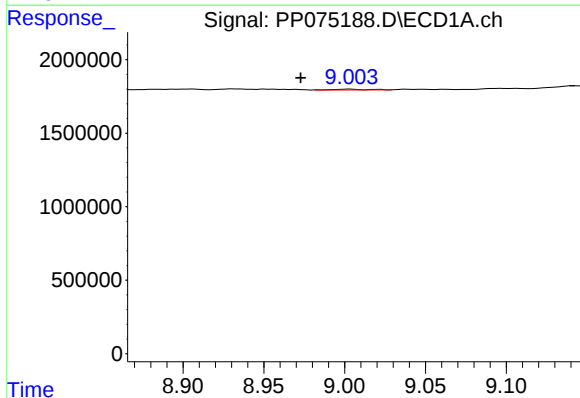


#42 AR-1268-2

R.T.: 9.004 min
Delta R.T.: 0.031 min
Response: 96171
Conc: 0.58 ng/ml

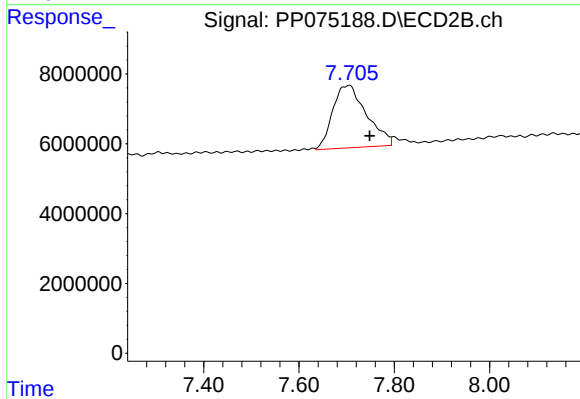

#42 AR-1268-2


R.T.: 7.706 min
Delta R.T.: -0.043 min
Response: 88089473
Conc: 61.16 ng/ml

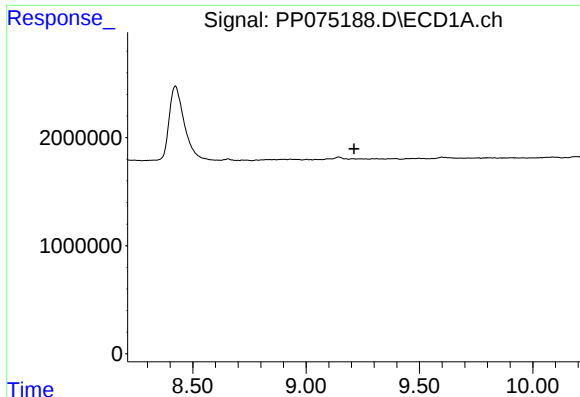

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.212 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

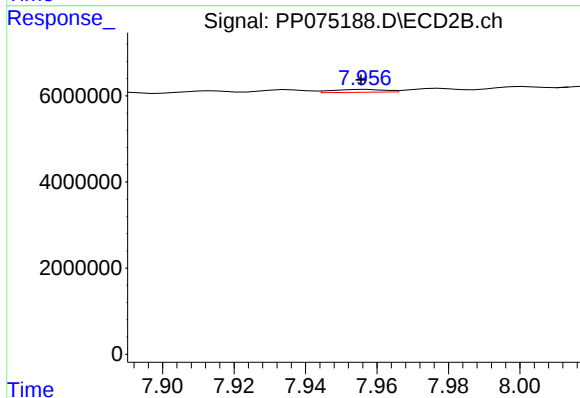


#43 AR-1268-3

R.T.: 7.957 min
Delta R.T.: 0.002 min
Response: 655536
Conc: 0.59 ng/ml

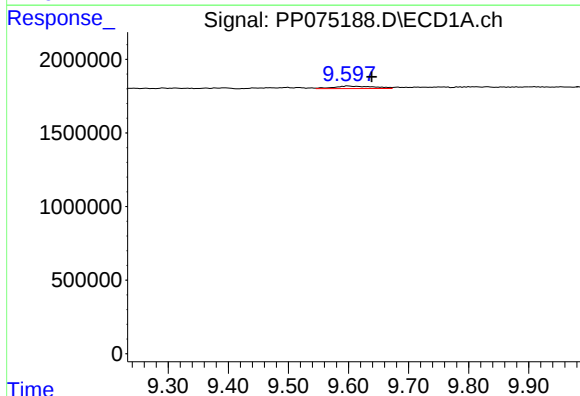


#44 AR-1268-4

R.T.: 9.599 min
Delta R.T.: -0.040 min
Response: 811619
Conc: 11.78 ng/ml

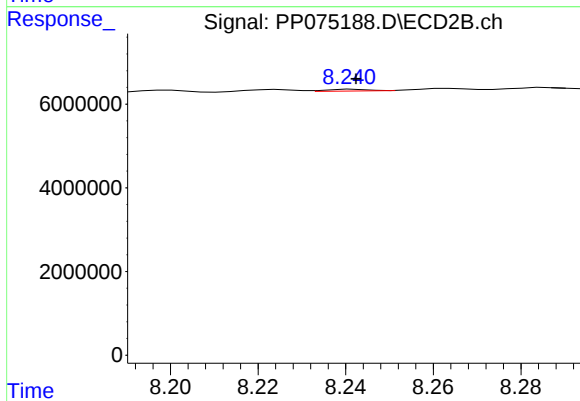

#44 AR-1268-4


R.T.: 8.242 min
Delta R.T.: 0.000 min
Response: 276607
Conc: 0.65 ng/ml

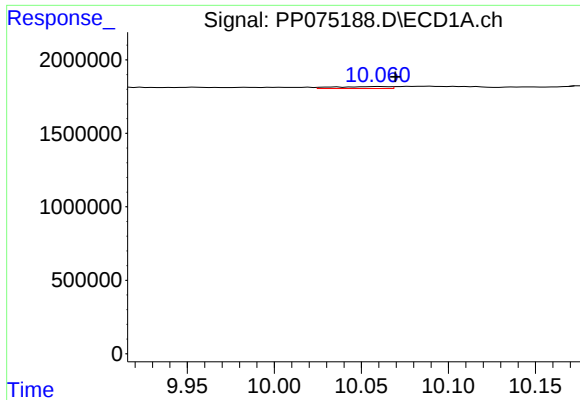

#45 AR-1268-5

R.T.: 10.061 min
Delta R.T.: -0.009 min
Response: 301851
Conc: 0.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

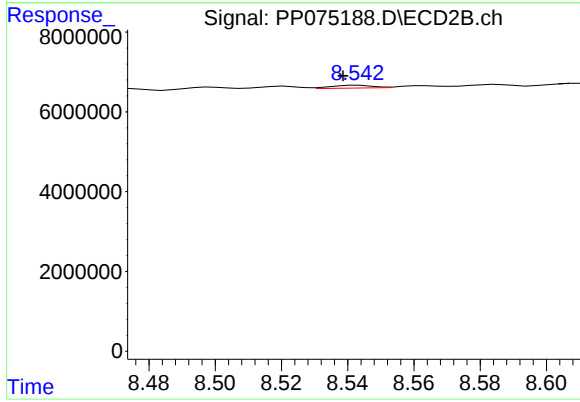

#45 AR-1268-5

R.T.: 8.543 min
Delta R.T.: 0.005 min
Response: 617886
Conc: 0.19 ng/ml