

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091625\
Data File : PP075188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 22:58
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:41:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 19:36:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
30) L6	AR-1254-5	7.944	6.860	479.8E6	3418.3E6	5859.740 6723.375



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091625\
Data File : PP075188.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2025 22:58
Operator : YP\AJ
Sample : DDT ANALOG
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:41:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091625.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 16 19:36:38 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

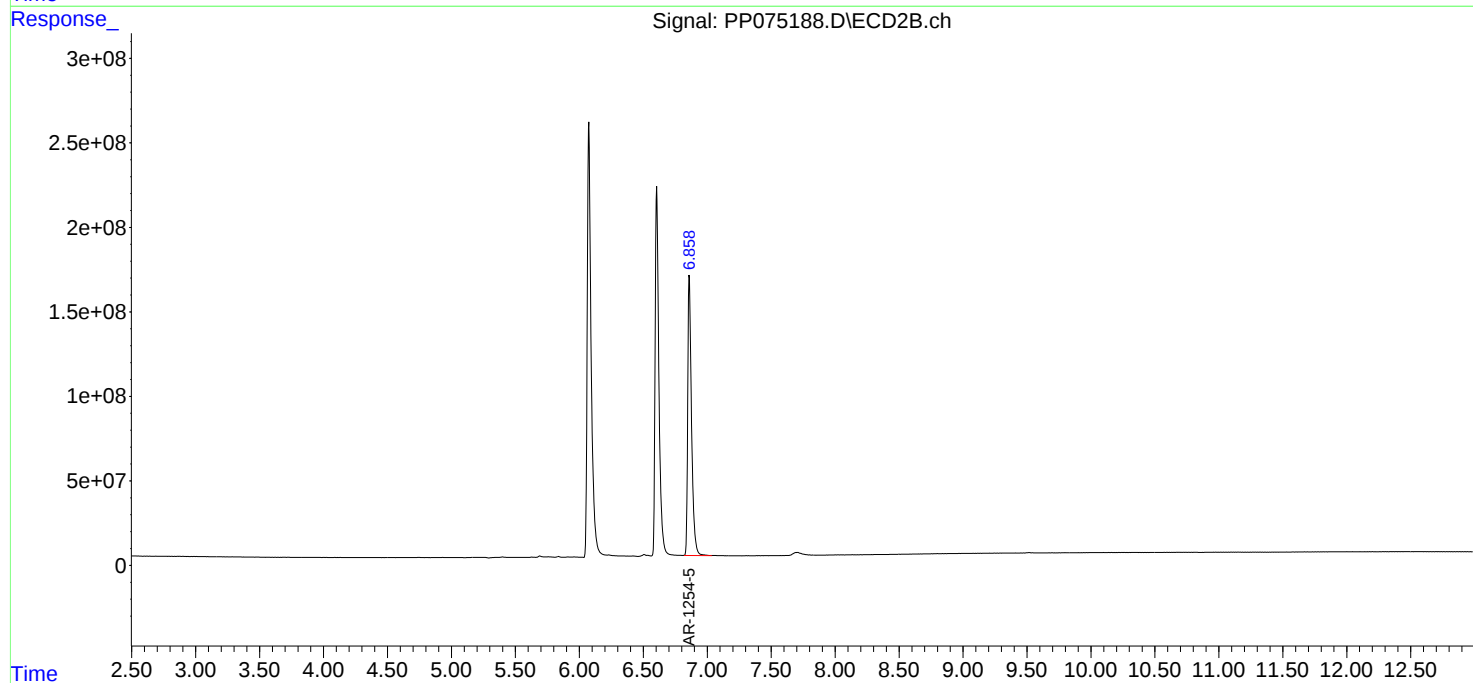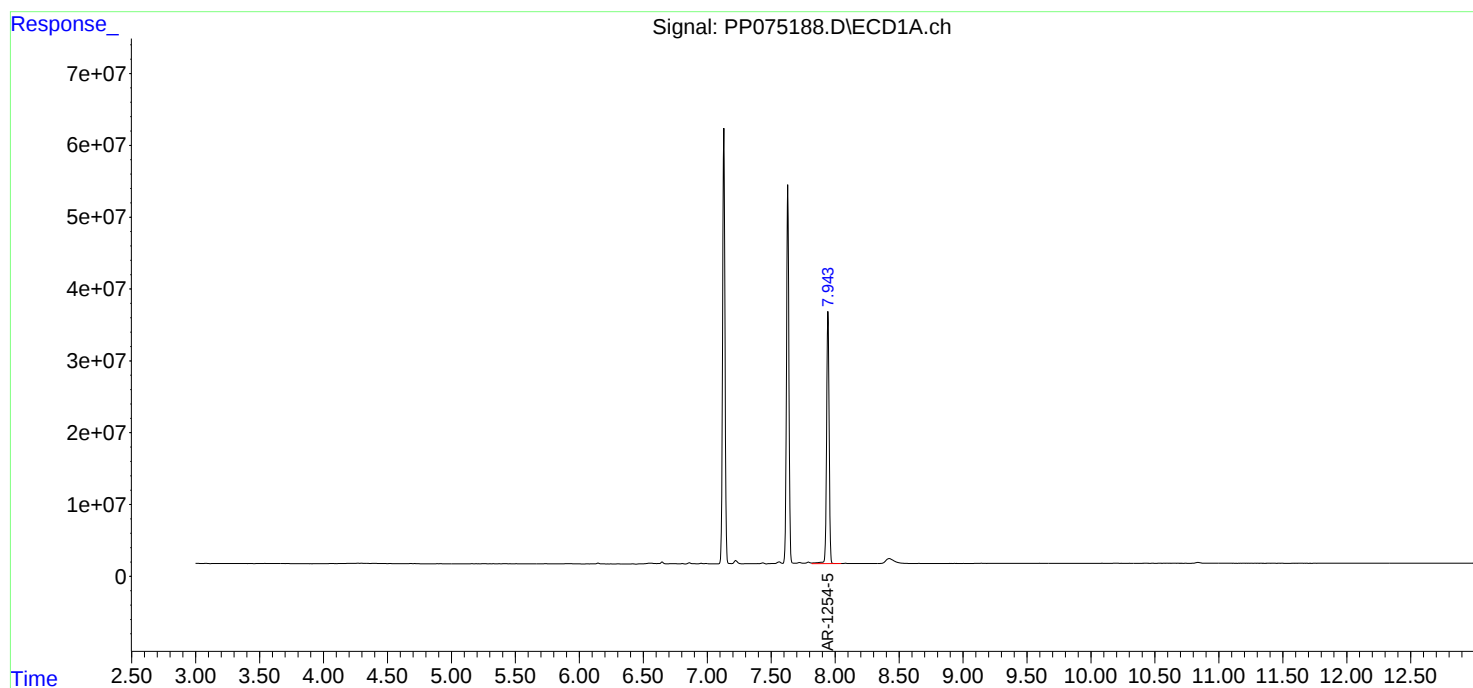


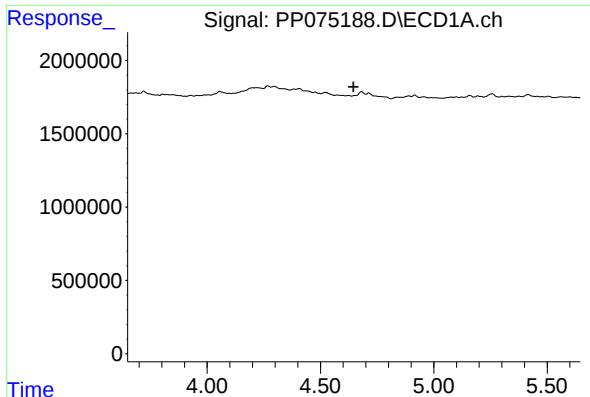

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.646 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

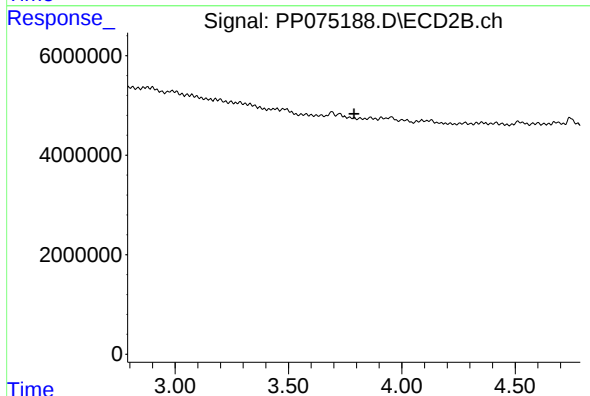


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.789 min
Response: 0
Conc: N.D.

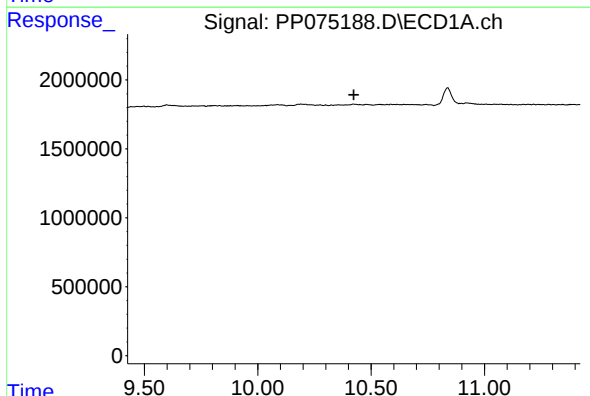


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.424 min
Response: 0
Conc: N.D.

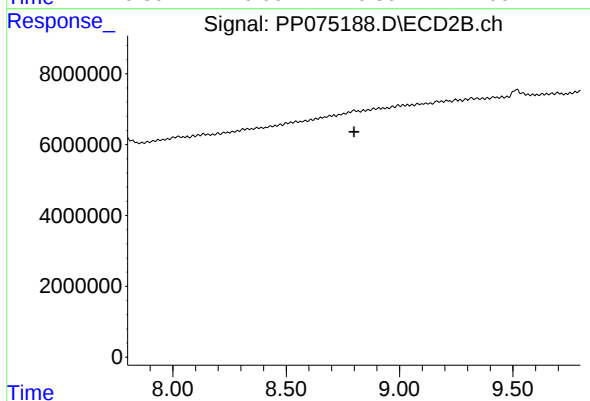

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.800 min
Response: 0
Conc: N.D.

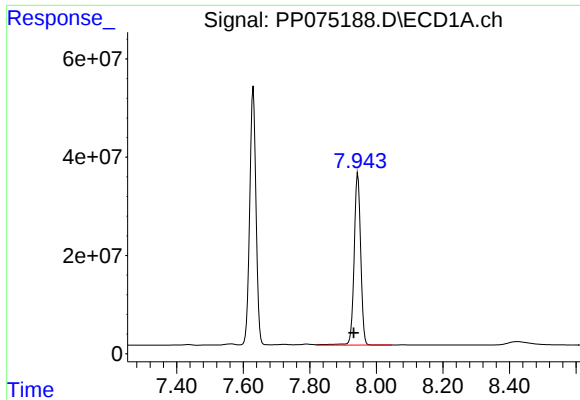

#30 AR-1254-5

R.T.: 7.944 min
Delta R.T.: 0.012 min
Response: 479830444
Conc: 5859.74 ng/m

Instrument :
ECD_P
ClientSampleId :
DDT ANALOG

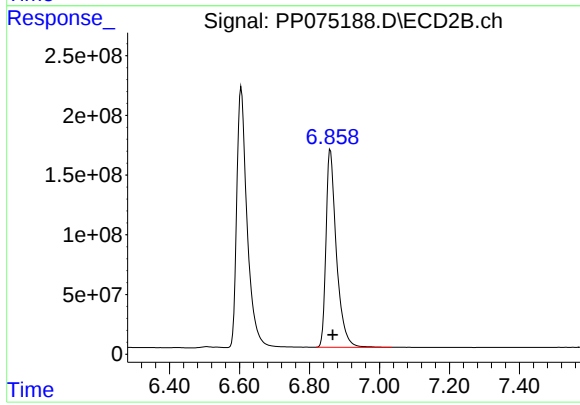

#30 AR-1254-5

R.T.: 6.860 min
Delta R.T.: -0.007 min
Response: 3418275524
Conc: 6723.37 ng/ml