

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091823\
 Data File : PP059928.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2023 06:39
 Operator : YP\AJ
 Sample : 04453-11
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FB-9-14

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 09/19/2023
 Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 08:02:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 19 07:23:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.509	3.668	43769077	34235687	21.040	21.018
2) SA Decachlor...	10.430	8.749	19502908	18719281	12.786	12.363m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091823\
Data File : PP059928.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2023 06:39
Operator : YP\AJ
Sample : 04453-11
Misc :
ALS Vial : 47 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FB-9-14


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 08:02:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091823.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 19 07:23:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

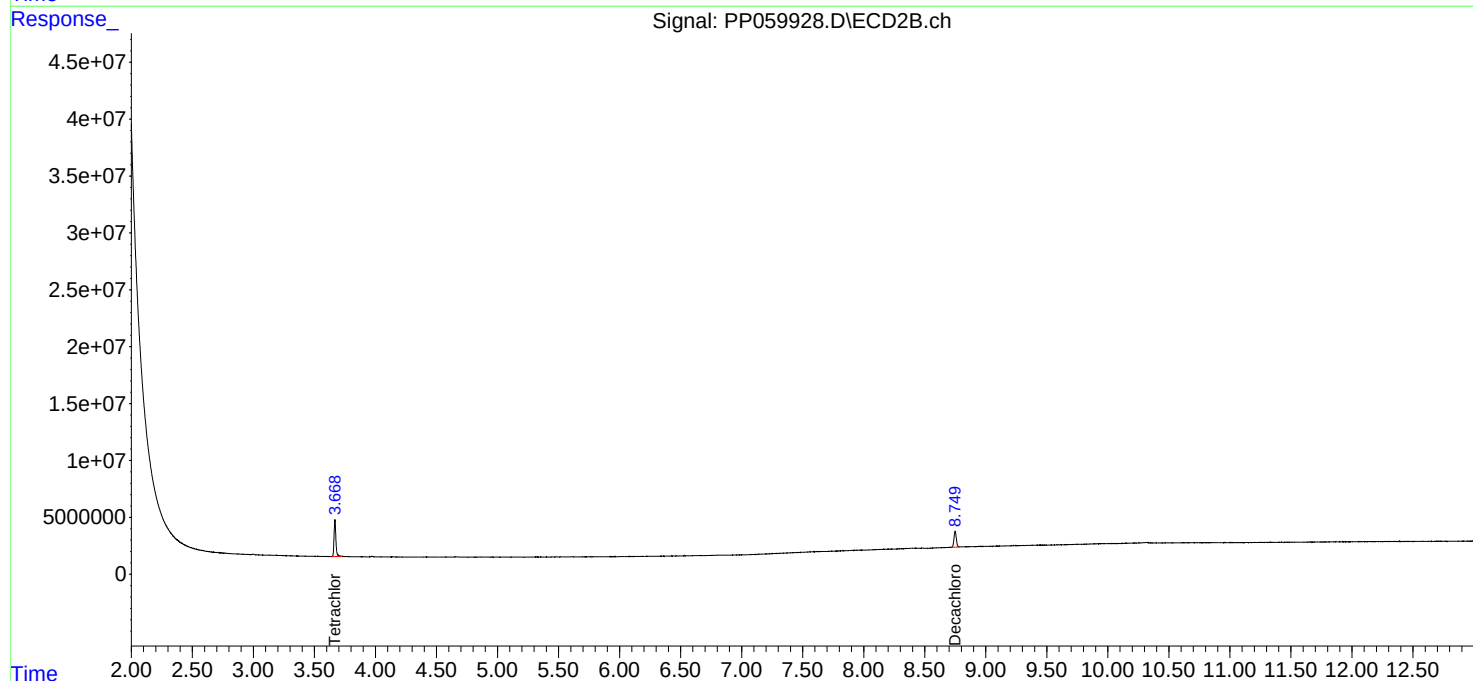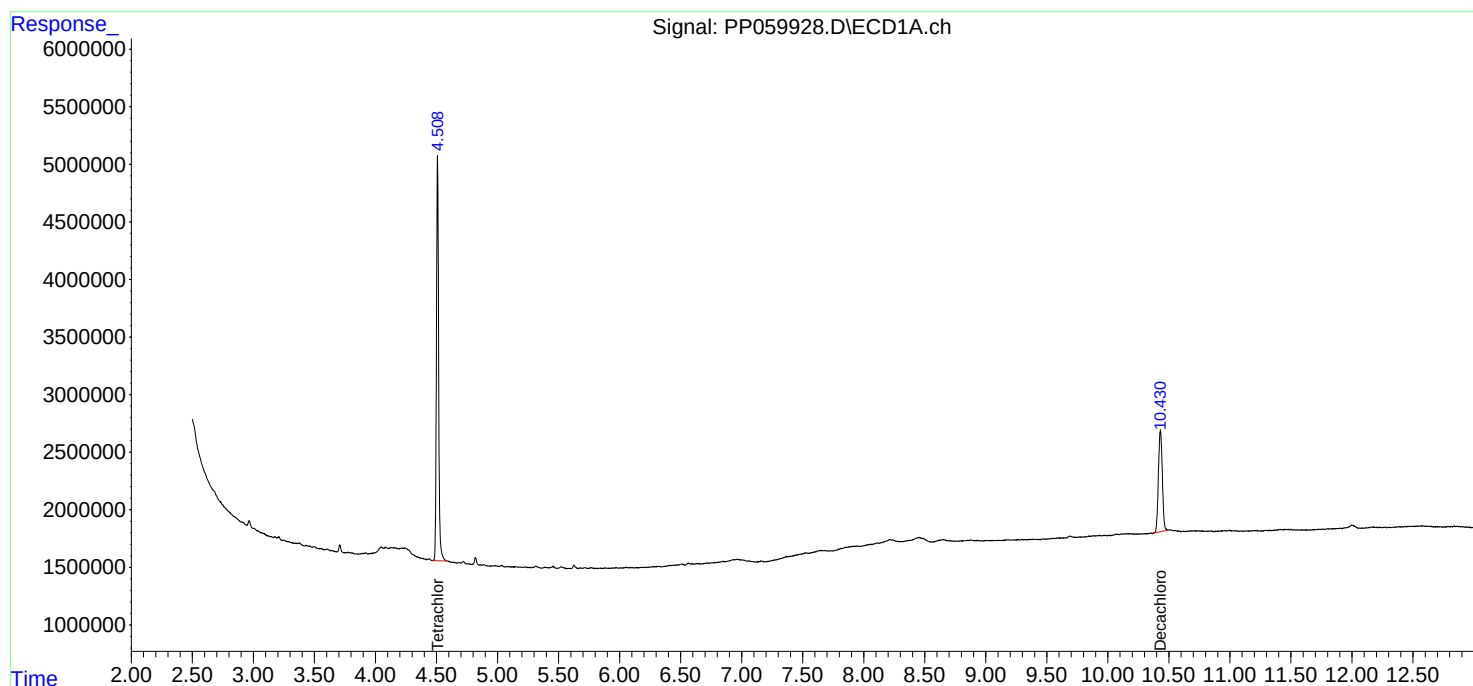

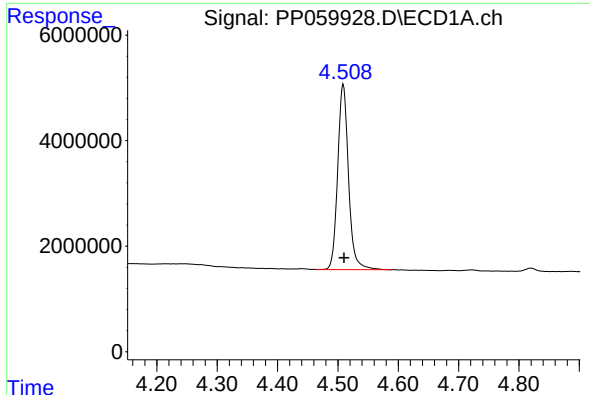

#1 Tetrachloro-m-xylene

R.T.: 4.509 min
Delta R.T.: -0.001 min
Response: 43769077
Conc: 21.04 ng/ml

Instrument :


ECD_P

ClientSampleId :

FB-9-14


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 09/19/2023
Supervised By :Ankita Jodhani 09/19/2023

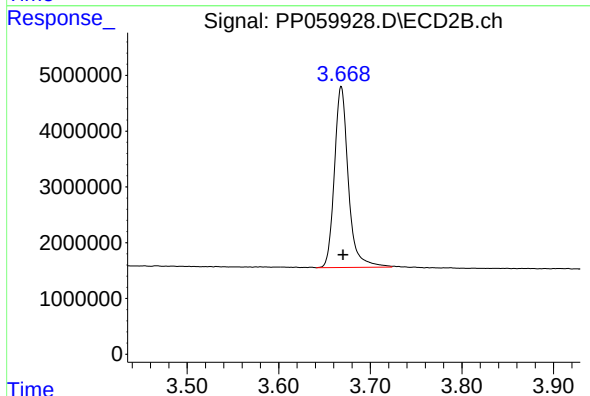


#1 Tetrachloro-m-xylene

R.T.: 3.668 min
Delta R.T.: -0.002 min
Response: 34235687
Conc: 21.02 ng/ml

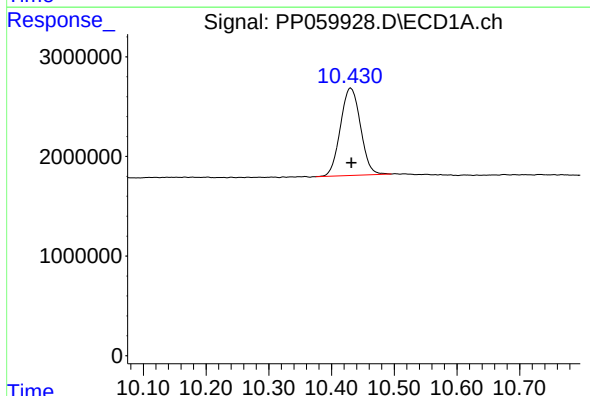

#2 Decachlorobiphenyl

R.T.: 10.430 min
Delta R.T.: -0.002 min
Response: 19502908
Conc: 12.79 ng/ml

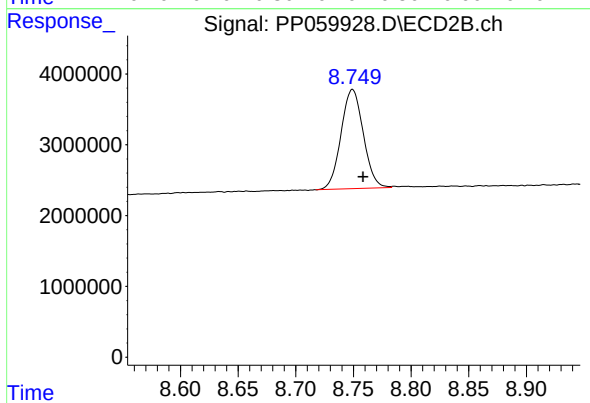

#2 Decachlorobiphenyl

R.T.: 8.749 min
Delta R.T.: -0.010 min
Response: 18719281
Conc: 12.36 ng/ml m