

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
 Data File : PP051438.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 22:47
 Operator : YP\AJ
 Sample : N4698-05 10X
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-31A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:02:37 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 00:25:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.433	3.686	3470796	2255700	1.953	1.493
2) SA Decachlor...	10.257	8.788	3186110	1872224	2.062	1.563
Target Compounds						
5) L1 AR-1016-3	5.686	0.000	368616	0	6.737	N.D. #
18) L4 AR-1242-3	5.686	0.000	368616	0	7.788	N.D. #
20) L4 AR-1242-5	6.530	5.632f	1011447	1277956	28.366	33.652
23) L5 AR-1248-3	6.116f	0.000	359174	0	5.721	N.D. #
24) L5 AR-1248-4	6.469f	0.000	967502	0	15.956	N.D. #
25) L5 AR-1248-5	6.530	5.657	1011447	288506	16.206	5.473 #
26) L6 AR-1254-1	6.469	5.632f	967502	1277956	15.572	15.733
27) L6 AR-1254-2	6.684	0.000	1132907	0	9.815	N.D. #
28) L6 AR-1254-3	7.055	6.167	546235	164200	4.487	1.463 #
30) L6 AR-1254-5	7.792f	0.000	179631	0	2.016	N.D. #
31) L7 AR-1260-1	7.219	0.000	250030	0	2.678	N.D. #
32) L7 AR-1260-2	0.000	6.473	0	384252	N.D.	4.346 #
33) L7 AR-1260-3	0.000	6.646	0	692451	N.D.	8.165 #
34) L7 AR-1260-4	8.079f	0.000	580833	0	6.545	N.D. #
38) L8 AR-1262-3	0.000	7.643	0	1221023	N.D.	18.832 #
41) L9 AR-1268-1	0.000	7.643	0	1221023	N.D.	6.477 #
45) L9 AR-1268-5	0.000	8.529	0	162462	N.D.	0.380 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
Data File : PP051438.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 22:47
Operator : YP\AJ
Sample : N4698-05 10X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:02:37 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 00:25:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

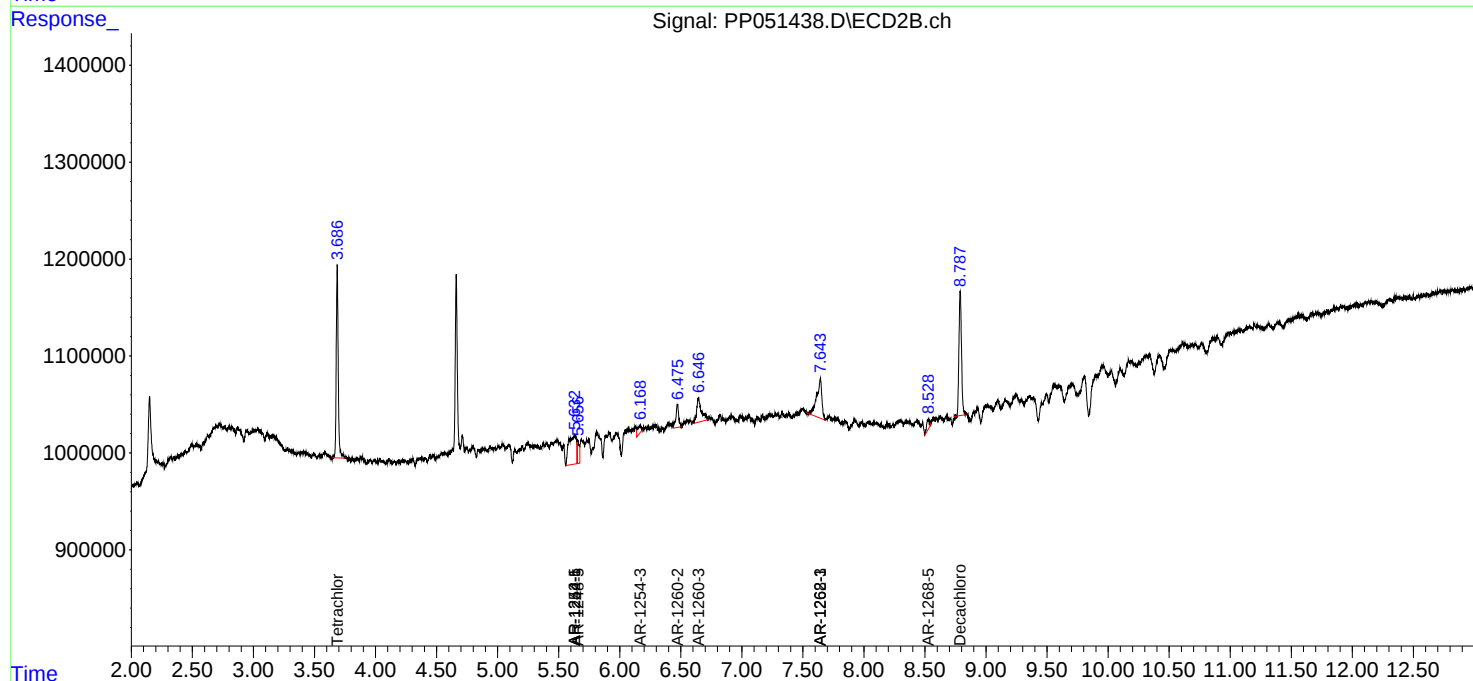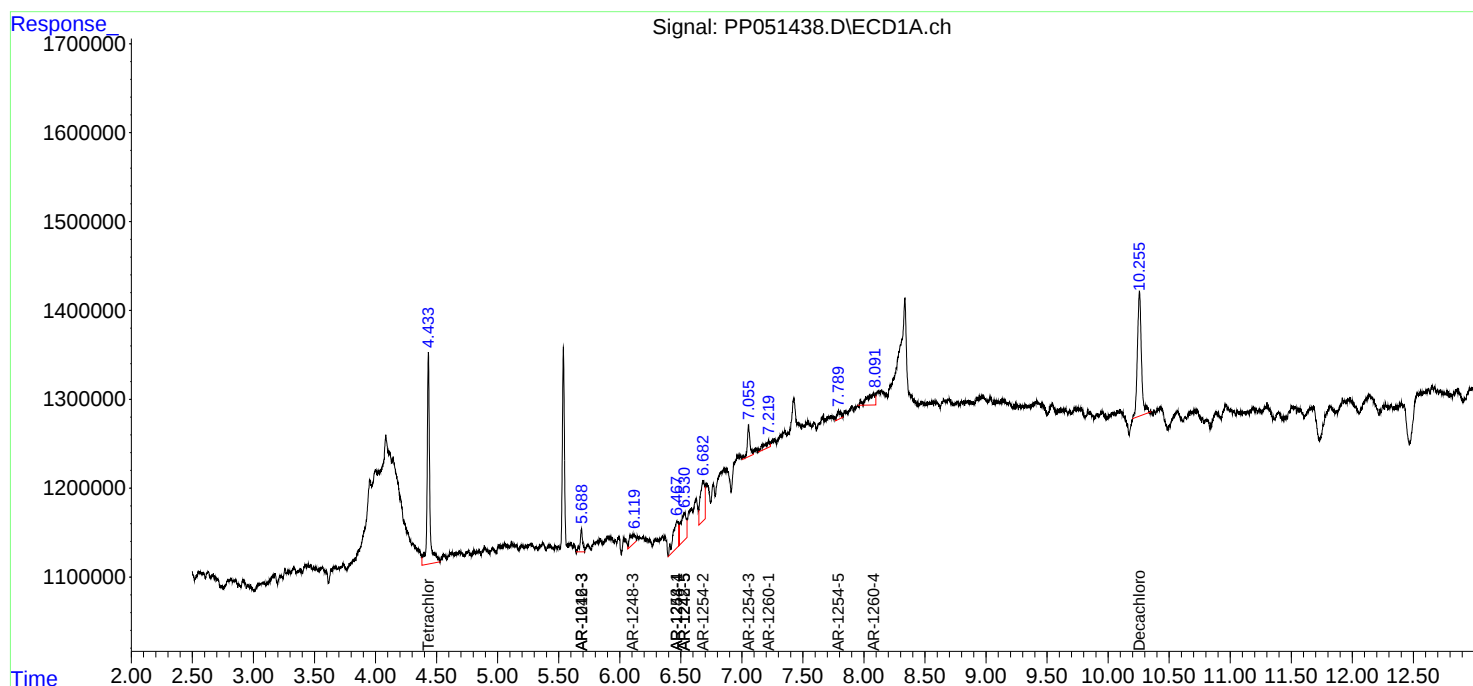


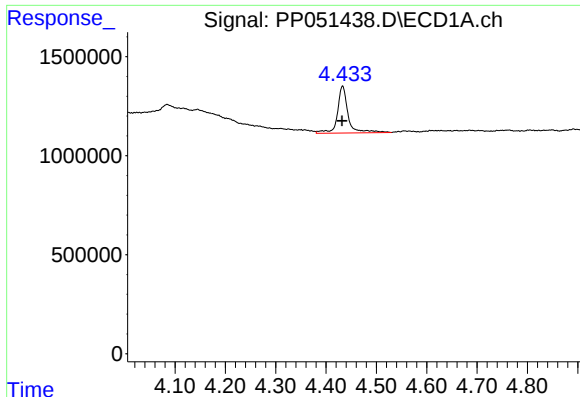

#1 Tetrachloro-m-xylene


R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 3470796
Conc: 1.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

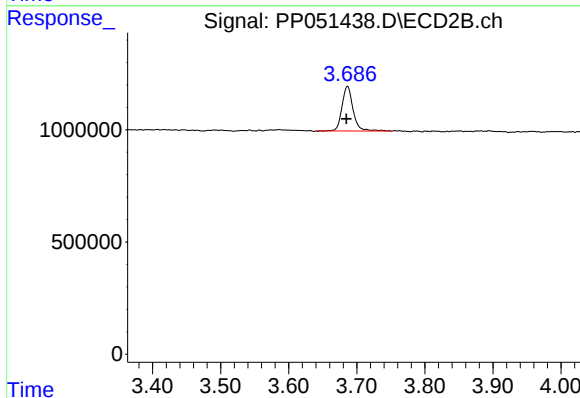


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: 0.002 min
Response: 2255700
Conc: 1.49 ng/ml

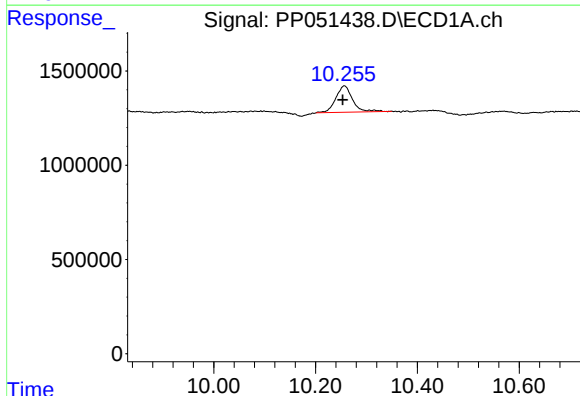


#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: 0.003 min
Response: 3186110
Conc: 2.06 ng/ml

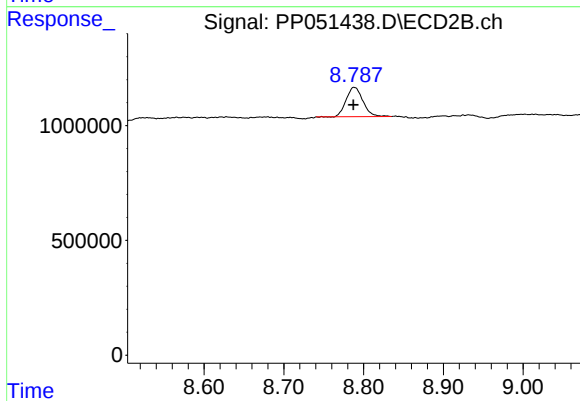

#2 Decachlorobiphenyl


R.T.: 8.788 min
Delta R.T.: 0.001 min
Response: 1872224
Conc: 1.56 ng/ml

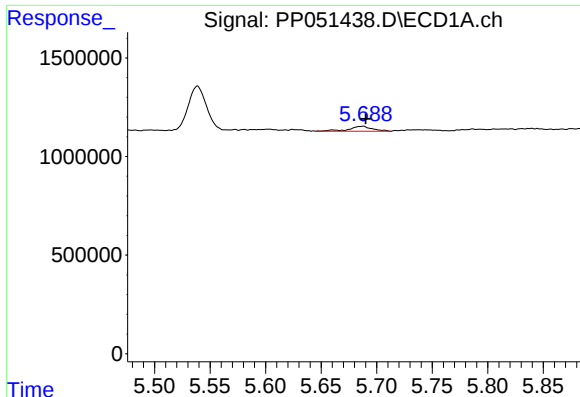

#5 AR-1016-3


R.T.: 5.686 min
Delta R.T.: -0.004 min
Response: 368616
Conc: 6.74 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

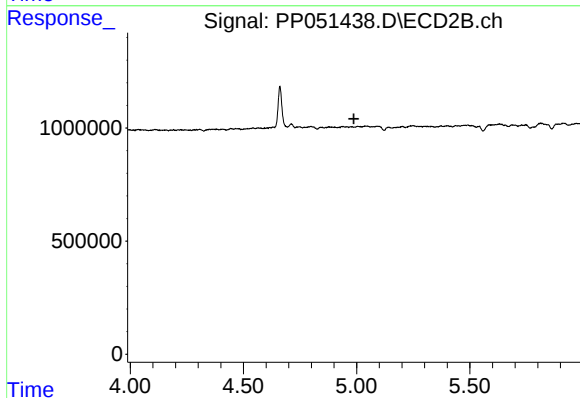


#5 AR-1016-3

R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

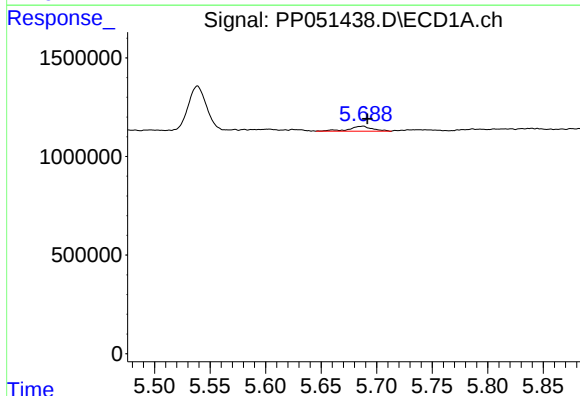


#18 AR-1242-3

R.T.: 5.686 min
Delta R.T.: -0.005 min
Response: 368616
Conc: 7.79 ng/ml

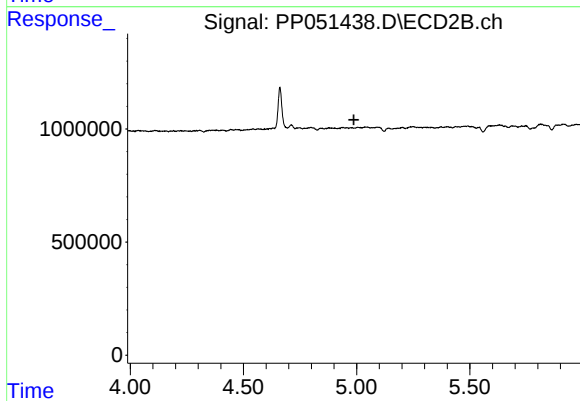

#18 AR-1242-3


R.T.: 0.000 min
Exp R.T. : 4.988 min
Response: 0
Conc: N.D.

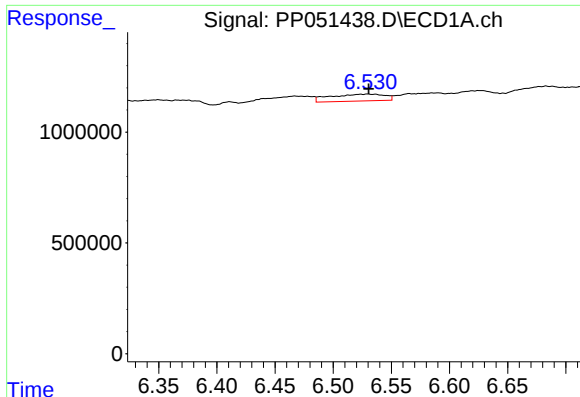

#20 AR-1242-5


R.T.: 6.530 min
Delta R.T.: 0.000 min
Response: 1011447
Conc: 28.37 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

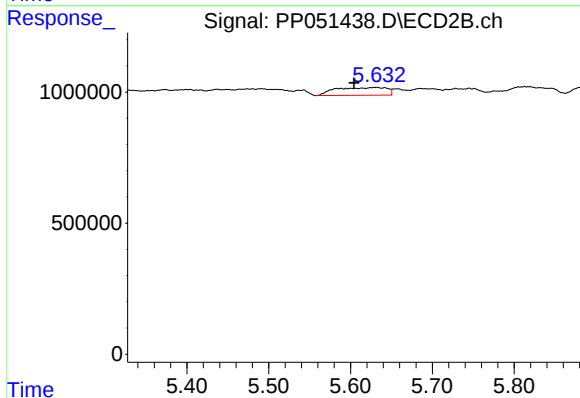


#20 AR-1242-5

R.T.: 5.632 min
Delta R.T.: 0.027 min
Response: 1277956
Conc: 33.65 ng/ml

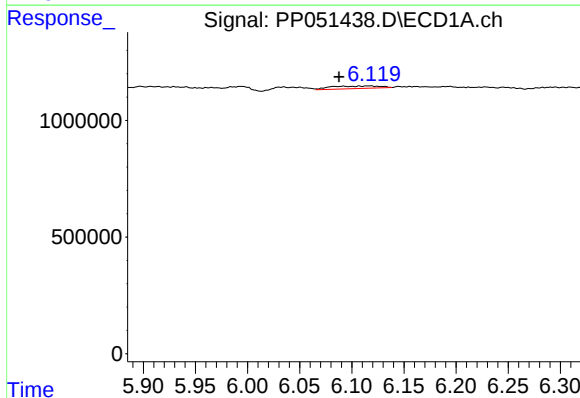


#23 AR-1248-3

R.T.: 6.116 min
Delta R.T.: 0.029 min
Response: 359174
Conc: 5.72 ng/ml

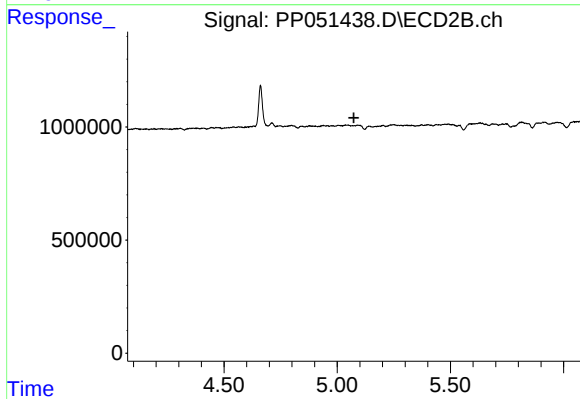

#23 AR-1248-3


R.T.: 0.000 min
Exp R.T.: 5.074 min
Response: 0
Conc: N.D.

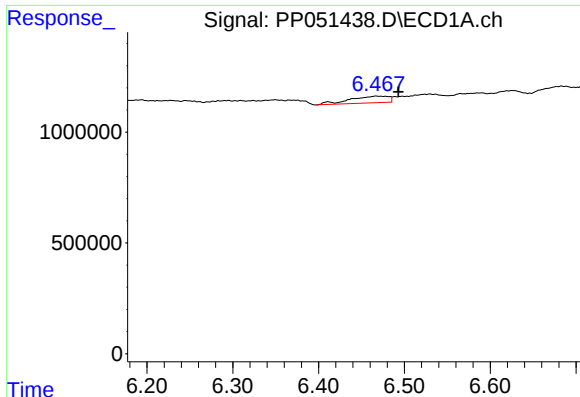

#24 AR-1248-4


R.T.: 6.469 min
Delta R.T.: -0.024 min
Response: 967502
Conc: 15.96 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

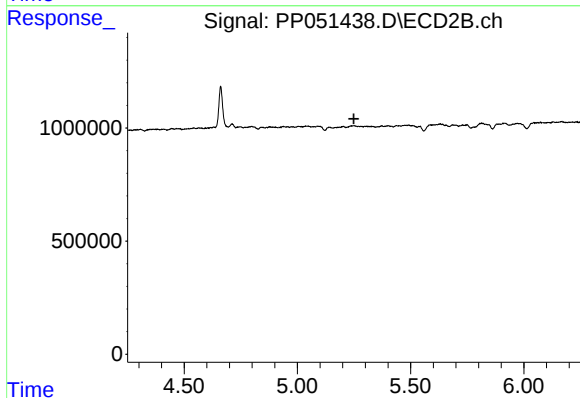


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

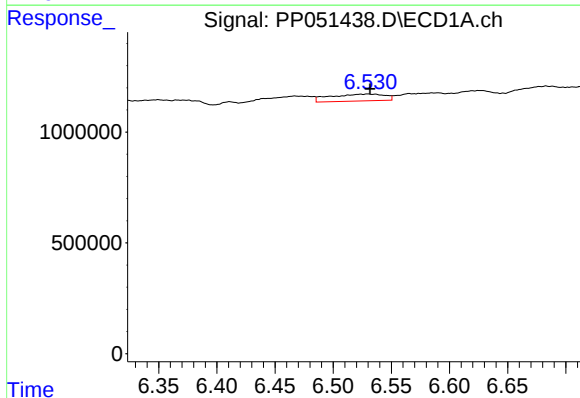


#25 AR-1248-5

R.T.: 6.530 min
Delta R.T.: -0.002 min
Response: 1011447
Conc: 16.21 ng/ml

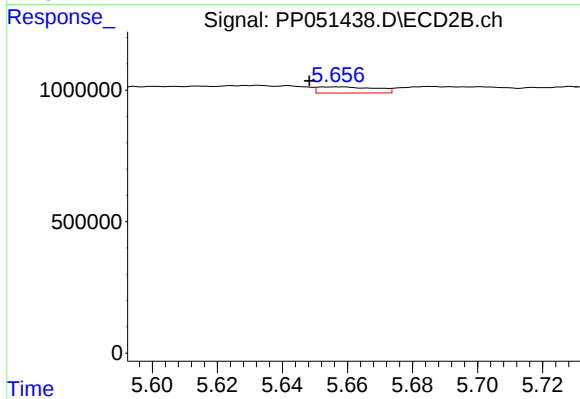

#25 AR-1248-5


R.T.: 5.657 min
Delta R.T.: 0.009 min
Response: 288506
Conc: 5.47 ng/ml

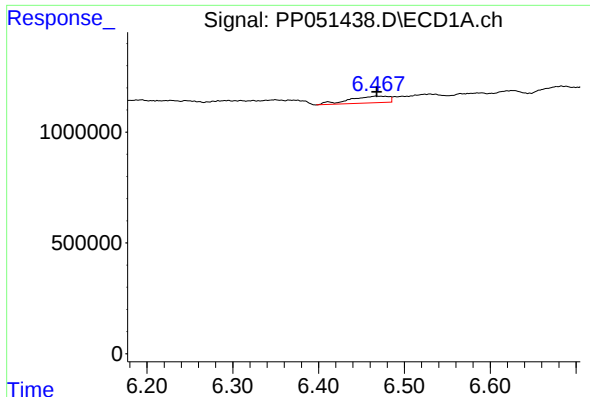

#26 AR-1254-1


R.T.: 6.469 min
Delta R.T.: 0.001 min
Response: 967502
Conc: 15.57 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

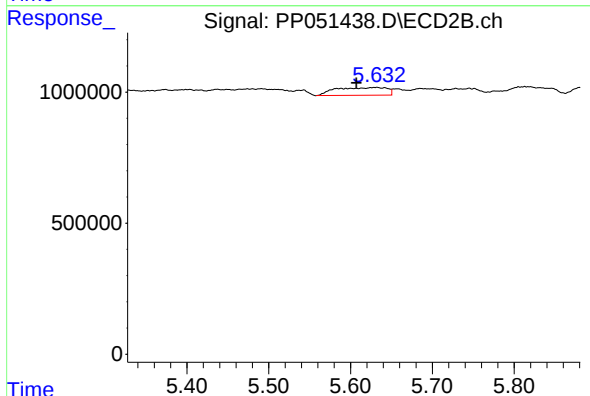


#26 AR-1254-1

R.T.: 5.632 min
Delta R.T.: 0.025 min
Response: 1277956
Conc: 15.73 ng/ml

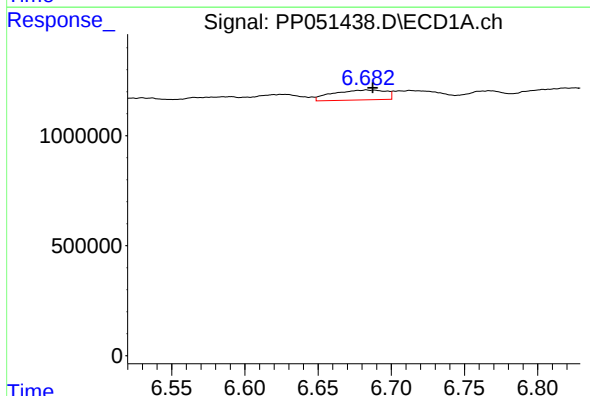


#27 AR-1254-2

R.T.: 6.684 min
Delta R.T.: -0.003 min
Response: 1132907
Conc: 9.81 ng/ml

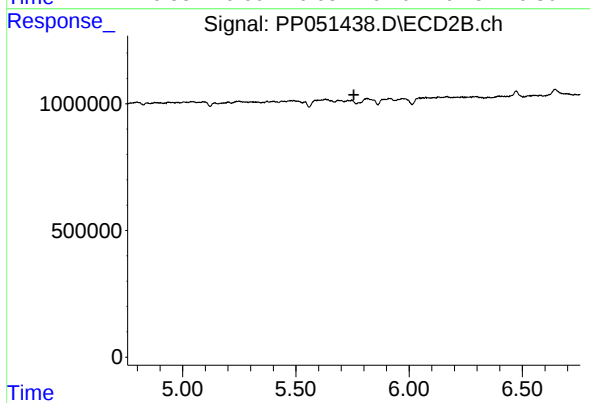

#27 AR-1254-2


R.T.: 0.000 min
Exp R.T.: 5.756 min
Response: 0
Conc: N.D.

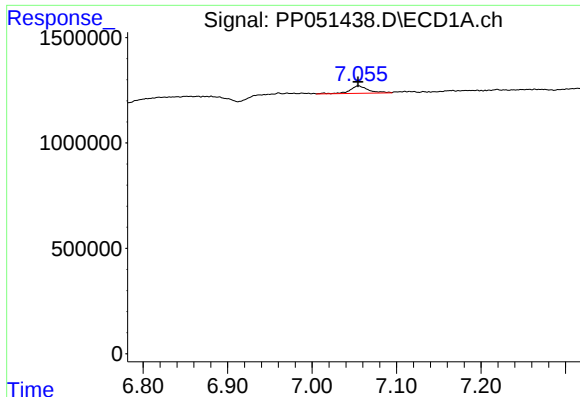

#28 AR-1254-3


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 546235
Conc: 4.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

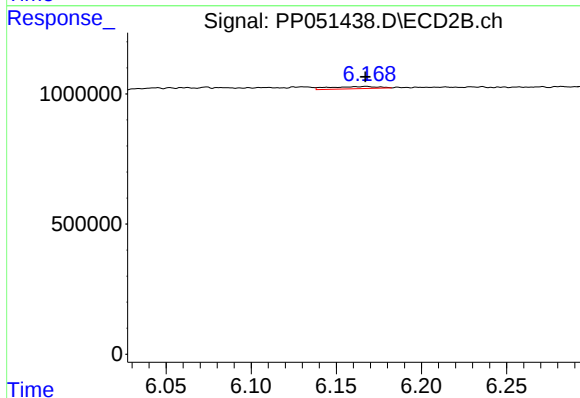


#28 AR-1254-3

R.T.: 6.167 min
Delta R.T.: 0.000 min
Response: 164200
Conc: 1.46 ng/ml

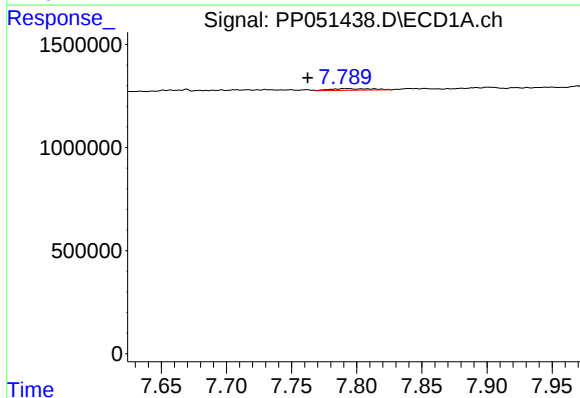


#30 AR-1254-5

R.T.: 7.792 min
Delta R.T.: 0.030 min
Response: 179631
Conc: 2.02 ng/ml

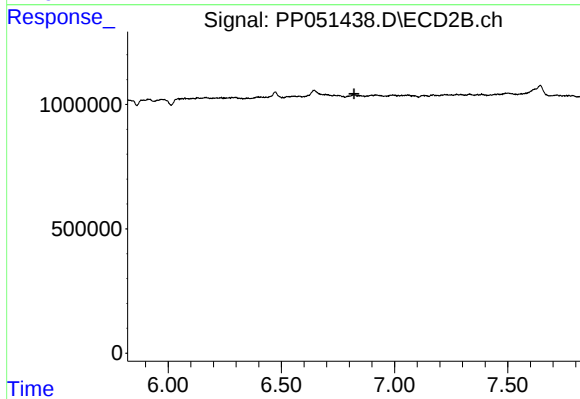

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 6.821 min
Response: 0
Conc: N.D.

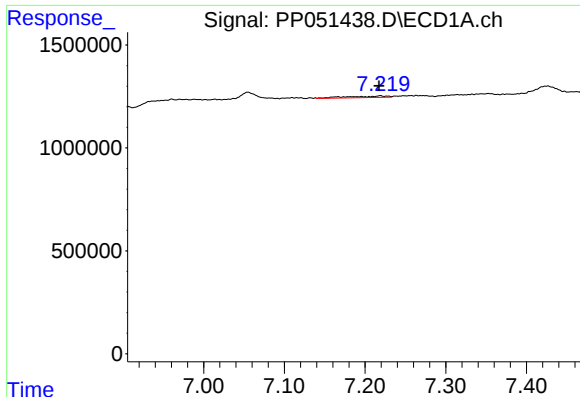

#31 AR-1260-1


R.T.: 7.219 min
Delta R.T.: 0.001 min
Response: 250030
Conc: 2.68 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

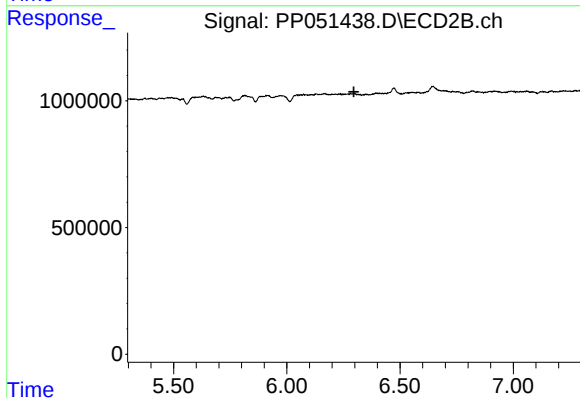


#31 AR-1260-1

R.T.: 0.000 min
Exp R.T. : 6.296 min
Response: 0
Conc: N.D.

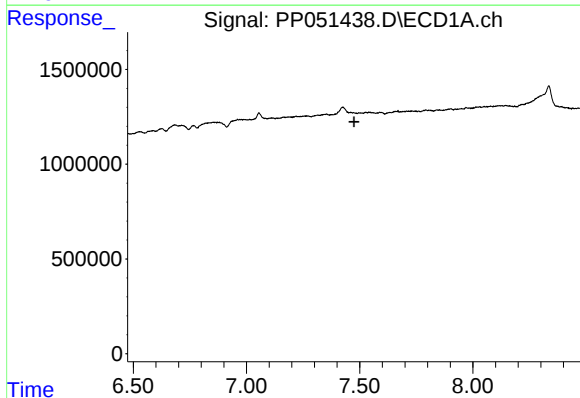


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.475 min
Response: 0
Conc: N.D.

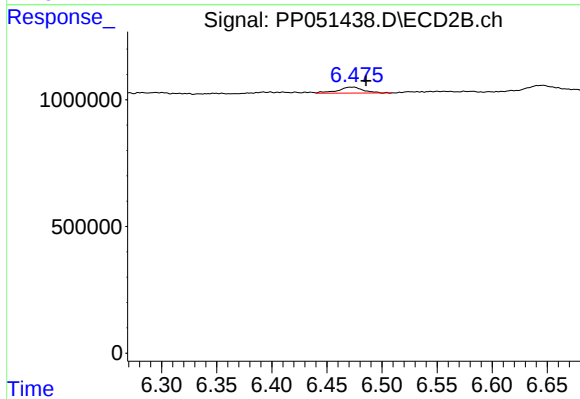

#32 AR-1260-2


R.T.: 6.473 min
Delta R.T.: -0.012 min
Response: 384252
Conc: 4.35 ng/ml

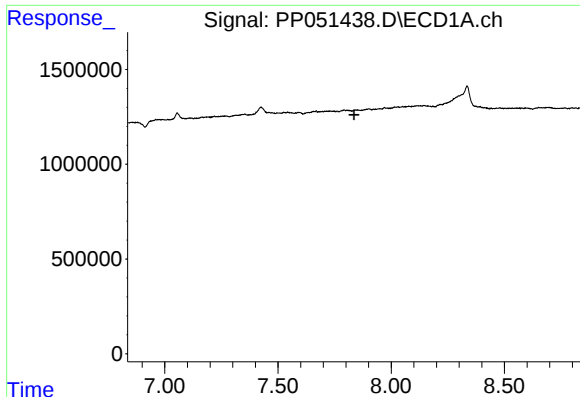

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 7.836 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

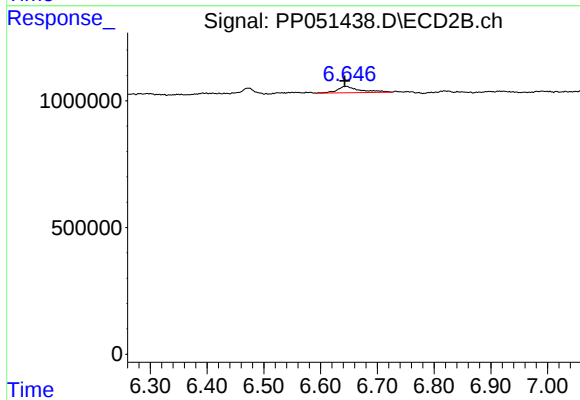


#33 AR-1260-3

R.T.: 6.646 min
Delta R.T.: 0.004 min
Response: 692451
Conc: 8.16 ng/ml

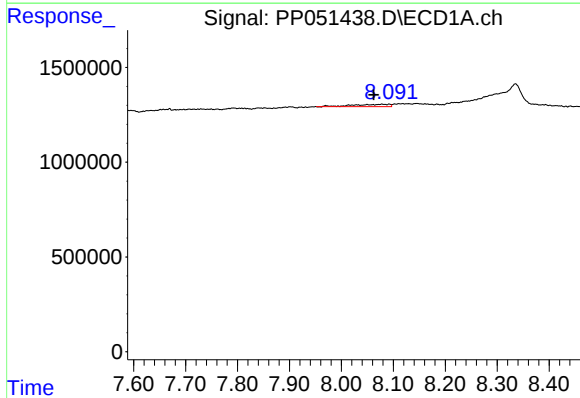


#34 AR-1260-4

R.T.: 8.079 min
Delta R.T.: 0.016 min
Response: 580833
Conc: 6.55 ng/ml

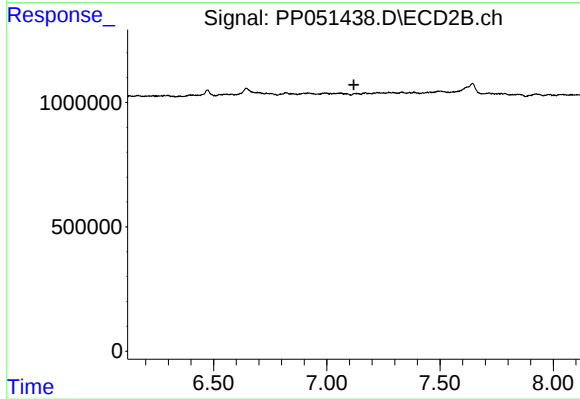

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

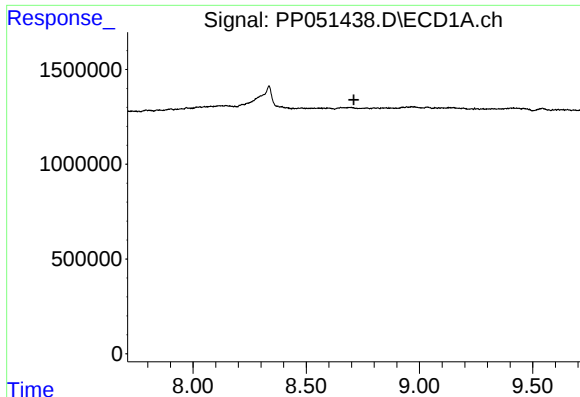

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T.: 8.710 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

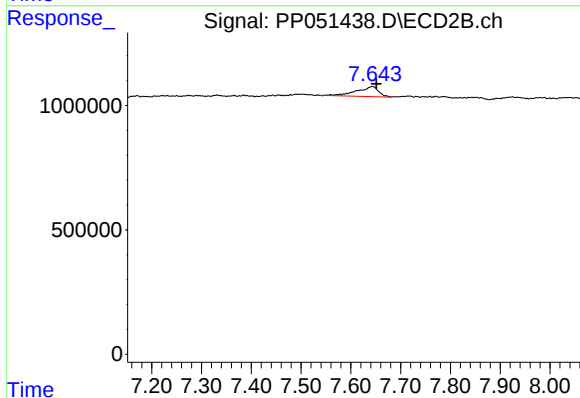


#38 AR-1262-3

R.T.: 7.643 min
Delta R.T.: -0.008 min
Response: 1221023
Conc: 18.83 ng/ml

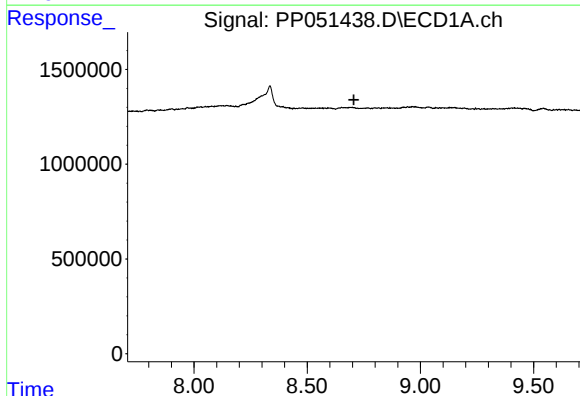


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

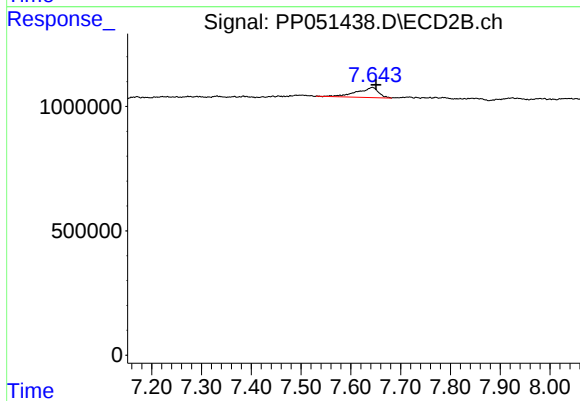

#41 AR-1268-1


R.T.: 7.643 min
Delta R.T.: -0.007 min
Response: 1221023
Conc: 6.48 ng/ml

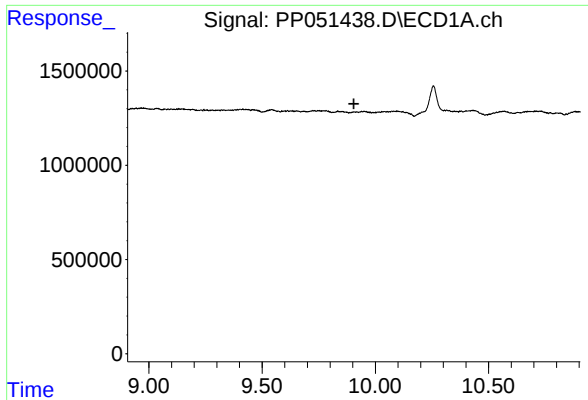

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 9.905 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31A

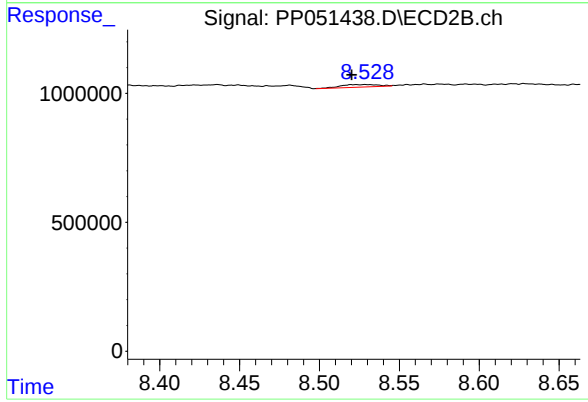

#45 AR-1268-5

R.T.: 8.529 min
Delta R.T.: 0.009 min
Response: 162462
Conc: 0.38 ng/ml