

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
 Data File : PP051439.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2022 23:03
 Operator : YP\AJ
 Sample : N4698-06 10X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MOO-2022-31B

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:03:01 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Sep 20 00:25:26 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.433	3.686	3438200	2441088	1.935	1.616
2)	SA Decachlor...	10.257	8.789	2791588	1990260	1.806	1.661
Target Compounds							
6)	L1 AR-1016-4	5.780	0.000	84036	0	1.974	N.D. #
14)	L3 AR-1232-4	5.780	0.000	84036	0	4.480	N.D. #
19)	L4 AR-1242-4	5.780	0.000	84036	0	2.287	N.D. #
20)	L4 AR-1242-5	6.532	5.596	1825112	3036175	51.184	79.951 #
24)	L5 AR-1248-4	6.472f	0.000	1791742	0	29.549	N.D. #
25)	L5 AR-1248-5	6.532	0.000	1825112	0	29.243	N.D. #
26)	L6 AR-1254-1	6.472	5.596	1791742	3036175	28.839	37.378 #
27)	L6 AR-1254-2	6.680	5.746	1672556	1822754	14.490	25.937 #
28)	L6 AR-1254-3	7.055	6.169	509288	2771691	4.184	24.697 #
32)	L7 AR-1260-2	0.000	6.473	0	416112	N.D.	4.706 #
33)	L7 AR-1260-3	7.840	6.647	355280	912276	4.599	10.757 #
34)	L7 AR-1260-4	8.066	0.000	489479	0	5.516	N.D. #
36)	L8 AR-1262-1	7.840	0.000	355280	0	3.465	N.D. #
38)	L8 AR-1262-3	0.000	7.640	0	1027865	N.D.	15.853 #
41)	L9 AR-1268-1	0.000	7.640	0	1027865	N.D.	5.453 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP091922\
Data File : PP051439.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2022 23:03
Operator : YP\AJ
Sample : N4698-06 10X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:03:01 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP091922.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Sep 20 00:25:26 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

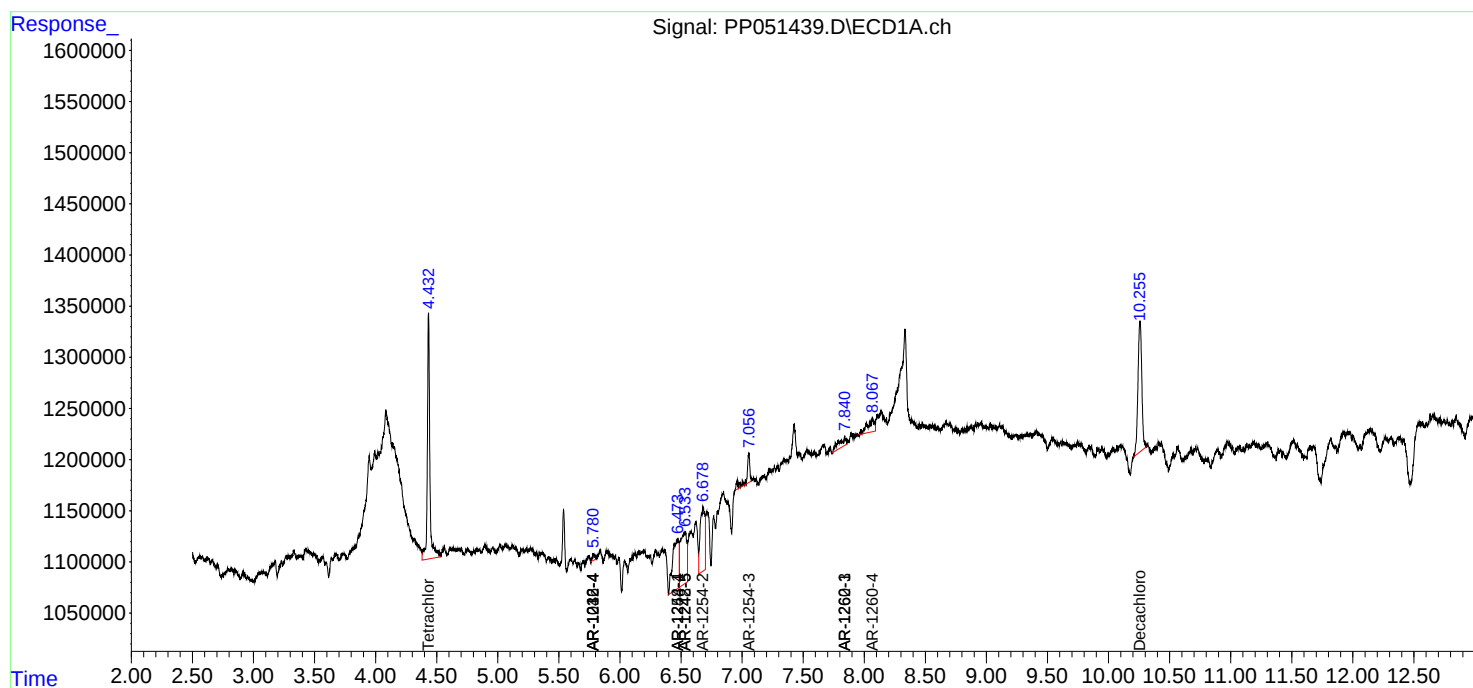


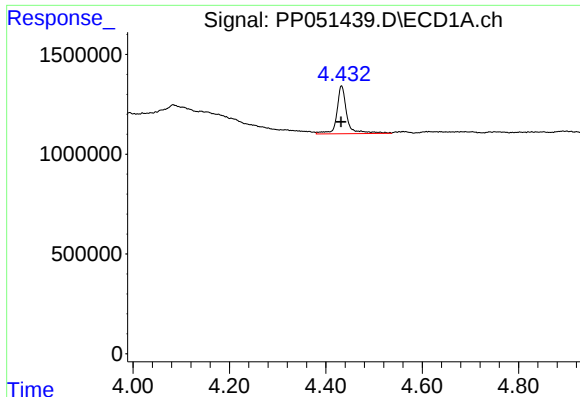

#1 Tetrachloro-m-xylene


R.T.: 4.433 min
Delta R.T.: 0.000 min
Response: 3438200
Conc: 1.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

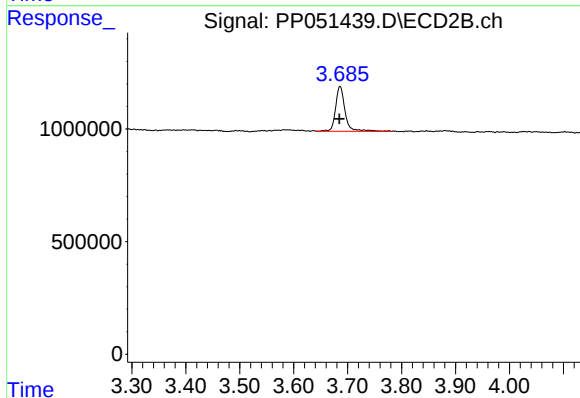


#1 Tetrachloro-m-xylene

R.T.: 3.686 min
Delta R.T.: 0.001 min
Response: 2441088
Conc: 1.62 ng/ml

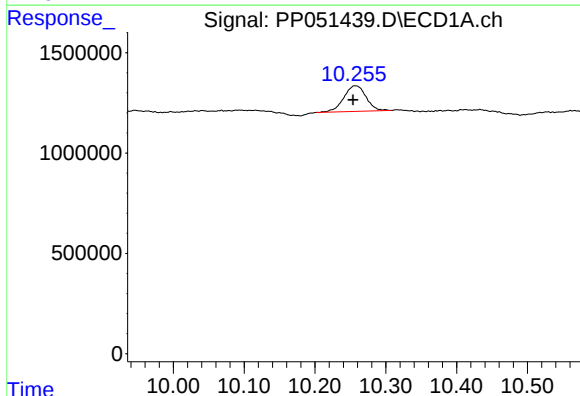


#2 Decachlorobiphenyl

R.T.: 10.257 min
Delta R.T.: 0.003 min
Response: 2791588
Conc: 1.81 ng/ml

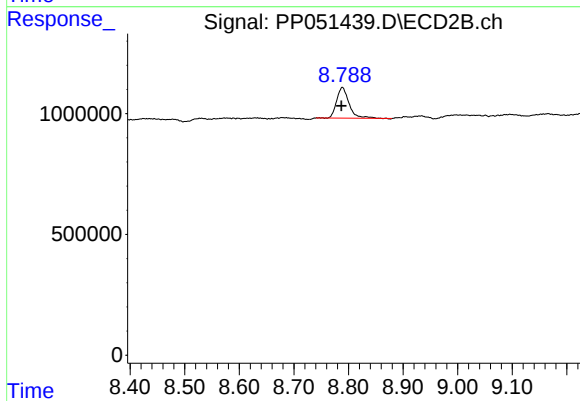

#2 Decachlorobiphenyl


R.T.: 8.789 min
Delta R.T.: 0.002 min
Response: 1990260
Conc: 1.66 ng/ml

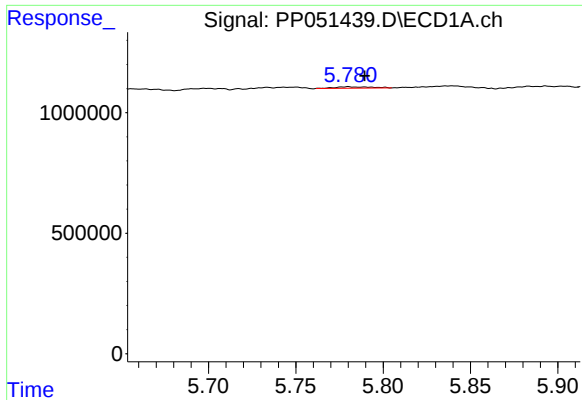

#6 AR-1016-4


R.T.: 5.780 min
Delta R.T.: -0.009 min
Response: 84036
Conc: 1.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

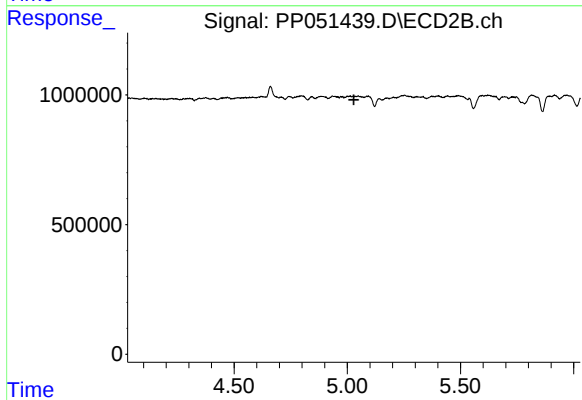


#6 AR-1016-4

R.T.: 0.000 min
Exp R.T. : 5.029 min
Response: 0
Conc: N.D.

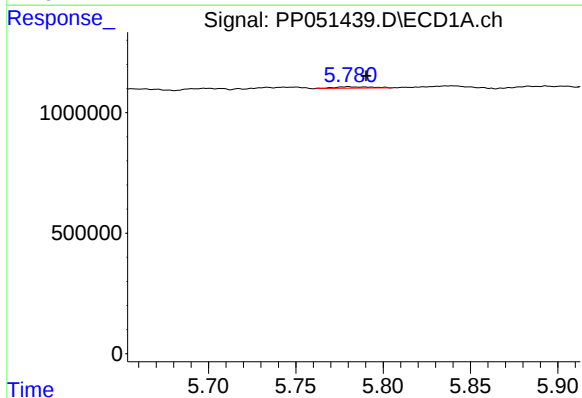


#14 AR-1232-4

R.T.: 5.780 min
Delta R.T.: -0.010 min
Response: 84036
Conc: 4.48 ng/ml

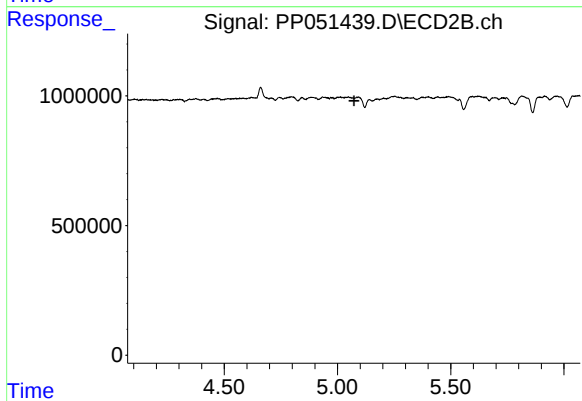

#14 AR-1232-4


R.T.: 0.000 min
Exp R.T. : 5.073 min
Response: 0
Conc: N.D.

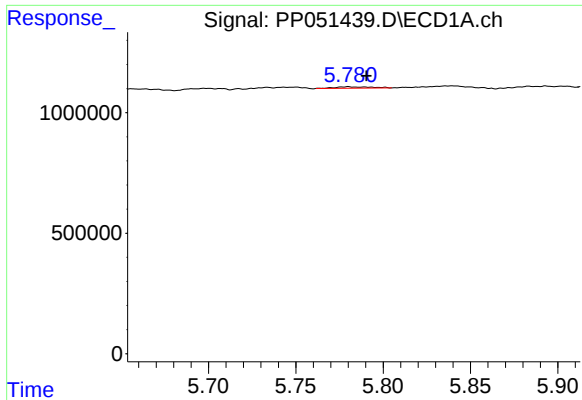

#19 AR-1242-4


R.T.: 5.780 min
Delta R.T.: -0.010 min
Response: 84036
Conc: 2.29 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

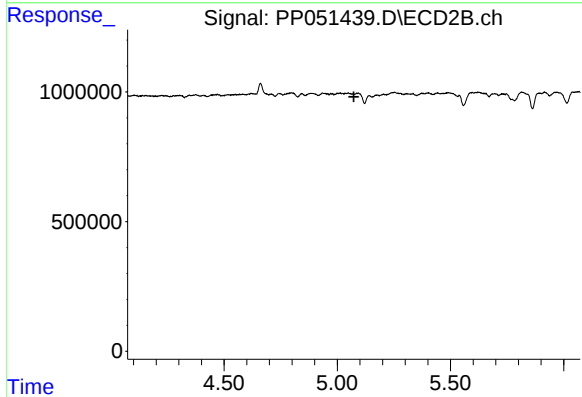


#19 AR-1242-4

R.T.: 0.000 min
Exp R.T. : 5.073 min
Response: 0
Conc: N.D.

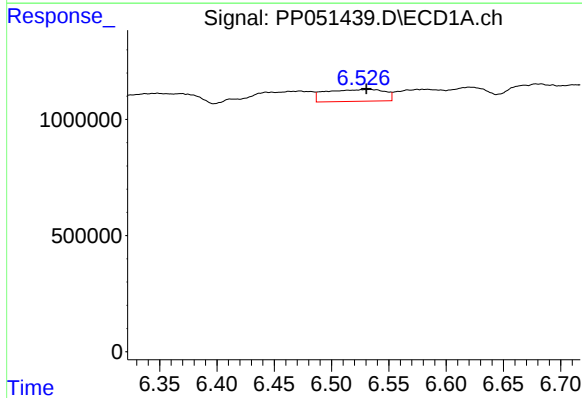


#20 AR-1242-5

R.T.: 6.532 min
Delta R.T.: 0.002 min
Response: 1825112
Conc: 51.18 ng/ml

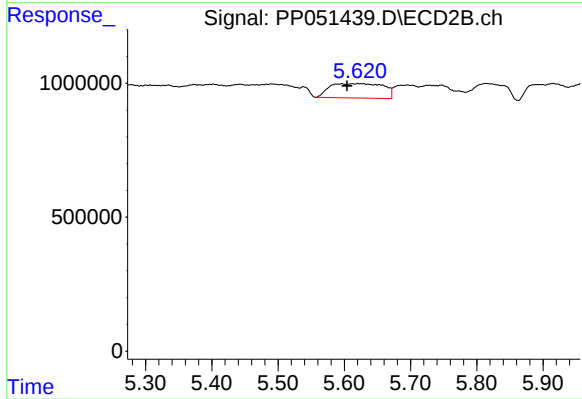

#20 AR-1242-5


R.T.: 5.596 min
Delta R.T.: -0.008 min
Response: 3036175
Conc: 79.95 ng/ml

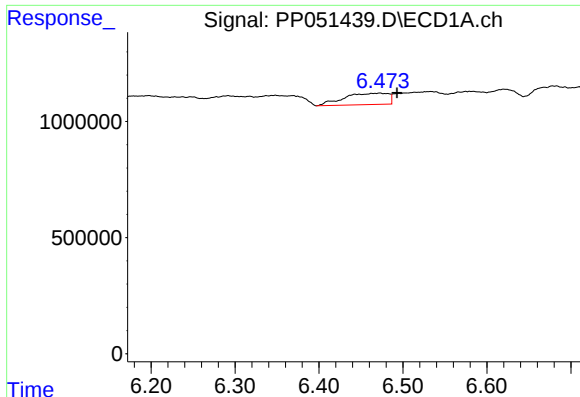

#24 AR-1248-4


R.T.: 6.472 min
Delta R.T.: -0.021 min
Response: 1791742
Conc: 29.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

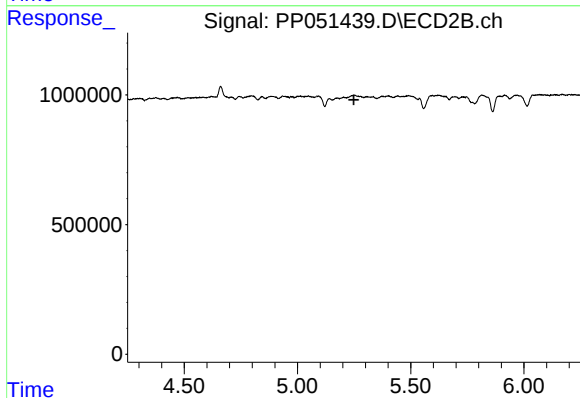


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.249 min
Response: 0
Conc: N.D.

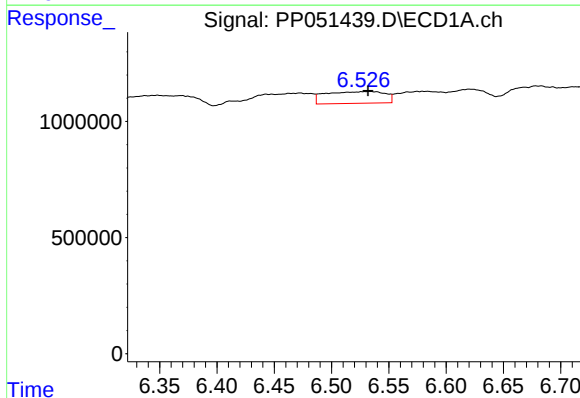


#25 AR-1248-5

R.T.: 6.532 min
Delta R.T.: 0.000 min
Response: 1825112
Conc: 29.24 ng/ml

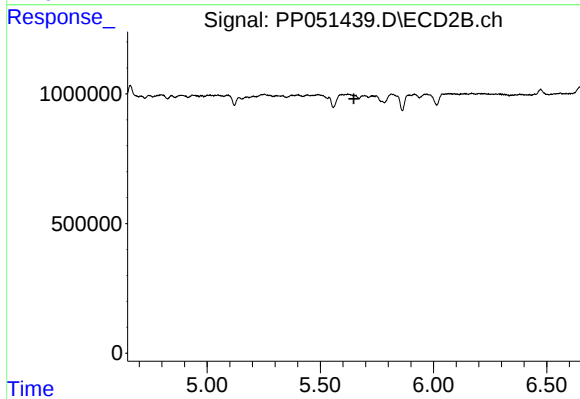

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 5.648 min
Response: 0
Conc: N.D.

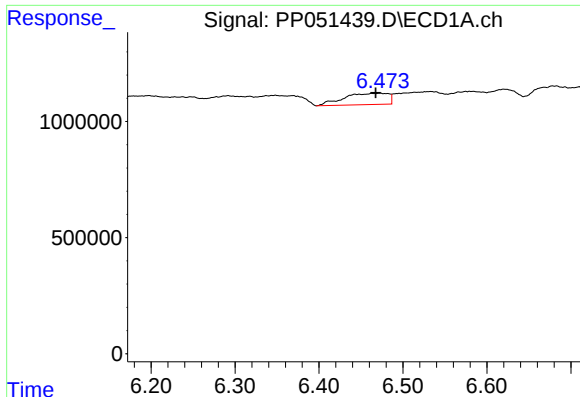

#26 AR-1254-1


R.T.: 6.472 min
Delta R.T.: 0.004 min
Response: 1791742
Conc: 28.84 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

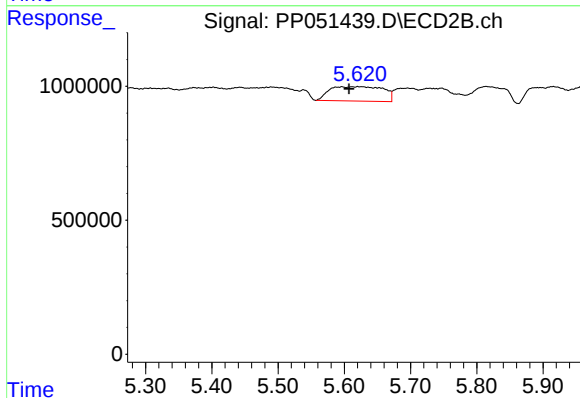


#26 AR-1254-1

R.T.: 5.596 min
Delta R.T.: -0.011 min
Response: 3036175
Conc: 37.38 ng/ml

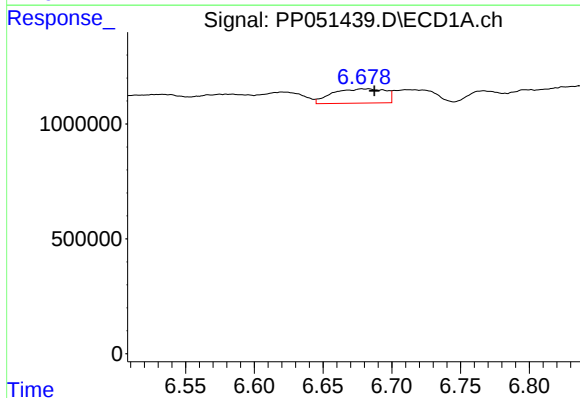


#27 AR-1254-2

R.T.: 6.680 min
Delta R.T.: -0.007 min
Response: 1672556
Conc: 14.49 ng/ml

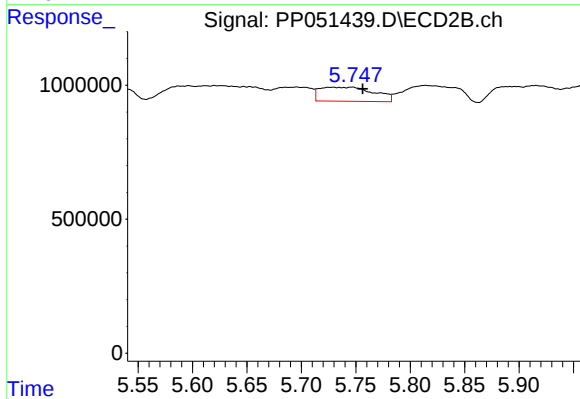

#27 AR-1254-2


R.T.: 5.746 min
Delta R.T.: -0.010 min
Response: 1822754
Conc: 25.94 ng/ml

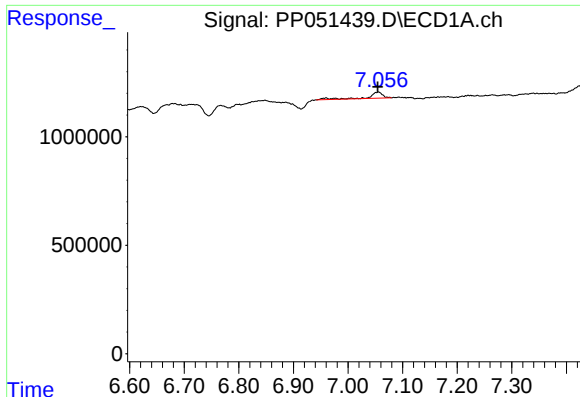

#28 AR-1254-3


R.T.: 7.055 min
Delta R.T.: 0.000 min
Response: 509288
Conc: 4.18 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

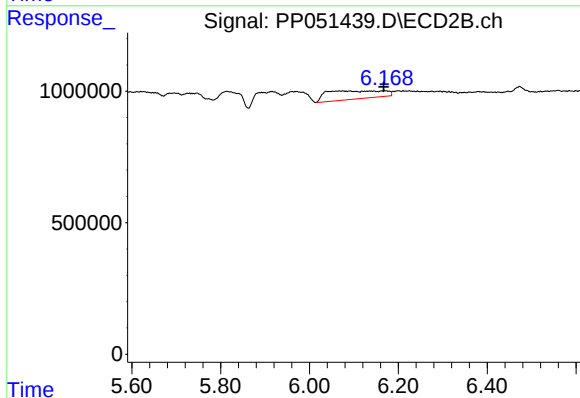


#28 AR-1254-3

R.T.: 6.169 min
Delta R.T.: 0.002 min
Response: 2771691
Conc: 24.70 ng/ml

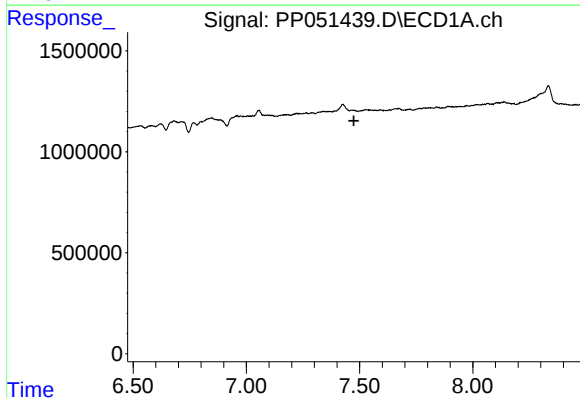


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 7.475 min
Response: 0
Conc: N.D.

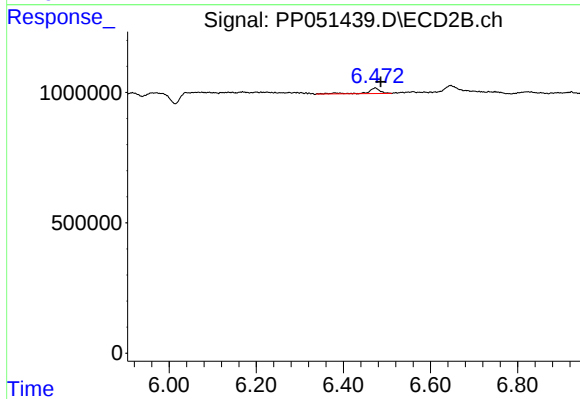

#32 AR-1260-2


R.T.: 6.473 min
Delta R.T.: -0.013 min
Response: 416112
Conc: 4.71 ng/ml

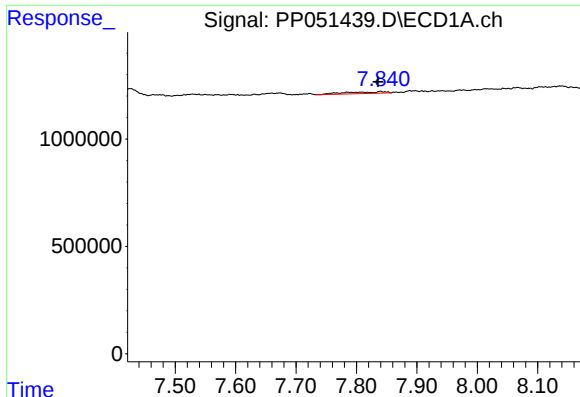

#33 AR-1260-3


R.T.: 7.840 min
Delta R.T.: 0.004 min
Response: 355280
Conc: 4.60 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

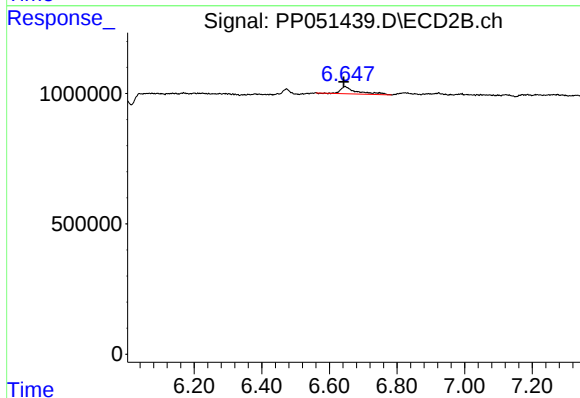


#33 AR-1260-3

R.T.: 6.647 min
Delta R.T.: 0.005 min
Response: 912276
Conc: 10.76 ng/ml

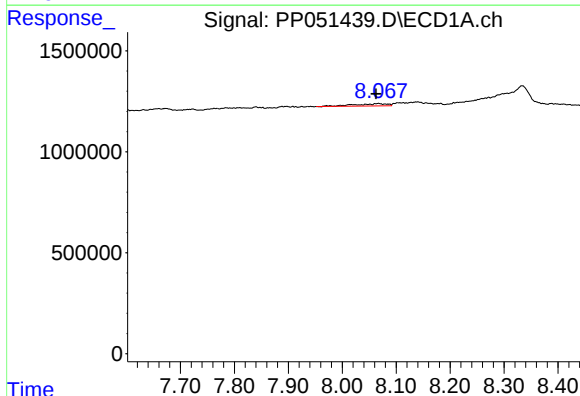


#34 AR-1260-4

R.T.: 8.066 min
Delta R.T.: 0.004 min
Response: 489479
Conc: 5.52 ng/ml

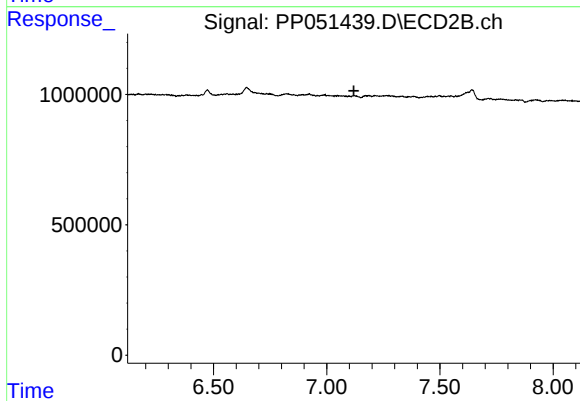

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 7.120 min
Response: 0
Conc: N.D.

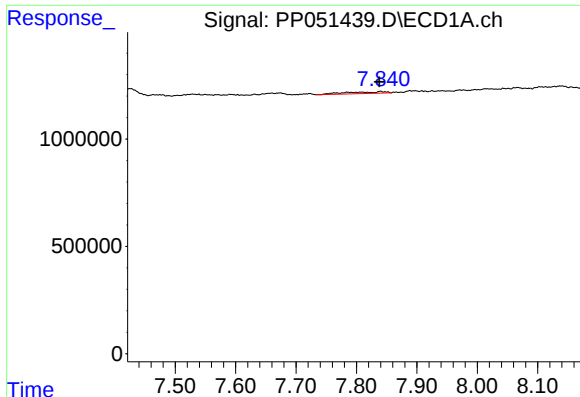

#36 AR-1262-1


R.T.: 7.840 min
Delta R.T.: 0.002 min
Response: 355280
Conc: 3.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

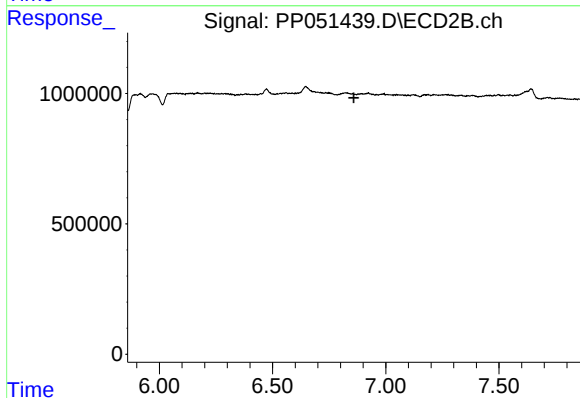


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 6.859 min
Response: 0
Conc: N.D.

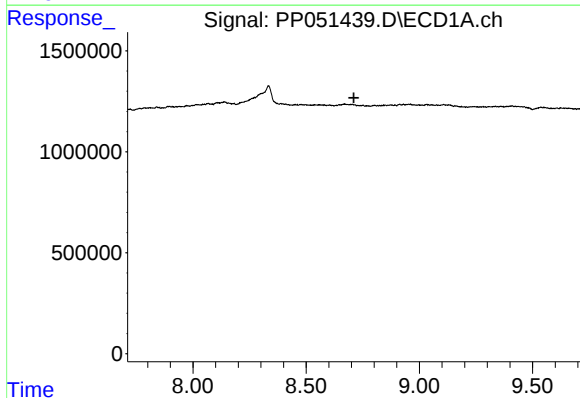


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 8.710 min
Response: 0
Conc: N.D.

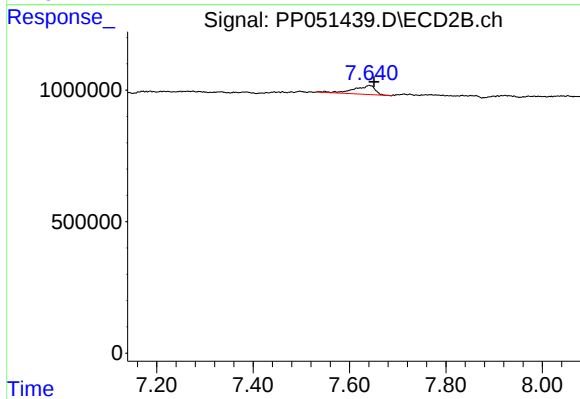

#38 AR-1262-3


R.T.: 7.640 min
Delta R.T.: -0.011 min
Response: 1027865
Conc: 15.85 ng/ml

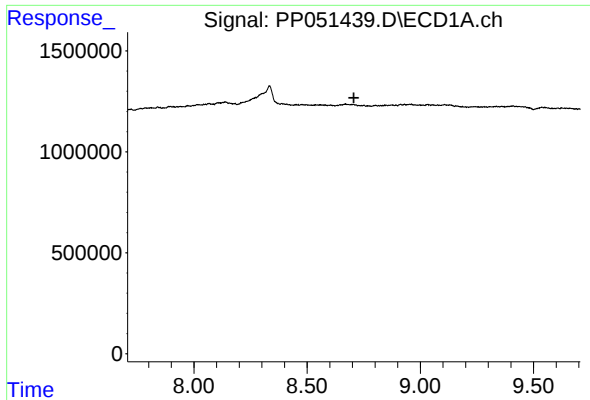

#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 8.706 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MOO-2022-31B

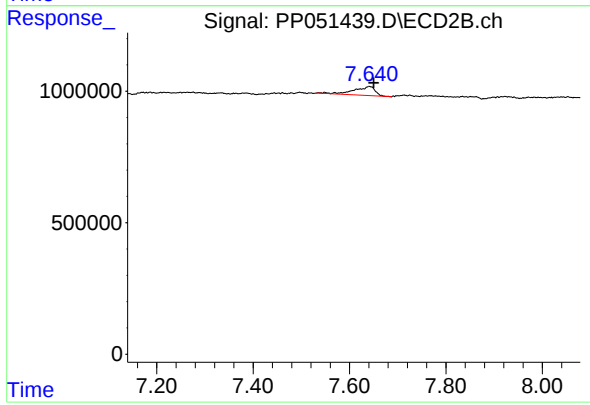

#41 AR-1268-1

R.T.: 7.640 min
Delta R.T.: -0.010 min
Response: 1027865
Conc: 5.45 ng/ml